

System Check_Head_13MHz

DUT: CLA13 - SN1022

Communication System: CW; Frequency: 13.000 MHz

Medium: HSL_4-250_260429 Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.757$ S/m; $\epsilon_r = 55.0$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(14.31, 15.32, 17.61); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.141 W/kg; SAR (10g) = 0.114 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 0.134 W/kg; SAR (8g) = 0.089 W/kg; SAR (10g) = 0.084 W/kg

Smallest distance from peaks to all points 3 dB below = 15.8 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

TSL Correction: Positive only

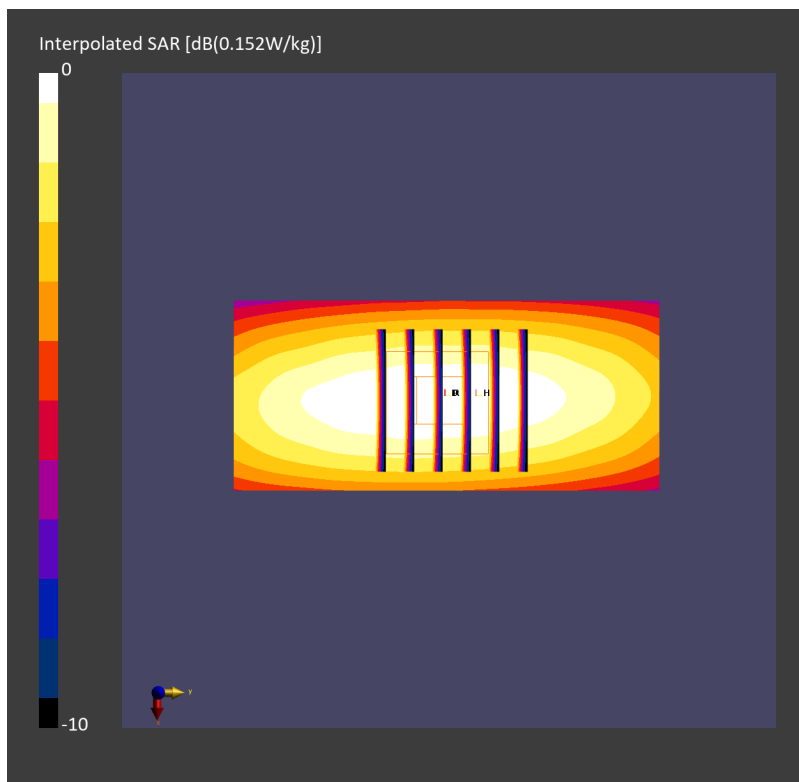

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260216 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.852$ S/m; $\epsilon_r = 45.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.12 W/kg; SAR (10g) = 1.39 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.14 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.40 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.9 %

TSL Correction: Positive only

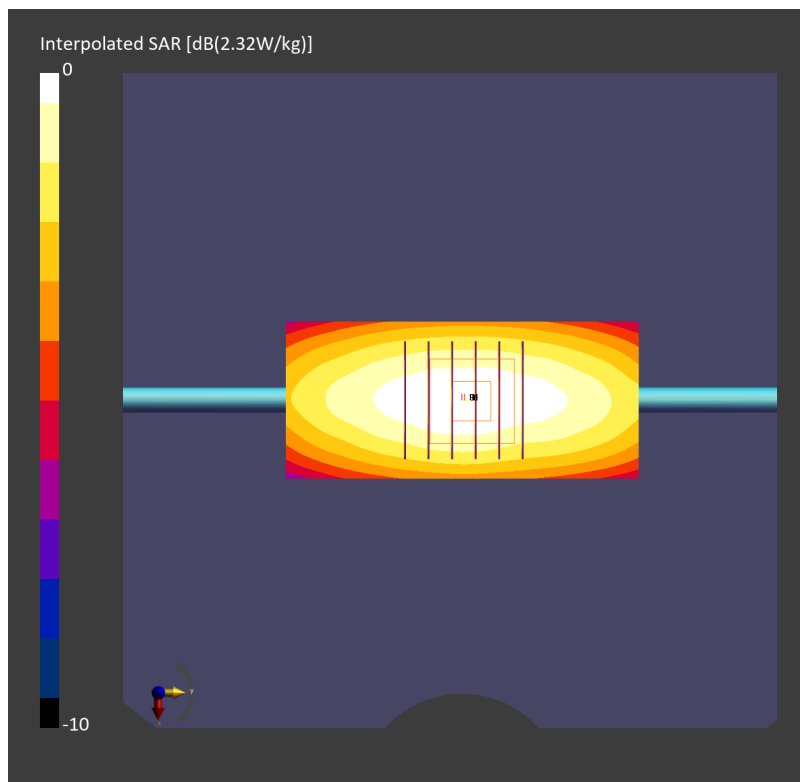

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260224 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.862$ S/m; $\epsilon_r = 44.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.11 W/kg; SAR (10g) = 1.39 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.13 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.41 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.7 %

TSL Correction: Positive only

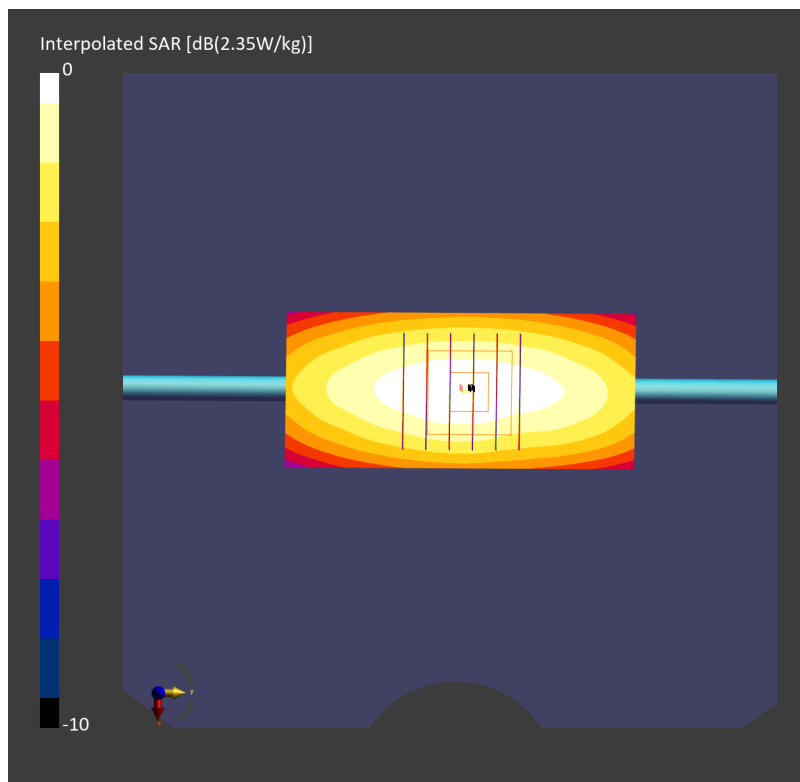

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260302 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.894$ S/m; $\epsilon_r = 44.2$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.72, 7.89, 10.05); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.10 W/kg; SAR (10g) = 1.39 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.10 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

TSL Correction: Positive only

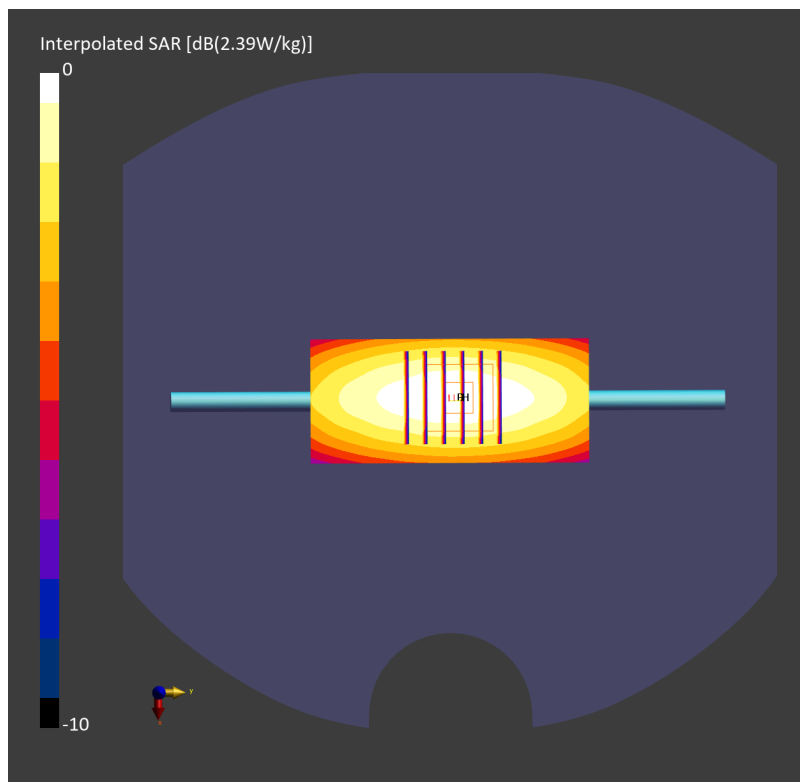

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260306 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.856$ S/m; $\epsilon_r = 45.4$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.39 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.15 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.41 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

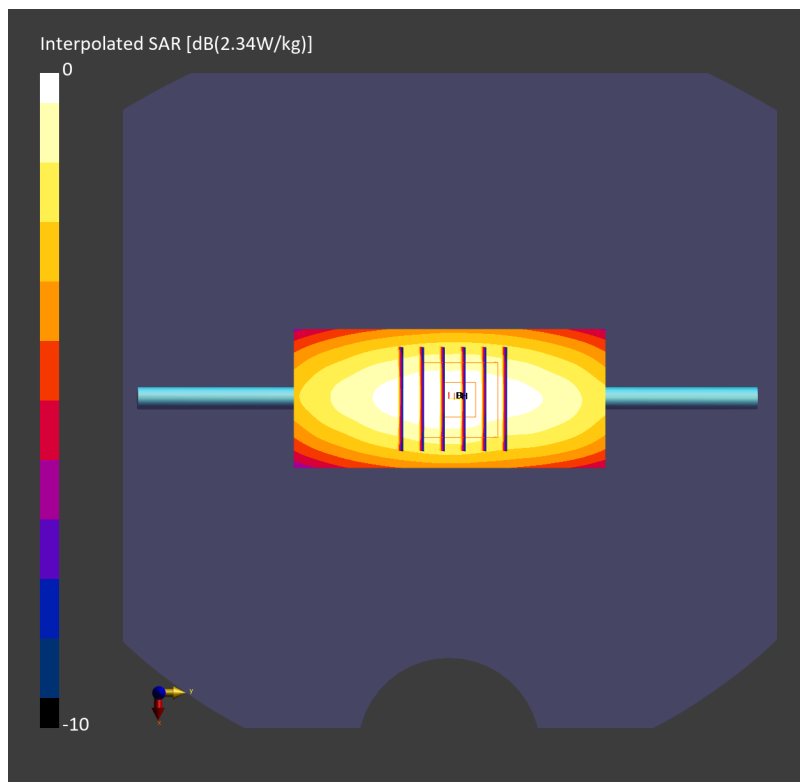

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260309 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.855$ S/m; $\epsilon_r = 44.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.11 W/kg; SAR (10g) = 1.38 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.14 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.40 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.1 %

TSL Correction: Positive only

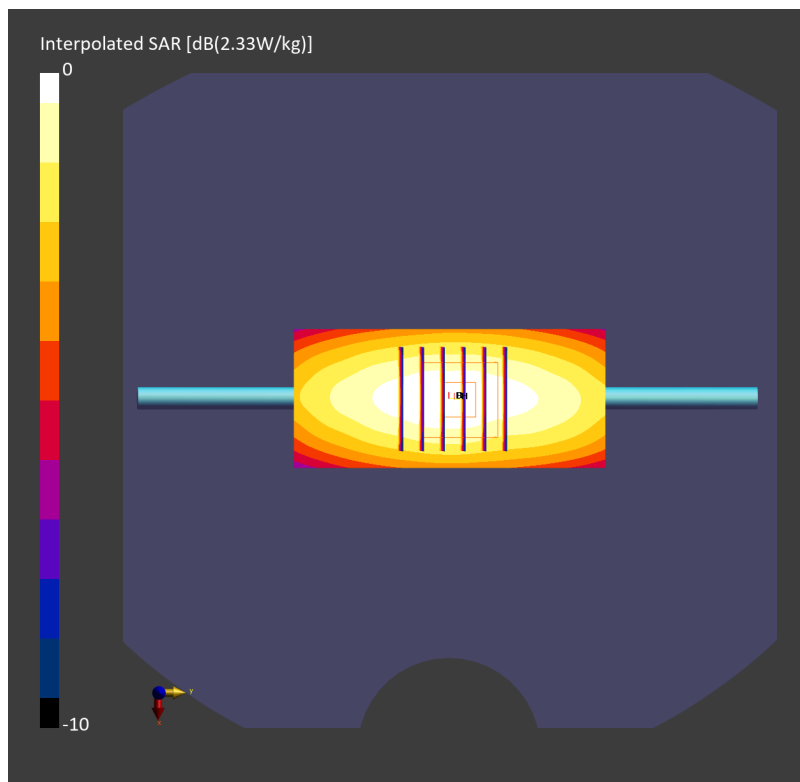

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260310 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.889$ S/m; $\epsilon_r = 44.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.72, 7.89, 10.05); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.09 W/kg; SAR (10g) = 1.38 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.09 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.41 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.6 %

TSL Correction: Positive only

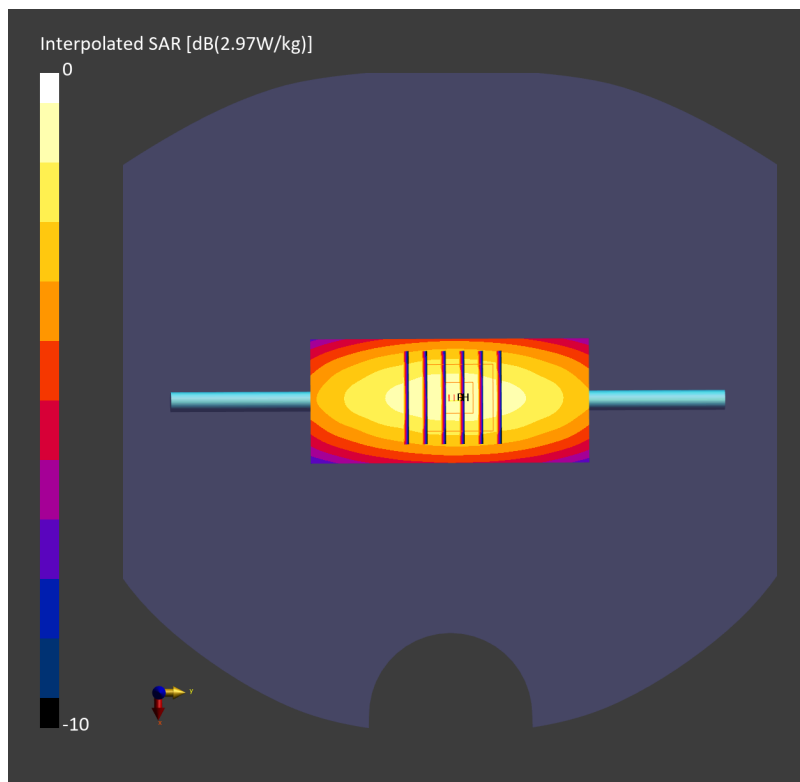

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260325 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.862$ S/m; $\epsilon_r = 44.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.40 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.14 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.41 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 86.7 %

TSL Correction: Positive only

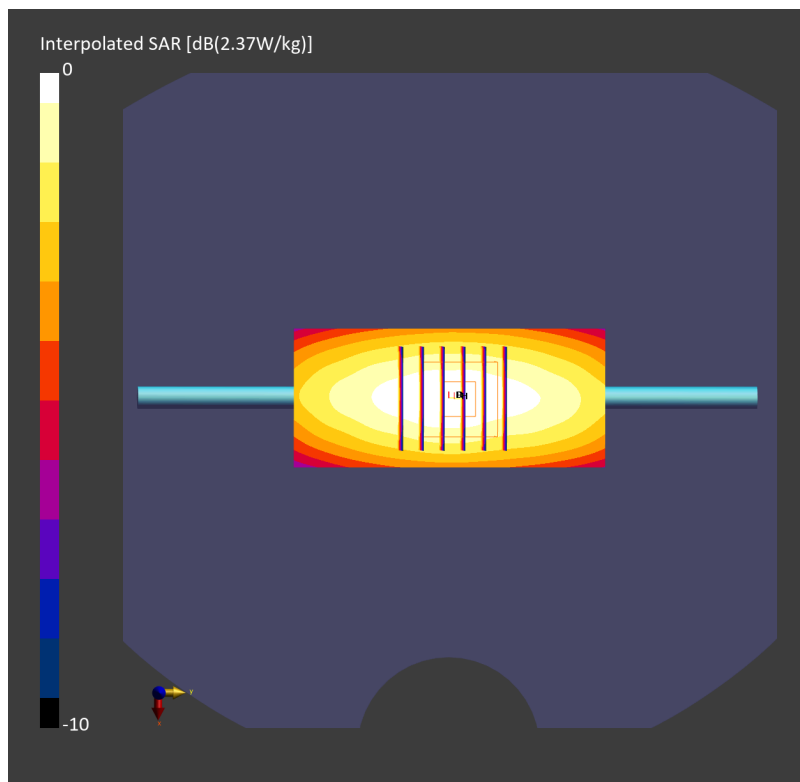

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260331 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.863$ S/m; $\epsilon_r = 44.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(9.12, 9.44, 9.21); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.14 W/kg; SAR (10g) = 1.41 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.16 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.6 %

TSL Correction: Positive only

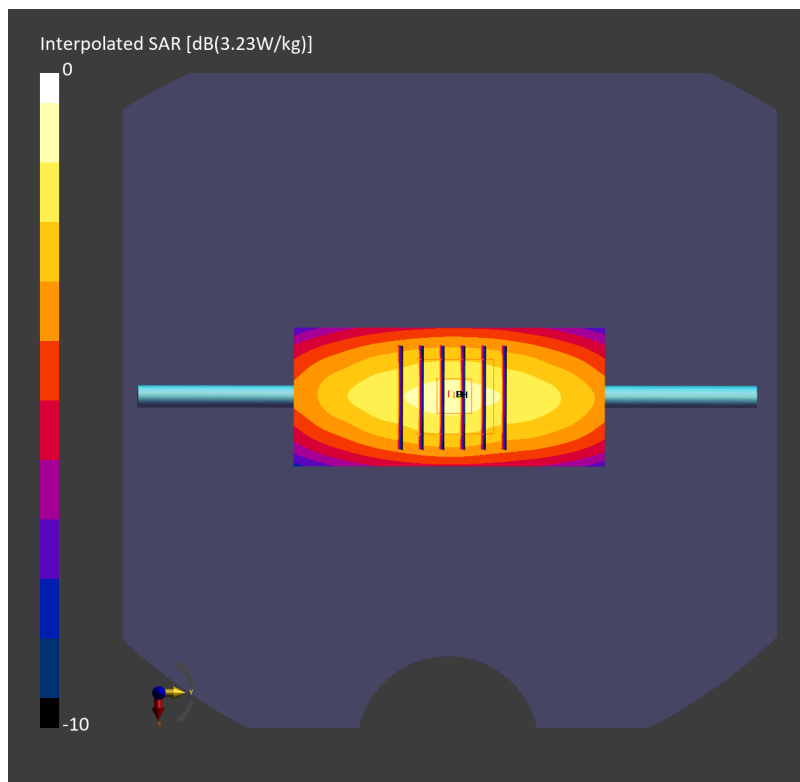

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260401 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.889$ S/m; $\epsilon_r = 43.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(10.53, 10.25, 10.24); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.20 W/kg; SAR (10g) = 1.46 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.19 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.46 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.2 %

TSL Correction: Positive only

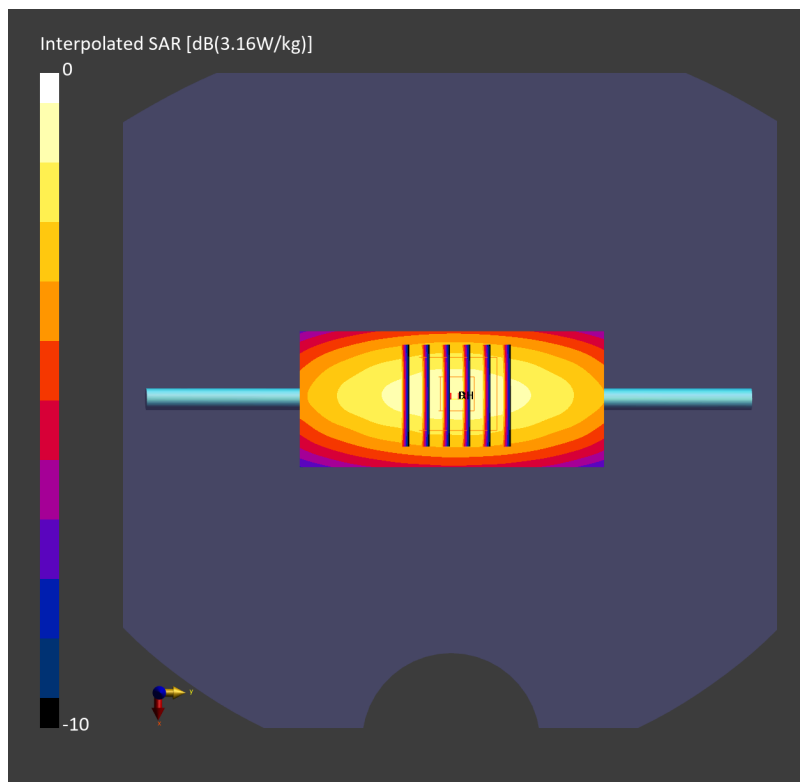

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260406 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.886$ S/m; $\epsilon_r = 43.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(10.53, 10.25, 10.24); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.21 W/kg; SAR (10g) = 1.46 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.19 W/kg; SAR (8g) = 1.54 W/kg; SAR (10g) = 1.46 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.2 %

TSL Correction: Positive only

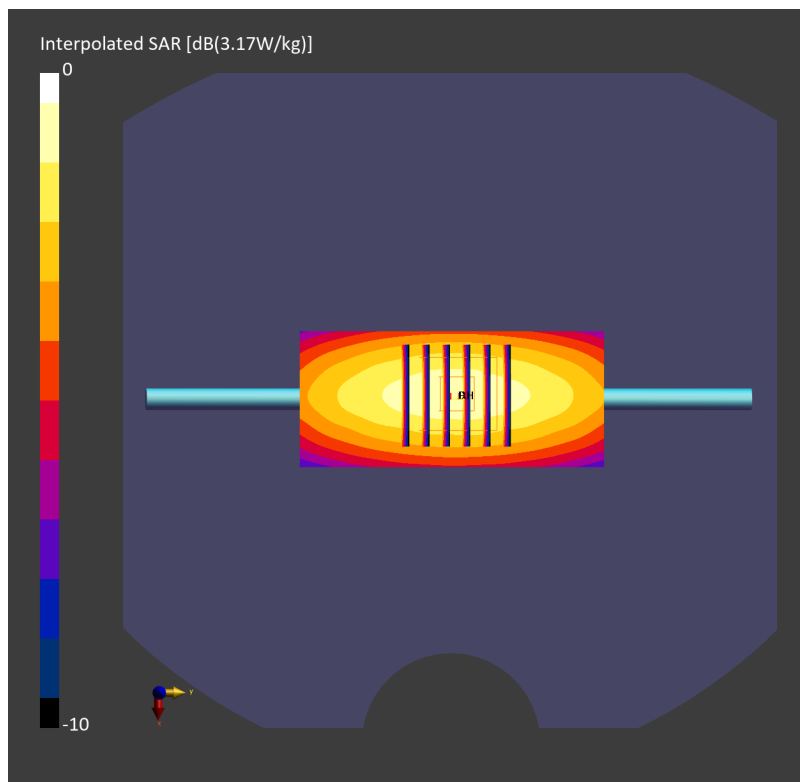

System Check_Head_835MHz

DUT: D835V2 - SN499

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260217 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.907$ S/m; $\epsilon_r = 44.8$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.57 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.65 W/kg; SAR (10g) = 1.57 W/kg

Smallest distance from peaks to all points 3 dB below = 14.5 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

TSL Correction: Positive only

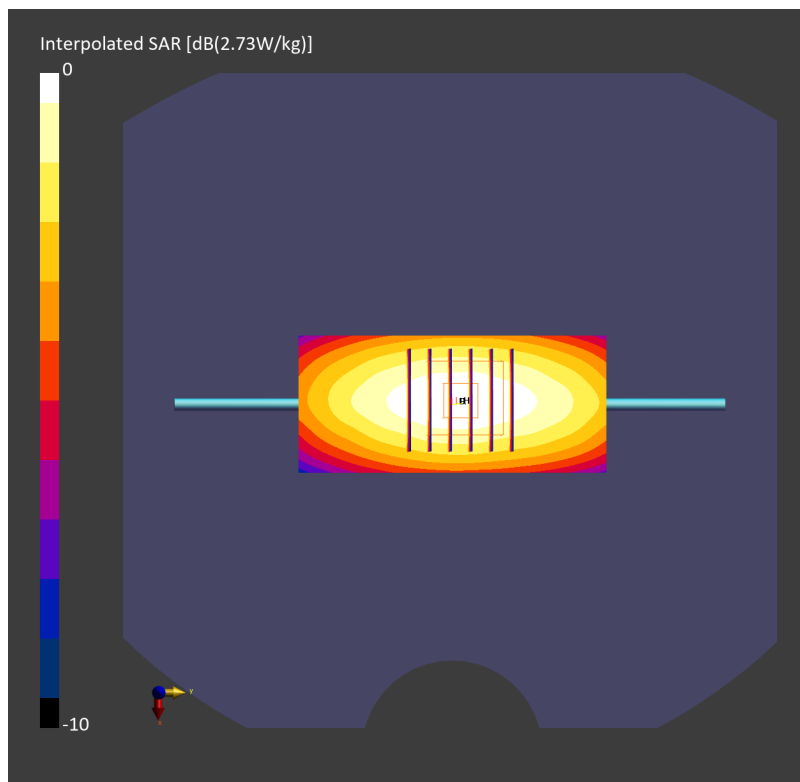

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260301 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.928$ S/m; $\epsilon_r = 44.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.36, 7.56, 9.63); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.30 W/kg; SAR (10g) = 1.52 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.32 W/kg; SAR (8g) = 1.65 W/kg; SAR (10g) = 1.57 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 89.6 %

TSL Correction: Positive only

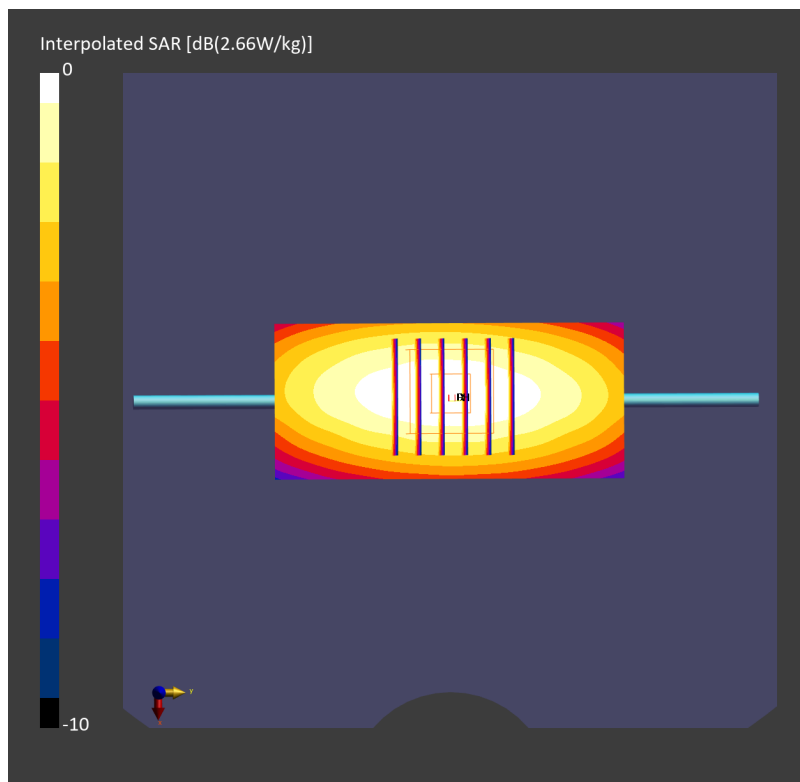

System Check_Head_835MHz

DUT: D835V2 - SN499

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260307 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.891$ S/m; $\epsilon_r = 45.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.56 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.39 W/kg; SAR (8g) = 1.64 W/kg; SAR (10g) = 1.56 W/kg

Smallest distance from peaks to all points 3 dB below = 15.6 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

TSL Correction: Positive only

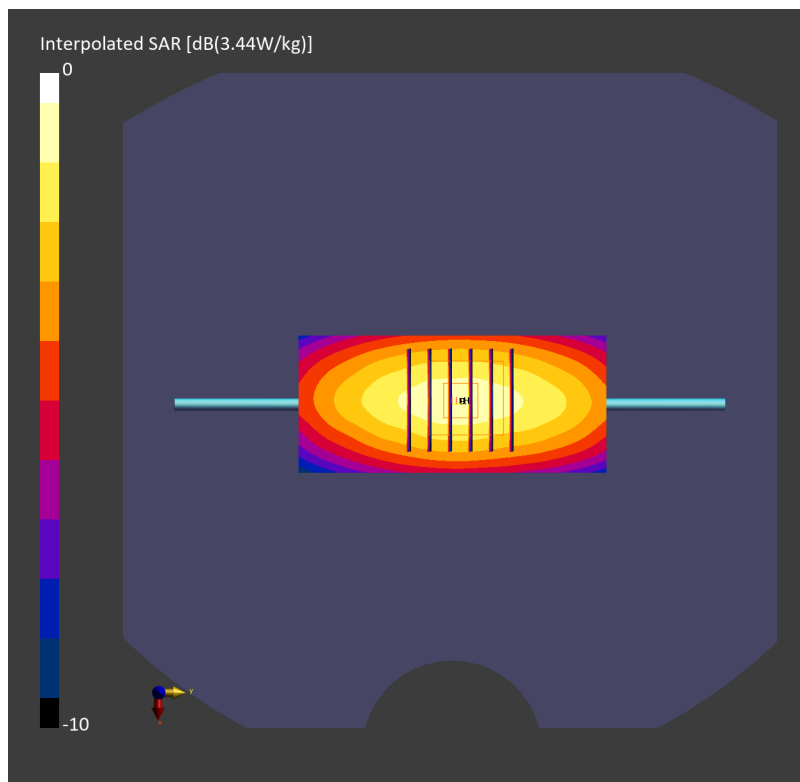

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260309 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.922$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(8.36, 7.56, 9.63); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.29 W/kg; SAR (10g) = 1.51 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.31 W/kg; SAR (8g) = 1.64 W/kg; SAR (10g) = 1.56 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 89.7 %

TSL Correction: Positive only

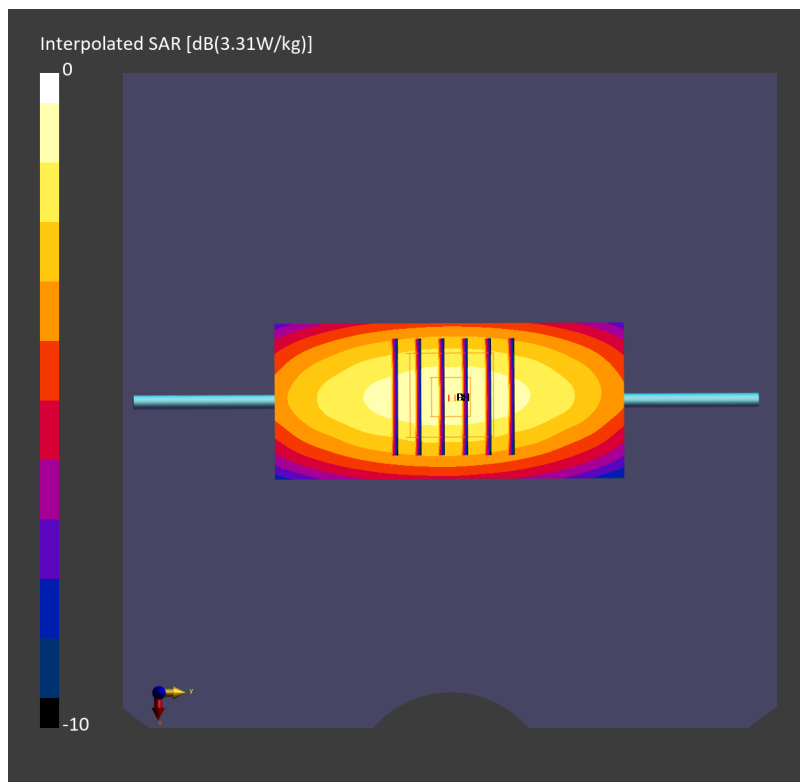

System Check_Head_835MHz

DUT: D835V2 - SN499

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260323 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.898$ S/m; $\epsilon_r = 44.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.52 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.32 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = 20.4 mm

Ratio of SAR at M2 to SAR at M1 = 89.2 %

TSL Correction: Positive only

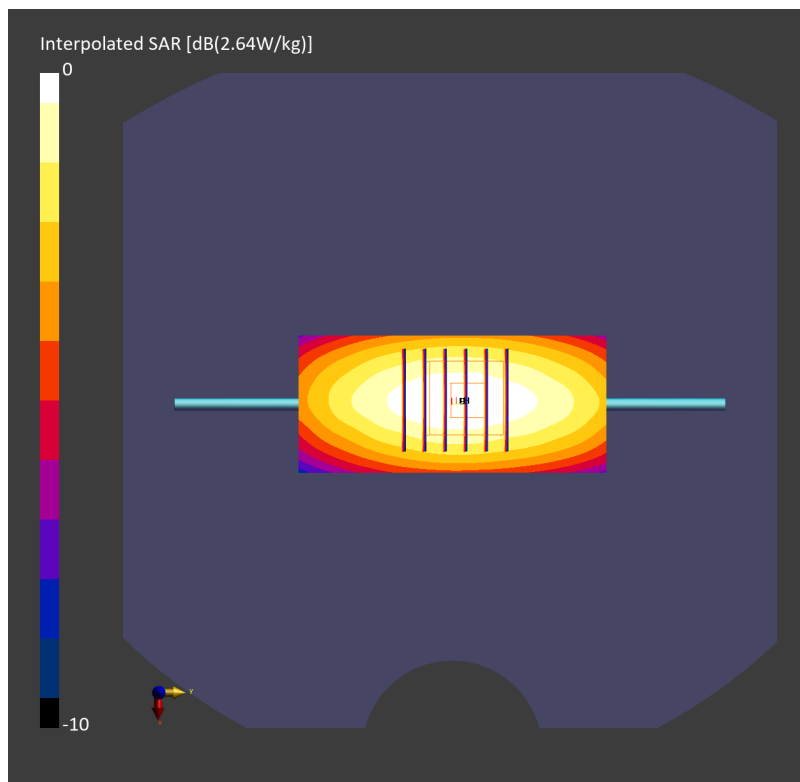

System Check_Head_835MHz

DUT: D835V2 - SN499

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260327 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.899$ S/m; $\epsilon_r = 44.2$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.98, 9.29, 9.07); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.31 W/kg; SAR (10g) = 1.51 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.31 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.51 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

TSL Correction: Positive only

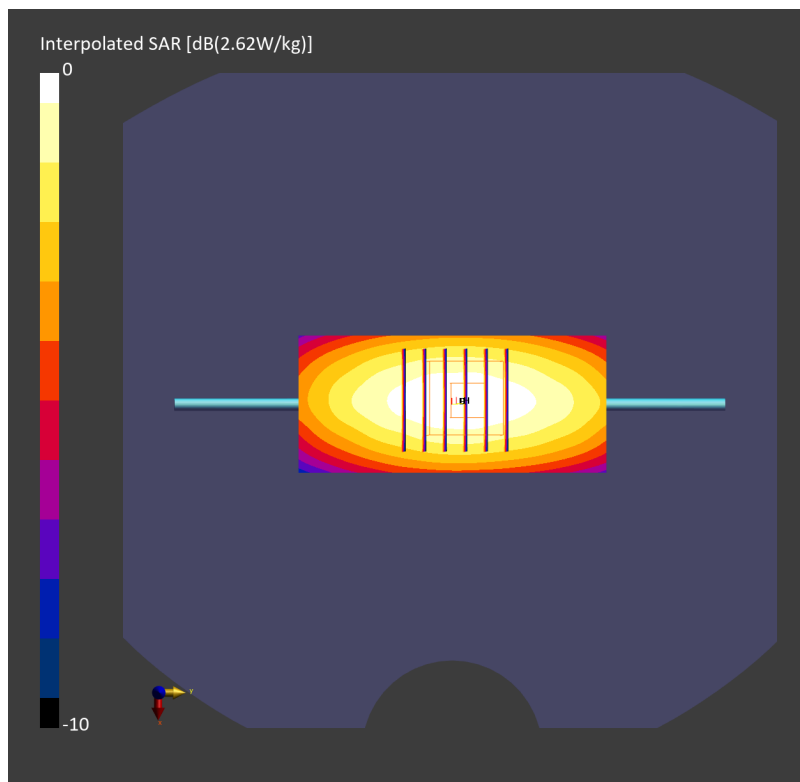

System Check_Head_835MHz

DUT: D835V2 - SN499

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260402 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.916$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(10.26, 9.98, 9.98); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.50 W/kg; SAR (10g) = 1.64 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.49 W/kg; SAR (8g) = 1.73 W/kg; SAR (10g) = 1.65 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

TSL Correction: Positive only

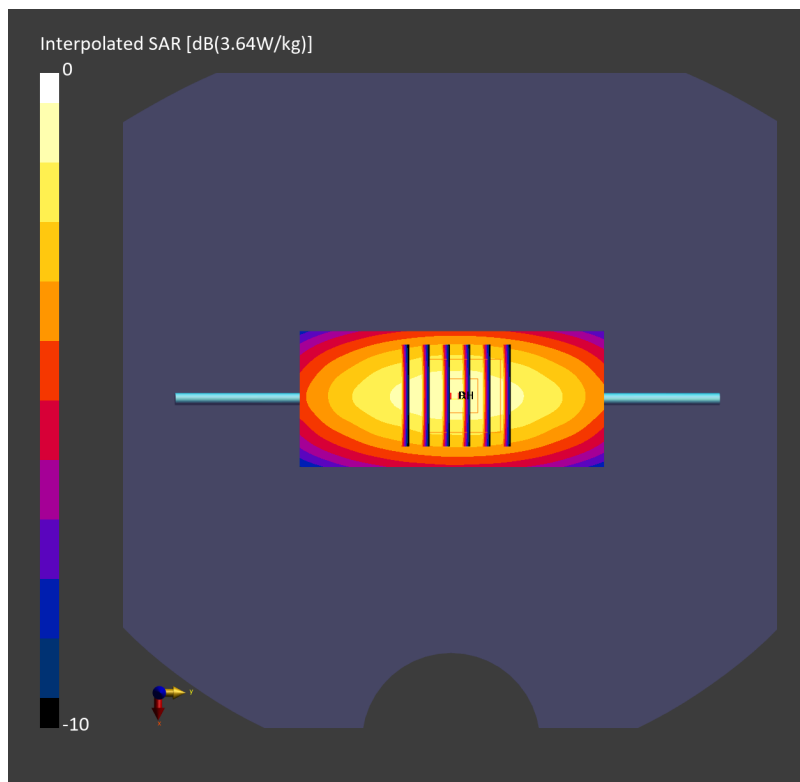

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260407 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.912$ S/m; $\epsilon_r = 43.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(10.26, 9.98, 9.98); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.34 W/kg; SAR (10g) = 1.53 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 2.34 W/kg; SAR (8g) = 1.67 W/kg; SAR (10g) = 1.59 W/kg

Smallest distance from peaks to all points 3 dB below = 16.6 mm

Ratio of SAR at M2 to SAR at M1 = 87.2 %

TSL Correction: Positive only

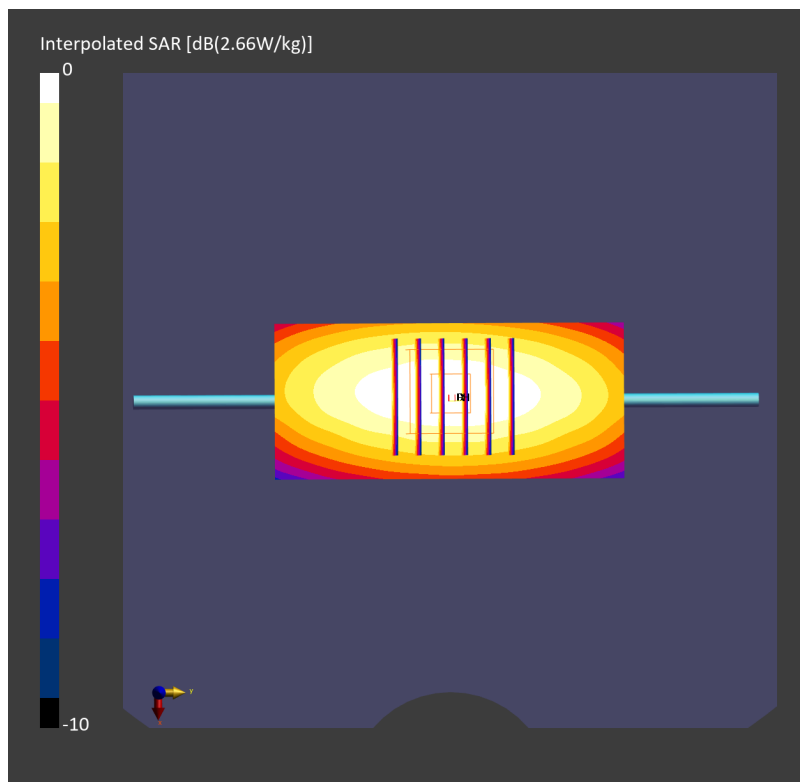

System Check_Head_1640MHz

DUT: D1640V2 - SN346

Communication System: CW; Frequency: 1640.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 1640.000$ MHz; $\sigma = 1.29$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(7.34, 7.33, 7.0); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.74 W/kg; SAR (10g) = 0.940 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.72 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.936 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

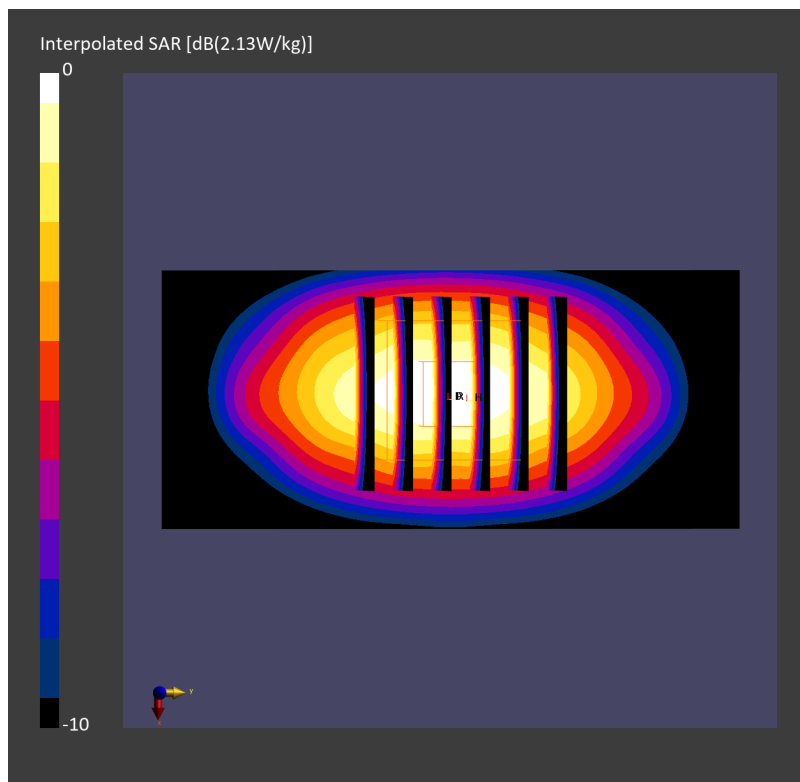

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260219 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 0.980 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.85 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.986 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.7 %

TSL Correction: Positive only

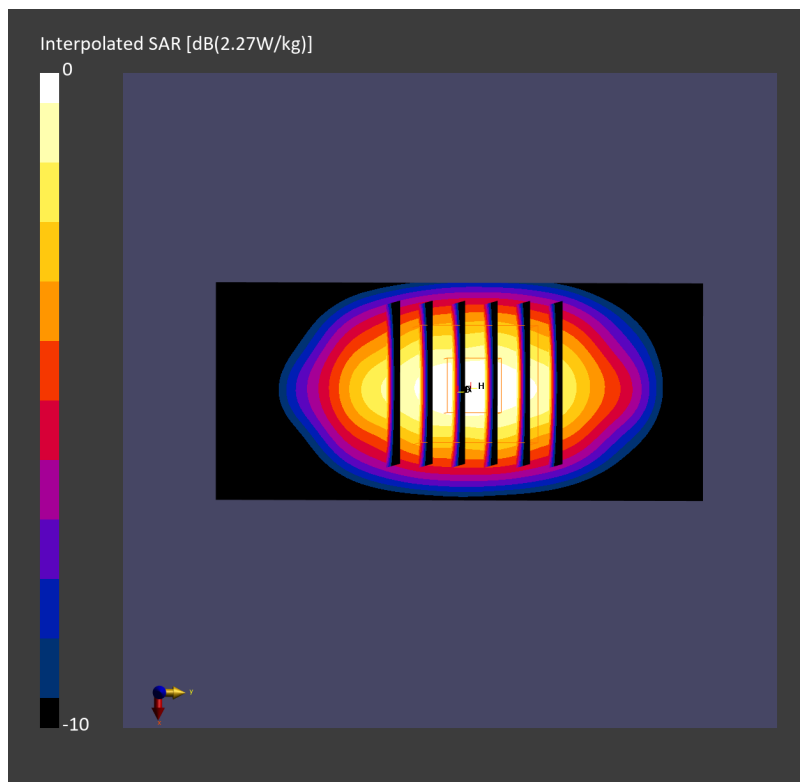

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260226 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.85 W/kg; SAR (10g) = 0.979 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.84 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.984 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.8 %

TSL Correction: Positive only

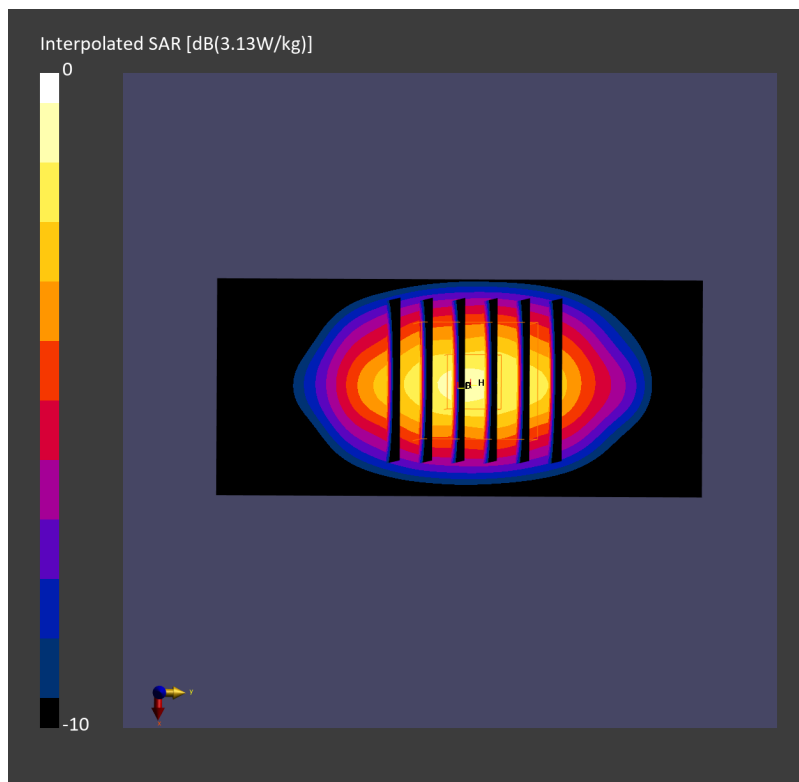

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260301 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.87 W/kg; SAR (10g) = 0.987 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.86 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.994 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

TSL Correction: Positive only

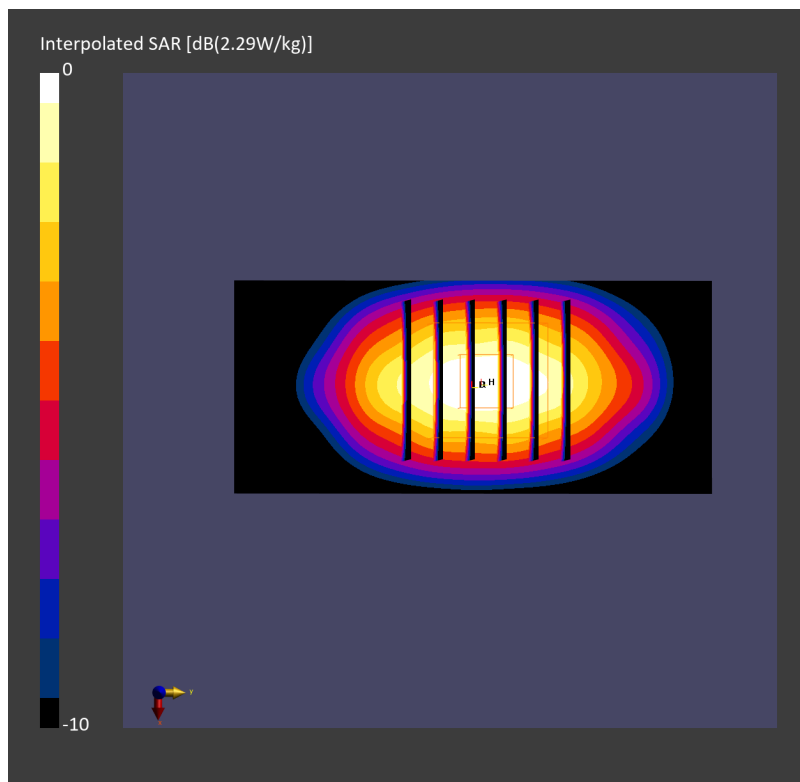

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260304 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.53, 6.81, 8.67); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.957 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 1.81 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 86.7 %

TSL Correction: Positive only

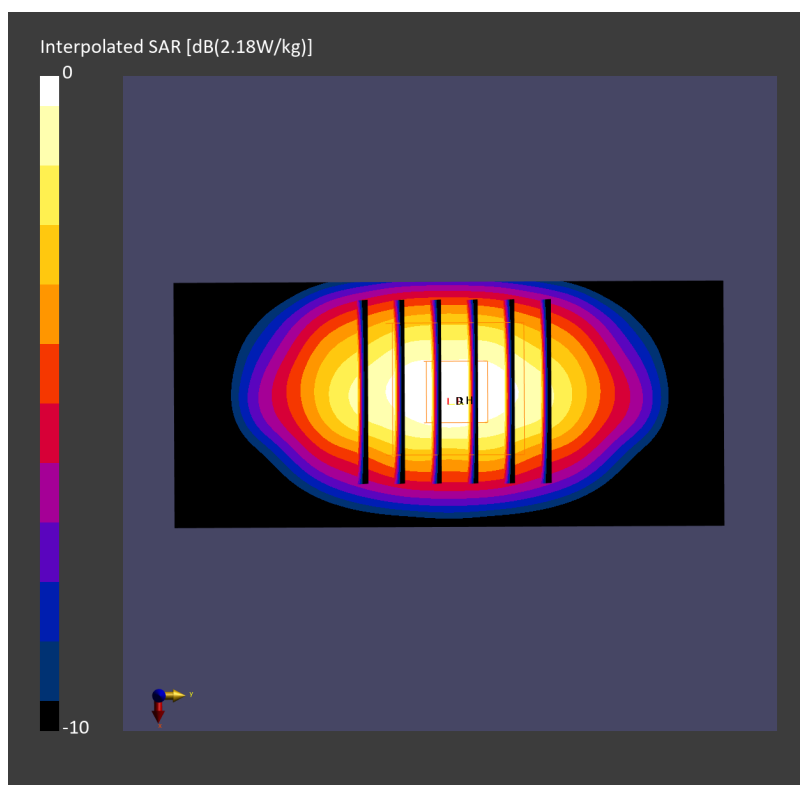

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260311 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.85 W/kg; SAR (10g) = 0.980 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 1.83 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.979 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

TSL Correction: Positive only

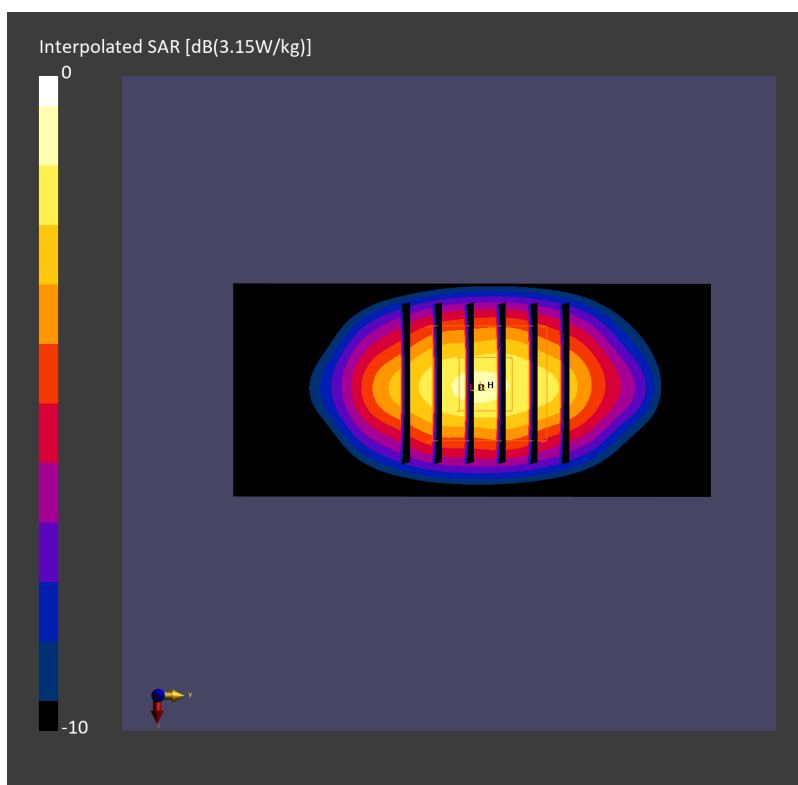

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260312 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.53, 6.81, 8.67); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.74 W/kg; SAR (10g) = 0.949 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.79 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.987 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 86.1 %

TSL Correction: Positive only

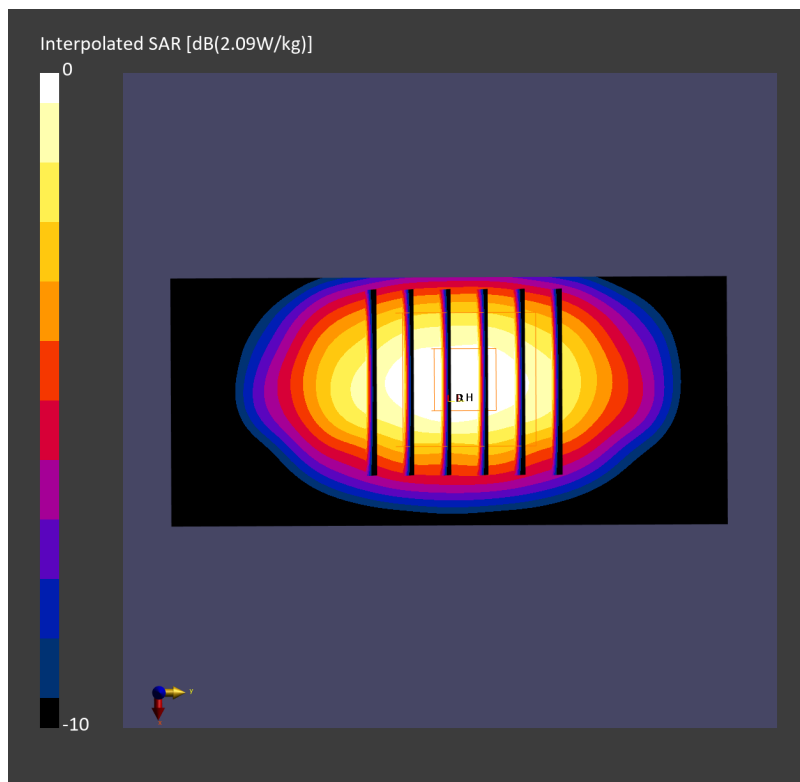

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260329 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.996 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.84 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.986 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.4 %

TSL Correction: Positive only

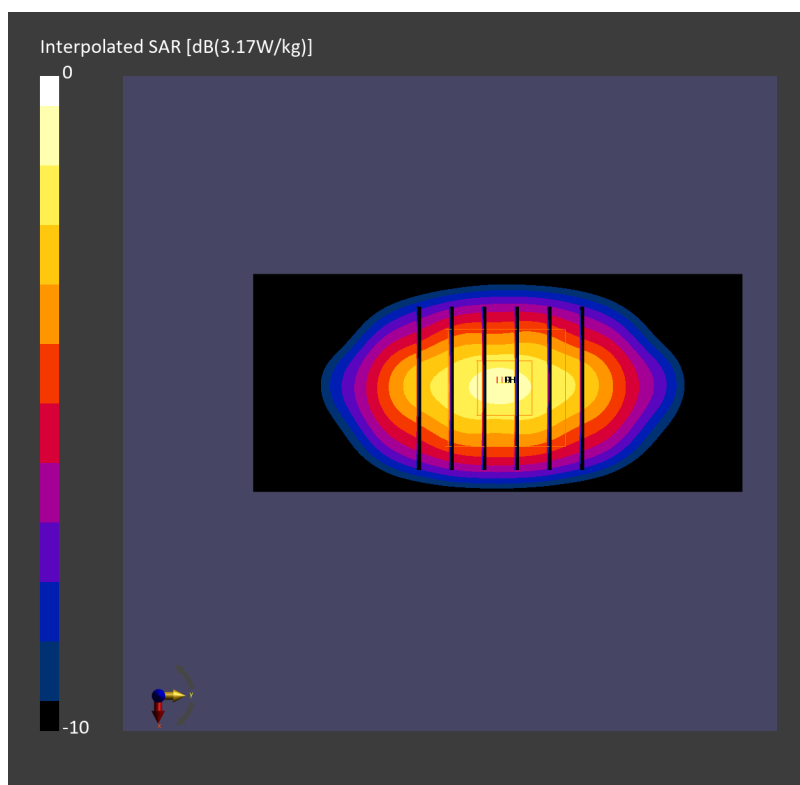

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260402 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.5, 7.76, 7.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.998 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.85 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.988 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: Positive only

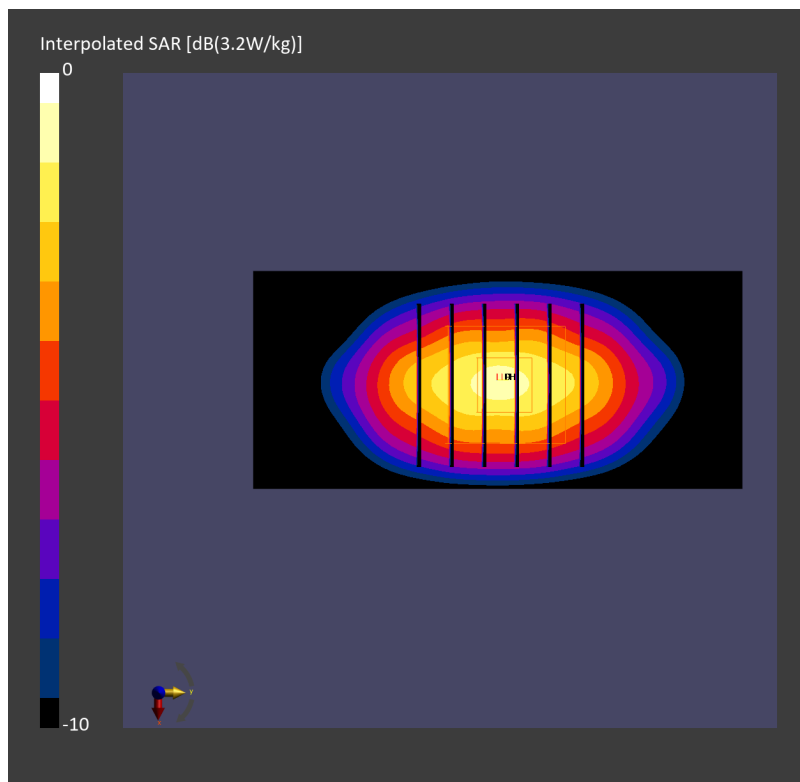

System Check_Head_1750MHz

DUT: D1750V2 - SN1120

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260404 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(8.44, 8.22, 8.21); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.62 W/kg; SAR (10g) = 0.870 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.07 dB

SAR (1g) = 1.67 W/kg; SAR (8g) = 0.964 W/kg; SAR (10g) = 0.889 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

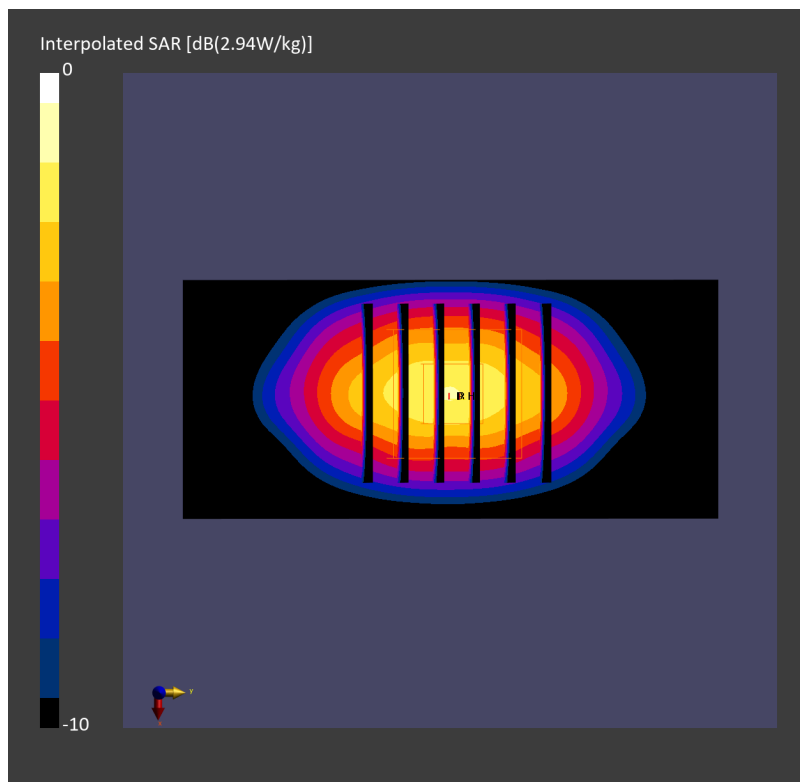

System Check_Head_1750MHz

DUT: D1750V2 - SN1120

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260408 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(8.44, 8.22, 8.21); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.62 W/kg; SAR (10g) = 0.870 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.05 dB

SAR (1g) = 1.69 W/kg; SAR (8g) = 0.983 W/kg; SAR (10g) = 0.907 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

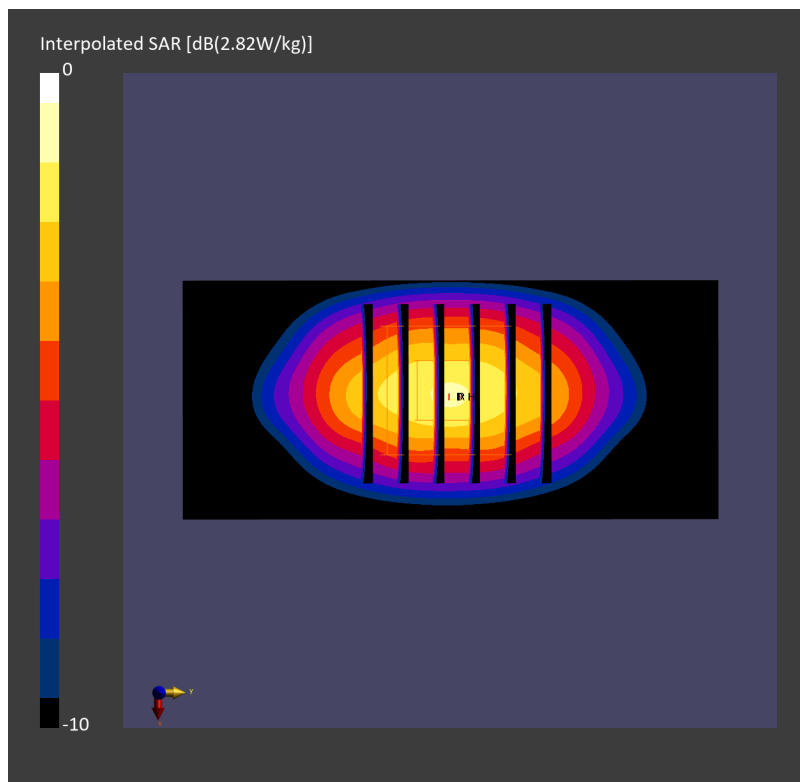

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260218 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 0.982 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.89 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.989 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

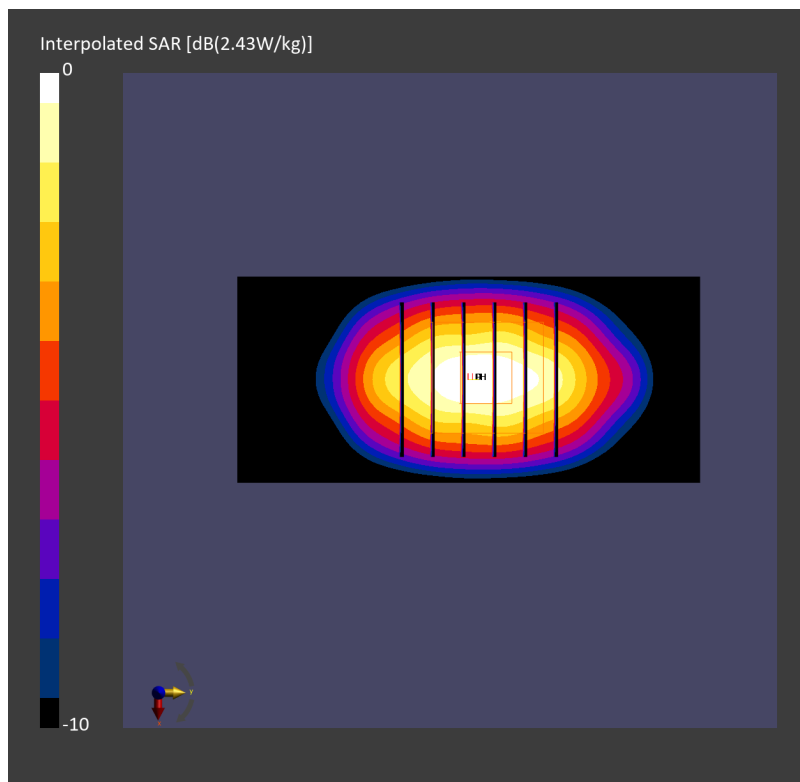

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260225 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.96 W/kg; SAR (10g) = 0.998 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 87.5 %

TSL Correction: Positive only

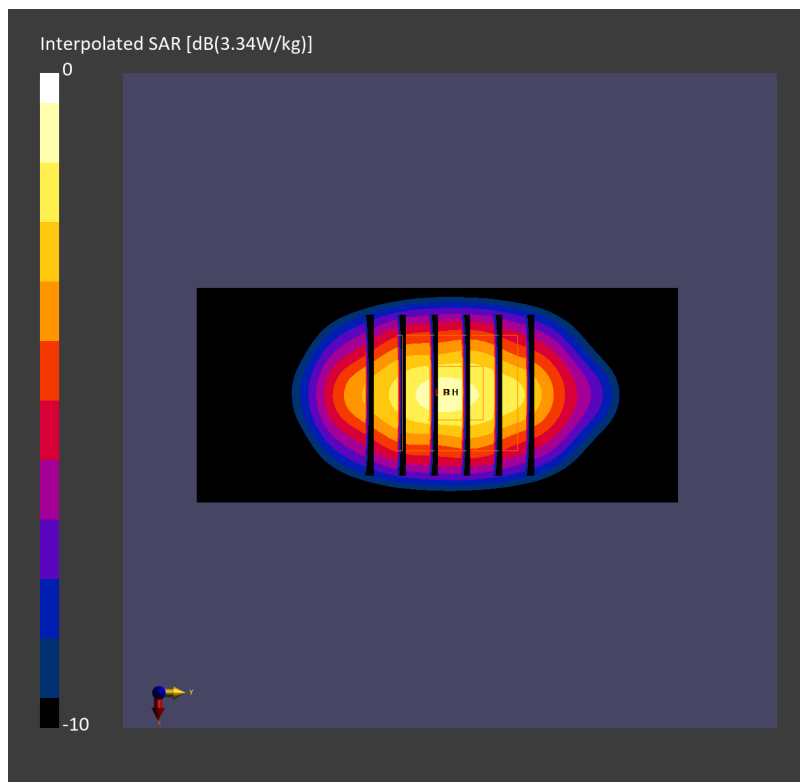

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260302 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.99 W/kg; SAR (10g) = 1.02 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.95 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 87.6 %

TSL Correction: Positive only

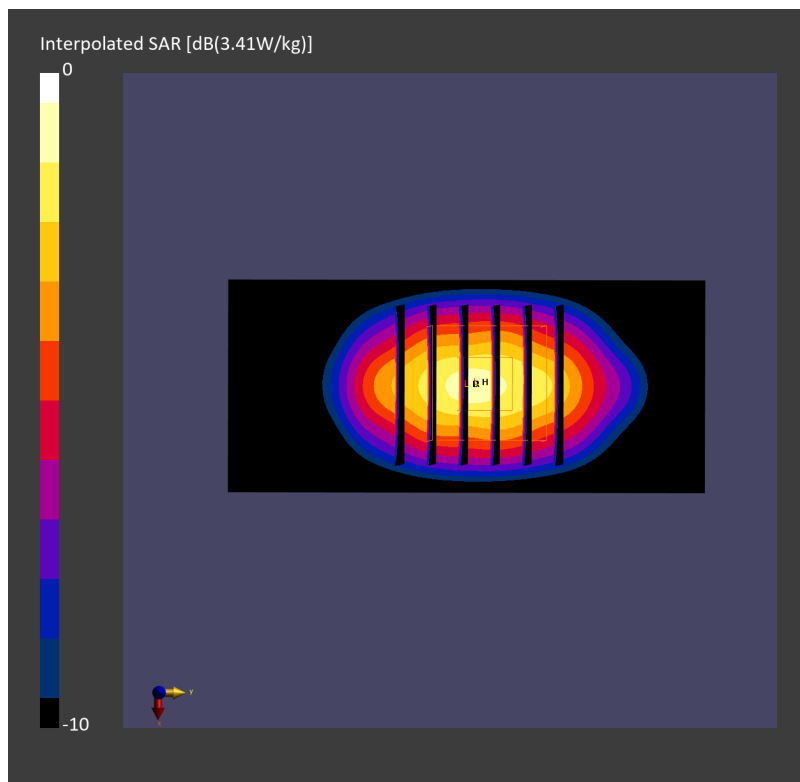

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260303 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 42.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.22, 6.53, 8.31); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.11 W/kg; SAR (10g) = 1.10 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.16 dB

SAR (1g) = 2.05 W/kg; SAR (8g) = 1.20 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 86.5 %

TSL Correction: Positive only

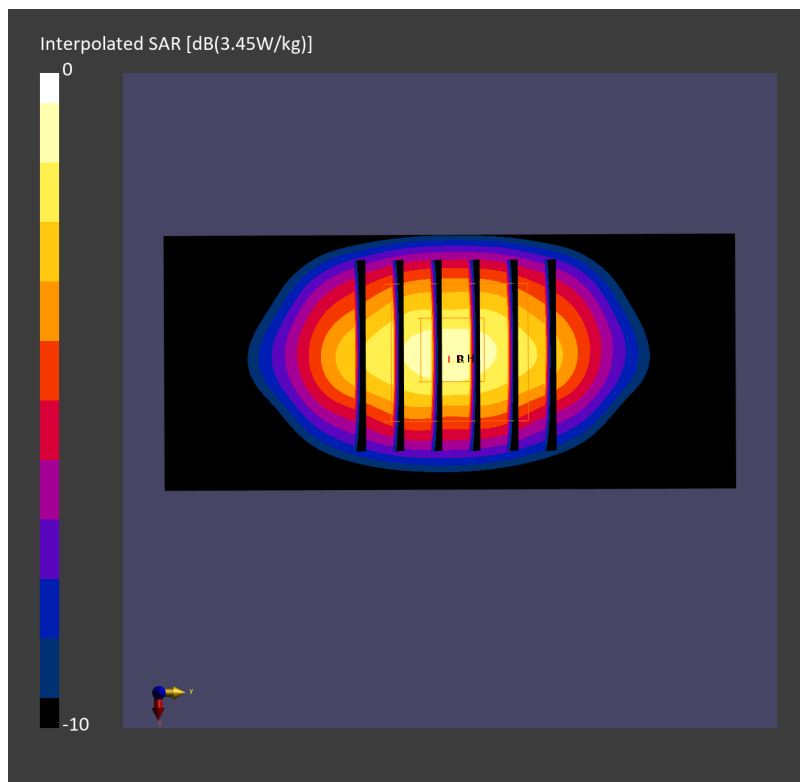

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260311 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.22, 6.53, 8.31); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.96 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 86.5 %

TSL Correction: Positive only

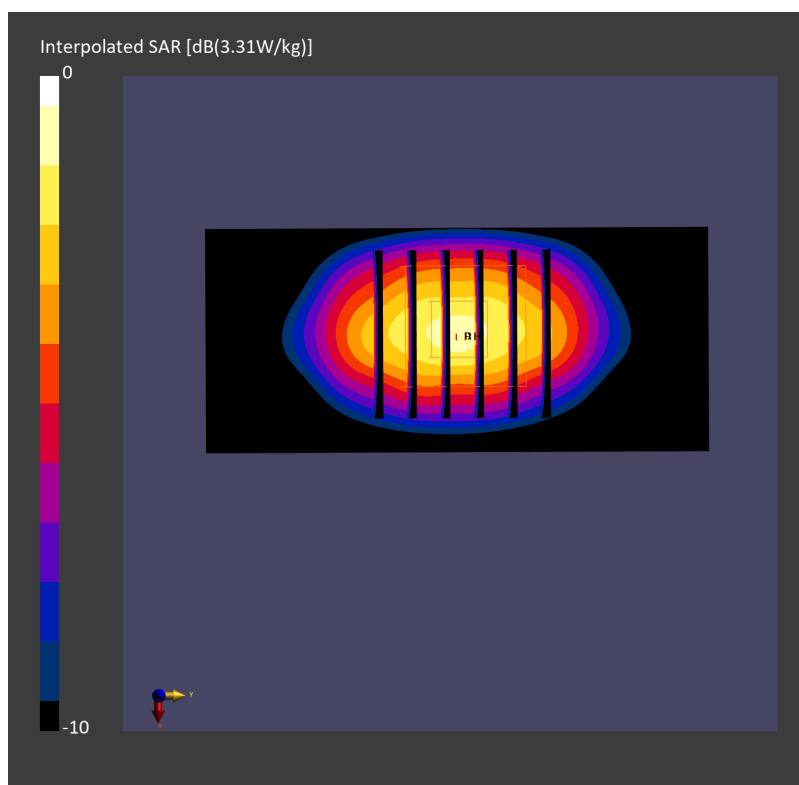

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260312 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.99 W/kg; SAR (10g) = 1.02 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.96 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

TSL Correction: Positive only

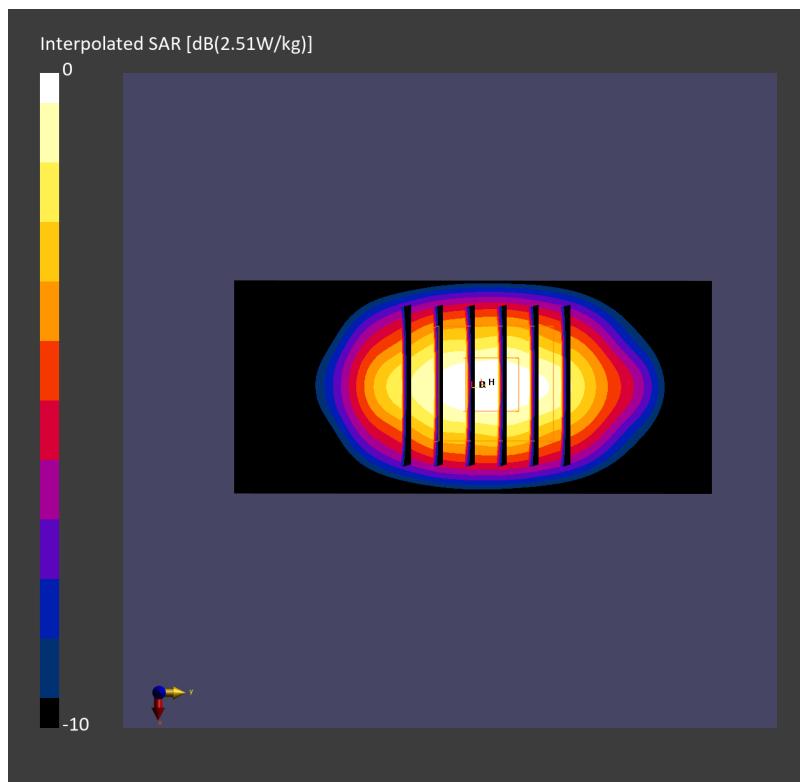

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260326 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.05 W/kg; SAR (10g) = 1.05 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.02 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.2 %

TSL Correction: Positive only

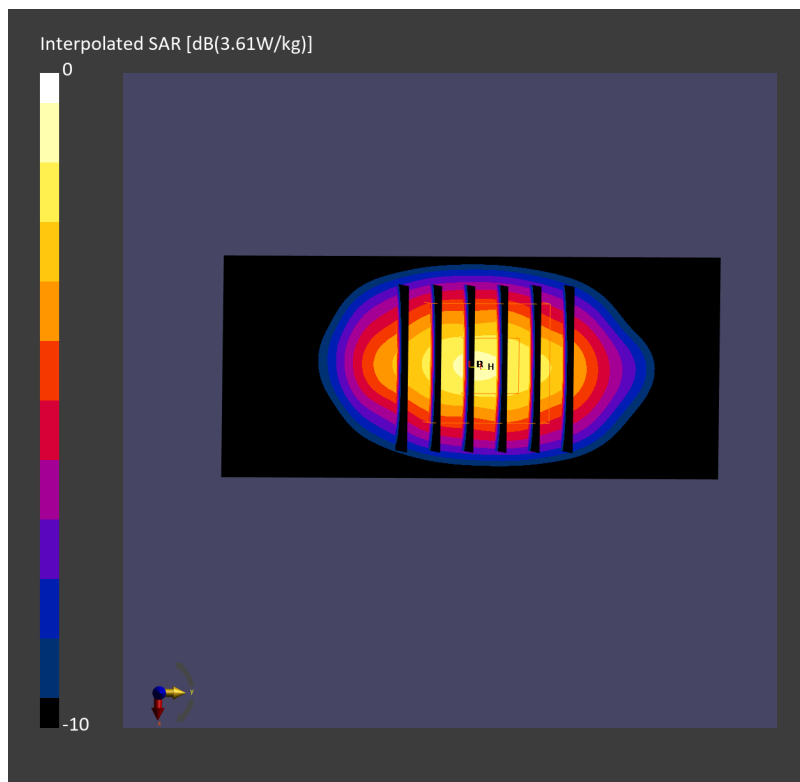

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260401 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.27, 7.52, 7.34); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.05 W/kg; SAR (10g) = 1.06 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.02 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

TSL Correction: Positive only

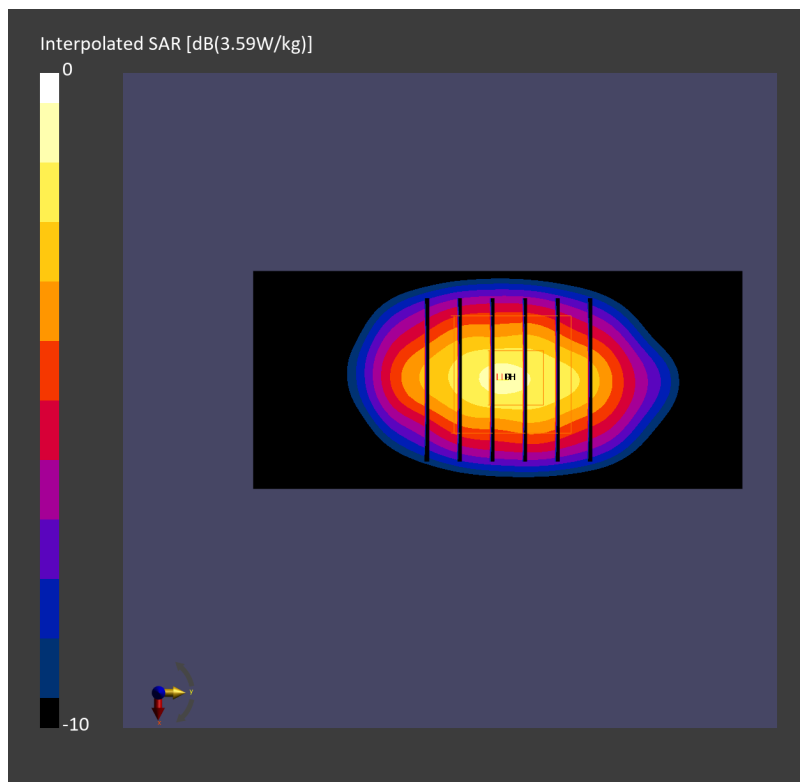

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260404 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.99, 7.78, 7.77); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.87 W/kg; SAR (10g) = 0.971 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.09 dB

SAR (1g) = 1.86 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.967 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

TSL Correction: Positive only

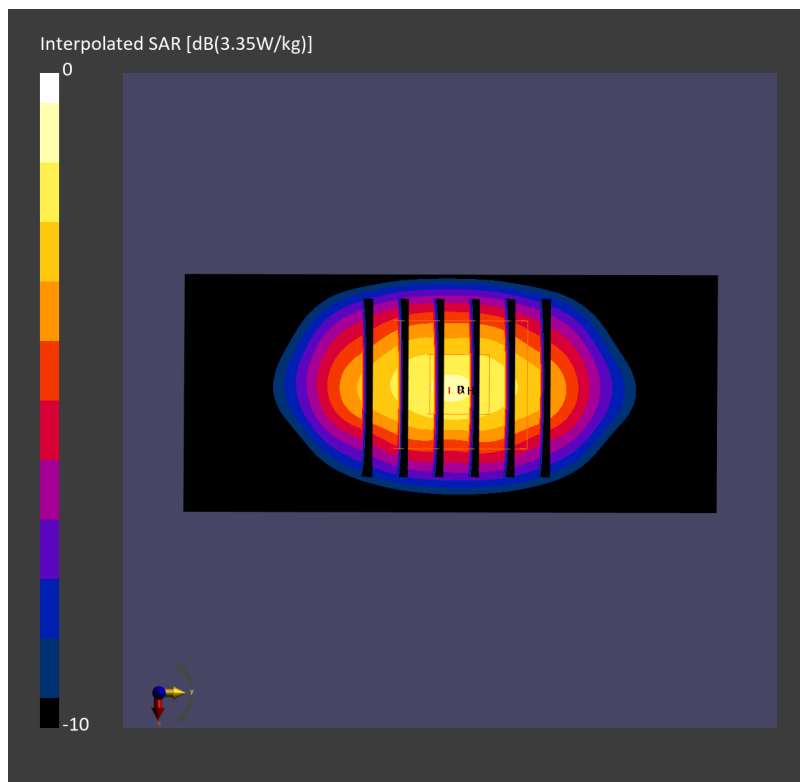

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260408 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.99, 7.78, 7.77); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.87 W/kg; SAR (10g) = 0.967 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.04 dB

SAR (1g) = 1.83 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.953 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: Positive only

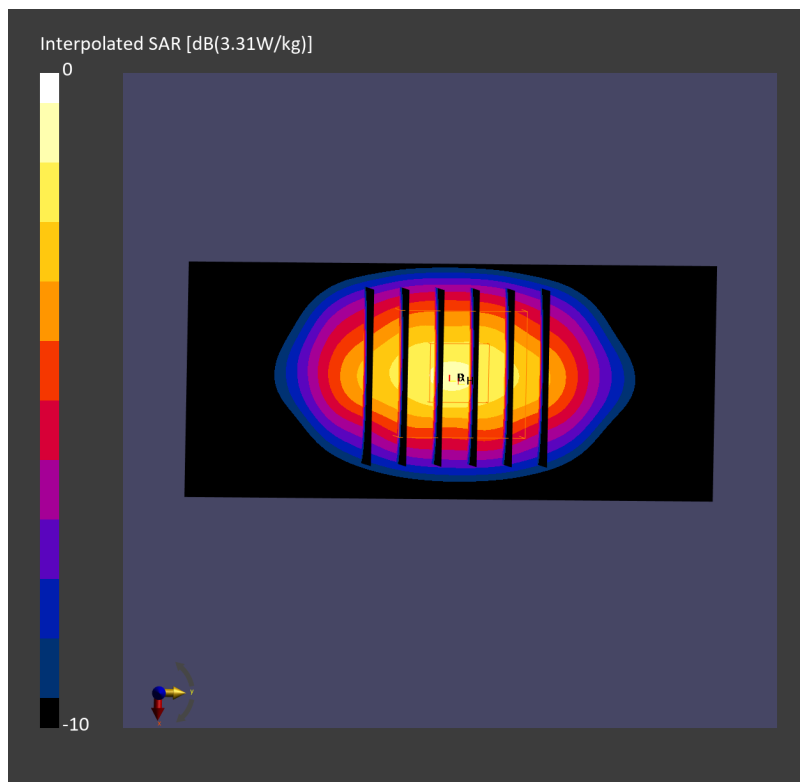

System Check_Head_2000MHz

DUT: D2000V2 - SN1070

Communication System: CW; Frequency: 2000.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 2000.000$ MHz; $\sigma = 1.53$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.89, 7.68, 7.67); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 1.92 W/kg; SAR (10g) = 0.974 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.11 dB

SAR (1g) = 1.96 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.989 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

TSL Correction: Positive only

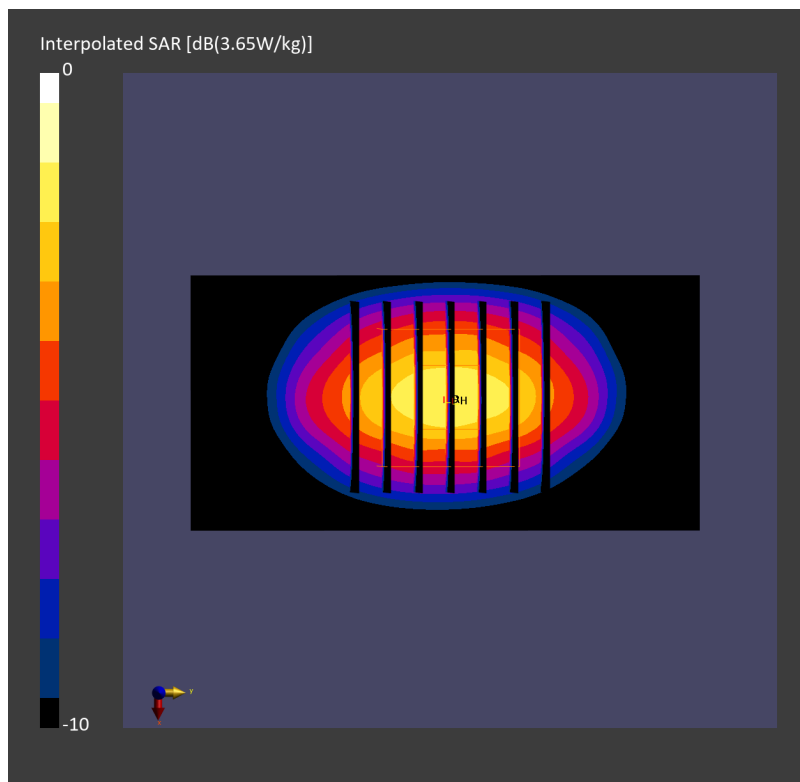

System Check_Head_2300MHz

DUT: D2300V2 - SN1088

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260220 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.74$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.78, 7.02, 6.85); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.12 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.04 dB

SAR (1g) = 2.36 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 83.4 %

TSL Correction: Positive only

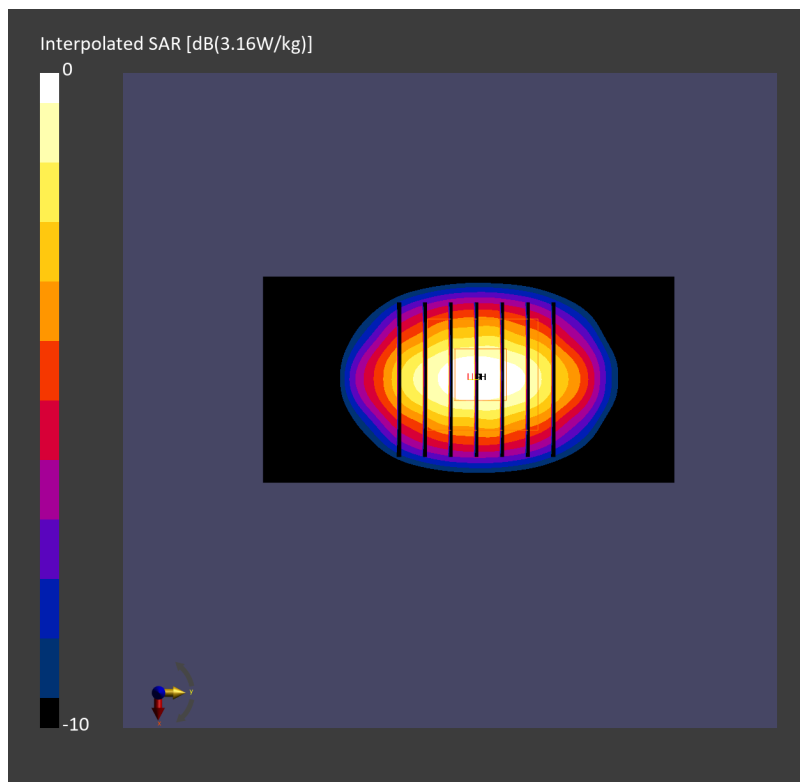

System Check_Head_2300MHz

DUT: D2300V2 - SN1088

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260305 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.74$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.95, 6.29, 8.0); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

TSL Correction: Positive only

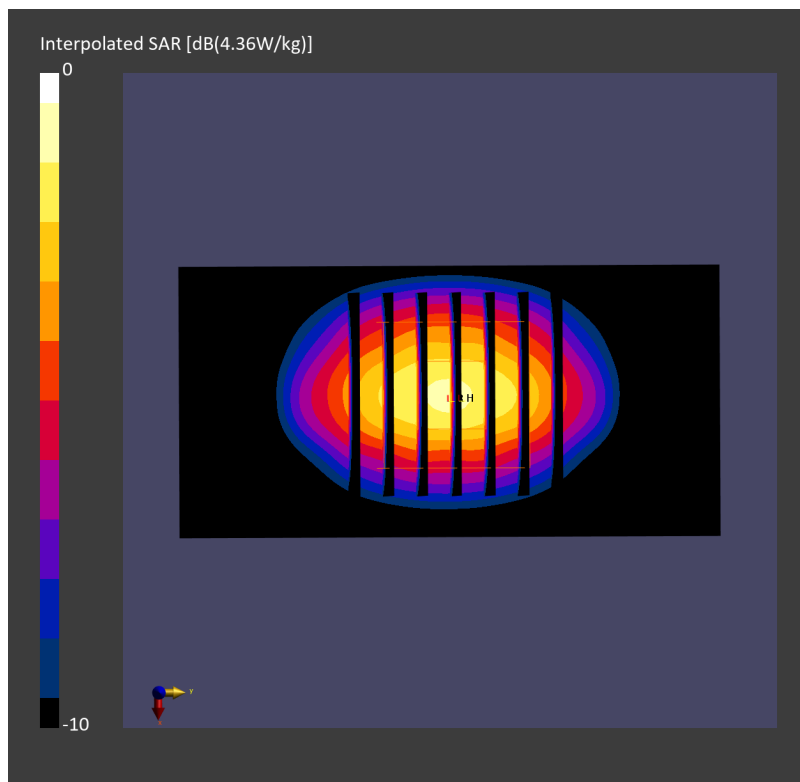

System Check_Head_2300MHz

DUT: D2300V2 - SN1088

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260308 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.75$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.78, 7.02, 6.85); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.12 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 2.37 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 83.7 %

TSL Correction: Positive only

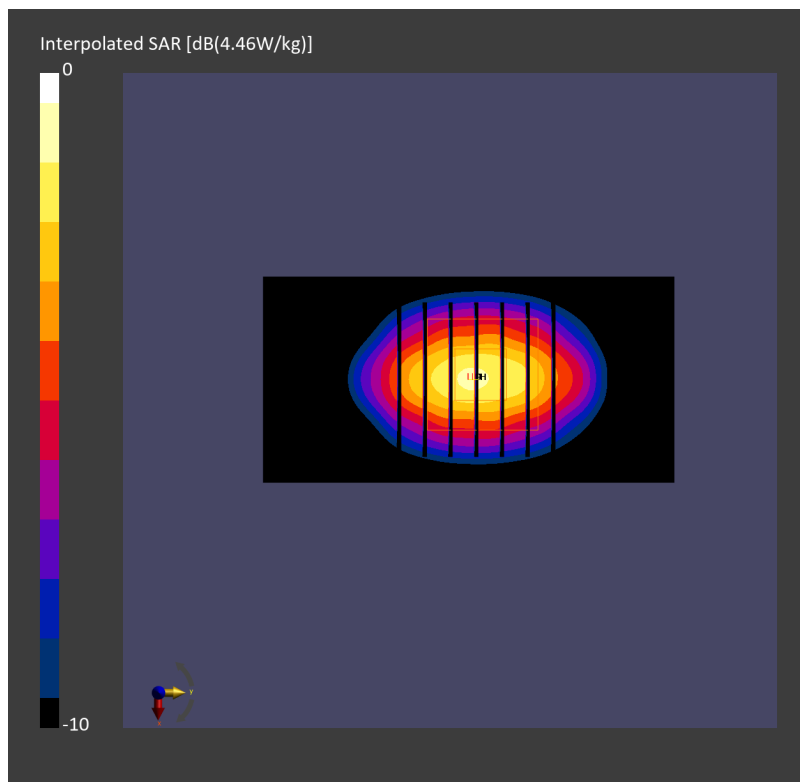

System Check_Head_2300MHz

DUT: D2300V2 - SN1088

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260328 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.74$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.78, 7.02, 6.85); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.51 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 82.4 %

TSL Correction: Positive only

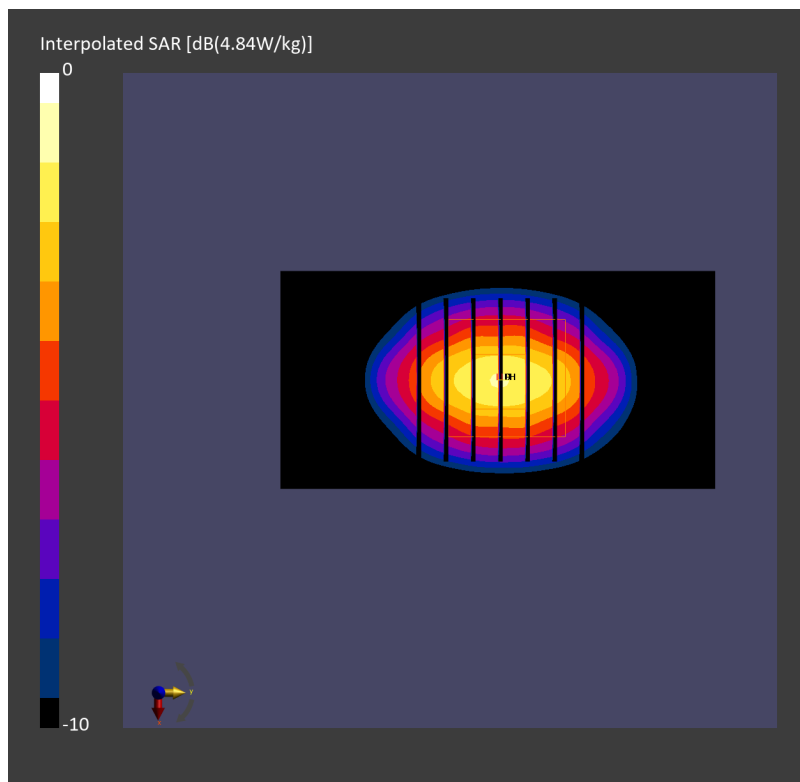

System Check_Head_2300MHz

DUT: D2300V2 - SN1088

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260405 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.75$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.57, 7.36, 7.36); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.45 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.42 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.3 %

TSL Correction: Positive only

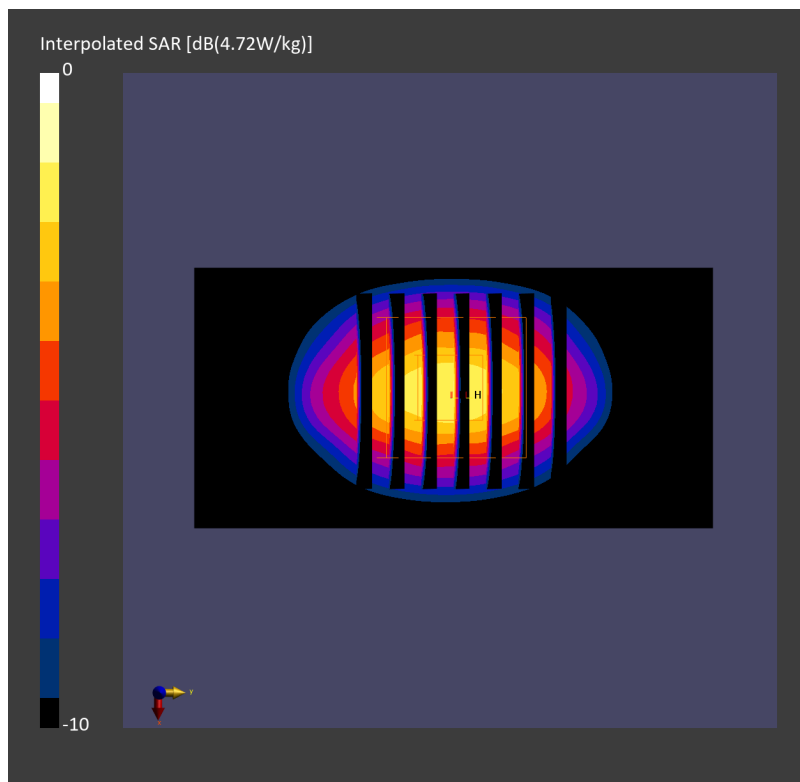

System Check_Head_2300MHz

DUT: D2300V2 - SN1088

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260407 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.73$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.57, 7.36, 7.36); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

TSL Correction: Positive only

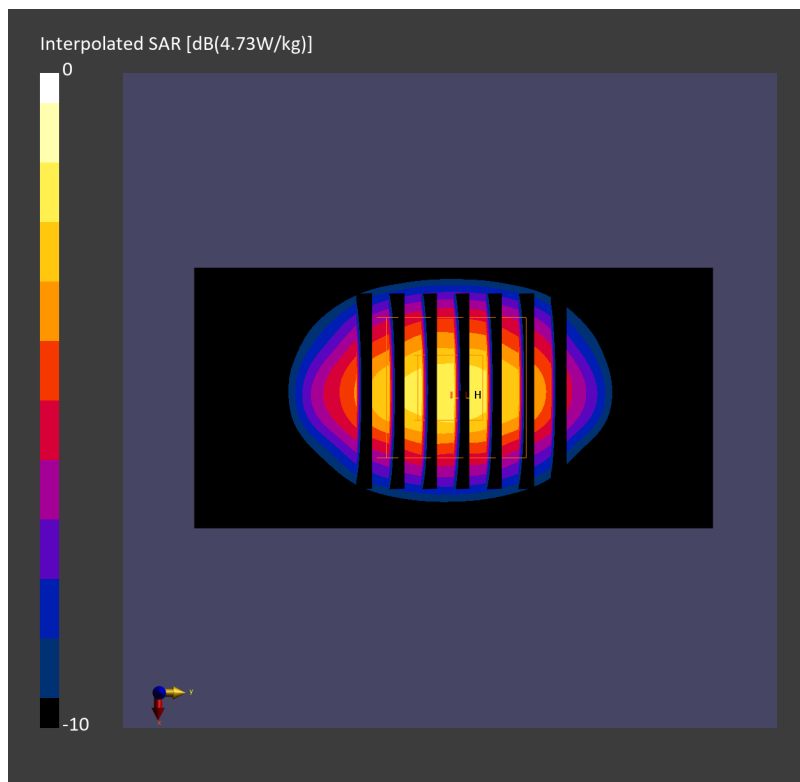

System Check_Head_2450MHz

DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260322 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.80$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.04, 6.37, 8.1); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.44 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 2.50 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.7 %

TSL Correction: Positive only

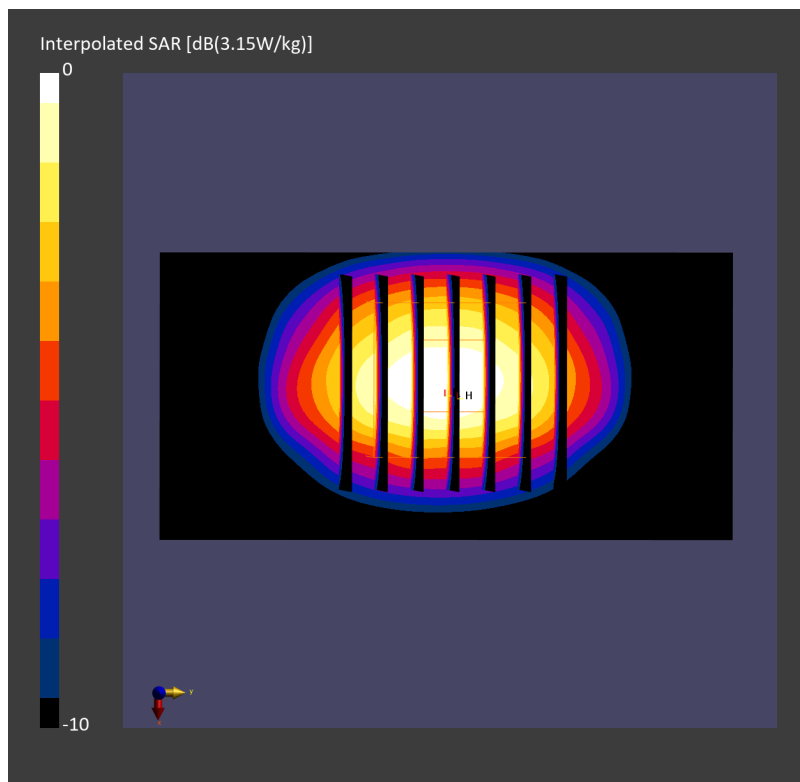

System Check_Head_2450MHz

DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260323 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.64$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.04, 6.37, 8.1); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.49 W/kg; SAR (10g) = 1.13 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.52 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: Positive only

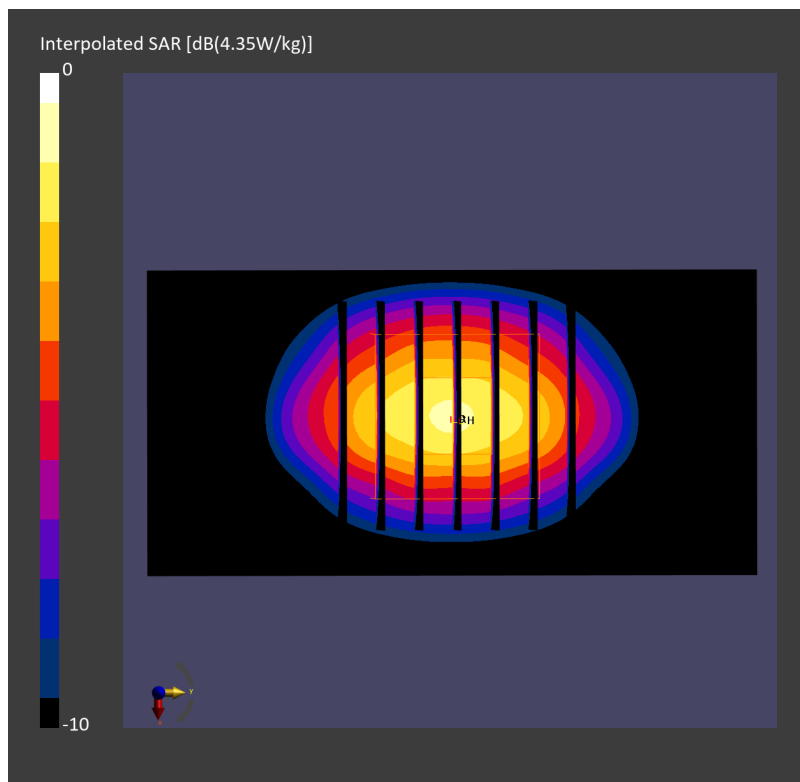

System Check_Head_2450MHz

DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260328 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.28, 7.08, 7.07); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.05 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

TSL Correction: Positive only

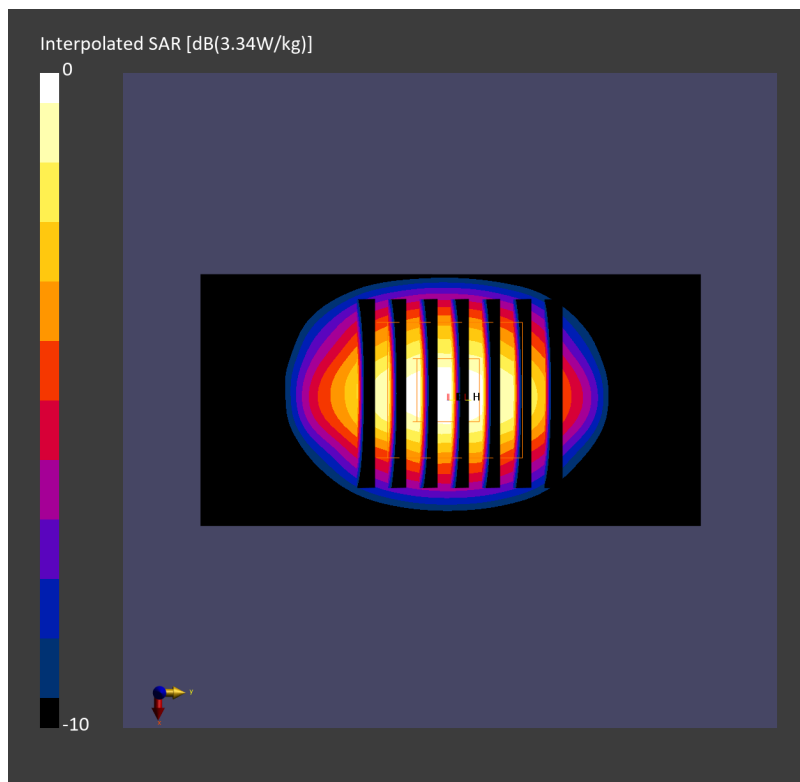

System Check_Head_2450MHz

DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260328 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.04, 6.37, 8.1); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.5 W/kg; SAR (10g) = 6.29 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 13.6 W/kg; SAR (8g) = 7.32 W/kg; SAR (10g) = 6.68 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.1 %

TSL Correction: Positive only

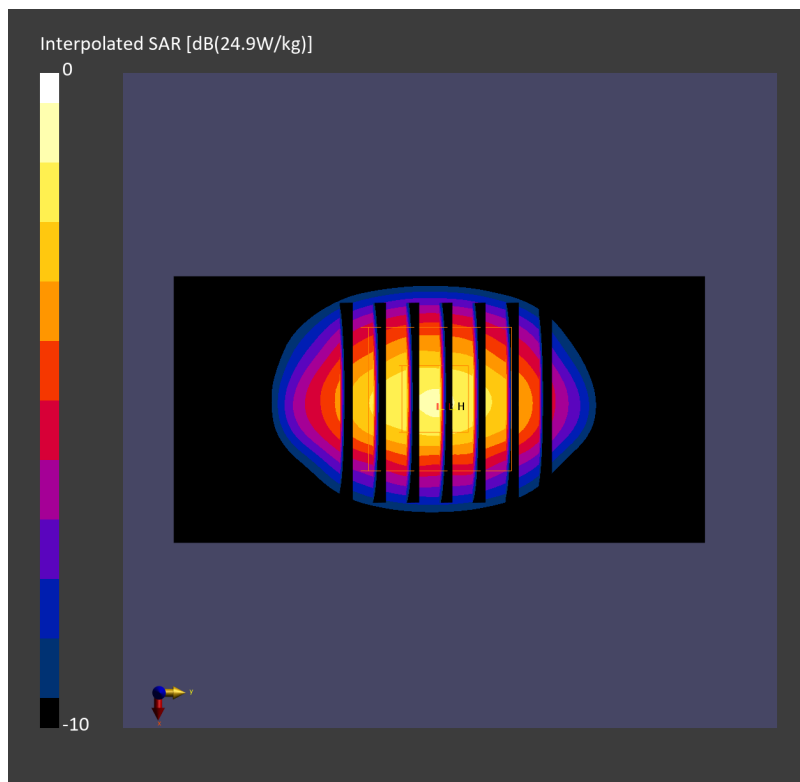

System Check_Head_2450MHz

DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260331 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.63$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.04, 6.37, 8.1); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 2.69 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

TSL Correction: Positive only

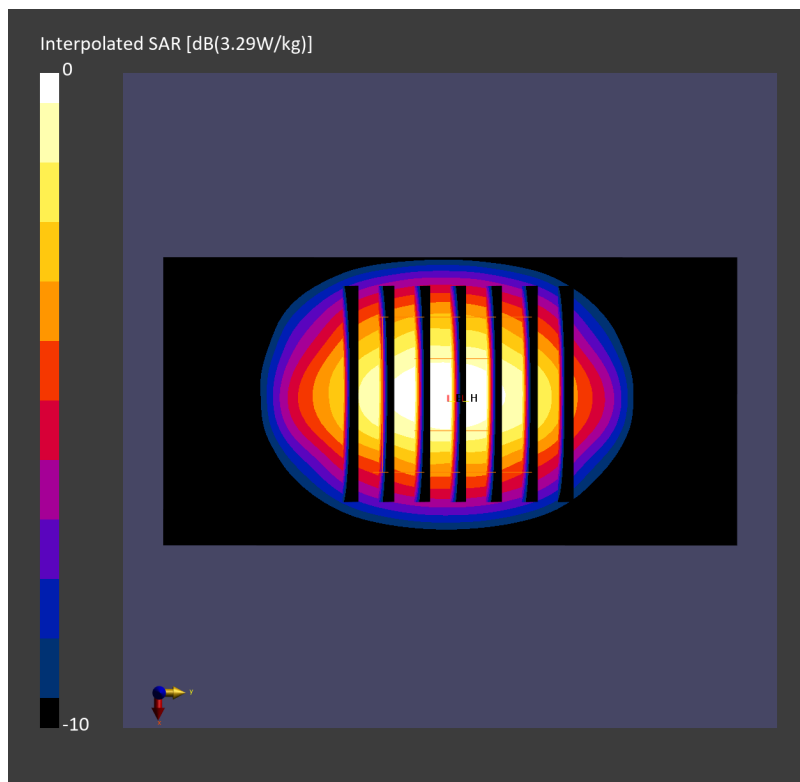

System Check_Head_2450MHz

DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260331 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.63$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.28, 7.08, 7.07); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.56 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.54 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.3 %

TSL Correction: Positive only

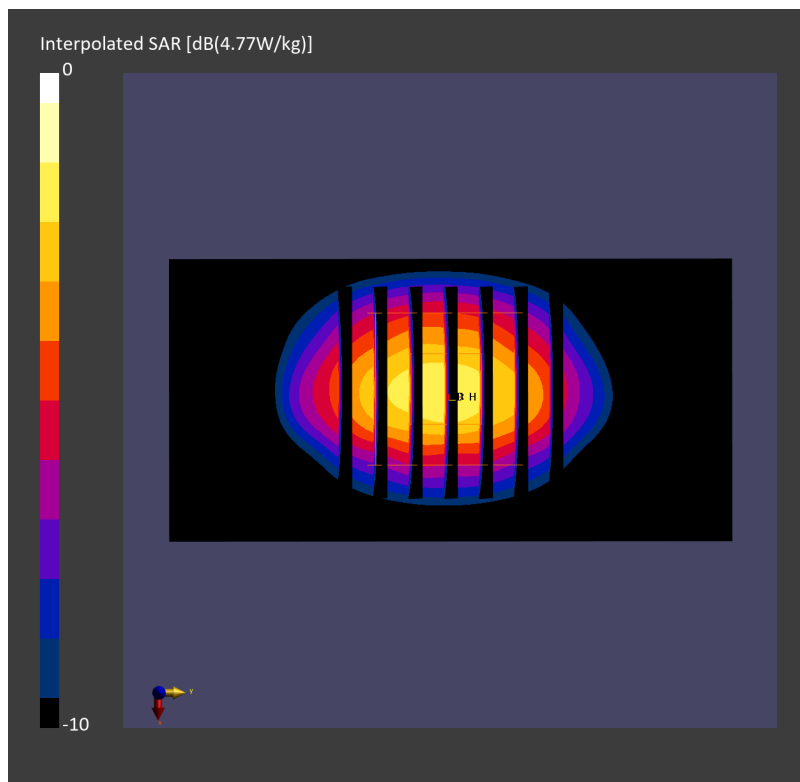

System Check_Head_2450MHz

DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260402 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.86$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.04, 6.37, 8.1); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.25 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 2.71 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.1 %

TSL Correction: Positive only

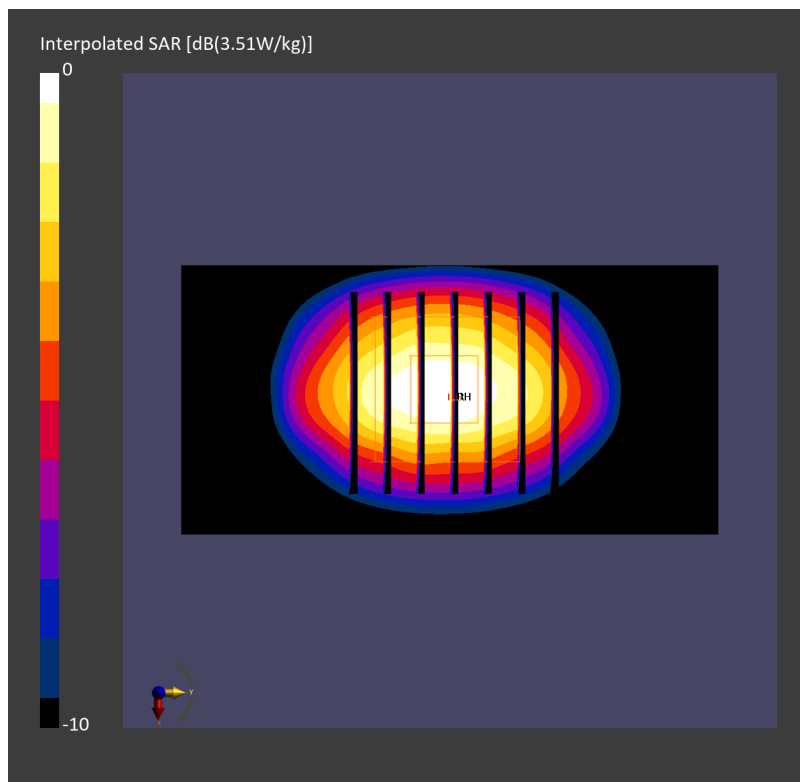

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260221 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.59 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.58 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 80.1 %

TSL Correction: Positive only

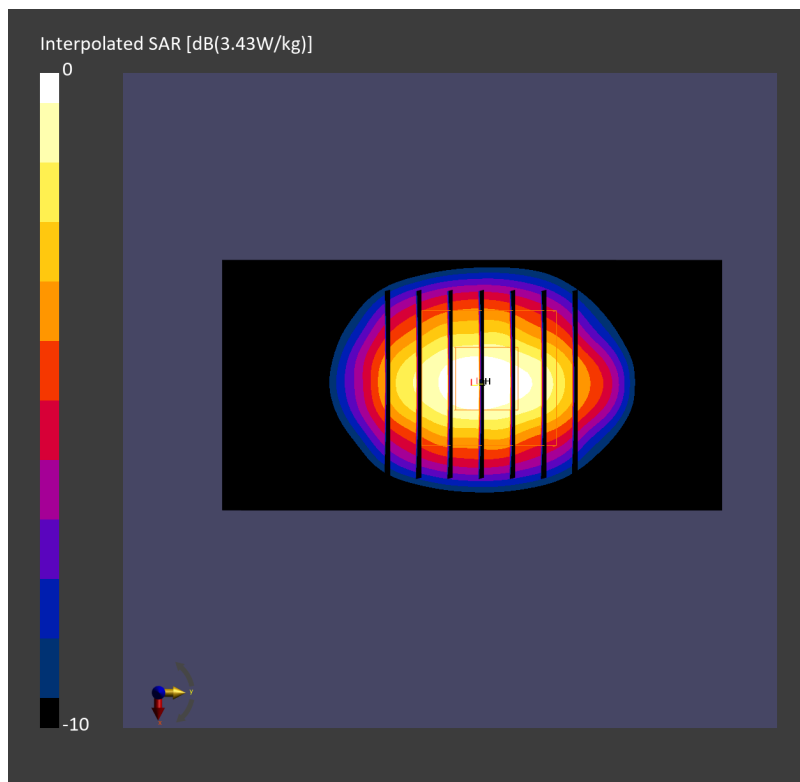

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260223 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.85 W/kg; SAR (10g) = 1.27 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.83 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.6 %

TSL Correction: Positive only

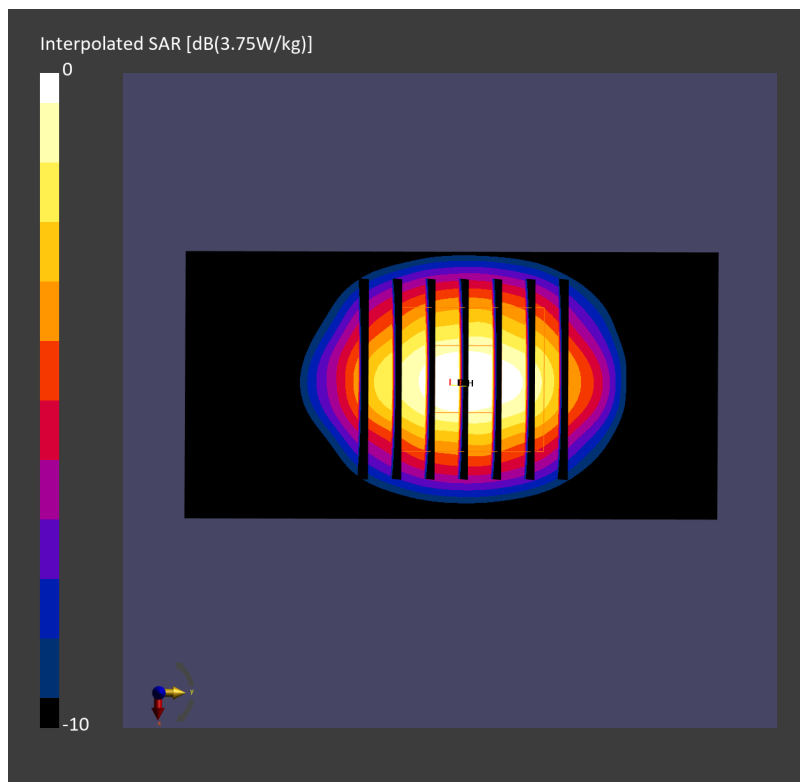

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260303 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.88 W/kg; SAR (10g) = 1.29 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.88 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

TSL Correction: Positive only

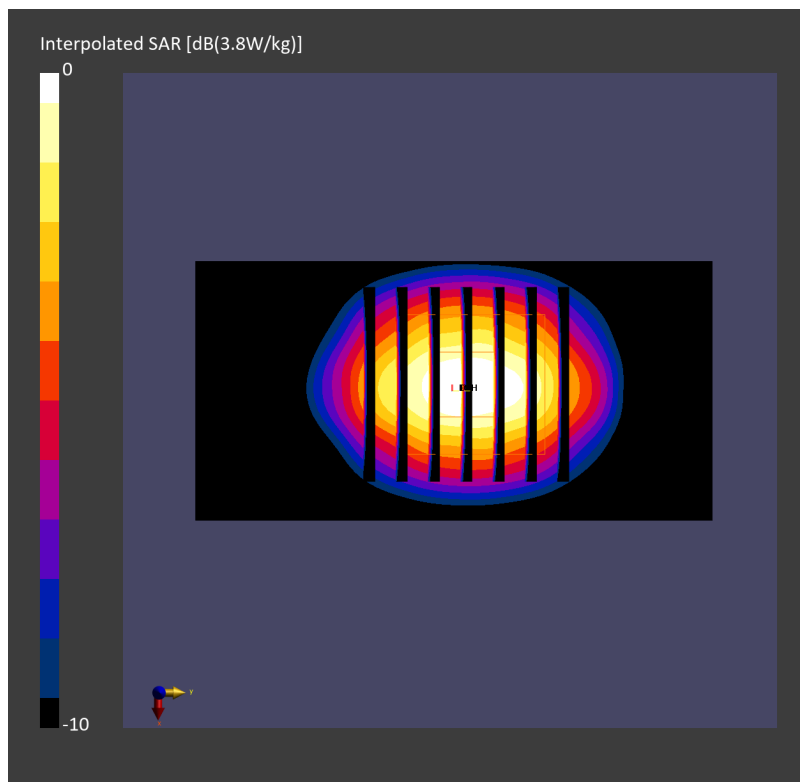

System Check_Head_2600MHz

DUT: D2600V2 - SN1089

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260306 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.98, 6.31, 8.03); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.58 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.3 %

TSL Correction: Positive only

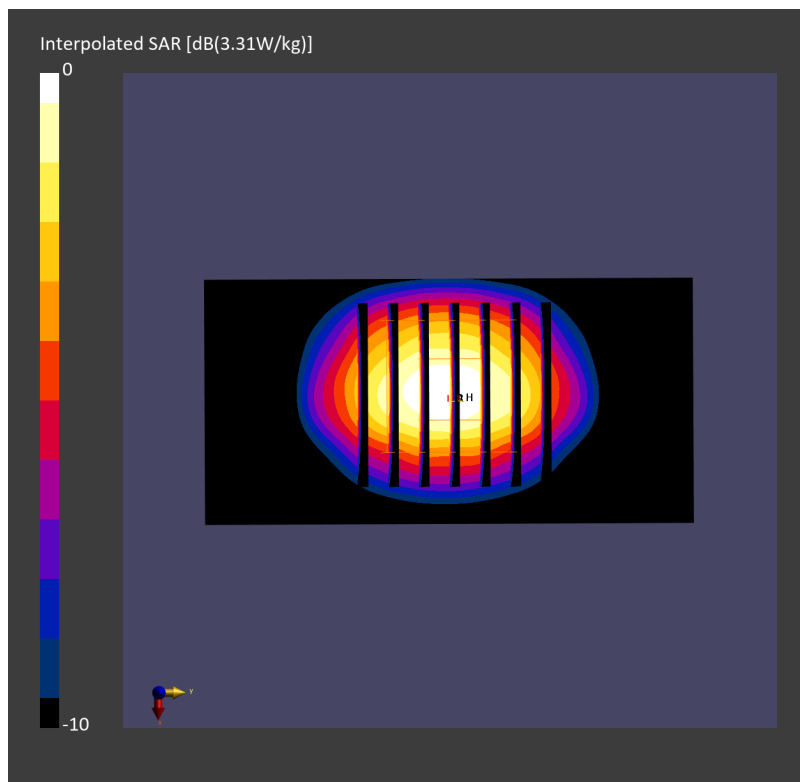

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260310 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.87 W/kg; SAR (10g) = 1.28 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.86 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.7 %

TSL Correction: Positive only

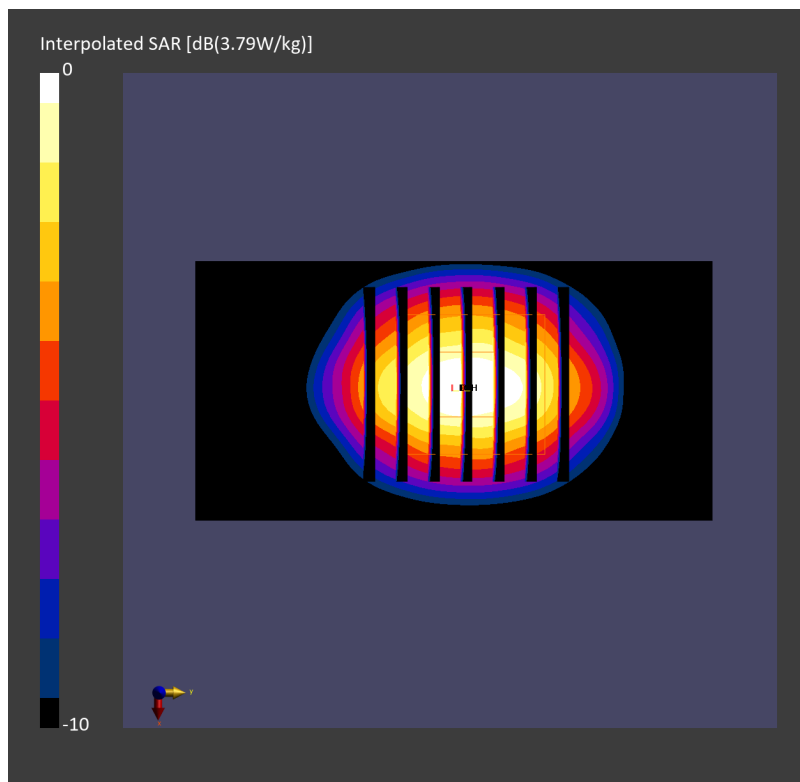

System Check_Head_2600MHz

DUT: D2600V2 - SN1089

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260313 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.98, 6.31, 8.03); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.57 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.0 %

TSL Correction: Positive only

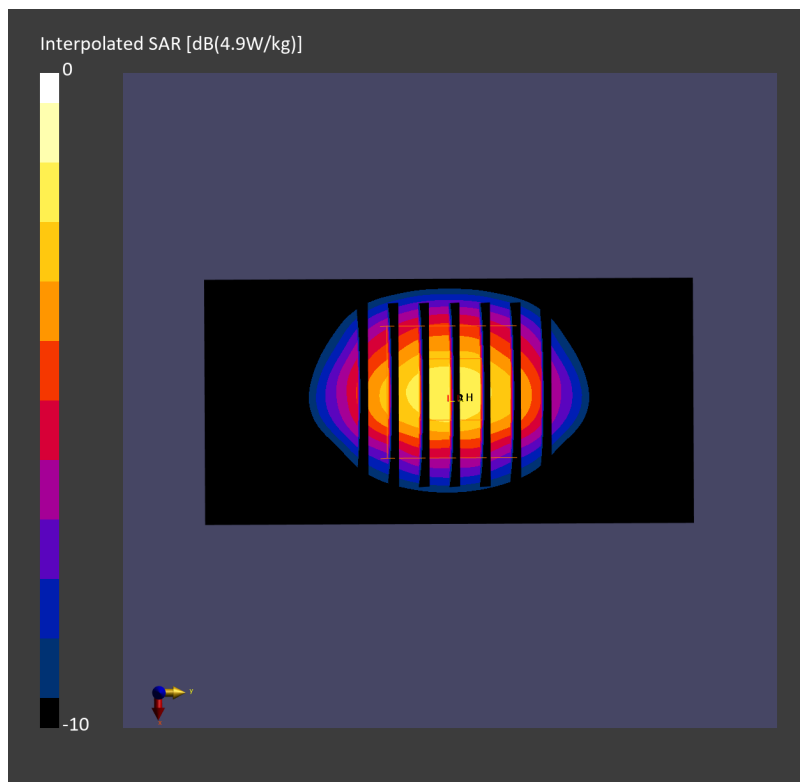

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260315 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.80 W/kg; SAR (10g) = 1.24 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.83 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 80.6 %

TSL Correction: Positive only

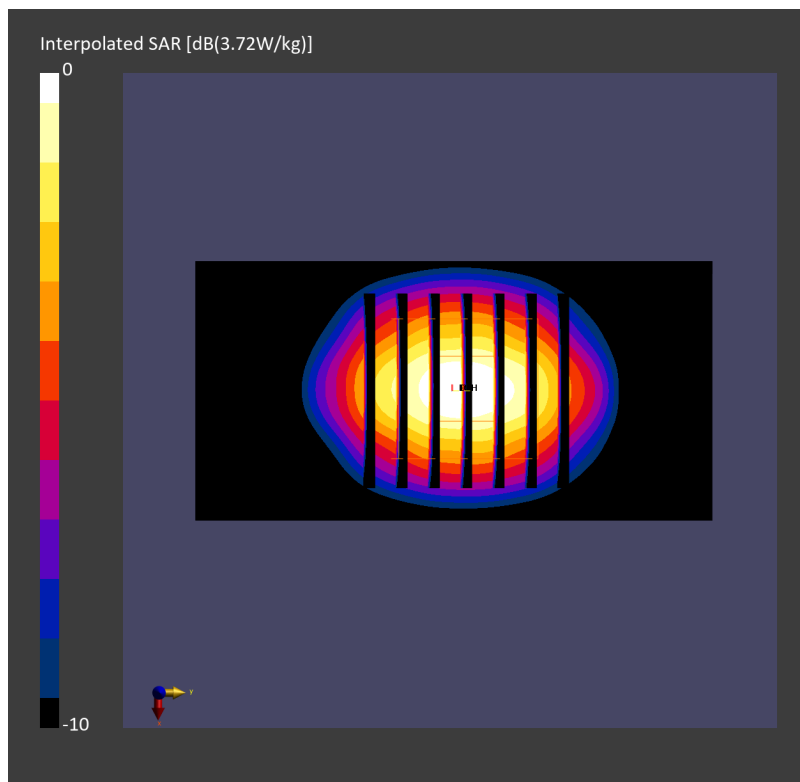

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260319 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.84 W/kg; SAR (10g) = 1.26 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.82 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.4 %

TSL Correction: Positive only

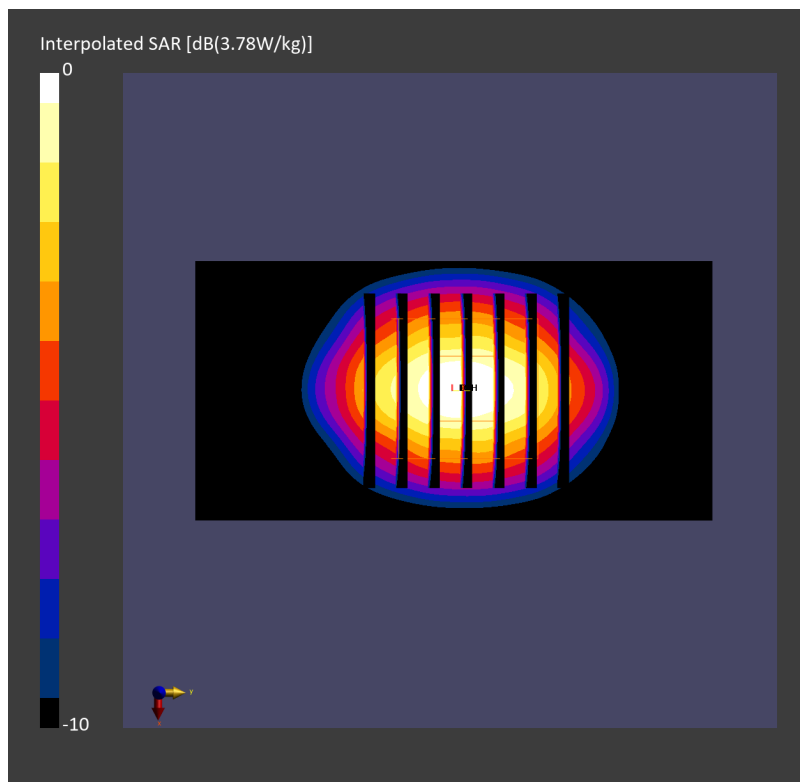

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260320 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.89 W/kg; SAR (10g) = 1.28 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.85 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

TSL Correction: Positive only

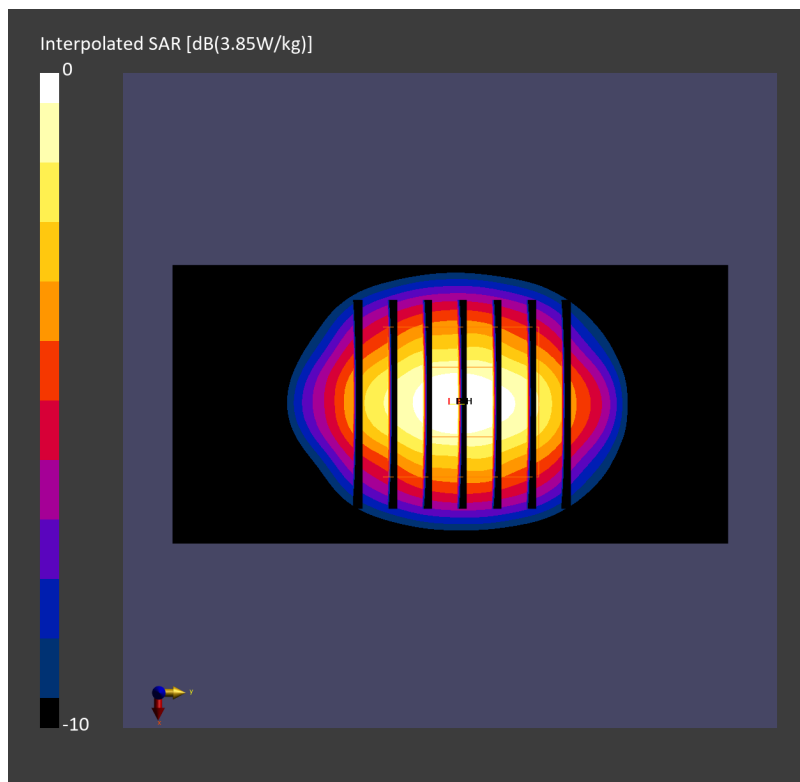

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260324 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.25 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.80 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 80.7 %

TSL Correction: Positive only

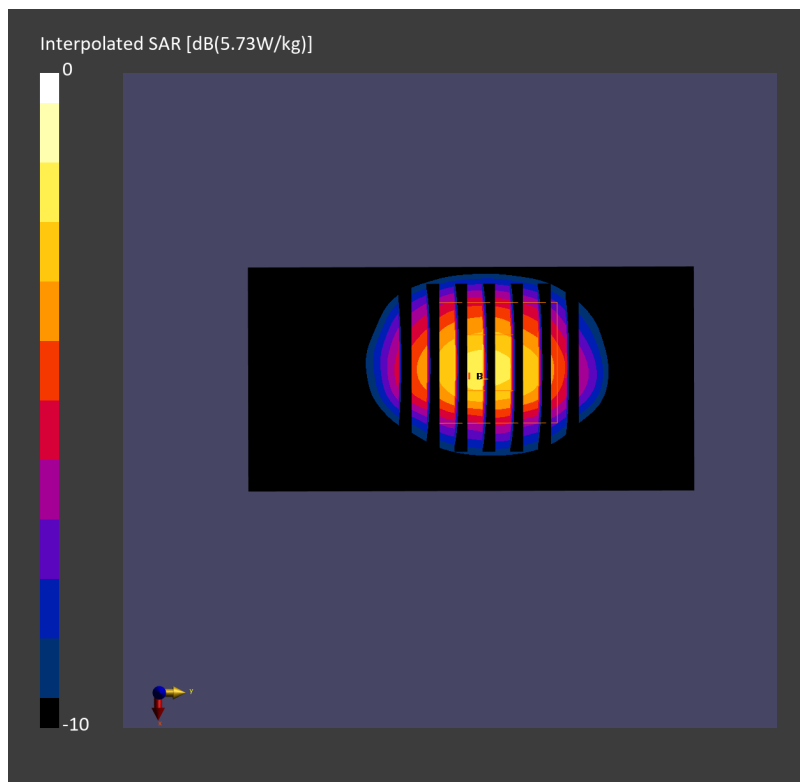

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260403 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.43, 7.23, 7.22); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.53 W/kg; SAR (10g) = 1.13 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.13 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

TSL Correction: Positive only

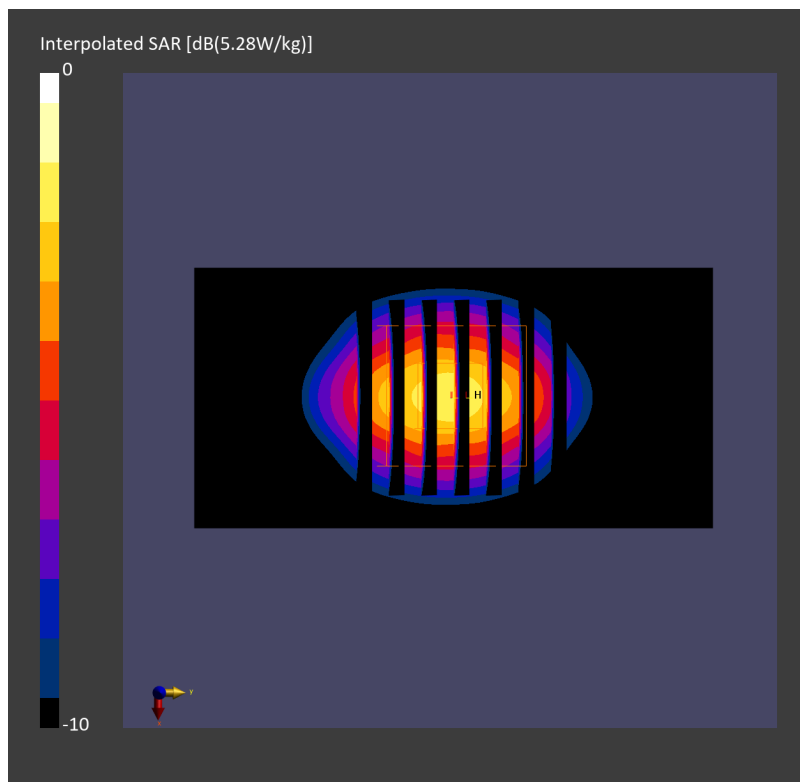

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260403 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.46, 6.69, 6.53); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.25 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.80 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 81.2 %

TSL Correction: Positive only

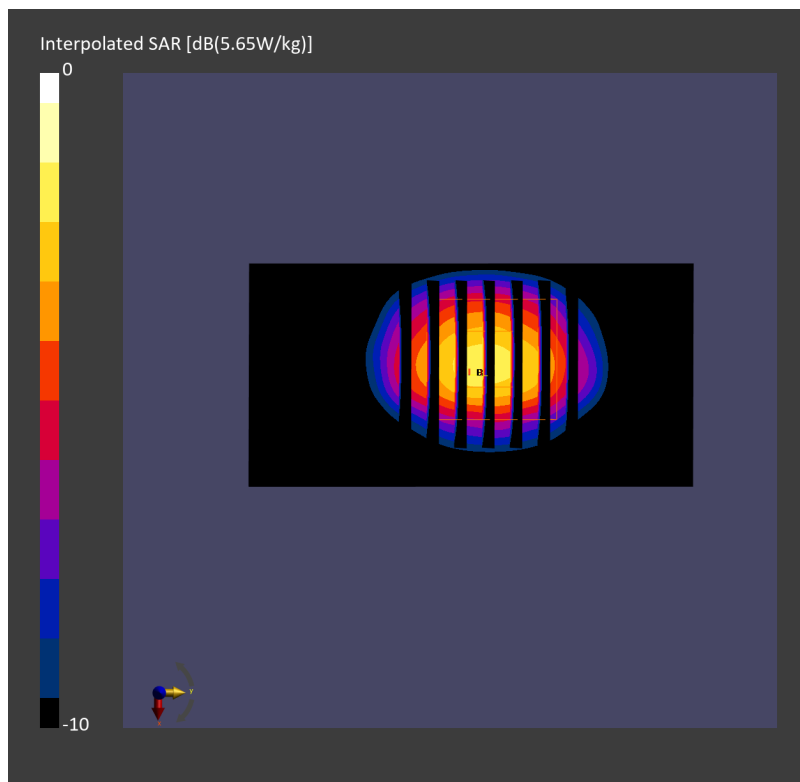

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260409 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.43, 7.23, 7.22); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.56 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

TSL Correction: Positive only

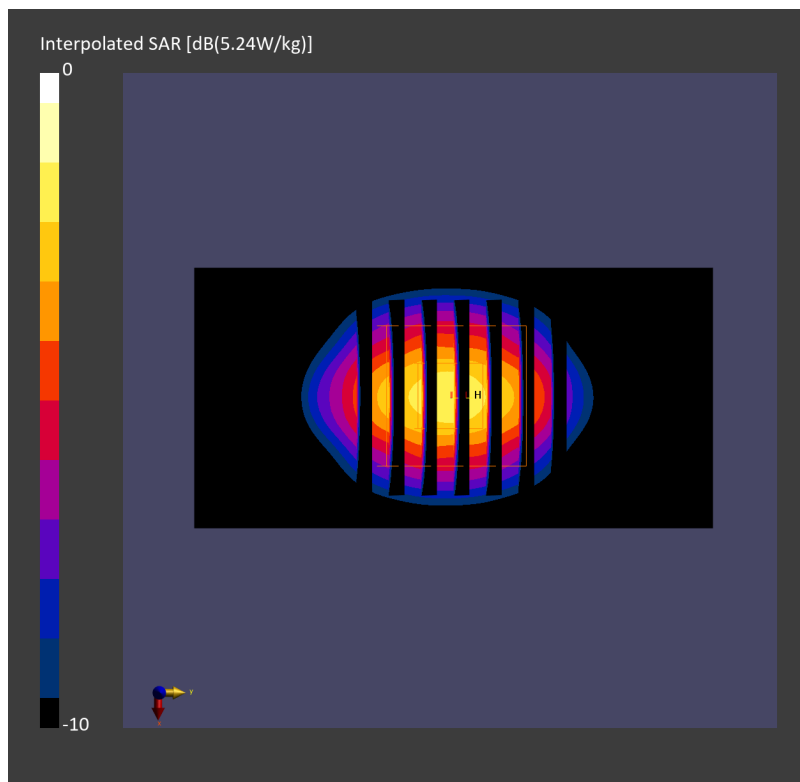

System Check_Head_2600MHz

DUT: D2600V2 - SN1089

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260411 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.43, 7.23, 7.22); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.64 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.9 %

TSL Correction: Positive only

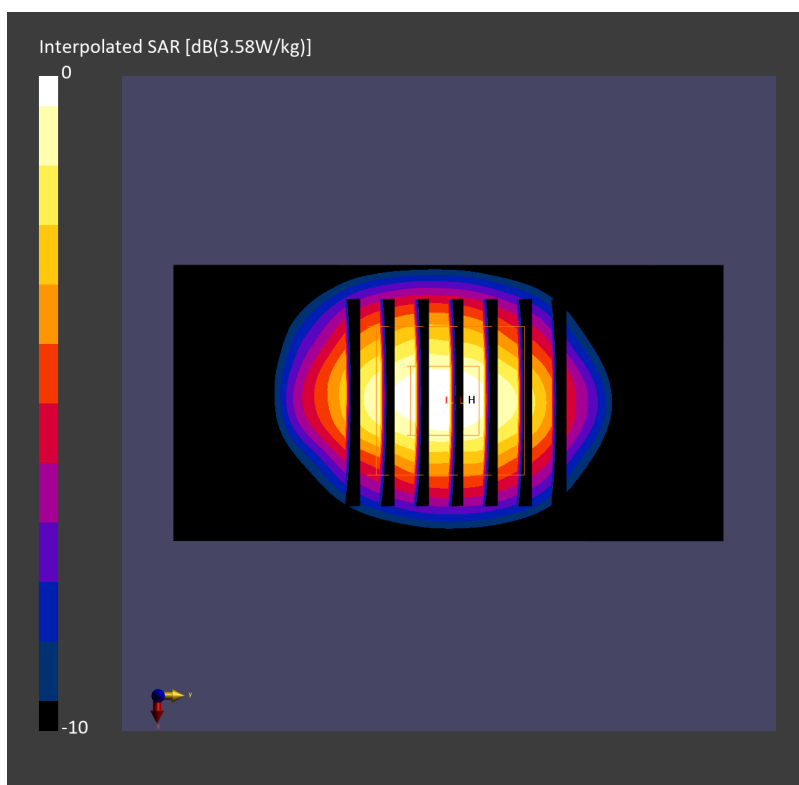

System Check_Head_2600MHz

DUT: D2600V2 - SN1089

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260412 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.43, 7.23, 7.22); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.62 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

TSL Correction: Positive only

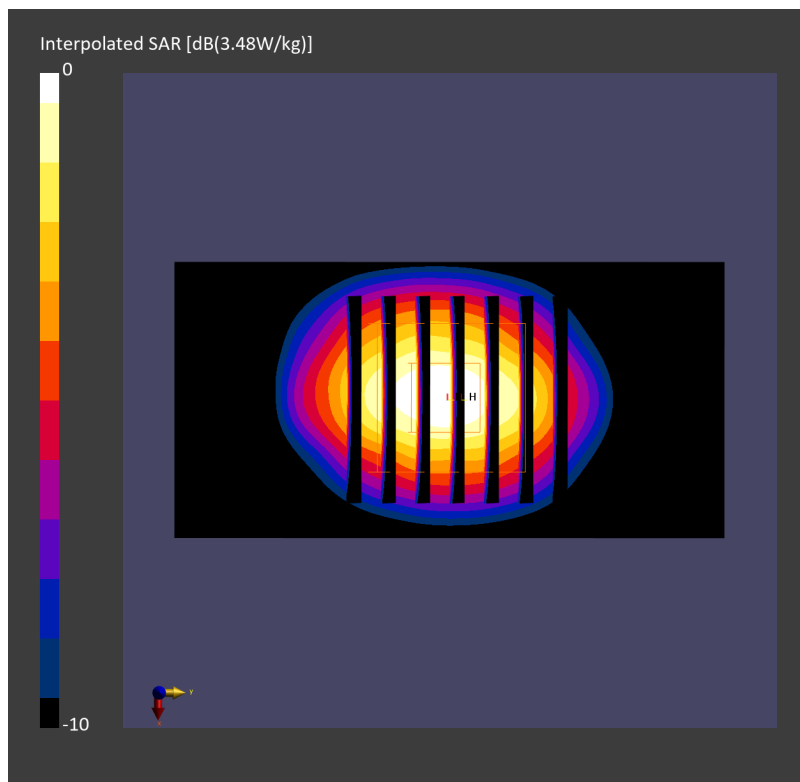

System Check_Head_2600MHz

DUT: D2600V2 - SN1089

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260413 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.43, 7.23, 7.22); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.63 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

TSL Correction: Positive only

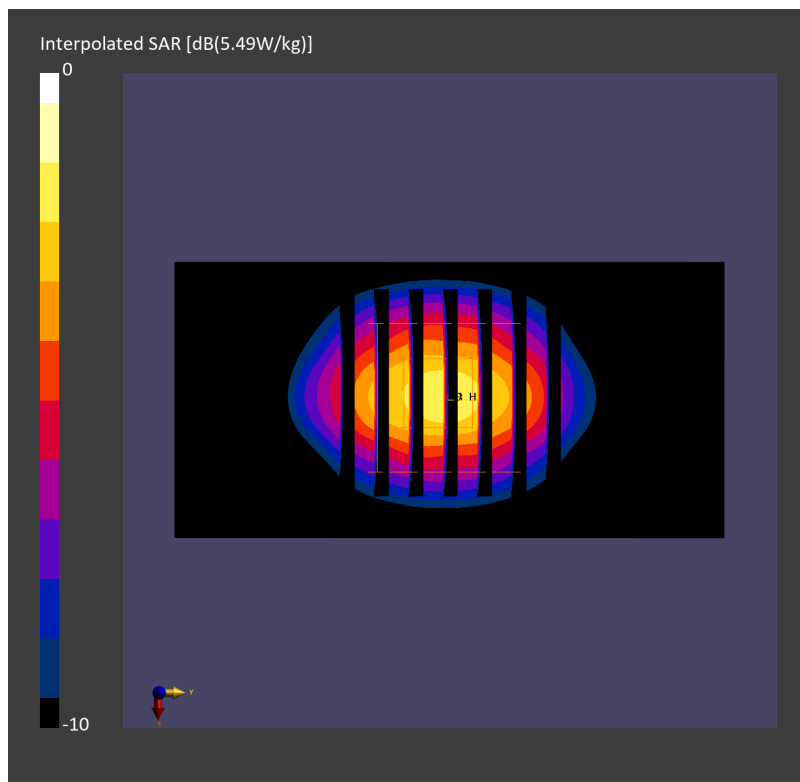

System Check_Head_2600MHz

DUT: D2600V2 - SN1089

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260414 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.43, 7.23, 7.22); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.65 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

TSL Correction: Positive only

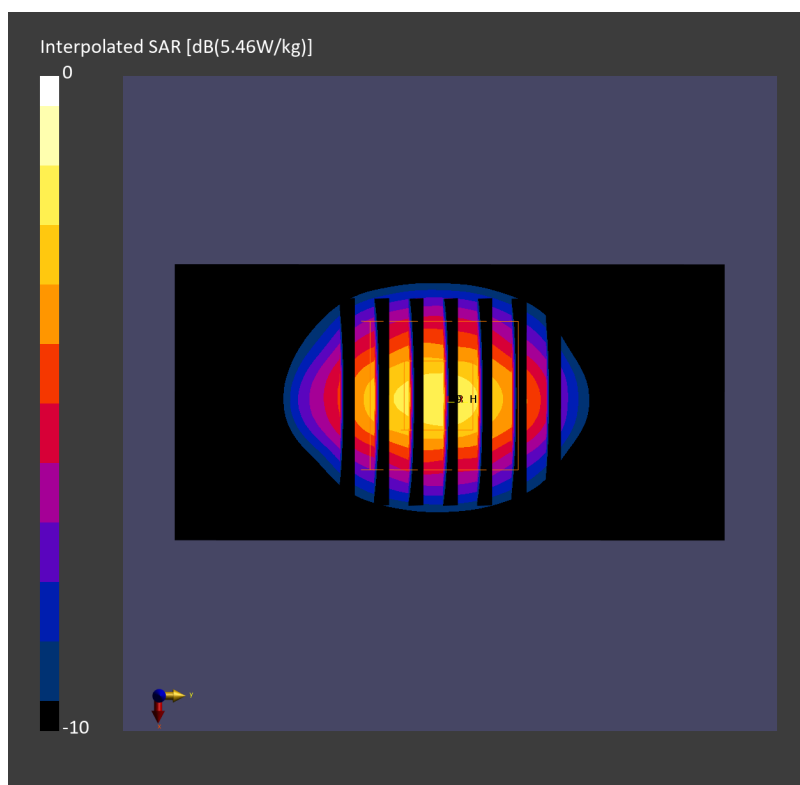

System Check_Head_2600MHz

DUT: D2600V2 - SN1089

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260504 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.43, 7.23, 7.22); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.62 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.1 %

TSL Correction: Positive only

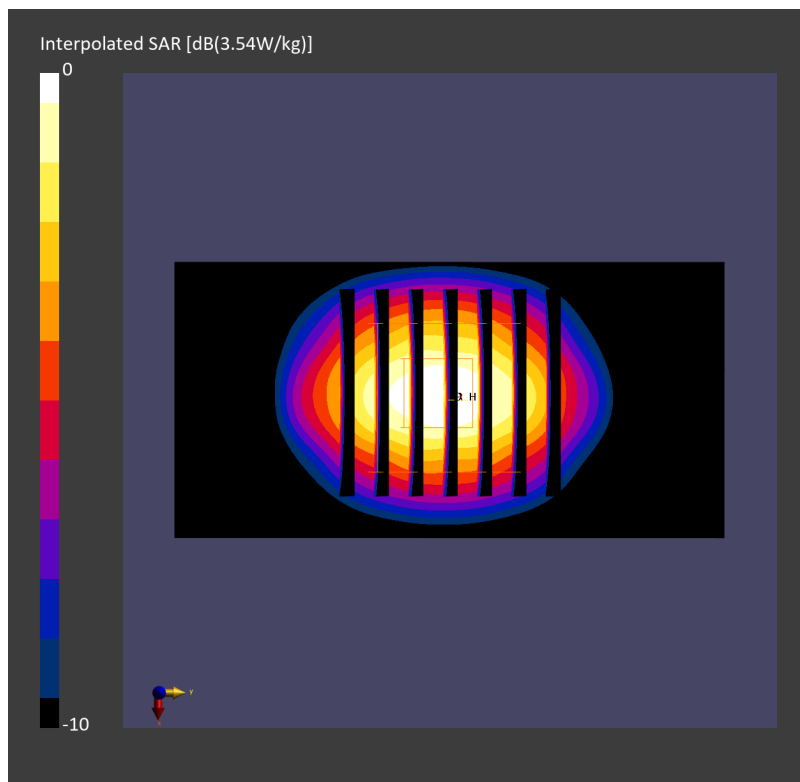

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260222 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.77$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.39 W/kg; SAR (10g) = 1.27 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.40 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.4 %

TSL Correction: Positive only

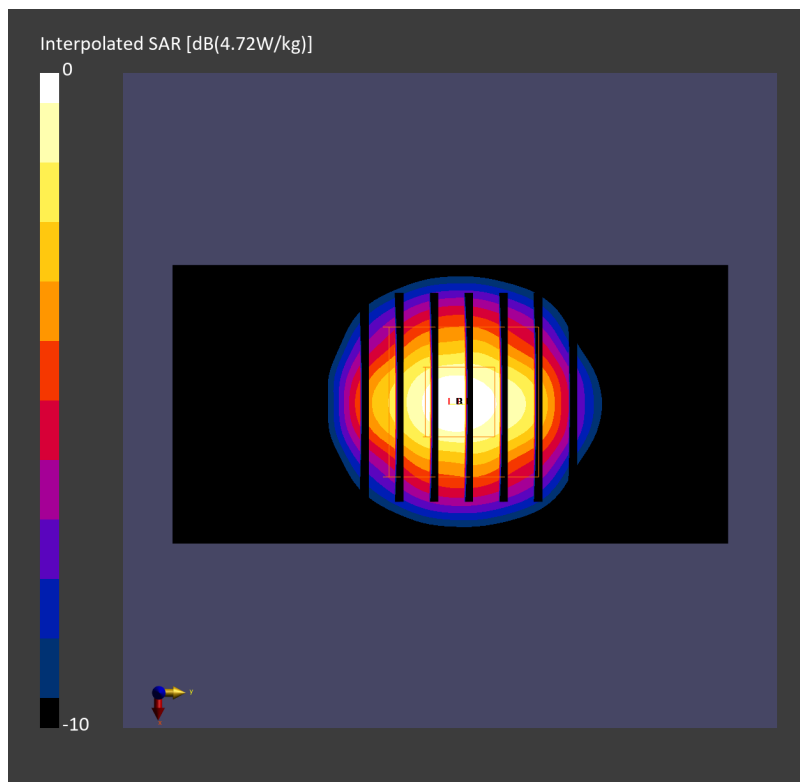

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260227 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.69$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

TSL Correction: Positive only

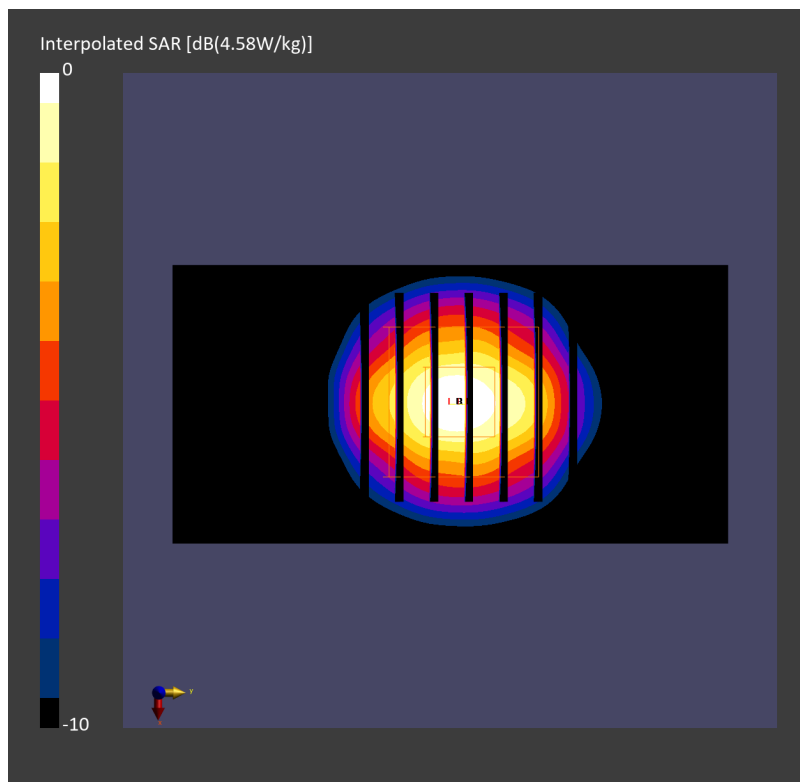

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260304 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.74$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.33 W/kg; SAR (10g) = 1.24 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.34 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

TSL Correction: Positive only

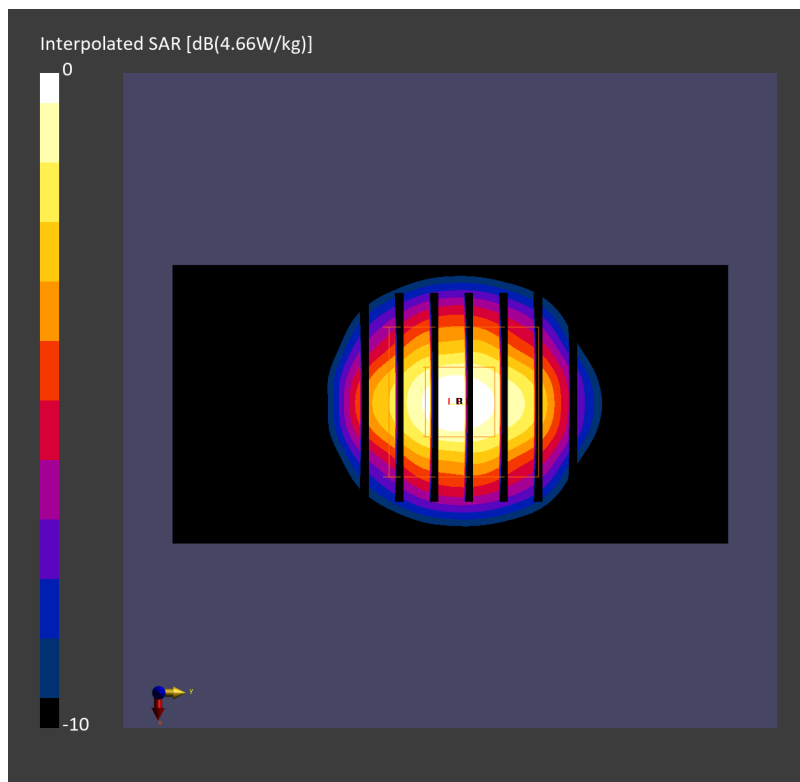

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260307 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.78$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.26, 5.66, 7.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.23 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.0 %

TSL Correction: Positive only

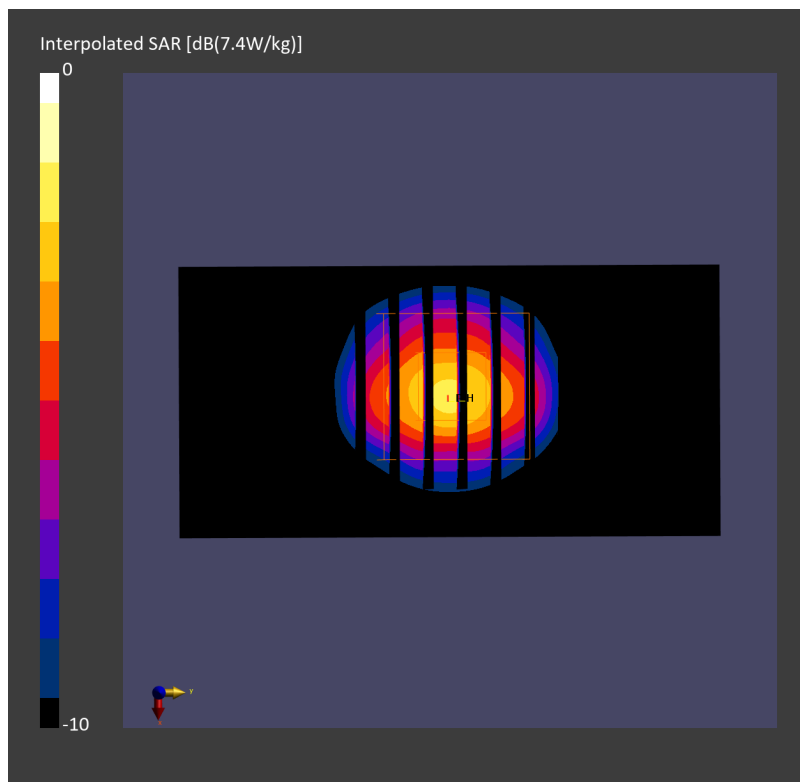

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260313 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.75$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.24 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.33 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

TSL Correction: Positive only

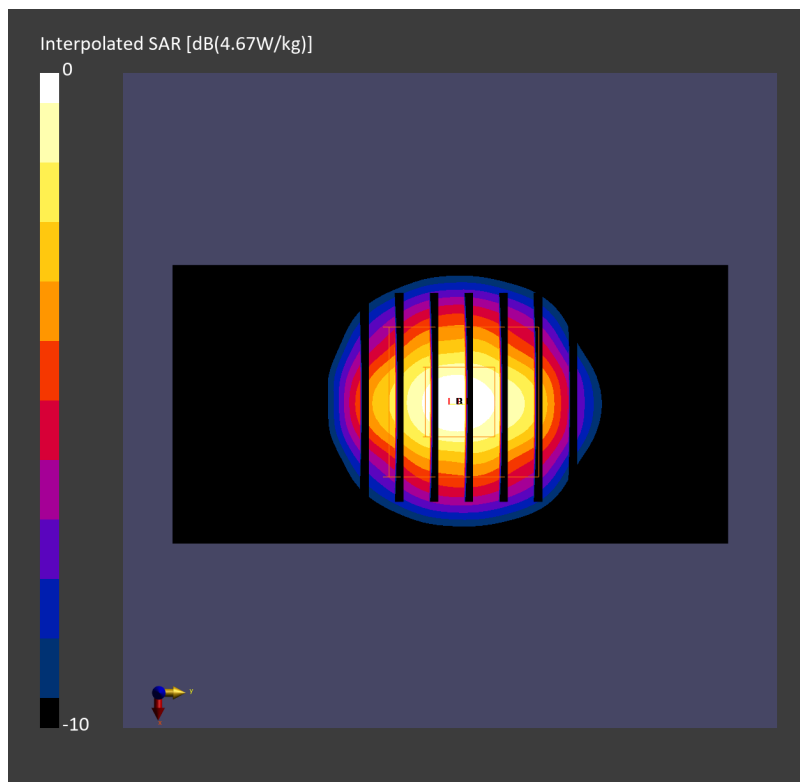

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260317 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.69$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.27 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

TSL Correction: Positive only

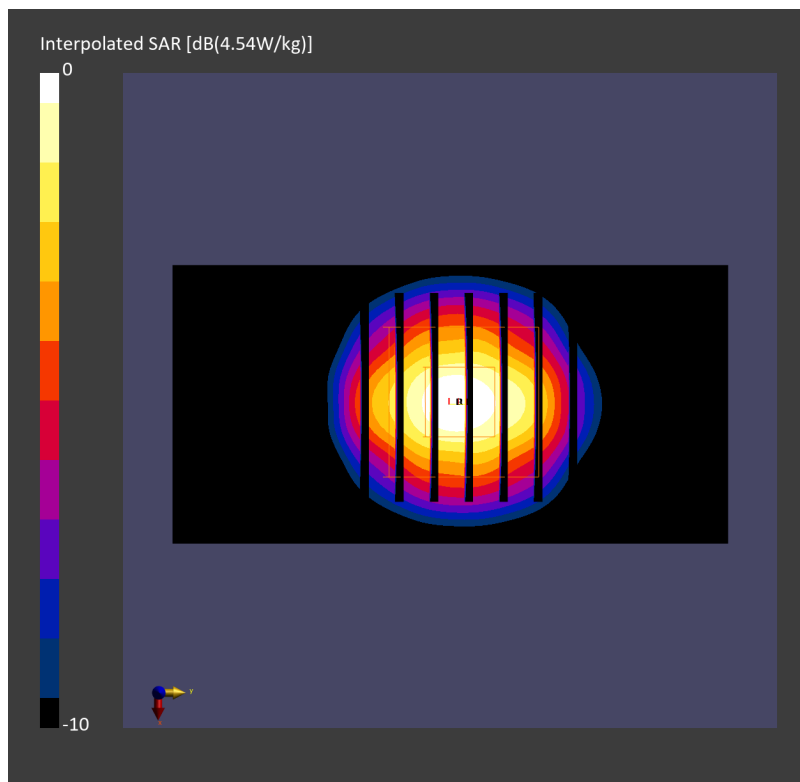

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260318 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.69$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

TSL Correction: Positive only

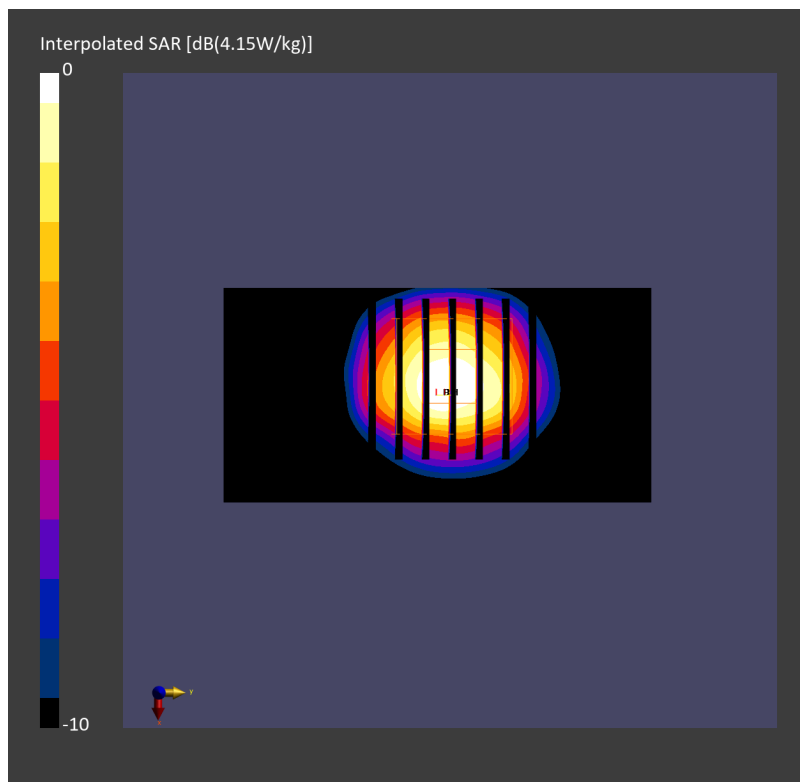

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260321 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.71$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

TSL Correction: Positive only

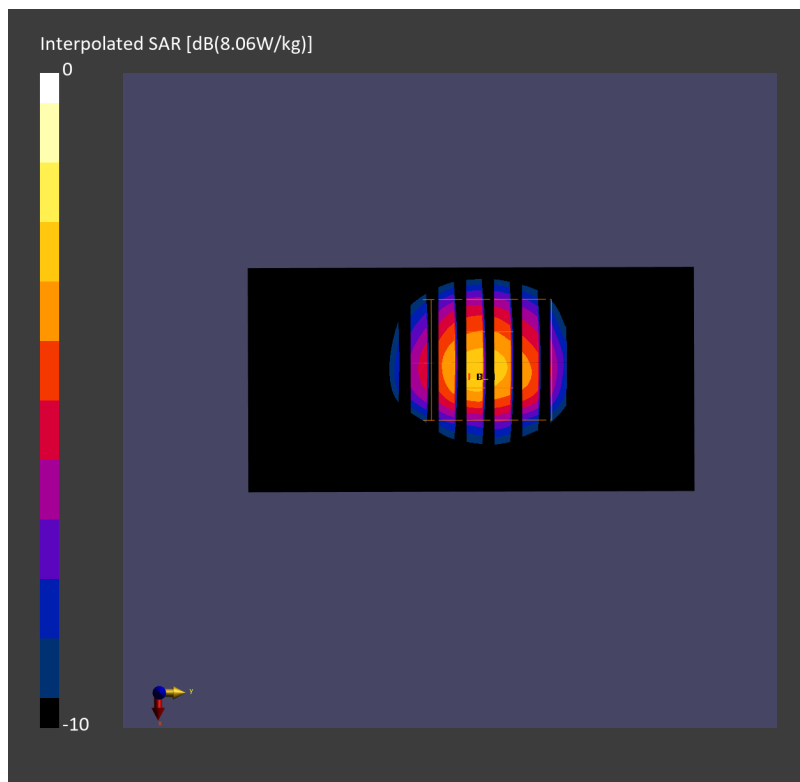

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260330 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.71$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.11, 6.32, 6.17); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.12 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 77.3 %

TSL Correction: Positive only

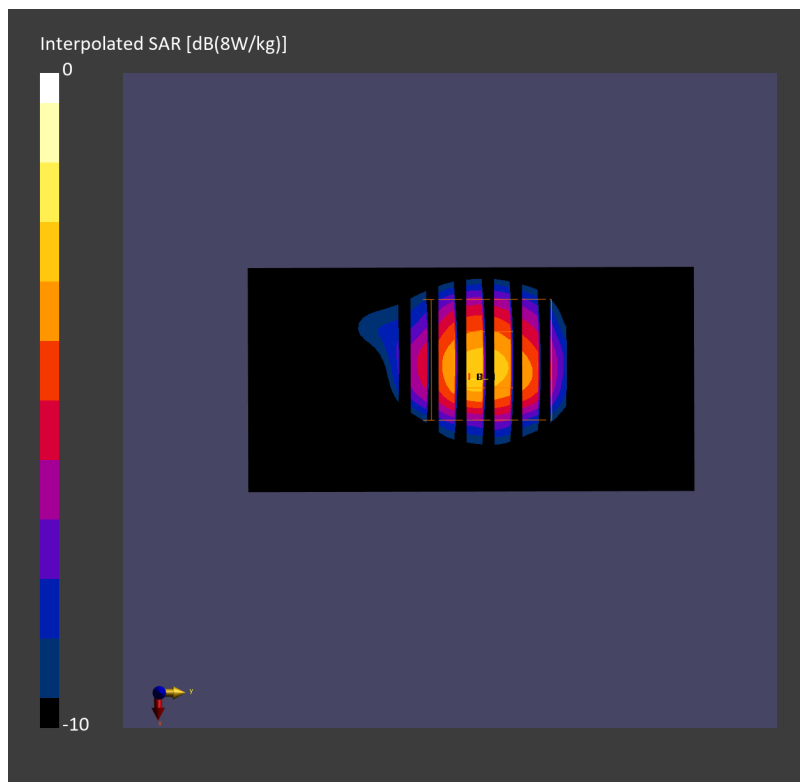

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260404 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.76$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7902; ConvF(6.44, 6.15, 6.1); Calibrated: 2025-12-12
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.23 W/kg; SAR (10g) = 0.818 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.03 dB

SAR (1g) = 3.53 W/kg; SAR (8g) = 1.51 W/kg; SAR (10g) = 1.34 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.4 %

TSL Correction: Positive only

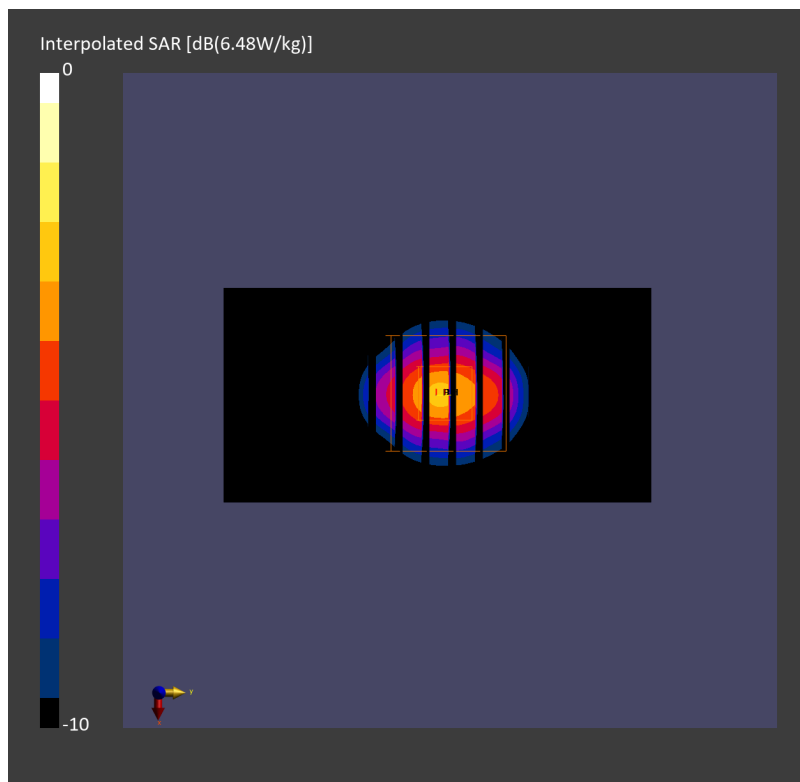

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260405 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.74$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.42, 6.23, 6.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.05 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.17 dB

SAR (1g) = 2.99 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

TSL Correction: Positive only

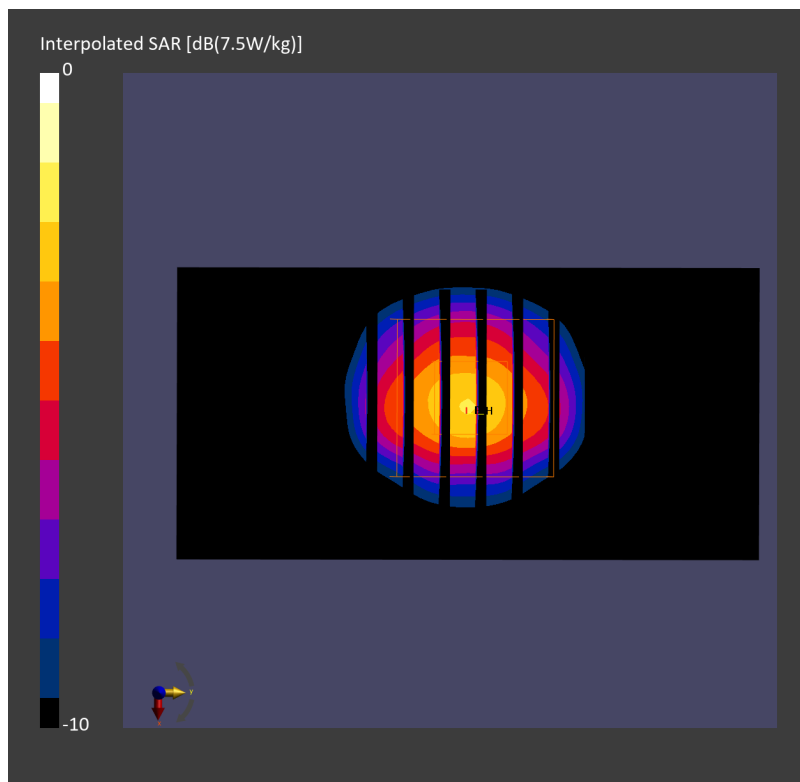

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260410 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.76$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.42, 6.23, 6.57); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.10 dB

SAR (1g) = 3.16 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

TSL Correction: Positive only

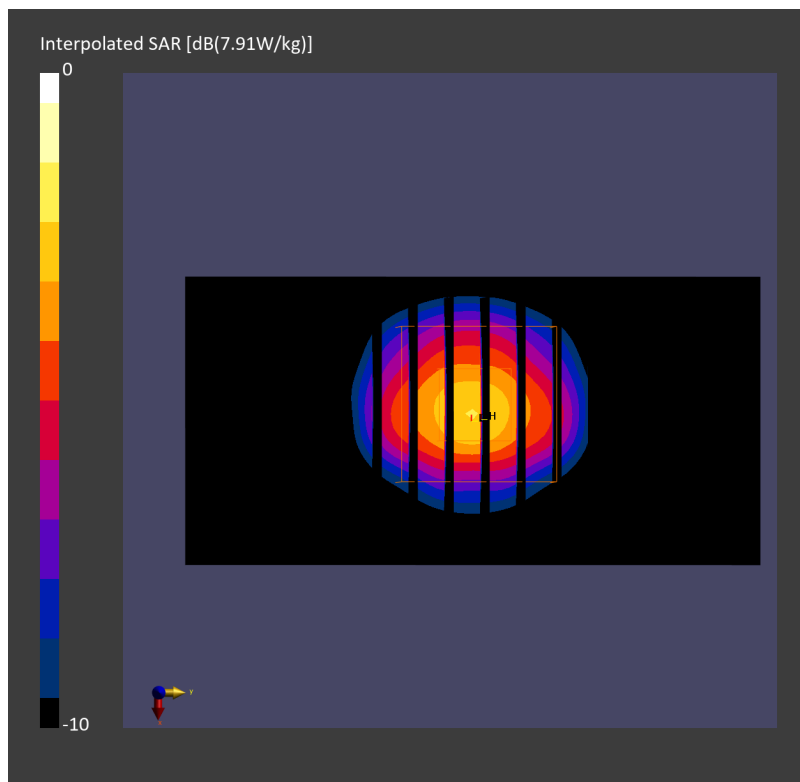

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260222 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.96$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.07, 6.28, 6.13); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.47 W/kg; SAR (10g) = 1.27 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.46 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.5 %

TSL Correction: Positive only

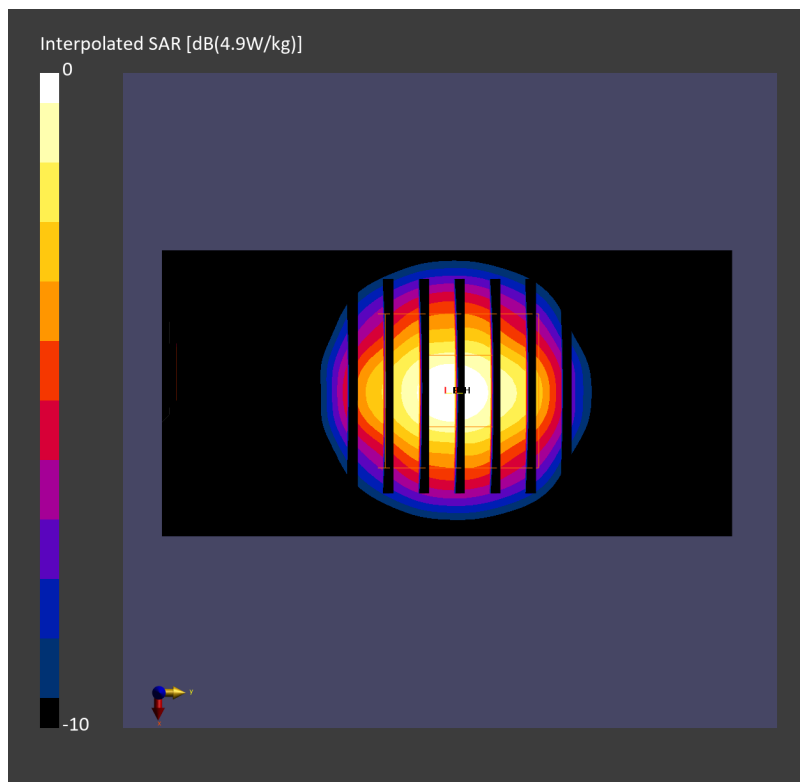

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260227 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.86$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.07, 6.28, 6.13); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.40 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.7 %

TSL Correction: Positive only

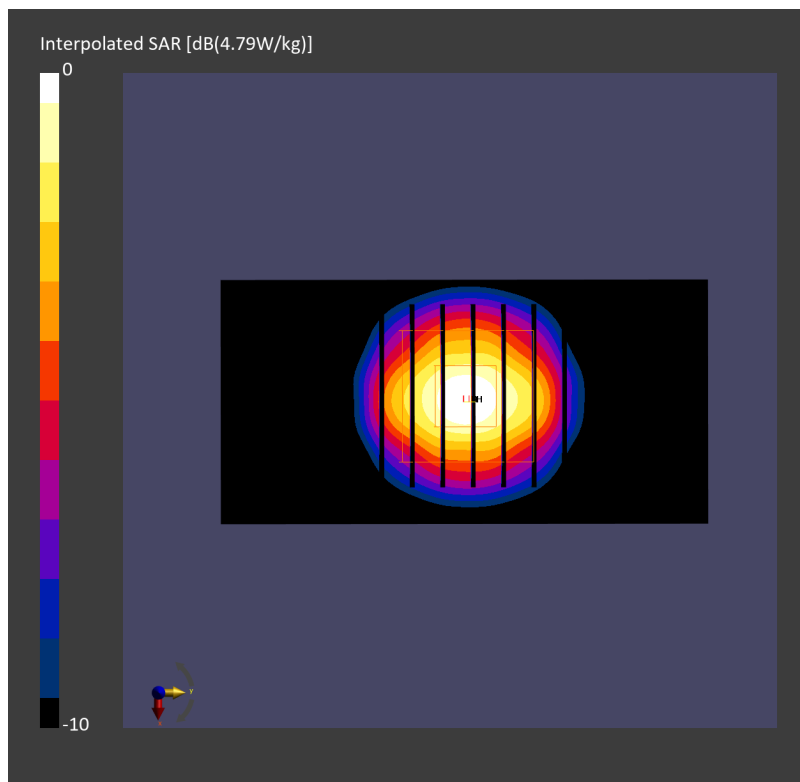

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260304 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.07, 6.28, 6.13); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.42 W/kg; SAR (10g) = 1.25 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.45 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.7 %

TSL Correction: Positive only

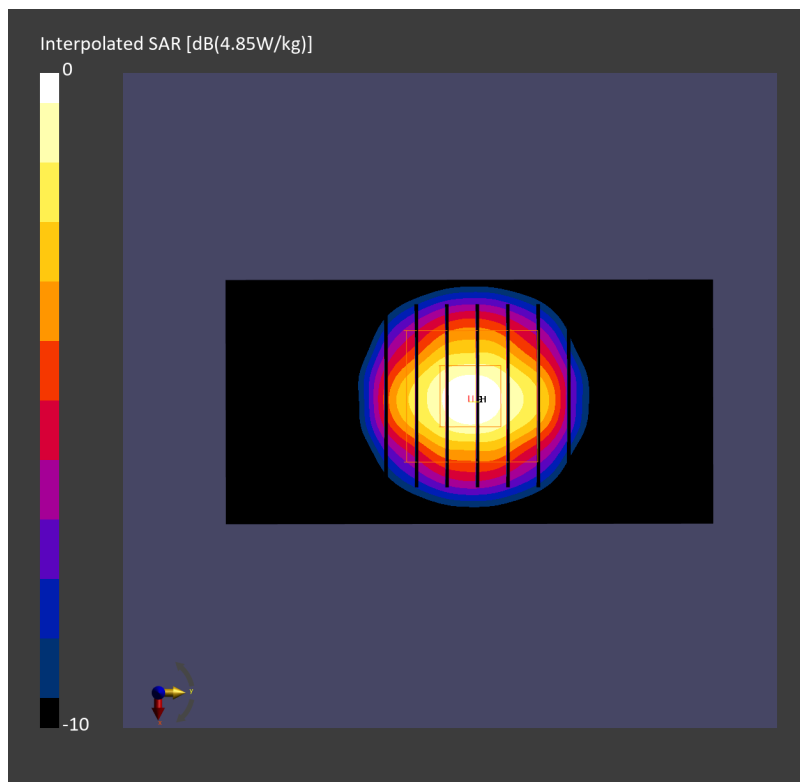

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260307 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.96$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(6.09, 5.51, 7.01); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.7 %

TSL Correction: Positive only

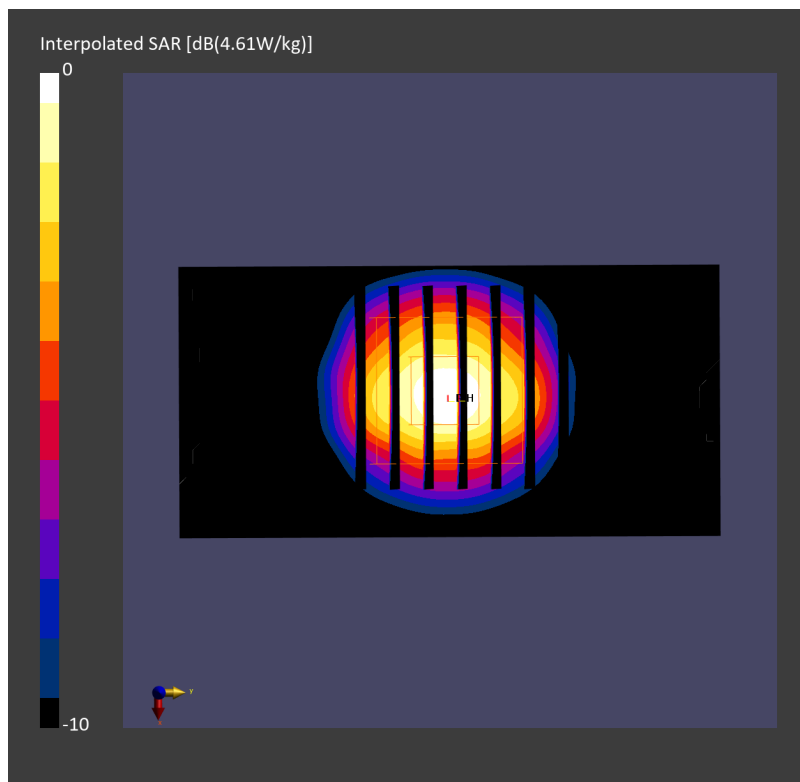

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260313 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.93$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.07, 6.28, 6.13); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.42 W/kg; SAR (10g) = 1.25 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.47 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

TSL Correction: Positive only

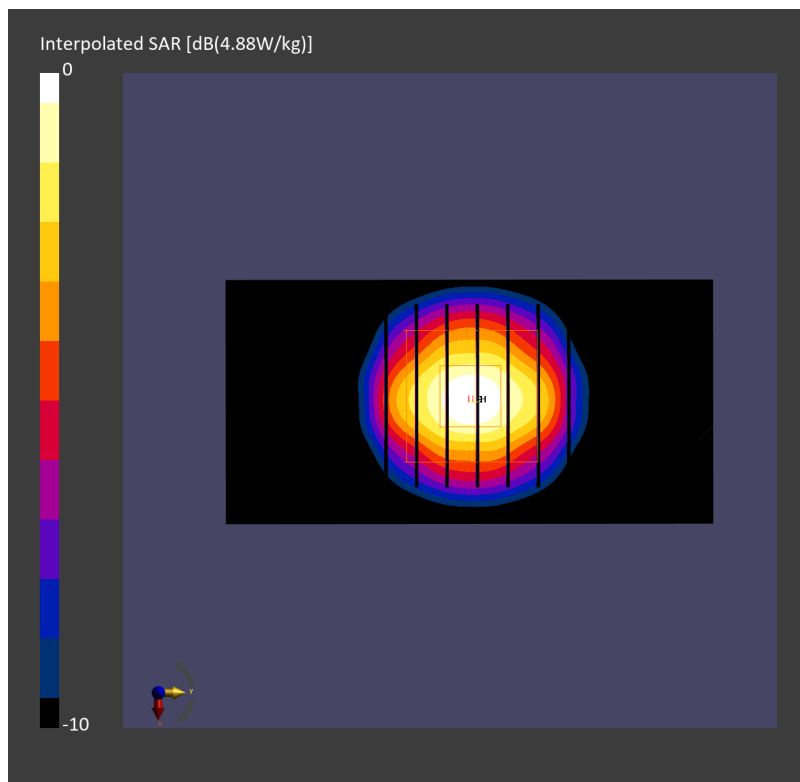

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260317 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.86$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.07, 6.28, 6.13); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.35 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.41 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.6 %

TSL Correction: Positive only

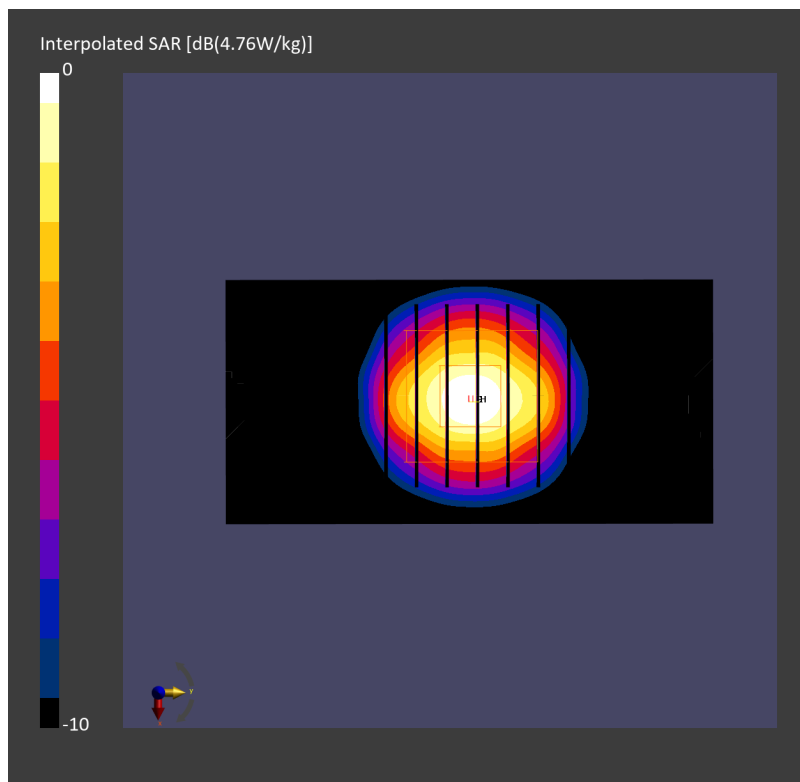

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260330 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.88$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.07, 6.28, 6.13); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.46 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

TSL Correction: Positive only

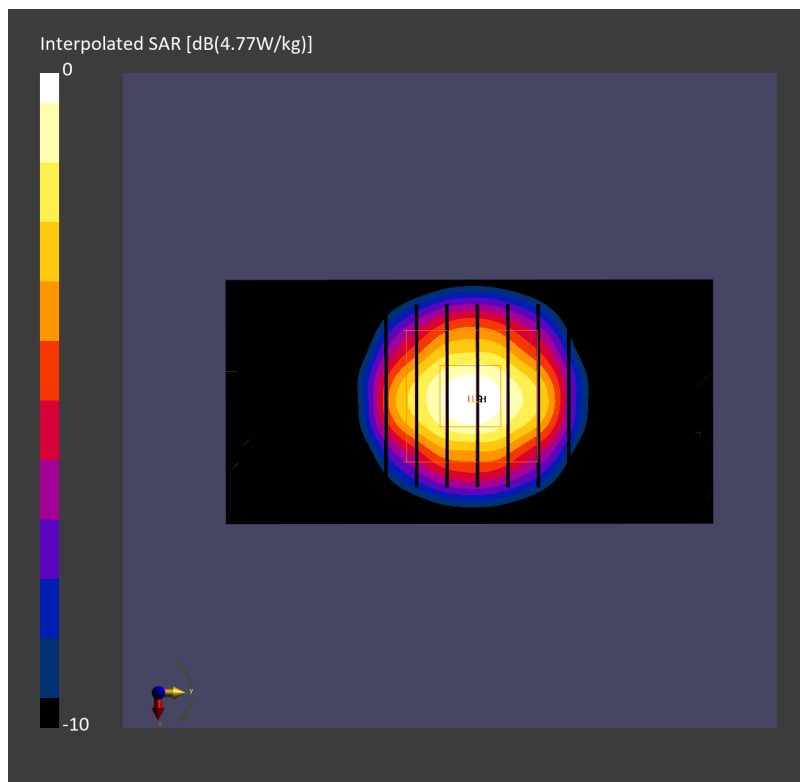

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260405 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.36, 6.17, 6.51); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.23 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.22 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

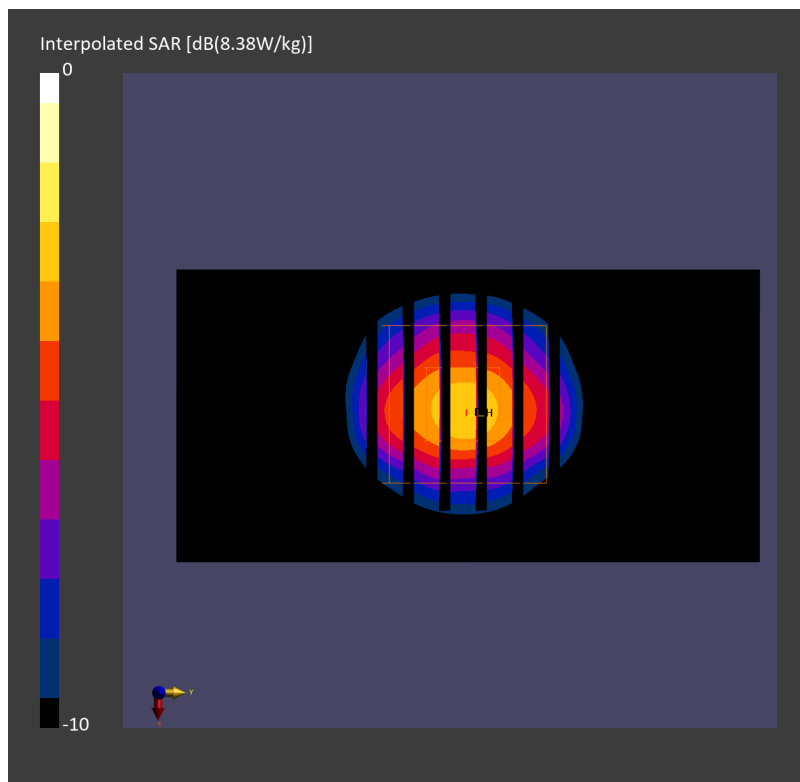

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260405 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.94$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7902; ConvF(6.44, 6.14, 6.1); Calibrated: 2025-12-12
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.27 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.04 dB

SAR (1g) = 3.50 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 70.7 %

TSL Correction: Positive only

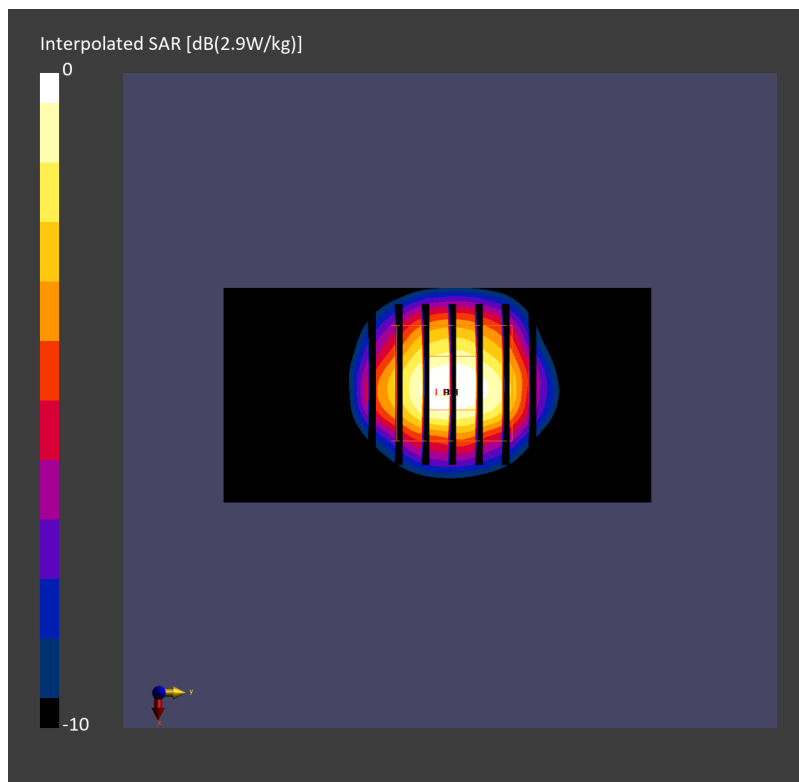

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260410 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.94$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.36, 6.17, 6.51); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 3.24 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

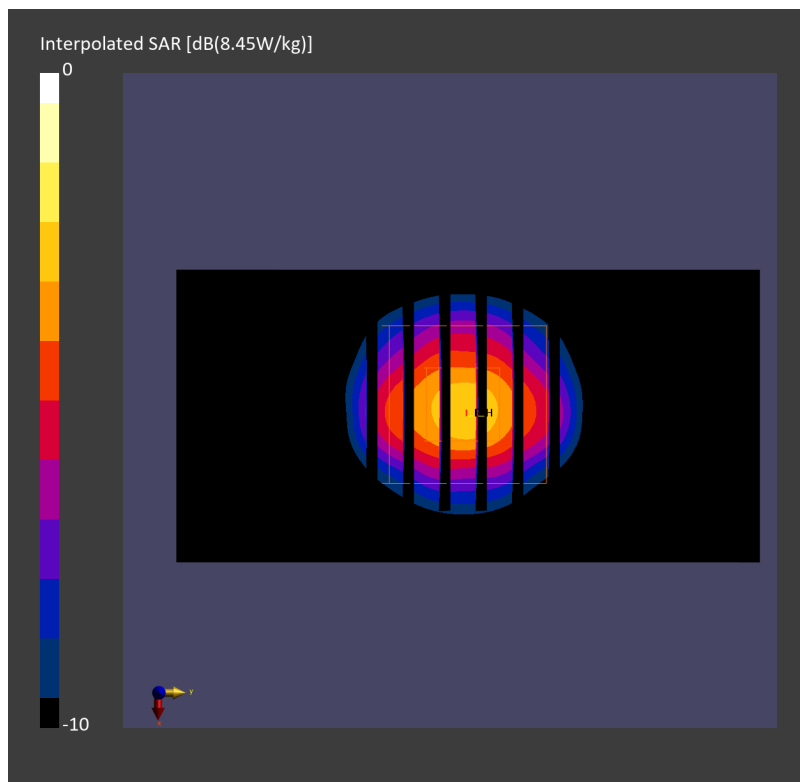

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260228 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.04$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7902; ConvF(6.28, 5.99, 5.95); Calibrated: 2025-12-12
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.29 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.36 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

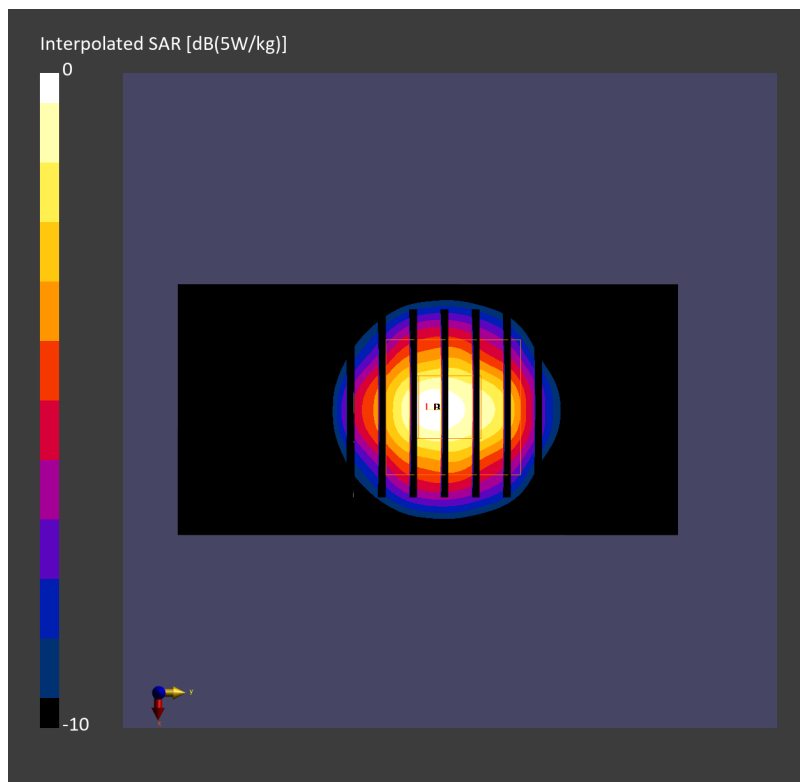

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260305 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7902; ConvF(6.28, 5.99, 5.95); Calibrated: 2025-12-12
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.43 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

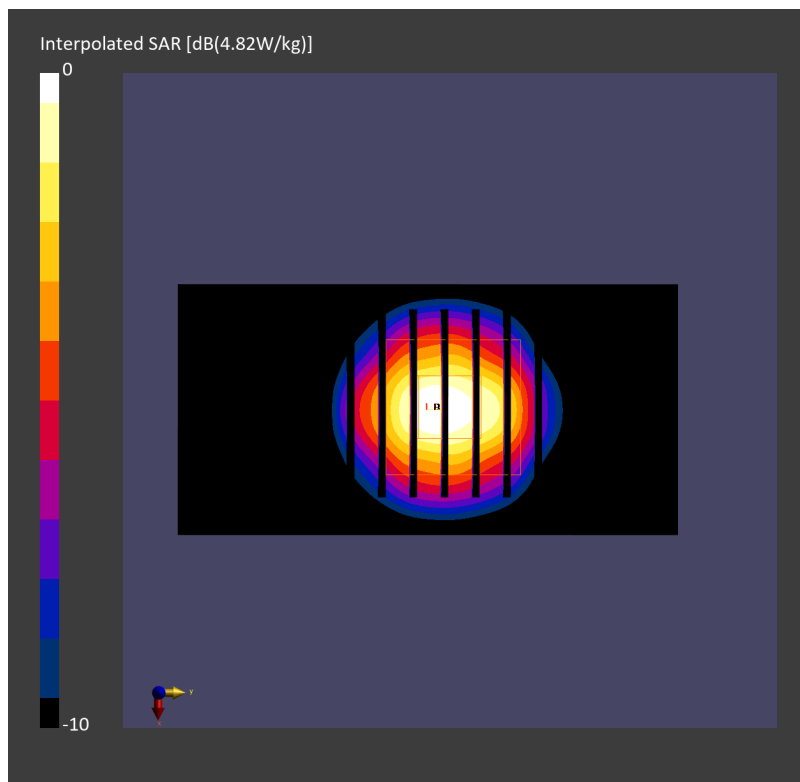

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260314 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.12$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7902; ConvF(6.28, 5.99, 5.95); Calibrated: 2025-12-12
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.46 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.7 %

TSL Correction: Positive only

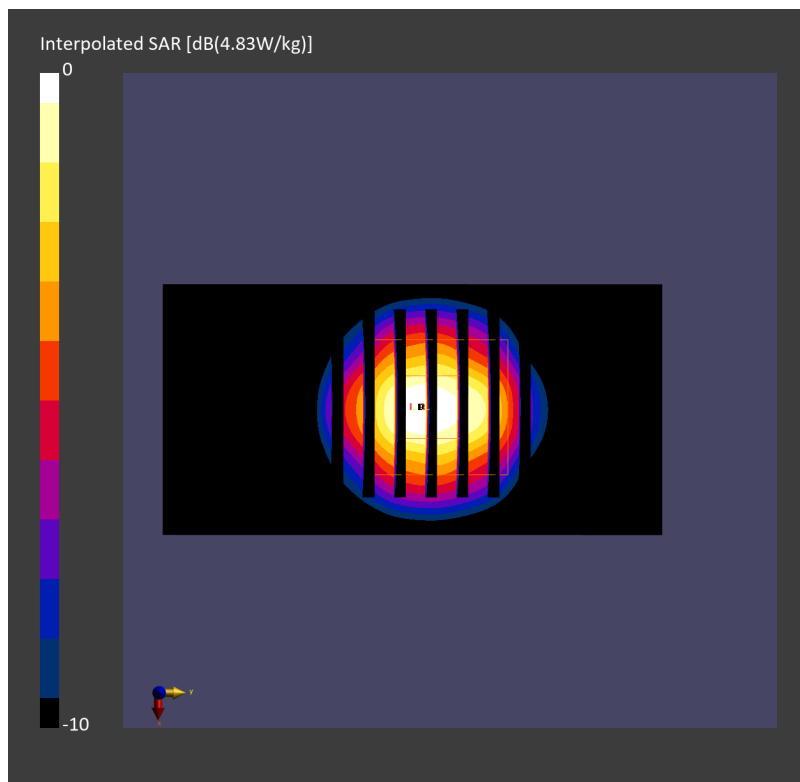

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260316 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.04$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7902; ConvF(6.28, 5.99, 5.95); Calibrated: 2025-12-12
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.35 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.7 %

TSL Correction: Positive only

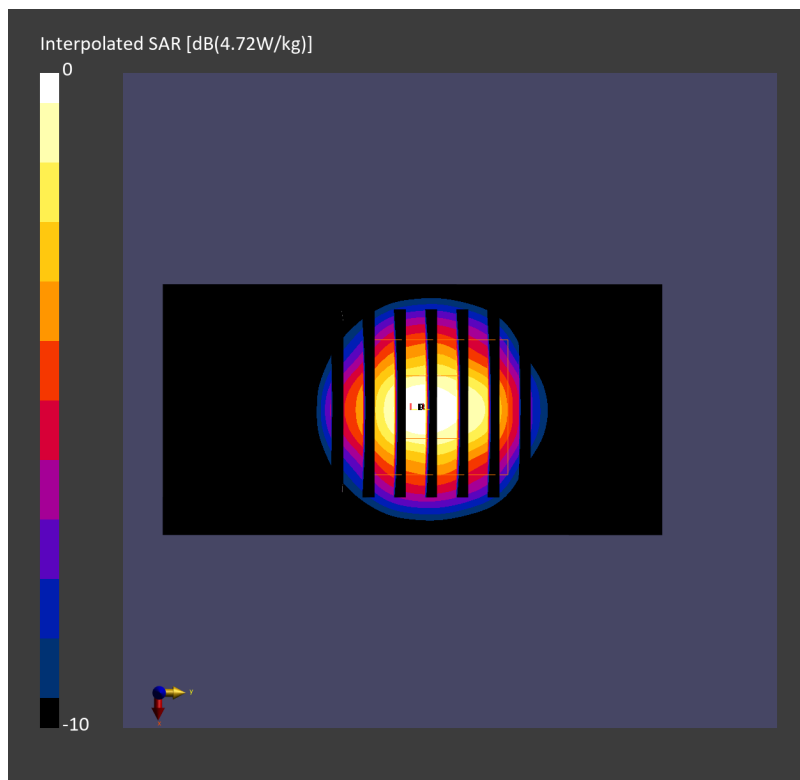

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260322 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.06$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7902; ConvF(6.28, 5.99, 5.95); Calibrated: 2025-12-12
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.41 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.2 %

TSL Correction: Positive only

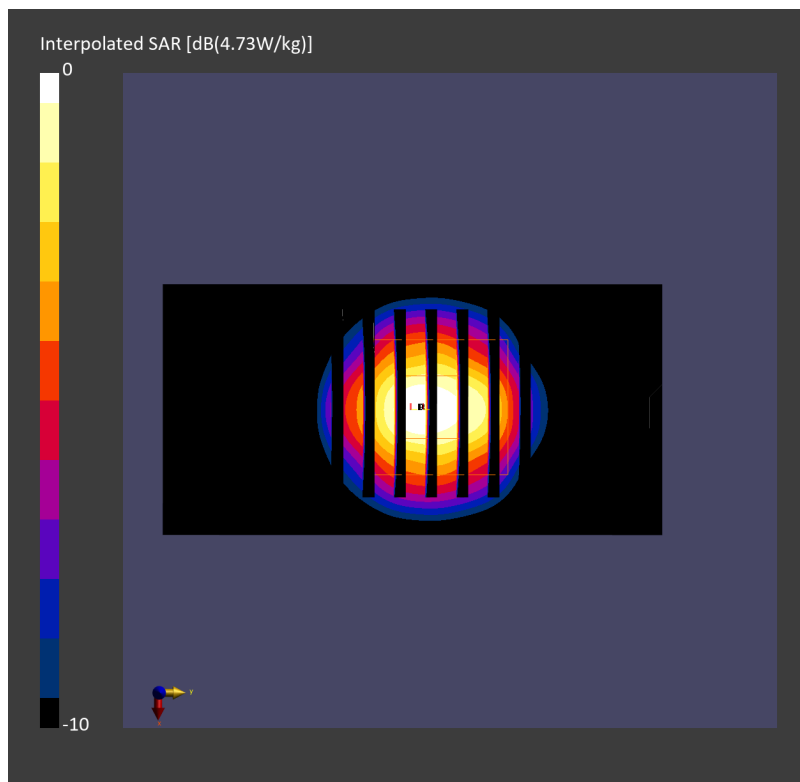

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260405 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.31, 6.12, 6.45); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.35 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 73.7 %

TSL Correction: Positive only

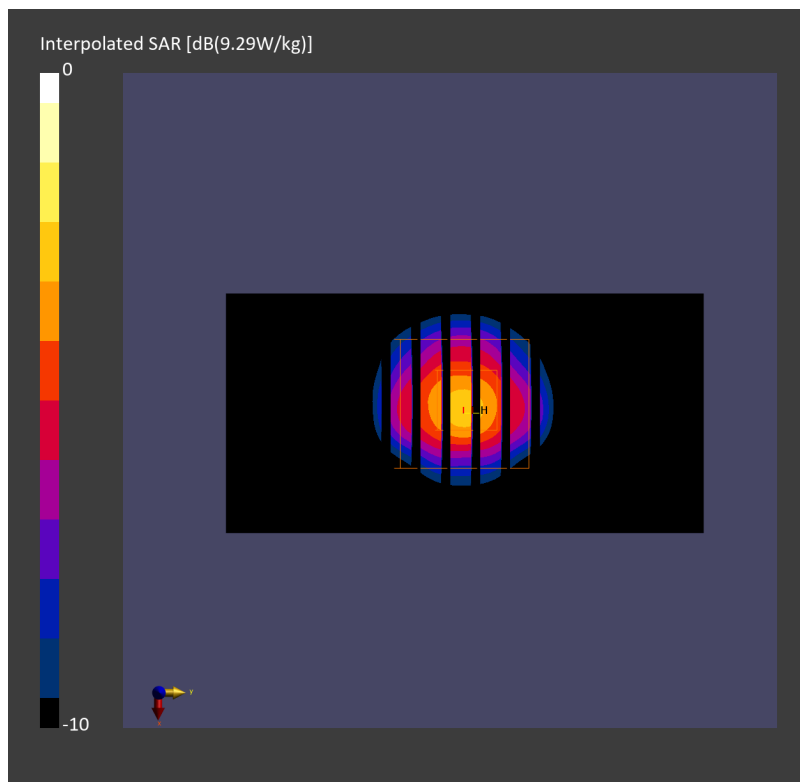

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260406 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.13$ S/m; $\epsilon_r = 36.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7902; ConvF(6.28, 5.99, 5.95); Calibrated: 2025-12-12
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1884; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.55 W/kg; SAR (10g) = 1.27 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.05 dB

SAR (1g) = 3.58 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 69.9 %

TSL Correction: Positive only

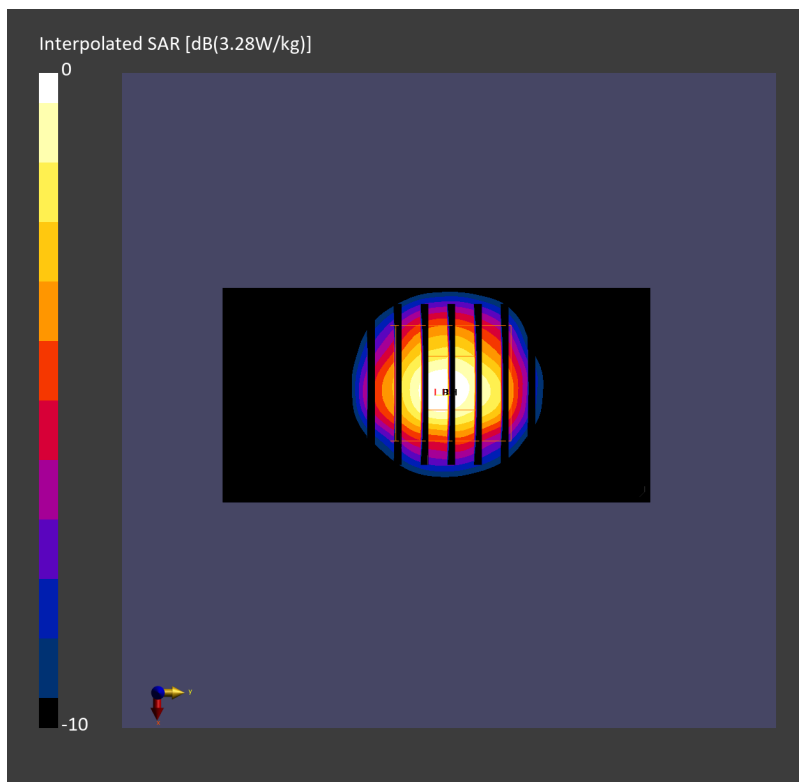

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260410 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.16$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(6.31, 6.12, 6.45); Calibrated: 2025-07-28
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.38 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 3.41 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 73.7 %

TSL Correction: Positive only

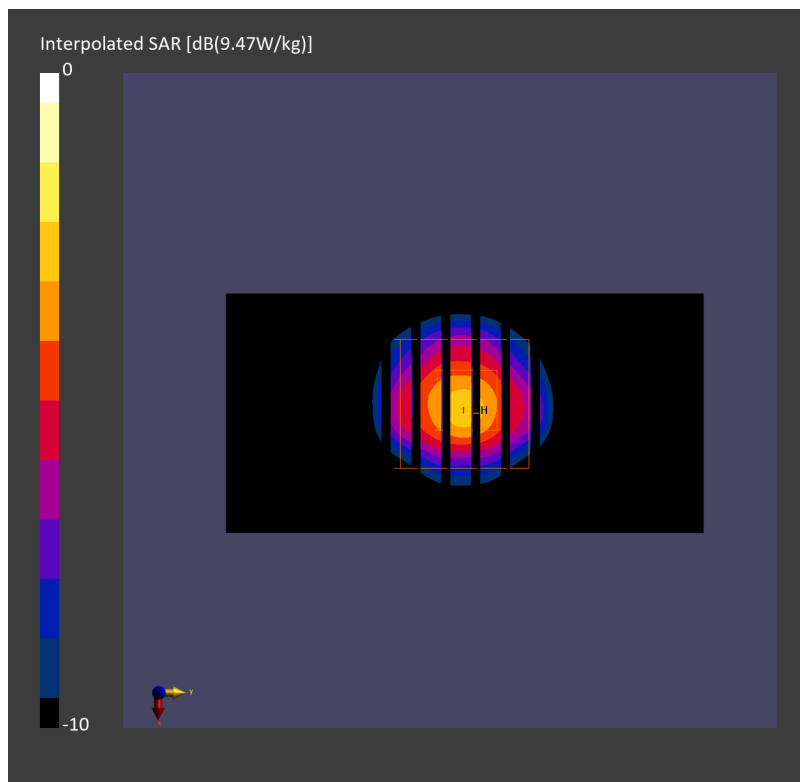

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260321 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.61$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.98, 5.82, 5.82); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.52 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.68 W/kg; SAR (8g) = 1.23 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.4 %

TSL Correction: Positive only

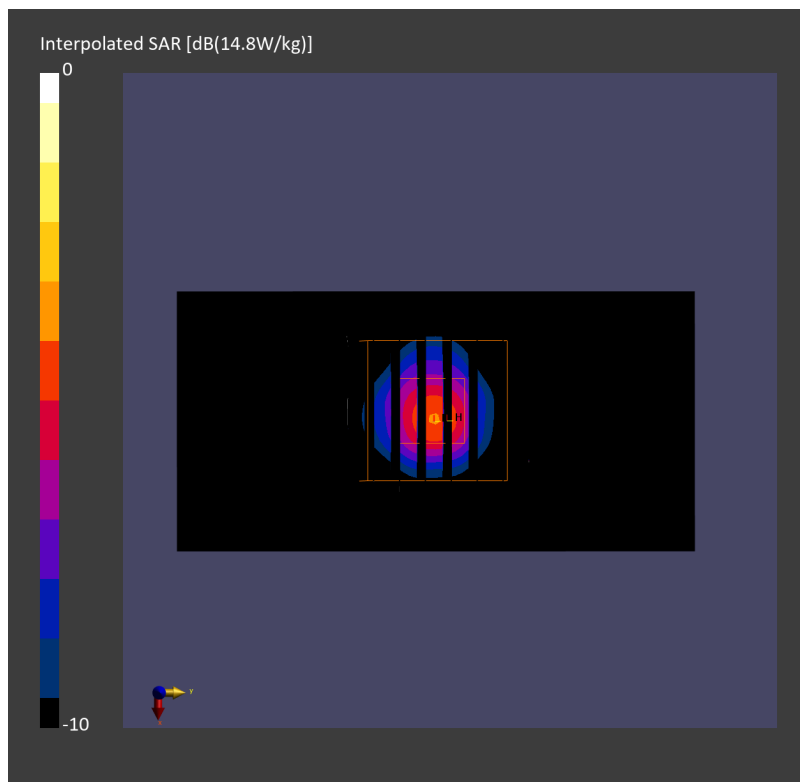

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260324 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.30$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.98, 5.82, 5.82); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 0.954 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.09 dB

SAR (1g) = 3.58 W/kg; SAR (8g) = 1.24 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 6.8 mm

Ratio of SAR at M2 to SAR at M1 = 54.9 %

TSL Correction: Positive only

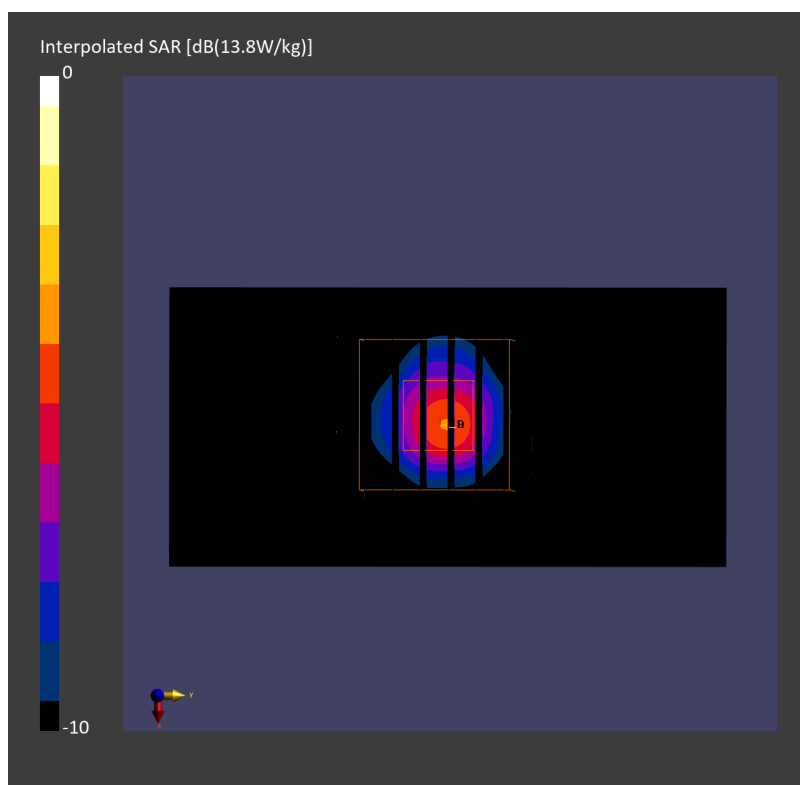

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260325 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.81$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.98, 5.82, 5.82); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.71 W/kg; SAR (10g) = 1.07 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.14 dB

SAR (1g) = 3.88 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 6.8 mm

Ratio of SAR at M2 to SAR at M1 = 72.3 %

TSL Correction: Positive only

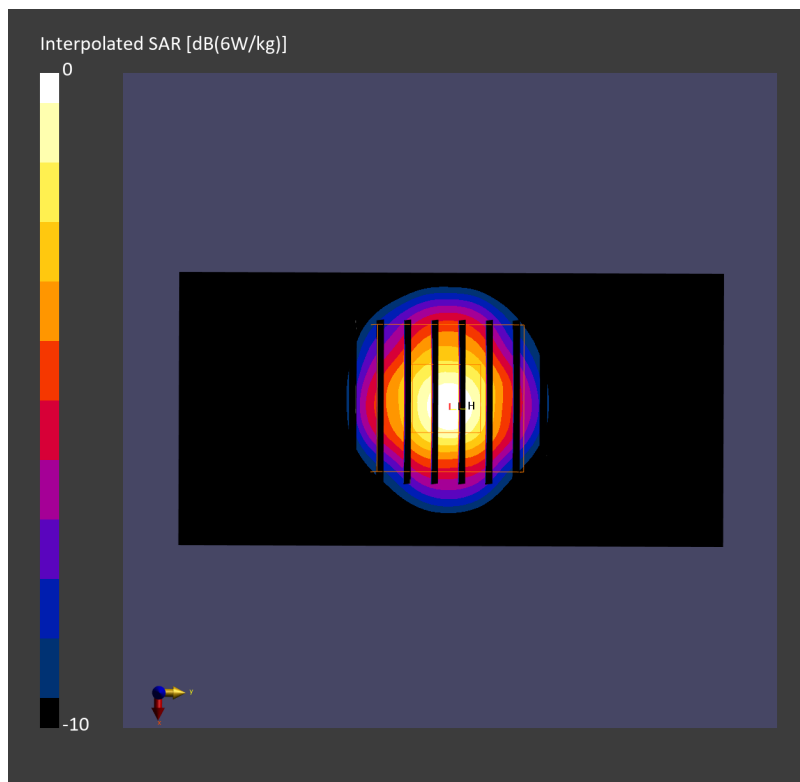

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260327 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.65$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.53, 4.1, 5.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.40 W/kg; SAR (10g) = 0.993 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.66 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 67.1 %

TSL Correction: Positive only

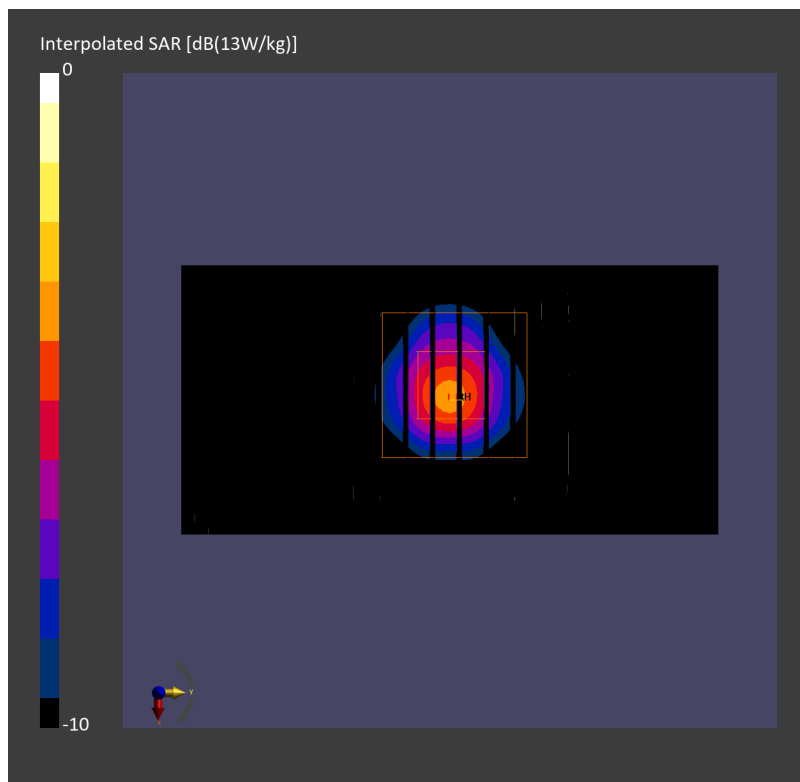

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260327 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.65$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.98, 5.82, 5.82); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.58 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.75 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.4 %

TSL Correction: Positive only

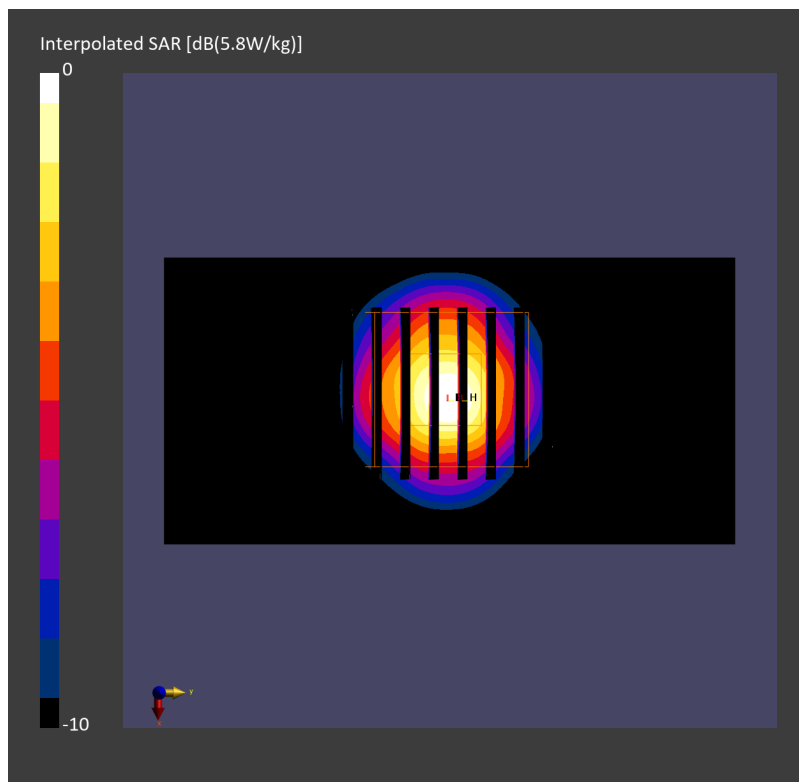

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260329 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.63$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.53, 4.1, 5.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.48 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (32.0 mm x 36.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.72 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 67.0 %

TSL Correction: Positive only

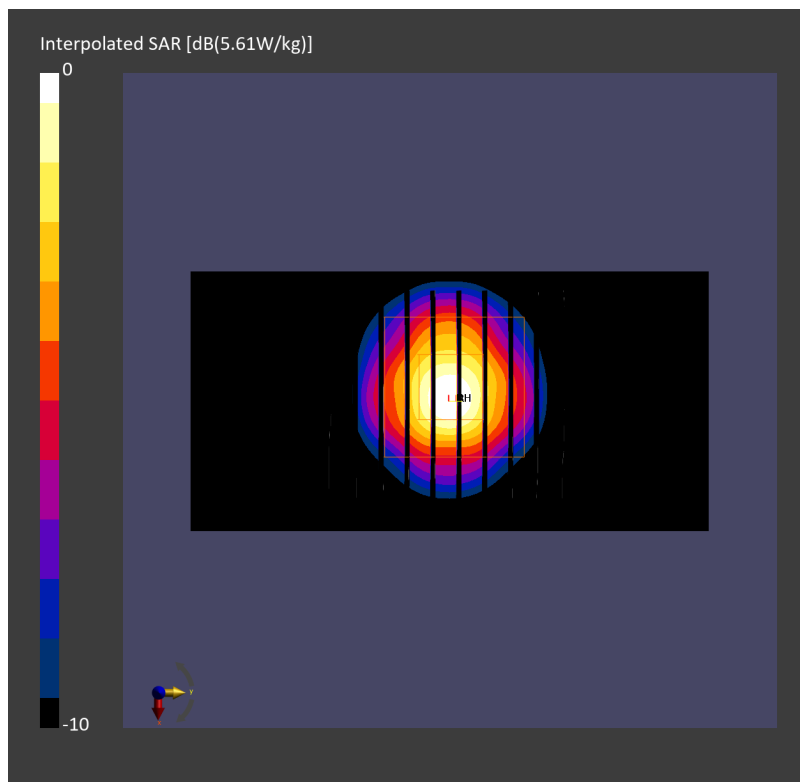

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260329 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.63$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.98, 5.82, 5.82); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.56 W/kg; SAR (10g) = 1.02 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.73 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.4 %

TSL Correction: Positive only

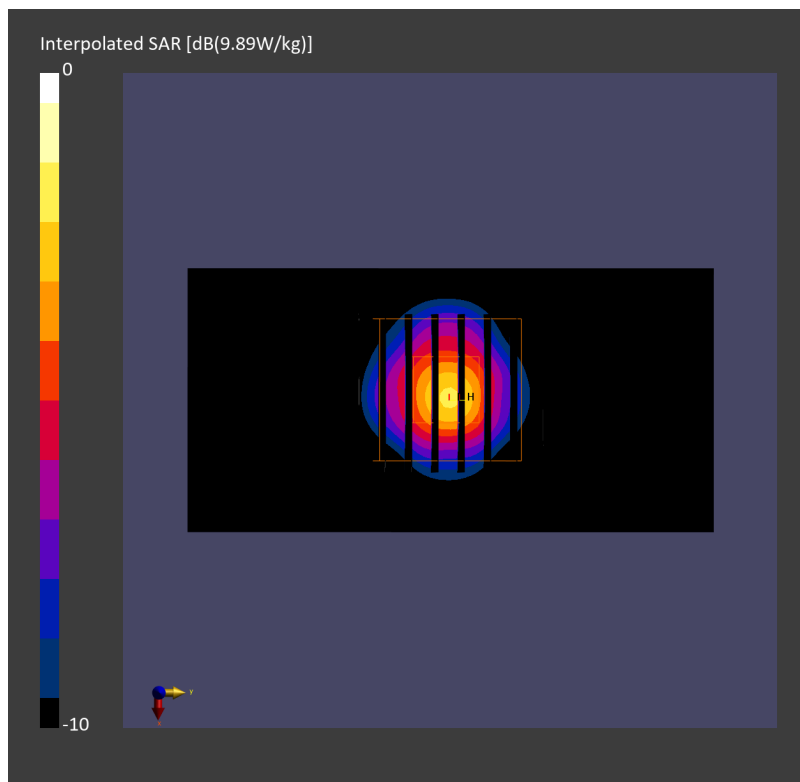

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260401 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.64$ S/m; $\epsilon_r = 35.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.53, 4.1, 5.21); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.48 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 3.71 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 67.2 %

TSL Correction: Positive only

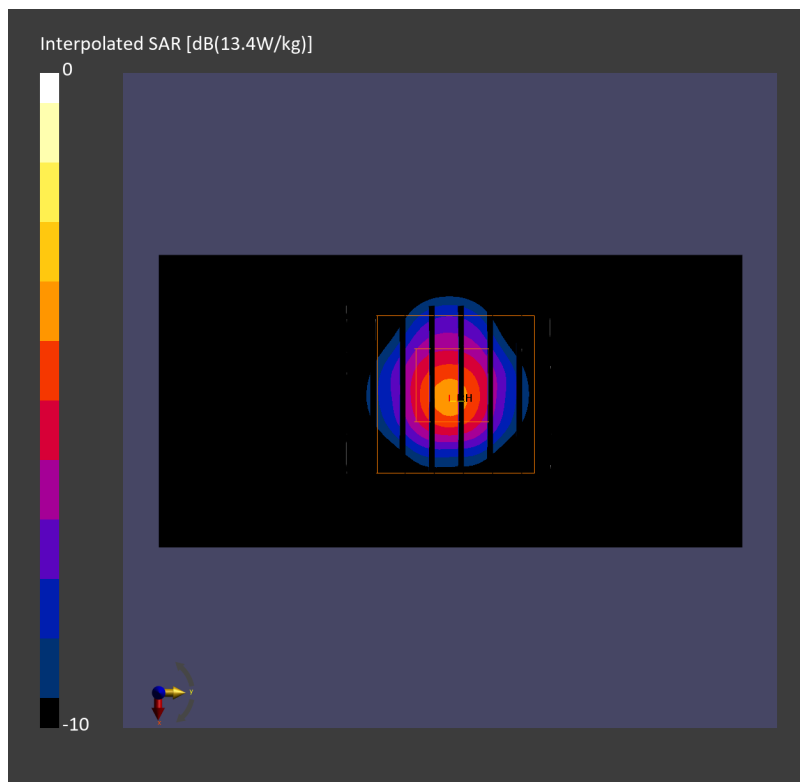

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260321 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.99$ S/m; $\epsilon_r = 34.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.3, 5.15, 5.15); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.06 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 4.24 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 61.2 %

TSL Correction: Positive only

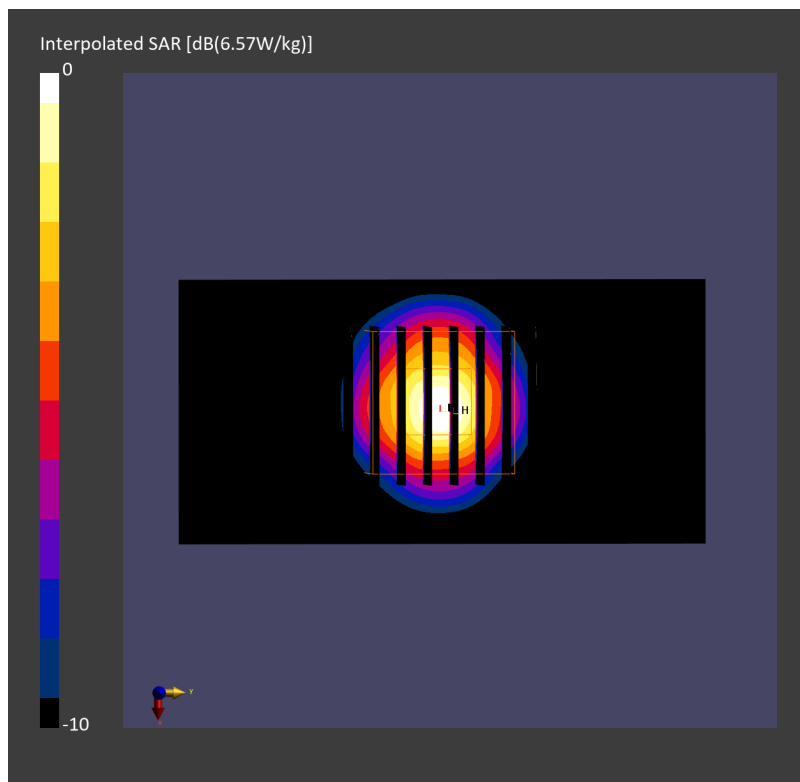

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260324 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.69$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.3, 5.15, 5.15); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.86 W/kg; SAR (10g) = 1.09 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.18 dB

SAR (1g) = 4.03 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 6.9 mm

Ratio of SAR at M2 to SAR at M1 = 56.1 %

TSL Correction: Positive only

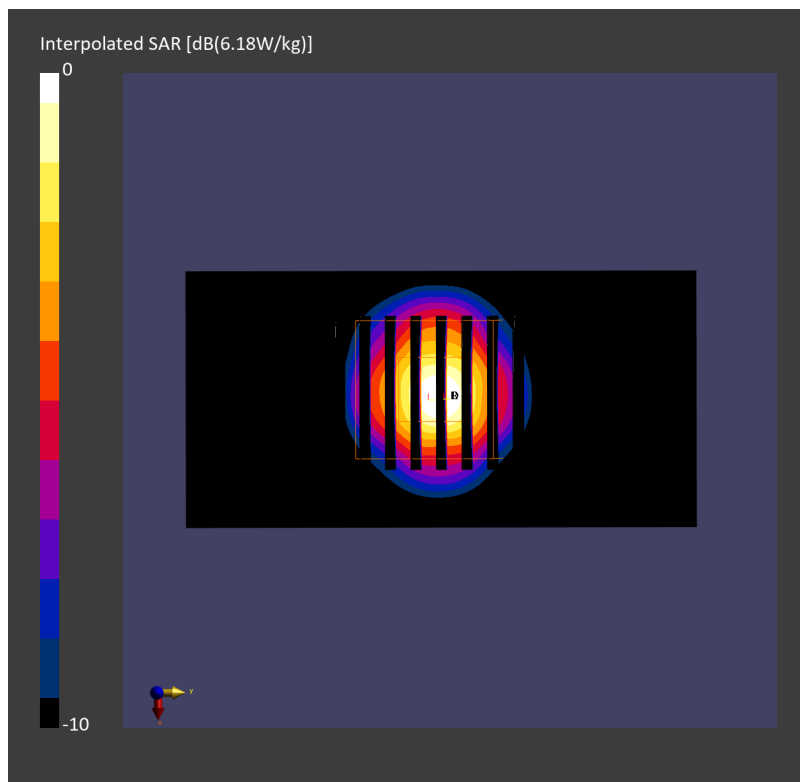

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260325 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.23$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.3, 5.15, 5.15); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.31 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.18 dB

SAR (1g) = 4.47 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 6.6 mm

Ratio of SAR at M2 to SAR at M1 = 59.4 %

TSL Correction: Positive only

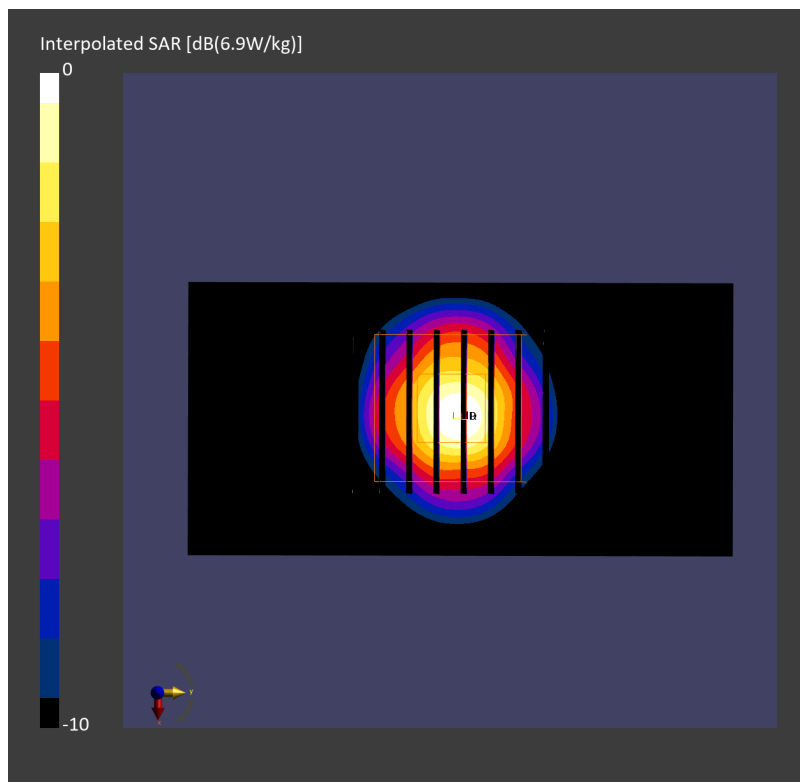

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260327 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.05$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.36, 3.94, 5.02); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.71 W/kg; SAR (10g) = 1.06 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 4.01 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 63.9 %

TSL Correction: Positive only

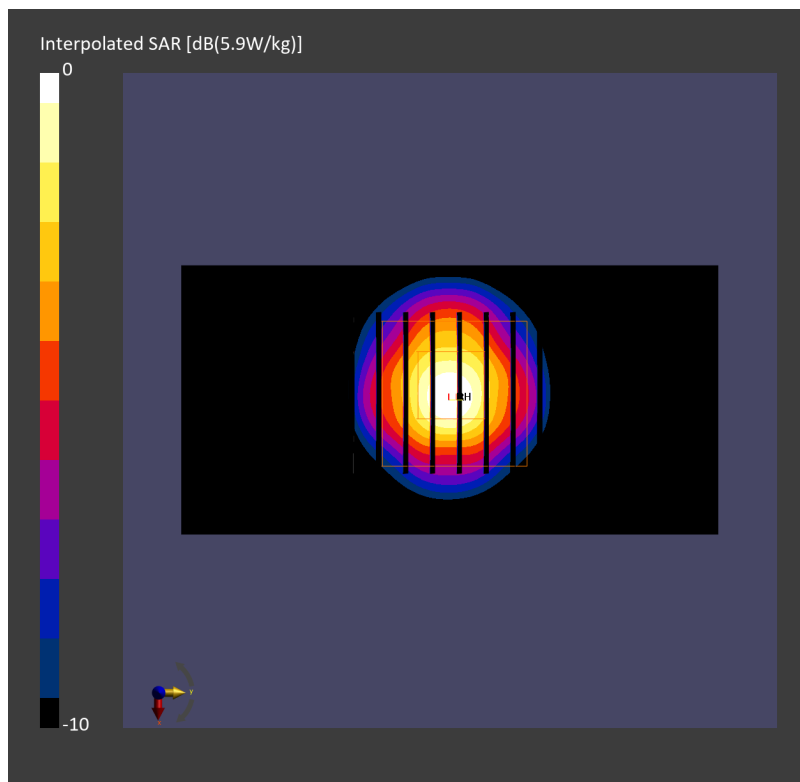

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260327 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.05$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.3, 5.15, 5.15); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.81 W/kg; SAR (10g) = 1.08 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 4.01 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 60.2 %

TSL Correction: Positive only

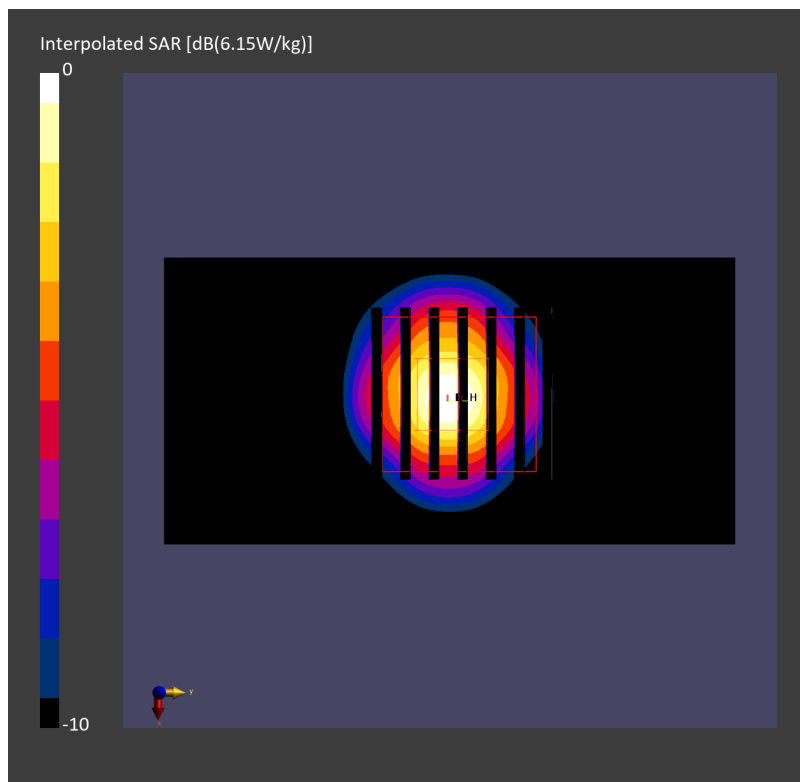

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260329 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.03$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.36, 3.94, 5.02); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.74 W/kg; SAR (10g) = 1.07 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 4.00 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 64.0 %

TSL Correction: Positive only

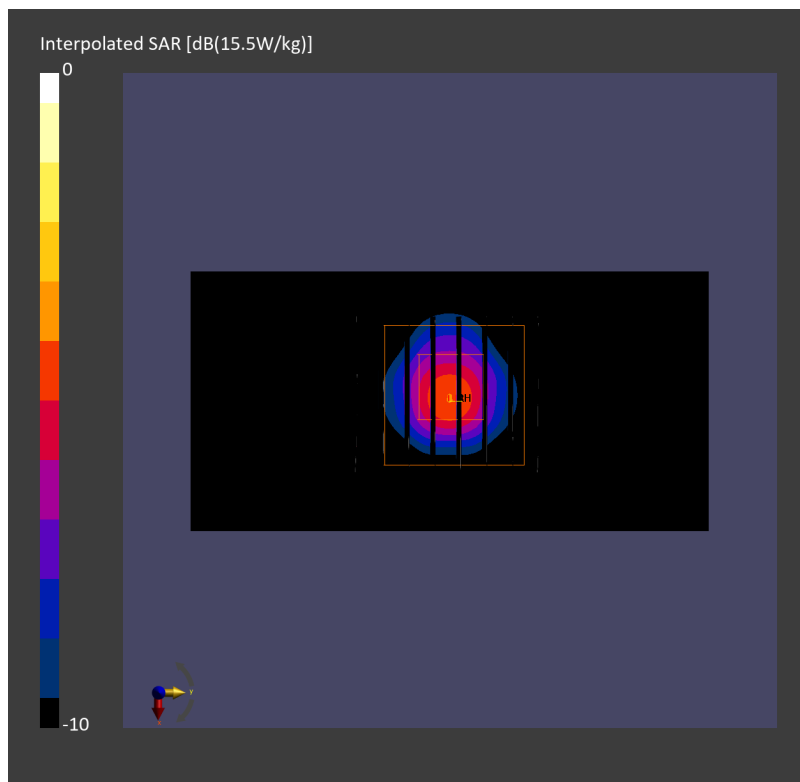

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260329 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.03$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.3, 5.15, 5.15); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.61 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.91 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 60.1 %

TSL Correction: Positive only

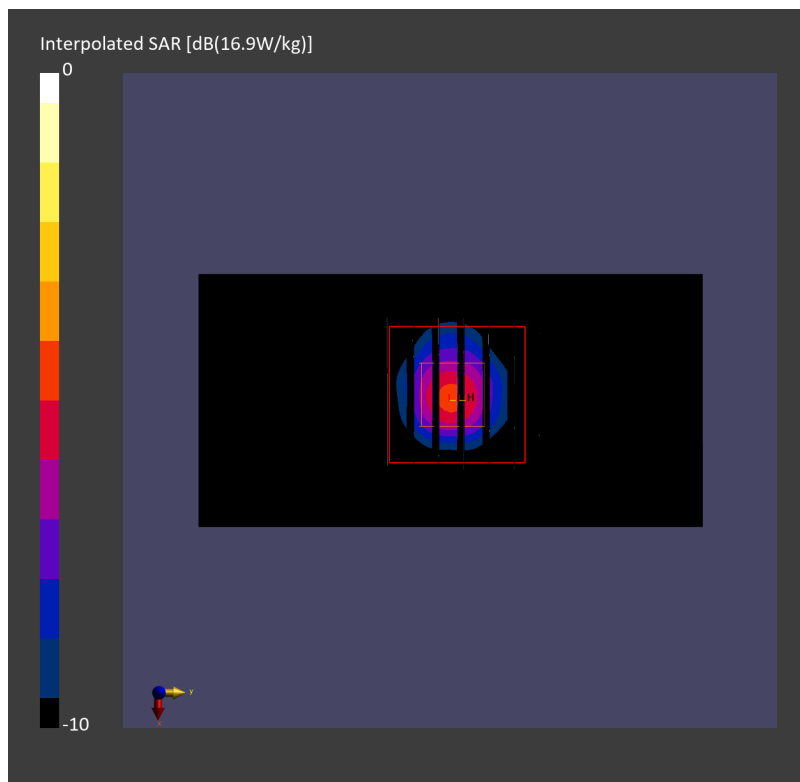

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260401 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.03$ S/m; $\epsilon_r = 34.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.36, 3.94, 5.02); Calibrated: 2025-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149_GAP; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.75 W/kg; SAR (10g) = 1.07 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 28.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 4.04 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.4 %

TSL Correction: Positive only

