

PCTEST Engineering Lab.

SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC


FCC 15.247

POWER OUT C-91

Operating Frequency: 2479.680 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

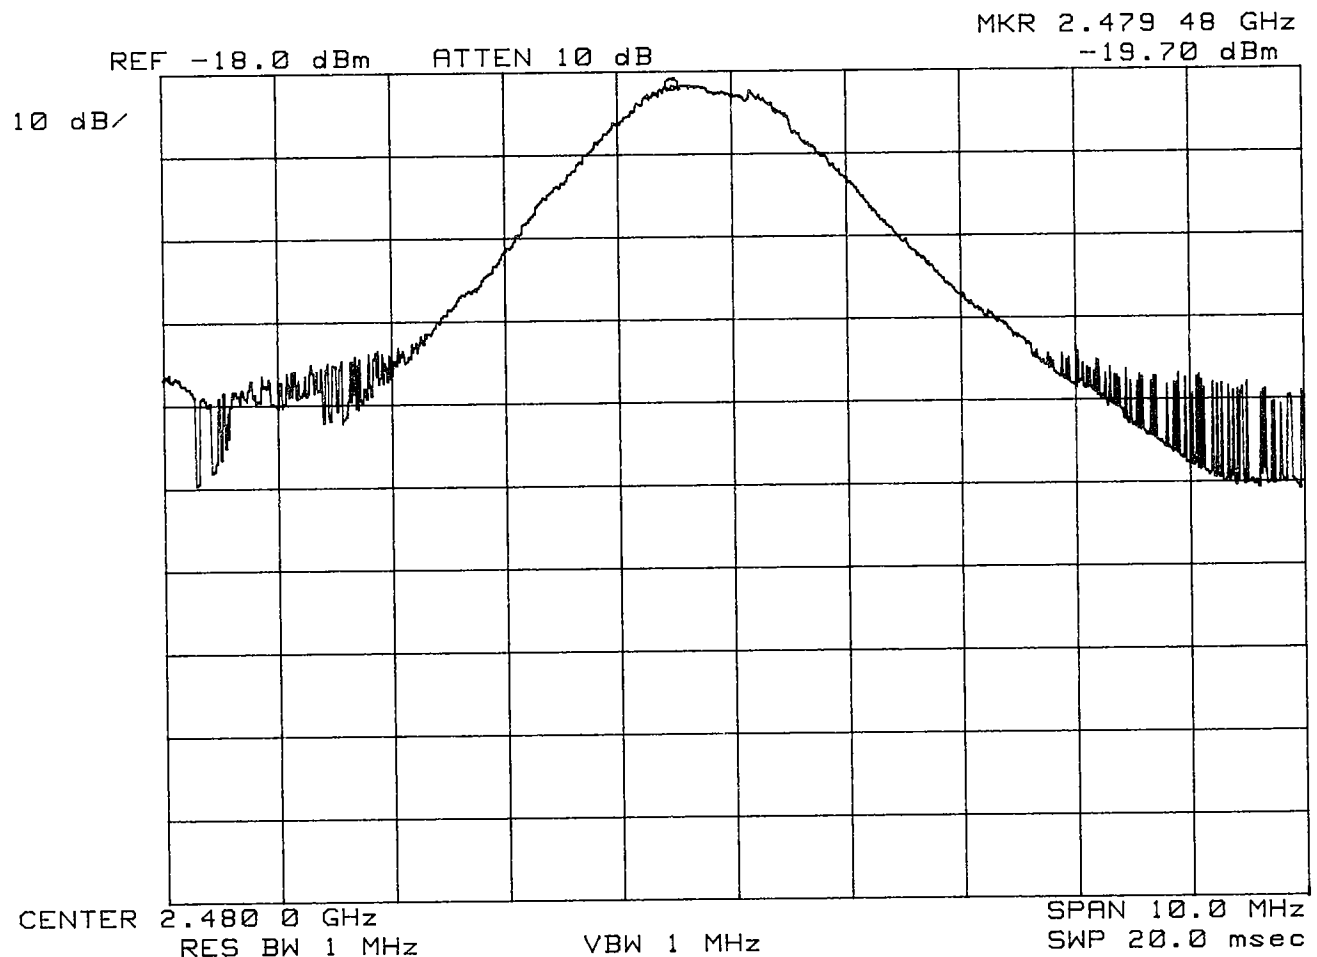

PCTEST Engineering Lab.

SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC HANDSET


FCC 15.247

POWER OUT C-46

Operating Frequency: 2440.800 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

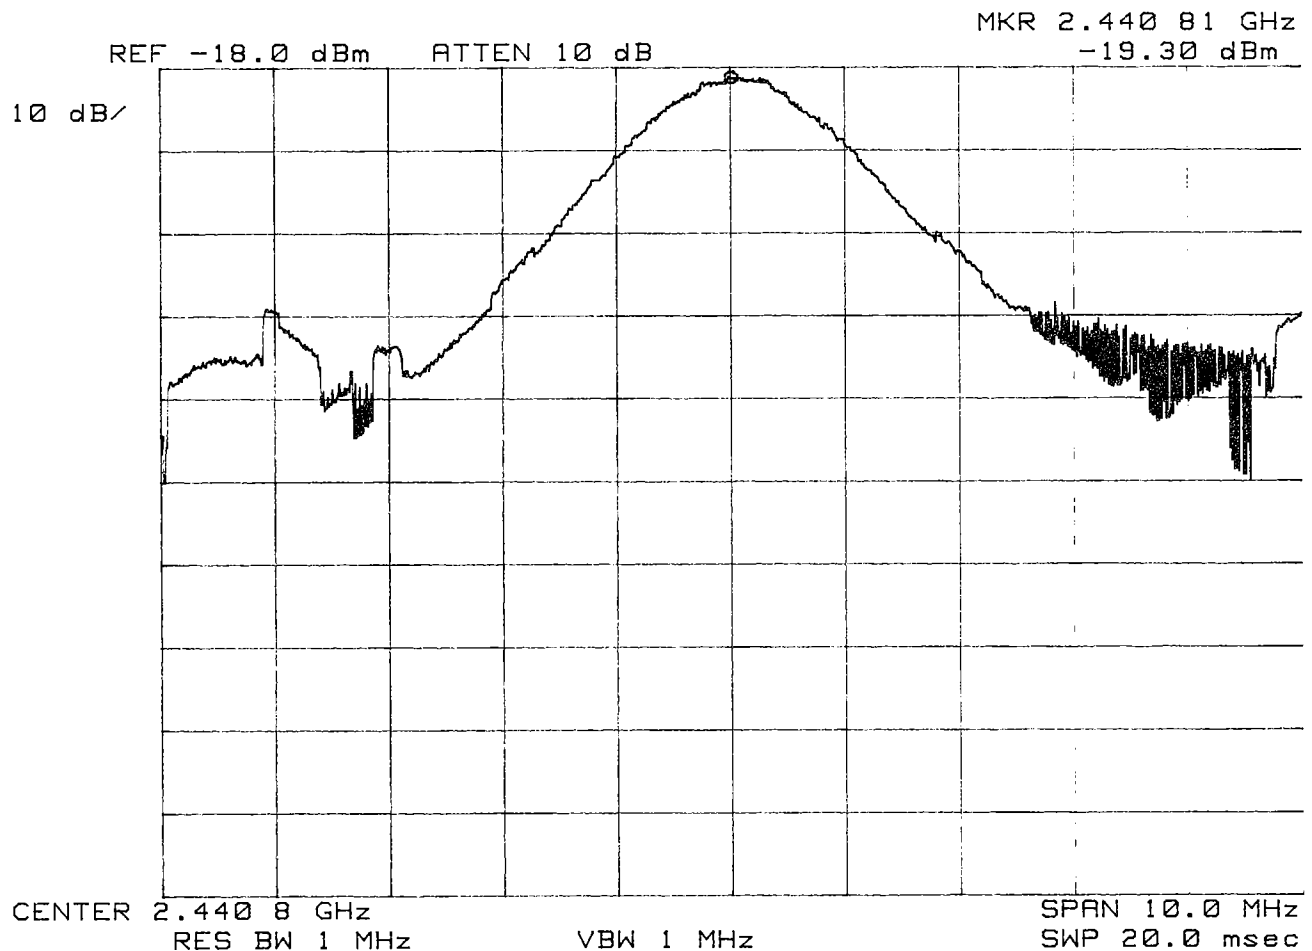

PCTEST Engineering Lab.

SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC HANDSET


FCC 15.247

POWER OUT C-01

Operating Frequency: 2401.056 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

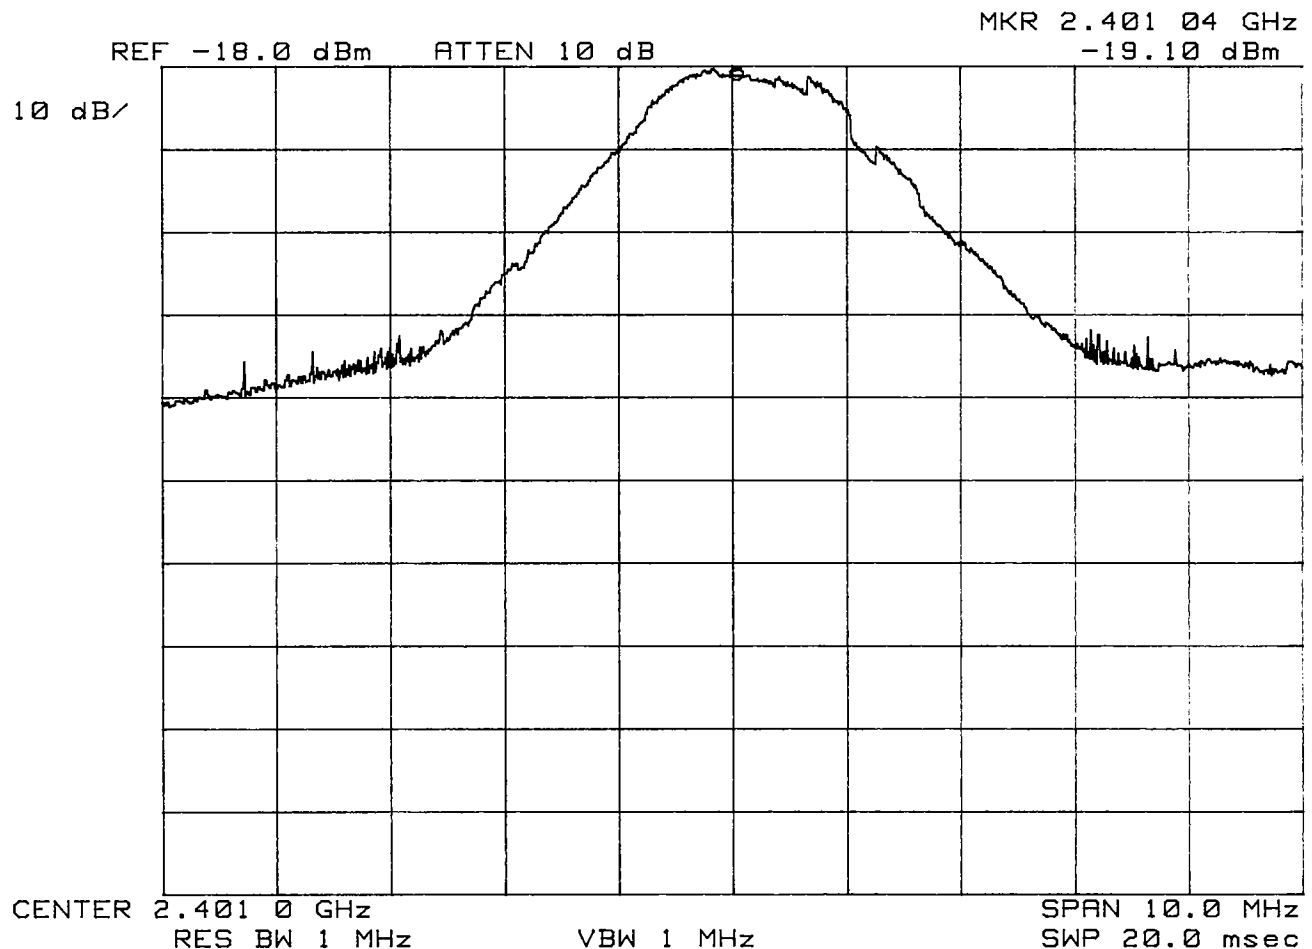

PCTEST Engineering Lab.

SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC


FCC 15.247

BAND EDGE C-1

Operating Frequency: 2401.056 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

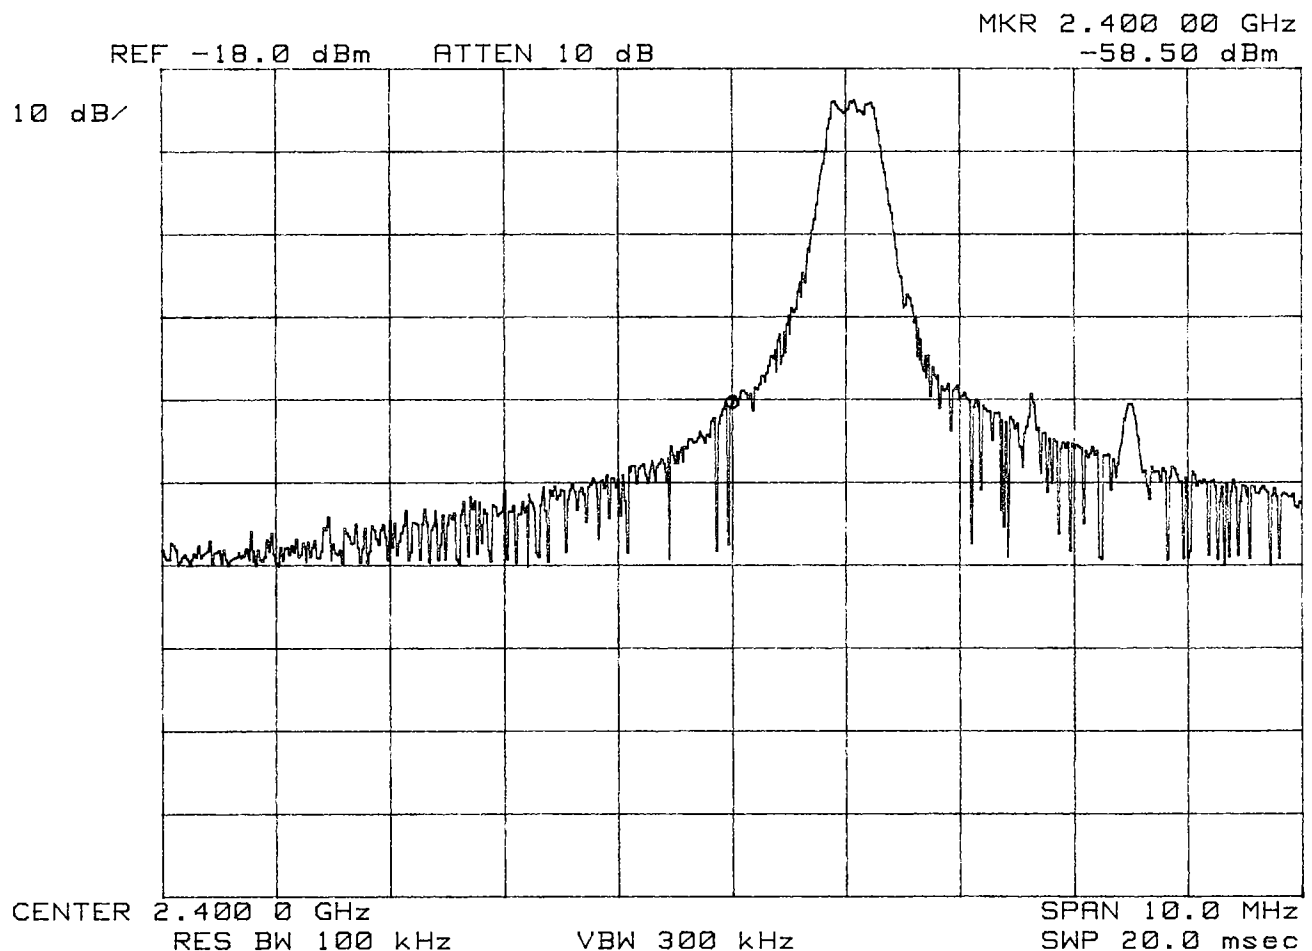

PCTEST Engineering Lab.

SPECTRUM ANALYZER PRESENTATION

FCC ID:ACJ96NKX-TD7680

PANASONIC


FCC 15.247

BAND EDGE C-91


Operating Frequency: 2479.680 MHz

Output Power : -20.0 dBm

Test Mode:Other Transmitter

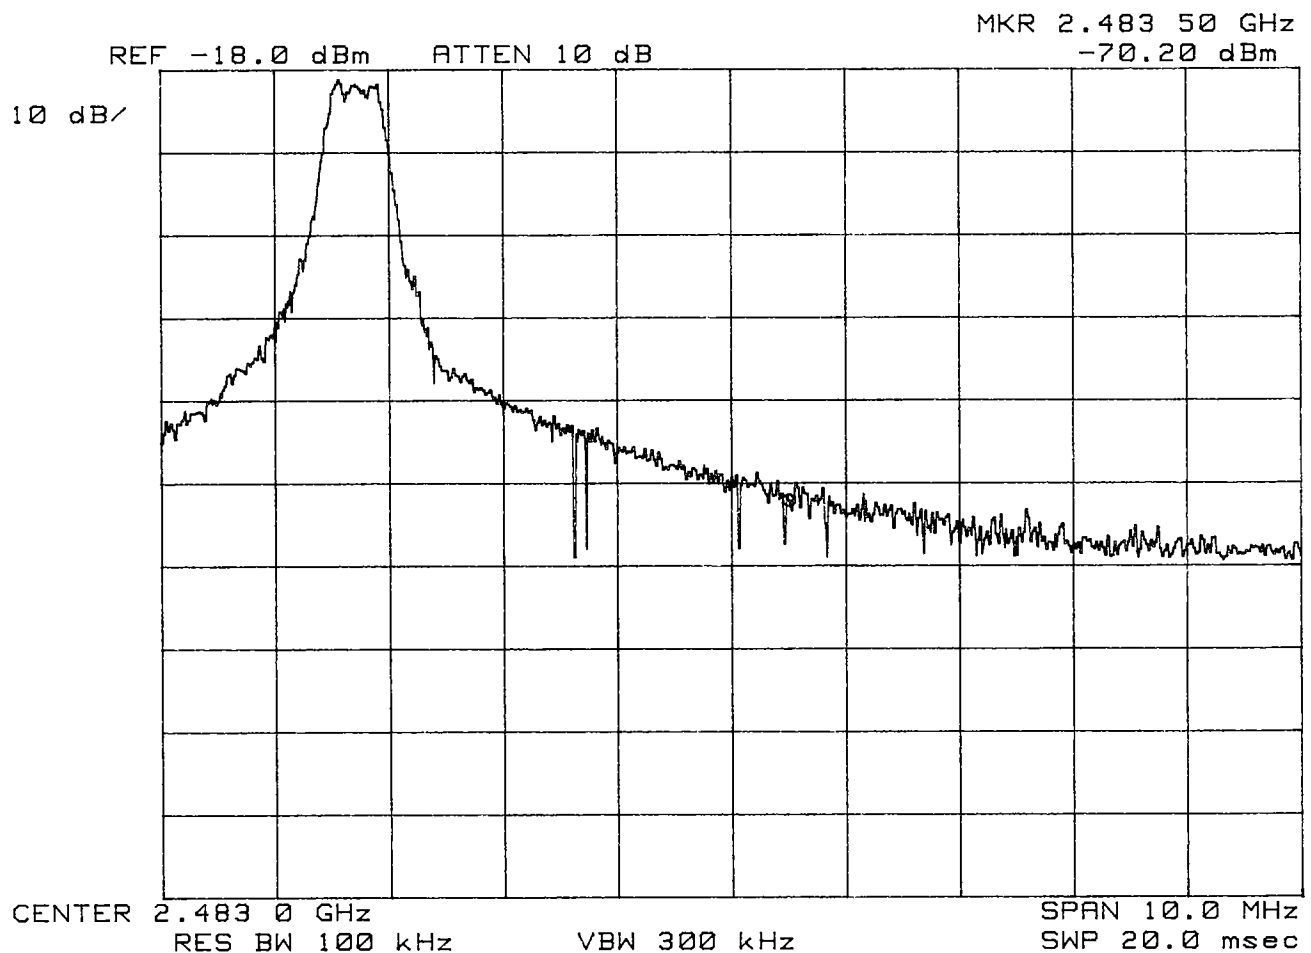

✳ Agilent

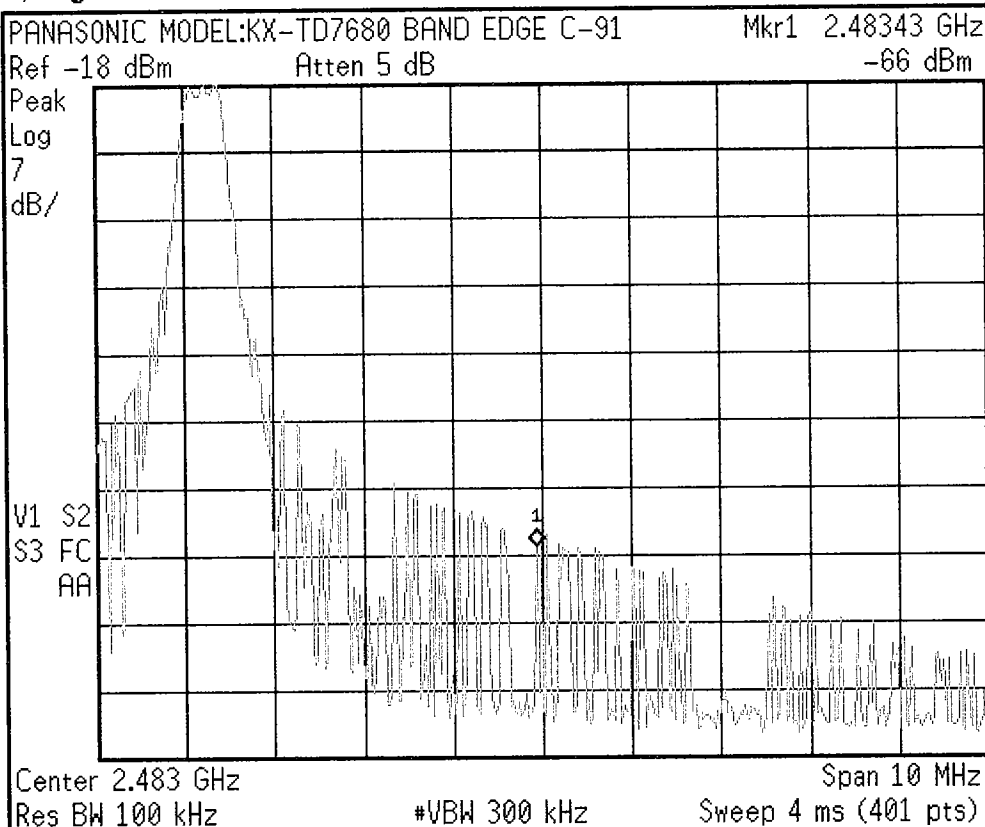

Freq/Channel

Center Freq
 2.48350000 GHz

Start Freq
 2.47850000 GHz

Stop Freq
 2.48850000 GHz


CF Step
 1.00000000 MHz
 Auto Man

Freq Offset
 0.00000000 Hz

Signal Track
 On Off

Scale Type
 Log Lin

✳ Agilent

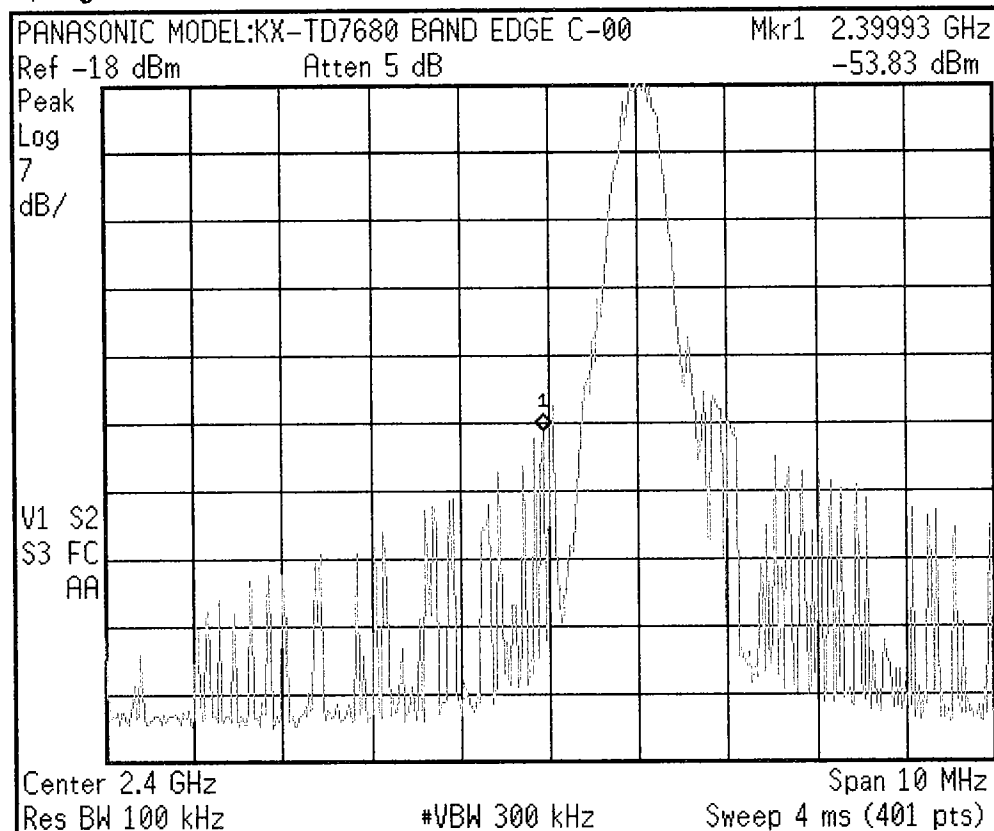

Freq/Channel

Center Freq
 2.40000000 GHz

Start Freq
 2.39500000 GHz

Stop Freq
 2.40500000 GHz


CF Step
 1.00000000 MHz
 Auto Man

Freq Offset
 0.00000000 Hz

Signal Track
 On Off

Scale Type
 Log Lin

Agilent

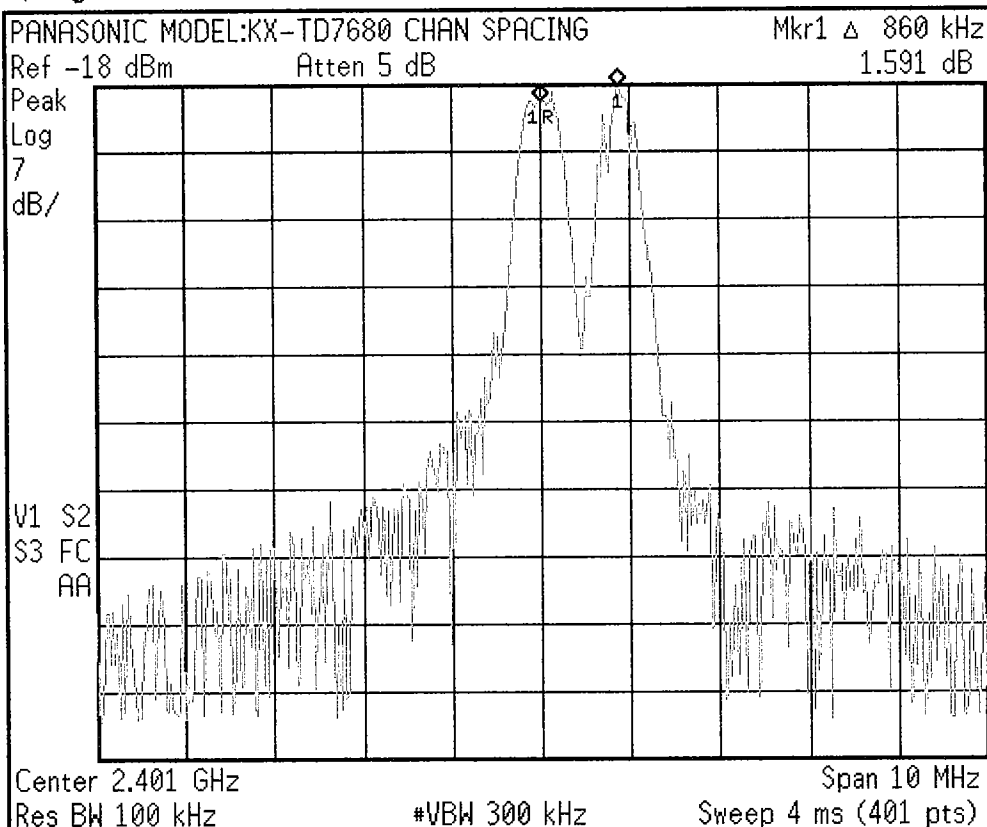

Freq/Channel

Center Freq
 2.40100000 GHz

Start Freq
 2.39600000 GHz

Stop Freq
 2.40600000 GHz


CF Step
 1.00000000 MHz
 Auto Man

Freq Offset
 0.00000000 Hz

Signal Track
 On Off

Scale Type
 Log Lin

Agilent

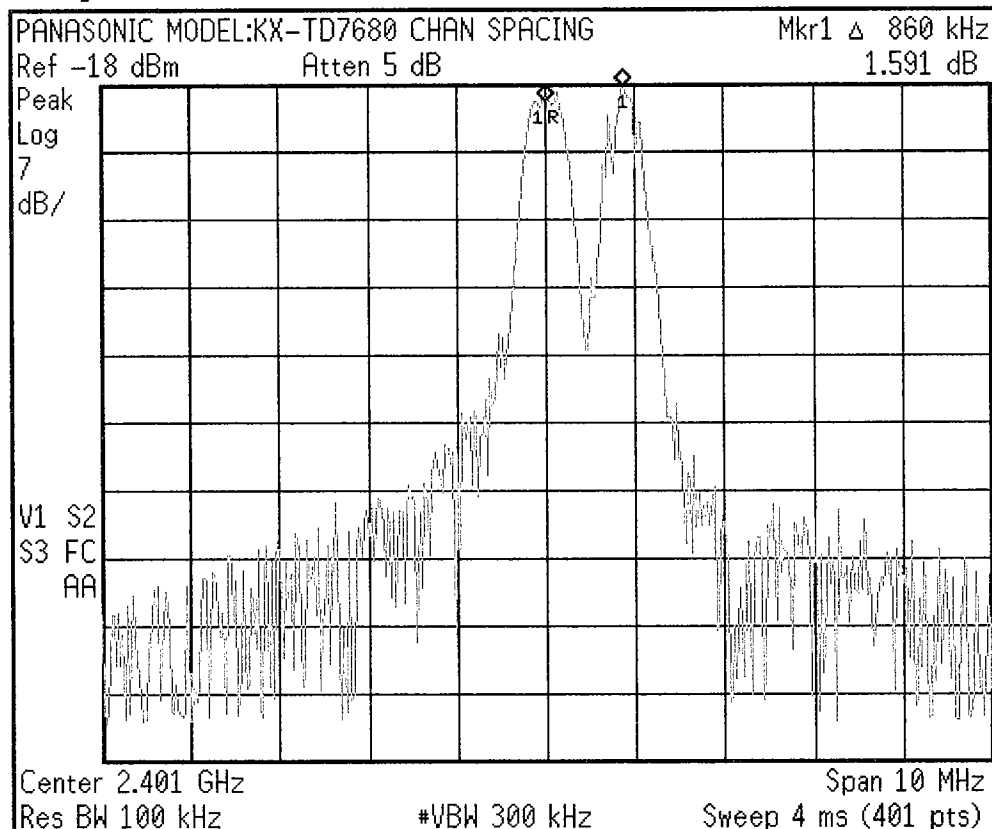

Marker

Select Marker
 1 2 3 4

Normal

Delta


Delta Pair
 (Tracking Ref)
 Ref Delta

Span Pair
 Span Center

Off

More
 1 of 2

Agilent

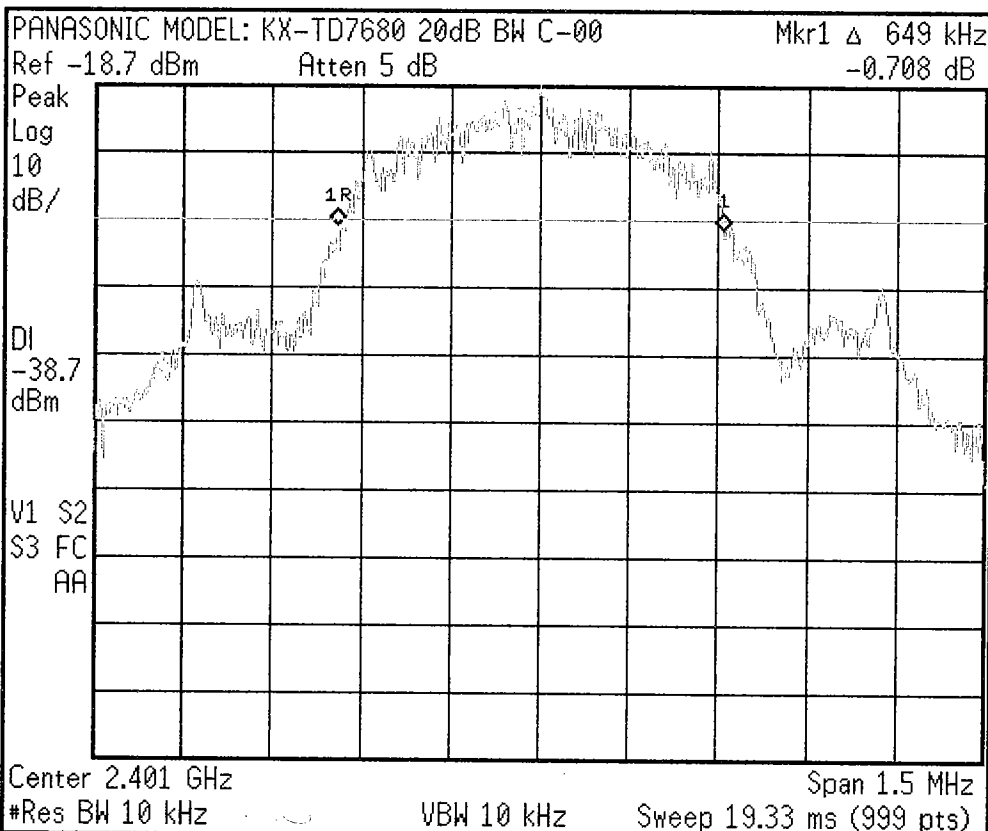

Freq/Channel

Center Freq

2.40101700 GHz

Start Freq

2.40026700 GHz

Stop Freq

2.40176700 GHz

CF Step

150.000000 kHz

Auto Man

Freq Offset

0.00000000 Hz


Signal Track

On Off

Scale Type

Log Lin

Agilent

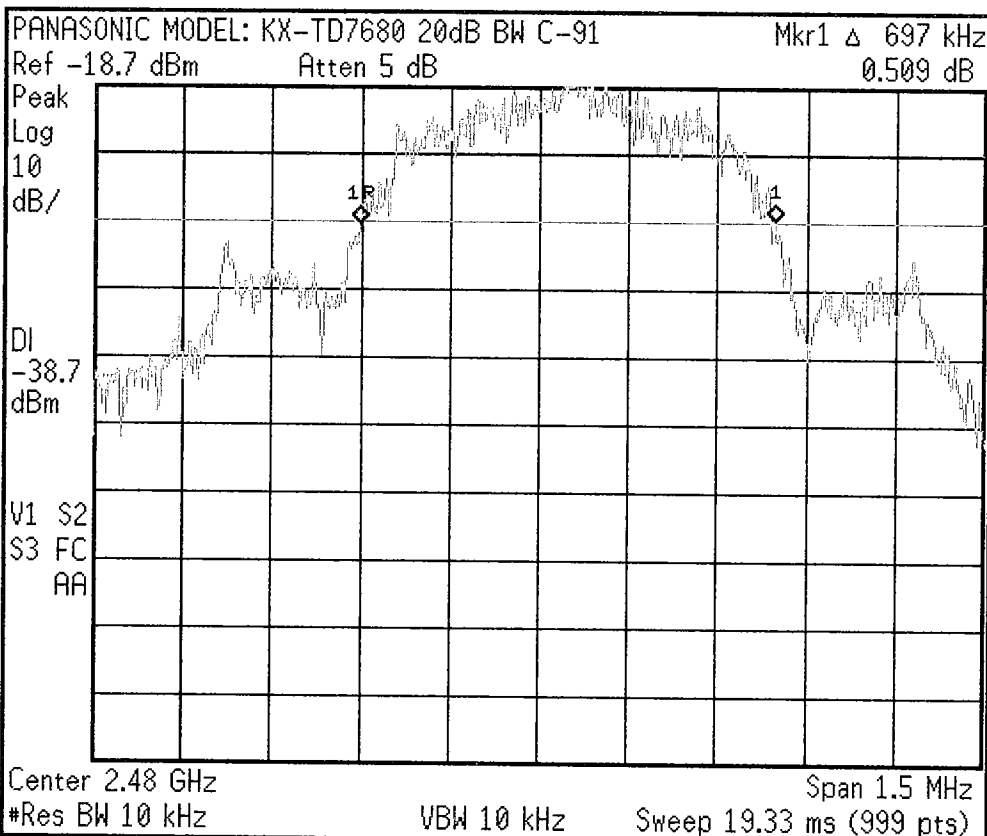

Freq/Channel

Center Freq

2.47968000 GHz

Start Freq

2.47893000 GHz

Stop Freq

2.48043000 GHz

CF Step

150.000000 kHz

Auto Man

Freq Offset

0.00000000 Hz


Signal Track

On Off

Scale Type

Log Lin

Agilent

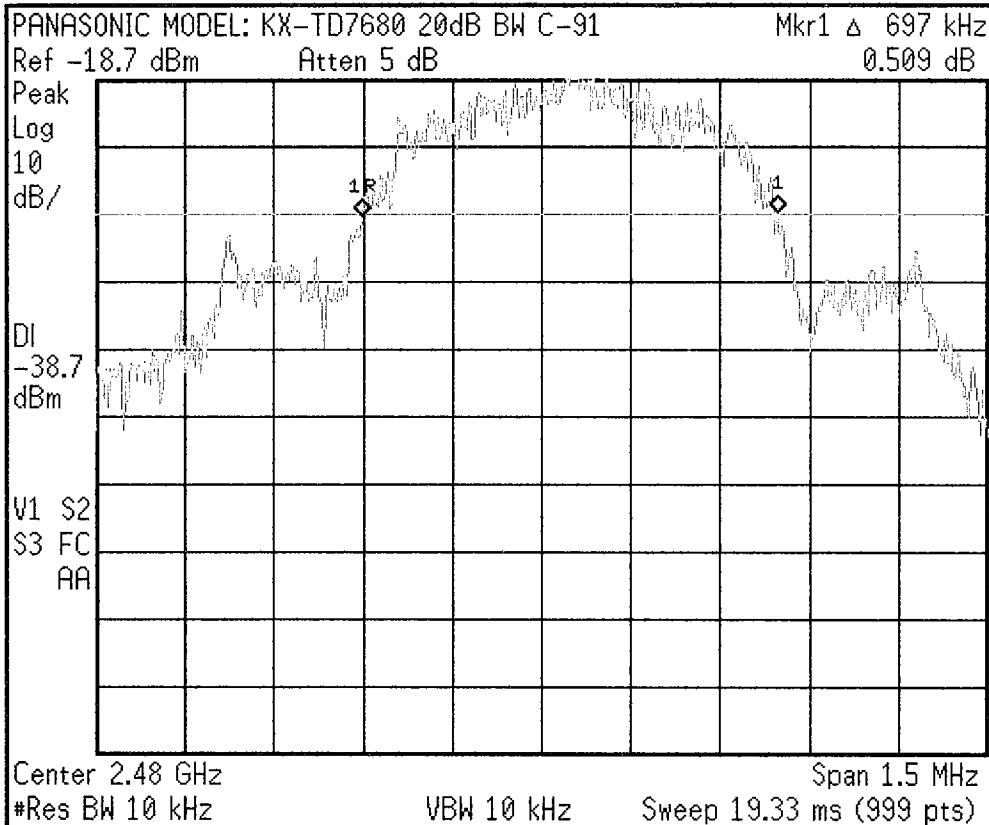

Freq/Channel

Center Freq

2.47968000 GHz

Start Freq

2.47893000 GHz

Stop Freq

2.48043000 GHz

CF Step

150.000000 kHz

Auto

Man

Freq Offset

0.00000000 Hz

Signal Track

On


Off

Scale Type

Log

Lin

Agilent

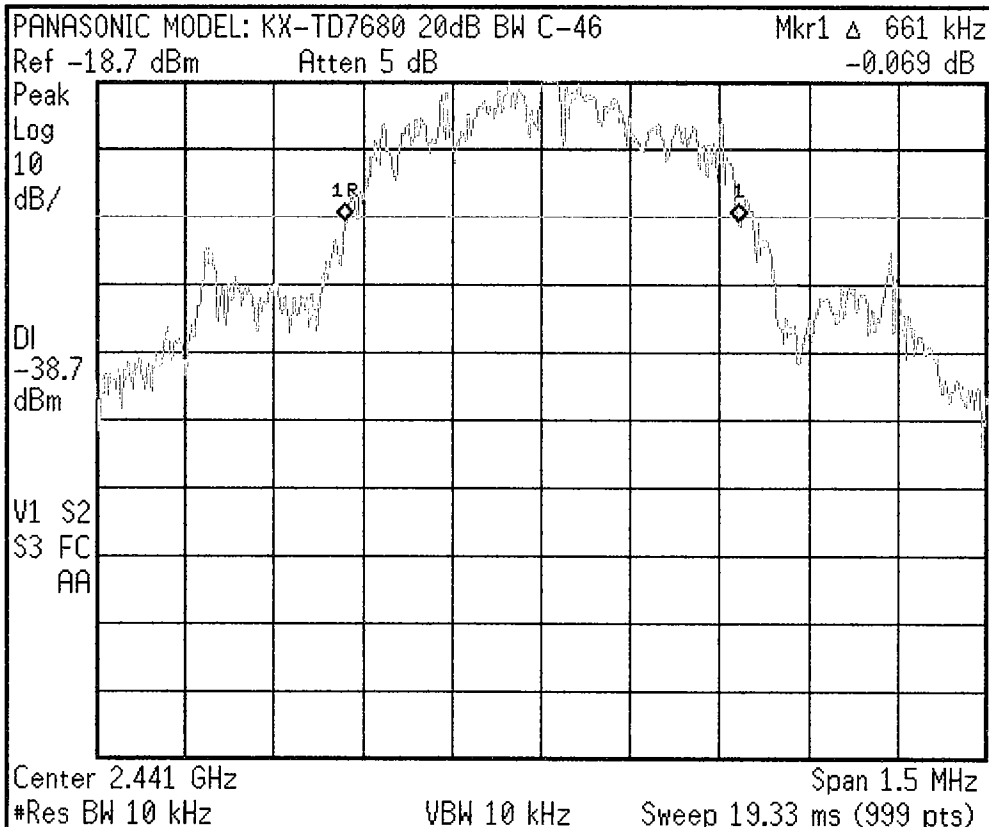

Freq/Channel

Center Freq

2.44080000 GHz

Start Freq

2.44005000 GHz

Stop Freq

2.44155000 GHz

CF Step

150.000000 kHz

Auto

Man

Freq Offset

0.00000000 Hz

Signal Track

On


Off

Scale Type

Log


Lin

* Agilent

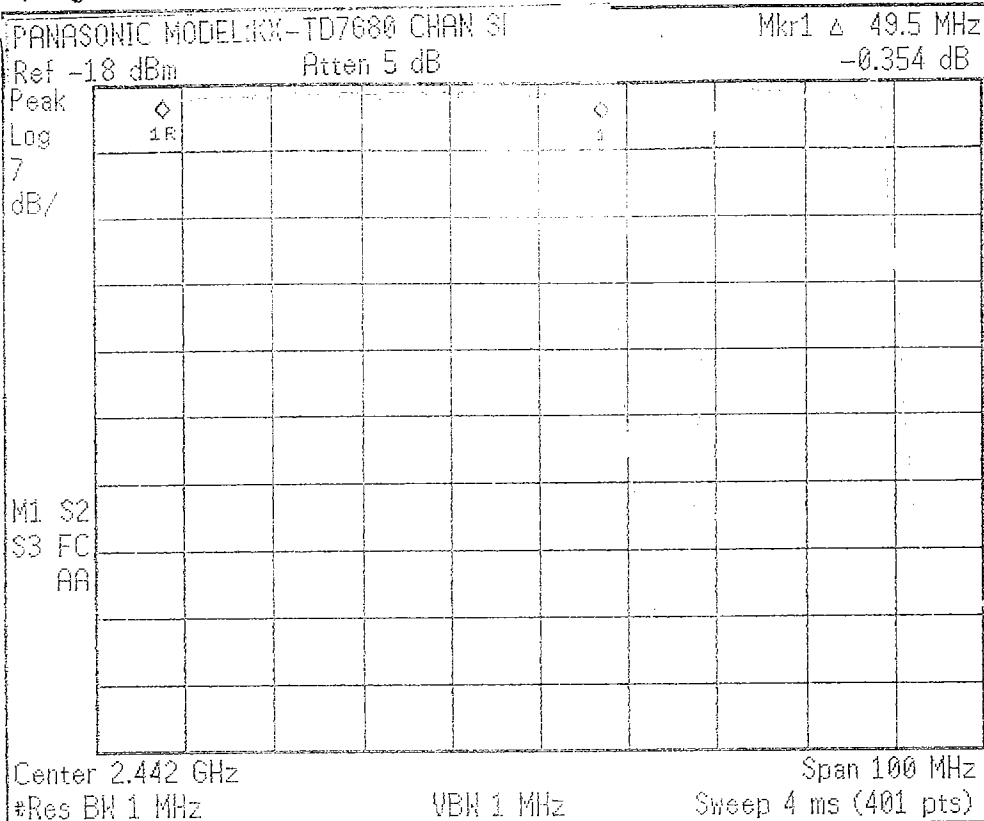

Marker			
Select Marker			
1	2	3	4
Normal			
Delta			
Delta Pair (Tracking Ref)			
Ref	Delta		
Span Pair			
Span	Center		
Off			
More 1 of 2			

* Agilent

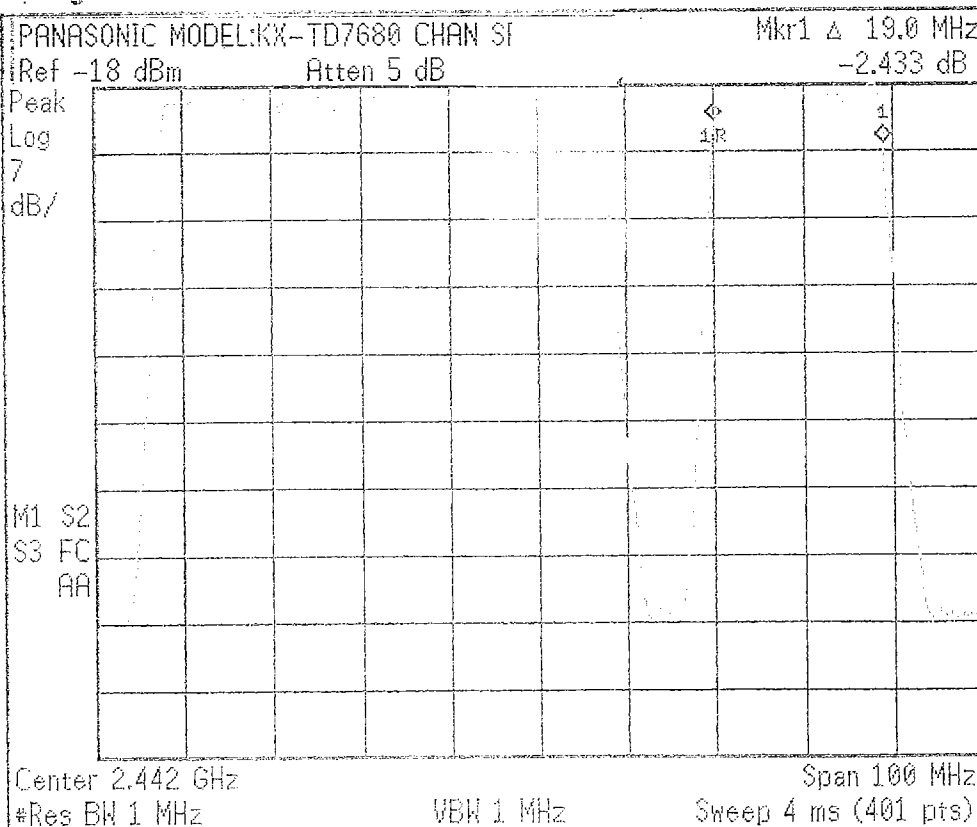

Marker			
Select Marker			
1	2	3	4
Normal			
Delta			
Delta Pair (Tracking Ref)			
Ref	Delta		
Span Pair			
Span	Center		
Off			
More 1 of 2			