

Date: 2025-11-07

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-10000_251107 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.52, 6.42, 6.64); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2025-05-06
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.65 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

TSL Correction: Positive only

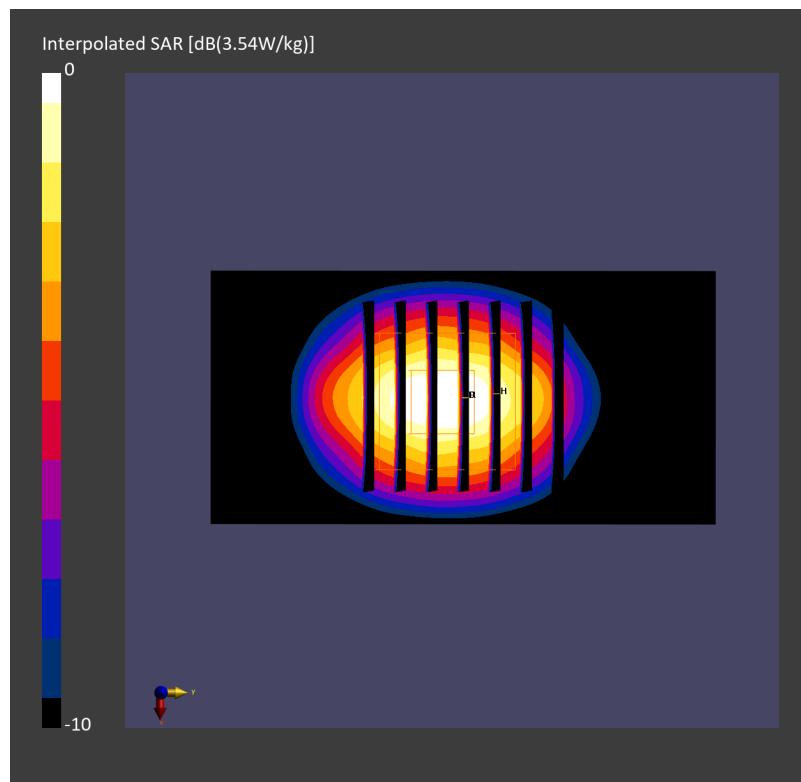

Date: 2025-11-08

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-10000_251108 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.73$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.22, 6.13, 6.33); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2025-05-06
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.02 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.03 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.2 %

TSL Correction: Positive only

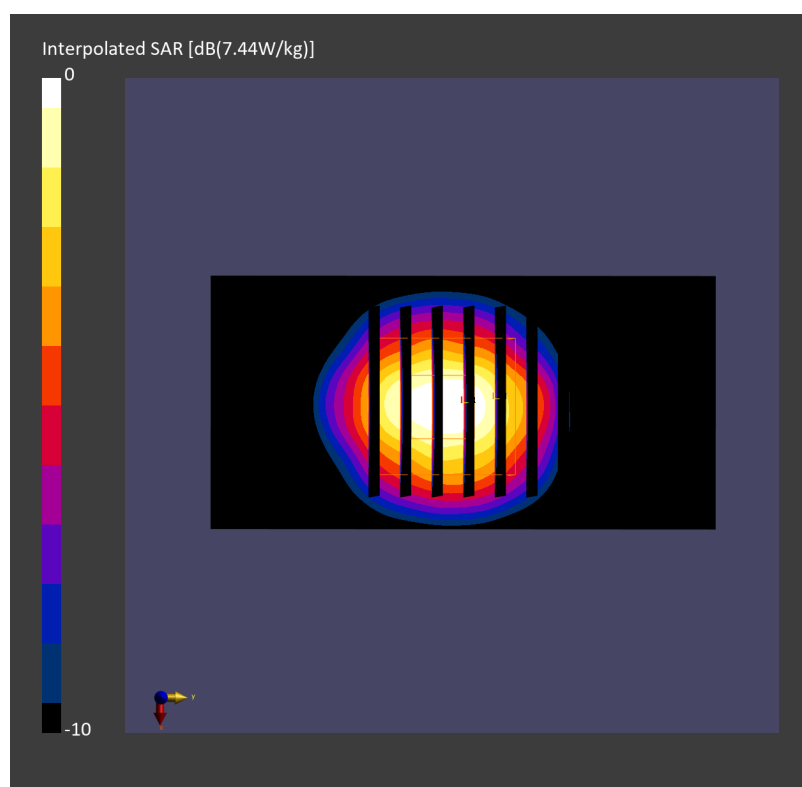

Date: 2025-11-09

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-10000_251109 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.72$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.42, 6.39, 6.83); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.39 W/kg; SAR (10g) = 2.60 W/kg;

TSL Correction: No correction

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.68 W/kg; SAR (8g) = 2.91 W/kg; SAR (10g) = 2.58 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.3 %

TSL Correction: No correction

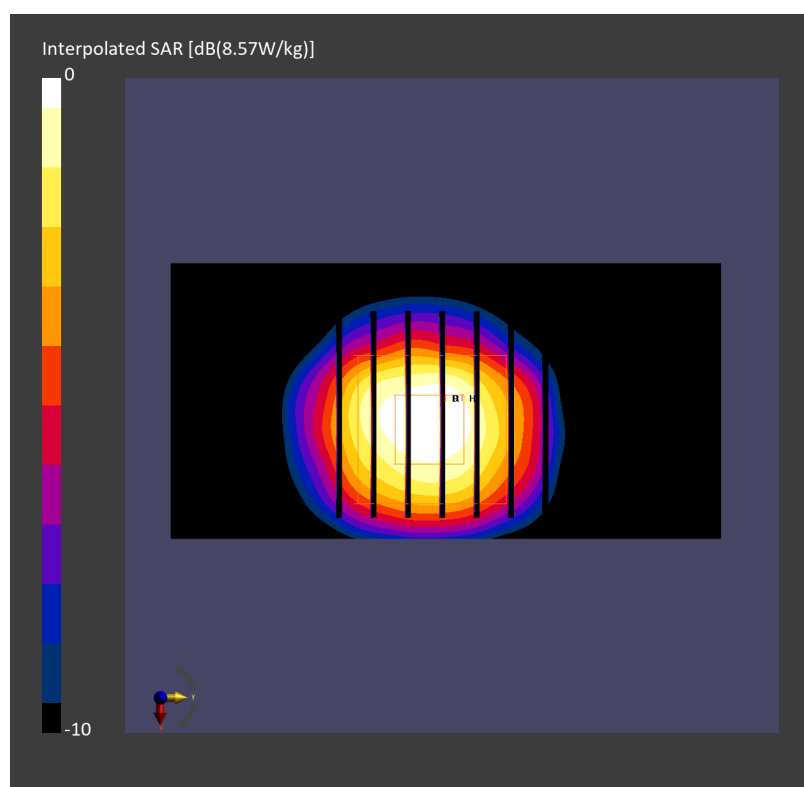

Date: 2025-11-08

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-10000_251108 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.14, 6.04, 6.25); Calibrated: 2025-03-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2025-05-06
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.03 dB

SAR (1g) = 3.21 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

TSL Correction: Positive only

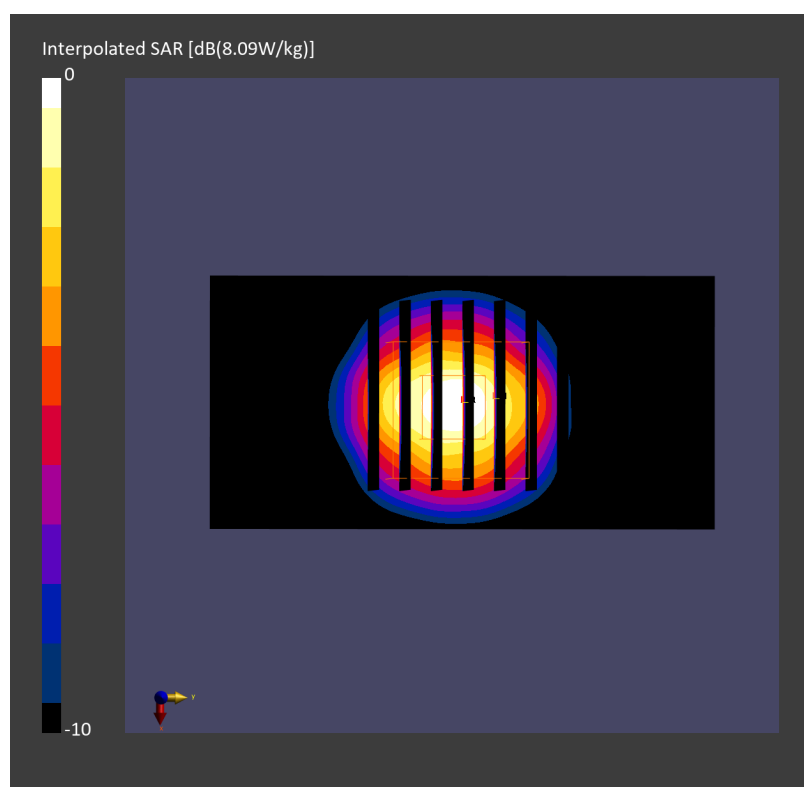

Date: 2025-11-09

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-10000_251109 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.90$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.36, 6.33, 6.77); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.73 W/kg; SAR (10g) = 2.56 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 7.01 W/kg; SAR (8g) = 2.93 W/kg; SAR (10g) = 2.59 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.0 %

TSL Correction: Positive only

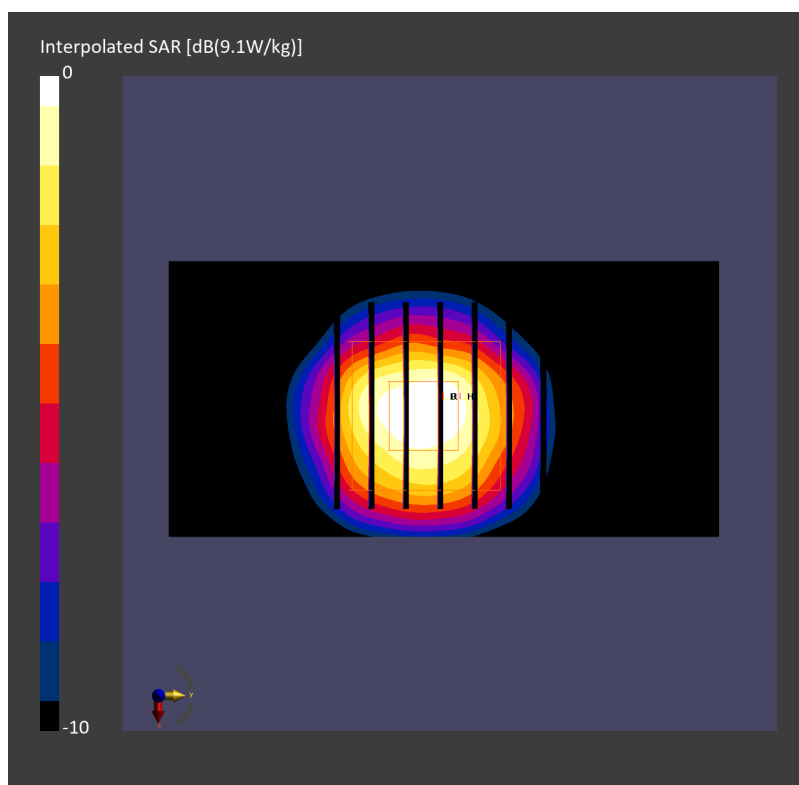

Date: 2025-11-09

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-10000_251109 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.07$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.37, 6.34, 6.78); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2024-12-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.39 W/kg; SAR (10g) = 2.30 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 6.62 W/kg; SAR (8g) = 2.66 W/kg; SAR (10g) = 2.33 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

TSL Correction: Positive only

