

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.850$ S/m; $\epsilon_r = 43.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.98, 9.68, 9.75); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.41 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.12 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.40 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 89.2 %

TSL Correction: Positive only

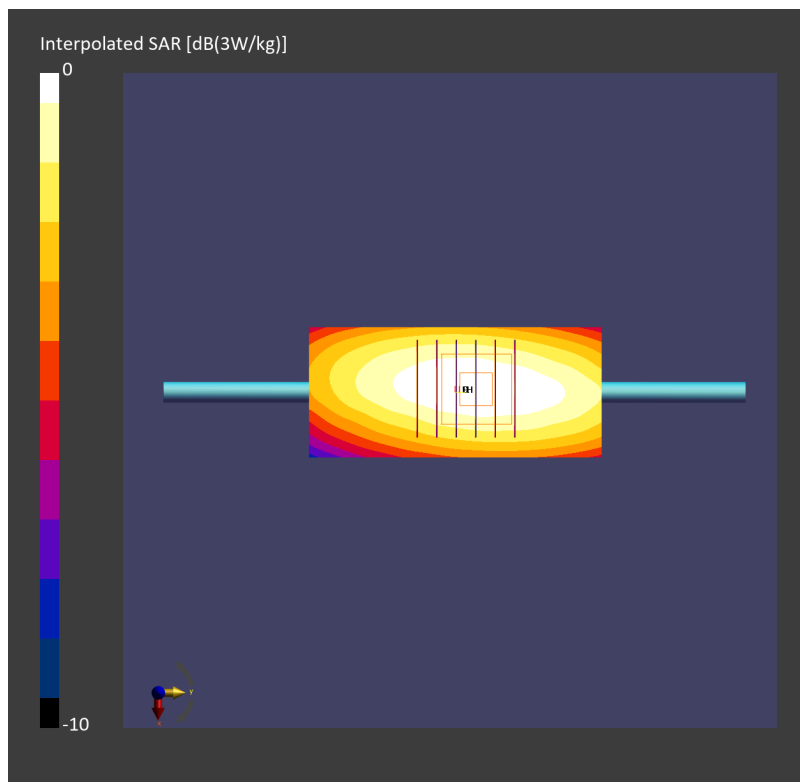

System Check_Head_750Mhz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260417 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.874$ S/m; $\epsilon_r = 43.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(9.46, 9.41, 10.07); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.18 W/kg; SAR (10g) = 1.45 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.18 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.45 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

TSL Correction: Positive only

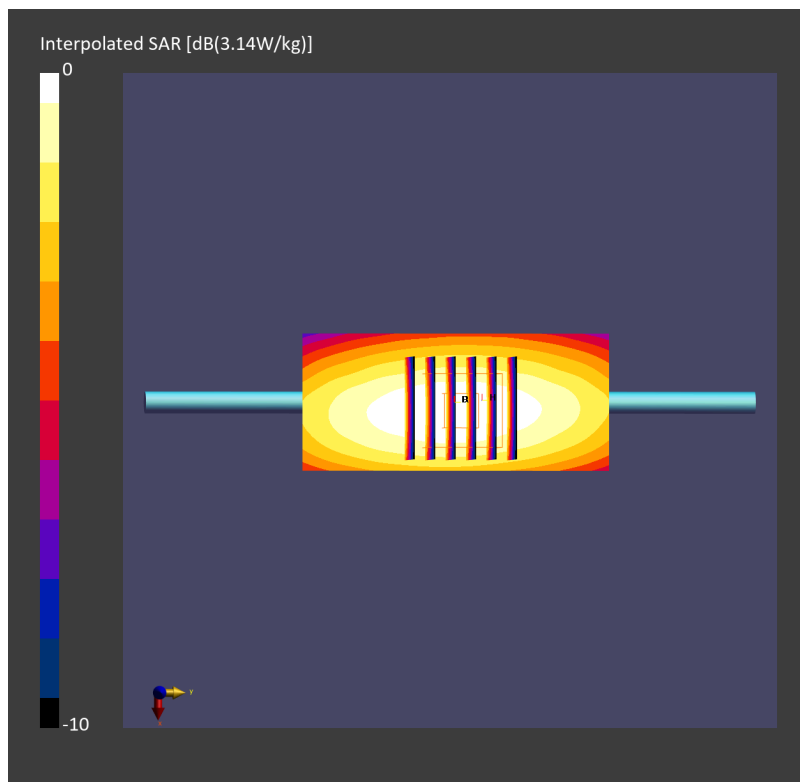

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260421 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.922$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.98, 9.68, 9.75); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.943 W/kg; SAR (10g) = 0.629 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 0.933 W/kg; SAR (8g) = 0.654 W/kg; SAR (10g) = 0.621 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

TSL Correction: Positive only

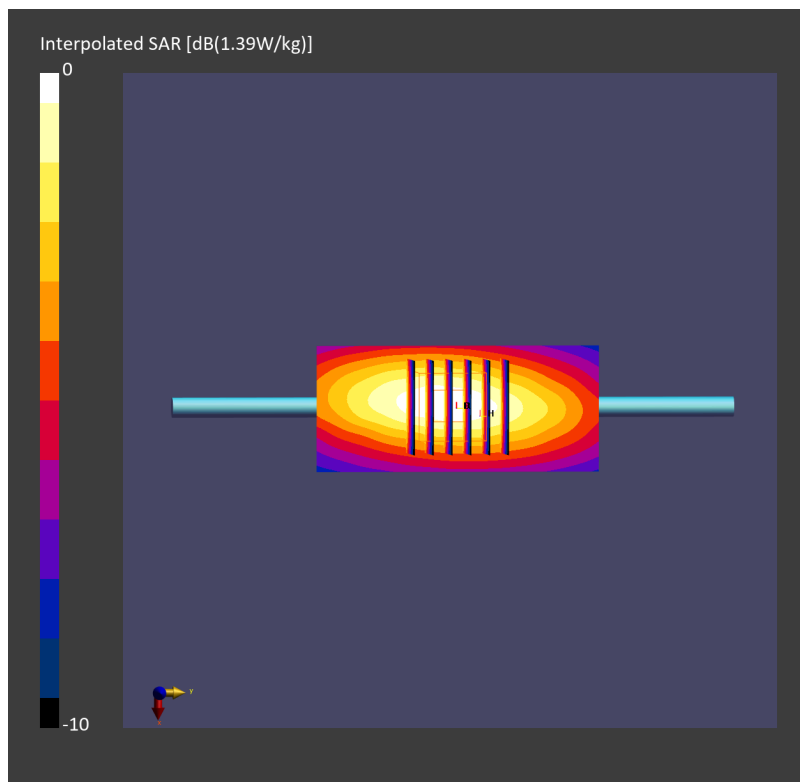

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260426 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.857$ S/m; $\epsilon_r = 44.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.98, 9.68, 9.75); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.17 W/kg; SAR (10g) = 1.43 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.16 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.0 %

TSL Correction: Positive only

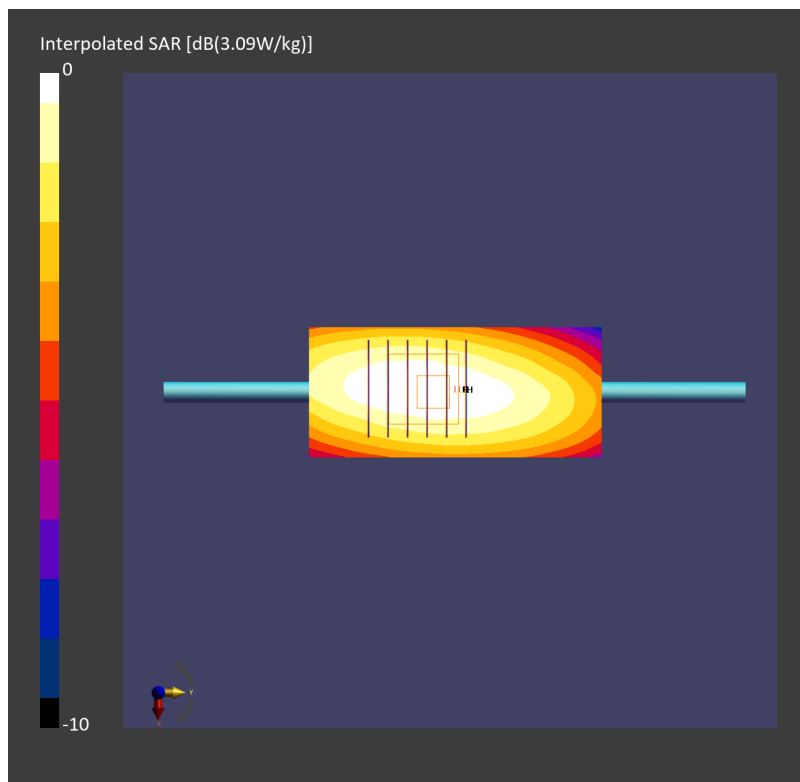

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260417 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.881$ S/m; $\epsilon_r = 43.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.97, 9.66, 9.74); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.29 W/kg; SAR (10g) = 1.49 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.29 W/kg; SAR (8g) = 1.57 W/kg; SAR (10g) = 1.49 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

TSL Correction: Positive only

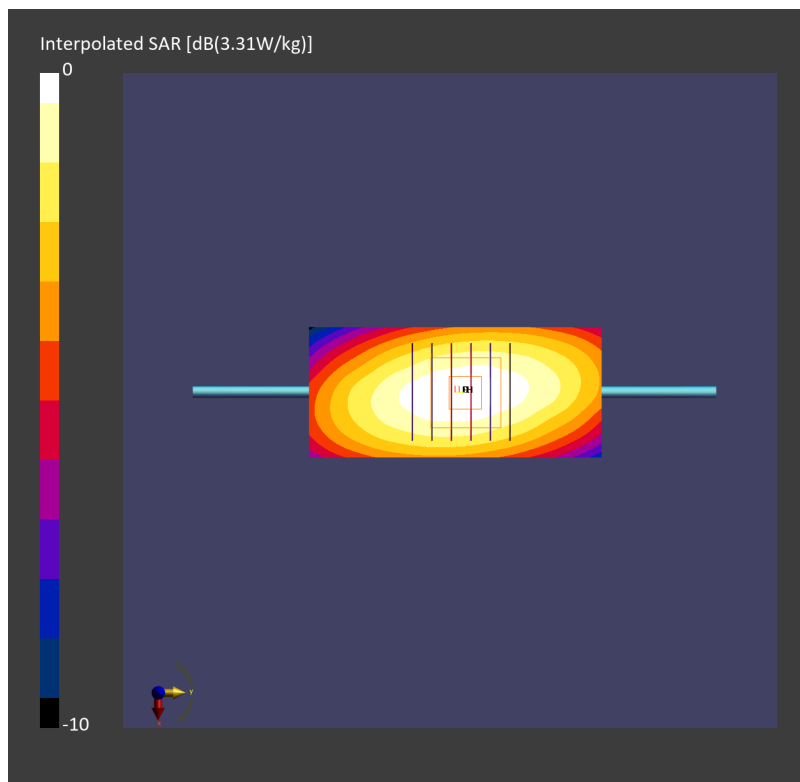

System Check_Head_835Mhz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260418 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.900$ S/m; $\epsilon_r = 43.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(9.11, 9.07, 9.7); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.51 W/kg; SAR (10g) = 1.66 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.51 W/kg; SAR (8g) = 1.74 W/kg; SAR (10g) = 1.65 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

TSL Correction: Positive only

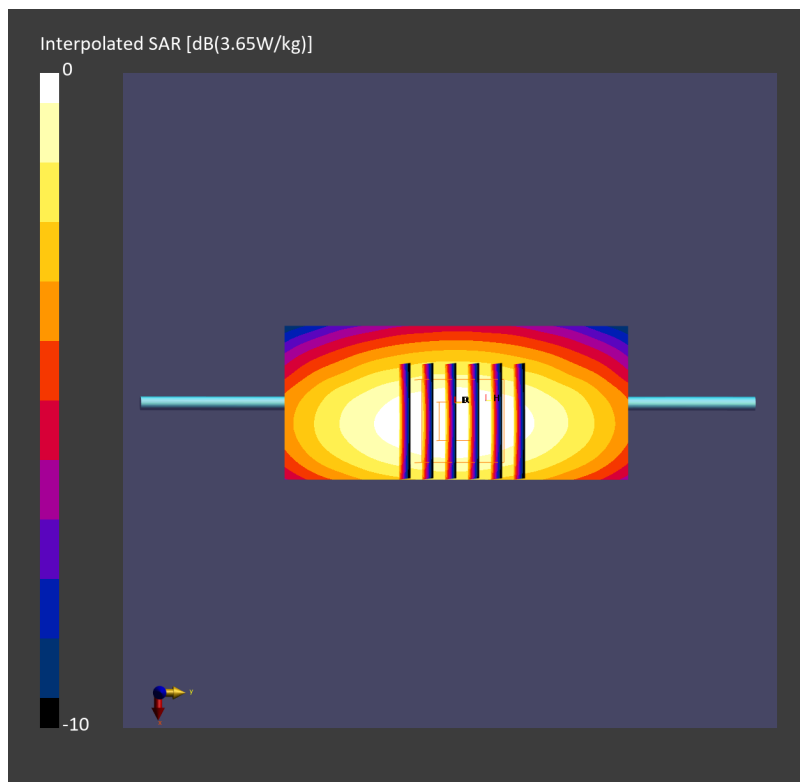

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260421 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.951$ S/m; $\epsilon_r = 42.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.97, 9.66, 9.74); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.975 W/kg; SAR (10g) = 0.641 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 0.968 W/kg; SAR (8g) = 0.671 W/kg; SAR (10g) = 0.636 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.9 %

TSL Correction: Positive only

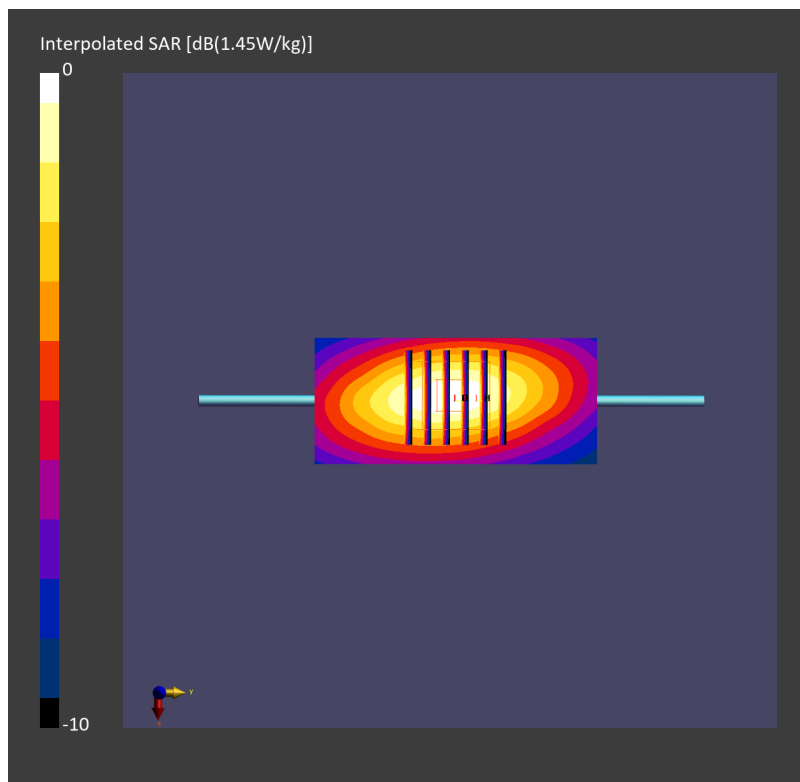

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260427 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 44.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.97, 9.66, 9.74); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.31 W/kg; SAR (10g) = 1.50 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.30 W/kg; SAR (8g) = 1.58 W/kg; SAR (10g) = 1.50 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 87.7 %

TSL Correction: Positive only

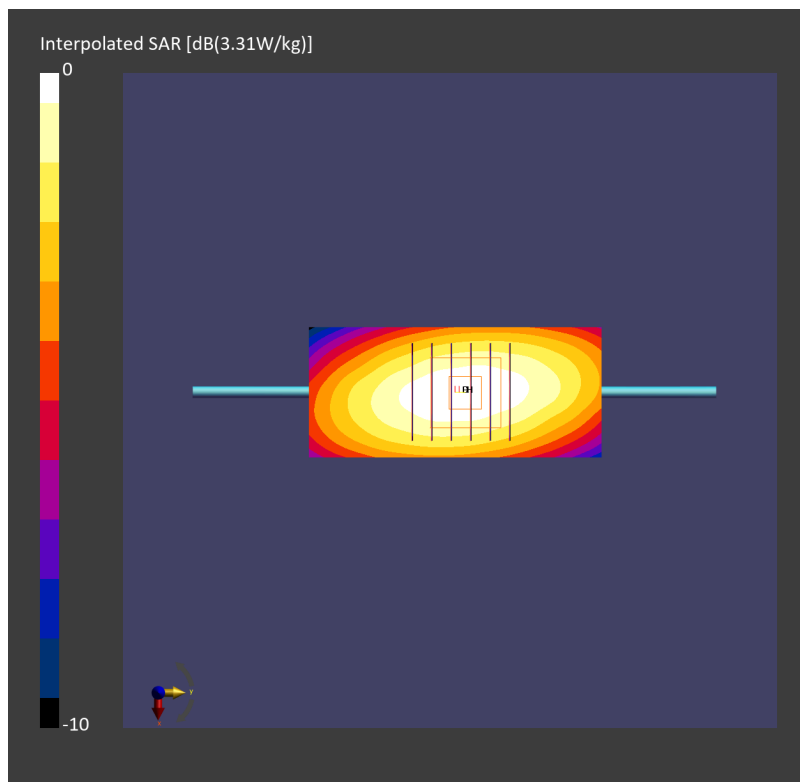

System Check_Head_900MHz

DUT: D900V2 - SN190

Communication System: CW; Frequency: 900.000 MHz

Medium: HSL_600-7200_260421 Medium parameters used: $f = 900.000$ MHz; $\sigma = 0.973$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.55, 9.25, 9.33); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.08 W/kg; SAR (10g) = 0.700 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.07 W/kg; SAR (8g) = 0.736 W/kg; SAR (10g) = 0.697 W/kg

Smallest distance from peaks to all points 3 dB below = 16.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

TSL Correction: Positive only

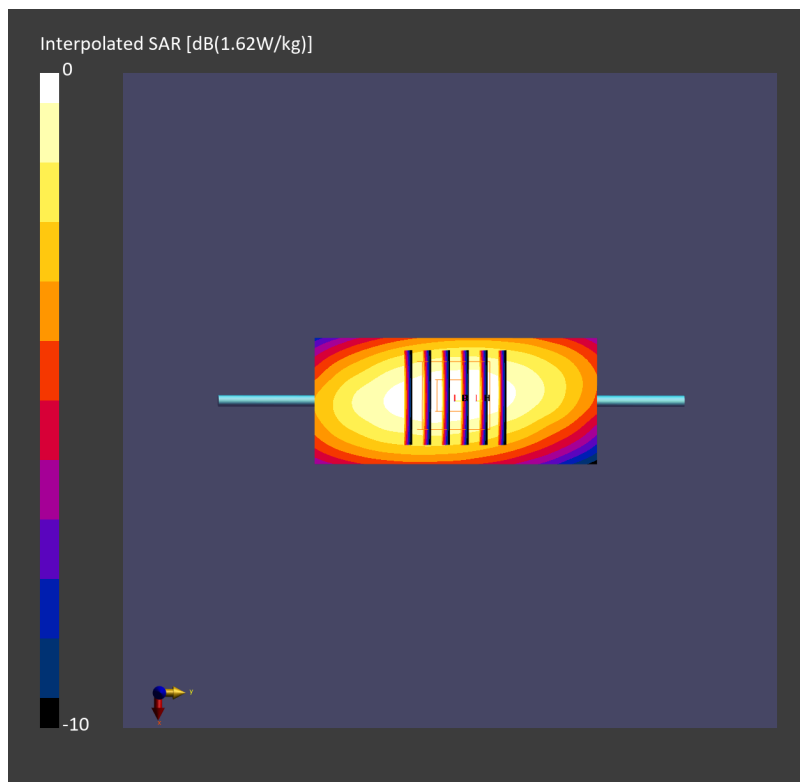

System Check_Head_900MHz

DUT: D900V2 - SN190

Communication System: CW; Frequency: 900.000 MHz

Medium: HSL_600-7200_260427 Medium parameters used: $f = 900.000$ MHz; $\sigma = 0.912$ S/m; $\epsilon_r = 44.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.55, 9.25, 9.33); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.71 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.67 W/kg; SAR (8g) = 1.81 W/kg; SAR (10g) = 1.72 W/kg

Smallest distance from peaks to all points 3 dB below = 15.8 mm

Ratio of SAR at M2 to SAR at M1 = 87.4 %

TSL Correction: Positive only

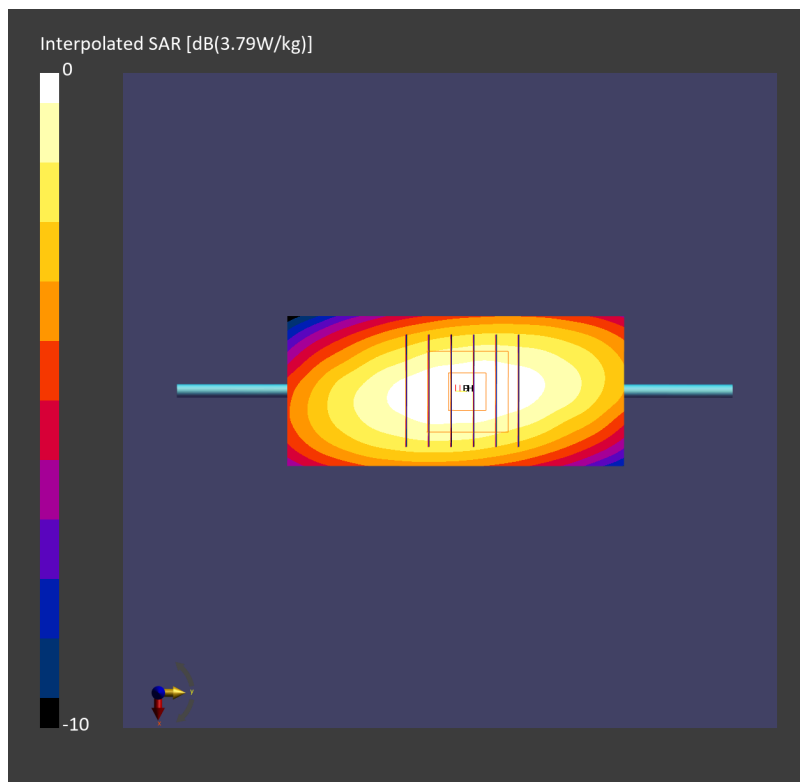

System Check_Head_1750Mhz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(7.7, 7.66, 8.2); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.11 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

TSL Correction: Positive only

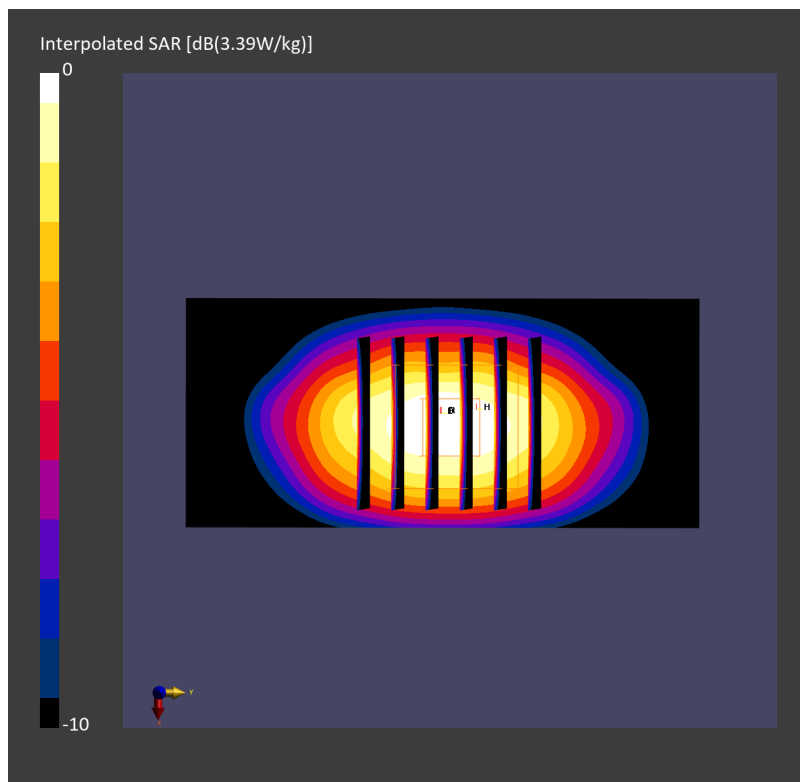

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260418 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.32$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.26, 8.0, 8.07); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 3.80 W/kg; SAR (10g) = 2.00 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 3.73 W/kg; SAR (8g) = 2.13 W/kg; SAR (10g) = 1.96 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.0 %

TSL Correction: Positive only

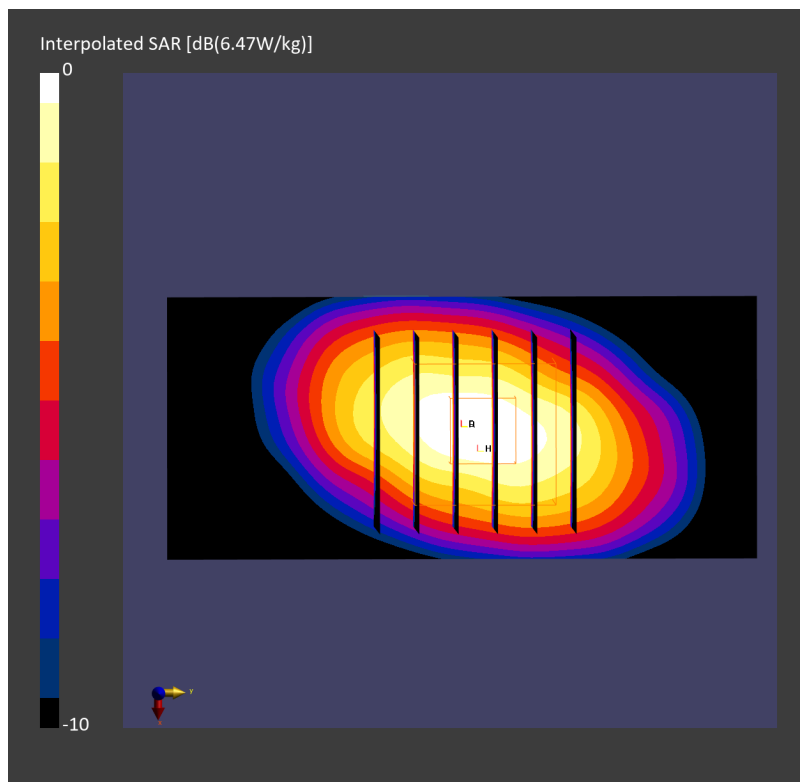

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260422 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.26, 8.0, 8.07); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.87 W/kg; SAR (10g) = 1.00 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.85 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.981 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 83.9 %

TSL Correction: Positive only

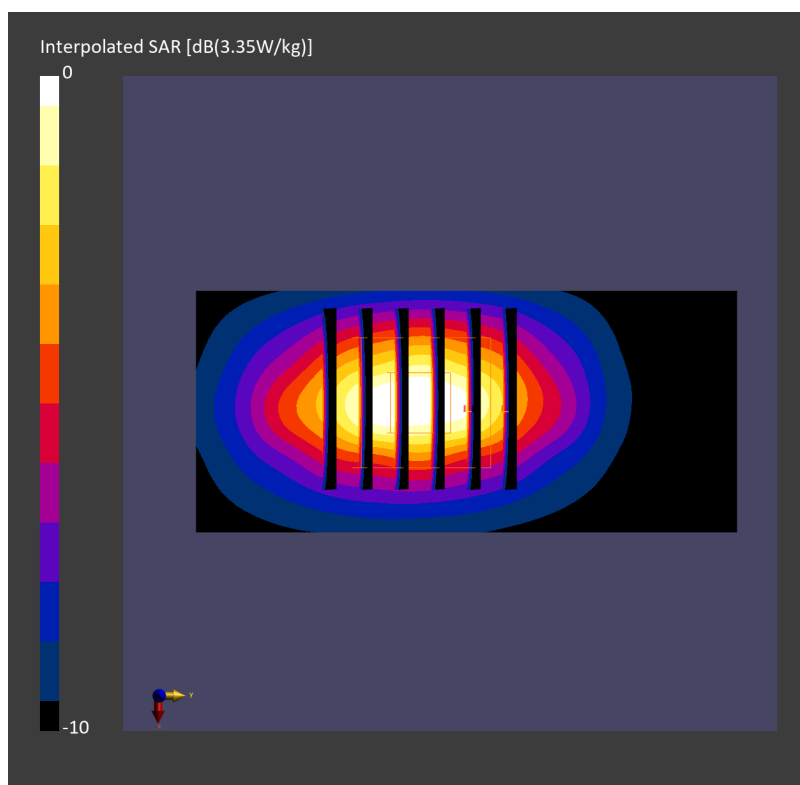

System Check_Head_1900Mhz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(7.47, 7.43, 7.95); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.99 W/kg; SAR (10g) = 1.06 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.98 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

TSL Correction: Positive only

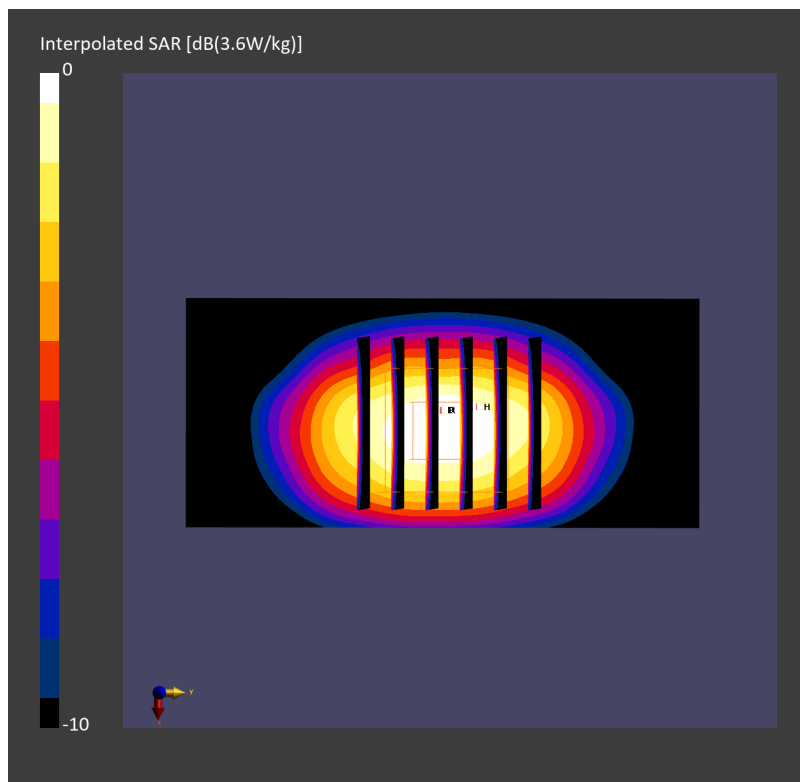

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260419 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.08, 7.83, 7.89); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 3.88 W/kg; SAR (10g) = 2.00 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 3.82 W/kg; SAR (8g) = 2.15 W/kg; SAR (10g) = 1.98 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.4 %

TSL Correction: Positive only

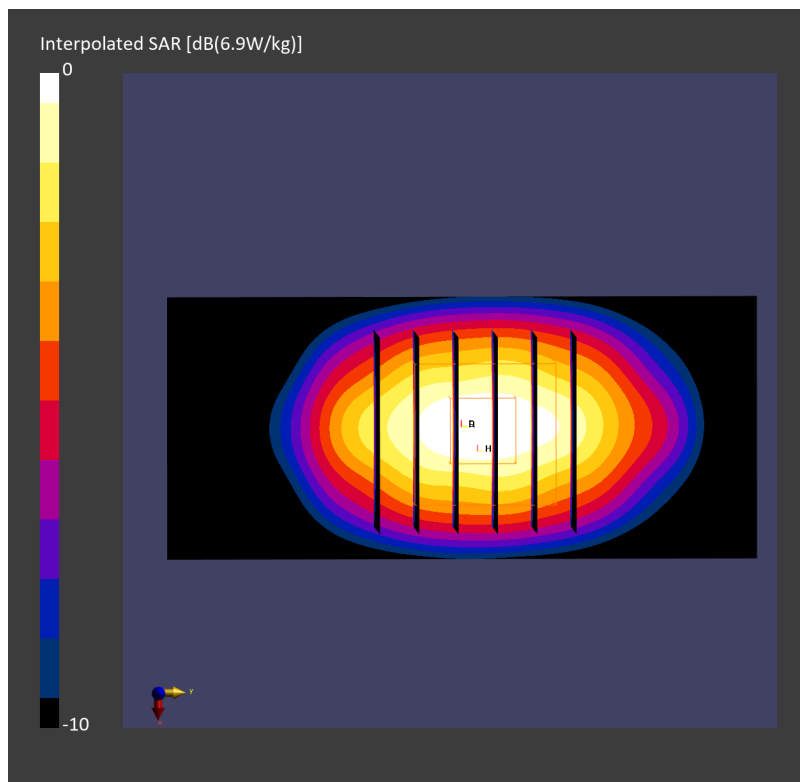

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260422 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.08, 7.83, 7.89); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.99 W/kg; SAR (10g) = 1.04 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.96 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

TSL Correction: Positive only

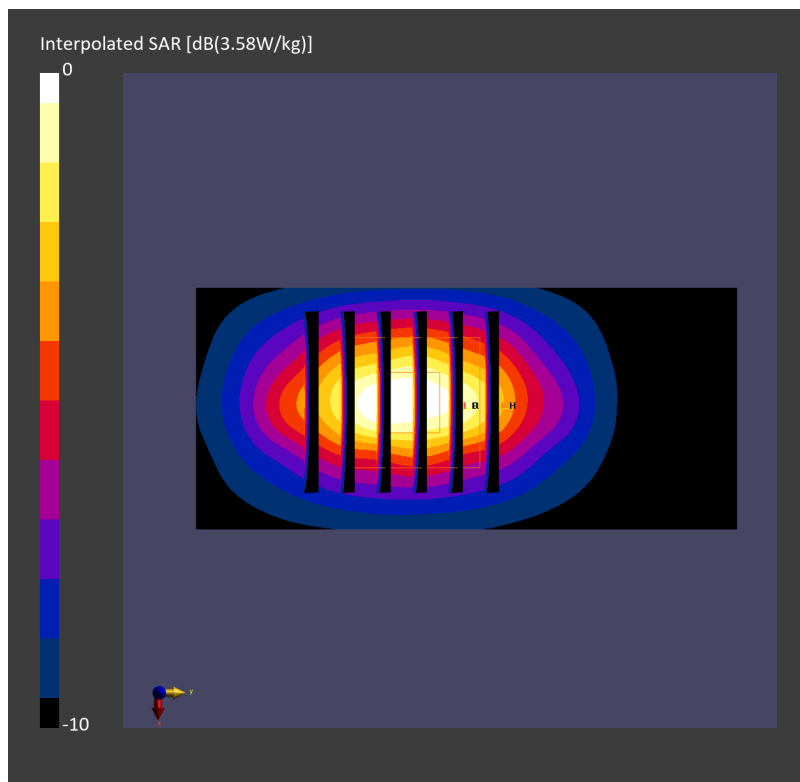

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260411 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(7.09, 7.06, 7.55); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.75 W/kg; SAR (10g) = 1.24 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.72 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.5 %

TSL Correction: Positive only

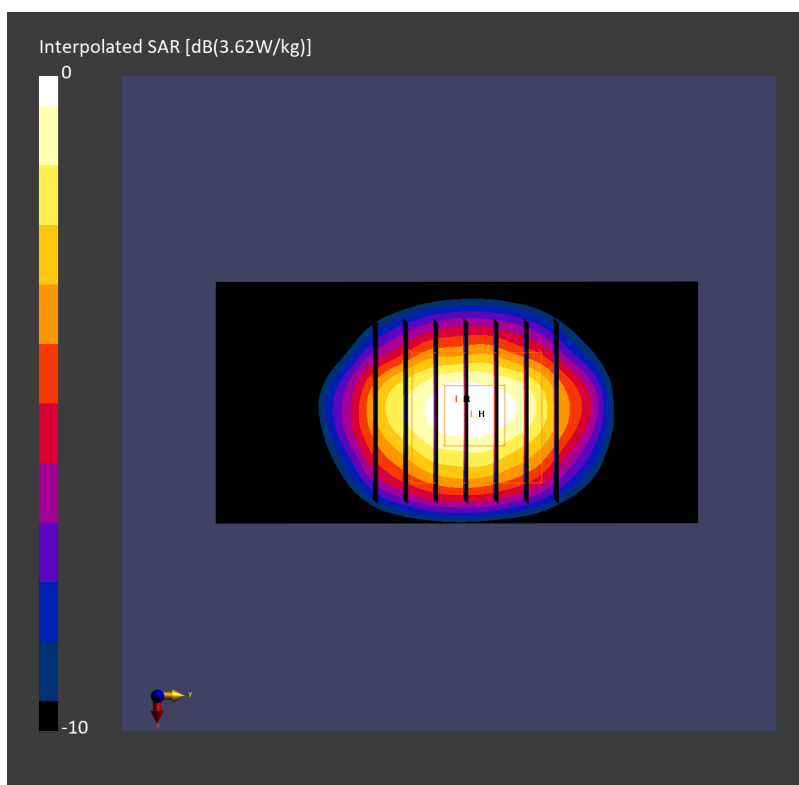

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260420 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 5.46 W/kg; SAR (10g) = 2.42 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 5.38 W/kg; SAR (8g) = 2.65 W/kg; SAR (10g) = 2.39 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.9 %

TSL Correction: Positive only

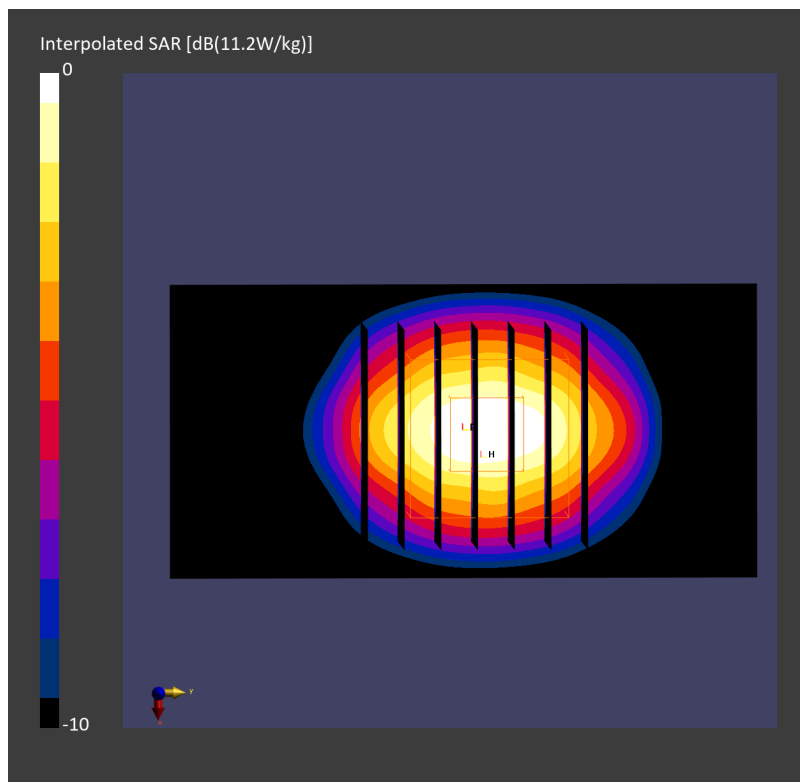

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260423 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.62 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.7 %

TSL Correction: Positive only

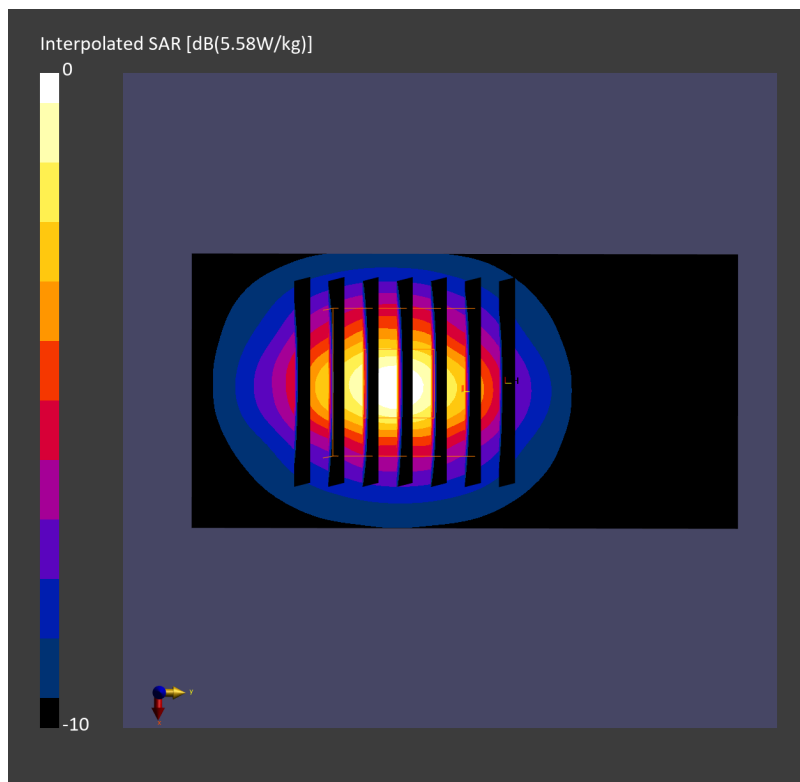

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260428 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 5.54 W/kg; SAR (10g) = 2.46 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 5.46 W/kg; SAR (8g) = 2.69 W/kg; SAR (10g) = 2.43 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

TSL Correction: Positive only

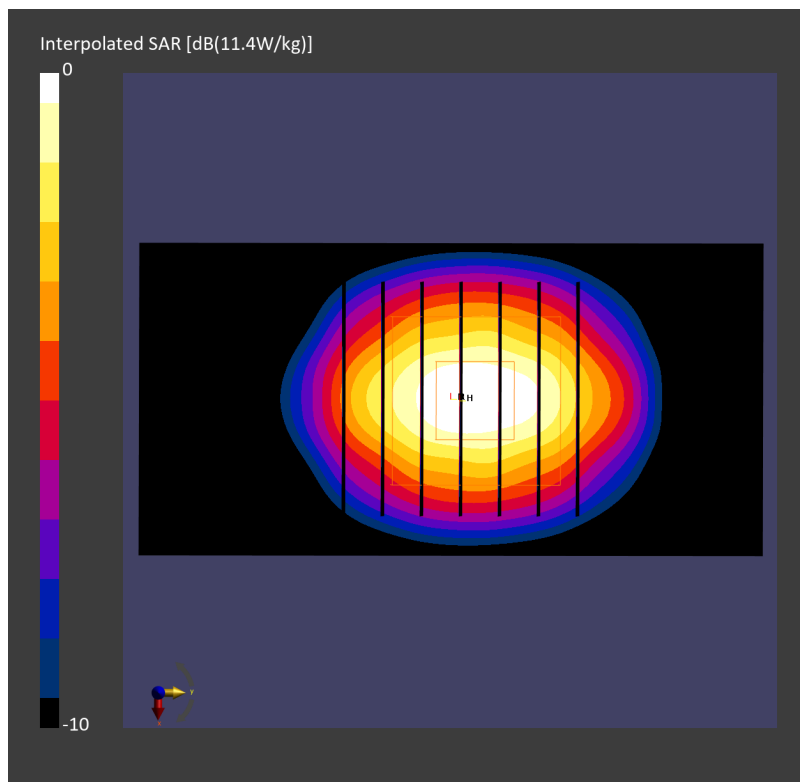

System Check_Head_3500Mhz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260412 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.80$ S/m; $\epsilon_r = 40.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.42, 6.39, 6.83); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.46 W/kg; SAR (10g) = 1.30 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.48 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 78.4 %

TSL Correction: Positive only

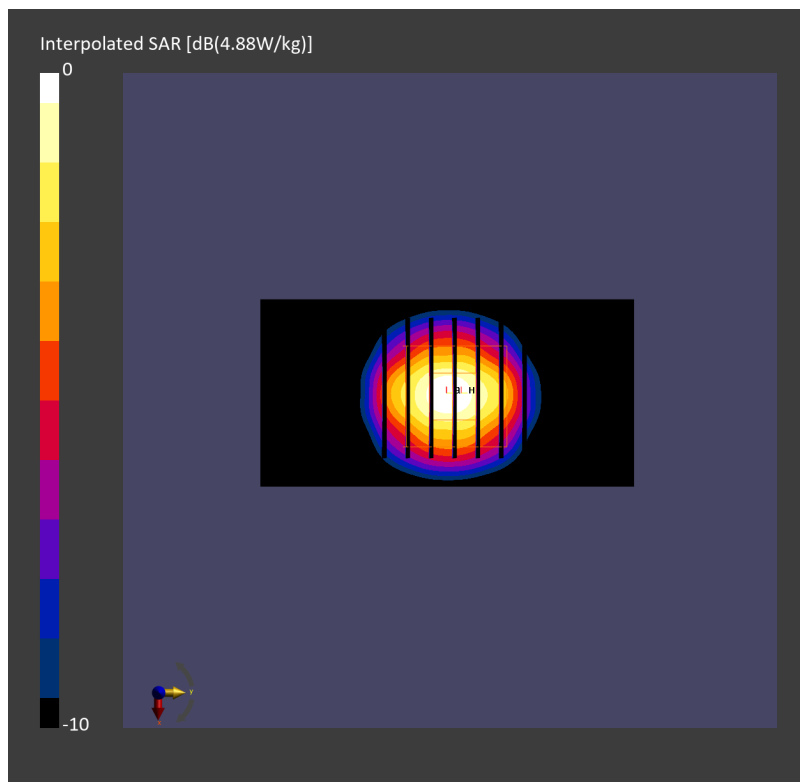

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260413 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.69$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.40 W/kg; SAR (10g) = 2.42 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.41 W/kg; SAR (8g) = 2.74 W/kg; SAR (10g) = 2.43 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.4 %

TSL Correction: Positive only

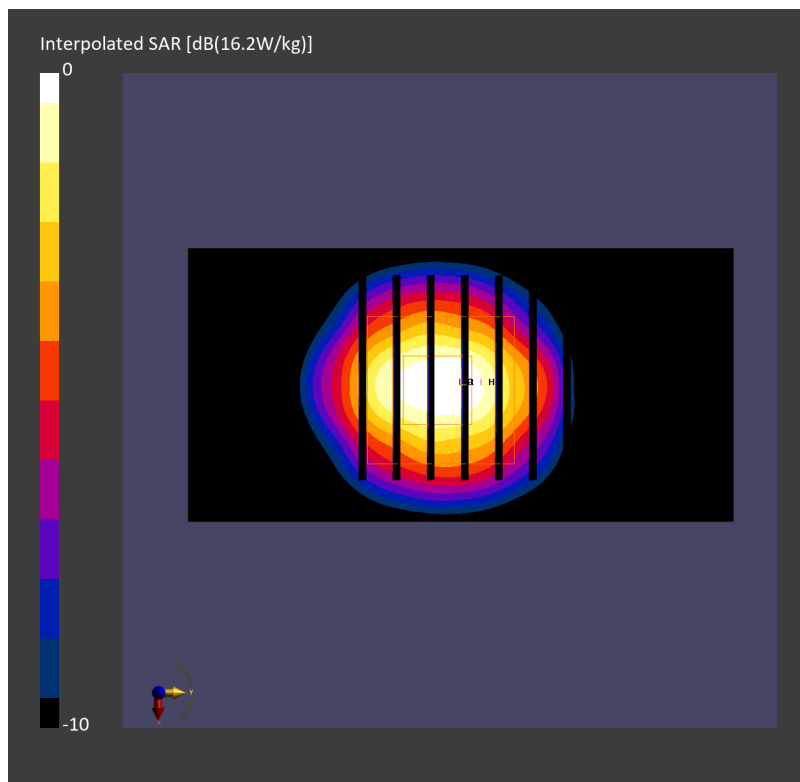

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260424 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.72$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.75 W/kg; SAR (10g) = 2.56 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.70 W/kg; SAR (8g) = 2.88 W/kg; SAR (10g) = 2.55 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

TSL Correction: Positive only

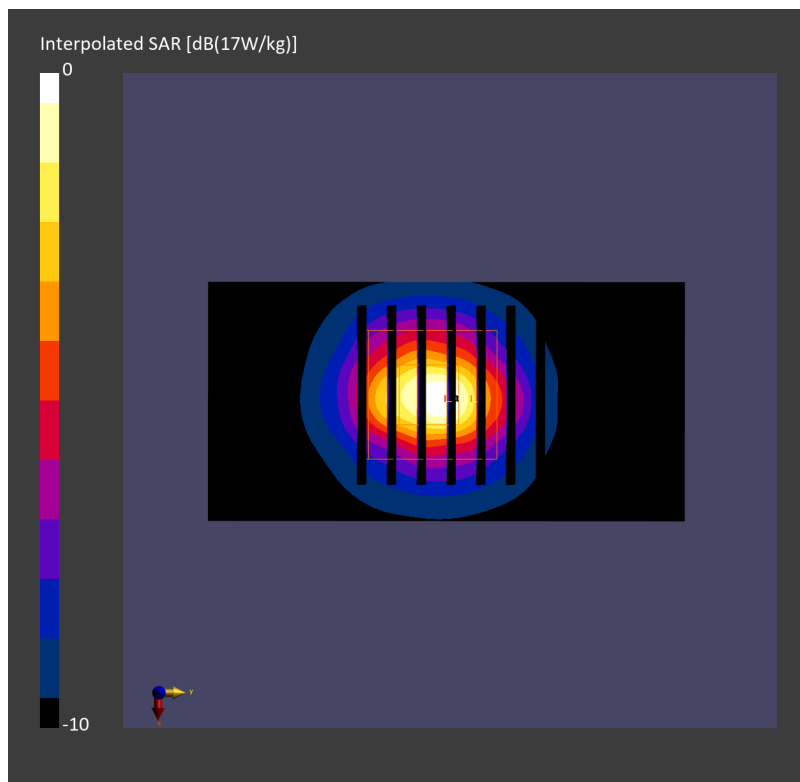

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260425 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.76$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.46 W/kg; SAR (10g) = 2.45 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.46 W/kg; SAR (8g) = 2.77 W/kg; SAR (10g) = 2.46 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.3 %

TSL Correction: Positive only

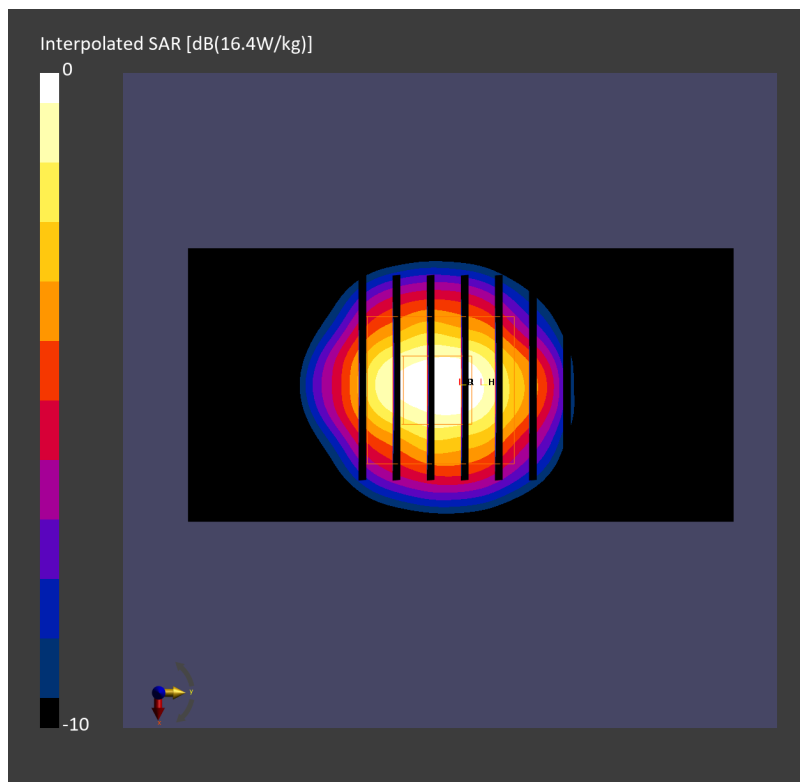

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260413 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.36, 6.33, 6.77); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.50 W/kg; SAR (10g) = 1.28 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.04 dB

SAR (1g) = 3.48 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

TSL Correction: Positive only

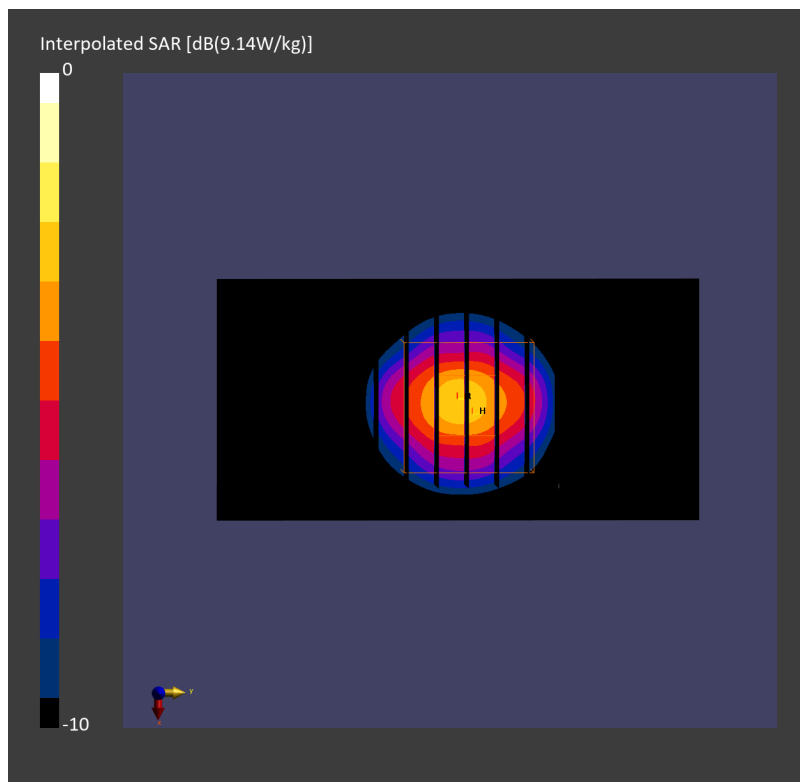

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260414 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.87$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.56 W/kg; SAR (10g) = 2.42 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 6.55 W/kg; SAR (8g) = 2.73 W/kg; SAR (10g) = 2.41 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

TSL Correction: Positive only

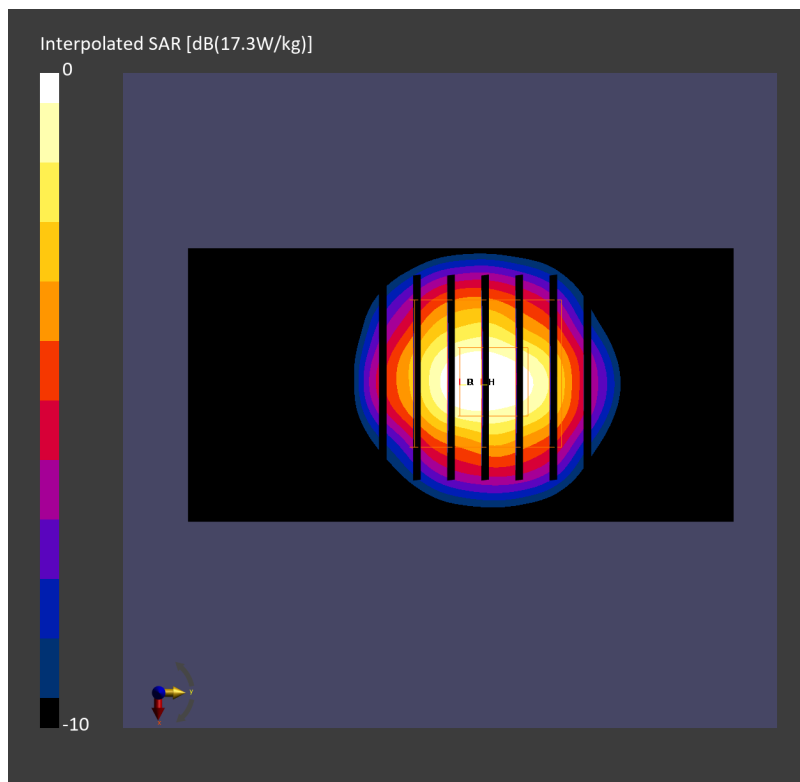

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260424 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.89$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.35 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.5 %

TSL Correction: Positive only

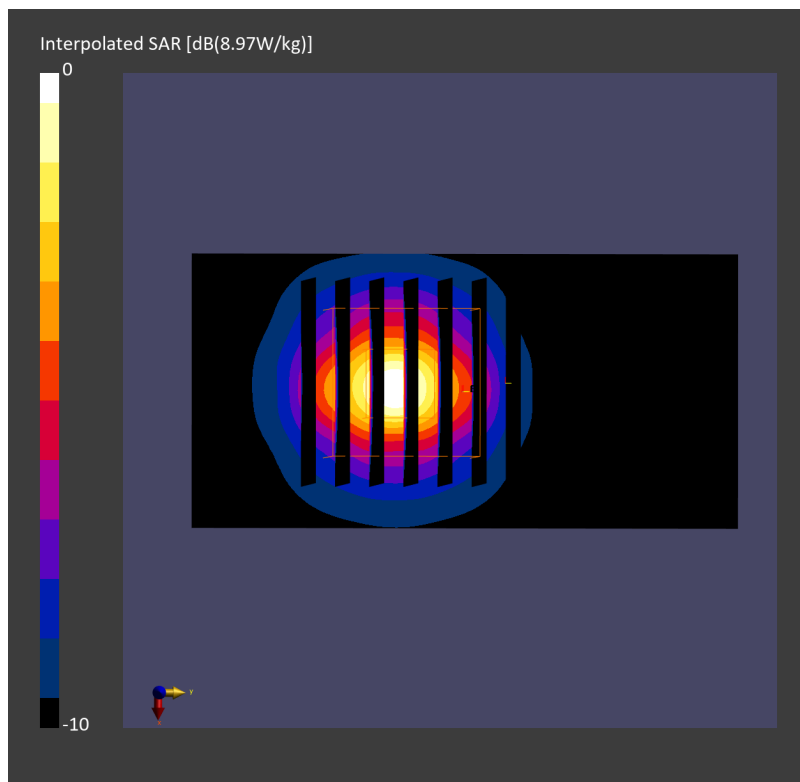

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260425 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.94$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.05 W/kg; SAR (10g) = 2.61 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 7.03 W/kg; SAR (8g) = 2.94 W/kg; SAR (10g) = 2.59 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 74.8 %

TSL Correction: Positive only

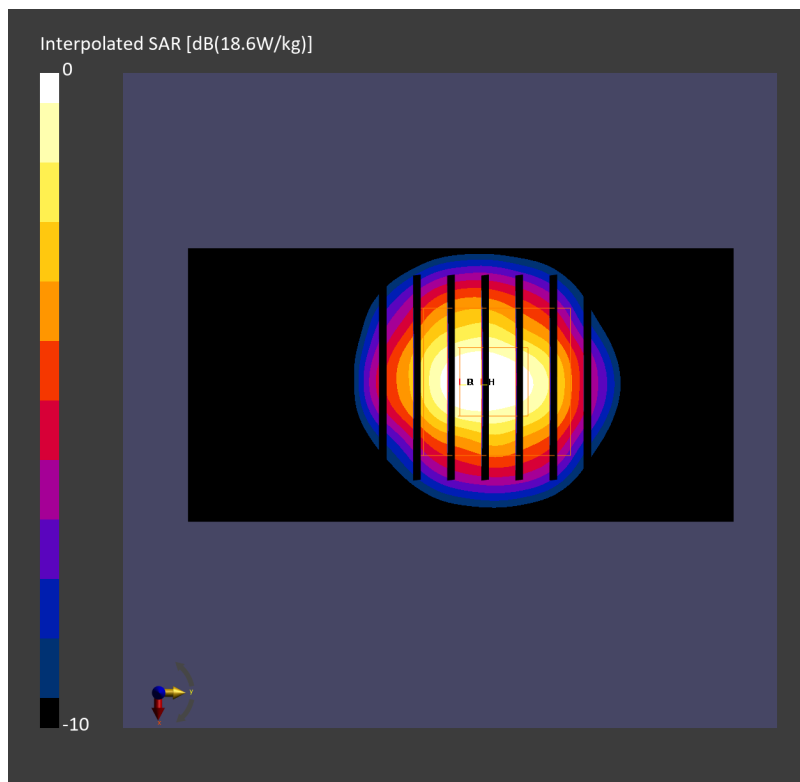

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260429 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.97$ S/m; $\epsilon_r = 40.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.12 W/kg; SAR (10g) = 2.64 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 7.10 W/kg; SAR (8g) = 2.97 W/kg; SAR (10g) = 2.62 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 74.8 %

TSL Correction: Positive only

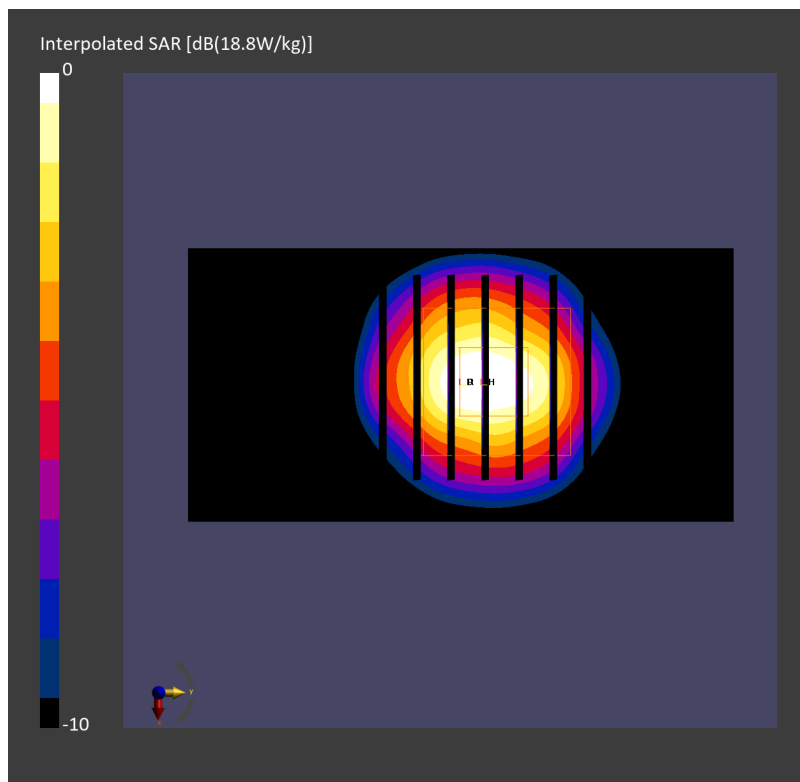

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260414 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(6.37, 6.34, 6.78); Calibrated: 2025-05-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.06 W/kg; SAR (10g) = 1.09 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.12 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.1 %

TSL Correction: Positive only

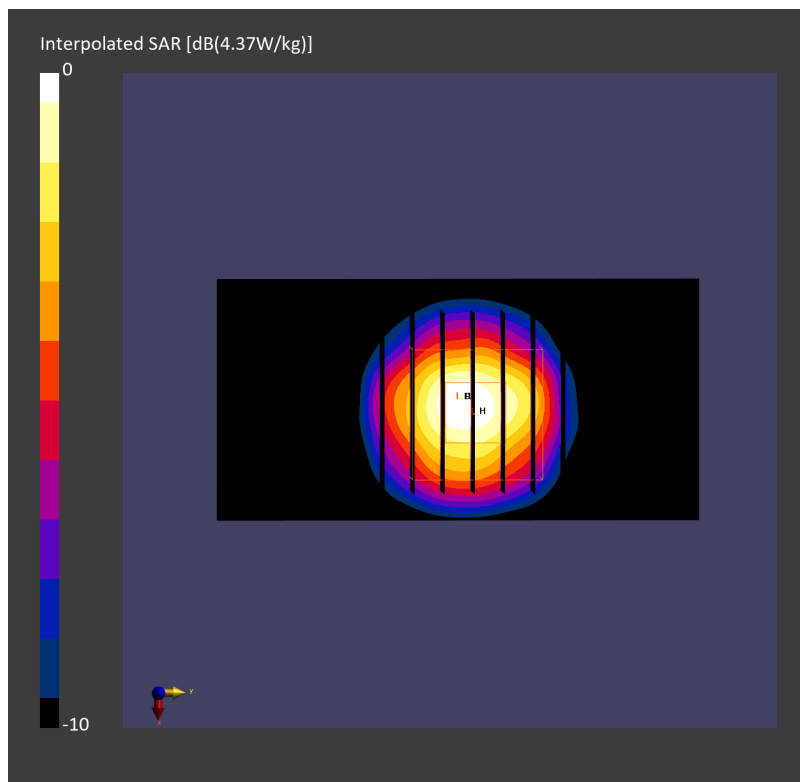

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.06$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.43 W/kg; SAR (10g) = 2.25 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.46 W/kg; SAR (8g) = 2.58 W/kg; SAR (10g) = 2.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.3 %

TSL Correction: Positive only

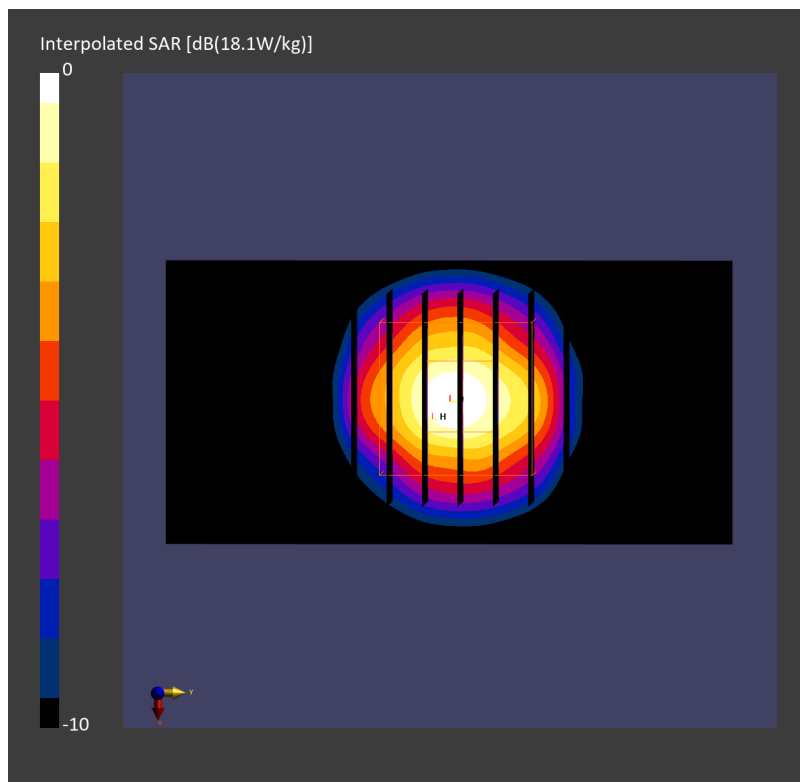

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260424 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.50 W/kg; SAR (10g) = 2.28 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 6.47 W/kg; SAR (8g) = 2.59 W/kg; SAR (10g) = 2.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.3 %

TSL Correction: Positive only

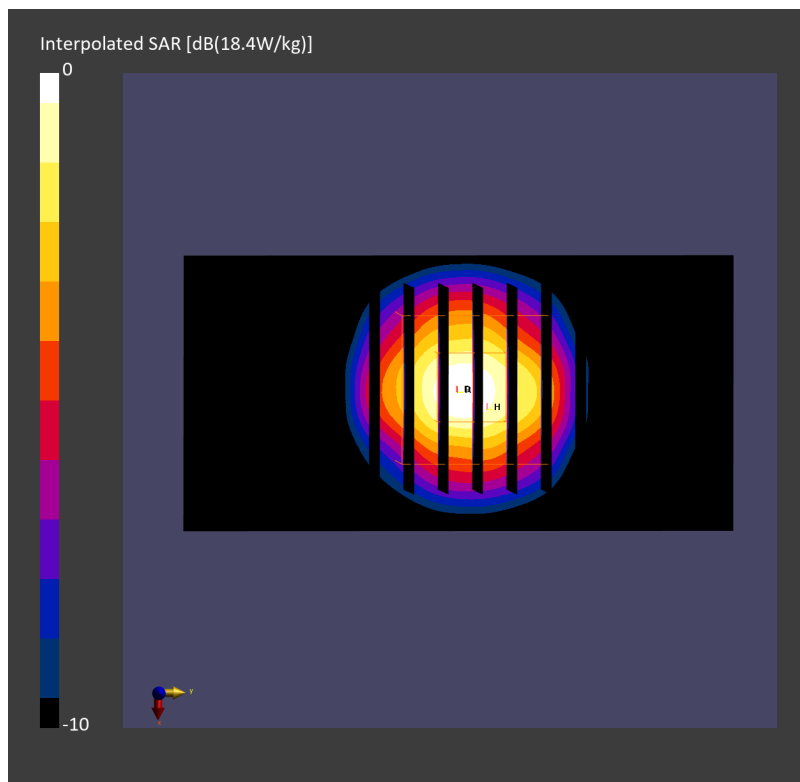

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260425 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.15$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.76 W/kg; SAR (10g) = 2.37 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.79 W/kg; SAR (8g) = 2.73 W/kg; SAR (10g) = 2.40 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.2 %

TSL Correction: Positive only

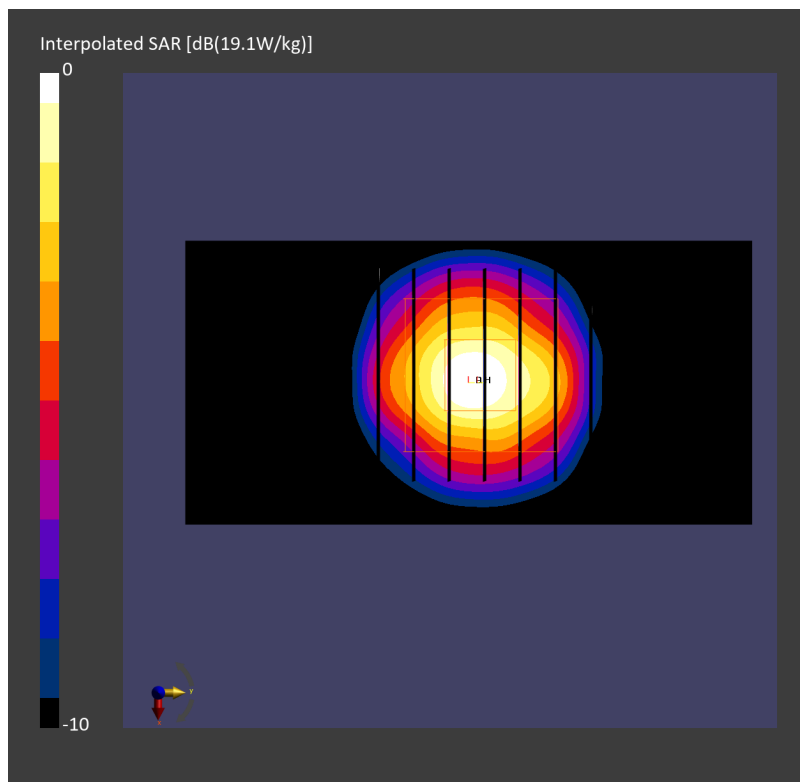

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260430 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2025-05-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.77 W/kg; SAR (10g) = 2.38 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 6.78 W/kg; SAR (8g) = 2.73 W/kg; SAR (10g) = 2.40 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.2 %

TSL Correction: Positive only

