

FCC and ISCED Test Report

Sensium Healthcare Ltd.

Base station, Model: Vitals Base Station US

In accordance with FCC 47 CFR Part 15B and ICES-003

Prepared for: Sensium Healthcare Ltd.
115 Olympic Avenue
Building 3
Milton Park
Abingdon
Oxfordshire
OX14 4SA
UNITED KINGDOM



Add value.
Inspire trust.

FCC ID: AEJSH202075 IC: 27456-SH202075

COMMERCIAL-IN-CONFIDENCE

Document 75953351-01 Issue 01

SIGNATURE

A. Lawson

NAME	JOB TITLE	RESPONSIBLE FOR	ISSUE DATE
Andy Lawson	EMC Chief Engineer	Authorised Signatory	23 December 2021

Signatures in this approval box have checked this document in line with the requirements of TÜV SÜD document control rules.

ENGINEERING STATEMENT

The measurements shown in this report were made in accordance with the procedures described on test pages. All reported testing was carried out on a sample equipment to demonstrate limited compliance with FCC 47 CFR Part 15B and ICES-003. The sample tested was found to comply with the requirements defined in the applied rules.

RESPONSIBLE FOR	NAME	DATE	SIGNATURE
Testing	Paul Dickson	23 December 2021	<i>Paul Dickson</i>

FCC Accreditation

90987 Octagon House, Fareham Test Laboratory

ISED Accreditation

12669A Octagon House, Fareham Test Laboratory

EXECUTIVE SUMMARY

A sample of this product was tested and found to be compliant with FCC 47 CFR Part 15B: 2020 and ICES-003: Issue 7: 2020 for the tests detailed in section 1.3.



DISCLAIMER AND COPYRIGHT

This non-binding report has been prepared by TÜV SÜD with all reasonable skill and care. The document is confidential to the potential Client and TÜV SÜD. No part of this document may be reproduced without the prior written approval of TÜV SÜD. © 2021 TÜV SÜD. This report relates only to the actual item/items tested.

ACCREDITATION

Our UKAS Accreditation does not cover opinions and interpretations and any expressed are outside the scope of our UKAS Accreditation. Results of tests not covered by our UKAS Accreditation Schedule are marked NUA (Not UKAS Accredited).

TÜV SÜD
is a trading name of TÜV SÜD Ltd
Registered in Scotland at East Kilbride,
Glasgow G75 0QF, United Kingdom
Registered number: SC215164

TÜV SÜD Ltd is a
TÜV SÜD Group Company

Phone: +44 (0) 1489 558100
Fax: +44 (0) 1489 558101
www.tuvsud.com/en

TÜV SÜD
Octagon House Concorde Way
Fareham
Hampshire PO15 5RL
United Kingdom

TÜV SÜD

TÜV®



Contents

1 **Report Summary2**

1.1 Report Modification Record.....2

1.2 Introduction.....2

1.3 Brief Summary of Results3

1.4 Declaration of Build Status4

1.5 Product Information5

1.6 Deviations from the Standard.....5

1.7 EUT Modification Record5

1.8 Test Location5

2 **Test Details6**

2.1 Radiated Disturbance.....6

3 **Incident Reports 16**

4 **Measurement Uncertainty 18**



1 Report Summary

1.1 Report Modification Record

Alterations and additions to this report will be issued to the holders of each copy in the form of a complete document.

Issue	Description of Change	Date of Issue
1	First Issue	23 December 2021

Table 1

1.2 Introduction

Applicant	Sensium Healthcare Ltd.
Manufacturer	Sensium Healthcare Ltd.
Model Number(s)	Vitals Base Station US
Serial Number(s)	Not serialised
Hardware Version(s)	SH202075 v1.5
Software Version(s)	PAT_US_915MHz_64K_P_CUS1_FW1-0-6
Number of Samples Tested	1
Test Specification/Issue/Date	FCC 47 CFR Part 15B: 2020 ICES-003: Issue 7: 2020
Order Number	0000005831
Date	14-September-2021
Date of Receipt of EUT	28-September-2021
Start of Test	27-October-2021
Finish of Test	27-October-2021
Name of Engineer(s)	Paul Dickson
Related Document(s)	ANSI C63.4: 2014



1.3 Brief Summary of Results

A brief summary of the tests carried out in accordance with FCC 47 CFR Part 15B and ICES-003 is shown below.

Section	Specification Clause		Test Description	Result	Comments/Base Standard
	Part 15B	ICES-003			
Configuration and Mode: DC Powered - Operating					
2.1	15.109	3.2	Radiated Disturbance	Pass	ANSI C63.4: 2014

Table 2



1.4 Declaration of Build Status

MAIN EUT			
MANUFACTURING DESCRIPTION	SensiumVitals Base Station		
MANUFACTURER	Sensium		
MODEL	Vitals Base Station US		
PART NUMBER	SH202075		
HARDWARE VERSION	SH202075 v1.5		
SOFTWARE VERSION	PAT_US_915MHz_64K_P_CUS1_FW1-0-6		
PSU VOLTAGE/FREQUENCY/CURRENT	3.3 V DC		
HIGHEST INTERNALLY GENERATED FREQUENCY	928MHz		
FCC ID (if applicable)	AEJSH202075		
INDUSTRY CANADA ID (if applicable)	27456-SH202075		
TECHNICAL DESCRIPTION (a brief technical description of the intended use and operation)	The SH202075 SensiumVitals Base Station is a radio module that communicates with the Sensium Vitals Patch. It collects data from the patches over ISM band link and passes that data to the Sensium Vitals Bridge, into which it is integrated. The Bridge takes the data and forwards it to the Sensium Servers for processing.		
COUNTRY OF ORIGIN	United Kingdom		
RF CHARACTERISTICS (if applicable)			
TRANSMITTER FREQUENCY OPERATING RANGE (MHz)	902 – 928 MHz		
RECEIVER FREQUENCY OPERATING RANGE (MHz)	902 – 928 MHz		
INTERMEDIATE FREQUENCIES	915 MHz		
EMISSION DESIGNATOR(S): https://fccid.io/Emissions-Designator/	120KFD		
MODULATION TYPES: (i.e. GMSK, QPSK)	FSK		
OUTPUT POWER (W or dBm)	-4 dBm		
SEPARATE BATTERY/POWER SUPPLY (if applicable)			
MODULES (if applicable)			
MANUFACTURING DESCRIPTION			
MANUFACTURER			
TYPE			
POWER			
FCC ID			
INDUSTRY CANADA ID			
EMISSION DESIGNATOR			
DHSS/FHSS/COMBINED OR OTHER			
COUNTRY OF ORIGIN			
ANCILLARIES (if applicable)			

Table 3

I hereby declare that the information supplied is correct and complete.

Name: Paul Dodds
Position held: RF Compliance Engineer
Date: 15 October 2021



1.5 Product Information

1.5.1 Technical Description

The Equipment under test (EUT) was a SensiumVitals Base Station.

The primary function of the EUT is to communicate with the Sensium Vitals Patch.

Additionally, the EUT has functionality to collect data from the patches over ISM band link and passes that data to the Sensium Vitals Bridge, into which it is integrated.

1.5.2 EUT Port/Cable Identification

Port	Max Cable Length specified	Usage	Type	Screened
None	-	-	-	-

Table 4

1.6 Deviations from the Standard

No deviations from the applicable test standard were made during testing.

1.7 EUT Modification Record

The table below details modifications made to the EUT during the test programme.

The modifications incorporated during each test are recorded on the appropriate test pages.

Modification State	Description of Modification still fitted to EUT	Modification Fitted By	Date Modification Fitted
Model: Vitals Base Station US, Serial Number: Not serialised			
0	As supplied by the customer	Not Applicable	Not Applicable

Table 5

1.8 Test Location

TÜV SÜD conducted the following tests at our Fareham Test Laboratory.

Test Name	Name of Engineer(s)	Accreditation
Configuration and Mode: DC Powered - Operating		
Radiated Disturbance	Paul Dickson	UKAS

Table 6

Office Address:

TÜV SÜD
Octagon House
Concorde Way
Fareham
Hampshire
PO15 5RL, United Kingdom



2 Test Details

2.1 Radiated Disturbance

2.1.1 Specification Reference

FCC 47 CFR Part 15B, Clause 15.109
ICES-003, Clause 3.2

2.1.2 Equipment Under Test and Modification State

Vitals Base Station US, S/N: Not serialised - Modification State 0

2.1.3 Date of Test

27-October-2021

2.1.4 Test Method

The EUT was set up on a non-conductive table 0.8 m above a reference ground plane within a semi-anechoic chamber on a remotely controlled turntable.

A pre-scan of the EUT emissions profile using a peak detector was made at a 3 m antenna distance whilst varying the antenna-to-EUT azimuth and polarisation.

Using a list of the highest emissions detected during the pre-scan along with their bearing and associated antenna polarisation, the EUT was then formally measured using a Quasi-Peak, Peak or CISPR Average detector as appropriate.

The readings were maximised by adjusting the antenna height, polarisation and turntable azimuth, in accordance with the specification.

2.1.5 Example Calculation

Below 1 GHz:

Quasi-Peak level (dB μ V/m) = Receiver level (dB μ V) + Correction Factor (dB/m)
Margin (dB) = Quasi-Peak level (dB μ V/m) - Limit (dB μ V/m)

Above 1 GHz:

CISPR Average level (dB μ V/m) = Receiver level (dB μ V) + Correction Factor (dB/m)
Margin (dB) = CISPR Average level (dB μ V/m) - Limit (dB μ V/m)

Peak level (dB μ V/m) = Receiver level (dB μ V) + Correction Factor (dB/m)
Margin (dB) = Peak level (dB μ V/m) - Limit (dB μ V/m)



2.1.6 Example Test Setup Diagram

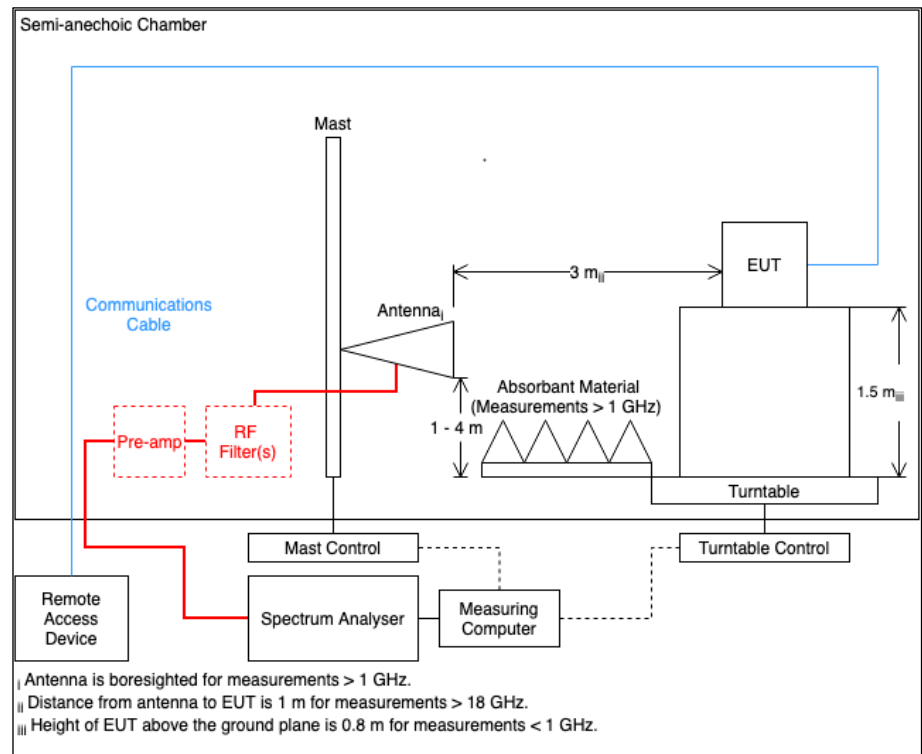


Figure 1

2.1.7 Environmental Conditions

Ambient Temperature 23.7 °C
Relative Humidity 46.6 %

2.1.8 Specification Limits

Required Specification Limits, Field Strength - Class B Test Limit at a 3 m Measurement Distance		
Frequency Range (MHz)	Test Limit (µV/m)	Test Limit (dBµV/m)
30 to 88	100	40.0
88 to 216	150	43.5
216 to 960	200	46.0
Above 960	500	54.0

Supplementary information:
Note 1. A Quasi-peak detector is to be used for measurements below 1 GHz.
Note 2. A CISPR Average detector is to be used for measurements above 1 GHz.
Note 3. The Peak test limit above 1 GHz is 20 dB higher than the CISPR Average test limit.

Table 7



2.1.9 Test Results

Results for Configuration and Mode: DC Powered - Operating.

This test was performed to the requirements of the Class B limits.

Performance assessment of the EUT made during this test: Pass.

Detailed results are shown below.

Highest frequency generated or used within the EUT: 928 MHz
Which necessitates an upper frequency test limit of: 5 GHz

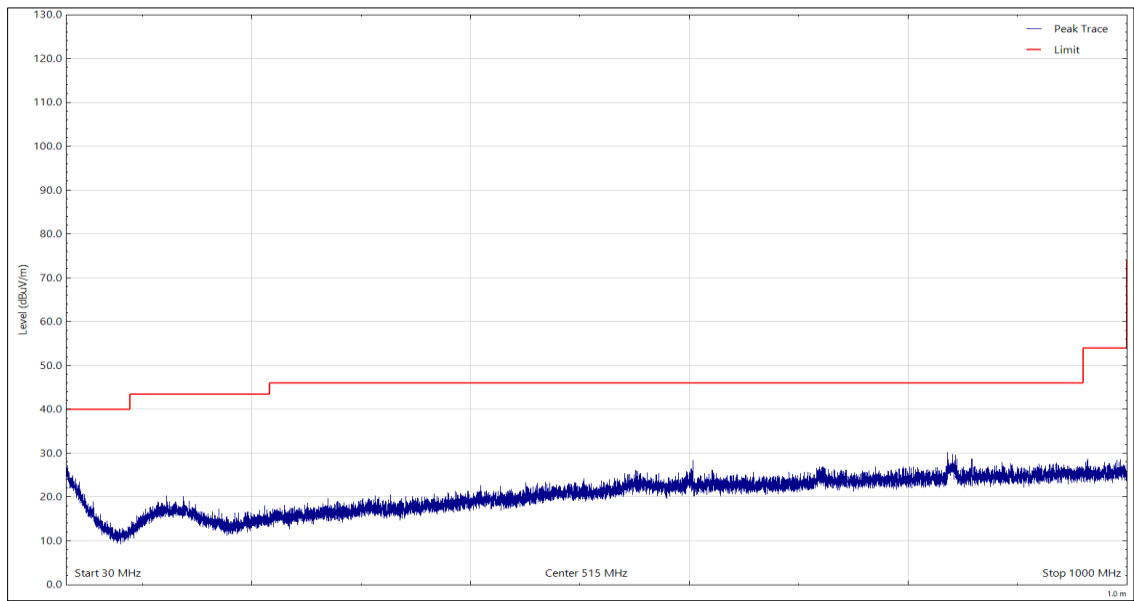


Figure 2 - 30 MHz to 1 GHz, Peak, Horizontal

Frequency (MHz)	Level (dBUV/m)	Limit (dBUV/m)	Margin (dB)	Detector	Angle (°)	Height (cm)	Polarisation
*							

Table 8

*No final measurements were made as all peak emissions seen above the measurement system noise floor during the pre-scan were greater than 10 dB below the test limit.

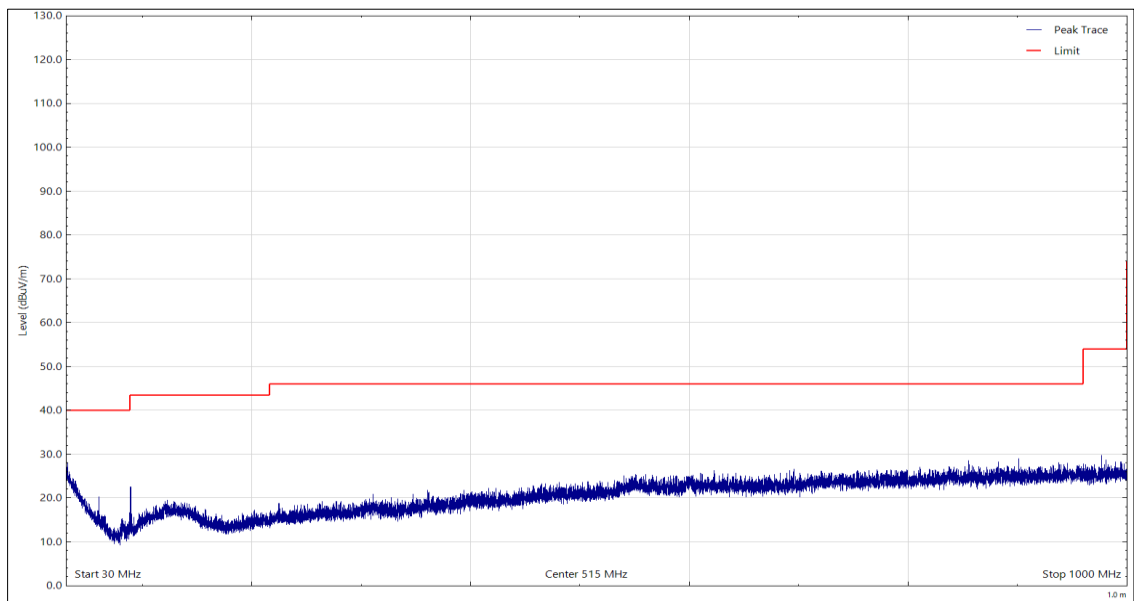


Figure 3 - 30 MHz to 1 GHz, Peak, Vertical

Frequency (MHz)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Angle (°)	Height (cm)	Polarisation
*							

Table 9

*No final measurements were made as all peak emissions seen above the measurement system noise floor during the pre-scan were greater than 10 dB below the test limit.

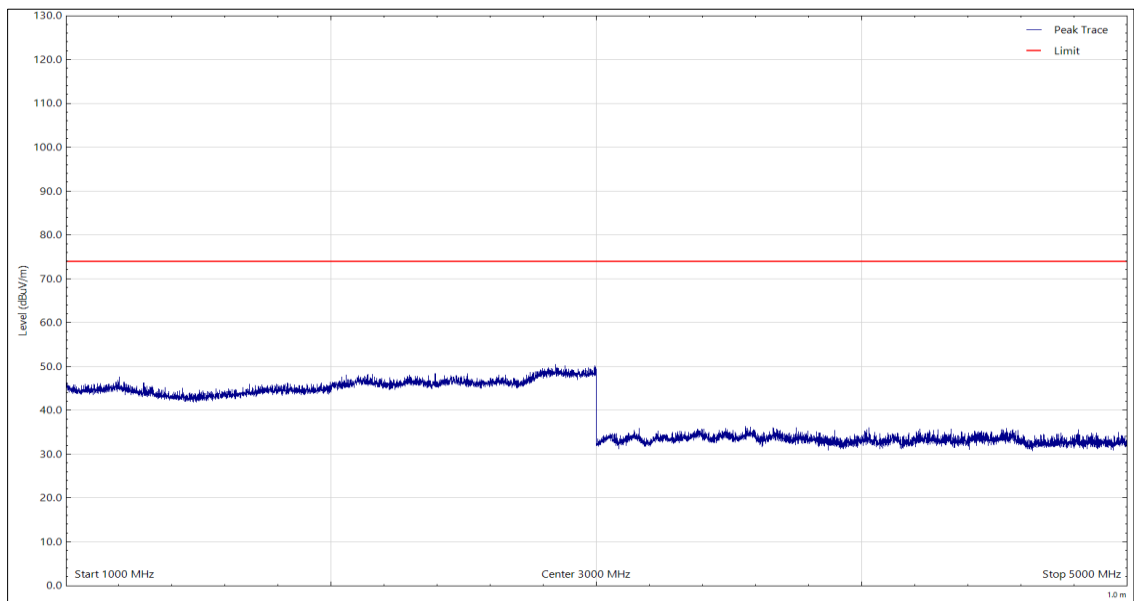


Figure 4 - 1 GHz to 5 GHz, Peak, Horizontal

Frequency (MHz)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Angle (°)	Height (cm)	Polarisation
*							

Table 10

*No final measurements were made as all peak emissions seen above the measurement system noise floor during the pre-scan were greater than 10 dB below the test limit.

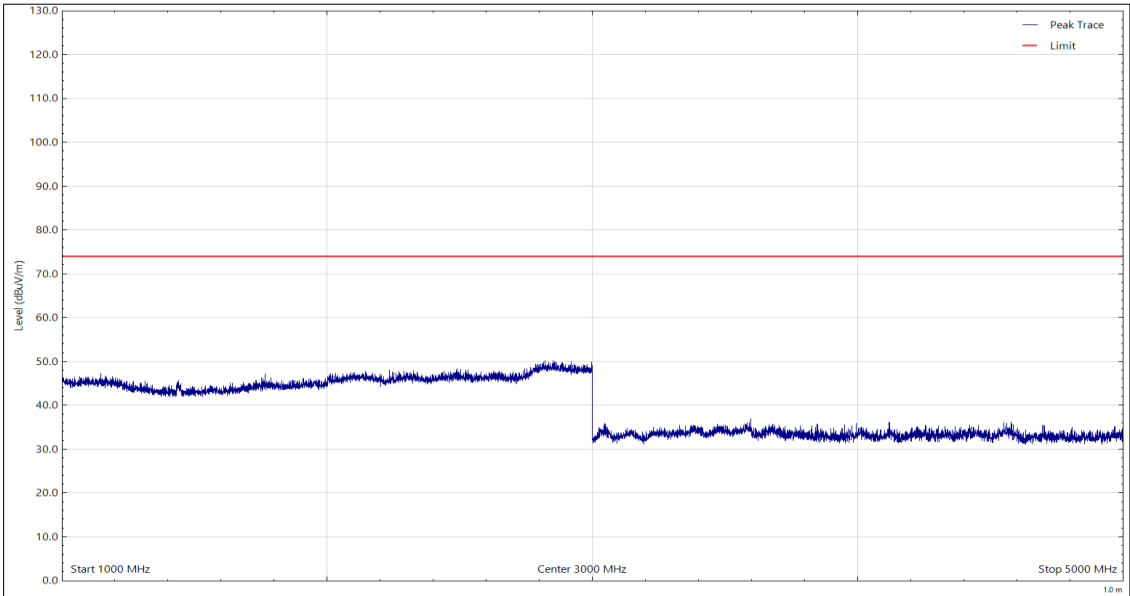


Figure 5 - 1 GHz to 5 GHz, Peak, Vertical

Frequency (MHz)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Angle (°)	Height (cm)	Polarisation
*							

Table 11

*No final measurements were made as all peak emissions seen above the measurement system noise floor during the pre-scan were greater than 10 dB below the test limit.

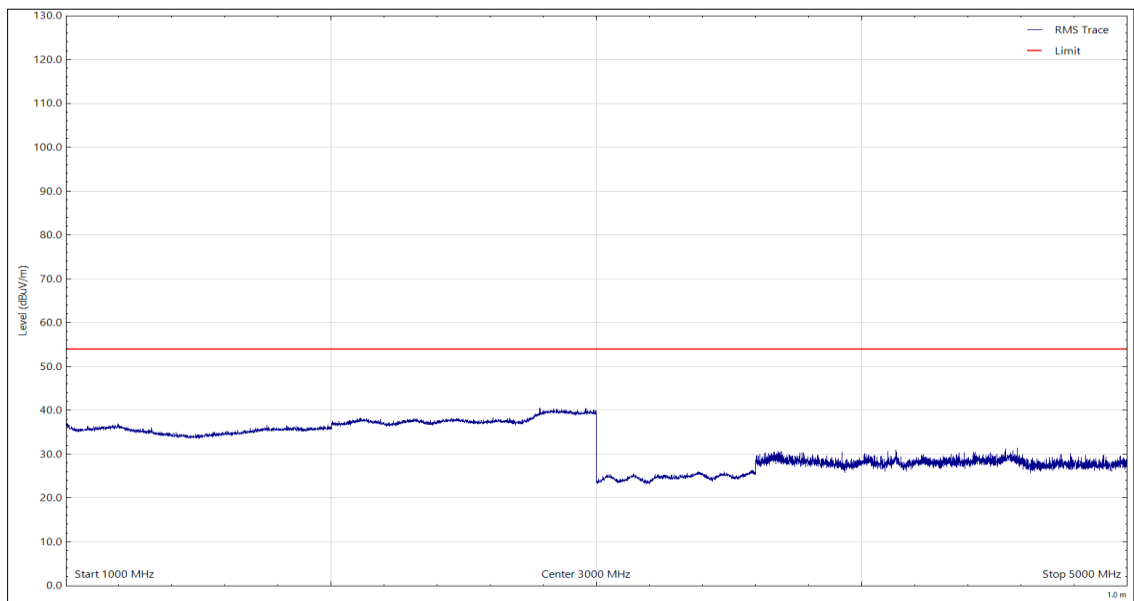


Figure 6 - 1 GHz to 5 GHz, CISPR Average, Horizontal

Frequency (MHz)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Angle (°)	Height (cm)	Polarisation
*							

Table 12

*No final measurements were made as all peak emissions seen above the measurement system noise floor during the pre-scan were greater than 10 dB below the test limit.

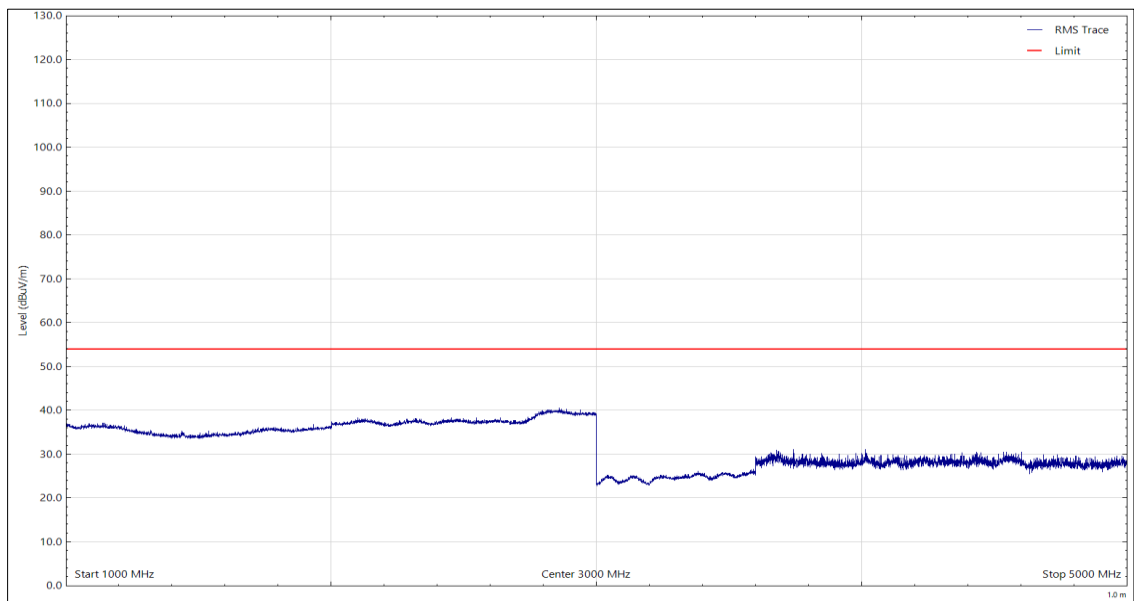


Figure 7 - 1 GHz to 5 GHz, CISPR Average, Vertical

Frequency (MHz)	Level (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Detector	Angle (°)	Height (cm)	Polarisation
*							

Table 13

*No final measurements were made as all peak emissions seen above the measurement system noise floor during the pre-scan were greater than 10 dB below the test limit.

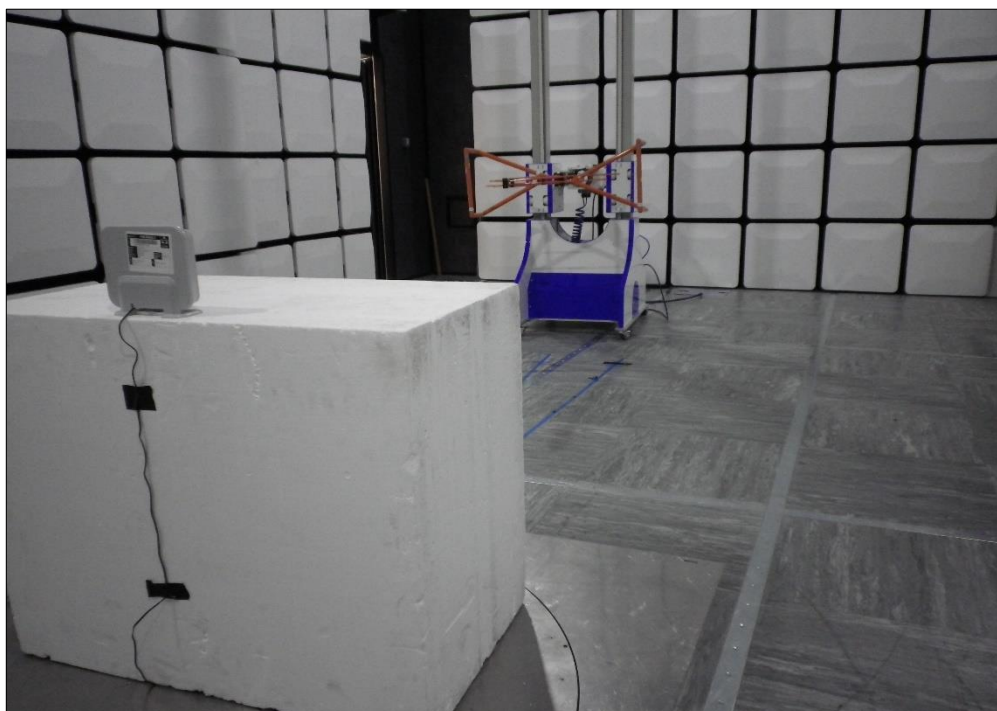


Figure 8 - Test Setup - 30 MHz to 1 GHz

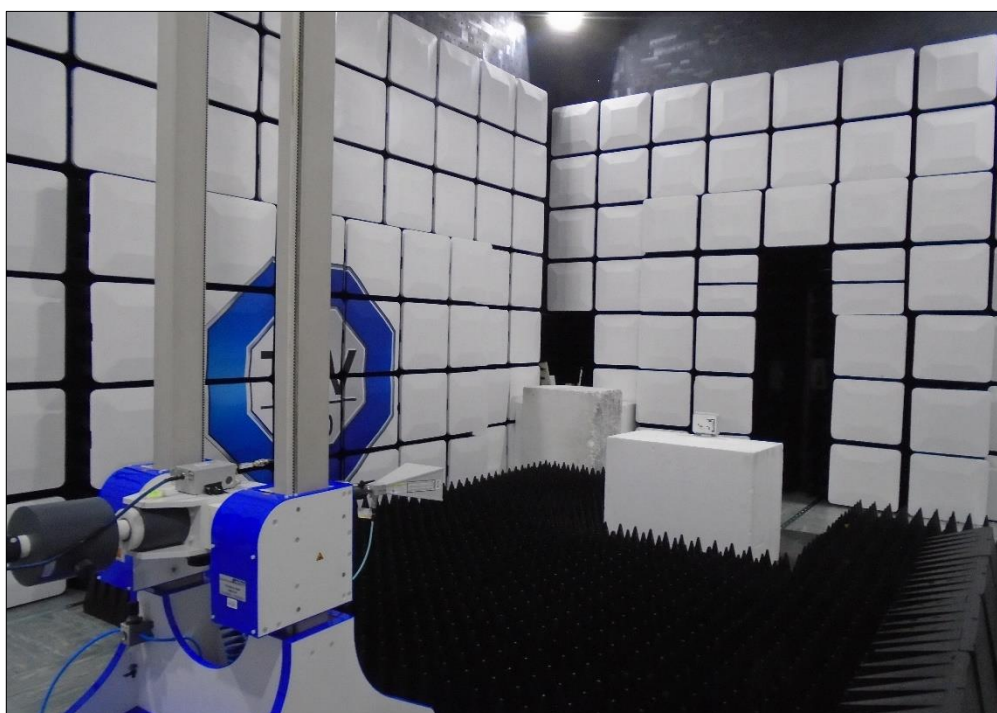


Figure 9 - Test Setup - 1 GHz to 5 GHz



2.1.10 Test Location and Test Equipment Used

This test was carried out in EMC Chamber 12.

Instrument	Manufacturer	Type No	TE No	Calibration Period (months)	Calibration Expires
Screened Room (12)	MVG	EMC-3	5621	36	11-Aug-2023
EmX Emissions Software	TUV SUD	V2.1.11	5125	-	Software
Test Receiver	Rohde & Schwarz	ESU40	3506	12	18-Mar-2022
Turntable & Mast Controller	Maturo Gmbh	NCD/498/2799.01	5612	-	TU
Tilt Antenna Mast	Maturo Gmbh	TAM 4.0-P	5613	-	TU
Cable (K-Type to K-Type, 2 m)	Scott Cables	KPS-1501-2000-KPS	4526	6	06-Mar-2022
Cable (N-Type to N-Type, 8 m)	Teledyne	PR90-088-8MTR	5450	6	08-Mar-2022
Cable (N-Type to N-Type, 1 m)	Rosenberger	LU7-036-1000	5031	12	23-Jul-2022
Preamplifier (30dB 1GHz to 18GHz)	Schwarzbeck	BBV 9718 C	5350	12	22-Sep-2022
Antenna with permanent attenuator (Bilog)	Schaffner	CBL6143	287	24	14-Oct-2022
Broadband Horn Antenna (1-10 GHz)	Schwarzbeck	BBHA 9120 B	5611	12	15-Oct-2022
Multimeter	Fluke	79 Series II	3057	12	23-Aug-2022
Thermo-Hygro-Barometer	PCE Instruments	PCE-THB-40	5481	12	31-Mar-2022

Table 14

TU - Traceability Unscheduled



3 Test Equipment Information

3.1 General Test Equipment Used

Instrument	Manufacturer	Type No	TE No	Calibration Period (months)	Calibration Expires
Multimeter	Fluke	79 Series II	3057	12	23-Aug-2022
Thermo-Hygro-Barometer	PCE Instruments	PCE-THB-40	5481	12	31-Mar-2022

Table 15



4 Incident Reports

No incidents reports were raised.



5 Measurement Uncertainty

For a 95% confidence level, the measurement uncertainties for defined systems are:

Test Name	Measurement Uncertainty
Radiated Disturbance	30 MHz to 1 GHz, Bilog Antenna, ± 5.2 dB 1 GHz to 40 GHz, Horn Antenna, ± 6.3 dB

Table 16

Worst case error for both Time and Frequency measurement 12 parts in 10^6 .

Measurement Uncertainty Decision Rule

Determination of conformity with the specification limits is based on the decision rule according to IEC Guide 115:2007, Clause 4.4.3 and 4.5.1. (Procedure 2). The measurement results are directly compared with the test limit to determine conformance with the requirements of the standard.

Risk: The uncertainty of measurement about the measured result is negligible with regard to the final pass/fail decision. The measurement result can be directly compared with the test limit to determine conformance with the requirement (compare IEC Guide 115). The level of risk to falsely accept and falsely reject items is further described in ILAC-G8.