


Appendix D



Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

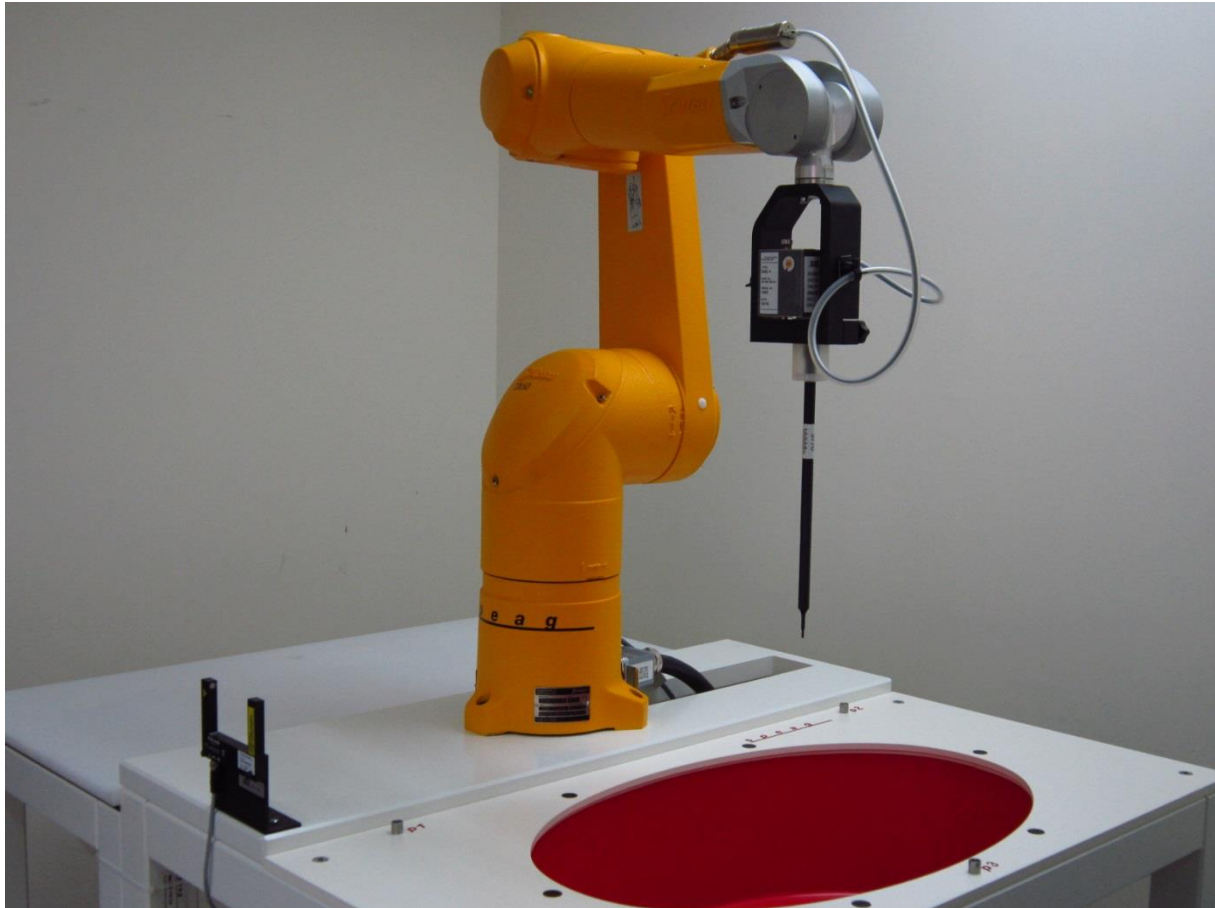

2. Photographs of Tissue Simulate Liquid

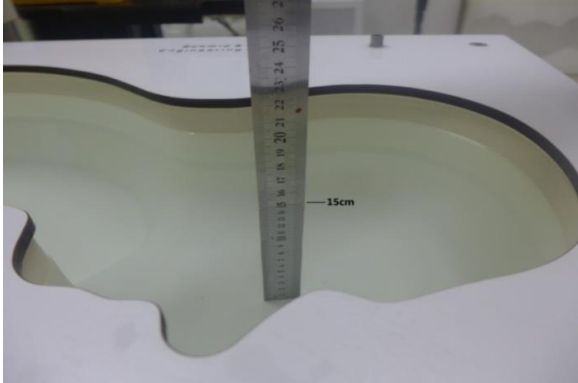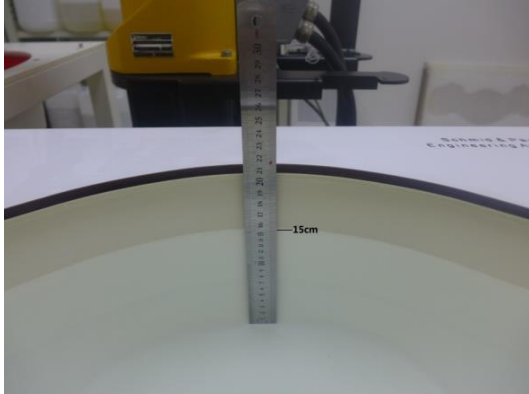Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 2450
	

3. Photographs of EUT test position

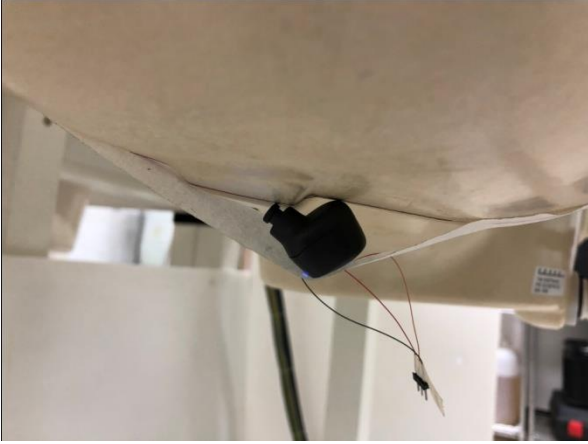
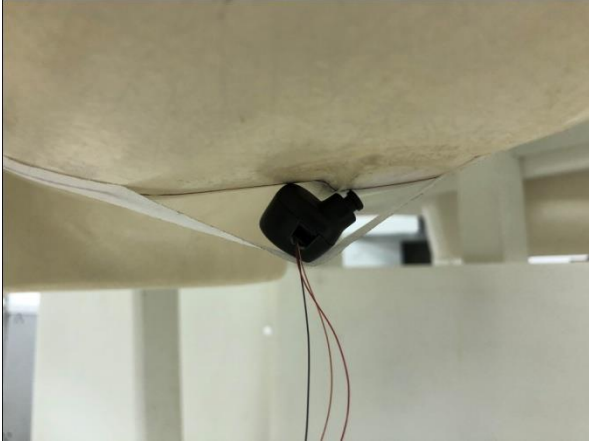
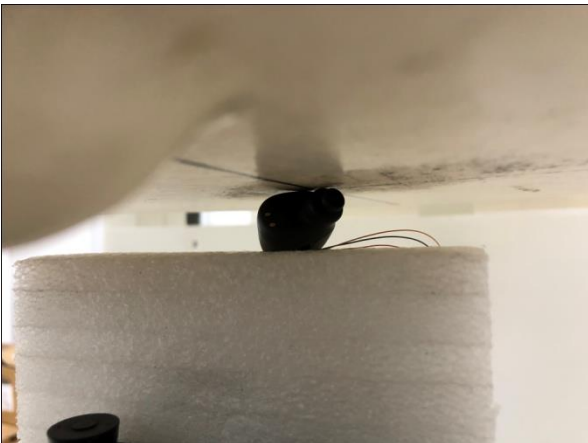
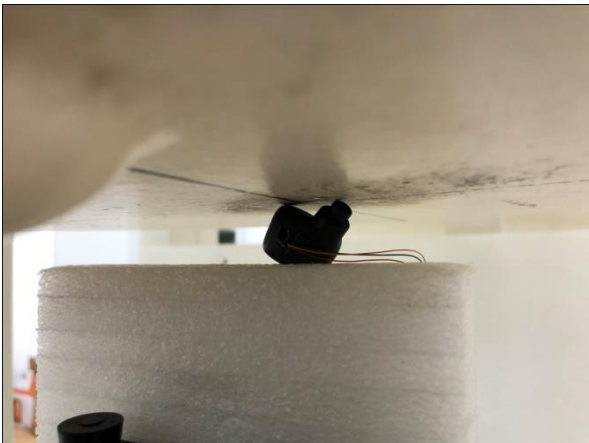
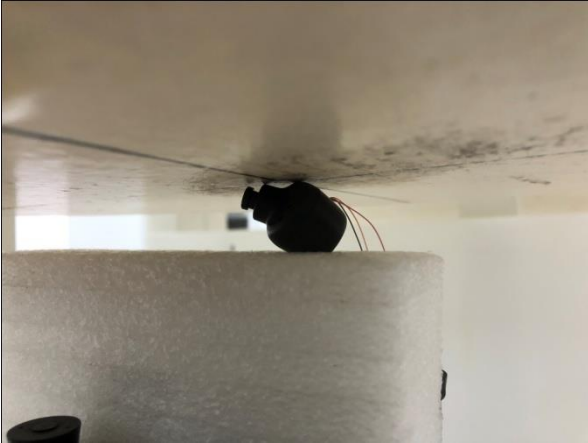
Photo 3: Right cheek 0mm	Photo 4: Left cheek 0mm
	
Photo 5: Side 1 0mm	Photo 6: Side 2 0mm
	
Photo 7: Side 3 0mm	Photo 8: Side 4 0mm
	

Photo 9: Side 5 0mm	Photo 10: Side 6 0mm
	
Photo 11: Side 7 0mm	Photo 12: Side 8 0mm
	

4. EUT Constructional Details

Details please Refer to the <External Photos>&<Internal Photos>.