

System Check_Head_13MHz

DUT: CLA-13 - SN1011

Communication System: CW; Frequency: 13.000 MHz

Medium: HSL_4-250_260610 Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.757$ S/m; $\epsilon_r = 55.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(17.55, 17.18, 17.51); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=30.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.543 W/kg; SAR (10g) = 0.439 W/kg;

TSL Correction: Positive only

Pin=30.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.04 dB

SAR (1g) = 0.515 W/kg; SAR (8g) = 0.338 W/kg; SAR (10g) = 0.319 W/kg

Smallest distance from peaks to all points 3 dB below = 15.8 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

TSL Correction: Positive only

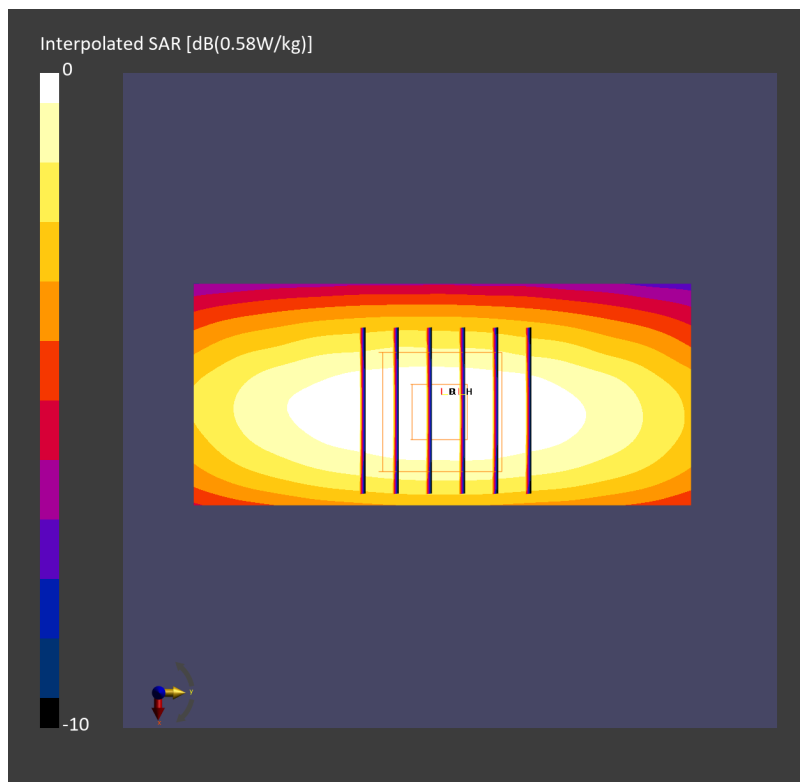

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260603 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.867$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(9.08, 8.91, 9.18); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.09 W/kg; SAR (10g) = 1.39 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.06 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.38 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 90.0 %

TSL Correction: Positive only

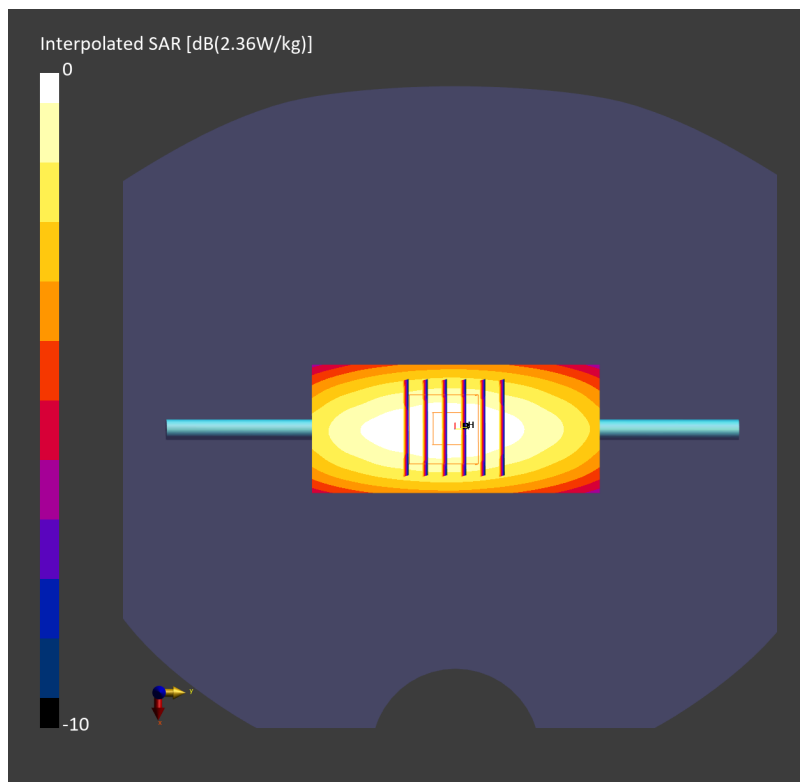

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260609 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.926$ S/m; $\epsilon_r = 43.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(9.69, 9.27, 10.31); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.22 W/kg; SAR (10g) = 1.48 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.05 dB

SAR (1g) = 2.25 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 86.4 %

TSL Correction: Positive only

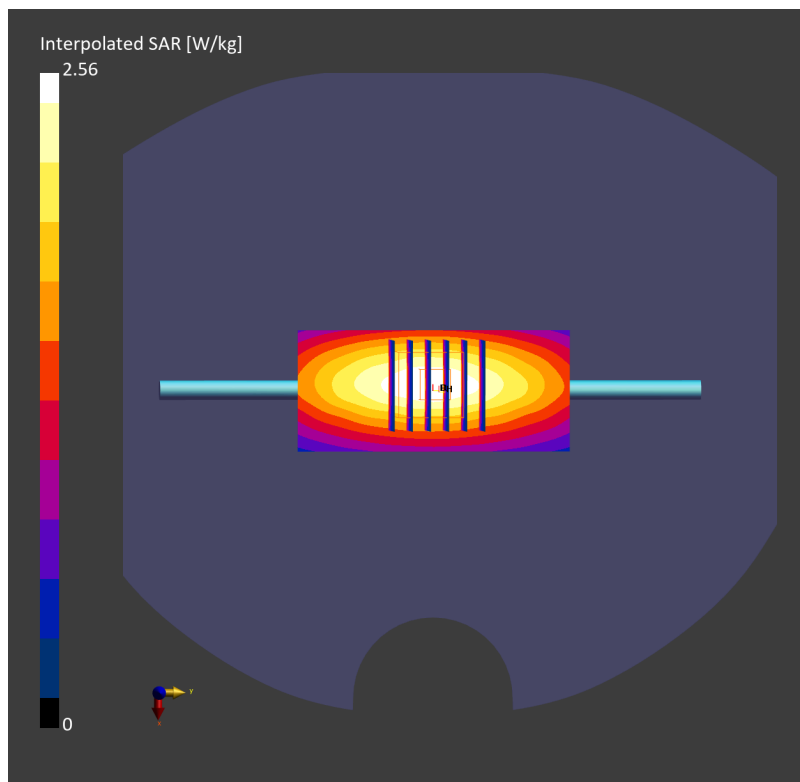

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260603 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.895$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(8.84, 8.67, 8.94); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.60 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.41 W/kg; SAR (8g) = 1.69 W/kg; SAR (10g) = 1.60 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 90.1 %

TSL Correction: Positive only

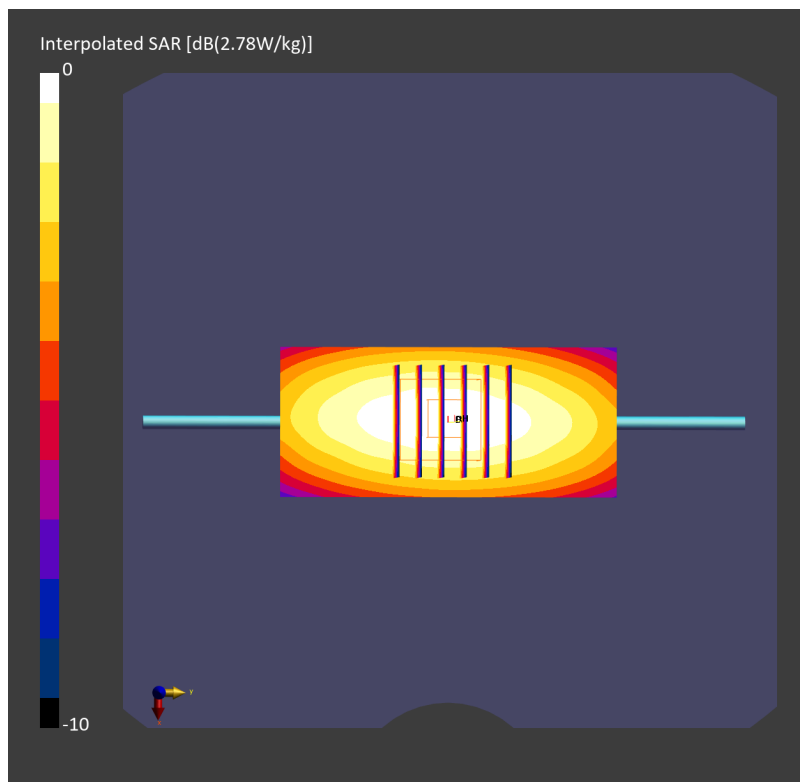

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260609 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.954$ S/m; $\epsilon_r = 43.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(9.56, 9.14, 10.17); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.37 W/kg; SAR (10g) = 1.56 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.06 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.69 W/kg; SAR (10g) = 1.61 W/kg

Smallest distance from peaks to all points 3 dB below = 20.4 mm

Ratio of SAR at M2 to SAR at M1 = 86.6 %

TSL Correction: Positive only

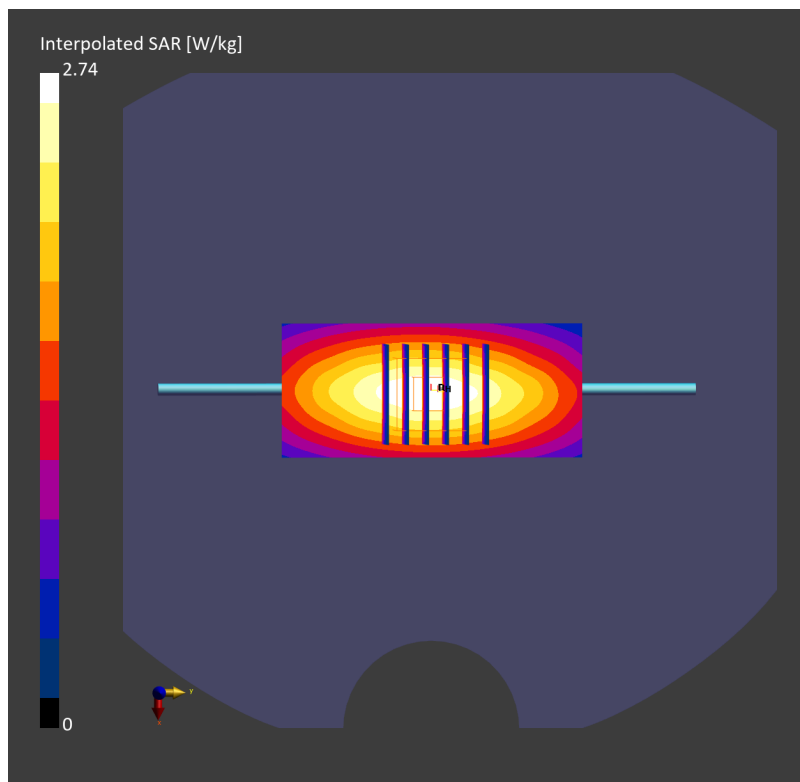

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260604 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.25, 7.12, 7.34); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.3 W/kg; SAR (10g) = 5.32 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 10.1 W/kg; SAR (8g) = 5.74 W/kg; SAR (10g) = 5.28 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.7 %

TSL Correction: Positive only

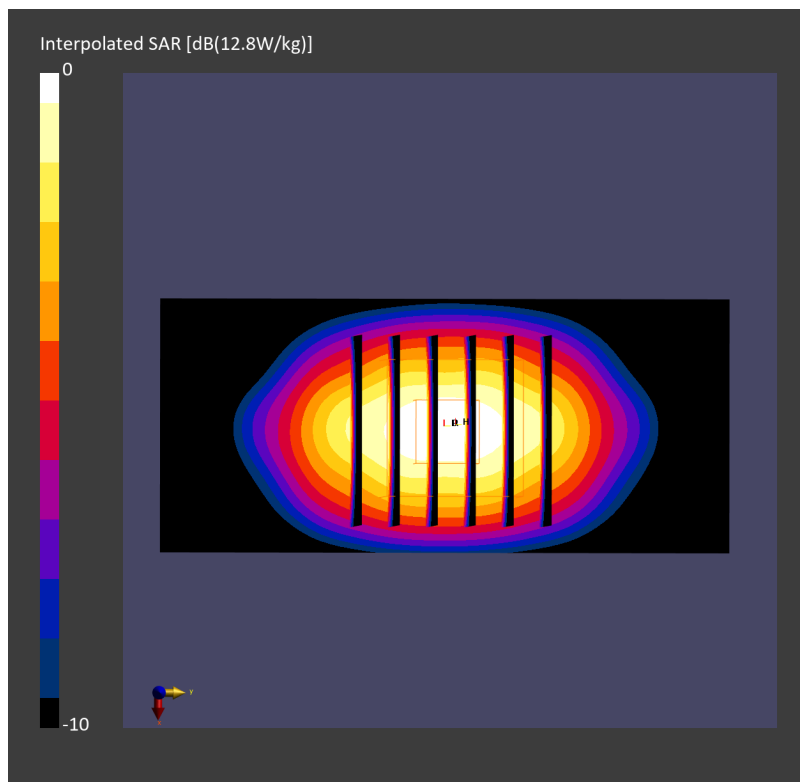

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260608 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.54, 7.21, 8.01); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.97 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 1.98 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 83.7 %

TSL Correction: Positive only

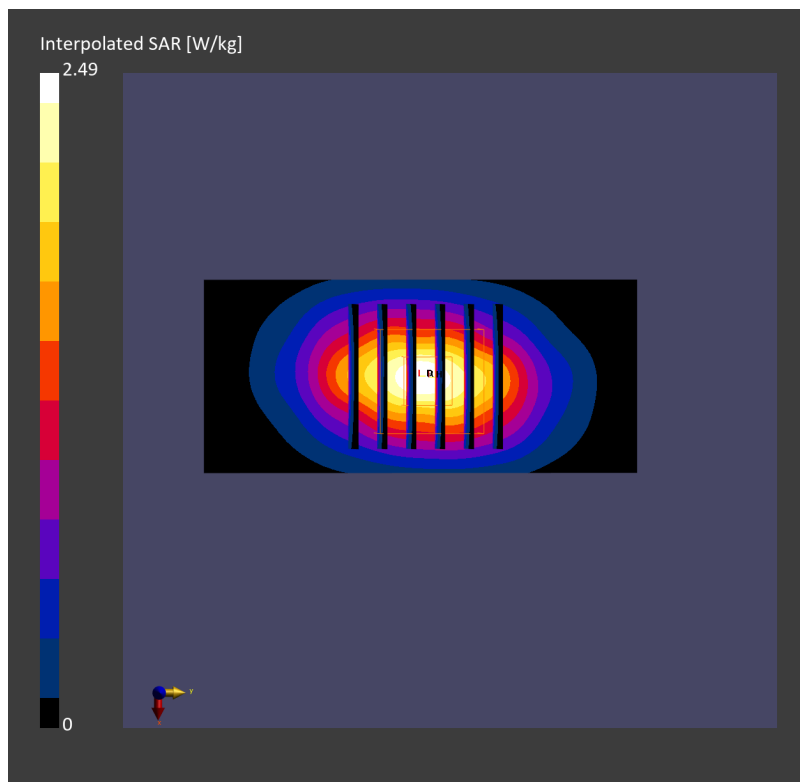

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260616 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 40.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.54, 7.21, 8.01); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.92 W/kg; SAR (10g) = 0.985 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.8 %

TSL Correction: Positive only

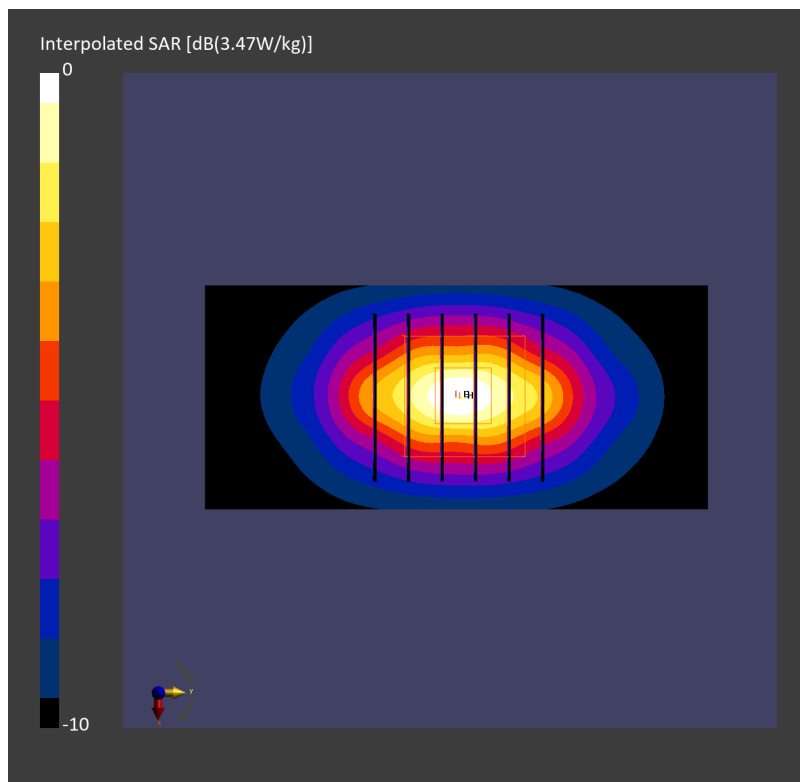

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260630 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.96 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.95 W/kg; SAR (8g) = 1.11 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 83.9 %

TSL Correction: Positive only

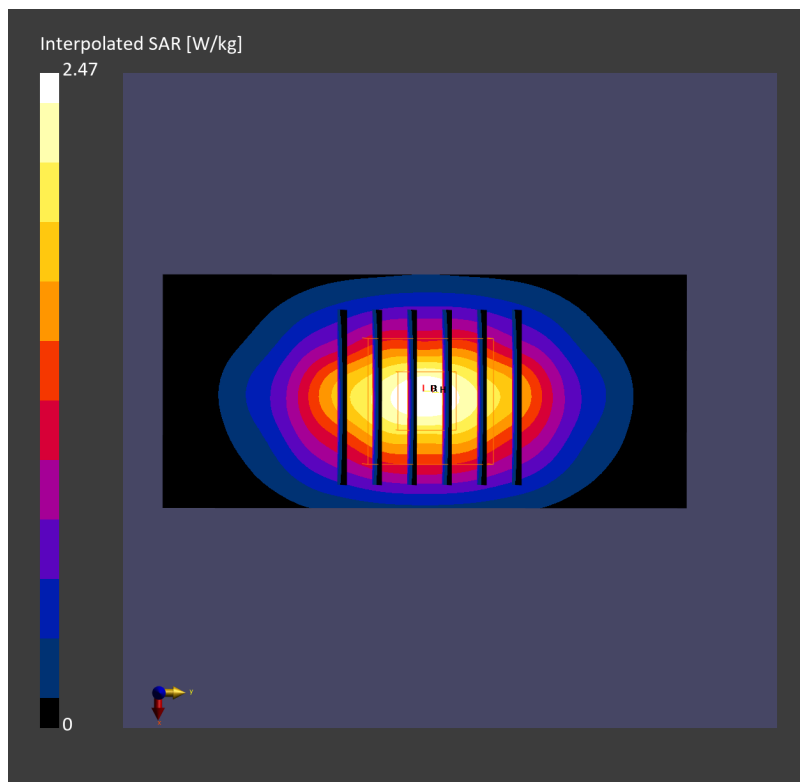

System Check_Head_2450MHz

DUT: D2450V2 - SN929

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260605 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.79$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.06, 6.75, 7.51); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.10 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.42 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

TSL Correction: Positive only

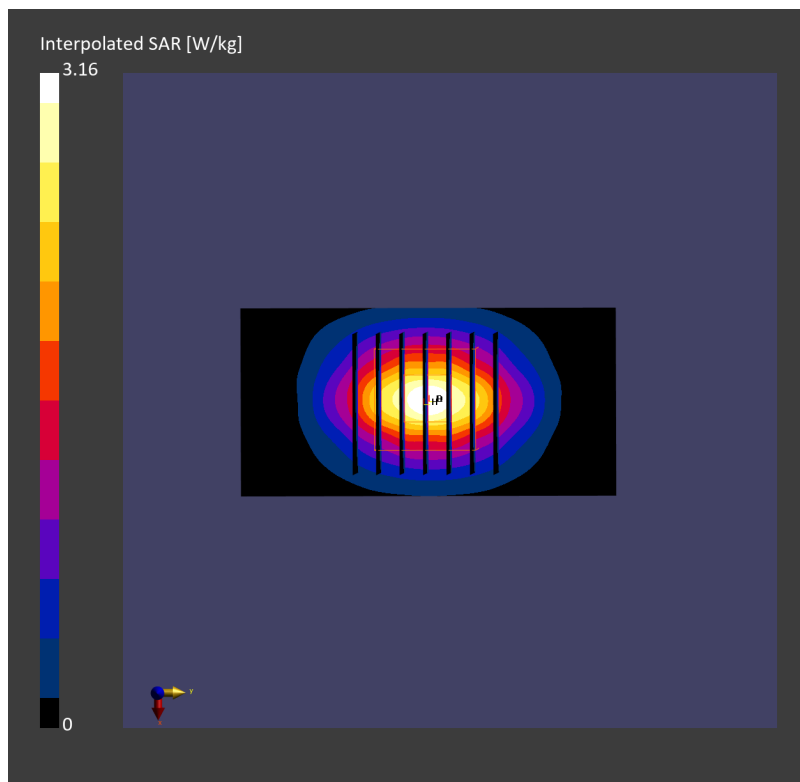

System Check_Head_2450MHz

DUT: D2450V2 - SN736

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260608 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.06, 6.75, 7.51); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.49 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

TSL Correction: Positive only

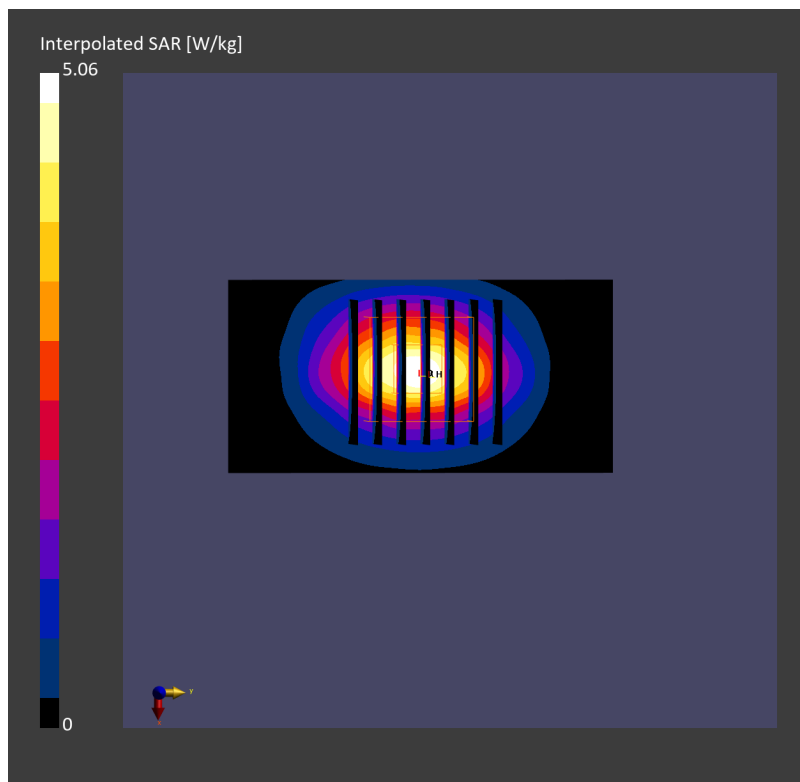

System Check_Head_2450MHz

DUT: D2450V2 - SN736

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260612 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.06, 6.75, 7.51); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.41 W/kg; SAR (10g) = 1.11 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.44 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

TSL Correction: Positive only

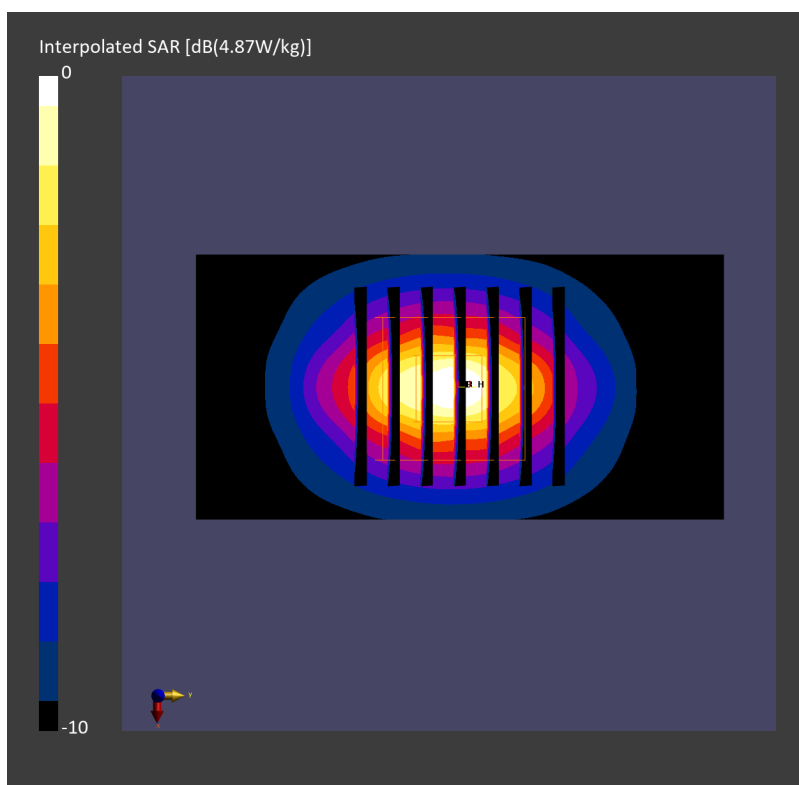

System Check_Head_2450MHz

DUT: D2450V2 - SN929

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260616 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.06, 6.75, 7.51); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.48 W/kg; SAR (10g) = 1.12 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.10 dB

SAR (1g) = 2.41 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

TSL Correction: Positive only

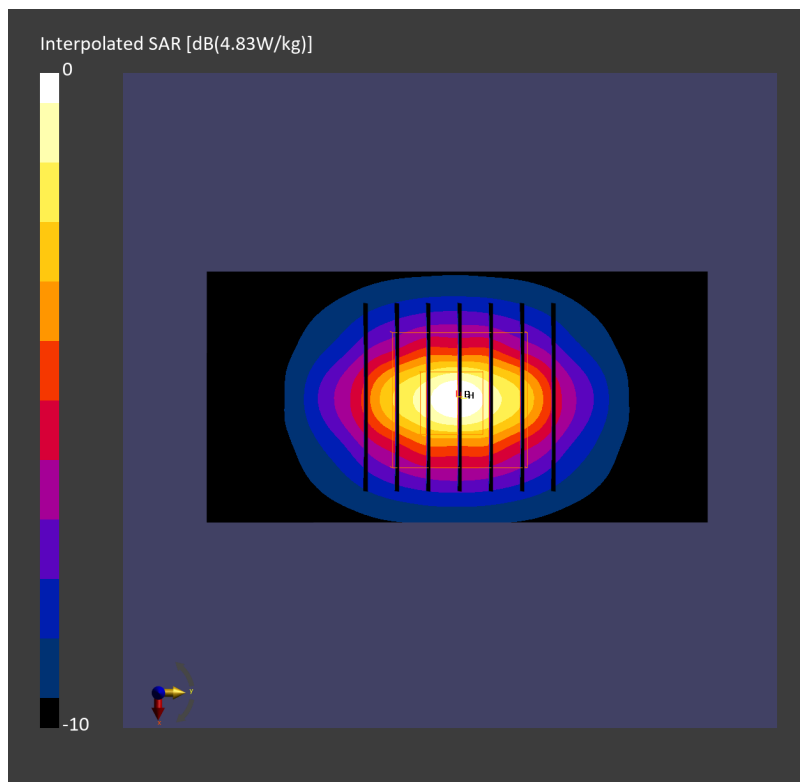

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260608 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.95, 6.65, 7.39); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=16.9dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.50 W/kg; SAR (10g) = 1.11 W/kg;

TSL Correction: Positive only

Pin=16.9dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.51 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.6 %

TSL Correction: Positive only

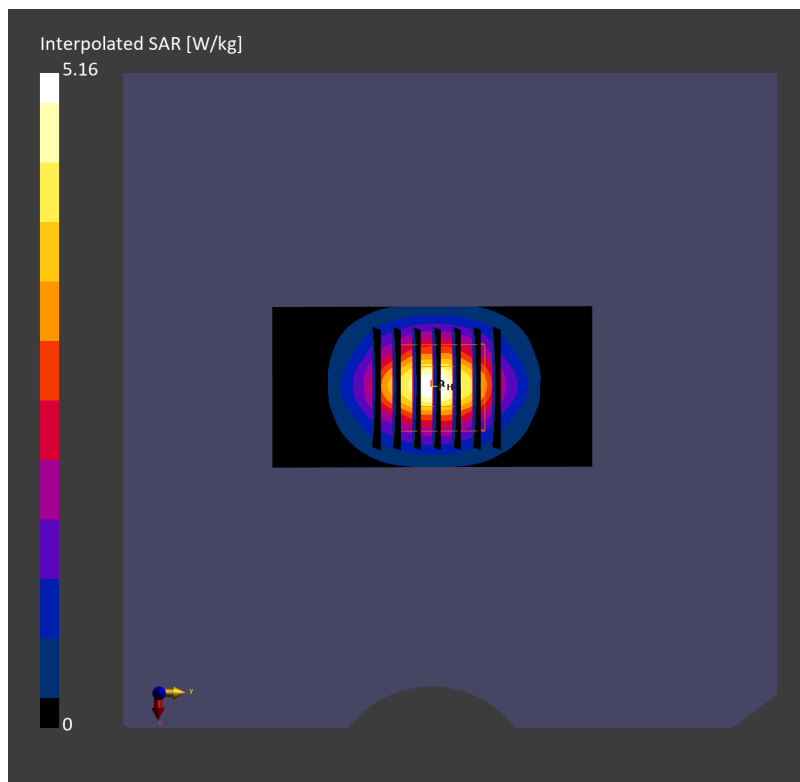

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260612 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(6.95, 6.65, 7.39); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.72 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.77 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.5 %

TSL Correction: Positive only

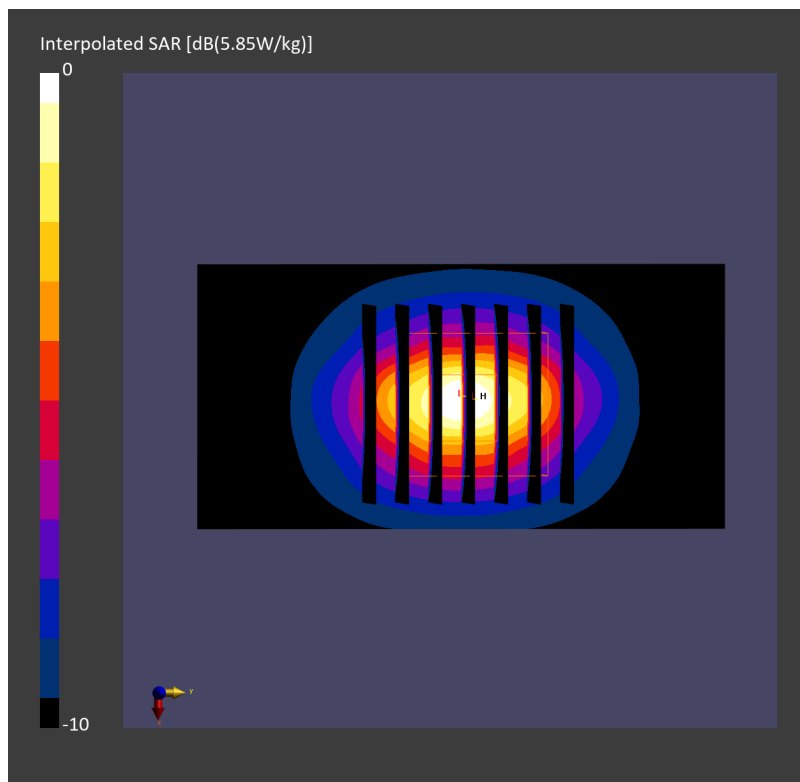

System Check_Head 2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260625 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.15, 7.62, 7.2); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.41 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 2.54 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.1 %

TSL Correction: Positive only

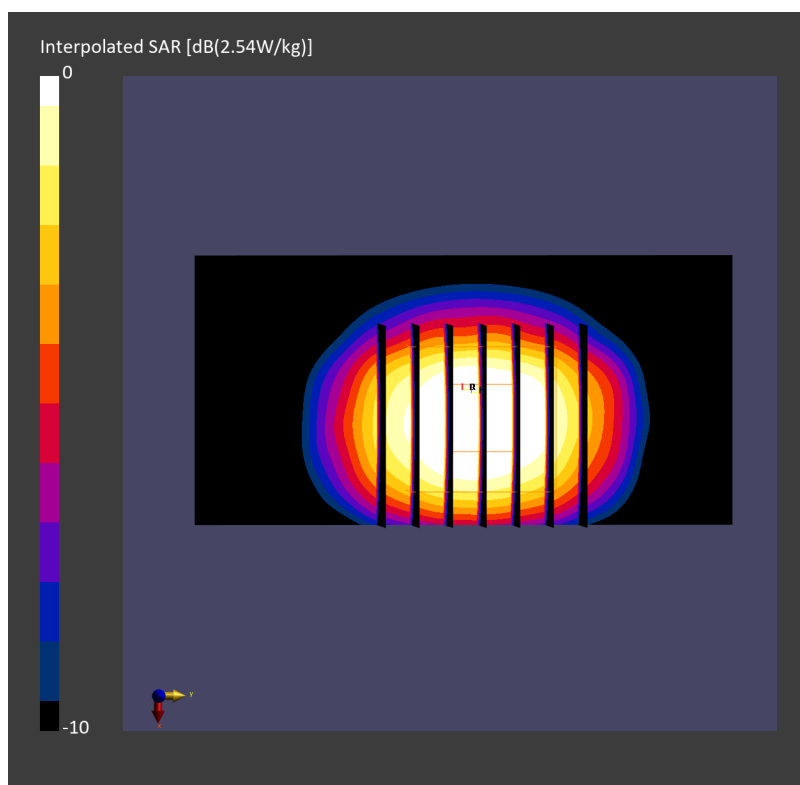

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260629 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.56 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.4 %

TSL Correction: Positive only

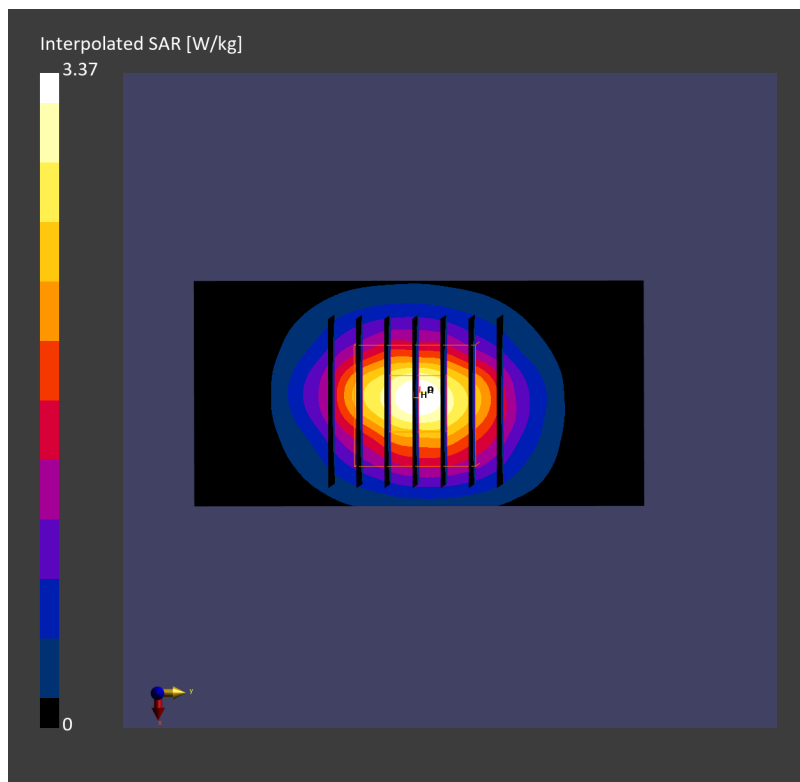

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260605 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.42$ S/m; $\epsilon_r = 33.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(5.46, 5.22, 5.81); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=16.7dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.03 W/kg; SAR (10g) = 0.880 W/kg;

TSL Correction: Positive only

Pin=16.7dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.03 dB

SAR (1g) = 3.41 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 0.986 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.9 %

TSL Correction: Positive only

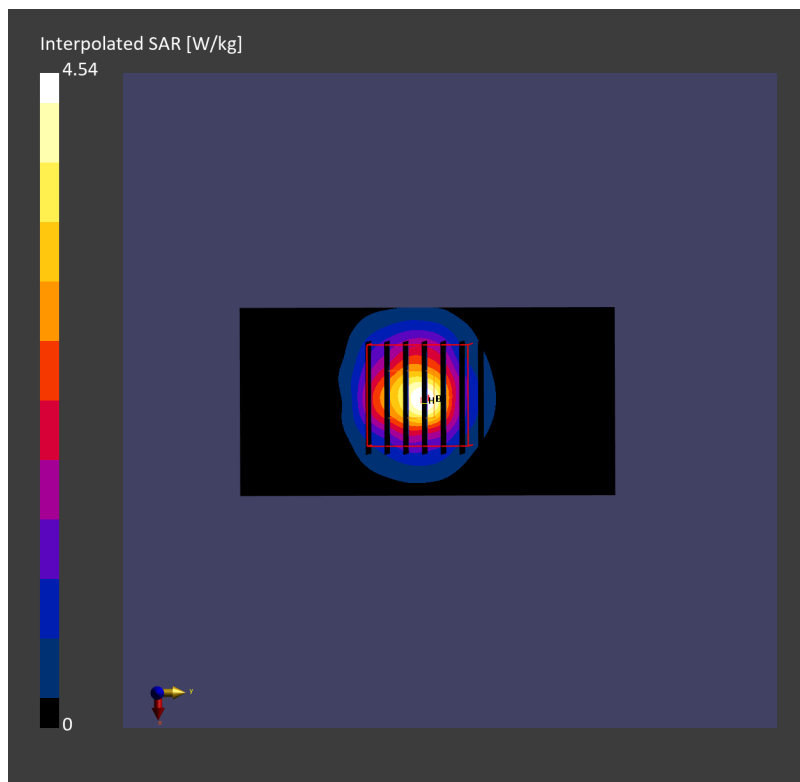

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260609 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.52$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(5.46, 5.22, 5.81); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=16.8dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.07 W/kg; SAR (10g) = 0.932 W/kg;

TSL Correction: Positive only

Pin=16.8dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.48 W/kg; SAR (8g) = 1.18 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 63.7 %

TSL Correction: Positive only

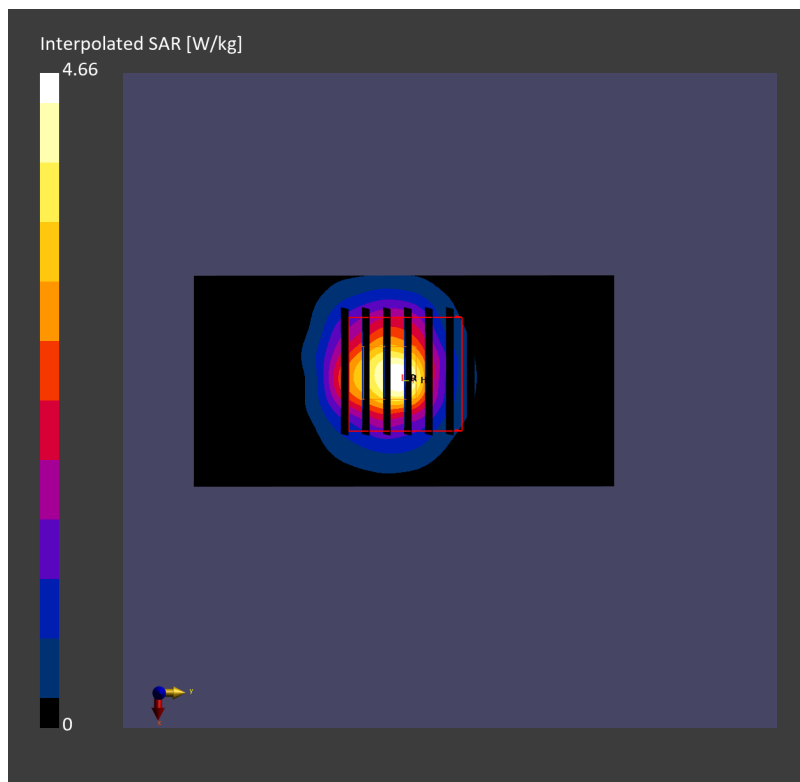

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260625 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.67$ S/m; $\epsilon_r = 36.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.8, 5.38, 5.76); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=16.8dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.18 W/kg; SAR (10g) = 0.615 W/kg;

TSL Correction: Positive only

Pin=16.8dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.18 dB

SAR (1g) = 3.51 W/kg; SAR (8g) = 0.972 W/kg; SAR (10g) = 0.996 W/kg

Smallest distance from peaks to all points 3 dB below = 6.8 mm

Ratio of SAR at M2 to SAR at M1 = 54.9 %

TSL Correction: Positive only

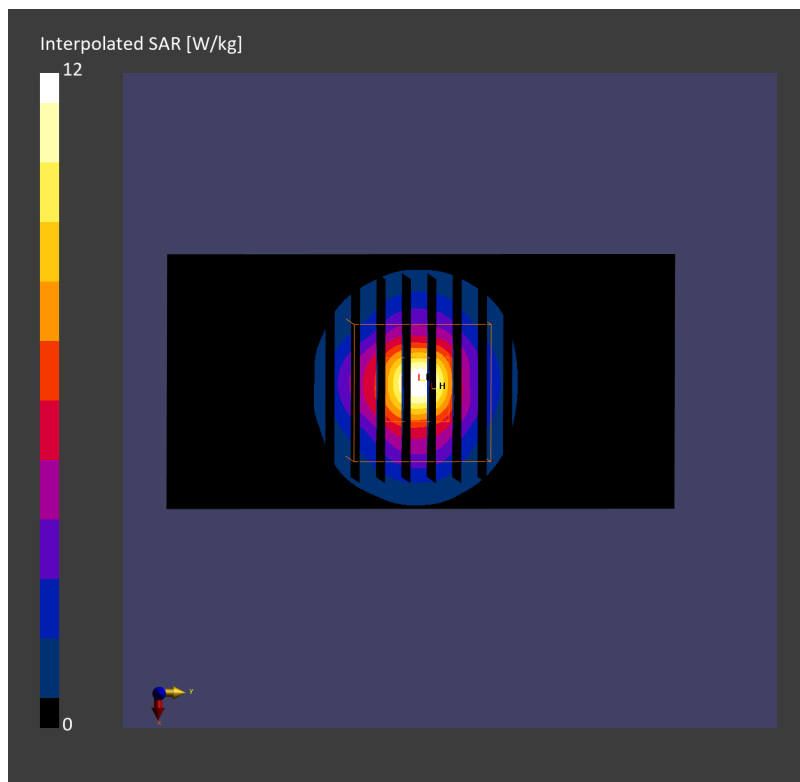

System Check_Head 5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260625 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.67$ S/m; $\epsilon_r = 36.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(5.4, 5.76, 5.43); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (28.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.86 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 62.9 %

TSL Correction: Positive only

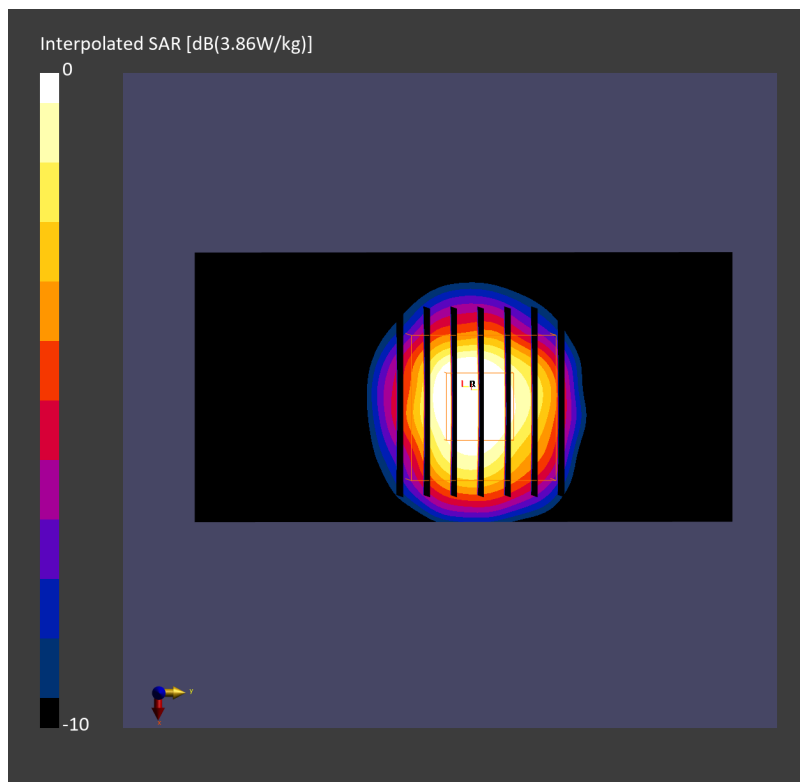

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260605 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.80$ S/m; $\epsilon_r = 33.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(5.03, 4.81, 5.35); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=16.7dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.22 W/kg; SAR (10g) = 0.948 W/kg;

TSL Correction: Positive only

Pin=16.7dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.62 W/kg; SAR (8g) = 1.22 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 6.9 mm

Ratio of SAR at M2 to SAR at M1 = 60.5 %

TSL Correction: Positive only

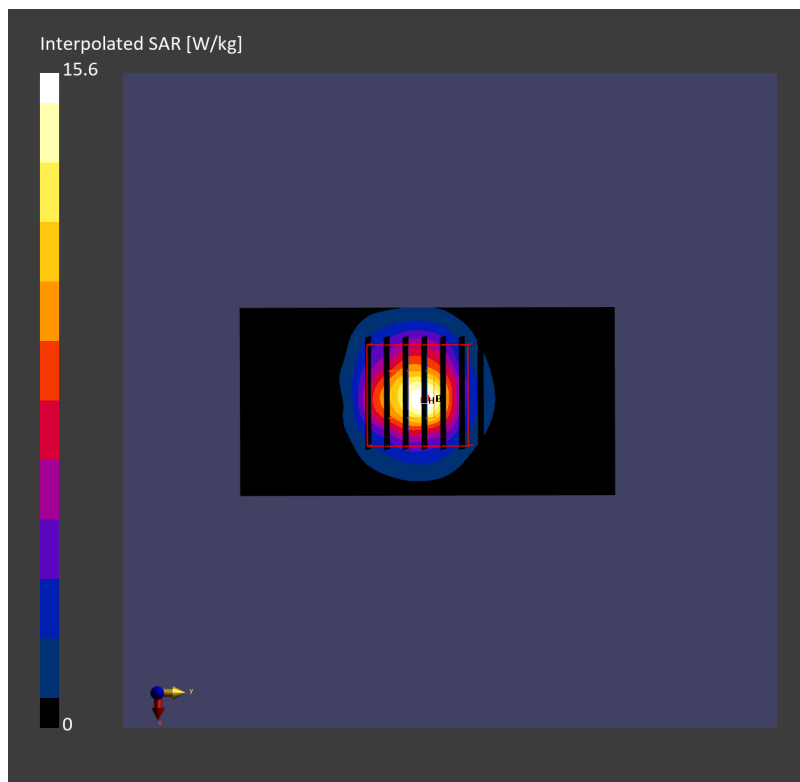

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260609 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.90$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(5.03, 4.81, 5.35); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.33 W/kg; SAR (10g) = 0.991 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.05 dB

SAR (1g) = 3.81 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 60.3 %

TSL Correction: Positive only

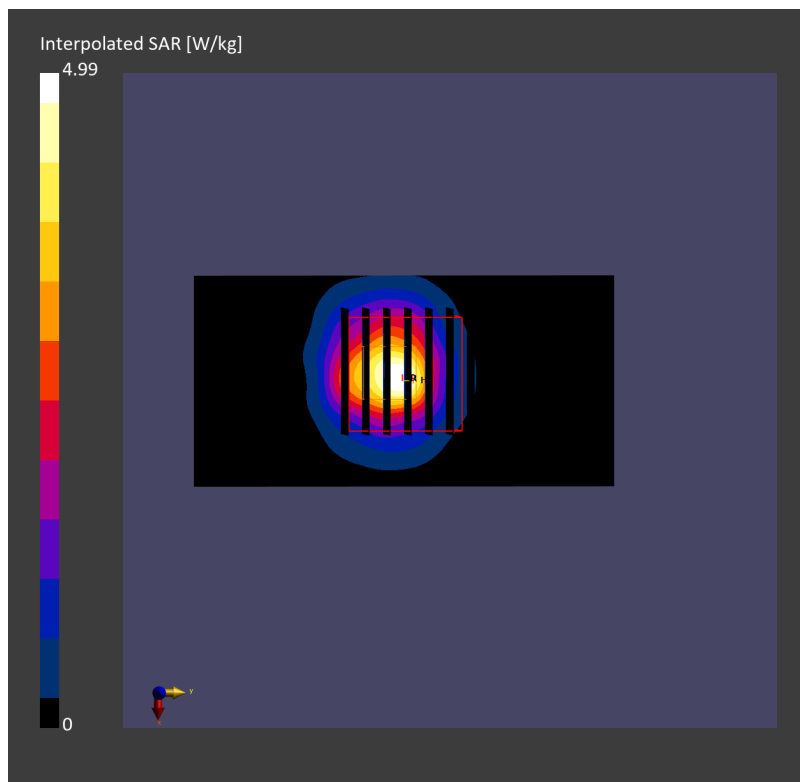

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260625 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.01$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.38, 5.0, 5.35); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=16.9dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.23 W/kg; SAR (10g) = 0.624 W/kg;

TSL Correction: Positive only

Pin=16.9dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.14 dB

SAR (1g) = 3.84 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 52.3 %

TSL Correction: Positive only

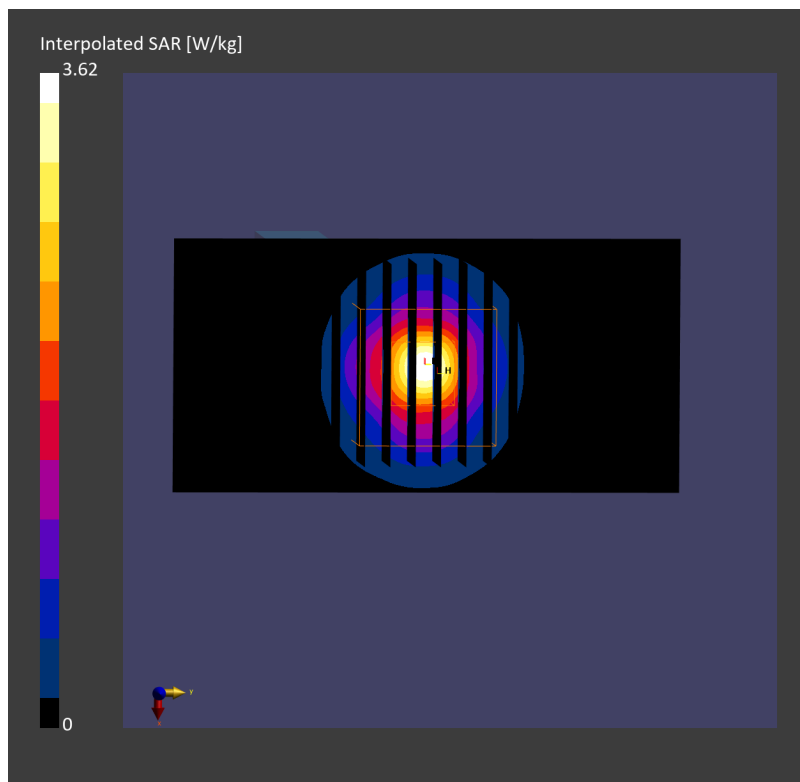

System Check_Head_5800MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260605 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.01$ S/m; $\epsilon_r = 32.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(4.92, 4.71, 5.23); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=16.8dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 0.930 W/kg;

TSL Correction: Positive only

Pin=16.8dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.03 dB

SAR (1g) = 3.55 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 58.1 %

TSL Correction: Positive only

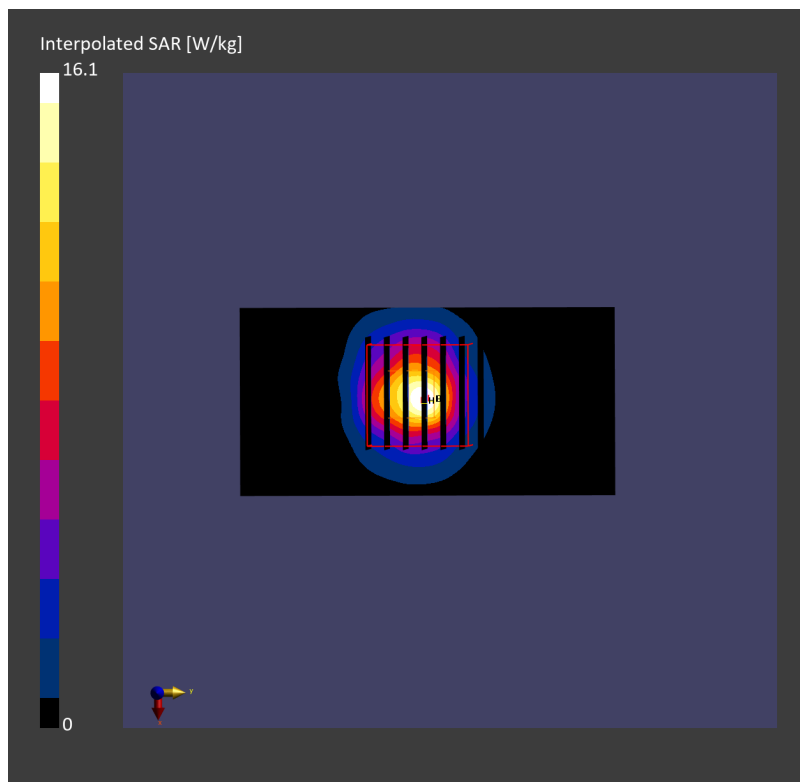

System Check_Head_5800MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260609 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.14$ S/m; $\epsilon_r = 35.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(4.92, 4.71, 5.23); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.23 W/kg; SAR (10g) = 0.969 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.05 dB

SAR (1g) = 3.73 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 58.1 %

TSL Correction: Positive only

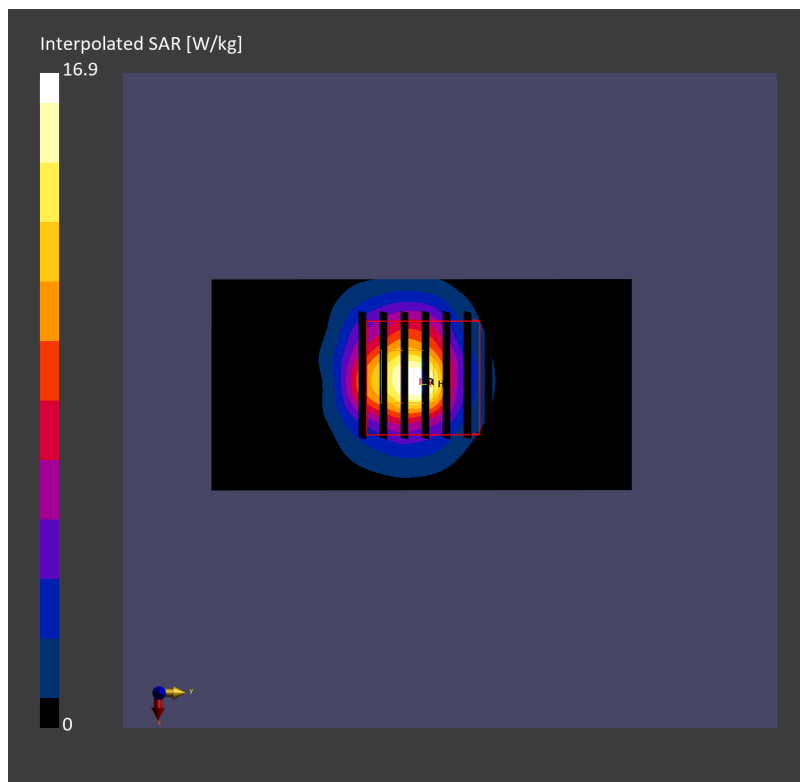

System Check_Head_5800MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260617 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.06$ S/m; $\epsilon_r = 33.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(4.92, 4.71, 5.23); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.28 W/kg; SAR (10g) = 0.924 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 3.81 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 57.6 %

TSL Correction: Positive only

