SN Label

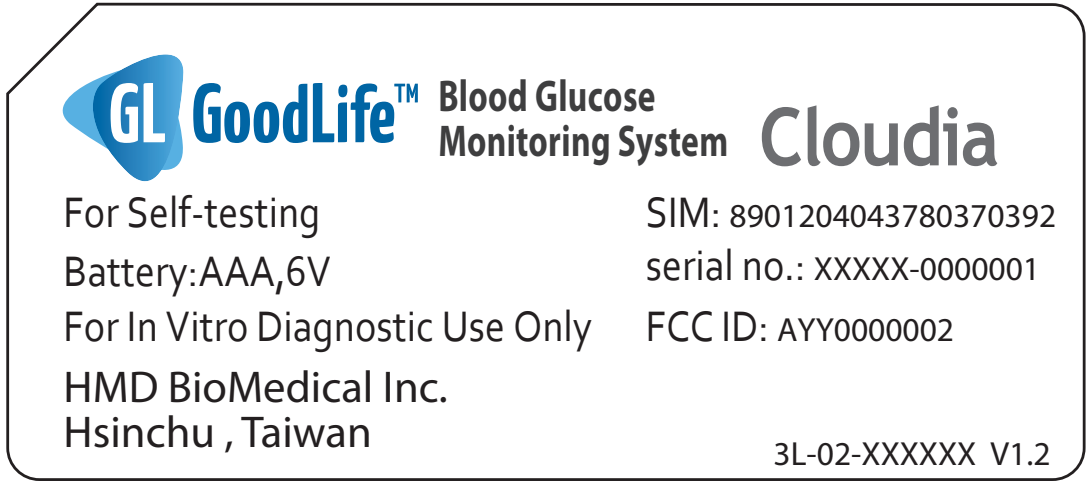
GL GoodLife™ Blood Glucose Monitoring System Cloudia
For Self-testing
Battery:AAA,6V
For In Vitro Diagnostic Use Only
HMD BioMedical Inc.
Hsinchu , Taiwan
SIM: 8901204043780370392
serial no.: XXXXX-0000001
FCC ID: AYY0000002
3L-02-XXXXXX V1.2