


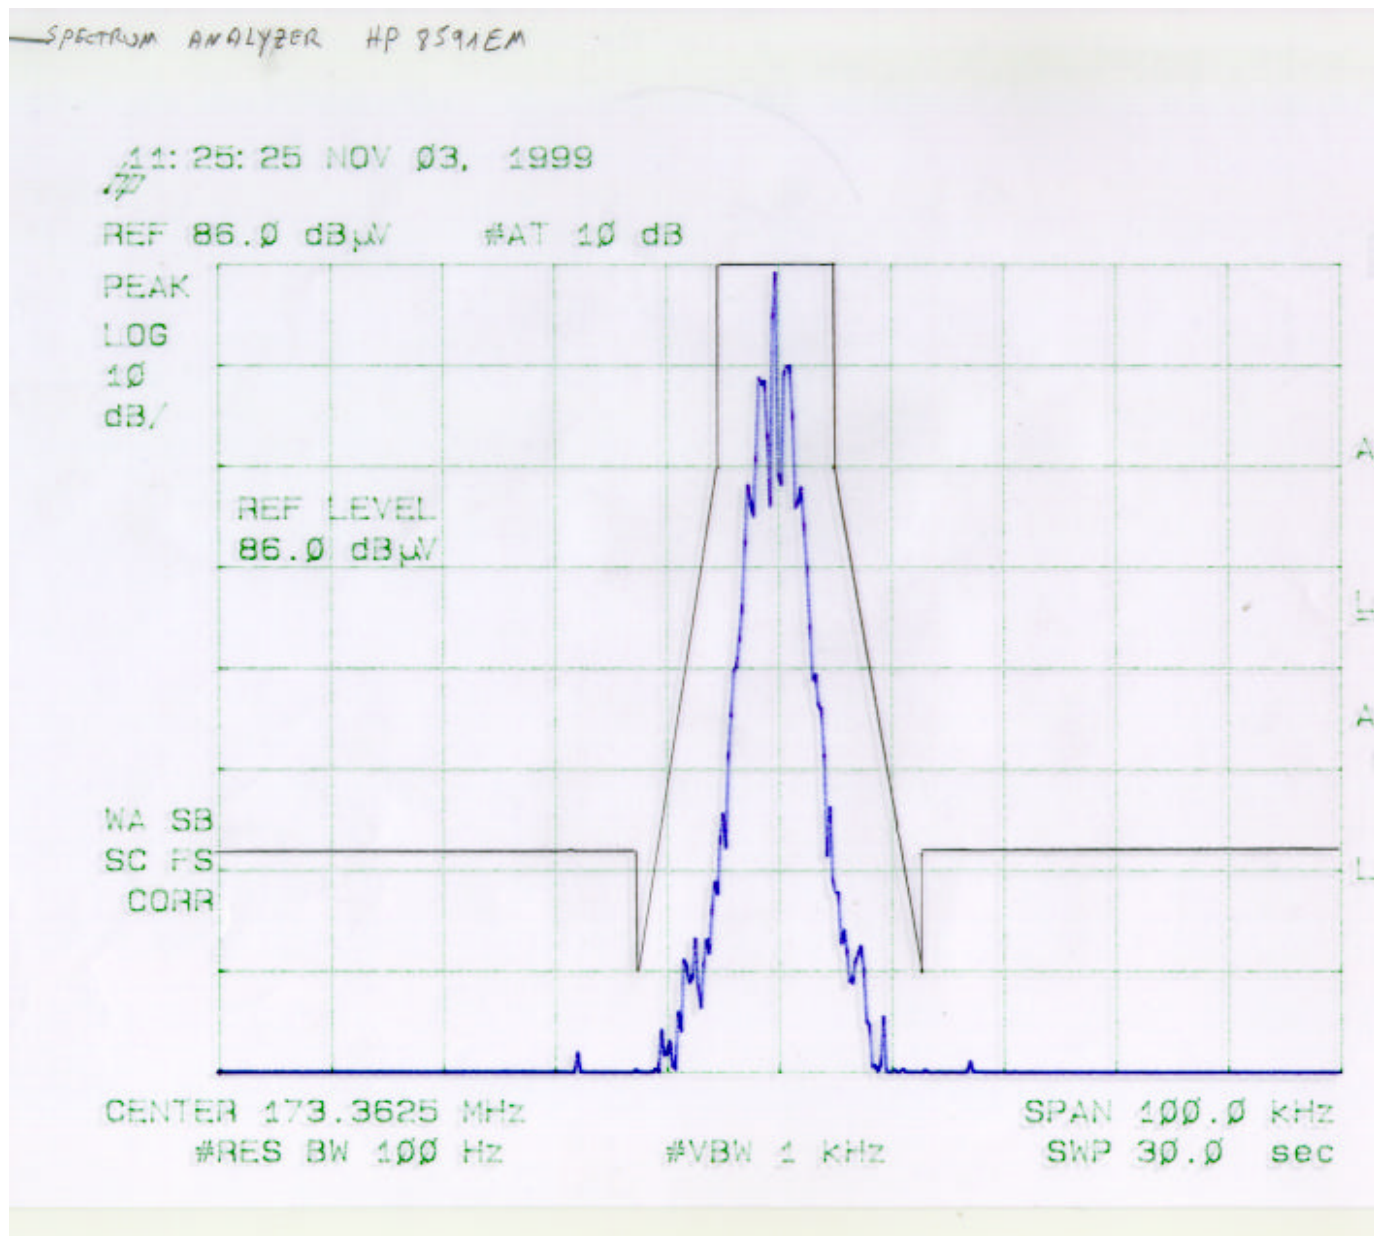

SPECTRUM ANALYZER HP 8594EM

11:20:16 NOV 03, 1999

REF 86.0 dB μ W #AT 10 dB

PEAK

LOG

10

dB/

REF LEVEL
86.0 dB μ W

WA SB

SC FS

CORR

CENTER 154.4563 MHz

#RES BW 100 Hz

#VBW 1 kHz

SPAN 100.0 kHz

SWP 30.0 sec

