

# CERTIFICATE OF CALIBRATION

ISSUED BY UL VS LTD

DATE OF ISSUE: 10/Oct/2017

CERTIFICATE NUMBER : 11903941JD01A



5248

UL VS LTD  
PAVILION A  
ASHWOOD PARK, ASHWOOD WAY  
BASINGSTOKE, HAMPSHIRE  
RG23 8BG, UK  
TEL: +44 (0) 1256 312000  
FAX: +44 (0) 1256 312001  
Email: LST.UK.Calibration@ul.com



Page 1 of 10

APPROVED SIGNATORY

Naseer Mirza

## Customer :

UL VS Inc  
47173 Benicia Street  
Fremont, CA 94538, USA

## Equipment Details:

|                    |                                           |                  |             |
|--------------------|-------------------------------------------|------------------|-------------|
| Description:       | Dipole Validation Kit                     | Date of Receipt: | 29/Sep/2017 |
| Manufacturer:      | Speag                                     |                  |             |
| Type/Model Number: | D900V2                                    |                  |             |
| Serial Number:     | 1d143                                     |                  |             |
| Calibration Date:  | 05/Oct/2017                               |                  |             |
| Calibrated By:     | Chanthu Thevarajah<br>Laboratory Engineer |                  |             |

Signature:

All Calibration have been conducted in the closed laboratory facility: Lab Temperature (22±3) °C and humidity < 70%

This certificate is issued in accordance with the laboratory accreditation requirements of the United Kingdom Accreditation Service. It provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

Use of the UKAS mark demonstrates that compliance with the requirements of BS/EN/ISO/IEC 17025 has been independently assessed.

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01A

Page 2 of 10

The calibration methods and procedures used were as detailed in:

1. **IEC 62209-1:2005**: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
2. **IEC 62209-2:2010**: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)
3. **IEEE 1528: 2013**: IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques
4. FCC KDB Publication Number: "KDB865664 D01 SAR Measurement 100 MHz to 6 GHz"
5. **SPEAG DASY4/ DASY5 System Handbook**

The measuring equipment used to perform the calibration, documented in this certificate has been calibrated in accordance with the manufacturers' recommendations, and is traceable to recognized national standards.

| UL No.     | Instrument                   | Manufacturer    | Type No.      | Serial No.  | Date Last Calibrated  | Cal. Interval (Months) |
|------------|------------------------------|-----------------|---------------|-------------|-----------------------|------------------------|
| A2546      | Data Acquisition Electronics | SPEAG           | DAE4          | 1435        | 10 Feb 2017           | 12                     |
| A2110      | Data Acquisition Electronics | SPEAG           | DAE4          | 431         | 18 Nov 2016           | 12                     |
| A2587      | Probe                        | SPEAG           | ES3DV3        | 3341        | 14 Aug 2017           | 12                     |
| A2201      | Dipole                       | SPEAG           | D900V2        | 035         | 14 Feb 2017           | 12                     |
| PRE0151451 | Power Monitoring Kit         | Art-Fi          | ART 100850-01 | 0001        | Cal as part of System | 12                     |
| PRE0151441 | Power Sensor                 | Rhode & Schwarz | NRP8S         | 102481      | 16 Nov 2016           | 12                     |
| PRE0151154 | Network Analyser             | Rhode & Schwarz | ZND8          | 100151      | 22 Nov 2016           | 12                     |
| PRE0151877 | Calibration Kit              | Rhode & Schwarz | Z135          | 102947-Bt   | 02 Dec 2016           | 12                     |
| M1908      | Signal Generator             | Rhode & Schwarz | SMIQ 03B      | 1125.555.03 | 08 Nov 2016           | 12                     |

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01A

Page 3 of 10

### SAR System Specification

|                          |                                            |
|--------------------------|--------------------------------------------|
| Robot System Positioner: | Stäubli Unimation Corp. Robot Model: TX60L |
| Robot Serial Number:     | F14/5T5ZA1/A/01                            |
| DASY Version:            | DASY 52 (v52.8.8.1258)                     |
| Phantom:                 | Flat section of SAM Twin Phantom           |
| Distance Dipole Centre:  | 15 mm (with spacer)                        |
| Frequency:               | 900 MHz                                    |

### Dielectric Property Measurements – Head Simulating Liquid (HSL)

| Simulant Liquid | Frequency (MHz) | Room Temp |         | Liquid Temp |        | Parameters  | Target Value | Measured Value | Uncertainty (%) |
|-----------------|-----------------|-----------|---------|-------------|--------|-------------|--------------|----------------|-----------------|
|                 |                 | Start     | End     | Start       | End    |             |              |                |                 |
| Head            | 900             | 23.0 °C   | 22.0 °C | 20.0°C      | 22.0°C | $\epsilon'$ | 41.50        | 41.34          | ± 5%            |
|                 |                 |           |         |             |        | $\sigma$    | 0.97         | 0.93           | ± 5%            |

### SAR Results – Head Simulating Liquid (HSL)

| Simulant Liquid | SAR Measured          | 250 mW input Power | Normalised to 1.00 W | Uncertainty (%) |
|-----------------|-----------------------|--------------------|----------------------|-----------------|
| Head            | SAR averaged over 1g  | 2.58 W/Kg          | 10.27 W/Kg           | ± 17.57%        |
|                 | SAR averaged over 10g | 1.66 W/Kg          | 6.60 W/Kg            | ± 17.32%        |

### Antenna Parameters – Head Simulating Liquid (HSL)

| Simulant Liquid | Parameter   | Measured Level                  | Uncertainty (%)                    |
|-----------------|-------------|---------------------------------|------------------------------------|
| Head            | Impedance   | 51.089 $\Omega$ 1.01 j $\Omega$ | ± 0.28 $\Omega$ ± 0.044 j $\Omega$ |
|                 | Return Loss | 30.67                           | ± 2.03 dB                          |

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01A

Page 4 of 10

### Dielectric Property Measurements – Body Simulating Liquid (MSL)

| Simulant Liquid | Frequency (MHz) | Room Temp |         | Liquid Temp |        | Parameters   | Target Value | Measured Value | Uncertainty (%) |
|-----------------|-----------------|-----------|---------|-------------|--------|--------------|--------------|----------------|-----------------|
|                 |                 | Start     | End     | Start       | End    |              |              |                |                 |
| Body            | 900             | 22.0 °C   | 22.0 °C | 22.0°C      | 22.0°C | $\epsilon_r$ | 55.00        | 53.32          | ± 5%            |
|                 |                 |           |         |             |        | $\sigma$     | 1.05         | 1.02           | ± 5%            |

### SAR Results – Body Simulating Liquid (MSL)

| Simulant Liquid | SAR Measured          | 250 mW input Power | Normalised to 1.00 W | Uncertainty (%) |
|-----------------|-----------------------|--------------------|----------------------|-----------------|
| Body            | SAR averaged over 1g  | 2.75 W/Kg          | <b>10.94 W/Kg</b>    | ± 18.06%        |
|                 | SAR averaged over 10g | 1.79 W/Kg          | <b>7.12 W/Kg</b>     | ± 17.44%        |

### Antenna Parameters – Body Simulating Liquid (MSL)

| Simulant Liquid | Parameter   | Measured Level                 | Uncertainty (%)                    |
|-----------------|-------------|--------------------------------|------------------------------------|
| Body            | Impedance   | 54.09 $\Omega$ 2.03 j $\Omega$ | ± 0.28 $\Omega$ ± 0.044 j $\Omega$ |
|                 | Return Loss | 25.35                          | ± 2.03 dB                          |

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD


UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01A

Page 5 of 10

### DASY Validation Scan for Head Stimulating Liquid (HSL)

DUT: Dipole 900 MHz; SN: 1d143; Type: D900V2; Serial: SN1d143

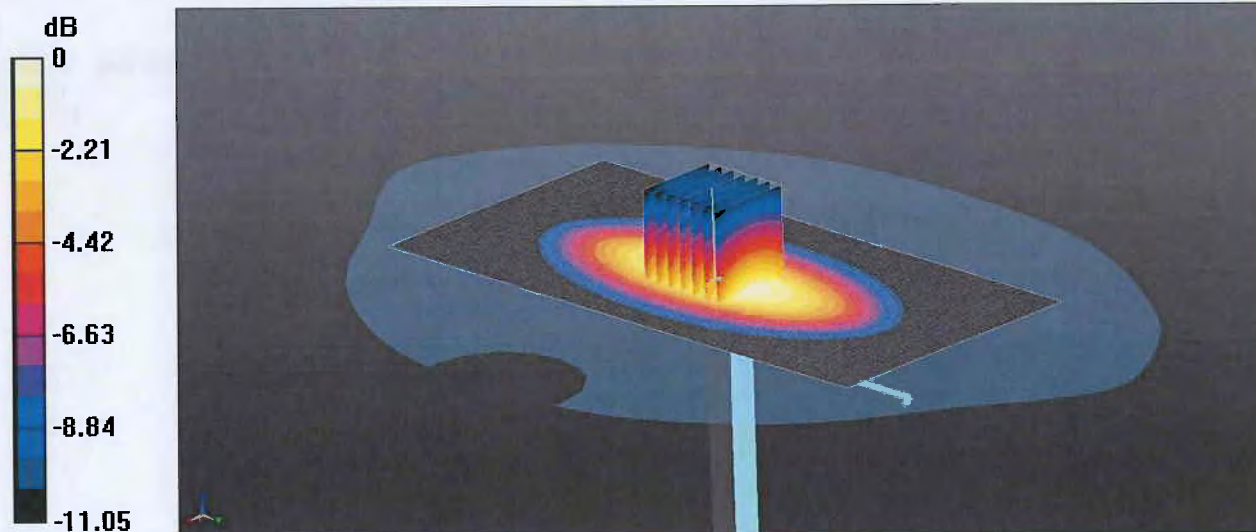

Communication System: UID 0, CW (0); Frequency: 900 MHz; Duty Cycle: 1:1

Medium: 900 MHz HSL Medium parameters used:  $f = 900$  MHz;  $\sigma = 0.934$  S/m;  $\epsilon_r = 41.343$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3341; ConvF(6.32, 6.32, 6.32); Calibrated: 14/08/2017;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1435; Calibrated: 10/02/2017
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD; Serial: TP:xxxx
- ; SEMCAD X Version 14.6.10 (7372)

**Configuration/d=15mm, Pin=250mW 2 2 /Area Scan (81x161x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 3.03 W/kg

**Configuration/d=15mm, Pin=250mW 2 2 /Zoom Scan (5x5x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.75 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 3.90 W/kg

**SAR(1 g) = 2.58 W/kg; SAR(10 g) = 1.66 W/kg**

Maximum value of SAR (measured) = 3.02 W/kg

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01A


Page 6 of 10

### Impedance Measurement Plot for Head Stimulating Liquid (HSL)

10/10/2017 8:09:16 AM  
1326.5170KS2-100151-MV

Trc1 — S11 Smith 200 mU/ Ref 1 U Cal Smo

1

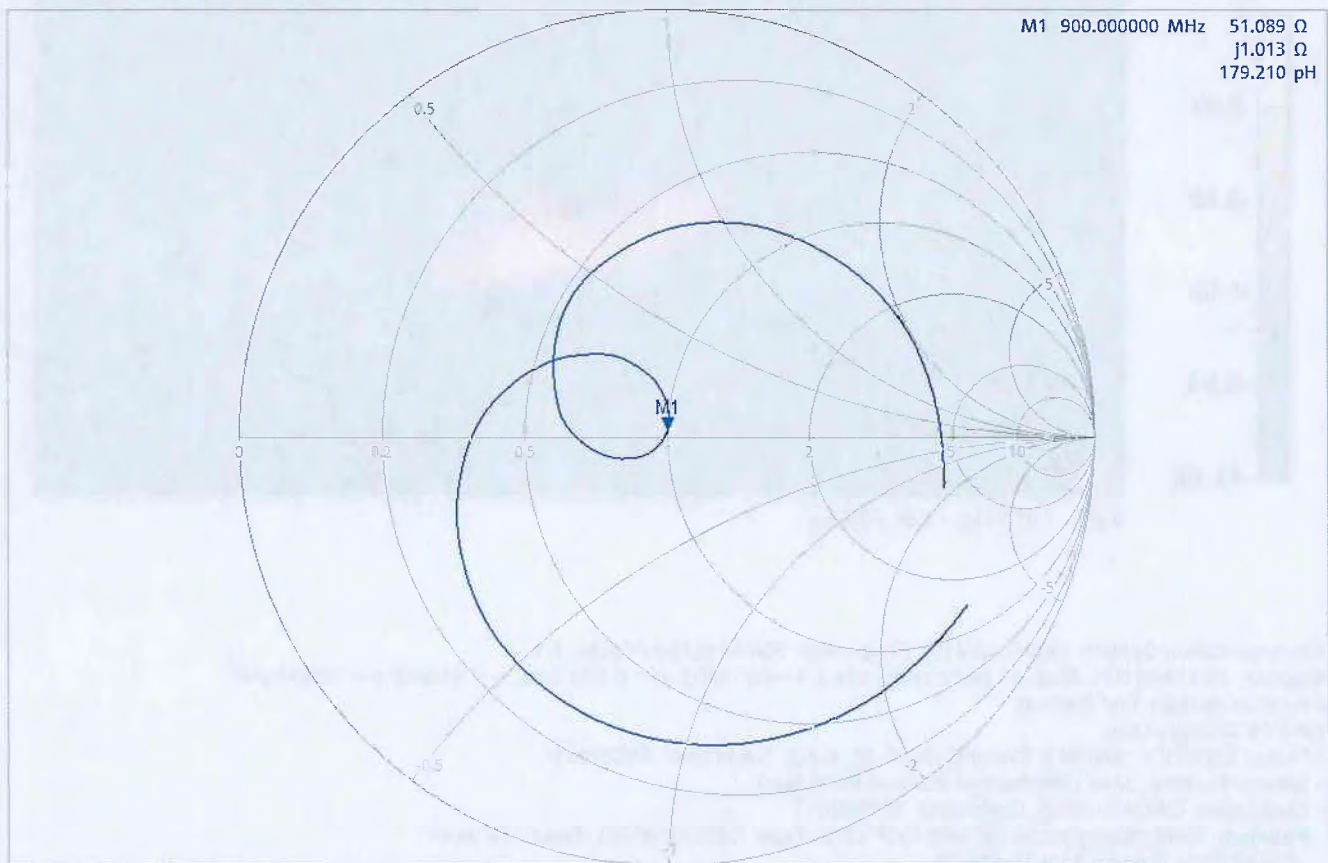

Ch1 Start 700 MHz

Pwr -10 dBm Bw 10 kHz

Stop 1.1 GHz

# CERTIFICATE OF CALIBRATION


## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01A

Page 7 of 10

### Return Loss Measurement Plot for Head Stimulating Liquid (HSL)

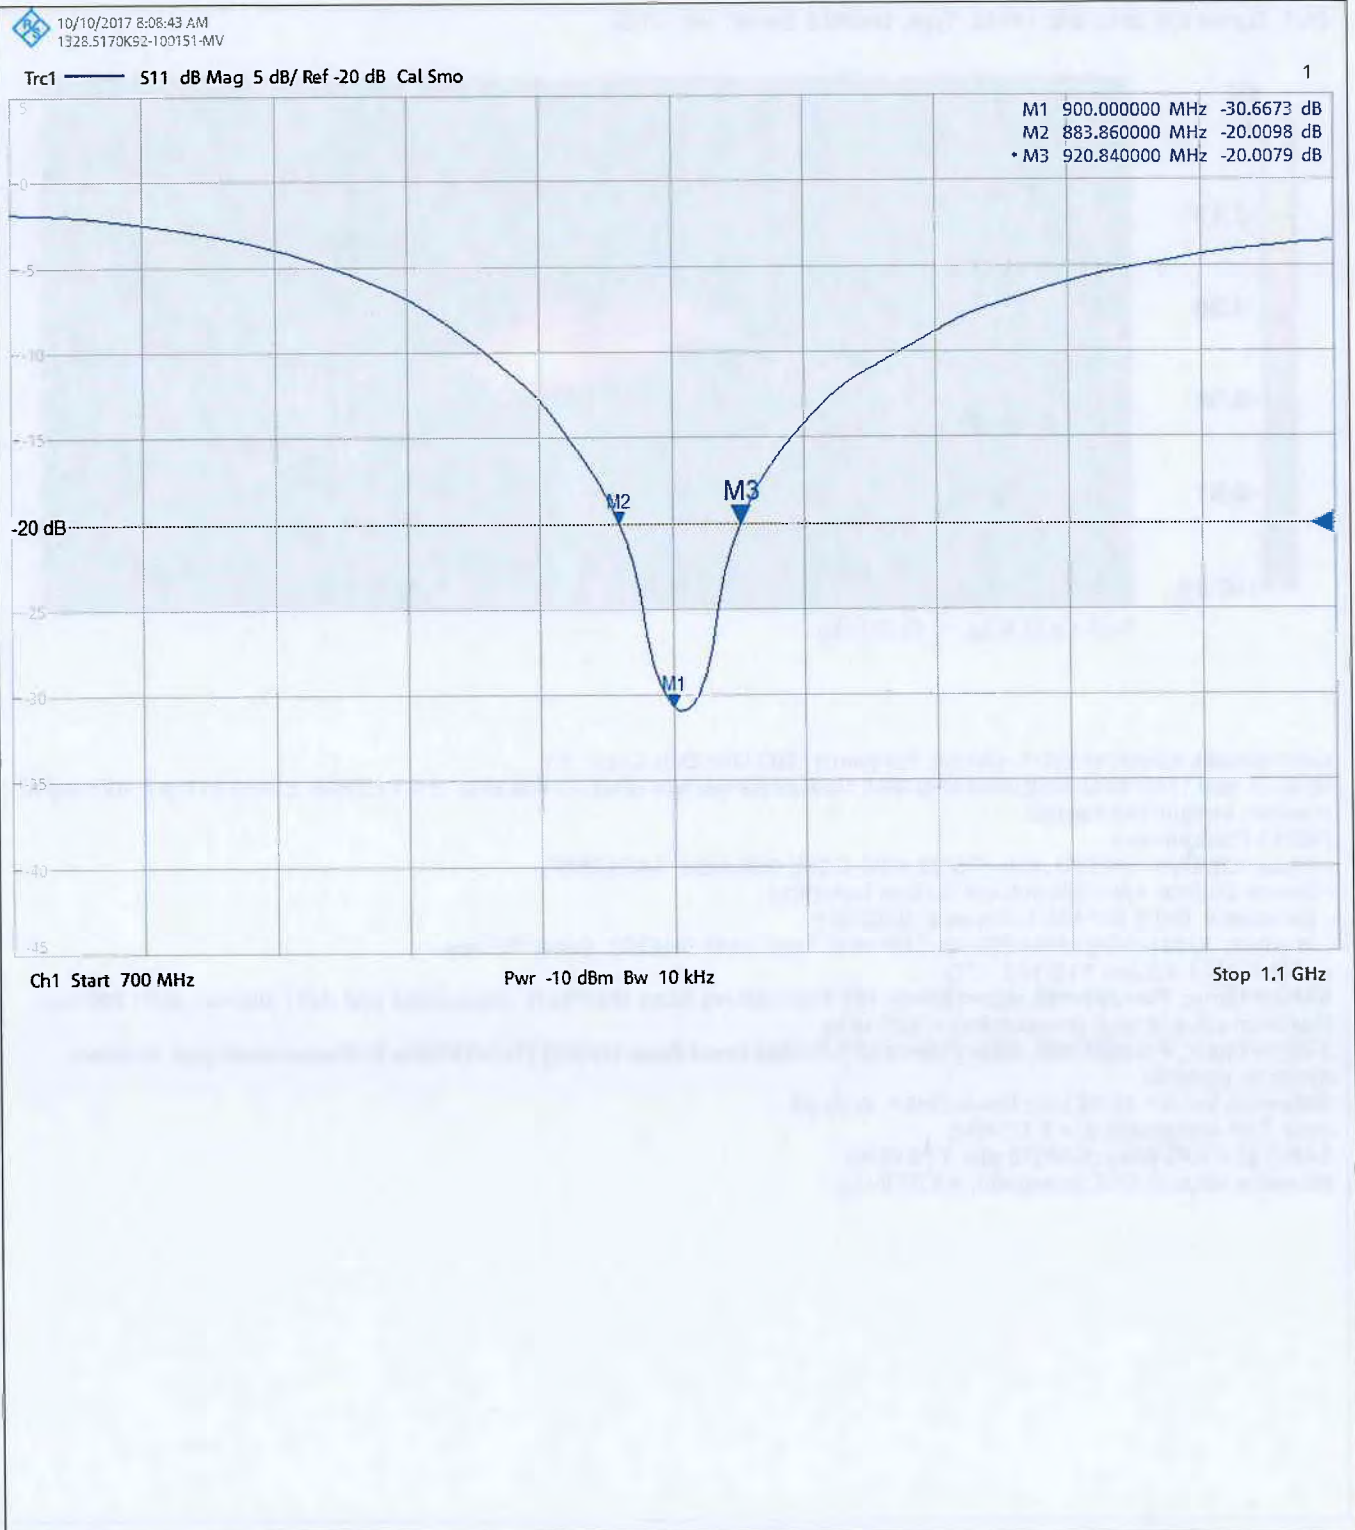

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD


UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01A

Page 8 of 10

### DASY Validation Scan for Body Stimulating Liquid (MSL)

DUT: Dipole 900 MHz; SN: 1d143; Type: D900V2; Serial: SN 1d143

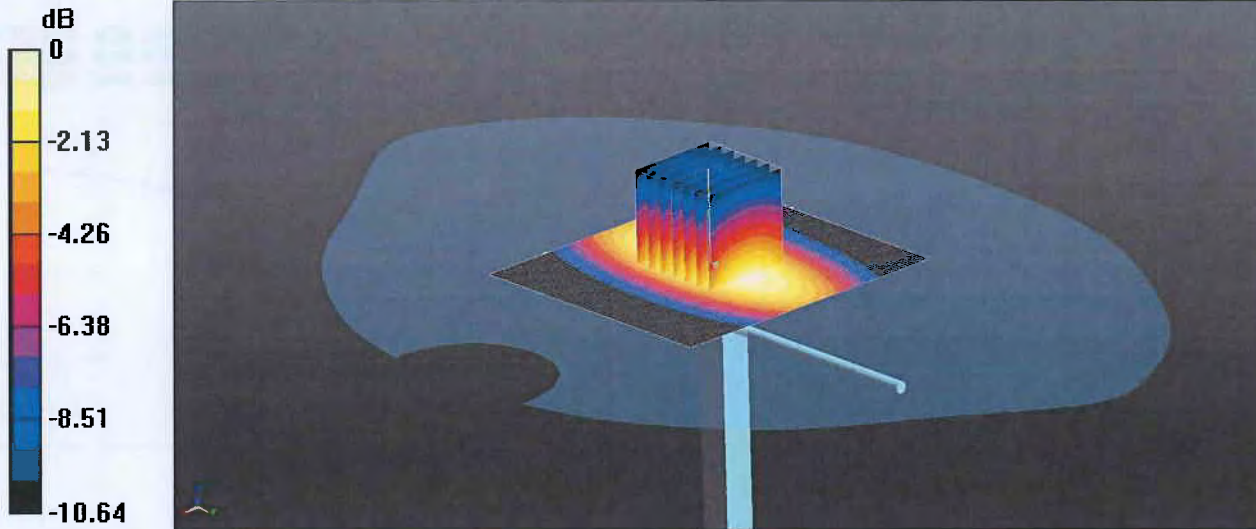

0 dB = 2.97 W/kg = 4.73 dBW/kg

Communication System: UID 0, CW (0); Frequency: 900 MHz; Duty Cycle: 1:1

Medium: 900, 1750, 1800, 1900, 2600 MHz MSL Medium parameters used:  $f = 900$  MHz;  $\sigma = 1.02$  S/m;  $\epsilon_r = 53.317$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3341; ConvF(6.24, 6.24, 6.24); Calibrated: 14/08/2017;

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn1435; Calibrated: 10/02/2017

- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD; Serial: TP:xxxx

- ; SEMCAD X Version 14.6.10 (7372)

**SAR/d=15mm, Pin=250 mW, dist=10.0mm (ET-Probe)/Area Scan (81x71x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 3.00 W/kg

**SAR/d=15mm, Pin=250 mW, dist=10.0mm (ET-Probe)/Zoom Scan (5x5x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 55.18 V/m; Power Drift = -0.10 dB

Peak SAR (extrapolated) = 4.12 W/kg

**SAR(1 g) = 2.75 W/kg; SAR(10 g) = 1.79 W/kg**

Maximum value of SAR (measured) = 2.97 W/kg

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

CERTIFICATE  
NUMBER :  
11903941JD01A

UKAS Accredited Calibration Laboratory No. 5248

Page 9 of 10

### Impedance Measurement Plot for Body Stimulating Liquid (MSL)




10/9/2017 2:34:21 PM  
1328.5170K92-100151-MV

Trc1 — S11 Smith 200 mU/ Ref 1 U Cal Smo

1

M1 900.000000 MHz 54.093  $\Omega$   
j2.028  $\Omega$   
358.611 pF

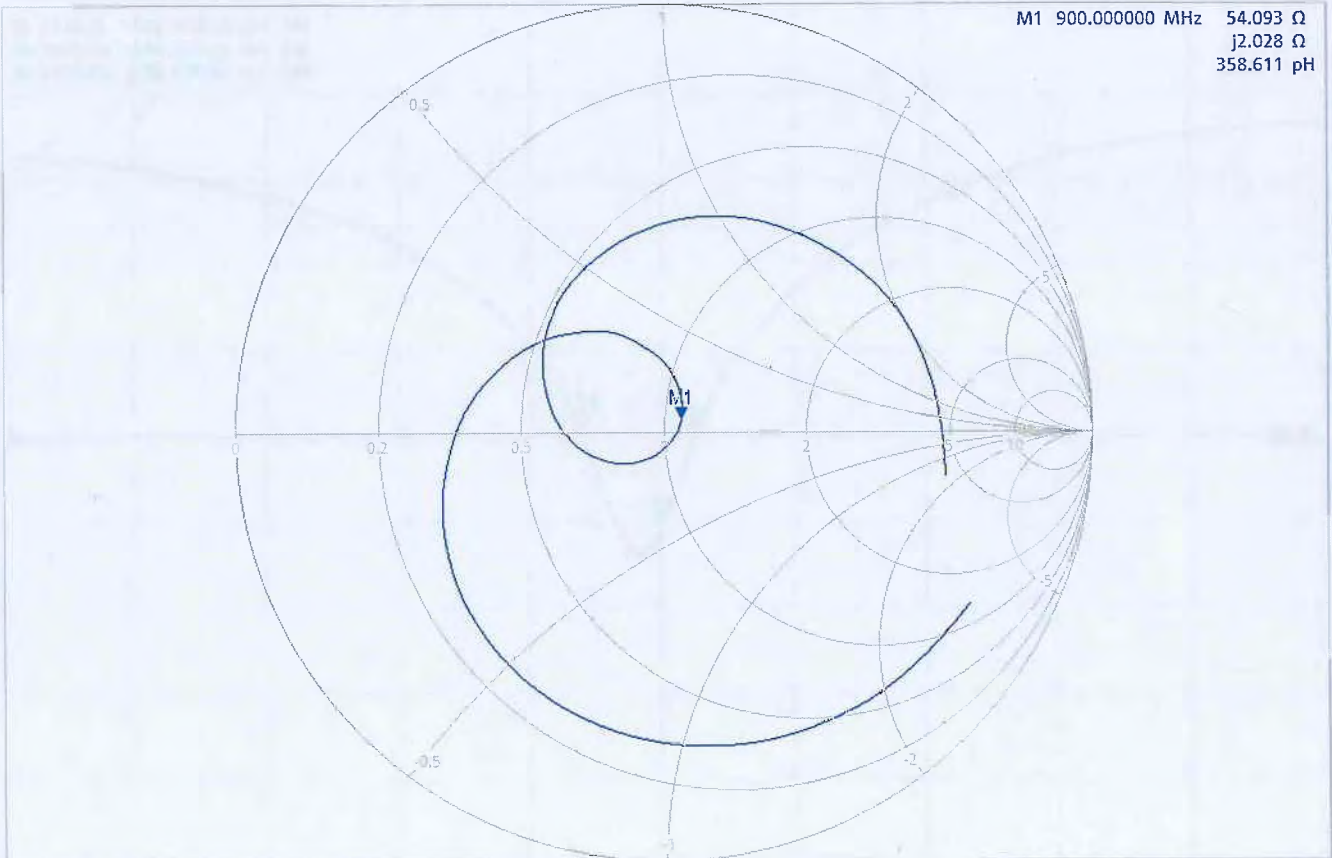

Ch1 Start 700 MHz

Pwr -10 dBm Bw 10 kHz

Stop 1.1 GHz

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01A

Page 10 of 10

### Return Loss Measurement Plot for Body Stimulating Liquid (MSL)




10/5/2017 2:33:24 PM  
1328.5170K92-100151-MV

Trc1 — S11 dB Mag 5 dB/ Ref -20 dB Cal Smo

1

M1 900.000000 MHz -25.3478 dB  
M2 890.220000 MHz -20.0201 dB  
• M3 924.320000 MHz -20.0113 dB

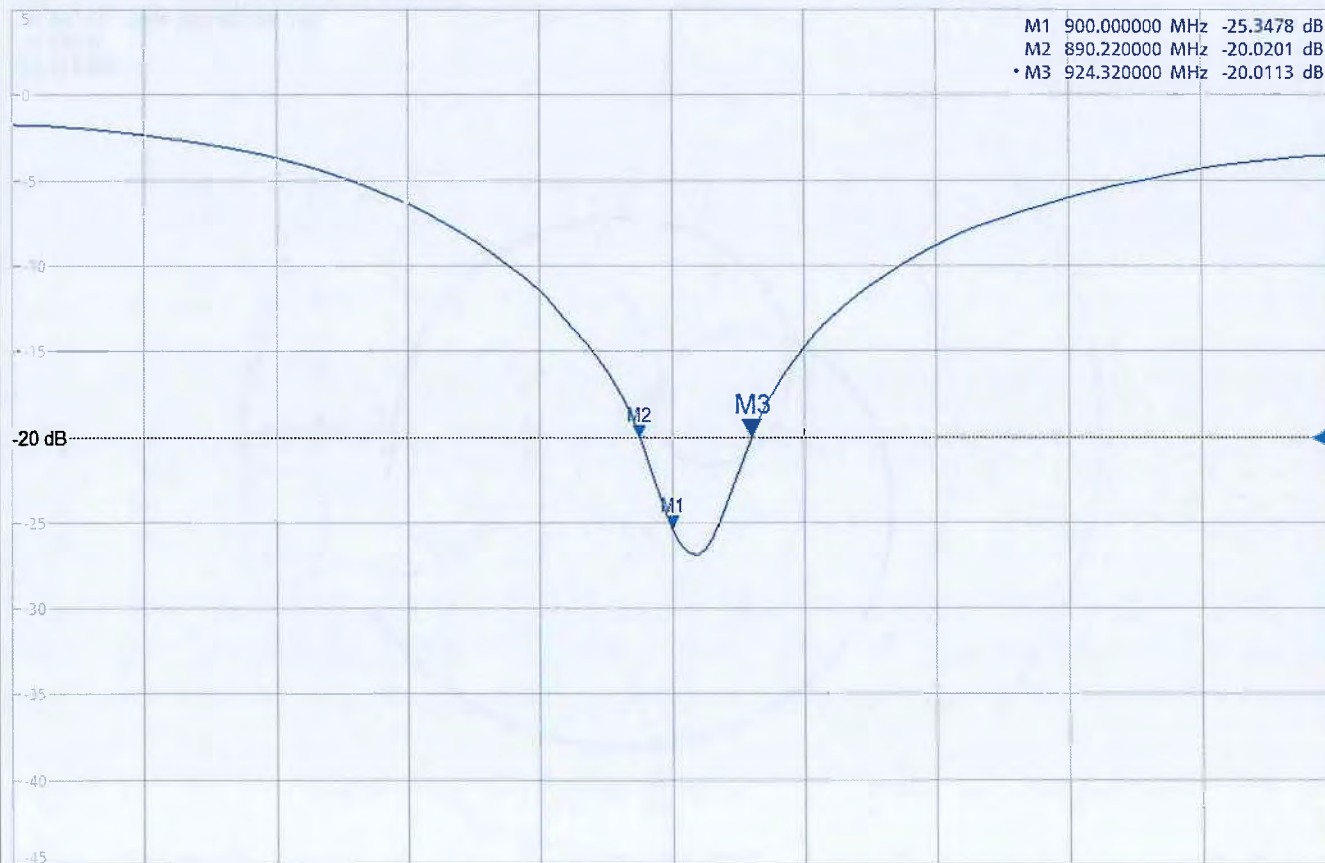

Ch1 Start 700 MHz

Pwr -10 dBm Bw 10 kHz

Stop 1.1 GHz

**Calibration Certificate Label:**

|                                                                                   |                                                                                                                                                                                          |
|-----------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  | <p><b>UL VS LTD - Tel: +44 (0) 1256312000</b></p> <p>Certificate Number: 11903941JD01A</p> <p>Instrument ID: 1d143</p> <p>Calibration Date: 05/Oct/2017</p> <p>Calibration Due Date:</p> |
|-----------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

|                                                                                   |                                                                                                                                                                                          |
|-----------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  | <p><b>UL VS LTD - Tel: +44 (0) 1256312000</b></p> <p>Certificate Number: 11903941JD01A</p> <p>Instrument ID: 1d143</p> <p>Calibration Date: 05/Oct/2017</p> <p>Calibration Due Date:</p> |
|-----------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

|                                                                                    |                                                                                                                                                                                          |
|------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  | <p><b>UL VS LTD - Tel: +44 (0) 1256312000</b></p> <p>Certificate Number: 11903941JD01A</p> <p>Instrument ID: 1d143</p> <p>Calibration Date: 05/Oct/2017</p> <p>Calibration Due Date:</p> |
|------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|



# CERTIFICATE OF CALIBRATION

ISSUED BY **UL VS LTD**

DATE OF ISSUE: 10/Oct/2017

CERTIFICATE NUMBER : 11903941JD01D



5248

UL VS LTD  
PAVILION A  
ASHWOOD PARK, ASHWOOD WAY  
BASINGSTOKE, HAMPSHIRE  
RG23 8BG, UK  
TEL: +44 (0) 1256 312000  
FAX: +44 (0) 1256 312001  
Email: LST.UK.Calibration@ul.com



Page 1 of 10

APPROVED SIGNATORY

Naseer Mirza

## Customer :

UL VS Ltd  
Pavilion A, Ashwood Park, Ashwood Way  
Basingstoke, RG23 8BG, England

## Equipment Details:

|                    |                                           |                  |             |
|--------------------|-------------------------------------------|------------------|-------------|
| Description:       | Dipole Validation Kit                     | Date of Receipt: | 29/Sep/2017 |
| Manufacturer:      | Speag                                     |                  |             |
| Type/Model Number: | D1900V2                                   |                  |             |
| Serial Number:     | 5d163                                     |                  |             |
| Calibration Date:  | 05/Oct/2017                               |                  |             |
| Calibrated By:     | Chanthu Thevarajah<br>Laboratory Engineer |                  |             |

Signature:

All Calibration have been conducted in the closed laboratory facility: Lab Temperature (22±3) °C and humidity < 70%

This certificate is issued in accordance with the laboratory accreditation requirements of the United Kingdom Accreditation Service. It provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

Use of the UKAS mark demonstrates that compliance with the requirements of BS/EN/ISO/IEC 17025 has been independently assessed.

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01D

Page 2 of 10

The calibration methods and procedures used were as detailed in:

1. **IEC 62209-1:2005**: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
2. **IEC 62209-2:2010**: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)
3. **IEEE 1528: 2013**: IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques
4. FCC KDB Publication Number: "KDB865664 D01 SAR Measurement 100 MHz to 6 GHz"
5. **SPEAG DASY4/ DASY5 System Handbook**

The measuring equipment used to perform the calibration, documented in this certificate has been calibrated in accordance with the manufacturers' recommendations, and is traceable to recognized national standards.

| UL No.     | Instrument                   | Manufacturer         | Type No.      | Serial No.  | Date Last Calibrated  | Cal. Interval (Months) |
|------------|------------------------------|----------------------|---------------|-------------|-----------------------|------------------------|
| A2546      | Data Acquisition Electronics | SPEAG                | DAE4          | 1435        | 10 Feb 2017           | 12                     |
| A2587      | Probe                        | SPEAG                | ES3DV3        | 3341        | 14 Aug 2017           | 12                     |
| A2200      | Dipole                       | SPEAG                | D1900V2       | 537         | 09 Feb 2017           | 12                     |
| PRE0151451 | Power Monitoring Kit         | Art-Fi               | ART 100850-01 | 0001        | Cal as part of System | 12                     |
| PRE0151441 | Power Sensor                 | Rhode & Schwarz      | NRP8S         | 102481      | 16 Nov 2016           | 12                     |
| M1015      | Network Analyser             | Agilent Technologies | 8753ES        | US39172406  | 26 Sept 2016          | 12                     |
| PRE0151154 | Network Analyser             | Rhode & Schwarz      | ZND8          | 100151      | 22 Nov 2016           | 12                     |
| PRE0151877 | Calibration Kit              | Rhode & Schwarz      | Z135          | 102947-Bt   | 02 Dec 2016           | 12                     |
| M1908      | Signal Generator             | Rhode & Schwarz      | SMIQ 03B      | 1125.555.03 | 08 Nov 2016           | 12                     |

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01D

Page 3 of 10

### SAR System Specification

|                          |                                            |
|--------------------------|--------------------------------------------|
| Robot System Positioner: | Stäubli Unimation Corp. Robot Model: TX60L |
| Robot Serial Number:     | F14/5T5ZA1/A/01                            |
| DASY Version:            | DASY 52 (v52.8.8.1258)                     |
| Phantom:                 | Flat section of SAM Twin Phantom           |
| Distance Dipole Centre:  | 10 mm (with spacer)                        |
| Frequency:               | 1900 MHz                                   |

### Dielectric Property Measurements – Head Simulating Liquid (HSL)

| Simulant Liquid | Frequency (MHz) | Room Temp |         | Liquid Temp |         | Parameters   | Target Value | Measured Value | Uncertainty (%) |
|-----------------|-----------------|-----------|---------|-------------|---------|--------------|--------------|----------------|-----------------|
|                 |                 | Start     | End     | Start       | End     |              |              |                |                 |
| Head            | 1900            | 23.0 °C   | 22.0 °C | 21.0 °C     | 22.0 °C | $\epsilon_r$ | 40.00        | 39.71          | ± 5%            |
|                 |                 |           |         |             |         | $\sigma$     | 1.40         | 1.36           | ± 5%            |

### SAR Results – Head Simulating Liquid (HSL)

| Simulant Liquid | SAR Measured          | 250 mW input Power | Normalised to 1.00 W | Uncertainty (%) |
|-----------------|-----------------------|--------------------|----------------------|-----------------|
| Head            | SAR averaged over 1g  | 9.74 W/Kg          | 38.77 W/Kg           | ± 17.57%        |
|                 | SAR averaged over 10g | 5.05 W/Kg          | 20.10 W/Kg           | ± 17.32%        |

### Antenna Parameters – Head Simulating Liquid (HSL)

| Simulant Liquid | Parameter   | Measured Level                   | Uncertainty (%)                    |
|-----------------|-------------|----------------------------------|------------------------------------|
| Head            | Impedance   | 50.143 $\Omega$ -3.33 j $\Omega$ | ± 0.28 $\Omega$ ± 0.044 j $\Omega$ |
|                 | Return Loss | 29.77                            | ± 2.03 dB                          |

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01D

Page 4 of 10

### Dielectric Property Measurements – Body Simulating Liquid (MSL)

| Simulant Liquid | Frequency (MHz) | Room Temp |         | Liquid Temp |        | Parameters   | Target Value | Measured Value | Uncertainty (%) |
|-----------------|-----------------|-----------|---------|-------------|--------|--------------|--------------|----------------|-----------------|
|                 |                 | Start     | End     | Start       | End    |              |              |                |                 |
| Body            | 1900            | 22.0 °C   | 22.0 °C | 22.0°C      | 22.0°C | $\epsilon_r$ | 53.30        | 52.22          | ± 5%            |
|                 |                 |           |         |             |        | $\sigma$     | 1.52         | 1.57           | ± 5%            |

### SAR Results – Body Simulating Liquid (MSL)

| Simulant Liquid | SAR Measured          | 250 mW input Power | Normalised to 1.00 W | Uncertainty (%) |
|-----------------|-----------------------|--------------------|----------------------|-----------------|
| Body            | SAR averaged over 1g  | 10.80 W/Kg         | <b>42.99 W/Kg</b>    | ± 18.06%        |
|                 | SAR averaged over 10g | 5.52 W/Kg          | <b>21.97 W/Kg</b>    | ± 17.44%        |

### Antenna Parameters – Body Simulating Liquid (MSL)

| Simulant Liquid | Parameter   | Measured Level                  | Uncertainty (%)                    |
|-----------------|-------------|---------------------------------|------------------------------------|
| Body            | Impedance   | 52.90 $\Omega$ -5.74 j $\Omega$ | ± 0.28 $\Omega$ ± 0.044 j $\Omega$ |
|                 | Return Loss | 24.03                           | ± 2.03 dB                          |

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD


UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01D

Page 5 of 10

### DASY Validation Scan for Head Stimulating Liquid (HSL)

DUT: D1900V2 - SN5d163; Type: D1900V2; Serial: SN5d163

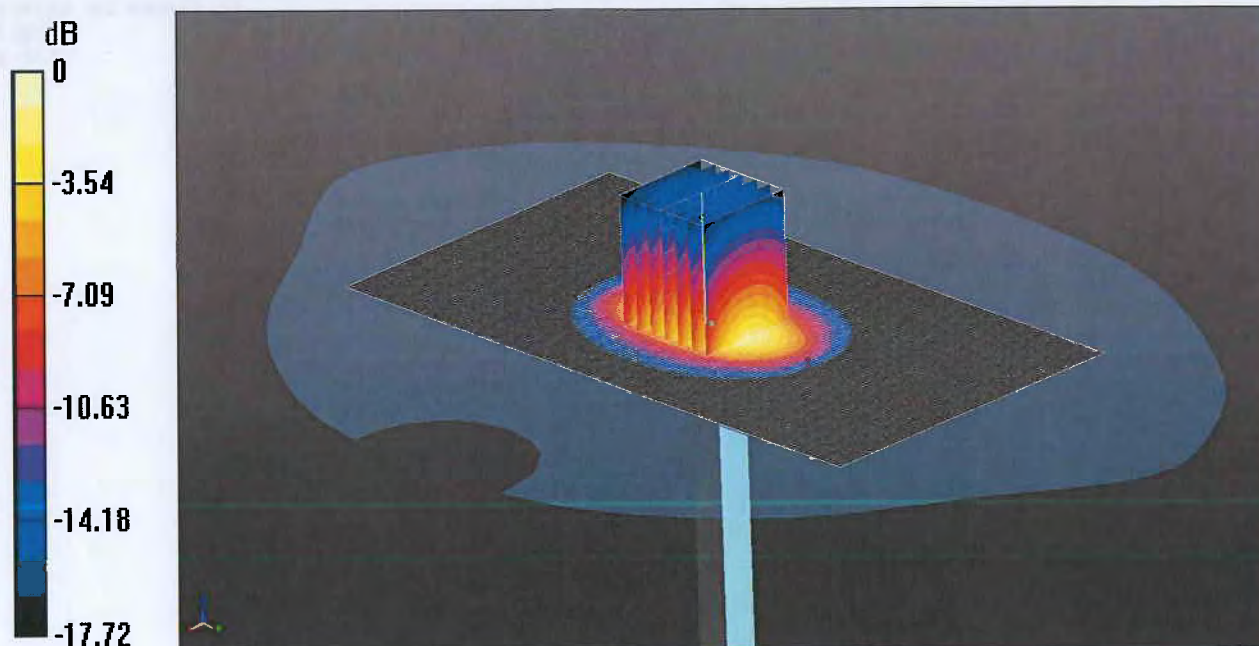

0 dB = 12.3 W/kg = 10.90 dBW/kg

Communication System: UID 0, CW (0); Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 MHz HSL Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.36$  S/m;  $\epsilon_r = 39.711$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3341; ConvF(5.28, 5.28, 5.28); Calibrated: 14/08/2017;

- Sensor-Surface: 3mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn1435; Calibrated: 10/02/2017

- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD; Serial: TP:xxxx

- ; SEMCAD X Version 14.6.10 (7372)

**Configuration/d=10mm, Pin=250mW 2/Area Scan (81x151x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 12.7 W/kg

**Configuration/d=10mm, Pin=250mW 2/Zoom Scan (5x5x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.37 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 17.9 W/kg

**SAR(1 g) = 9.74 W/kg; SAR(10 g) = 5.05 W/kg**

Maximum value of SAR (measured) = 12.3 W/kg

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01D

Page 6 of 10

### Impedance Measurement Plot for Head Stimulating Liquid (HSL)




10/10/2017 1:00:08 PM  
1325.5170K92-100151-MV

Trc1 — S11 Smith 200 mU/ Ref 1 U Cal Smo

1

M1 1.900000 GHz 50.143  $\Omega$   
-j3.330  $\Omega$   
25.154 pF

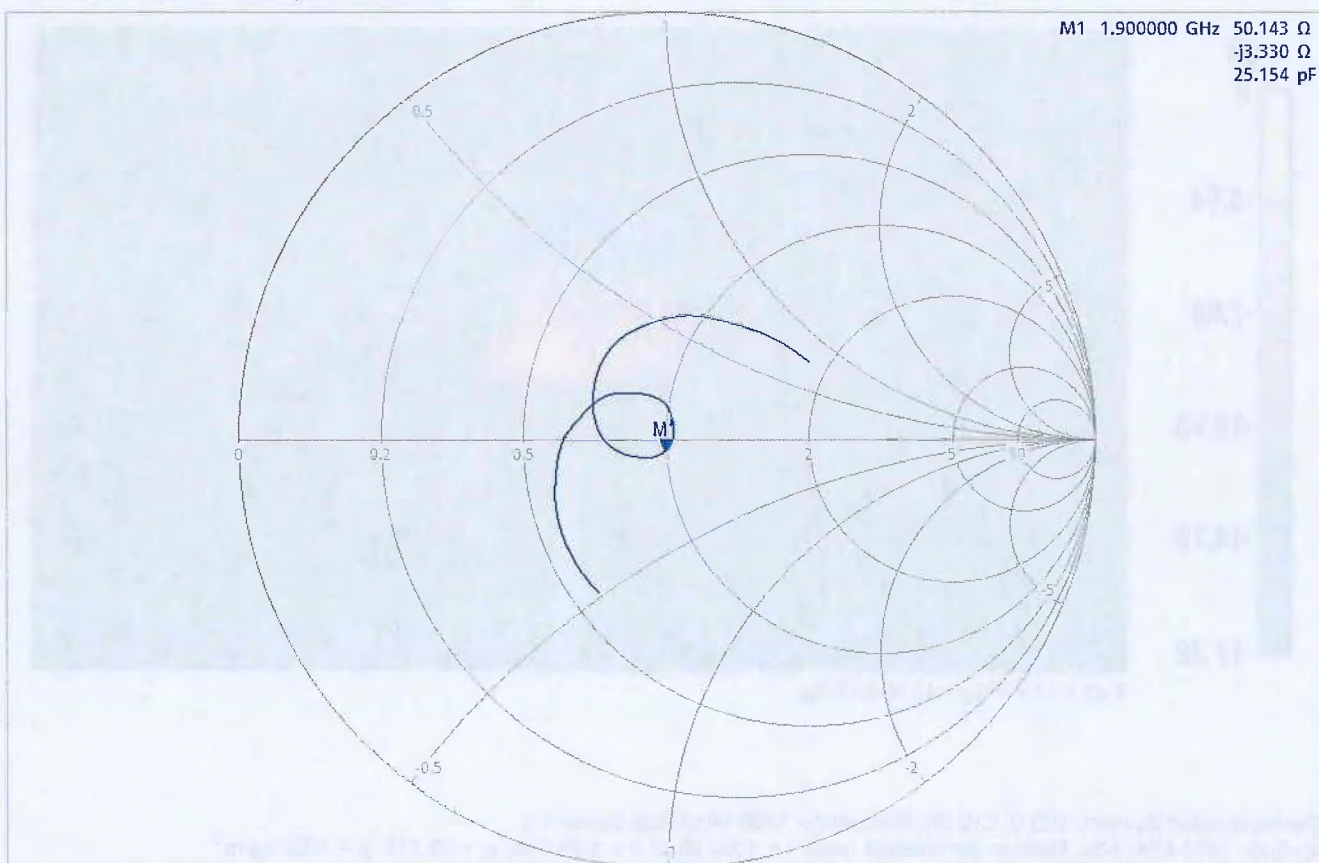

Ch1 Start 1.7 GHz

Pwr -10 dBm Bw 10 kHz

Stop 2.1 GHz

# CERTIFICATE OF CALIBRATION


## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01D

Page 7 of 10

### Return Loss Measurement Plot for Head Stimulating Liquid (HSL)

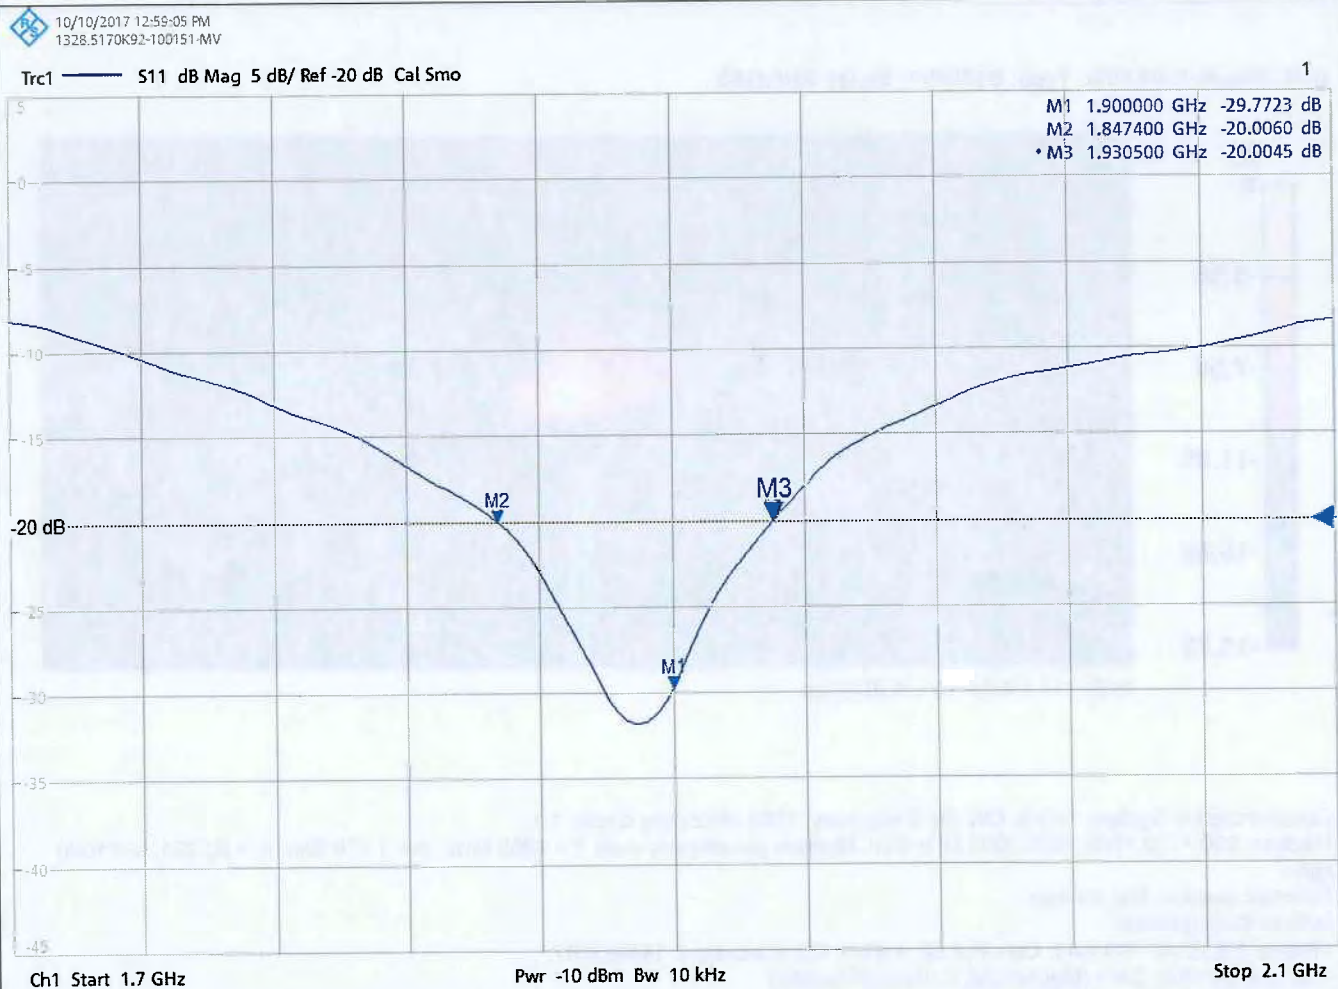

# CERTIFICATE OF CALIBRATION

## ISSUED BY UL VS LTD



UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01D

Page 8 of 10

### DASY Validation Scan for Body Stimulating Liquid (MSL)

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: SN5d163

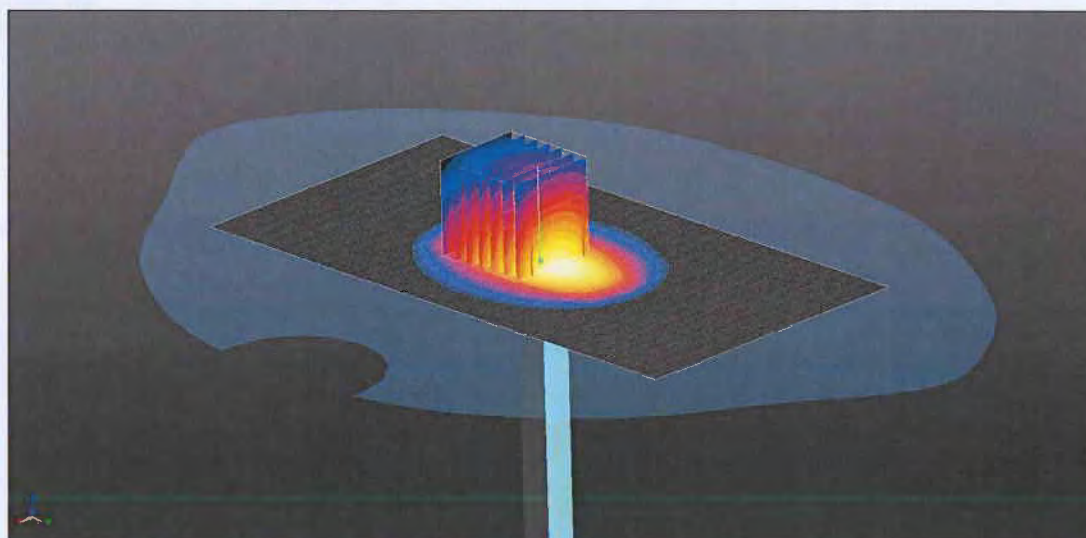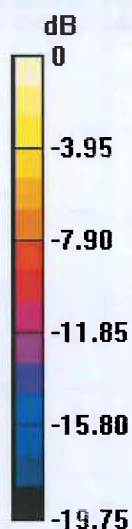

0 dB = 13.5 W/kg = 11.30 dBW/kg

Communication System: UID 0, CW (0); Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 900,1750,1800,1900,2600 MHz MSL Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.576$  S/m;  $\epsilon_r = 52.221$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3341; ConvF(4.92, 4.92, 4.92); Calibrated: 14/08/2017;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1435; Calibrated: 10/02/2017
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD; Serial: TP:xxxx
- ; SEMCAD X Version 14.6.10 (7372)

**SAR/d=10mm, Pin=250mW 2/Area Scan (81x151x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 14.3 W/kg

**SAR/d=10mm, Pin=250mW 2/Zoom Scan (5x5x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.36 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 19.5 W/kg

**SAR(1 g) = 10.8 W/kg; SAR(10 g) = 5.52 W/kg**


Maximum value of SAR (measured) = 13.5 W/kg

CERTIFICATE  
NUMBER :  
11903941JD01D

UKAS Accredited Calibration Laboratory No. 5248

Page 9 of 10

### Impedance Measurement Plot for Body Stimulating Liquid (MSL)

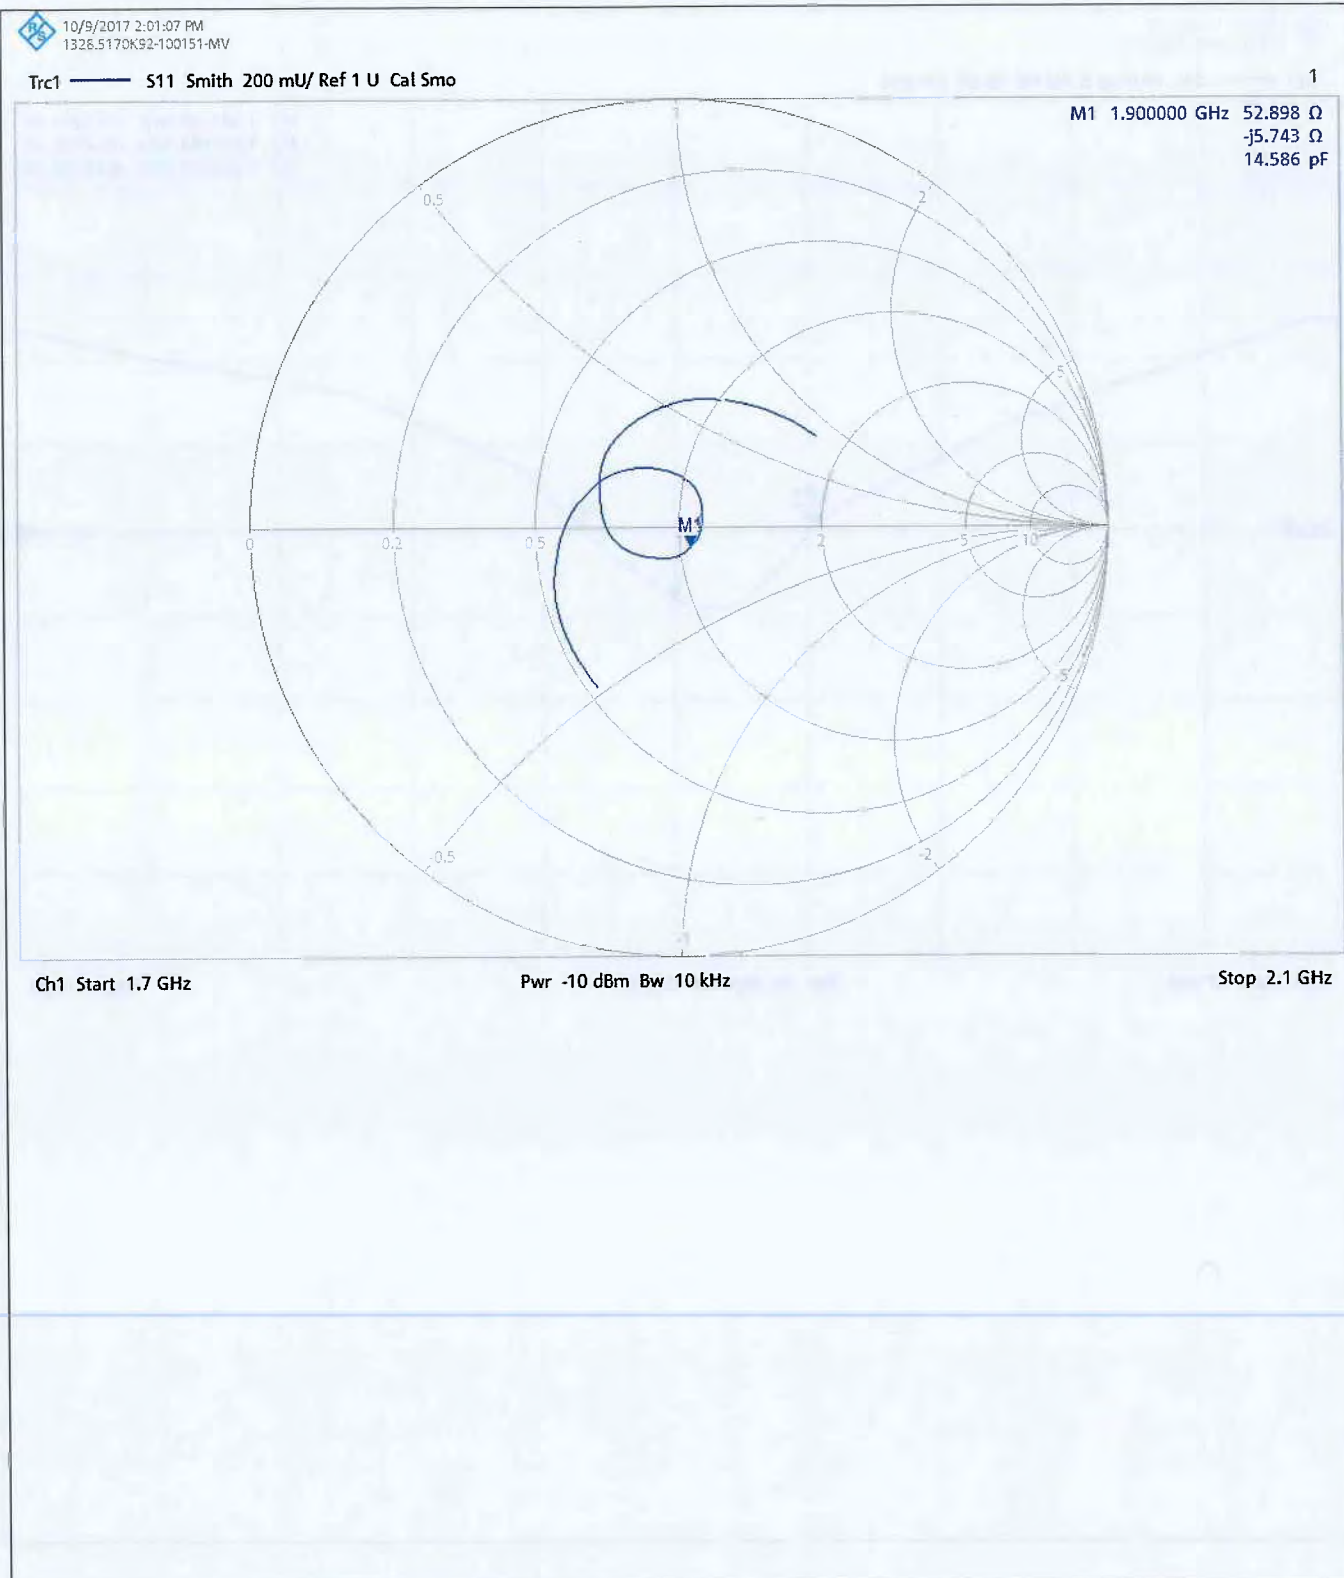

# CERTIFICATE OF CALIBRATION


## ISSUED BY UL VS LTD

UKAS Accredited Calibration Laboratory No. 5248

CERTIFICATE  
NUMBER :  
11903941JD01D

Page 10 of 10

### Return Loss Measurement Plot for Body Stimulating Liquid (MSL)

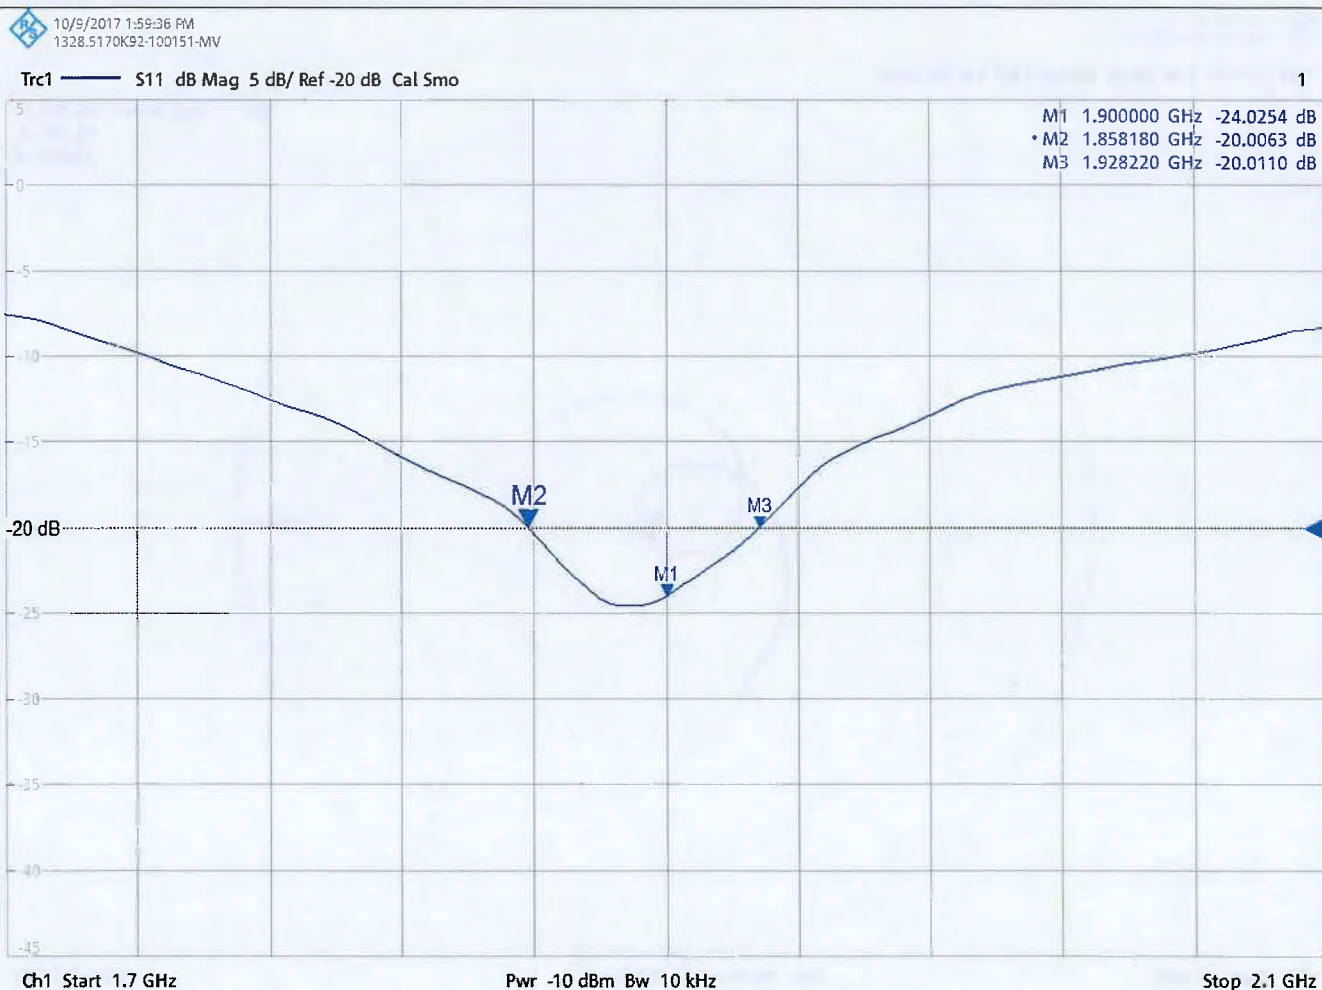

**Calibration Certificate Label:**

|                                                                                                                        |                                                                                                                                                                                          |
|------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  <p>UKAS<br/>CALIBRATION<br/>5248</p> | <p><b>UL VS LTD - Tel: +44 (0) 1256312000</b></p> <p>Certificate Number: 11903941JD01D</p> <p>Instrument ID: 5d163</p> <p>Calibration Date: 05/Oct/2017</p> <p>Calibration Due Date:</p> |
|------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

|                                                                                                                        |                                                                                                                                                                                          |
|------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  <p>UKAS<br/>CALIBRATION<br/>5248</p> | <p><b>UL VS LTD - Tel: +44 (0) 1256312000</b></p> <p>Certificate Number: 11903941JD01D</p> <p>Instrument ID: 5d163</p> <p>Calibration Date: 05/Oct/2017</p> <p>Calibration Due Date:</p> |
|------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

|                                                                                                                         |                                                                                                                                                                                          |
|-------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  <p>UKAS<br/>CALIBRATION<br/>5248</p> | <p><b>UL VS LTD - Tel: +44 (0) 1256312000</b></p> <p>Certificate Number: 11903941JD01D</p> <p>Instrument ID: 5d163</p> <p>Calibration Date: 05/Oct/2017</p> <p>Calibration Due Date:</p> |
|-------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

