



## APPENDIX

### 11. Photographs of Test Setup

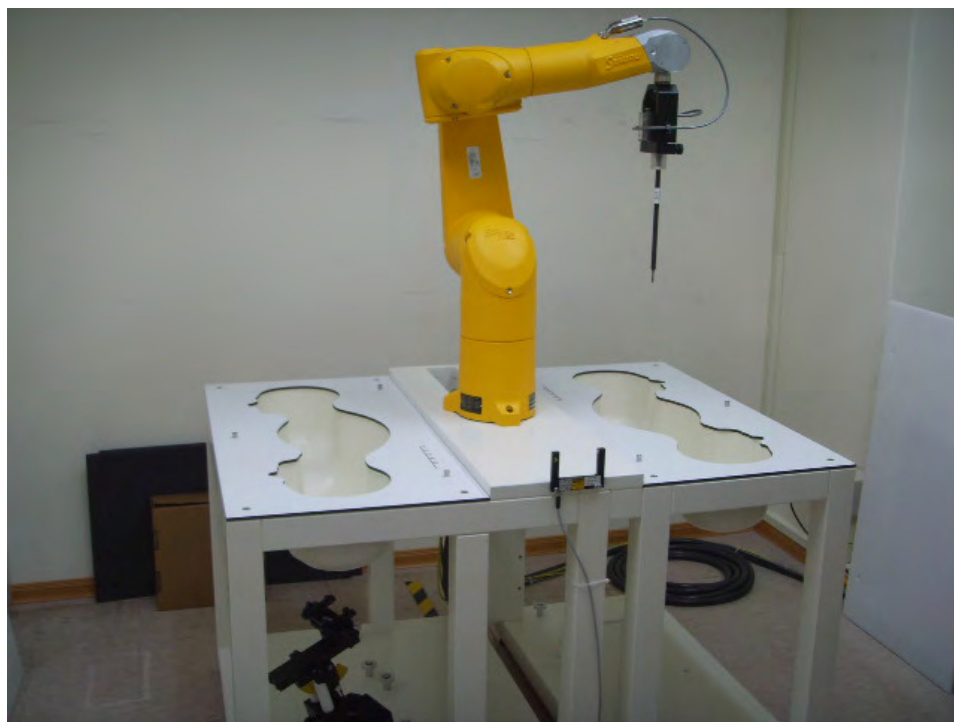


**Fig.1 Photograph of the SAR measurement system**


**Photograph of the Tissue Simulant Fluid Liquid Depth**

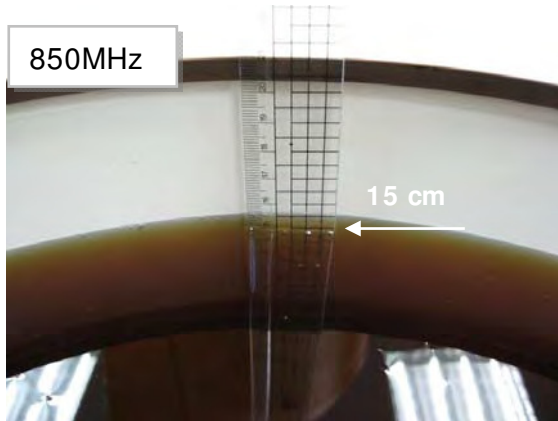


**Fig.2.1**

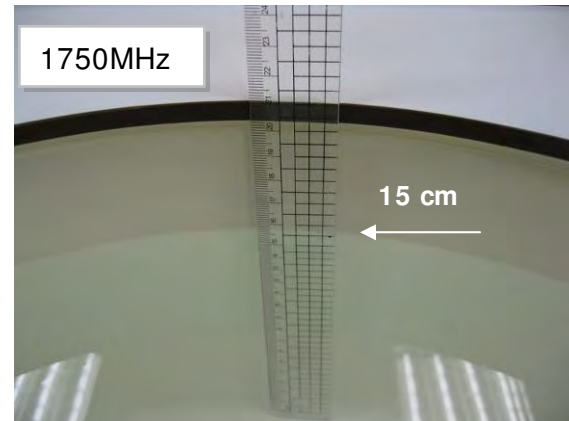


**Fig.2.2**

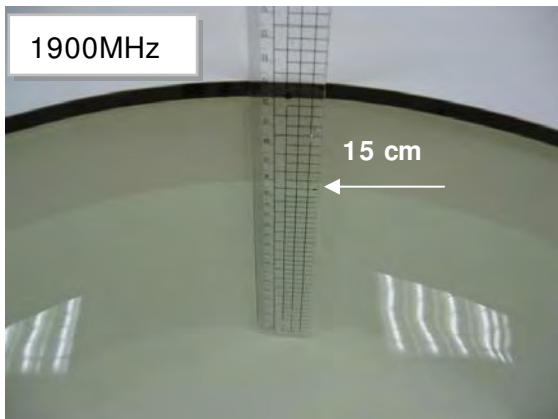

**Fig.2.3**

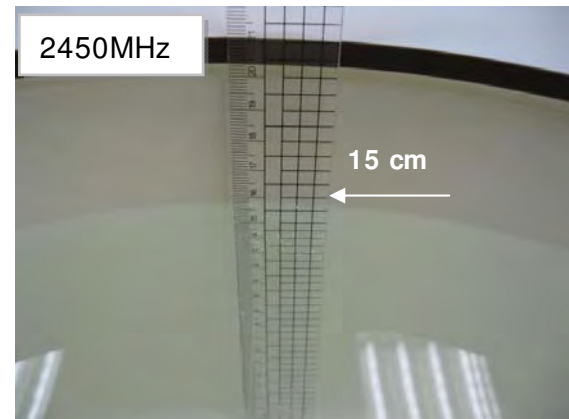


**Fig.2.4**

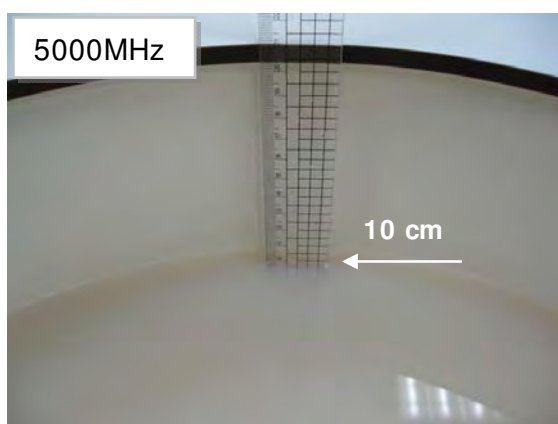


**Fig.2.5**



**Body - distance between flat phantom and EUT is 0 mm**

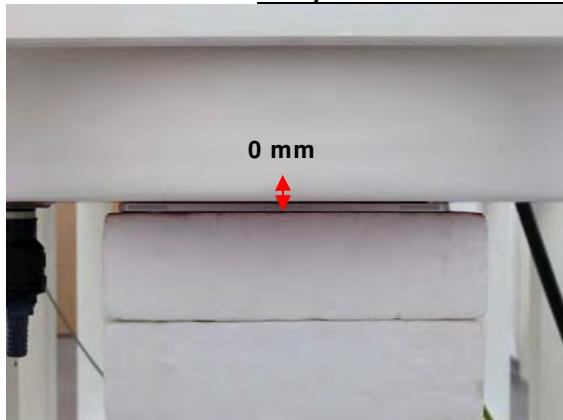

**Fig.3 EUT Back side to flat phantom**


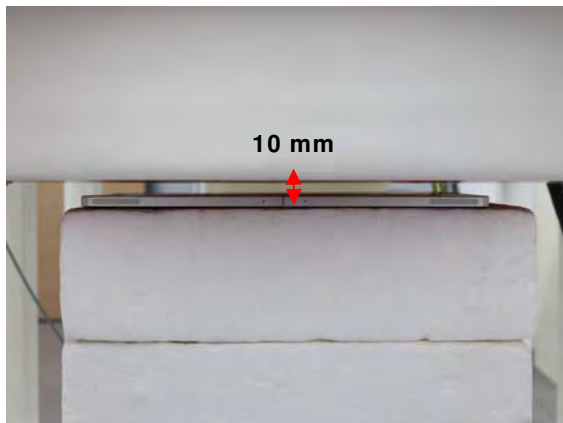


**Fig.4 EUT Back side (10mm) to flat phantom**

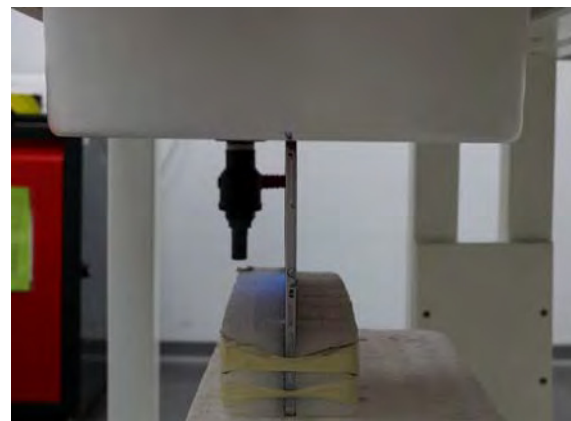
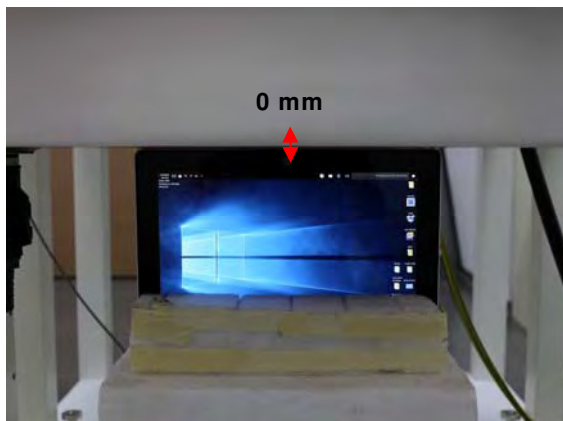


**Fig.5 EUT Bottom side to flat phantom**



**Body - distance between flat phantom and EUT is 0 mm**

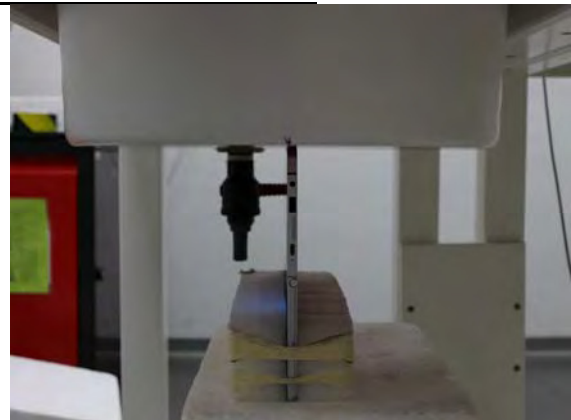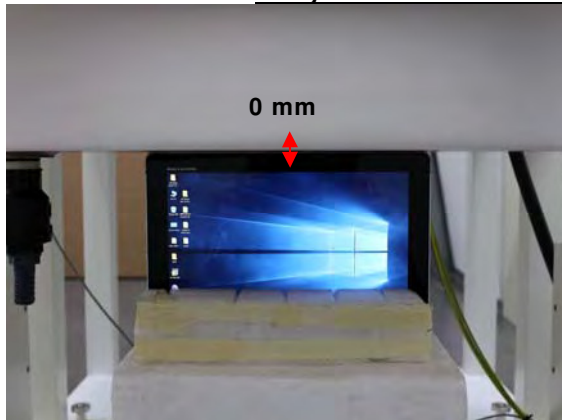

**Fig.6 EUT Top side to flat phantom**

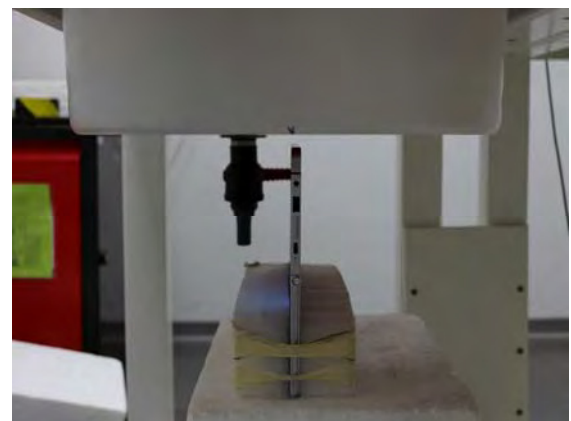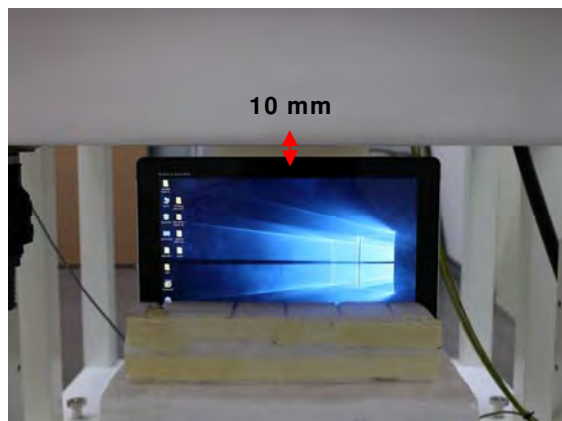


**Fig.7 EUT Top side (10mm) to flat phantom**

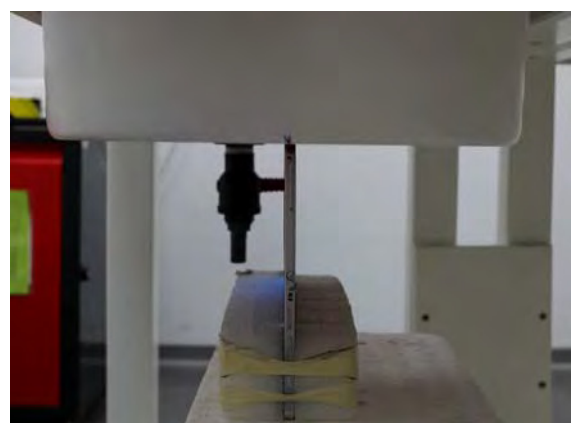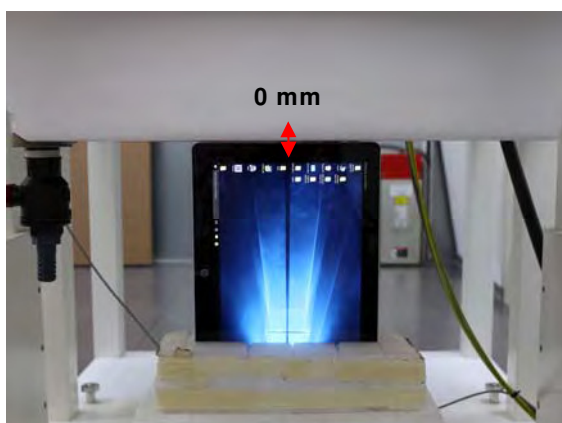

**Fig.8 EUT Left side to flat phantom**

**Body - distance between flat phantom and EUT is 0 mm**

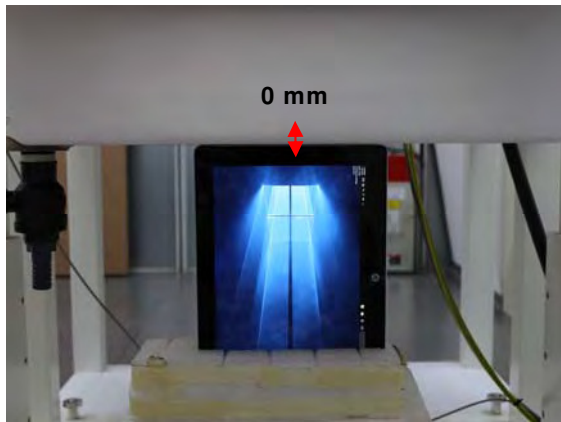

**Fig.9 EUT Right side to flat phantom**

## 12. Photographs of the EUT



**Fig.10 Front view of EUT**



**Fig.11 Back view of EUT**

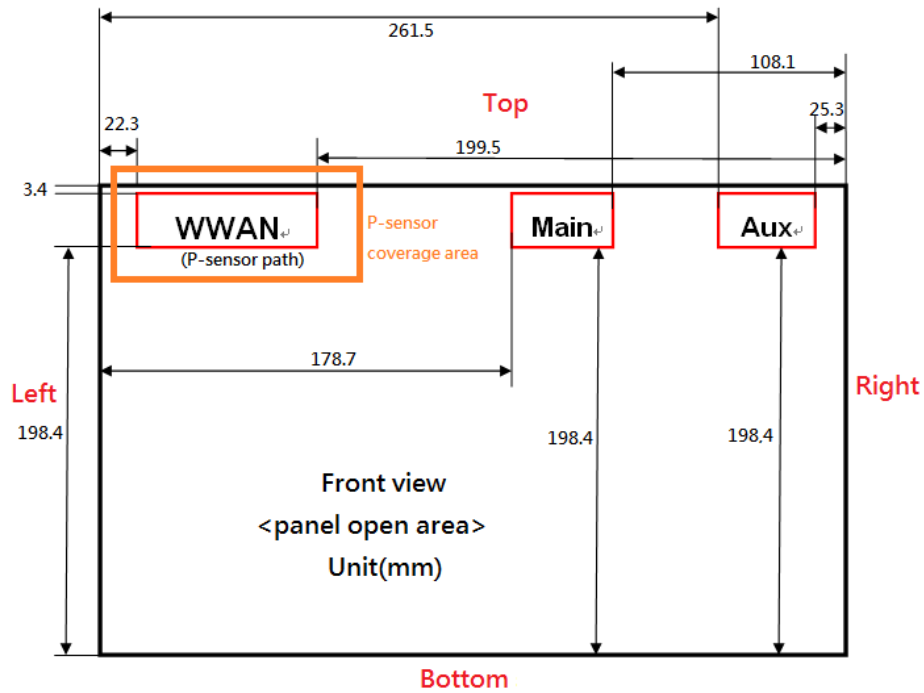


Fig.12 Antenna position of EUT (Front view)

- End of Report -