

## System Check\_Head\_750MHz

### DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_600-7200\_260729 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.875$  S/m;  $\epsilon_r = 44.2$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.98, 9.68, 9.75); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156\_Gap\_0414; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.422 W/kg; SAR (10g) = 0.279 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 0.427 W/kg; SAR (8g) = 0.302 W/kg; SAR (10g) = 0.287 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

TSL Correction: Positive only

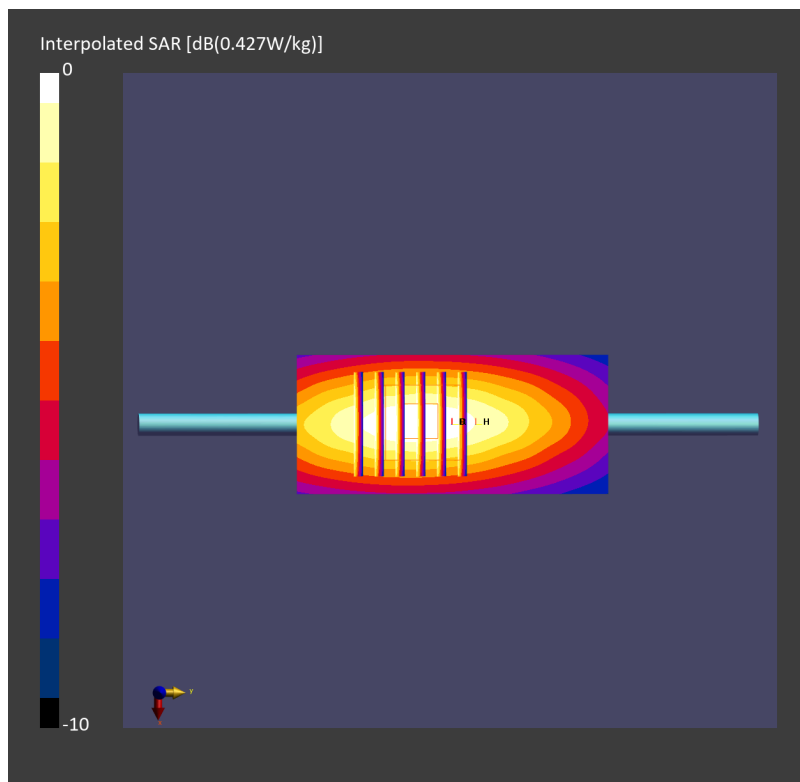

## System Check\_Head\_750MHz

### DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_600-7200\_260802 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.904$  S/m;  $\epsilon_r = 44.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.98, 9.68, 9.75); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.430 W/kg; SAR (10g) = 0.286 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 0.431 W/kg; SAR (8g) = 0.304 W/kg; SAR (10g) = 0.289 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

TSL Correction: Positive only

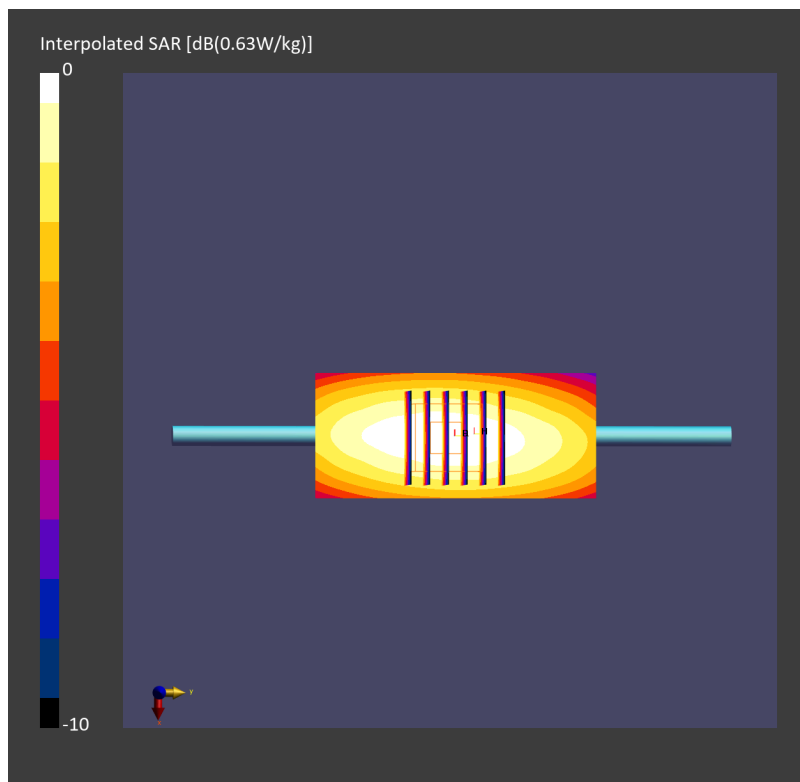

## System Check\_Head\_750MHz

### DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_600-7200\_260803 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.906$  S/m;  $\epsilon_r = 44.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.98, 9.68, 9.75); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.430 W/kg; SAR (10g) = 0.286 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 0.431 W/kg; SAR (8g) = 0.305 W/kg; SAR (10g) = 0.290 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 88.1 %

TSL Correction: Positive only

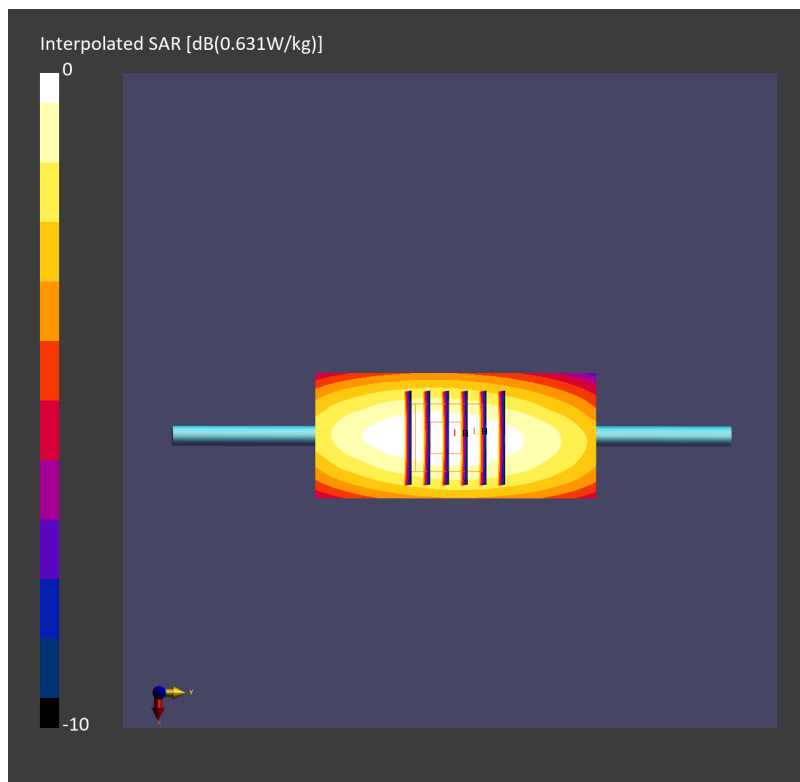

## System Check\_Head\_750MHz

### DUT: D750V3 - SN1117

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_600-7200\_260805 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.869$  S/m;  $\epsilon_r = 45.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.98, 9.68, 9.75); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.428 W/kg; SAR (10g) = 0.282 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 0.429 W/kg; SAR (8g) = 0.301 W/kg; SAR (10g) = 0.286 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

TSL Correction: Positive only

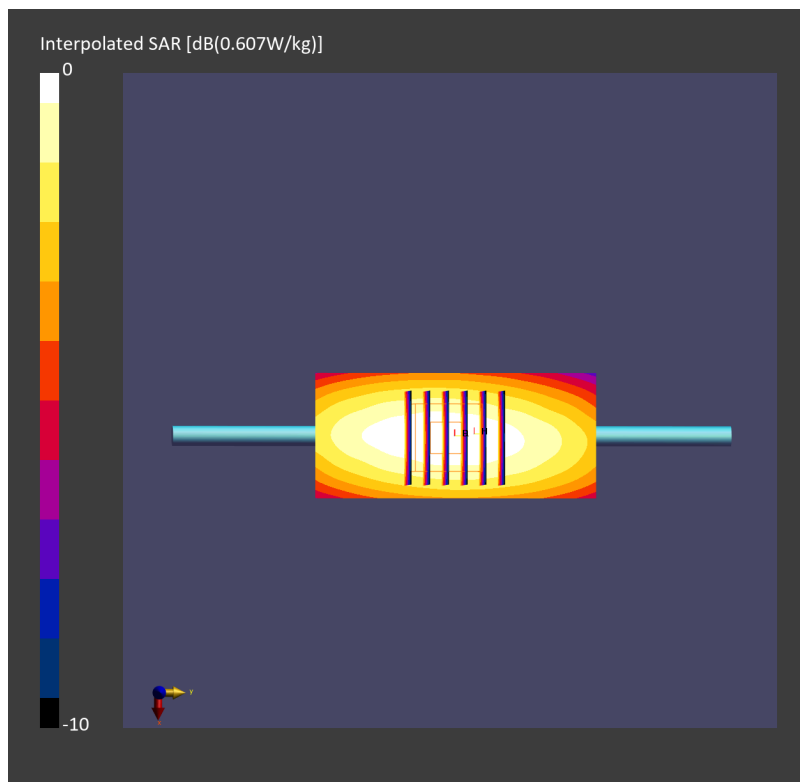

## System Check\_Head\_835MHz

### DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL\_600-7200\_260729 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.912$  S/m;  $\epsilon_r = 43.9$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.97, 9.66, 9.74); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156\_Gap\_0414; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.464 W/kg; SAR (10g) = 0.305 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 0.471 W/kg; SAR (8g) = 0.330 W/kg; SAR (10g) = 0.313 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

TSL Correction: Positive only

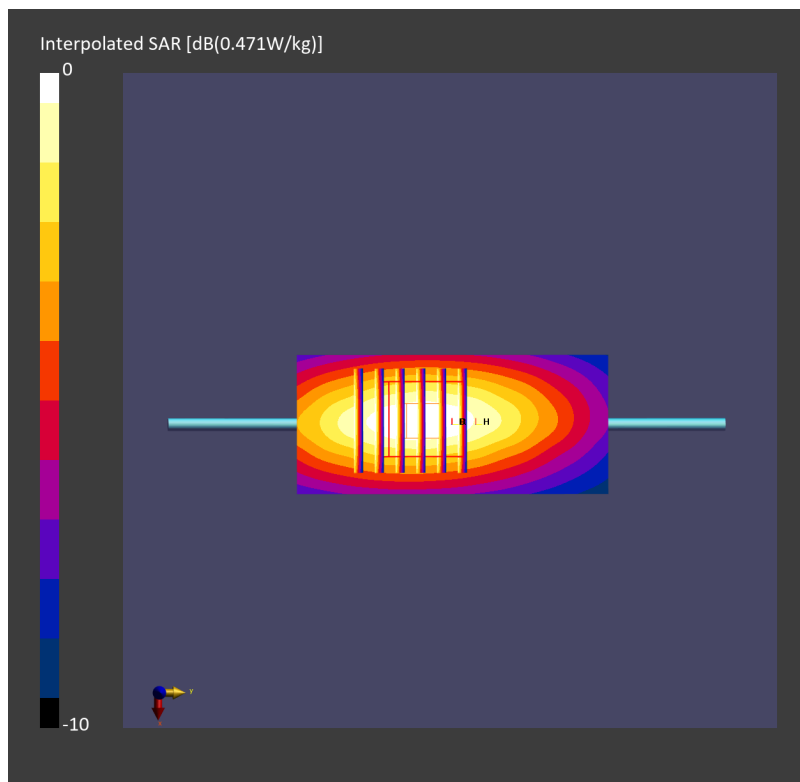

## System Check\_Head\_835MHz

### DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL\_600-7200\_260804 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.876$  S/m;  $\epsilon_r = 43.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.97, 9.66, 9.74); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.469 W/kg; SAR (10g) = 0.306 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 0.470 W/kg; SAR (8g) = 0.327 W/kg; SAR (10g) = 0.310 W/kg

Smallest distance from peaks to all points 3 dB below = 15.7 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

TSL Correction: Positive only

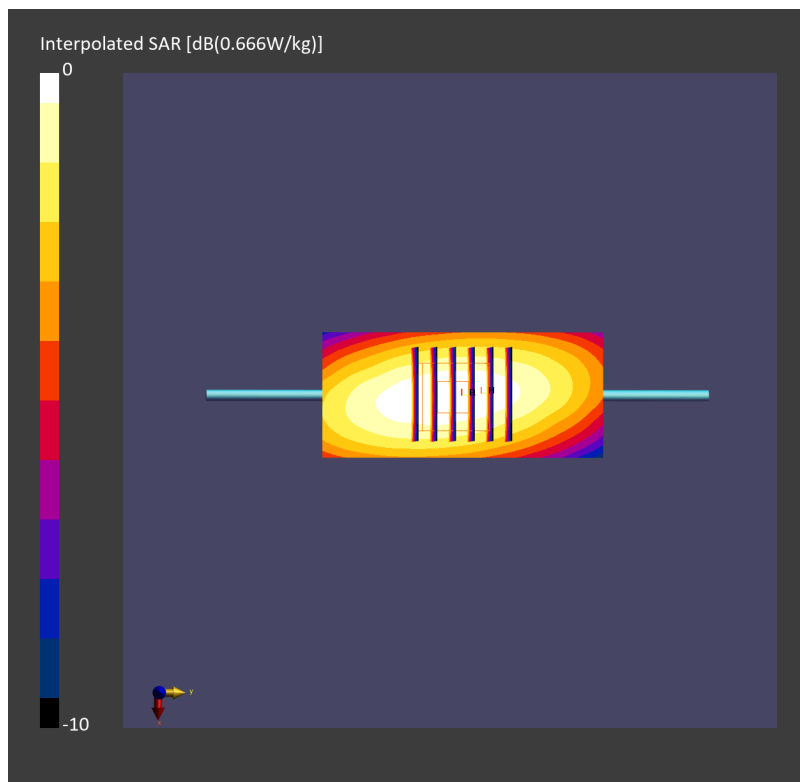

## System Check\_Head\_835MHz

### DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL\_600-7200\_260805 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.903$  S/m;  $\epsilon_r = 45.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.97, 9.66, 9.74); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.477 W/kg; SAR (10g) = 0.311 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 0.478 W/kg; SAR (8g) = 0.333 W/kg; SAR (10g) = 0.316 W/kg

Smallest distance from peaks to all points 3 dB below = 15.7 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

TSL Correction: Positive only

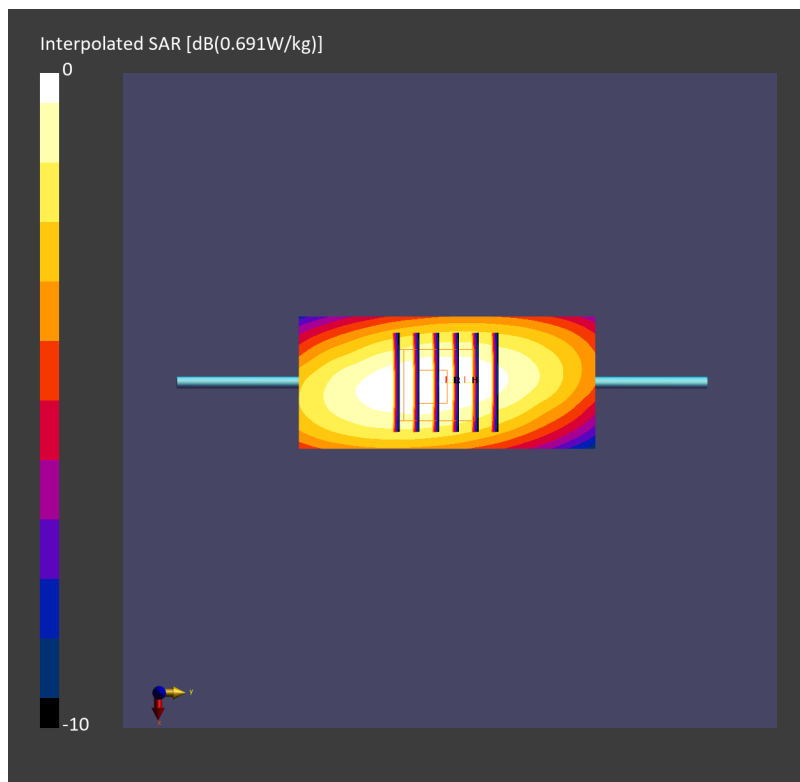

## System Check\_Head\_900MHz

### DUT: D900V2 - SN1d165

Communication System: CW; Frequency: 900.000 MHz

Medium: HSL\_600-7200\_260729 Medium parameters used:  $f = 900.000$  MHz;  $\sigma = 0.939$  S/m;  $\epsilon_r = 43.7$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.55, 9.25, 9.33); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.510 W/kg; SAR (10g) = 0.333 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 0.516 W/kg; SAR (8g) = 0.360 W/kg; SAR (10g) = 0.341 W/kg

Smallest distance from peaks to all points 3 dB below = 16.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

TSL Correction: Positive only

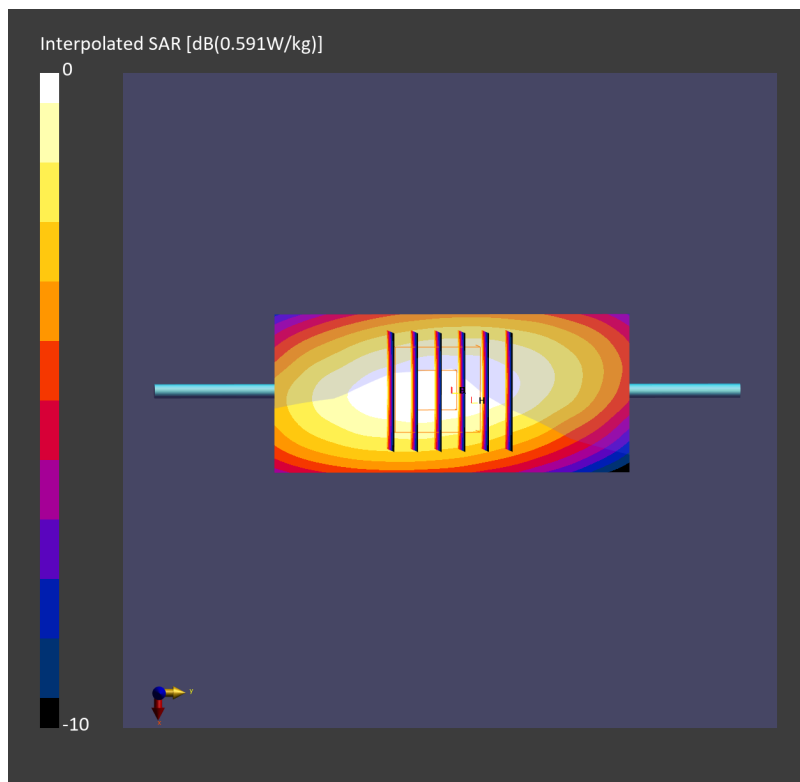

## System Check\_Head\_900MHz

### DUT: D900V2 - SN1d165

Communication System: CW; Frequency: 900.000 MHz

Medium: HSL\_600-7200\_260805 Medium parameters used:  $f = 900.000$  MHz;  $\sigma = 0.929$  S/m;  $\epsilon_r = 45.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.55, 9.25, 9.33); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.531 W/kg; SAR (10g) = 0.341 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 0.536 W/kg; SAR (8g) = 0.369 W/kg; SAR (10g) = 0.350 W/kg

Smallest distance from peaks to all points 3 dB below = 16.1 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

TSL Correction: Positive only

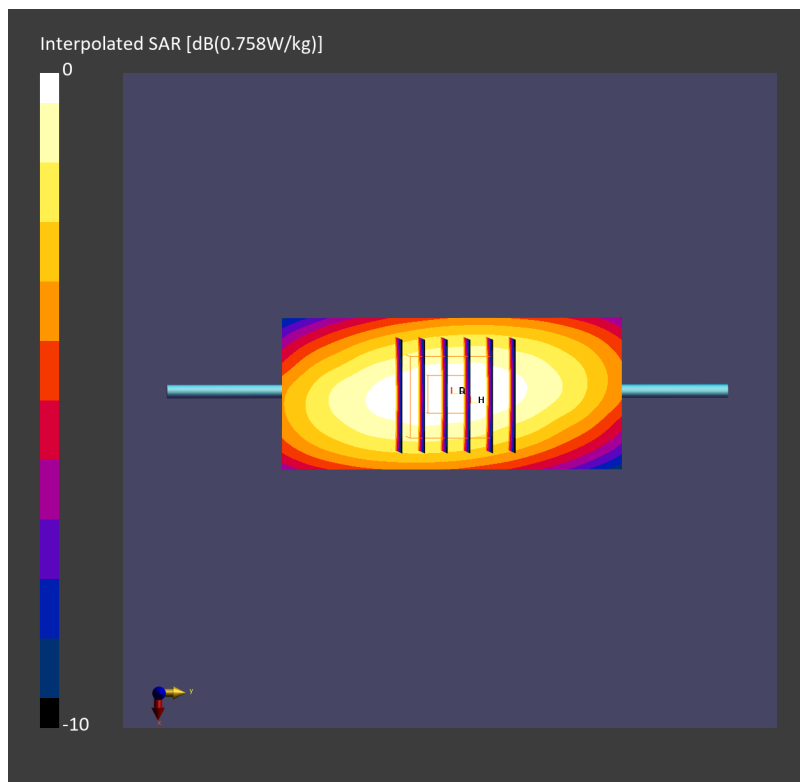

## System Check\_Head\_1750MHz

### DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL\_600-7200\_260729 Medium parameters used:  $f = 1750.000$  MHz;  $\sigma = 1.36$  S/m;  $\epsilon_r = 41.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.9, 7.56, 8.41); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2026-06-02
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.80 W/kg; SAR (10g) = 0.947 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.85 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 81.3 %

TSL Correction: Positive only

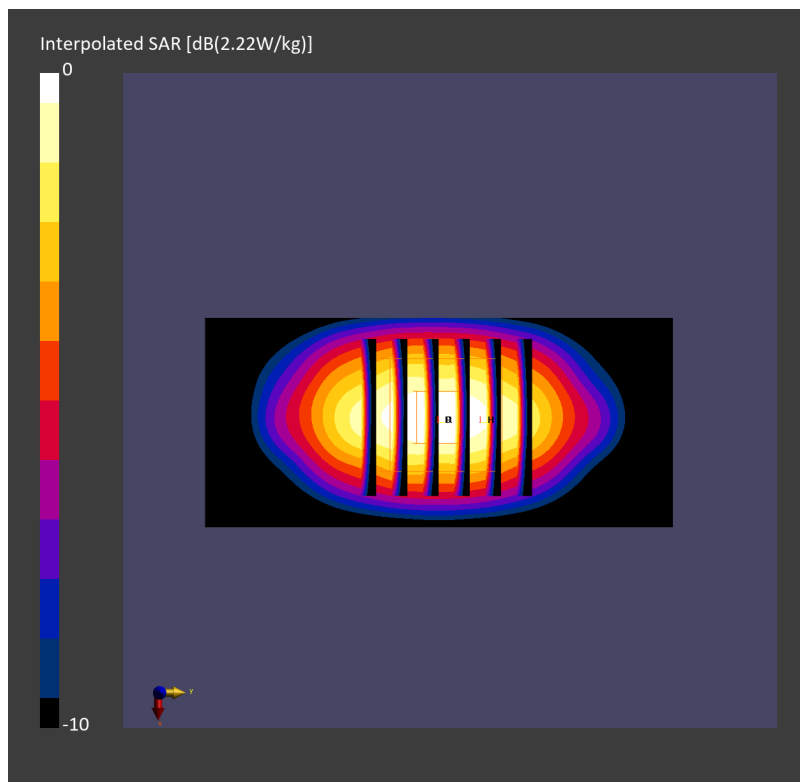

## System Check\_Head\_1750MHz

### DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL\_600-7200\_260730 Medium parameters used:  $f = 1750.000$  MHz;  $\sigma = 1.37$  S/m;  $\epsilon_r = 40.9$

Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.26, 8.0, 8.07); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156\_Gap\_0414; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.80 W/kg; SAR (10g) = 0.958 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.81 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.970 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

TSL Correction: Positive only

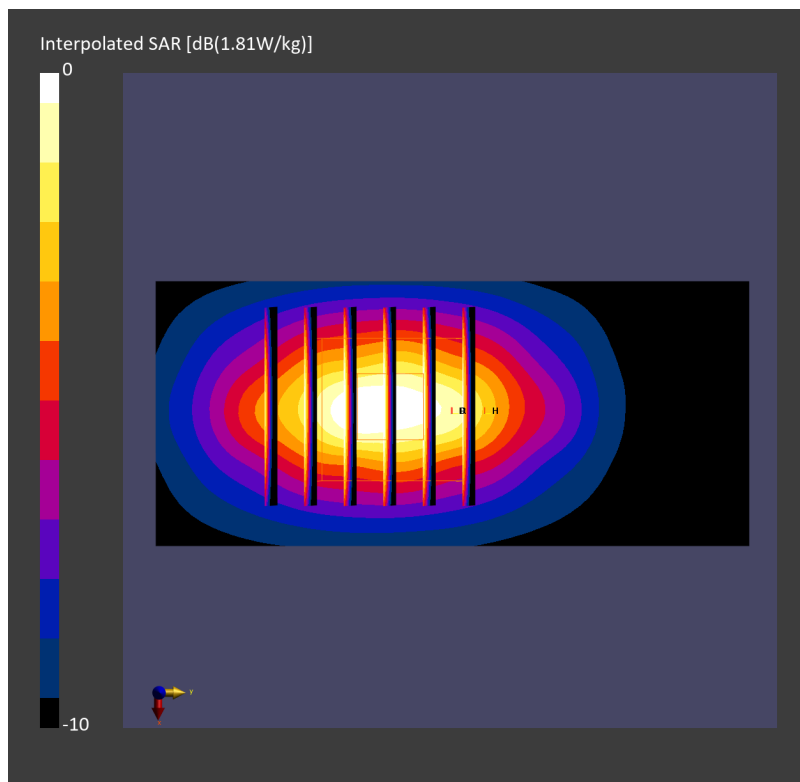

## System Check\_Head\_1900MHz

### DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL\_600-7200\_260728 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.38$  S/m;  $\epsilon_r = 39.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.54, 7.21, 8.01); Calibrated: 2025-12-09
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2026-06-02
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 0.954 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 1.93 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 78.5 %

TSL Correction: Positive only

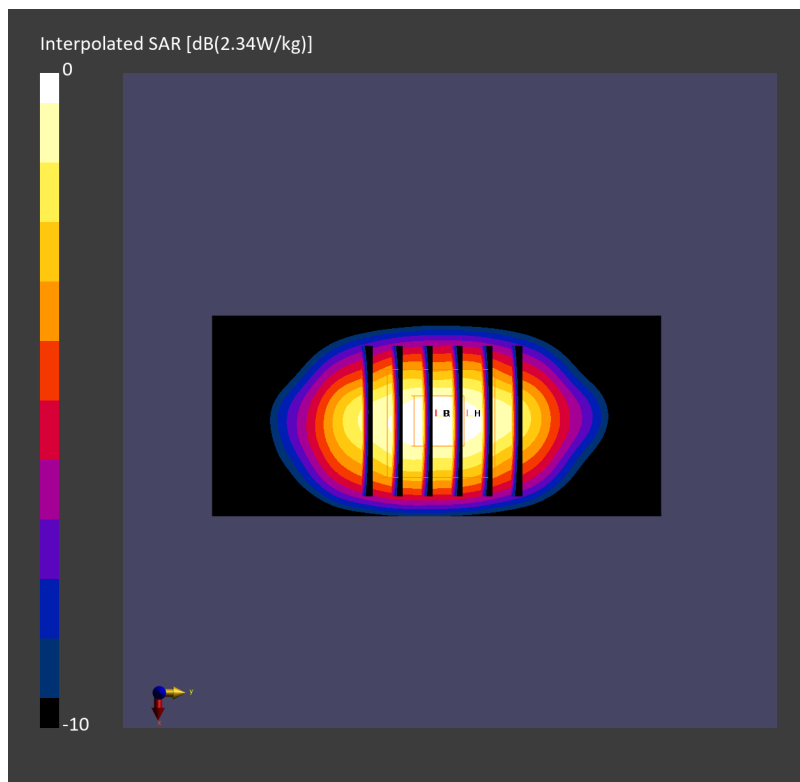

## System Check\_Head\_1900MHz

### DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL\_600-7200\_260730 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.46$  S/m;  $\epsilon_r = 40.7$

Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.08, 7.83, 7.89); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156\_Gap\_0414; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.88 W/kg; SAR (10g) = 0.983 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.90 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.995 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.0 %

TSL Correction: Positive only

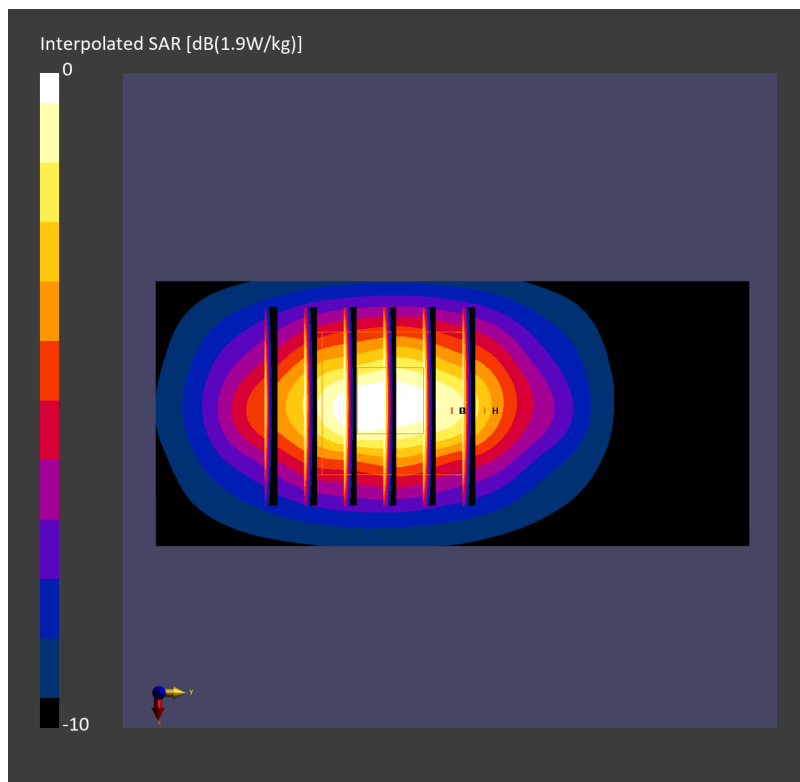

## System Check\_Head\_2300MHz

### DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL\_600-7200\_260731 Medium parameters used:  $f = 2300.000$  MHz;  $\sigma = 1.72$  S/m;  $\epsilon_r = 42.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.76, 7.52, 7.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.29 W/kg; SAR (10g) = 1.08 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.29 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

TSL Correction: Positive only

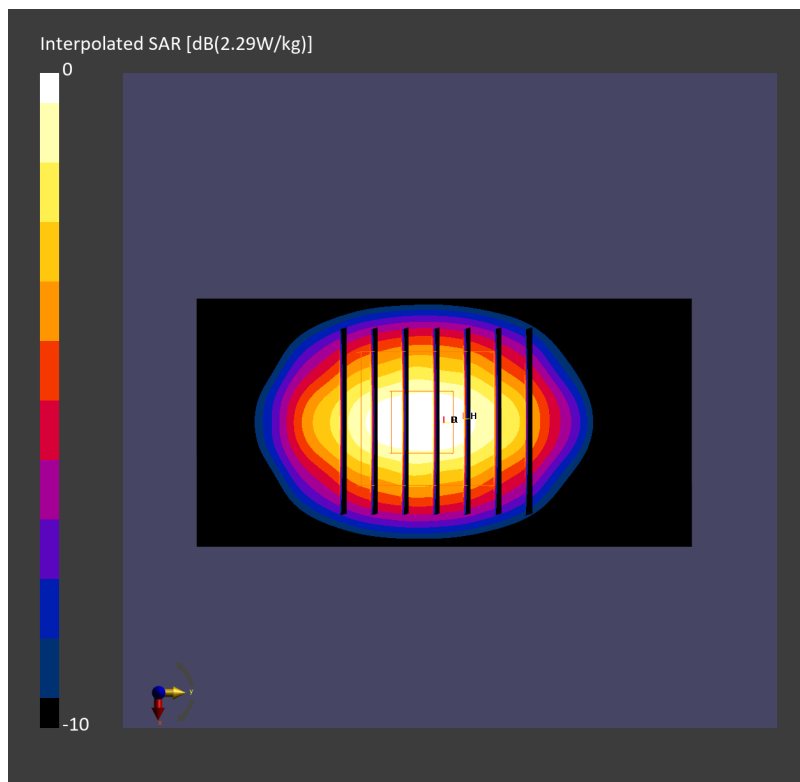

## System Check\_Head\_2300MHz

### DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL\_600-7200\_260808 Medium parameters used:  $f = 2300.000$  MHz;  $\sigma = 1.69$  S/m;  $\epsilon_r = 43.1$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.76, 7.52, 7.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.31 W/kg; SAR (10g) = 1.08 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.26 W/kg; SAR (8g) = 1.18 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

TSL Correction: Positive only

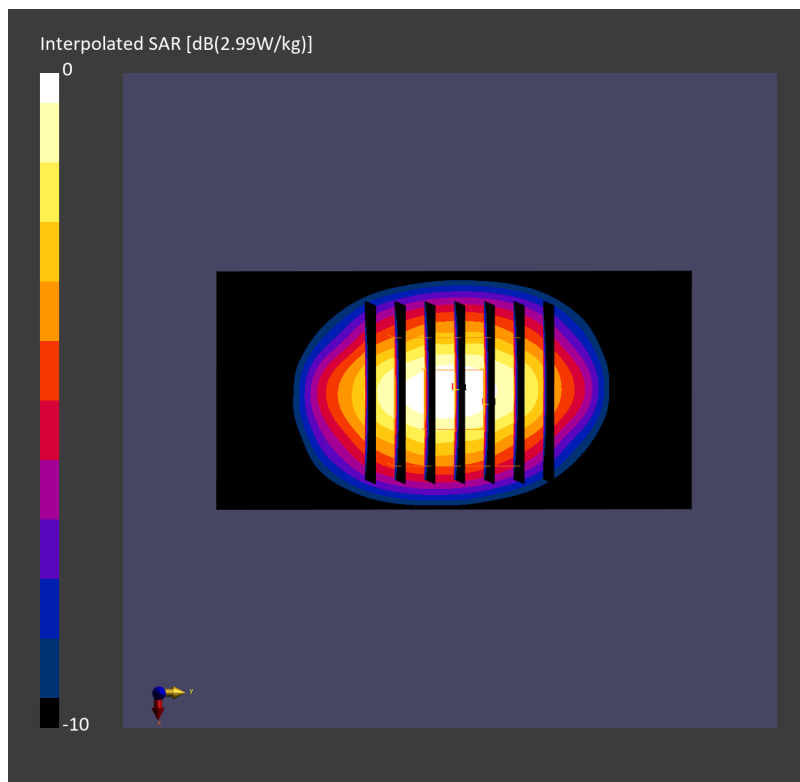

## System Check\_Head\_2600MHz

### DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_600-7200\_260731 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.96$  S/m;  $\epsilon_r = 42.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.64 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.64 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.8 %

TSL Correction: Positive only

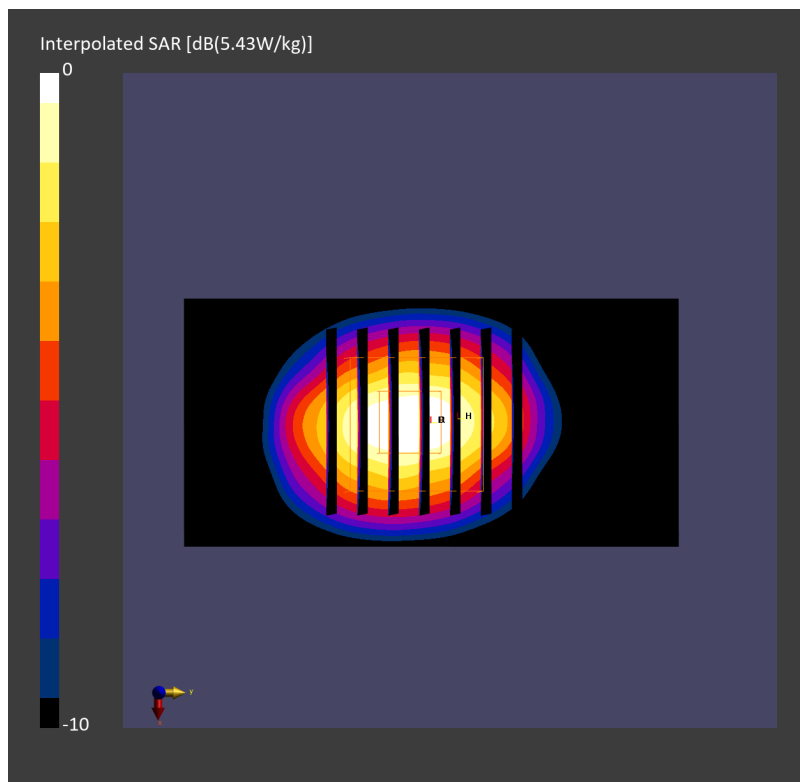

## System Check\_Head\_2600MHz

### DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_600-7200\_260806 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.91$  S/m;  $\epsilon_r = 42.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.61 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.59 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.9 %

TSL Correction: Positive only

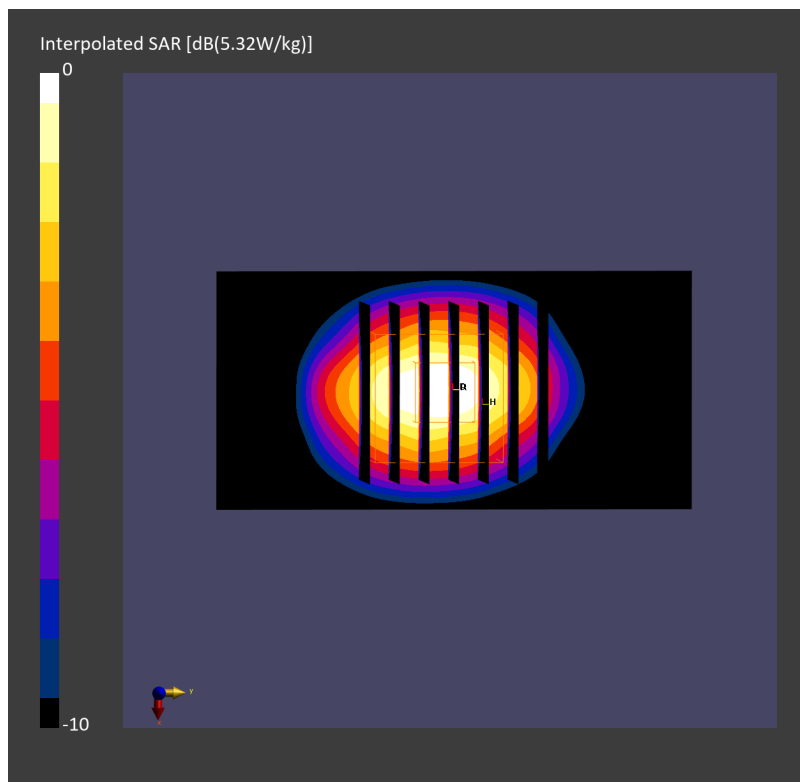

## System Check\_Head\_2600MHz

### DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_600-7200\_260807 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.97$  S/m;  $\epsilon_r = 42.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.63 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

TSL Correction: Positive only

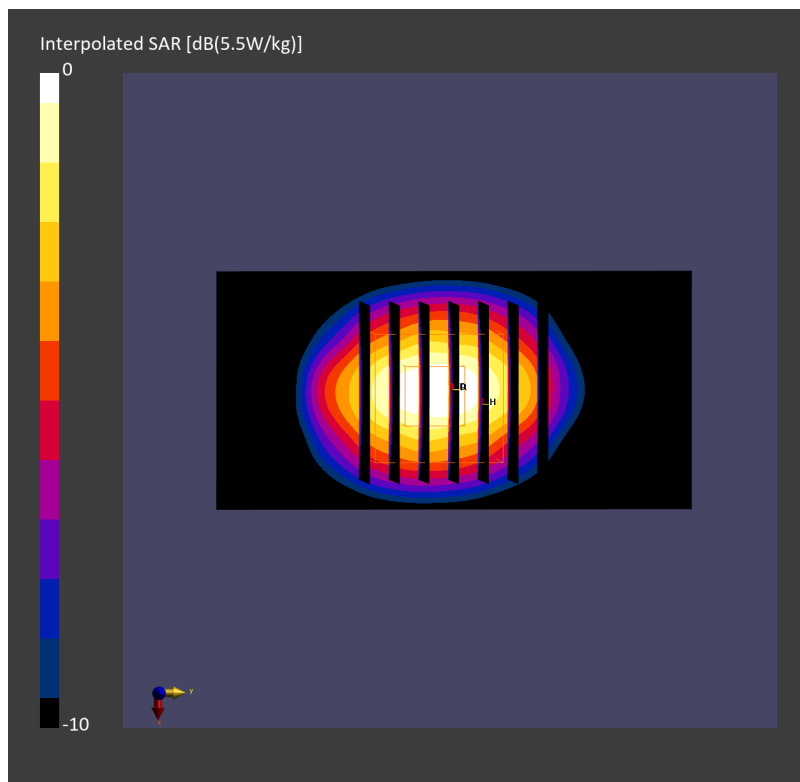

## System Check\_Head\_2600MHz

### DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_600-7200\_260808 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.91$  S/m;  $\epsilon_r = 42.8$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.63 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.59 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.1 %

TSL Correction: Positive only

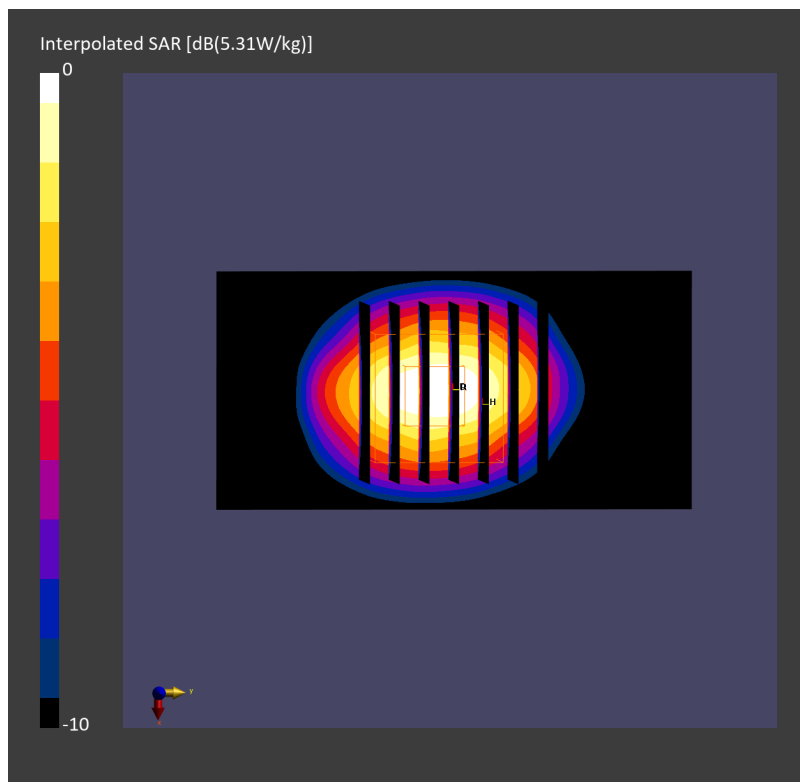

## System Check\_Head\_3500MHz

### DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_600-7200\_260725 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.68$  S/m;  $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.27 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.5 %

TSL Correction: Positive only

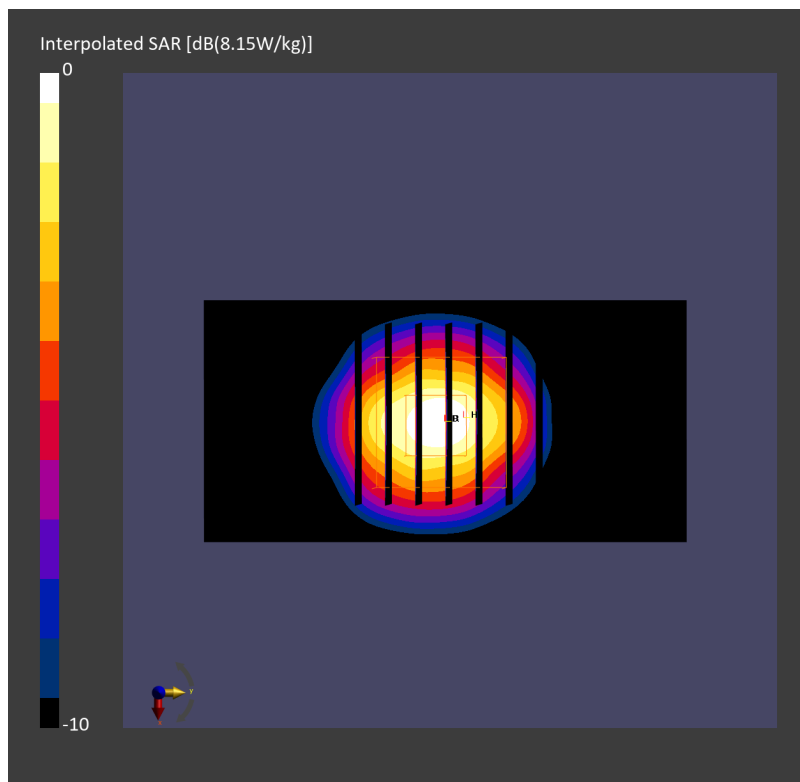

## System Check\_Head\_3500MHz

### DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_600-7200\_260801 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.78$  S/m;  $\epsilon_r = 37.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.32 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.5 %

TSL Correction: Positive only

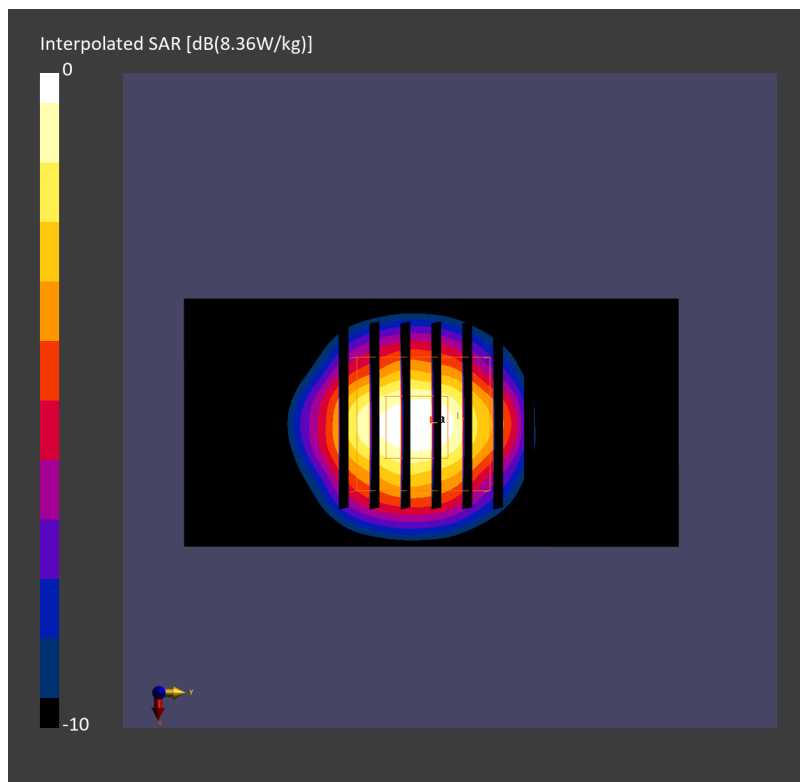

## System Check\_Head\_3500MHz

### DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_600-7200\_260809 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.69$  S/m;  $\epsilon_r = 39.9$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.33 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

TSL Correction: Positive only

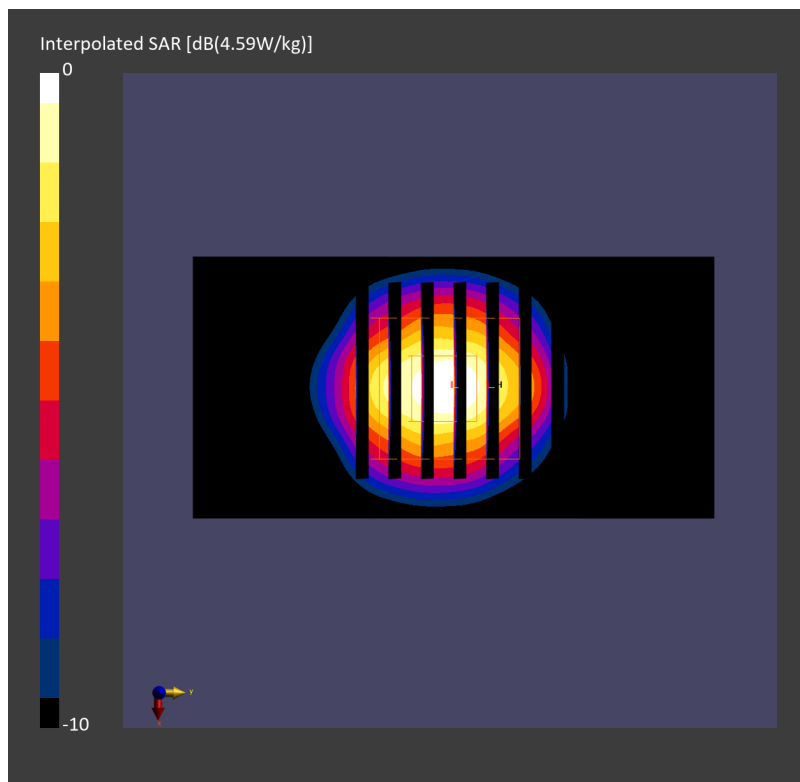

## System Check\_Head\_3500MHz

### DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_600-7200\_260810 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.78$  S/m;  $\epsilon_r = 37.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.35 W/kg; SAR (10g) = 1.26 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.37 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

TSL Correction: Positive only

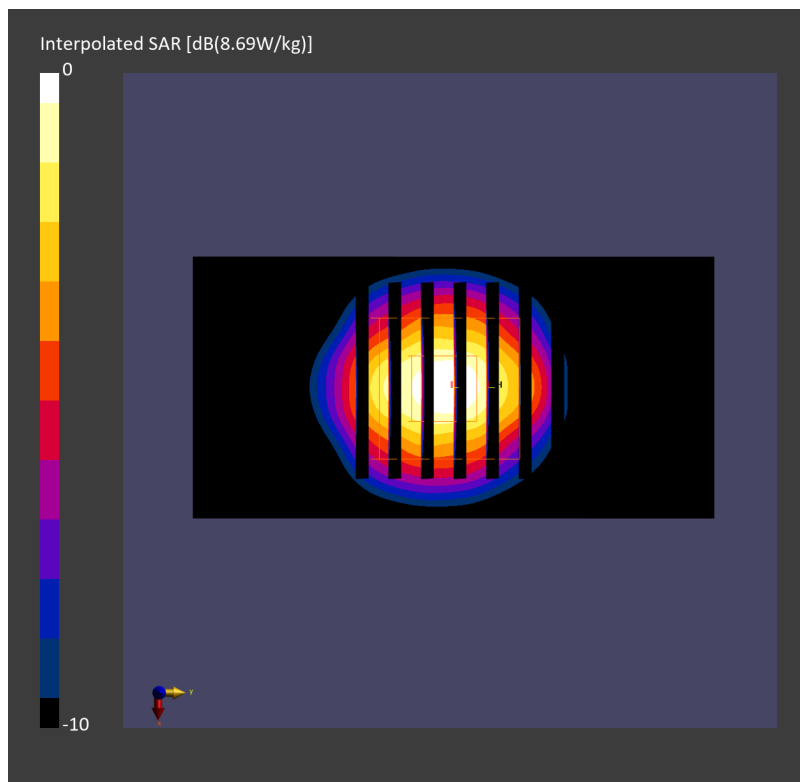

## System Check\_Head\_3500MHz

### DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_600-7200\_260811 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.69$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.22 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.33 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.3 %

TSL Correction: Positive only

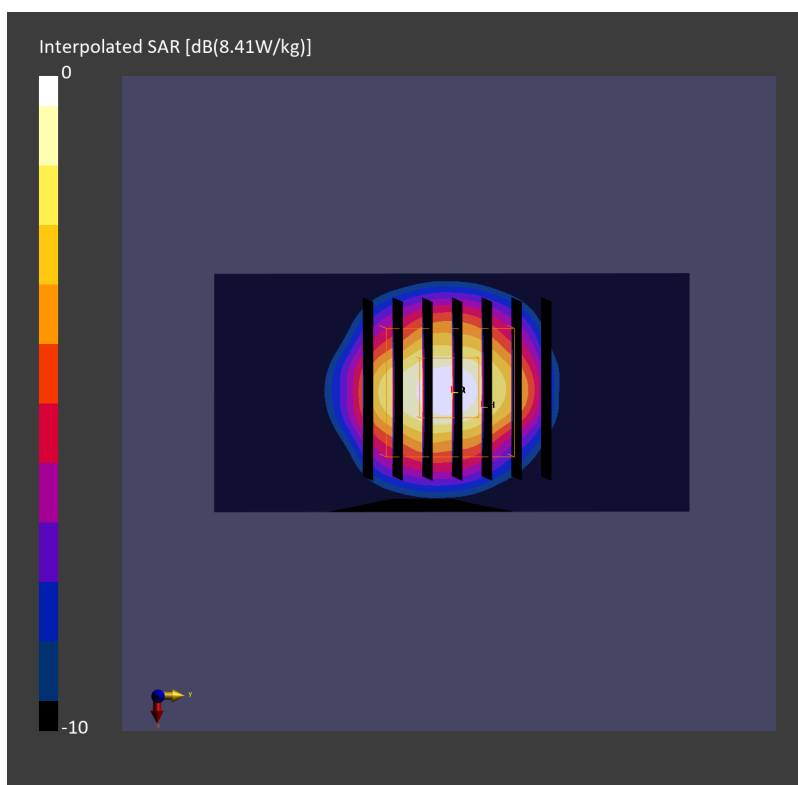

## System Check\_Head\_3500MHz

### DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_600-7200\_260812 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.68$  S/m;  $\epsilon_r = 39.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.24 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.6 %

TSL Correction: Positive only

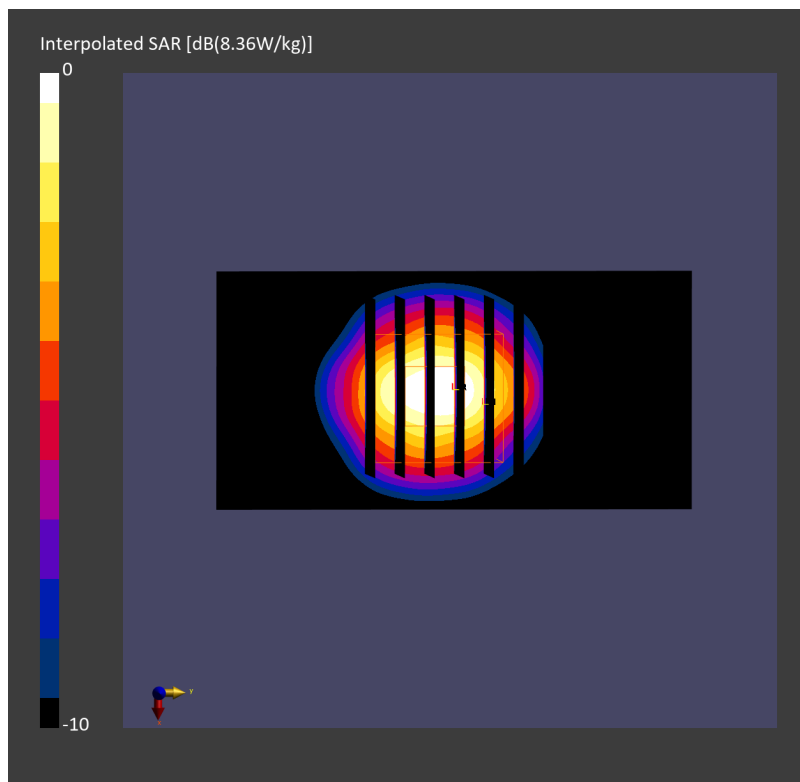

## System Check\_Head\_3500MHz

### DUT: D3500V2 - SN1014

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL\_600-7200\_260813 Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.70$  S/m;  $\epsilon_r = 38.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.29 W/kg; SAR (10g) = 1.24 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.29 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.5 %

TSL Correction: Positive only

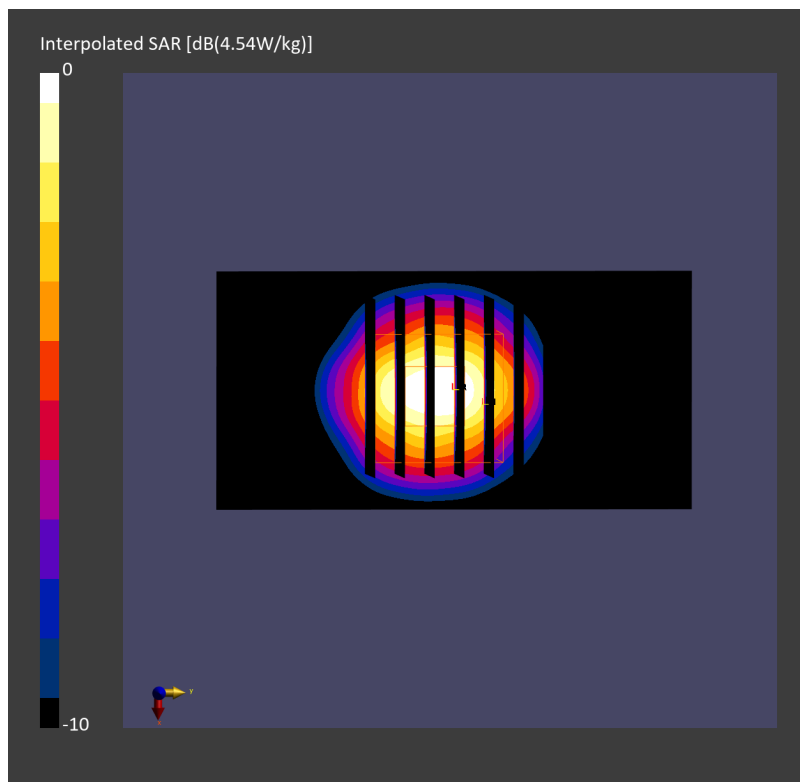

## System Check\_Head\_3700MHz

### DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_600-7200\_260725 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 2.86$  S/m;  $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.12 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.21 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 73.7 %

TSL Correction: Positive only

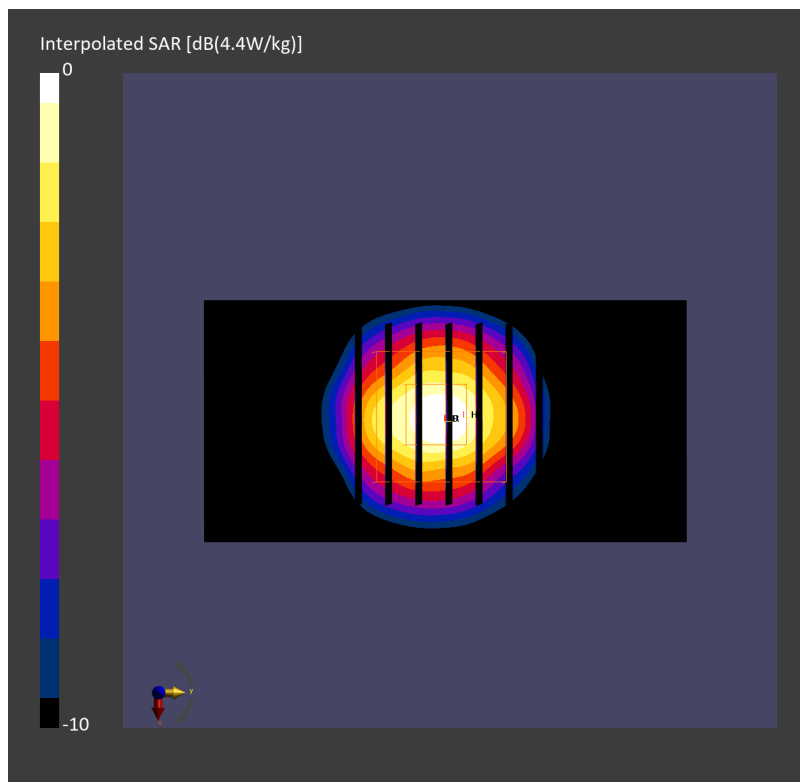

## System Check\_Head\_3700MHz

### DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_600-7200\_260801 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 2.96$  S/m;  $\epsilon_r = 37.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.23 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.1 %

TSL Correction: Positive only

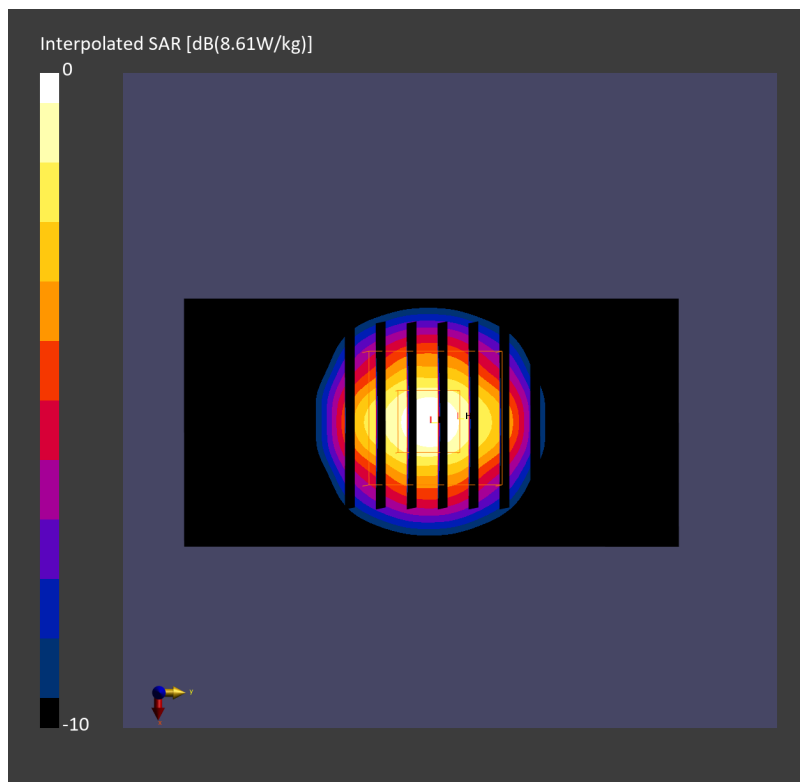

## System Check\_Head\_3700MHz

### DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_600-7200\_260809 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 2.87$  S/m;  $\epsilon_r = 39.6$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.26 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 73.7 %

TSL Correction: Positive only

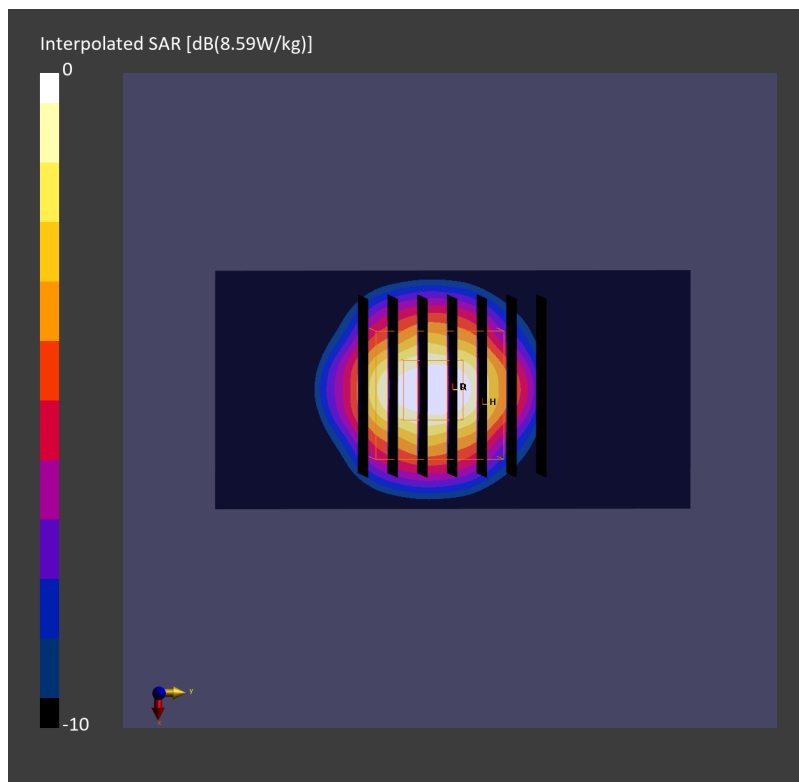

## System Check\_Head\_3700MHz

### DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_600-7200\_260810 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 2.96$  S/m;  $\epsilon_r = 37.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.20 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 73.7 %

TSL Correction: Positive only

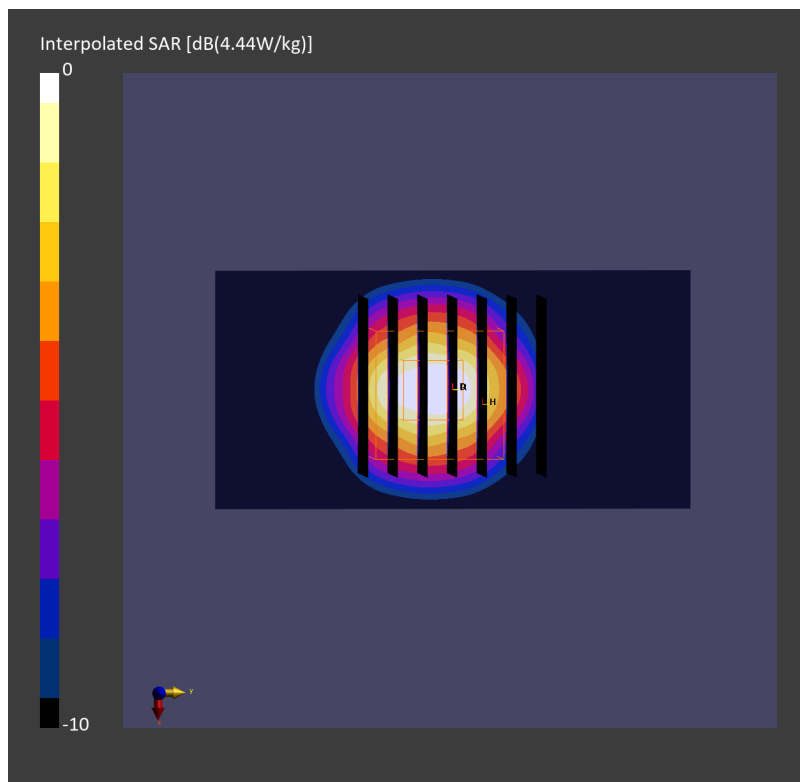

## System Check\_Head\_3700MHz

### DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_600-7200\_260811 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 2.86$  S/m;  $\epsilon_r = 38.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.15 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.23 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 73.8 %

TSL Correction: Positive only

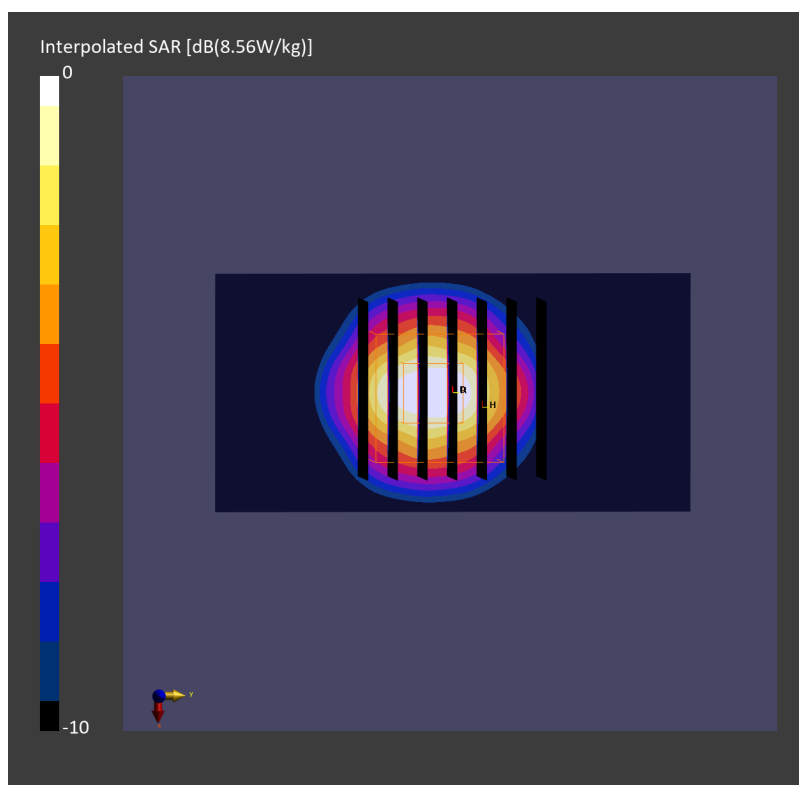

## System Check\_Head\_3700MHz

### DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_600-7200\_260812 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 2.85$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.22 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 73.9 %

TSL Correction: Positive only

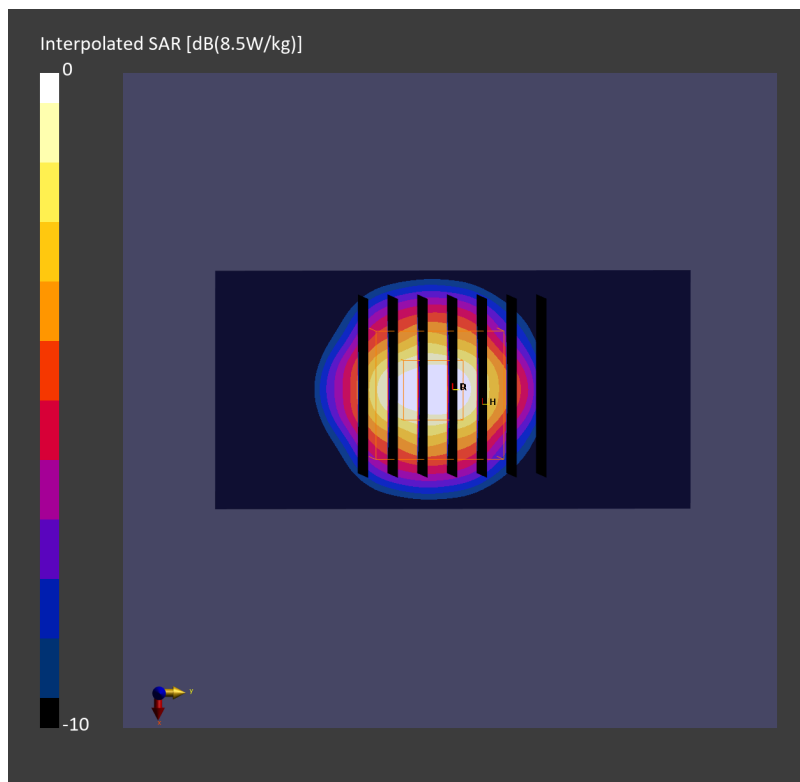

## System Check\_Head\_3700MHz

### DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL\_600-7200\_260813 Medium parameters used:  $f = 3700.000$  MHz;  $\sigma = 2.87$  S/m;  $\epsilon_r = 37.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.22 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 74.0 %

TSL Correction: Positive only

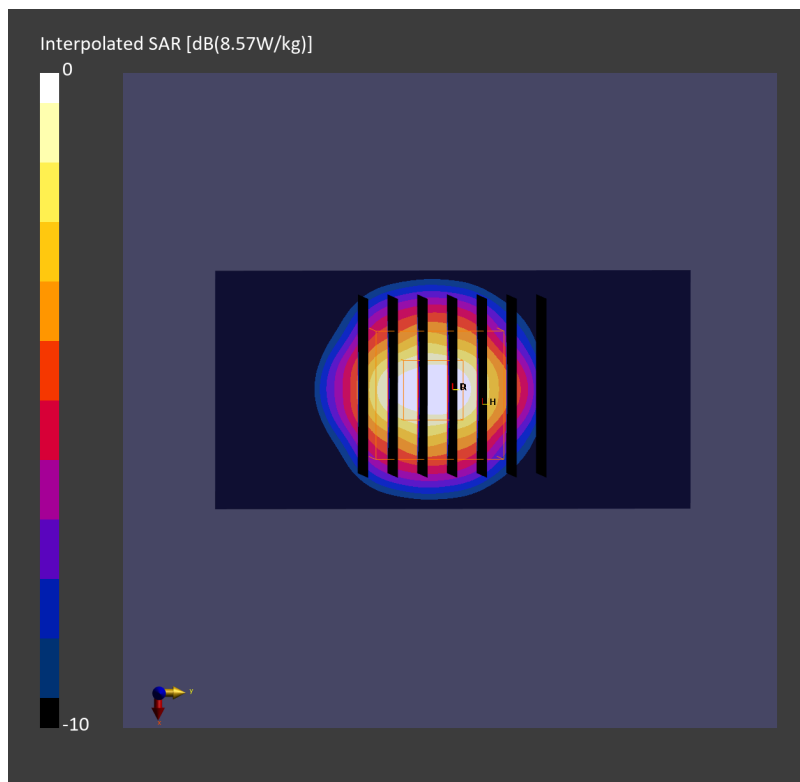

## System Check\_Head\_3900MHz

### DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_600-7200\_260725 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.05$  S/m;  $\epsilon_r = 38.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156\_Gap\_0414; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 5.92 W/kg; SAR (10g) = 2.05 W/kg;

TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.08 W/kg; SAR (8g) = 2.43 W/kg; SAR (10g) = 2.13 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 72.6 %

TSL Correction: Positive only

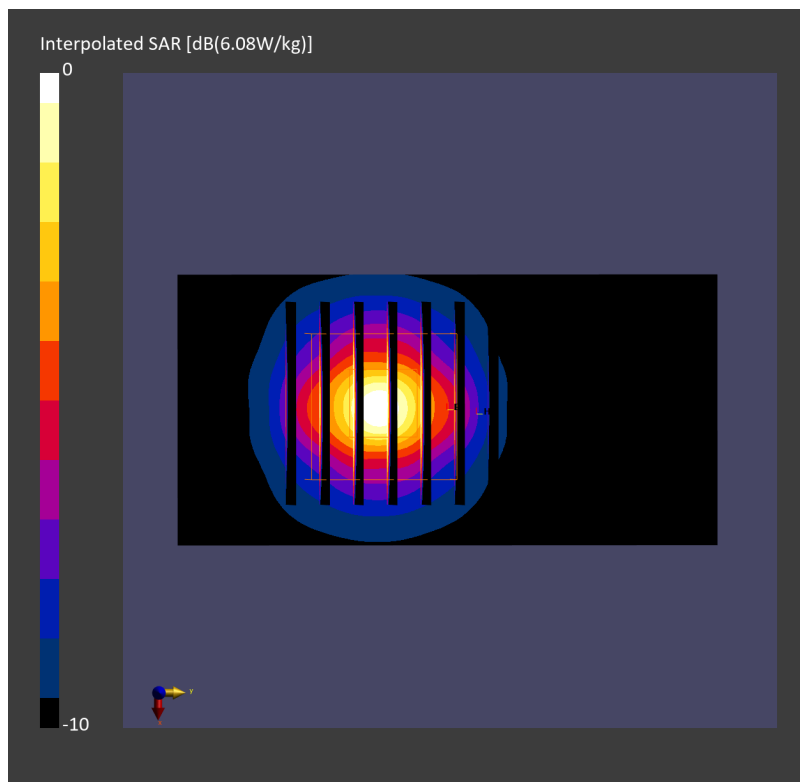

## System Check\_Head\_3900MHz

### DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_600-7200\_260801 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.13$  S/m;  $\epsilon_r = 37.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156\_Gap\_0414; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.00 W/kg; SAR (10g) = 2.09 W/kg;

TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 6.17 W/kg; SAR (8g) = 2.47 W/kg; SAR (10g) = 2.17 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 72.6 %

TSL Correction: Positive only

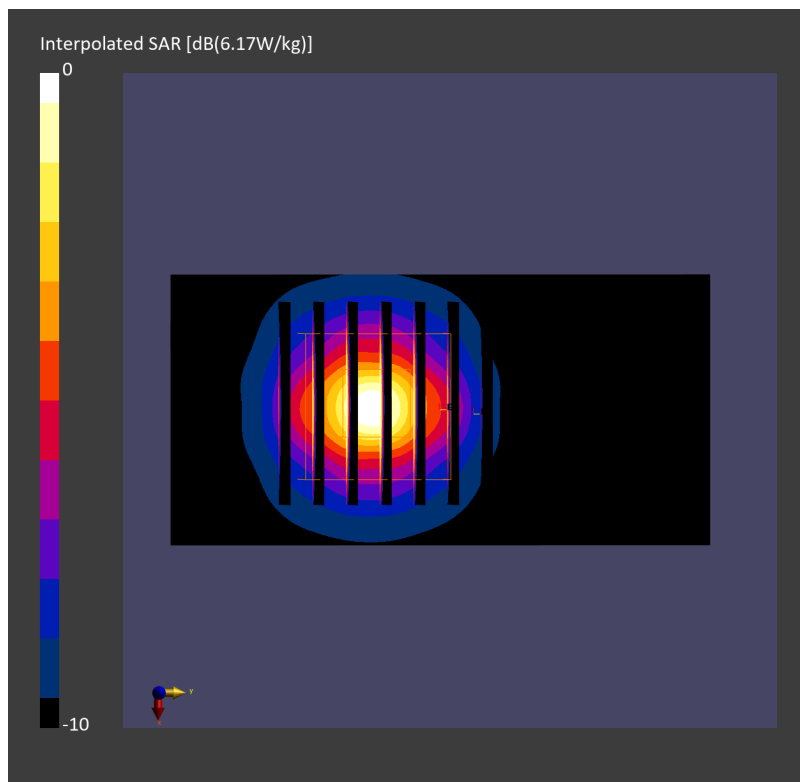

## System Check\_Head\_3900MHz

### DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_600-7200\_260809 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.07$  S/m;  $\epsilon_r = 39.4$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 5.97 W/kg; SAR (10g) = 2.09 W/kg;

TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 6.07 W/kg; SAR (8g) = 2.42 W/kg; SAR (10g) = 2.13 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.3 %

TSL Correction: Positive only

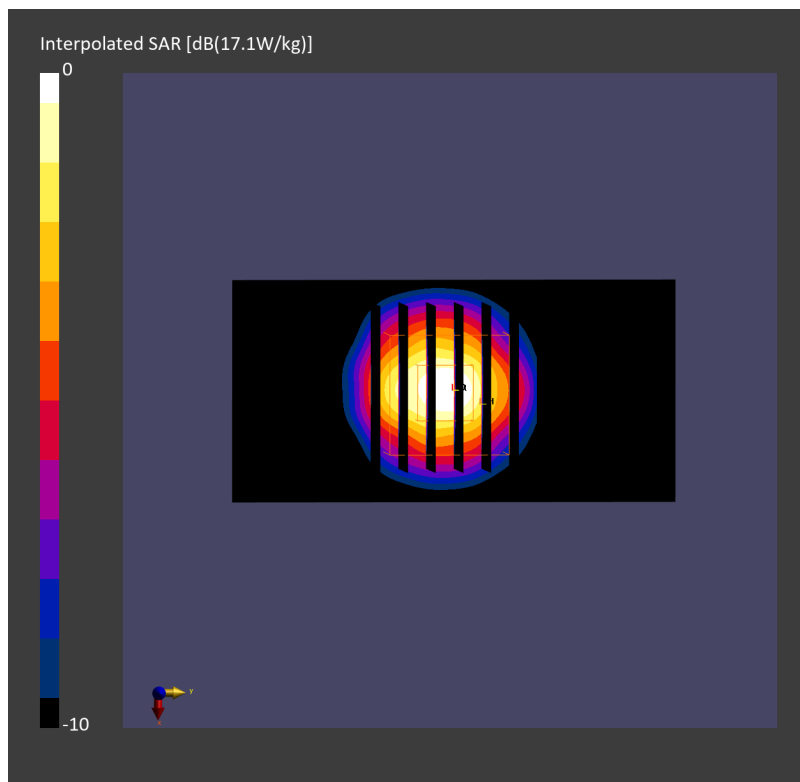

## System Check\_Head\_3900MHz

### DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_600-7200\_260810 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.13$  S/m;  $\epsilon_r = 37.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.12 W/kg; SAR (10g) = 2.15 W/kg;

TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 6.21 W/kg; SAR (8g) = 2.48 W/kg; SAR (10g) = 2.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.2 %

TSL Correction: Positive only

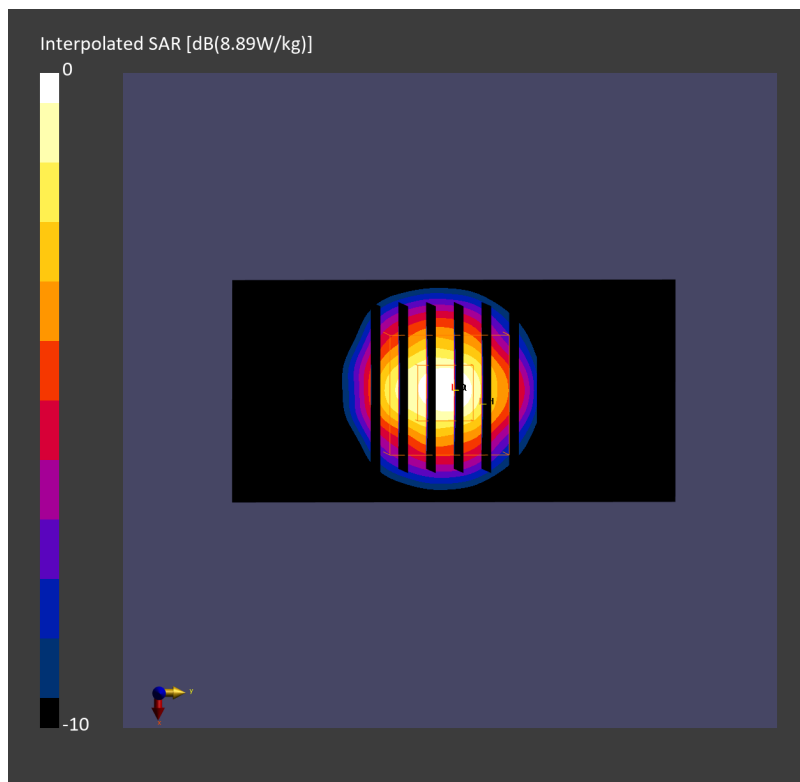

## System Check\_Head\_3900MHz

### DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_600-7200\_260811 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.04$  S/m;  $\epsilon_r = 38.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.02 W/kg; SAR (10g) = 2.10 W/kg;

TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 6.10 W/kg; SAR (8g) = 2.43 W/kg; SAR (10g) = 2.14 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.4 %

TSL Correction: Positive only

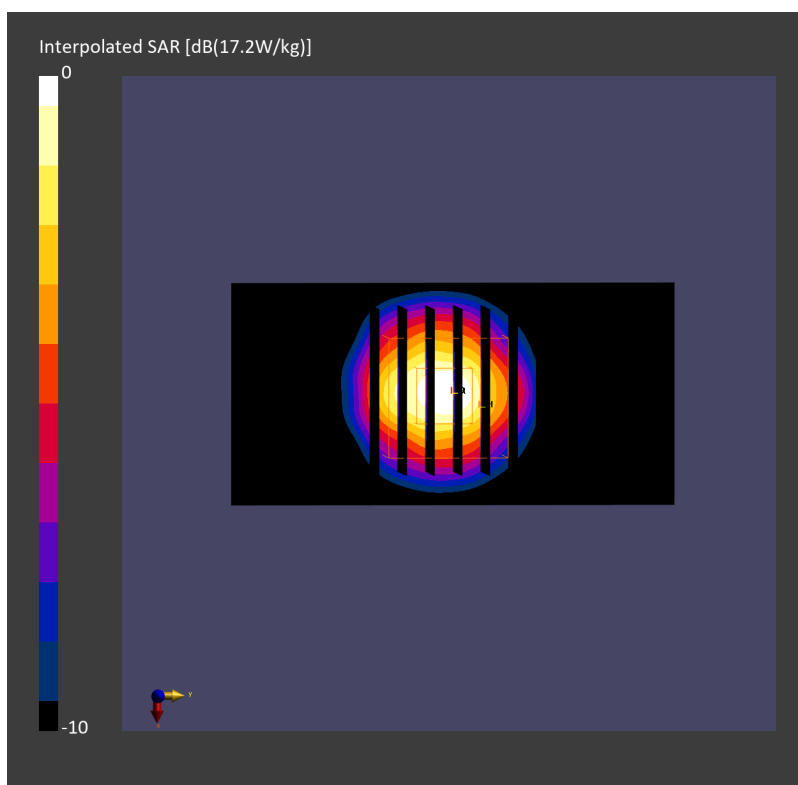

## System Check\_Head\_3900MHz

### DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_600-7200\_260812 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.04$  S/m;  $\epsilon_r = 38.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.06 W/kg; SAR (10g) = 2.11 W/kg;

TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 6.15 W/kg; SAR (8g) = 2.45 W/kg; SAR (10g) = 2.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.3 %

TSL Correction: Positive only

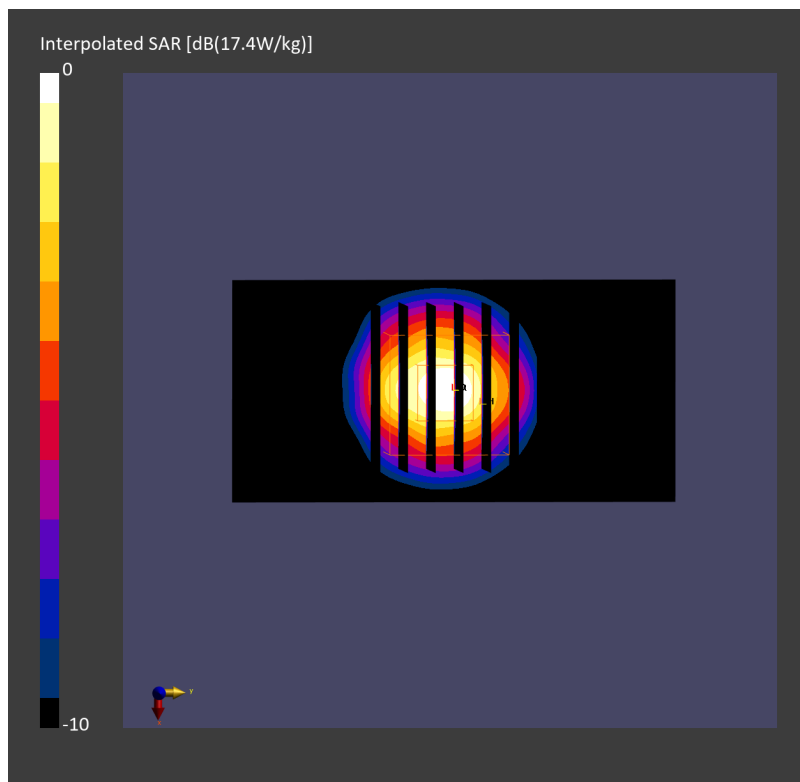

## System Check\_Head\_3900MHz

### DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL\_600-7200\_260813 Medium parameters used:  $f = 3900.000$  MHz;  $\sigma = 3.06$  S/m;  $\epsilon_r = 37.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2026-03-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

**Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.20 W/kg; SAR (10g) = 2.17 W/kg;

TSL Correction: Positive only

**Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 6.29 W/kg; SAR (8g) = 2.51 W/kg; SAR (10g) = 2.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.5 %

TSL Correction: Positive only

