

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

FCC ID: BCG-A3584	RF EXPOSURE REPORT		Approved by: Technical Manager
DUT Type: Watch		This report is Blockchain Verified. To verify the report authenticity, please visit https://www.blockchain-verified.com or by clicking on the Blockchain logo.	Appendix B

ELEMENT

DUT: Dipole 13.0 MHz; Type: CLA13 - SN1004

Communication System: UID: 0, CW; Frequency: 13.0 MHz
Medium: 30 Head; Medium parameters used:
 $f = 13.0$ MHz; $\text{cond} = 0.752$ S/m; $\text{perm} = 53.5$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 0 mm

Test Date: 07/08/2026; Ambient Temp: 21.1°C; Tissue Temp: 24.6°C

Probe: EX3DV4 - SN7782; ConvF:(18.49,15.42,16.82); Calibrated: 2025-09-15
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2025-09-10
Phantom: ELI V6.0; Serial: 2044
Measurement SW: DASY Module SAR V16.4.0.5005

13.0 MHz System Verification at 30.0 dBm (1000 mW)


Area Scan (40.0 x 90.0): Measurement grid: $dx=10.0$ mm, $dy=15.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=6.0$ mm, $dy=6.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 1.11 W/kg

SAR(1 g) = 0.544 W/kg; SAR(10 g) = 0.334 W/kg

Deviation (1 g) = -7.01%; Deviation (10 g) = -6.70%

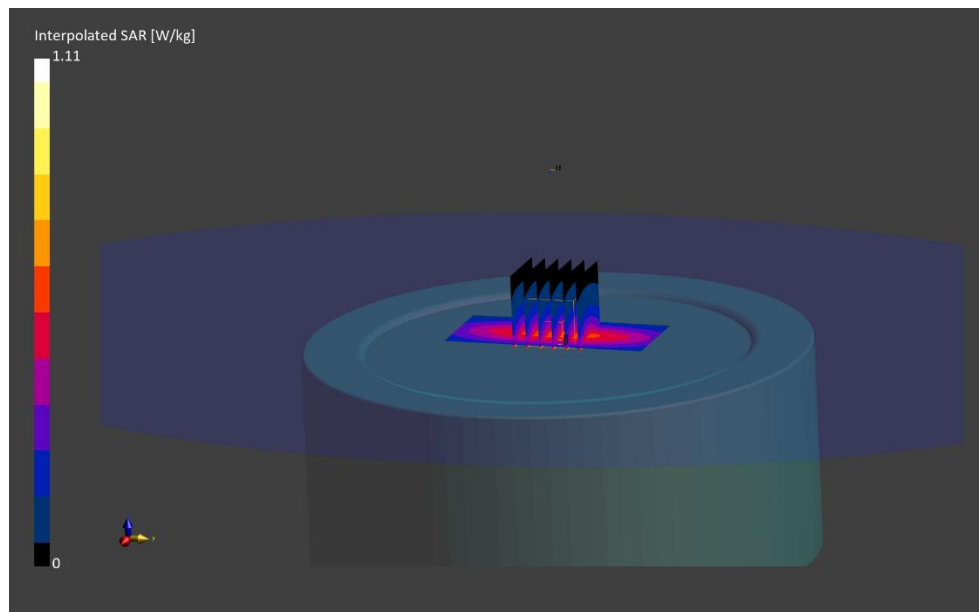

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN855

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\text{cond} = 1.86$ S/m; $\text{perm} = 38.2$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 06/16/2026; Ambient Temp: 22.5°C; Tissue Temp: 23.1°C

Probe: EX3DV4 - SN7551; ConvF:(6.86,6.94,7.06); Calibrated: 2026-03-10

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1323; Calibrated: 2026-03-10

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.6 W/kg

SAR(1 g) = 5.43 W/kg; SAR(10 g) = 2.45 W/kg

Deviation (1 g) = 1.88%; Deviation (10 g) = -2.00%

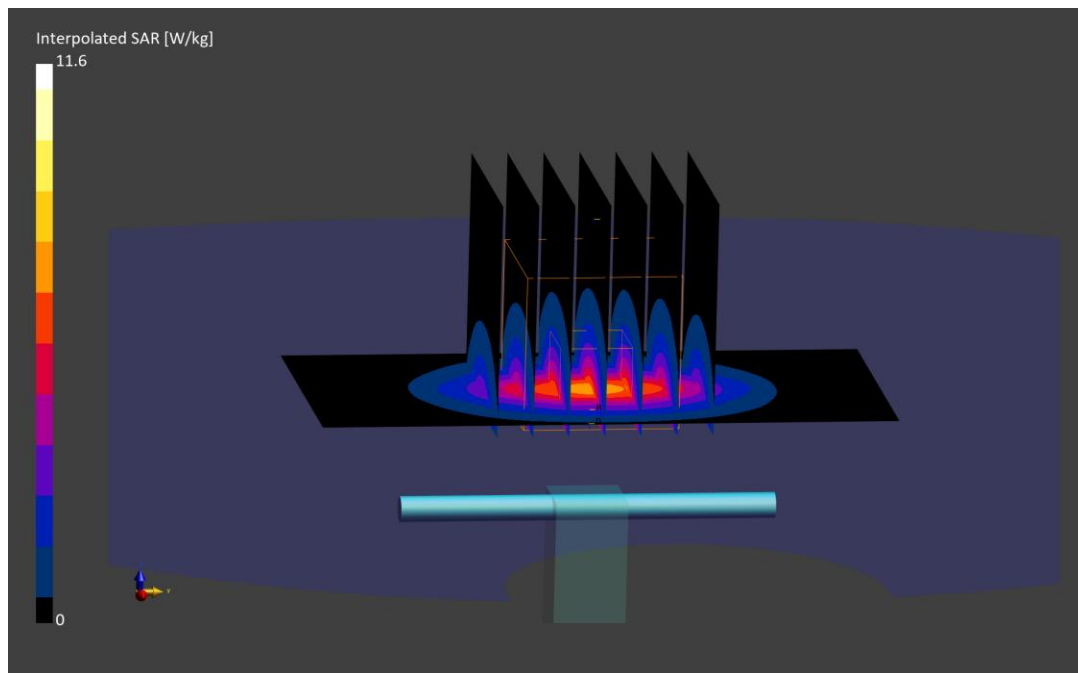

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN855

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\text{cond} = 1.86$ S/m; $\text{perm} = 38.4$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/07/2026; Ambient Temp: 24.0°C; Tissue Temp: 23.2°C

Probe: EX3DV4 - SN7551; ConvF:(6.86,6.94,7.06); Calibrated: 2026-03-10

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1323; Calibrated: 2026-03-10

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.3 W/kg

SAR(1 g) = 5.33 W/kg; SAR(10 g) = 2.42 W/kg

Deviation (1 g) = 0.00%; Deviation (10 g) = -3.20%

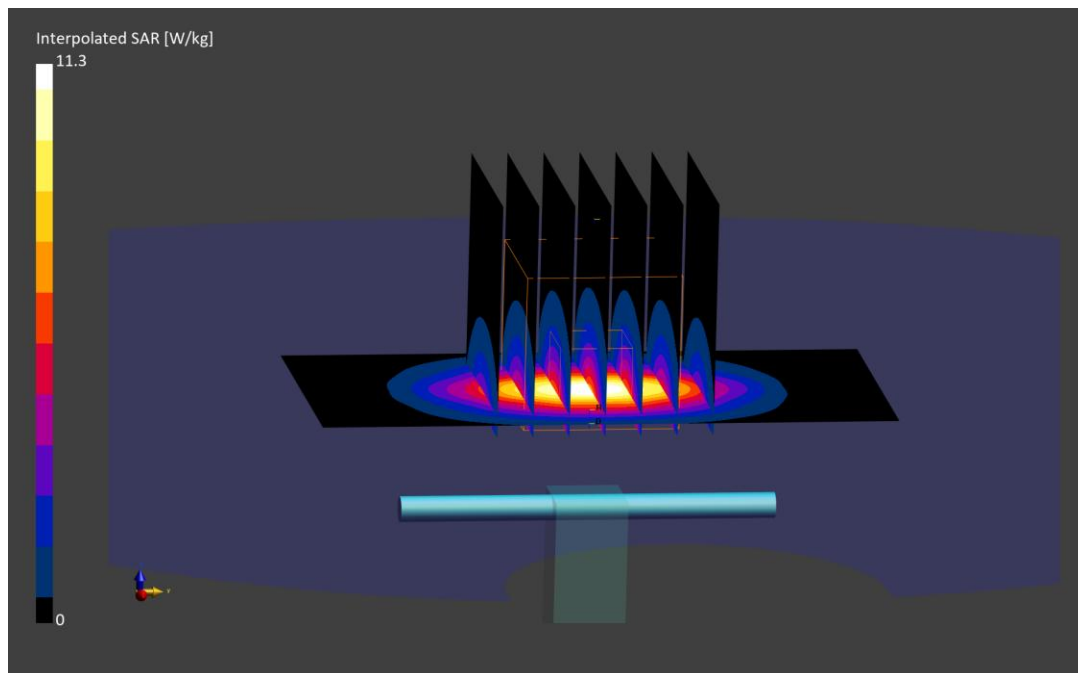

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5250.0$ MHz; $\text{cond} = 4.50$ S/m; $\text{perm} = 36.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/14/2026; Ambient Temp: 19.0°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(5.25,5.33,5.09); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.8 W/kg

SAR(1 g) = 3.73 W/kg; SAR(10 g) = 1.10 W/kg

Deviation (1 g) = -6.98%; Deviation (10 g) = -3.93%

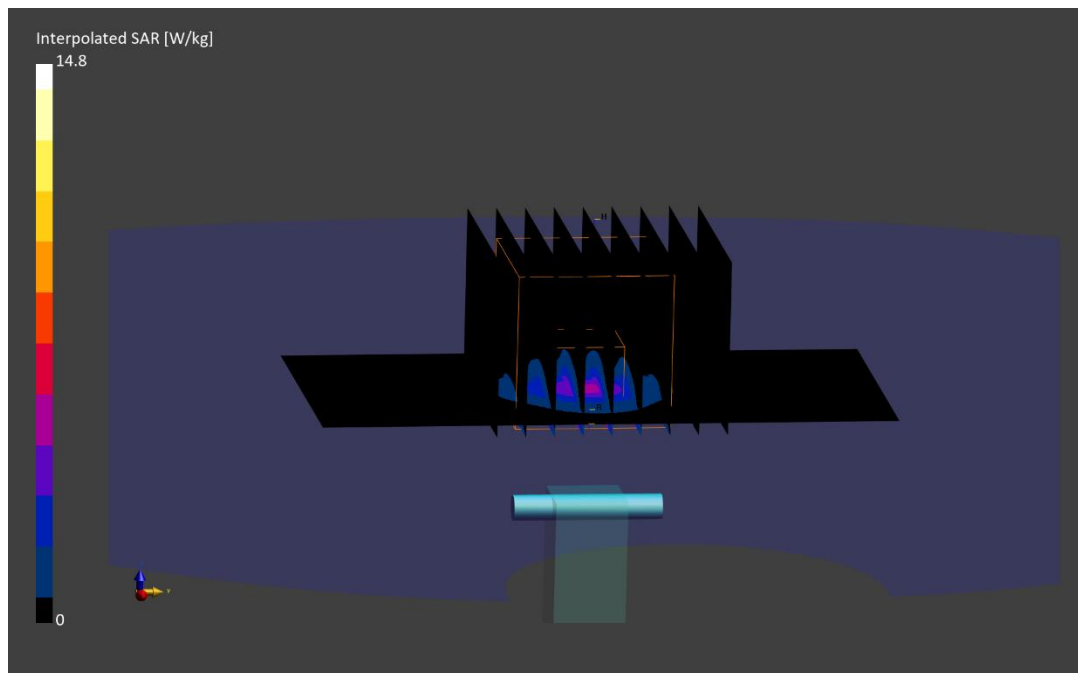

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5250.0$ MHz; $\text{cond} = 4.53$ S/m; $\text{perm} = 35.7$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2026; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(5.25,5.33,5.09); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.9 W/kg

SAR(1 g) = 3.73 W/kg; SAR(10 g) = 1.10 W/kg

Deviation (1 g) = -6.98%; Deviation (10 g) = -3.93%

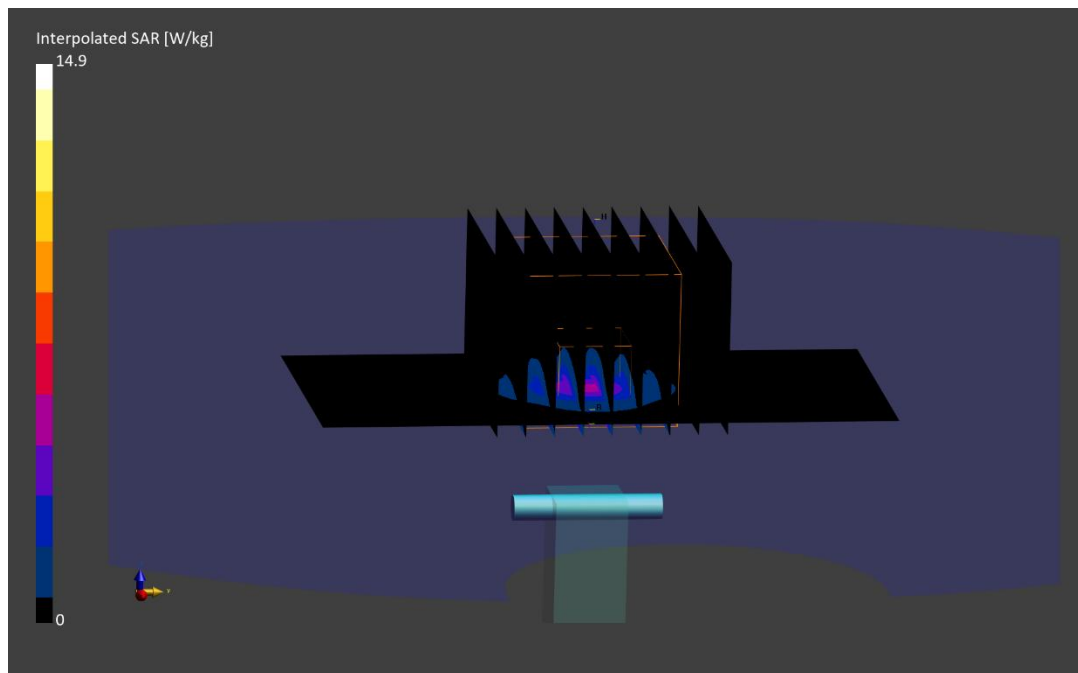

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5250.0$ MHz; $\text{cond} = 4.51$ S/m; $\text{perm} = 35.1$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/22/2026; Ambient Temp: 22.0°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7490; ConvF:(5.24,5.35,5.52); Calibrated: 2025-12-23
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2025-12-03
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.6 W/kg

SAR(1 g) = 3.93 W/kg; SAR(10 g) = 1.13 W/kg

Deviation (1 g) = 0.90%; Deviation (10 g) = 0.44%

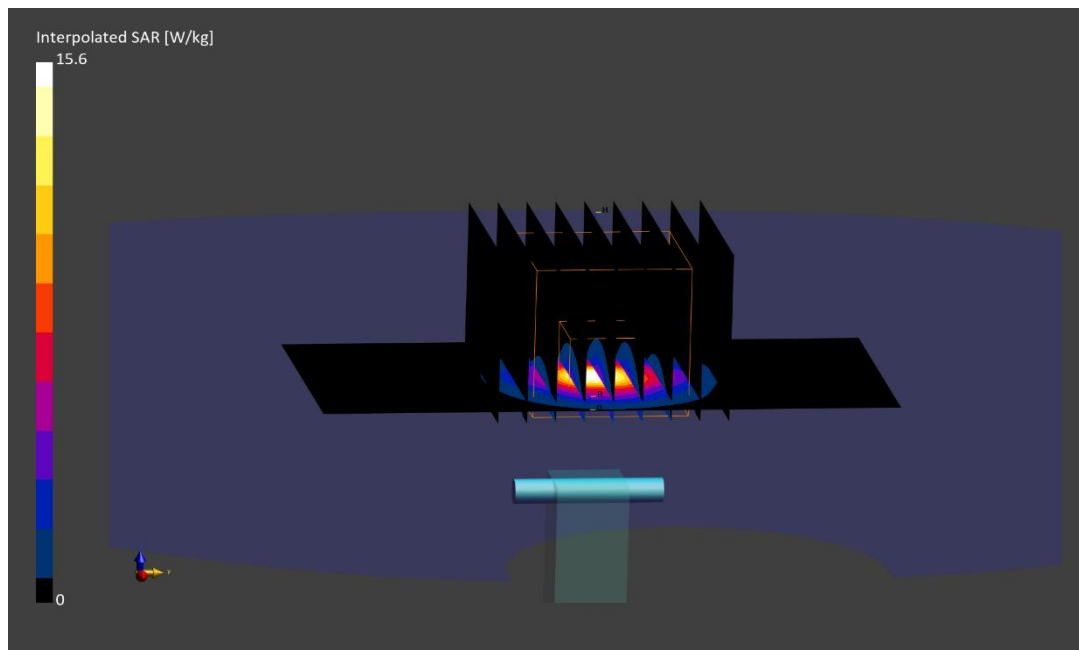

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.89 S/m; perm = 35.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/14/2026; Ambient Temp: 19.0°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.85,4.92,4.7); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.3 W/kg

SAR(1 g) = 3.86 W/kg; SAR(10 g) = 1.13 W/kg

Deviation (1 g) = -5.97%; Deviation (10 g) = -3.83%

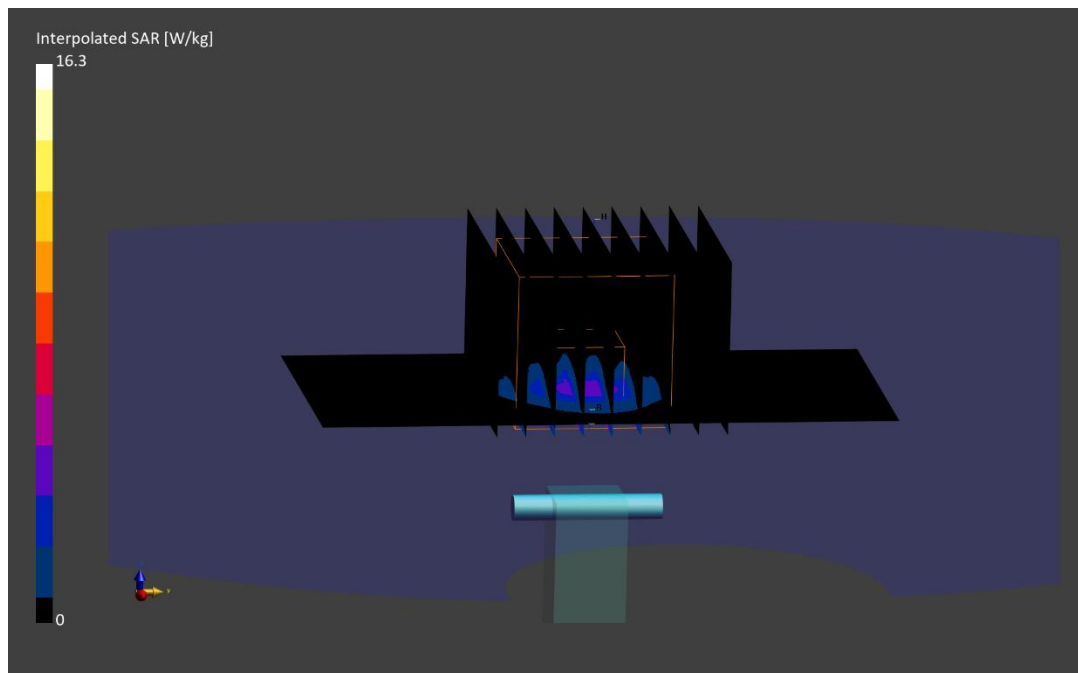

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.92 S/m; perm = 35.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2026; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.85,4.92,4.7); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.5 W/kg

SAR(1 g) = 4.06 W/kg; SAR(10 g) = 1.19 W/kg

Deviation (1 g) = -1.10%; Deviation (10 g) = 1.28%

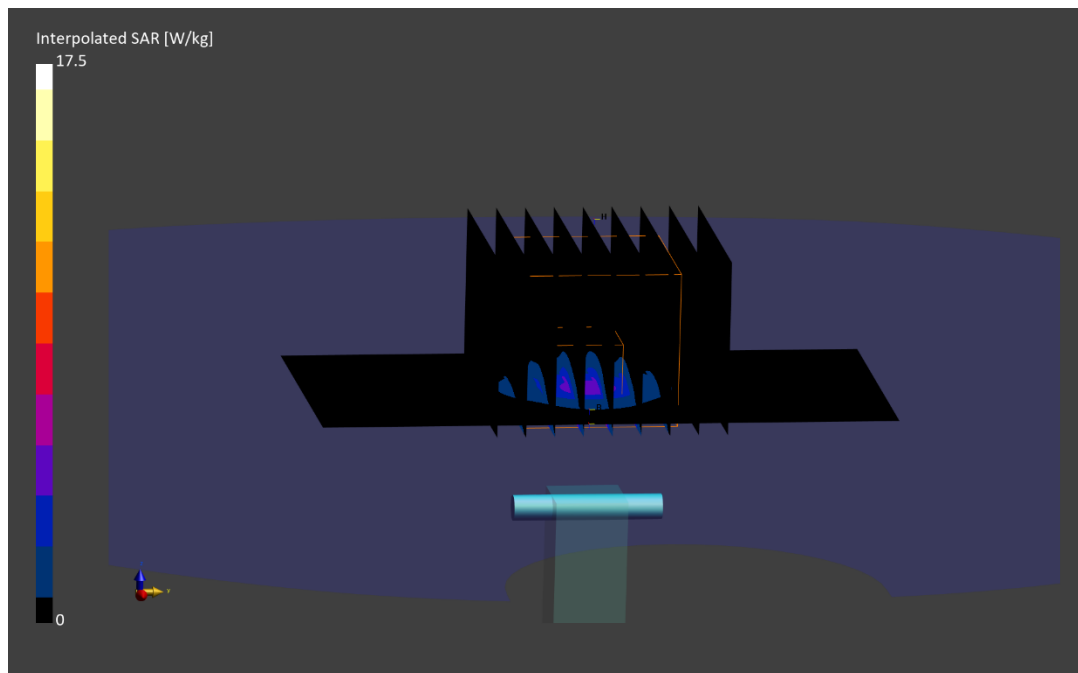

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5600.0$ MHz; $\text{cond} = 4.91$ S/m; $\text{perm} = 34.4$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/22/2026; Ambient Temp: 22.0°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7490; ConvF:(4.77,4.87,5.03); Calibrated: 2025-12-23
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2025-12-03
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.4 W/kg

SAR(1 g) = 4.07 W/kg; SAR(10 g) = 1.16 W/kg

Deviation (1 g) = -0.49%; Deviation (10 g) = -2.11%

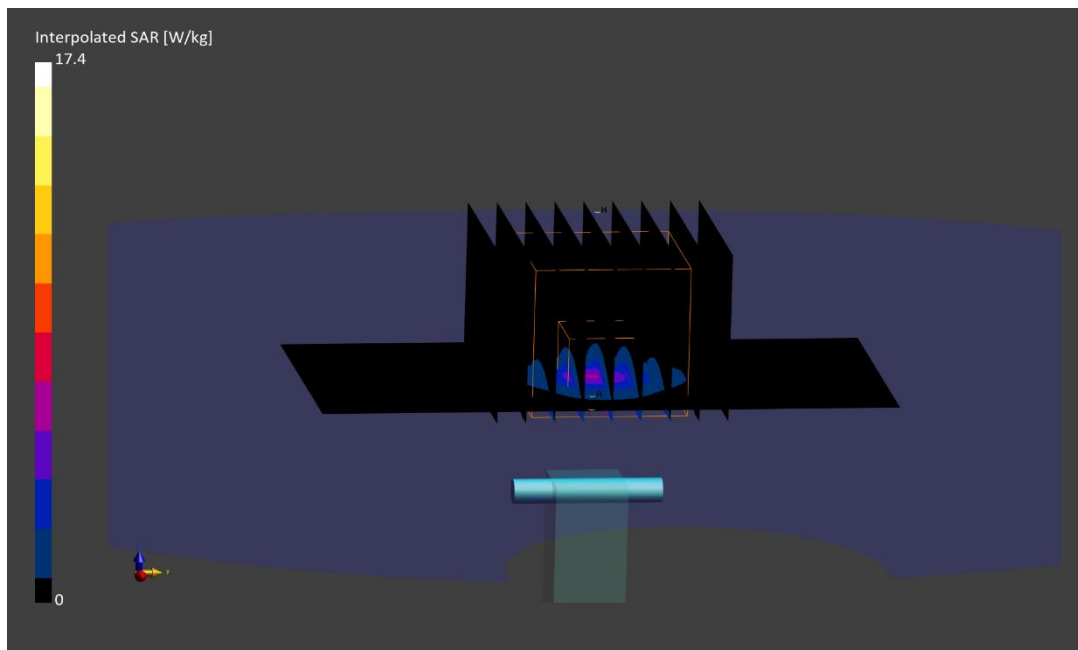

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5750.0$ MHz; $\text{cond} = 5.05$ S/m; $\text{perm} = 35.1$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/14/2026; Ambient Temp: 19.0°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.84,4.91,4.69); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.1 W/kg

SAR(1 g) = 3.69 W/kg; SAR(10 g) = 1.09 W/kg

Deviation (1 g) = -5.99%; Deviation (10 g) = -2.24%

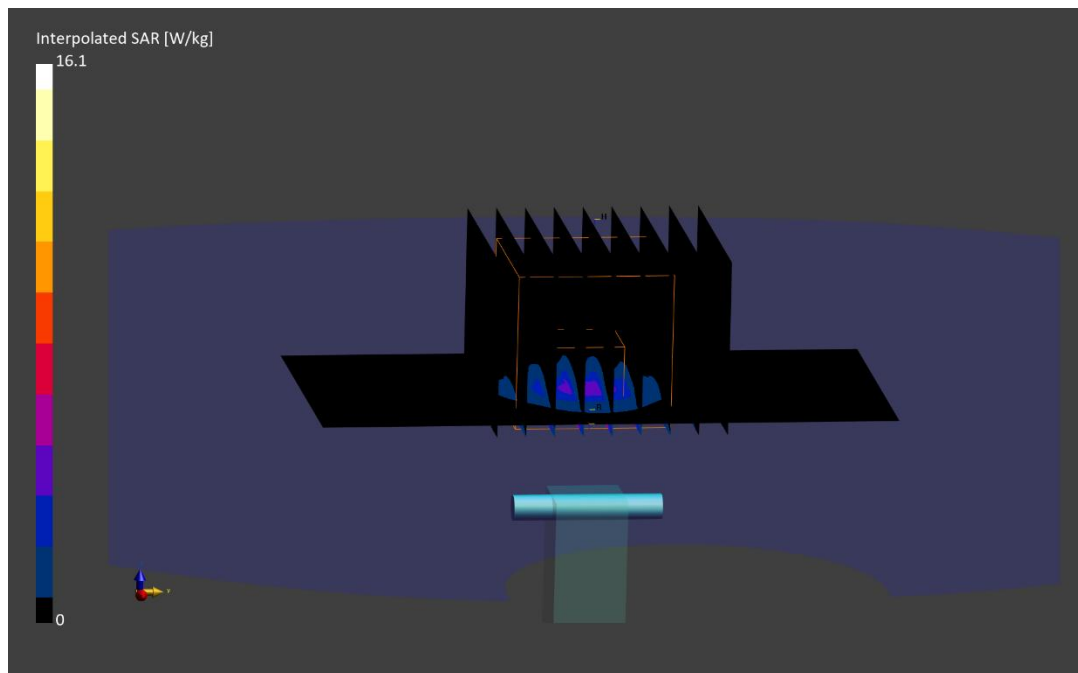

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5750.0$ MHz; $\text{cond} = 5.09$ S/m; $\text{perm} = 34.8$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2026; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.84,4.91,4.69); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.5 W/kg

SAR(1 g) = 3.97 W/kg; SAR(10 g) = 1.18 W/kg

Deviation (1 g) = 1.15%; Deviation (10 g) = 5.83%

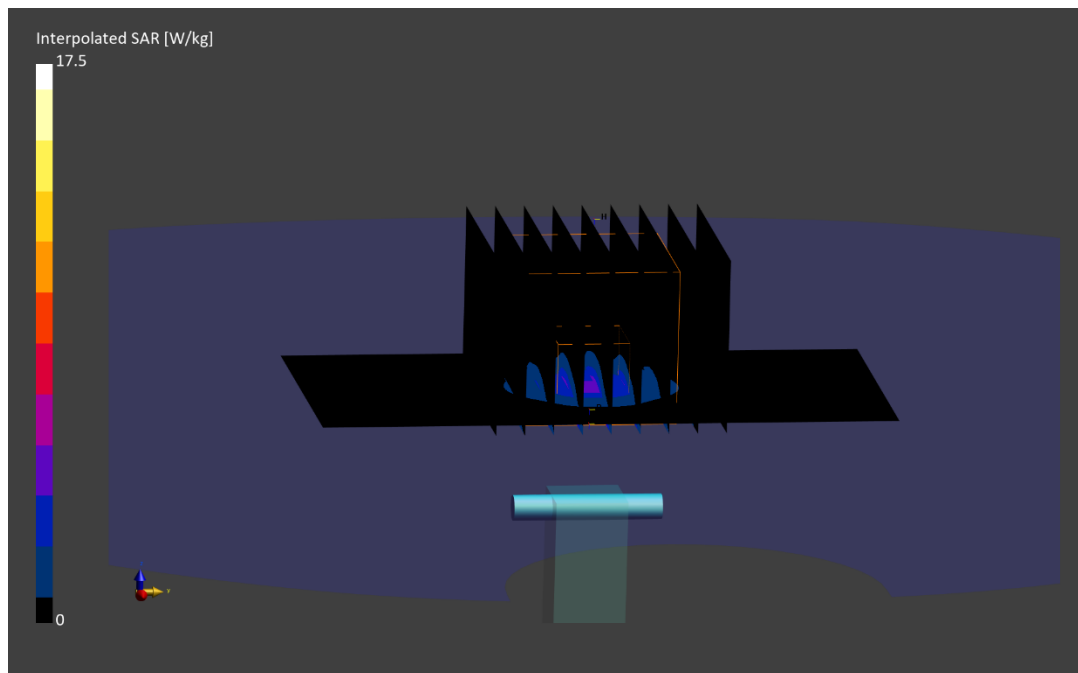

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5750.0$ MHz; $\text{cond} = 5.07$ S/m; $\text{perm} = 34.1$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/22/2026; Ambient Temp: 22.0°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7490; ConvF:(4.92,5.02,5.19); Calibrated: 2025-12-23
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2025-12-03
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 4.13 W/kg; SAR(10 g) = 1.18 W/kg

Deviation (1 g) = 2.35%; Deviation (10 g) = 1.72%

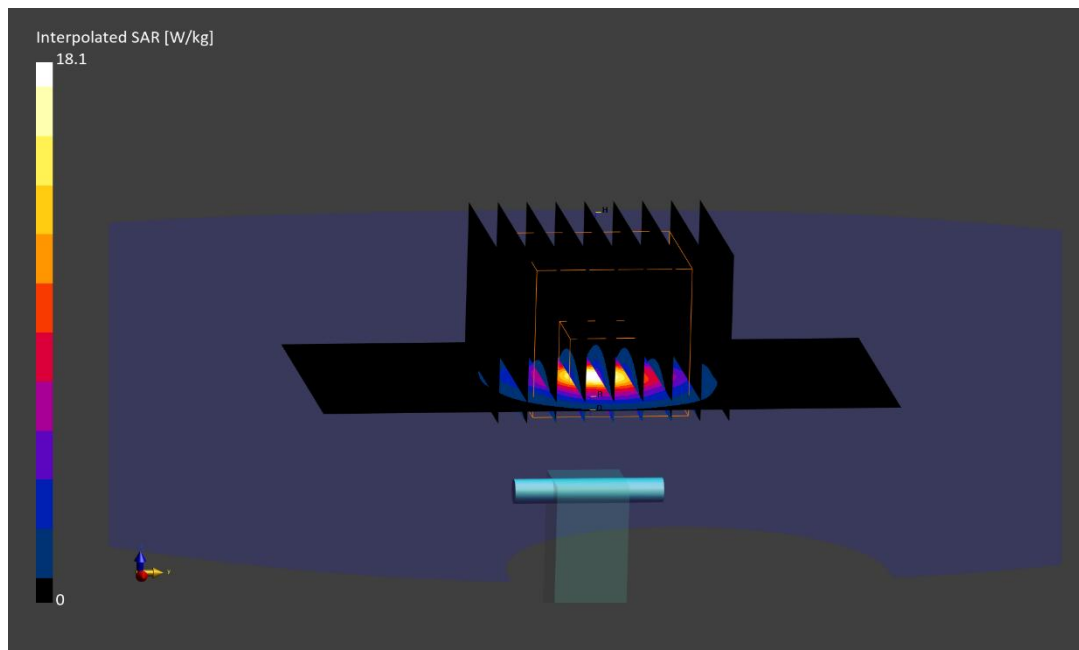

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5850.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5850.0$ MHz; $\text{cond} = 5.17$ S/m; $\text{perm} = 34.9$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/14/2026; Ambient Temp: 19.0°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.67,4.74,4.52); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 3.82 W/kg; SAR(10 g) = 1.11 W/kg

Deviation (1 g) = -7.17%; Deviation (10 g) = -5.13%

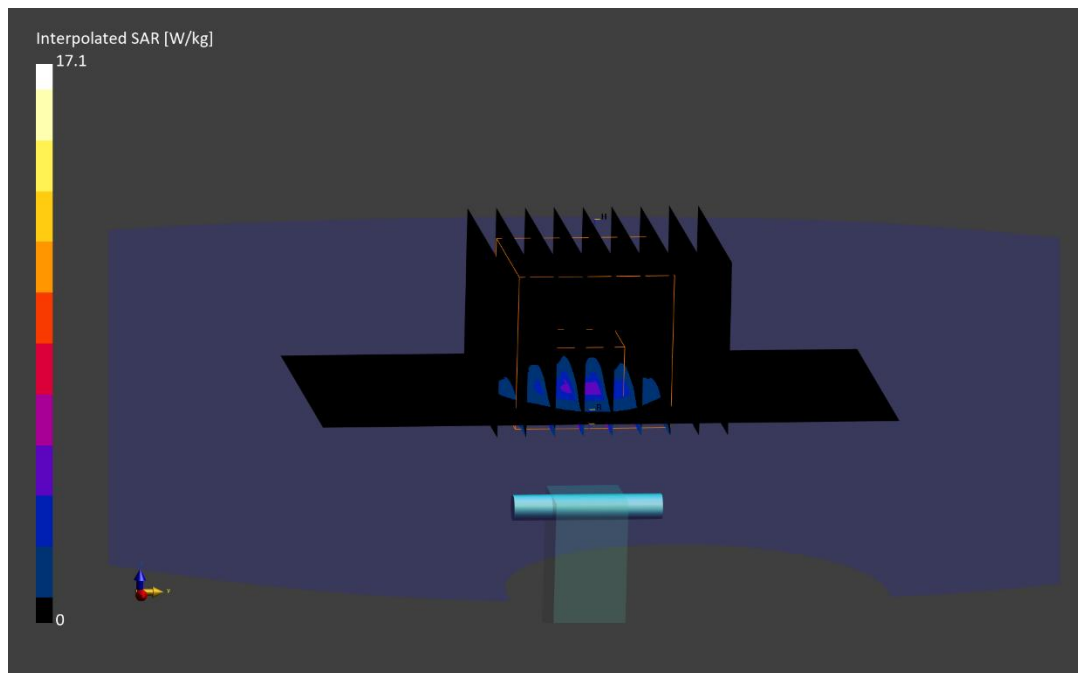

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5850.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5850.0 MHz; cond = 5.20 S/m; perm = 34.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2026; Ambient Temp: 19.1°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.67,4.74,4.52); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 4.01 W/kg; SAR(10 g) = 1.16 W/kg

Deviation (1 g) = -2.55%; Deviation (10 g) = -0.85%

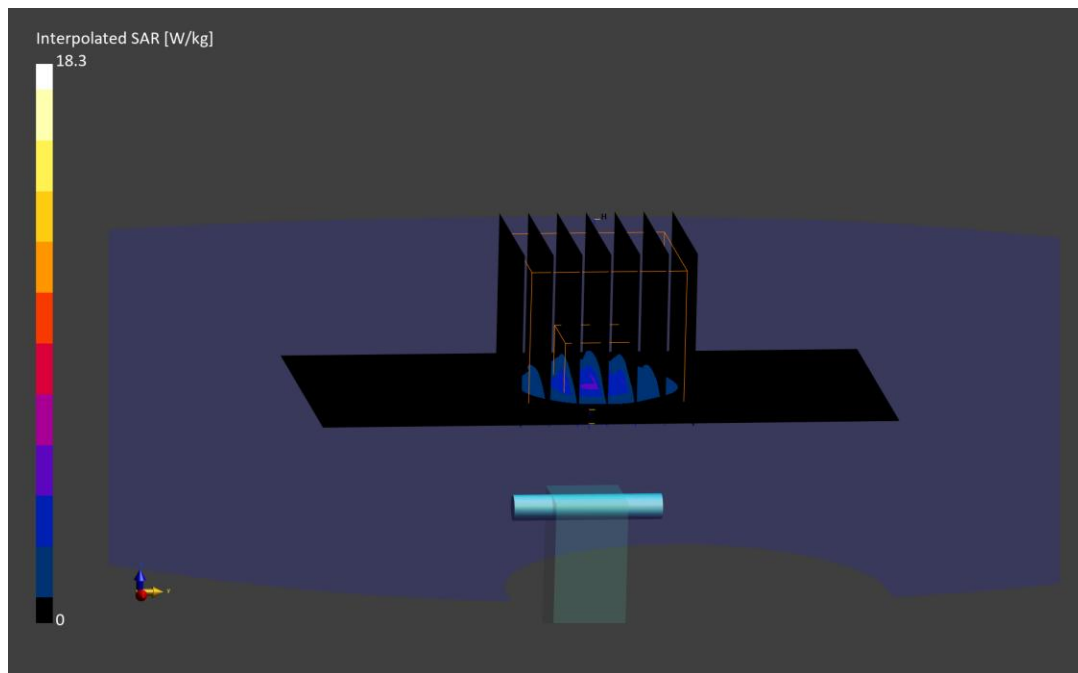

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5850.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5850.0$ MHz; $\text{cond} = 5.19$ S/m; $\text{perm} = 33.9$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 06/22/2026; Ambient Temp: 22.0°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7490; ConvF:(4.69,4.79,4.95); Calibrated: 2025-12-23

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1644; Calibrated: 2025-12-03

Phantom: Twin-SAM V8.0; Serial: 2070

Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.5 W/kg

SAR(1 g) = 4.13 W/kg; SAR(10 g) = 1.17 W/kg

Deviation (1 g) = 6.72%; Deviation (10 g) = 5.41%

