

APPENDIX A: VERIFICATION PLOTS

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1057

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 600 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.867 S/m; perm = 41.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/15/2024; Ambient Temp: 22.6°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7682; ConvF:(11.36,11.36,11.36); 2023-05-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1683; 2023-05-11
Phantom: Twin-SAM V4.0; Serial: 1598
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.68 W/kg

SAR(1 g) = 1.68 W/kg; SAR(10 g) = 1.10 W/kg

Deviation (1 g) = -1.29%

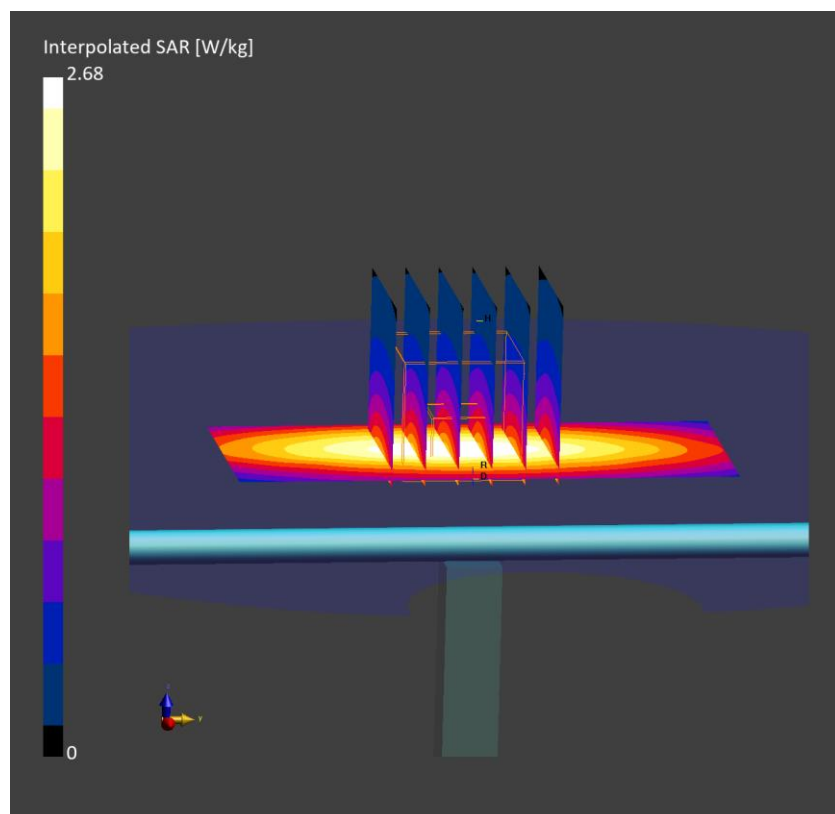

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1034

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.899 S/m; perm = 42.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 02/14/2024; Ambient Temp: 21.5°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7782; ConvF:(9.26,9.26,9.26); 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.63 W/kg

SAR(1 g) = 1.64 W/kg; SAR(10 g) = 1.06 W/kg

Deviation (1 g) = -5.09%

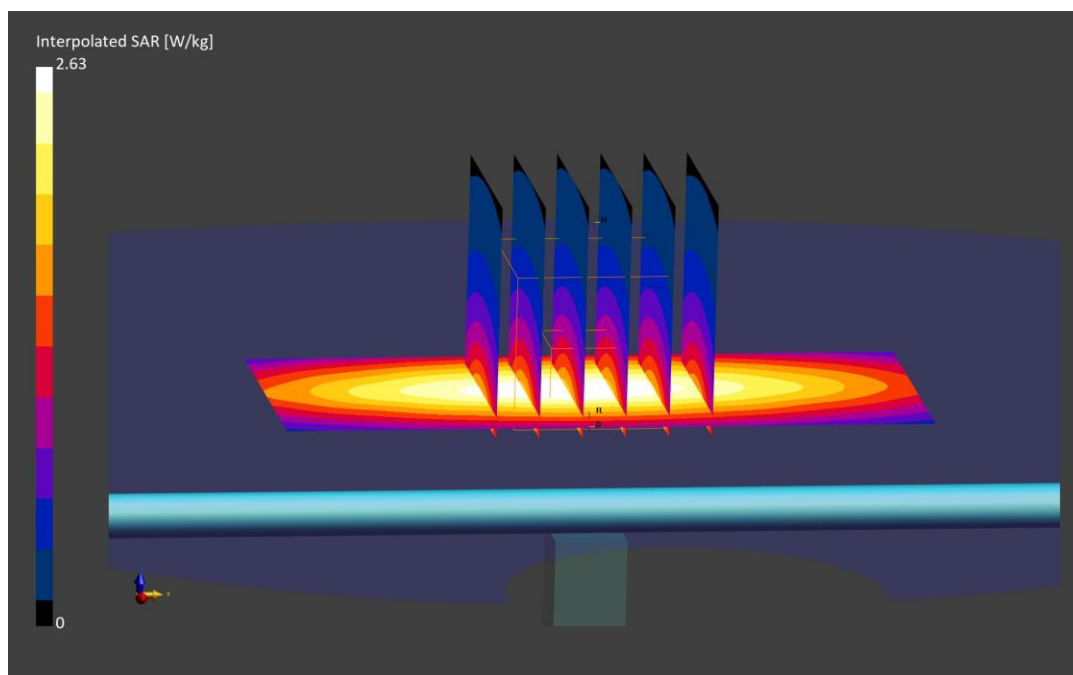

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN460

Communication System: UID: 0, CW; Frequency: 835.0 MHz

Medium: 600 Head; Medium parameters used:

f = 835.0 MHz; cond = 0.896 S/m; perm = 41.1; density = 1000 kg/m³

Phantom Section: Flat; Space: 15 mm

Test Date: 01/15/2024; Ambient Temp: 22.6°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7682; ConvF:(10.9,10.9,10.9); 2023-05-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1683; 2023-05-11

Phantom: Twin-SAM V4.0; Serial: 1598

Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.98 W/kg

SAR(1 g) = 1.84 W/kg; SAR(10 g) = 1.21 W/kg

Deviation (1 g) = -5.35%

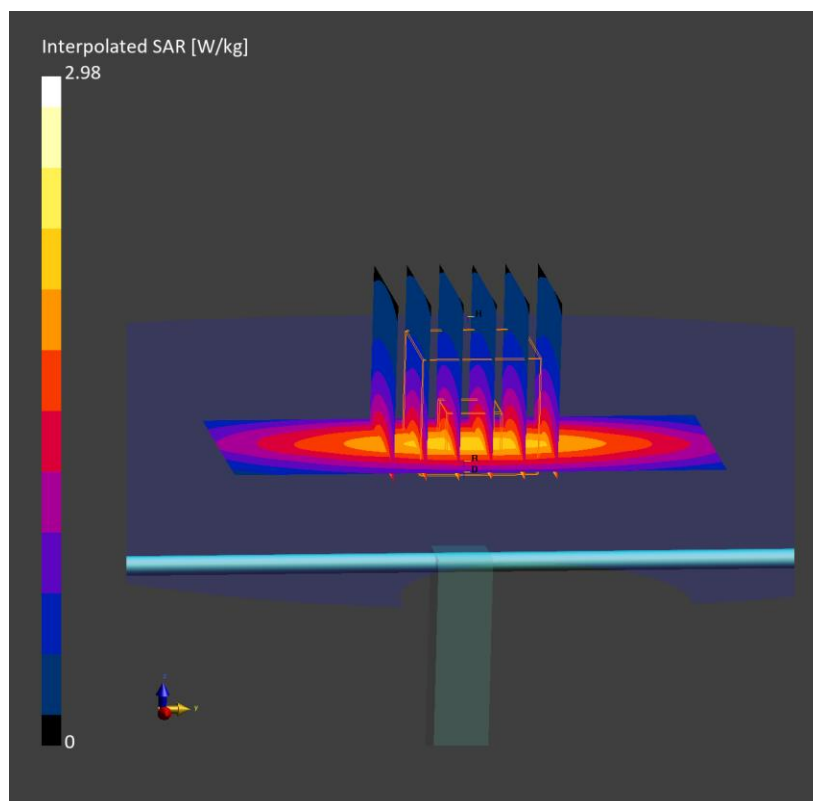

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d030

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 600 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.42 S/m; perm = 39.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/17/2024; Ambient Temp: 22.6°C; Tissue Temp: 22.7°C

Probe: EX3DV4 - SN7682; ConvF:(8.85,8.85,8.85); 2023-05-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1683; 2023-05-11
Phantom: Twin-SAM V4.0; Serial: 1598
Measurement SW: DASY Module SAR V16.2.0.1425

1900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.81 W/kg

SAR(1 g) = 3.77 W/kg; SAR(10 g) = 1.94 W/kg

Deviation (1 g) = -5.28%

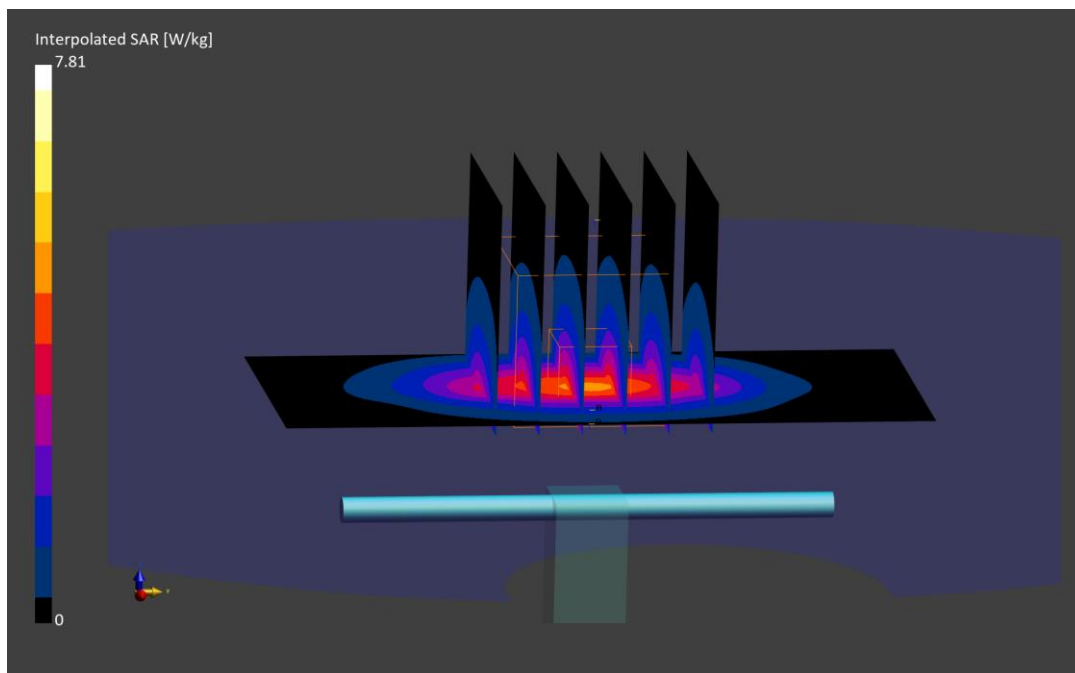

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 2.99 S/m; perm = 36.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/31/2024; Ambient Temp: 22.4°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7782; ConvF:(6.19,6.19,6.19); 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.3 W/kg

SAR(1 g) = 7.08 W/kg; SAR(10 g) = 2.61 W/kg

Deviation (1 g) = 5.67%

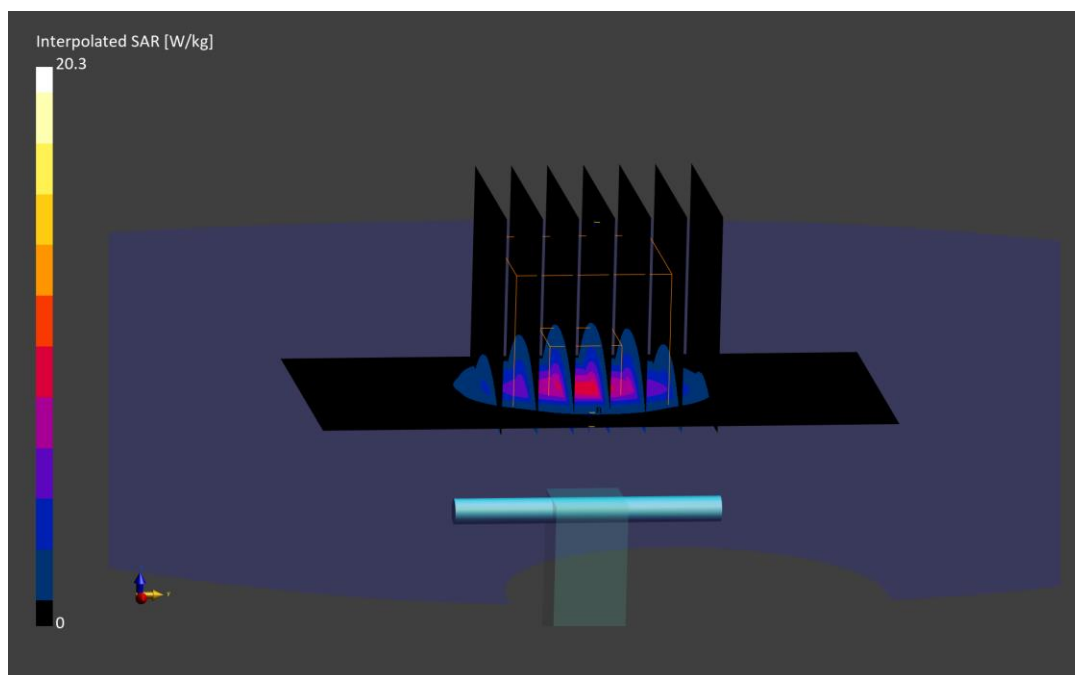

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.14 S/m; perm = 36.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/31/2024; Ambient Temp: 22.4°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 21.1 W/kg

SAR(1 g) = 7.13 W/kg; SAR(10 g) = 2.58 W/kg

Deviation (1 g) = 4.70%

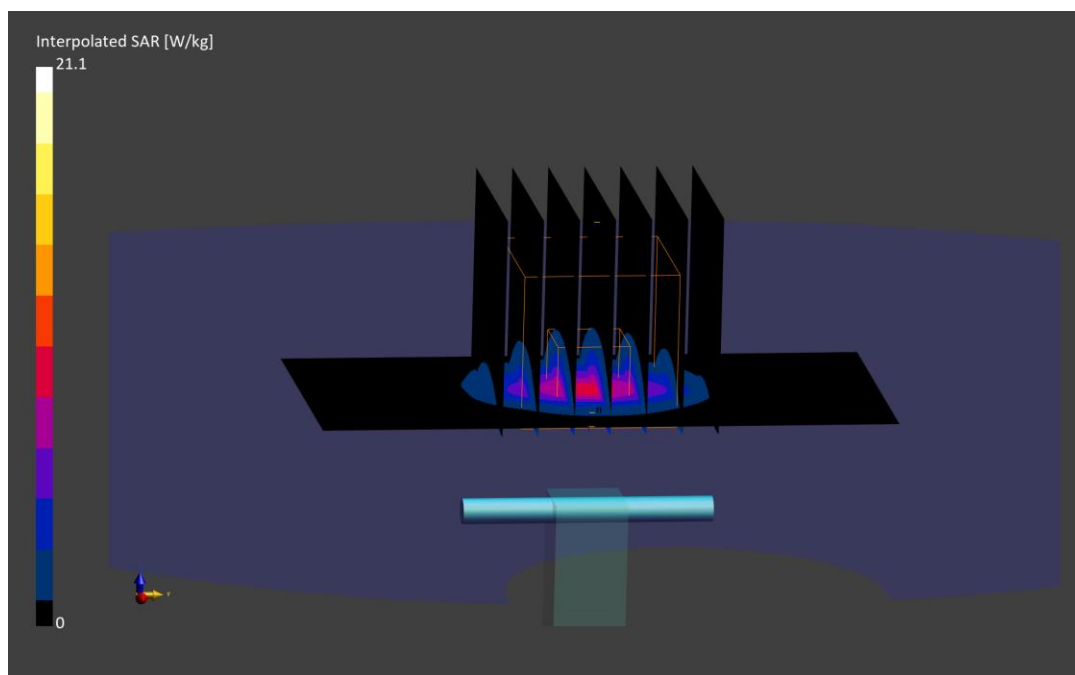

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.11 S/m; perm = 36.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 2/4/2024; Ambient Temp: 20.8°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 19.3 W/kg

SAR(1 g) = 6.56 W/kg; SAR(10 g) = 2.37 W/kg

Deviation (1 g) = -3.67%

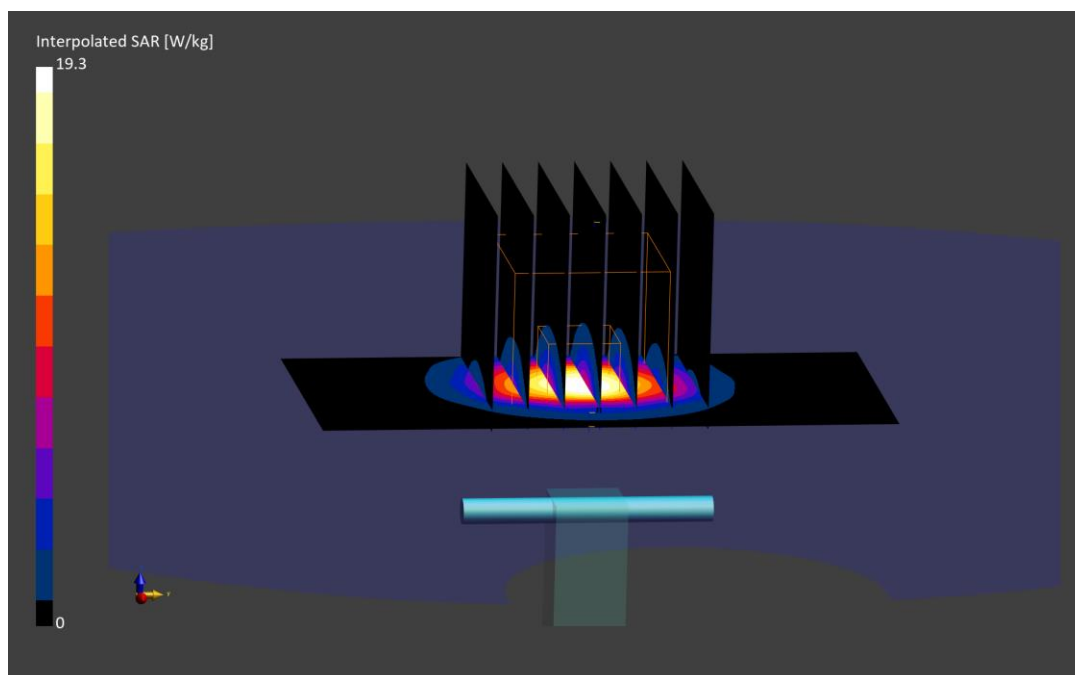

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1073

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.28 S/m; perm = 36.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 2/4/2024; Ambient Temp: 20.8°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7782; ConvF:(5.65,5.65,5.65); 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3900.0 MHz System Verification at 20.0 dBm (100 mW)

Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.1 W/kg

SAR(1 g) = 6.92 W/kg; SAR(10 g) = 2.40 W/kg

Deviation (1 g) = -0.72%

