

APPENDIX B: SYSTEM VERIFICATION

ELEMENT

DUT: Dipole 13.0 MHz; Type: CLA13 - SN1004

Communication System: UID: 0, CW; Frequency: 13.0 MHz
Medium: 30 Head; Medium parameters used:
 $f = 13.0$ MHz; $\text{cond} = 0.761$ S/m; $\text{perm} = 53.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 0 mm

Test Date: 12/15/2025; Ambient Temp: 23.0°C; Tissue Temp: 24.0°C

Probe: EX3DV4 - SN7782; ConvF:(18.49,15.42,16.82); Calibrated: 2025-09-15
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn1646; Calibrated: 2025-09-10
Phantom: ELI V6.0; Serial: 2003
Measurement SW: DASY Module SAR V16.4.0.5005

13.0 MHz System Verification at 30.0 dBm (1000 mW)


Area Scan (40.0 x 90.0): Measurement grid: $dx=10.0$ mm, $dy=15.0$ mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: $dx=6.0$ mm, $dy=6.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 1.20 W/kg

SAR(1 g) = 0.571 W/kg

Deviation (1 g) = -2.39%

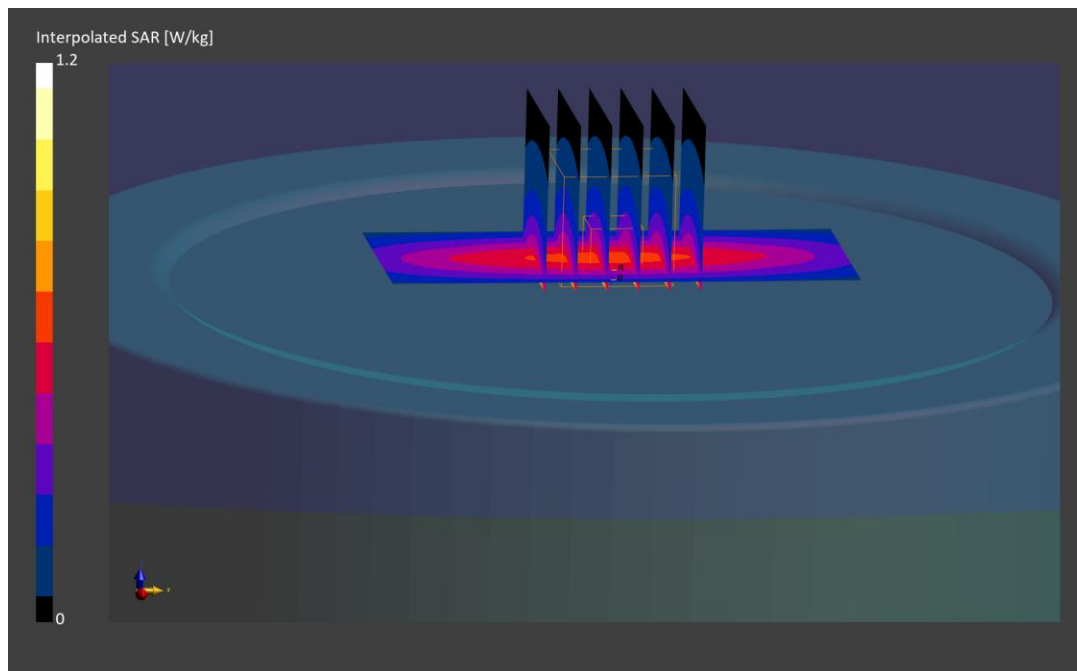

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.81 S/m; perm = 38.5; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 11/13/2025; Ambient Temp: 22.3°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7532; ConvF:(6.89,6.81,7.65); Calibrated: 2025-04-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn501; Calibrated: 2025-04-09

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.1 W/kg

SAR(1 g) = 5.18 W/kg

Deviation (1 g) = -2.81%

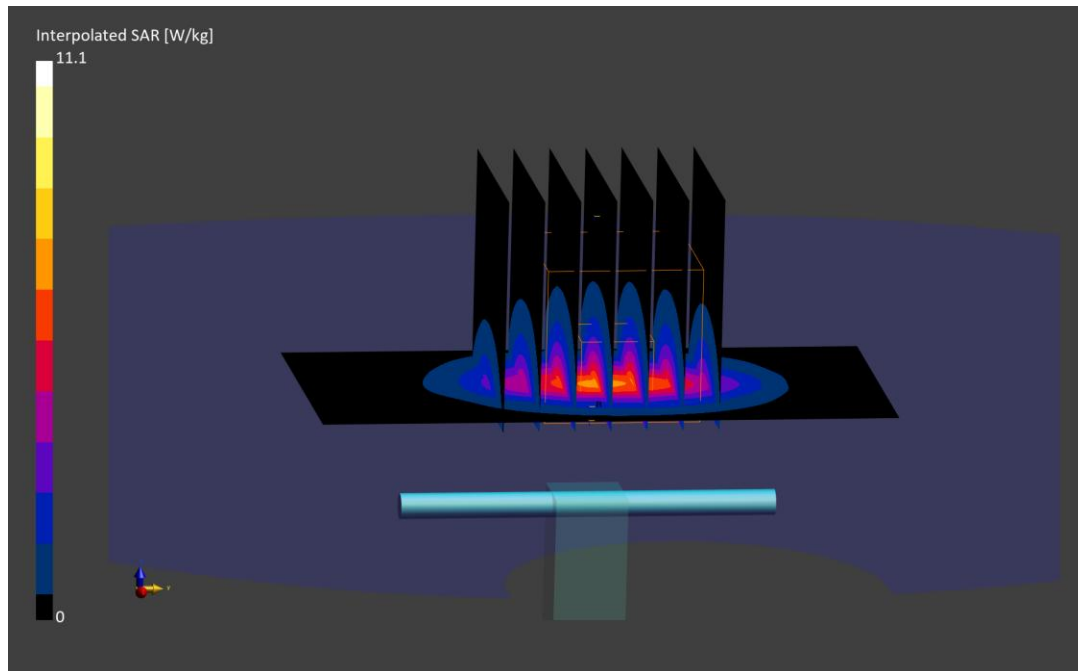

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.79 S/m; perm = 38.9; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 11/19/2025; Ambient Temp: 20.0°C; Tissue Temp: 23.4°C

Probe: EX3DV4 - SN7532; ConvF:(6.89,6.81,7.65); Calibrated: 2025-04-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn501; Calibrated: 2025-04-09

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.6 W/kg

SAR(1 g) = 5.20 W/kg

Deviation (1 g) = -2.44%

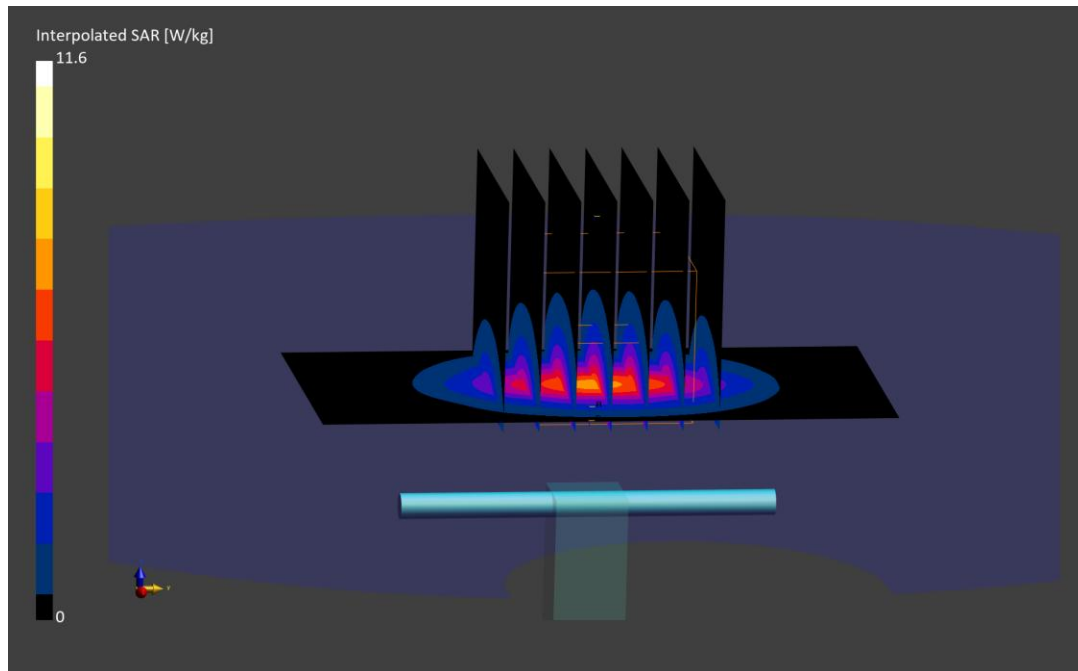

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.83 S/m; perm = 38.9; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 11/22/2025; Ambient Temp: 19.2°C; Tissue Temp: 22.7°C

Probe: EX3DV4 - SN7532; ConvF:(6.89,6.81,7.65); Calibrated: 2025-04-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn501; Calibrated: 2025-04-09

Phantom: Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.0 W/kg

SAR(1 g) = 5.39 W/kg

Deviation (1 g) = 1.13%

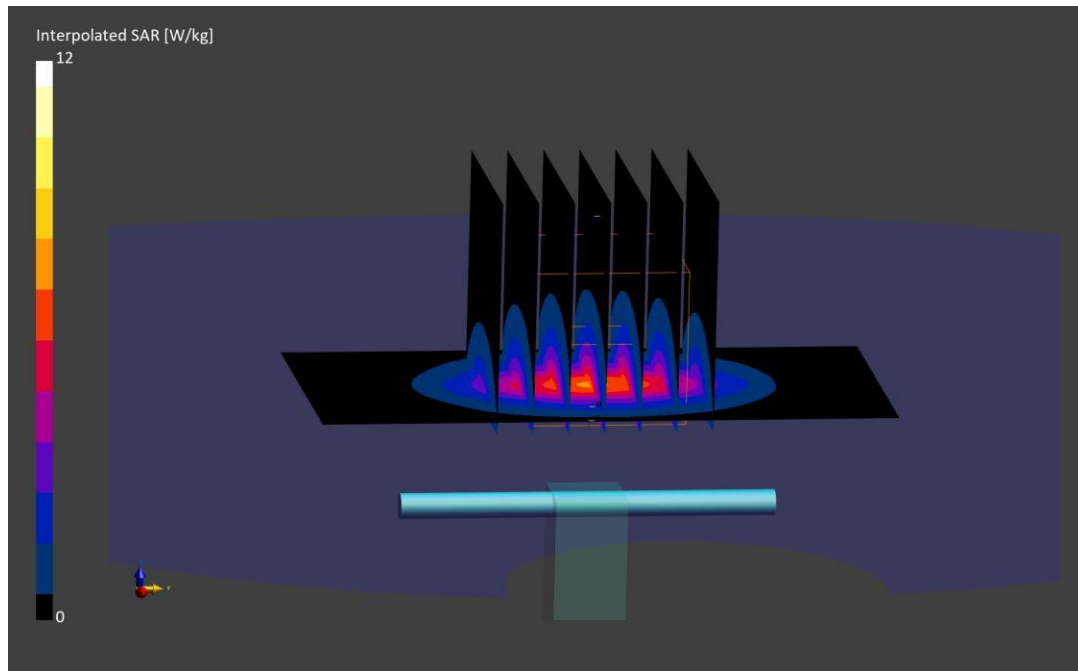

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5250.0 MHz; cond = 4.50 S/m; perm = 34.8; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 10/23/2025; Ambient Temp: 22.3°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(5.25,5.33,5.09); Calibrated: 2025-08-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2025-08-08

Phantom: Twin-SAM V8.0; Serial: 2027

Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.1 W/kg

SAR(1 g) = 4.02 W/kg

Deviation (1 g) = 2.03%

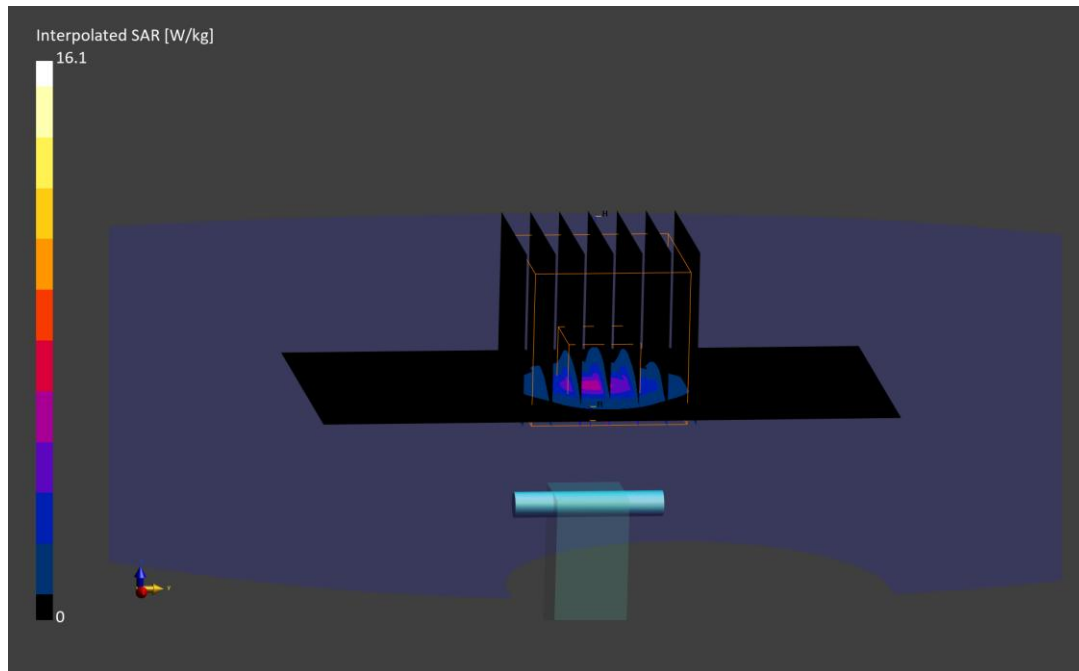

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5250.0 MHz; cond = 4.53 S/m; perm = 36.0; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 11/12/2025; Ambient Temp: 20.4°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7668; ConvF:(5.25,5.33,5.09); Calibrated: 2025-08-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2025-08-08

Phantom: Twin-SAM V8.0; Serial: 2027

Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.6 W/kg

SAR(1 g) = 3.87 W/kg

Deviation (1 g) = -1.78%

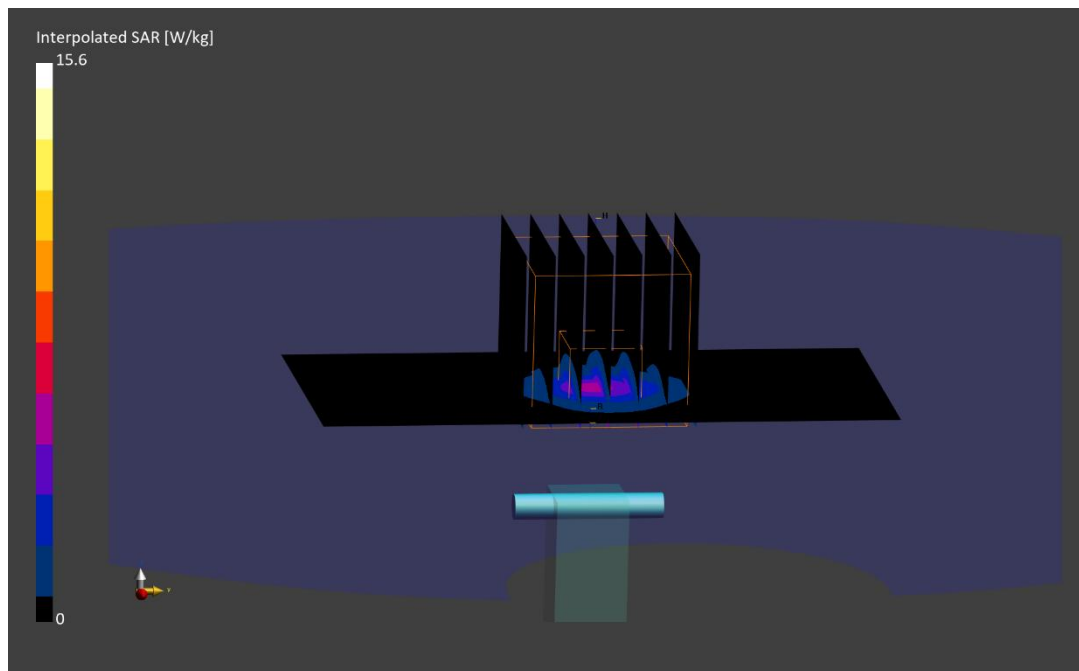

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5600.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5600.0 MHz; cond = 4.88 S/m; perm = 34.2; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 10/23/2025; Ambient Temp: 22.3°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.85,4.92,4.7); Calibrated: 2025-08-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2025-08-08

Phantom: Twin-SAM V8.0; Serial: 2027

Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 4.20 W/kg

Deviation (1 g) = 3.83%

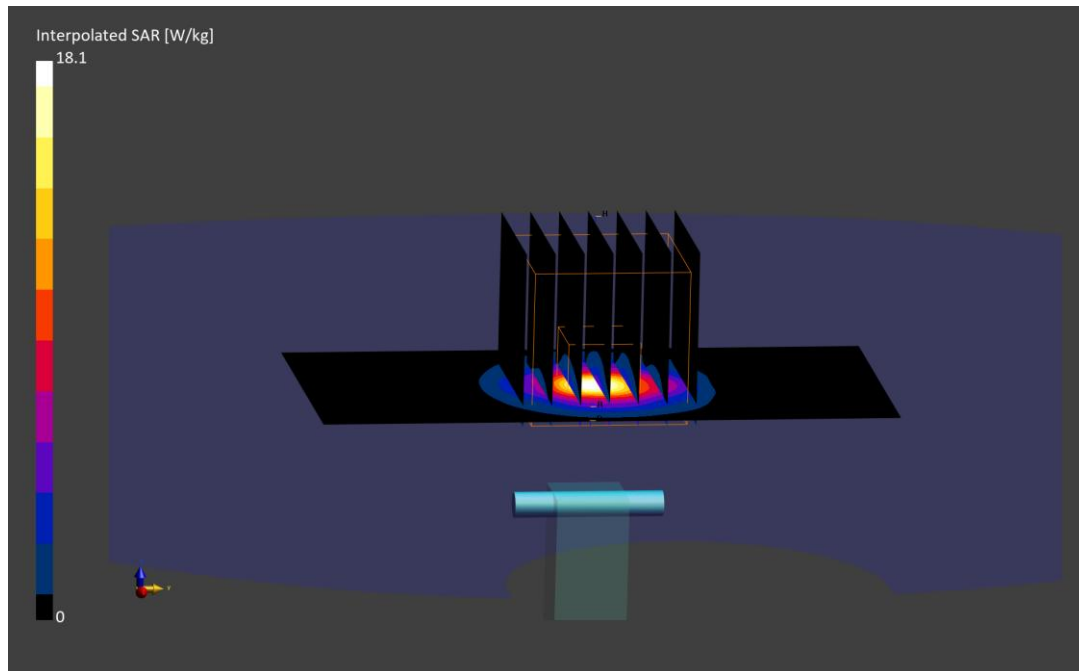

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.91 S/m; perm = 35.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 11/12/2025; Ambient Temp: 20.4°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7668; ConvF:(4.85,4.92,4.7); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.8 W/kg

SAR(1 g) = 4.03 W/kg

Deviation (1 g) = -0.37%

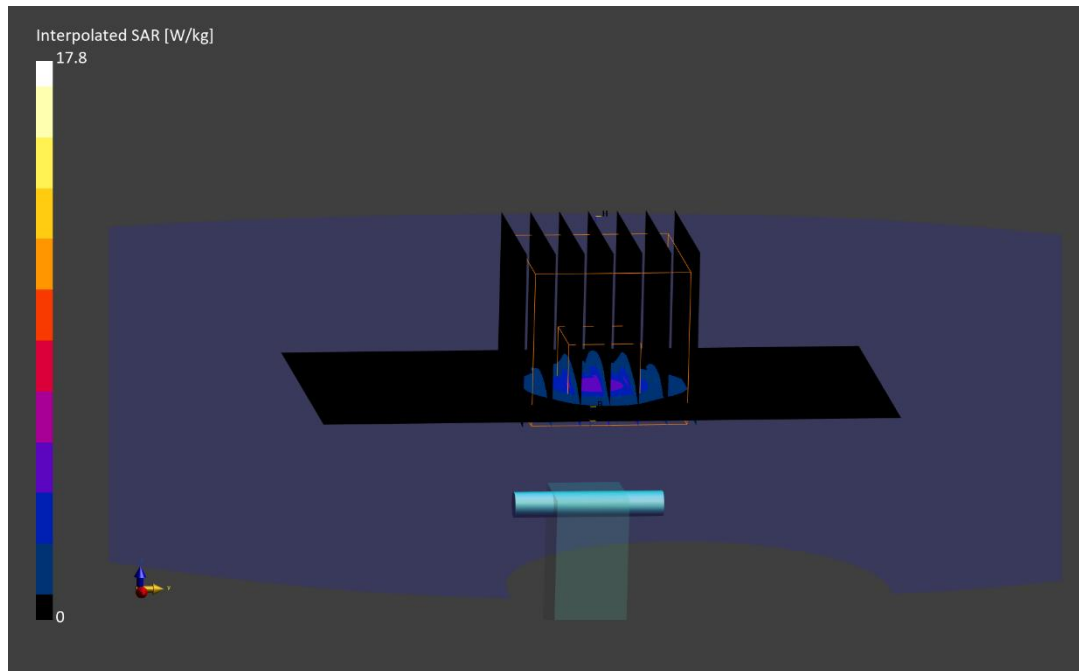

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5750.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5750.0$ MHz; $\text{cond} = 5.04$ S/m; $\text{perm} = 34.0$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 10/23/2025; Ambient Temp: 22.3°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.84,4.91,4.69); Calibrated: 2025-08-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2025-08-08

Phantom: Twin-SAM V8.0; Serial: 2027

Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.7 W/kg

SAR(1 g) = 3.77 W/kg

Deviation (1 g) = -3.46%

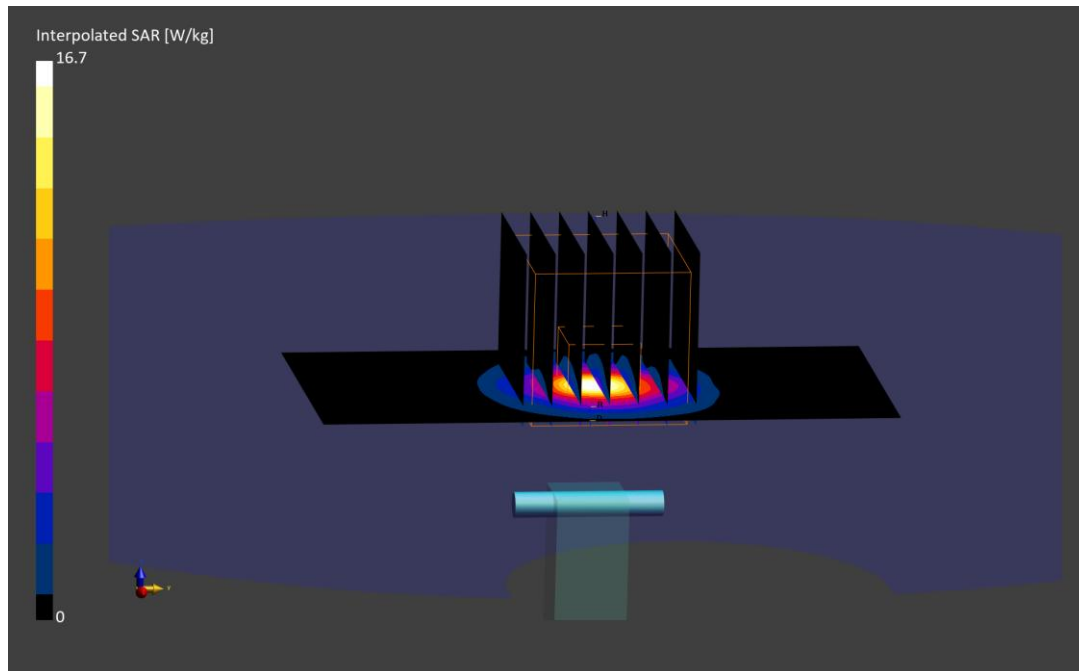

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.07 S/m; perm = 35.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 11/12/2025; Ambient Temp: 20.4°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7668; ConvF:(4.84,4.91,4.69); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.3 W/kg

SAR(1 g) = 3.79 W/kg

Deviation (1 g) = -2.94%

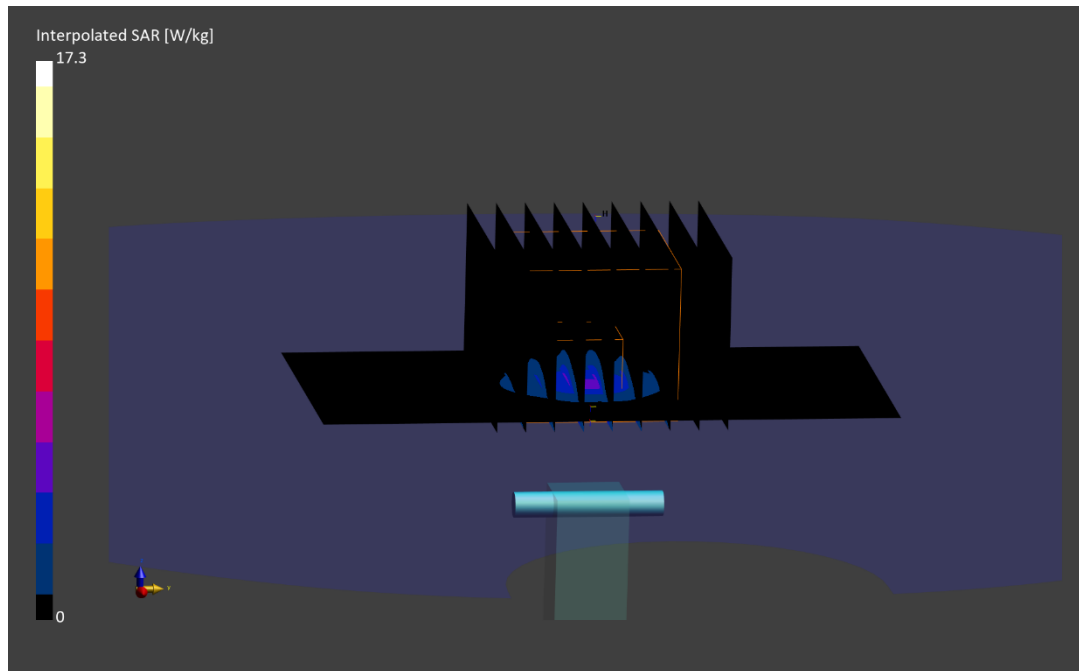

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5850.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5850.0 MHz; cond = 5.15 S/m; perm = 33.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 10/23/2025; Ambient Temp: 22.3°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.67,4.74,4.52); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.7 W/kg

SAR(1 g) = 3.69 W/kg

Deviation (1 g) = -7.52%

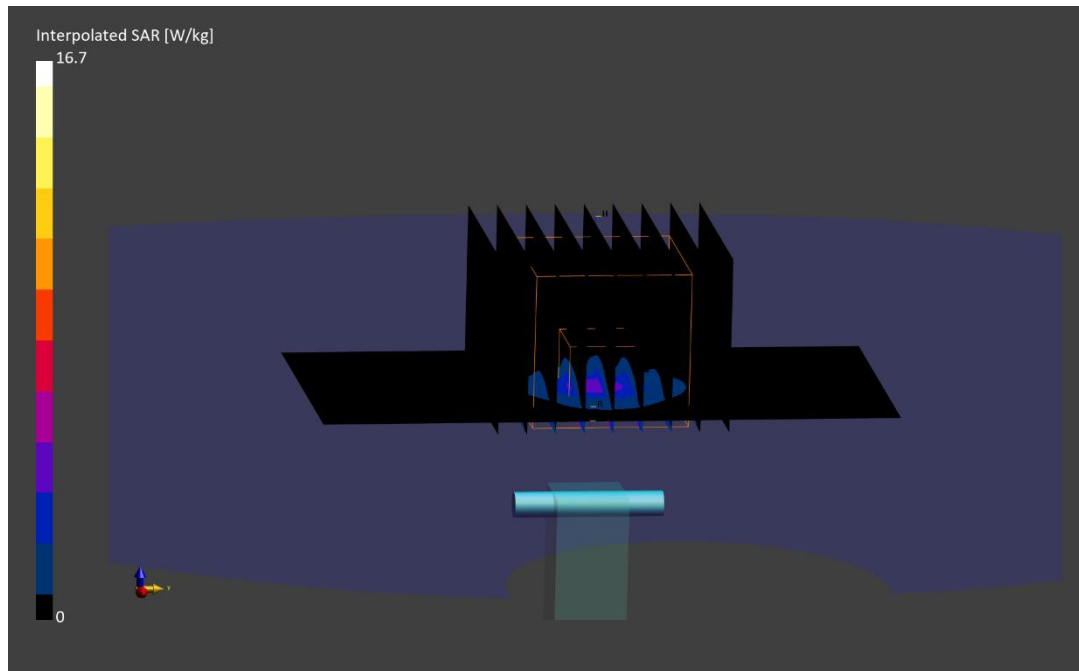

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5850.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5850.0 MHz; cond = 5.19 S/m; perm = 35.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm


Test Date: 11/12/2025; Ambient Temp: 20.4°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7668; ConvF:(4.67,4.74,4.52); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4
Peak SAR (extrapolated) = 17.3 W/kg
SAR(1 g) = 3.70 W/kg
Deviation (1 g) = -7.27%

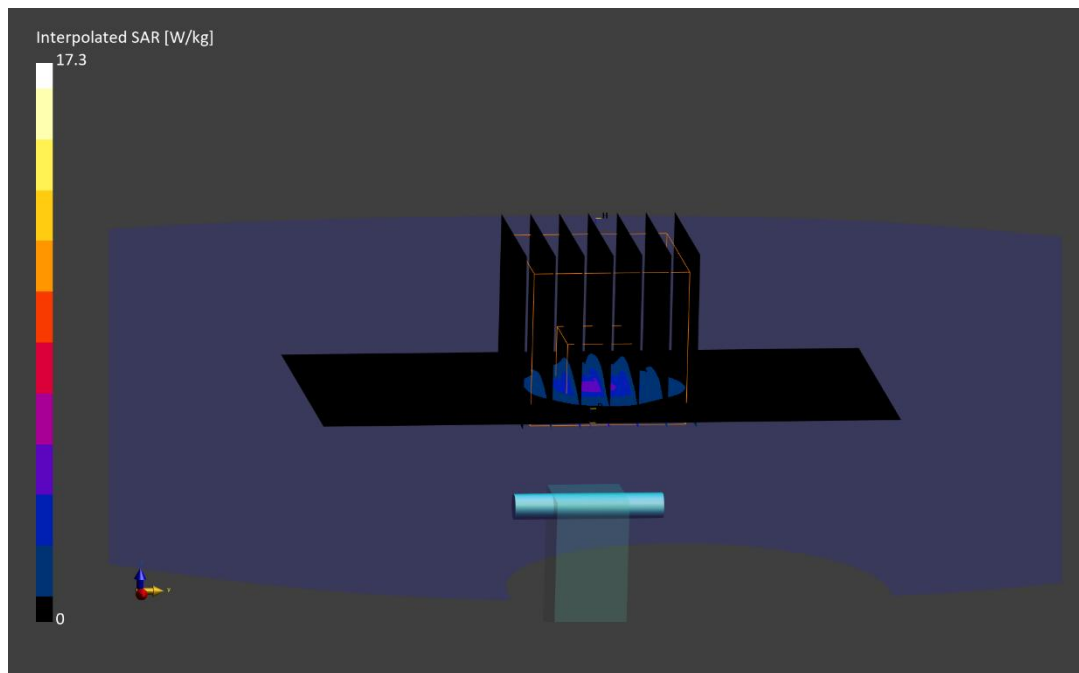

ELEMENT

DUT: Dipole 6500.0 MHz; Type: D6.5GHzV2 - SN1018

Communication System: UID: 0, CW; Frequency: 6500.0 MHz

Medium: 6000 Head; Medium parameters used:

$f = 6500.0$ MHz; $\text{cond} = 5.90$ S/m; $\text{perm} = 35.1$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 5 mm

Test Date: 10/27/2025; Ambient Temp: 22.5°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN3837; ConvF:(5.38,5.14,5.25); Calibrated: 2025-08-13

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn793; Calibrated: 2025-08-06

Phantom: Twin-SAM V4.0; Serial: 1275

Measurement SW: DASY Module SAR V16.4.0.5005

6500.0 MHz System Verification at 14.0 dBm (25 mW)


Area Scan (51.0 x 85.0): Measurement grid: $dx=8.5$ mm, $dy=8.5$ mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: $dx=3.4$ mm, $dy=3.4$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 43.9 W/kg

SAR(1 g) = 7.38 W/kg; APD(4cm²) = 33.0 W/m²

Deviation (1 g) = 1.10%; Deviation (W/m²) = 0.76%

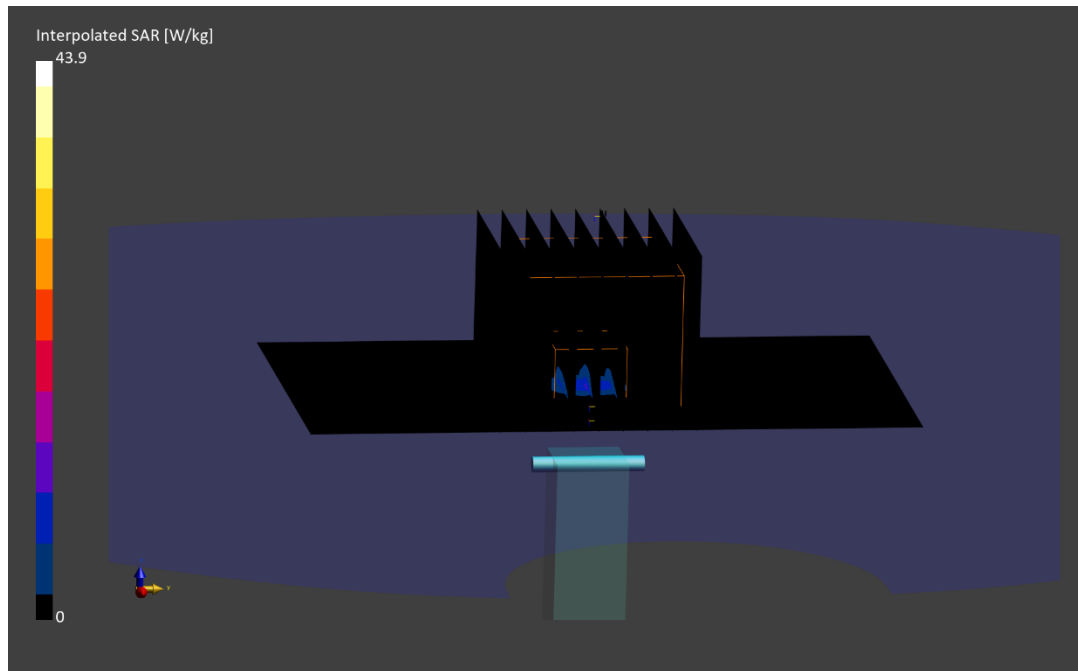

Date: 10/08/2025

10 GHz System Verification

Device Under Test Properties

DUT	Serial Number
10 GHz Verification Source	1004

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00	Validation band	10000.0

Hardware Setup

Probe, Calibration Date	DAE, Calibration Date
EUmmWV3 – SN9364, 06/11/2025	DAE4 – SN1402, 04/10/2025

Software Setup


Software	Software Version
cDASY6 Module mmWave	3.2.0.1840

Scans Setup


Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

Scan Type	5G Scan
Avg. Area [cm²]	4.00
pS _{tot} avg [W/m²]	61.4
pS _n avg [W/m²]	61.2
E _{peak} [V/m]	162
Deviation [dB] pS _{tot}	0.43
Deviation [dB] pS _n	0.50

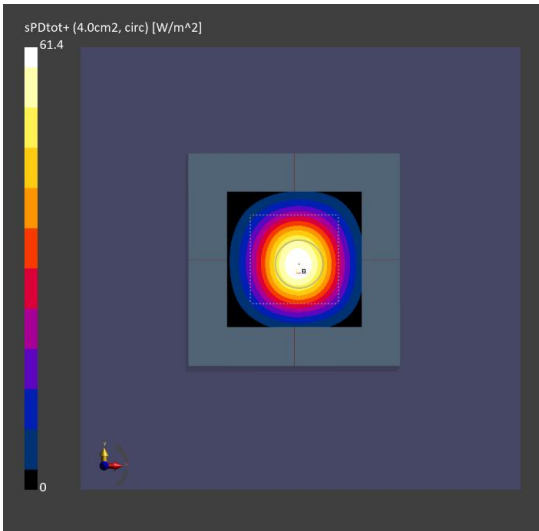

10 GHz System Verification

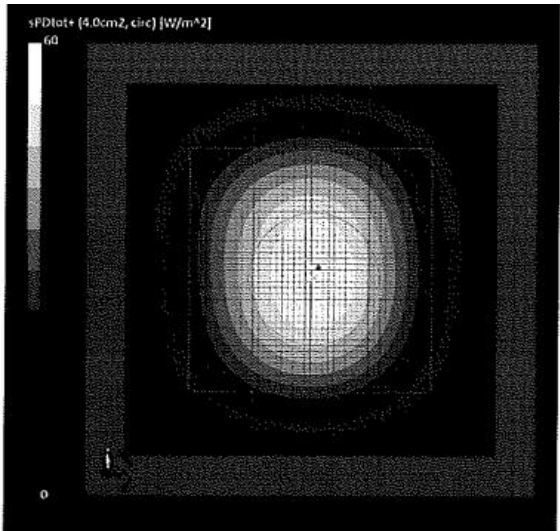

Calibration Certificate



Date: 12/15/2025

10 GHz Verification

Device Under Test Properties

DUT	Serial Number
10 GHz Verification Source	1004

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00	Validation band	10000.0

Hardware Setup

Probe, Calibration Date	DAE, Calibration Date
EUmmWV3 - SN9364, 06/11-2025	DAE4 - SN1402, 04/10/2025

Software Setup


Software	Software Version
cDASY6 Module mmWave	3.2.0.1840

Scans Setup


Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0

Measurement Results

Scan Type	5G Scan
Avg. Area [cm²]	4.00
pStot avg [W/m²]	55.4
pSn avg [W/m²]	55.3
Epeak [V/m]	155
Deviation [dB] pStot	-0.02
Deviation [dB] pSn	0.06

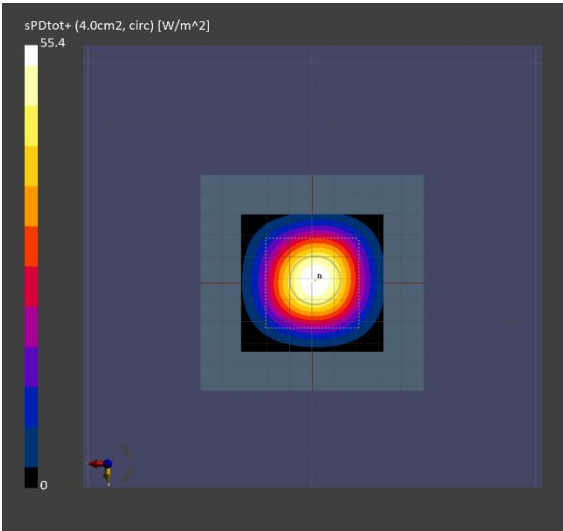

10 GHz System Verification

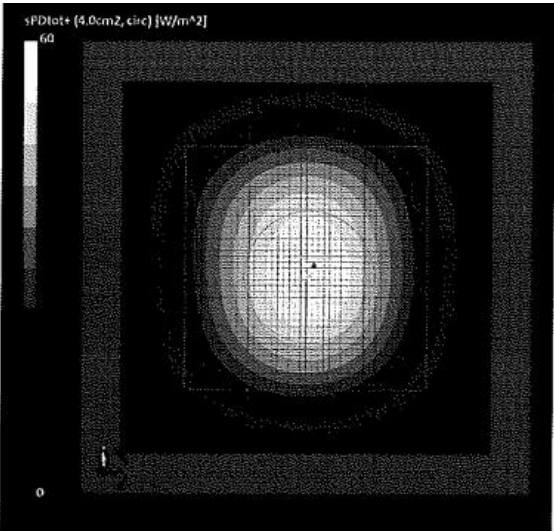

Calibration Certificate

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN855

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.81 S/m; perm = 38.7; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 12/29/2025; Ambient Temp: 21.0°C; Tissue Temp: 24.0°C

Probe: EX3DV4 - SN7532; ConvF:(6.89,6.81,7.65); Calibrated: 2025-04-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn501; Calibrated: 2025-04-09

Phantom: Twin-SAM V8.0; Twin-SAM V8.0; Serial: 2058

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.9 W/kg

SAR(1 g) = 5.35 W/kg

Deviation (1 g) = 0.38%

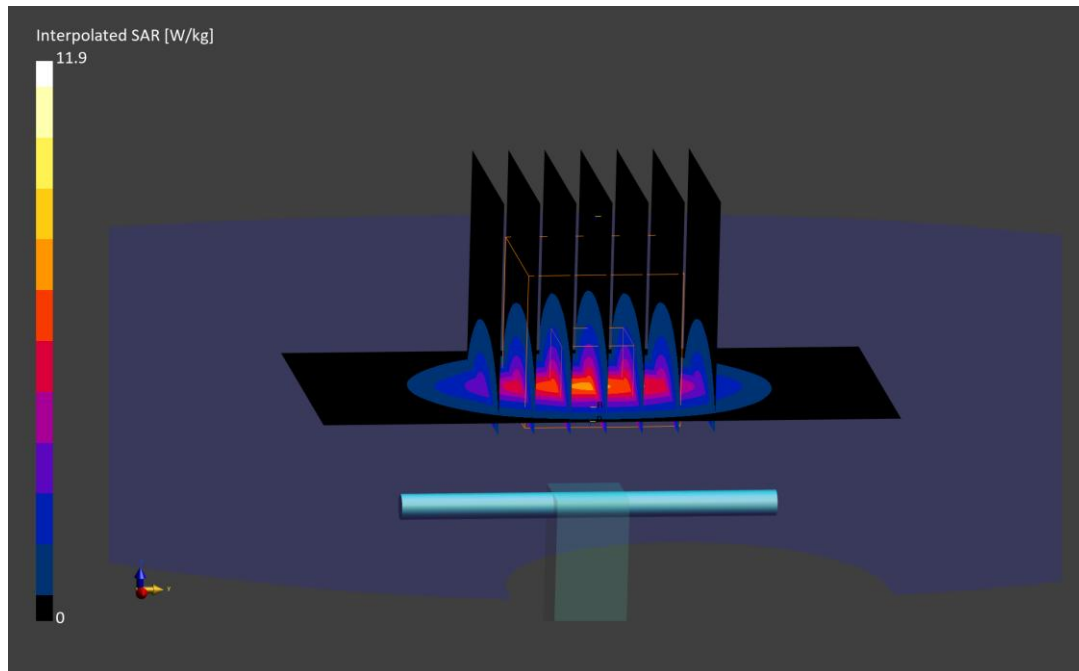

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5250.0 MHz; cond = 4.51 S/m; perm = 35.5; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 12/10/2025; Ambient Temp: 22.0°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7668; ConvF:(5.25,5.33,5.09); Calibrated: 2025-08-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2025-08-08

Phantom: Twin-SAM V8.0; Serial: 2027

Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.5 W/kg

SAR(1 g) = 4.20 W/kg

Deviation (1 g) = 6.60%

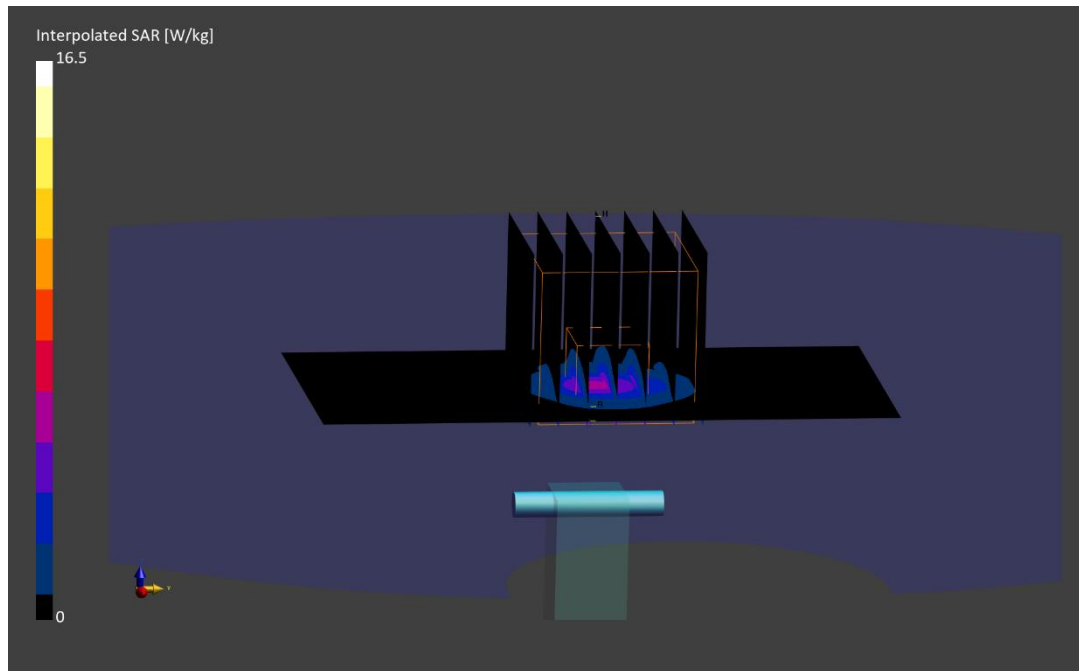

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5600.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5600.0 MHz; cond = 4.91 S/m; perm = 35.0; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 12/10/2025; Ambient Temp: 22.0°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.85,4.92,4.7); Calibrated: 2025-08-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2025-08-08

Phantom: Twin-SAM V8.0; Serial: 2027

Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.9 W/kg

SAR(1 g) = 4.33 W/kg

Deviation (1 g) = 7.05%

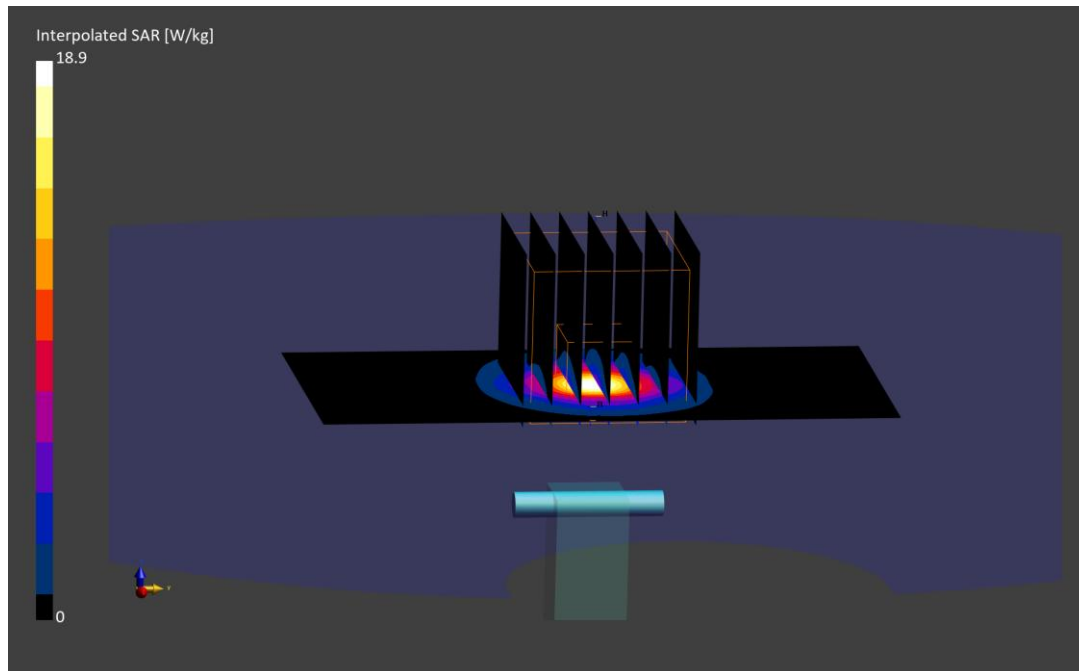

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.06 S/m; perm = 34.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm


Test Date: 12/10/2025; Ambient Temp: 22.0°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.84,4.91,4.69); Calibrated: 2025-08-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2025-08-08
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4
Peak SAR (extrapolated) = 16.6 W/kg
SAR(1 g) = 3.79 W/kg
Deviation (1 g) = -2.94%

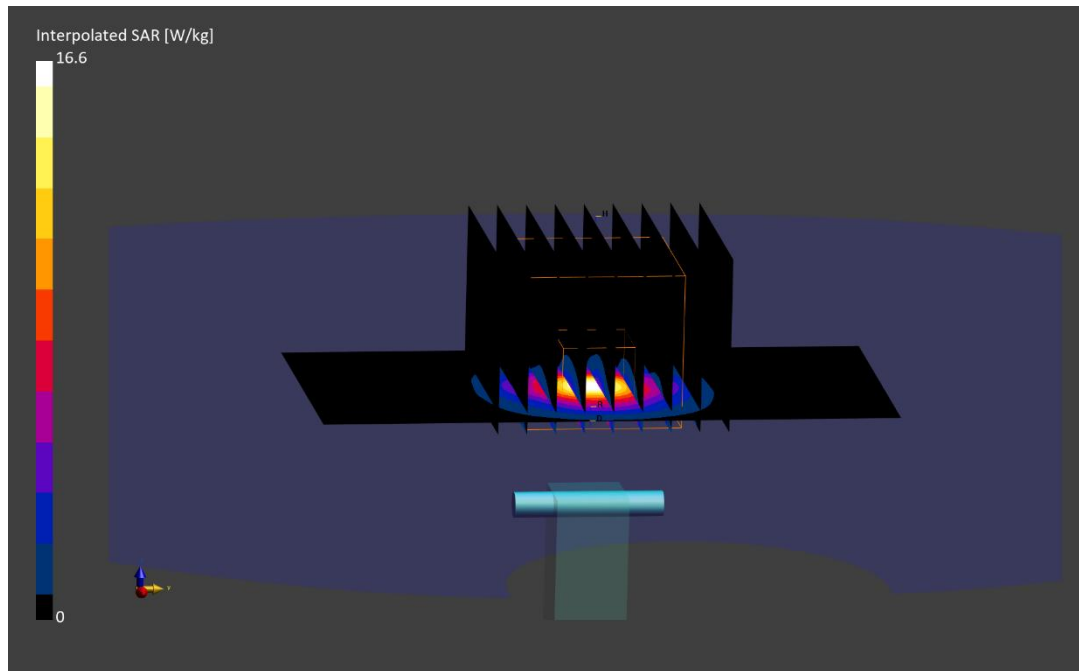

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5850.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5850.0$ MHz; $\text{cond} = 5.17$ S/m; $\text{perm} = 34.6$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 12/10/2025; Ambient Temp: 22.0°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7668; ConvF:(4.67,4.74,4.52); Calibrated: 2025-08-11

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1681; Calibrated: 2025-08-08

Phantom: Twin-SAM V8.0; Serial: 2027

Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.9 W/kg

SAR(1 g) = 3.79 W/kg

Deviation (1 g) = -5.01%

