

PCTEST ENGINEERING LABORATORY, INC.

DUT: Dipole 835 MHz; Type: D835V2; Serial: 406

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Brain ($\sigma = 0.90$ mho/m, $\epsilon_r = 40.44$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 11-08-2006; Ambient Temp: 23.5°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN3589; ConvF(8.36, 8.36, 8.36); Calibrated: 7/14/2006

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn704; Calibrated: 6/1/2006

Phantom: SAM Main; Type: SAM 4.0; Serial: TP:1197

Measurement SW: DASY4, V4.7 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 171

835MHz Dipole Validation


Area Scan (7x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Input Power = 24.0 dBm (250 mW)

SAR(1 g) = 2.49 mW/g; SAR(10 g) = 1.68 mW/g

Target SAR(1g) = 2.375 mW/g; Deviation = +4.84 %

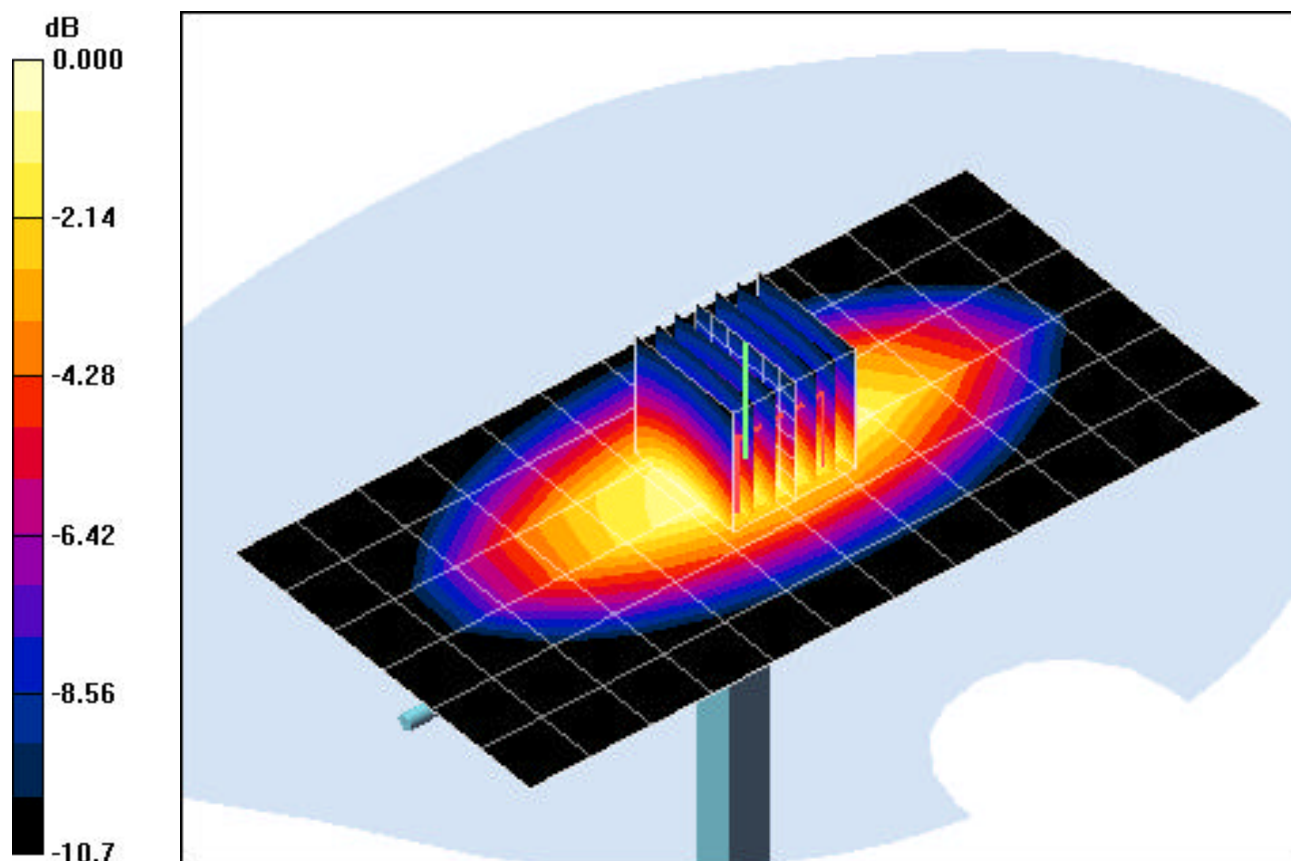

0 dB = 2.96mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: Dipole 1900 MHz; Type: D1900V2; SN: 502

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Brain ($\sigma = 1.46$ mho/m, $\epsilon_r = 40.13$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

Test Date: 11-09-2006; Ambient Temp: 23.4°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN3589; ConvF(7.11, 7.11, 7.11); Calibrated: 7/14/2006

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn704; Calibrated: 6/1/2006

Phantom: SAM Main; Type: SAM 4.0; Serial: TP:1197

Measurement SW: DASY4, V4.7 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 171

1900MHz Dipole Validation


Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 20.0 dBm (100 mW)

SAR(1 g) = 4.13 mW/g; SAR(10 g) = 2.65 mW/g

Target SAR(1g) = 3.97 mW/g; Deviation = + 3.77 %

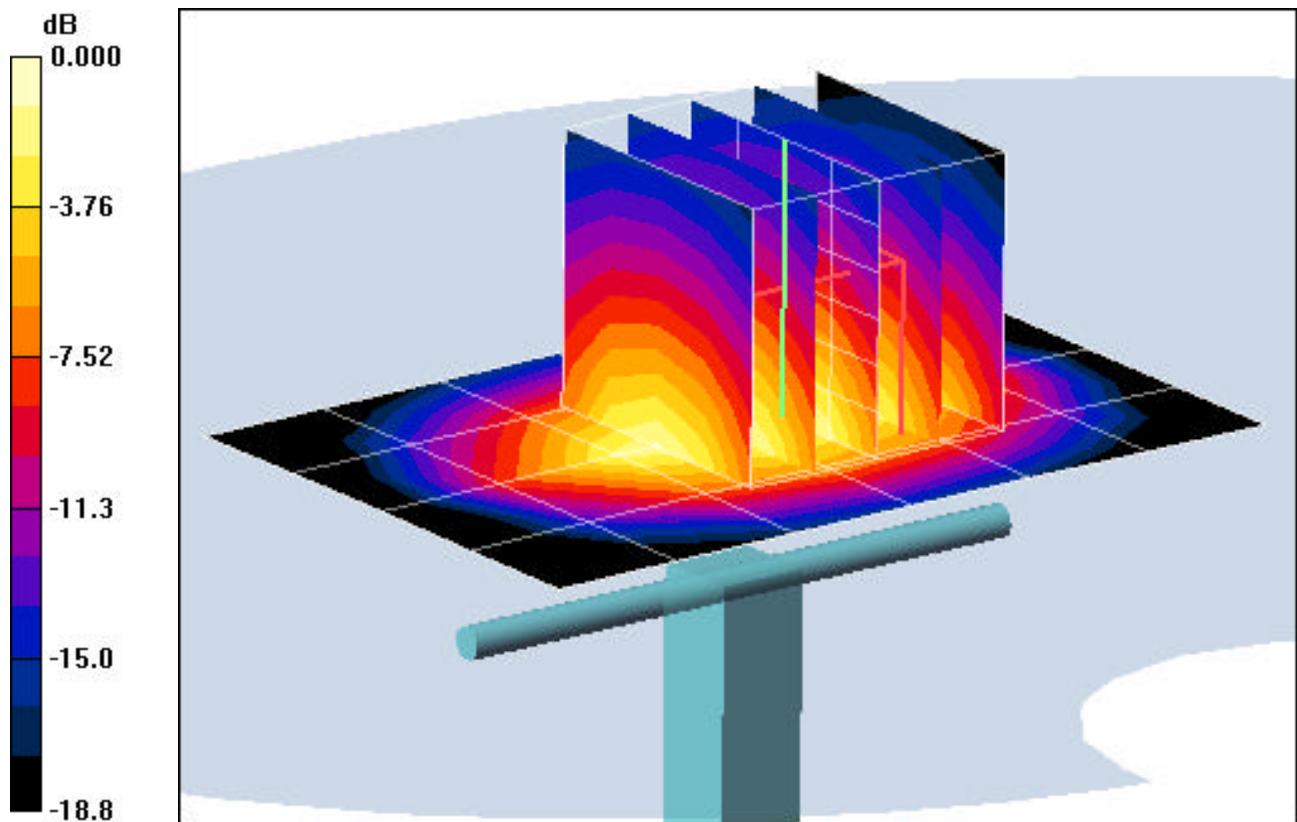

0 dB = 5.37mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: Dipole 835 MHz; Type: D835V2; Serial: 406

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Brain ($\sigma = 0.90$ mho/m, $\epsilon_r = 40.44$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 11-10-2006; Ambient Temp: 23.3°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN3589; ConvF(8.36, 8.36, 8.36); Calibrated: 7/14/2006

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn704; Calibrated: 6/1/2006

Phantom: SAM Main; Type: SAM 4.0; Serial: TP:1197

Measurement SW: DASY4, V4.7 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 171

835MHz Dipole Validation


Area Scan (7x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Input Power = 24.0 dBm (250 mW)

SAR(1 g) = 2.51 mW/g; SAR(10 g) = 1.64 mW/g

Target SAR(1g) = 2.375 mW/g; Deviation = +5.68 %

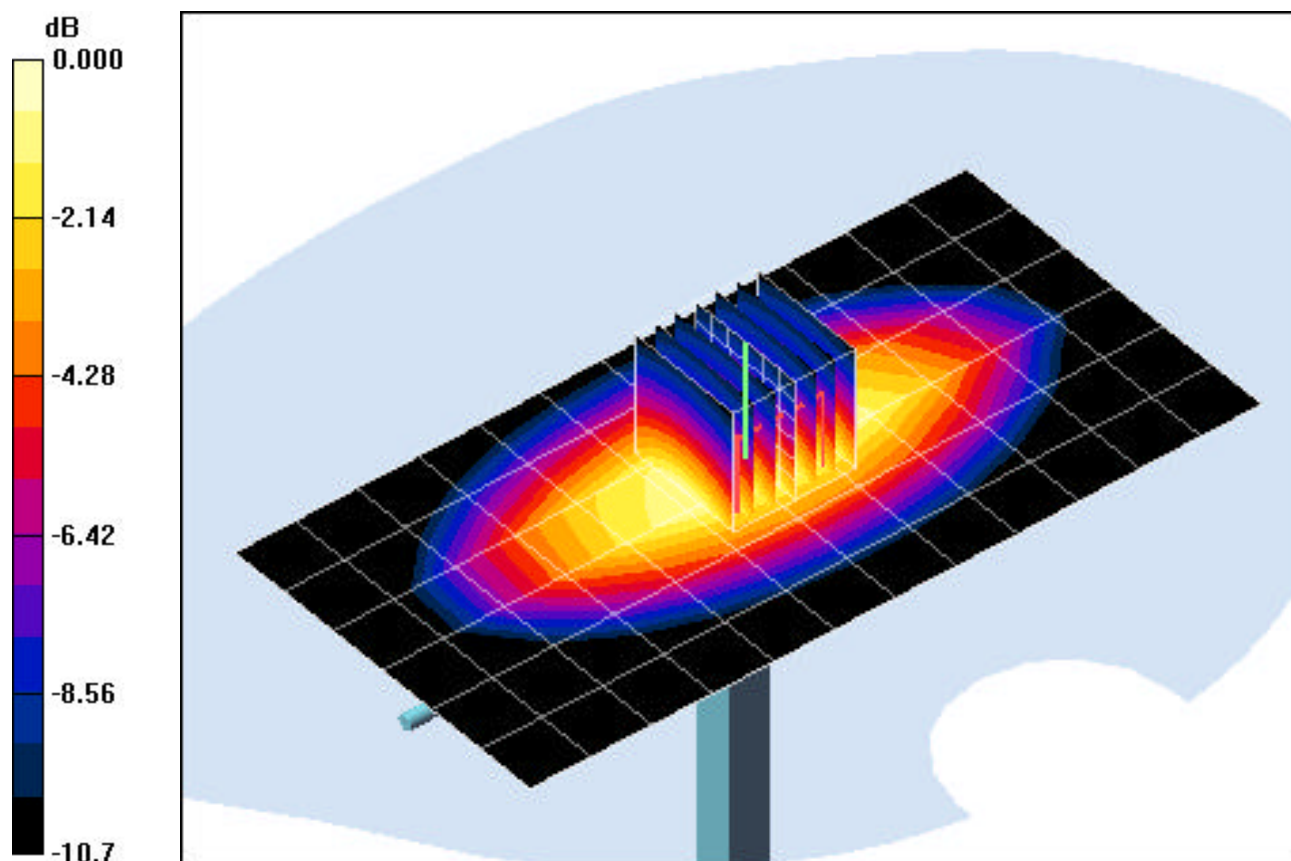

0 dB = 2.83mW/g

PCTEST ENGINEERING LABORATORY, INC.

DUT: Dipole 1900 MHz; Type: D1900V2; SN: 502

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Brain ($\sigma = 1.46$ mho/m, $\epsilon_r = 40.13$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

Test Date: 11-10-2006; Ambient Temp: 23.3°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN3589; ConvF(7.11, 7.11, 7.11); Calibrated: 7/14/2006

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn704; Calibrated: 6/1/2006

Phantom: SAM Main; Type: SAM 4.0; Serial: TP:1197

Measurement SW: DASY4, V4.7 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 171

1900MHz Dipole Validation


Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Input Power = 20.0 dBm (100 mW)

SAR(1 g) = 4.15 mW/g; SAR(10 g) = 2.71 mW/g

Target SAR(1g) = 3.97 mW/g; Deviation = + 4.53 %

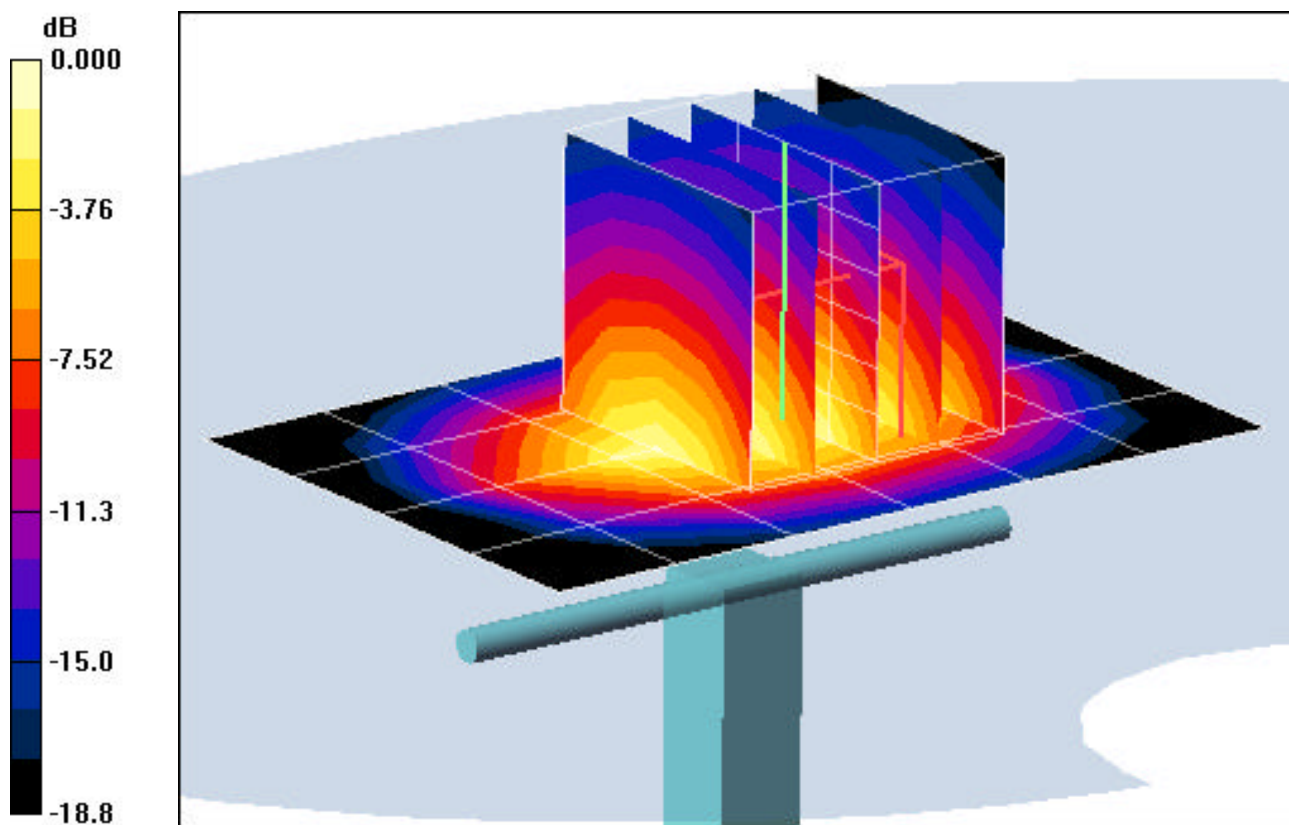

0 dB = 5.43mW/g