

**HCT CO.,LTD.**

2-6, 73, 74, Seoicheon-ro 578beon-gil, Majang-myeon, Icheon-si, Gyeonggi-do, Republic of Korea
Tel. +82 31 645 6300 Fax. +82 31 645 6401

Appendix A: Test Setup Photo

FCC ID
BEJTM19FNEUHD2

File No.		
HCT-RF-2412-FC051-P	HCT-RF-2412-FC052-P	HCT-RF-2412-FC053-P
HCT-RF-2412-FC054-P	HCT-RF-2412-FC055-P	HCT-RF-2412-FC056-P
HCT-RF-2412-FC057-P	HCT-RF-2412-FC058-P	HCT-RF-2412-FC059-P
HCT-RF-2412-FC060-P	HCT-RF-2412-FC088-P	


REVISION HISTORY

The revision history for this document is shown in table.


Revision No.	Date of Issue	Description
0	December 31, 2024	Initial Release

File No.	HCT-RF-2412-FC051-P	HCT-RF-2412-FC052-P	HCT-RF-2412-FC053-P	HCT-RF-2412-FC054-P	HCT-RF-2412-FC055-P
	HCT-RF-2412-FC056-P	HCT-RF-2412-FC057-P	HCT-RF-2412-FC058-P	HCT-RF-2412-FC059-P	HCT-RF-2412-FC060-P
	HCT-RF-2412-FC088-P				

1. Radiated Test Setup Photo

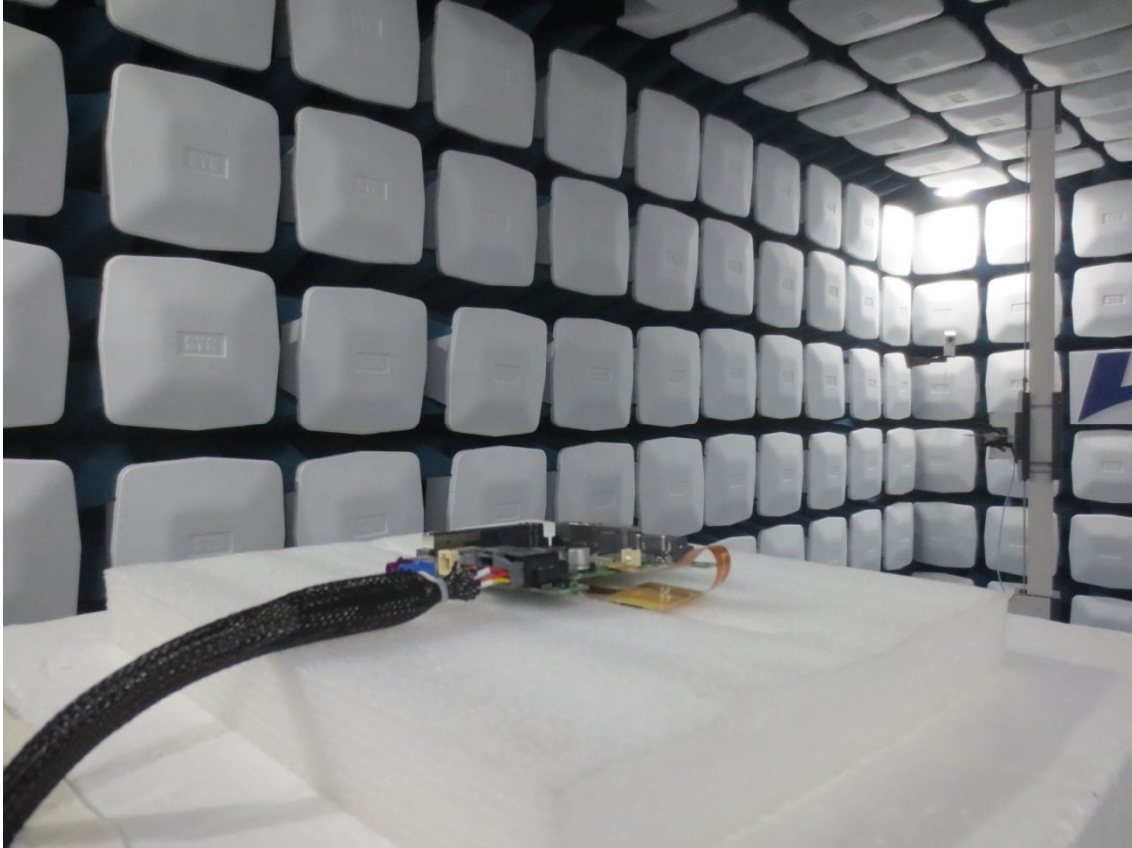

File	HCT-RF-2412-FC051-P	HCT-RF-2412-FC052-P	HCT-RF-2412-FC053-P	HCT-RF-2412-FC054-P	HCT-RF-2412-FC055-P
No.	HCT-RF-2412-FC056-P	HCT-RF-2412-FC057-P	HCT-RF-2412-FC058-P	HCT-RF-2412-FC059-P	HCT-RF-2412-FC060-P
	HCT-RF-2412-FC088-P				

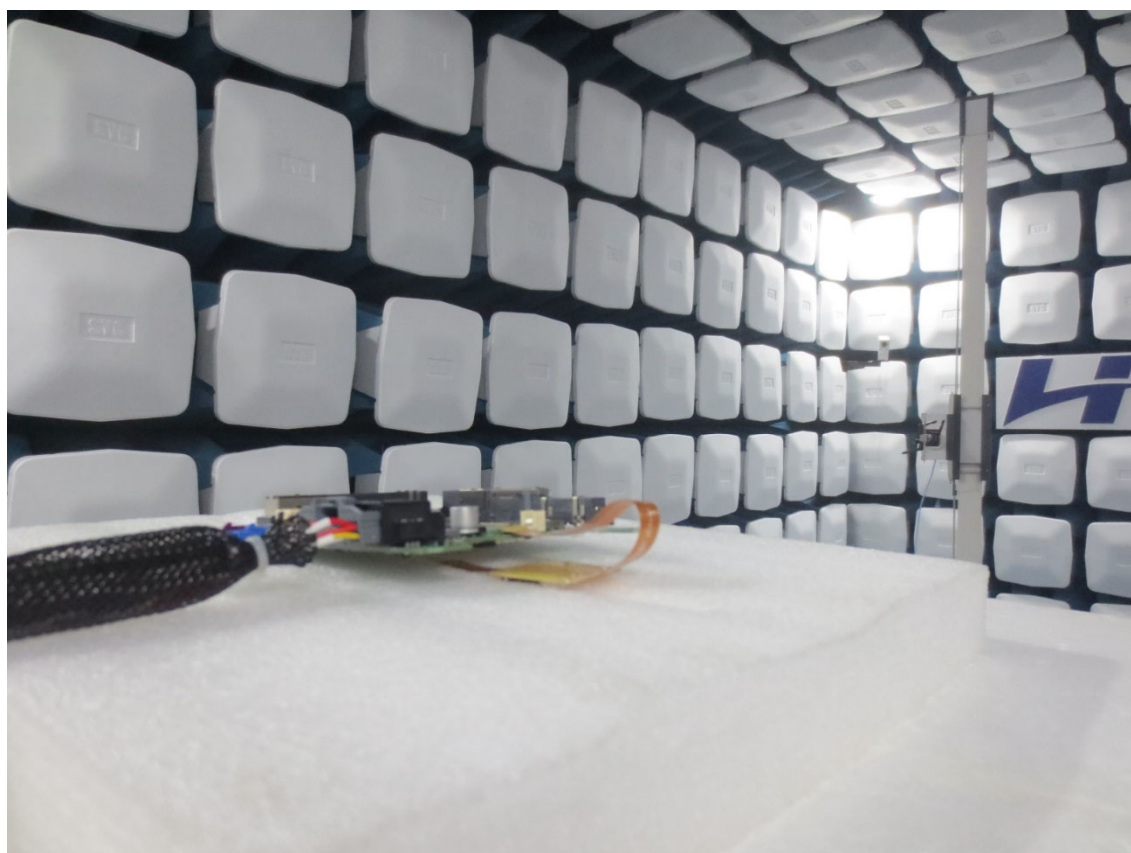

File
No.


HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

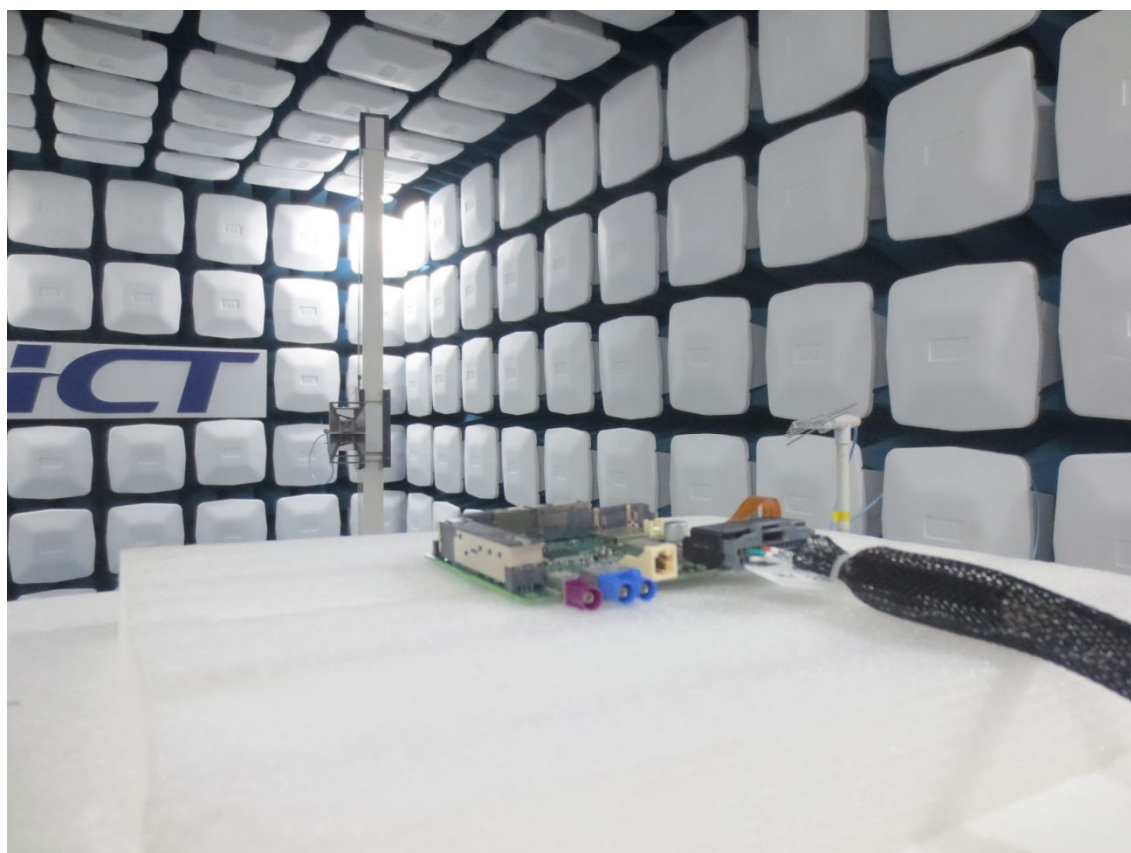

File
No.


HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

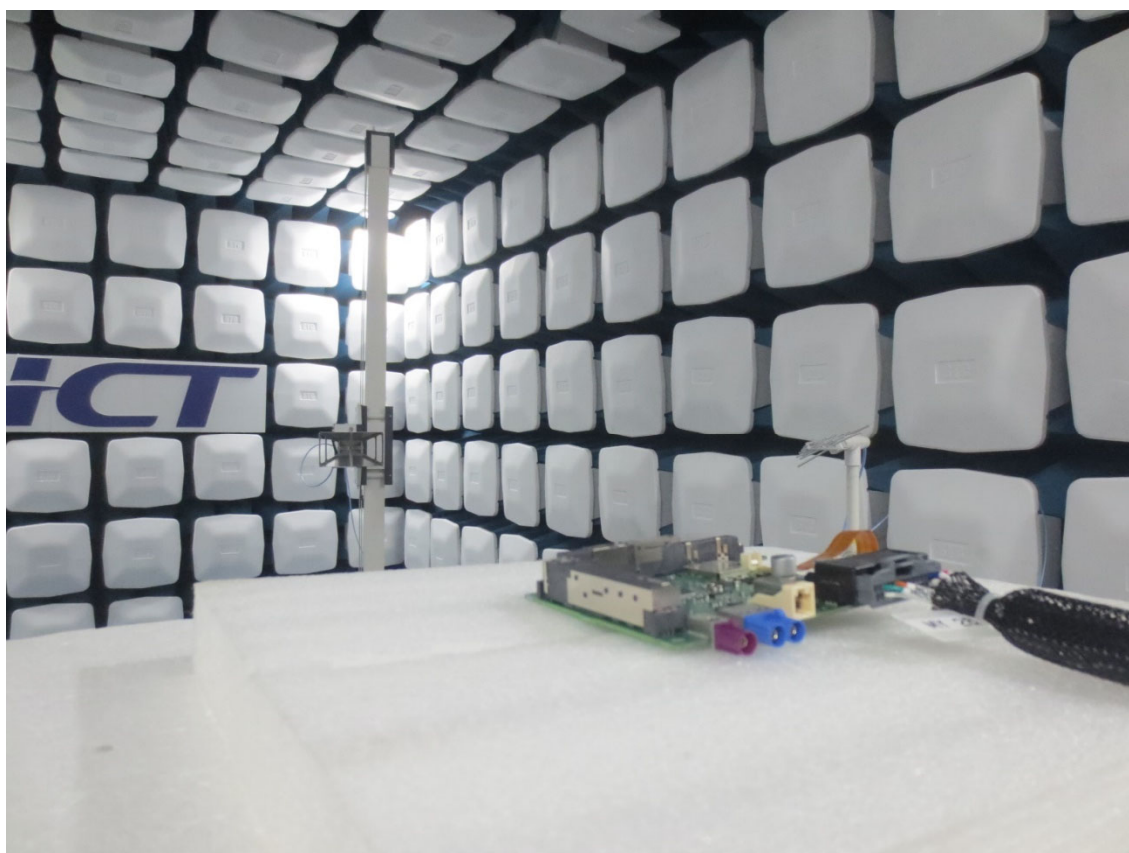

File
No.

HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P



File
No.


HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

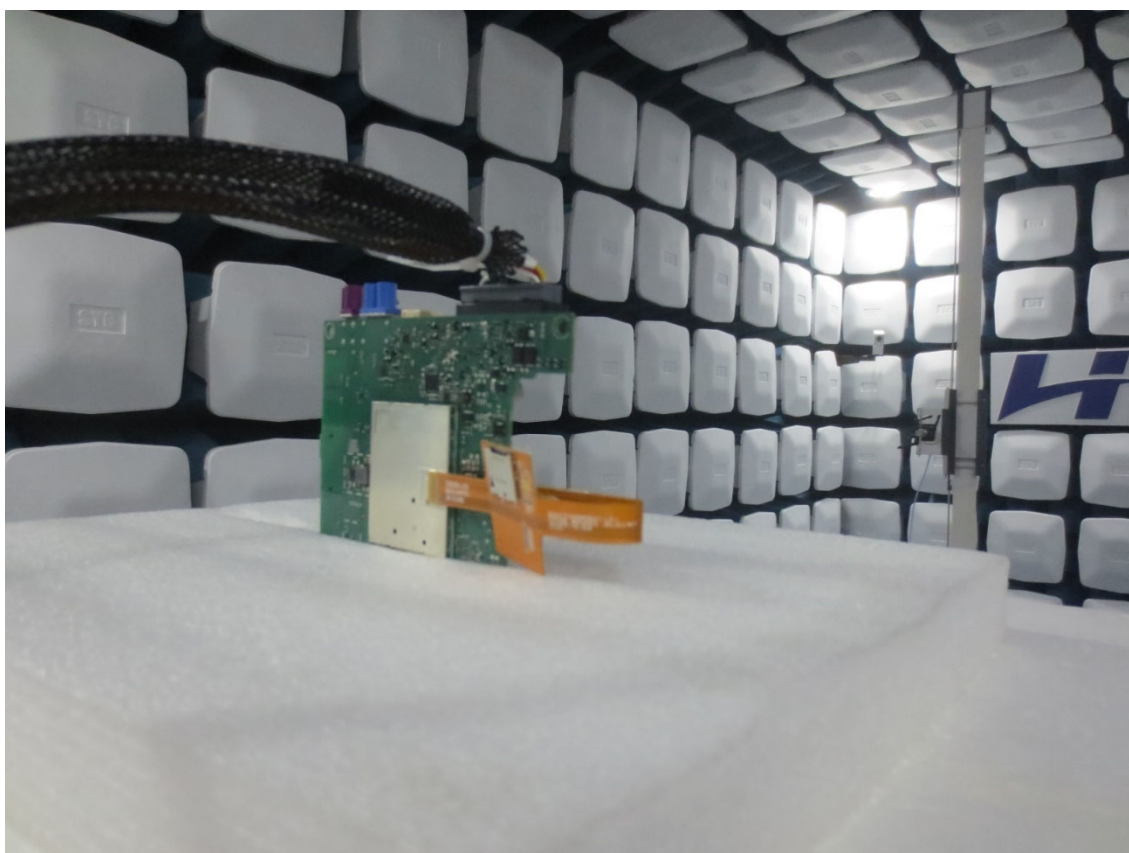

File
No.


HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

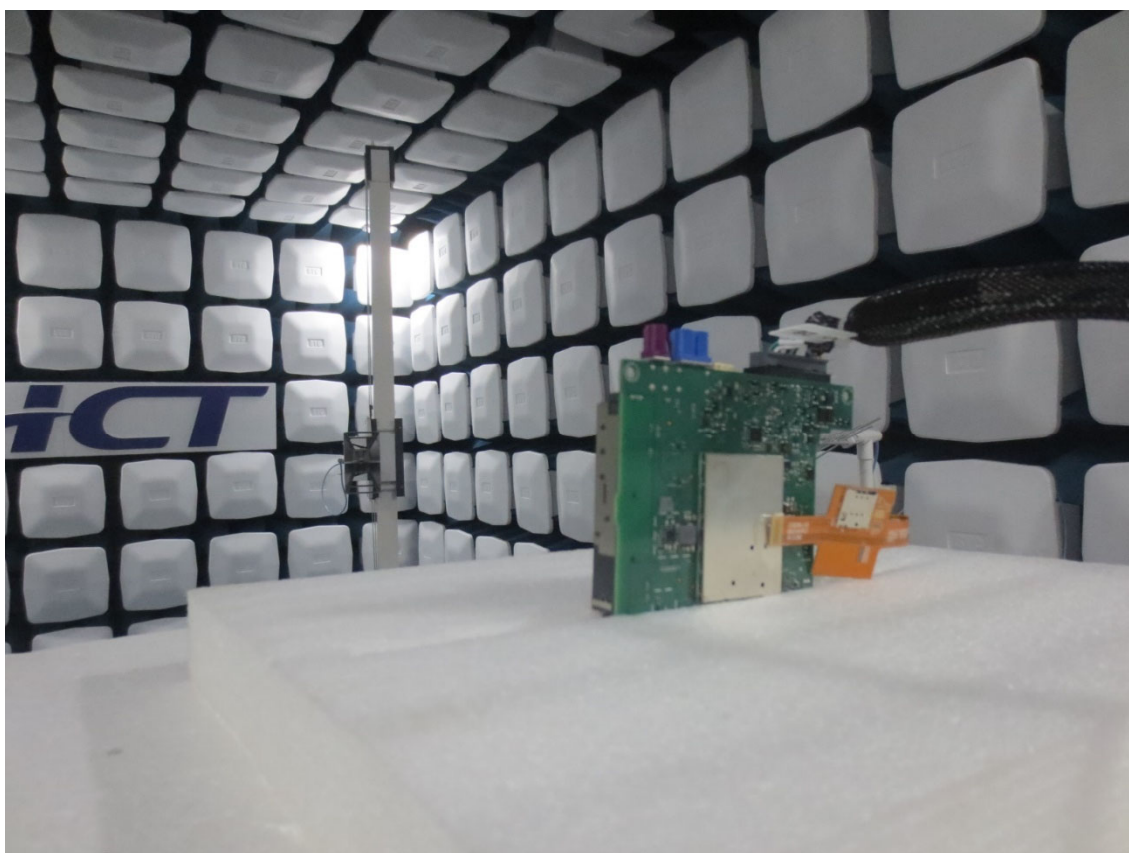

File
No.


HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

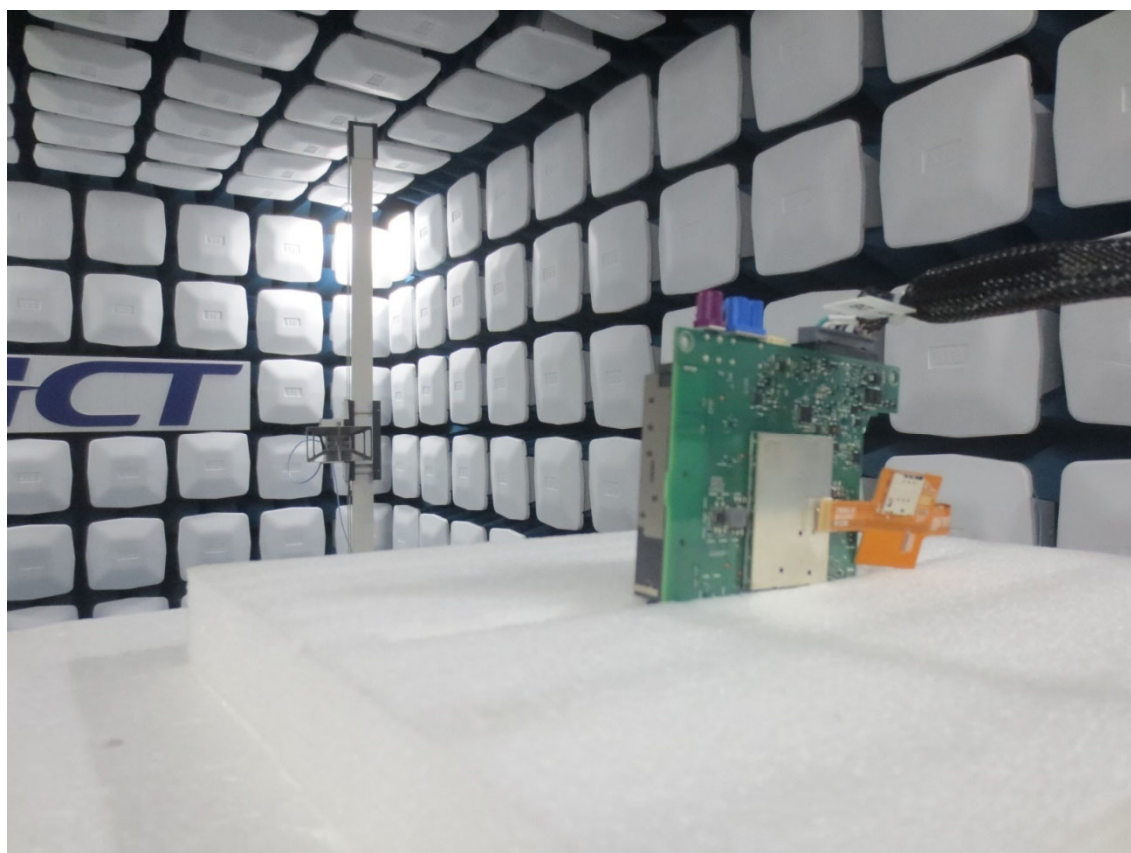

File
No.


HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

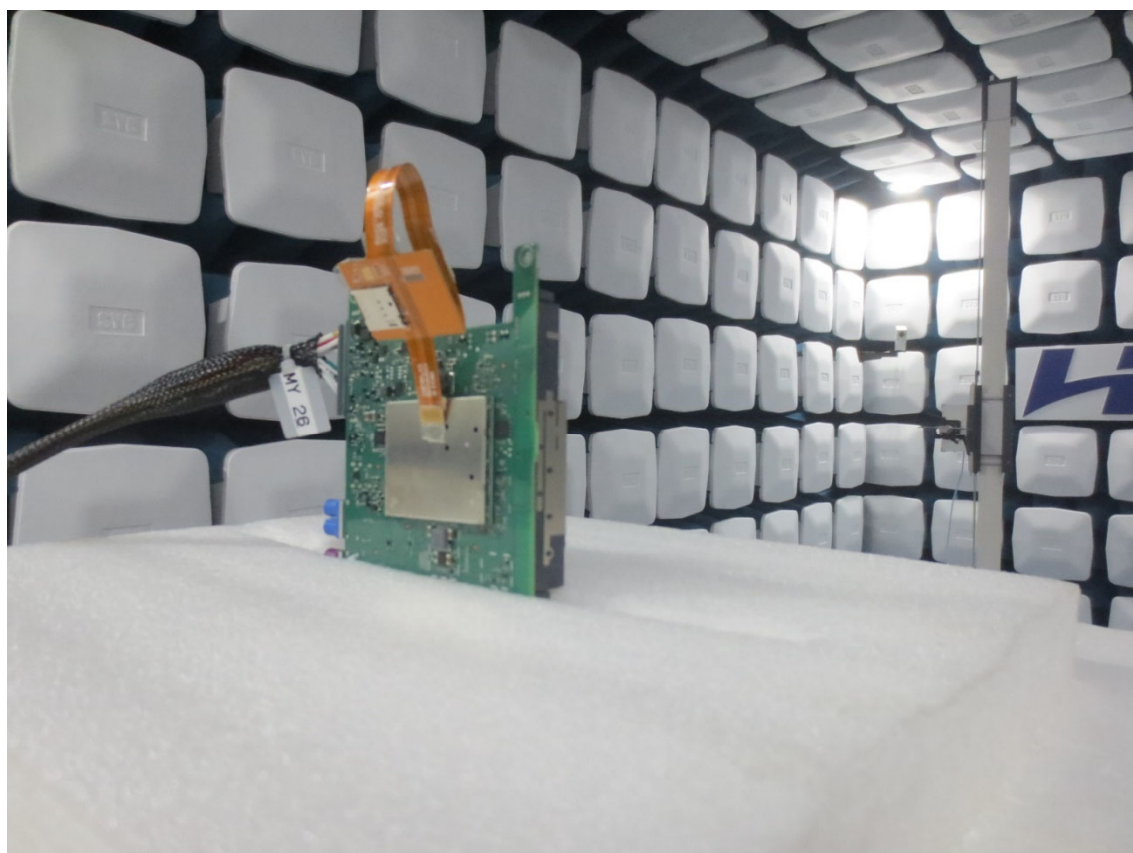

File
No.


HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

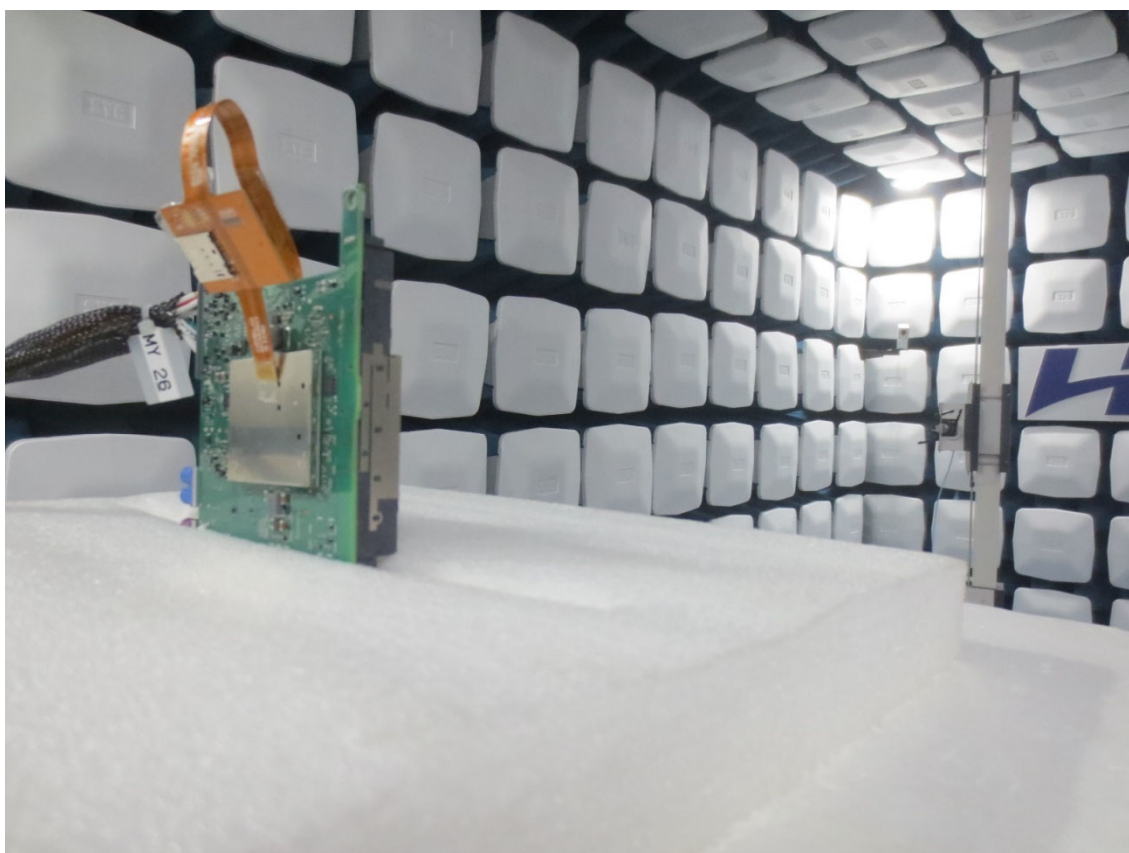

File
No.

HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P



File
No.


HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P

HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

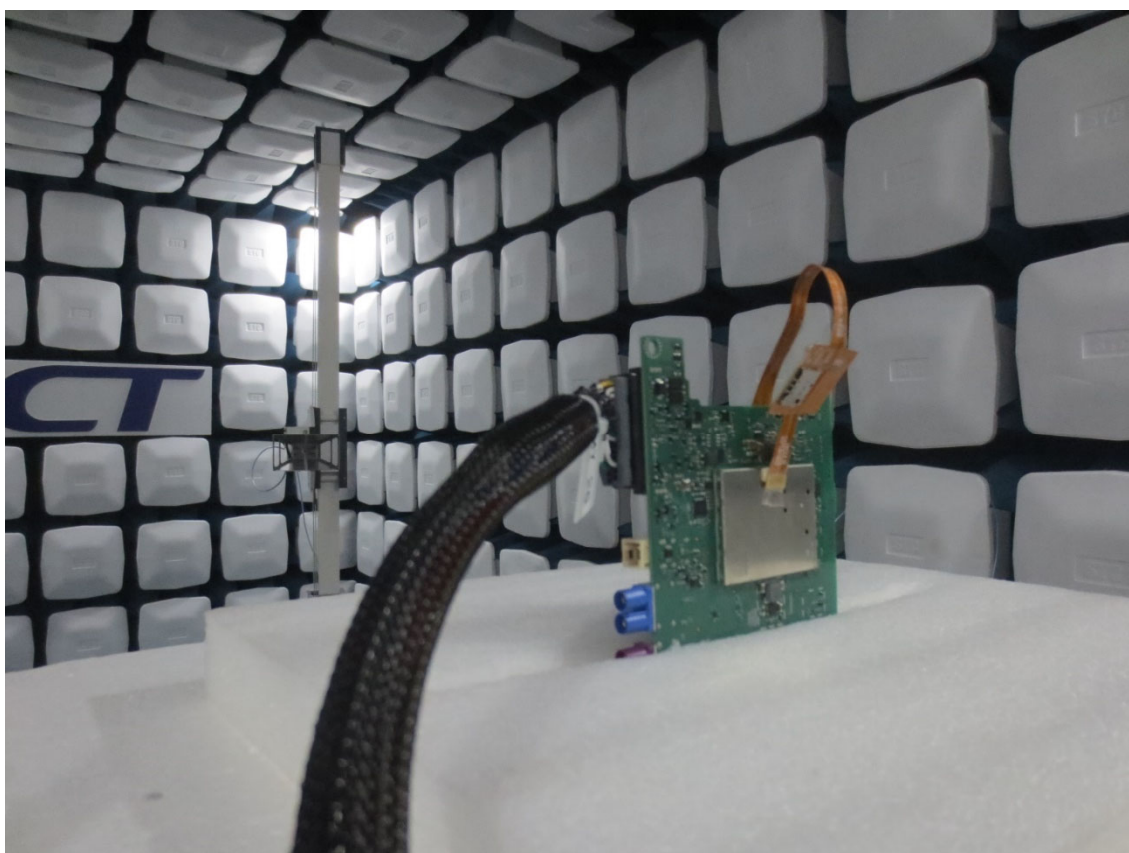

File
No.

HCT-RF-2412-FC051-P
HCT-RF-2412-FC056-P
HCT-RF-2412-FC088-P


HCT-RF-2412-FC052-P
HCT-RF-2412-FC057-P

HCT-RF-2412-FC053-P
HCT-RF-2412-FC058-P

HCT-RF-2412-FC054-P
HCT-RF-2412-FC059-P

HCT-RF-2412-FC055-P
HCT-RF-2412-FC060-P

2. Conducted Test Setup Photo

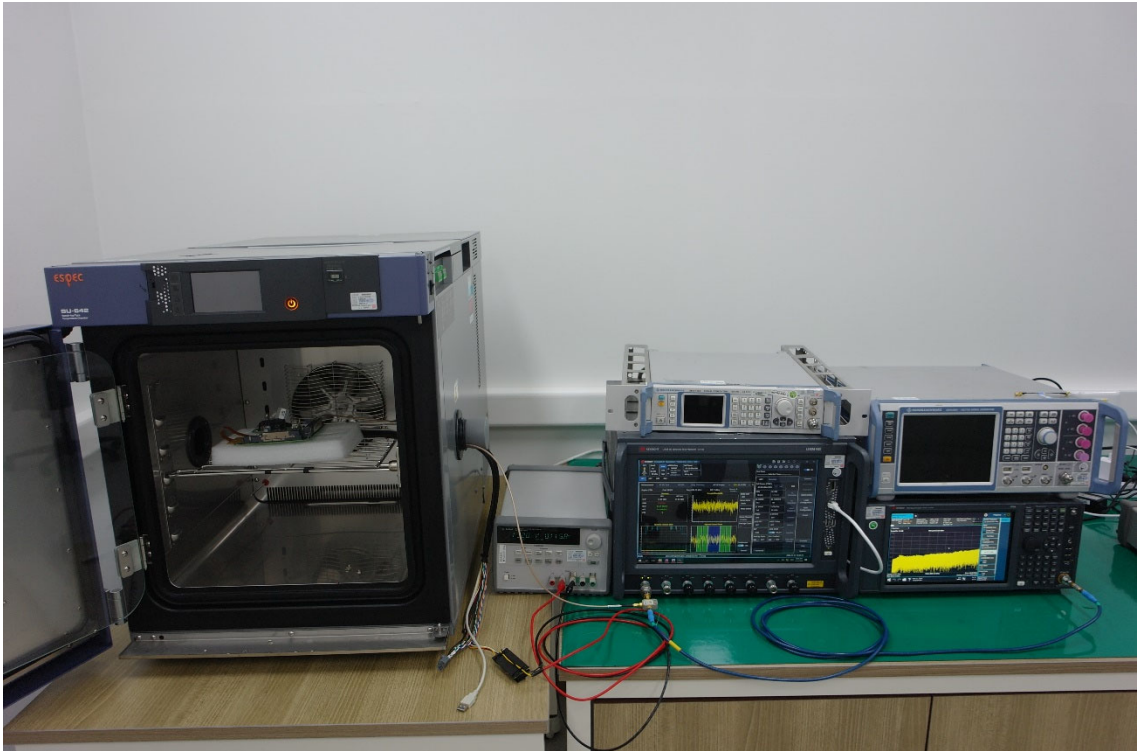

File	HCT-RF-2412-FC051-P	HCT-RF-2412-FC052-P	HCT-RF-2412-FC053-P	HCT-RF-2412-FC054-P	HCT-RF-2412-FC055-P
No.	HCT-RF-2412-FC056-P	HCT-RF-2412-FC057-P	HCT-RF-2412-FC058-P	HCT-RF-2412-FC059-P	HCT-RF-2412-FC060-P
	HCT-RF-2412-FC088-P				