
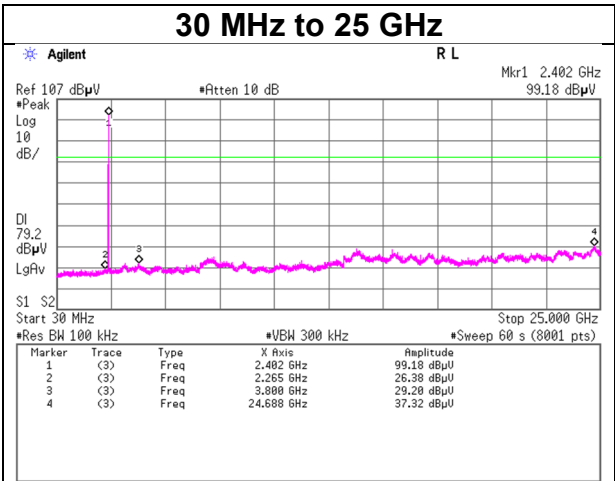


Conducted Spurious Emission

Mode	Tx, Hopping Off, 3DH5			
Date	Test site	Temperature	Humidity	Engineer
August 23, 2025	MR1	24 deg. C	51 % RH	Kenichi Adachi



2402 MHz

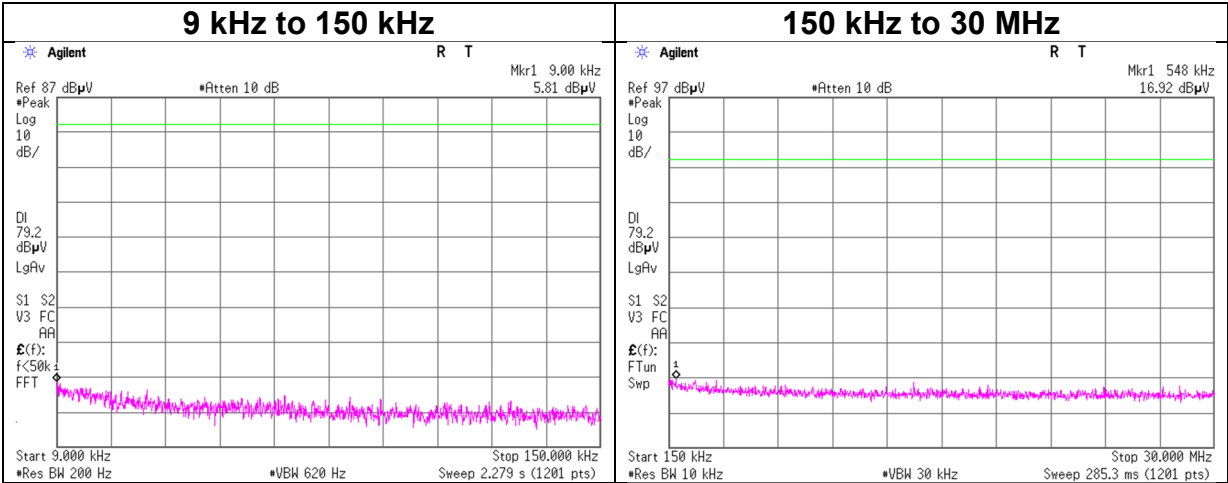

Conducted Spurious Emission

Mode	Tx, Hopping Off, 3DH5			
Date	Test site	Temperature	Humidity	Engineer
August 23, 2025	MR1	24 deg. C	51 % RH	Kenichi Adachi



2441 MHz

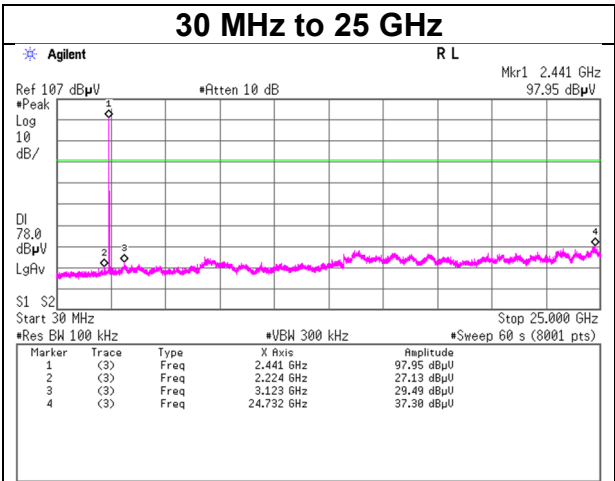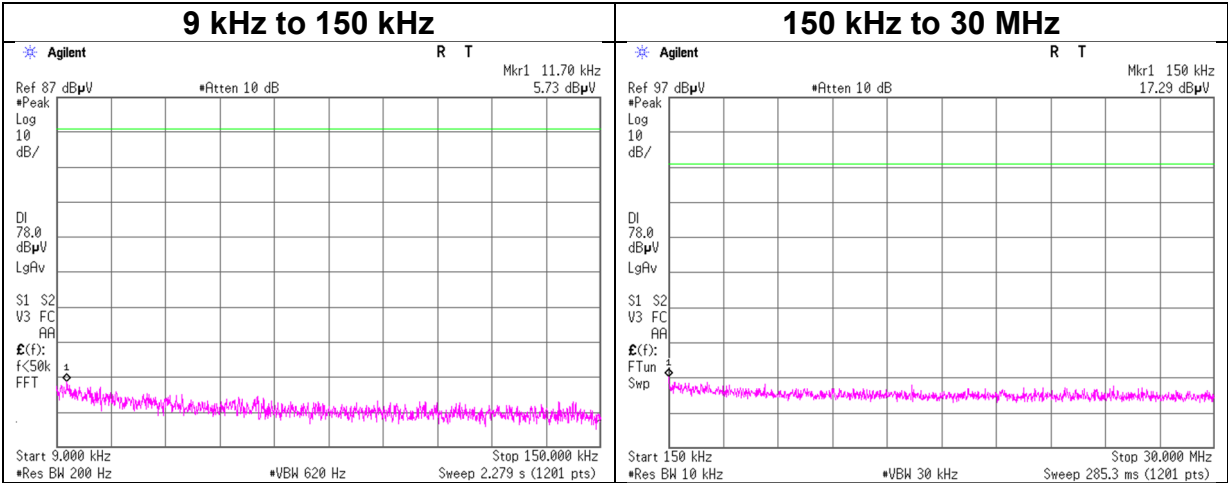

Conducted Spurious Emission

Mode	Tx, Hopping Off, 3DH5			
Date	Test site	Temperature	Humidity	Engineer
August 23, 2025	MR1	24 deg. C	51 % RH	Kenichi Adachi


2480 MHz

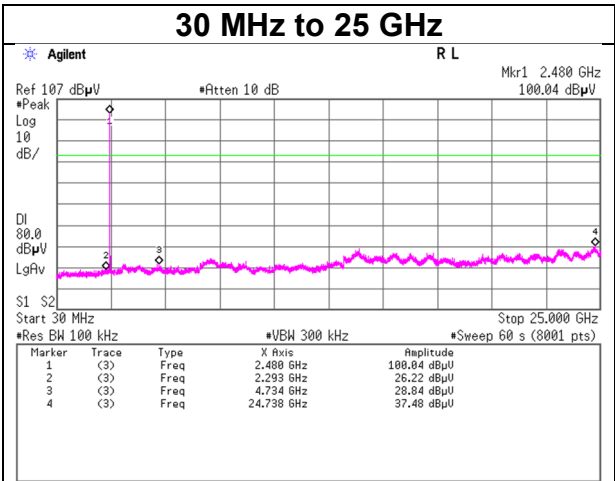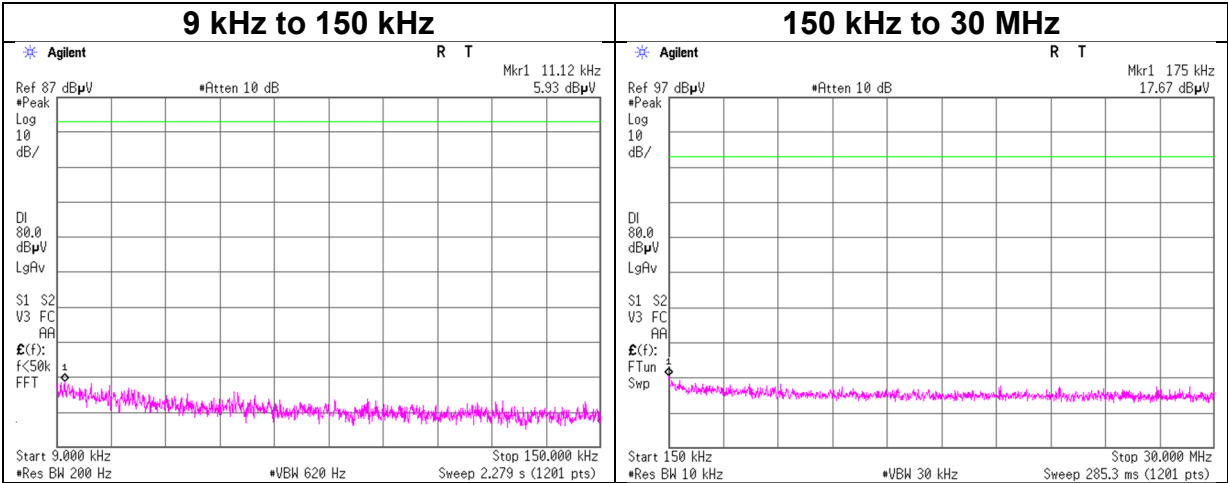


Conducted Emission Band Edge compliance

Mode	Tx, Hopping On / Off, DH5			
Date	Test site	Temperature	Humidity	Engineer
August 23, 2025	MR1	24 deg. C	51 % RH	Kenichi Adachi

Hopping On

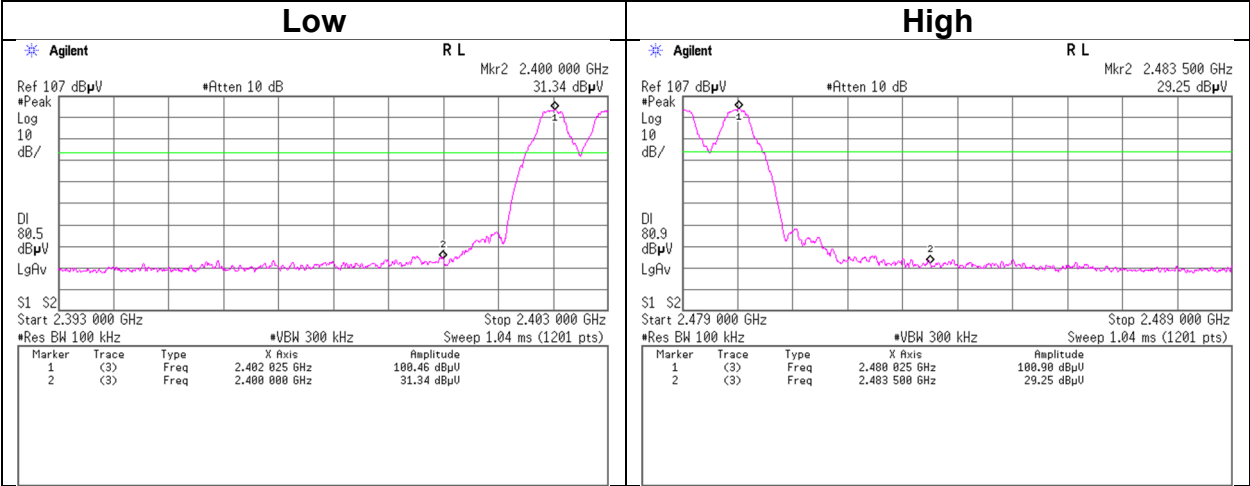


Hopping Off

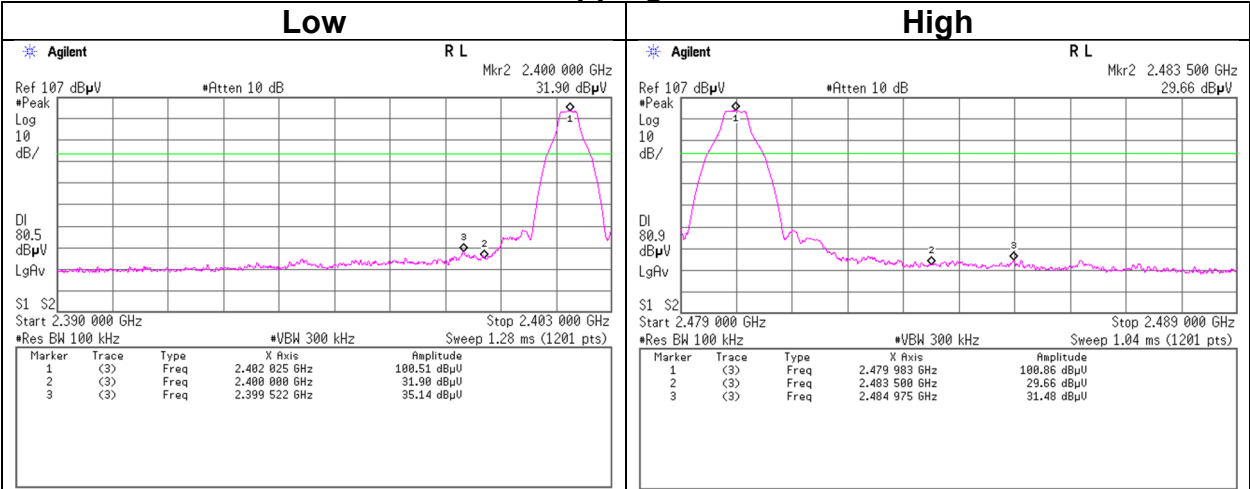


Conducted Emission Band Edge compliance

Mode	Tx, Hopping On / Off, 3DH5			
Date	Test site	Temperature	Humidity	Engineer
August 23, 2025	MR1	24 deg. C	51 % RH	Kenichi Adachi

Hopping On

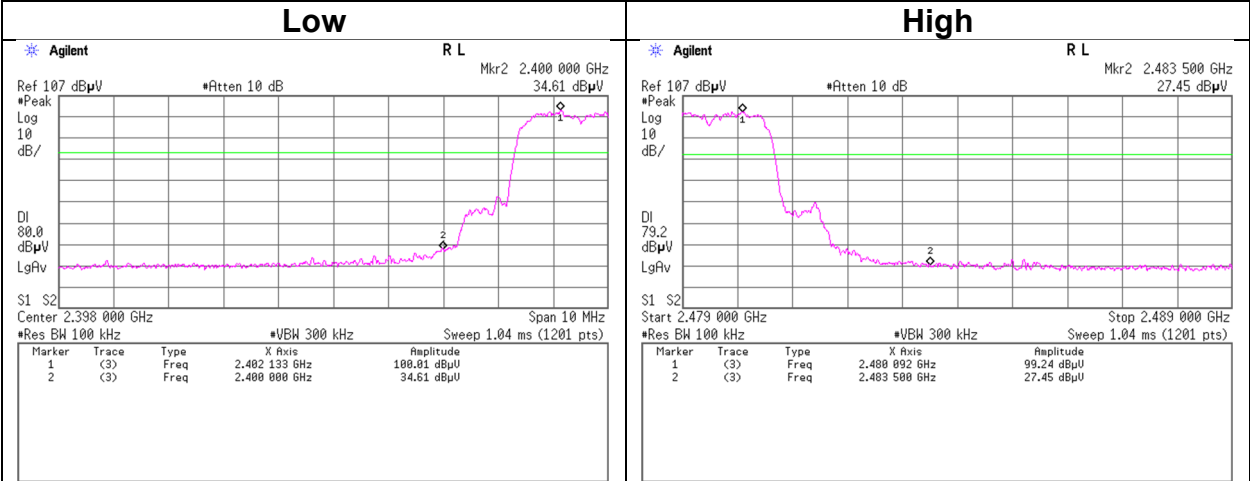

Hopping Off

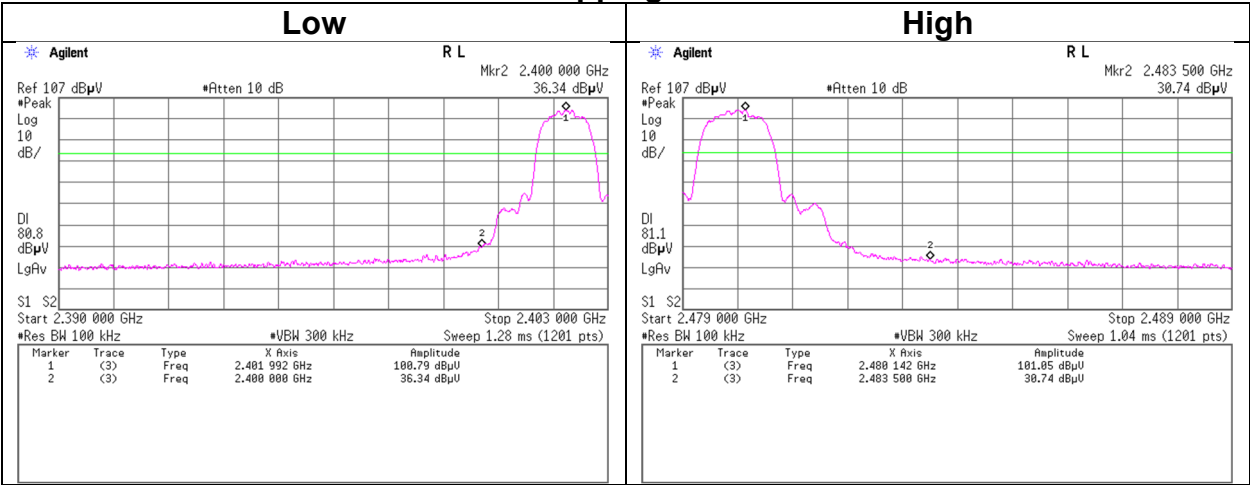

APPENDIX 2: Test Instruments

Test Equipment (1/2)

Test Item	LIMS ID	Description	Manufacturer	Model	Serial	Last Calibration Date	Cal Int
AT	160493	Attenuator	Weinschel Corp.	54A-10	83406	2025/12/07	12
AT	160494	Attenuator	Weinschel Corp.	54A-10	83420	2025/12/07	12
AT	239651	Coaxial Cable	Huber+Suhner	SUCOFLEX 102	2001219/2	2025/08/27	12
AT	239652	Coaxial Cable	Huber+Suhner	SUCOFLEX 102	2001220/2	2025/08/27	12
AT	145095	Digital Tester	SANWA	PC500	7019224	2025/05/22	12
AT	146267	Power Meter	Anritsu Corporation	ML2495A	850009	2025/05/21	12
AT	236796	Power Meter	Raditeq (Formerly DARE!! Instruments)	RPR3008W	RPR8W-2301014	2025/05/21	12
AT	236797	Power Meter	Raditeq (Formerly DARE!! Instruments)	RPR3008W	RPR8W-2301015	2025/05/21	12
AT	146309	Power sensor	Anritsu Corporation	MA2411B	917063	2025/05/21	12
AT	145089	Spectrum Analyzer	Keysight Technologies Inc	E4446A	MY46180525	2025/09/12	12
AT	171614	Terminator	Weinschel - API Technologies Corp	M1459A	88995	2025/05/27	12
AT	249685	Terminator	To-Conne Co., Ltd.	SMA50-SP 1W	-	-	-
AT	259715	Thermo-Hygrometer	CUSTOM. Inc	CTH-230	-	2025/04/11	12
CE	248304	Attenuator	JFW	50HFFA-006-2/18N	-	2025/05/14	12
CE	144969	Coaxial Cable&RF Selector	Suhner/Suhner/TOYO	RG223U/141PE/NS 4906	-/0901-270(RF Selector)	2025/04/05	12
CE	145793	Digital Hitester	HIOKI E. E. CORPORATION	3805-50	80997819	2025/05/23	12
CE	145539	LISN	Rohde & Schwarz	ENV216	100512	2025/02/01	12
CE	145541	LISN	Rohde & Schwarz	ENV216	100514	2025/02/01	12
CE	207277	Tape Measure	ASKUL	-	-	-	-
CE	146188	Terminator	TME	CT-01 BP	-	2025/11/12	12
CE	144200	Test Receiver	Rohde & Schwarz	ESW8	100952	2025/10/23	12
CE	259710	Thermo-Hygrometer	CUSTOM. Inc	CTH-230	-	2025/04/11	12
CE,RE	170932	EMI Software	TSJ (Techno Science Japan)	TEPTO-DV3(RE,CE,ME,PE)	Ver 3.1.0612	-	-
RE	199783	Attenuator	JFW	50HF-006N	-	2025/06/04	12
RE	239787	Biconical Antenna	Schwarzbeck Mess-Elektronik OHG	VHBB 9124+BBA9106	01908	2025/08/14	12
RE	236709	Coaxial Cable	Hayashi-Repic co., Ltd.	NMS079B-GL310C-SMS117B-2m	47256-02-04	2025/05/28	12
RE	236711	Coaxial Cable	Hayashi-Repic co., Ltd.	KMS020B-GL140sE-KMS020B-7.0m	47256-03-02	2025/05/27	12
RE	236720	Coaxial Cable	Huber+Suhner	SF106/SF106/SF106	2001167/2001168/2001161	2025/05/28	12
RE	236724	Coaxial Cable	Hayashi-Repic co., Ltd.	SF106(HUBER+SUHNER)/LMR400UF/GL310C/GL310C	2000430/47753-2/47256-01-04/47256-01-02	2025/05/12	12
RE	236756	Coaxial Cable	Huber+Suhner	SF106/11N/11N/6000	2001167	2025/05/28	12
RE	239644	Coaxial Cable	Junkosha	MWX221-01000NFSNMS/B	2306S022	2025/08/27	12
RE	243210	Coaxial Cable	Hayashi-Repic co., Ltd.	SMS13-13A26-NFS13-1.0m	49190-01-02	2025/12/04	12
RE	264042	Coaxial Cable	Hayashi-Repic co., Ltd.	SMS13-13A26-SFS13-0.5m	53292-01-02	2025/06/20	12
RE	235640	DIGITAL MULTIMETER	HIOKI E. E. CORPORATION	DT4261	230313157	2025/05/22	12
RE	236584	Horn Antenna	AINFO Inc.	LB-8180-NF	2030013000112	2025/04/25	12
RE	236586	Horn Antenna	AINFO Inc.	LB-42-25-C2-KF	2020087000114	2025/04/25	12
RE	236687	Horn Antenna	Schwarzbeck Mess-Elektronik OHG	BBHA 9120 C	788	2025/04/25	12
RE	145528	Logperiodic Antenna	Schwarzbeck Mess-Elektronik OHG	VUSLP9111B	195	2025/03/18	12
RE	236967	Pre Amplifier	TSJ (Techno Science Japan)	MLA-9K01-L01	23050010	2025/06/04	12
RE	237719	Pre Amplifier	TSJ (Techno Science Japan)	MLA-18265-J03	23060017	2025/06/19	12

Test Equipment (2/2)

Test Item	LIMS ID	Description	Manufacturer	Model	Serial	Last Calibration Date	Cal Int
RE	237786	RF RELAY MATRIX with preamplifier	TSJ (Techno Science Japan)	RFM-E221261R	07796	2025/11/23	12
RE	236615	Semi-Anechoic Chamber	TDK	SWAC-02(NSA)	2	2025/05/12	12
RE	236617	Semi-Anechoic Chamber	TDK	SWAC-02(SVSWR)	2	2025/06/13	12
RE	207281	Tape Measure	ASKUL	-	-	-	-
RE	235268	Test Receiver	Rohde & Schwarz	ESW44	103212	2025/12/19	12
RE	235738	Thermo-Hygrometer	CUSTOM. Inc	CTH-230	-	2025/04/16	12

*Hyphens for Last Calibration Date and Cal Int (month) are instruments that Calibration is not required (e.g. software), or instruments checked in advance before use.

The expiration date of the calibration is the end of the expired month.

As for some calibrations performed after the tested dates, those test equipment have been controlled by means of an unbroken chains of calibrations.

All equipment is calibrated with valid calibrations. Each measurement data is traceable to the national or international standards.

Test item:

AT: Antenna Terminal Conducted test

CE: Conducted Emission

RE: Radiated Emission