

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
 $f = 2450.000$ MHz; $\text{cond} = 1.82$ S/m; $\text{perm} = 39.6$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 11/03/2025; Ambient Temp: 20.9°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7718; ConvF:(7.07,7.06,7.3); Calibrated: 2025-04-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1407; Calibrated: 2025-04-07
Phantom: Twin-SAM V8.0; Serial: 2060
Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.76 W/kg

SAR(1 g) = 4.88 W/kg; SAR(10 g) = 2.28 W/kg

Deviation (1 g) = -7.22%; Deviation (10 g) = -8.06%

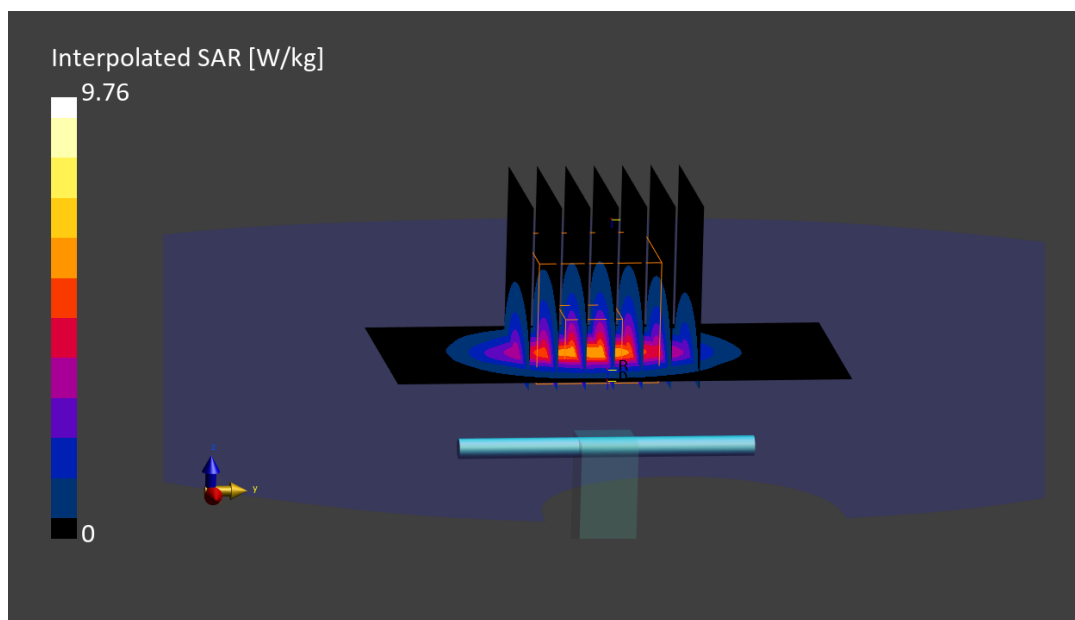

ELEMENT

DUT: Dipole 5250.000 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5250.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
 $f = 5250.000$ MHz; $\text{cond} = 4.69$ S/m; $\text{perm} = 35.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 10/20/2025; Ambient Temp: 19.5°C; Tissue Temp: 19.2°C

Probe: EX3DV4 - SN7718; ConvF:(5.41,5.4,5.59); Calibrated: 2025-04-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1407; Calibrated: 2025-04-07
Phantom: Twin-SAM V8.0; Serial: 2060
Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (28.0 x 28.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.2 W/kg

SAR(1 g) = 3.70 W/kg; SAR(10 g) = 1.06 W/kg

Deviation (1 g) = -6.21%; Deviation (10 g) = -6.61%

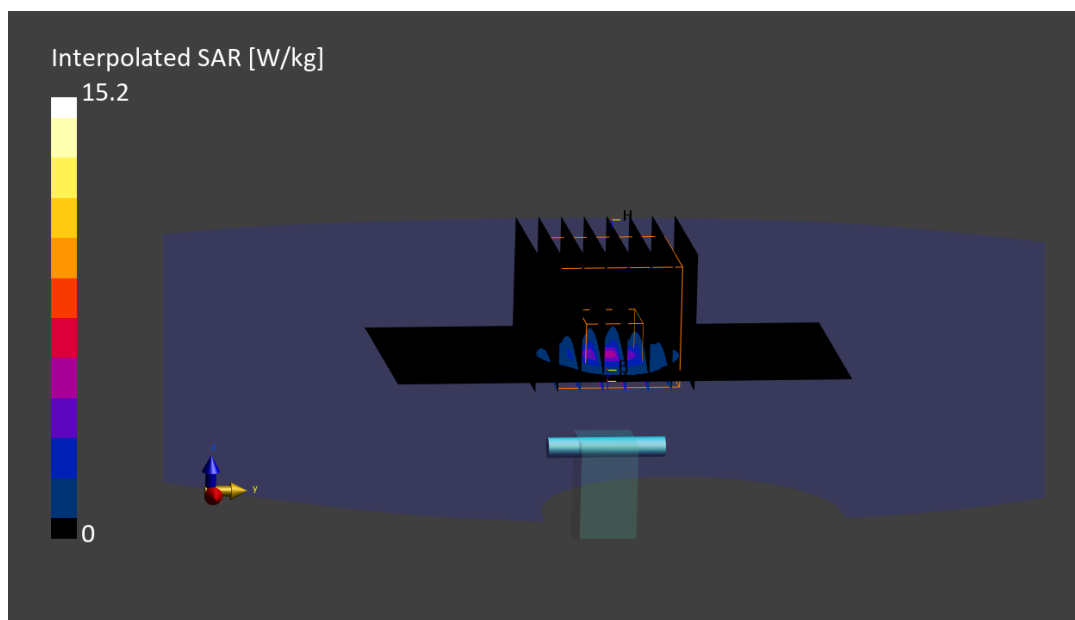

ELEMENT

DUT: Dipole 5250.000 MHz; Type: D5GHzV2 - SN1057

Communication System: UID: 0, CW; Frequency: 5250.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
f = 5250.000 MHz; cond = 4.67 S/m; perm = 35.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 11/03/2025; Ambient Temp: 20.7°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7661; ConvF:(5.7,6.07,6.06); Calibrated: 2025-06-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1558; Calibrated: 2025-06-05
Phantom: Twin-SAM V8.0; Serial: 2065
Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.0 W/kg

SAR(1 g) = 3.71 W/kg; SAR(10 g) = 1.07 W/kg

Deviation (1 g) = -6.55%; Deviation (10 g) = -5.73%

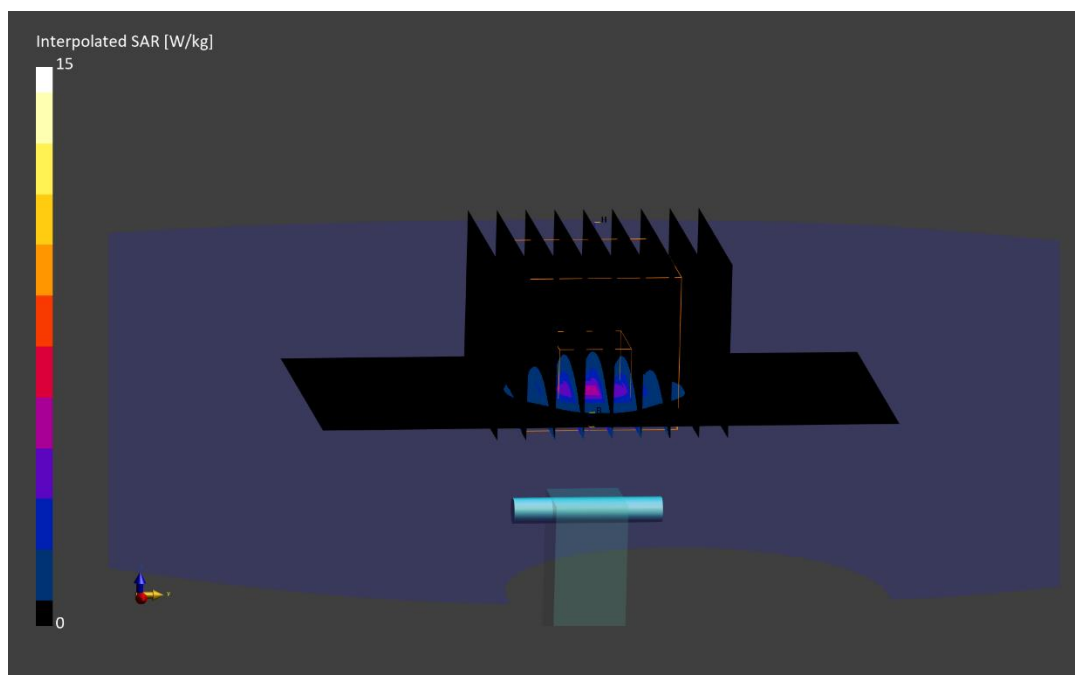

ELEMENT

DUT: Dipole 5600.000 MHz; Type: D5GHzV2 - SN1057

Communication System: UID: 0, CW; Frequency: 5600.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
 $f = 5600.000$ MHz; $\text{cond} = 5.07$ S/m; $\text{perm} = 34.7$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 11/03/2025; Ambient Temp: 20.7°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7661; ConvF:(5.13,5.46,5.46); Calibrated: 2025-06-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1558; Calibrated: 2025-06-05
Phantom: Twin-SAM V8.0; Serial: 2065
Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (24.0 x 28.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.6 W/kg

SAR(1 g) = 3.82 W/kg; SAR(10 g) = 1.09 W/kg

Deviation (1 g) = -7.73%; Deviation (10 g) = -7.63%

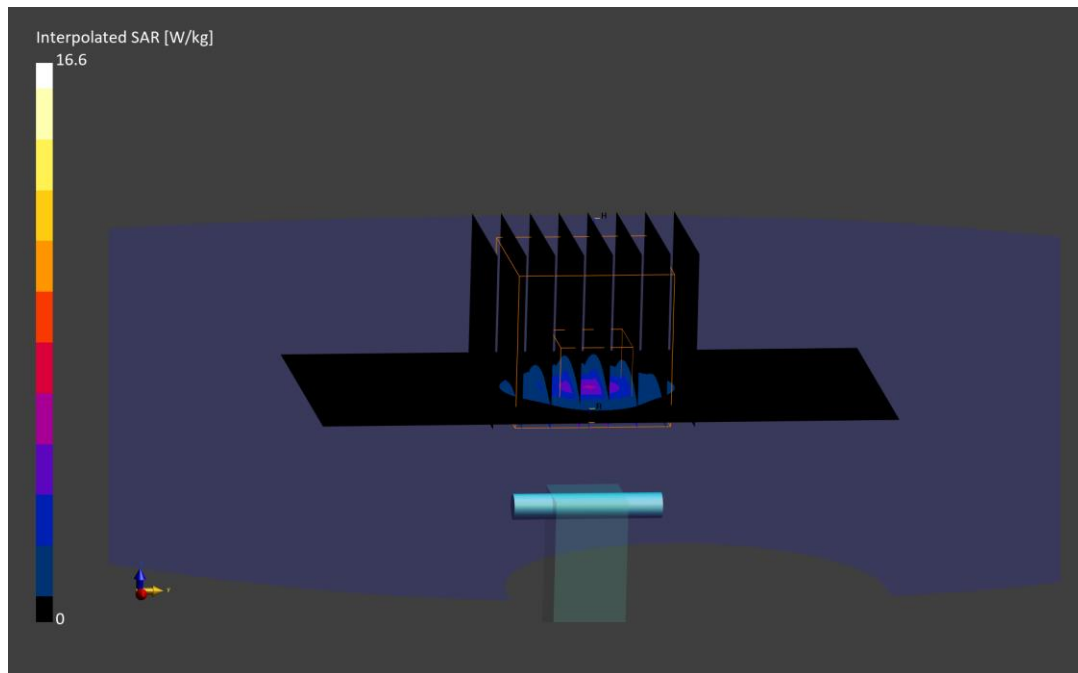

ELEMENT

DUT: Dipole 5750.000 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5750.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
f = 5750.000 MHz; cond = 5.26 S/m; perm = 34.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 10/20/2025; Ambient Temp: 19.5°C; Tissue Temp: 19.2°C

Probe: EX3DV4 - SN7718; ConvF:(5.03,5.02,5.19); Calibrated: 2025-04-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1407; Calibrated: 2025-04-07
Phantom: Twin-SAM V8.0; Serial: 2060
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.5 W/kg

SAR(1 g) = 3.80 W/kg; SAR(10 g) = 1.08 W/kg

Deviation (1 g) = -3.68%; Deviation (10 g) = -3.57%

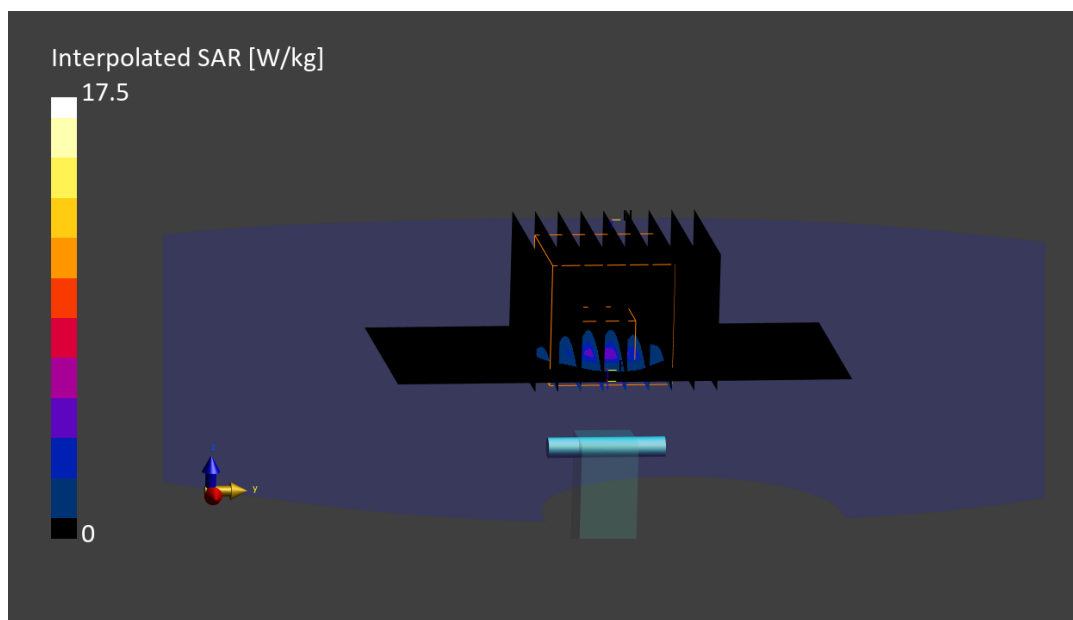

ELEMENT

DUT: Dipole 5750.000 MHz; Type: D5GHzV2 - SN1057

Communication System: UID: 0, CW; Frequency: 5750.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
 $f = 5750.000$ MHz; $\text{cond} = 5.25$ S/m; $\text{perm} = 34.4$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 11/03/2025; Ambient Temp: 20.7°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7661; ConvF:(5.27,5.61,5.61); Calibrated: 2025-06-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1558; Calibrated: 2025-06-05
Phantom: Twin-SAM V8.0; Serial: 2065
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (24.0 x 28.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.8 W/kg

SAR(1 g) = 3.72 W/kg; SAR(10 g) = 1.06 W/kg

Deviation (1 g) = -6.77%; Deviation (10 g) = -6.61%

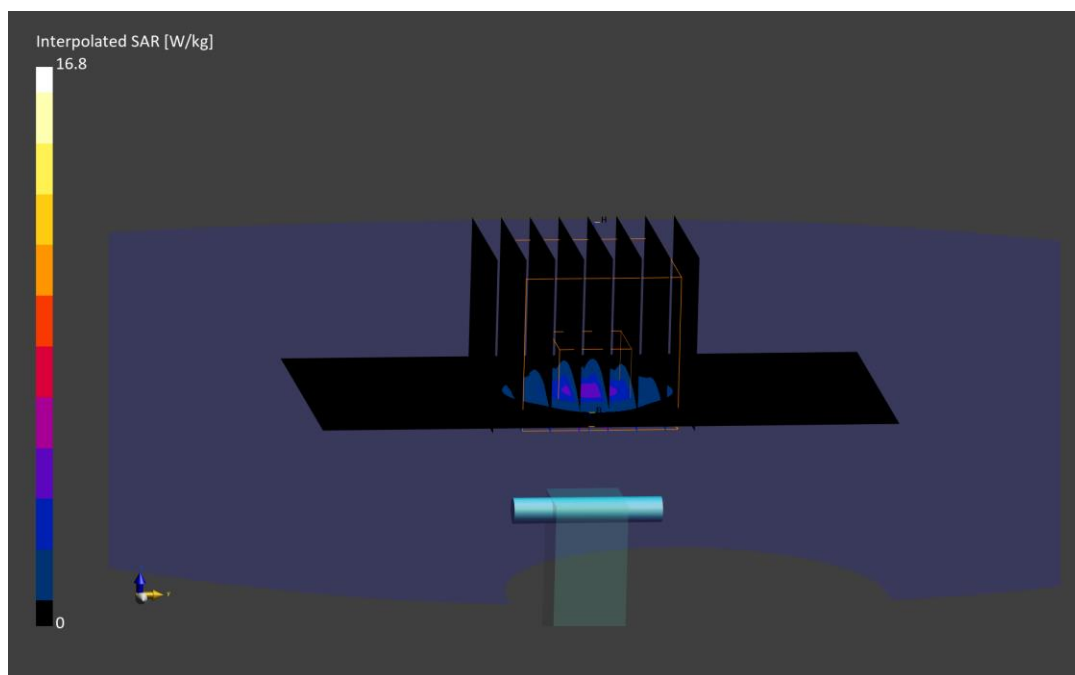

ELEMENT

DUT: Dipole 5850.000 MHz; Type: D5GHzV2 - SN1191

Communication System: UID: 0, CW; Frequency: 5850.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
f = 5850.000 MHz; cond = 5.38 S/m; perm = 33.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 10/20/2025; Ambient Temp: 19.5°C; Tissue Temp: 19.2°C

Probe: EX3DV4 - SN7718; ConvF:(5.03,5.02,5.2); Calibrated: 2025-04-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1407; Calibrated: 2025-04-07
Phantom: Twin-SAM V8.0; Serial: 2060
Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.8 W/kg

SAR(1 g) = 3.80 W/kg; SAR(10 g) = 1.07 W/kg

Deviation (1 g) = -3.55%; Deviation (10 g) = -4.89%

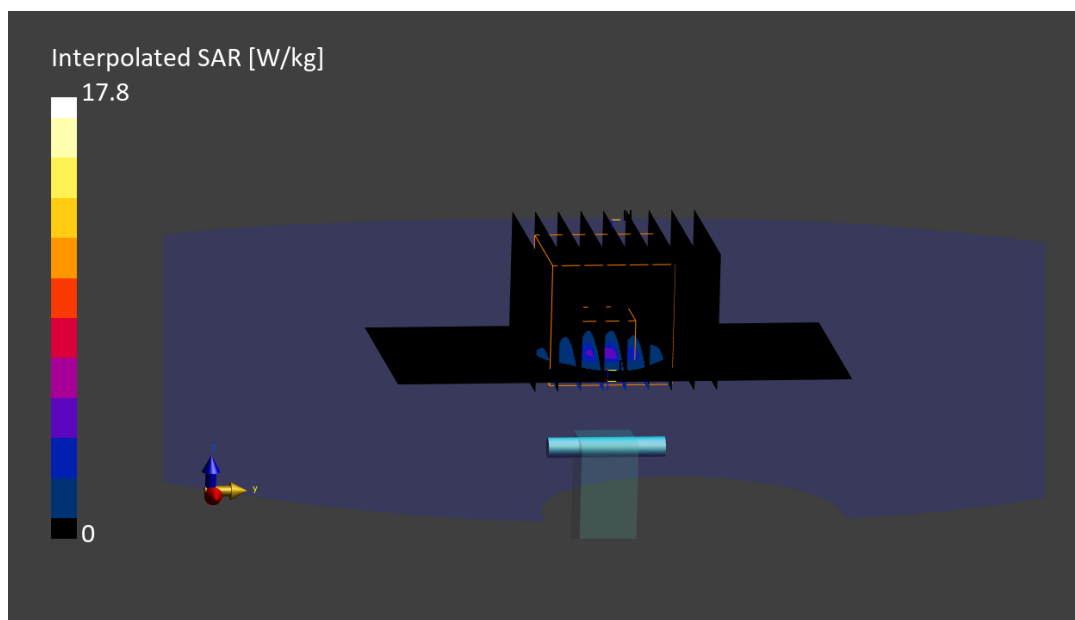

ELEMENT

DUT: Dipole 5850.000 MHz; Type: D5GHzV2 - SN1057

Communication System: UID: 0, CW; Frequency: 5850.000 MHz
Medium: Head Simulating Liquid; Medium parameters used:
f = 5850.000 MHz; cond = 5.36 S/m; perm = 34.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 11/03/2025; Ambient Temp: 20.7°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7661; ConvF:(5.07,5.39,5.38); Calibrated: 2025-06-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1558; Calibrated: 2025-06-05
Phantom: Twin-SAM V8.0; Serial: 2065
Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.7 W/kg

SAR(1 g) = 4.06 W/kg; SAR(10 g) = 1.16 W/kg

Deviation (1 g) = -0.37%; Deviation (10 g) = 0.87%

