

System Check_Head_2450MHz

DUT: D2450V2 - SN929

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_240216 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.80$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(7.67, 7.67, 7.67); Calibrated: 2023-12-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2023-11-17
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.14 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.44 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

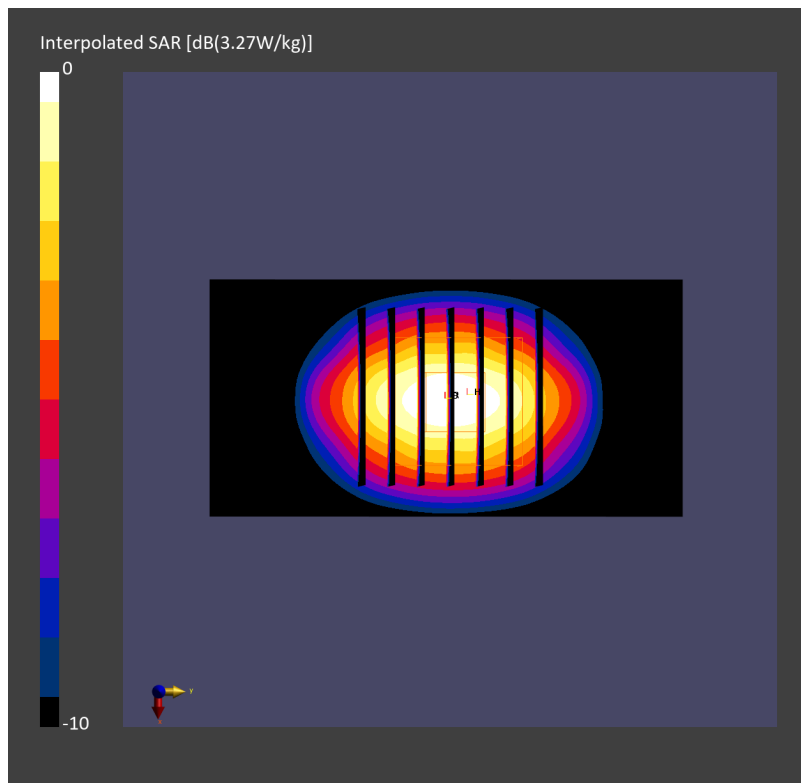

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_240217 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.63$ S/m; $\epsilon_r = 36.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(5.48, 5.48, 5.48); Calibrated: 2023-12-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2023-11-17
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.54 W/kg; SAR (10g) = 1.01 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.81 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.4 %

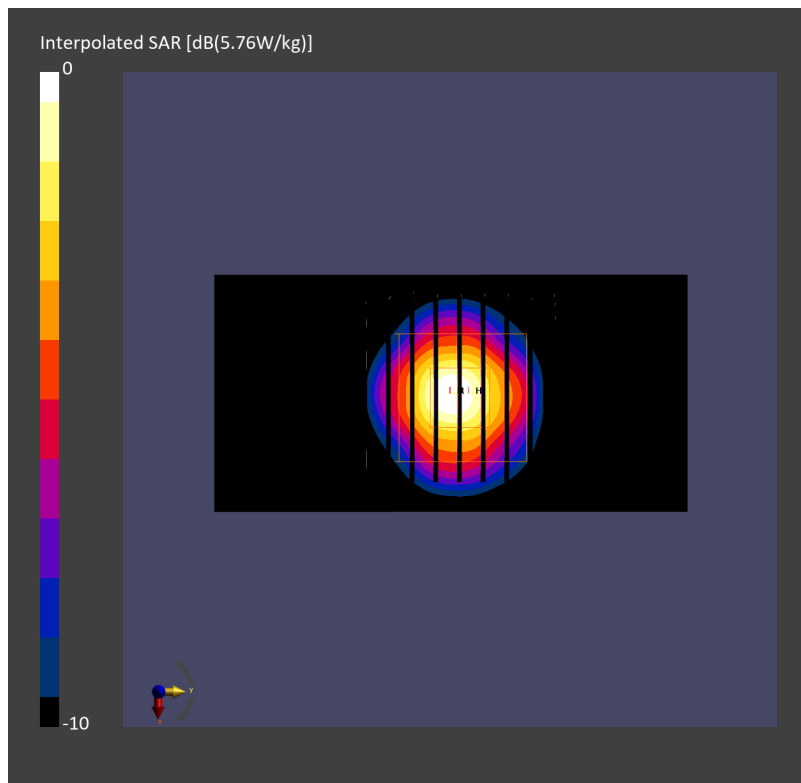

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_240217 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.97$ S/m; $\epsilon_r = 36.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(4.87, 4.87, 4.87); Calibrated: 2023-12-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2023-11-17
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.97 W/kg; SAR (10g) = 1.13 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.05 dB

SAR (1g) = 4.25 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.0 %

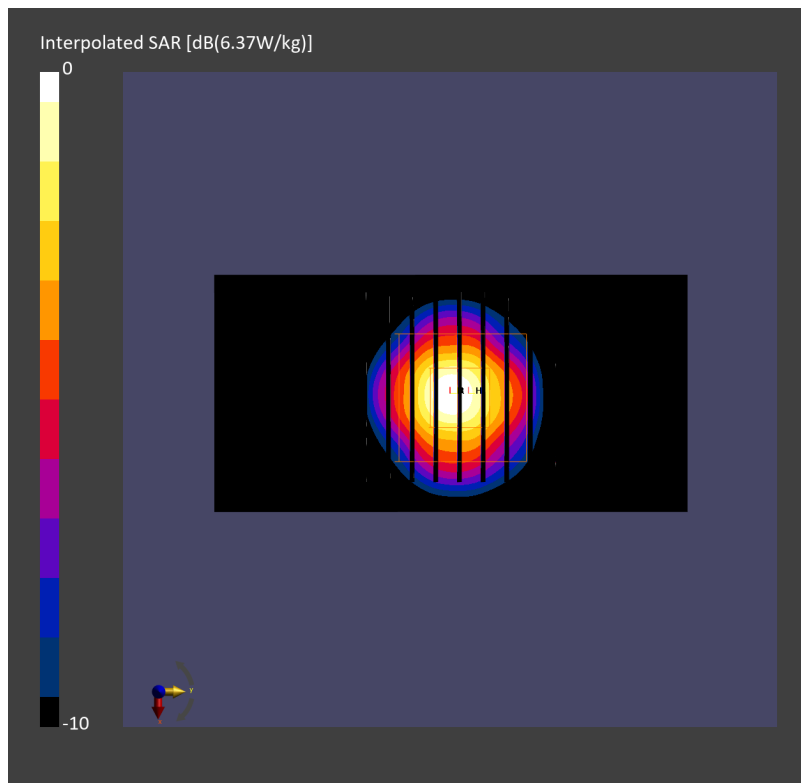

System Check_Head_5750MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_240217 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.12$ S/m; $\epsilon_r = 36.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(4.96, 4.96, 4.96); Calibrated: 2023-12-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2023-11-17
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.43 W/kg; SAR (10g) = 0.964 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.72 W/kg; SAR (8g) = 1.23 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 59.3 %

