

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260327 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.914$ S/m; $\epsilon_r = 45.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(9.16, 9.01, 9.31); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.19 W/kg; SAR (10g) = 1.46 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.18 W/kg; SAR (8g) = 1.52 W/kg; SAR (10g) = 1.44 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.1 %

TSL Correction: Positive only

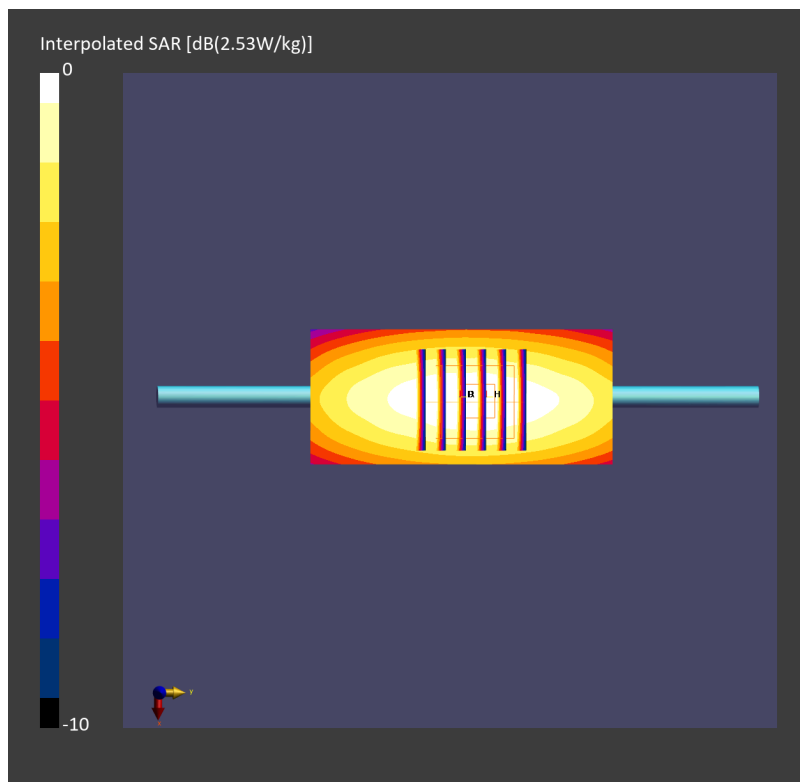

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260328 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.839$ S/m; $\epsilon_r = 44.1$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(9.16, 9.01, 9.31); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.40 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 2.12 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.39 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

TSL Correction: Positive only

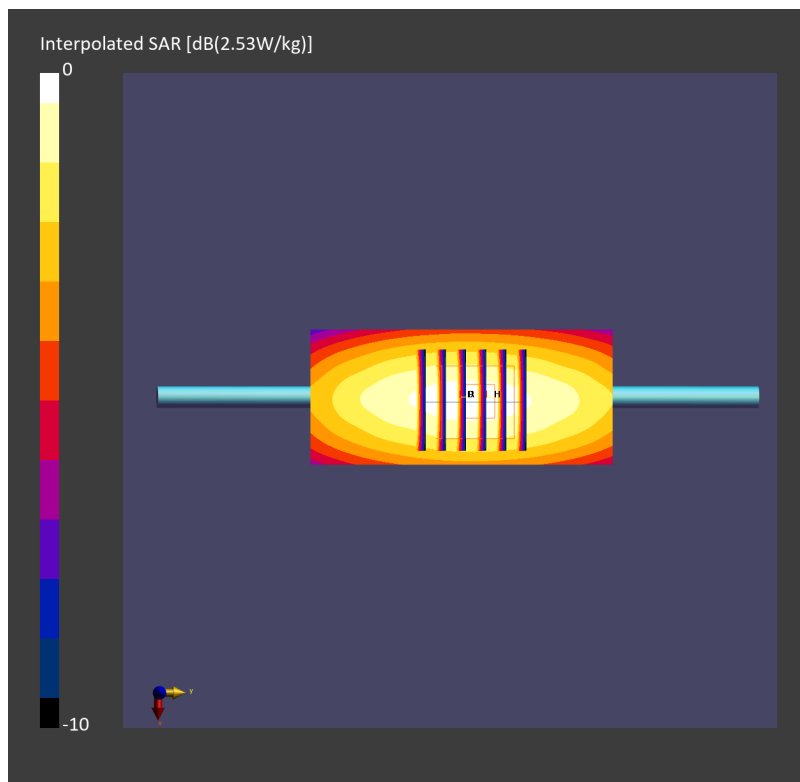

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260327 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.944$ S/m; $\epsilon_r = 44.8$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(9.03, 8.87, 9.17); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.61 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.04 dB

SAR (1g) = 2.42 W/kg; SAR (8g) = 1.67 W/kg; SAR (10g) = 1.59 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 86.8 %

TSL Correction: Positive only

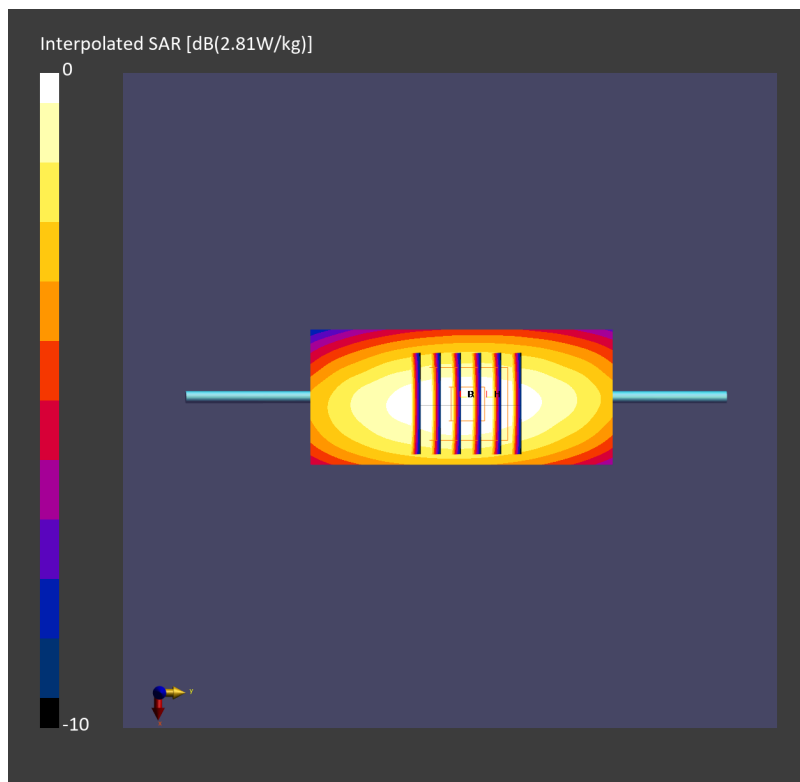

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260328 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.893$ S/m; $\epsilon_r = 43.8$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(9.03, 8.87, 9.17); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.34 W/kg; SAR (10g) = 1.54 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.34 W/kg; SAR (8g) = 1.61 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = 16.1 mm

Ratio of SAR at M2 to SAR at M1 = 87.7 %

TSL Correction: Positive only

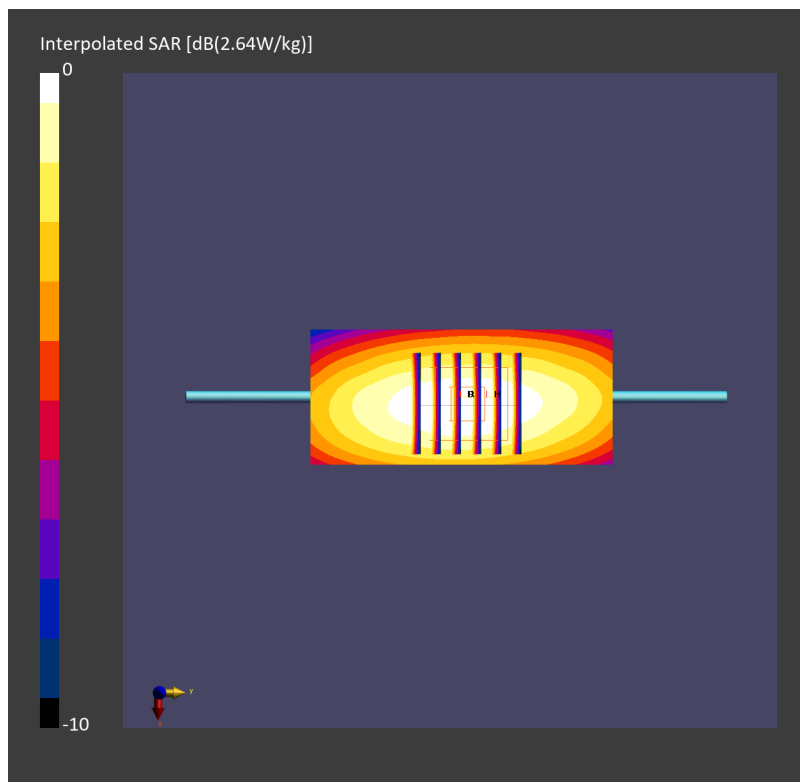

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260329 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.41, 7.28, 7.53); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.50 W/kg; SAR (10g) = 4.52 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 8.40 W/kg; SAR (8g) = 4.85 W/kg; SAR (10g) = 4.47 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

TSL Correction: Positive only

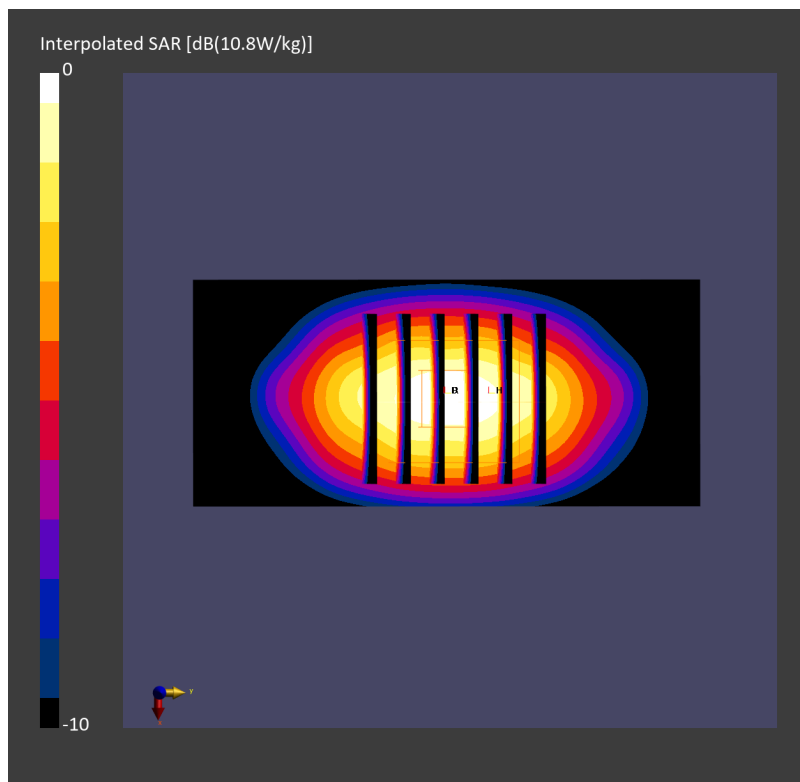

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260330 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.33$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.41, 7.28, 7.53); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.50 W/kg; SAR (10g) = 4.49 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 8.52 W/kg; SAR (8g) = 4.85 W/kg; SAR (10g) = 4.48 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.0 %

TSL Correction: Positive only

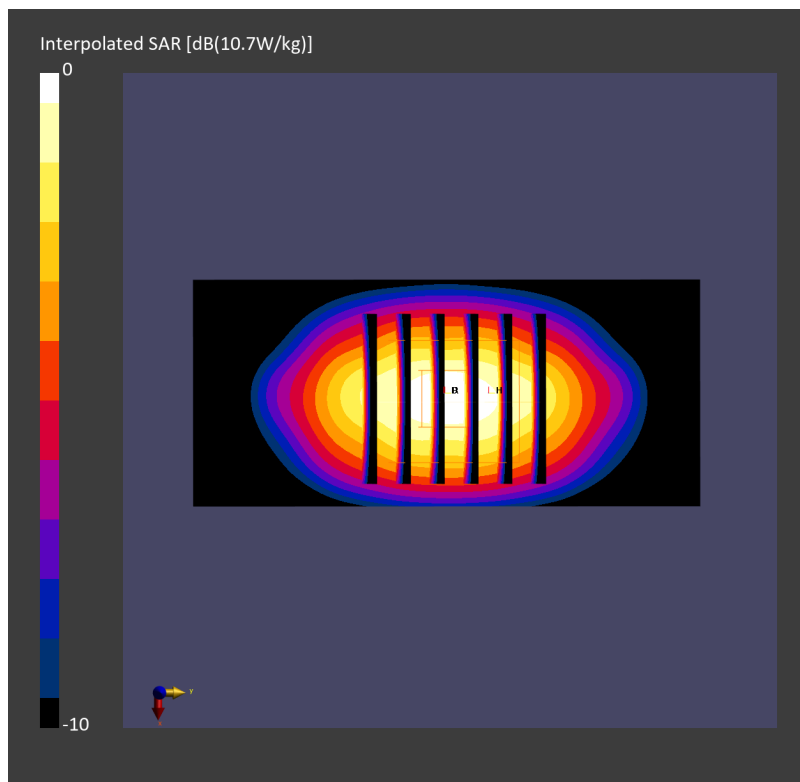

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260401 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.41, 7.28, 7.53); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.62 W/kg; SAR (10g) = 4.58 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 8.61 W/kg; SAR (8g) = 4.96 W/kg; SAR (10g) = 4.57 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.4 %

TSL Correction: Positive only

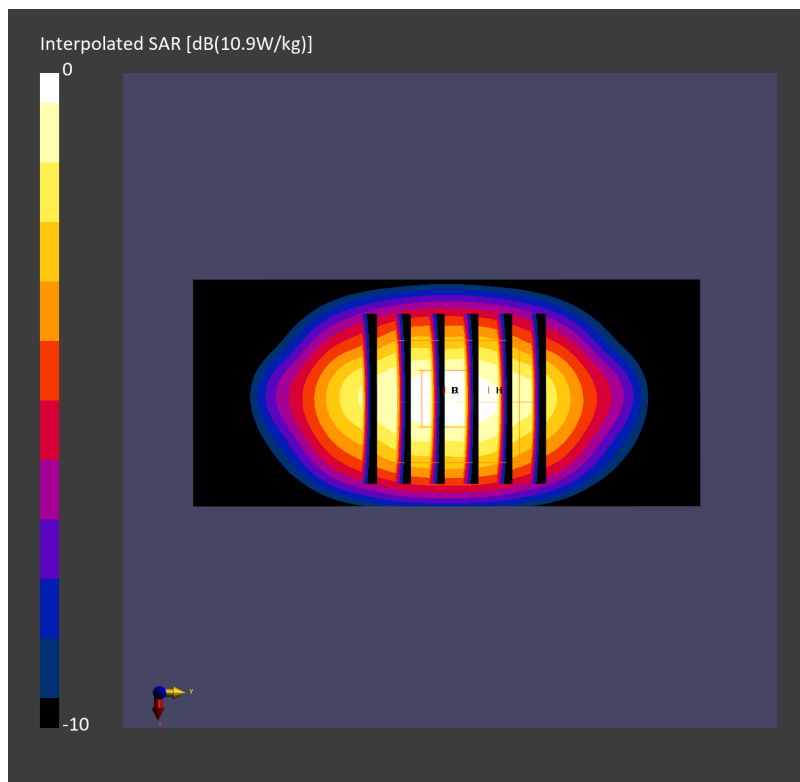

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260402 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.41, 7.28, 7.53); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.74 W/kg; SAR (10g) = 4.65 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 8.71 W/kg; SAR (8g) = 5.04 W/kg; SAR (10g) = 4.65 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

TSL Correction: Positive only

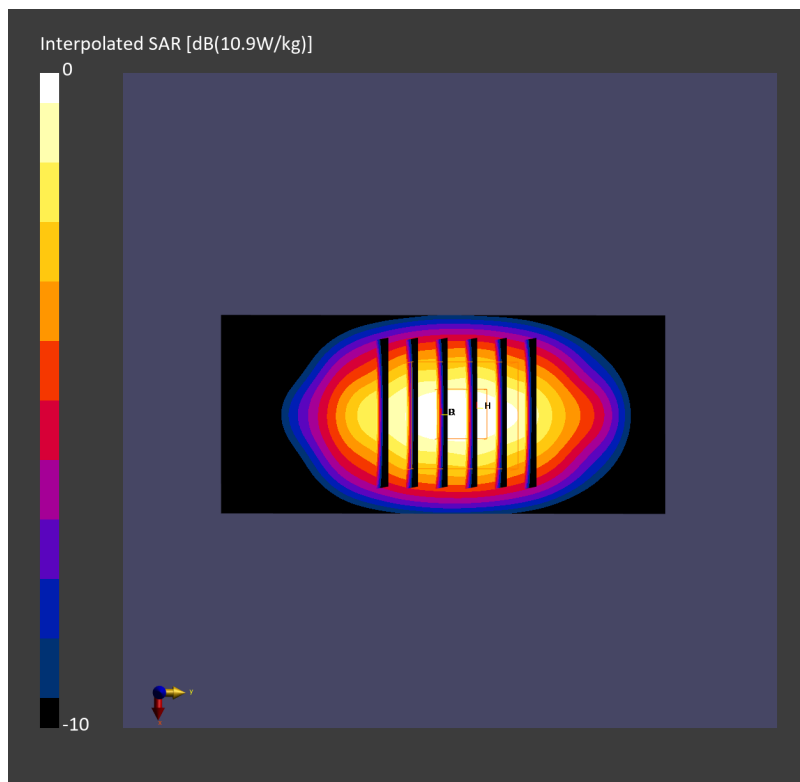

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260403 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.41, 7.28, 7.53); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.59 W/kg; SAR (10g) = 4.72 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 8.87 W/kg; SAR (8g) = 5.11 W/kg; SAR (10g) = 4.71 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

TSL Correction: Positive only

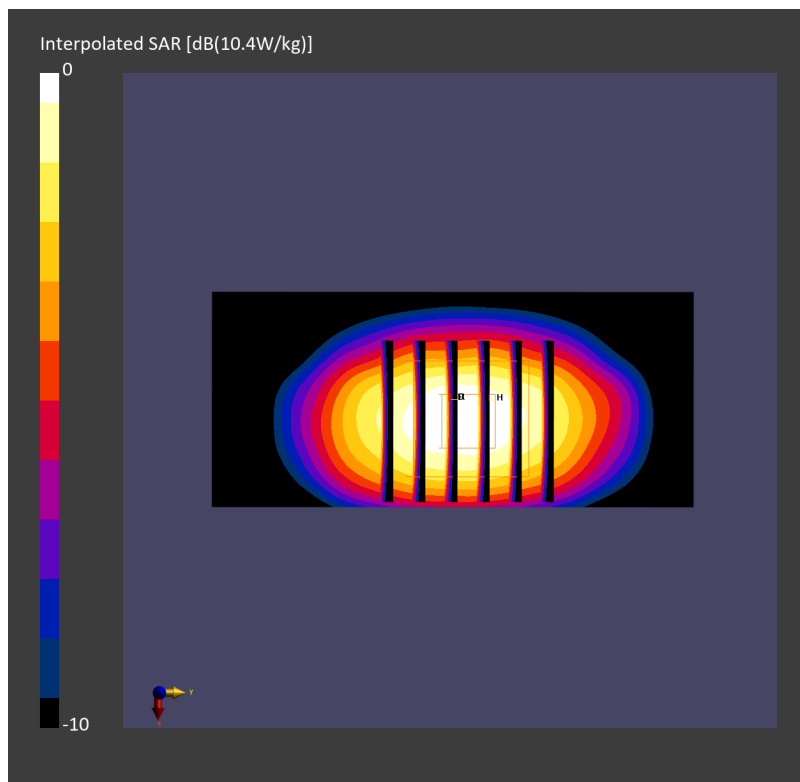

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260404 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 42.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.41, 7.28, 7.53); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.88 W/kg; SAR (10g) = 4.75 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 8.91 W/kg; SAR (8g) = 5.14 W/kg; SAR (10g) = 4.74 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.2 %

TSL Correction: Positive only

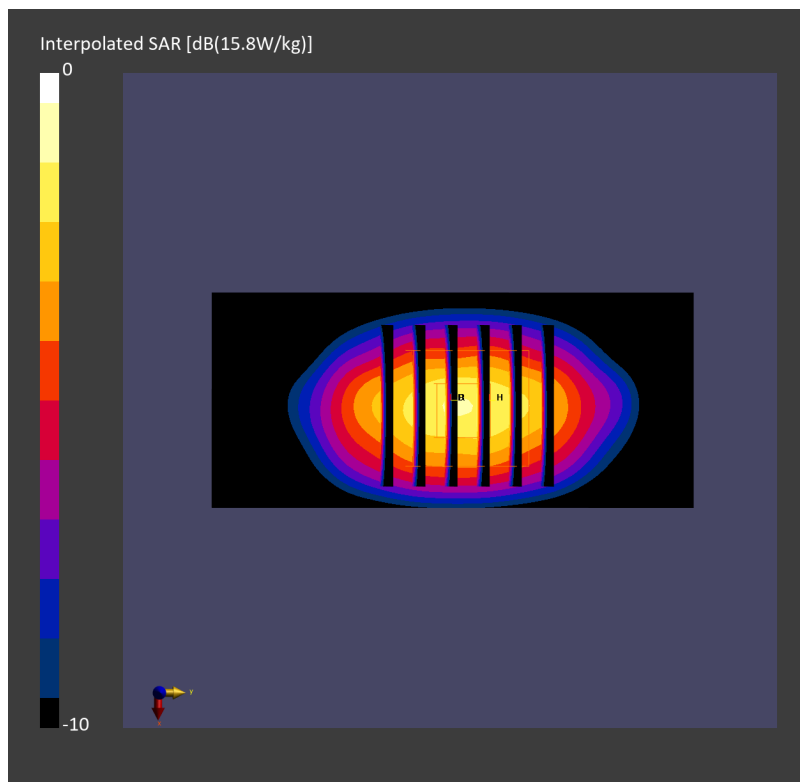

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260329 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.24, 7.11, 7.35); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.5 W/kg; SAR (10g) = 5.44 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 10.5 W/kg; SAR (8g) = 5.94 W/kg; SAR (10g) = 5.46 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.0 %

TSL Correction: Positive only

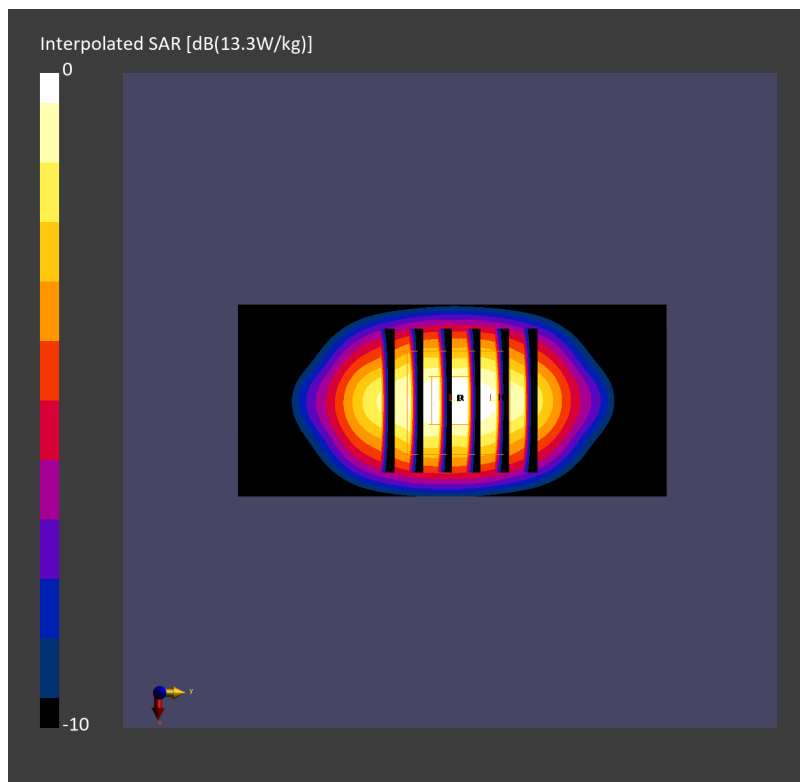

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260330 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 42.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.24, 7.11, 7.35); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.1 W/kg; SAR (10g) = 5.21 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 10.0 W/kg; SAR (8g) = 5.68 W/kg; SAR (10g) = 5.23 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.8 %

TSL Correction: Positive only

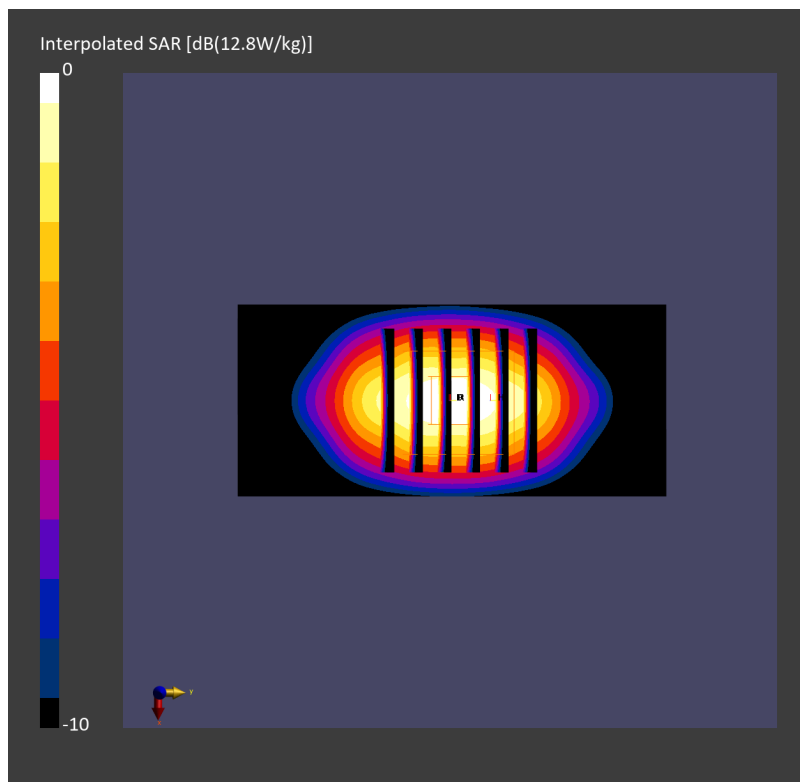

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260401 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.24, 7.11, 7.35); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.5 W/kg; SAR (10g) = 5.49 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 10.5 W/kg; SAR (8g) = 5.97 W/kg; SAR (10g) = 5.48 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

TSL Correction: Positive only

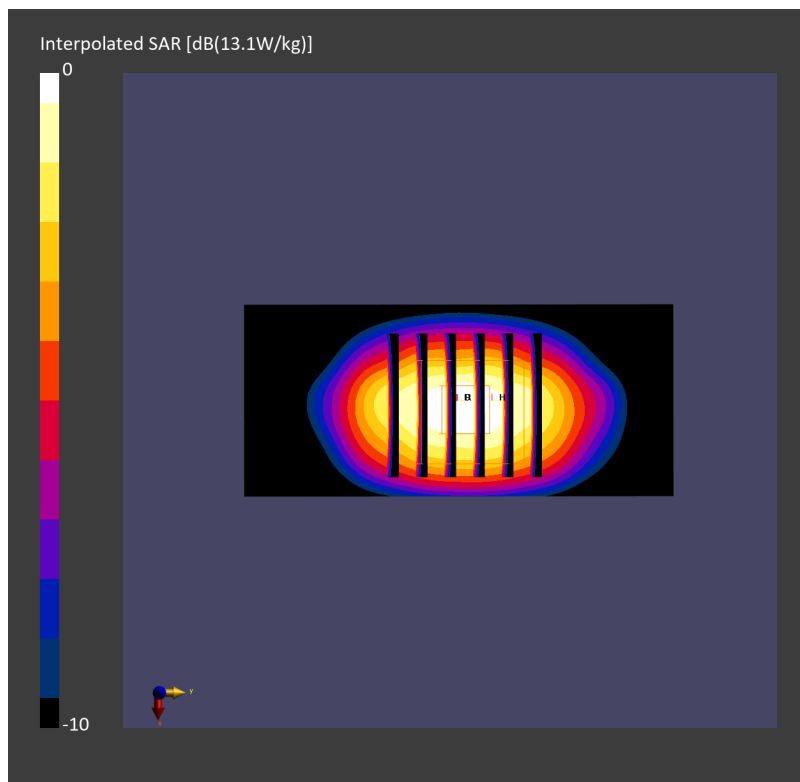

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260402 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.24, 7.11, 7.35); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.6 W/kg; SAR (10g) = 5.45 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 10.5 W/kg; SAR (8g) = 5.96 W/kg; SAR (10g) = 5.48 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

TSL Correction: Positive only

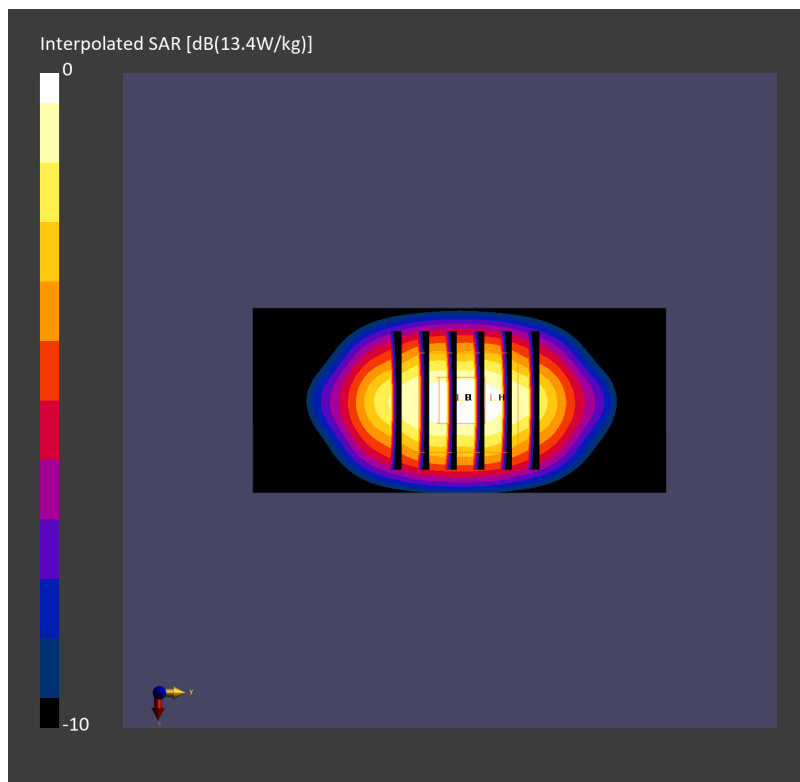

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260403 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.24, 7.11, 7.35); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.4 W/kg; SAR (10g) = 5.41 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 10.3 W/kg; SAR (8g) = 5.88 W/kg; SAR (10g) = 5.41 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.0 %

TSL Correction: Positive only

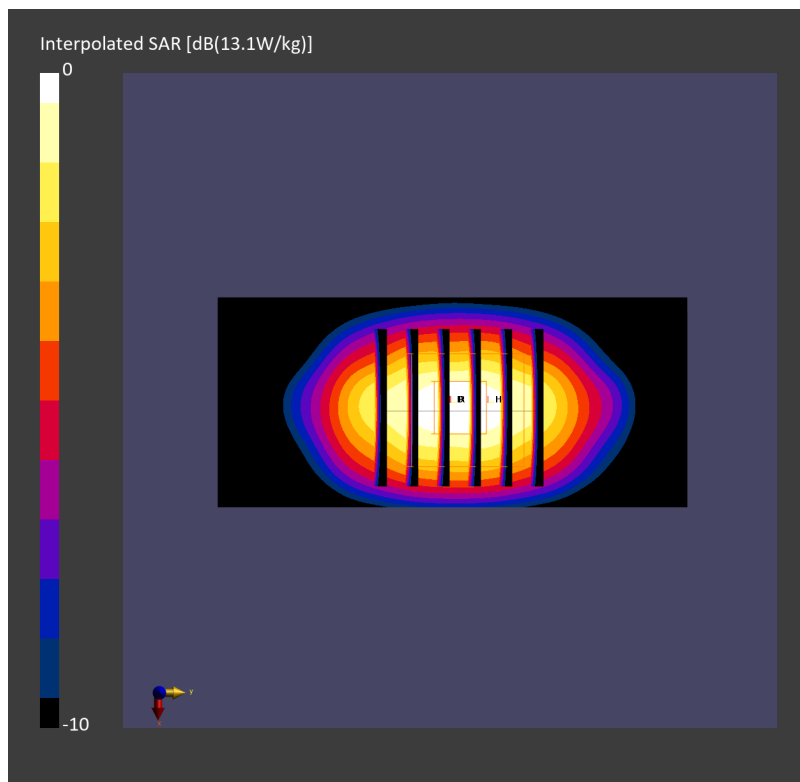

System Check_Head_1900MHz

DUT: D1900V2 - SN5d093

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260404 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(7.24, 7.11, 7.35); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.0 W/kg; SAR (10g) = 5.20 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 9.97 W/kg; SAR (8g) = 5.66 W/kg; SAR (10g) = 5.20 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.2 %

TSL Correction: Positive only

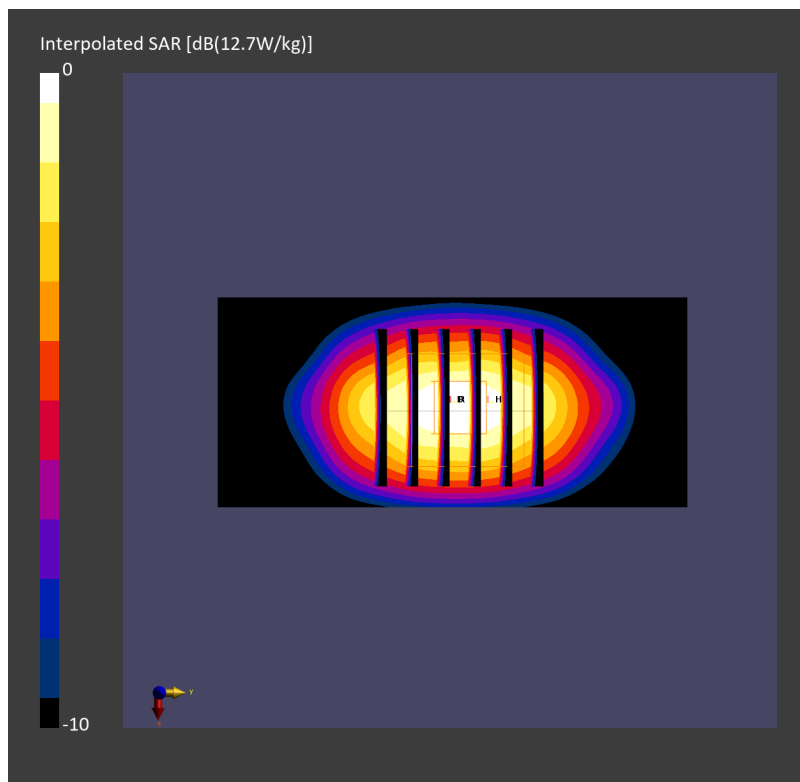

System Check_Head_2300MHz

DUT: D2300V2 - SN1088

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260405 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.76$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.82, 6.71, 6.93); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.6 W/kg; SAR (10g) = 5.97 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 12.4 W/kg; SAR (8g) = 6.53 W/kg; SAR (10g) = 5.94 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 81.6 %

TSL Correction: Positive only

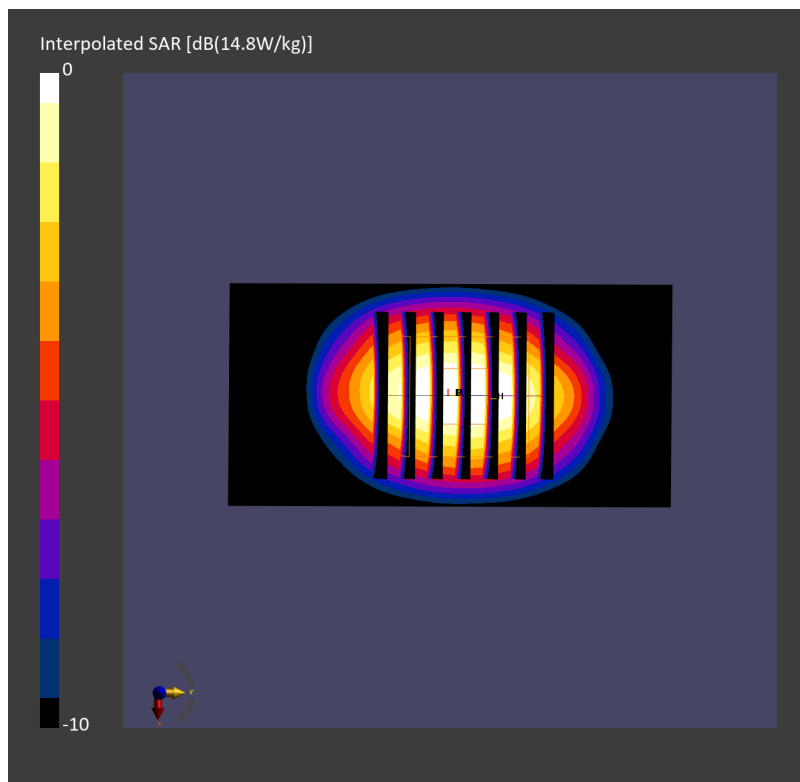

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260406 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.46, 6.35, 6.56); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.8 W/kg; SAR (10g) = 6.70 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 14.9 W/kg; SAR (8g) = 7.39 W/kg; SAR (10g) = 6.66 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

TSL Correction: Positive only

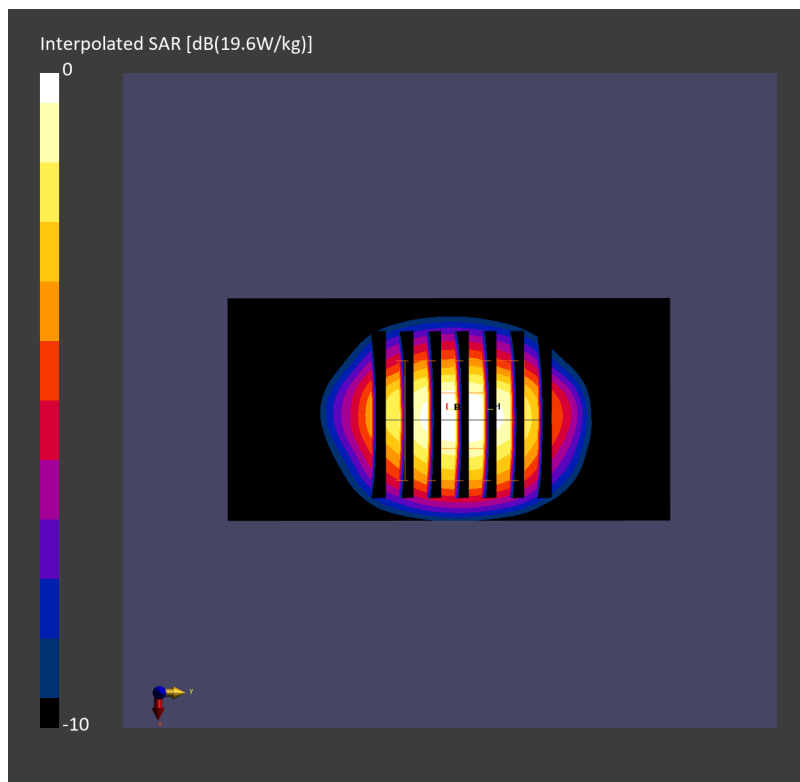

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260407 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.46, 6.35, 6.56); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.3 W/kg; SAR (10g) = 6.40 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 14.3 W/kg; SAR (8g) = 7.04 W/kg; SAR (10g) = 6.35 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

TSL Correction: Positive only

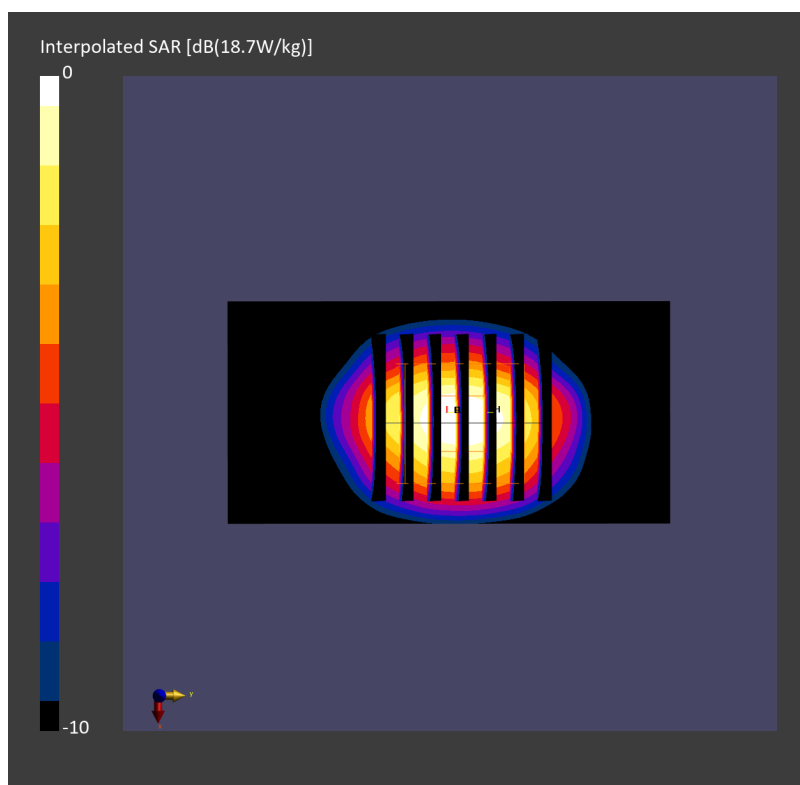

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260408 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.46, 6.35, 6.56); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.5 W/kg; SAR (10g) = 6.53 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 14.5 W/kg; SAR (8g) = 7.17 W/kg; SAR (10g) = 6.46 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.8 %

TSL Correction: Positive only

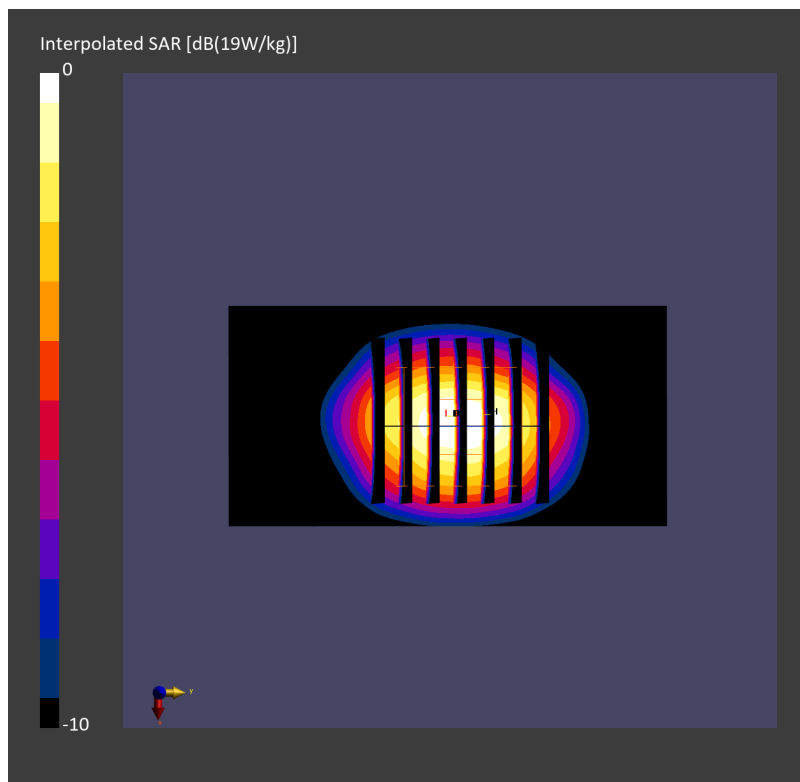

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260409 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.46, 6.35, 6.56); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.5 W/kg; SAR (10g) = 6.56 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 14.5 W/kg; SAR (8g) = 7.20 W/kg; SAR (10g) = 6.49 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

TSL Correction: Positive only

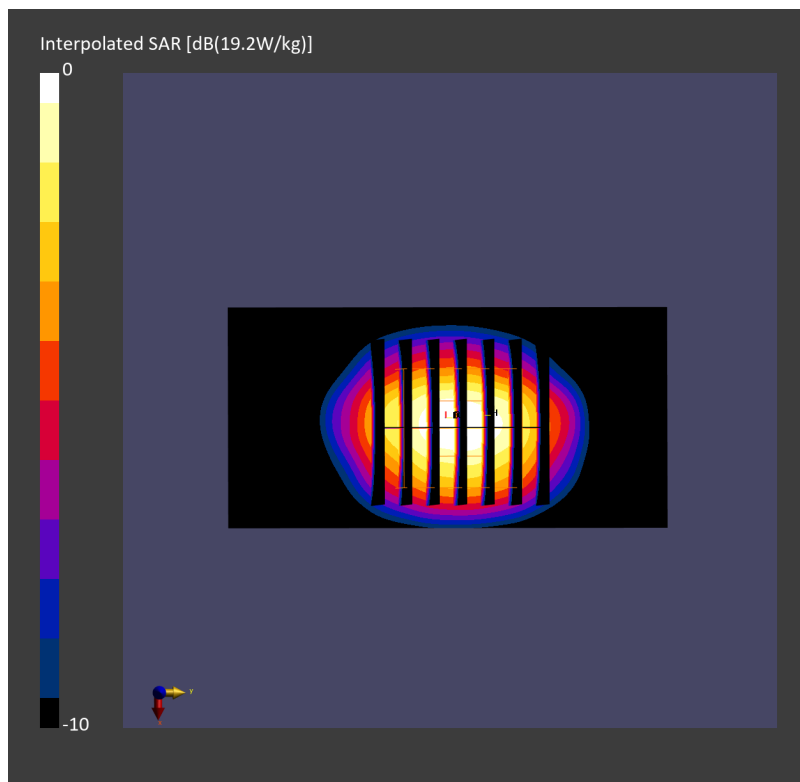

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260410 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.46, 6.35, 6.56); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.6 W/kg; SAR (10g) = 6.53 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 14.4 W/kg; SAR (8g) = 7.15 W/kg; SAR (10g) = 6.44 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.6 %

TSL Correction: Positive only

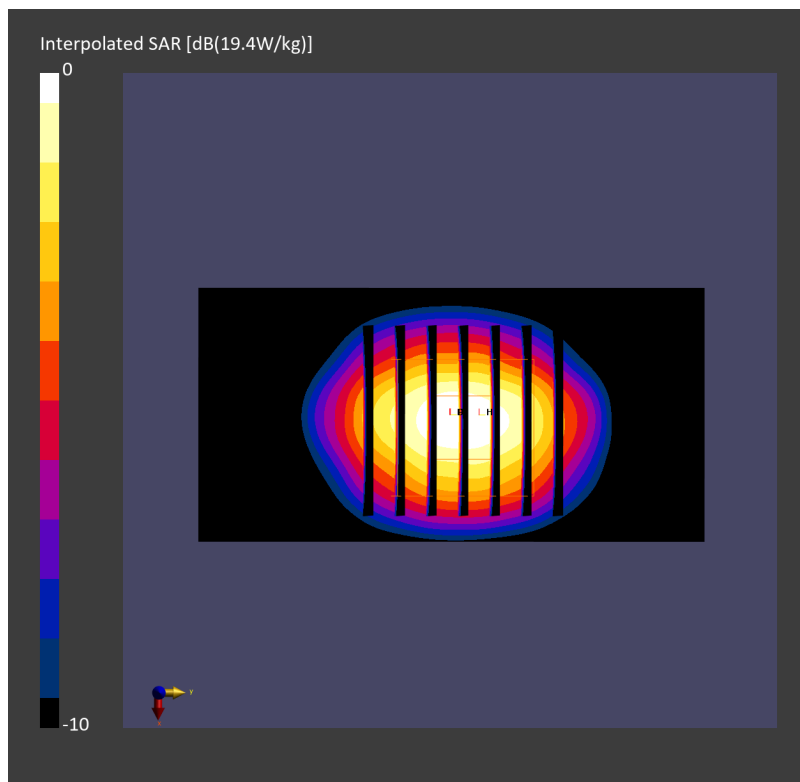

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260411 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.74$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.07, 5.97, 6.17); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 16.7 W/kg; SAR (10g) = 6.39 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.06 dB

SAR (1g) = 17.6 W/kg; SAR (8g) = 7.56 W/kg; SAR (10g) = 6.70 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

TSL Correction: Positive only

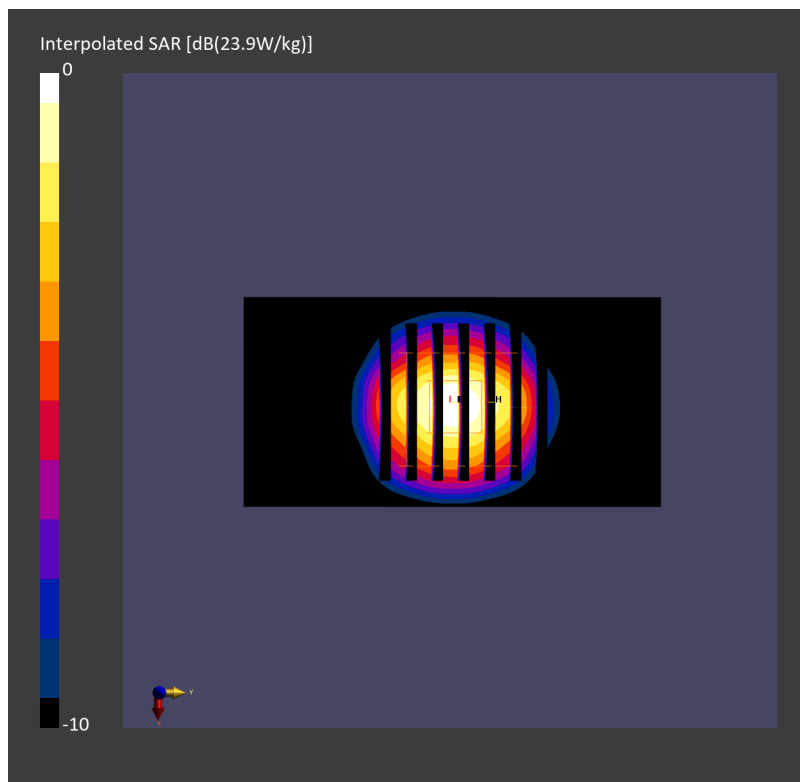

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260412 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.73$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.07, 5.97, 6.17); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.3 W/kg; SAR (10g) = 6.58 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 17.6 W/kg; SAR (8g) = 7.60 W/kg; SAR (10g) = 6.73 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.4 %

TSL Correction: Positive only

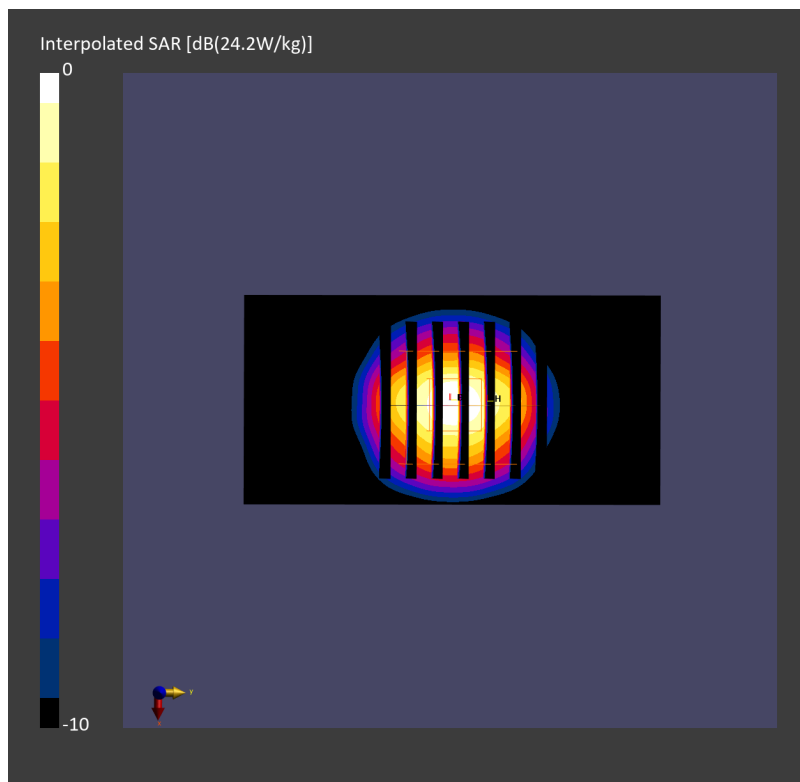

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260413 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.74$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.07, 5.97, 6.17); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 16.9 W/kg; SAR (10g) = 6.43 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 17.3 W/kg; SAR (8g) = 7.45 W/kg; SAR (10g) = 6.61 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

TSL Correction: Positive only

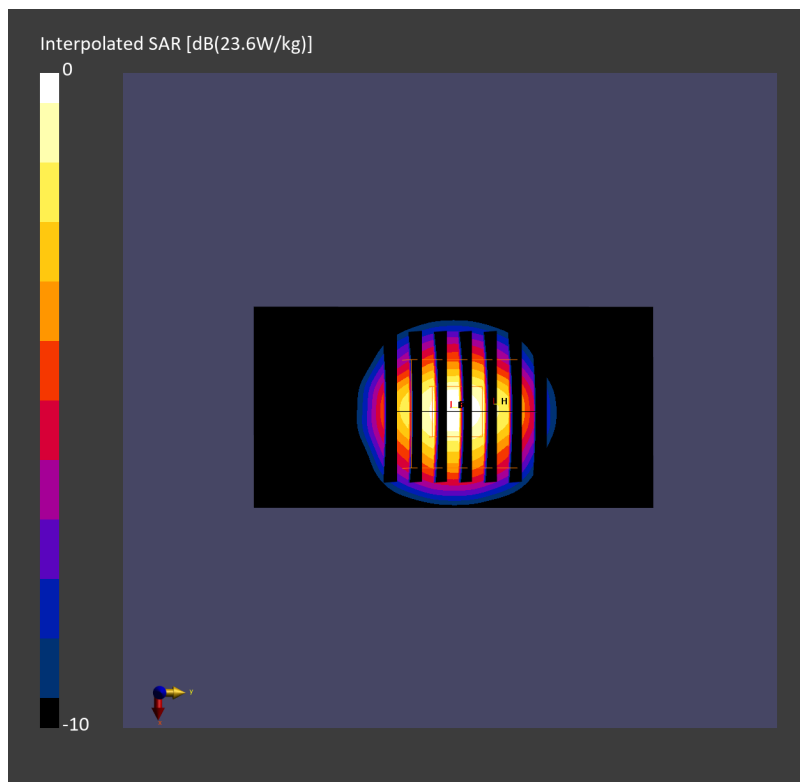

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.83$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.07, 5.97, 6.17); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.6 W/kg; SAR (10g) = 6.70 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 17.8 W/kg; SAR (8g) = 7.73 W/kg; SAR (10g) = 6.83 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

TSL Correction: Positive only

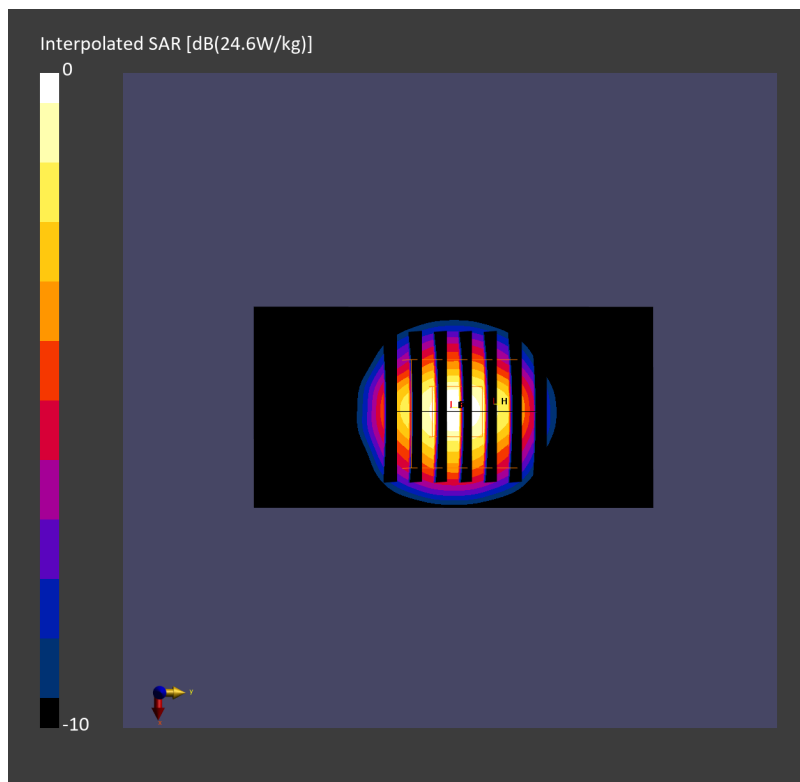

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.84$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.07, 5.97, 6.17); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.5 W/kg; SAR (10g) = 6.71 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 17.5 W/kg; SAR (8g) = 7.57 W/kg; SAR (10g) = 6.72 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.4 %

TSL Correction: Positive only

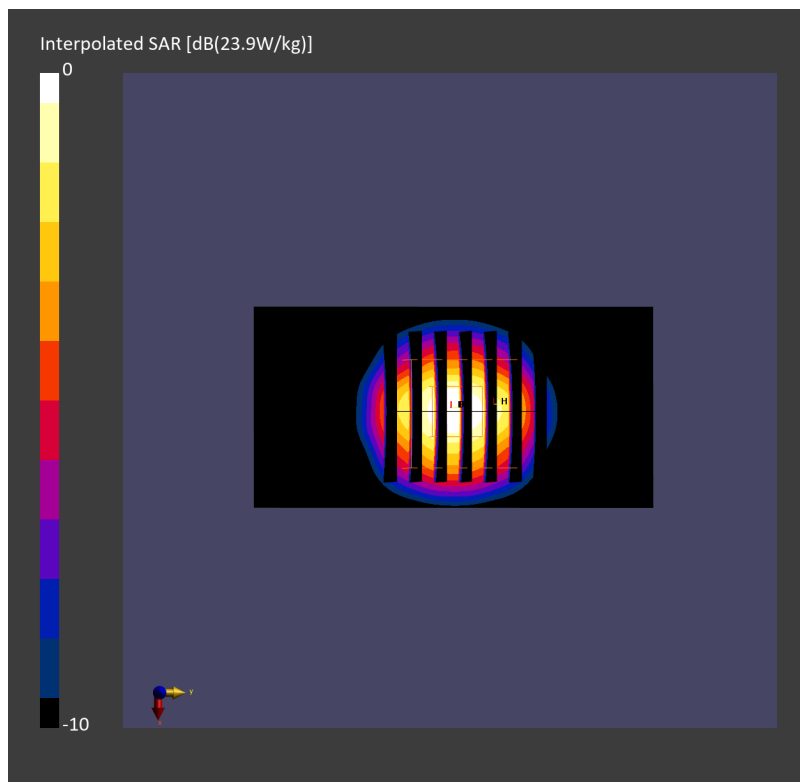

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260418 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.72$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.07, 5.97, 6.17); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 16.3 W/kg; SAR (10g) = 6.18 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 16.6 W/kg; SAR (8g) = 7.14 W/kg; SAR (10g) = 6.33 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

TSL Correction: Positive only

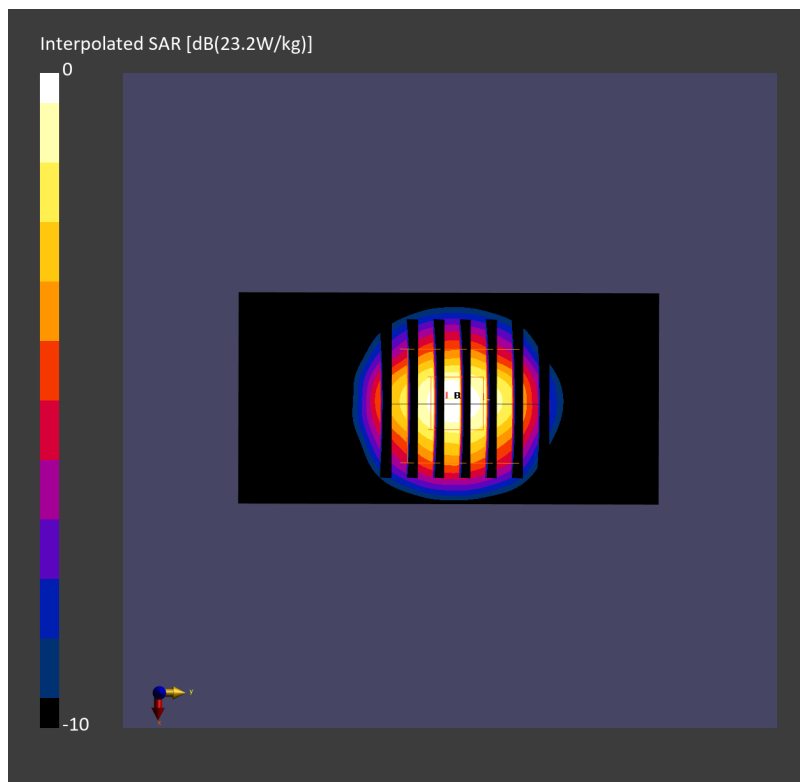

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260411 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.89$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.01, 5.91, 6.11); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.2 W/kg; SAR (10g) = 6.38 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.08 dB

SAR (1g) = 17.7 W/kg; SAR (8g) = 7.42 W/kg; SAR (10g) = 6.55 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

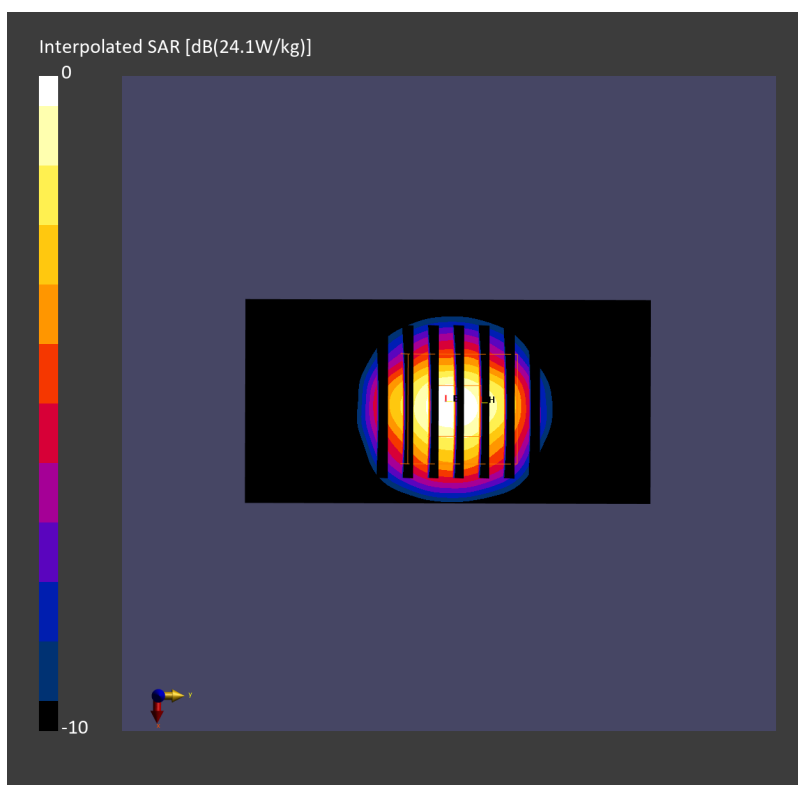

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260412 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.90$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.01, 5.91, 6.11); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.1 W/kg; SAR (10g) = 6.39 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 17.6 W/kg; SAR (8g) = 7.43 W/kg; SAR (10g) = 6.56 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.2 %

TSL Correction: Positive only

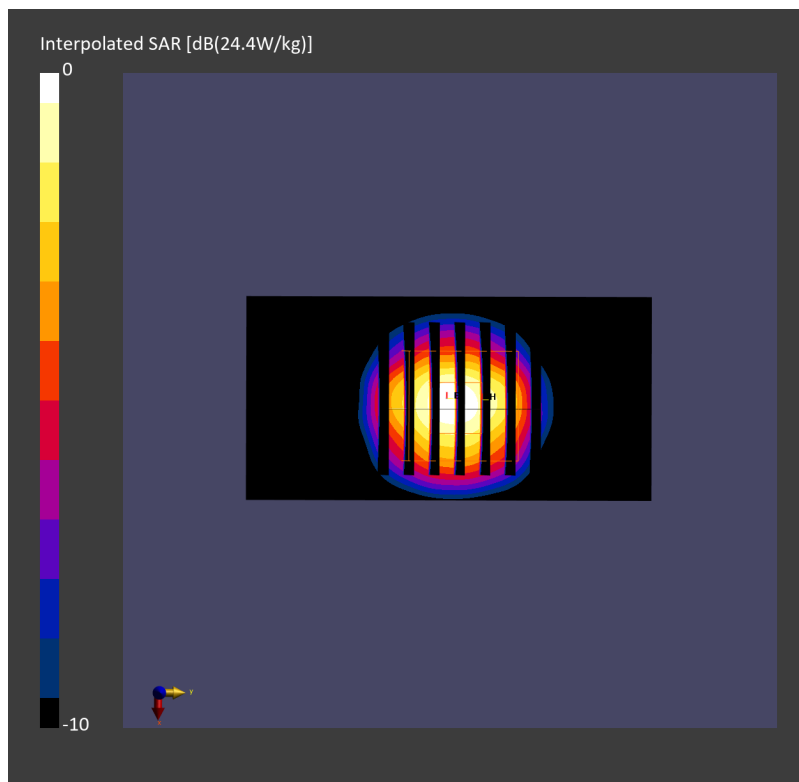

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260414 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.01, 5.91, 6.11); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.3 W/kg; SAR (10g) = 6.47 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 17.9 W/kg; SAR (8g) = 7.52 W/kg; SAR (10g) = 6.64 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

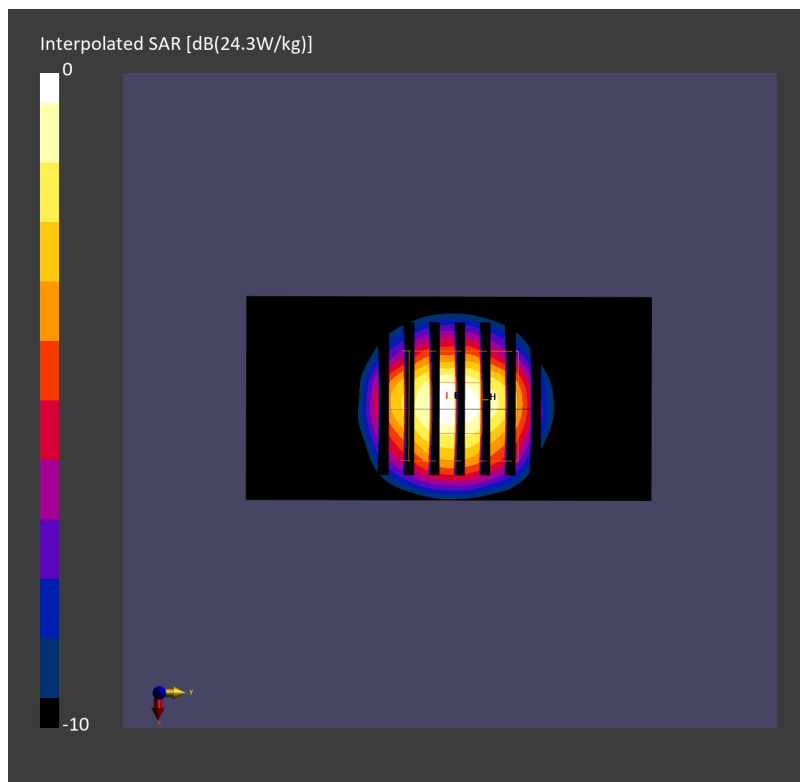

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.02$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.01, 5.91, 6.11); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 18.0 W/kg; SAR (10g) = 6.74 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 18.3 W/kg; SAR (8g) = 7.73 W/kg; SAR (10g) = 6.79 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

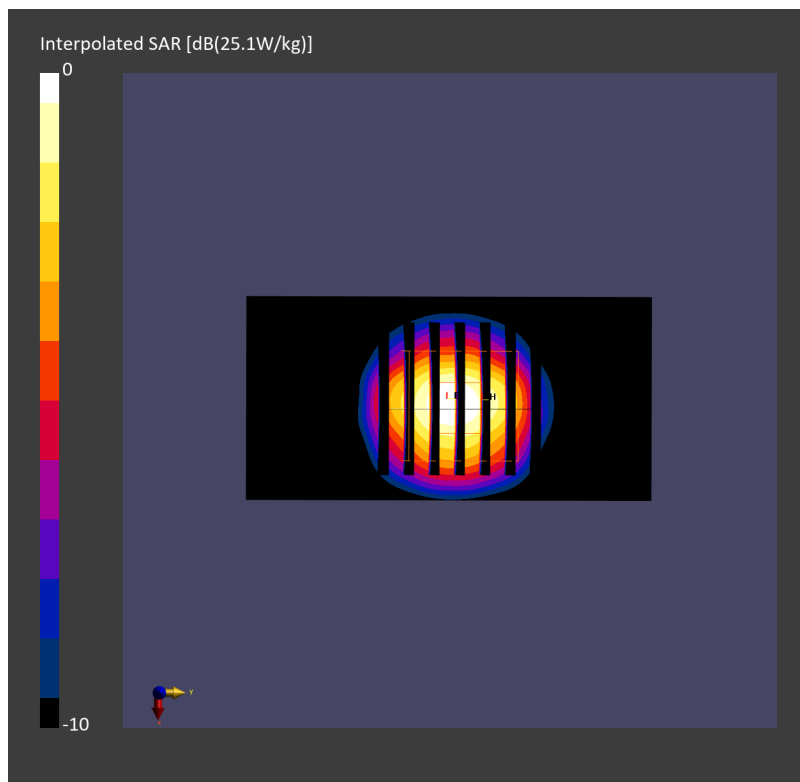

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.03$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.01, 5.91, 6.11); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 18.0 W/kg; SAR (10g) = 6.75 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 18.5 W/kg; SAR (8g) = 7.81 W/kg; SAR (10g) = 6.90 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

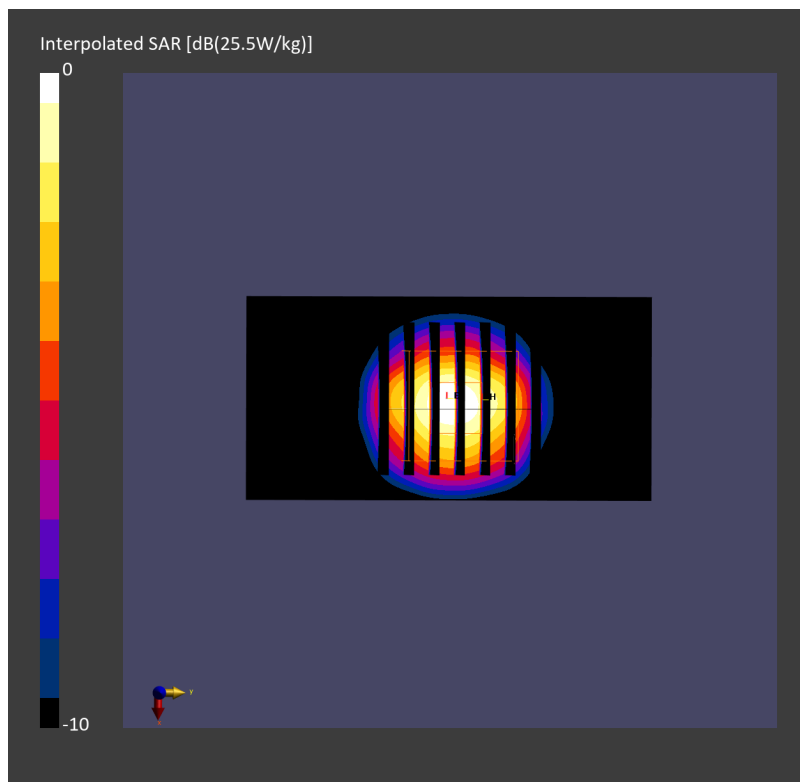

System Check_Head_3700MHz

DUT: D3700V2 - SN1022

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260418 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.86$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.01, 5.91, 6.11); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 16.5 W/kg; SAR (10g) = 6.12 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 17.0 W/kg; SAR (8g) = 7.10 W/kg; SAR (10g) = 6.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

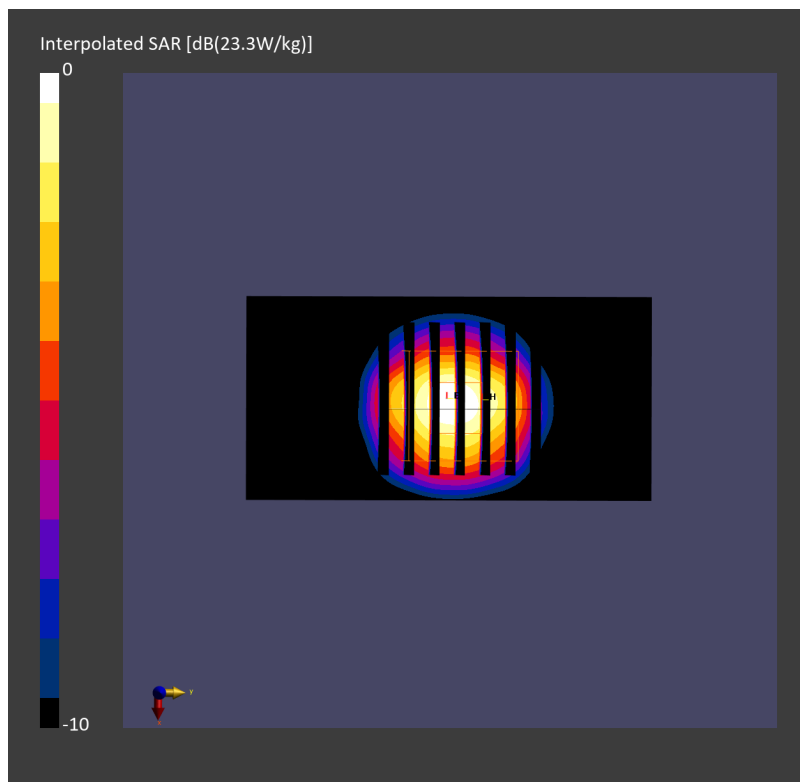

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260414 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(5.94, 5.83, 6.03); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 15.5 W/kg; SAR (10g) = 5.48 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.07 dB

SAR (1g) = 17.8 W/kg; SAR (8g) = 7.14 W/kg; SAR (10g) = 6.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.2 %

TSL Correction: Positive only

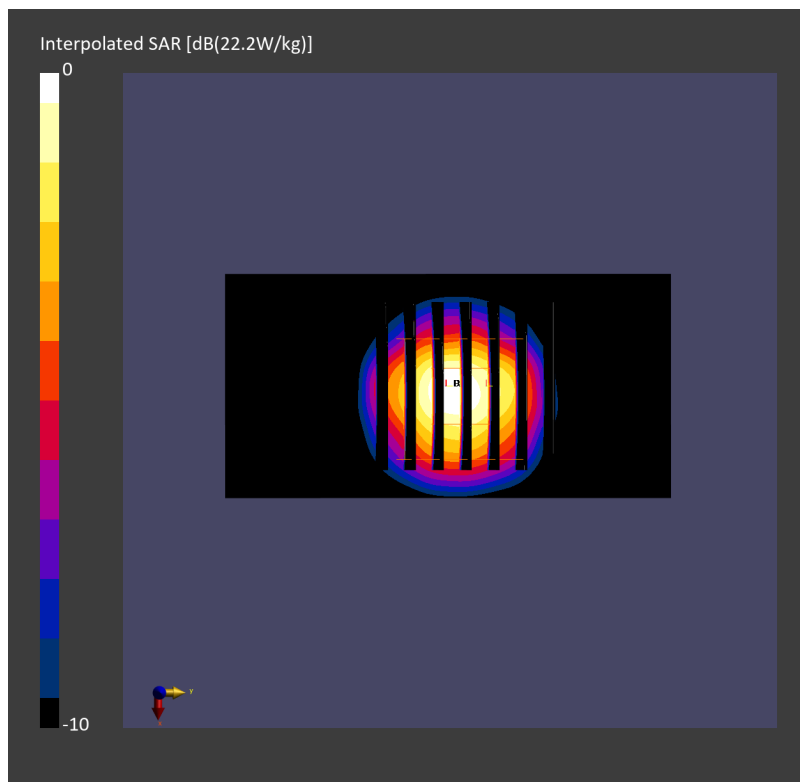

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260415 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.22$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(5.94, 5.83, 6.03); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.4 W/kg; SAR (10g) = 6.21 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.14 dB

SAR (1g) = 17.6 W/kg; SAR (8g) = 7.06 W/kg; SAR (10g) = 6.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.9 %

TSL Correction: Positive only

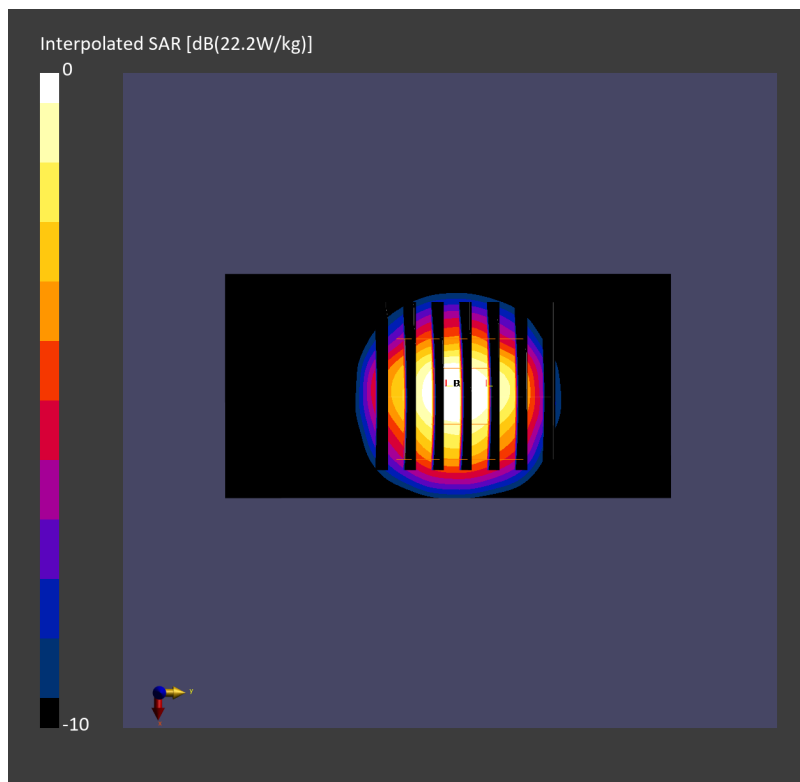

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260416 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.23$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(5.94, 5.83, 6.03); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 16.0 W/kg; SAR (10g) = 5.75 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 18.7 W/kg; SAR (8g) = 7.51 W/kg; SAR (10g) = 6.59 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.0 %

TSL Correction: Positive only

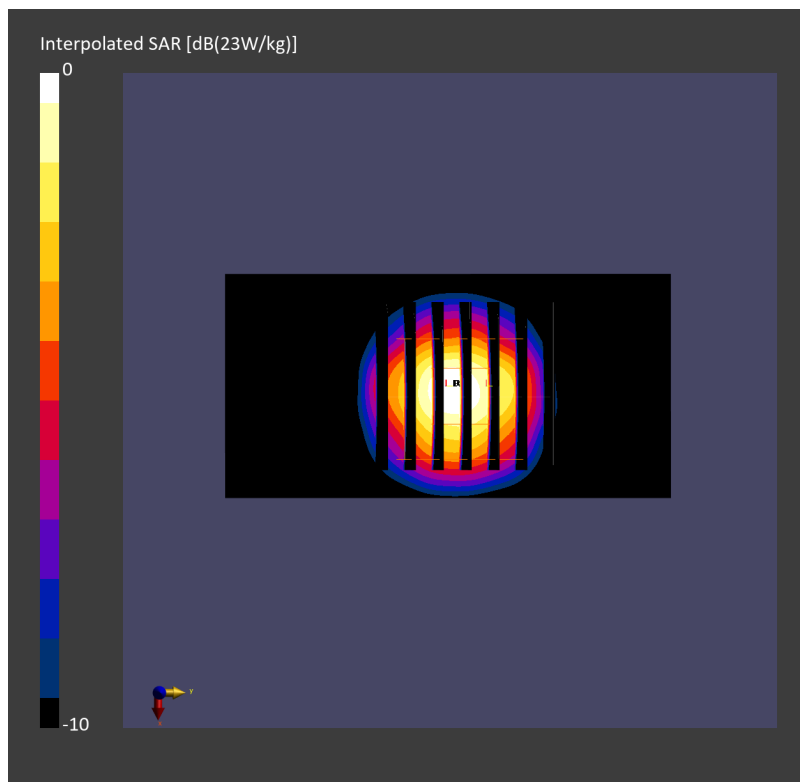

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260417 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.08$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(5.94, 5.83, 6.03); Calibrated: 2025-09-11
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn853; Calibrated: 2025-09-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041-; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 17.1 W/kg; SAR (10g) = 6.06 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 18.0 W/kg; SAR (8g) = 7.18 W/kg; SAR (10g) = 6.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.0 %

TSL Correction: Positive only

