Date: 2024-10-11

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_750_241011 Medium parameters used: f= 750.000 MHz; σ= 0.891 S/m; ε_r = 41.8
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(8.94, 9.37, 8.85); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.436 W/kg; SAR (10g) = 0.291 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 0.434 W/kg; SAR (8g) = 0.301 W/kg; SAR (10g) = 0.285 W/kg
Smallest distance from peaks to all points 3 dB below = 18.4 mm
Ratio of SAR at M2 to SAR at M1 = 86.9 %

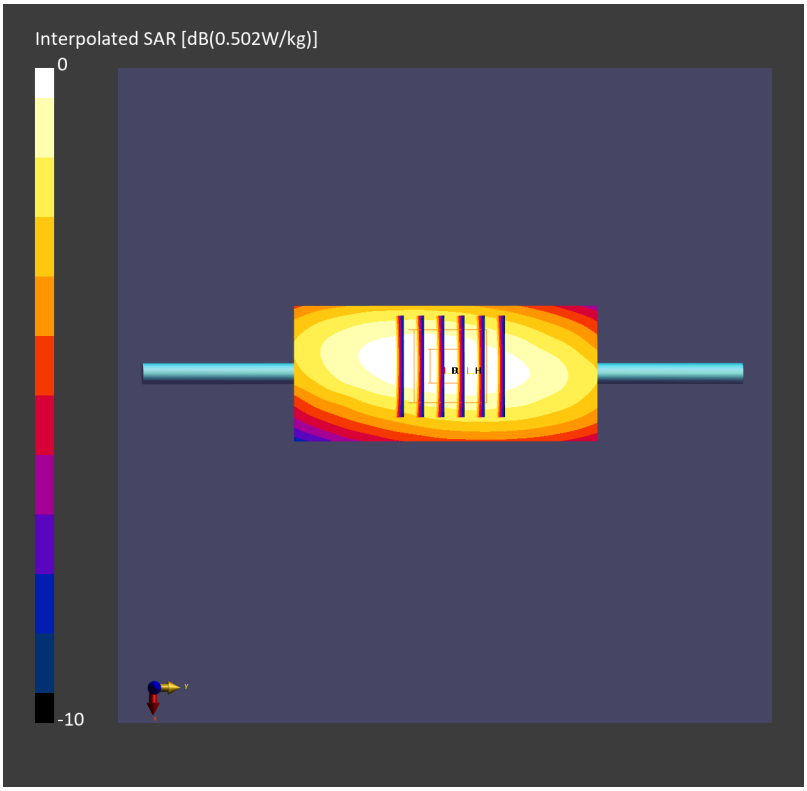

Date: 2024-10-13

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_750_241013 Medium parameters used: f= 750.000 MHz; σ= 0.889 S/m; ε_r = 41.4
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(8.94, 9.37, 8.85); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.436 W/kg; SAR (10g) = 0.290 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 0.433 W/kg; SAR (8g) = 0.301 W/kg; SAR (10g) = 0.285 W/kg
Smallest distance from peaks to all points 3 dB below = 20.5 mm
Ratio of SAR at M2 to SAR at M1 = 86.7 %

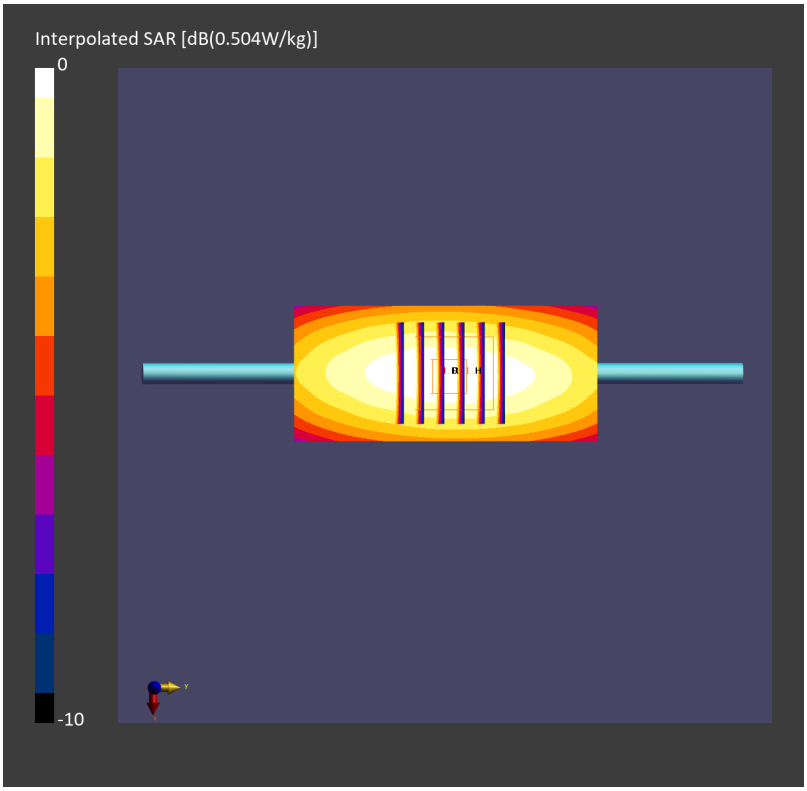

Date: 2024-10-17

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_750_241017 Medium parameters used: f= 750.000 MHz; σ= 0.902 S/m; ε_r = 43.0
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(8.94, 9.37, 8.85); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.429 W/kg; SAR (10g) = 0.286 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 0.427 W/kg; SAR (8g) = 0.300 W/kg; SAR (10g) = 0.285 W/kg
Smallest distance from peaks to all points 3 dB below = > 15.0 mm
Ratio of SAR at M2 to SAR at M1 = 85.7 %

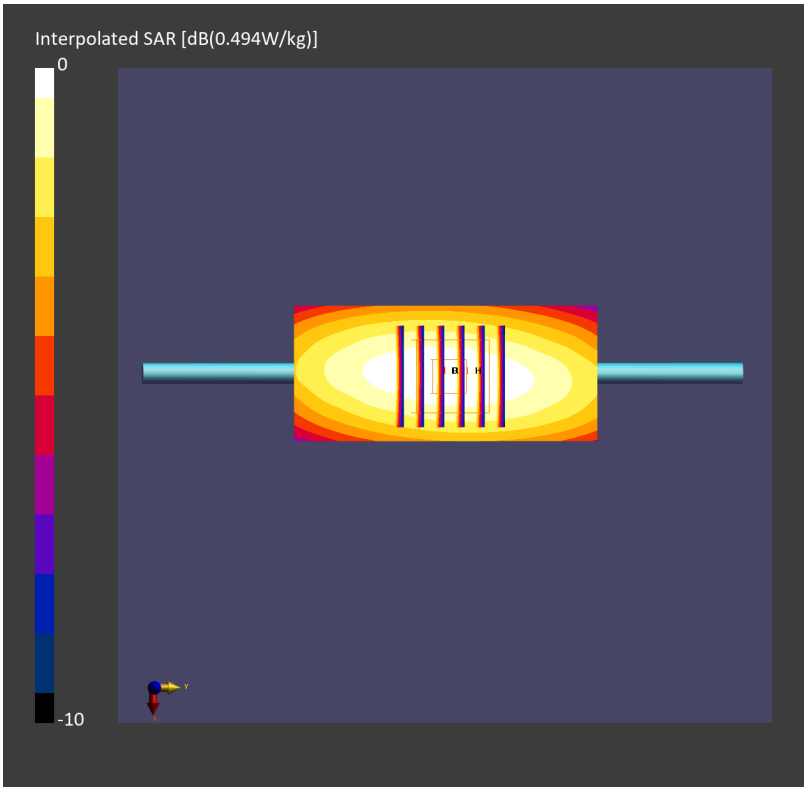

Date: 2024-10-19

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz
Medium: HSL_750_241019 Medium parameters used: f= 750.000 MHz; σ= 0.898 S/m; ε_r = 42.6
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(8.94, 9.37, 8.85); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.415 W/kg; SAR (10g) = 0.278 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 0.417 W/kg; SAR (8g) = 0.292 W/kg; SAR (10g) = 0.277 W/kg
Smallest distance from peaks to all points 3 dB below = > 15.0 mm
Ratio of SAR at M2 to SAR at M1 = 84.4 %

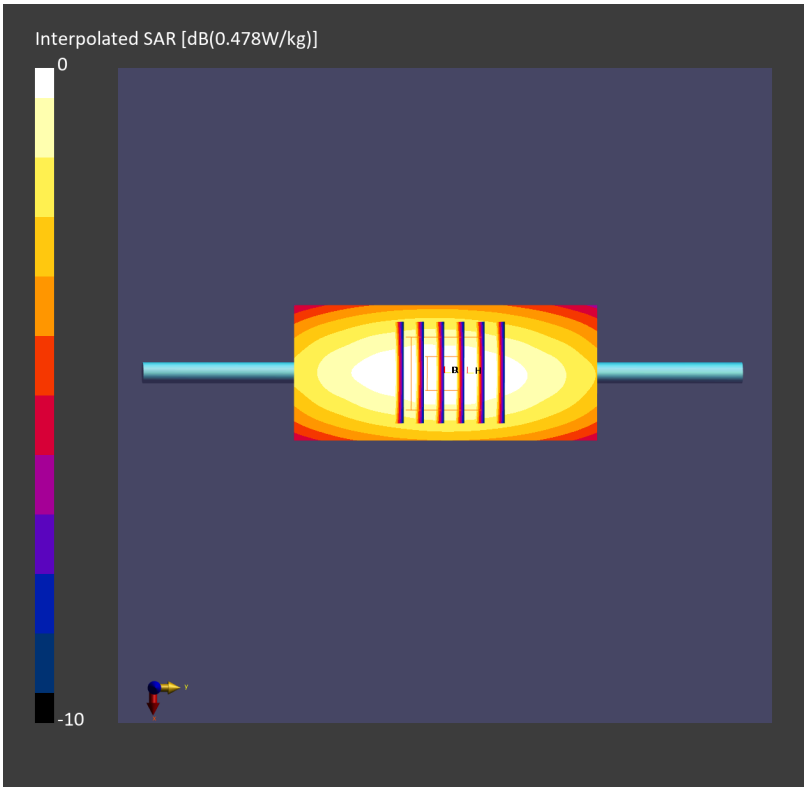

Date: 2024-10-13

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_850_241013 Medium parameters used: f= 835.000 MHz; σ= 0.923 S/m; ε_r = 41.2
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(8.67, 9.09, 8.59); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.486 W/kg; SAR (10g) = 0.322 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 0.490 W/kg; SAR (8g) = 0.340 W/kg; SAR (10g) = 0.322 W/kg
Smallest distance from peaks to all points 3 dB below = 18.4 mm
Ratio of SAR at M2 to SAR at M1 = 85.1 %

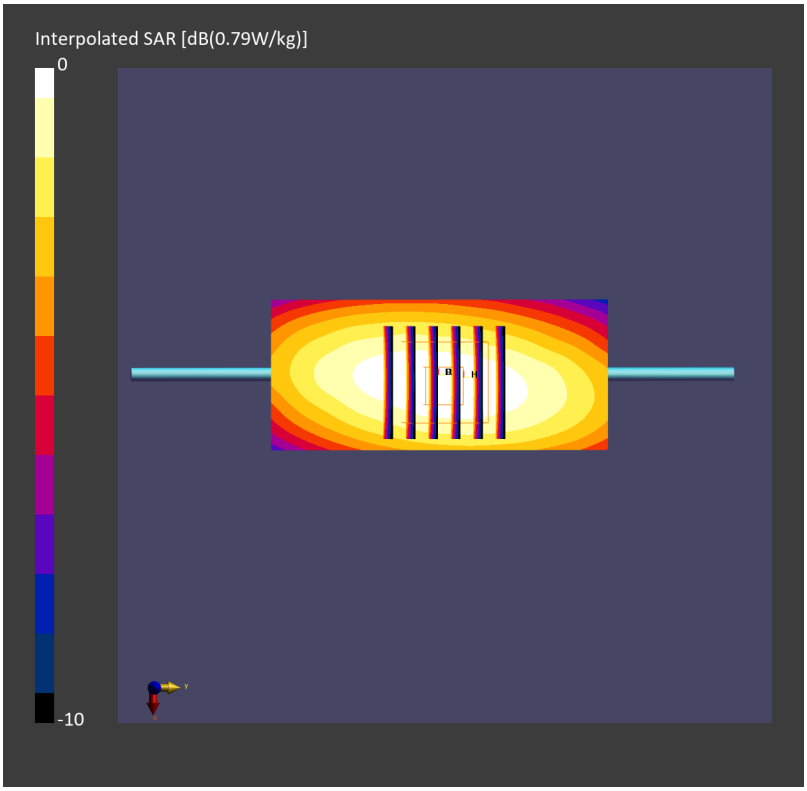

Date: 2024-10-19

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz
Medium: HSL_850_241019 Medium parameters used: f= 835.000 MHz; σ= 0.933 S/m; ε_r = 42.4
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(8.67, 9.09, 8.59); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.512 W/kg; SAR (10g) = 0.336 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 0.509 W/kg; SAR (8g) = 0.351 W/kg; SAR (10g) = 0.333 W/kg
Smallest distance from peaks to all points 3 dB below = 19.0 mm
Ratio of SAR at M2 to SAR at M1 = 86.8 %

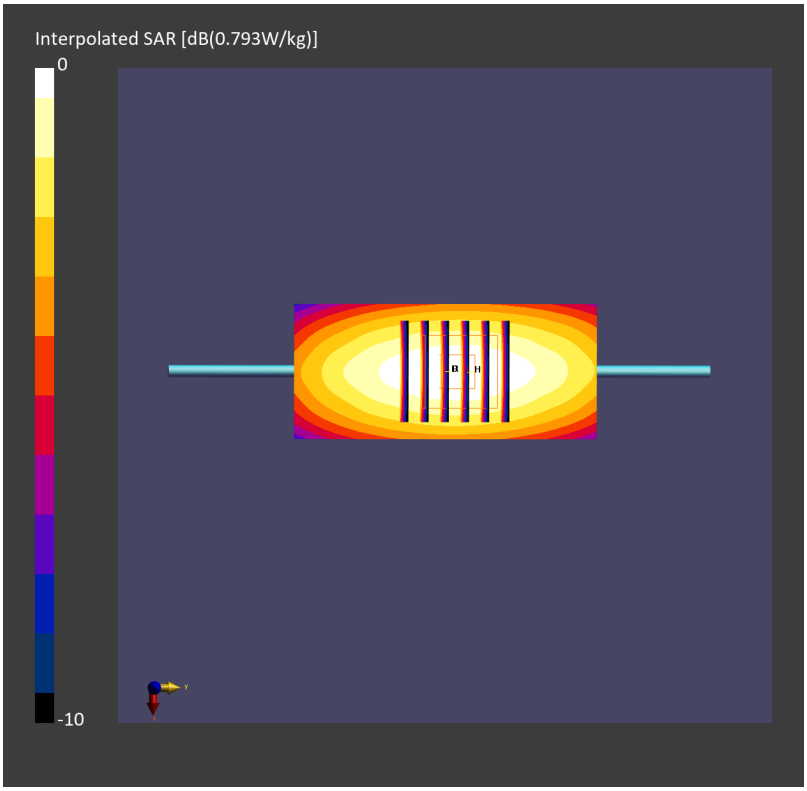

Date: 2024-10-12

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_1750_241012 Medium parameters used: f= 1750.000 MHz; σ= 1.36 S/m; ε_r = 40.7
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.49, 7.86, 7.42); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.84 W/kg; SAR (10g) = 0.977 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 1.82 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.967 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 82.7 %

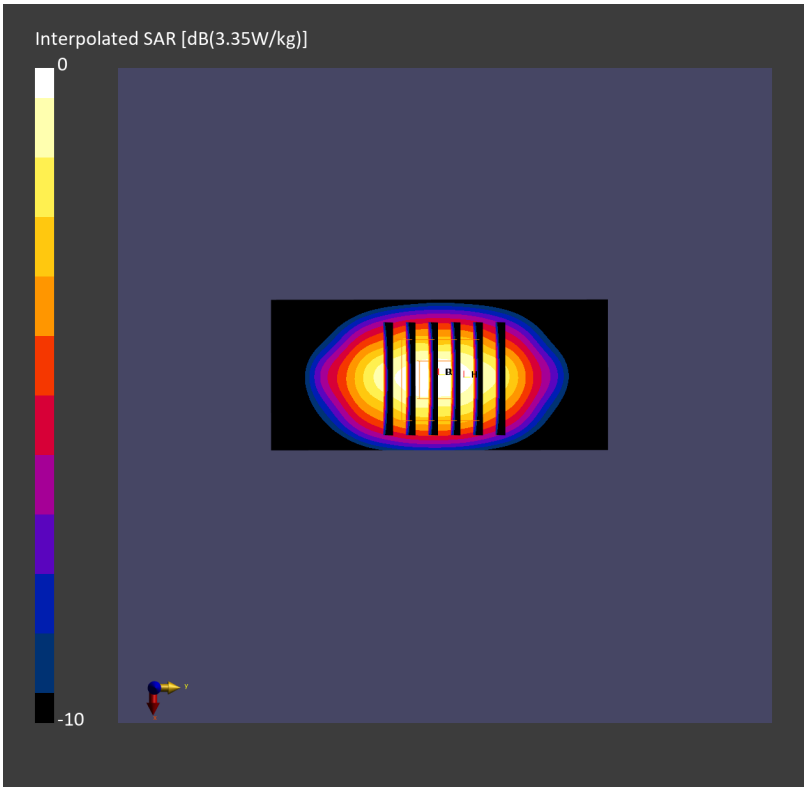

Date: 2024-10-18

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_1750_241018 Medium parameters used: f= 1750.000 MHz; σ= 1.35 S/m; ε_r = 40.5
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.49, 7.86, 7.42); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.68 W/kg; SAR (10g) = 0.903 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 1.69 W/kg; SAR (8g) = 0.980 W/kg; SAR (10g) = 0.905 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 81.8 %

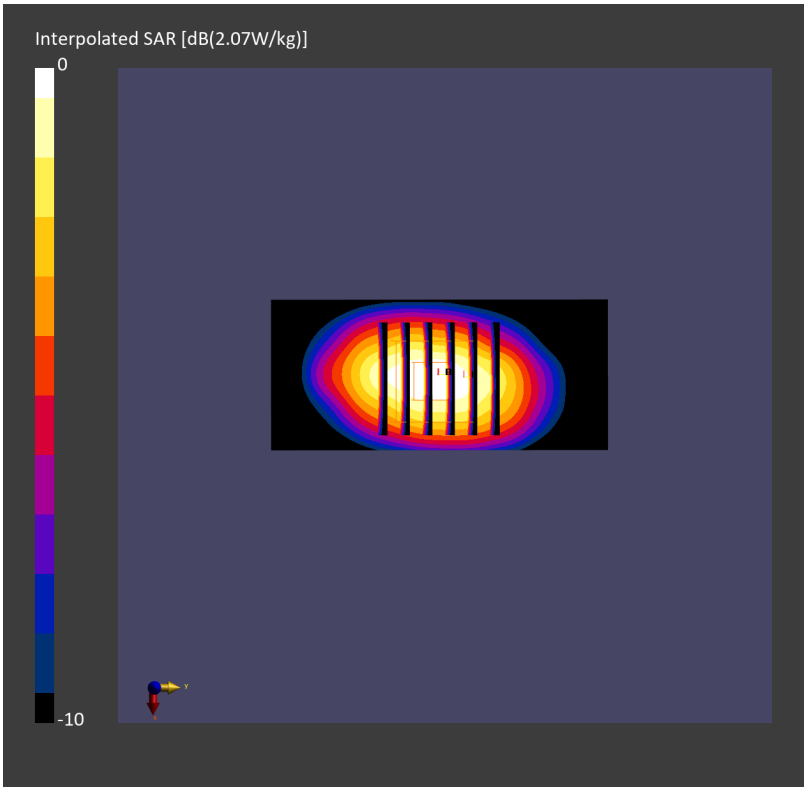

Date: 2024-10-25

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_1750_241025 Medium parameters used: f= 1750.000 MHz; σ= 1.34 S/m; ε_r = 40.4
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.49, 7.86, 7.42); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.81 W/kg; SAR (10g) = 0.961 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 1.80 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.954 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 82.2 %

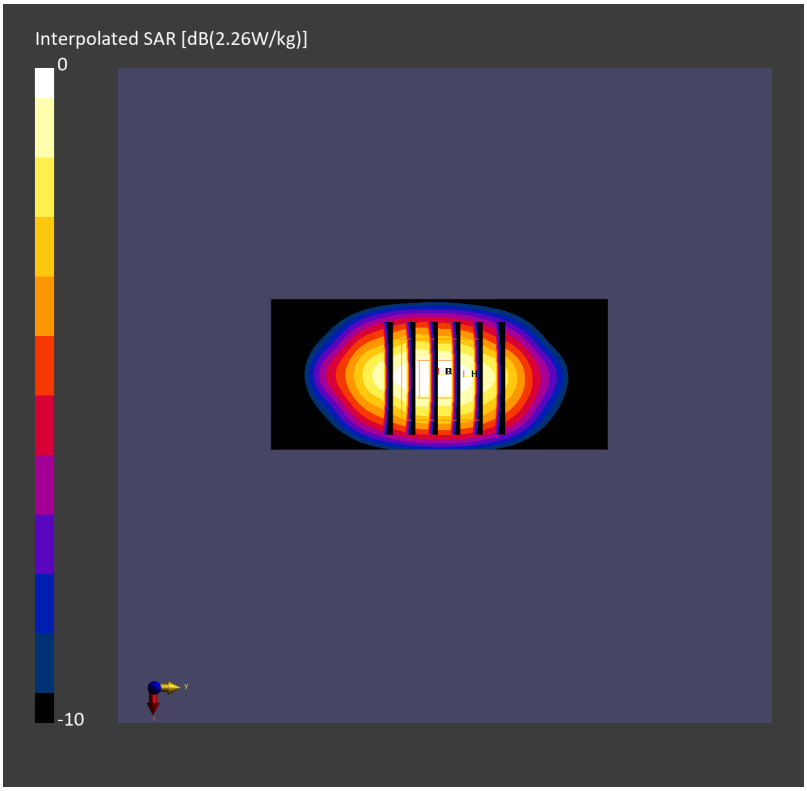

Date: 2024-11-01

System Check_Head_1750MHz

DUT: D1750V2 - SN1068

Communication System: CW; Frequency: 1750.000 MHz
Medium: HSL_1750_241101 Medium parameters used: f= 1750.000 MHz; σ= 1.34 S/m; ε_r = 39.9
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.49, 7.86, 7.42); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 1.82 W/kg; SAR (10g) = 0.964 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 1.80 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.957 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 82.2 %

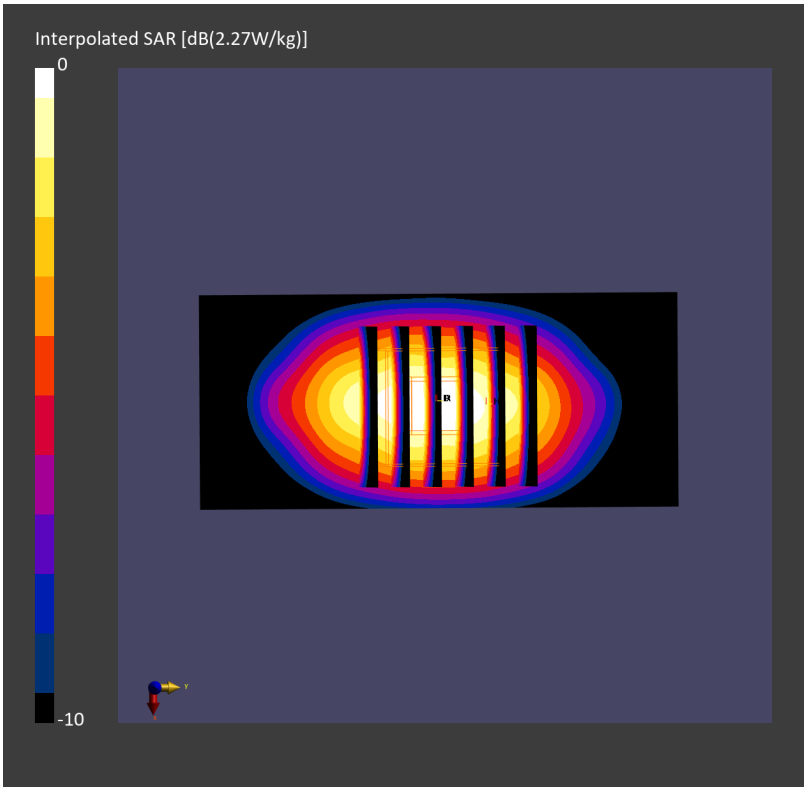

Date: 2024-10-15

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_1900_241015 Medium parameters used: f= 1900.000 MHz; σ= 1.42 S/m; ε_r = 38.8
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.28, 7.63, 7.21); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.996 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 1.91 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 0.999 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 81.2 %

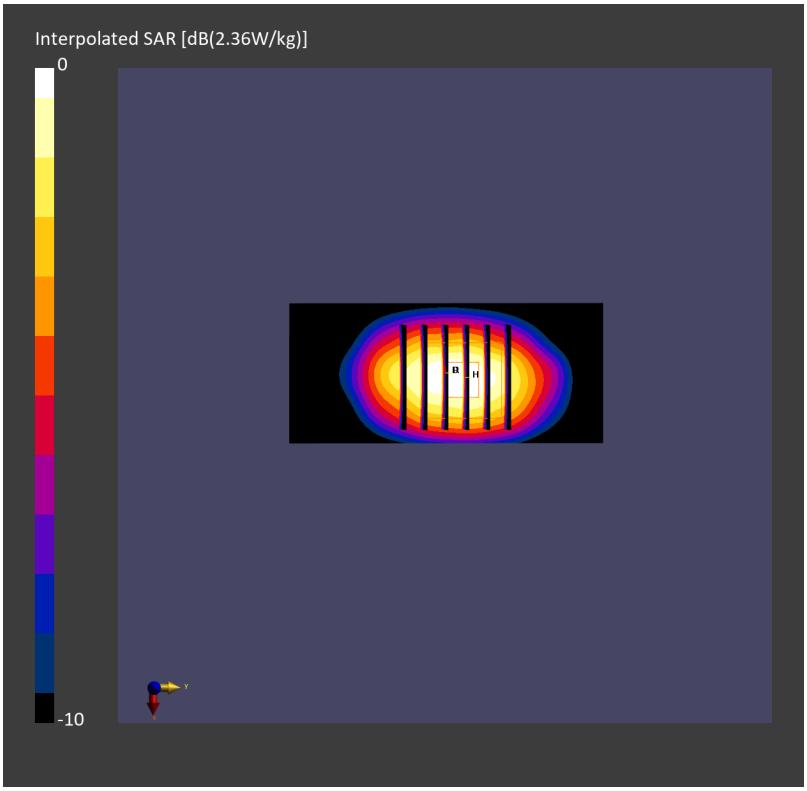

Date: 2024-10-18

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: CW; Frequency: 1900.000 MHz
Medium: HSL_1900_241018 Medium parameters used: f= 1900.000 MHz; σ= 1.43 S/m; ε_r = 38.9
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.28, 7.63, 7.21); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.01 W/kg; SAR (10g) = 1.04 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 1.99 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 83.4 %

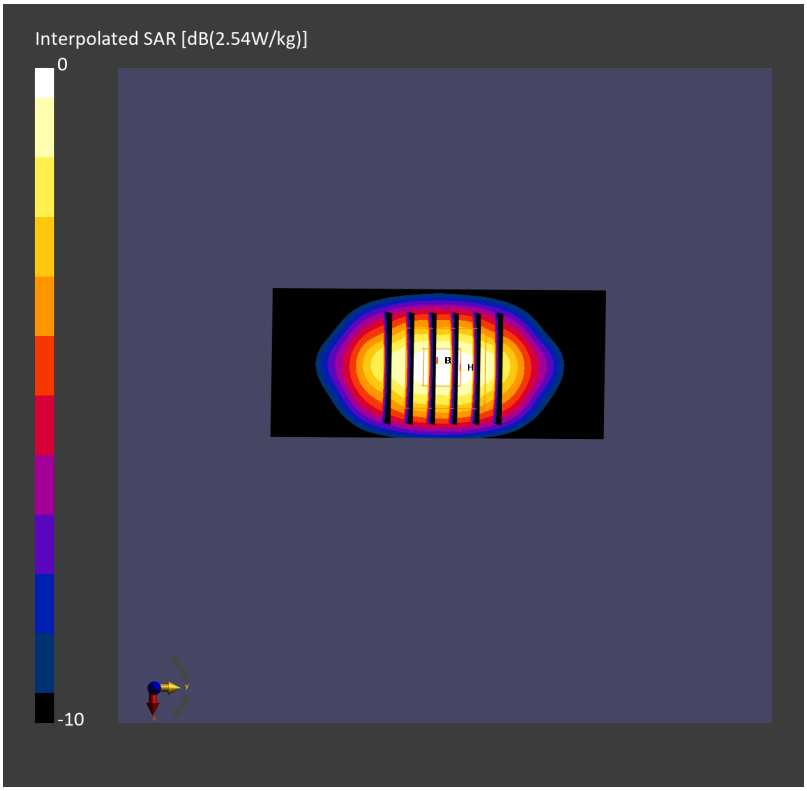

Date: 2024-10-20

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_2300_241020 Medium parameters used: f= 2300.000 MHz; σ= 1.65 S/m; ε_r = 39.7
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.19, 7.54, 7.12); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.25 W/kg; SAR (10g) = 1.06 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 2.22 W/kg; SAR (8g) = 1.16 W/kg; SAR (10g) = 1.06 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.4 %

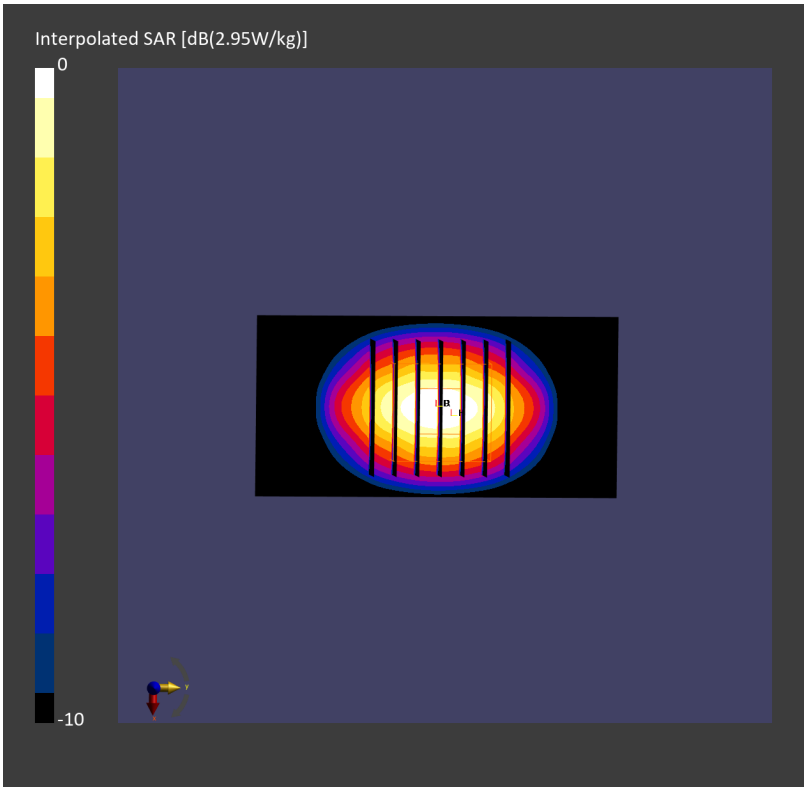

Date: 2024-10-26

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz
Medium: HSL_2300_241026 Medium parameters used: f= 2300.000 MHz; σ= 1.68 S/m; ε_r = 40.2
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.19, 7.54, 7.12); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.28 W/kg; SAR (10g) = 1.08 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.24 W/kg; SAR (8g) = 1.18 W/kg; SAR (10g) = 1.07 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.9 %

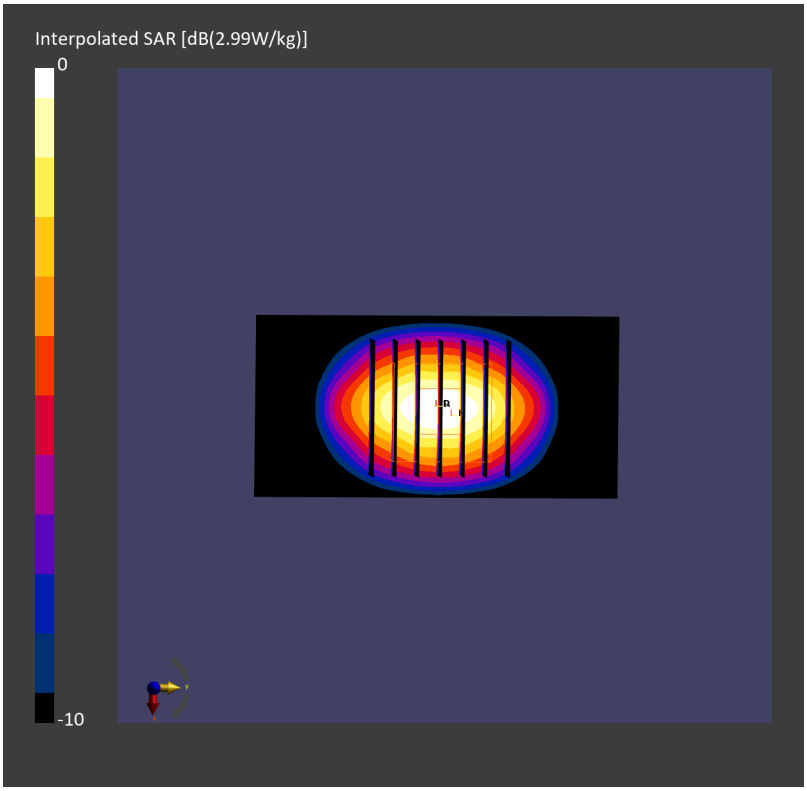

Date: 2024-10-14

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_2600_241014 Medium parameters used: f= 2600.000 MHz; σ= 1.96 S/m; ε_r = 38.1
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.02, 7.36, 6.95); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.10 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 2.59 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.18 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 79.6 %

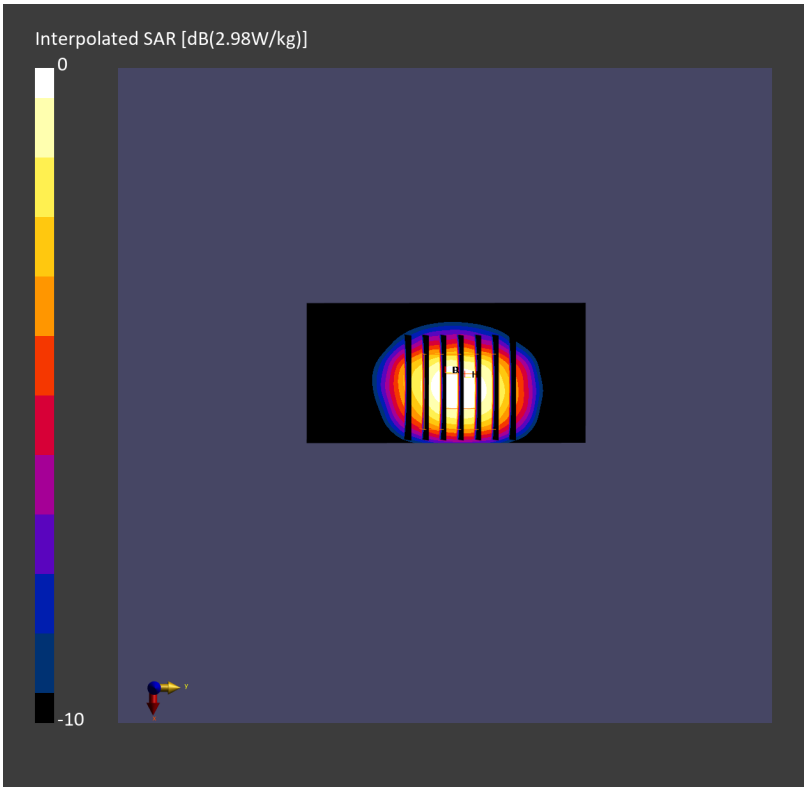

Date: 2024-10-16

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_2600_241016 Medium parameters used: f= 2600.000 MHz; σ= 1.98 S/m; ε_r = 38.8
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.02, 7.36, 6.95); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.25 W/kg; SAR (10g) = 1.01 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 2.52 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.14 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 80.4 %

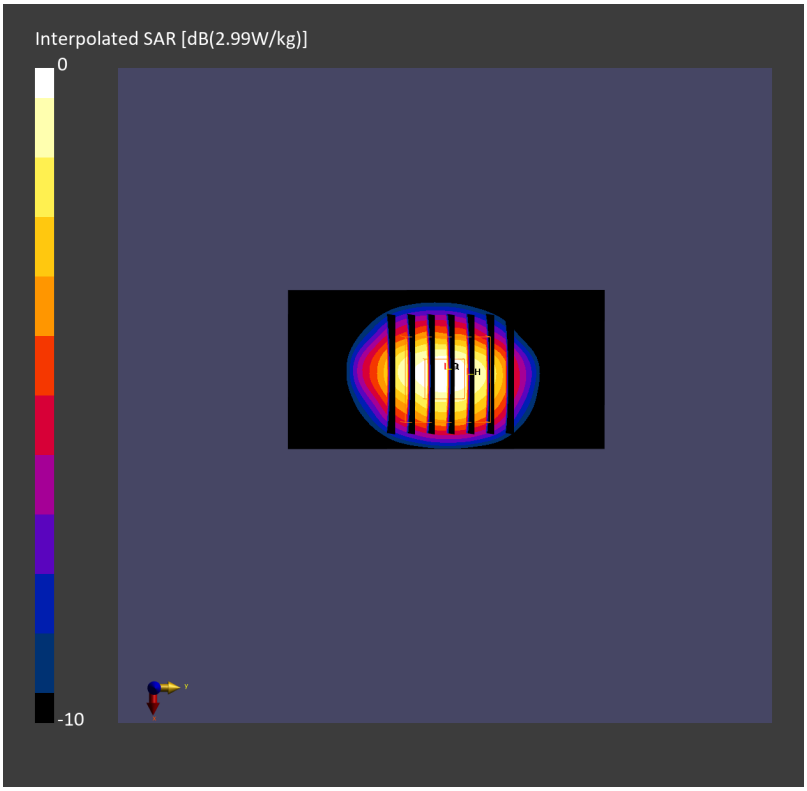

Date: 2024-10-21

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_2600_241021 Medium parameters used: f= 2600.000 MHz; σ= 1.97 S/m; ε_r = 38.7
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.02, 7.36, 6.95); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.21 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.06 dB
SAR (1g) = 2.71 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.25 W/kg
Smallest distance from peaks to all points 3 dB below = 8.1 mm
Ratio of SAR at M2 to SAR at M1 = 80.2 %

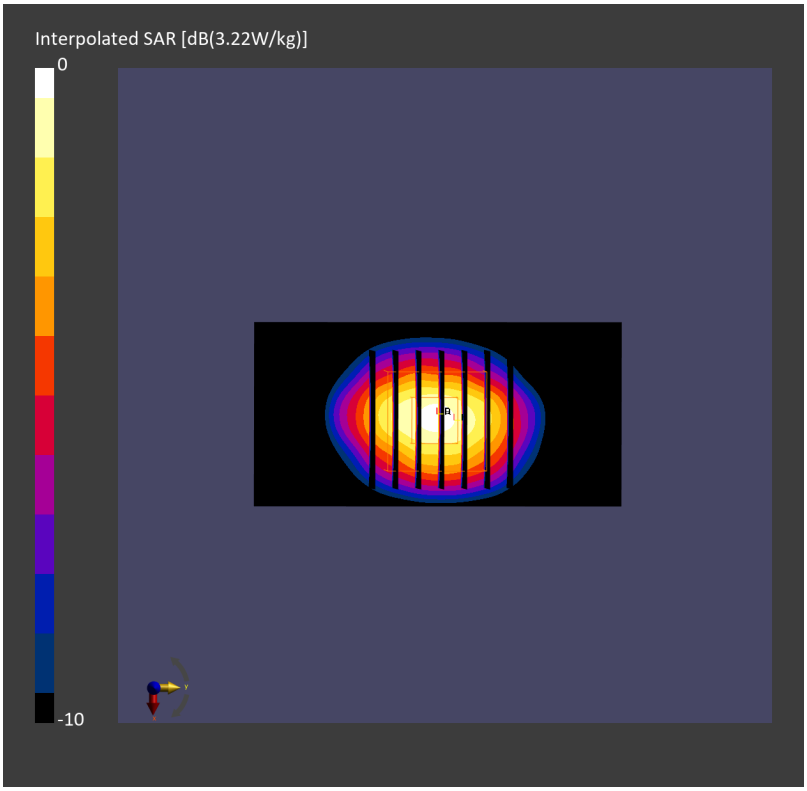

Date: 2024-10-28

System Check_Head_2600MHz

DUT: D2600V2 - SN1008

Communication System: CW; Frequency: 2600.000 MHz
Medium: HSL_2600_241028 Medium parameters used: f= 2600.000 MHz; σ= 2.00 S/m; ε_r = 39.2
Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(7.02, 7.36, 6.95); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.26 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.05 dB
SAR (1g) = 2.53 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.27 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.8 %

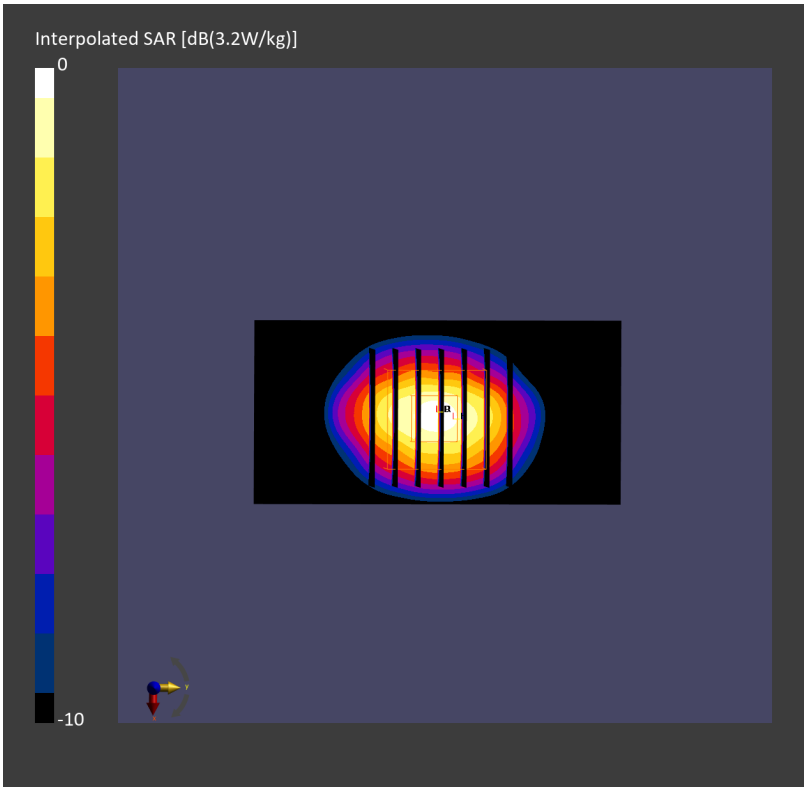

Date: 2024-10-22

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_3500_241022 Medium parameters used: f= 3500.000 MHz; σ= 2.89 S/m; ε_r = 38.0
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.03); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.01 W/kg; SAR (10g) = 1.19 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.12 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 74.2 %

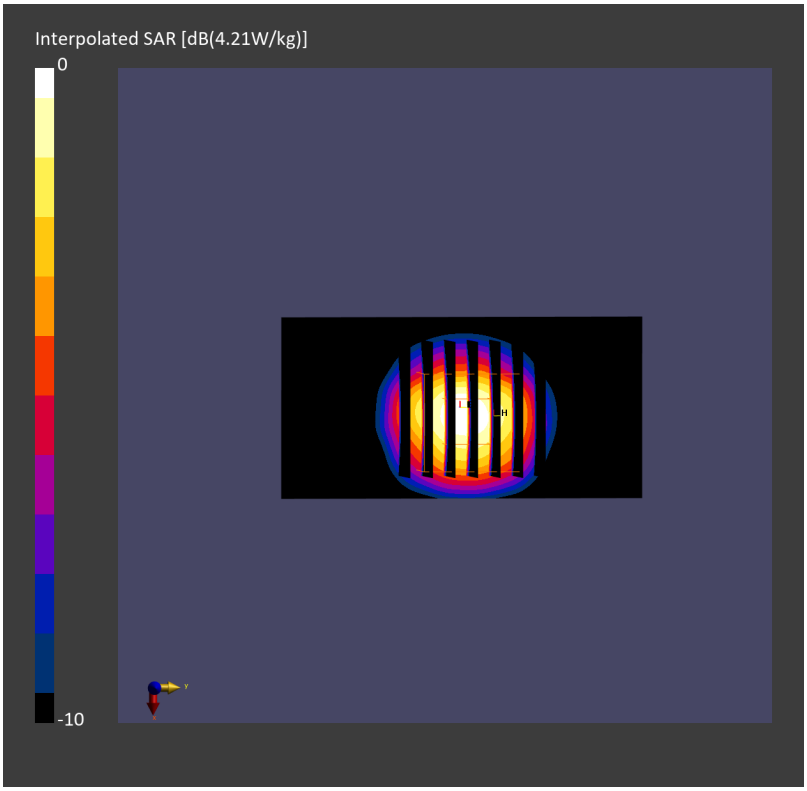

Date: 2024-10-24

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_3500_241024 Medium parameters used: f= 3500.000 MHz; σ= 2.88 S/m; ε_r = 37.9
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.03); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.25 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 3.28 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.24 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 76.6 %

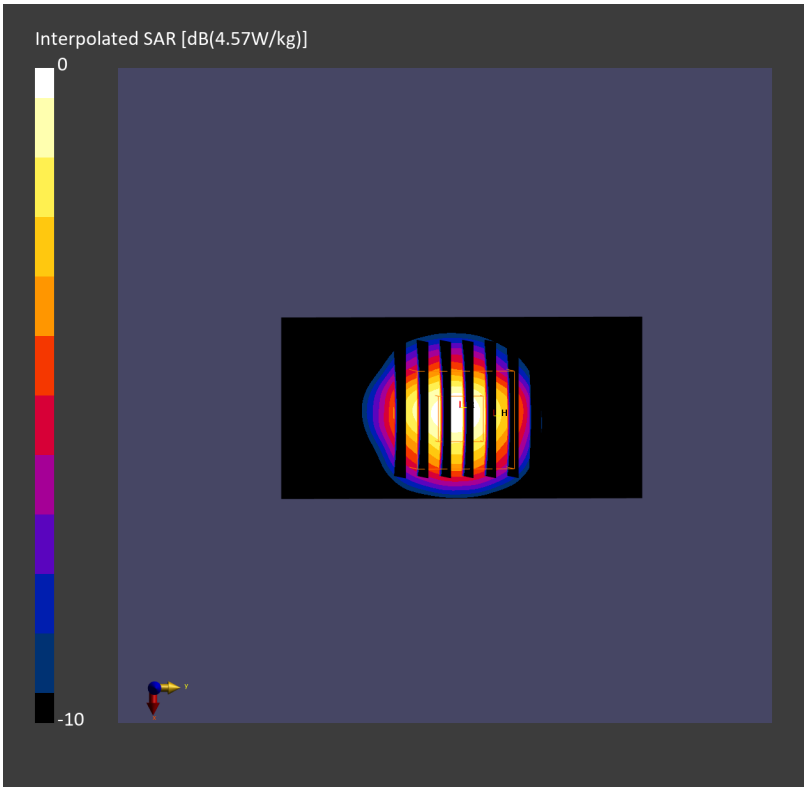

Date: 2024-10-27

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_3500_241027 Medium parameters used: f= 3500.000 MHz; σ= 2.88 S/m; ε_r = 37.7
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7822; ConvF(6.28, 6.16, 6.53); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.34 W/kg; SAR (10g) = 1.27 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 3.26 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.23 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 76.6 %

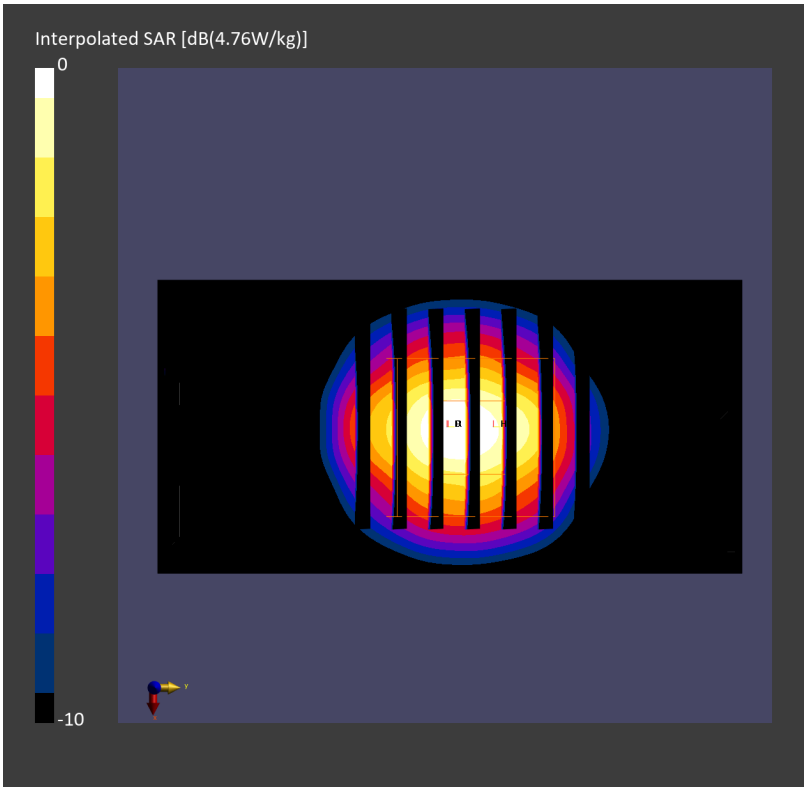

Date: 2024-10-29

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_3500_241029 Medium parameters used: f= 3500.000 MHz; σ= 2.87 S/m; ε_r = 37.7
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7822; ConvF(6.28, 6.16, 6.53); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.23 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.00 dB
SAR (1g) = 3.25 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 76.8 %

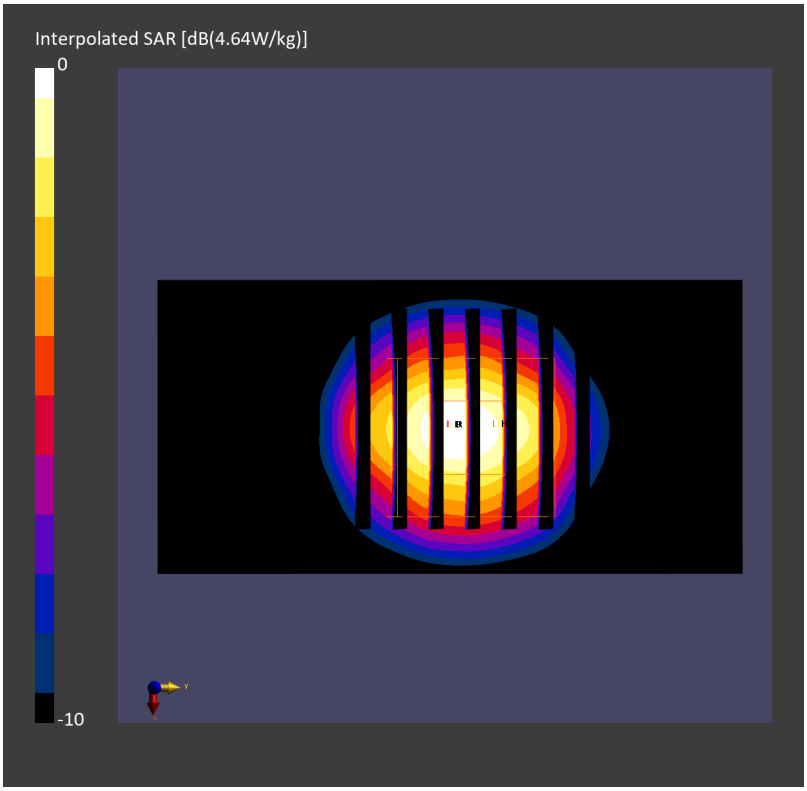

Date: 2024-10-30

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz
Medium: HSL_3500_241030 Medium parameters used: f= 3500.000 MHz; σ= 2.86 S/m; ε_r = 37.8
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.03); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.23 W/kg; SAR (10g) = 1.25 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.25 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 76.7 %

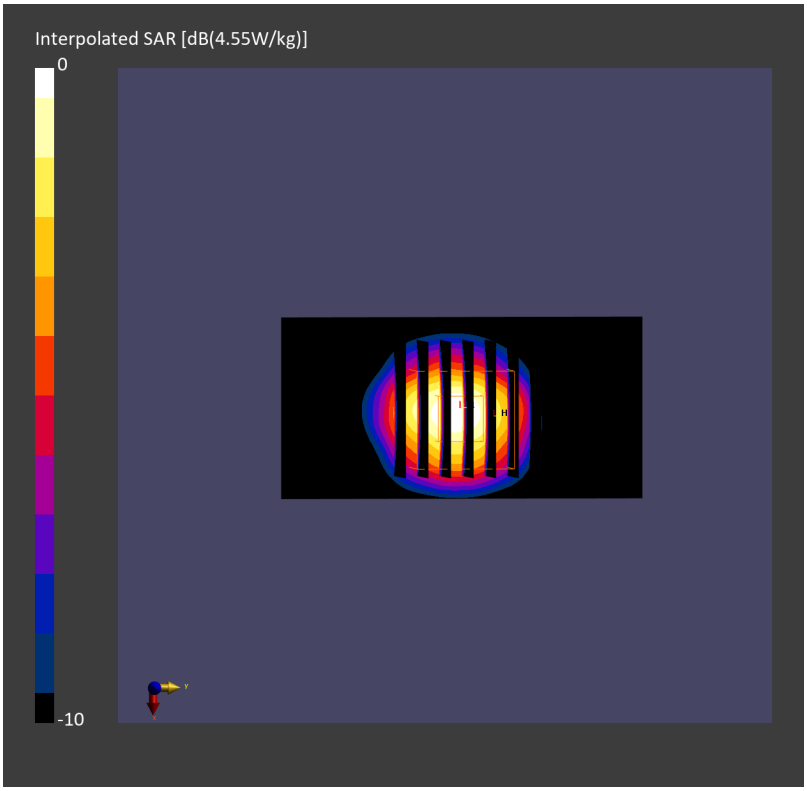

Date: 2024-10-23

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_3700_241023 Medium parameters used: f= 3700.000 MHz; σ= 3.08 S/m; ε_r = 37.8
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.02); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 1.23 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.35 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.23 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 74.2 %

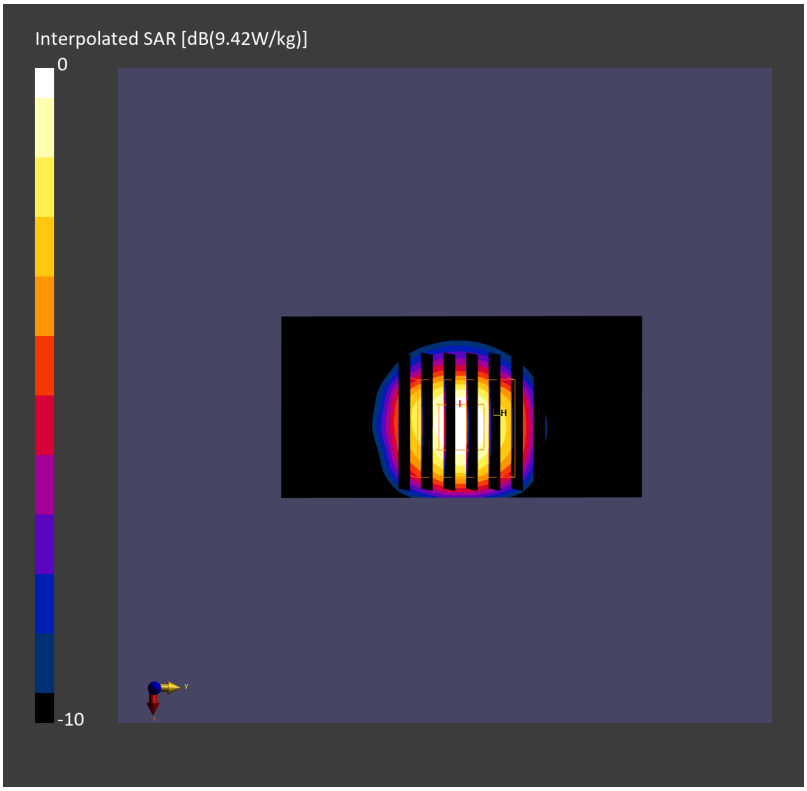

Date: 2024-10-24

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_3700_241024 Medium parameters used: f= 3700.000 MHz; σ= 3.06 S/m; ε_r = 37.7
Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.02); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.23 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.00 dB
SAR (1g) = 3.33 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.22 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 73.9 %

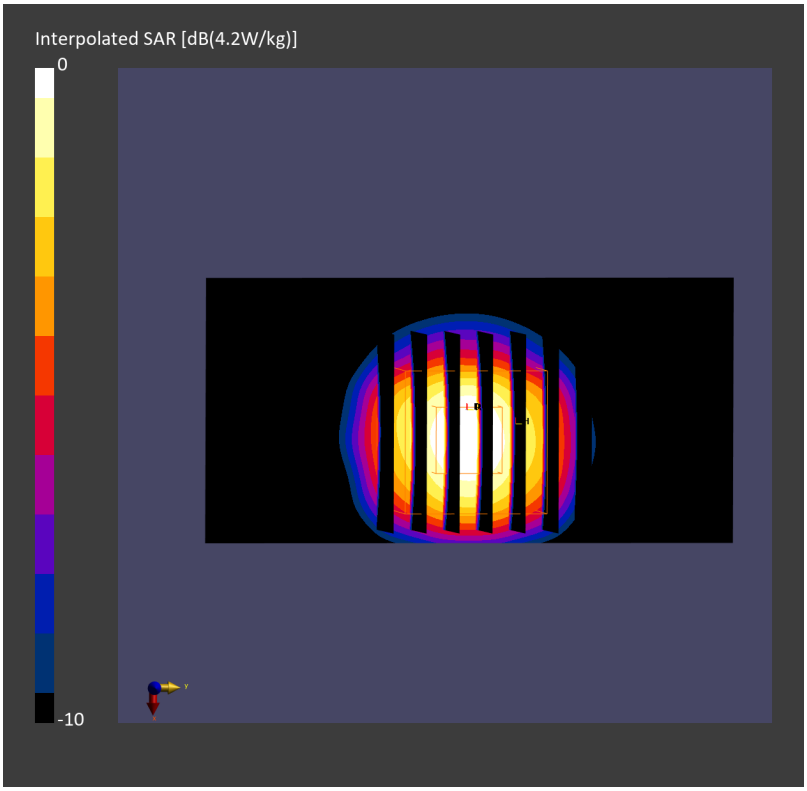

Date: 2024-10-27

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_3700_241027 Medium parameters used: f= 3700.000 MHz; σ= 3.09 S/m; ε_r = 37.5
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7822; ConvF(6.3, 6.18, 6.55); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.19 W/kg; SAR (10g) = 1.20 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 3.26 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 76.3 %

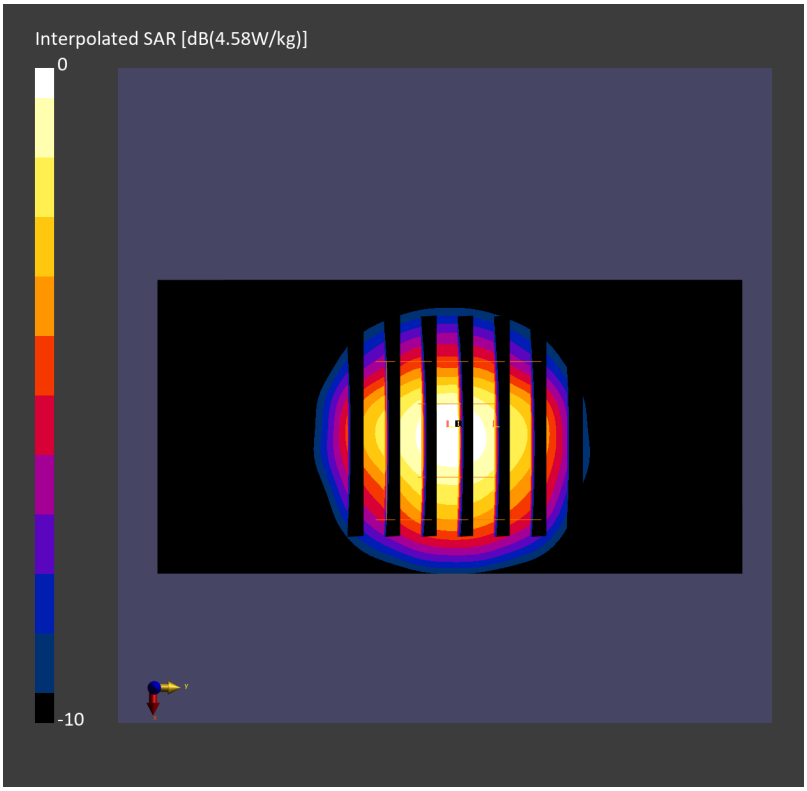

Date: 2024-10-29

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_3900_241029 Medium parameters used: f= 3700.000 MHz; σ= 3.06 S/m; ε_r = 37.6
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7822; ConvF(6.3, 6.18, 6.55); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.19 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.23 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg
Smallest distance from peaks to all points 3 dB below = 8.3 mm
Ratio of SAR at M2 to SAR at M1 = 75.9 %

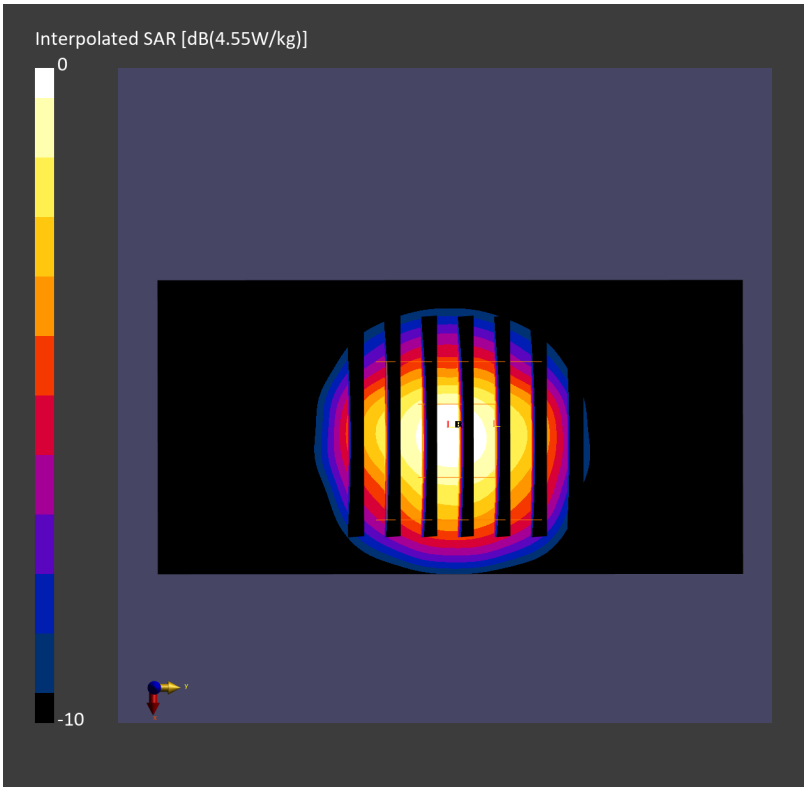

Date: 2024-10-30

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz
Medium: HSL_3700_241030 Medium parameters used: f= 3700.000 MHz; σ= 3.05 S/m; ε_r = 37.6
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.02); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.07 W/kg; SAR (10g) = 1.17 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.00 dB
SAR (1g) = 3.19 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.18 W/kg
Smallest distance from peaks to all points 3 dB below = 8.6 mm
Ratio of SAR at M2 to SAR at M1 = 72.9 %

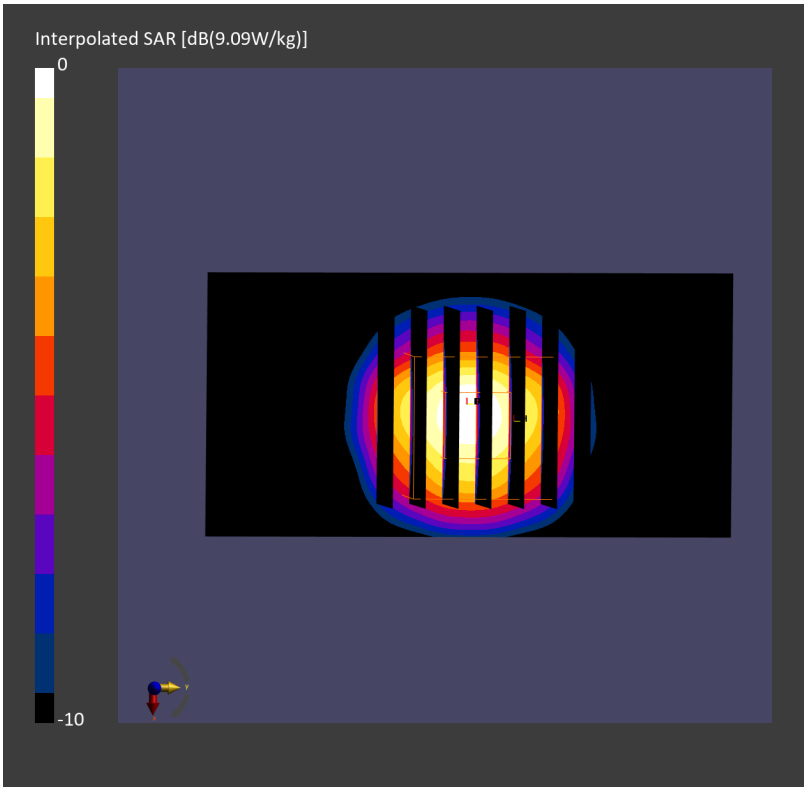

Date: 2024-10-27

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_3900_241027 Medium parameters used: f= 3900.000 MHz; σ= 3.29 S/m; ε_r = 37.3
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7822; ConvF(6.16, 6.04, 6.41); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.16 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.30 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.16 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 75.0 %

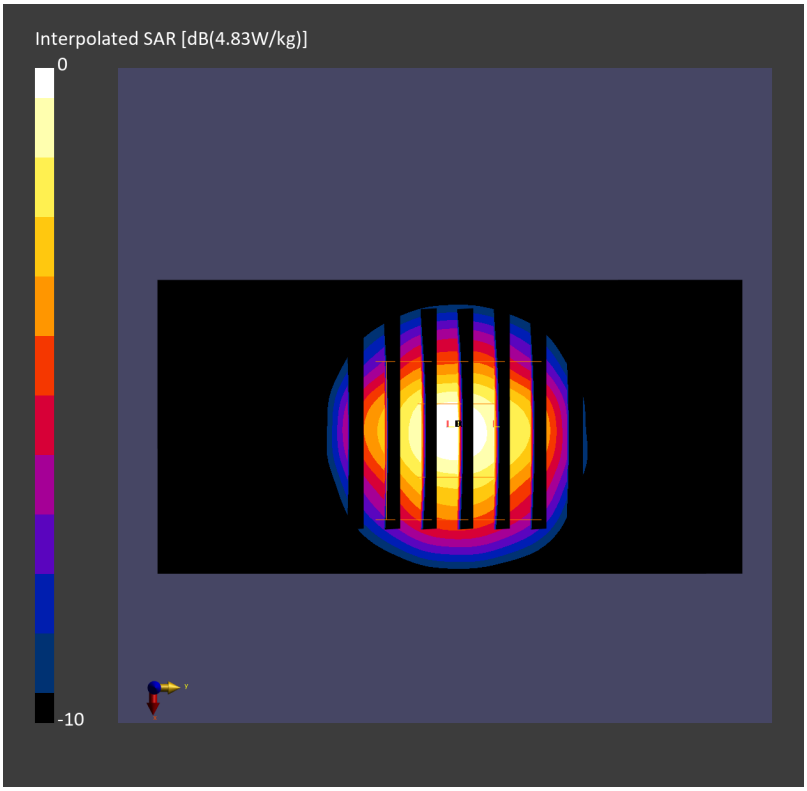

Date: 2024-10-29

System Check_Head_3900MHz

DUT: D3900V2 - SN1017

Communication System: CW; Frequency: 3900.000 MHz
Medium: HSL_3900_241029 Medium parameters used: f= 3900.000 MHz; σ= 3.24 S/m; ε_r = 37.5
Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7822; ConvF(6.16, 6.04, 6.41); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.22 W/kg; SAR (10g) = 1.14 W/kg;
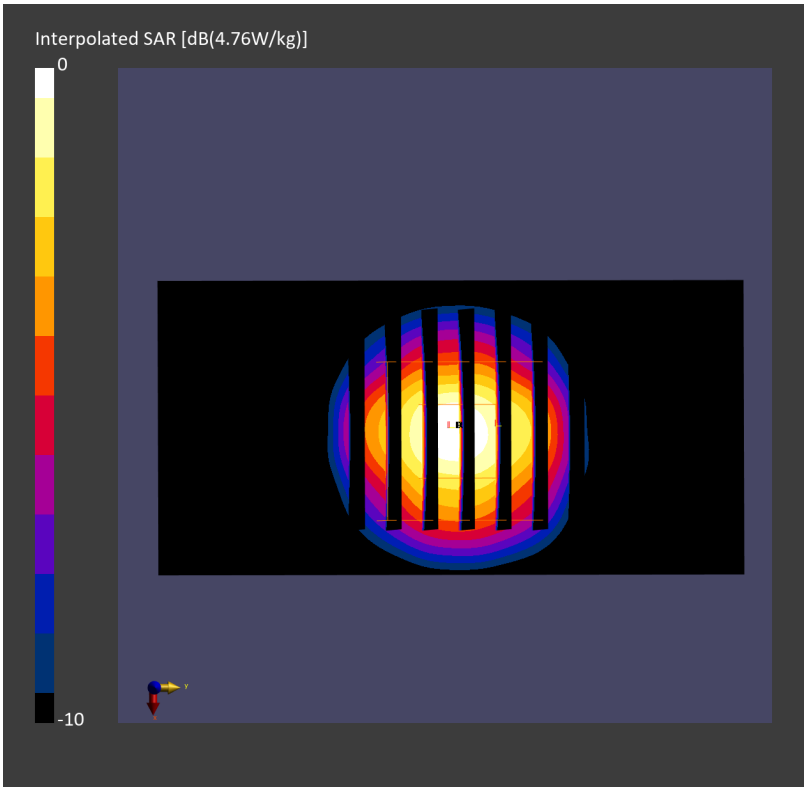
Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 3.25 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.15 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 74.5 %