

System Check_H750

Frequency: 750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.2°C; Liquid Temperature: 20.5°C
Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.895 \text{ S/m}$; $\epsilon_r = 40.99$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(9.9, 10.1, 9.47) @ 750 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x13x1):

Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 2.62 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 57.97 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 2.93 W/kg

SAR(1 g) = 2.01 W/kg; SAR(10 g) = 1.35 W/kg

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 68.6%

Maximum value of SAR (measured) = 2.64 W/kg

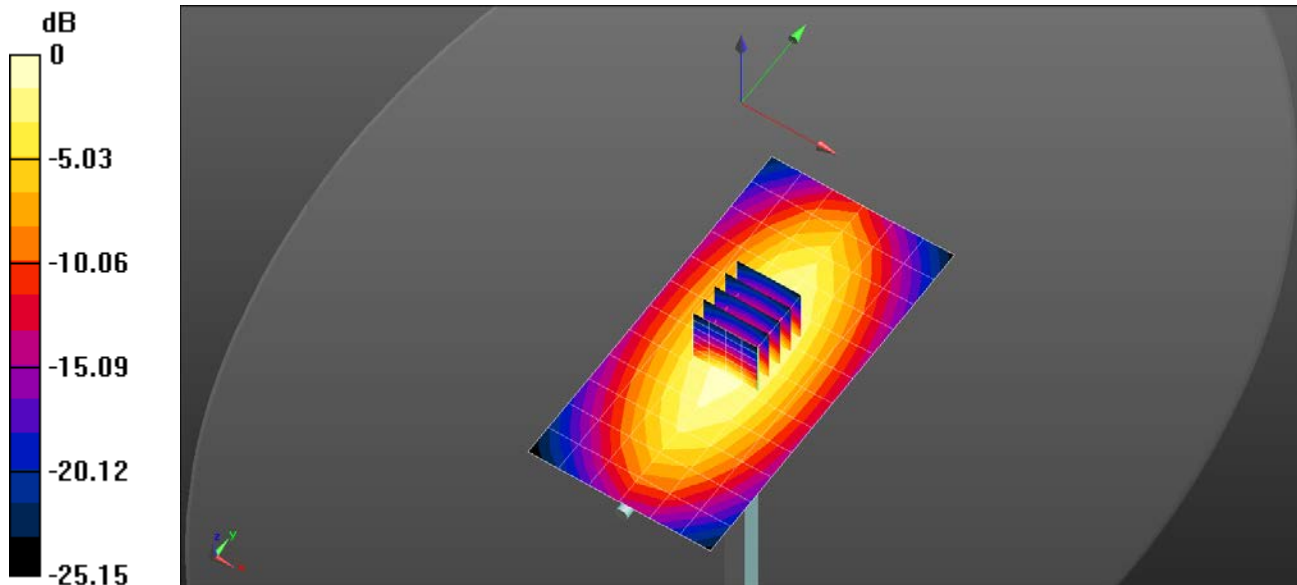

0 dB = 2.62 W/kg = 4.19 dBW/kg

System Check_H750

Frequency: 750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.5°C; Liquid Temperature: 20.3°C
Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.886 \text{ S/m}$; $\epsilon_r = 43.516$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(9.9, 10.1, 9.47) @ 750 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x13x1):

Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 2.64 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 58.29 V/m; Power Drift = -0.01 dB



Peak SAR (extrapolated) = 3.00 W/kg

SAR(1 g) = 2.15 W/kg; SAR(10 g) = 1.47 W/kg

Smallest distance from peaks to all points 3 dB below = 17.9 mm

Ratio of SAR at M2 to SAR at M1 = 71.6%

Maximum value of SAR (measured) = 2.74 W/kg

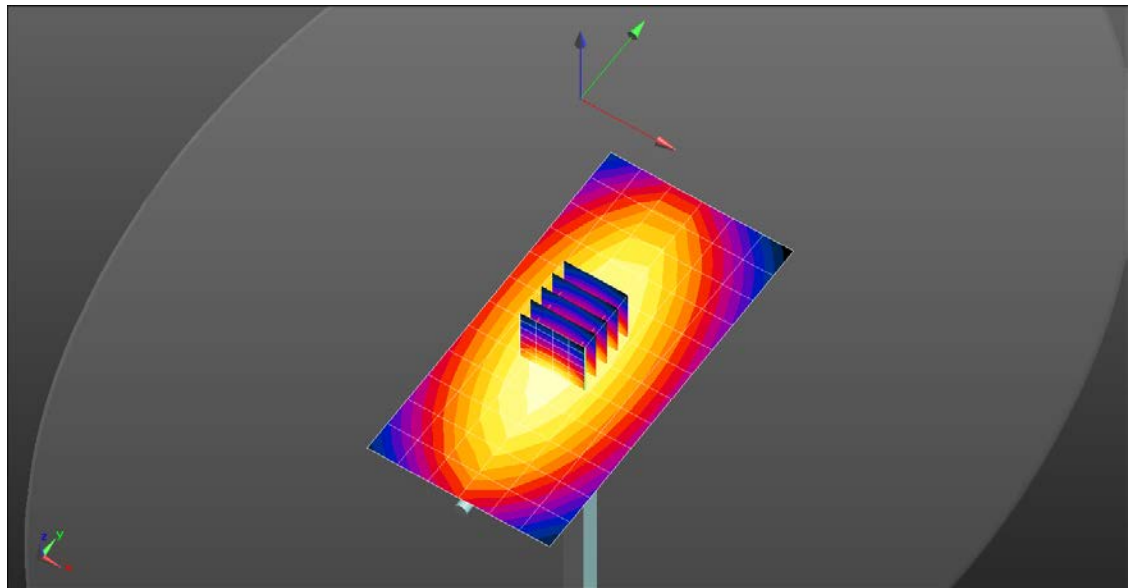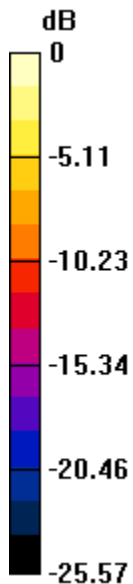

0 dB = 2.64 W/kg = 4.22 dBW/kg

System Check_H750

Frequency: 750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.8°C; Liquid Temperature: 20.9°C
Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.884 \text{ S/m}$; $\epsilon_r = 42.211$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(9.9, 10.1, 9.47) @ 750 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x13x1):

Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 2.44 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 54.67 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 3.04 W/kg

SAR(1 g) = 2.22 W/kg; SAR(10 g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = 21.5 mm

Ratio of SAR at M2 to SAR at M1 = 72.3%

Maximum value of SAR (measured) = 2.72 W/kg

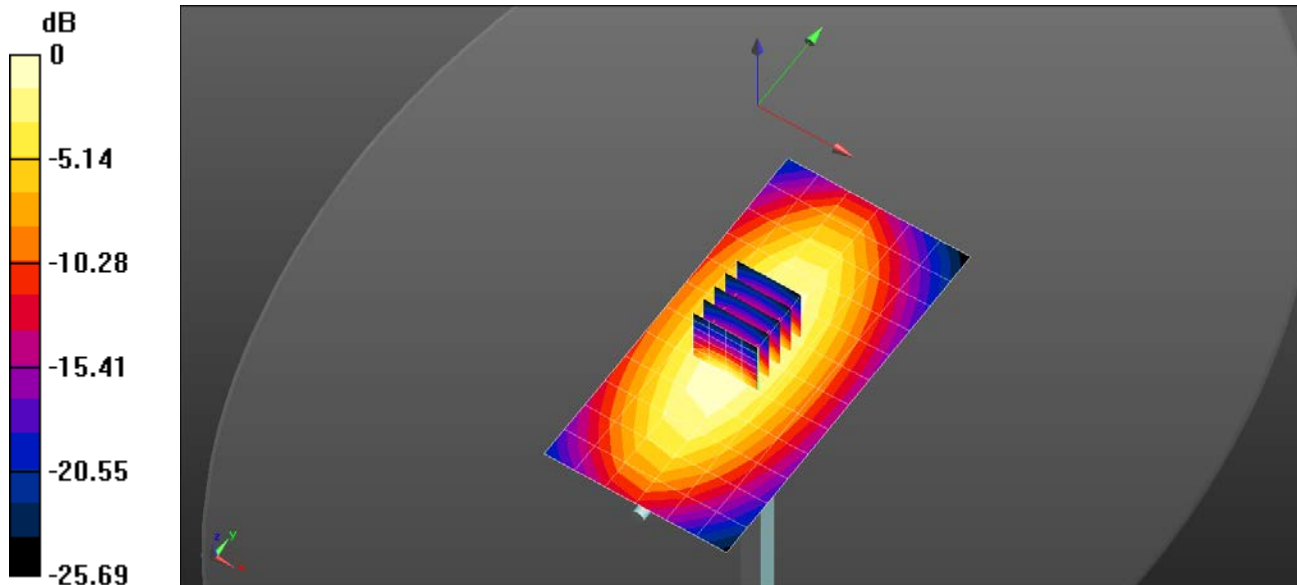

0 dB = 2.44 W/kg = 3.87 dBW/kg

System Check_H750

Frequency: 750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.2°C; Liquid Temperature: 21.1°C
Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.907 \text{ S/m}$; $\epsilon_r = 43.55$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(9.9, 10.1, 9.47) @ 750 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x13x1):

Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 2.59 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 56.25 V/m; Power Drift = 0.11 dB


Peak SAR (extrapolated) = 2.92 W/kg

SAR(1 g) = 2.09 W/kg; SAR(10 g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 71.3%

Maximum value of SAR (measured) = 2.69 W/kg

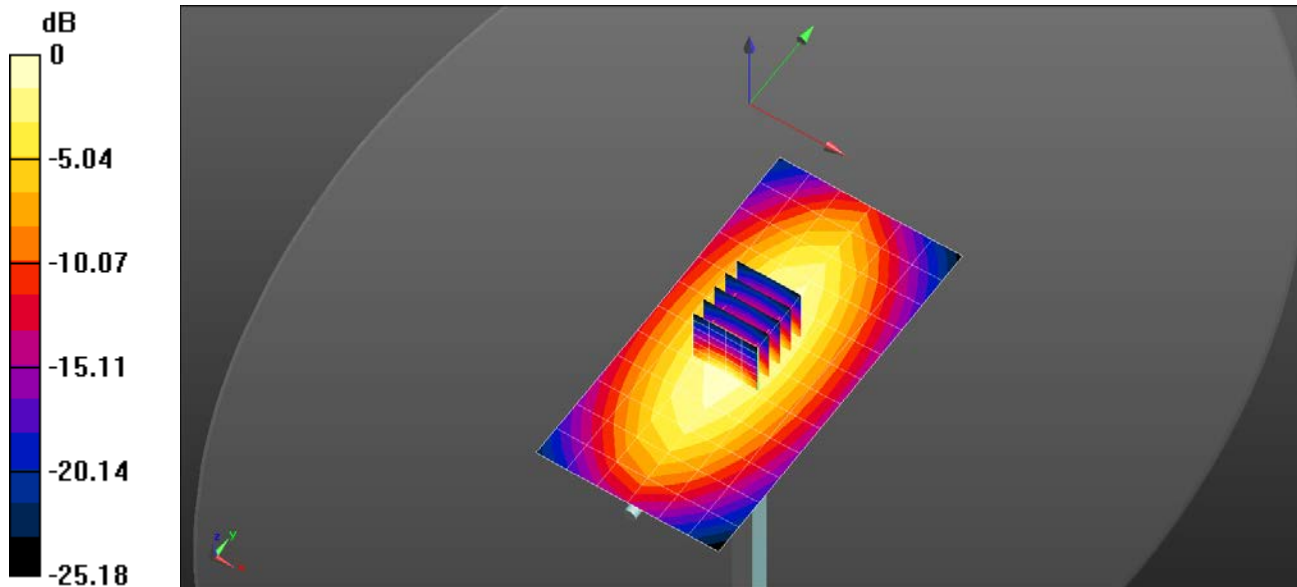

0 dB = 2.59 W/kg = 4.14 dBW/kg

System Check_H835

Frequency: 835 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.7°C; Liquid Temperature: 20.5°C
Medium parameters used: $f = 835$ MHz; $\sigma = 0.918$ S/m; $\epsilon_r = 42.065$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(9.37, 9.57, 8.97) @ 835 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x13x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 2.87 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 58.05 V/m; Power Drift = 0.04 dB


Peak SAR (extrapolated) = 3.31 W/kg

SAR(1 g) = 2.38 W/kg; SAR(10 g) = 1.61 W/kg

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 71.3%

Maximum value of SAR (measured) = 2.94 W/kg

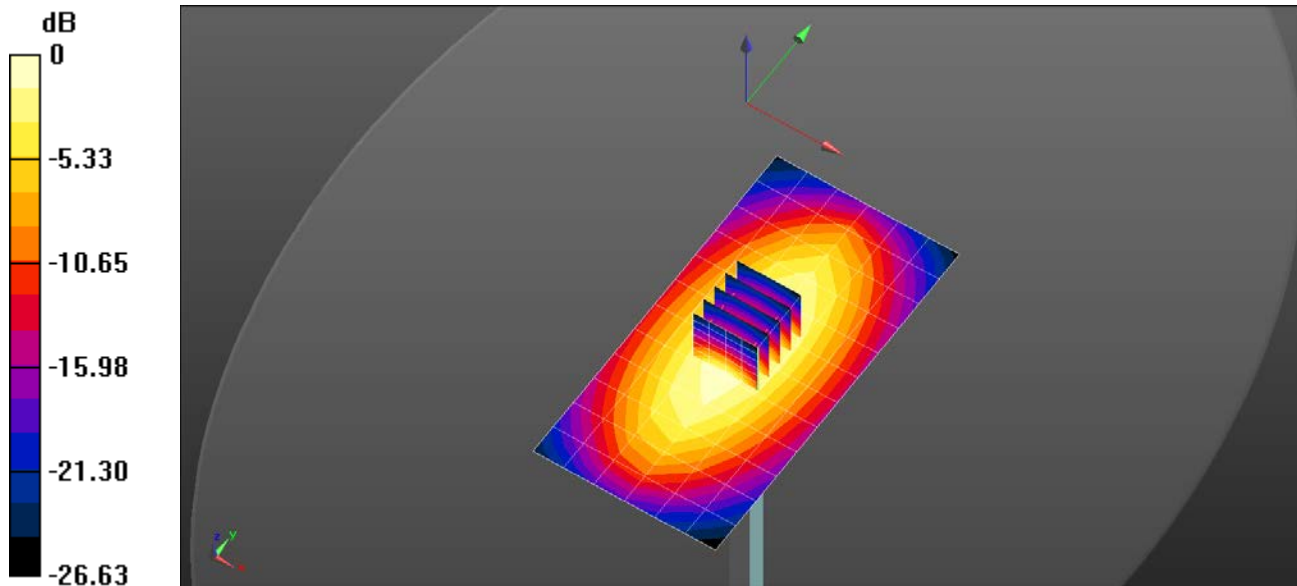

0 dB = 2.87 W/kg = 4.58 dBW/kg

System Check_H835

Frequency: 835 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.3°C; Liquid Temperature: 20.6°C
Medium parameters used: $f = 835$ MHz; $\sigma = 0.928$ S/m; $\epsilon_r = 43.115$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(9.37, 9.57, 8.97) @ 835 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x13x1):

Measurement grid: $dx=15$ mm, $dy=15$ mm

Maximum value of SAR (measured) = 3.01 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm

Reference Value = 59.29 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 3.38 W/kg

SAR(1 g) = 2.46 W/kg; SAR(10 g) = 1.67 W/kg

Smallest distance from peaks to all points 3 dB below = 17.6 mm

Ratio of SAR at M2 to SAR at M1 = 72%

Maximum value of SAR (measured) = 3.00 W/kg

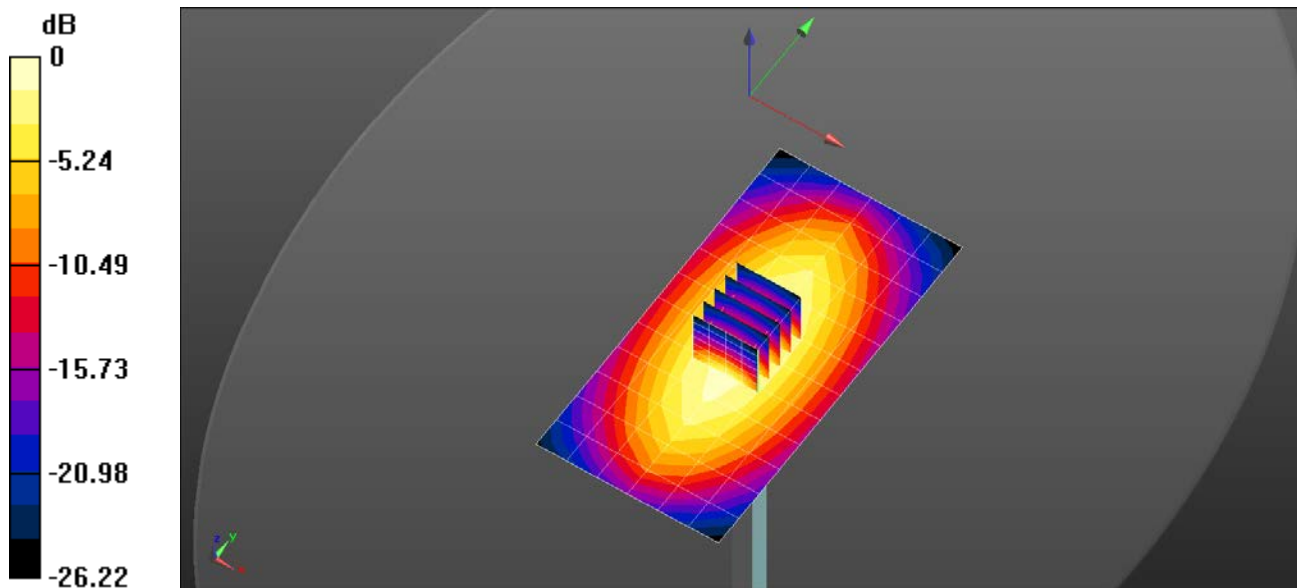

0 dB = 3.01 W/kg = 4.79 dBW/kg

System Check_H835

Frequency: 835 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 22.0°C; Liquid Temperature: 21.3°C
Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.918 \text{ S/m}$; $\epsilon_r = 42.137$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(9.37, 9.57, 8.97) @ 835 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x13x1):

Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (measured) = 3.01 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 59.53 V/m; Power Drift = 0.00 dB


Peak SAR (extrapolated) = 3.57 W/kg

SAR(1 g) = 2.39 W/kg; SAR(10 g) = 1.53 W/kg

Smallest distance from peaks to all points 3 dB below = 14.3 mm

Ratio of SAR at M2 to SAR at M1 = 66.3%

Maximum value of SAR (measured) = 3.09 W/kg

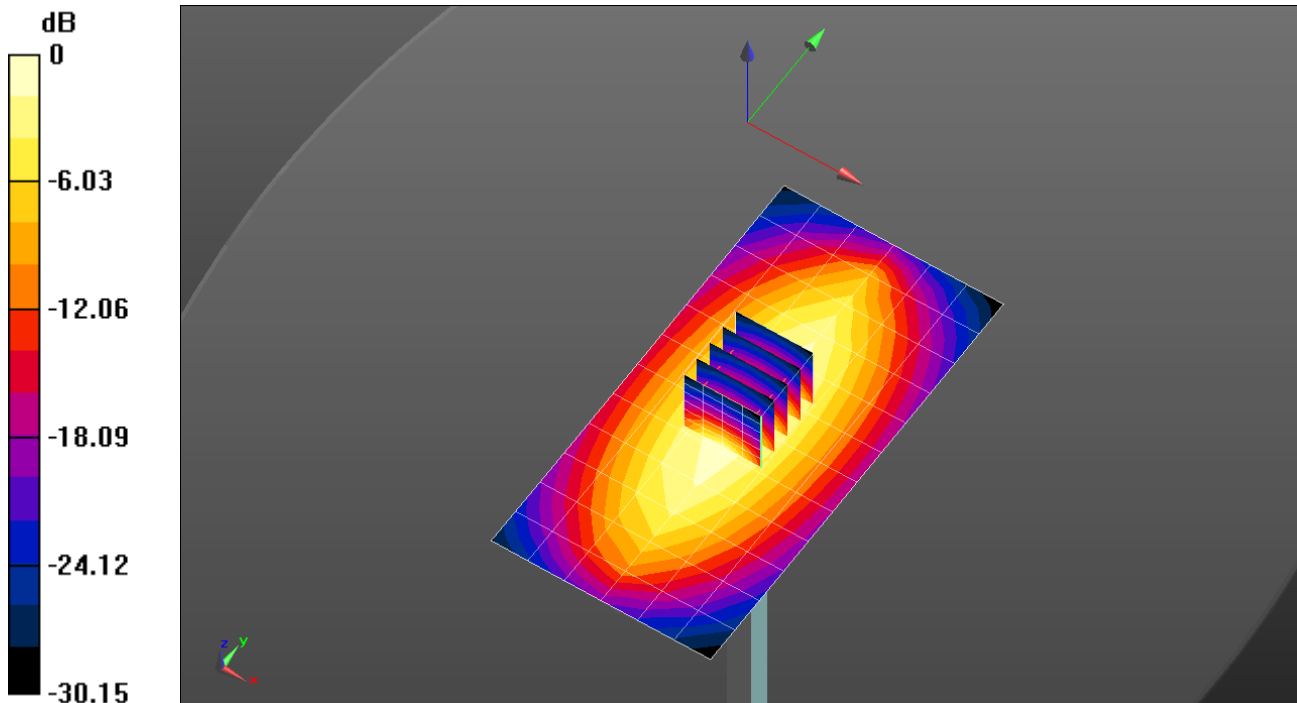

0 dB = 3.01 W/kg = 4.79 dBW/kg

System Check_H1800

Frequency: 1800 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.7°C; Liquid Temperature: 20.4°C
Medium parameters used: $f = 1800$ MHz; $\sigma = 1.464$ S/m; $\epsilon_r = 41.378$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(7.96, 8.13, 7.62) @ 1800 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x7x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 13.1 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 98.02 V/m; Power Drift = -0.00 dB


Peak SAR (extrapolated) = 15.8 W/kg

SAR(1 g) = 9.64 W/kg; SAR(10 g) = 5.28 W/kg

Smallest distance from peaks to all points 3 dB below = 11.2 mm

Ratio of SAR at M2 to SAR at M1 = 60.8%

Maximum value of SAR (measured) = 13.2 W/kg

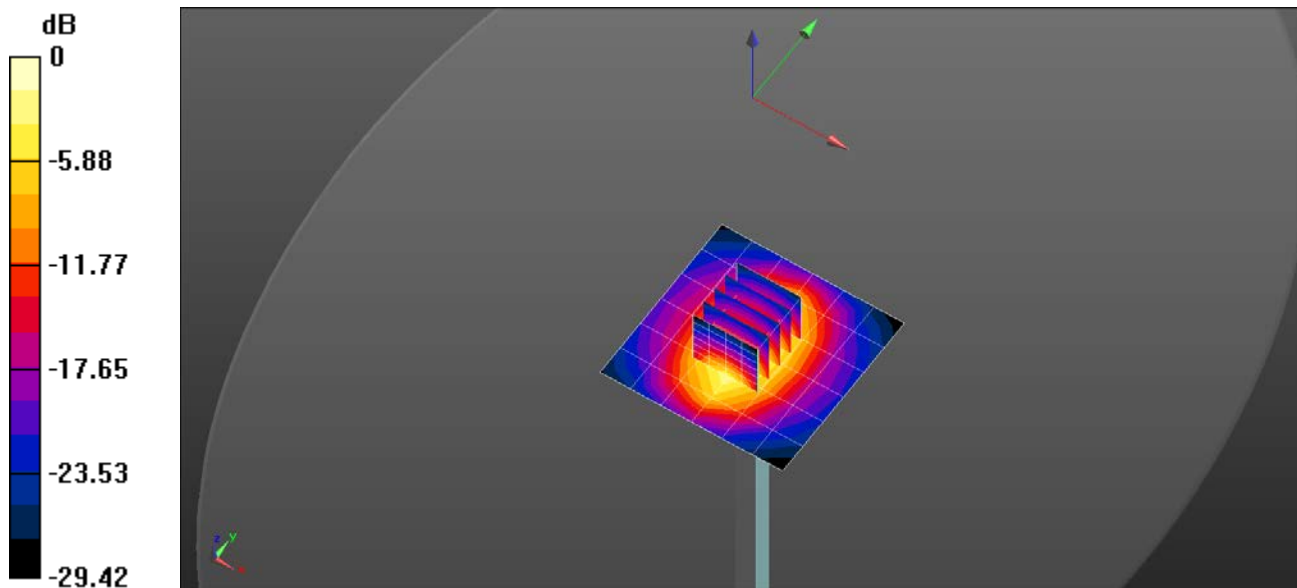

0 dB = 13.1 W/kg = 11.18 dBW/kg

System Check_H1800

Frequency: 1800 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.3°C; Liquid Temperature: 20.8°C
Medium parameters used: $f = 1800$ MHz; $\sigma = 1.434$ S/m; $\epsilon_r = 41.289$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(7.96, 8.13, 7.62) @ 1800 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x7x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 13.0 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 98.68 V/m; Power Drift = 0.13 dB


Peak SAR (extrapolated) = 15.9 W/kg

SAR(1 g) = 9.73 W/kg; SAR(10 g) = 5.3 W/kg

Smallest distance from peaks to all points 3 dB below = 10.1 mm

Ratio of SAR at M2 to SAR at M1 = 60.9%

Maximum value of SAR (measured) = 13.4 W/kg

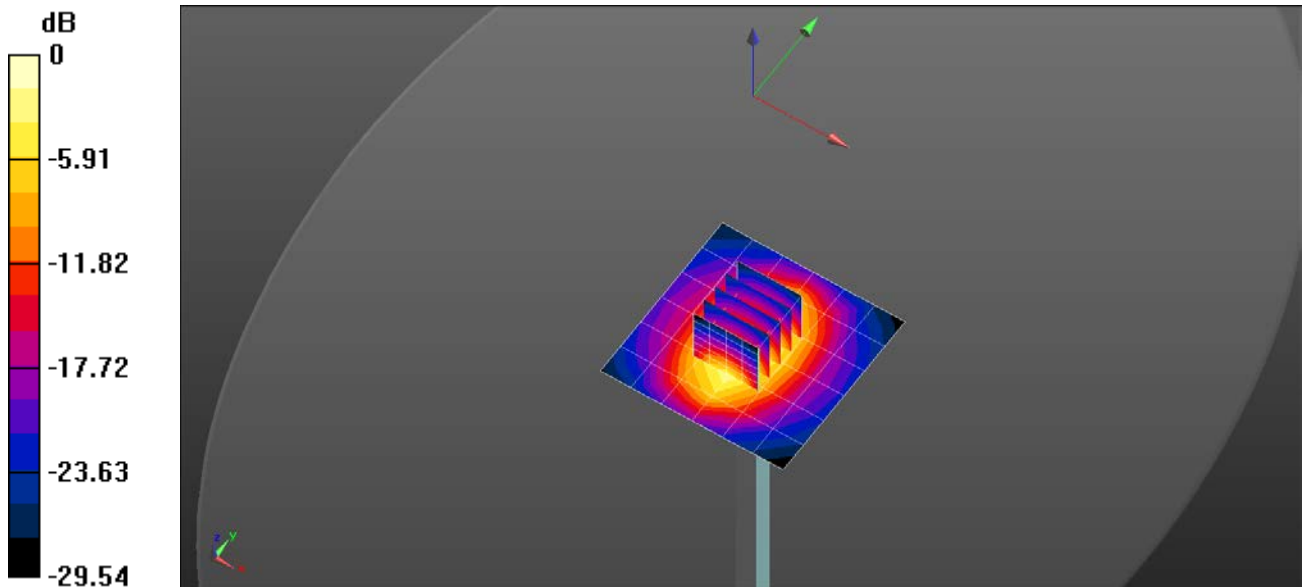

0 dB = 13.0 W/kg = 11.15 dBW/kg

System Check_H1900

Frequency: 1900 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.1°C; Liquid Temperature: 20.3°C
Medium parameters used: $f = 1900$ MHz; $\sigma = 1.397$ S/m; $\epsilon_r = 38.876$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(7.72, 7.88, 7.39) @ 1900 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x7x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 14.7 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 103.3 V/m; Power Drift = -0.01 dB



Peak SAR (extrapolated) = 16.8 W/kg

SAR(1 g) = 10 W/kg; SAR(10 g) = 5.41 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 59.8%

Maximum value of SAR (measured) = 14.8 W/kg

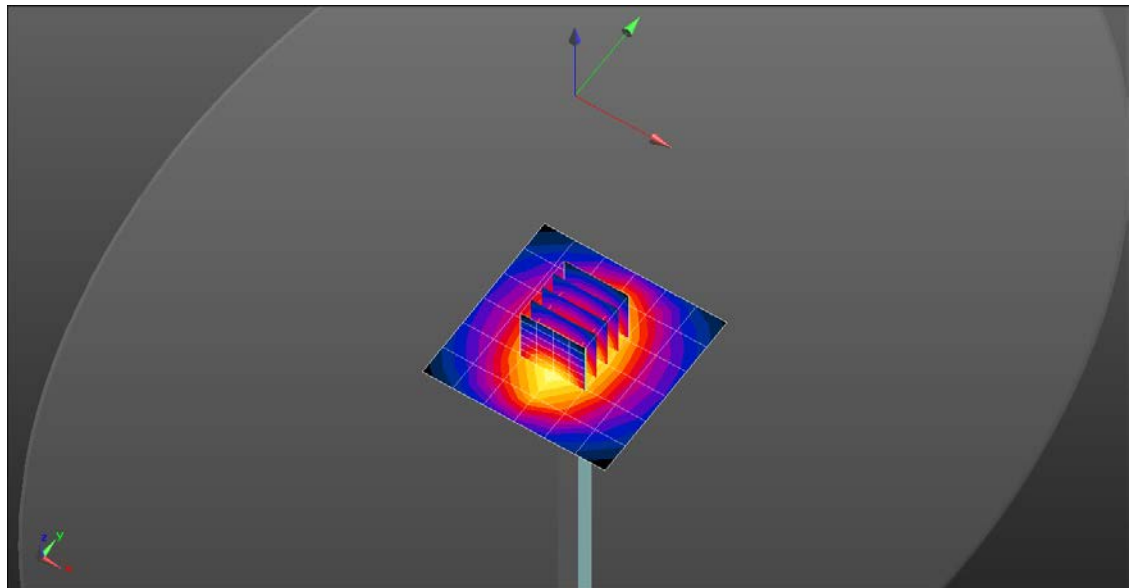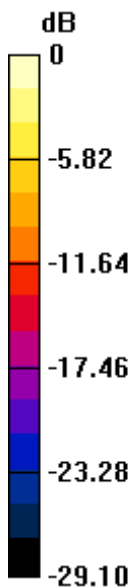

0 dB = 14.7 W/kg = 11.68 dBW/kg

System Check_H1900

Frequency: 1900 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.3°C; Liquid Temperature: 20.5°C
Medium parameters used: $f = 1900$ MHz; $\sigma = 1.388$ S/m; $\epsilon_r = 40.452$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(7.72, 7.88, 7.39) @ 1900 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x7x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 11.9 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 95.18 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 16.0 W/kg

SAR(1 g) = 9.69 W/kg; SAR(10 g) = 5.23 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 60.2%

Maximum value of SAR (measured) = 13.3 W/kg

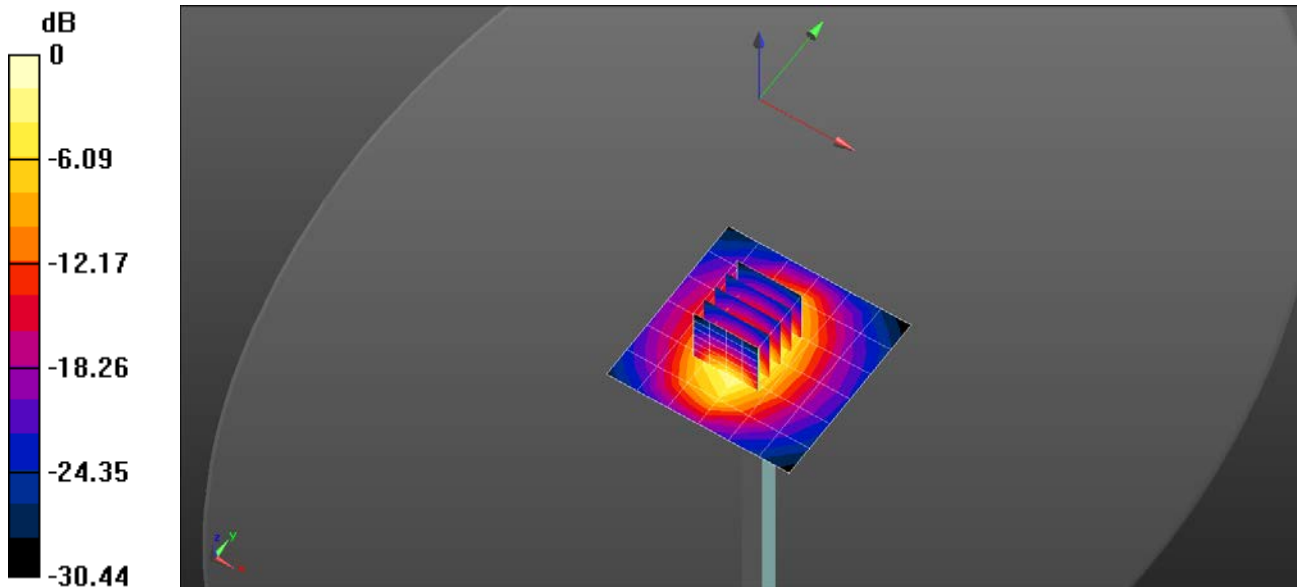

0 dB = 11.9 W/kg = 10.74 dBW/kg

System Check_H1900

Frequency: 1900 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 22.0°C; Liquid Temperature: 20.9°C

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.396$ S/m; $\epsilon_r = 39.36$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(7.72, 7.88, 7.39) @ 1900 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 2mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 2mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (7x7x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 13.2 W/kg

Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 101.0 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 16.5 W/kg

SAR(1 g) = 9.88 W/kg; SAR(10 g) = 5.34 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 59.6%

Maximum value of SAR (measured) = 13.6 W/kg

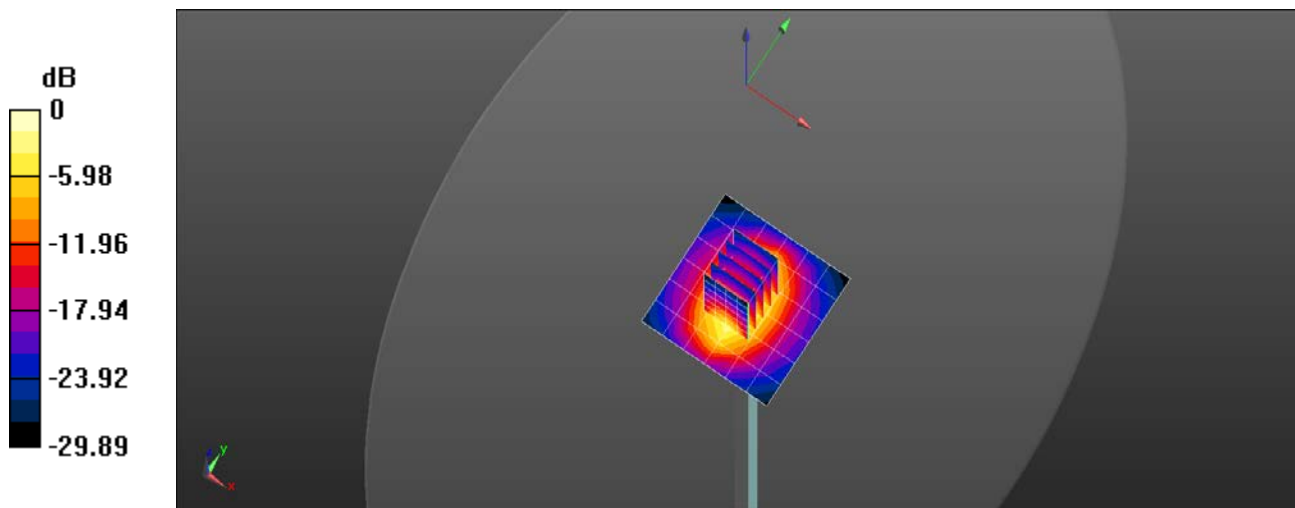

0 dB = 13.2 W/kg = 11.21 dBW/kg

System Check_H2600

Frequency: 2600 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.2°C; Liquid Temperature: 21.0°C
Medium parameters used: $f = 2600$ MHz; $\sigma = 1.942$ S/m; $\epsilon_r = 39.553$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(7.12, 7.26, 6.81) @ 2600 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (9x9x1):

Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 24.1 W/kg

Configuration/Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 119.3 V/m; Power Drift = -0.09 dB


Peak SAR (extrapolated) = 29.1 W/kg

SAR(1 g) = 14.7 W/kg; SAR(10 g) = 6.75 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 52.3%

Maximum value of SAR (measured) = 23.2 W/kg

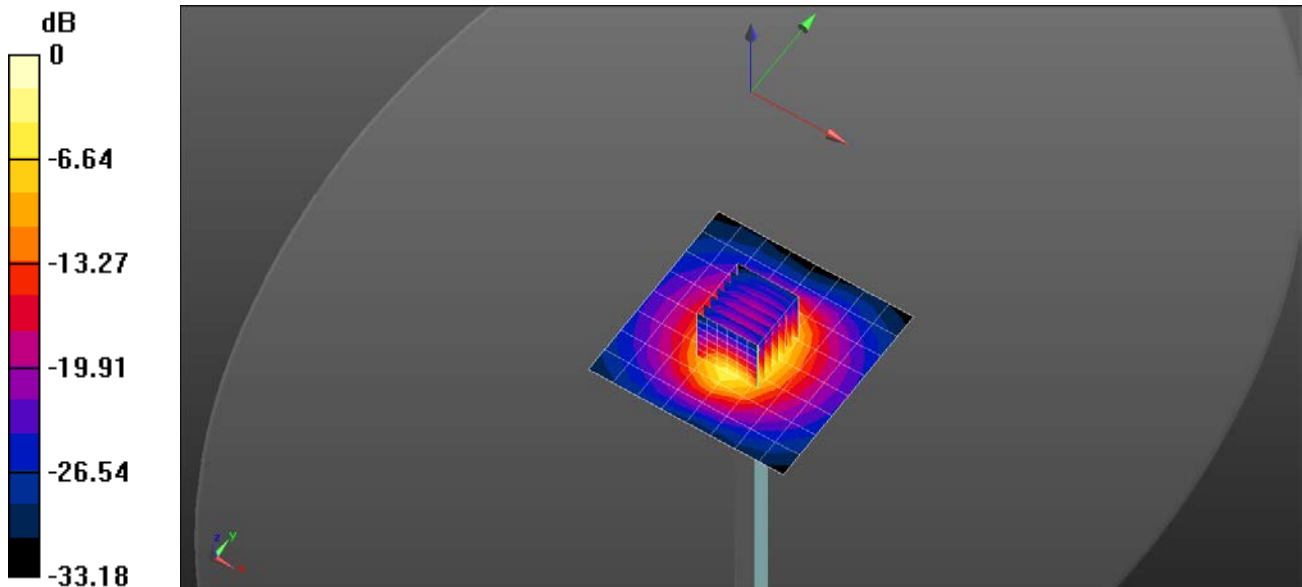

0 dB = 24.1 W/kg = 13.81 dBW/kg

System Check_H2600

Frequency: 2600 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.2°C; Liquid Temperature: 20.3°C
Medium parameters used: $f = 2600$ MHz; $\sigma = 1.945$ S/m; $\epsilon_r = 39.915$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(7.12, 7.26, 6.81) @ 2600 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (9x9x1):

Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 23.7 W/kg

Configuration/Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 114.8 V/m; Power Drift = -0.07 dB


Peak SAR (extrapolated) = 28.7 W/kg

SAR(1 g) = 14.8 W/kg; SAR(10 g) = 6.85 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 52.2%

Maximum value of SAR (measured) = 24.0 W/kg

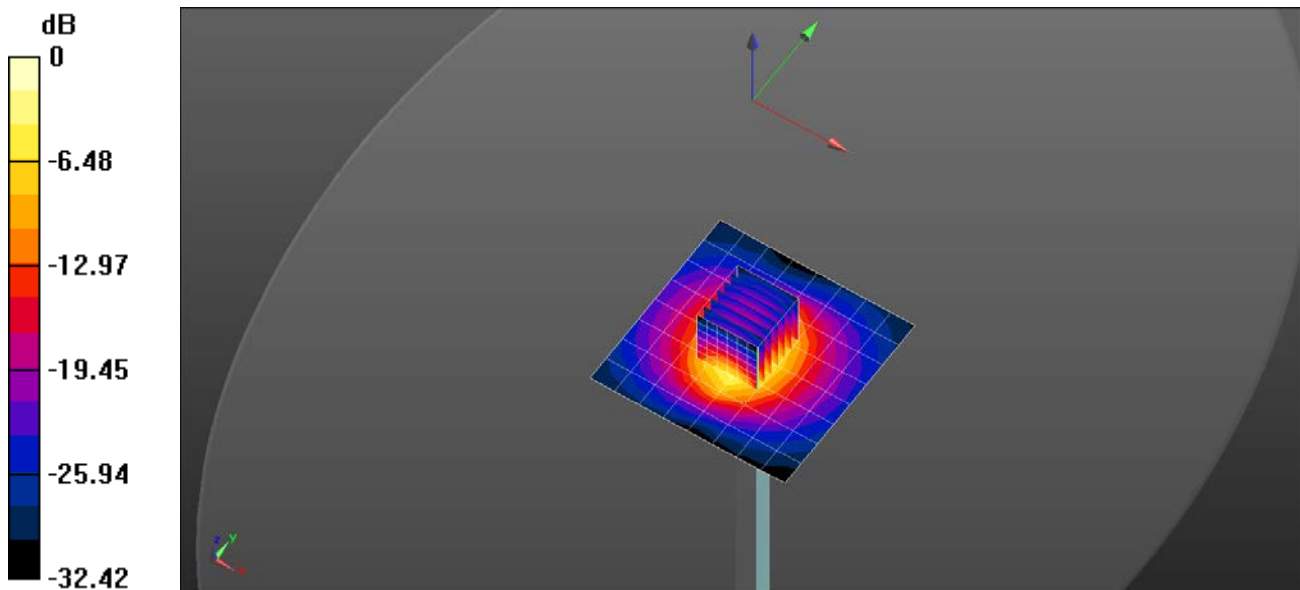

0 dB = 23.7 W/kg = 13.75 dBW/kg

System Check_H2600

Frequency: 2600 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.2°C; Liquid Temperature: 20.1°C
Medium parameters used: $f = 2600$ MHz; $\sigma = 1.985$ S/m; $\epsilon_r = 40.6$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(7.12, 7.26, 6.81) @ 2600 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=250mW/Area Scan (9x9x1):

Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 23.7 W/kg

Configuration/Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 112.9 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 26.8 W/kg

SAR(1 g) = 13.8 W/kg; SAR(10 g) = 6.4 W/kg

Smallest distance from peaks to all points 3 dB below = 8.5 mm

Ratio of SAR at M2 to SAR at M1 = 52.4%

Maximum value of SAR (measured) = 22.5 W/kg

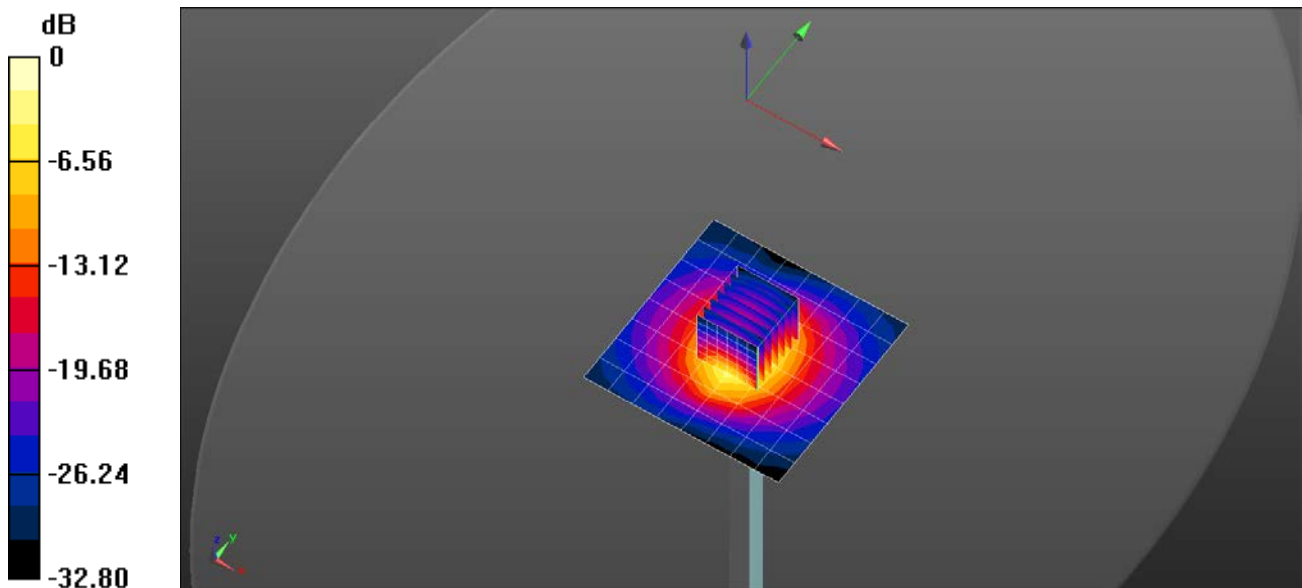

0 dB = 23.7 W/kg = 13.75 dBW/kg

System Check_H3700

Frequency: 3700 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.6°C; Liquid Temperature: 20.7°C
Medium parameters used: $f = 3700$ MHz; $\sigma = 3.072$ S/m; $\epsilon_r = 35.892$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(6.63, 6.77, 6.34) @ 3700 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=100mW/Area Scan (10x10x1):

Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 8.65 W/kg

Configuration/Pin=100mW/Zoom Scan (7x7x12)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 67.89 V/m; Power Drift = -0.02 dB



Peak SAR (extrapolated) = 16.6 W/kg

SAR(1 g) = 6.4 W/kg; SAR(10 g) = 2.44 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 67.1%

Maximum value of SAR (measured) = 12.3 W/kg

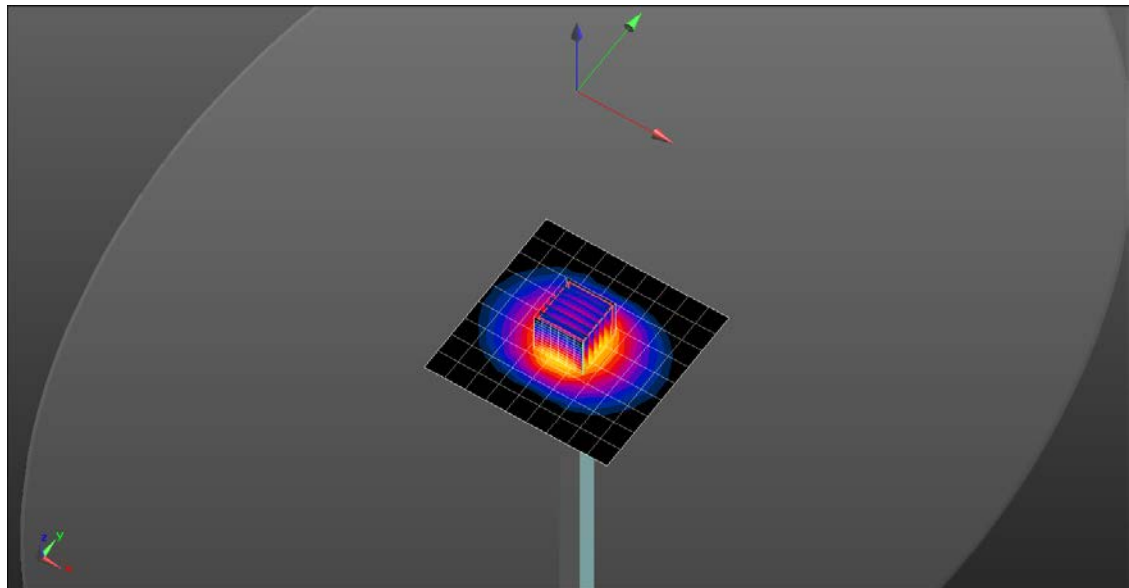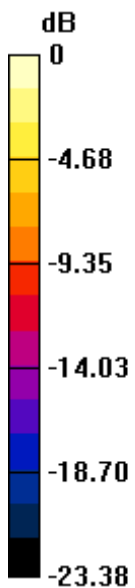

0 dB = 12.3 W/kg = 10.90 dBW/kg

System Check_H3700

Frequency: 3700 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 21.2°C; Liquid Temperature: 20.2°C
 Medium parameters used: $f = 3700$ MHz; $\sigma = 3.068$ S/m; $\epsilon_r = 37.837$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1486; Calibrated: 2025/6/24
- Probe: EX3DV4 - SN7369; ConvF(6.63, 6.77, 6.34) @ 3700 MHz; Calibrated: 2025/5/21
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: ELI V5.0 (20deg probe tilt); Type: QD OVA 002 AA; Serial: 1240

Configuration/Pin=100mW/Area Scan (10x10x1):

Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 11.8 W/kg

Configuration/Pin=100mW/Zoom Scan (7x7x12)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 66.85 V/m; Power Drift = 0.13 dB


Peak SAR (extrapolated) = 17.6 W/kg

SAR(1 g) = 7.08 W/kg; SAR(10 g) = 2.68 W/kg

Smallest distance from peaks to all points 3 dB below = 8.4 mm

Ratio of SAR at M2 to SAR at M1 = 68.9%

Maximum value of SAR (measured) = 13.6 W/kg

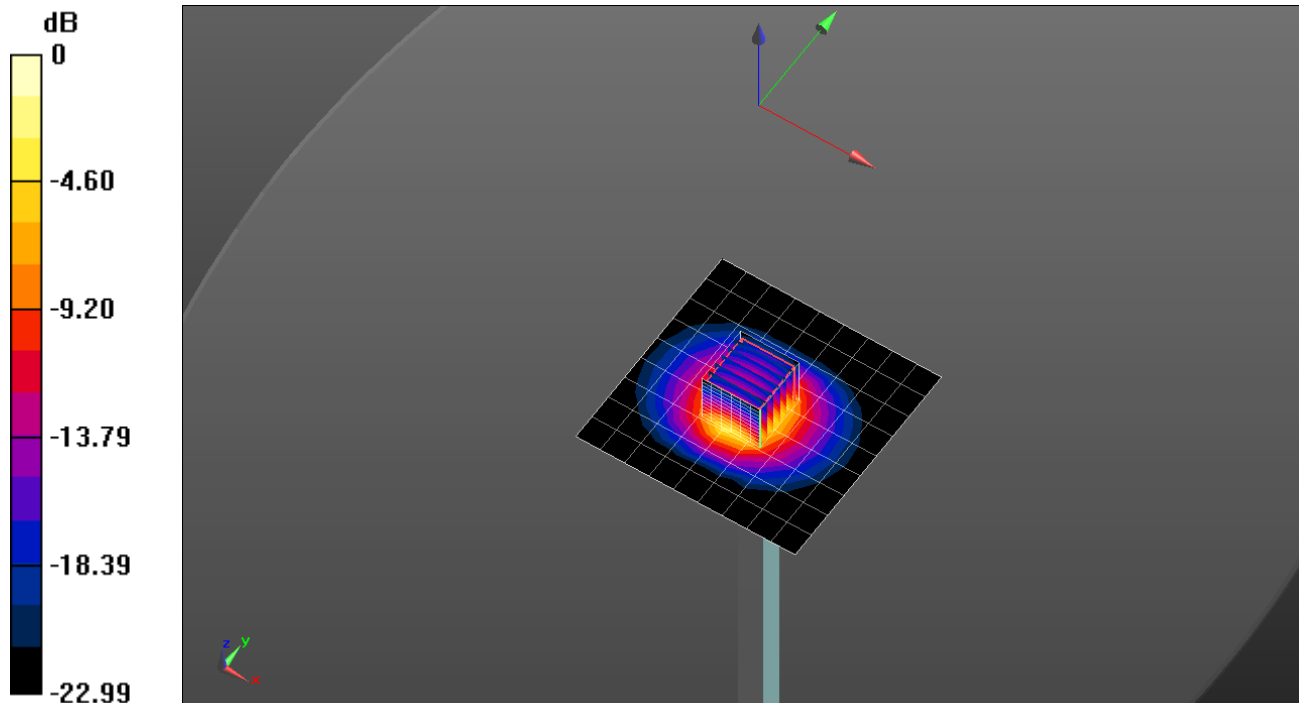

0 dB = 13.6 W/kg = 11.34 dBW/kg