

Date: 2024-08-08

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.77$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.47, 8.61, 7.55); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2024-07-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 12.0 mm

SAR (1g) = 2.76 W/kg; SAR (10g) = 1.28 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0mmx 1.5 mm

Power Drift = 0.11 dB

SAR (1g) = 2.80 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.4 %

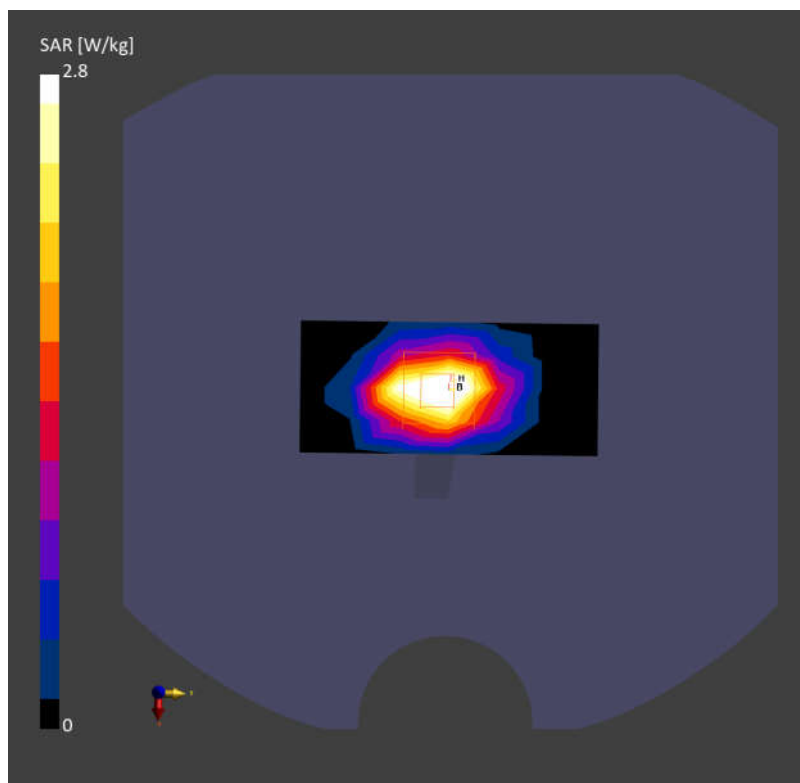

Date: 2024-08-10

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.58$ S/m; $\epsilon_r = 35.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.84, 6.82, 5.88); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2024-07-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.74 W/kg; SAR (10g) = 1.12 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0mm x 1.4 mm

Power Drift = 0.09 dB

SAR (1g) = 4.17 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 6.5 mm

Ratio of SAR at M2 to SAR at M1 = 65.9 %

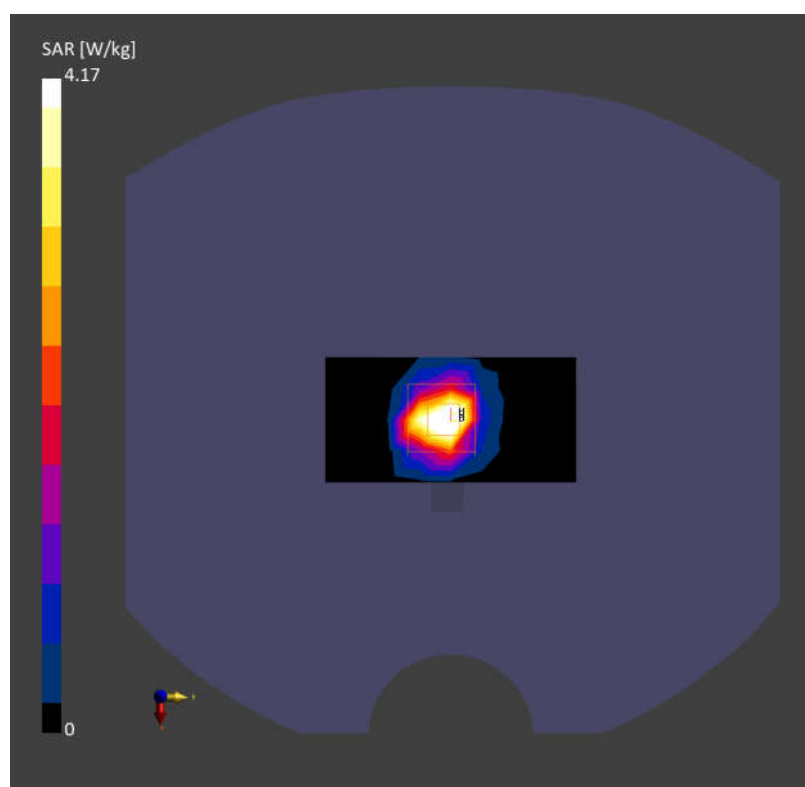

Date: 2024-08-10

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.91$ S/m; $\epsilon_r = 34.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(4.83, 5.71, 4.9); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2024-07-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.88 W/kg; SAR (10g) = 1.14 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 4.34 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 6.9 mm

Ratio of SAR at M2 to SAR at M1 = 61.0 %

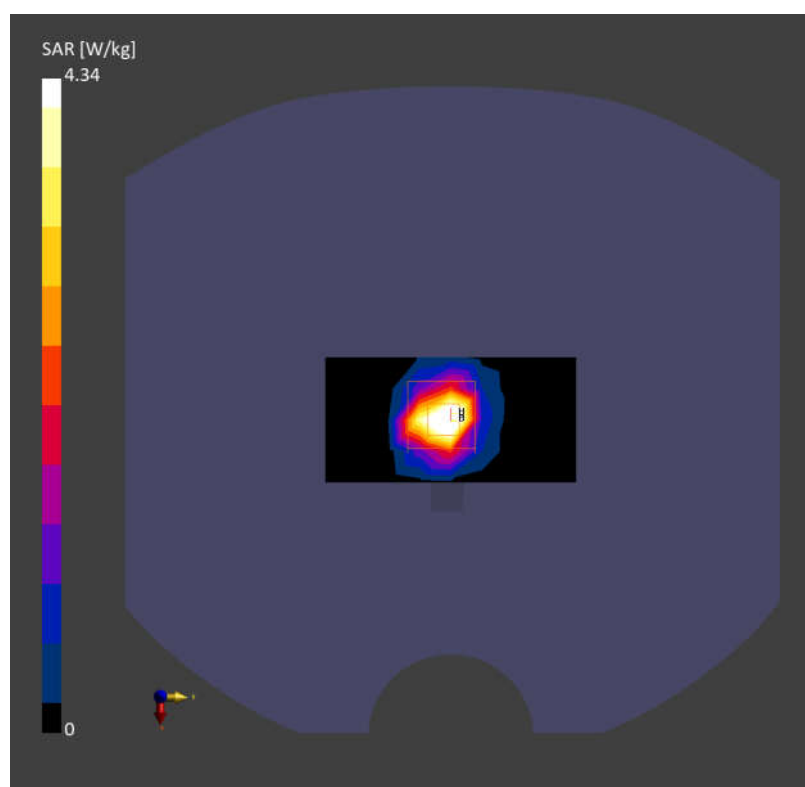

Date: 2024-08-10

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.11$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.03, 5.88, 5.16); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2024-07-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.50 W/kg; SAR (10g) = 1.04 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 3.90 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 6.5 mm

Ratio of SAR at M2 to SAR at M1 = 63.7 %

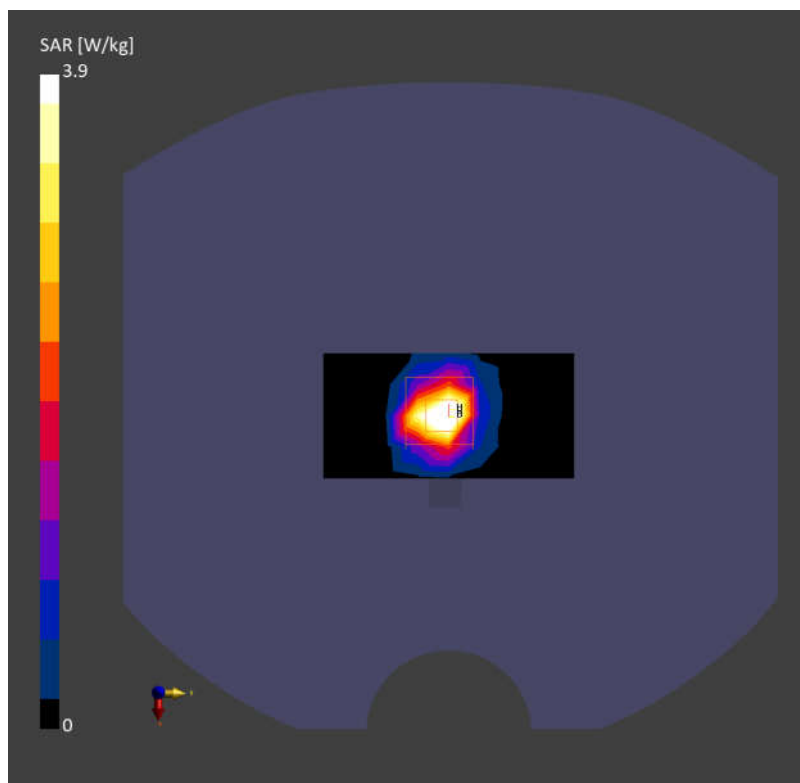

Date: 2024-08-10

System Check_Head_6500MHz**DUT:D6.5GHzV2 - SN:1031**

Communication System: ; Frequency: 6500.000

Medium: HSL. Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.16$ S/m; $\epsilon_r = 34.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.27, 6.32, 5.24); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2024-07-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.4.0.5005

Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 12.0 W/kg; SAR (10g) = 2.55 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm;
Graded Ratio: 1.4

Power Drift = -0.01 dB

SAR (1g) = 13.8 W/kg; SAR (10g) = 2.59 W/kg;

psAPD (4.0cm², sq) = 60.9[W/m²]

Smallest distance from peaks to all points 3dB below is 4.1 mm

Ratio of SAR at M2 to SAR at M1 = 50.7 %

