

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid Depth

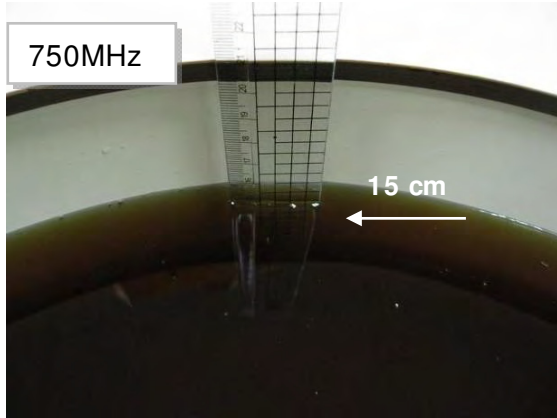


Fig.2.1

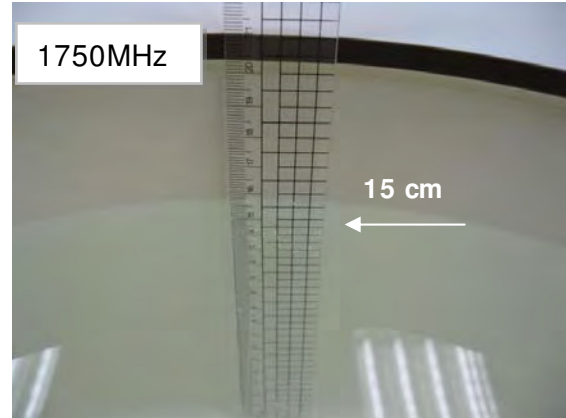


Fig.2.2

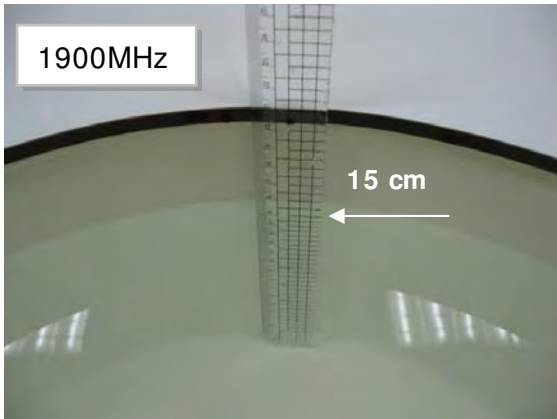


Fig.2.3

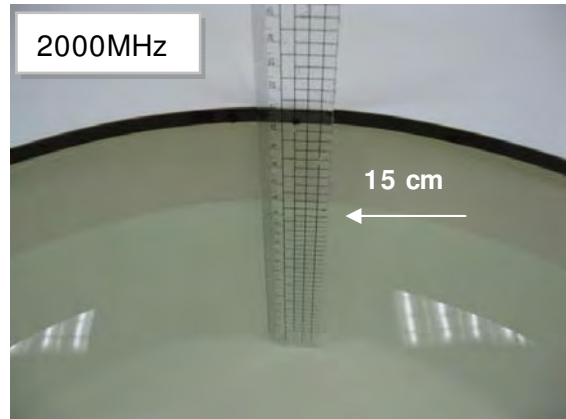


Fig.2.4

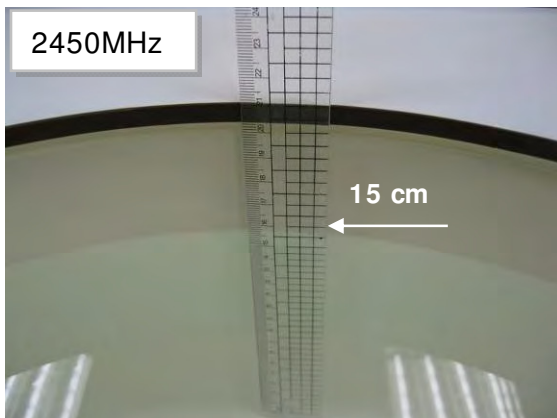


Fig.2.5

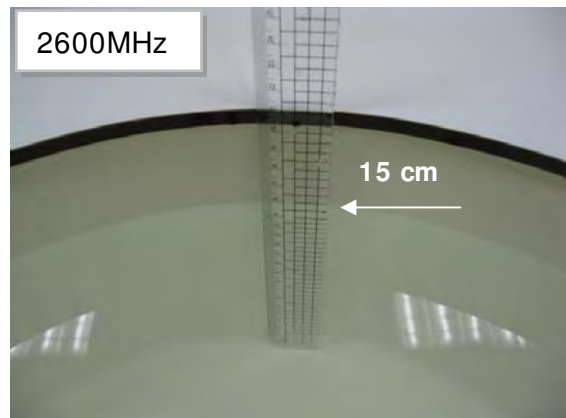


Fig.2.6

Photograph of the Tissue Simulant Fluid Liquid Depth

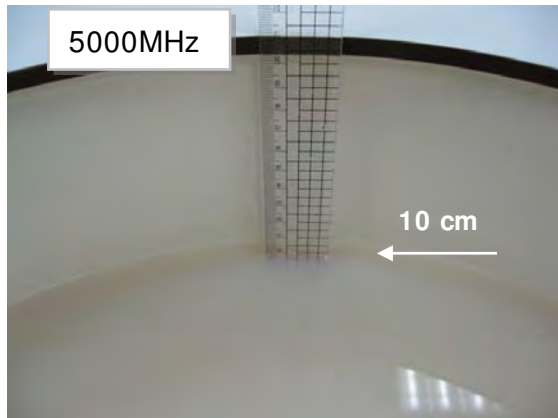


Fig.2.7

Body - distance between flat phantom and EUT is 0 mm & 17mm

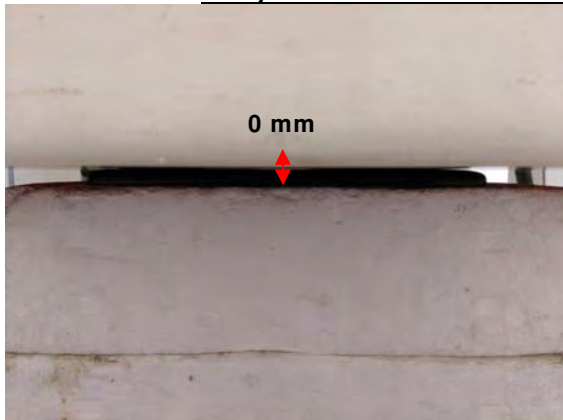


Fig.3 EUT Back side to flat phantom

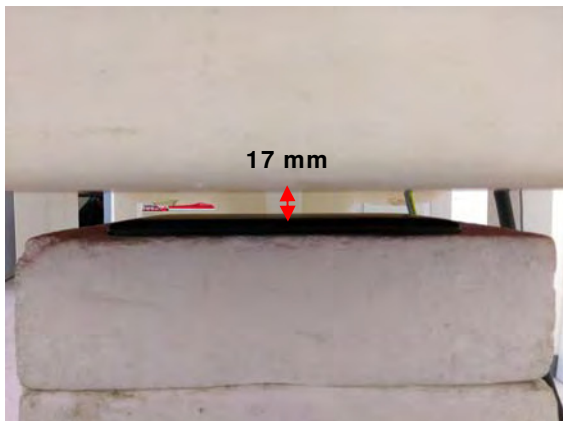


Fig.4 EUT Back side (17mm) to flat phantom

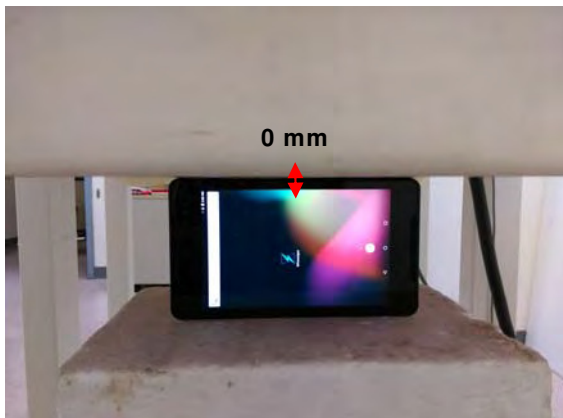


Fig.5 EUT Right side to flat phantom

Body - distance between flat phantom and EUT is 0 mm & 13mm

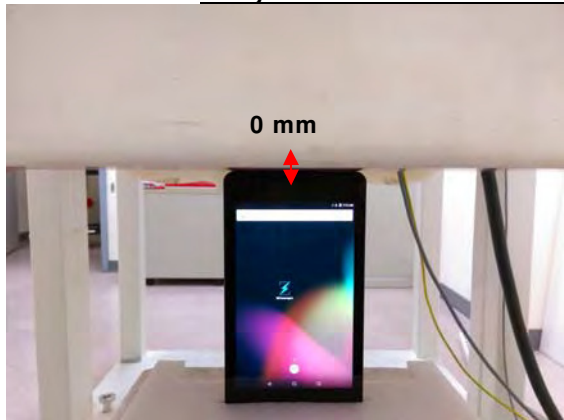


Fig.6 EUT Top side to flat phantom

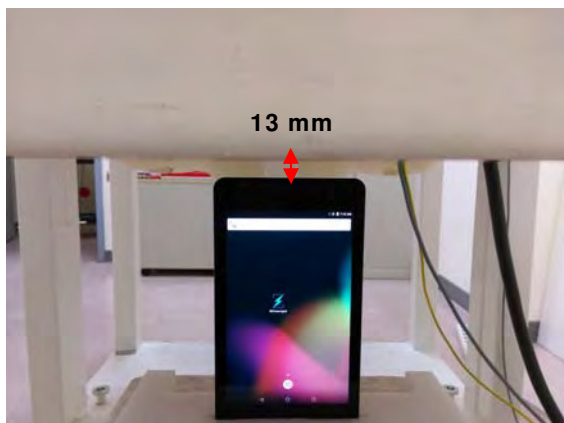


Fig.7 EUT Top side (13mm) to flat phantom



Fig.8 EUT Left side to flat phantom



Body - distance between flat phantom and EUT is 0 mm & 15mm



Fig.9 EUT Left side (15mm) to flat phantom



Fig.10 EUT Bottom side to flat phantom

12. Photographs of the EUT



Fig.11 Front view of EUT



Fig.12 Back view of EUT

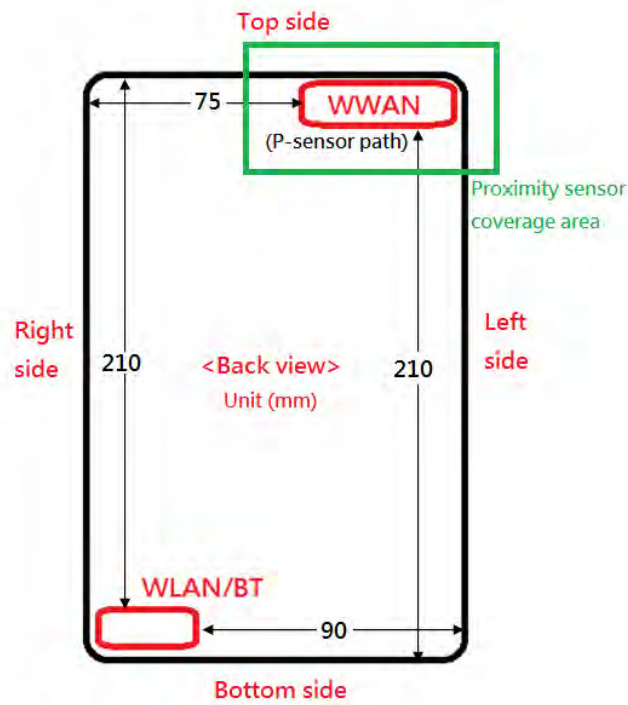


Fig.13 Antenna position of EUT (Front view)

- End of Report -