


EX3DV4 - SN:7957

October 06, 2025

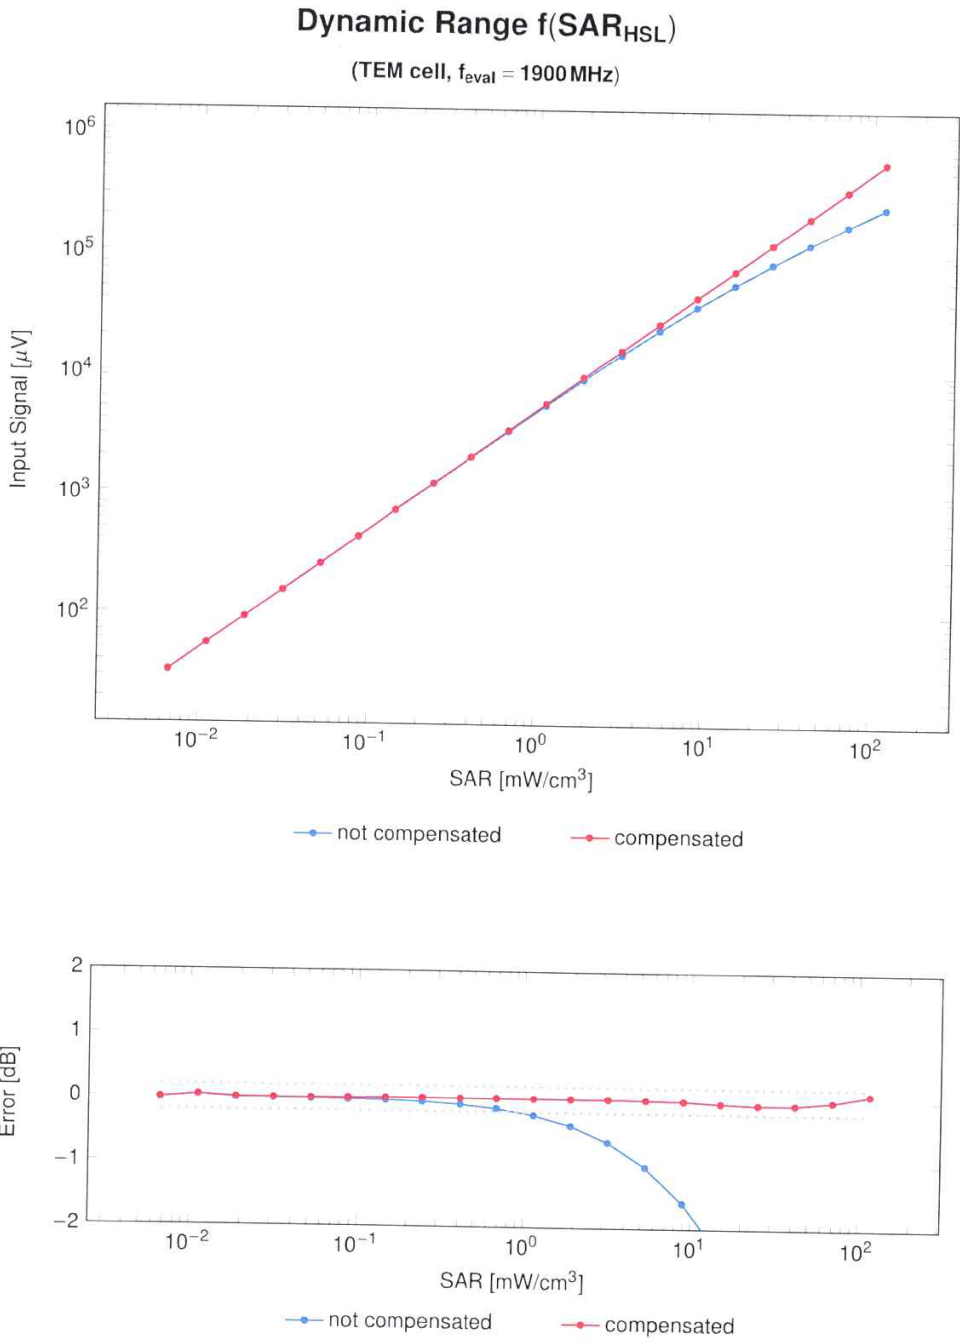


Uncertainty of Linearity Assessment: ±0.6% (k=2)

EX3DV4 - SN:7957

October 06, 2025

Conversion Factor Assessment

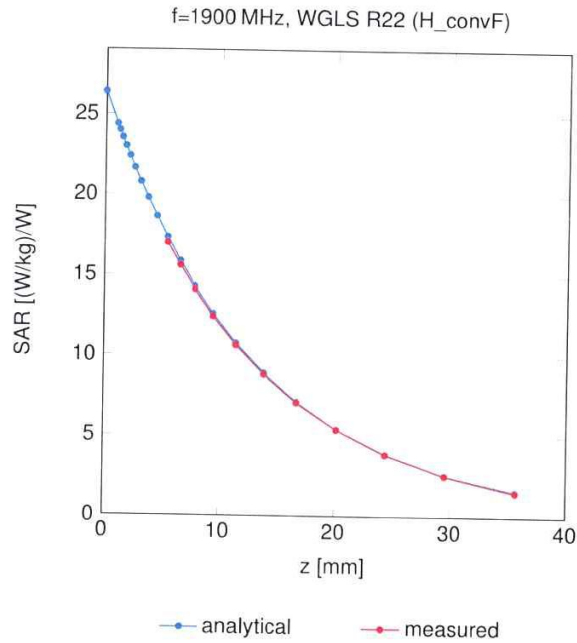

Deviation from Isotropy in Liquid

Error (ϕ, θ), $f = 900\text{ MHz}$

