

Date: 2025/11/25

System Check_750MHz**DUT:D750V3-SN:1099**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.882$ S/m; $\epsilon_r = 43.5$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(9.71, 9.32, 9.31); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (42.0 mm x 210.0 mm): Measurement Grid: 7.0 mm x 15.0 mm
SAR (1g) = 2.17 W/kg; SAR (10g) = 1.40 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.15 W/kg; SAR (10g) = 1.40 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 87.3 %

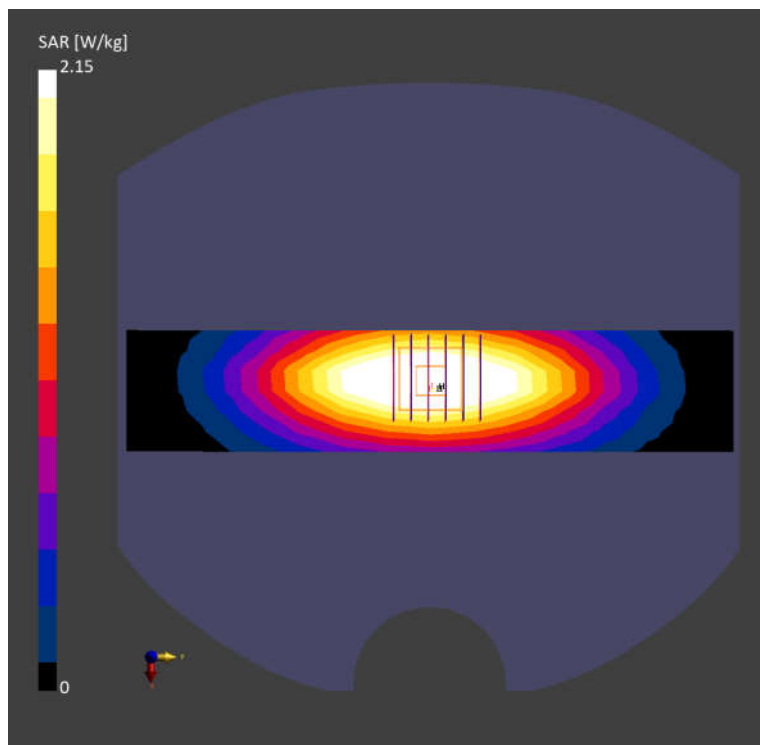

Date: 2025/11/27

System Check_750MHz**DUT:D750V3-SN:1099**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(9.71, 9.32, 9.31); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 2.16 W/kg; SAR (10g) = 1.41 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.14 W/kg; SAR (10g) = 1.39 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

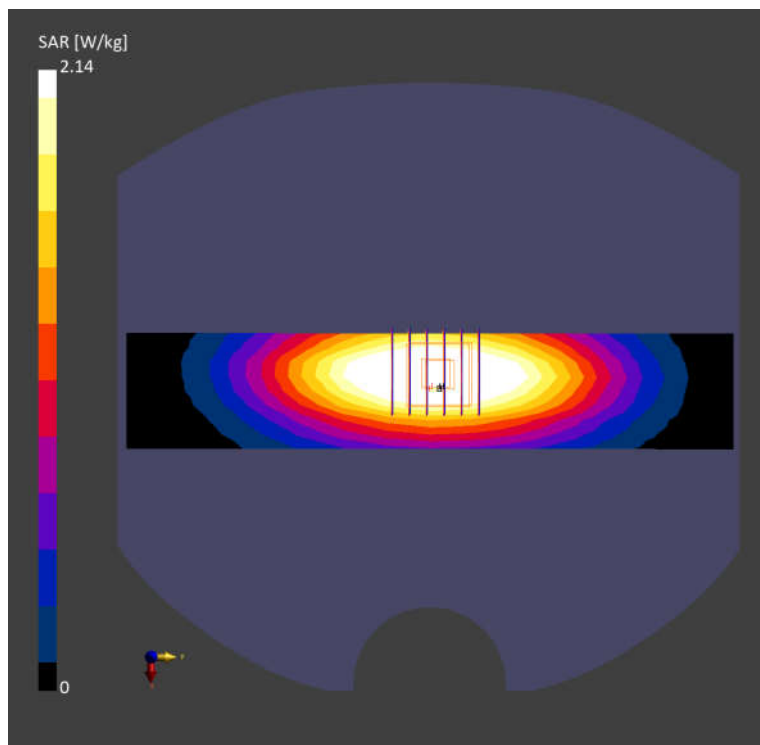

Date: 2025/12/2

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.914$ S/m; $\epsilon_r = 43.3$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(9.59, 9.21, 9.2); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 2.32 W/kg; SAR (10g) = 1.53 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.25 W/kg; SAR (10g) = 1.51 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

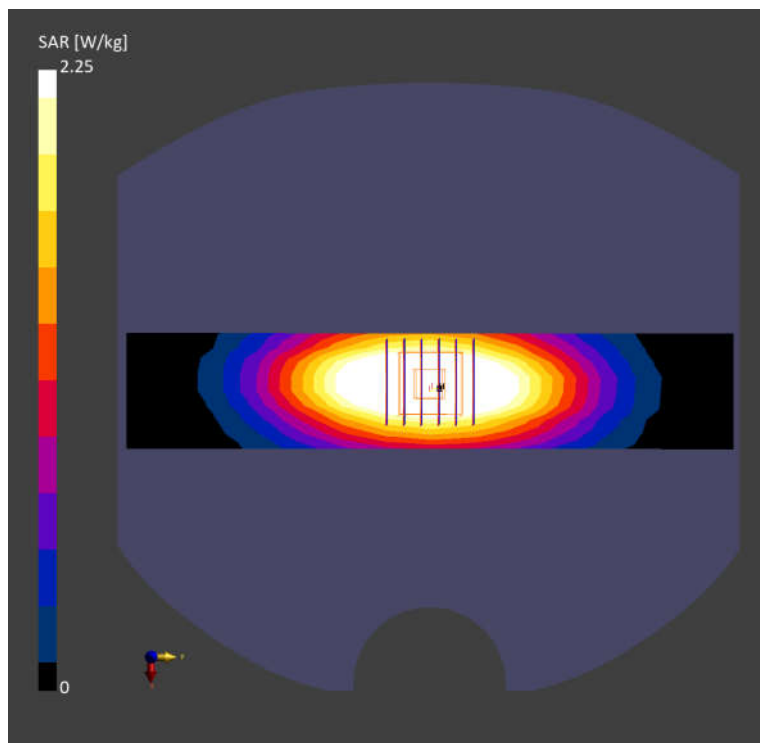

Date: 2025/12/5

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.919$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(9.59, 9.21, 9.2); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (42.0 mm x 210.0 mm): Measurement Grid: 7.0 mm x 15.0 mm
SAR (1g) = 2.43 W/kg; SAR (10g) = 1.55 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.37 W/kg; SAR (10g) = 1.51 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 88.5 %

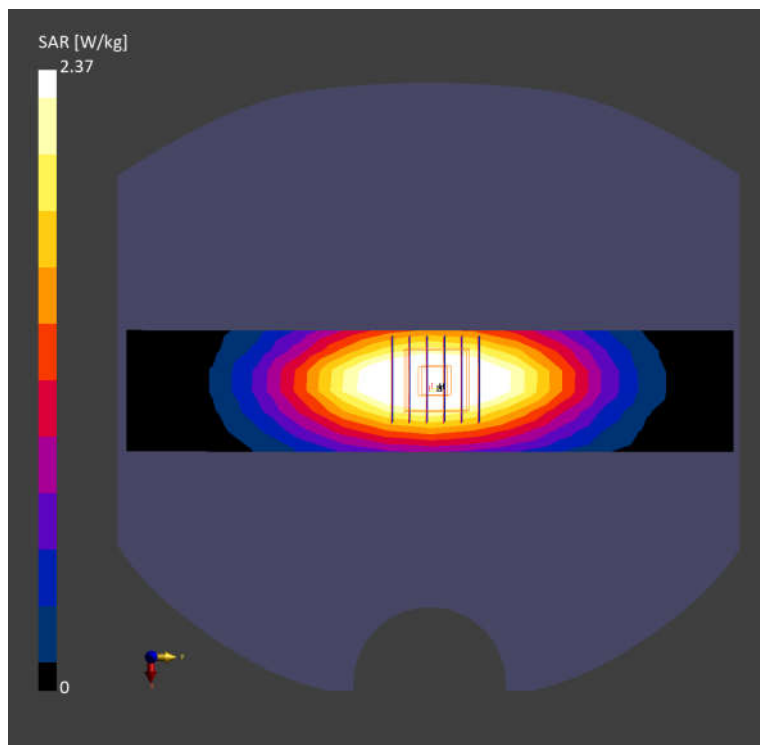

Date: 2025/12/9

System Check_1750MHz**DUT:D1750V2-SN:1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(8.14, 7.82, 7.81); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 9.27 W/kg; SAR (10g) = 5.00 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 9.18 W/kg; SAR (10g) = 4.95 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

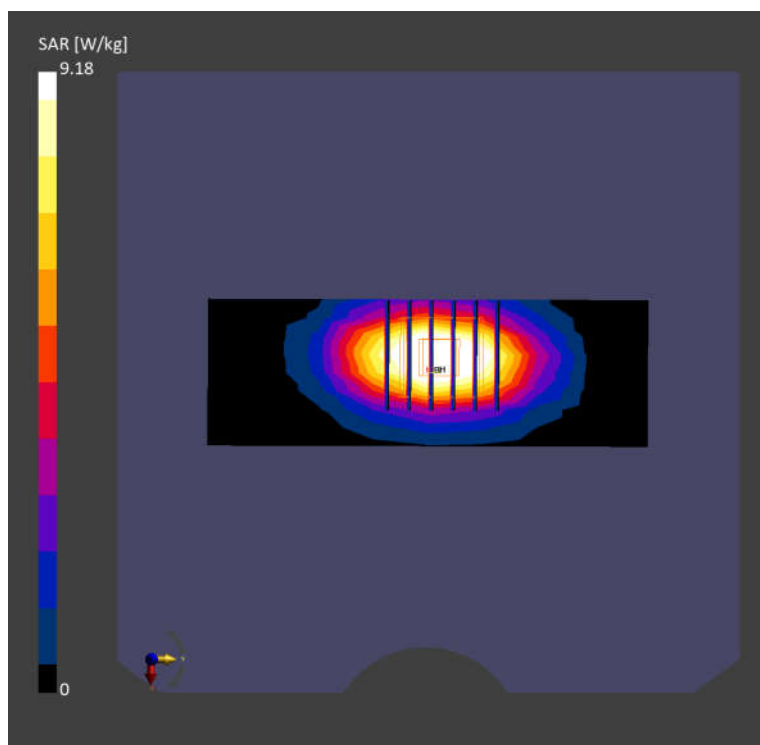

Date: 2025/12/11

System Check_1750MHz**DUT:D1750V2-SN:1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(8.14, 7.82, 7.81); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 8.82 W/kg; SAR (10g) = 4.75 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 8.81 W/kg; SAR (10g) = 4.69 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 82.8 %

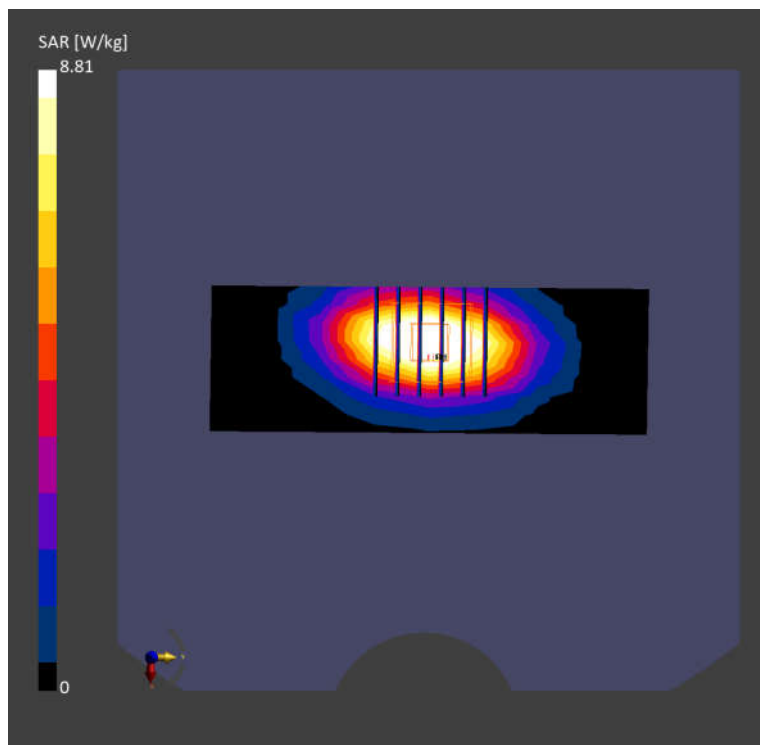

Date: 2025/12/13

System Check_1900MHz**DUT:D1900V2-SN:5d182**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.9, 7.58, 7.57); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 10.3 W/kg; SAR (10g) = 5.38 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 10.1 W/kg; SAR (10g) = 5.32 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

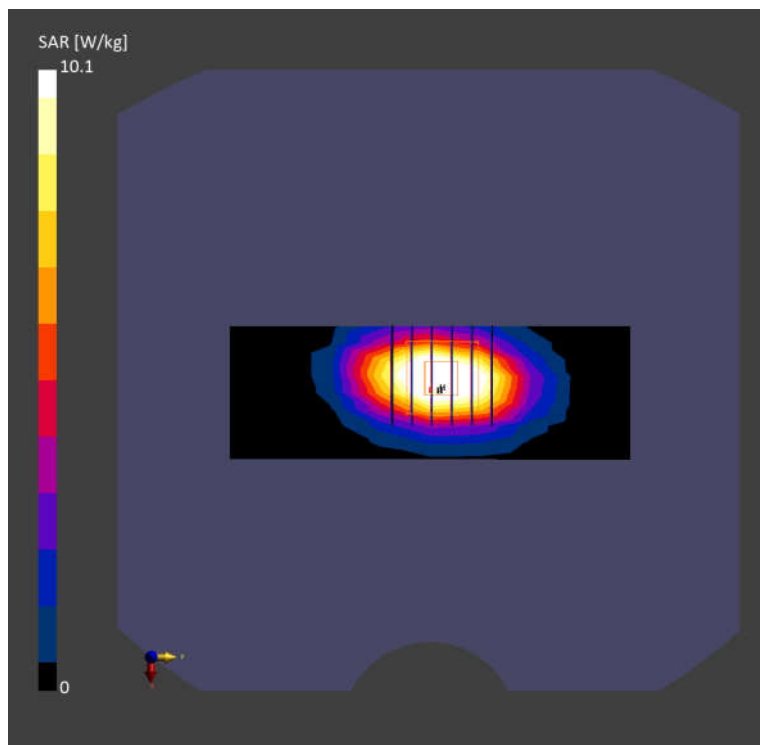

Date: 2025/12/14

System Check_1900MHz**DUT:D1900V2-SN:5d182**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.9, 7.58, 7.57); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 9.85 W/kg; SAR (10g) = 5.19 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 9.73 W/kg; SAR (10g) = 5.01 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 81.2 %

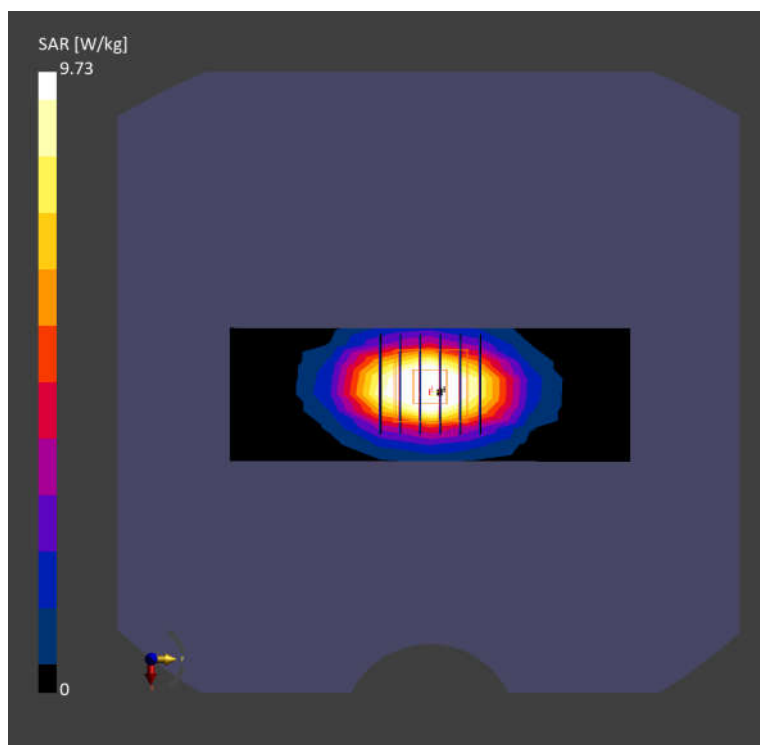

Date: 2025/11/26

System Check_2300MHz**DUT:D2300V2-SN:1055**

Communication System: CW; Frequency: 2300.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.72$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.24, 8.09, 8.13); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 12.2 W/kg; SAR (10g) = 5.88 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 11.9 W/kg; SAR (10g) = 5.68 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

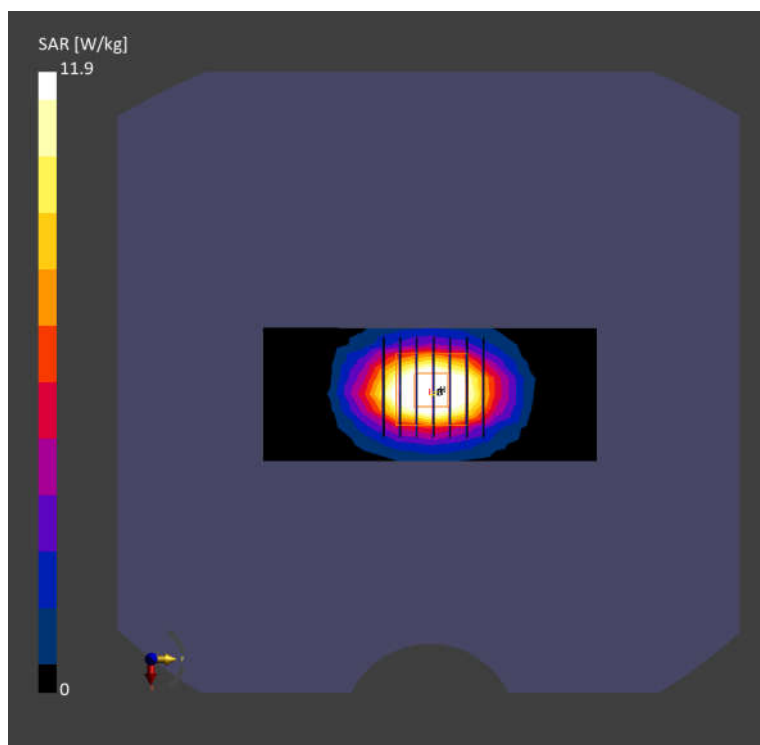

Date: 2025/11/28

System Check_2300MHz**DUT:D2300V2-SN:1055**

Communication System: CW; Frequency: 2300.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.71$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.24, 8.09, 8.13); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 12.1 W/kg; SAR (10g) = 5.86 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 11.9 W/kg; SAR (10g) = 5.67 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.9 %

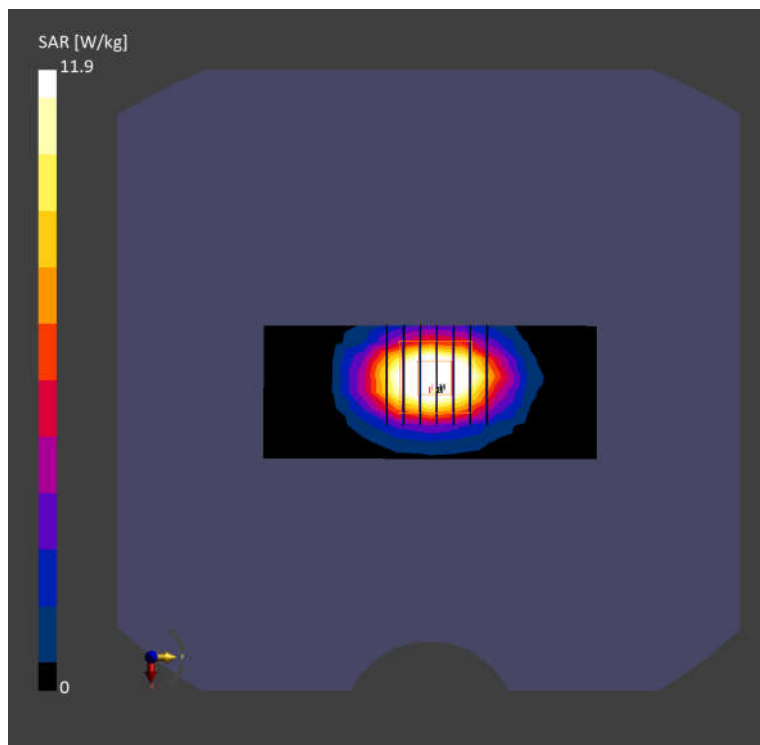

Date: 2025/11/29

System Check_2450MHz**DUT:D2450V2-SN:1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 12.4 W/kg; SAR (10g) = 5.91 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 12.5 W/kg; SAR (10g) = 5.91 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.6 %

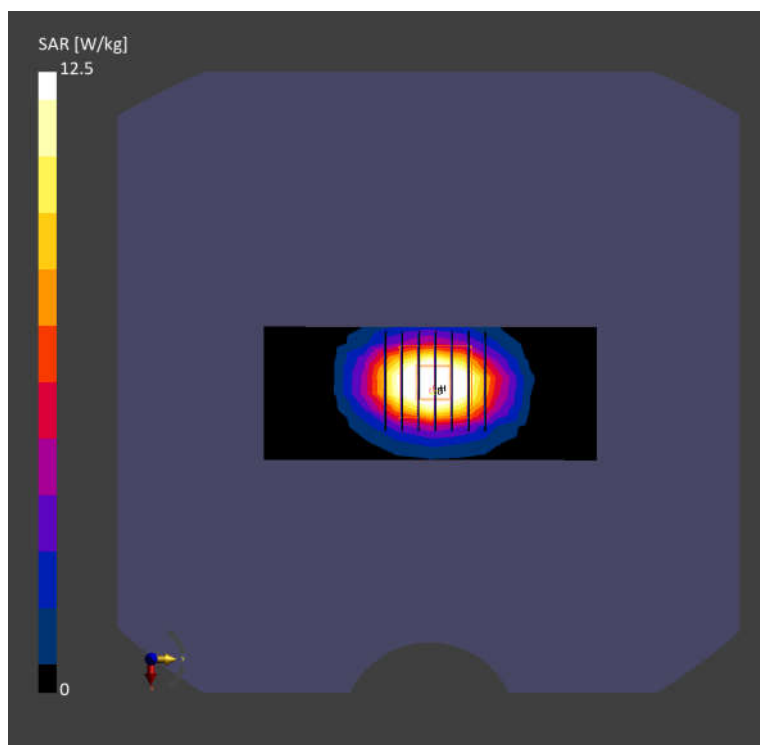

Date: 2025/11/30

System Check_2450MHz**DUT:D2450V2-SN:1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.2 W/kg; SAR (10g) = 6.25 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 13.0 W/kg; SAR (10g) = 6.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

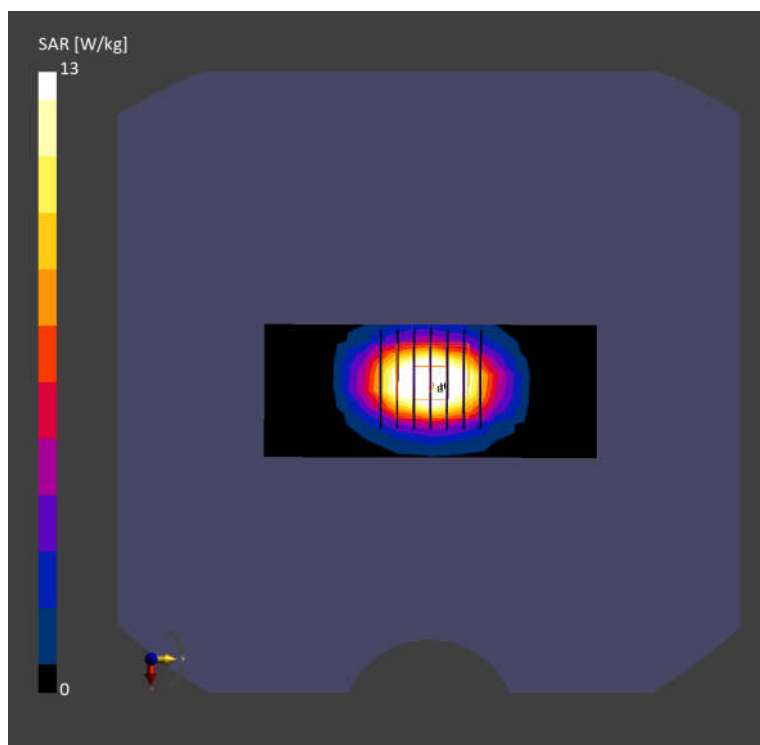

Date: 2025/12/1

System Check_2600MHz**DUT:D2600V2-SN:1070**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.13, 6.85, 6.84); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.9 W/kg; SAR (10g) = 6.35 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 13.6 W/kg; SAR (10g) = 6.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

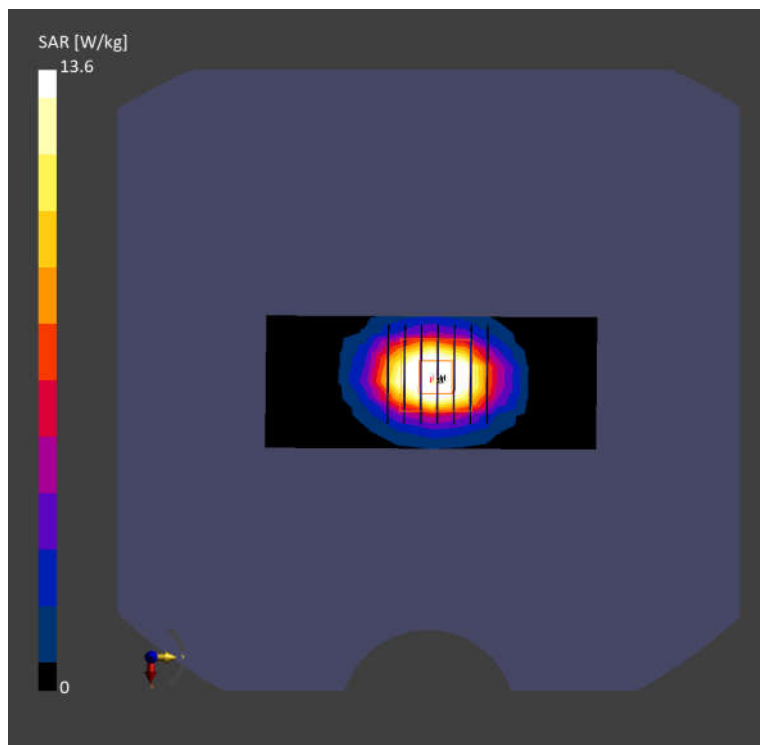

Date: 2025/12/3

System Check_2600MHz**DUT:D2600V2-SN:1070**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.13, 6.85, 6.84); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=250 mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.8 W/kg; SAR (10g) = 6.24 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 13.5 W/kg; SAR (10g) = 6.05 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.4 %

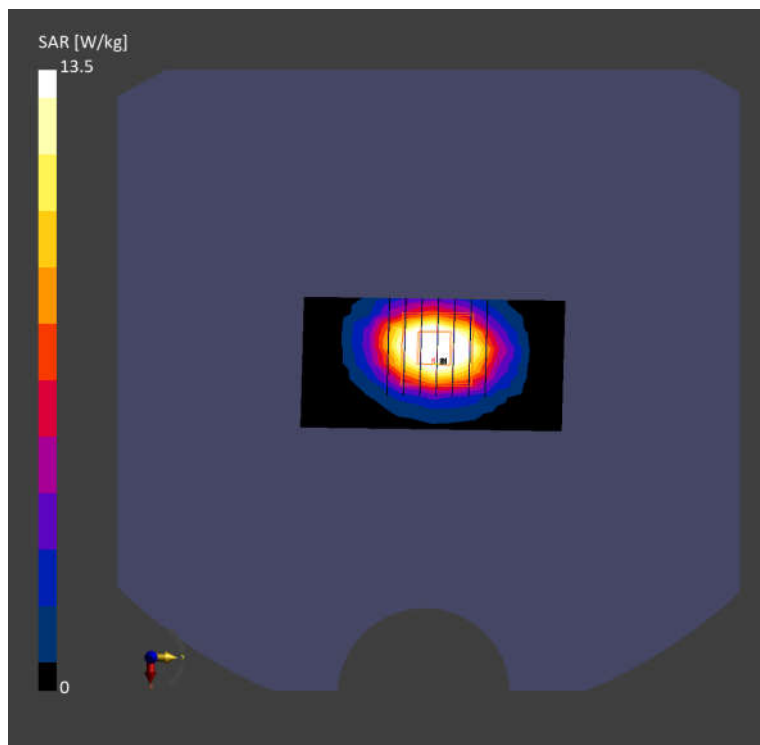

Date: 2025/12/4

System Check_3500MHz**DUT:D3500V2-SN:1076**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.82$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(6.78, 6.51, 6.5); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 6.42 W/kg; SAR (10g) = 2.51 W/kg;**Pin=100 mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 6.41 W/kg; SAR (10g) = 2.47 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.9 %

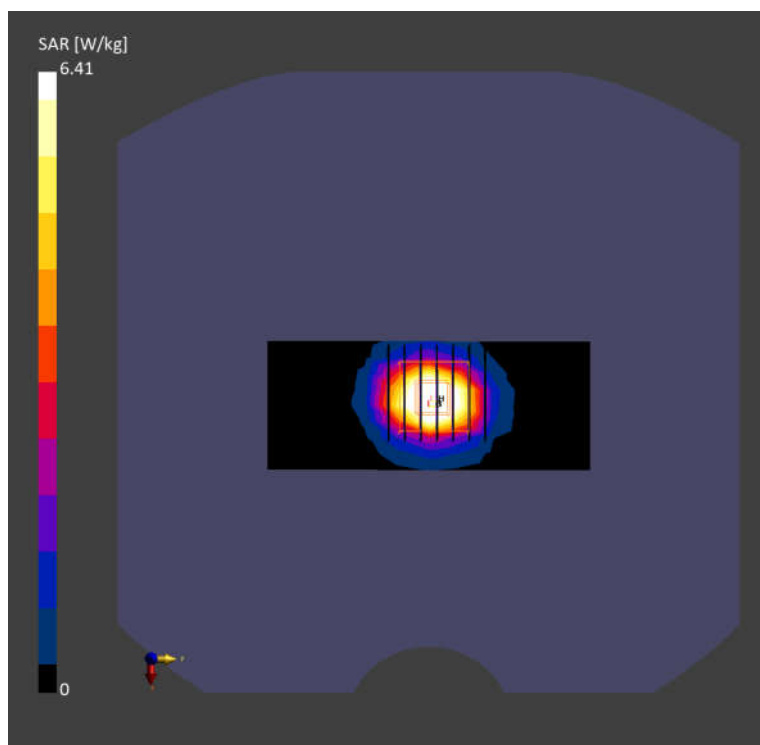

Date: 2025/12/6

System Check_3500MHz**DUT:D3500V2-SN:1076**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.77$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(6.78, 6.51, 6.5); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 6.47 W/kg; SAR (10g) = 2.41 W/kg;**Pin=100 mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 6.51 W/kg; SAR (10g) = 2.49 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.7 %

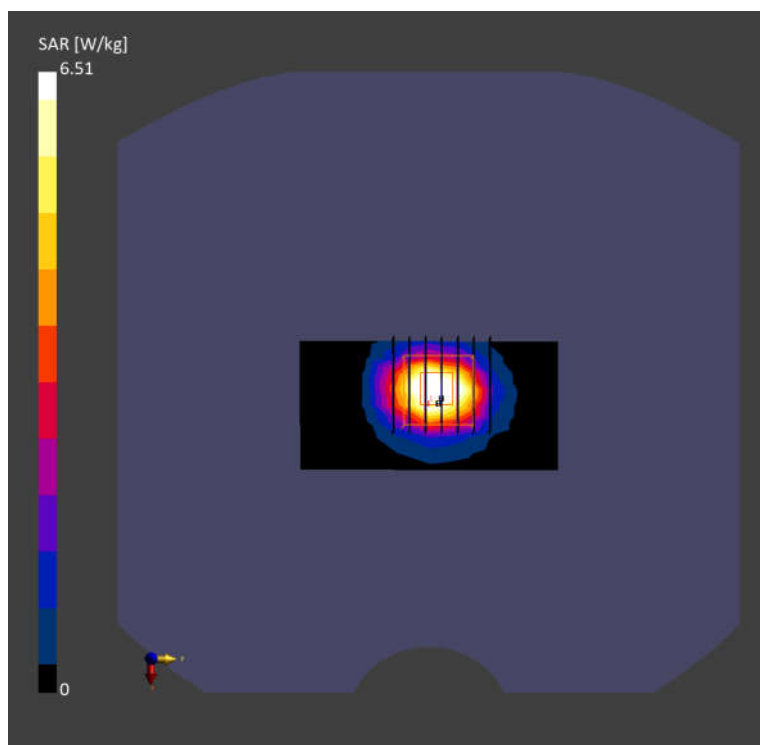

Date: 2025/12/7

System Check_3700MHz**DUT:D3700V2-SN:1037**

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.12$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(6.71, 6.44, 6.43); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.64 W/kg; SAR (10g) = 2.86 W/kg;**Pin=100 mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 7.01 W/kg; SAR (10g) = 2.50 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

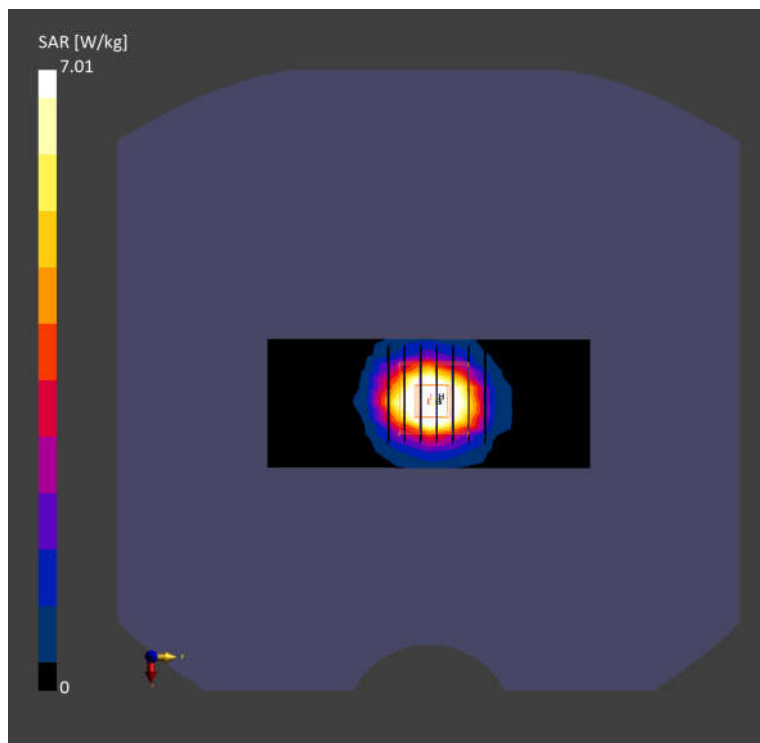

Date: 2025/12/8

System Check_3700MHz**DUT:D3700V2-SN:1037**

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(6.71, 6.44, 6.43); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 6.96 W/kg; SAR (10g) = 2.54 W/kg;**Pin=100 mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 7.02 W/kg; SAR (10g) = 2.53 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

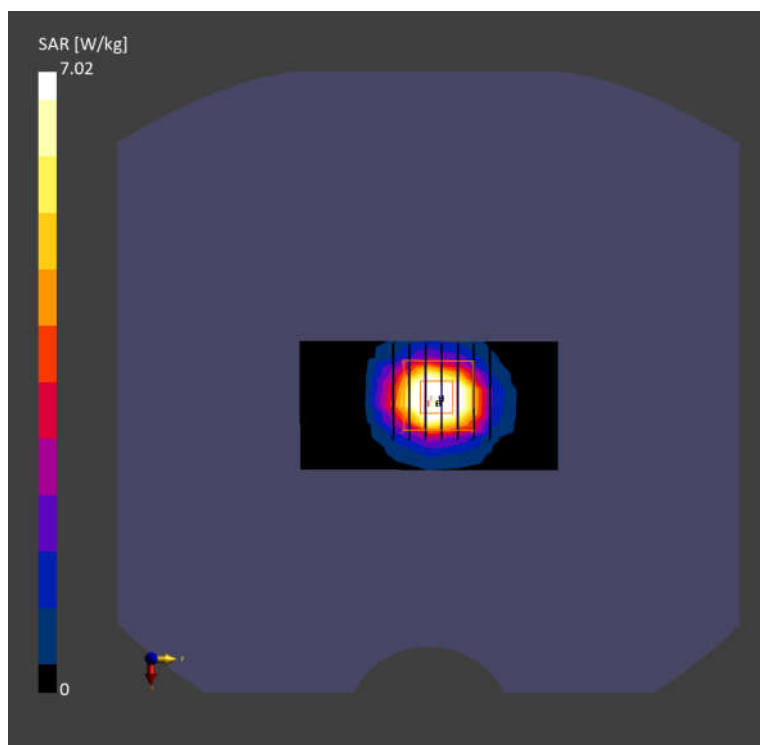

Date: 2025/12/10

System Check_3900MHz**DUT:D3900V2-SN:1022**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.24$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(6.68, 6.41, 6.4); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 6.76 W/kg; SAR (10g) = 2.43 W/kg;


Pin=100 mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 6.85 W/kg; SAR (10g) = 2.42 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

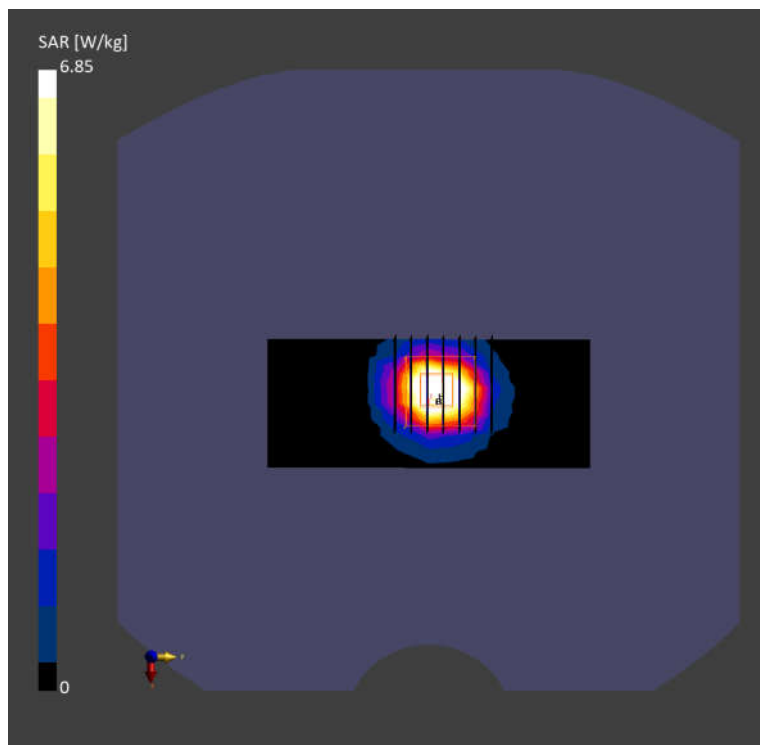

Date: 2025/12/12

System Check_3900MHz**DUT:D3900V2-SN:1022**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.20$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(6.68, 6.41, 6.4); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=100 mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.16 W/kg; SAR (10g) = 2.57 W/kg;


Pin=100 mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 7.21 W/kg; SAR (10g) = 2.57 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

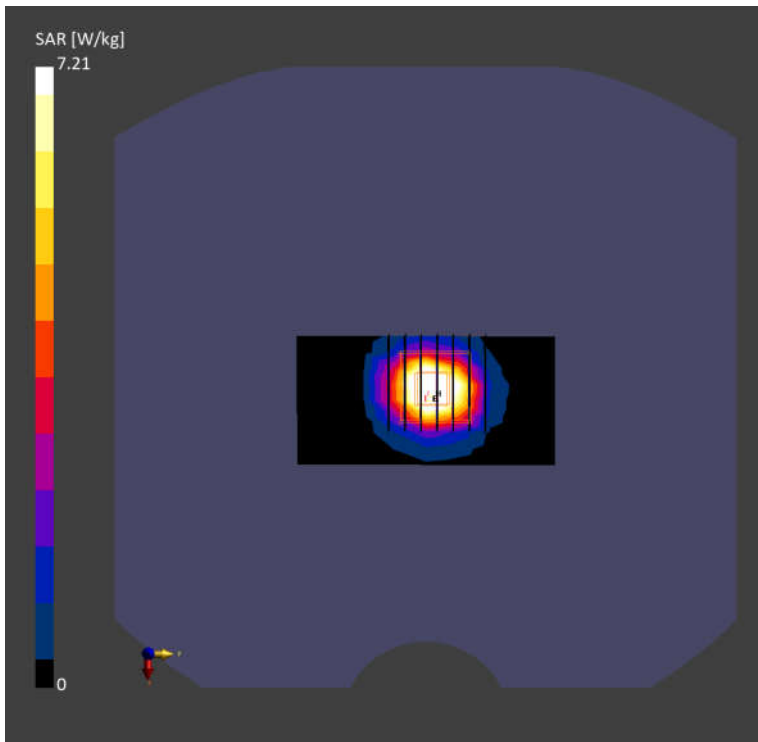

Date: 2025/12/8

System Check_5250MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.62$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.8, 5.57, 5.56); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.36 W/kg; SAR (10g) = 2.13 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 7.75 W/kg; SAR (10g) = 2.20 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 63.7 %

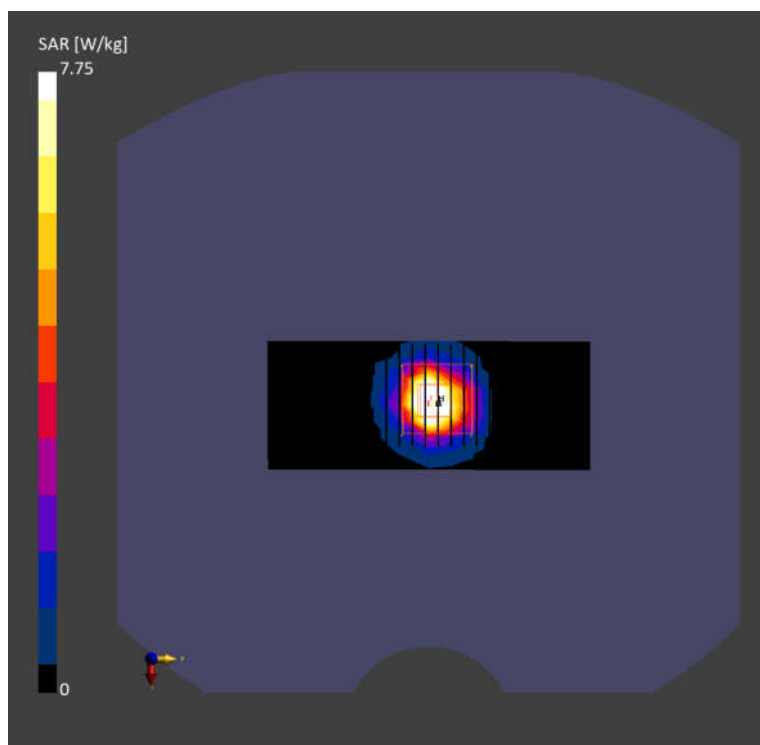

Date: 2025/11/27

System Check_5250MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.59$ S/m; $\epsilon_r = 36.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.8, 5.57, 5.56); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.73 W/kg; SAR (10g) = 2.22 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.08 dB

SAR (1g) = 8.11 W/kg; SAR (10g) = 2.34 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.3 %

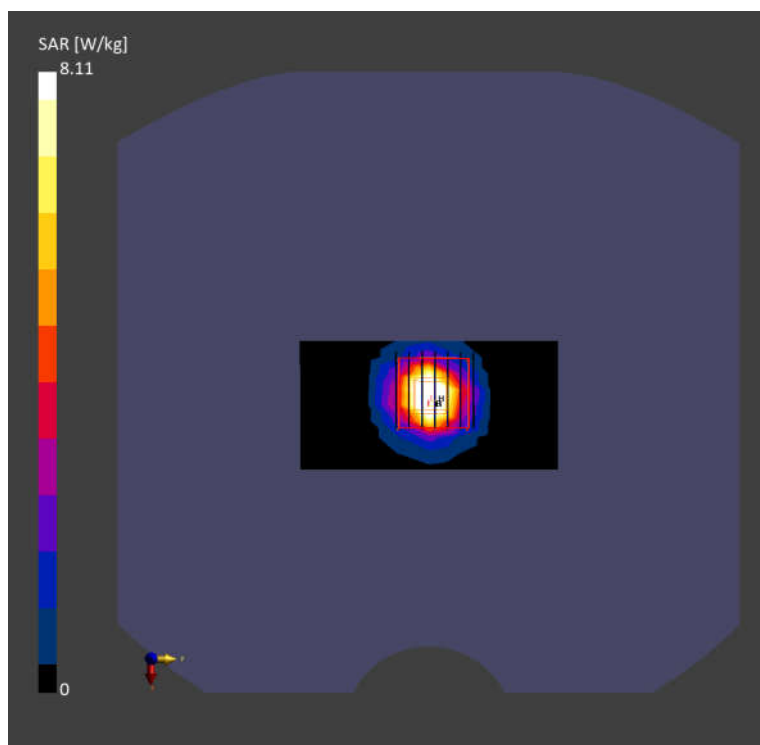

Date: 2025/11/26

System Check_5600MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.05$ S/m; $\epsilon_r = 35.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.84 W/kg; SAR (10g) = 2.24 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 8.30 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.1 %

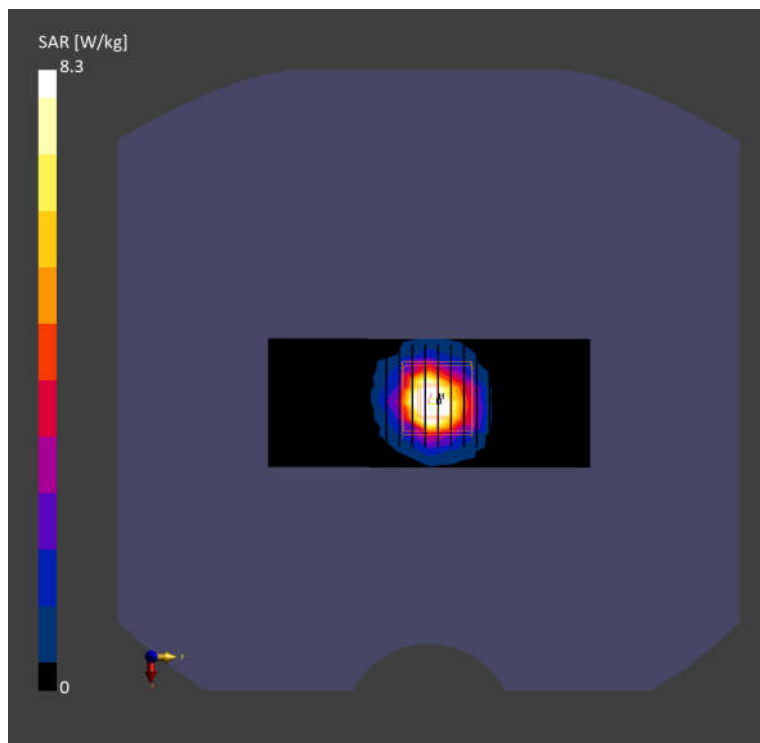

Date: 2025/12/1

System Check_5600MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.00$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.63 W/kg; SAR (10g) = 2.17 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 8.66 W/kg; SAR (10g) = 2.49 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.8 %

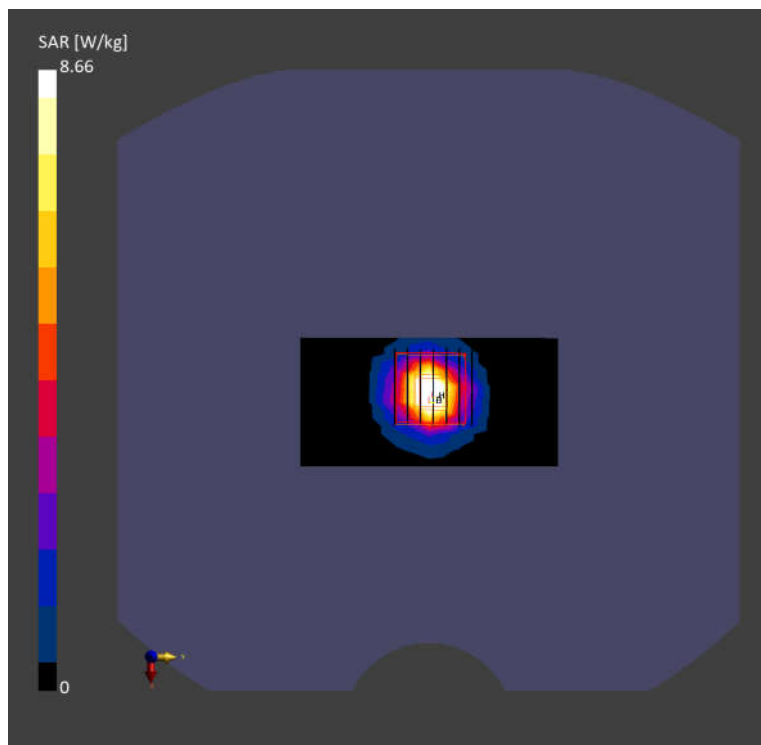

Date: 2025/12/6

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.25$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.22, 5.02, 5.01); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.22 W/kg; SAR (10g) = 2.35 W/kg;


Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 8.35 W/kg; SAR (10g) = 2.32 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 58.4 %

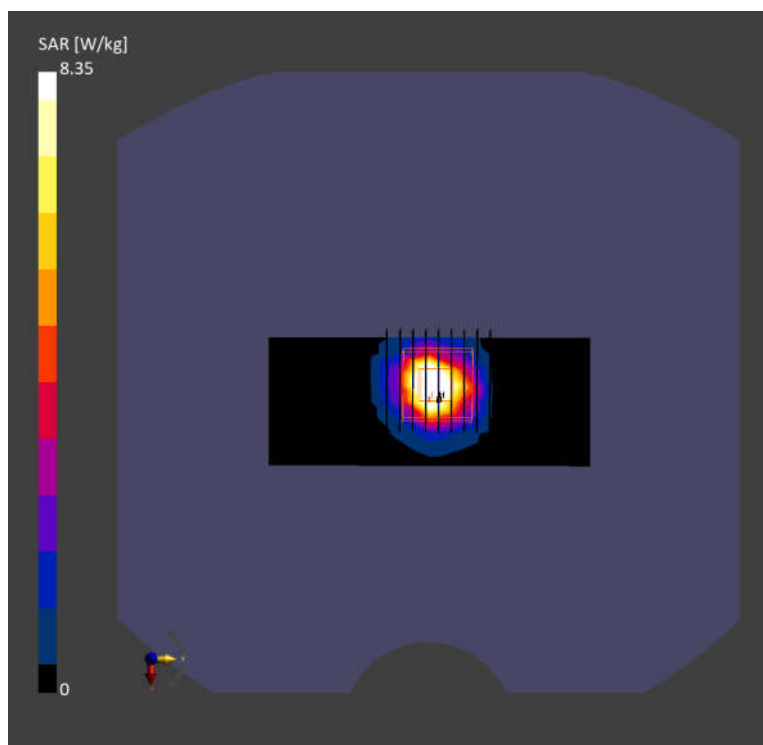

Date: 2025/12/8

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.23$ S/m; $\epsilon_r = 35.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.22, 5.02, 5.01); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 7.23 W/kg; SAR (10g) = 2.00 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 7.69 W/kg; SAR (10g) = 2.21 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 59.1 %

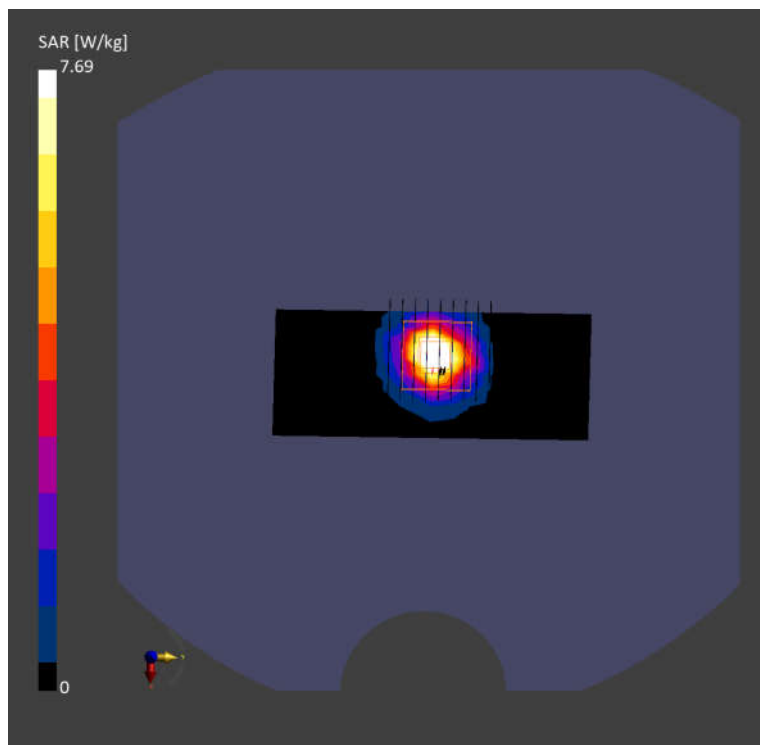

Date: 2025/12/12

System Check_6500MHz**DUT:D6.5GHzV2-SN:1026**

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.02$ S/m; $\epsilon_r = 34.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.58, 5.36, 5.35); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=100 mW/Area Scan (40.0 mm x 102.0 mm): Measurement Grid: 5.0 mm x 8.5 mm

SAR (1g) = 24.6 W/kg; SAR (10g) = 4.93 W/kg;

Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mmx 1.4 mm


Power Drift = -0.09 dB

SAR (1g) = 29.1 W/kg; SAR (10g) = 5.29 W/kg

Smallest distance from peaks to all points 3 dB below = 4.4 mm

Ratio of SAR at M2 to SAR at M1 = 51.6 %

psAPD (4.0cm2, sq) = 128 [W/m2]

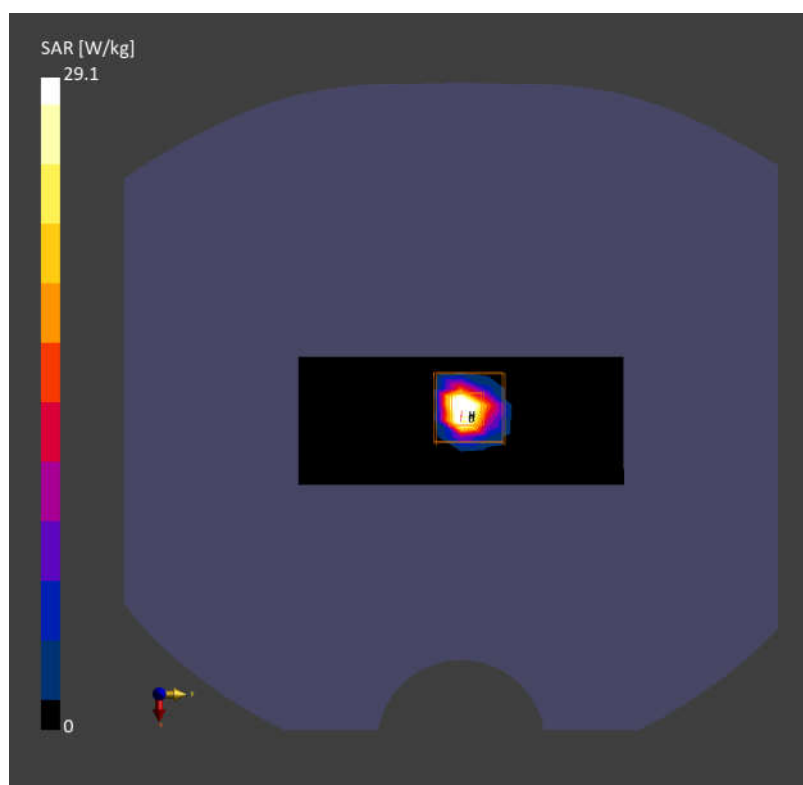

Date: 2025/12/14

System Check_6500MHz**DUT:D6.5GHzV2-SN:1026**

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.08$ S/m; $\epsilon_r = 34.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.58, 5.36, 5.35); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2025/9/10
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=100 mW/Area Scan (40.0 mm x 102.0 mm): Measurement Grid: 5.0 mm x 8.5 mm

SAR (1g) = 26.7 W/kg; SAR (10g) = 5.19 W/kg;


Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 31.4 W/kg; SAR (10g) = 5.73 W/kg

Smallest distance from peaks to all points 3 dB below = 4.4 mm

Ratio of SAR at M2 to SAR at M1 = 50.8 %

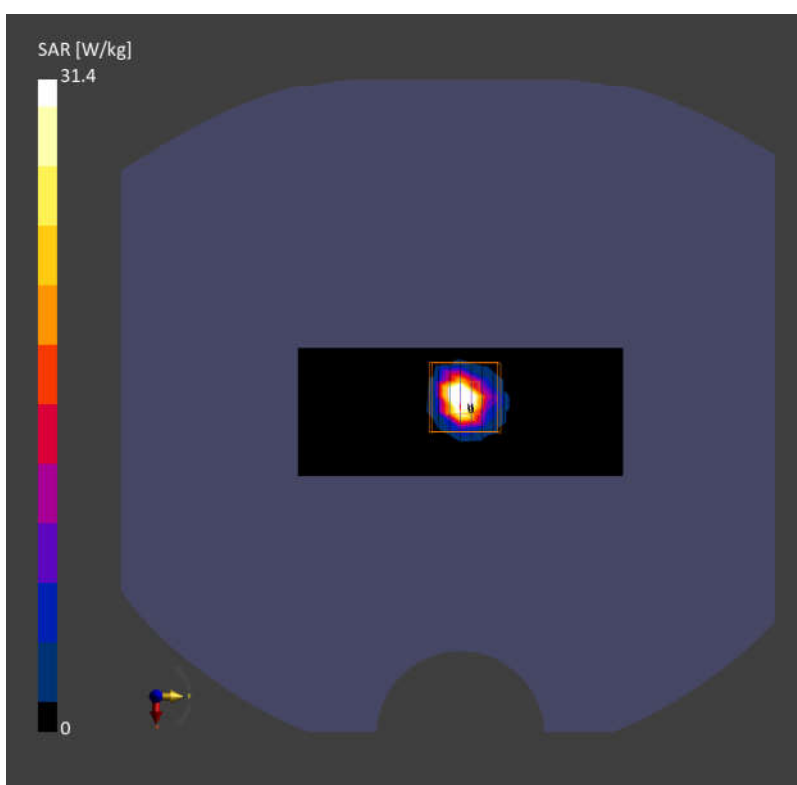psAPD (4.0cm², sq) = 139 [W/m²]

Date: 2025/11/29

System Check_13MHz**DUT: CLA13-SN:1023**

Communication System: CW; Frequency: 13.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.743$ S/m; $\epsilon_r = 54.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(18.57, 19.41, 16.88); Calibrated: 2025/6/26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025/7/11
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 2131; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=1000mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0mm

SAR (1g) = 0.596 W/kg; SAR (10g) = 0.322 W/kg;


Pin=1000mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.08 dB

SAR (1g) = 0.602 W/kg; SAR (10g) = 0.373 W/kg

Smallest distance from peaks to all points 3 dB below = 14.5 mm

Ratio of SAR at M2 to SAR at M1 = 78.5 %

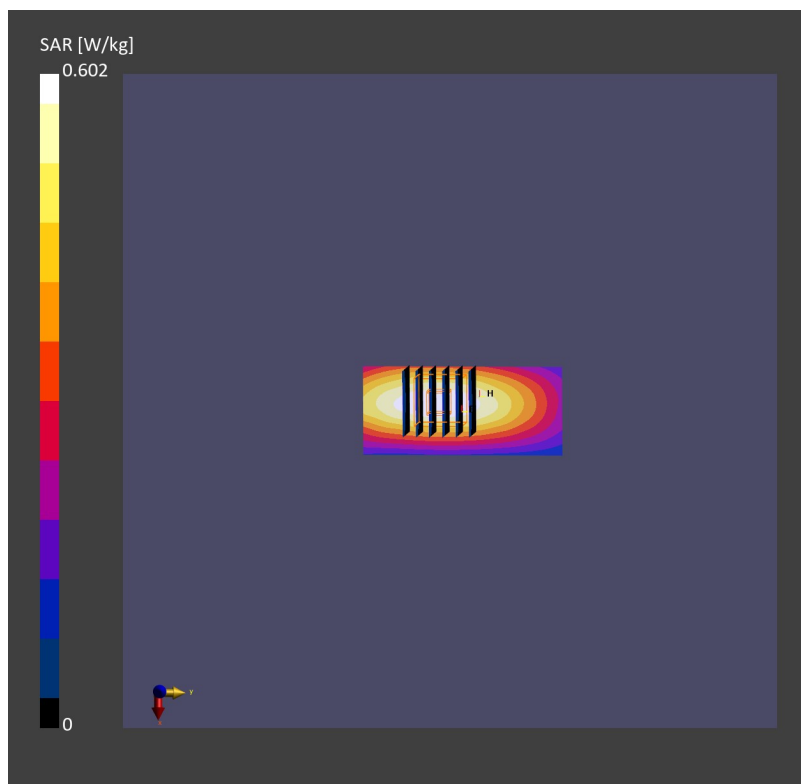

Measurement Report for Device, FRONT, Validation band, CW, Channel 10000 (10000.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	100.0 x 100.0 x 105.0		Source

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor
5G	FRONT, 10.00	Validation band	CW, 0--	10000.0, 10000	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave	Air -	EUmmWV4 - SN9432_F1-55GHz, 2025-01-08	DAE4 Sn1696, 2025-09-10

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120.0 x 120.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0
MAIA	N/A

Measurement Results

Scan Type	5G Scan
Date	2025-11-28
Avg. Area [cm²]	4.00
psPDn+ [W/m²]	156
psPDtot+ [W/m²]	158
psPDmod+ [W/m²]	160
E _{max} [V/m]	299
Power Drift [dB]	0.01

