

System Check_Head_750MHz

DUT: D750V3 - SN:1087

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.900$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.19, 10.19, 10.19); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.446 W/kg; SAR (10g) = 0.296 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.02 dB

SAR (1g) = 0.444 W/kg; SAR (10g) = 0.297 W/kg;

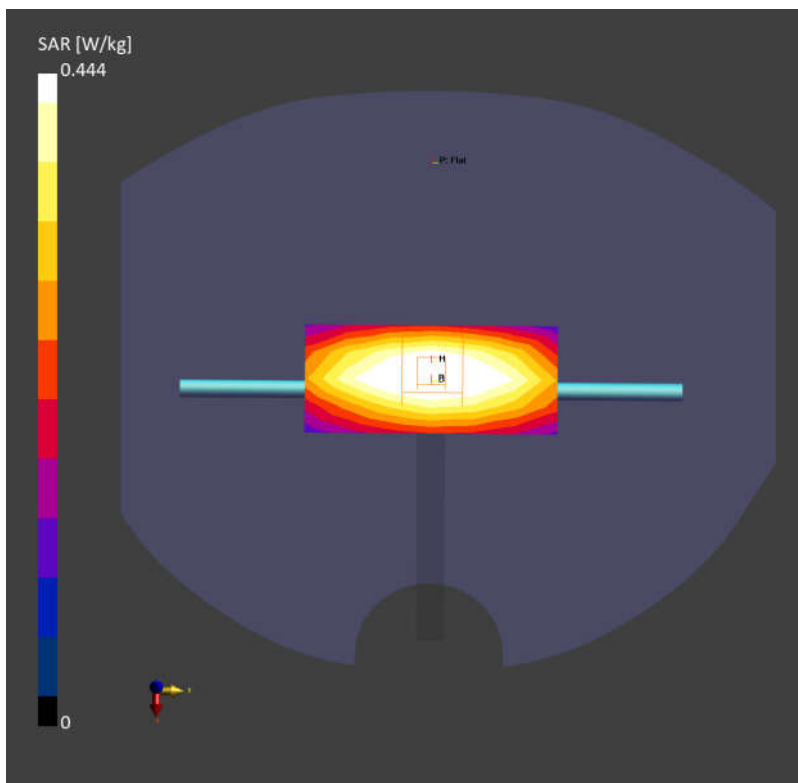

System Check_Head_835MHz

DUT: D835V2 - SN:4d091

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.902$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(9.78, 9.78, 9.78); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.488 W/kg; SAR (10g) = 0.320 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.03 dB

SAR (1g) = 0.486 W/kg; SAR (10g) = 0.322 W/kg;

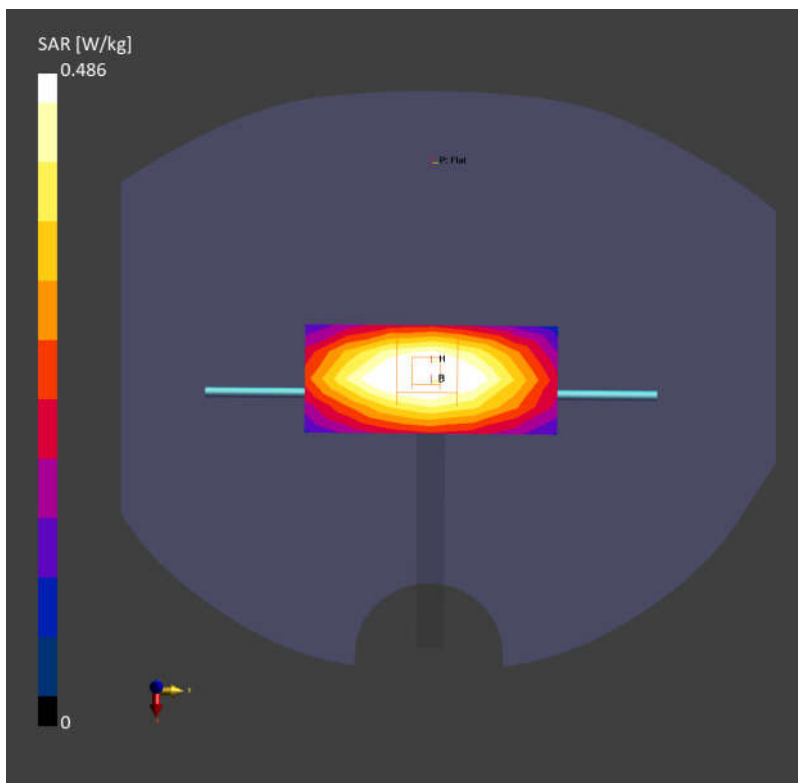

System Check_Head_1750MHz

DUT:D1750V2 - SN:1090

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.78, 8.78, 8.78); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.03 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.03 dB

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.993 W/kg;

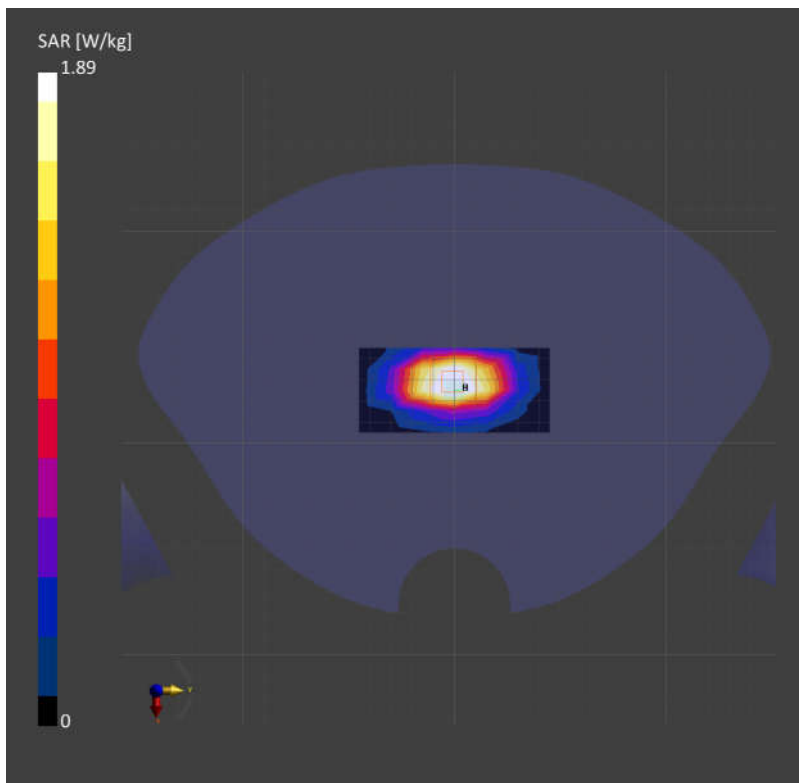

System Check_Head_1900MHz

DUT: D1900V2 - SN:5d118

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.46, 8.46, 8.46); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 2.06 W/kg; SAR (10g) = 1.06 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.05 dB

SAR (1g) = 2.07 W/kg; SAR (10g) = 1.08 W/kg;

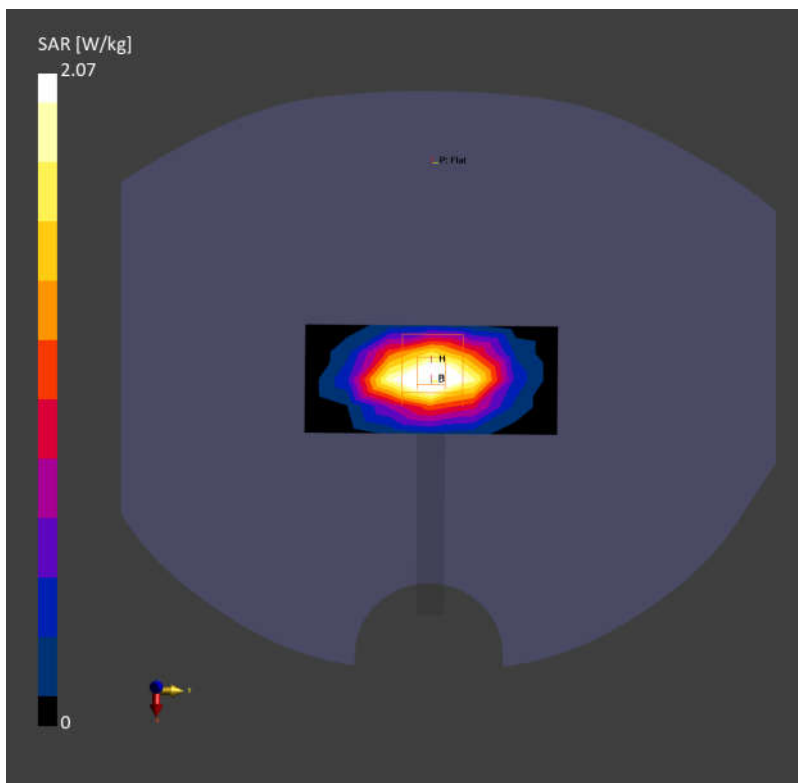

System Check_Head_2600MHz

DUT: D2600V2 - SN:1070

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.02, 8.02, 8.02); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.81 W/kg; SAR (10g) = 1.26 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 2.82 W/kg; SAR (10g) = 1.28 W/kg;

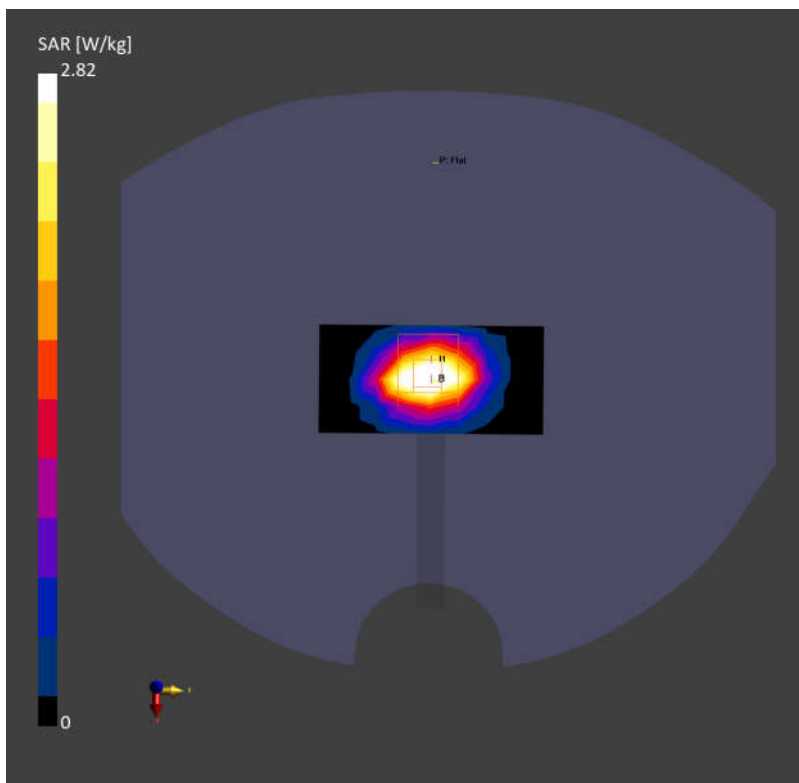

System Check_Head_3500MHz

DUT: D3500V2 - SN:1037

Communication System: ; Frequency: 3500.000

Medium: HSL. Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.78$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.11, 7.11, 7.11); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.21 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.26 W/kg;

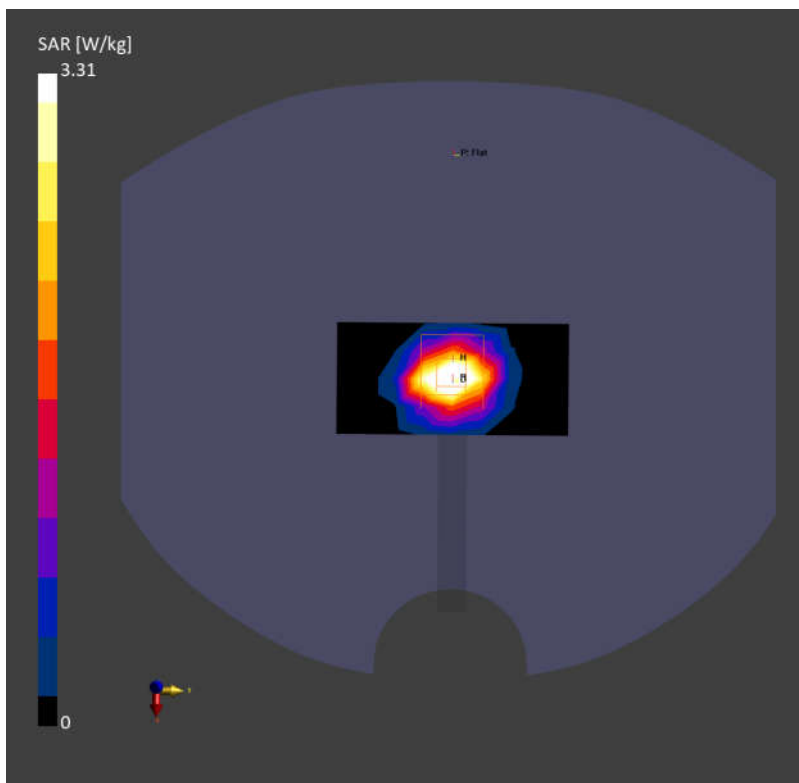

System Check_Head_3700MHz

DUT: D3700V2 - SN:1008

Communication System: ; Frequency: 3700.000

Medium: HSL. Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.10, 7.10, 7.10); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.28 W/kg; SAR (10g) = 1.22 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.46 W/kg; SAR (10g) = 1.29 W/kg;

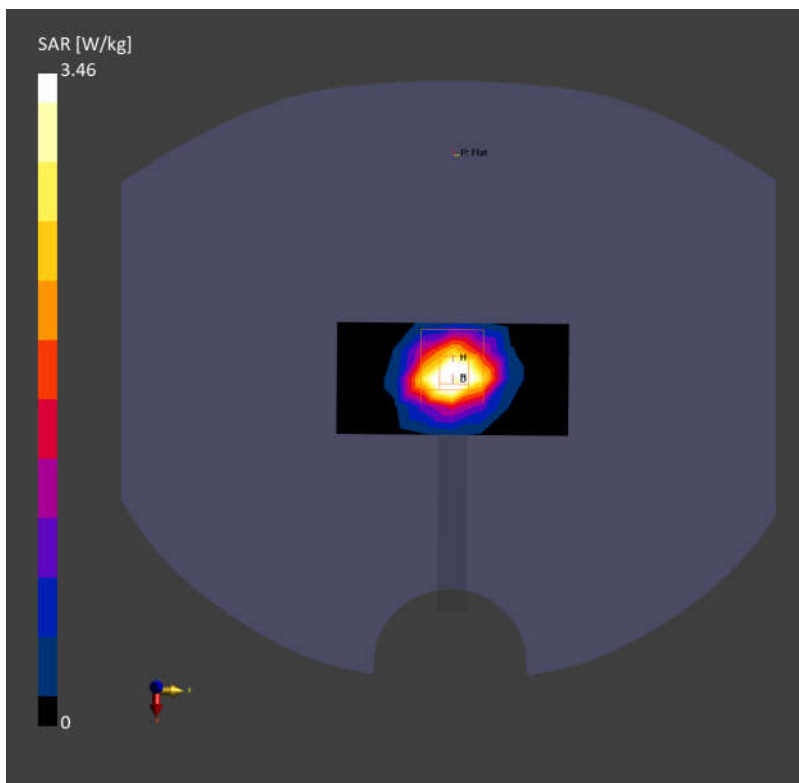

System Check_Head_3900MHz

DUT: D3900V2 - SN:1048

Communication System: ; Frequency: 3900.000

Medium: HSL. Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.19$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.74, 6.74, 6.74); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.15 W/kg; SAR (10g) = 1.22 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.09 dB

SAR (1g) = 3.42 W/kg; SAR (10g) = 1.24 W/kg;

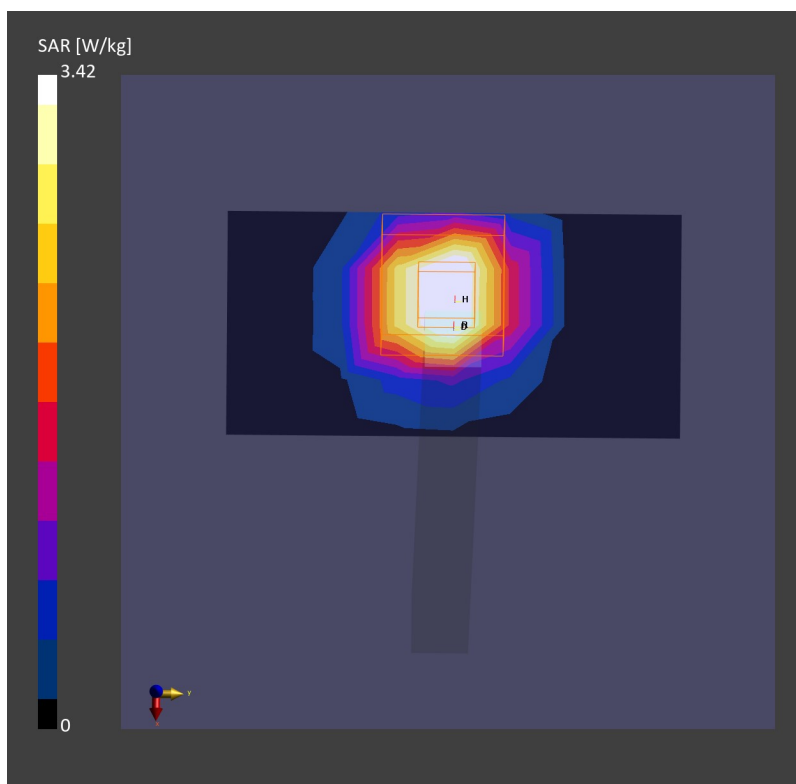

System Check_Head_750MHz

DUT:D750V3 - SN:1087

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.926$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(10.17, 10.07, 10.45); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.457 W/kg; SAR (10g) = 0.304 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 0.457 W/kg; SAR (10g) = 0.305 W/kg;

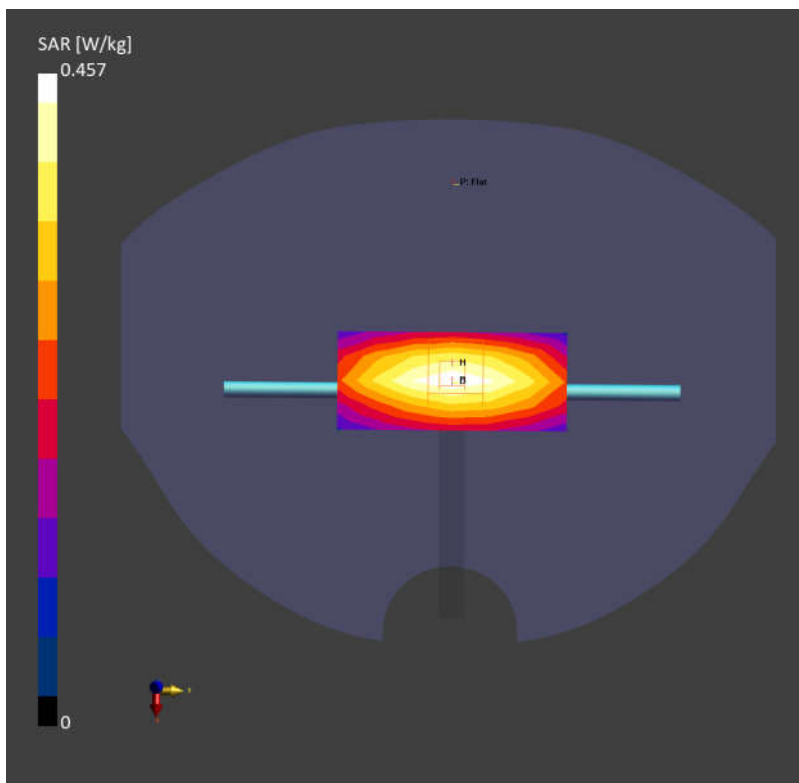

System Check_Head_835MHz

DUT: D835V2 - SN:4d091

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.938$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(10.13, 10.02, 10.22); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.515 W/kg; SAR (10g) = 0.338 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 0.502 W/kg; SAR (10g) = 0.335 W/kg;

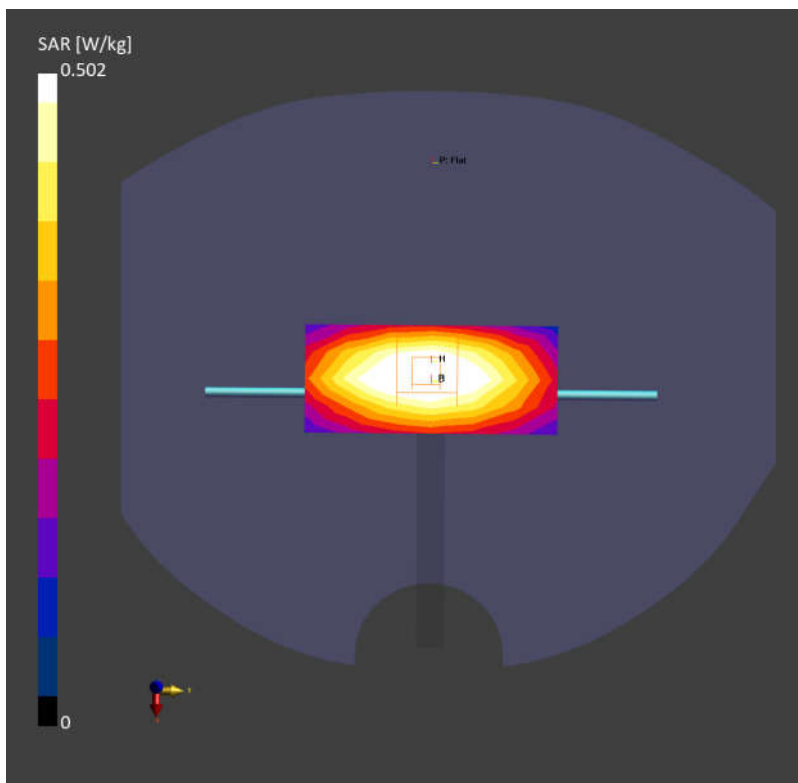

System Check_Head_1750MHz

DUT:D1750V2 - SN:1090

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(8.79, 8.61, 8.89); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.03 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 1.86 W/kg; SAR (10g) = 0.980 W/kg;

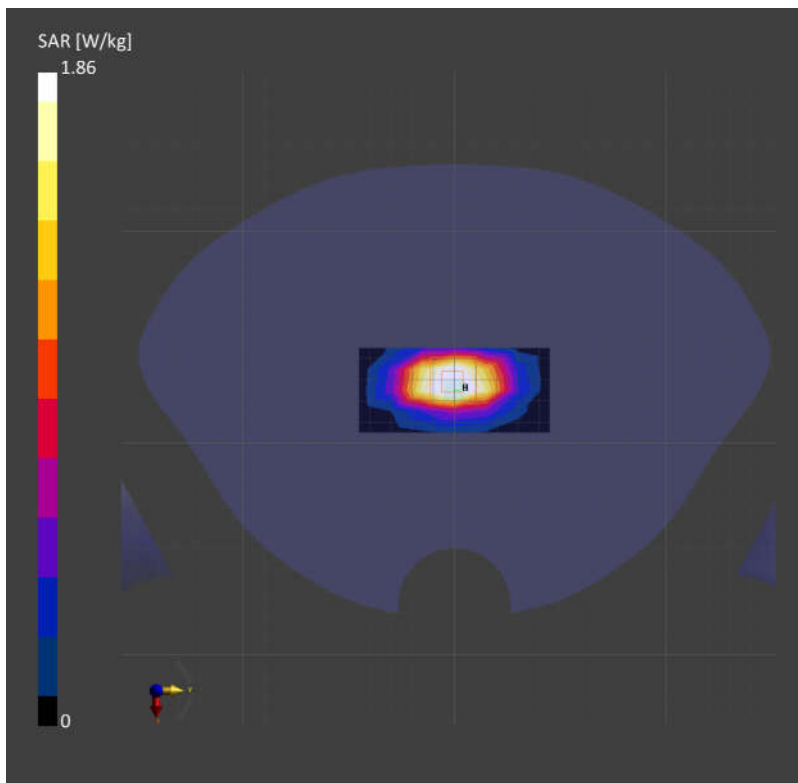

System Check_Head_1900MHz

DUT:D1900V2 - SN:5d118

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 40.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(8.41, 8.15, 8.28); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 2.11 W/kg; SAR (10g) = 1.09 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.02 dB

SAR (1g) = 2.09 W/kg; SAR (10g) = 1.09 W/kg;

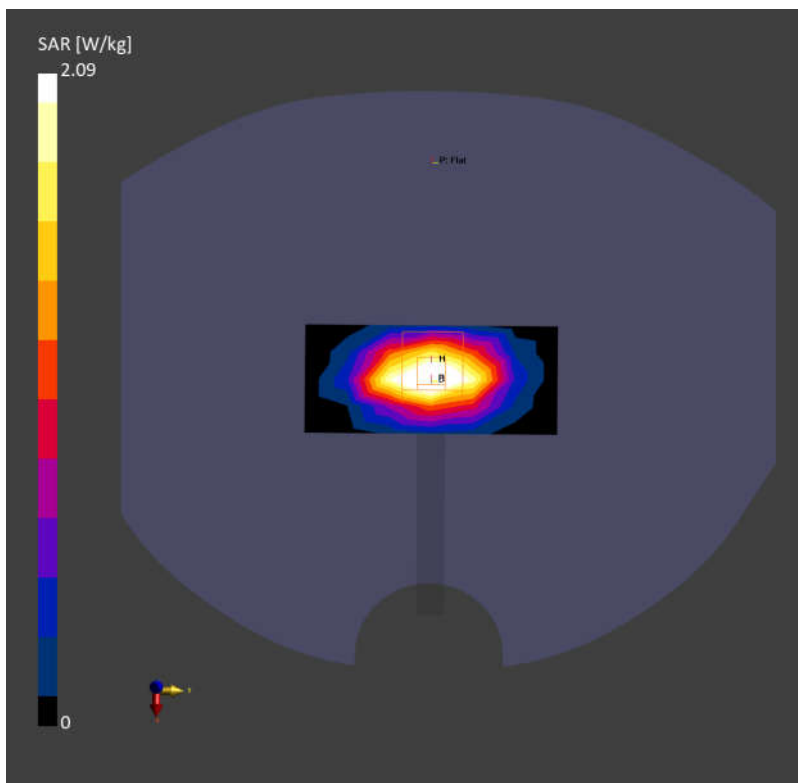

System Check_Head_2600MHz

DUT: D2600V2 - SN:1070

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.54, 7.41, 7.52); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.85 W/kg; SAR (10g) = 1.27 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.02 dB

SAR (1g) = 2.83 W/kg; SAR (10g) = 1.29 W/kg;

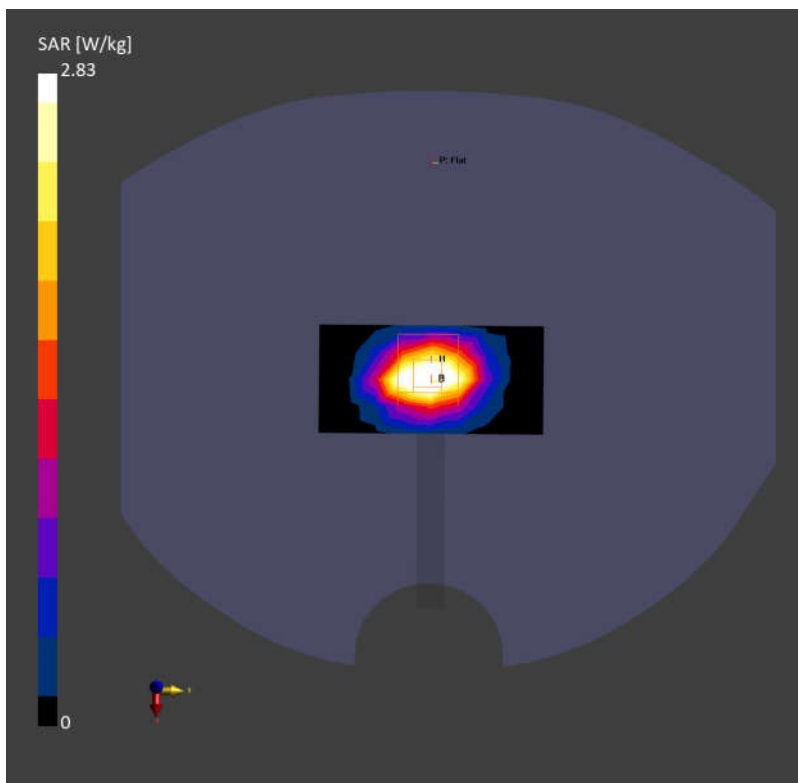

System Check_Head_3500MHz

DUT:D3500V2 - SN:1037

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.79$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.34, 7.2, 7.31); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.09 W/kg; SAR (10g) = 1.18 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.21 W/kg;

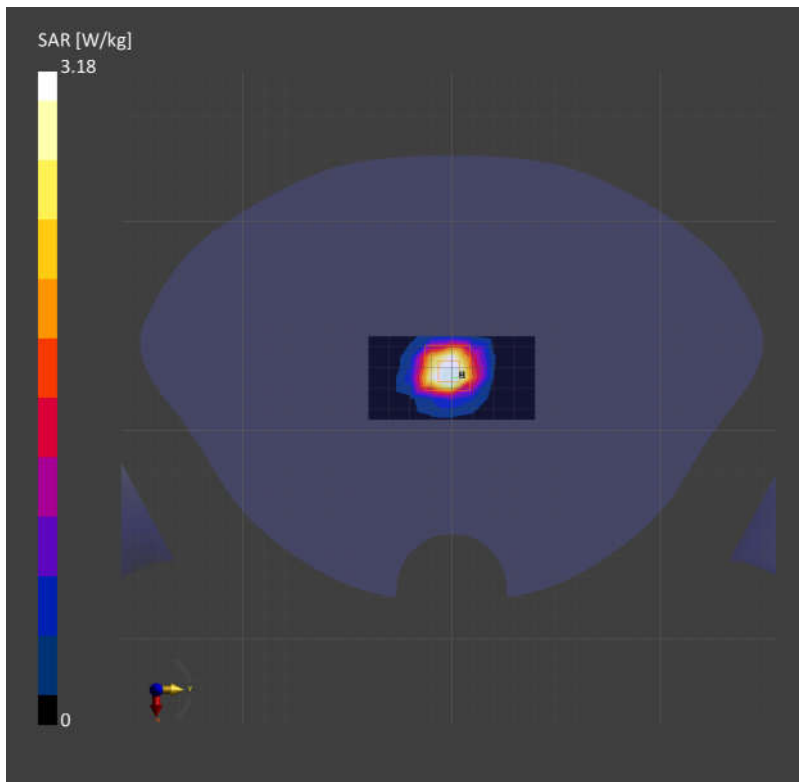

System Check_Head_3700MHz

DUT:D3700V2 - SN:1008

Communication System: ; Frequency: 3700.0

Medium: HSL. Medium parameters used: $f = 3700.0$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.29, 7.14, 7.26); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 1.17 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.15 W/kg; SAR (10g) = 1.18 W/kg;

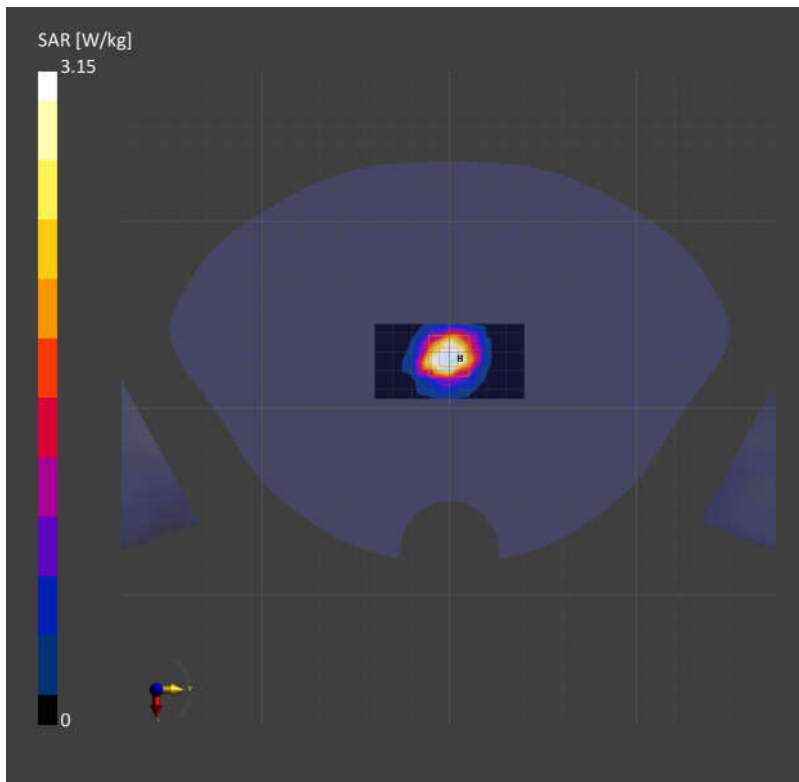

System Check_Head_3900MHz

DUT:D3900V2 - SN:1048

Communication System: ; Frequency: 3900.0

Medium: HSL. Medium parameters used: $f = 3900.0$ MHz; $\sigma = 3.19$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.74, 6.74, 6.74); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.15 W/kg; SAR (10g) = 1.14 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.28 W/kg; SAR (10g) = 1.18 W/kg;

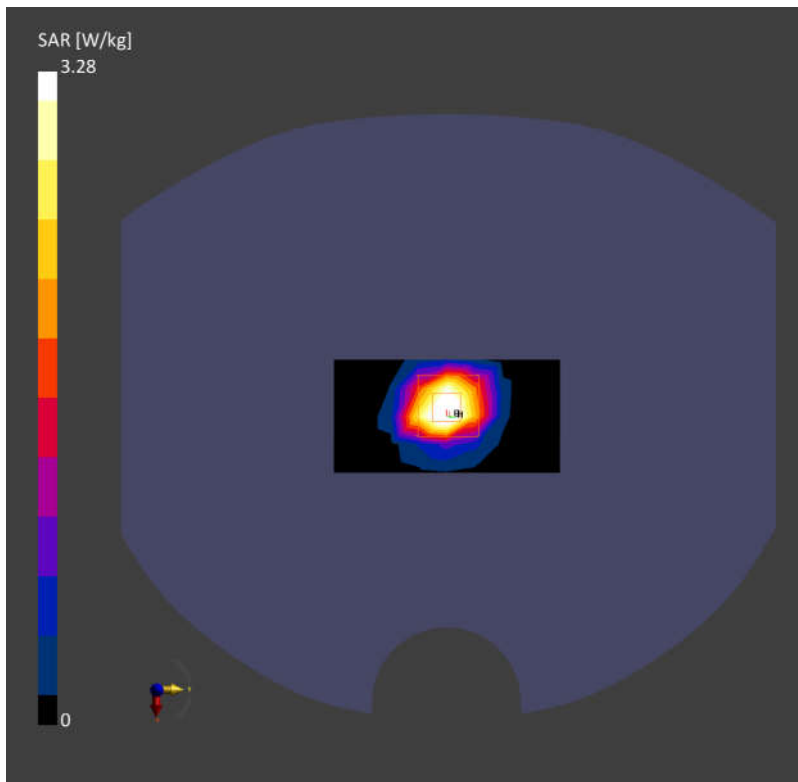

System Check_Head_2450MHz

DUT: D2450V2 - SN:1040

Communication System: ; Frequency: 2450.000

Medium: MSL. Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.86$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.66, 7.57, 7.66); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.57 W/kg; SAR (10g) = 1.19 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = 0.03 dB

SAR (1g) = 2.53 W/kg; SAR (10g) = 1.20 W/kg;

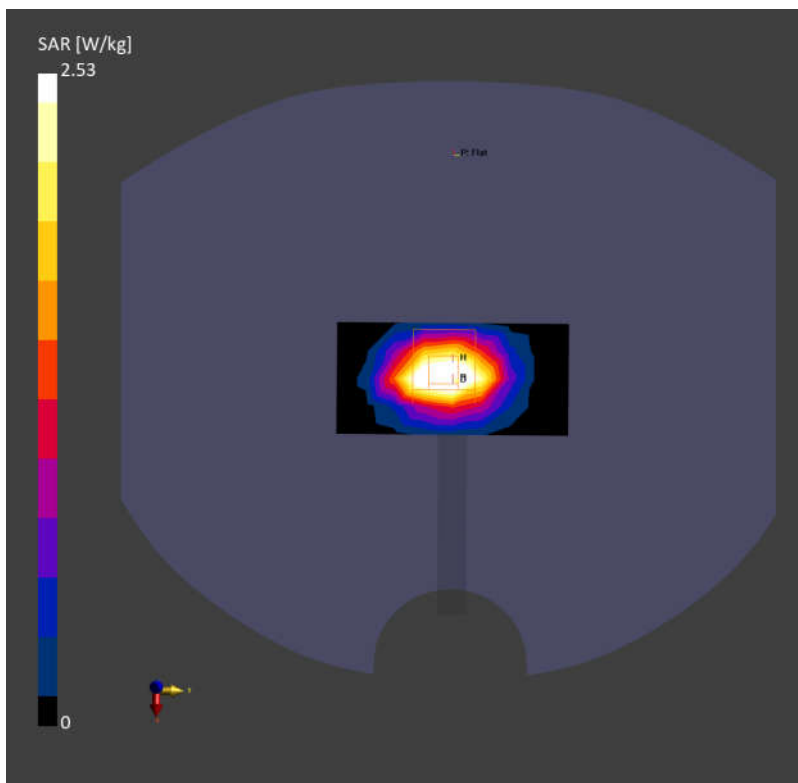

System Check_Head_5250MHz

DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used: $f= 5250.000$ MHz; $\sigma= 4.60$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(6.05, 5.94, 5.93); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.56 W/kg; SAR (10g) = 1.02 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.81 W/kg; SAR (10g) = 1.08 W/kg;

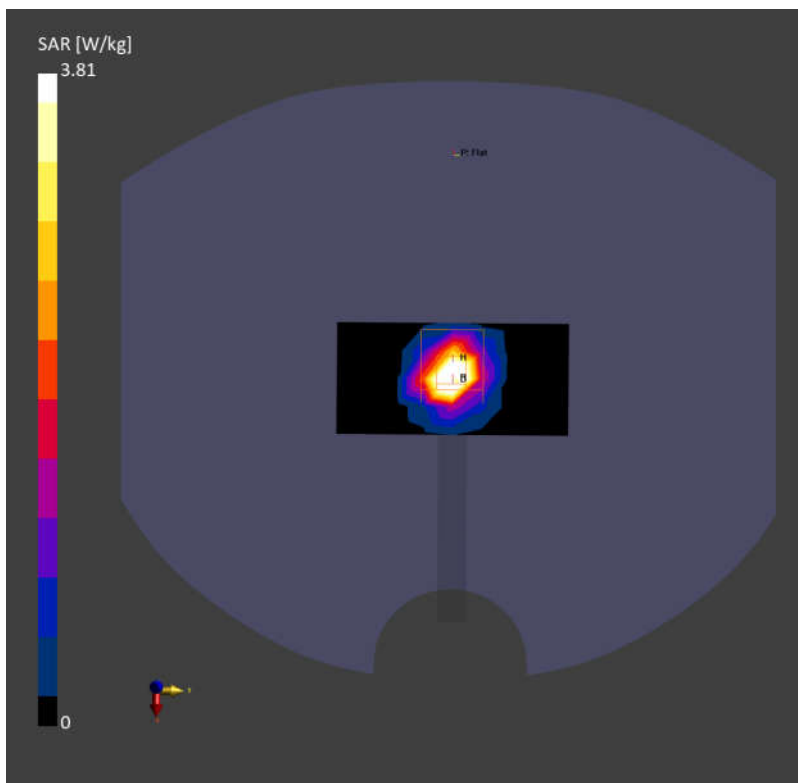

System Check_Head_5600MHz

DUT: D5GHzV2 - SN:1113

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.00$ S/m; $\epsilon_r = 35.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.24, 5.12, 5.19); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.64 W/kg; SAR (10g) = 1.19 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 4.33 W/kg; SAR (10g) = 1.25 W/kg;

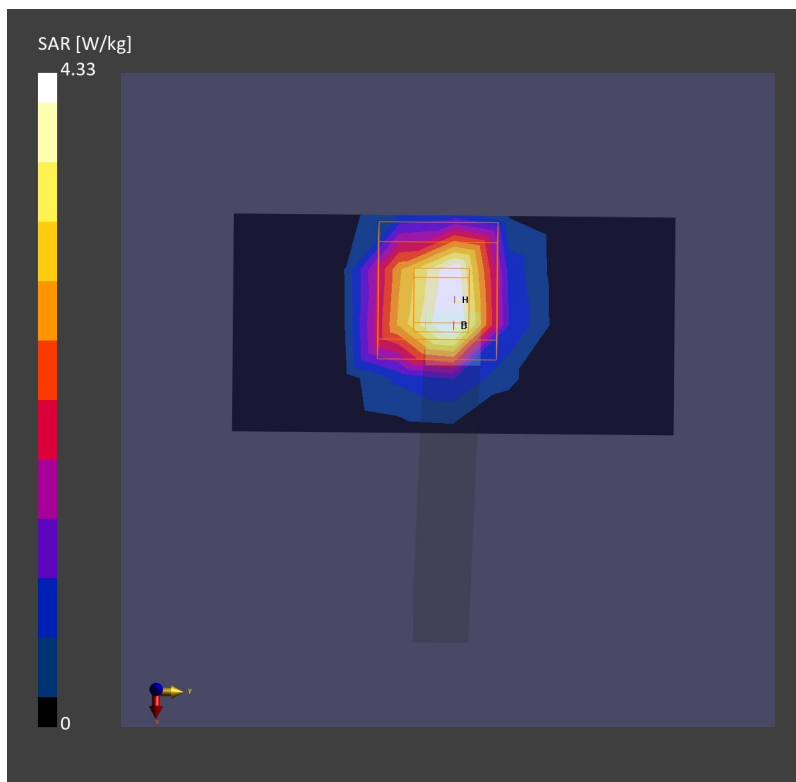

System Check_Head_5750MHz

DUT: D5GHzV2 - SN:1113

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.17$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.34, 5.2, 5.26); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.53 W/kg; SAR (10g) = 1.15 W/kg;

Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 4.22 W/kg; SAR (10g) = 1.21 W/kg;

