Date: 2024-02-19

System Check_Head_13MHz

DUT: CLA13 - SN:1020

Communication System: ; Frequency: 13.000
Medium: HSL. Medium parameters used: f= 13.000 MHz; σ= 0.757 S/m; ε_r = 53.7
Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:
- Probe: EX3DV4 - SN7764; ConvF(15.05, 15.05, 15.05); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2134
- Measurement Software: cDASY6 V6.6.0.13926

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm
SAR (1g) = 0.130 W/kg; SAR (10g) = 0.092 W/kg;
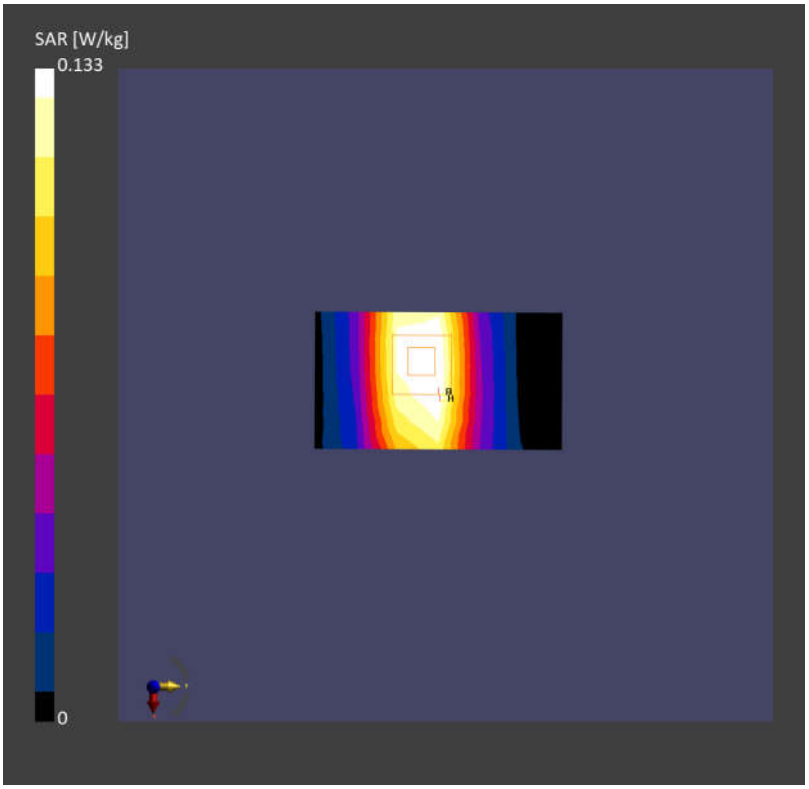
Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 5.0 mm
Power Drift = 0.05 dB
SAR (1g) = 0.133 W/kg; SAR (10g) = 0.094 W/kg;