

Date: 2025-08-22

System Check_Head_750MHz**DUT: D750V3 - SN1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL_750_250822 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.886$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(10.48, 10.38, 10.54); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.412 W/kg; SAR (10g) = 0.277 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.279 W/kg

Smallest distance from peaks to all points 3 dB below = 16.1 mm

Ratio of SAR at M2 to SAR at M1 = 88.1 %

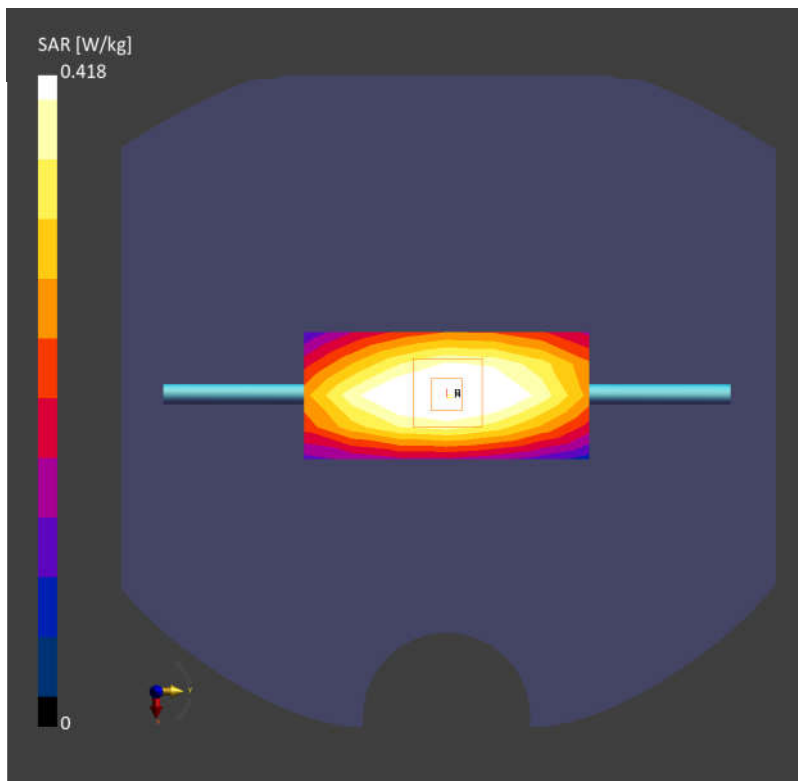

Date: 2025-08-23

System Check_Head_835MHz**DUT: D835V2 - SN4d298**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_835_250823 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.914$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(10.22, 10.12, 10.28); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.490 W/kg; SAR (10g) = 0.328 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.503 W/kg; SAR (10g) = 0.333 W/kg

Smallest distance from peaks to all points 3 dB below = 15.2 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

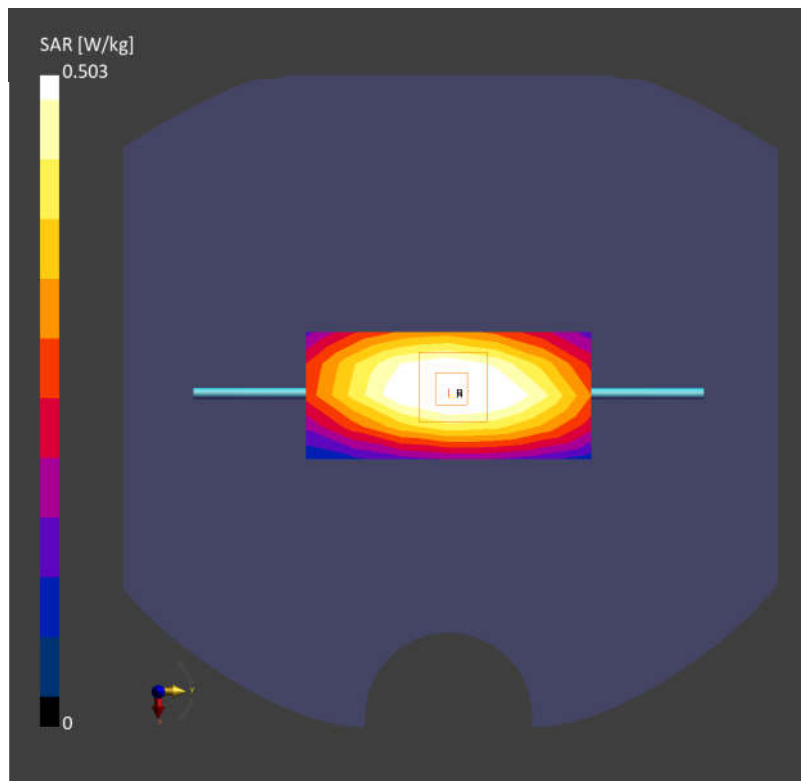

Date: 2025-08-24

System Check_Head_1900MHz**DUT: D1900V2 - SN5d182**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL_1900_250824 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(8.15, 8.07, 8.2); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.97 W/kg; SAR (10g) = 1.03 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.02 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

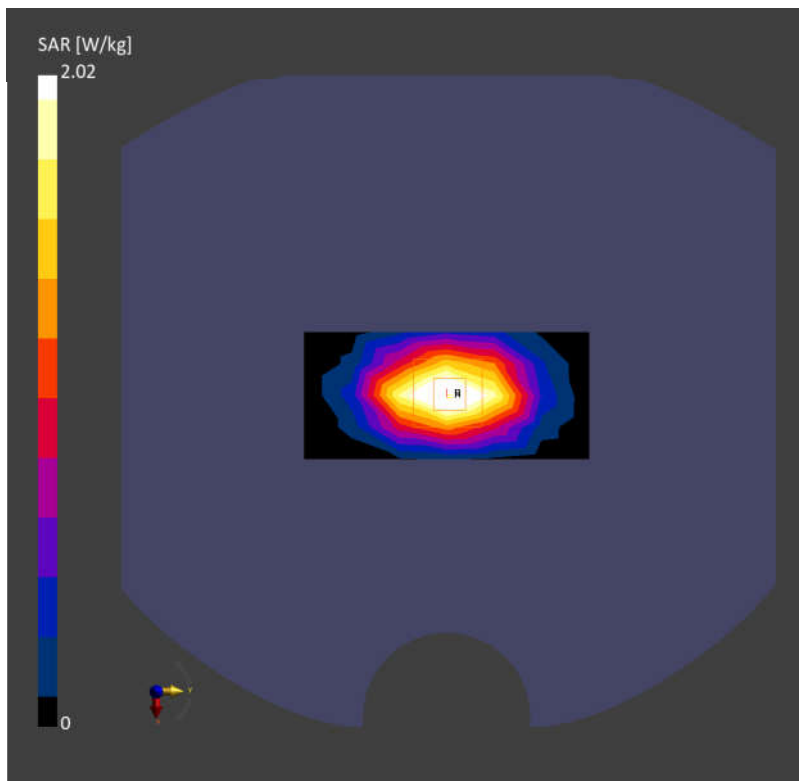

Date: 2025-08-25

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_250825 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.77$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.61, 7.54, 7.66); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.13 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.9 %

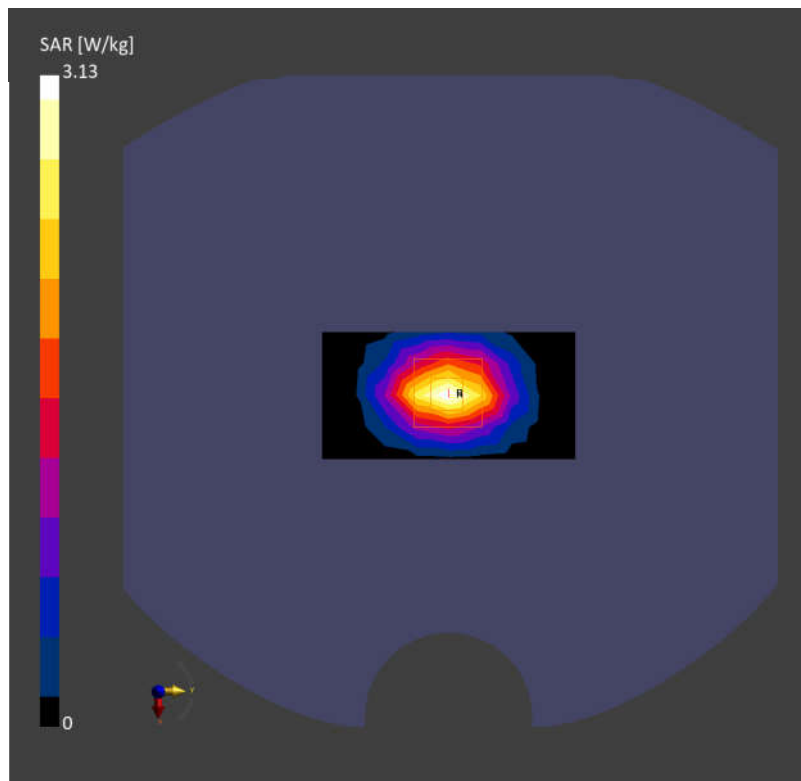

Date: 2025-08-26

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600_250826 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.53, 7.46, 7.57); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.34 W/kg; SAR (10g) = 1.08 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.51 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.2 %

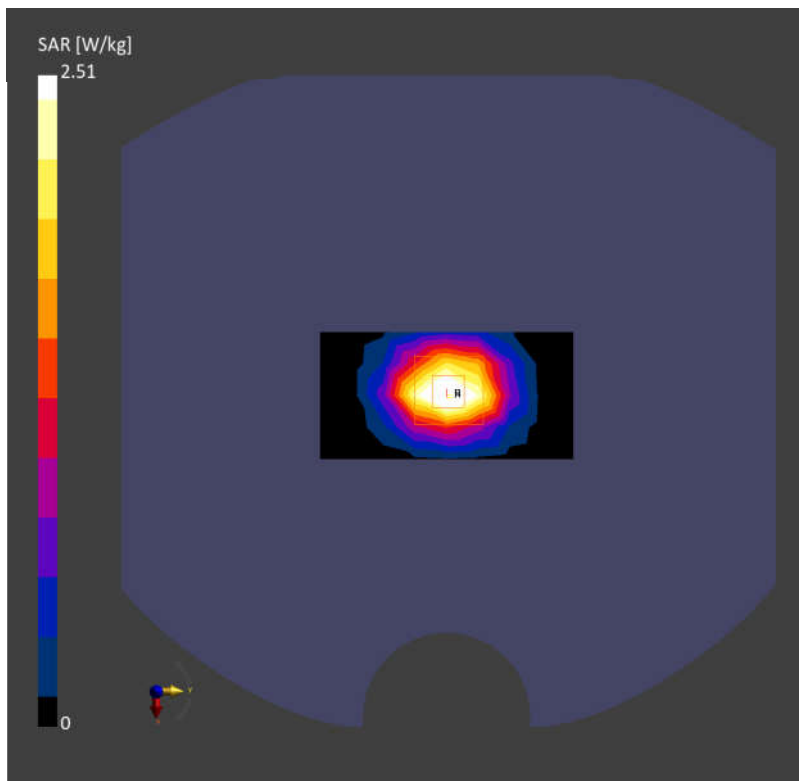

Date: 2025-08-27

System Check_Head_3500MHz**DUT: D3500V2 - SN1037**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500_250827 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.98$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.03, 6.96, 7.07); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.92 W/kg; SAR (10g) = 1.16 W/kg;


Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

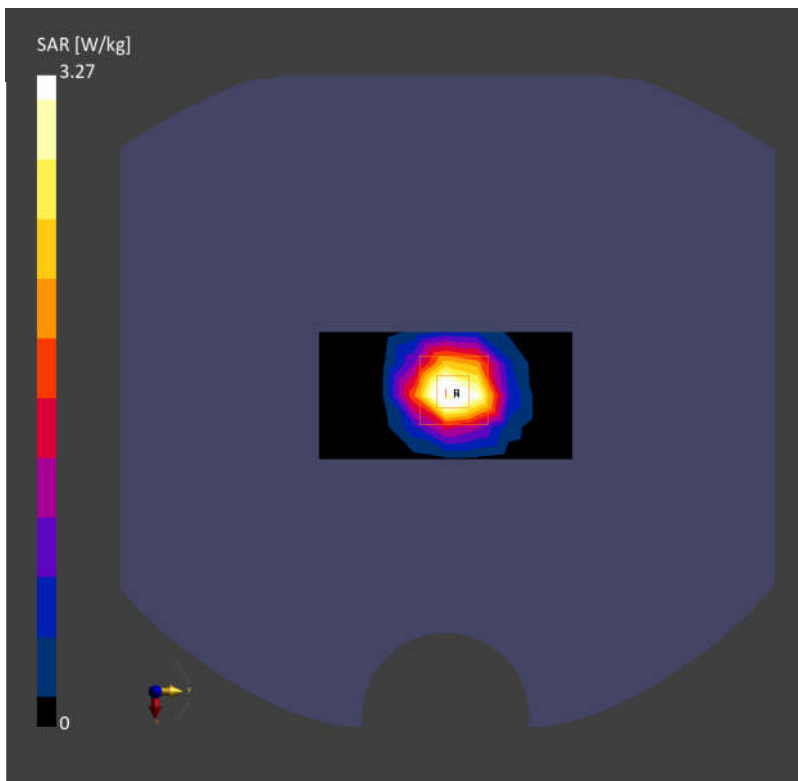

Date: 2025-08-28

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: HSL_3900_250828 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.37$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(5.49, 5.93, 5.62); Calibrated: 2025-07-25
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.04 W/kg; SAR (10g) = 1.13 W/kg;


Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.44 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

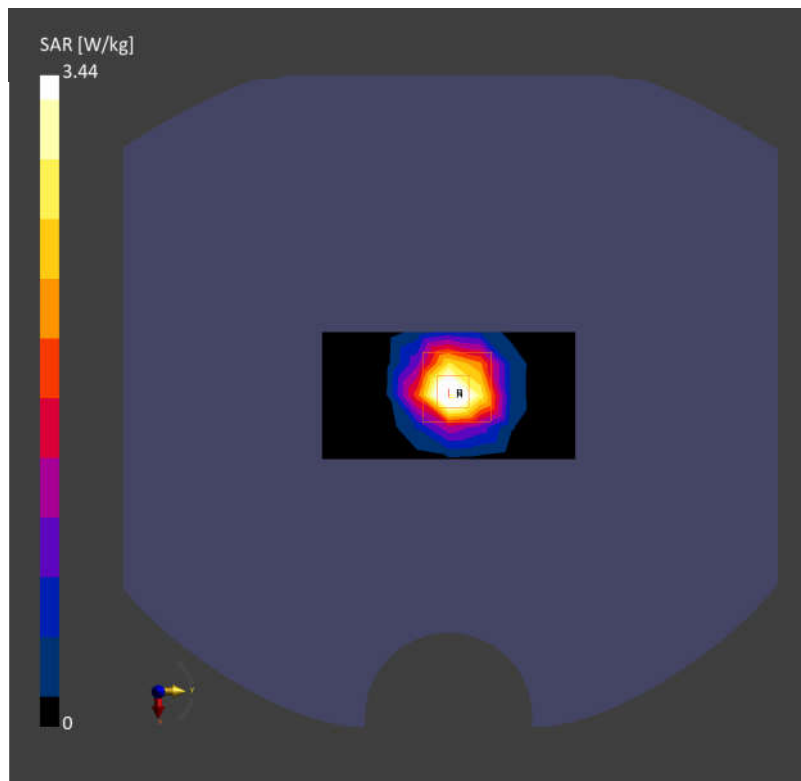

Date: 2025-08-29

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5250_250829 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.69$ S/m; $\epsilon_r = 36.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.92, 5.86, 5.95); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.98 W/kg; SAR (10g) = 0.891 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.83 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.6 %

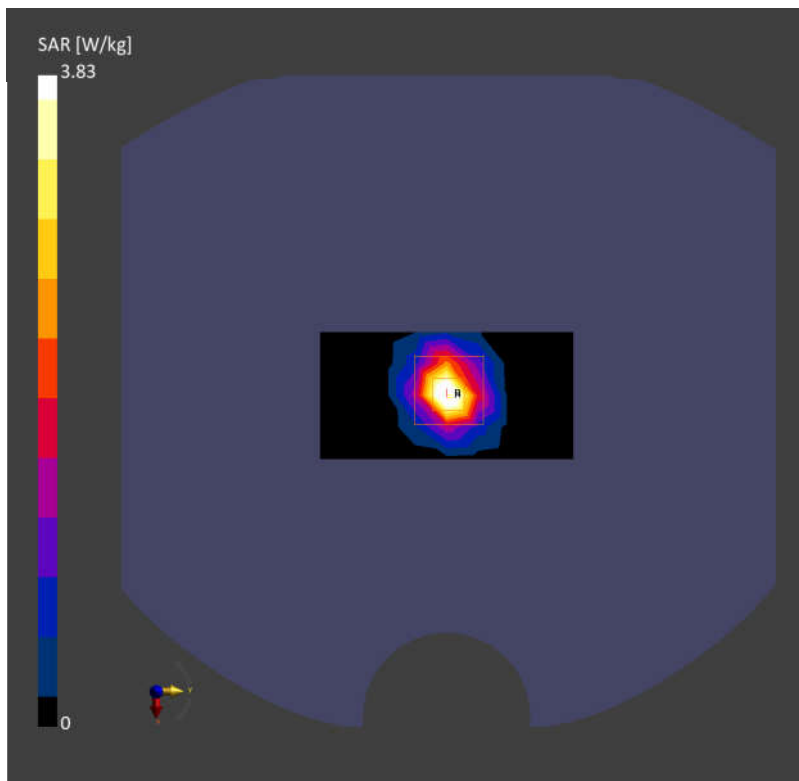

Date: 2025-08-30

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5600_250830 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.98$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.48, 5.43, 5.51); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 0.919 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.83 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 59.1 %

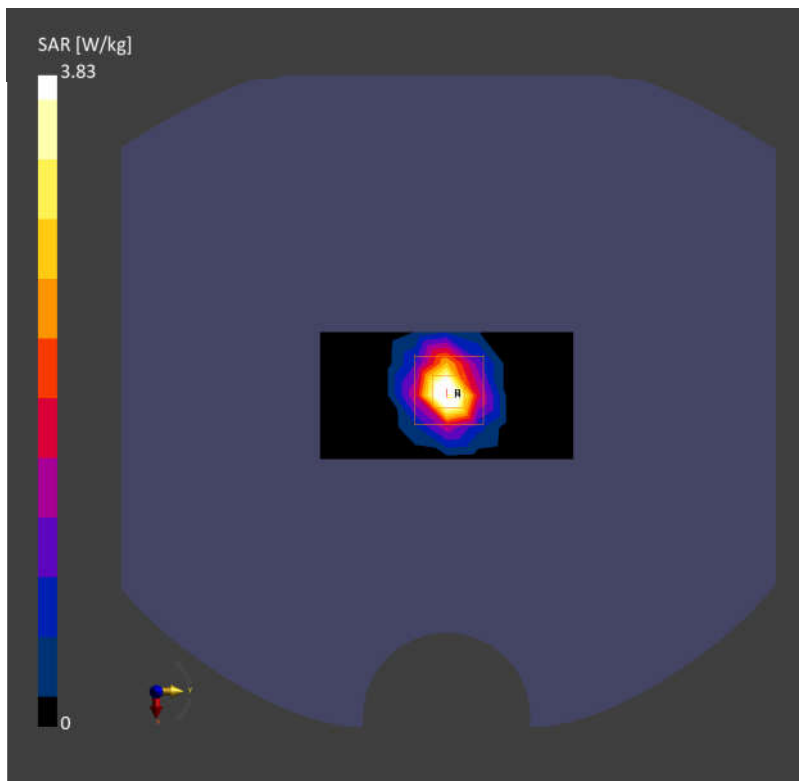

Date: 2025-08-31

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5750_250831 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.18$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.57, 5.52, 5.6); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2021; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.76 W/kg; SAR (10g) = 0.826 W/kg;


Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.71 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 57.8 %

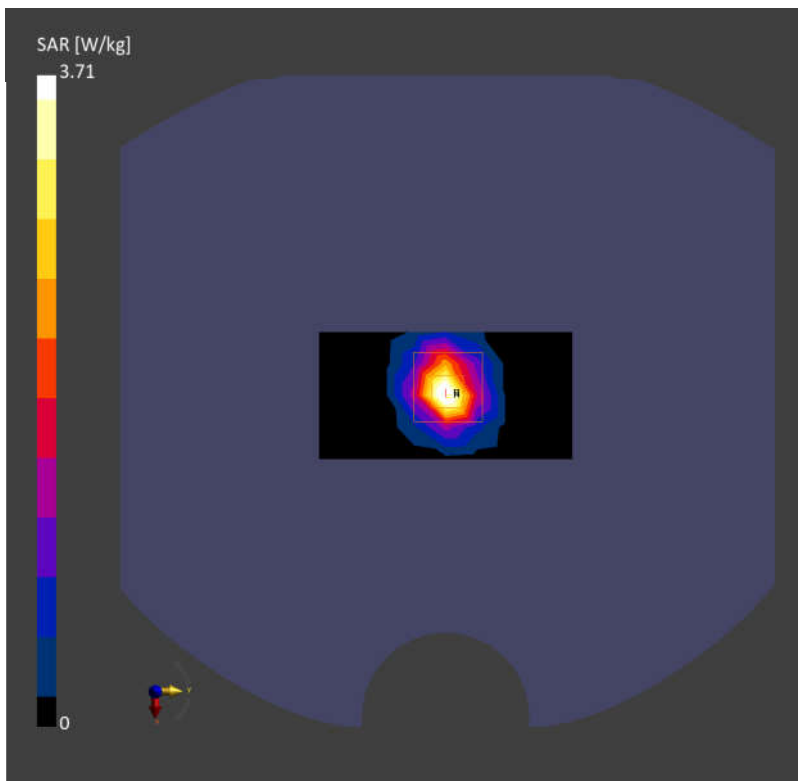

Date: 2025-08-27

System Check_Head_13MHz**DUT: CLA13 - SN:1023**

Communication System: ; Frequency: 13.000

Medium: HSL_13.0MHz_250827 Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.757$ S/m; $\epsilon_r = 53.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(16.06, 16.97, 16.03); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151; Section: Flat
- Measurement Software: 16.4.0.5005

Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.130 W/kg; SAR (10g) = 0.089 W/kg;

Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm;

Graded Ratio:1.4

Power Drift = 0.05 dB

SAR (1g) = 0.143 W/kg; SAR (10g) = 0.090 W/kg;

Smallest distance from peaks to all points 3dB below is 15.7 mm

Ratio of SAR at M2 to SAR at M1 = 73.9 %

