

Date: 2026-02-13

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600_260213 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.92$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7576; ConvF(7.35, 6.92, 7.0); Calibrated: 2025-11-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.75 W/kg; SAR (10g) = 1.23 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.76 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 7.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.2 %

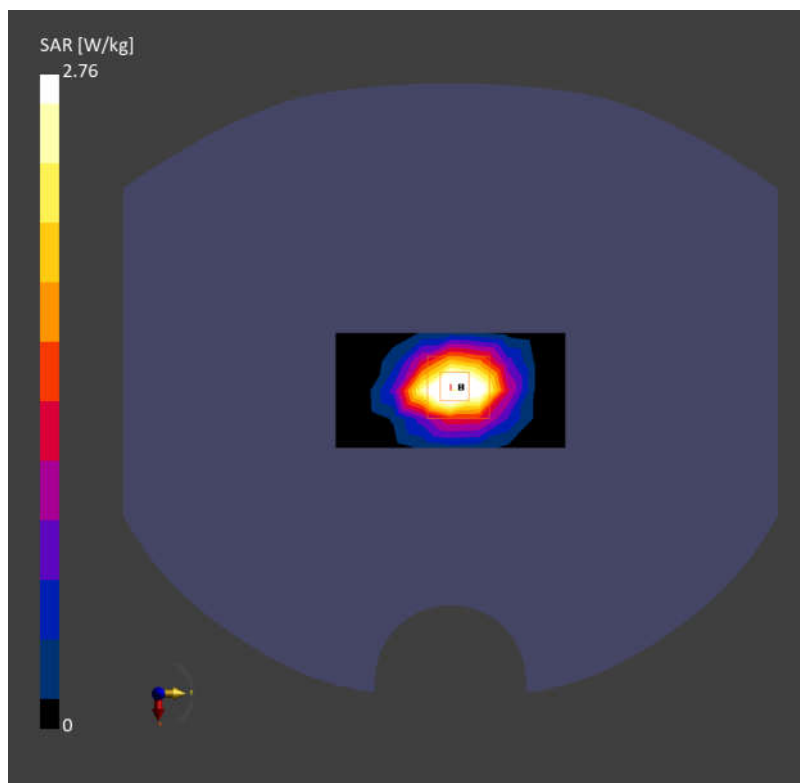

Date: 2026-02-14

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: HSL_3900_260214 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.38$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7576; ConvF(6.82, 6.42, 6.49); Calibrated: 2025-11-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.19 W/kg; SAR (10g) = 1.15 W/kg;

Pin=50mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm
mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.28 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 7.0 mm

Ratio of SAR at M2 to SAR at M1 = 72.6 %

