

Date: 2025/11/18

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.916$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(9.59, 9.21, 9.2); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.63 W/kg; SAR (10g) = 1.77 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.49 W/kg

Smallest distance from peaks to all points 3 dB below = 16.3 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

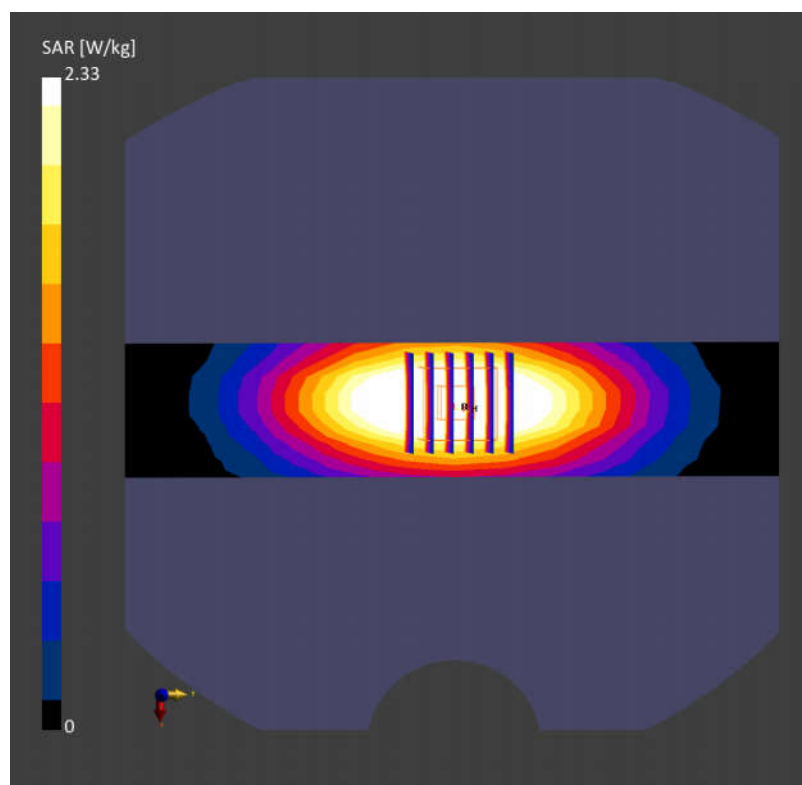

Date: 2025/11/18

System Check_1750MHz**DUT:D1750V2-SN:1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(8.14, 7.82, 7.81); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (36.0 mm x 120.0 mm): Measurement Grid: 3.0 mm x 15.0 mm

SAR (1g) = 8.86 W/kg; SAR (10g) = 4.82 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 8.75 W/kg; SAR (10g) = 4.71 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

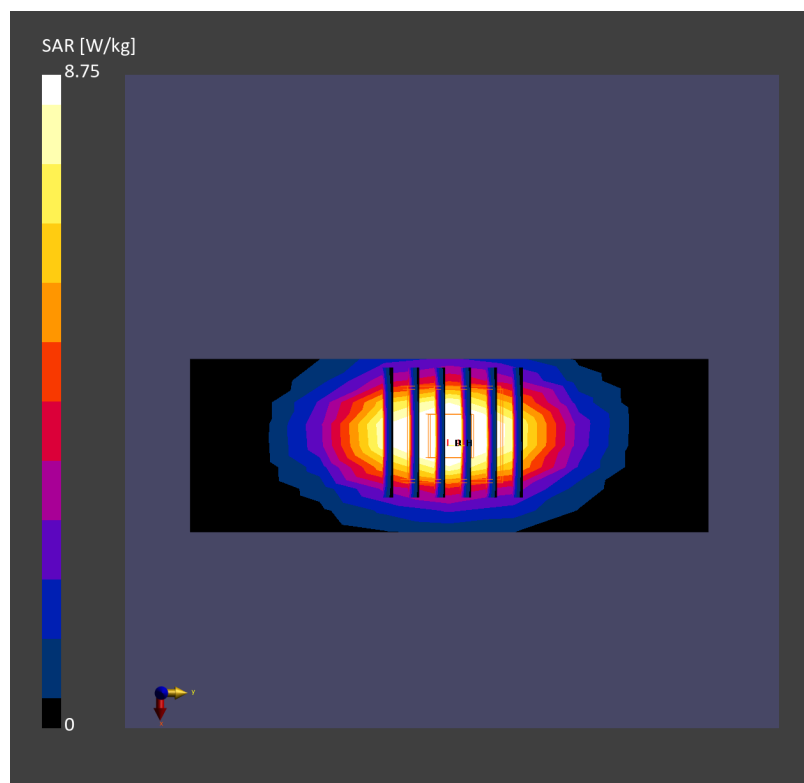

Date: 2025/11/18

System Check_1900MHz**DUT:D1900V2-SN:5d182**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.9, 7.58, 7.57); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 11.5 W/kg; SAR (10g) = 5.62 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 10.3 W/kg; SAR (10g) = 5.46 W/kg

Smallest distance from peaks to all points 3 dB below = 9.3 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

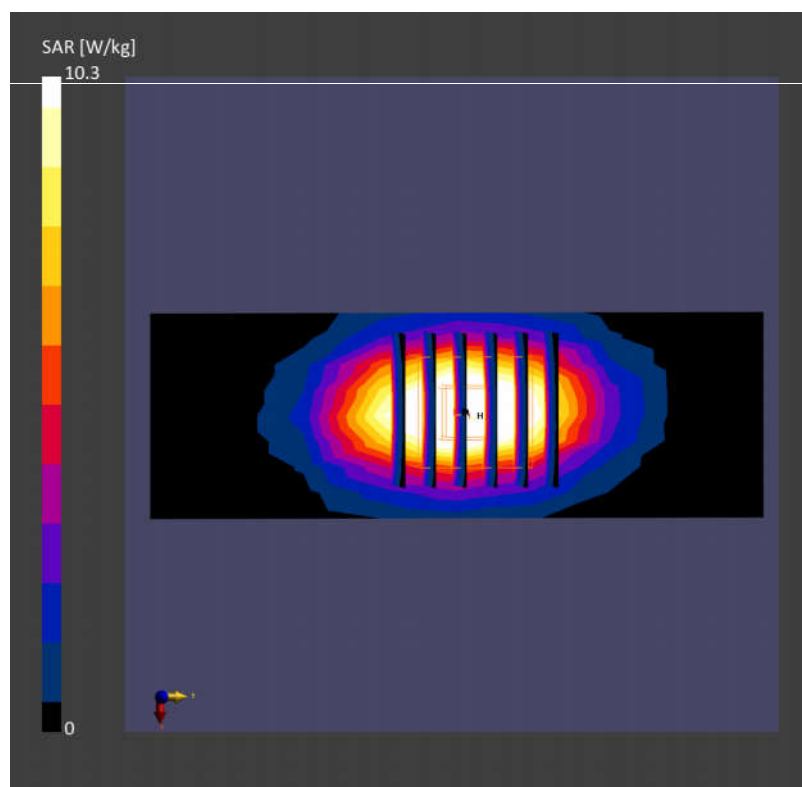

Date: 2025/11/18

System Check_2450MHz**DUT:D2450V2-SN:1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 13.9 W/kg; SAR (10g) = 6.56 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 13.8 W/kg; SAR (10g) = 6.43 W/kg

Smallest distance from peaks to all points 3 dB below = 9.3 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

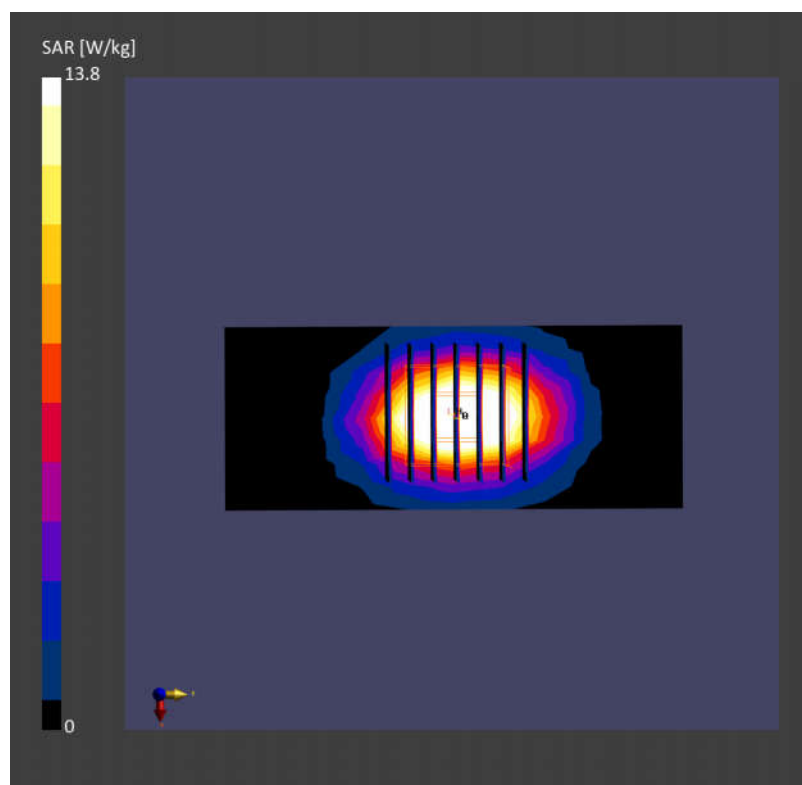

Date: 2025/11/18

System Check_2600MHz**DUT:D2600V2-SN:1070**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.13, 6.85, 6.84); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 14.4 W/kg; SAR (10g) = 6.17 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 13.8 W/kg; SAR (10g) = 6.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

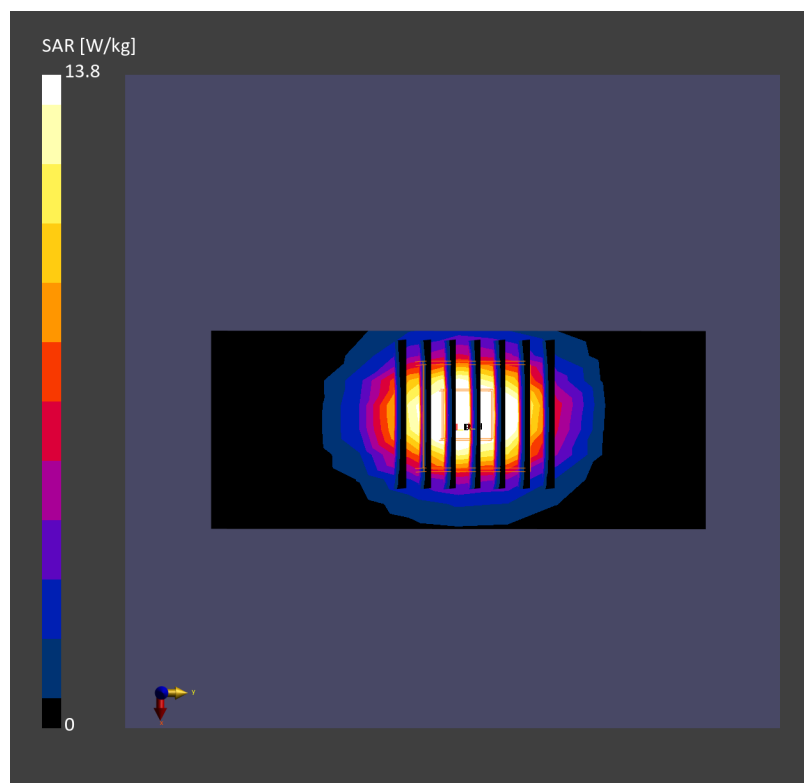

Date: 2025/11/18

System Check_5250MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.61$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.8, 5.57, 5.56); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.98W/kg; SAR (10g) = 2.34W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 7.87 W/kg; SAR (10g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.9 %

