

Date: 2025-08-15

System Check_Head_750MHz**DUT: D750V3 - SN1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL_750MHz_250815 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.883$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(9.82, 9.54, 9.21); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.427 W/kg; SAR (10g) = 0.285 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 0.426 W/kg; SAR (10g) = 0.287 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

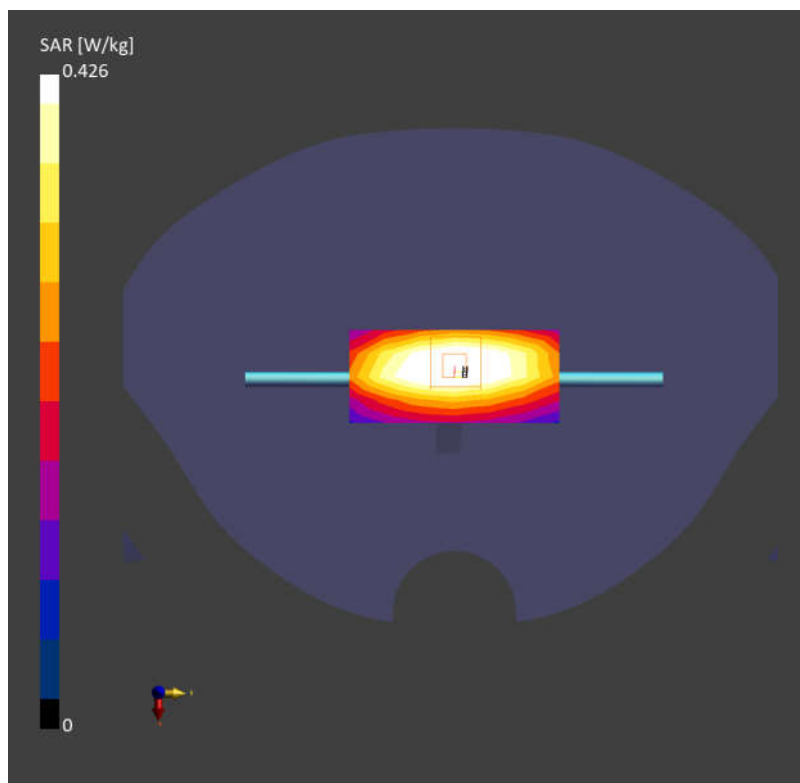

Date: 2025-08-23

System Check_Head_750MHz**DUT: D750V3 - SN1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL_750MHz_250823 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.886$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(9.82, 9.54, 9.21); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.432 W/kg; SAR (10g) = 0.288 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 0.426 W/kg; SAR (10g) = 0.288 W/kg

Smallest distance from peaks to all points 3 dB below = 17.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.2 %

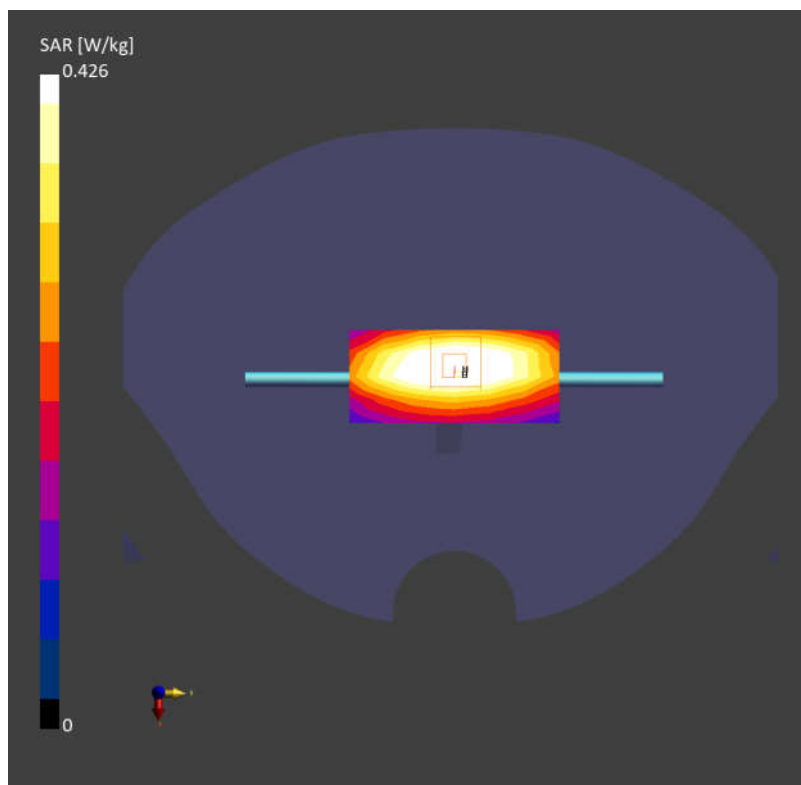

Date: 2025-08-16

System Check_Head_835MHz**DUT: D835V2 - SN4d298**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_835MHz_250816 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.917$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(9.69, 9.42, 9.09); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.507 W/kg; SAR (10g) = 0.334 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.508 W/kg; SAR (10g) = 0.347 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

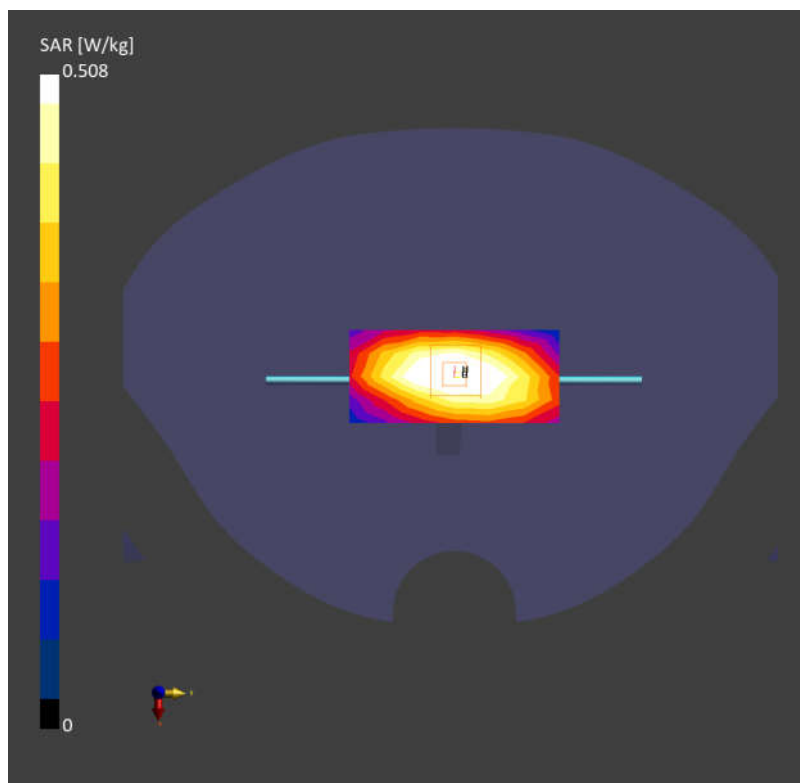

Date: 2025-08-24

System Check_Head_835MHz**DUT: D835V2 - SN4d298**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_835MHz_250824 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.916$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(9.69, 9.42, 9.09); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.511 W/kg; SAR (10g) = 0.336 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.518 W/kg; SAR (10g) = 0.347 W/kg

Smallest distance from peaks to all points 3 dB below = 16.4 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

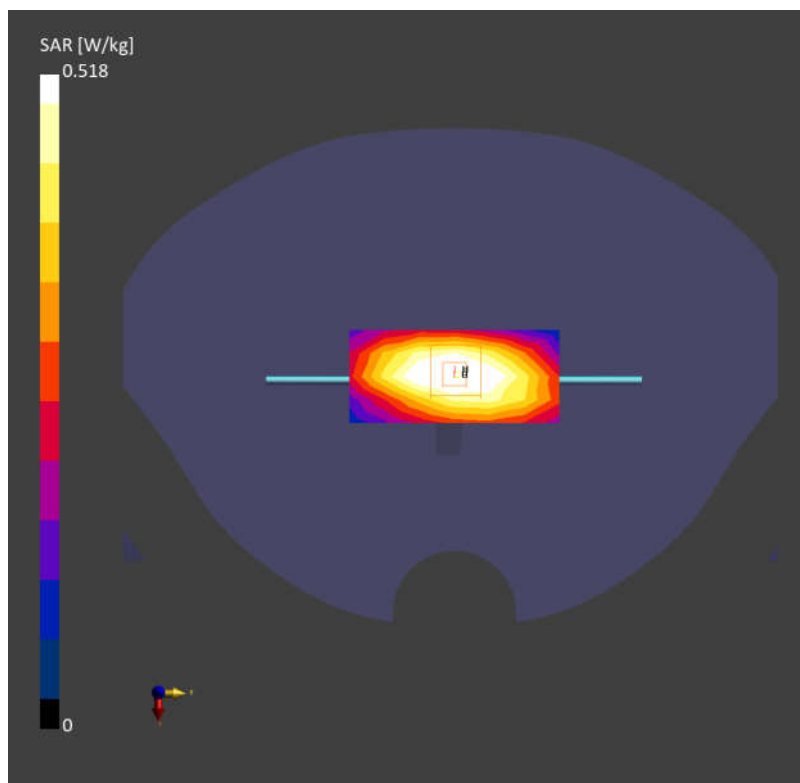

Date: 2025-08-17

System Check_Head_1750MHz**DUT: D1750V2 - SN1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: HSL_1750MHz_250817 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.3C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(8.23, 8.0, 7.73); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.19 W/kg; SAR (10g) = 1.17 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.94 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.9 %

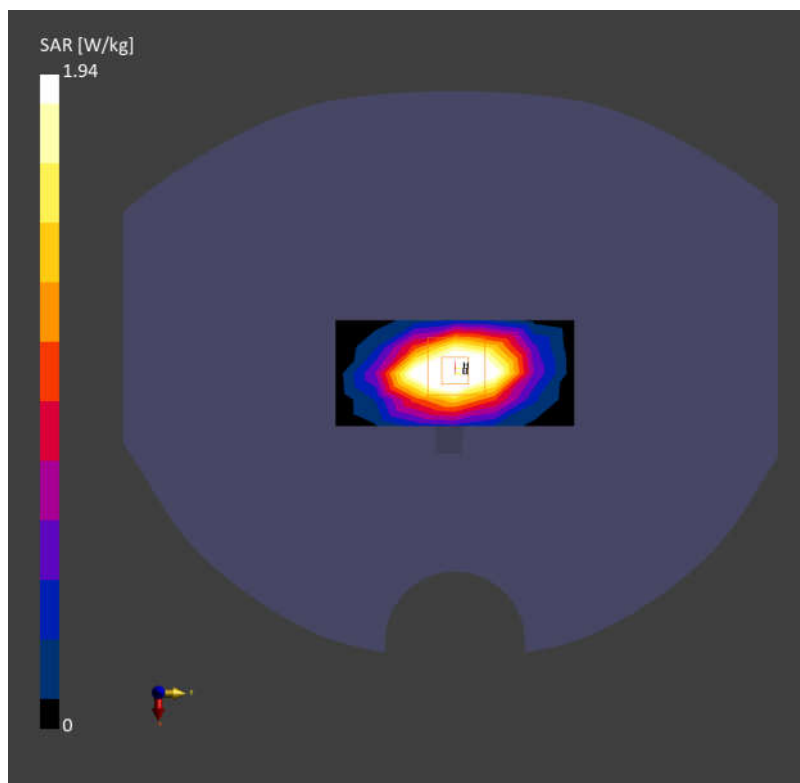

Date: 2025-08-25

System Check_Head_1750MHz**DUT: D1750V2 - SN1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: HSL_1750MHz_250825 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(8.23, 8.0, 7.73); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.17 W/kg; SAR (10g) = 1.16 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.92 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

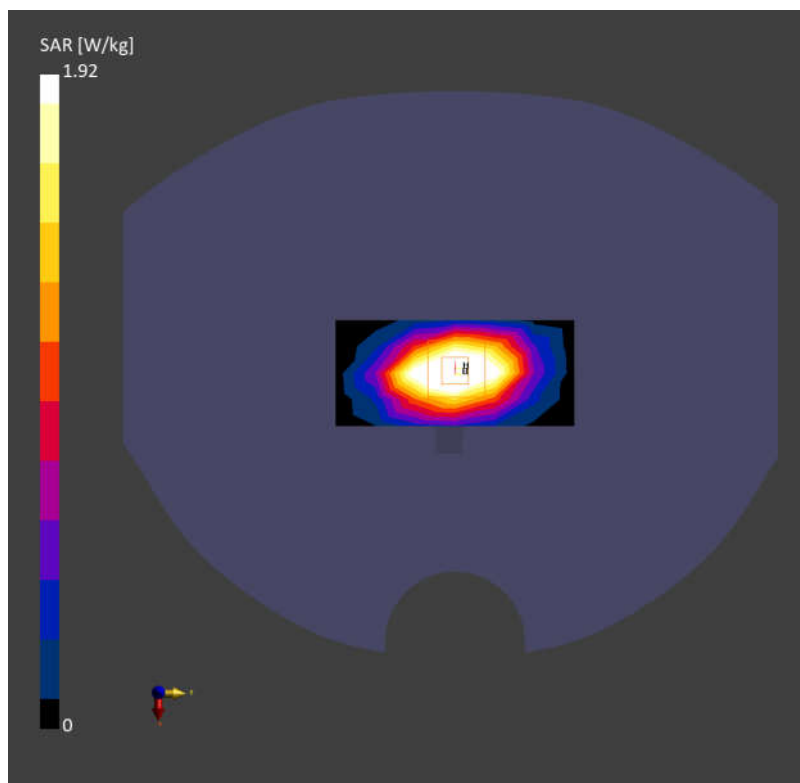

Date: 2025-08-18

System Check_Head_1900MHz**DUT: D1900V2 - SN5d170**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL_1900MHz_250818 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(8.01, 7.78, 7.51); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.02 W/kg; SAR (10g) = 1.07 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.10 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.2 %

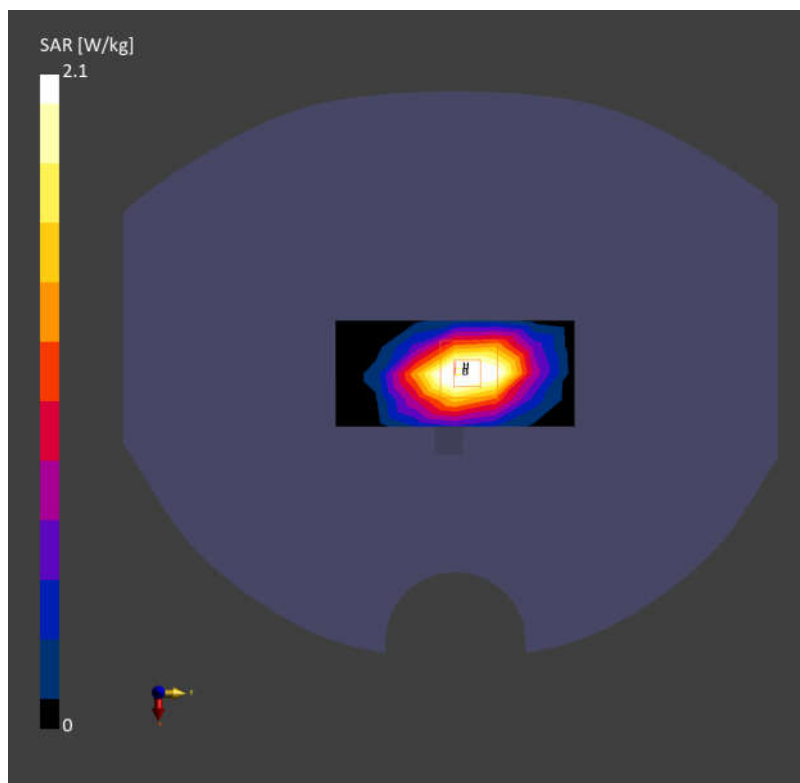

Date: 2025-08-25

System Check_Head_1900MHz**DUT: D1900V2 - SN5d170**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL_1900MHz_250825 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(8.01, 7.78, 7.51); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm
SAR (1g) = 2.04 W/kg; SAR (10g) = 1.08 W/kg;


Pin=50mW/Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.12 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

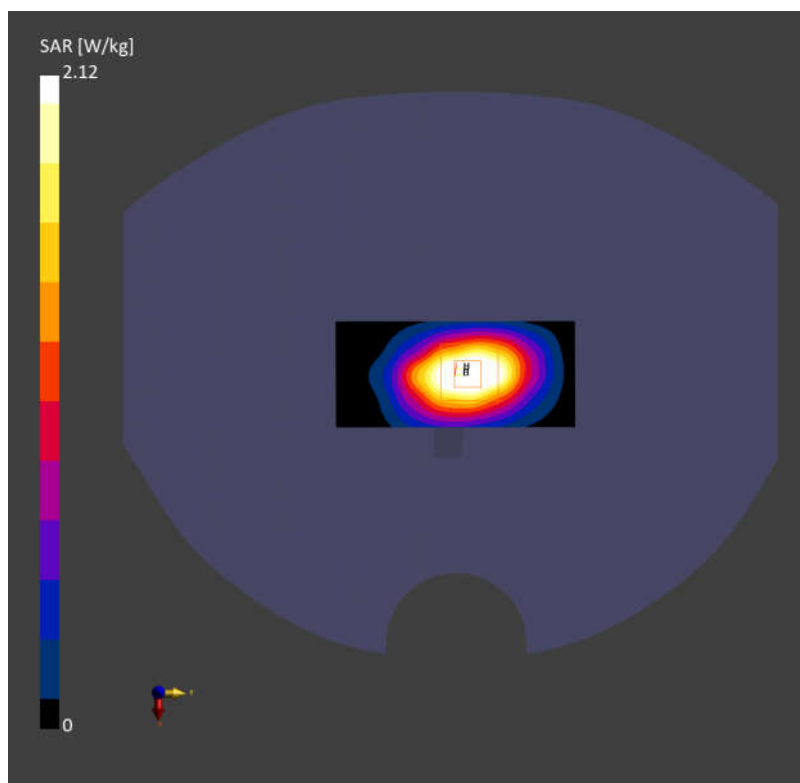

Date: 2025-08-30

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450MHz_250830 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.78$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(7.36, 7.16, 6.91); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
 SAR (1g) = 2.84 W/kg; SAR (10g) = 1.33 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 2.84 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.8 %

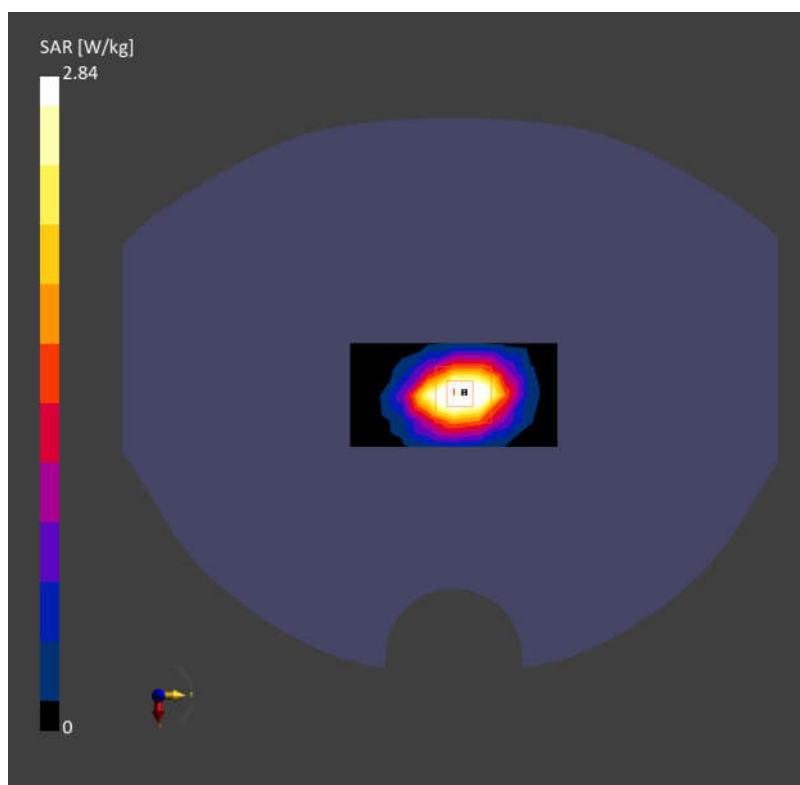

Date: 2025-08-19

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600MHz_250819 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(7.22, 7.02, 6.78); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.94 W/kg; SAR (10g) = 1.32 W/kg;**Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.94 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

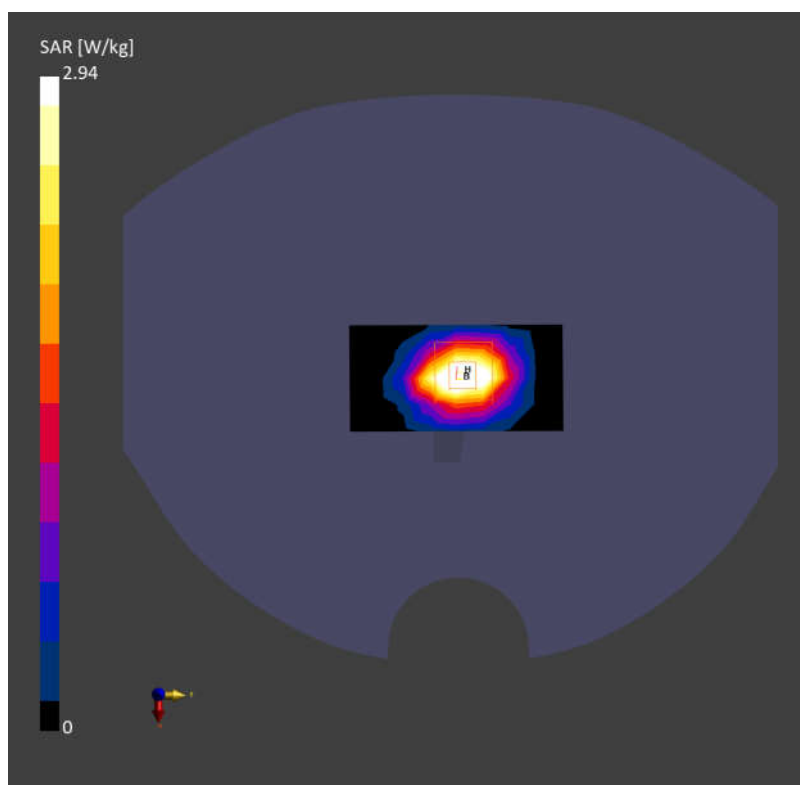

Date: 2025-08-26

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600MHz_250826 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 38.9$


Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(7.22, 7.02, 6.78); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.94 W/kg; SAR (10g) = 1.32 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.04 dB
SAR (1g) = 2.96 W/kg; SAR (10g) = 1.32 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 81.6 %

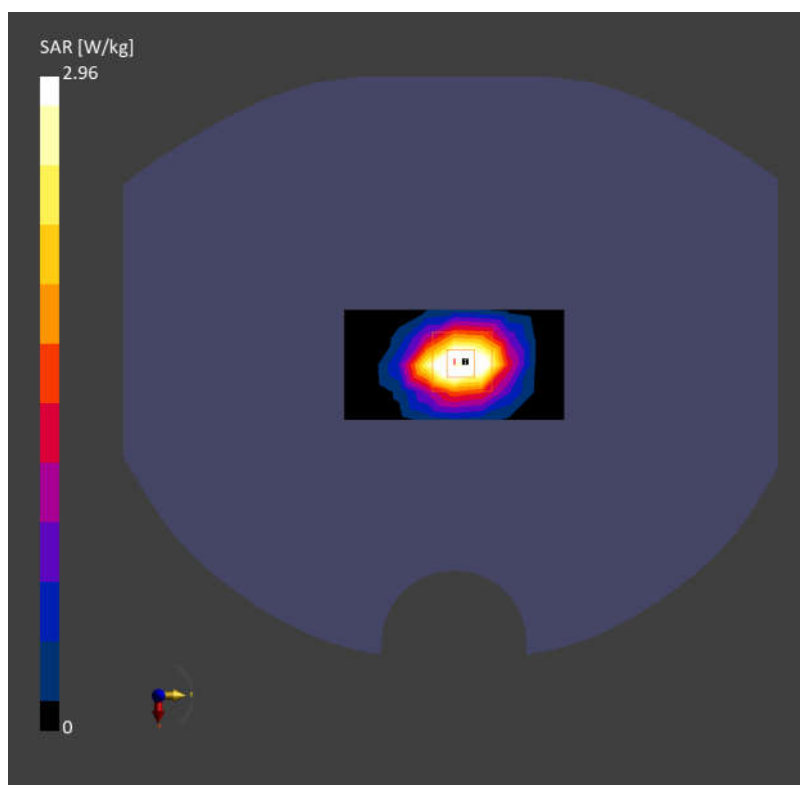

Date: 2025-08-20

System Check_Head_3500MHz**DUT: D3500V2 - SN1037**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500MHz_250820 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.98$ S/m; $\epsilon_r = 37.7$


Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(6.86, 6.67, 6.44); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.42 W/kg; SAR (10g) = 1.22 W/kg;

Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 3.55 W/kg; SAR (10g) = 1.25 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 76.7 %

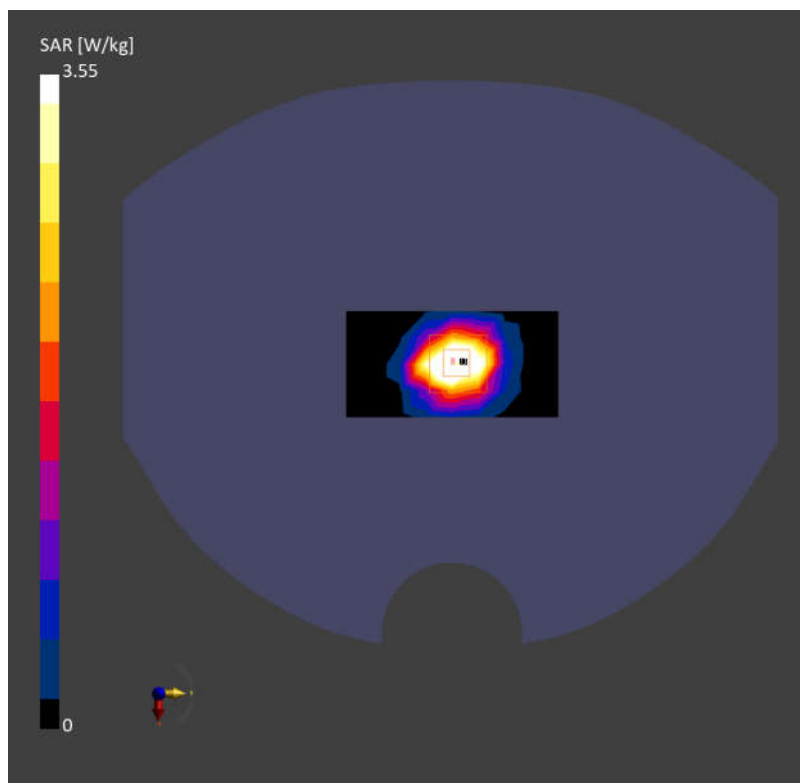

Date: 2025-08-27

System Check_Head_3500MHz**DUT: D3500V2 - SN1037**

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500MHz_250827 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.95$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(6.86, 6.67, 6.44); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
 SAR (1g) = 2.96 W/kg; SAR (10g) = 1.17 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.07 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 77.6 %

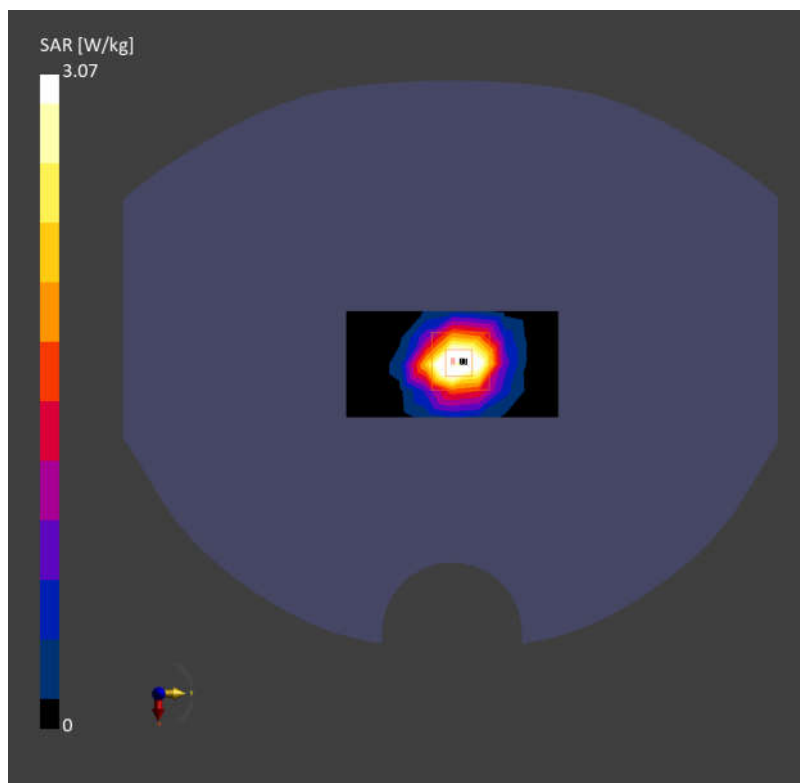

Date: 2025-08-21

System Check_Head_3700MHz**DUT: D3700V2 - SN1008**

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: HSL_3700MHz_250821 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.19$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(6.77, 6.58, 6.35); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 1.20 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.45 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

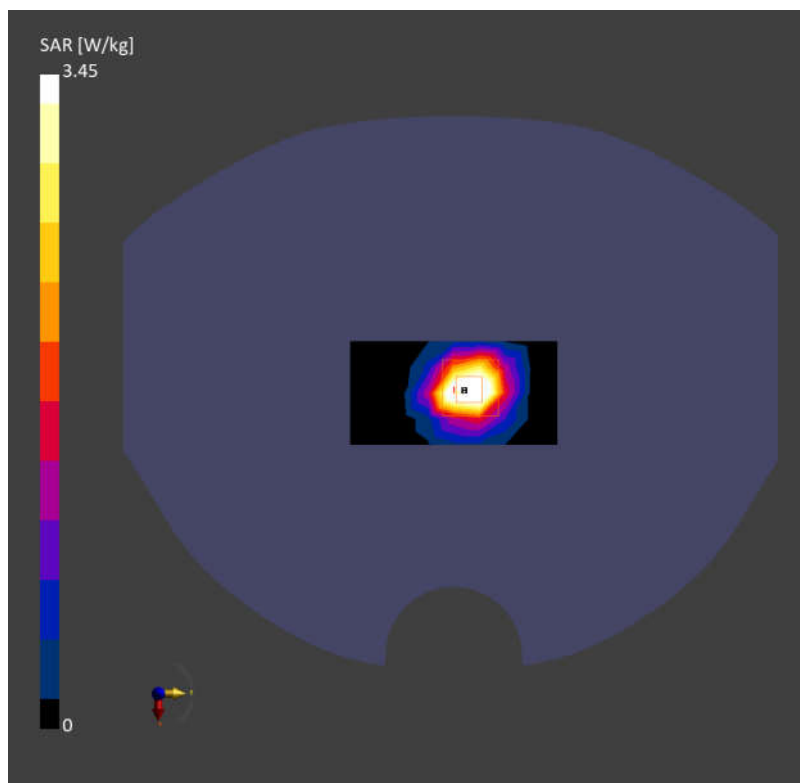

Date: 2025-08-28

System Check_Head_3700MHz**DUT: D3700V2 - SN1008**

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: HSL_3700MHz_250828 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(6.77, 6.58, 6.35); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 2.95 W/kg; SAR (10g) = 1.16 W/kg;**Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.04 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9.3 mm

Ratio of SAR at M2 to SAR at M1 = 74.8 %

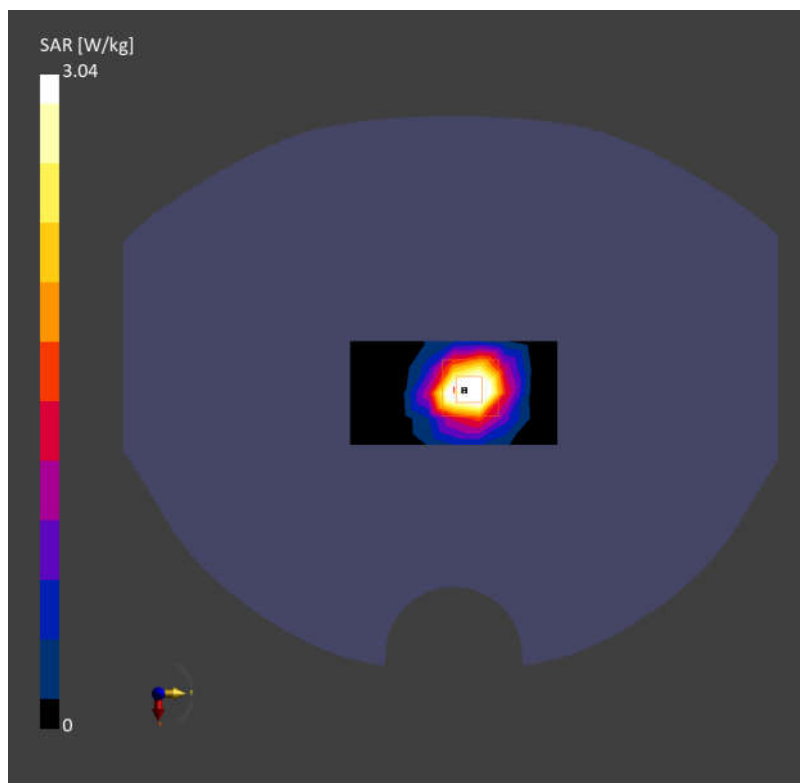

Date: 2025-08-22

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: HSL_3900MHz_250822 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.38$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(6.68, 6.49, 6.27); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
 SAR (1g) = 3.77 W/kg; SAR (10g) = 1.25 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.65 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 7.0 mm

Ratio of SAR at M2 to SAR at M1 = 71.5 %

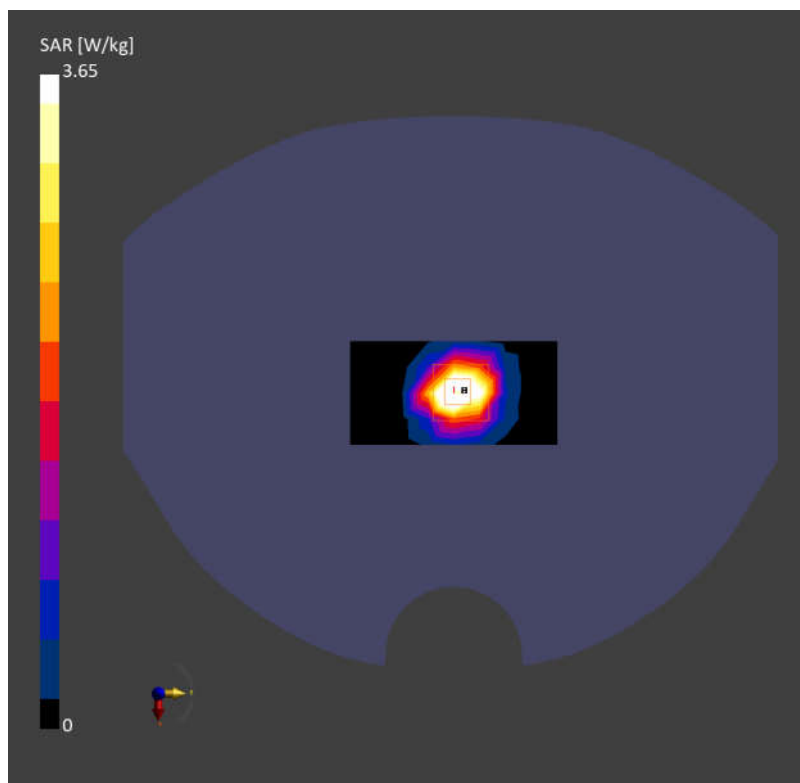

Date: 2025-08-29

System Check_Head_3900MHz**DUT: D3900V2 - SN1048**

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: HSL_3900MHz_250829 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.40$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(6.68, 6.49, 6.27); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.32 W/kg; SAR (10g) = 1.21 W/kg;**Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.51 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 7.7 mm

Ratio of SAR at M2 to SAR at M1 = 72.2 %

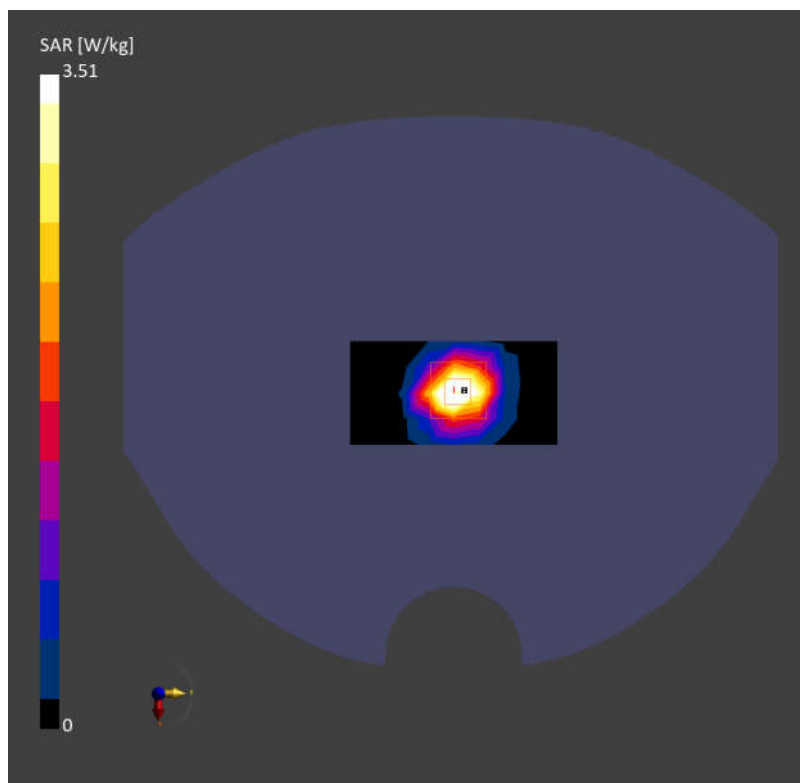

Date: 2025-08-31

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5250MHz_250831 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.74$ S/m; $\epsilon_r = 36.5$


Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(5.93, 5.77, 5.57); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 4.05 W/kg; SAR (10g) = 1.13 W/kg;

Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.01 dB
SAR (1g) = 4.45 W/kg; SAR (10g) = 1.17 W/kg
Smallest distance from peaks to all points 3 dB below = 6.4 mm
Ratio of SAR at M2 to SAR at M1 = 64.5 %

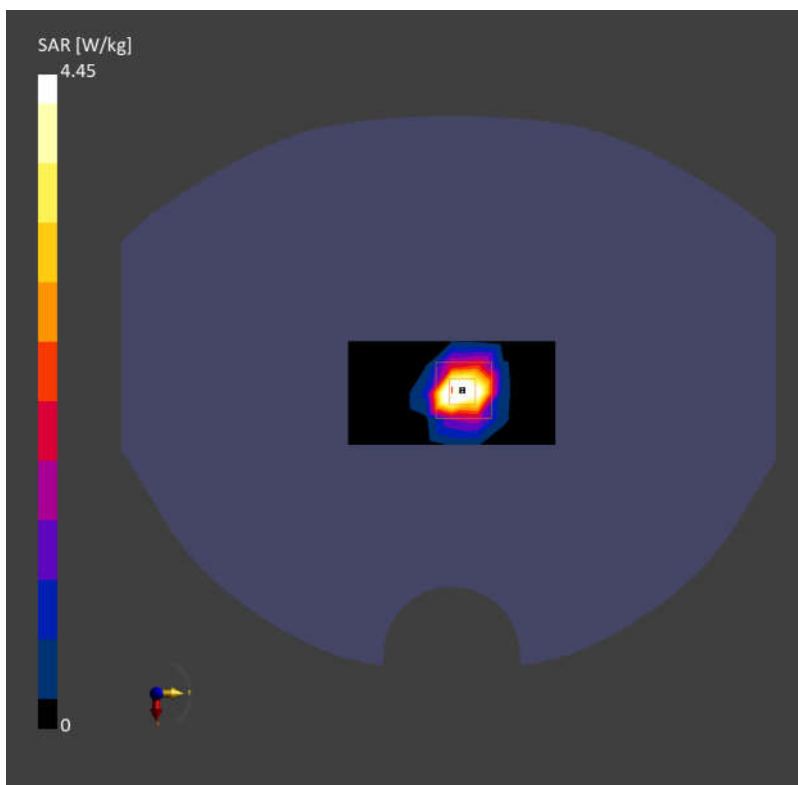

Date: 2025-08-31

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5600MHz_250831 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.03$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(5.42, 5.27, 5.08); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 4.11 W/kg; SAR (10g) = 1.15 W/kg;**Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 4.46 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 60.9 %

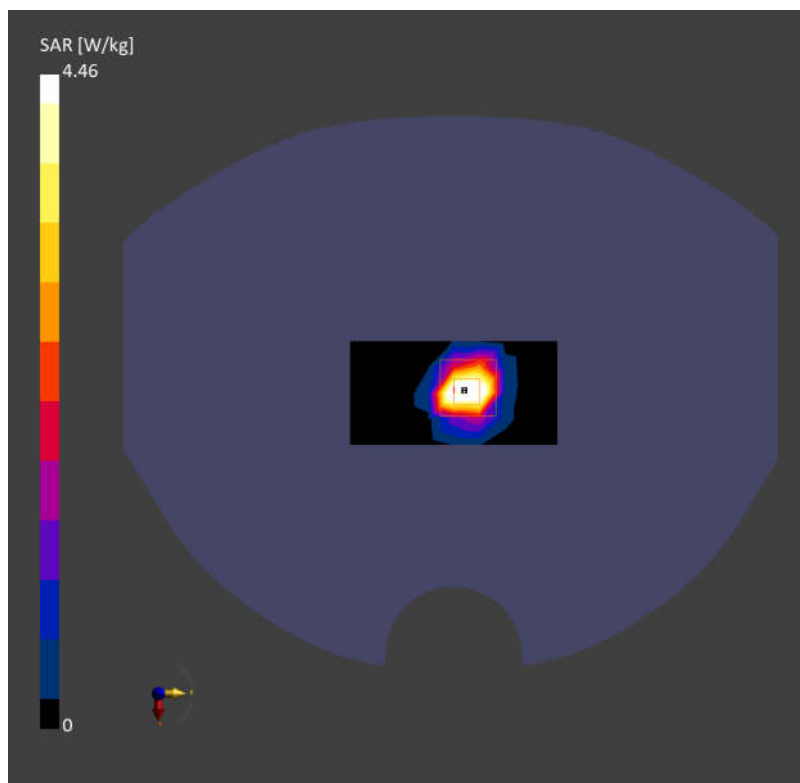

Date: 2025-09-01

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5750MHz_250901 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.25$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(5.53, 5.38, 5.19); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--


Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.27 W/kg; SAR (10g) = 1.01 W/kg;**Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 3.64 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 61.5 %

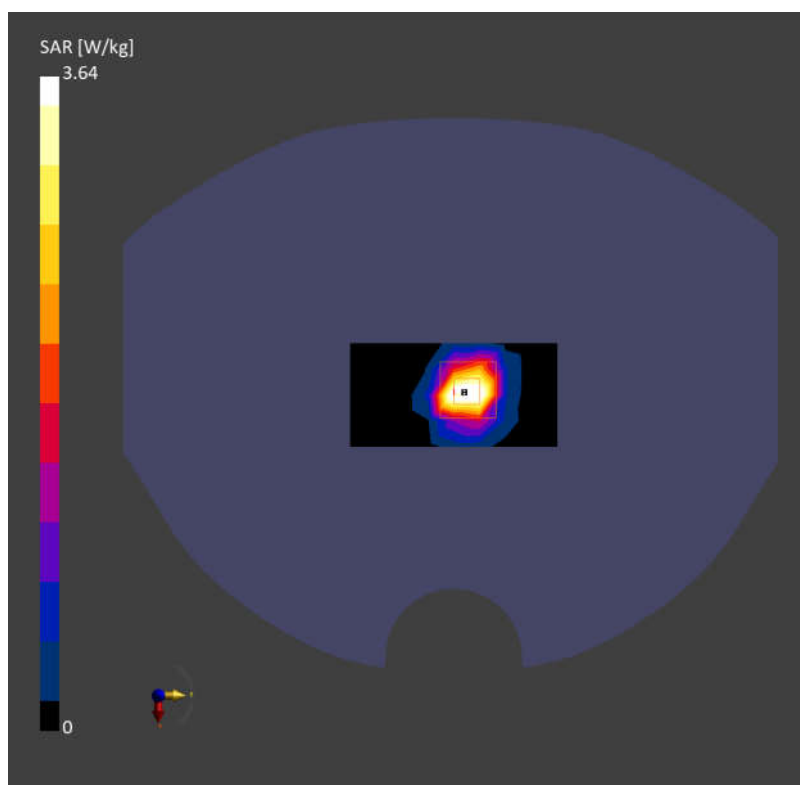

Date: 2025-09-01

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1026**

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: HSL_6500MHz_250901 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.10$ S/m; $\epsilon_r = 34.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.34, 6.3, 5.44); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1650; Calibrated: 2024-11-25
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 10.8 W/kg; SAR (10g) = 2.30 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 15.2 W/kg; SAR (10g) = 2.98 W/kg

Smallest distance from peaks to all points 3 dB below = 4.6 mm

Ratio of SAR at M2 to SAR at M1 = 53.0 %

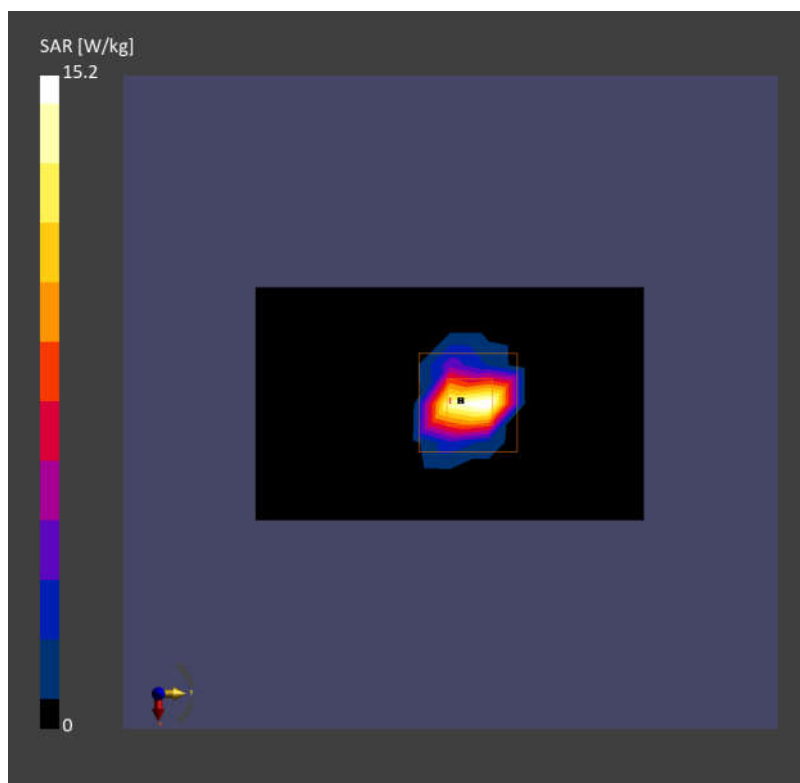psAPD (4.0cm², sq) = 67.0 [W/m²]

Date: 2025-09-25

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1341**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5600_250925 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.99$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(5.42, 5.27, 5.08); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.58 W/kg; SAR (10g) = 1.08 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 4.28 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 59.2 %

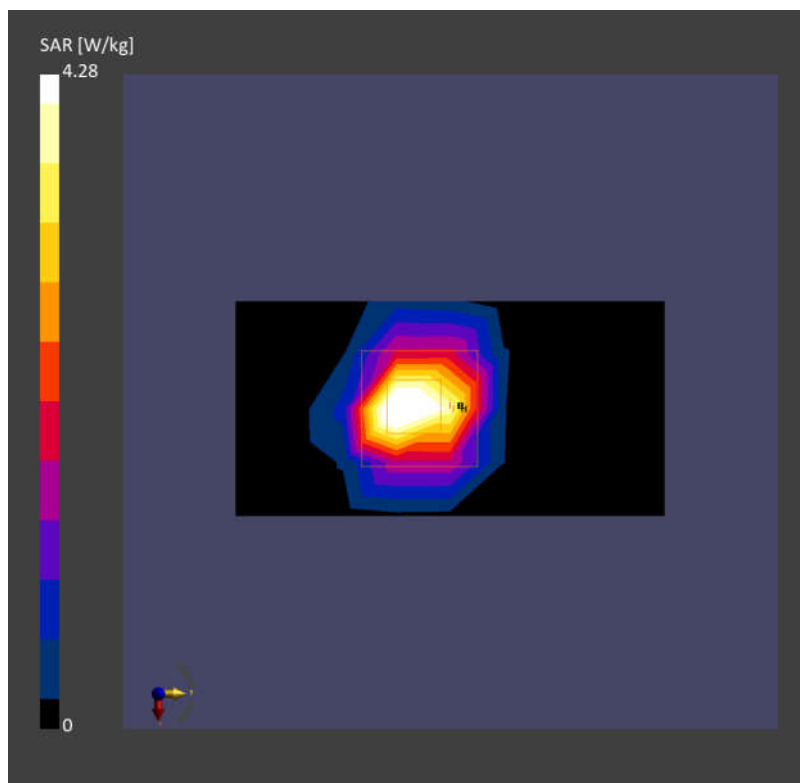

Date: 2025-09-26

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1341**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5750_250926 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.17$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7918; ConvF(5.53, 5.38, 5.19); Calibrated: 2025-03-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 0.991 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.99 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 57.4 %

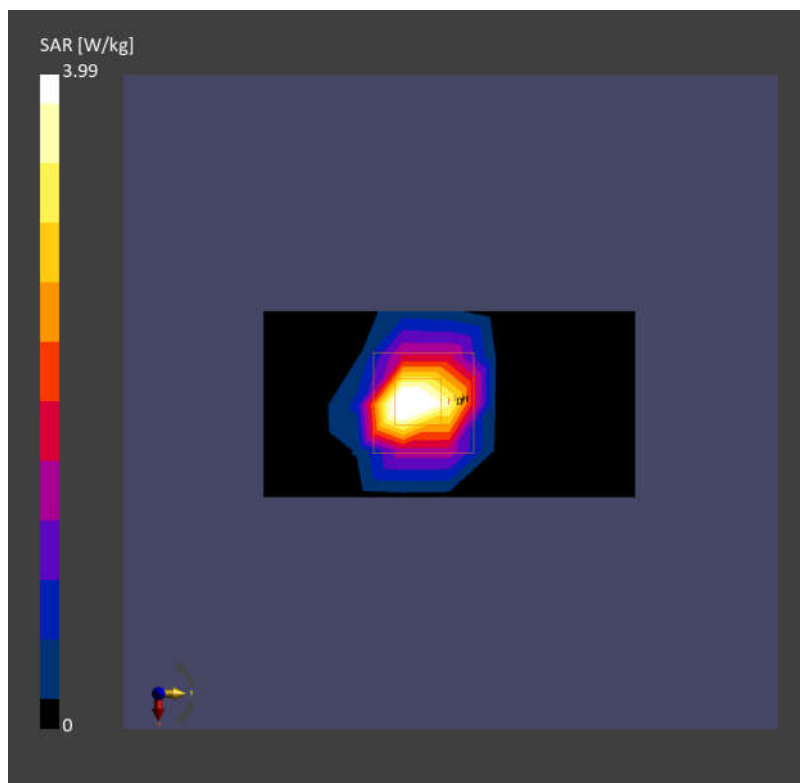

Measurement Report for Source 10G, FRONT, Validation band, CW, Channel 10000 (10000.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]
Source 10G,	100.0 x 100.0 x 105.0

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor
5G	FRONT, 10.00	Validation band	CW, 0--	10000.0, 10000	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave – 1065	Air –	EUmmWV4 – SN9553_F1–55GHz, 2024–11–15	DAE4 Sn1650, 2024–11–25

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0
MAIA	N/A

Measurement Results

Scan Type	5G Scan
Date	2025–08–30
Avg. Area [cm ²]	4.00
psPDn+ [W/m ²]	96.8
psPDtot+ [W/m ²]	97.7
psPDmod+ [W/m ²]	102
E _{max} [V/m]	232
Power Drift [dB]	0.05

