

Date: 2026-01-22

System Check_Head_750MHz**DUT: D750V3 - SN1087**

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL_750_260122 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.37, 10.09, 10.28); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.427 W/kg; SAR (10g) = 0.284 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.278 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

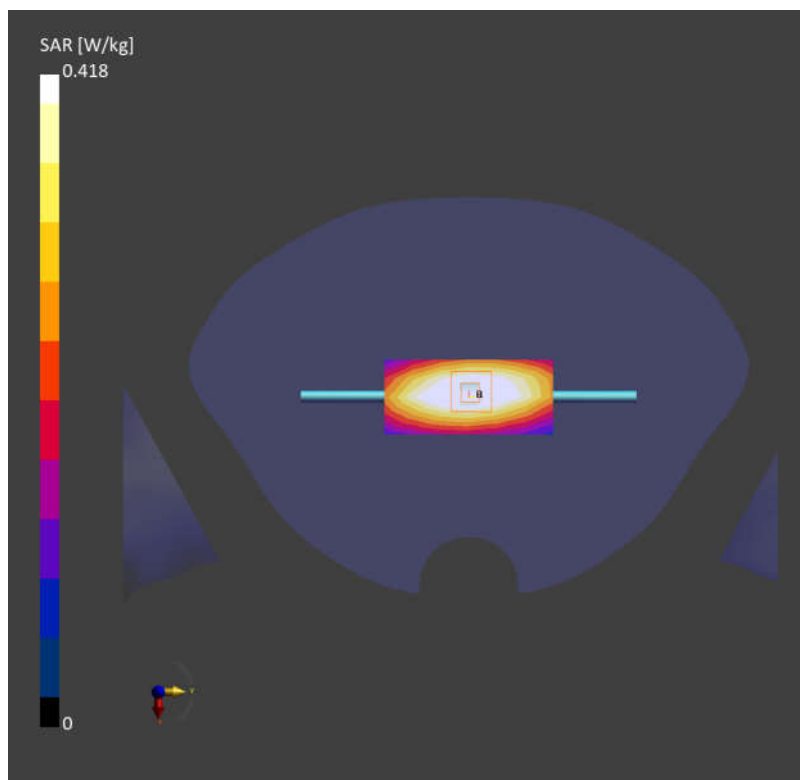

Date: 2026-01-23

System Check_Head_835MHz**DUT: D835V2 - SN4d298**

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_835_260123 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.920$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.17, 9.9, 10.08); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.439 W/kg; SAR (10g) = 0.288 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.461 W/kg; SAR (10g) = 0.294 W/kg

Smallest distance from peaks to all points 3 dB below = 14.4 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

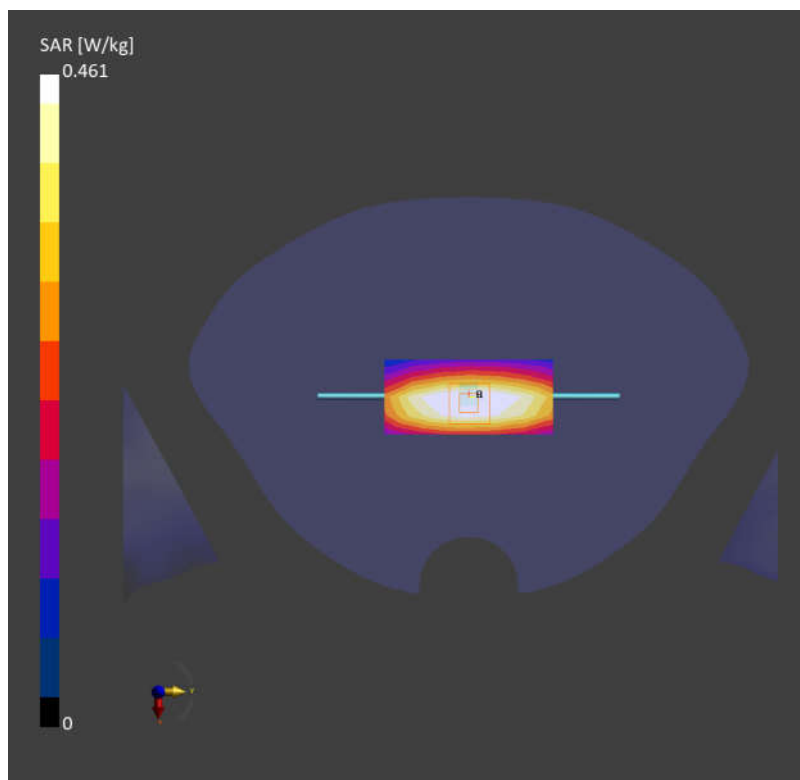

Date: 2026-01-24

System Check_Head_1750MHz**DUT: D1750V2 - SN1090**

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: HSL_1750_260124 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.4, 8.17, 8.33); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.82 W/kg; SAR (10g) = 0.967 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 1.80 W/kg; SAR (10g) = 0.968 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

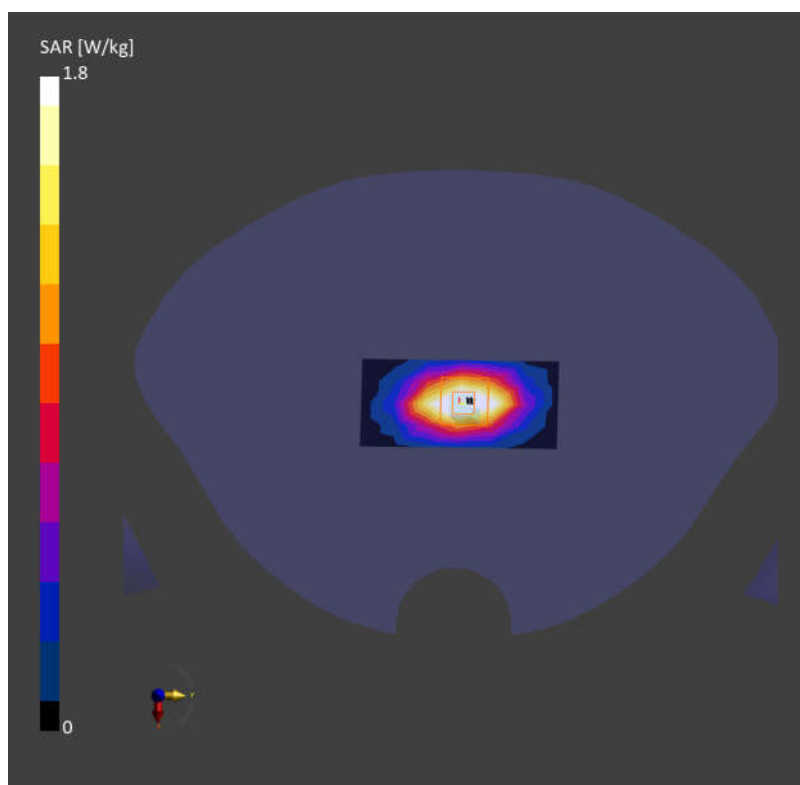

Date: 2026-01-25

System Check_Head_1900MHz**DUT: D1900V2 - SN5d170**

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL_1900_260125 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.21, 7.99, 8.14); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.09 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.12 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

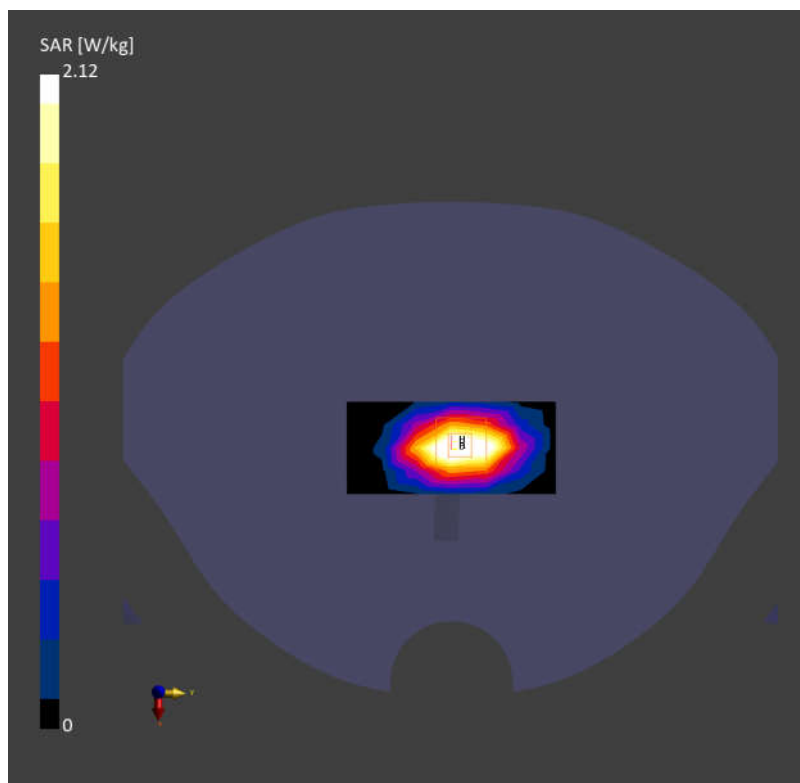

Date: 2026-01-29

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_260129 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.76$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.65, 7.44, 7.58); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.24 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.8 %

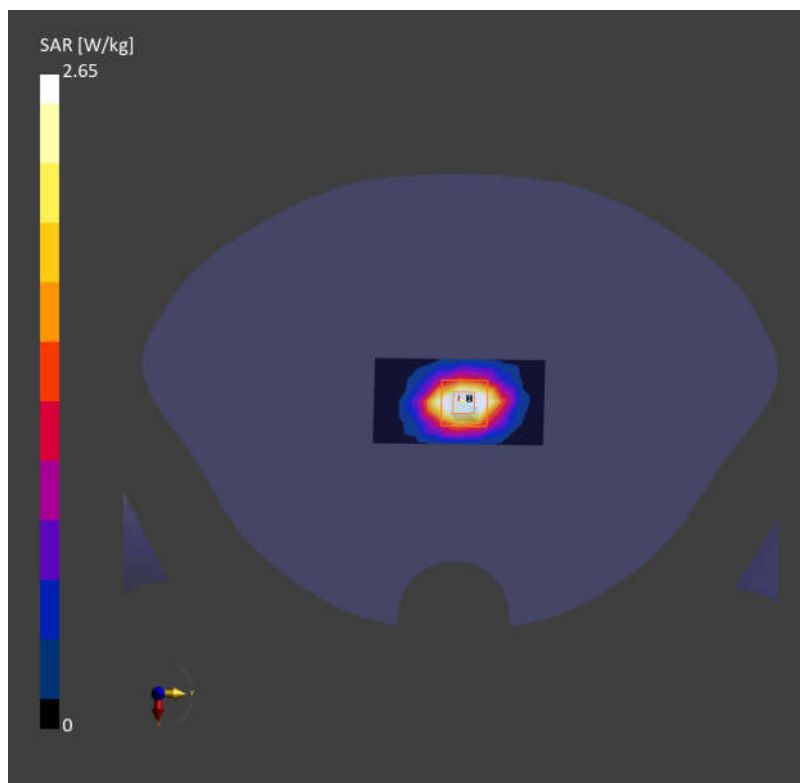

Date: 2026-01-27

System Check_Head_2600MHz**DUT: D2600V2 - SN1112**

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600_260127 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.49, 7.28, 7.42); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.77 W/kg; SAR (10g) = 1.23 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 2.74 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.6 %

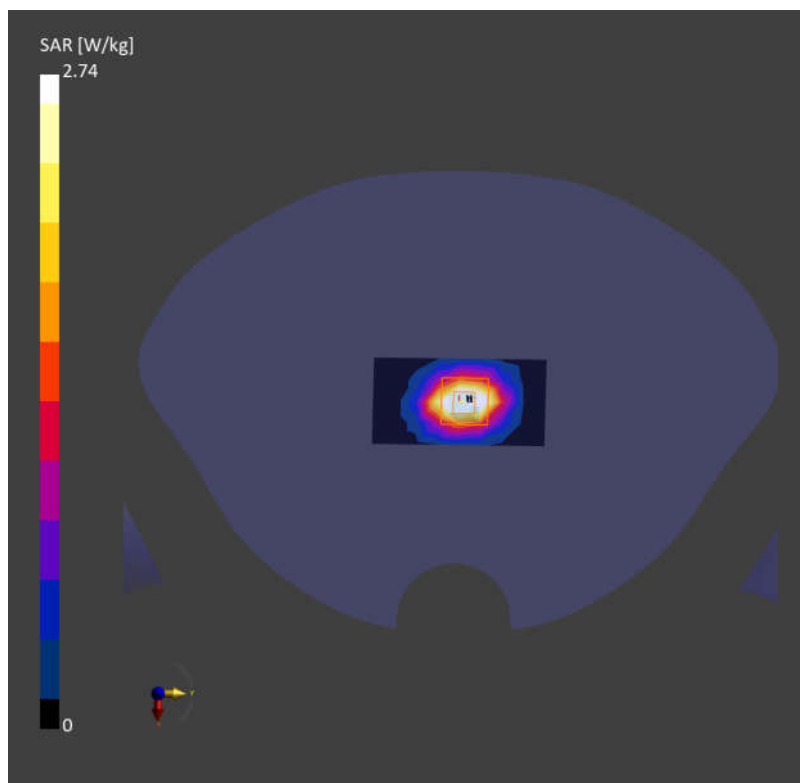

Date: 2026-01-31

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5250_260131 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.74$ S/m; $\epsilon_r = 36.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.9, 5.74, 5.85); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.64 W/kg; SAR (10g) = 1.09 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 4.03 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.4 %

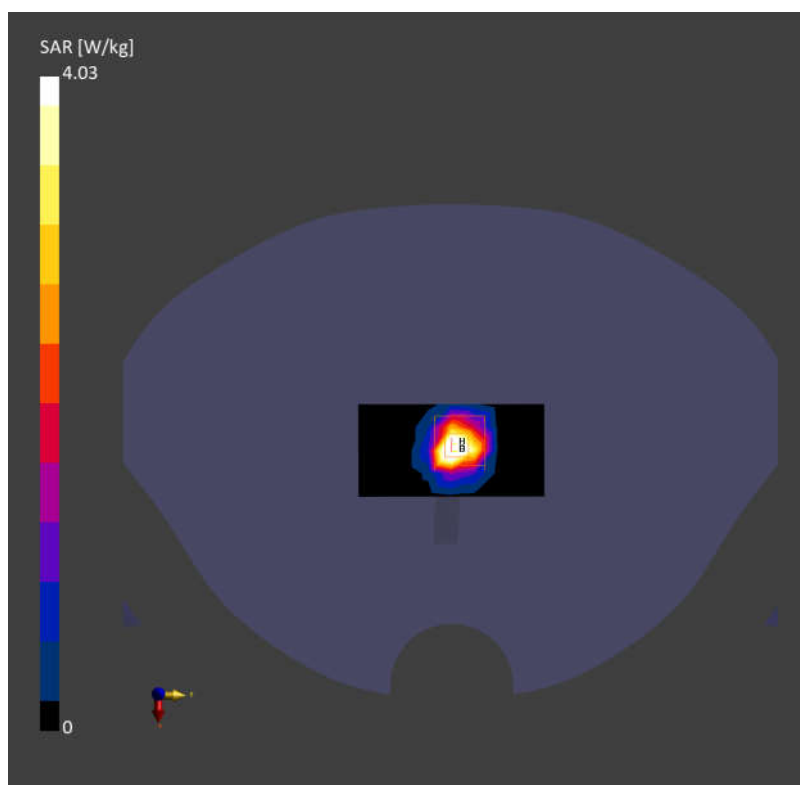

Date: 2026-02-02

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5600_260202 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.07$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.45, 5.3, 5.4); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.60 W/kg; SAR (10g) = 1.11 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 4.23 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 58.8 %

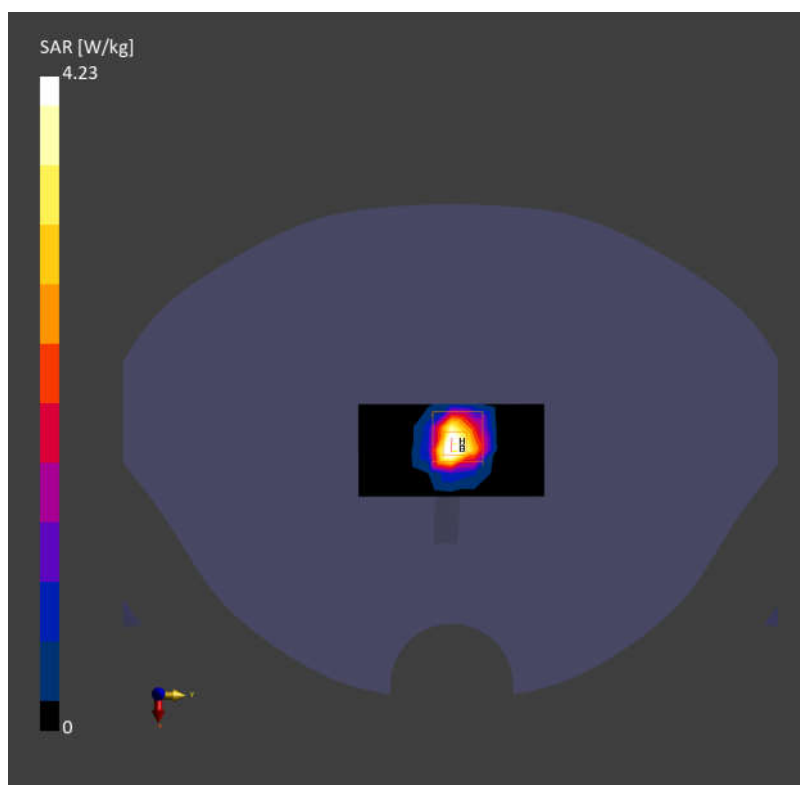

Date: 2026-02-04

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1

Medium: HSL_5800_260204 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.22$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.31, 5.17, 5.27); Calibrated: 2025-10-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 1753; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.02 W/kg;

Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.92 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 57.0 %

