

System Check_Head_13MHz**DUT: CLA-13 - SN1011**

Communication System: CW; Frequency: 13.000 MHz

Medium: HSL_4-250_260707 Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.757$ S/m; $\epsilon_r = 54.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(17.55, 17.18, 17.51); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=30.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.543 W/kg; SAR (10g) = 0.439 W/kg;

TSL Correction: Positive only

Pin=30.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.04 dB

SAR (1g) = 0.515 W/kg; SAR (8g) = 0.338 W/kg; SAR (10g) = 0.319 W/kg

Smallest distance from peaks to all points 3 dB below = 15.8 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

TSL Correction: Positive only

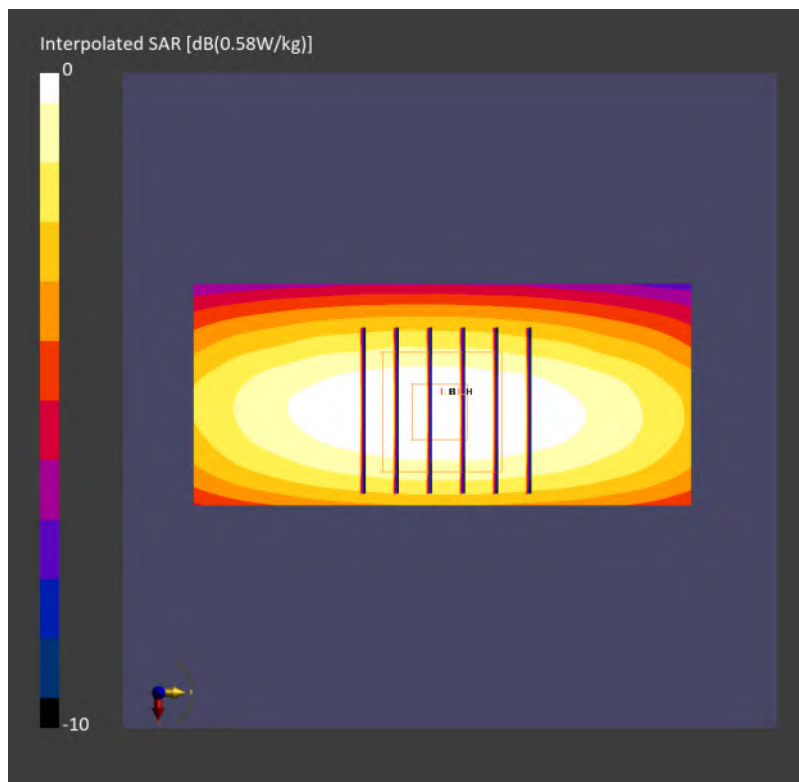

System Check_Head_750MHz**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.876$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(8.9, 9.61, 8.78); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.11 W/kg; SAR (10g) = 1.41 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.11 W/kg; SAR (8g) = 1.48 W/kg; SAR (10g) = 1.41 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

TSL Correction: Positive only

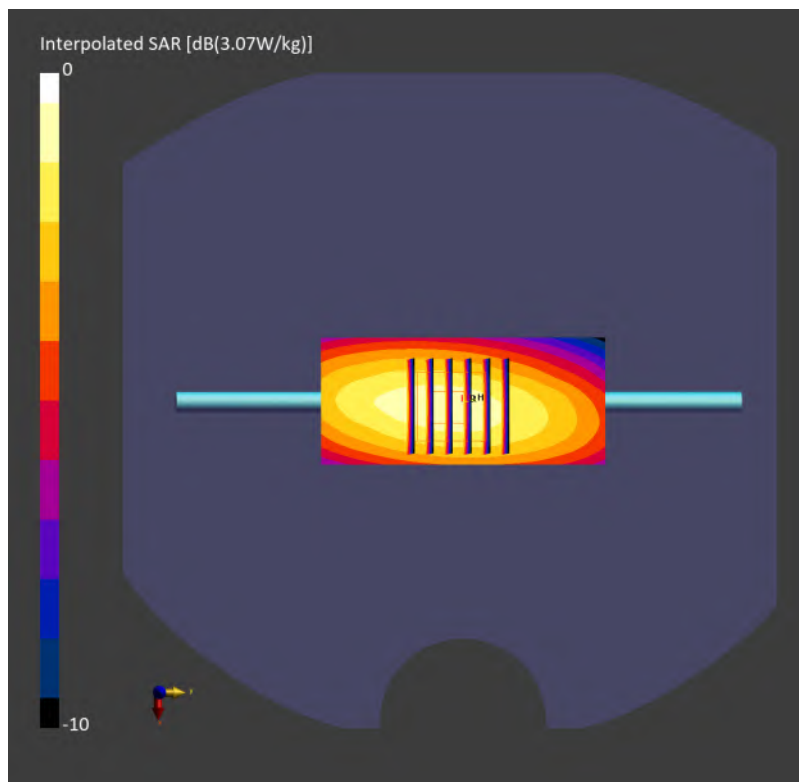

System Check_Head_750MHz**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.876$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(9.08, 8.91, 9.18); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.96 W/kg; SAR (10g) = 1.30 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.95 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.7 %

TSL Correction: Positive only

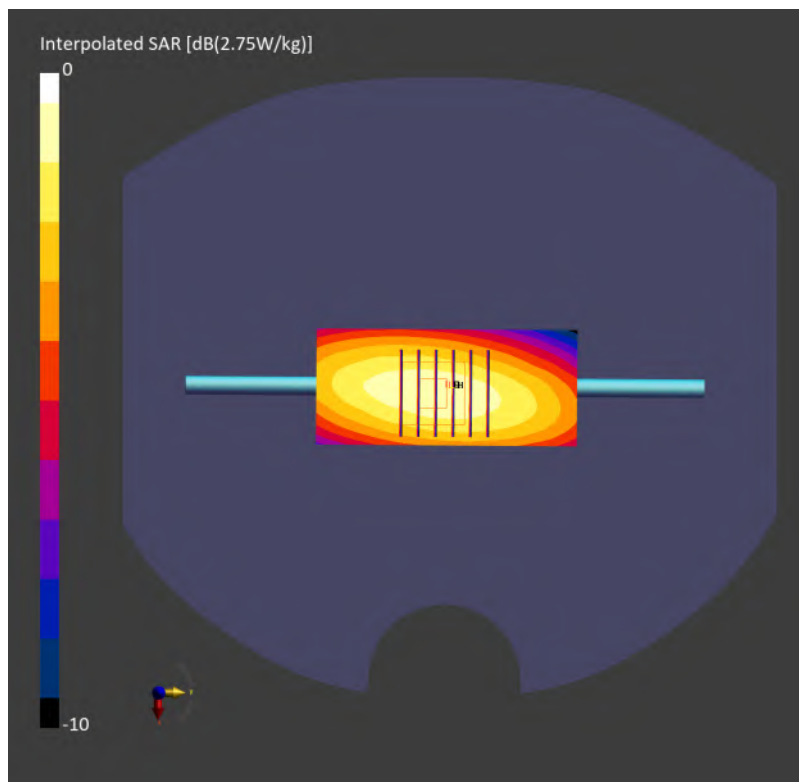

System Check_Head_750MHz**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260622 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(9.08, 8.91, 9.18); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.19 W/kg; SAR (10g) = 1.47 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.15 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.41 W/kg

Smallest distance from peaks to all points 3 dB below = 25.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

TSL Correction: Positive only

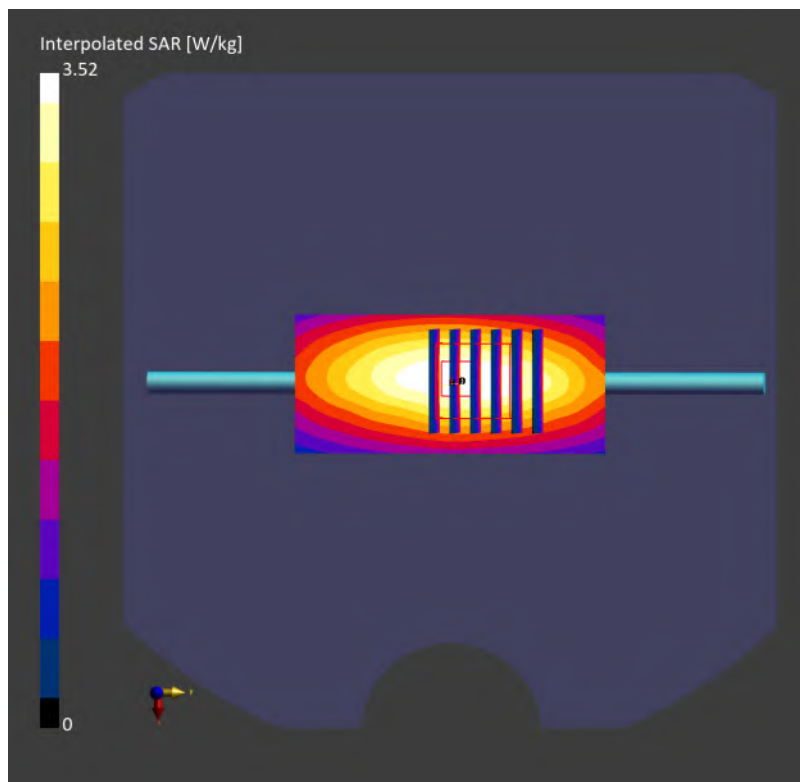

System Check_Head_750MHz**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260623 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.875$ S/m; $\epsilon_r = 45.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(8.9, 9.61, 8.78); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.17 W/kg; SAR (10g) = 1.44 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.15 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.41 W/kg

Smallest distance from peaks to all points 3 dB below = 17.9 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

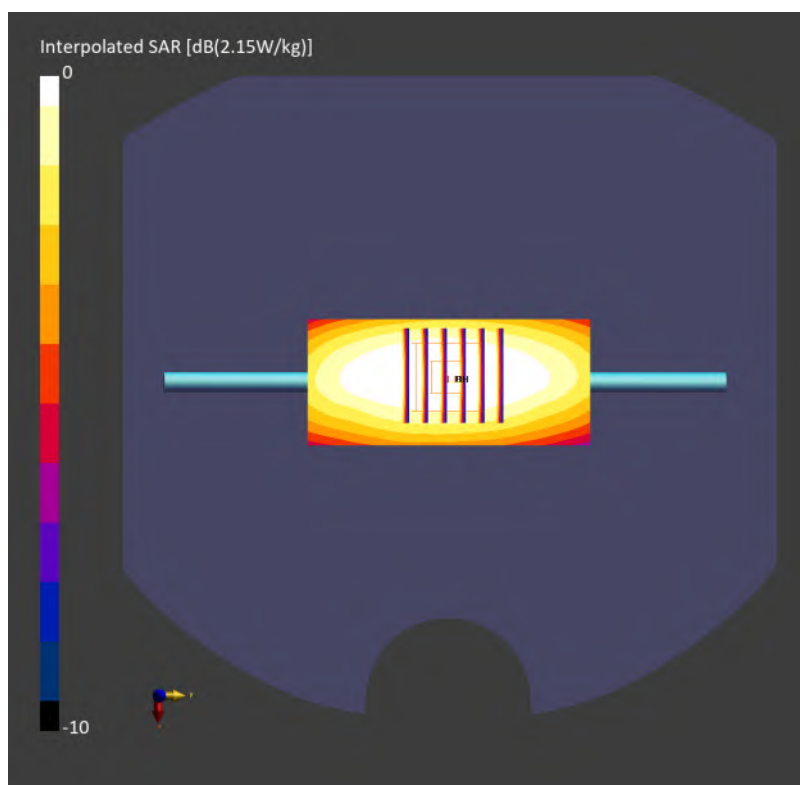

System Check_Head_750MHz**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260623 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.876$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(9.08, 8.91, 9.18); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.16 W/kg; SAR (10g) = 1.43 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 2.13 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.43 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.8 %

TSL Correction: Positive only

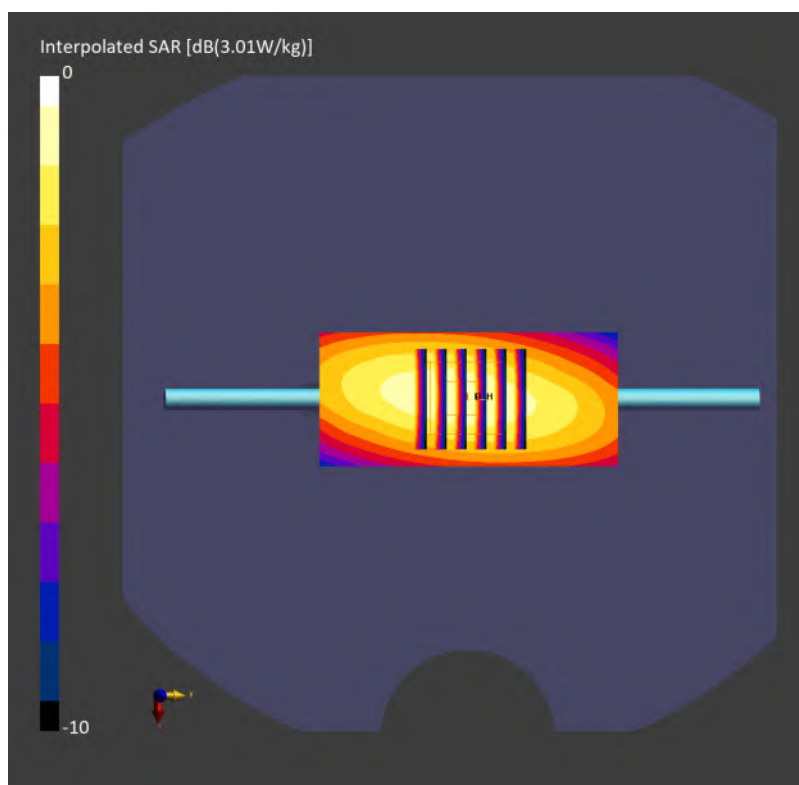

System Check_Head_750MHz**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260627 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.895$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(8.9, 9.61, 8.78); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.09 W/kg; SAR (10g) = 1.40 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.10 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.39 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

TSL Correction: Positive only

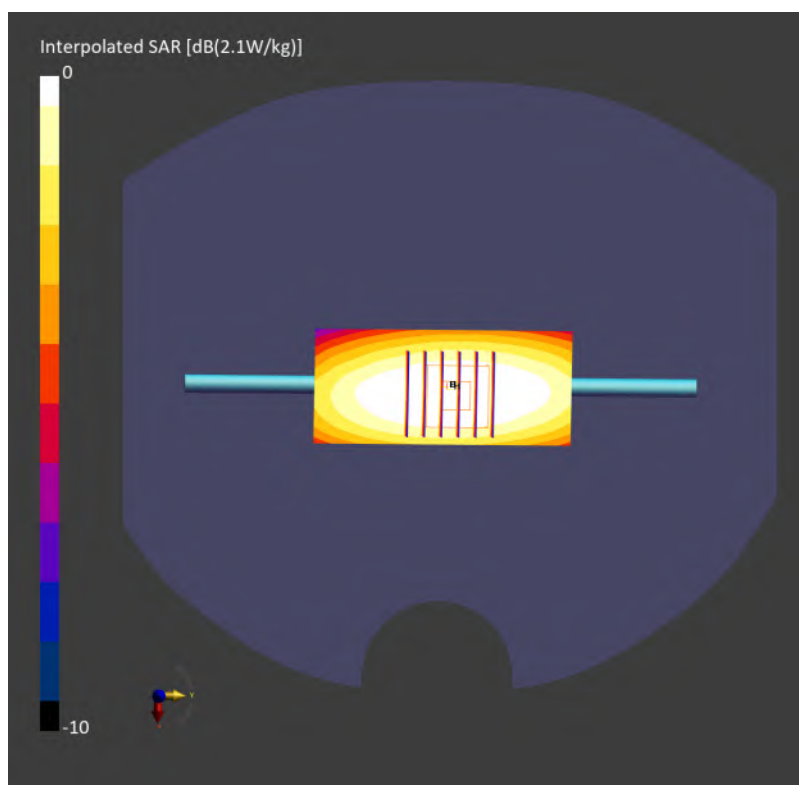

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(8.84, 8.67, 8.94); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.60 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.41 W/kg; SAR (8g) = 1.69 W/kg; SAR (10g) = 1.60 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 89.8 %

TSL Correction: Positive only

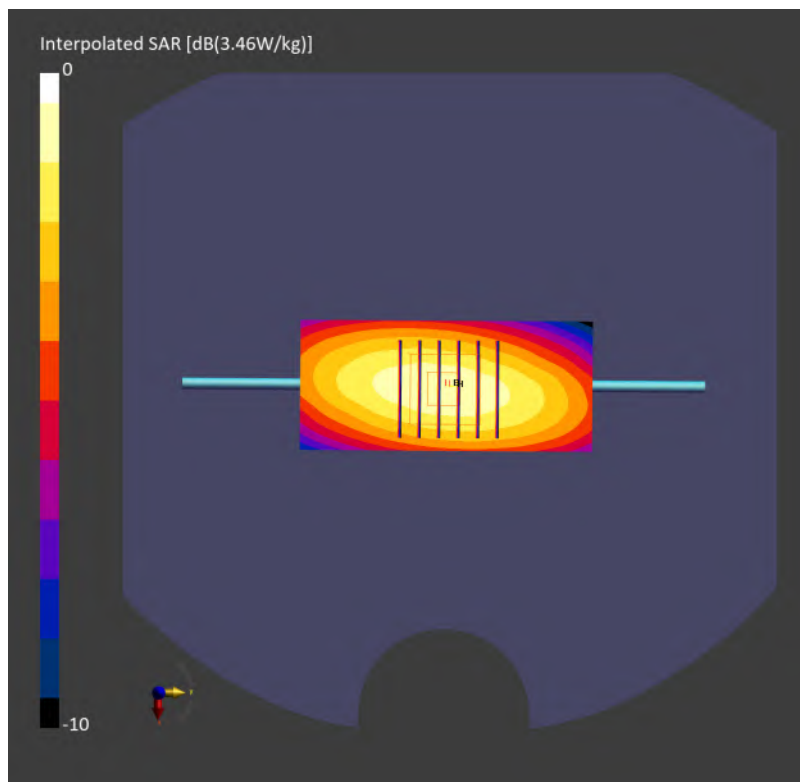

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.898$ S/m; $\epsilon_r = 44.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(8.74, 9.44, 8.62); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.57 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.37 W/kg; SAR (8g) = 1.64 W/kg; SAR (10g) = 1.55 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

TSL Correction: Positive only

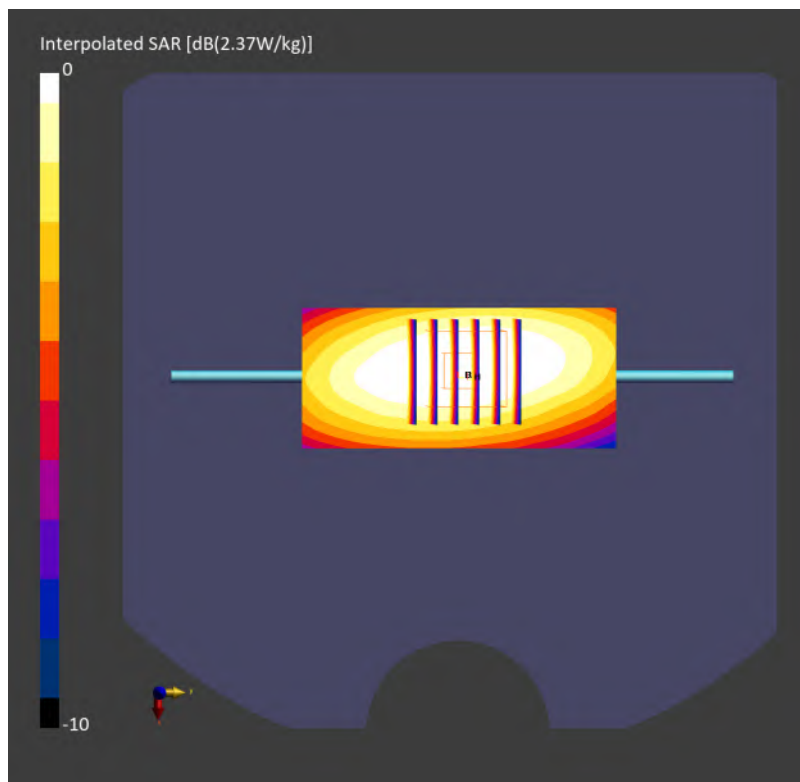

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260622 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.937$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(8.84, 8.67, 8.94); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.75 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.55 W/kg; SAR (8g) = 1.75 W/kg; SAR (10g) = 1.65 W/kg

Smallest distance from peaks to all points 3 dB below = 13.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: Positive only

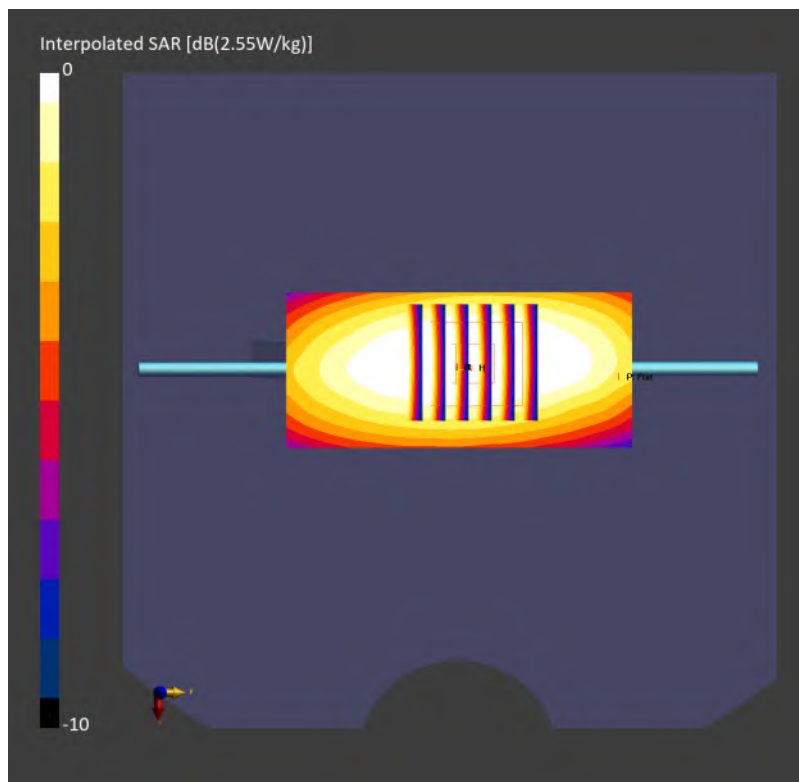

System Check_Head_850MHz_20260623**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260623 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.904$ S/m; $\epsilon_r = 45.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(8.74, 9.44, 8.62); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.60 W/kg; SAR (10g) = 1.70 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.60 W/kg; SAR (8g) = 1.79 W/kg; SAR (10g) = 1.70 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

TSL Correction: Positive only

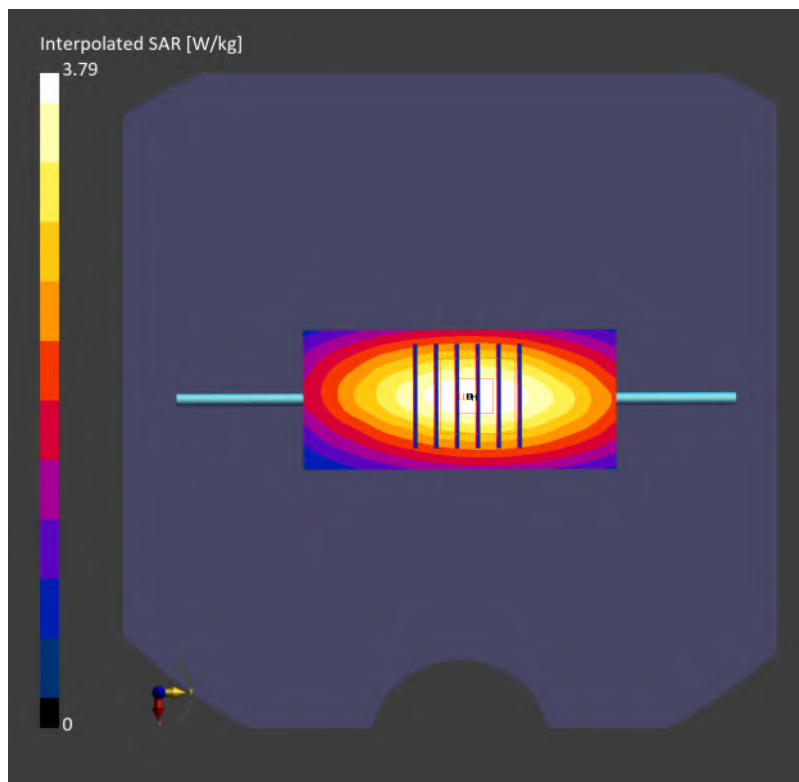

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260623 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(8.84, 8.67, 8.94); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.66 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 2.51 W/kg; SAR (8g) = 1.76 W/kg; SAR (10g) = 1.67 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 89.9 %

TSL Correction: Positive only

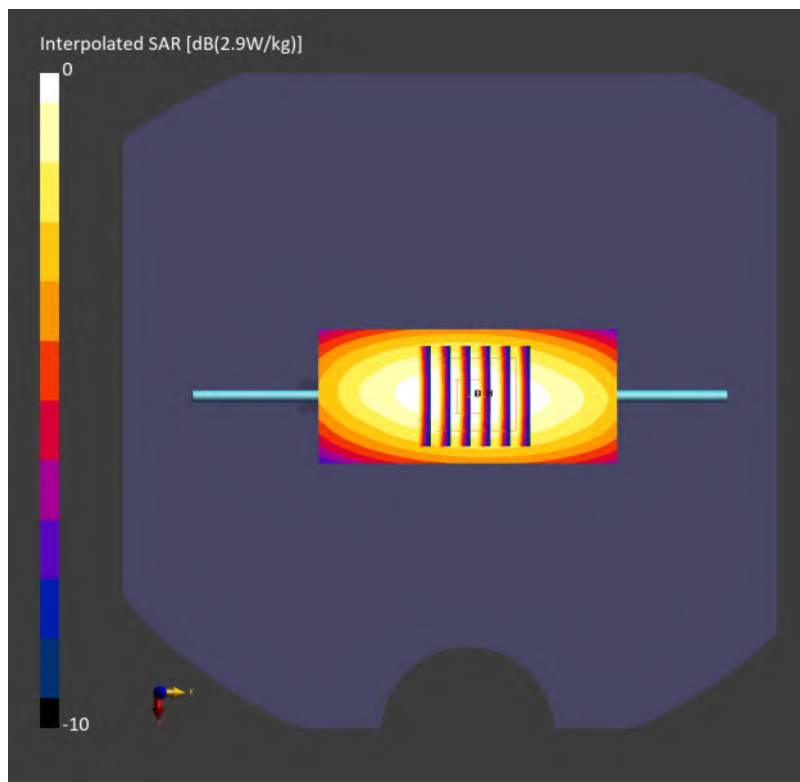

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260627 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.926$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(8.74, 9.44, 8.62); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.41 W/kg; SAR (10g) = 1.60 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.42 W/kg; SAR (8g) = 1.68 W/kg; SAR (10g) = 1.60 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

TSL Correction: Positive only

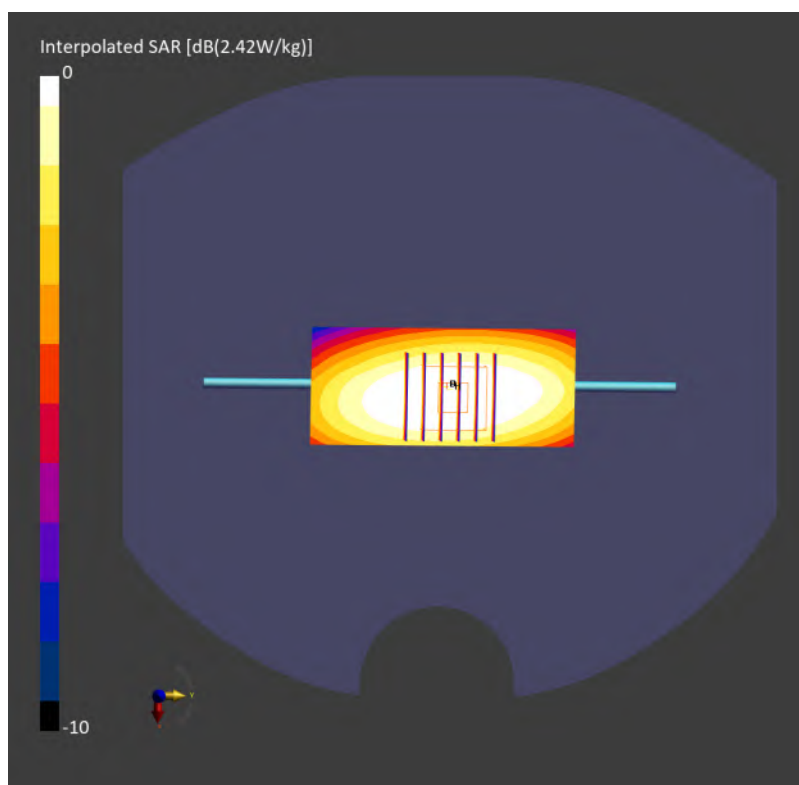

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.32$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.44, 7.3, 7.52); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.77 W/kg; SAR (10g) = 0.932 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.74 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.929 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.6 %

TSL Correction: Positive only

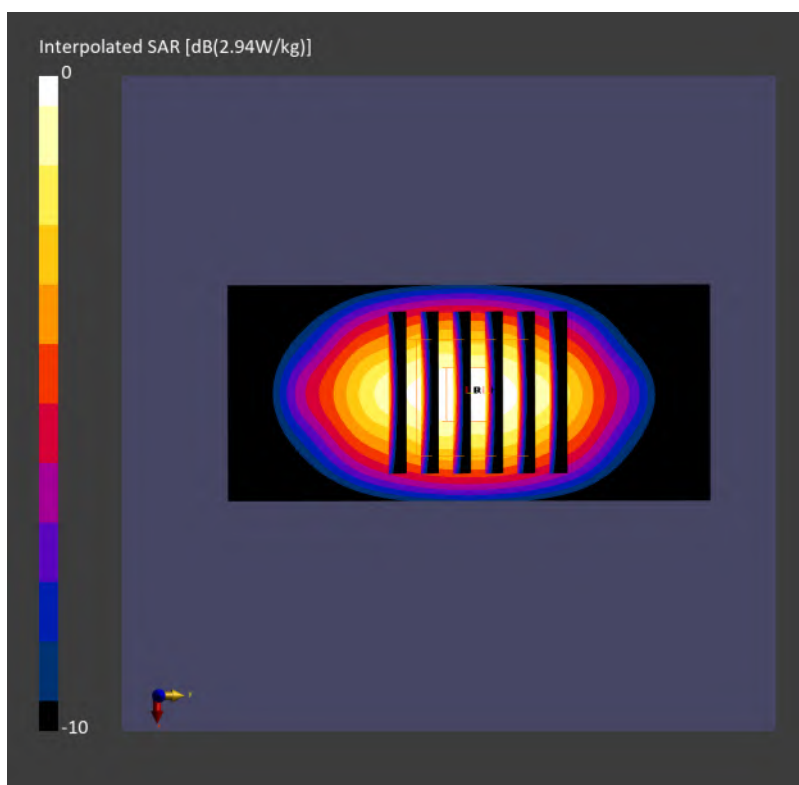

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.32$ S/m; $\epsilon_r = 43.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.42, 8.01, 7.32); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.71 W/kg; SAR (10g) = 0.899 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.71 W/kg; SAR (8g) = 0.979 W/kg; SAR (10g) = 0.905 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 82.4 %

TSL Correction: Positive only

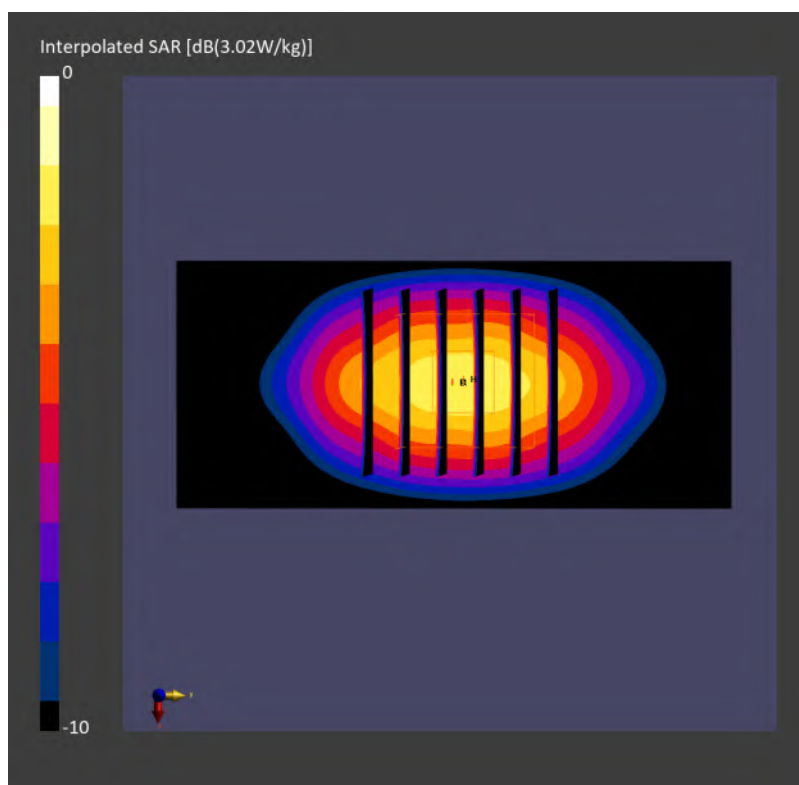

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260623 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 43.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.42, 8.01, 7.32); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.82 W/kg; SAR (10g) = 4.65 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 8.76 W/kg; SAR (8g) = 5.01 W/kg; SAR (10g) = 4.63 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

TSL Correction: Positive only

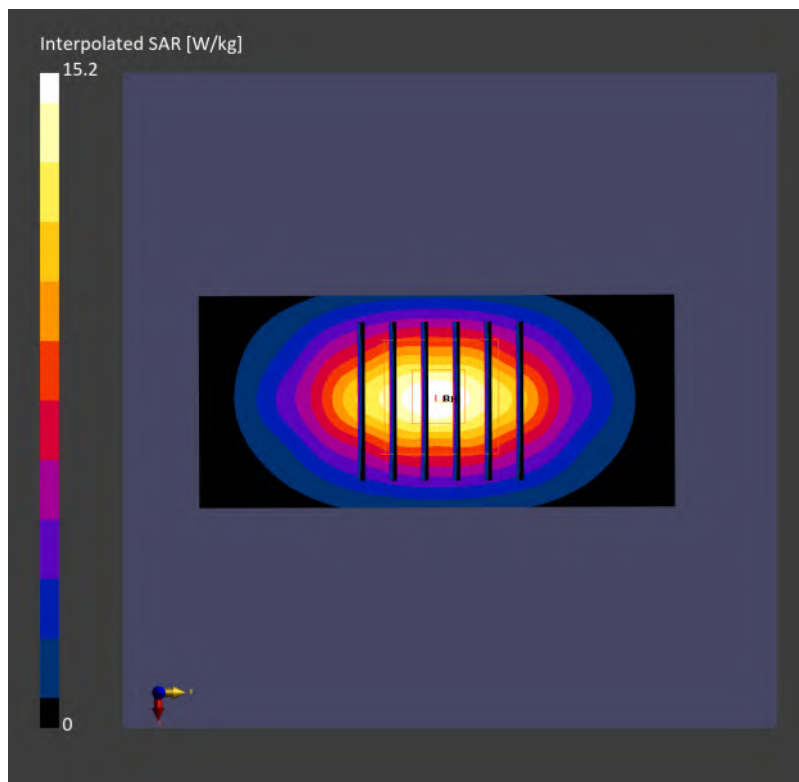

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260624 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.44, 7.3, 7.52); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.936 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.75 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.938 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

TSL Correction: Positive only

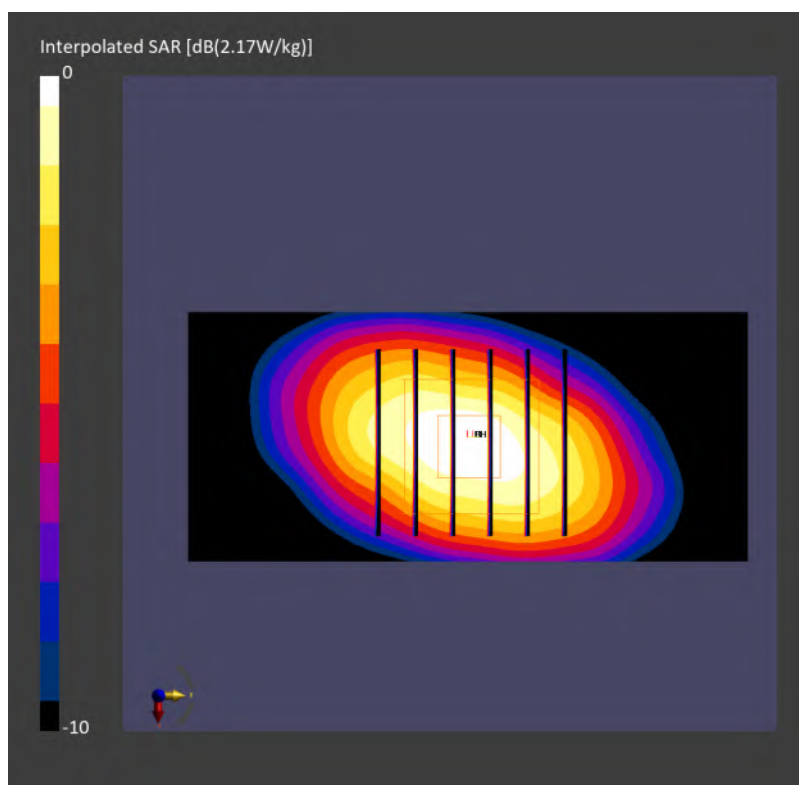

System Check_Head 1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260626 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.32$ S/m; $\epsilon_r = 42.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.89, 8.41, 7.94); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.71 W/kg; SAR (10g) = 0.915 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 1.74 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.931 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.4 %

TSL Correction: Positive only

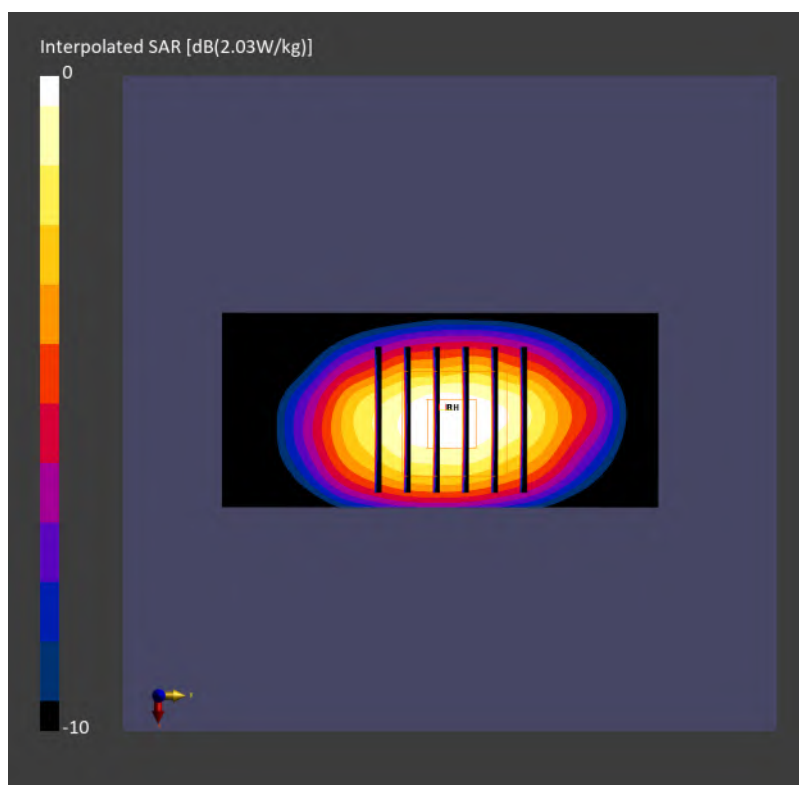

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260627 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.44, 7.3, 7.52); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.949 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.950 W/kg

Smallest distance from peaks to all points 3 dB below = 10.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

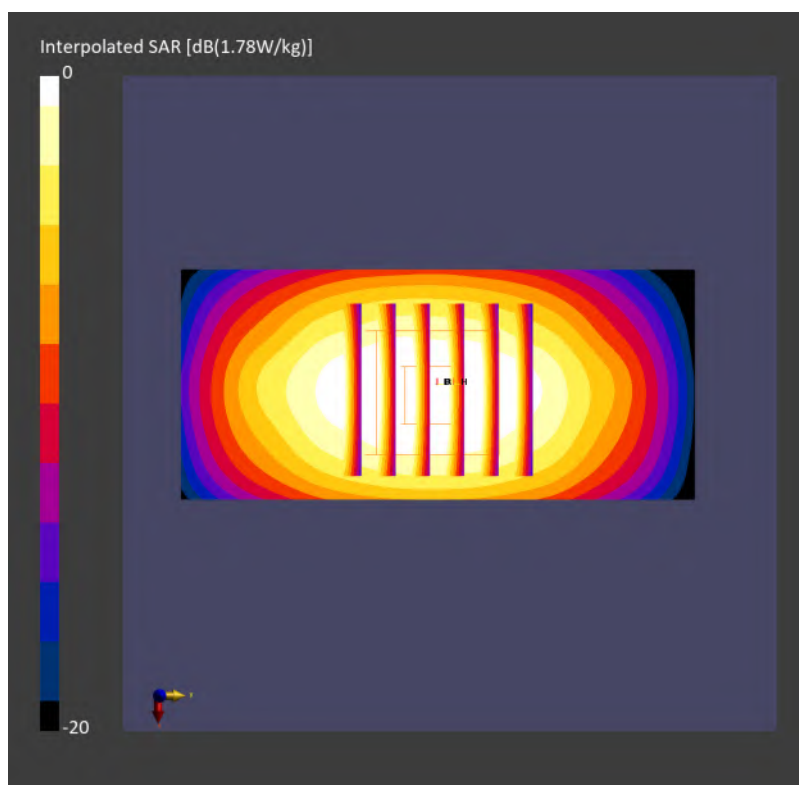

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260628 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.42, 8.01, 7.32); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.34 W/kg; SAR (10g) = 5.07 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 9.42 W/kg; SAR (8g) = 5.45 W/kg; SAR (10g) = 5.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

TSL Correction: Positive only

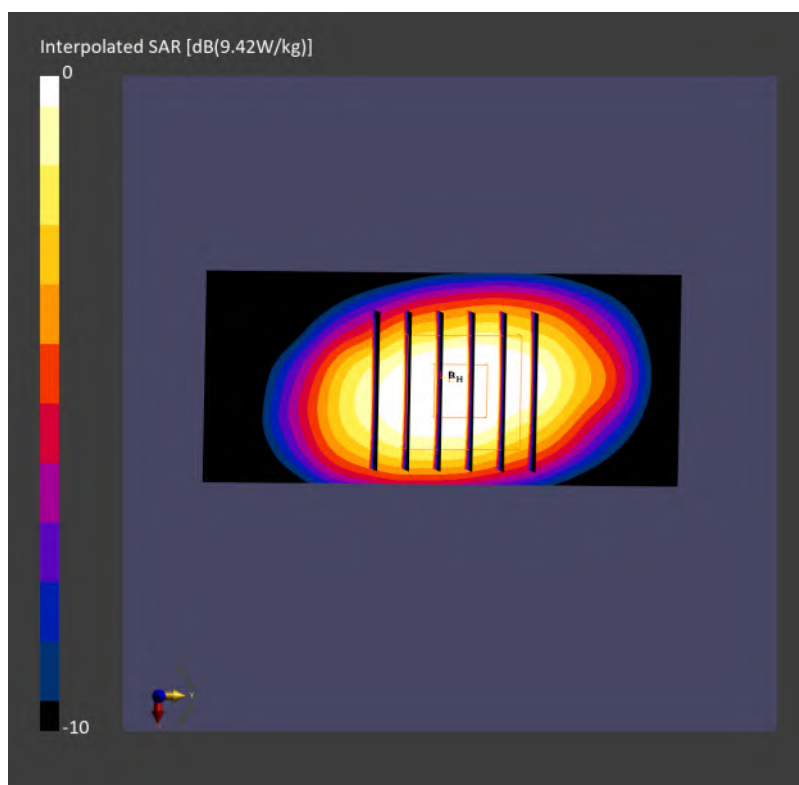

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260701 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.44, 7.3, 7.52); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.79 W/kg; SAR (10g) = 0.958 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.77 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.947 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

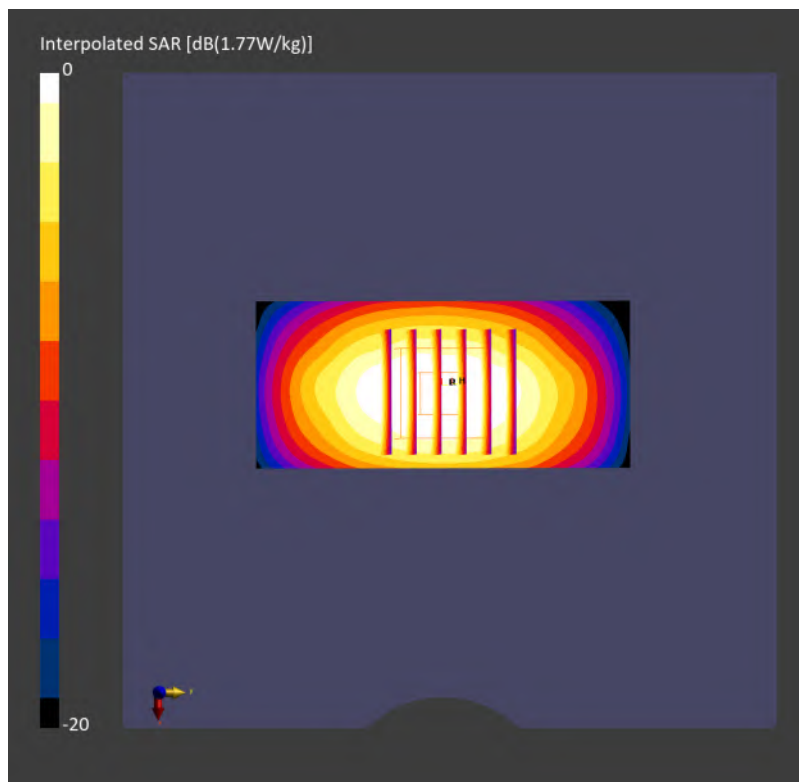

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260703 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.44, 7.3, 7.52); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.77 W/kg; SAR (10g) = 0.945 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.76 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.945 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

TSL Correction: Positive only

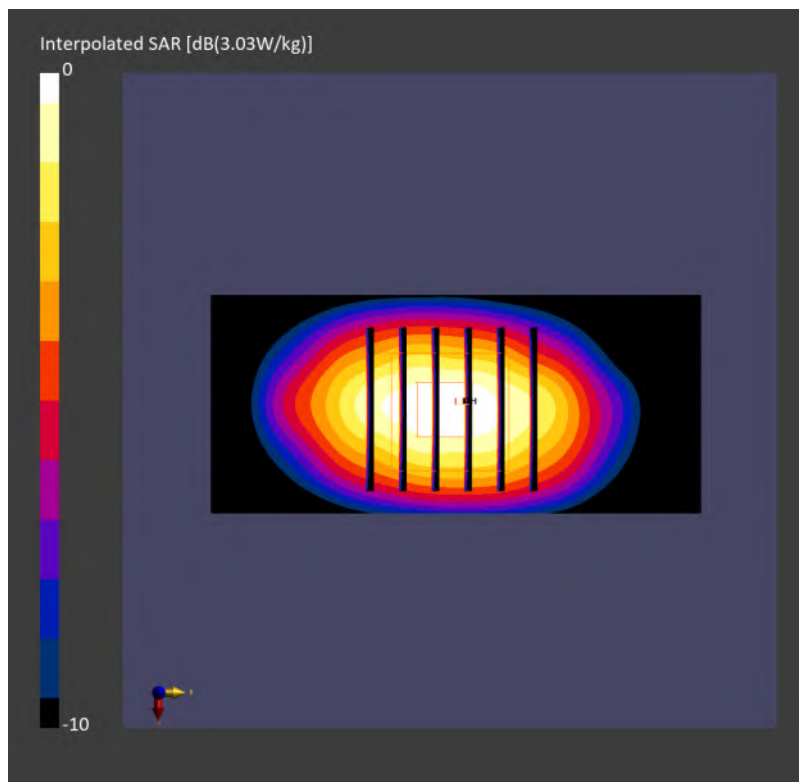

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.25, 7.12, 7.34); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.94 W/kg; SAR (10g) = 0.999 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.90 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.998 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

TSL Correction: Positive only

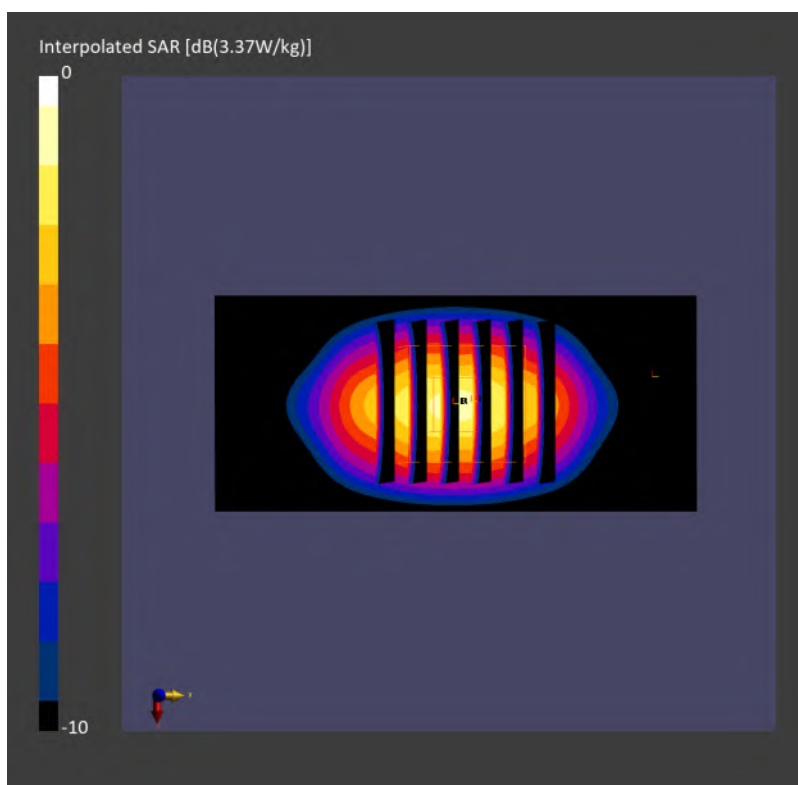

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.41$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.02, 7.58, 6.92); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.92 W/kg; SAR (10g) = 0.987 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.90 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.990 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

TSL Correction: Positive only

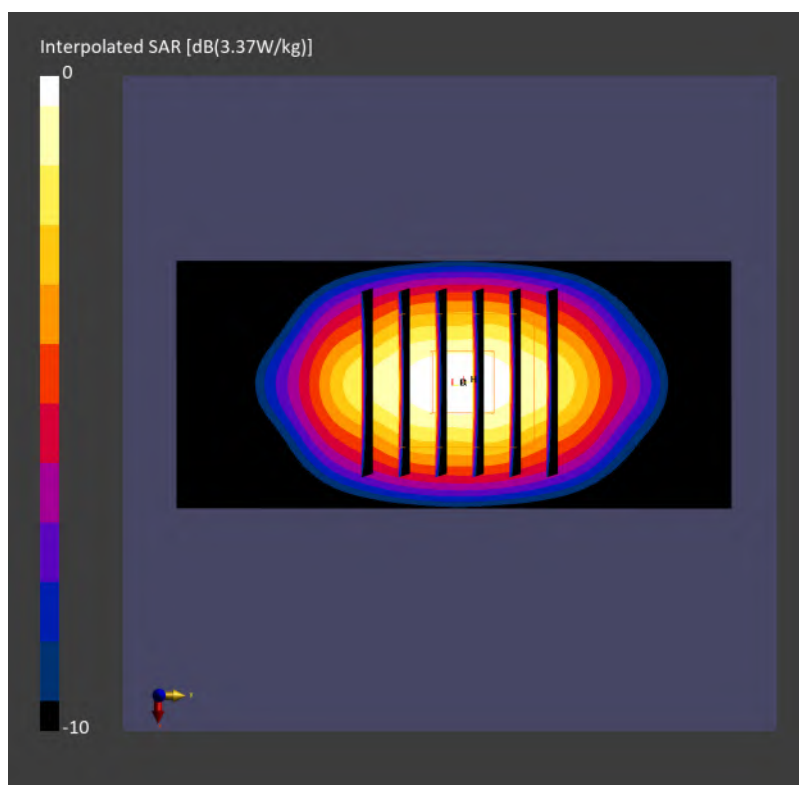

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260623 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 43.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.02, 7.58, 6.92); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.3 W/kg; SAR (10g) = 5.27 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.05 dB

SAR (1g) = 10.2 W/kg; SAR (8g) = 5.78 W/kg; SAR (10g) = 5.31 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 81.3 %

TSL Correction: Positive only

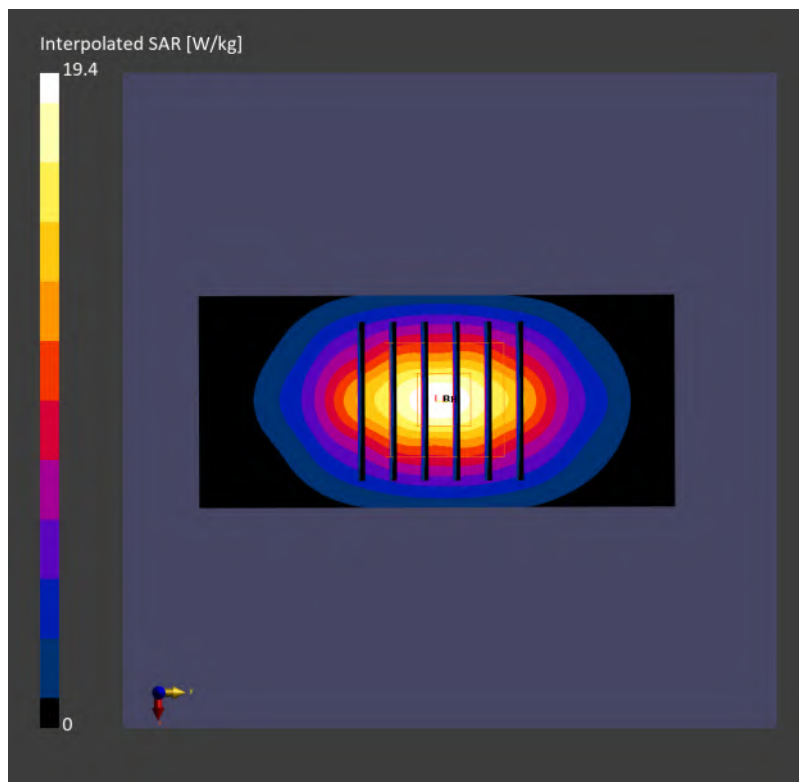

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260624 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.25, 7.12, 7.34); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.92 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

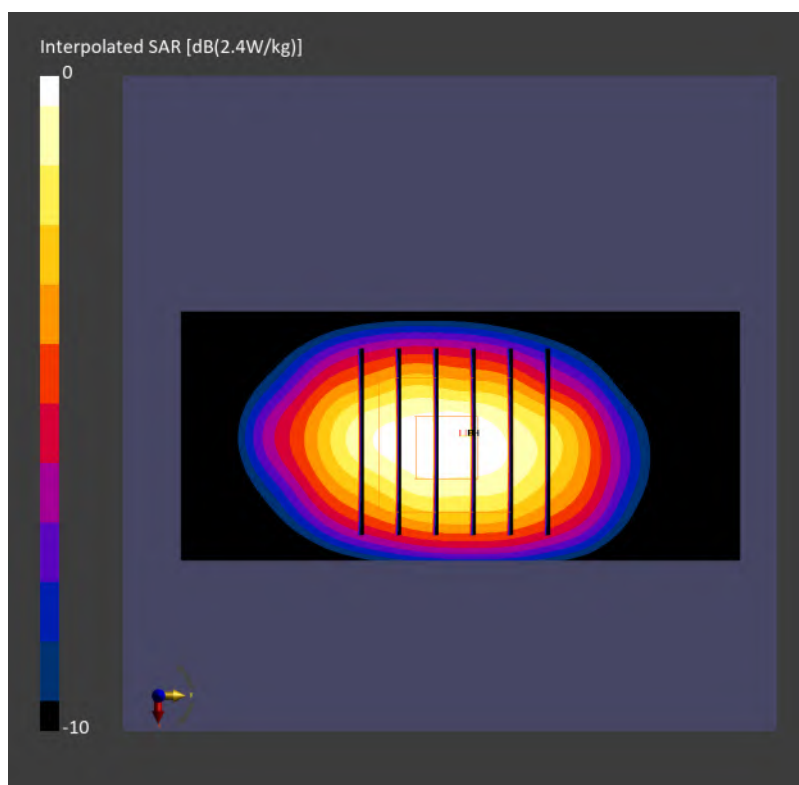

System Check_Head 1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260627 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 43.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.64, 8.14, 7.69); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.84 W/kg; SAR (10g) = 0.980 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.1 %

TSL Correction: Positive only

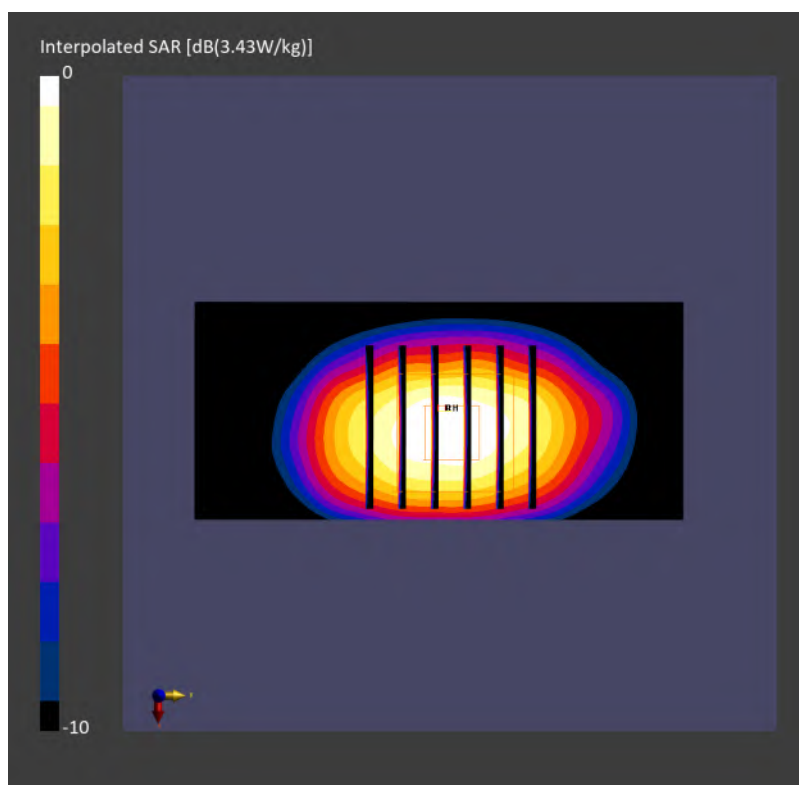

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260627 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.25, 7.12, 7.34); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.90 W/kg; SAR (10g) = 1.00 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

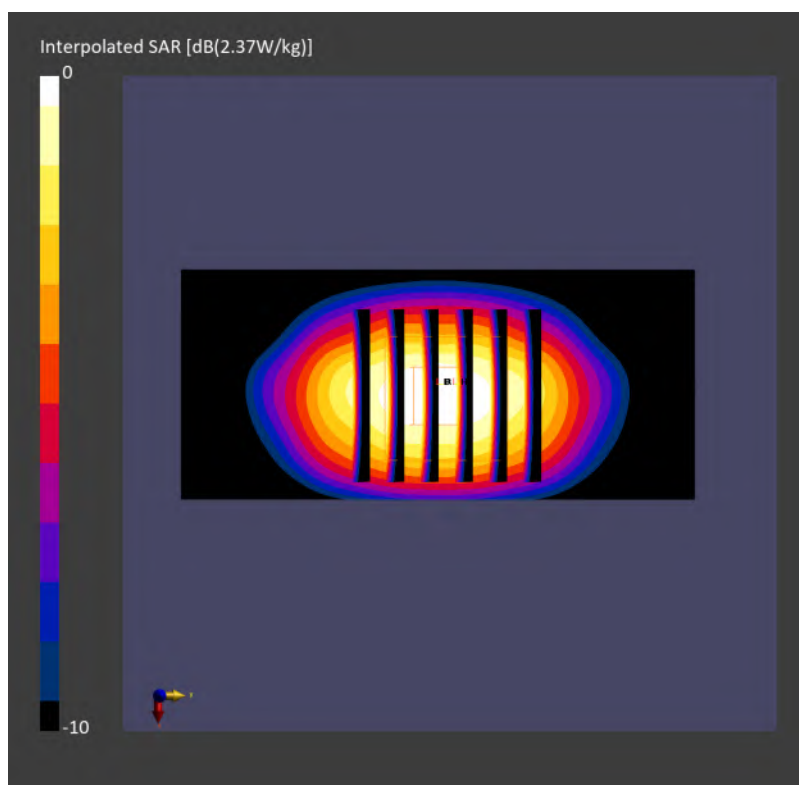

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260628 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.02, 7.58, 6.92); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.80 W/kg; SAR (10g) = 5.10 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 9.77 W/kg; SAR (8g) = 5.53 W/kg; SAR (10g) = 5.09 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

TSL Correction: Positive only

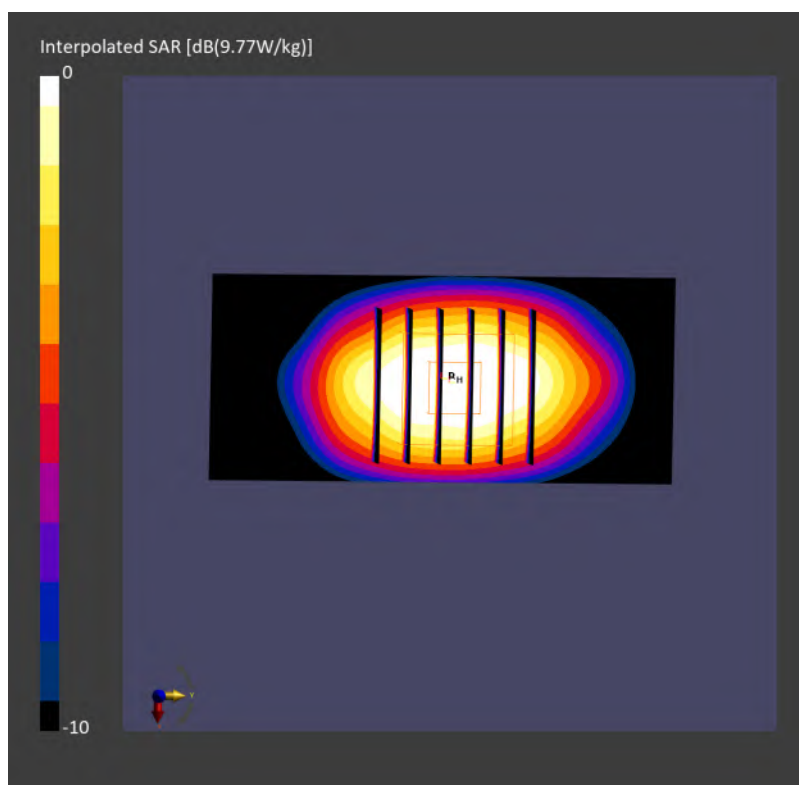

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260701 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.25, 7.12, 7.34); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.90 W/kg; SAR (10g) = 0.986 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.87 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.979 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

TSL Correction: Positive only

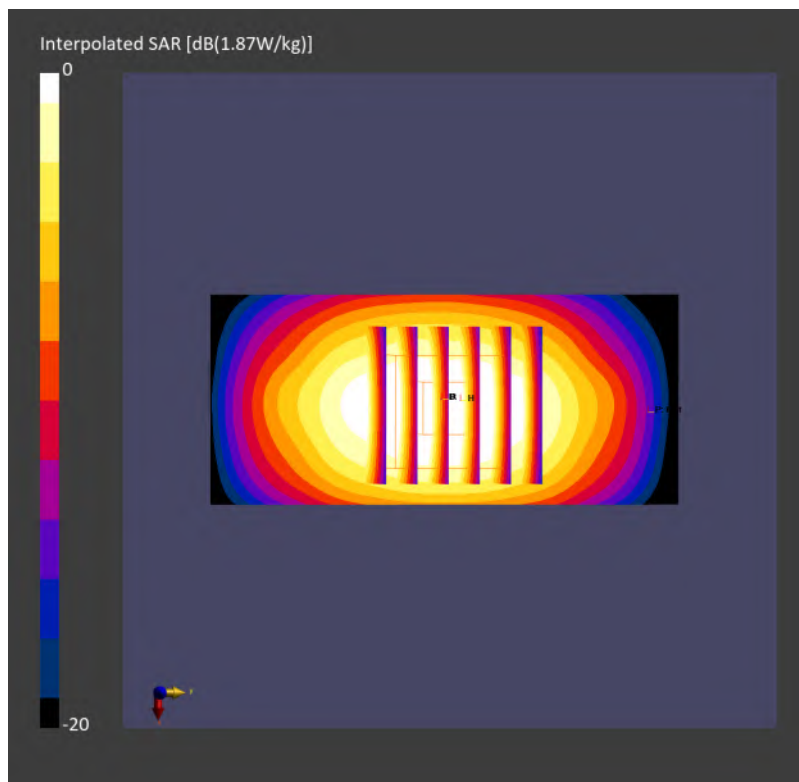

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260703 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.25, 7.12, 7.34); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.94 W/kg; SAR (10g) = 1.02 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.93 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

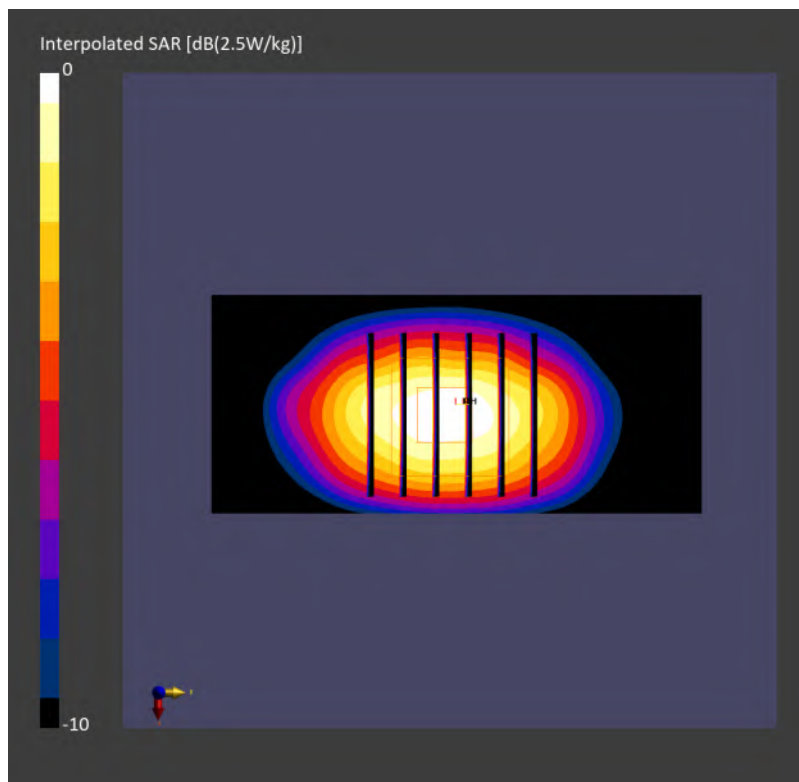

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260701 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(6.56, 7.09, 6.47); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.54 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.50 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.1 %

TSL Correction: Positive only

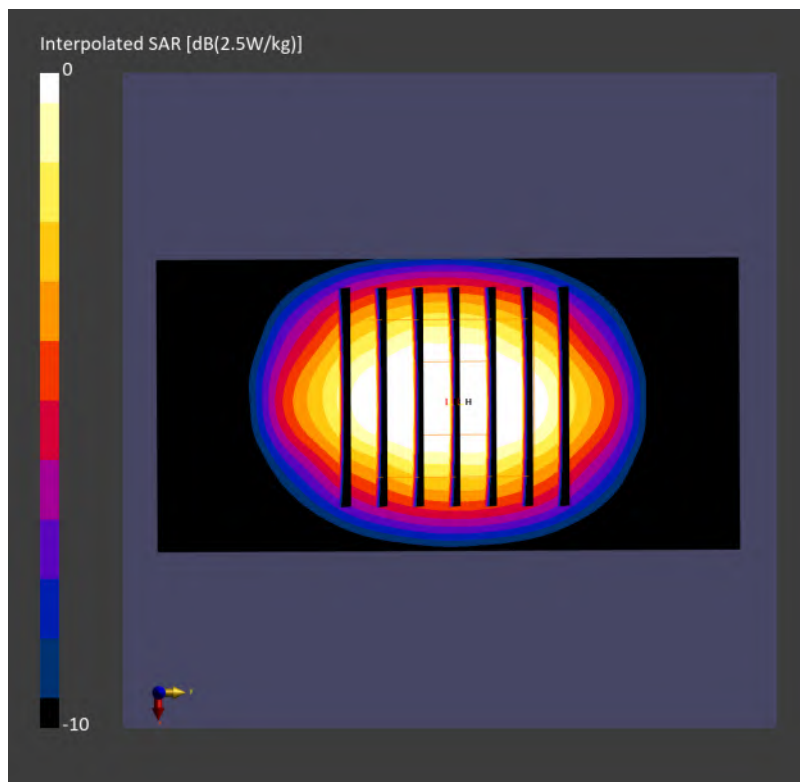

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260702 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.79$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.79, 6.67, 6.87); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.50 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.48 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

TSL Correction: Positive only

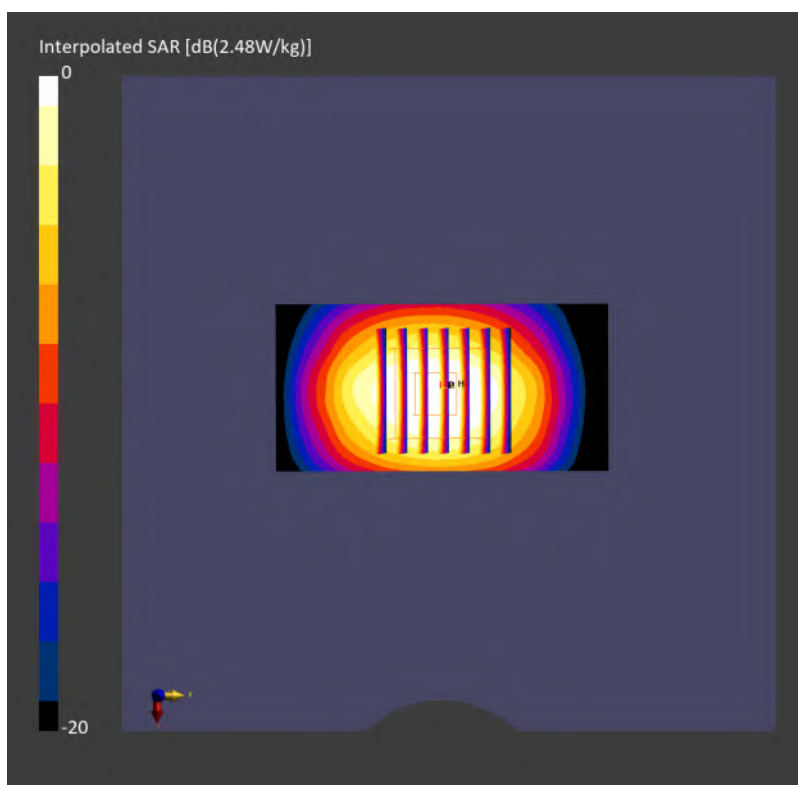

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260713 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(6.56, 7.09, 6.47); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.45 W/kg; SAR (10g) = 1.13 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.46 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.6 %

TSL Correction: Positive only

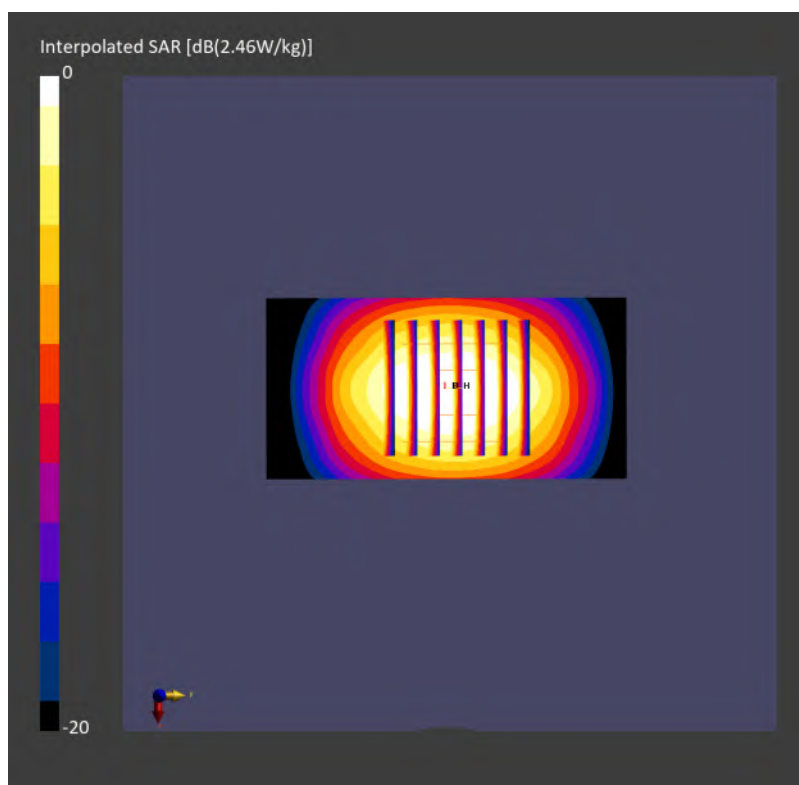

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.90$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.66, 6.54, 6.74); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=16.7dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.50 W/kg; SAR (10g) = 1.11 W/kg;

TSL Correction: Positive only

Pin=16.7dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.49 W/kg; SAR (8g) = 1.24 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.9 %

TSL Correction: Positive only

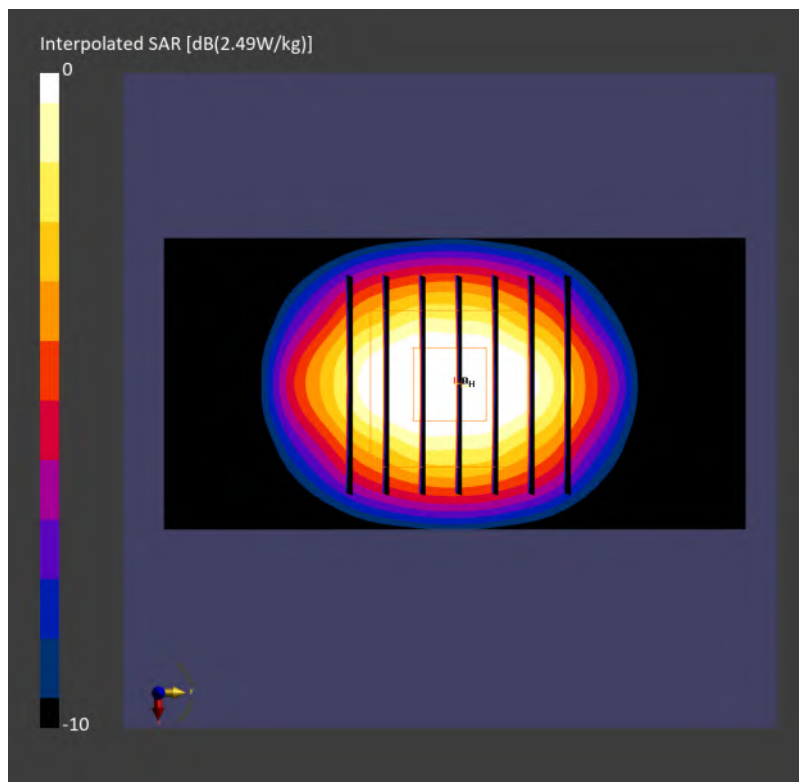

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260618 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(6.73, 7.27, 6.64); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.93 W/kg; SAR (10g) = 1.30 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.17 dB

SAR (1g) = 3.05 W/kg; SAR (8g) = 1.45 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

TSL Correction: Positive only

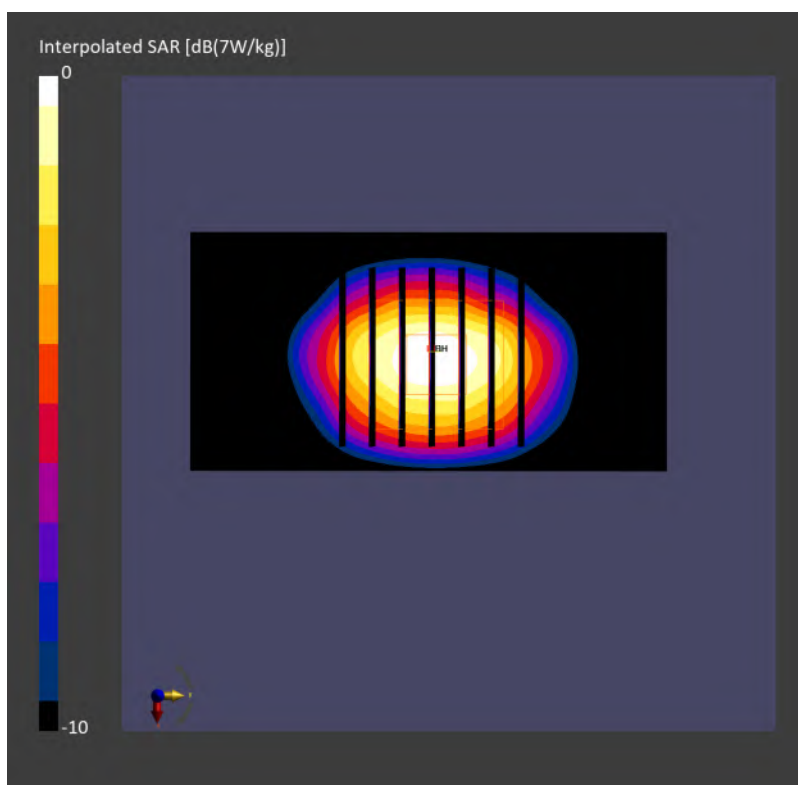

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260622 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.66, 6.54, 6.74); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.5 W/kg; SAR (10g) = 6.26 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 13.8 W/kg; SAR (8g) = 6.83 W/kg; SAR (10g) = 6.16 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

TSL Correction: Positive only

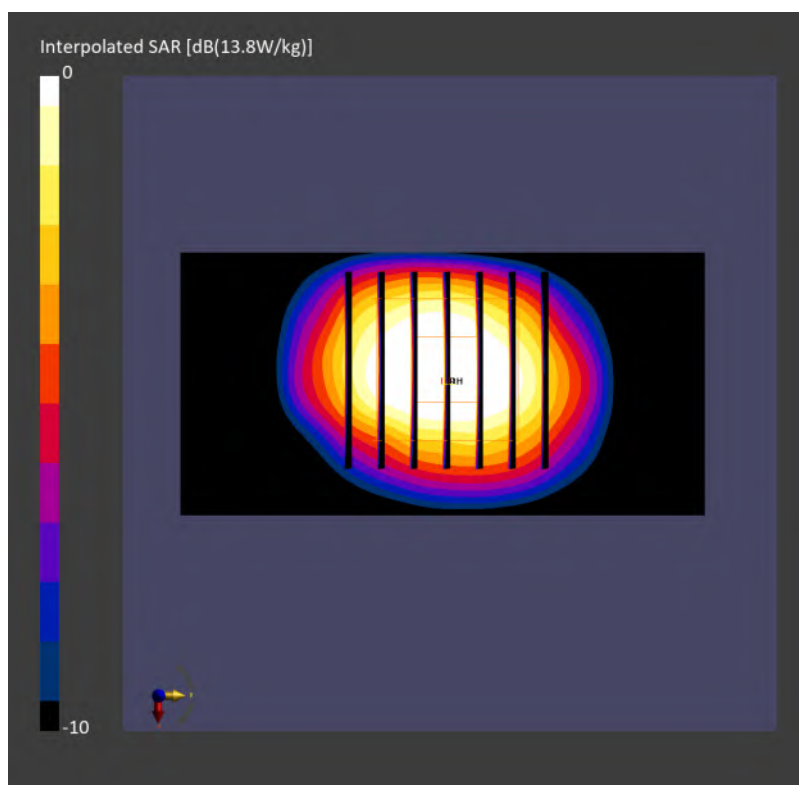

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260623 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.90$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.66, 6.54, 6.74); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.2 W/kg; SAR (10g) = 5.92 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 13.3 W/kg; SAR (8g) = 6.65 W/kg; SAR (10g) = 6.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 81.1 %

TSL Correction: Positive only

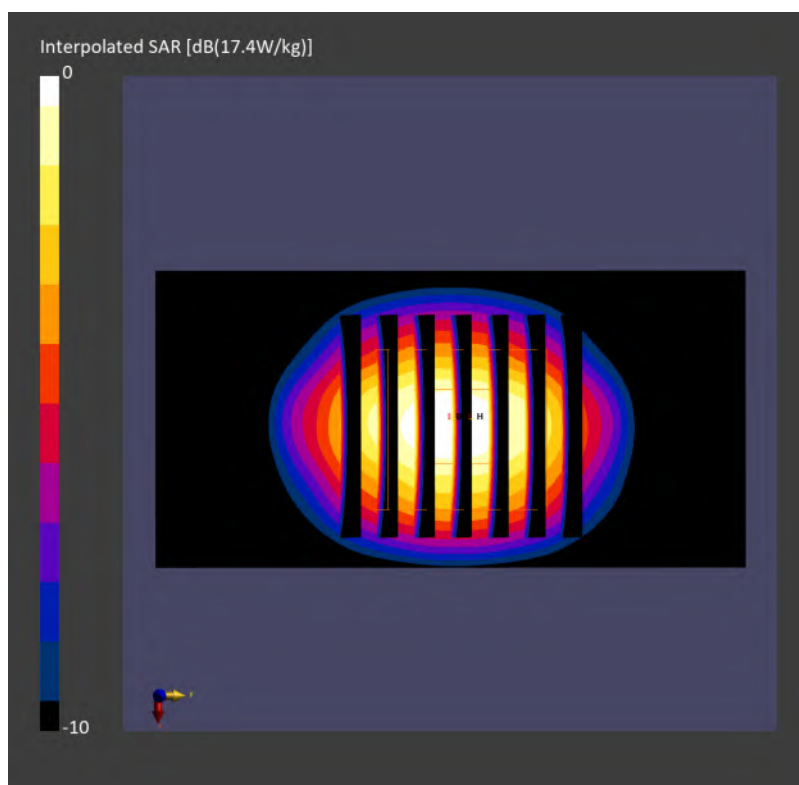

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260624 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.90$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(6.73, 7.27, 6.64); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=16.7dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.57 W/kg; SAR (10g) = 1.12 W/kg;

TSL Correction: Positive only

Pin=16.7dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.07 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.22 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

TSL Correction: Positive only

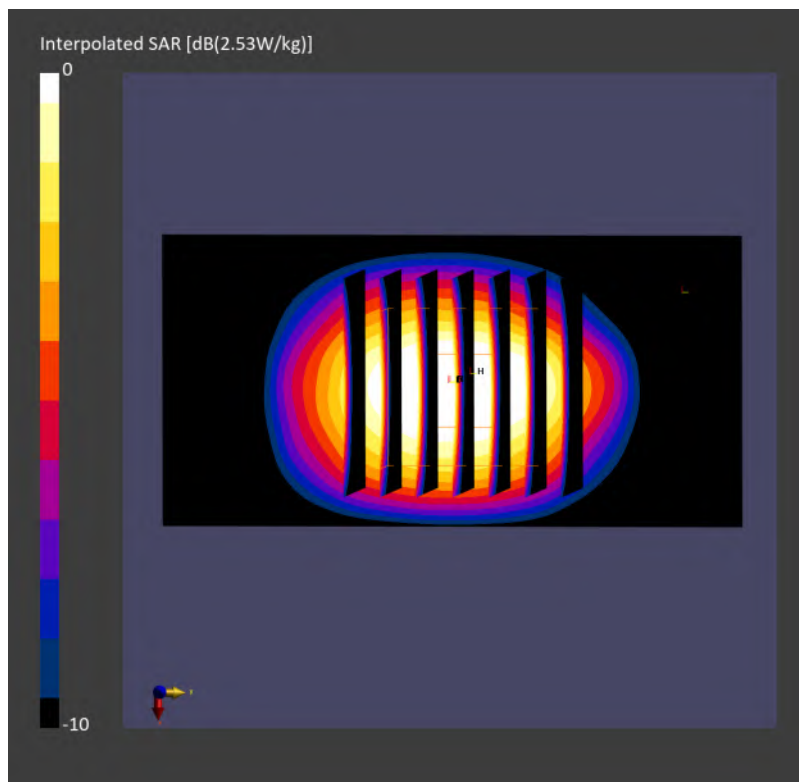

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260626 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.66, 6.54, 6.74); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.56 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.58 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 81.2 %

TSL Correction: Positive only

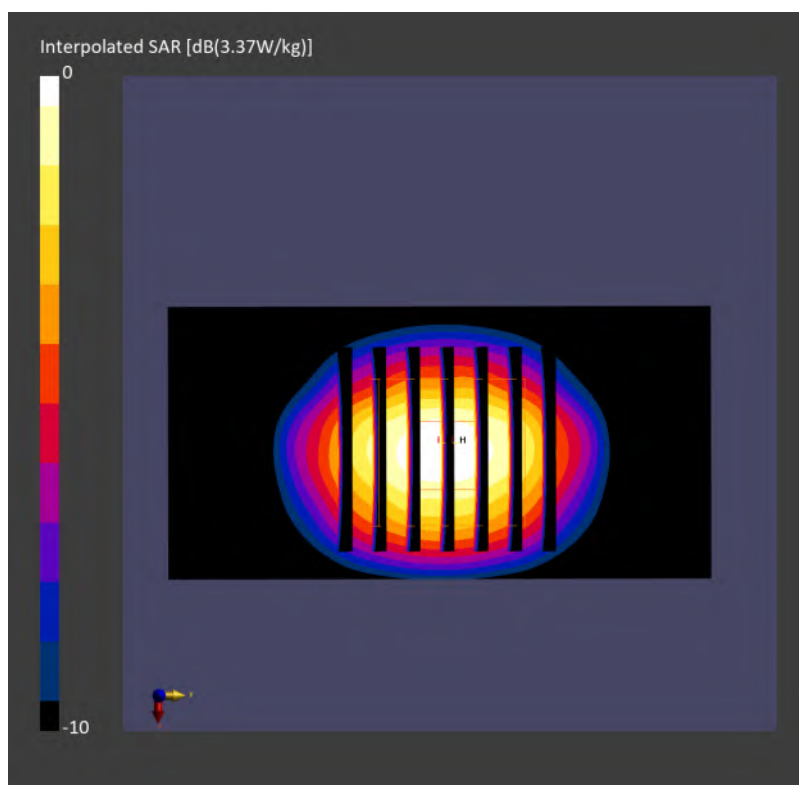

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260629 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(6.73, 7.27, 6.64); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.7 W/kg; SAR (10g) = 6.78 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 15.1 W/kg; SAR (8g) = 7.54 W/kg; SAR (10g) = 6.80 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.7 %

TSL Correction: Positive only

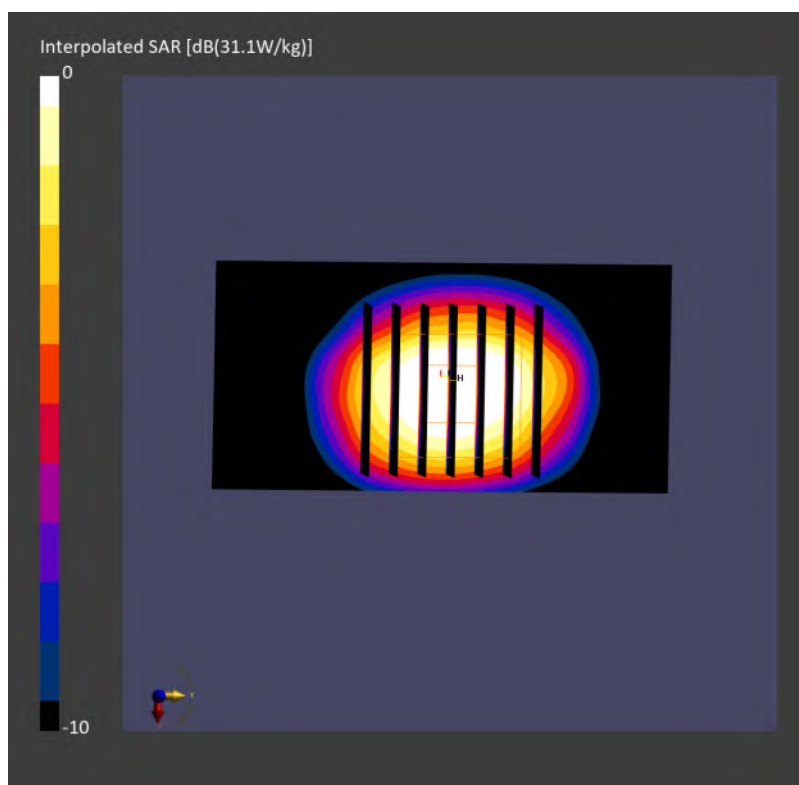

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260629 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.66, 6.54, 6.74); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.63 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.63 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.2 %

TSL Correction: Positive only

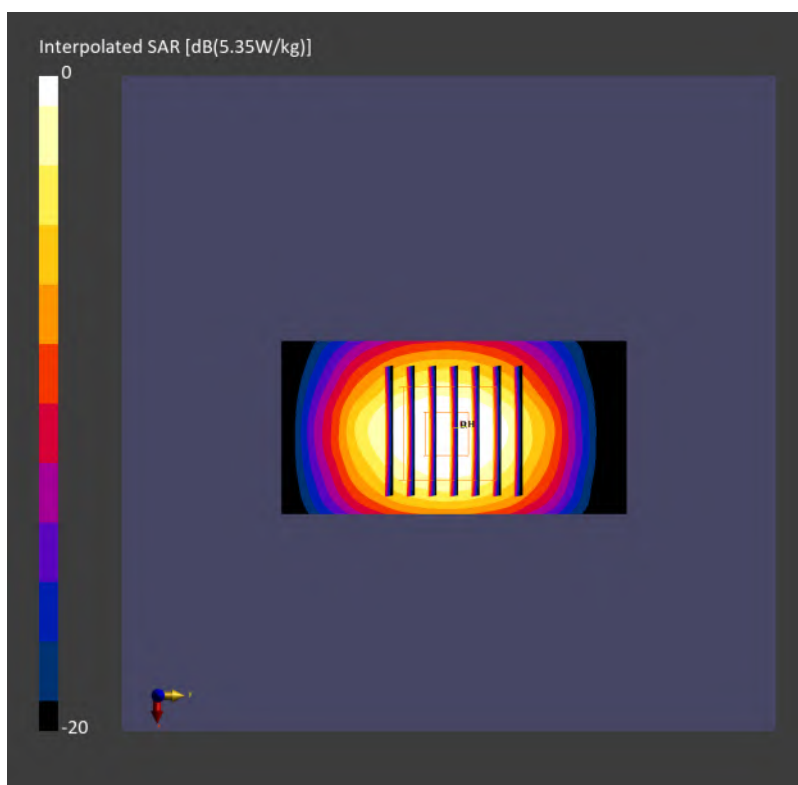

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260704 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(6.66, 6.54, 6.74); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.56 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.56 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

TSL Correction: Positive only

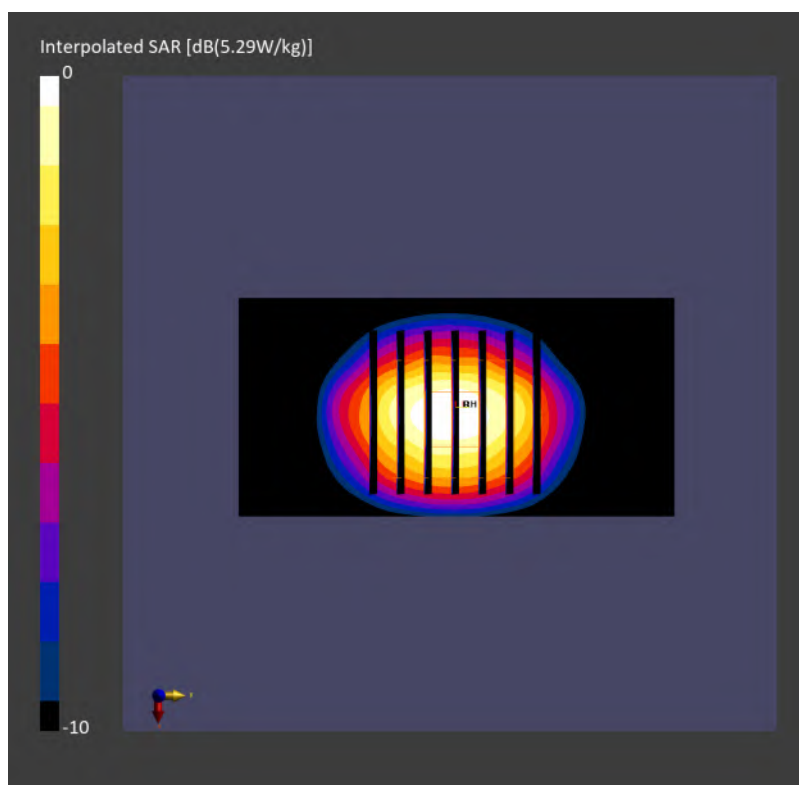

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260619 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.80$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.96, 6.44, 5.88); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.44 W/kg; SAR (10g) = 2.51 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.74 W/kg; SAR (8g) = 2.92 W/kg; SAR (10g) = 2.59 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

TSL Correction: Positive only

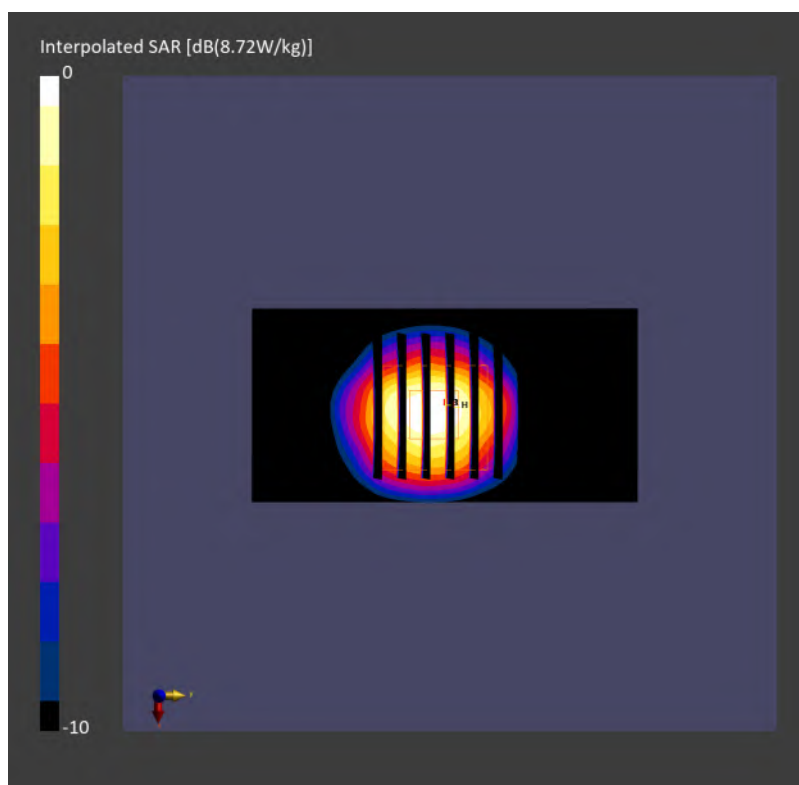

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260624 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.66$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.96, 6.44, 5.88); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.02 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.13 dB

SAR (1g) = 3.04 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

TSL Correction: Positive only

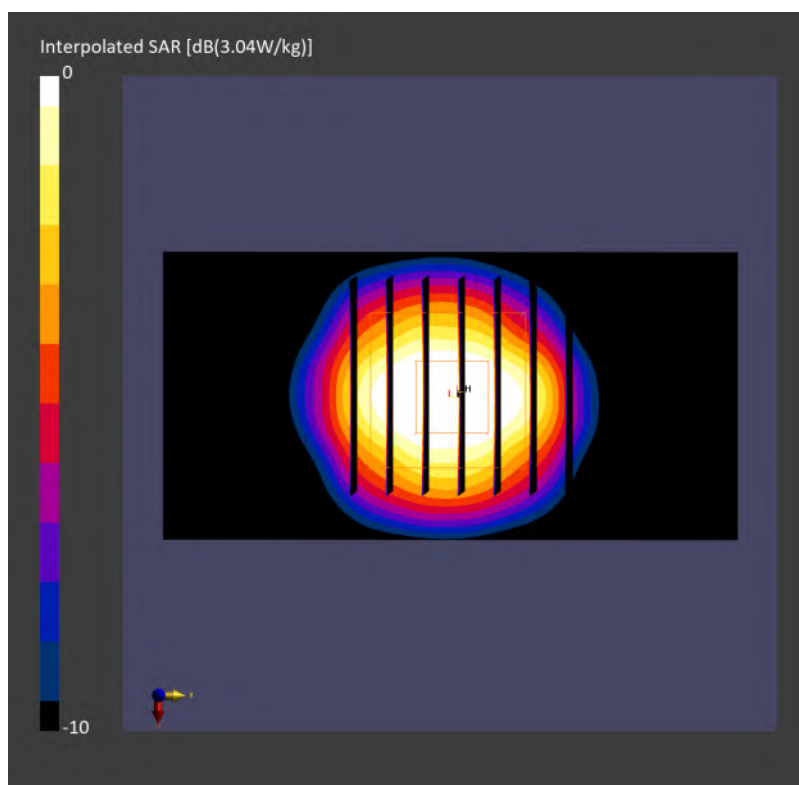

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260625 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.71$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.96, 6.44, 5.88); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.21 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

TSL Correction: Positive only

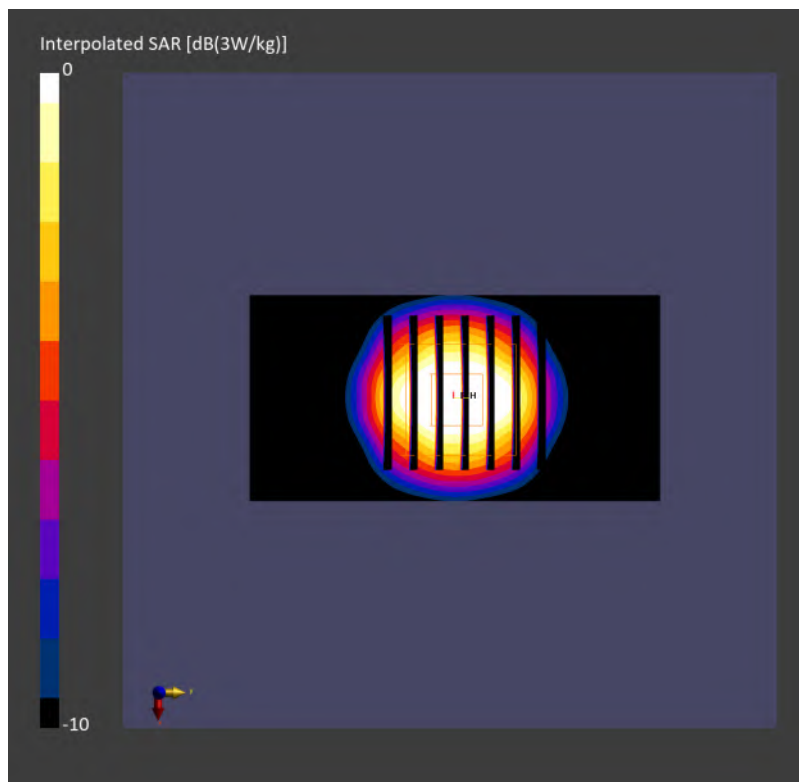

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260626 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.75$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.96, 6.44, 5.88); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.20 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

TSL Correction: Positive only

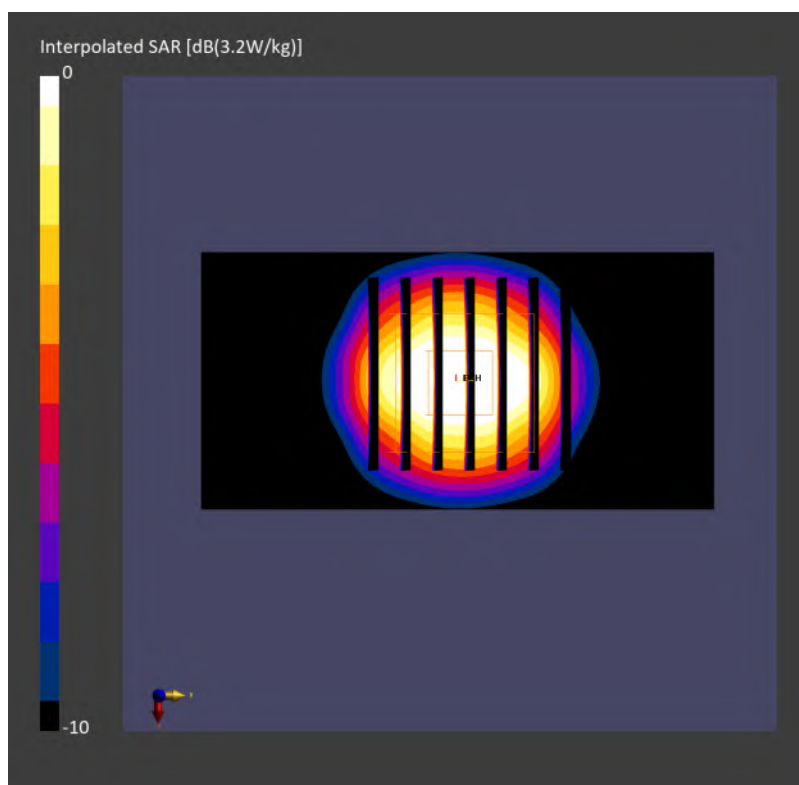

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260630 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.65$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.96, 6.44, 5.88); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.05 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.08 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.7 %

TSL Correction: Positive only

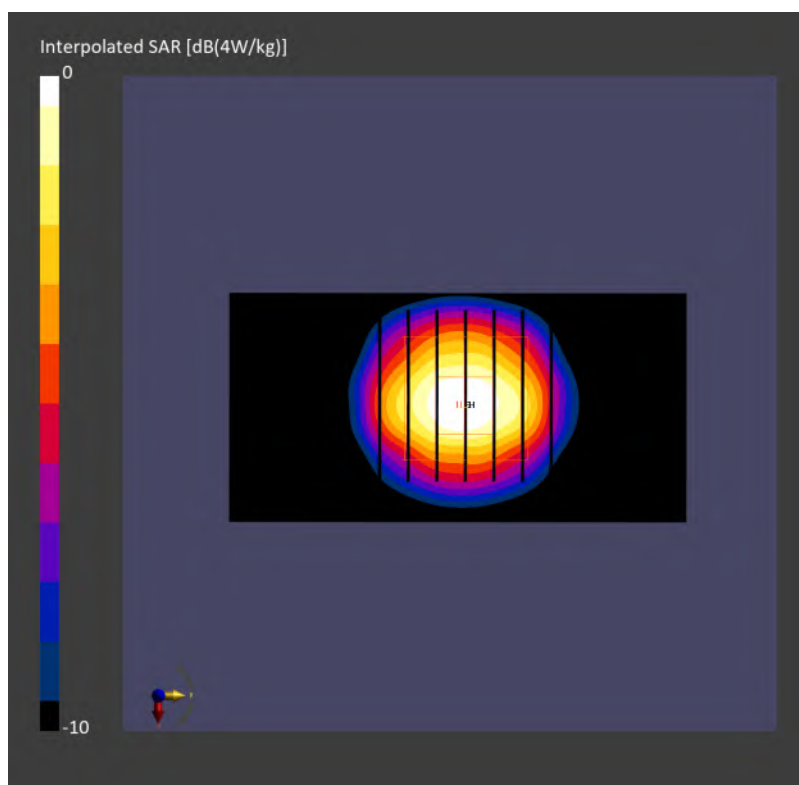

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260702 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.73$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.96, 6.44, 5.88); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.00 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.07 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

TSL Correction: Positive only

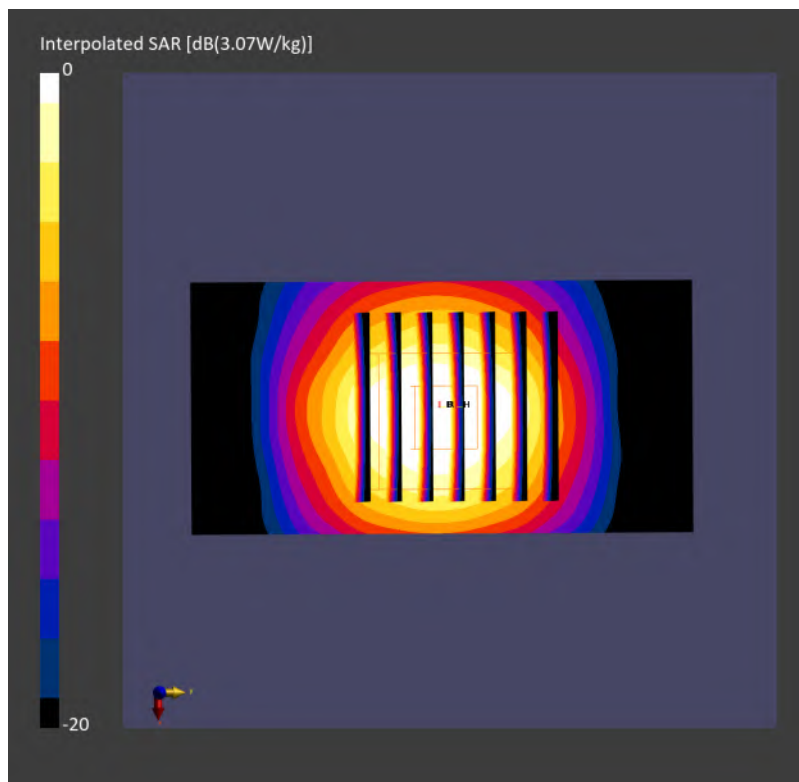

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260619 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.96$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.88, 6.35, 5.8); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.18 W/kg; SAR (10g) = 2.73 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 7.43 W/kg; SAR (8g) = 3.13 W/kg; SAR (10g) = 2.77 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

TSL Correction: Positive only

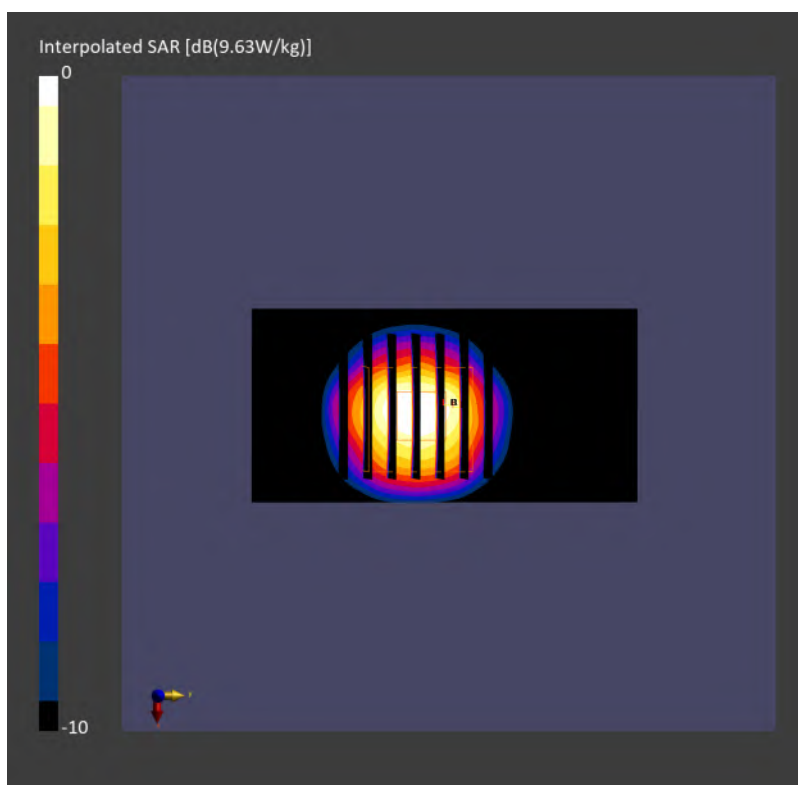

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260619 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.98$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.88, 6.35, 5.8); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.09 dB

SAR (1g) = 3.31 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

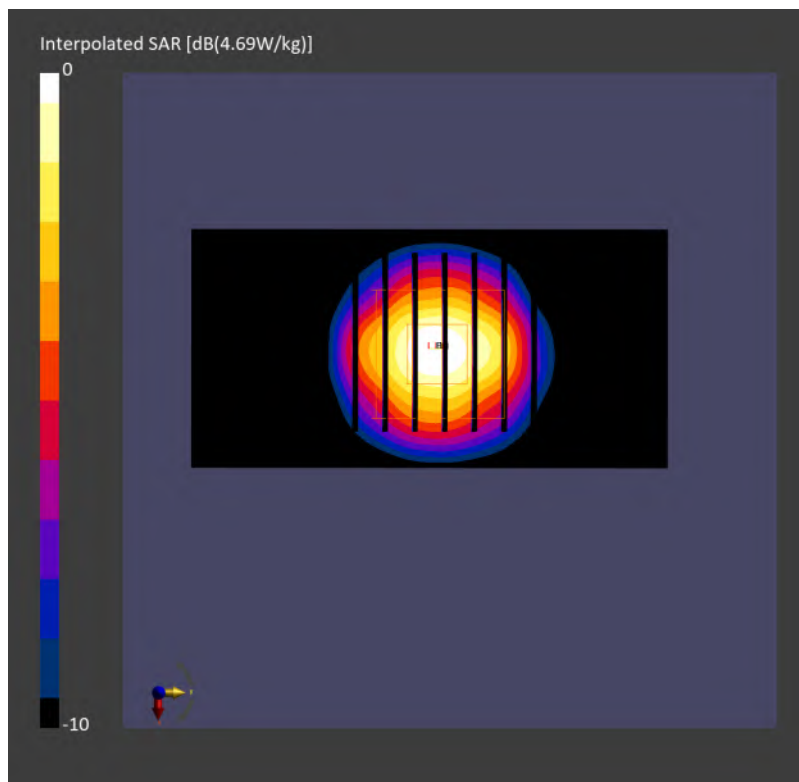

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260624 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.84$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.88, 6.35, 5.8); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.04 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.14 dB

SAR (1g) = 3.31 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 72.7 %

TSL Correction: Positive only

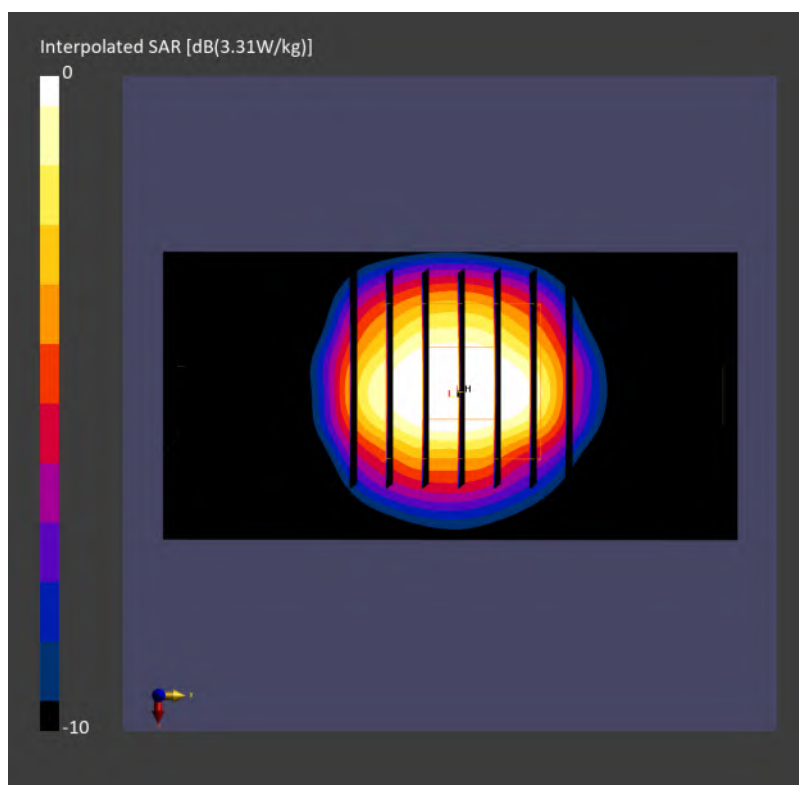

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260625 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.90$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.88, 6.35, 5.8); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.36 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.5 %

TSL Correction: Positive only

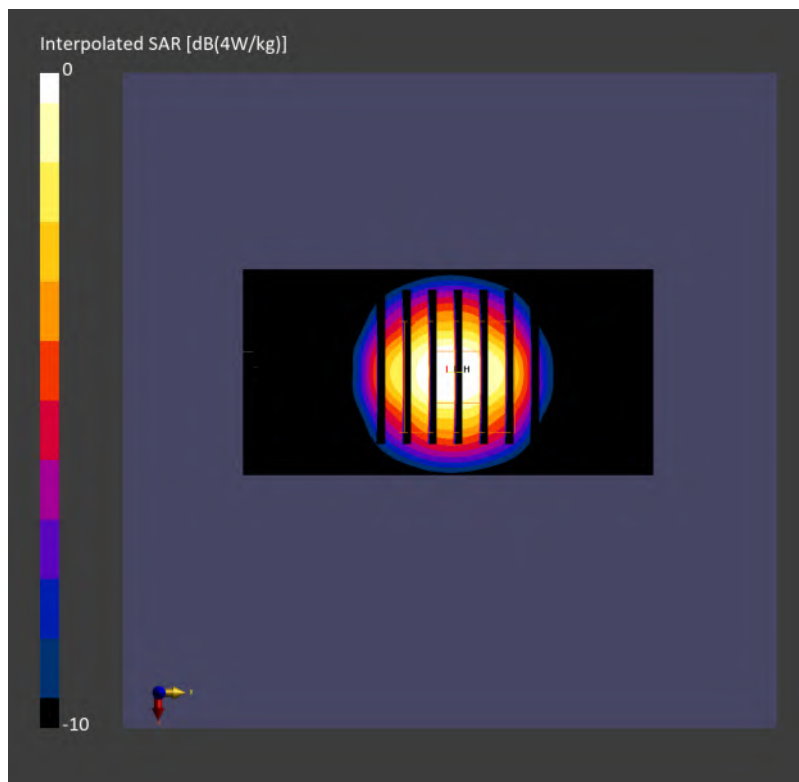

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260626 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.93$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.88, 6.35, 5.8); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.34 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.5 %

TSL Correction: Positive only

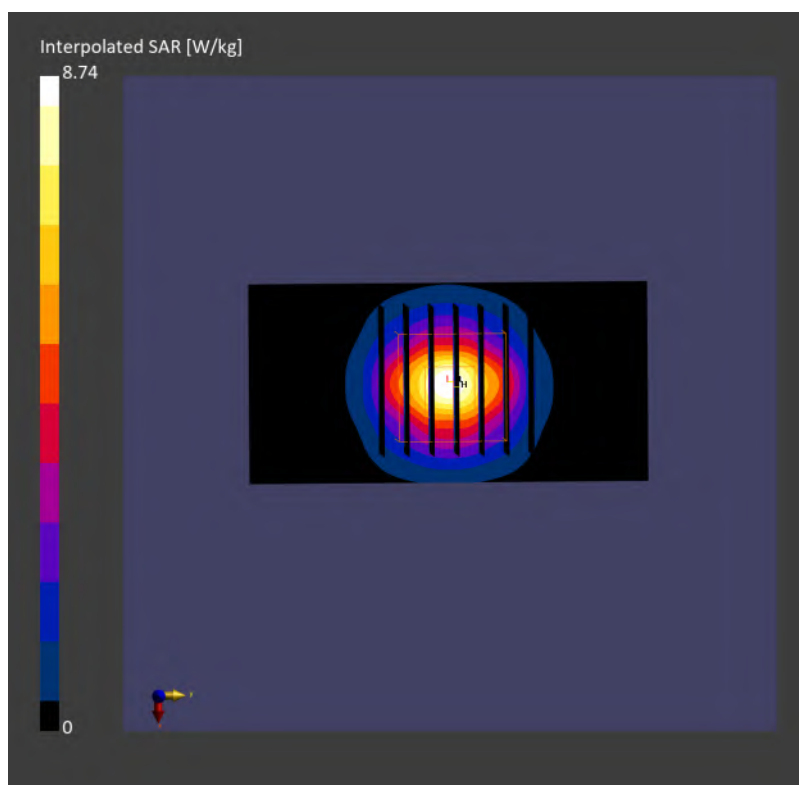

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260630 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.87$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.88, 6.35, 5.8); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.19 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.25 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 75.2 %

TSL Correction: Positive only

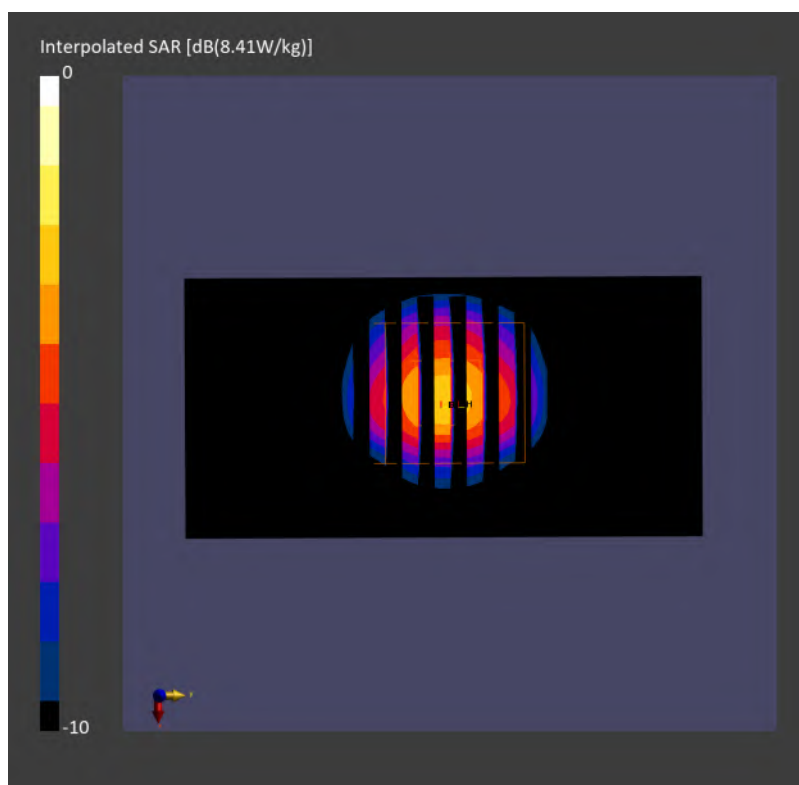

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260702 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.88, 6.35, 5.8); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.16 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.24 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.3 %

TSL Correction: Positive only

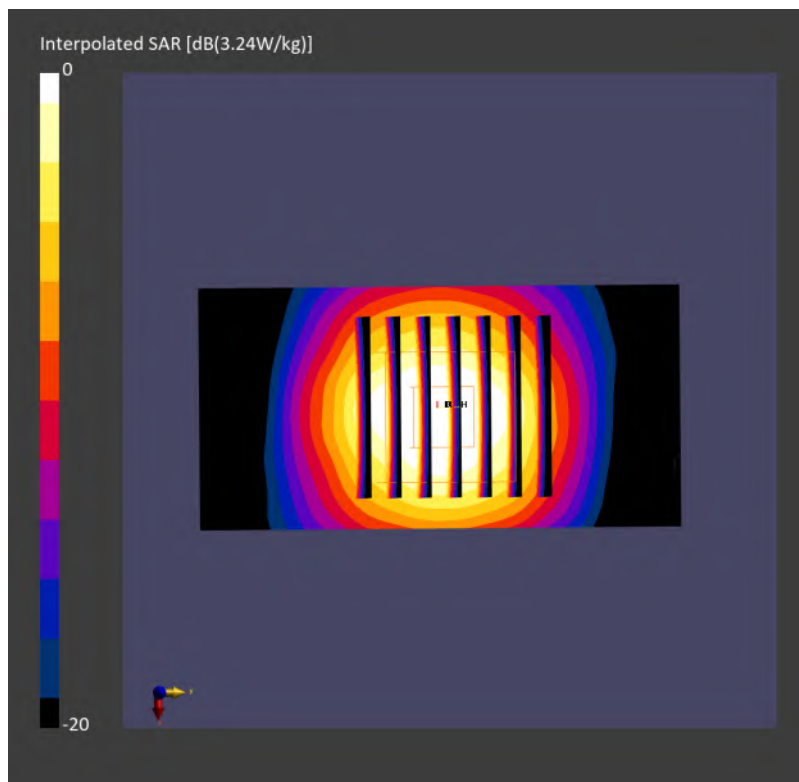

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260625 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.79, 6.25, 5.71); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.04 W/kg; SAR (10g) = 1.08 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.7 %

TSL Correction: Positive only

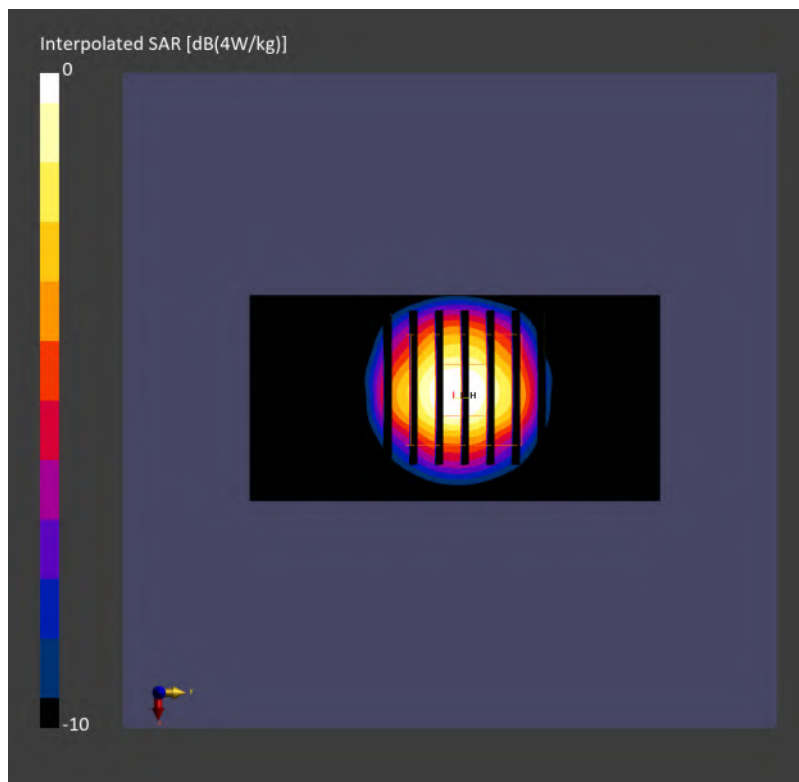

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260626 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.79, 6.25, 5.71); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.04 W/kg; SAR (10g) = 1.07 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.12 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.1 %

TSL Correction: Positive only

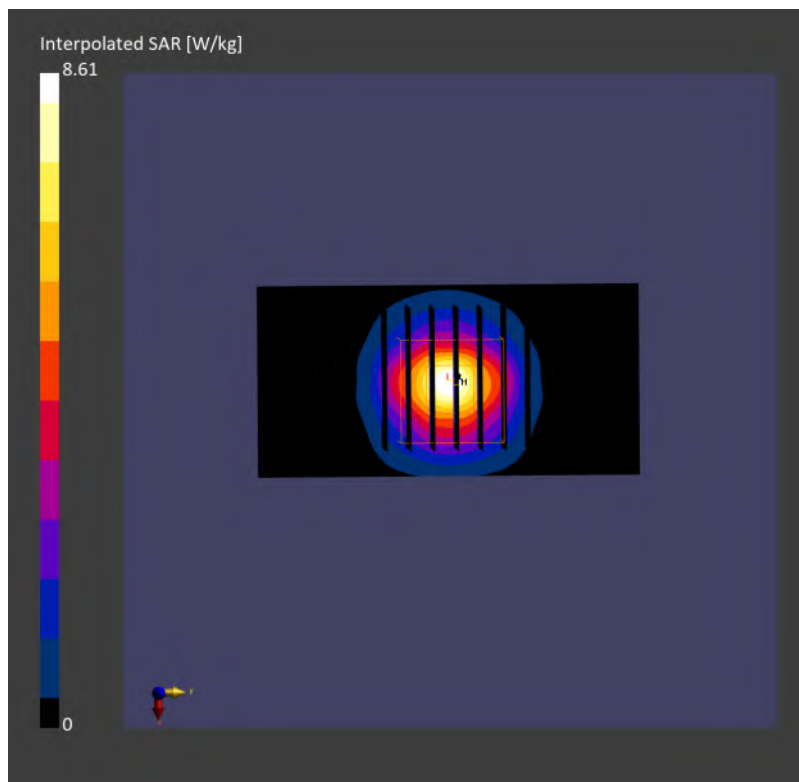

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260630 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.01$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.79, 6.25, 5.71); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.01 W/kg; SAR (10g) = 1.05 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.03 W/kg; SAR (8g) = 1.22 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.9 %

TSL Correction: Positive only

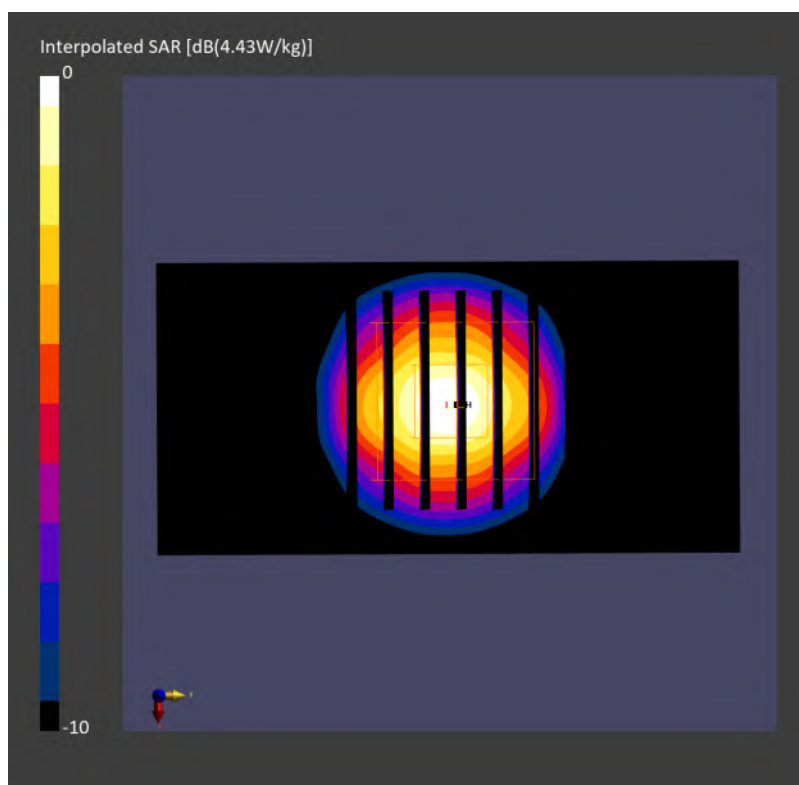

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260702 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.11$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.79, 6.25, 5.71); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.20 W/kg; SAR (10g) = 1.11 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.06 dB

SAR (1g) = 3.21 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.5 %

TSL Correction: Positive only

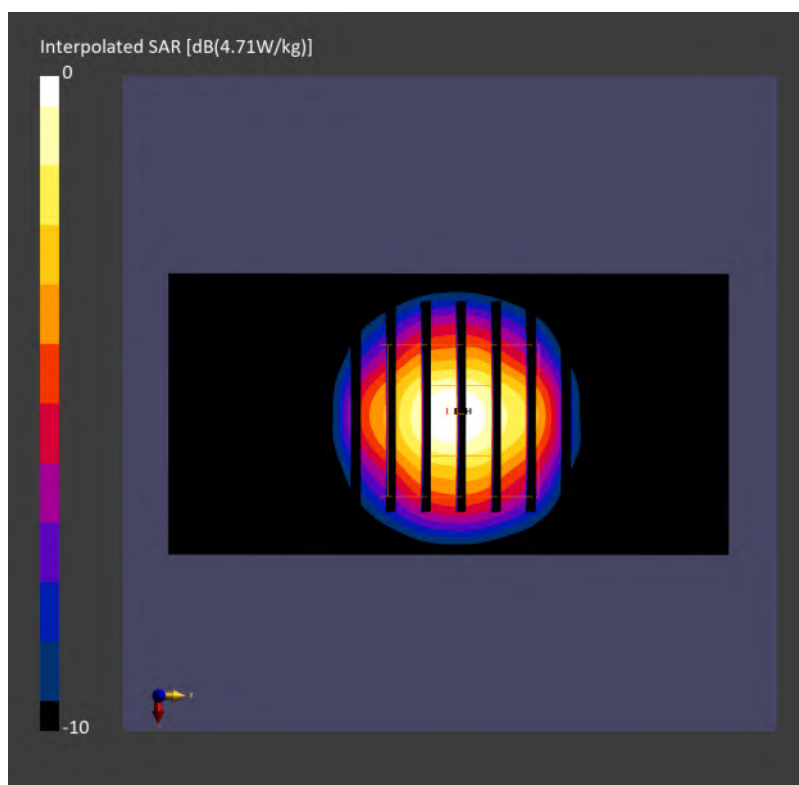

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260701 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.50$ S/m; $\epsilon_r = 34.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(5.03, 5.43, 4.96); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.62 W/kg; SAR (10g) = 1.04 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.85 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.1 %

TSL Correction: Positive only

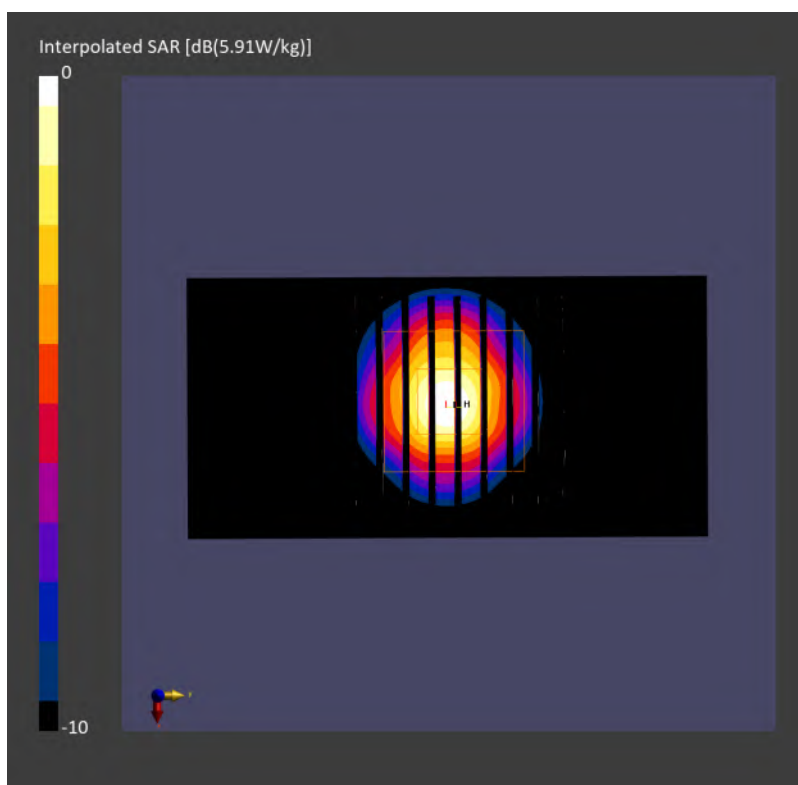

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260707 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.60$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(5.44, 5.34, 5.5); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.72 W/kg; SAR (10g) = 1.07 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 4.11 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 63.7 %

TSL Correction: Positive only

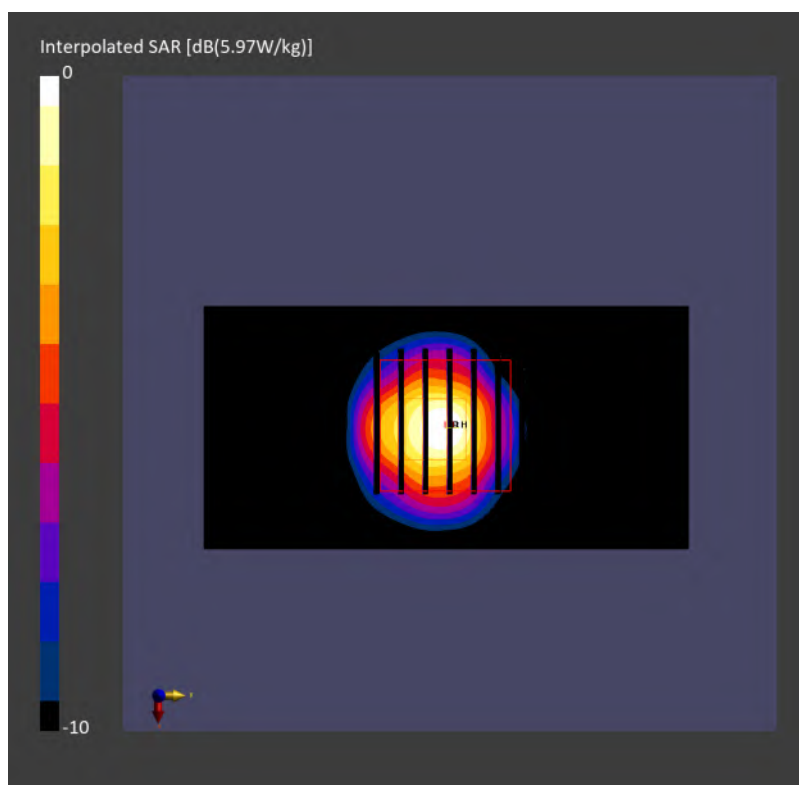

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260701 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.81$ S/m; $\epsilon_r = 34.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(4.61, 4.98, 4.54); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.83 W/kg; SAR (10g) = 1.09 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 4.10 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 60.0 %

TSL Correction: Positive only

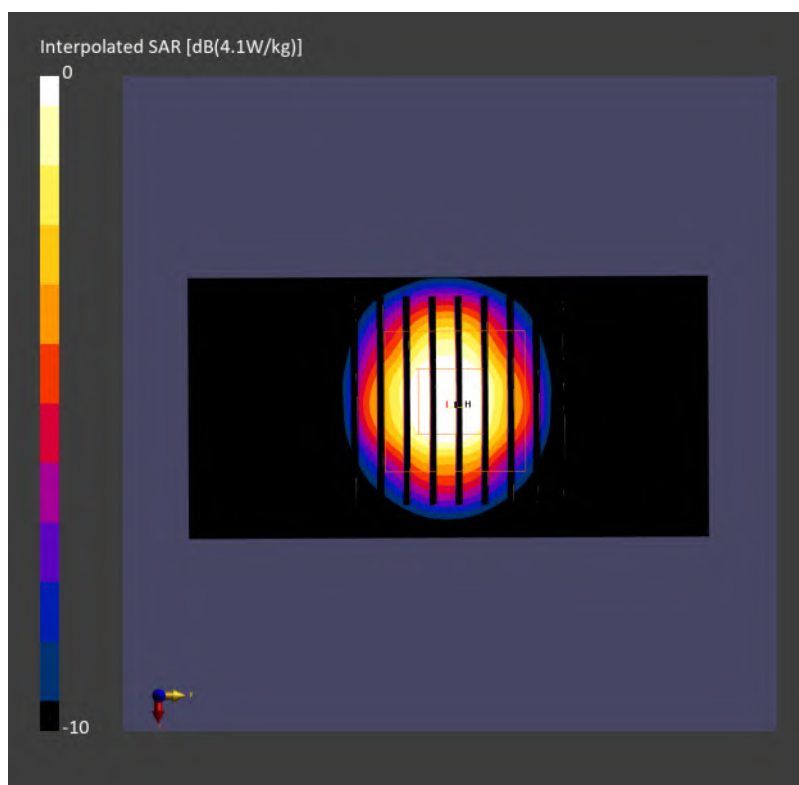

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260707 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.98$ S/m; $\epsilon_r = 34.3$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.97, 4.88, 5.03); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.10 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 4.56 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.5 %

TSL Correction: Positive only

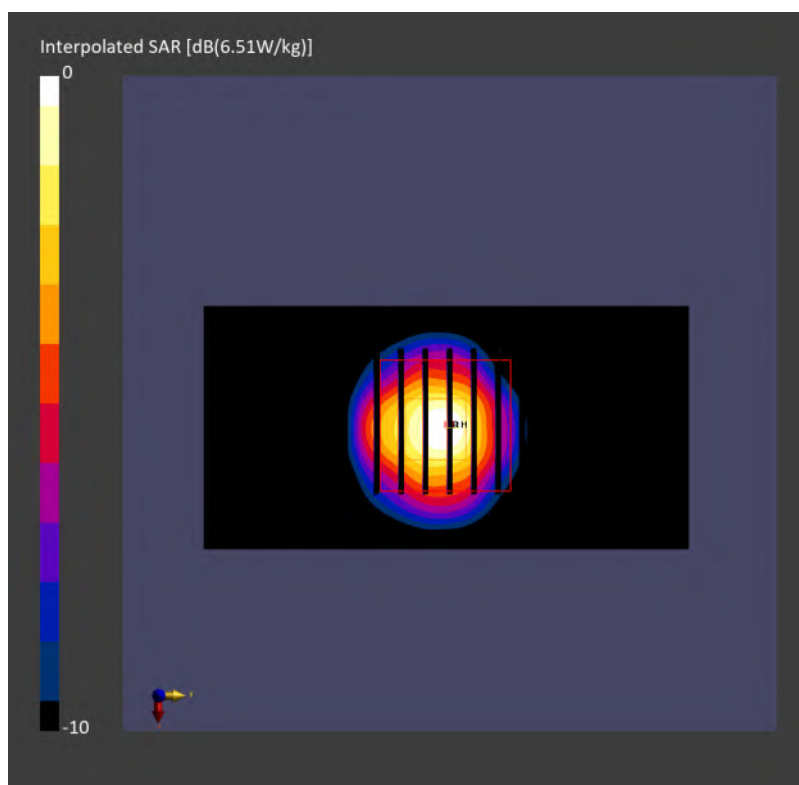

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260701 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.14$ S/m; $\epsilon_r = 33.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(4.54, 4.9, 4.48); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.67 W/kg; SAR (10g) = 1.05 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.03 dB

SAR (1g) = 3.94 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 58.1 %

TSL Correction: Positive only

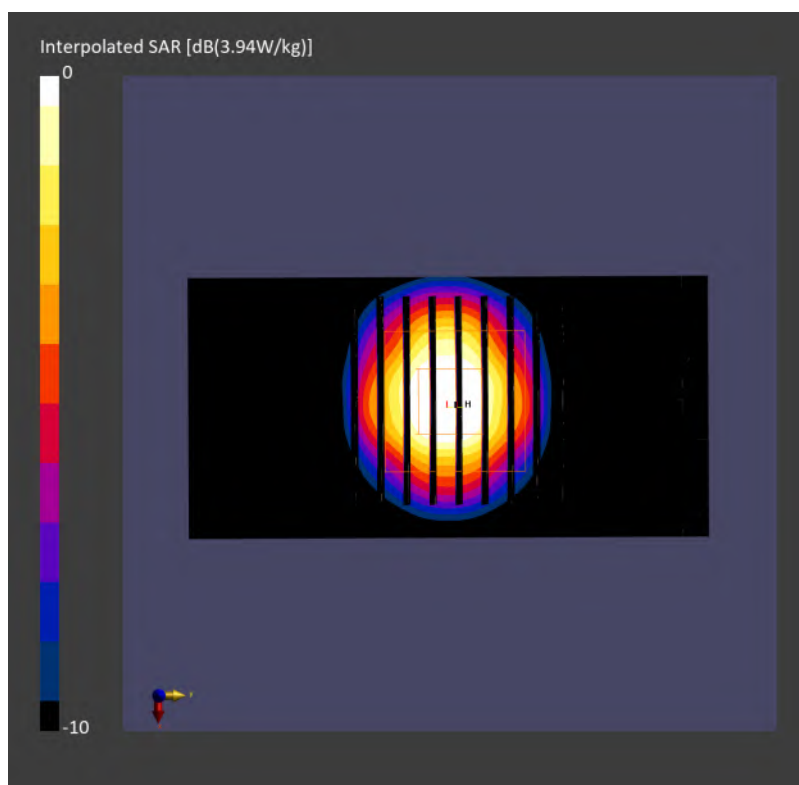

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260707 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.23$ S/m; $\epsilon_r = 34.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.92, 4.83, 4.98); Calibrated: 2026-03-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2026-04-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.57 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 3.98 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 58.5 %

TSL Correction: Positive only

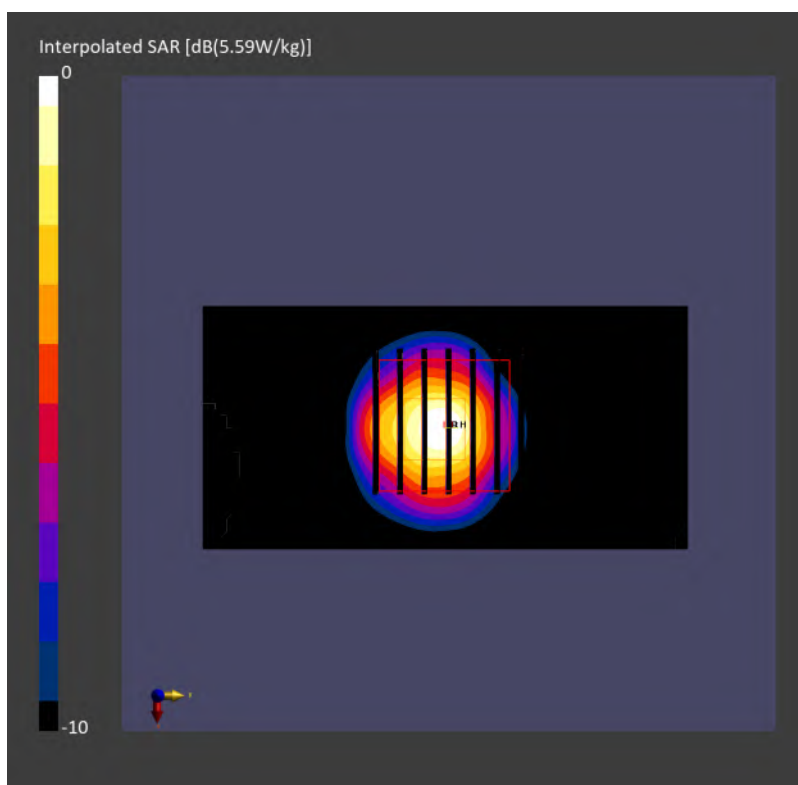

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1083**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_600-7200_260703 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 5.94$ S/m; $\epsilon_r = 32.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(4.76, 5.14, 4.7); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 26.1 W/kg; SAR (10g) = 5.52 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (23.8 mm x 23.8 mm x 22.9 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.02 dB


SAR (1g) = 32.0 W/kg; SAR (8g) = 7.25 W/kg; SAR (10g) = 5.97 W/kg

Smallest distance from peaks to all points 3 dB below = 4.9 mm

Ratio of SAR at M2 to SAR at M1 = 51.3 %

psAPD (1.0cm², sq) = 320 [W/m²]; psAPD (4.0cm², sq) = 145 [W/m²]

TSL Correction: Positive only

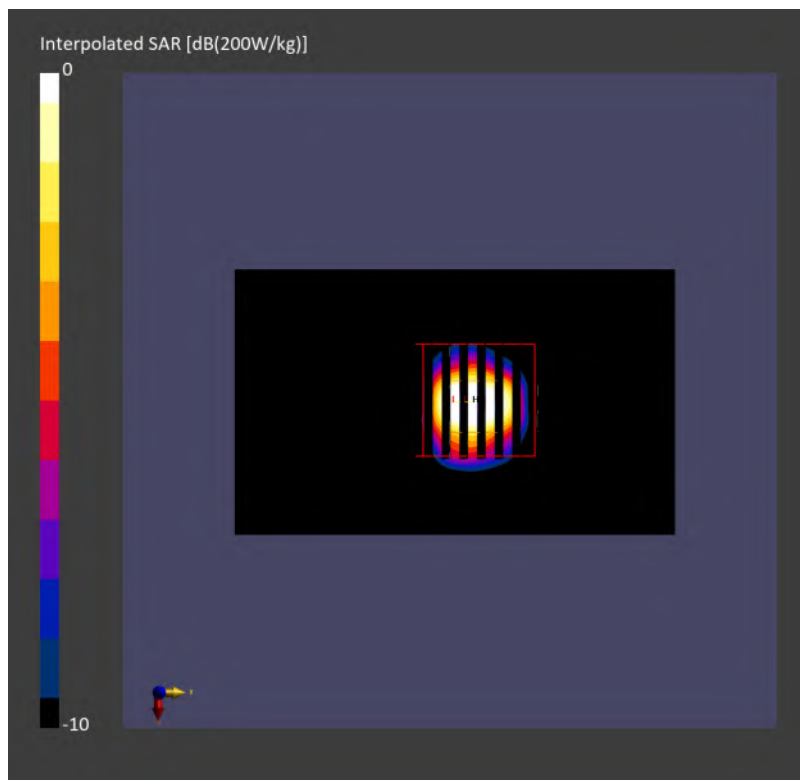

Measurement Report for Device
Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	Software Version	DUT Type
Device,	70.0 x 50.0 x 8.0	3.2.0.1840	5G Verification Source

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor
5G	FRONT, 10.00	10000.0	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave – 1044	Air –	EUmmWV3 – SN9424_F1–55GHz, 2026–03–12	DAE4 Sn699, 2026–02–13

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120.0 x 120.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0

Measurement Results

Date	2026–07–08
Avg. Area [cm ²]	4.00
psPDn+ [W/m ²]	54.7
psPDtot+ [W/m ²]	54.8
H _{max} [A/m]	0.399
E _{max} [V/m]	154
max _(Stot) [W/m ²]	61.4
Power Drift [dB]	0.08
IPDn	97.4

