

System Check_Head_13.56MHz**DUT: CLA-13 - SN1022**

Communication System: CW; Frequency: 13.000 MHz

Medium: HSL_4-250_260906 Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.758$ S/m; $\epsilon_r = 55.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(14.15, 14.46, 14.12); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156_Gap_0414; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=30.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.511 W/kg; SAR (10g) = 0.413 W/kg;

TSL Correction: Positive only

Pin=30.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 0.491 W/kg; SAR (8g) = 0.321 W/kg; SAR (10g) = 0.308 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 75.7 %

TSL Correction: Positive only

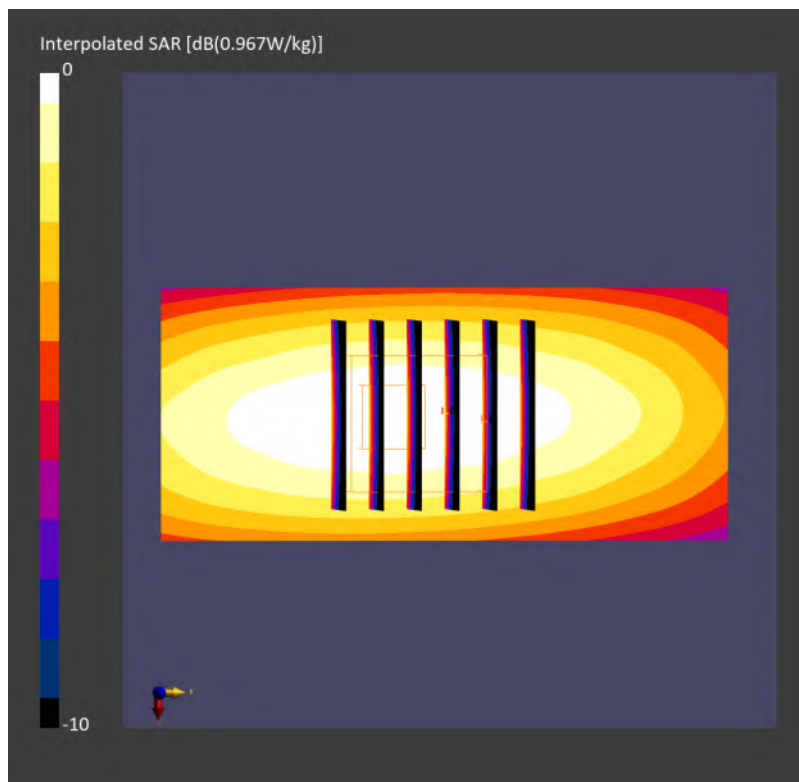

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260818 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.890$ S/m; $\epsilon_r = 43.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(10.04, 9.32, 9.97); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.21 W/kg; SAR (10g) = 1.47 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.16 W/kg; SAR (8g) = 1.52 W/kg; SAR (10g) = 1.44 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.9 %

TSL Correction: Positive only

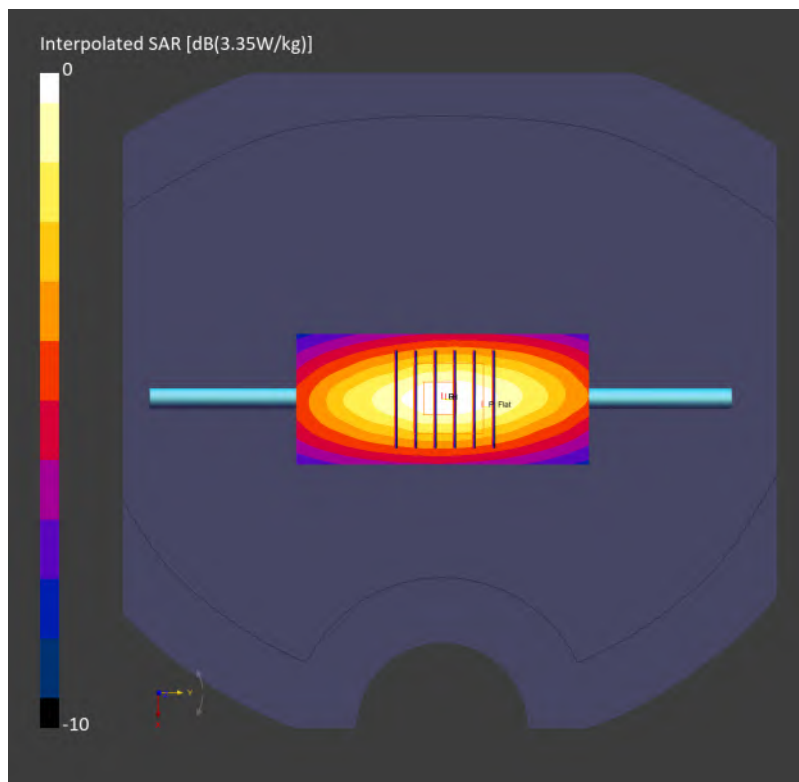

System Check_Head_750MHz**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260820 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.927$ S/m; $\epsilon_r = 43.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(9.87, 10.04, 9.6); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.23 W/kg; SAR (10g) = 1.52 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 2.22 W/kg; SAR (8g) = 1.61 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 91.7 %

TSL Correction: Positive only

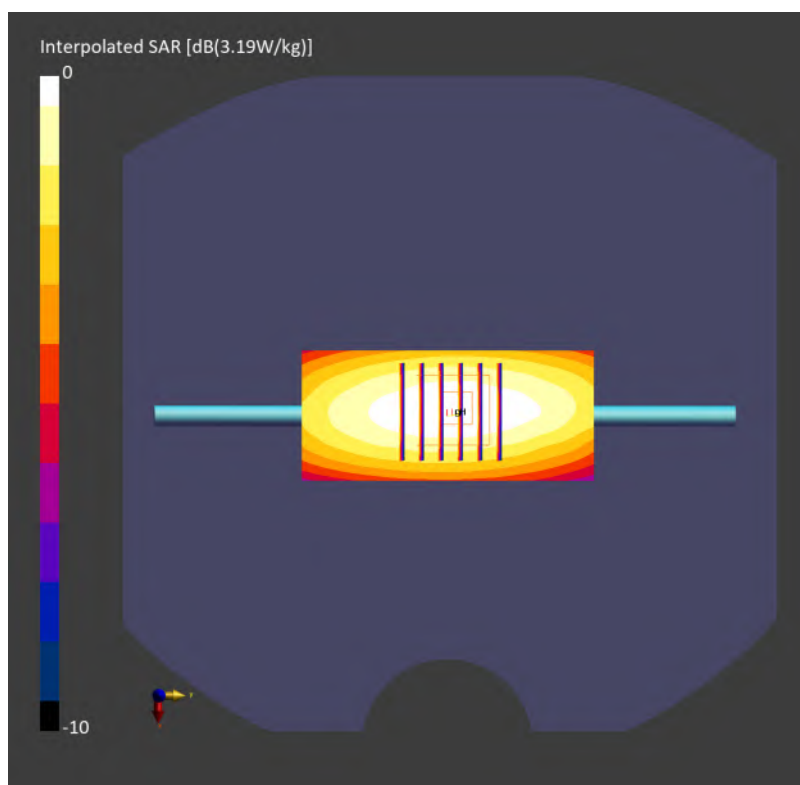

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260821 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.901$ S/m; $\epsilon_r = 45.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(9.53, 10.16, 9.59); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.416 W/kg; SAR (10g) = 0.275 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.04 dB

SAR (1g) = 0.418 W/kg; SAR (8g) = 0.295 W/kg; SAR (10g) = 0.281 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

TSL Correction: Positive only

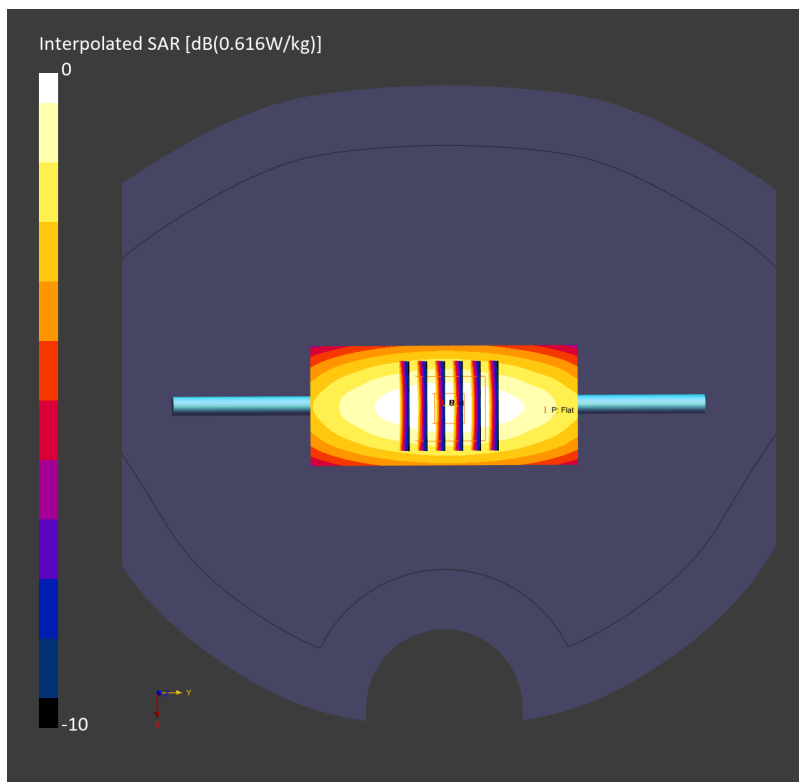

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.902$ S/m; $\epsilon_r = 43.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(9.53, 10.16, 9.59); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.07 W/kg; SAR (10g) = 1.38 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.06 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.39 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

TSL Correction: Positive only

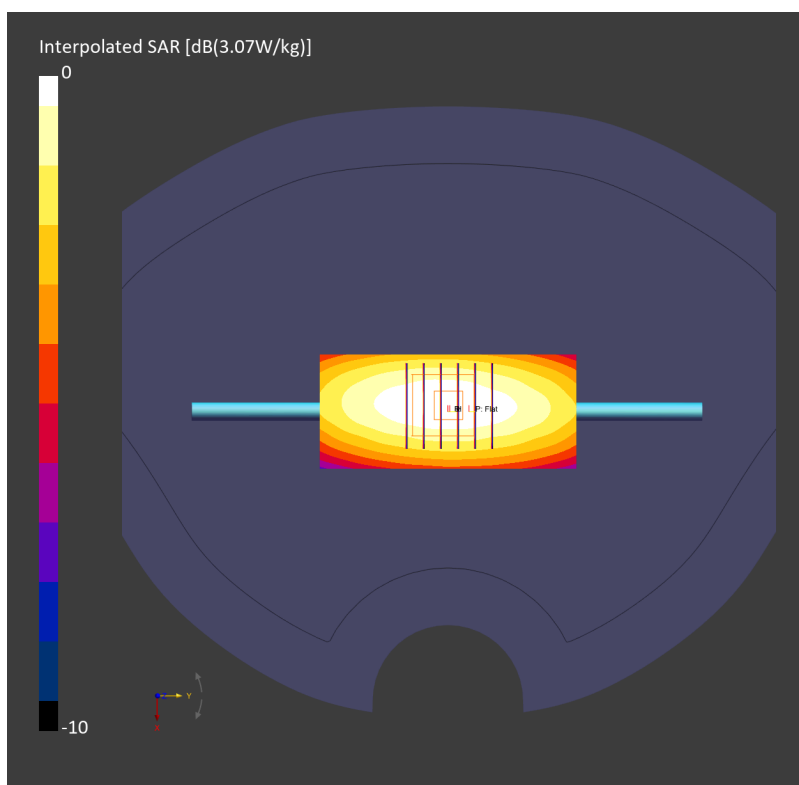

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.906$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(10.04, 9.32, 9.97); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.14 W/kg; SAR (10g) = 1.42 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.03 dB

SAR (1g) = 2.12 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = 23.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

TSL Correction: Positive only

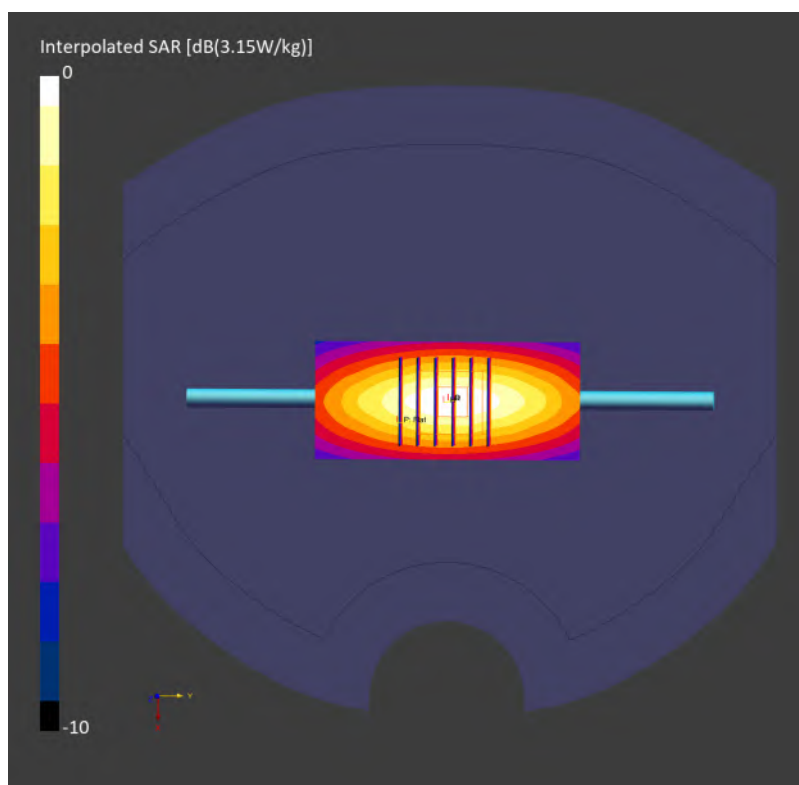

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.887$ S/m; $\epsilon_r = 43.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(9.53, 10.16, 9.59); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.415 W/kg; SAR (10g) = 0.275 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 0.420 W/kg; SAR (8g) = 0.296 W/kg; SAR (10g) = 0.282 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

TSL Correction: Positive only

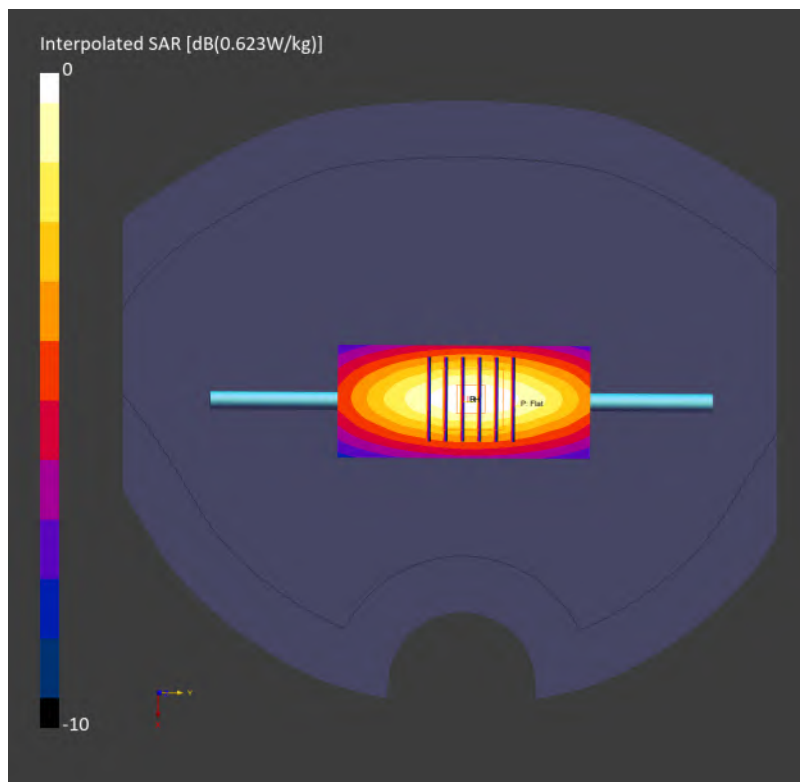

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.921$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(10.04, 9.32, 9.97); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.55 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.32 W/kg; SAR (8g) = 1.64 W/kg; SAR (10g) = 1.55 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.8 %

TSL Correction: Positive only

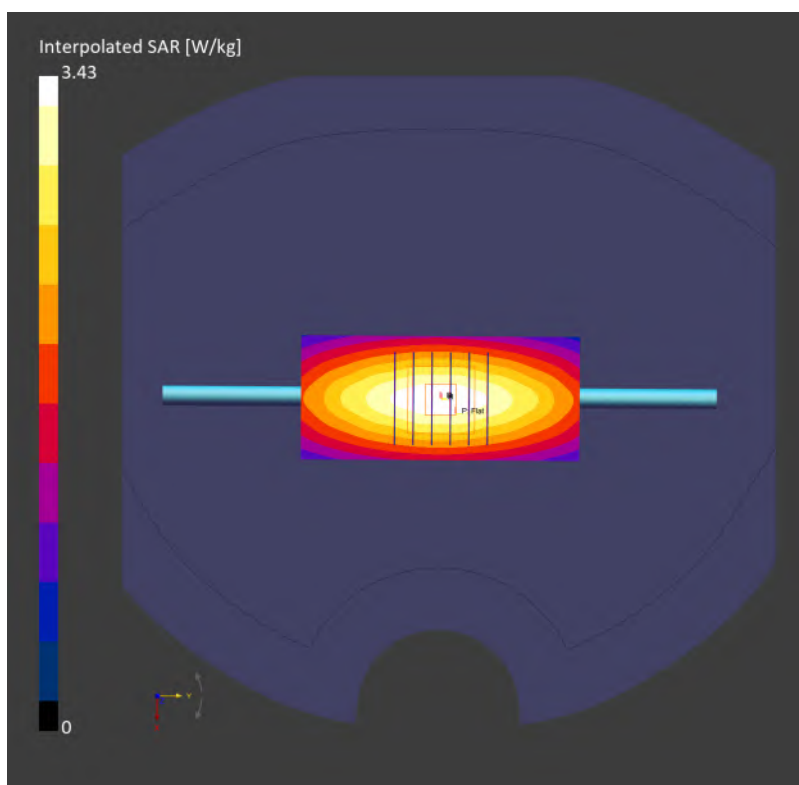

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.898$ S/m; $\epsilon_r = 44.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(9.53, 10.16, 9.59); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.25 W/kg; SAR (10g) = 1.49 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.05 dB

SAR (1g) = 2.27 W/kg; SAR (8g) = 1.61 W/kg; SAR (10g) = 1.53 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 87.8 %

TSL Correction: Positive only

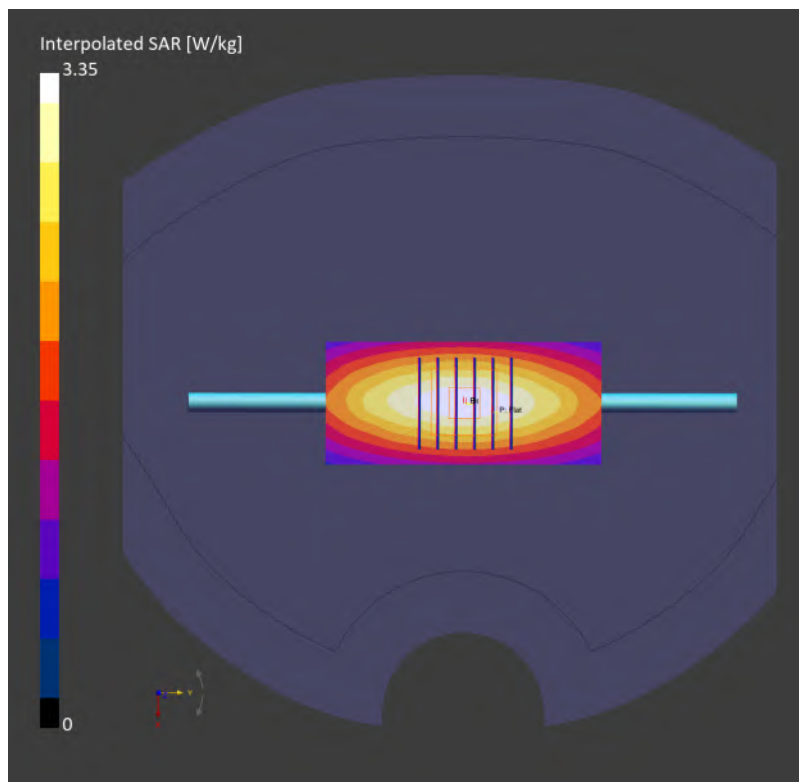

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: UID 0, CW; Frequency: 750 MHz

Medium: HSL_600~7200_260908 Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.902 \text{ S/m}$; $\epsilon_r = 42.689$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature : 23.5°C ; Liquid Temperature : 22.5°C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.14, 9.72, 9.56) @ 750 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (51x51x1): Interpolated grid: $dx=1.500 \text{ mm}$, $dy=1.500 \text{ mm}$

Maximum value of SAR (interpolated) = 2.73 W/kg

Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 59.36 V/m ; Power Drift = -0.07 dB


Peak SAR (extrapolated) = 3.13 W/kg

SAR(1 g) = 2.12 W/kg ; SAR(10 g) = 1.39 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 67.3%

Maximum value of SAR (measured) = 2.81 W/kg

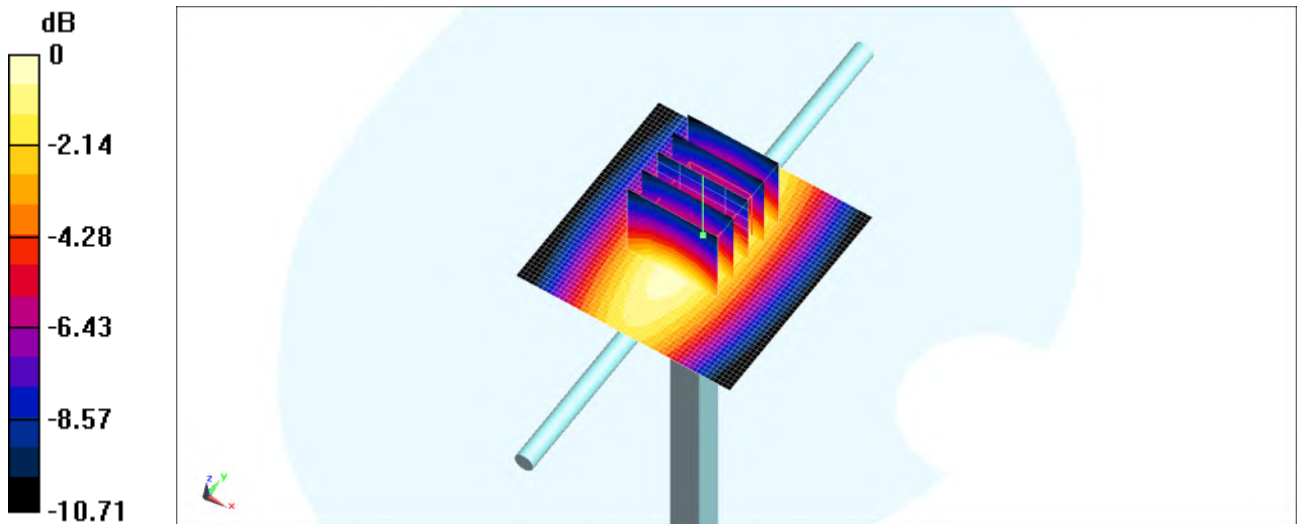

0 dB = 2.81 W/kg = 4.49 dBW/kg

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: UID 0, CW; Frequency: 750 MHz

Medium: HSL_600~7200_260909 Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.905 \text{ S/m}$; $\epsilon_r = 42.619$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature : $23.5 \text{ }^\circ\text{C}$; Liquid Temperature : $22.5 \text{ }^\circ\text{C}$

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.14, 9.72, 9.56) @ 750 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (51x51x1): Interpolated grid: $dx=1.500 \text{ mm}$, $dy=1.500 \text{ mm}$

Maximum value of SAR (interpolated) = 2.94 W/kg

Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 61.02 V/m ; Power Drift = -0.05 dB


Peak SAR (extrapolated) = 3.35 W/kg

SAR(1 g) = 2.27 W/kg ; SAR(10 g) = 1.49 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 67.4%

Maximum value of SAR (measured) = 3.01 W/kg

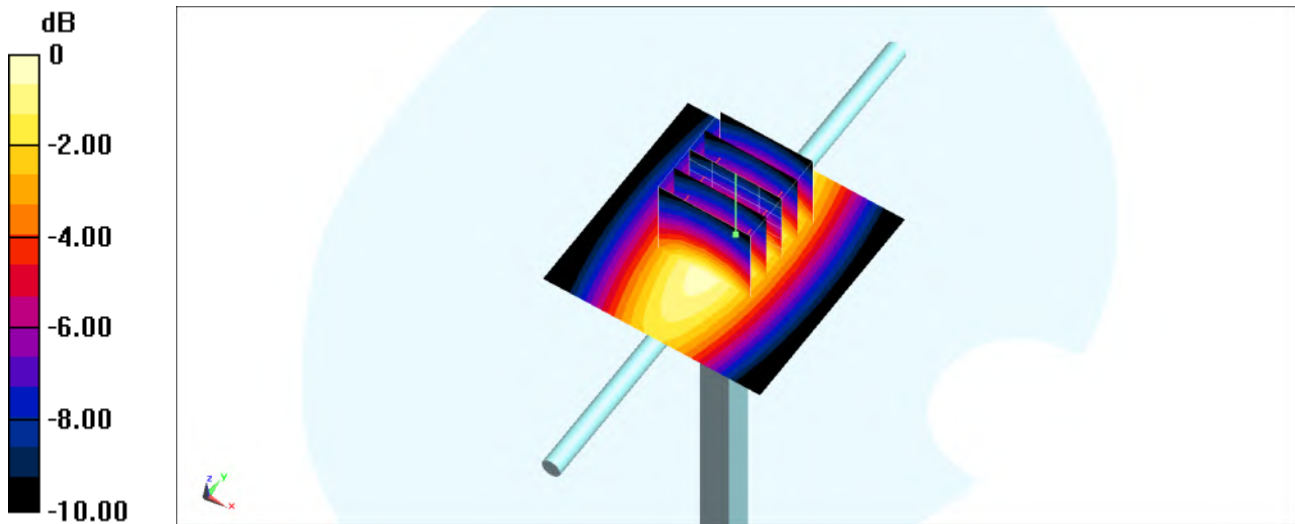

0 dB = 3.01 W/kg = 4.79 dBW/kg

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: UID 0, CW; Frequency: 750 MHz

Medium: HSL_600~7200_260910 Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.903 \text{ S/m}$; $\epsilon_r = 42.679$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature : $23.5 \text{ }^\circ\text{C}$; Liquid Temperature : $22.5 \text{ }^\circ\text{C}$

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.14, 9.72, 9.56) @ 750 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (51x51x1): Interpolated grid: $dx=1.500 \text{ mm}$, $dy=1.500 \text{ mm}$

Maximum value of SAR (interpolated) = 2.74 W/kg

Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 59.36 V/m ; Power Drift = -0.07 dB


Peak SAR (extrapolated) = 3.14 W/kg

SAR(1 g) = 2.13 W/kg ; SAR(10 g) = 1.39 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 67.3%

Maximum value of SAR (measured) = 2.81 W/kg

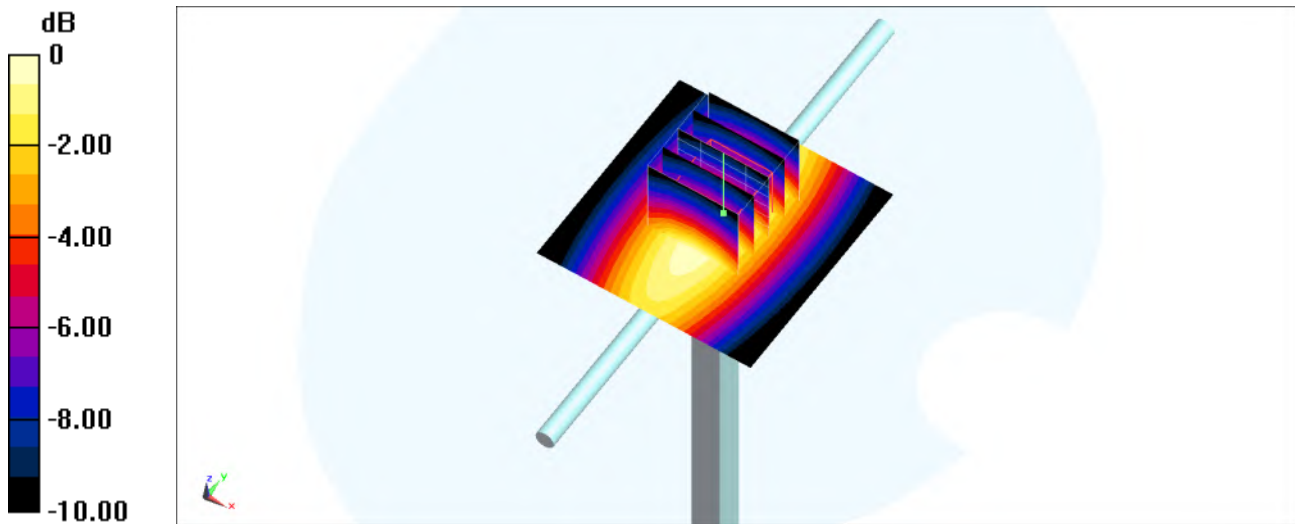

0 dB = 2.81 W/kg = 4.49 dBW/kg

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: UID 0, CW; Frequency: 750 MHz

Medium: HSL_600~7200_260911 Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.907 \text{ S/m}$; $\epsilon_r = 42.749$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature : $23.5 \text{ }^\circ\text{C}$; Liquid Temperature : $22.5 \text{ }^\circ\text{C}$

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.14, 9.72, 9.56) @ 750 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (51x51x1): Interpolated grid: $dx=1.500 \text{ mm}$, $dy=1.500 \text{ mm}$

Maximum value of SAR (interpolated) = 3.03 W/kg

Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 62.03 V/m ; Power Drift = -0.04 dB



Peak SAR (extrapolated) = 3.47 W/kg

SAR(1 g) = 2.34 W/kg ; SAR(10 g) = 1.53 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 67%

Maximum value of SAR (measured) = 3.11 W/kg

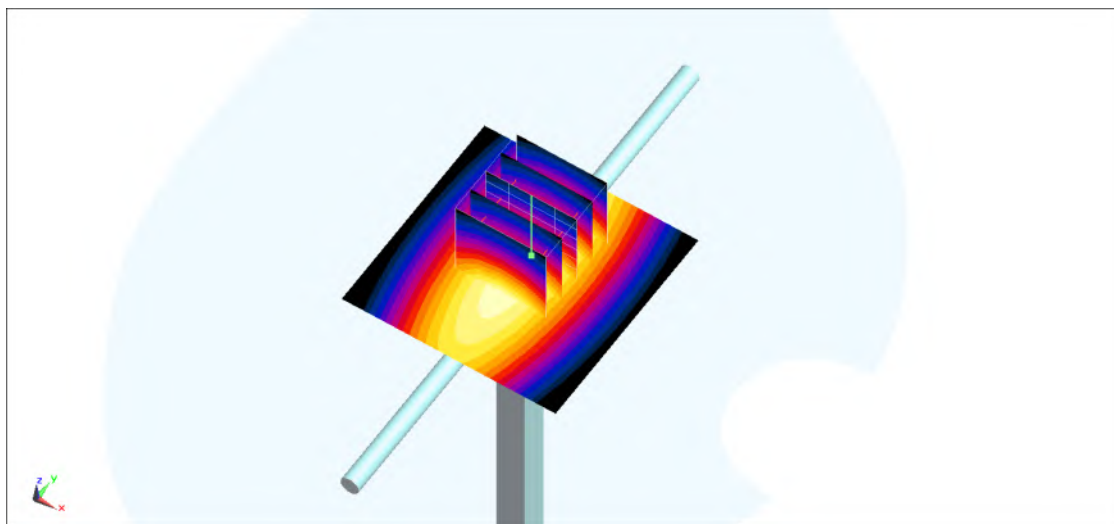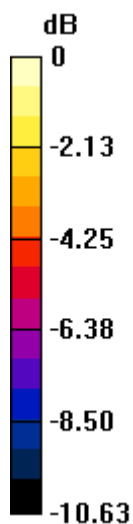

0 dB = 3.11 W/kg = 4.93 dBW/kg

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: UID 0, CW; Frequency: 750 MHz

Medium: HSL_600~7200_260912 Medium parameters used: $f = 750$ MHz; $\sigma = 0.91$ S/m; $\epsilon_r = 42.719$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.14, 9.72, 9.56) @ 750 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (51x51x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Maximum value of SAR (interpolated) = 2.93 W/kg

Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 60.75 V/m; Power Drift = -0.04 dB



Peak SAR (extrapolated) = 3.32 W/kg

SAR(1 g) = 2.26 W/kg; SAR(10 g) = 1.49 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 67.5%

Maximum value of SAR (measured) = 2.99 W/kg

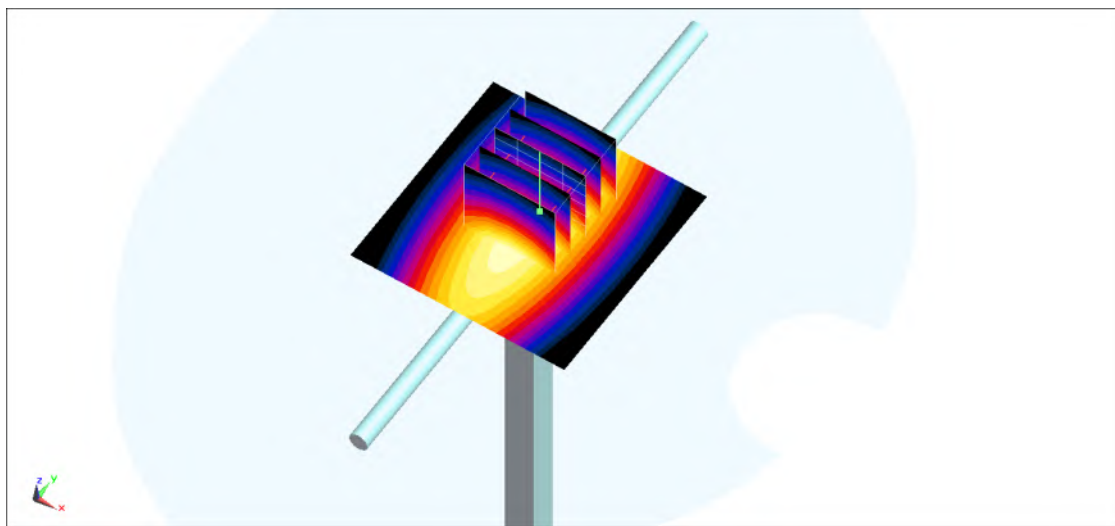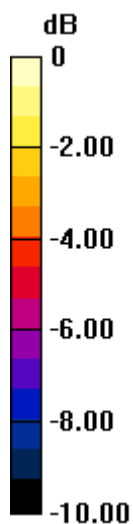

0 dB = 2.99 W/kg = 4.76 dBW/kg

System Check_Head_750MHz

DUT: D750V3 - SN1117

Communication System: UID 0, CW; Frequency: 750 MHz

Medium: HSL_600~7200_260913 Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.901 \text{ S/m}$; $\epsilon_r = 42.649$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature : $23.5 \text{ }^\circ\text{C}$; Liquid Temperature : $22.5 \text{ }^\circ\text{C}$

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.14, 9.72, 9.56) @ 750 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (51x51x1): Interpolated grid: $dx=1.500 \text{ mm}$, $dy=1.500 \text{ mm}$

Maximum value of SAR (interpolated) = 3.03 W/kg

Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 61.83 V/m ; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 3.44 W/kg

SAR(1 g) = 2.33 W/kg ; SAR(10 g) = 1.53 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 67.1%

Maximum value of SAR (measured) = 3.09 W/kg

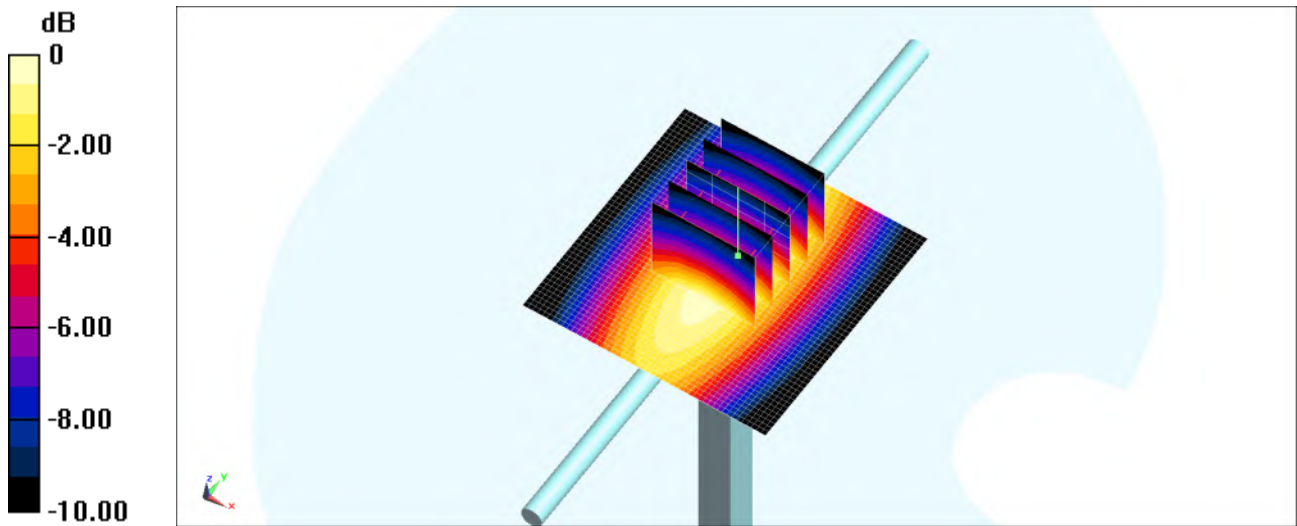

0 dB = 3.09 W/kg = 4.90 dBW/kg

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260818 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.913$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.82, 9.12, 9.75); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.56 W/kg; SAR (10g) = 1.67 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 2.49 W/kg; SAR (8g) = 1.73 W/kg; SAR (10g) = 1.64 W/kg

Smallest distance from peaks to all points 3 dB below = 15.1 mm

Ratio of SAR at M2 to SAR at M1 = 85.4 %

TSL Correction: Positive only

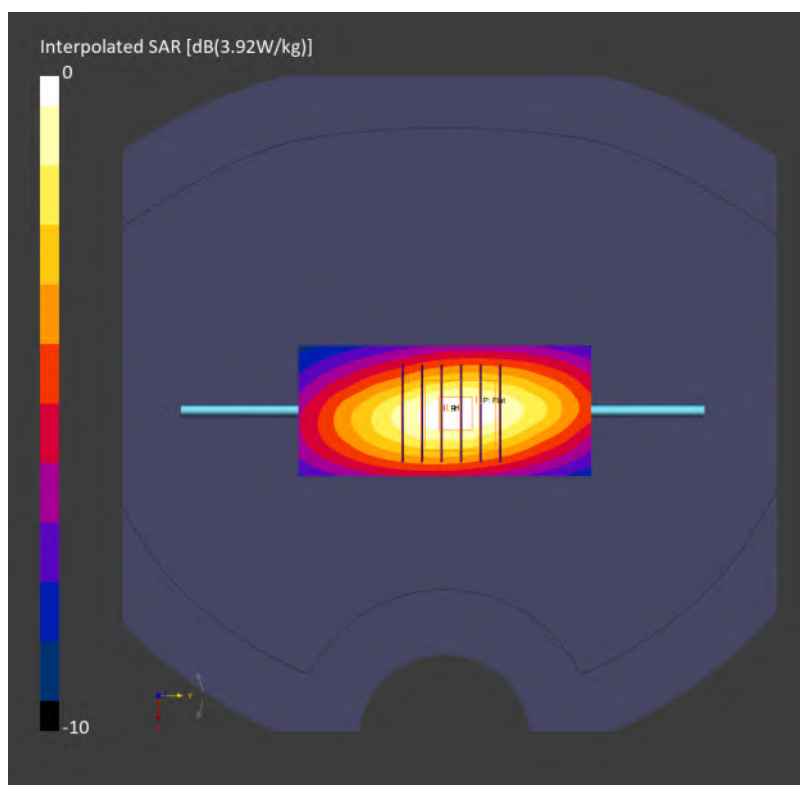

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260821 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.932$ S/m; $\epsilon_r = 44.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(9.51, 10.14, 9.57); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.50 W/kg; SAR (10g) = 1.64 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.71 W/kg; SAR (10g) = 1.63 W/kg

Smallest distance from peaks to all points 3 dB below = 15.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

TSL Correction: Positive only

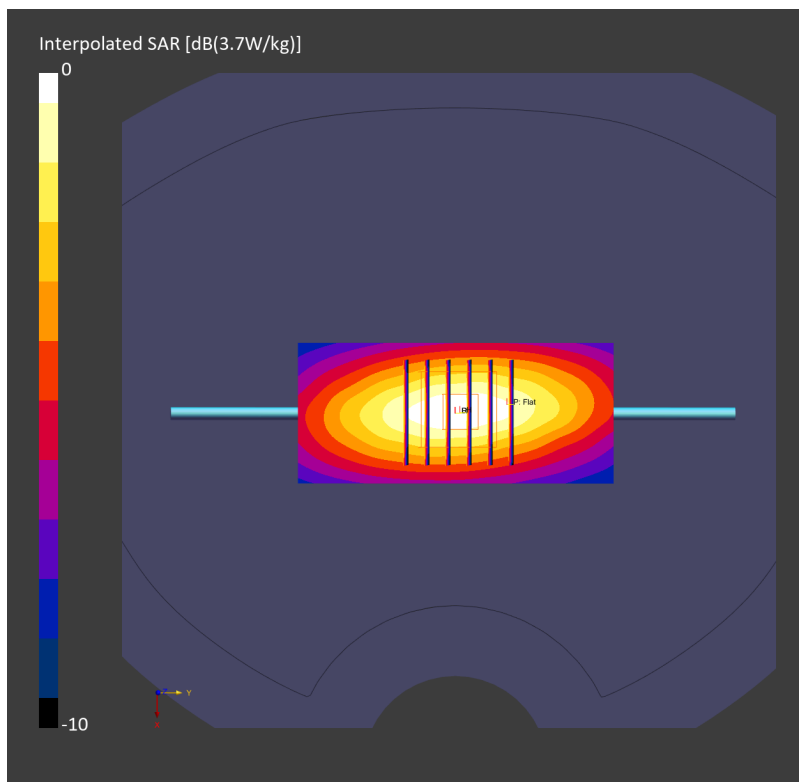

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.933$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(9.51, 10.14, 9.57); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.496 W/kg; SAR (10g) = 0.326 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 0.500 W/kg; SAR (8g) = 0.351 W/kg; SAR (10g) = 0.333 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

TSL Correction: Positive only

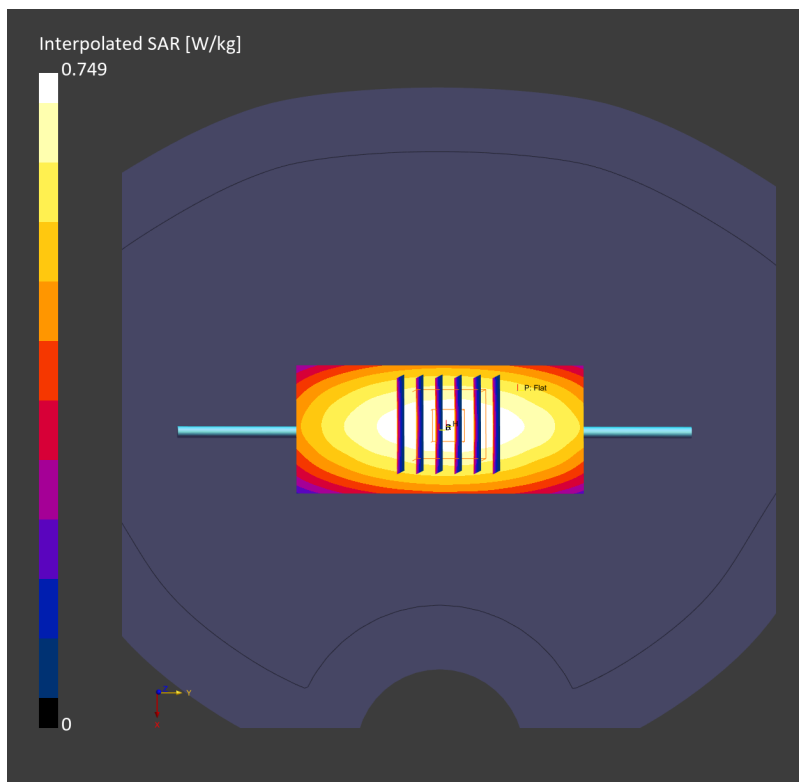

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.938$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.82, 9.12, 9.75); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.58 W/kg; SAR (10g) = 1.69 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.57 W/kg; SAR (8g) = 1.80 W/kg; SAR (10g) = 1.71 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

TSL Correction: Positive only

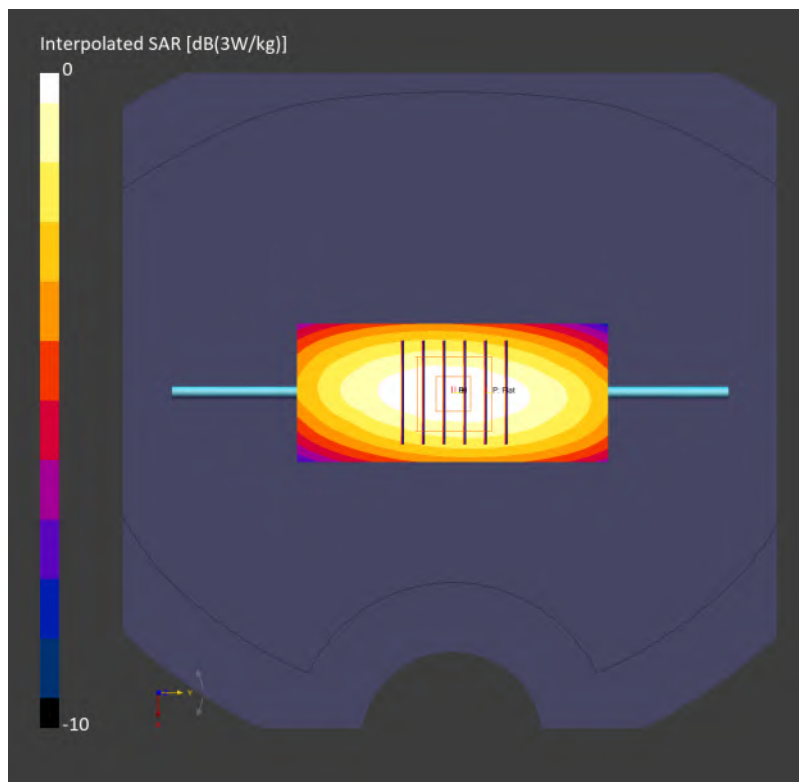

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.913$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(9.51, 10.14, 9.57); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.477 W/kg; SAR (10g) = 0.313 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 0.481 W/kg; SAR (8g) = 0.338 W/kg; SAR (10g) = 0.321 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

TSL Correction: Positive only

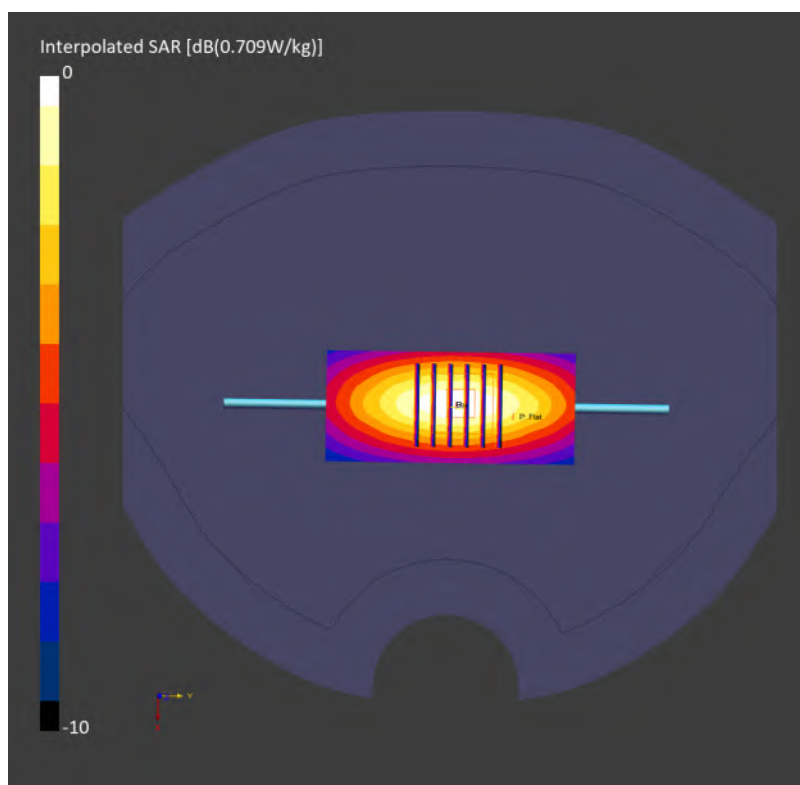

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.949$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.82, 9.12, 9.75); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.63 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.45 W/kg; SAR (8g) = 1.73 W/kg; SAR (10g) = 1.64 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

TSL Correction: Positive only

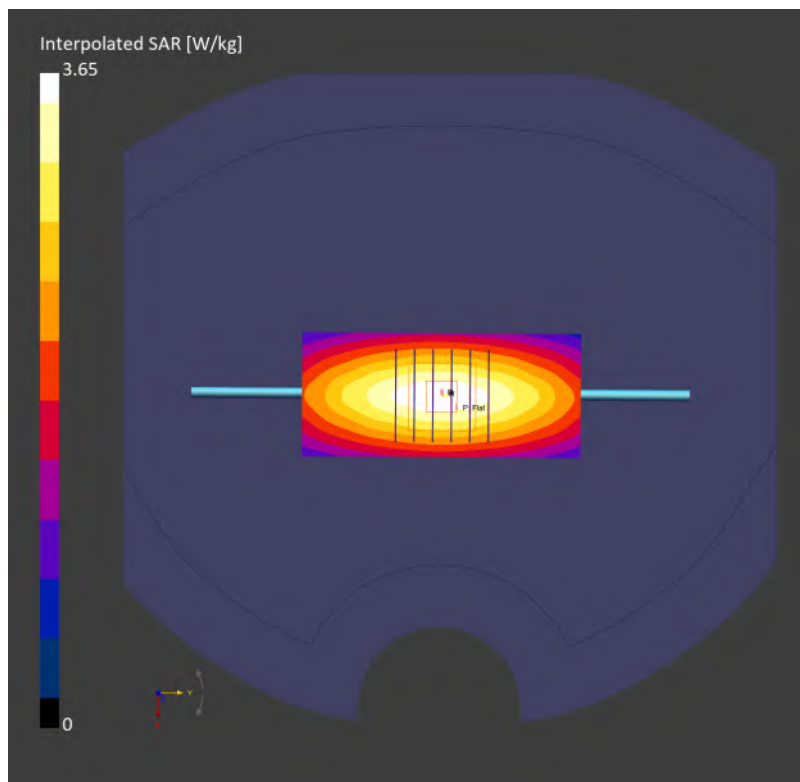

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.928$ S/m; $\epsilon_r = 44.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(9.51, 10.14, 9.57); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.30 W/kg; SAR (10g) = 1.51 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.04 dB

SAR (1g) = 2.33 W/kg; SAR (8g) = 1.65 W/kg; SAR (10g) = 1.57 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 88.0 %

TSL Correction: Positive only

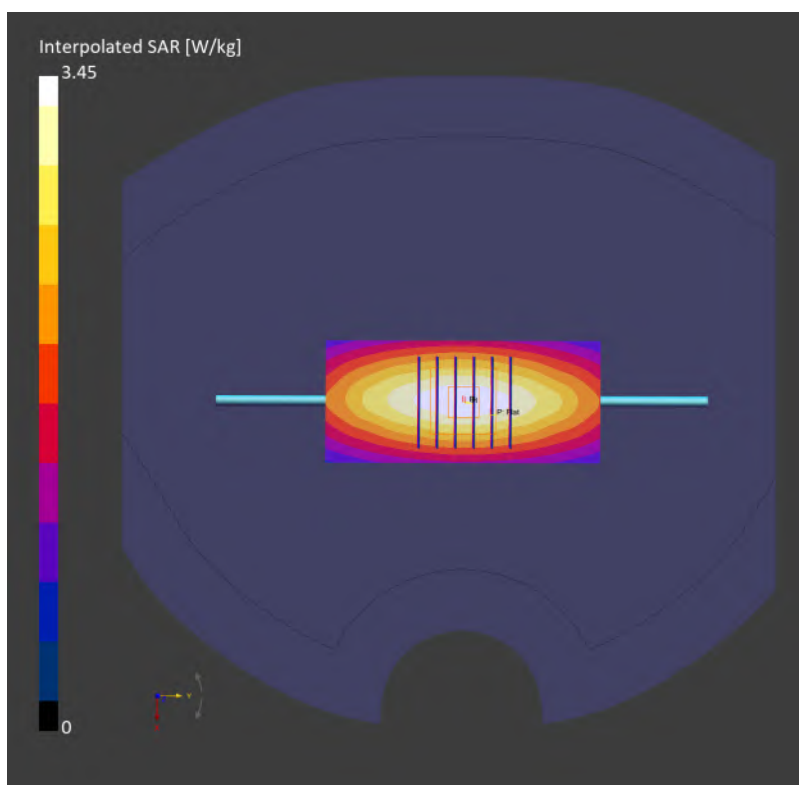

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260819 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.25, 7.66, 8.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.84 W/kg; SAR (10g) = 0.976 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.81 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.973 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

TSL Correction: Positive only

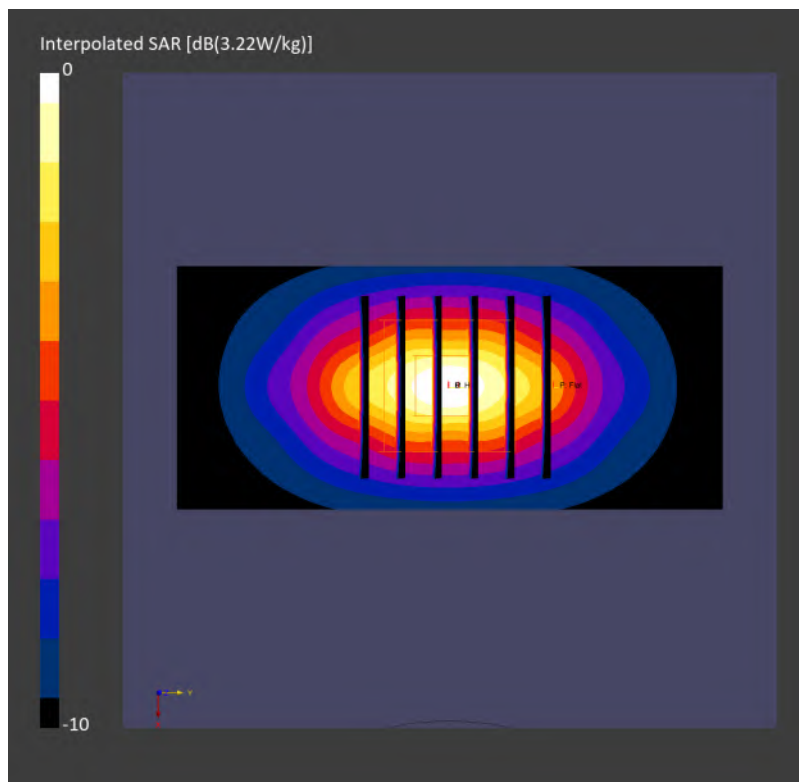

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260819 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.42, 8.01, 7.32); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.85 W/kg; SAR (10g) = 4.73 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 8.74 W/kg; SAR (8g) = 5.07 W/kg; SAR (10g) = 4.68 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.2 %

TSL Correction: Positive only

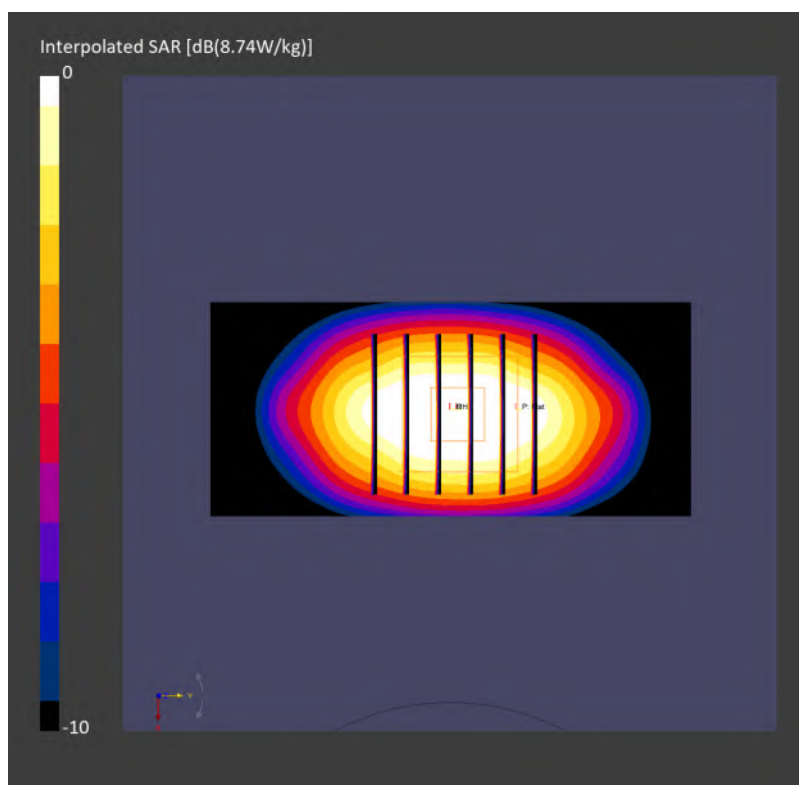

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260821 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(8.12, 8.25, 7.9); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.33 W/kg; SAR (10g) = 4.48 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 8.55 W/kg; SAR (8g) = 5.10 W/kg; SAR (10g) = 4.73 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

TSL Correction: Positive only

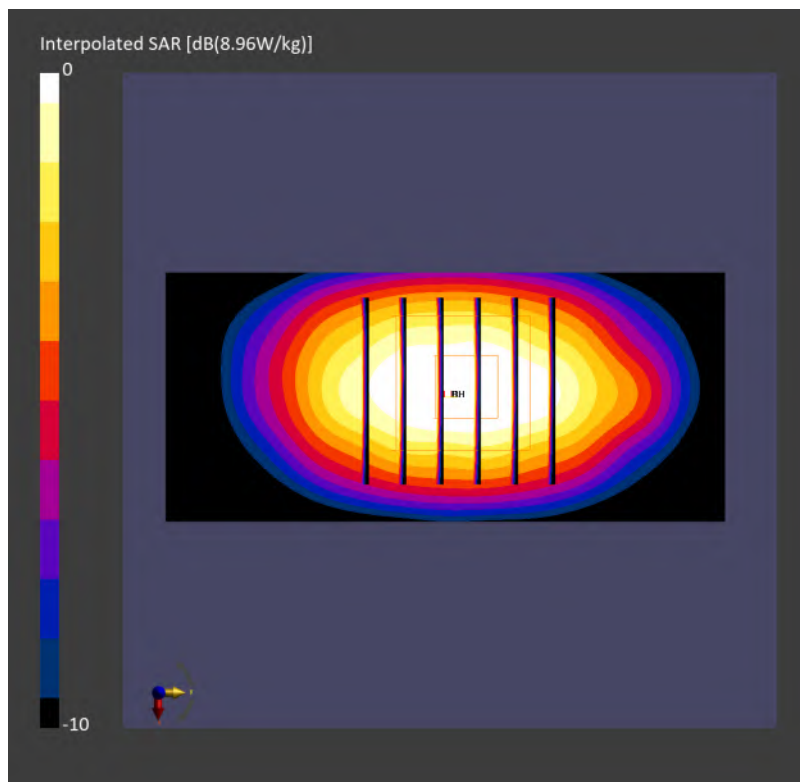

System Check_Head 1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260822 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.89, 8.41, 7.94); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.83 W/kg; SAR (10g) = 4.69 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 8.82 W/kg; SAR (8g) = 5.16 W/kg; SAR (10g) = 4.78 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.1 %

TSL Correction: Positive only

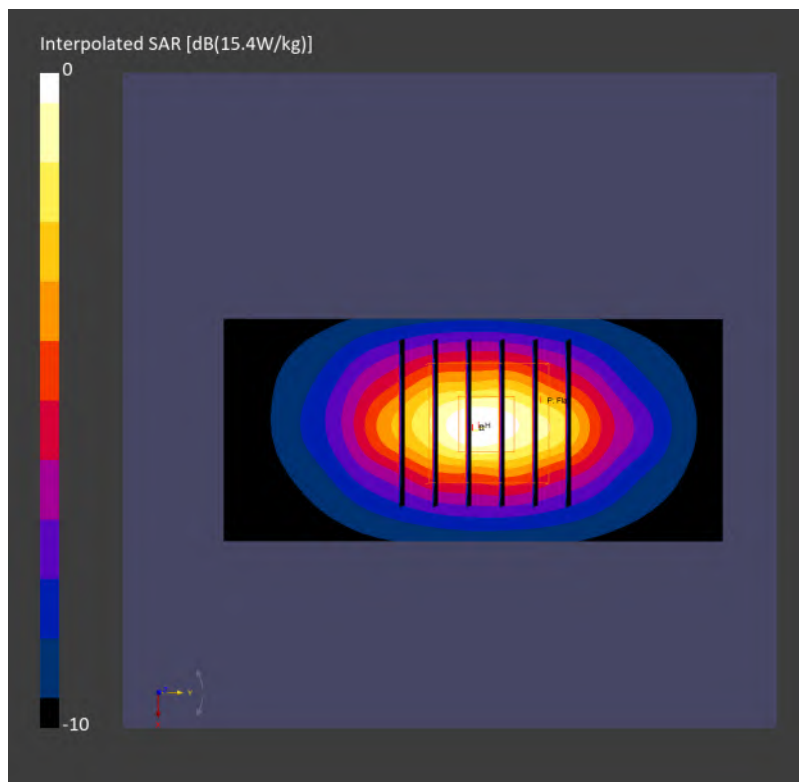

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.3, 5.21, 5.09); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.943 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.75 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.930 W/kg

Smallest distance from peaks to all points 3 dB below = 11.4 mm

Ratio of SAR at M2 to SAR at M1 = 83.7 %

TSL Correction: Positive only

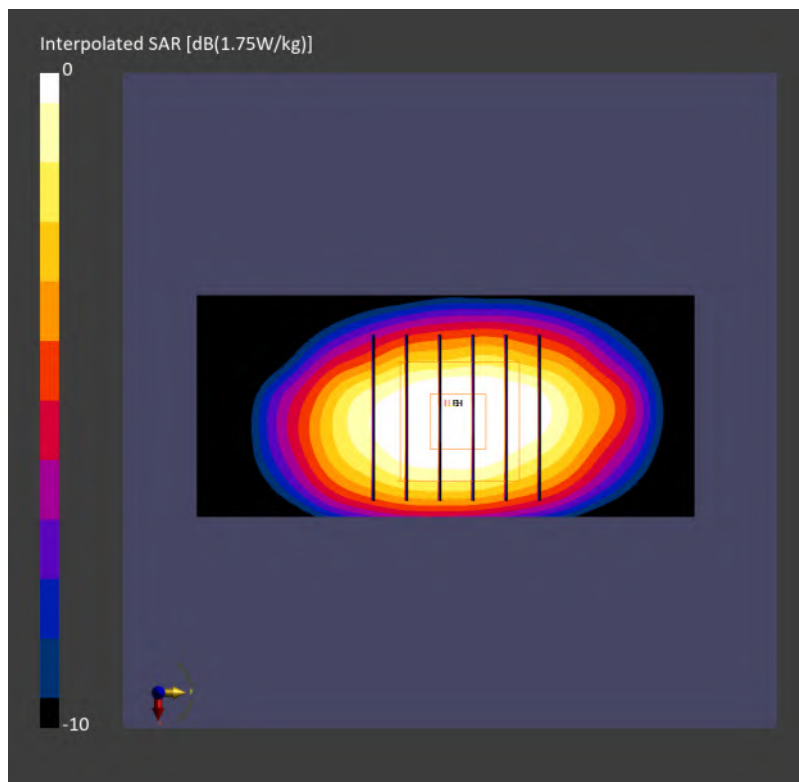

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.32$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.3, 5.21, 5.09); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.73 W/kg; SAR (10g) = 0.930 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.73 W/kg; SAR (8g) = 0.994 W/kg; SAR (10g) = 0.918 W/kg

Smallest distance from peaks to all points 3 dB below = 11.4 mm

Ratio of SAR at M2 to SAR at M1 = 83.7 %

TSL Correction: Positive only

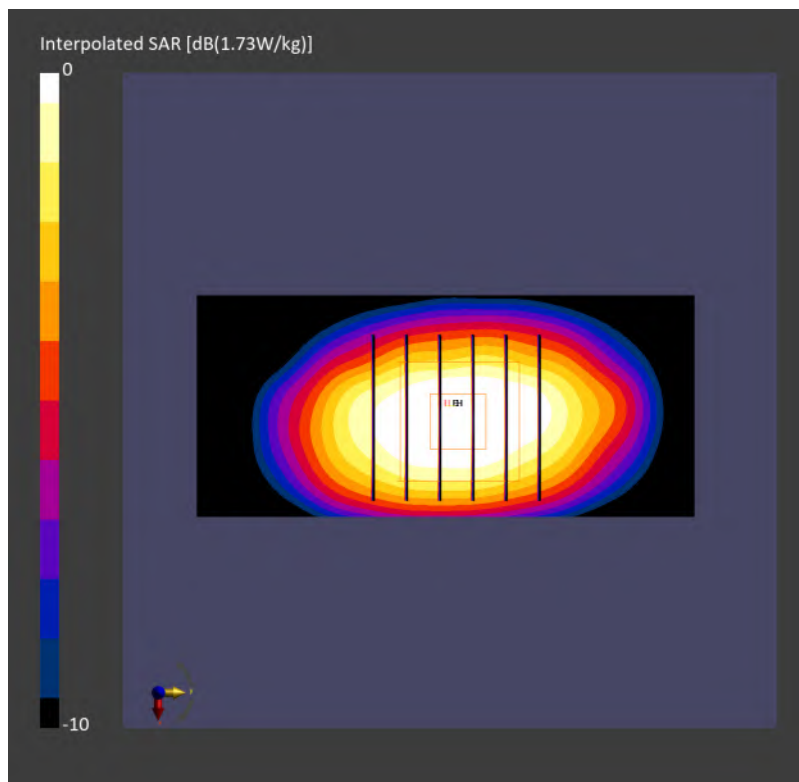

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260826 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.31$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.3, 5.21, 5.09); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.73 W/kg; SAR (10g) = 0.926 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.72 W/kg; SAR (8g) = 0.990 W/kg; SAR (10g) = 0.914 W/kg

Smallest distance from peaks to all points 3 dB below = 11.4 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

TSL Correction: Positive only

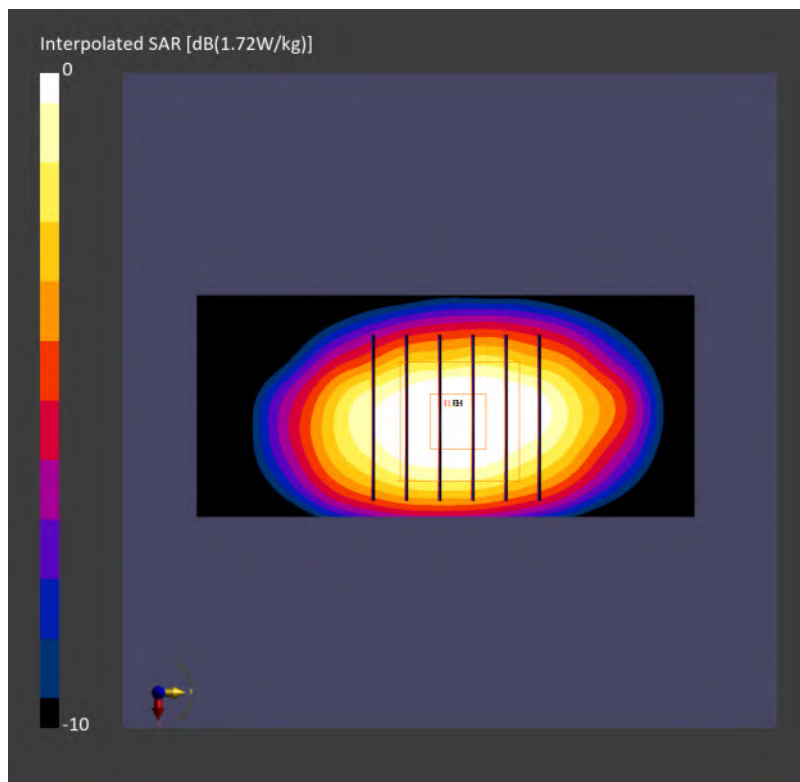

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260826 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.25, 7.66, 8.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.83 W/kg; SAR (10g) = 0.967 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.80 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.963 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

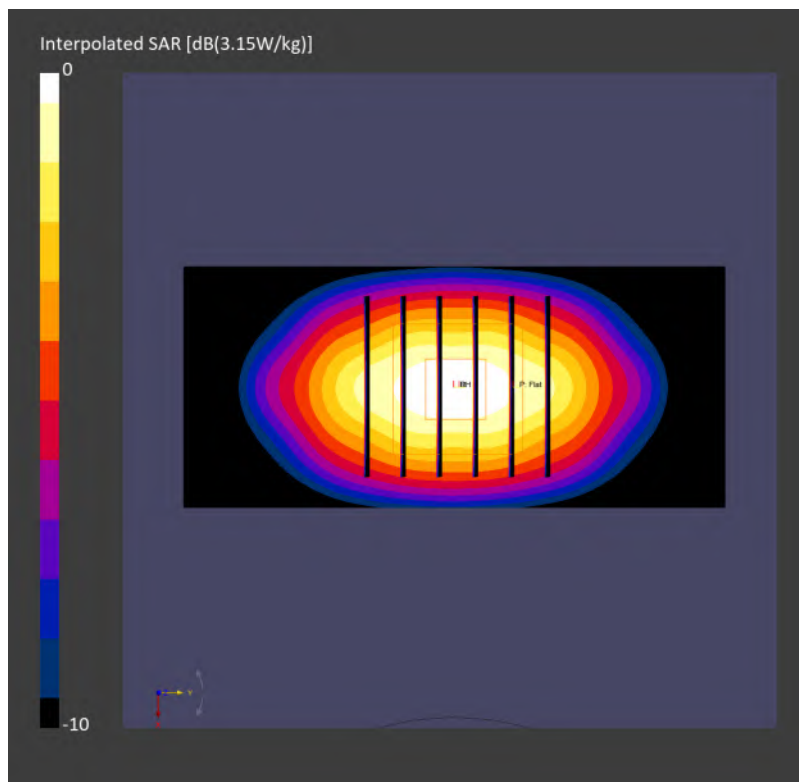

System Check_Head 1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260826 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.89, 8.41, 7.94); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.942 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.959 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.4 %

TSL Correction: Positive only

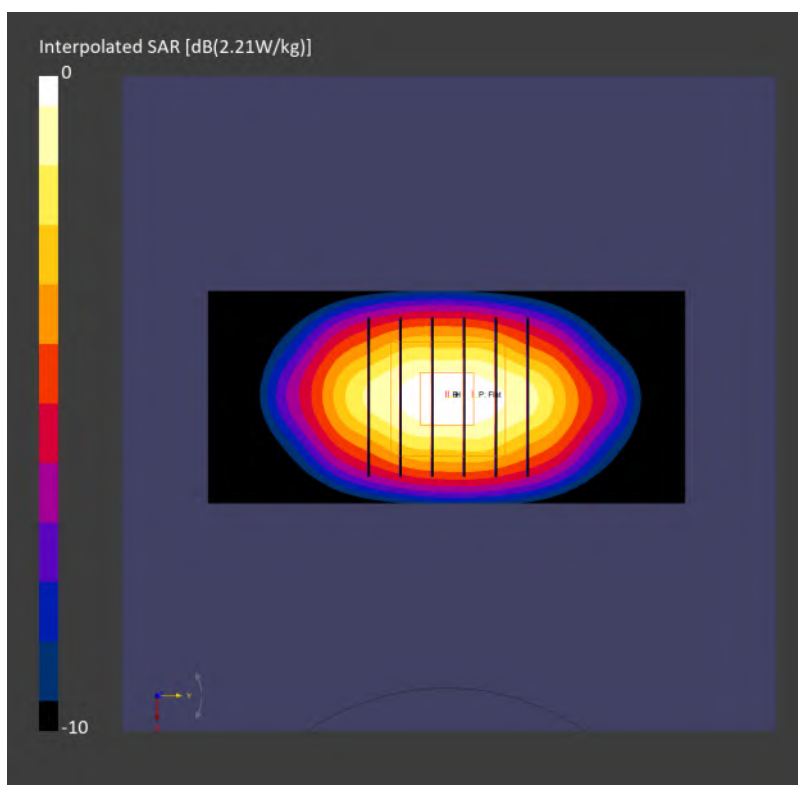

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.33$ S/m; $\epsilon_r = 41.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.3, 5.21, 5.09); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.942 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.75 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.928 W/kg

Smallest distance from peaks to all points 3 dB below = 11.4 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

TSL Correction: Positive only

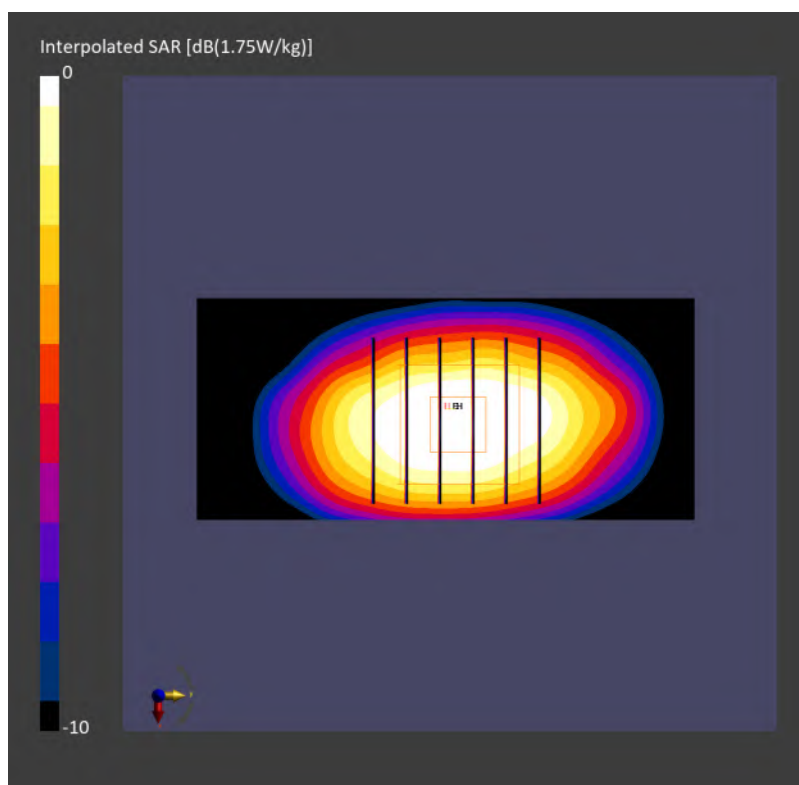

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.29$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.3, 5.21, 5.09); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.71 W/kg; SAR (10g) = 0.917 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.71 W/kg; SAR (8g) = 0.980 W/kg; SAR (10g) = 0.905 W/kg

Smallest distance from peaks to all points 3 dB below = 11.4 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

TSL Correction: Positive only

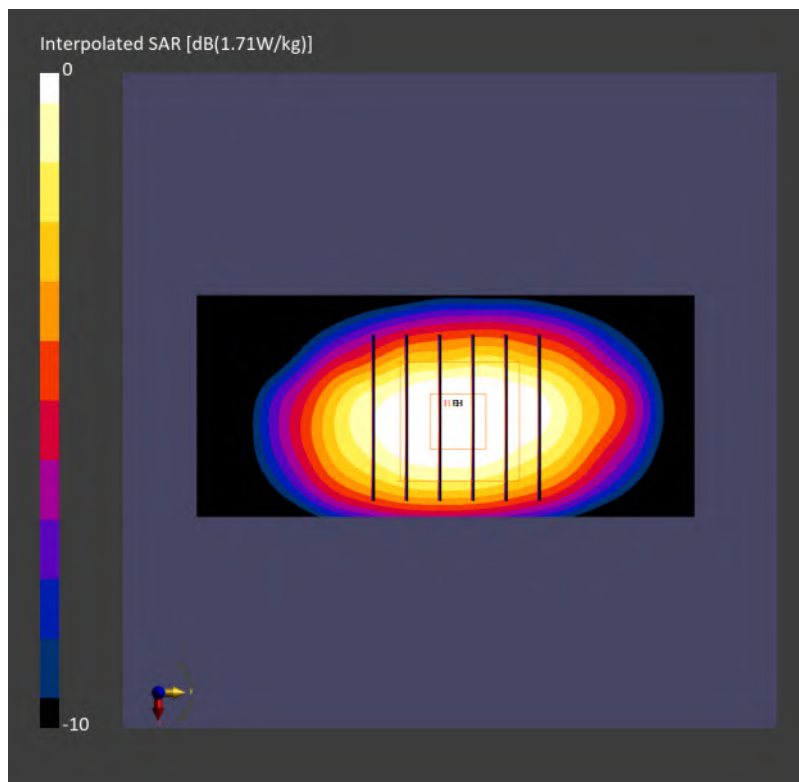

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.3, 5.21, 5.09); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.943 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.75 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.932 W/kg

Smallest distance from peaks to all points 3 dB below = 11.4 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

TSL Correction: Positive only

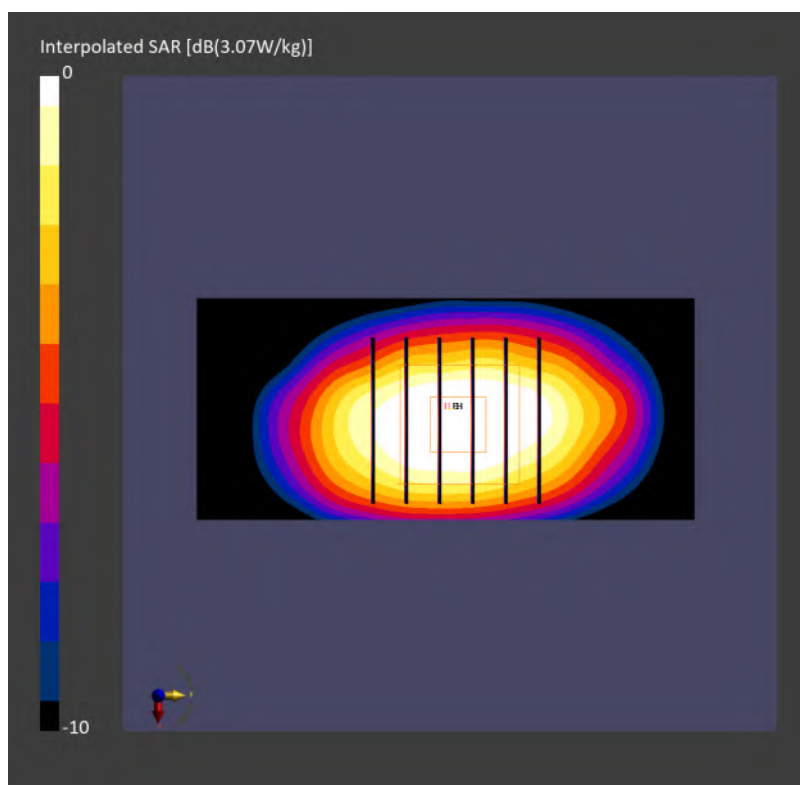

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.3, 5.21, 5.09); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.948 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.76 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.937 W/kg

Smallest distance from peaks to all points 3 dB below = 11.4 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

TSL Correction: Positive only

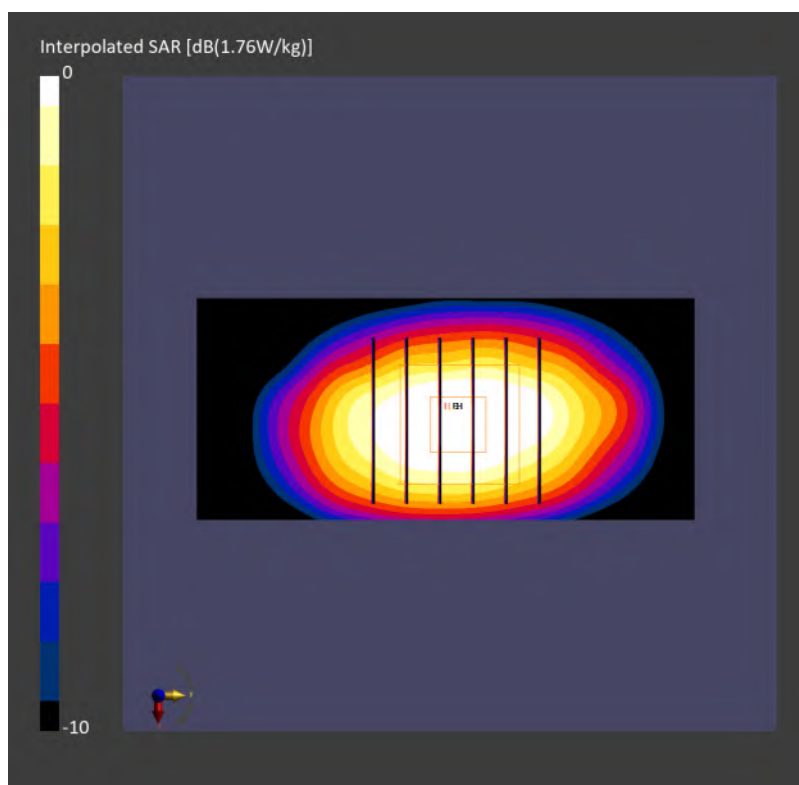

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.25, 7.66, 8.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.81 W/kg; SAR (10g) = 0.958 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.952 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

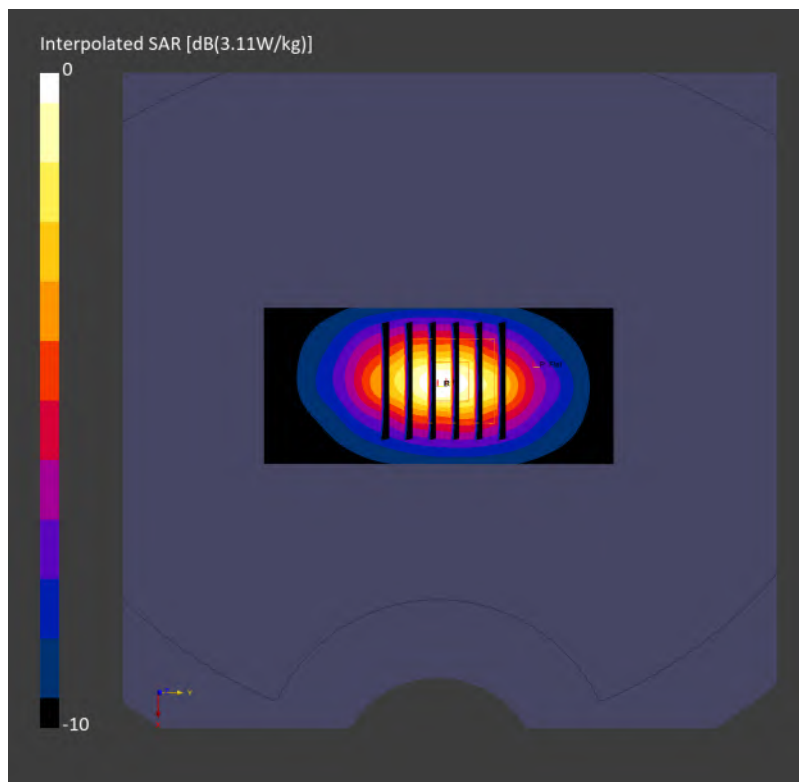

System Check_Head_1750MHz**DUT: D1750V2 - SN1120**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.3, 5.21, 5.09); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.76 W/kg; SAR (10g) = 0.951 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.76 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.938 W/kg

Smallest distance from peaks to all points 3 dB below = 11.4 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

TSL Correction: Positive only

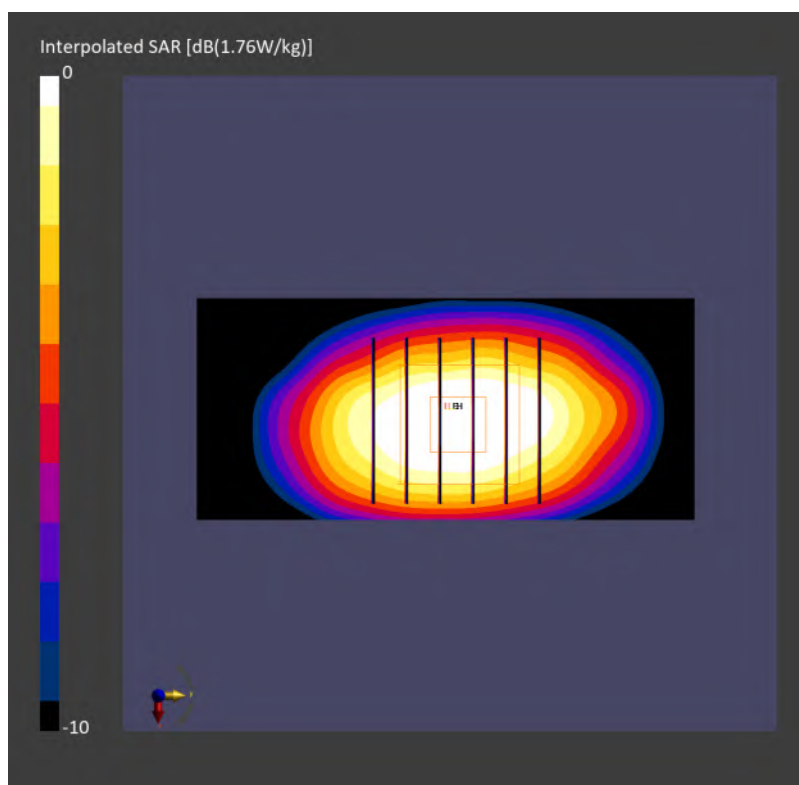

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260901 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.25, 7.66, 8.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.79 W/kg; SAR (10g) = 0.954 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.77 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.947 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

TSL Correction: Positive only

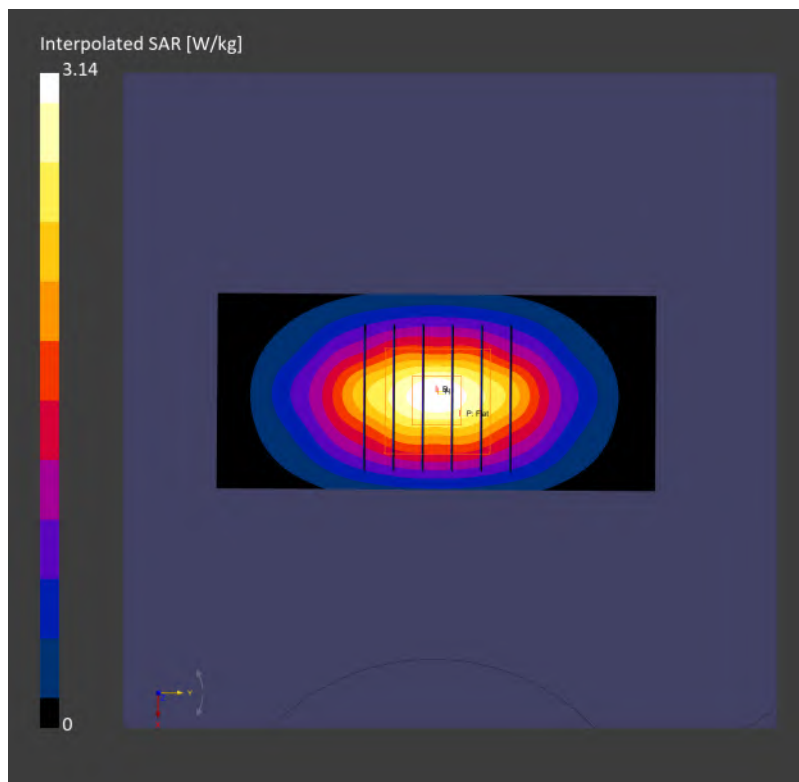

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260901 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.89, 8.41, 7.94); Calibrated: 2026-01-27

- Sensor-Surface: 1.4 mm

- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13

- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat

- Measurement Software: 18.0.0.7250

- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.73 W/kg; SAR (10g) = 0.920 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.74 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.936 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

TSL Correction: Positive only

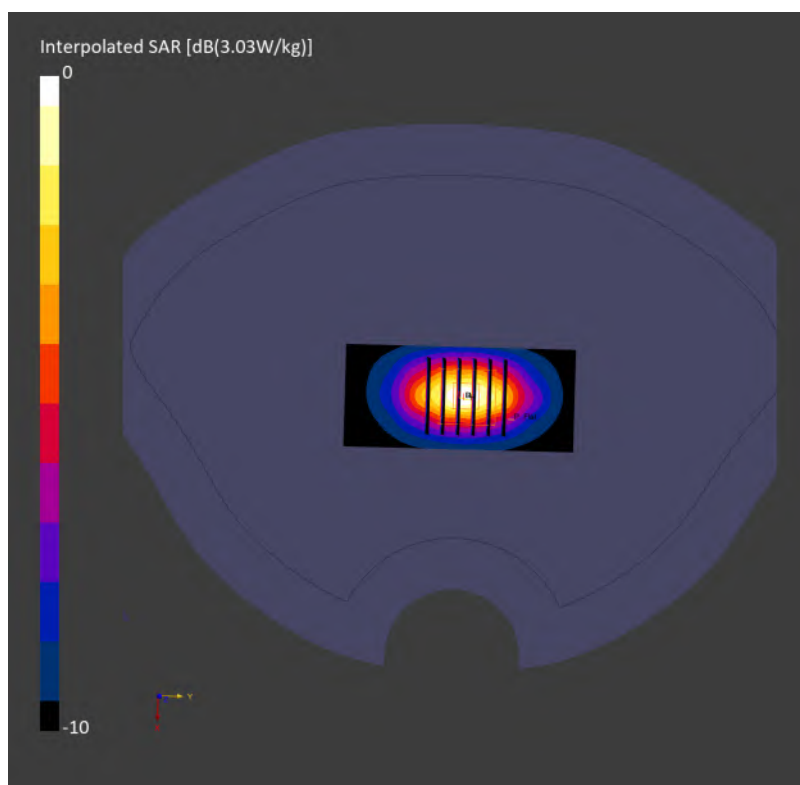

System Check_Head 1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.89, 8.41, 7.94); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.942 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.04 dB

SAR (1g) = 1.80 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.976 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.1 %

TSL Correction: Positive only

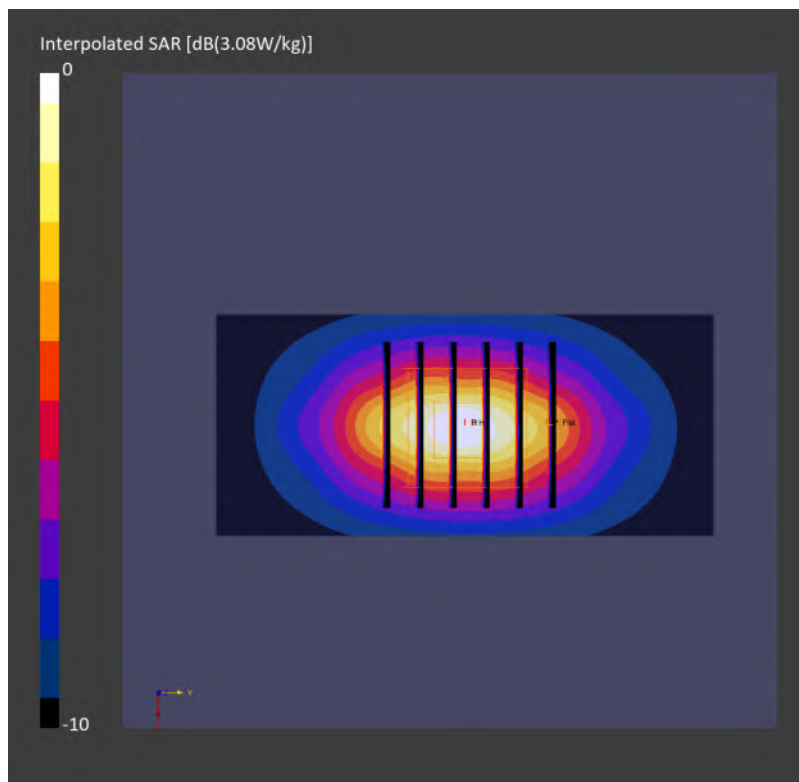

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260819 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.05 W/kg; SAR (10g) = 1.05 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.02 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.9 %

TSL Correction: Positive only

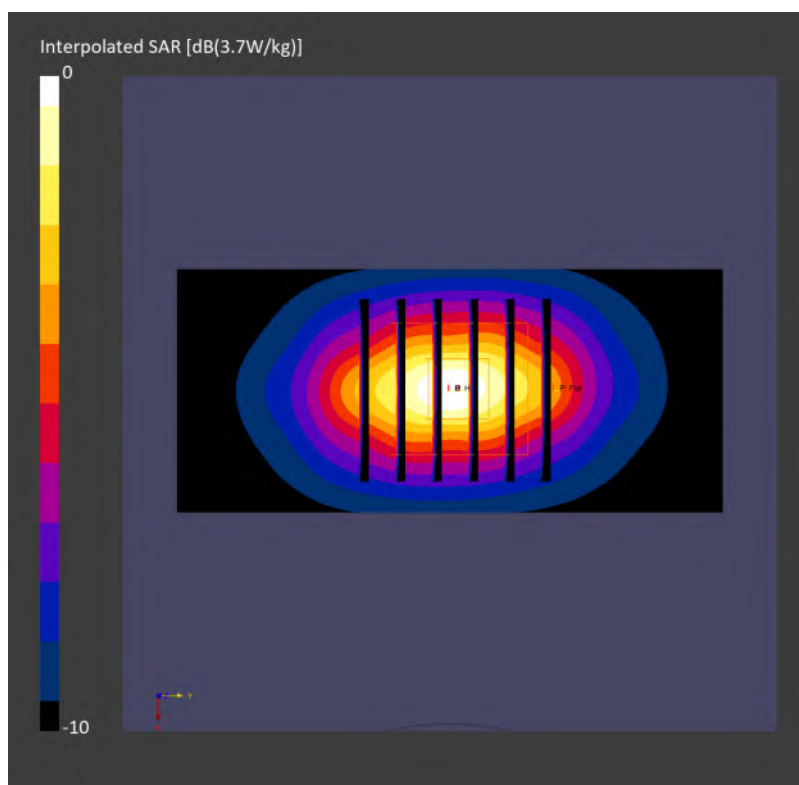

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260819 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.02, 7.58, 6.92); Calibrated: 2026-02-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2026-03-11
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.2 W/kg; SAR (10g) = 5.40 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 10.2 W/kg; SAR (8g) = 5.81 W/kg; SAR (10g) = 5.35 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.7 %

TSL Correction: Positive only

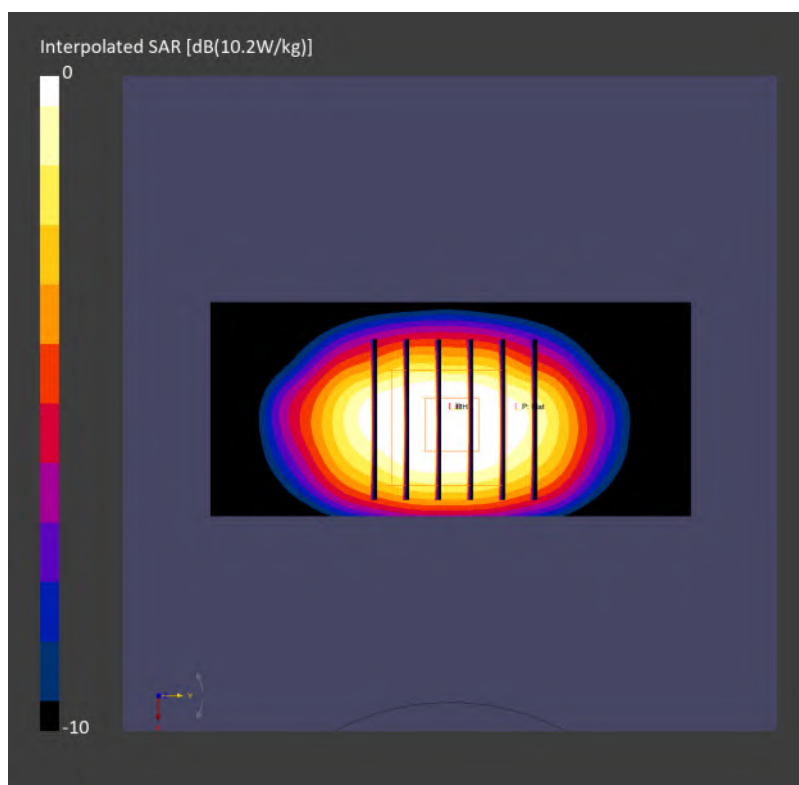

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260821 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.72, 7.85, 7.52); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.72 W/kg; SAR (10g) = 5.08 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 9.99 W/kg; SAR (8g) = 5.83 W/kg; SAR (10g) = 5.39 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

TSL Correction: Positive only

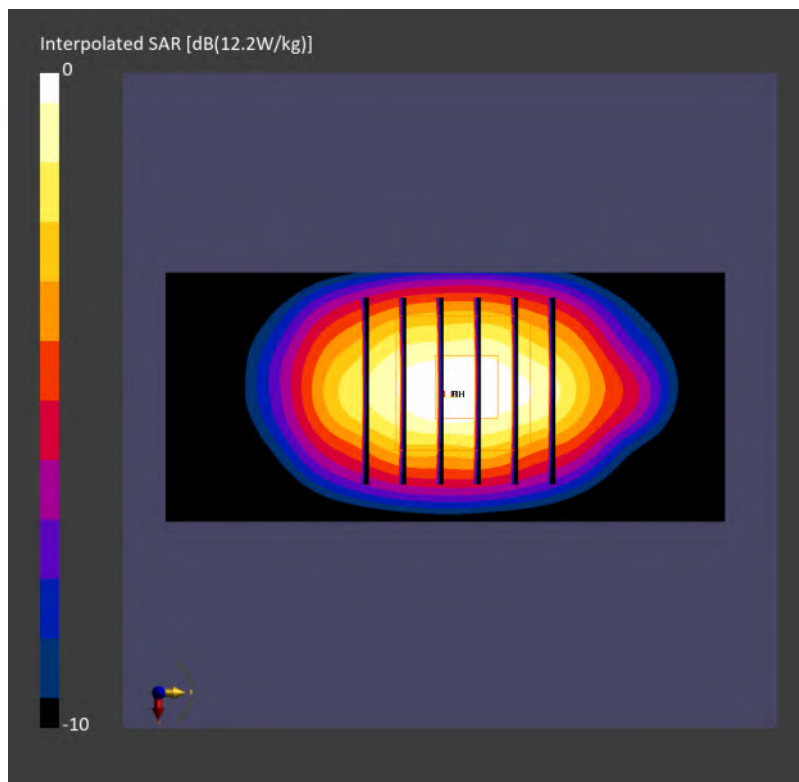

System Check_Head 1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260822 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.64, 8.14, 7.69); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.0 W/kg; SAR (10g) = 5.16 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 10.0 W/kg; SAR (8g) = 5.73 W/kg; SAR (10g) = 5.28 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.9 %

TSL Correction: Positive only

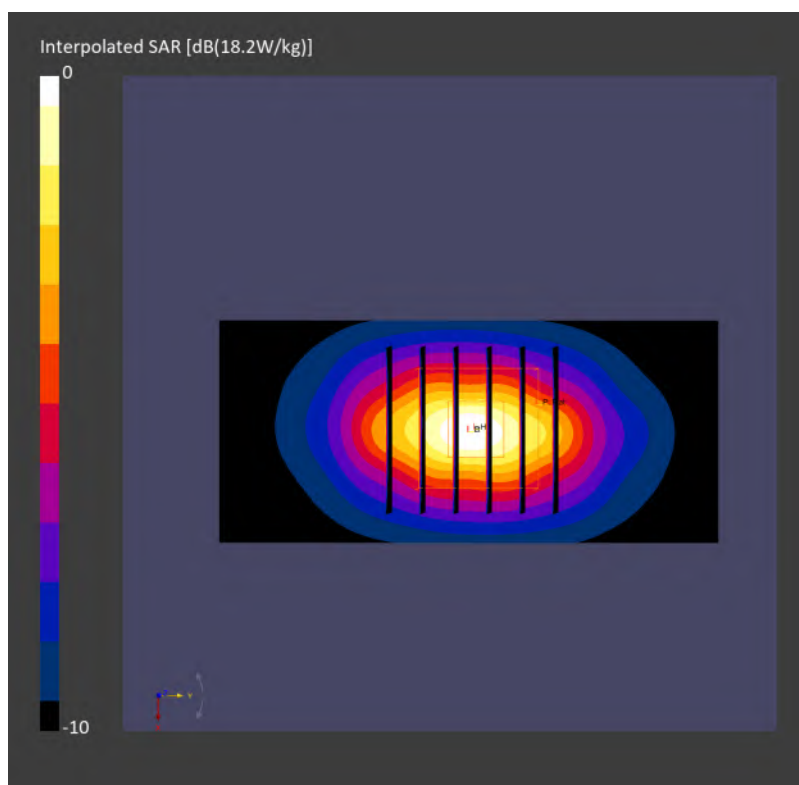

System Check_Head 1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260826 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.64, 8.14, 7.69); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 0.998 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.94 W/kg; SAR (8g) = 1.11 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.3 %

TSL Correction: Positive only

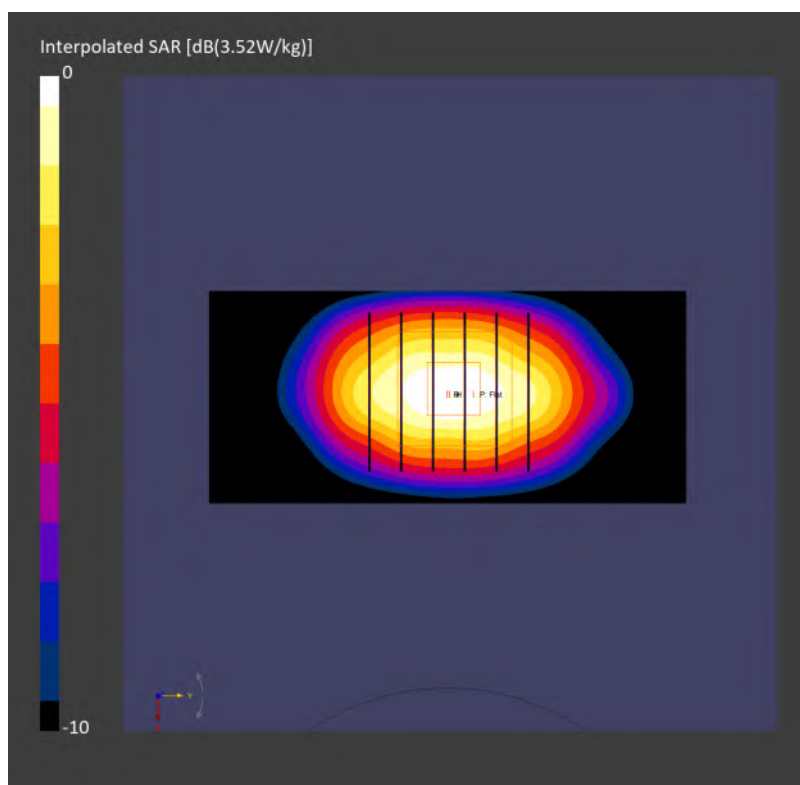

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260826 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.03 W/kg; SAR (10g) = 1.04 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.99 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

TSL Correction: Positive only

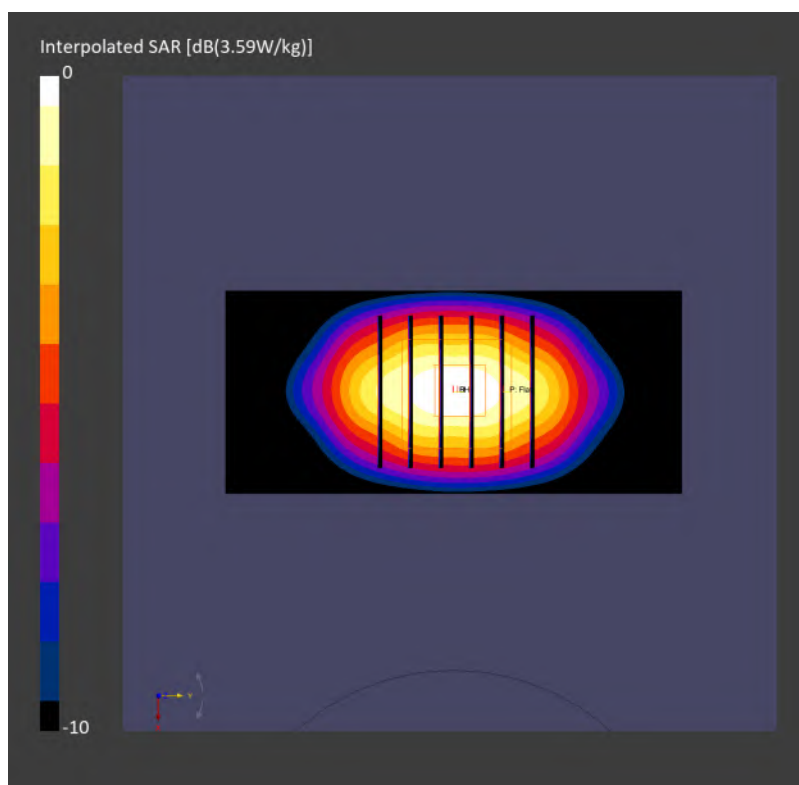

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.97 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 1.96 W/kg; SAR (8g) = 1.11 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.9 %

TSL Correction: Positive only

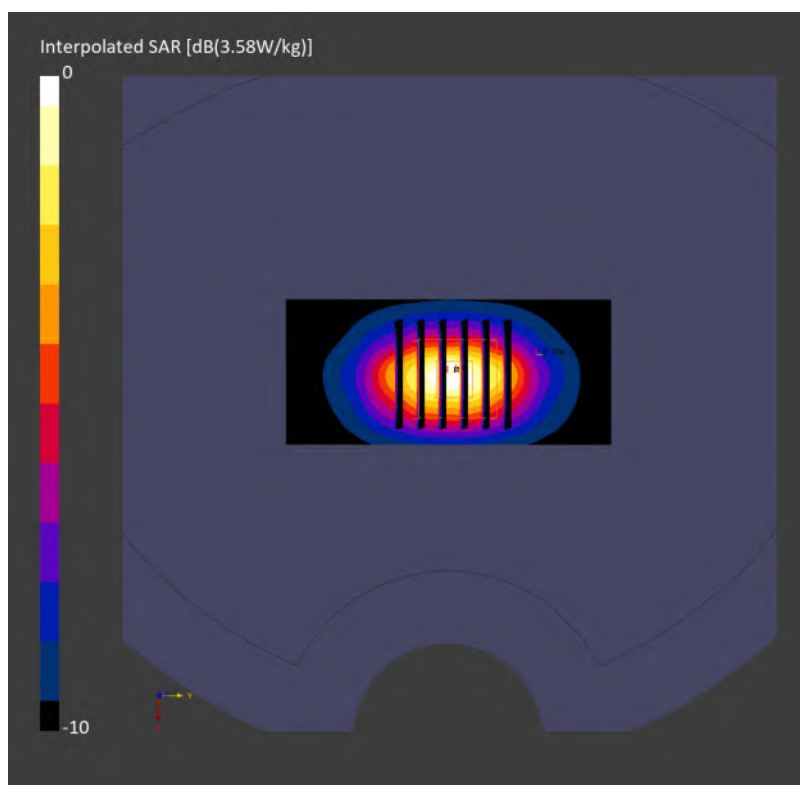

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260901 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 43.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.18, 5.08, 4.96); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.90 W/kg; SAR (10g) = 0.983 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 1.88 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.977 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.1 %

TSL Correction: Positive only

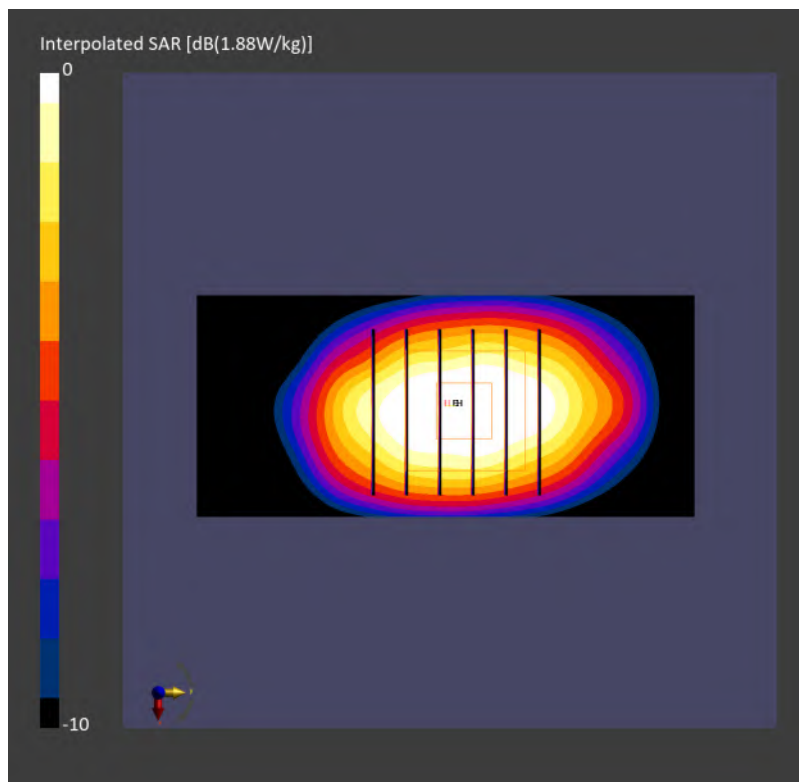

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260901 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.44$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.97, 7.4, 7.91); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.03 W/kg; SAR (10g) = 1.04 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.00 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

TSL Correction: Positive only

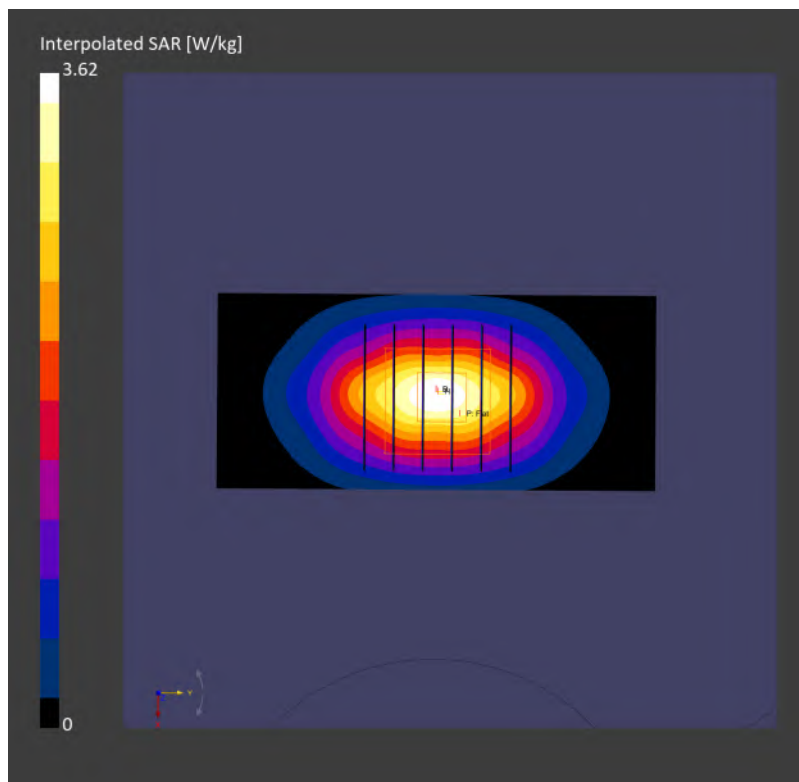

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260901 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 41.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.64, 8.14, 7.69); Calibrated: 2026-01-27

- Sensor-Surface: 1.4 mm

- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13

- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat

- Measurement Software: 18.0.0.7250

- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 0.961 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 1.88 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.989 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

TSL Correction: Positive only

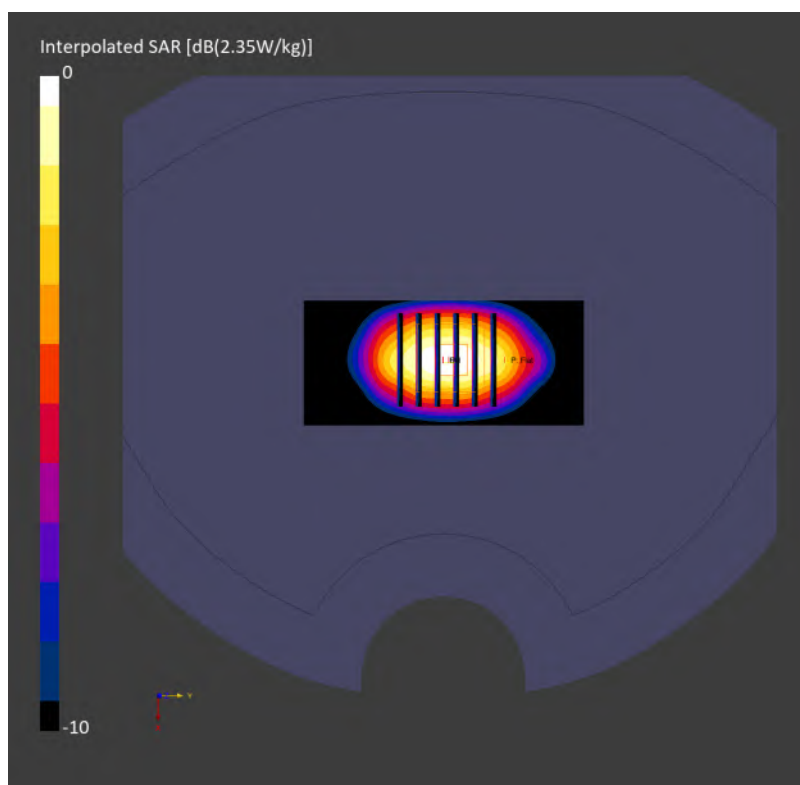

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.18, 5.08, 4.96); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.979 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.86 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.970 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.1 %

TSL Correction: Positive only

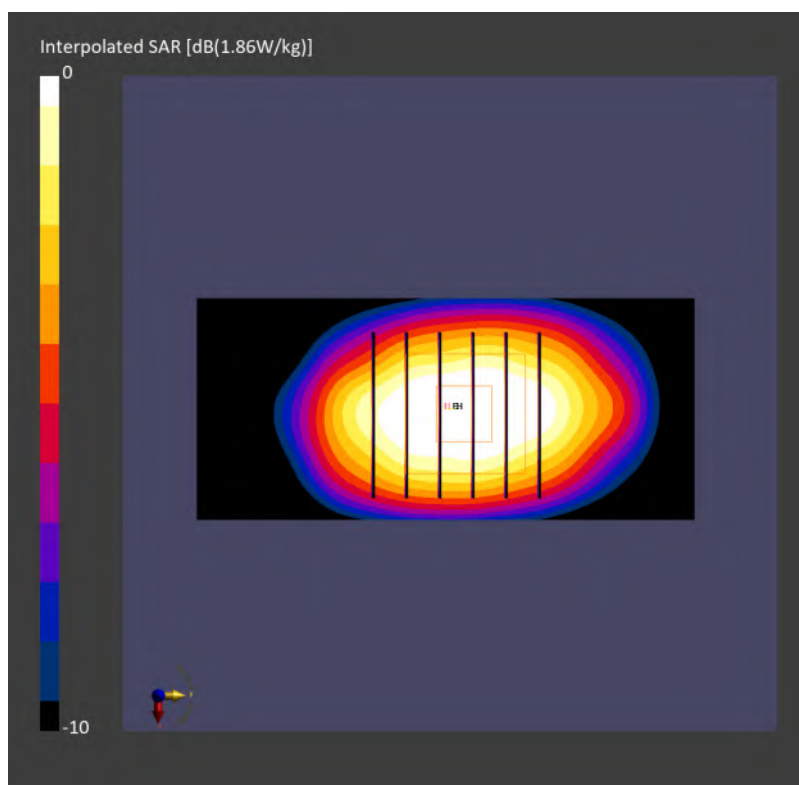

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.51$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.18, 5.08, 4.96); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.99 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.96 W/kg; SAR (8g) = 1.11 W/kg; SAR (10g) = 1.02 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.0 %

TSL Correction: Positive only

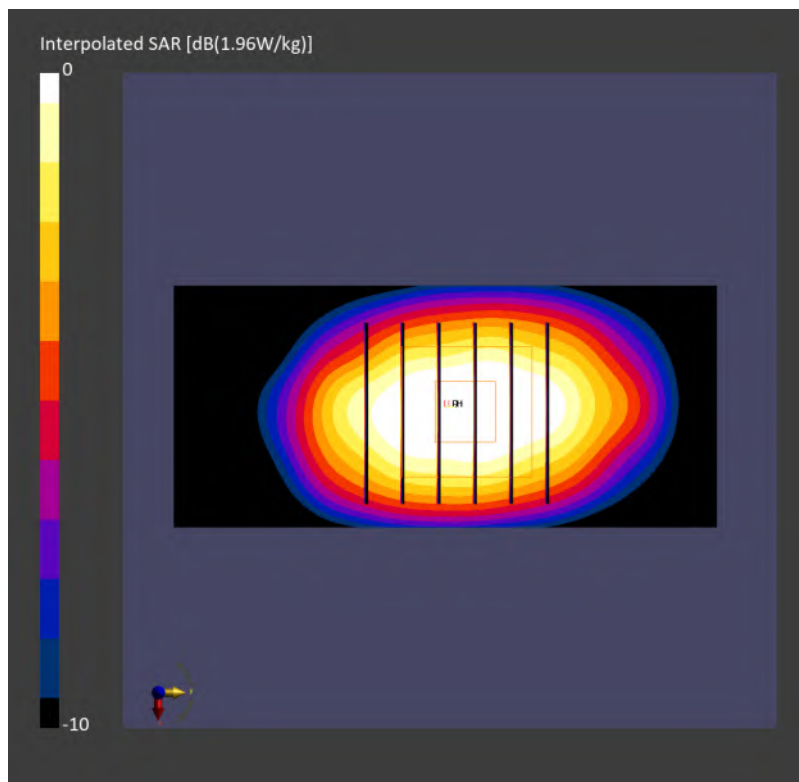

System Check_Head 1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 42.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.64, 8.14, 7.69); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.98 W/kg; SAR (10g) = 1.02 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.01 W/kg; SAR (8g) = 1.16 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

TSL Correction: Positive only

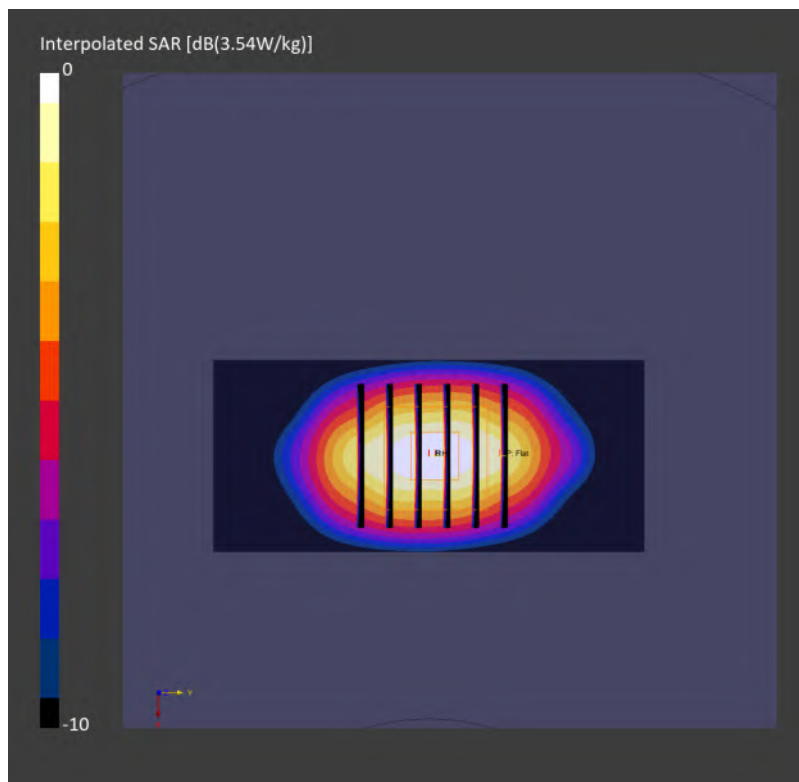

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(5.18, 5.08, 4.96); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 0.993 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 1.89 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.984 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 84.0 %

TSL Correction: Positive only

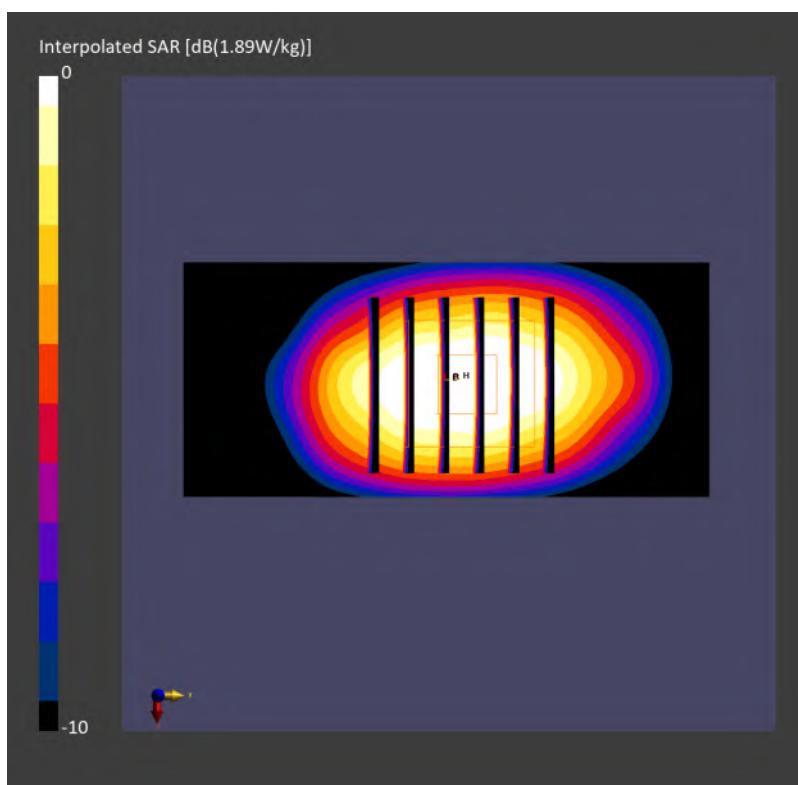

System Check_Head_1900MHz

DUT: D1900V2 - SN5d041

Communication System: UID 0, CW ; Frequency: 1900 MHz

Medium: HSL_600~7200_260918 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.474$ S/m; $\epsilon_r = 39.819$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.49, 7.97, 7.84) @ 1900 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (61x61x1): Interpolated grid: $dx=1.500$ mm, $dy=1.500$ mm

Maximum value of SAR (interpolated) = 16.4 W/kg

Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm


Reference Value = 110.8 V/m; Power Drift = -0.01 dBPeak SAR (extrapolated) = 19.0 W/kg

SAR(1 g) = 10.3 W/kg; SAR(10 g) = 5.38 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 55.7%

Maximum value of SAR (measured) = 16.4 W/kg

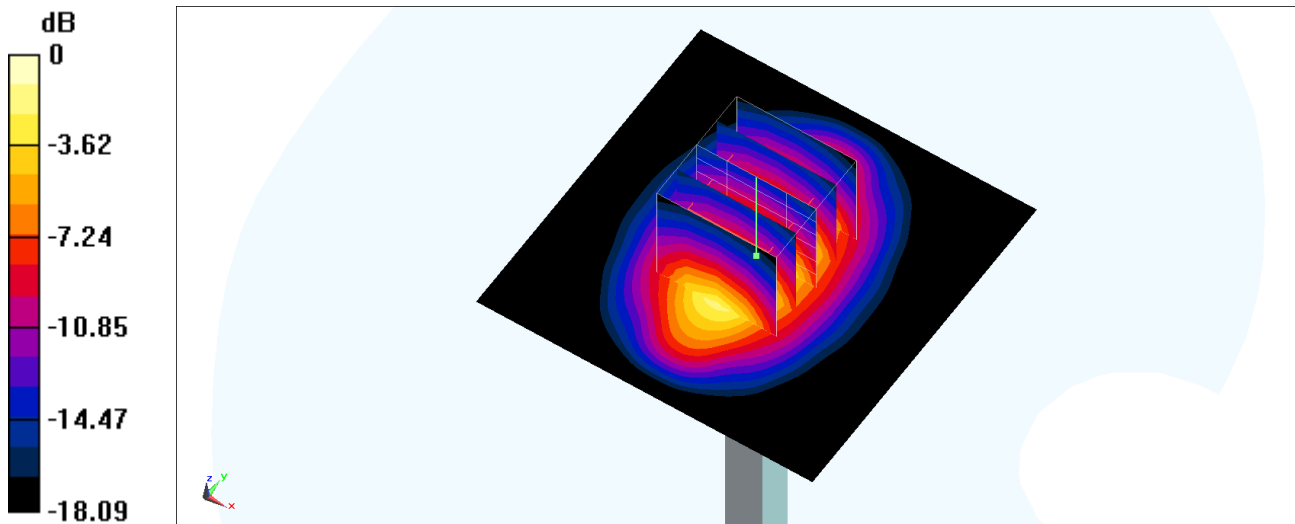

0 dB = 16.4 W/kg = 12.15 dBW/kg

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260820 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.71$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

TSL Correction: Positive only

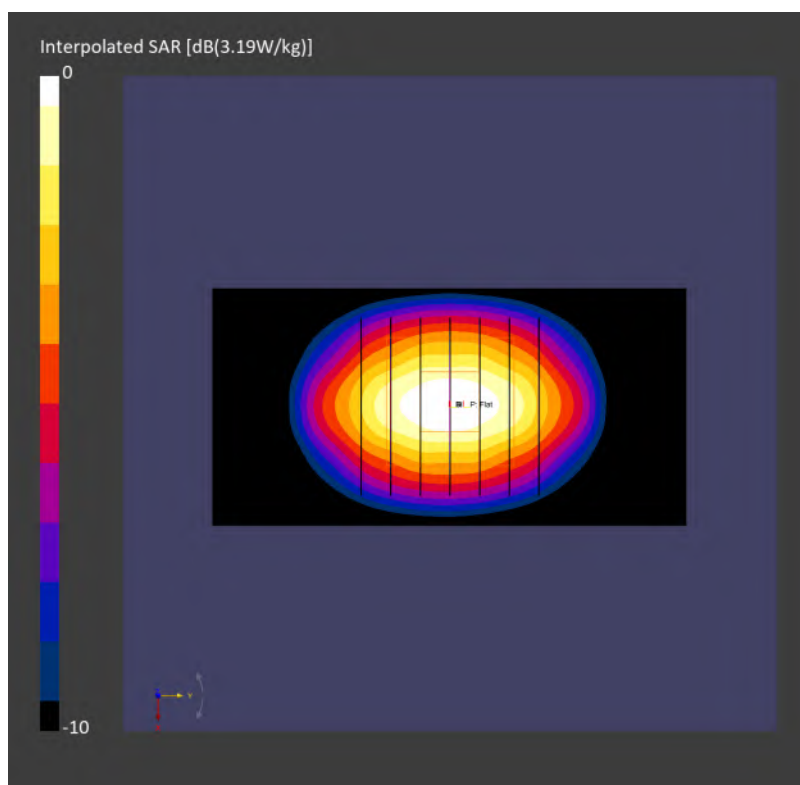

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260822 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.72$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.28, 7.41, 7.09); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.0 W/kg; SAR (10g) = 5.75 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 12.3 W/kg; SAR (8g) = 6.69 W/kg; SAR (10g) = 6.11 W/kg

Smallest distance from peaks to all points 3 dB below = 9.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

TSL Correction: Positive only

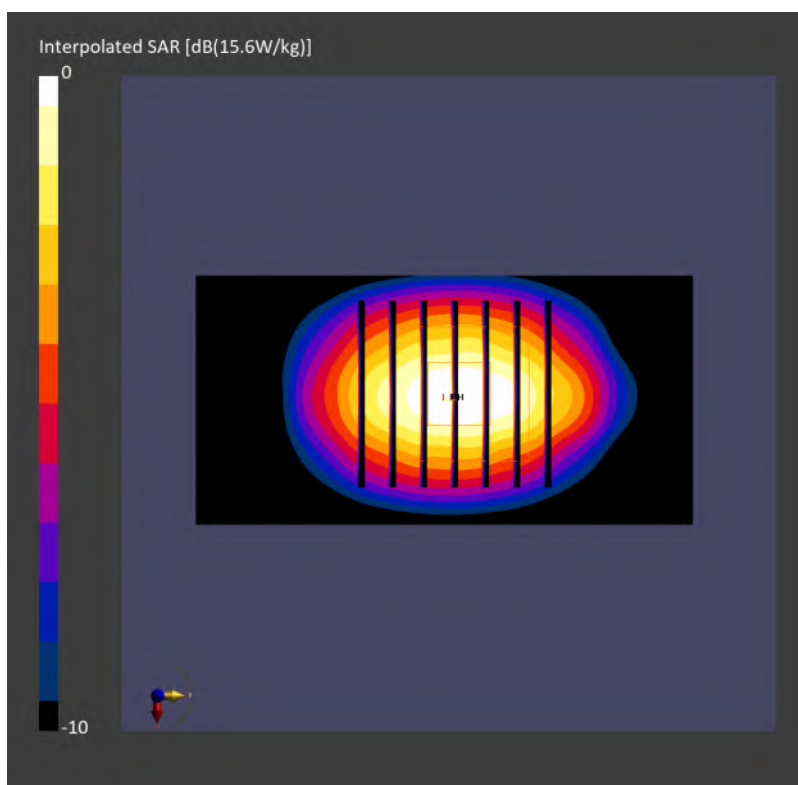

System Check_Head 2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260823 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.72$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.35, 7.83, 7.39); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.3 W/kg; SAR (10g) = 5.79 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 12.3 W/kg; SAR (8g) = 6.51 W/kg; SAR (10g) = 5.93 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.8 %

TSL Correction: Positive only

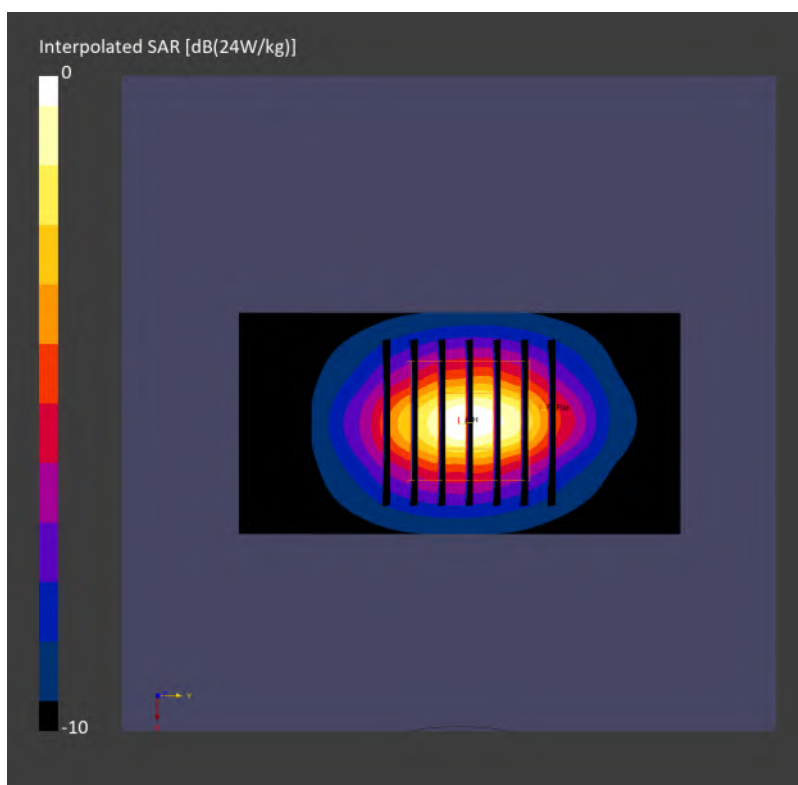

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.71$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.8 W/kg; SAR (10g) = 6.04 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 12.6 W/kg; SAR (8g) = 6.68 W/kg; SAR (10g) = 6.08 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

TSL Correction: Positive only

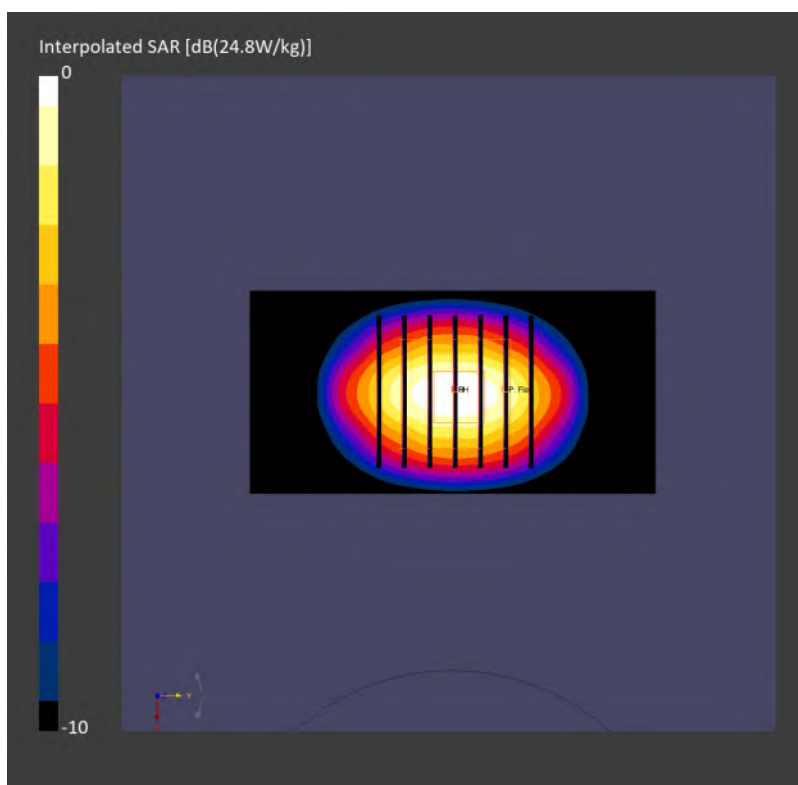

System Check_Head 2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.76$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.35, 7.83, 7.39); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.36 W/kg; SAR (10g) = 1.11 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.04 dB

SAR (1g) = 2.38 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.2 %

TSL Correction: Positive only

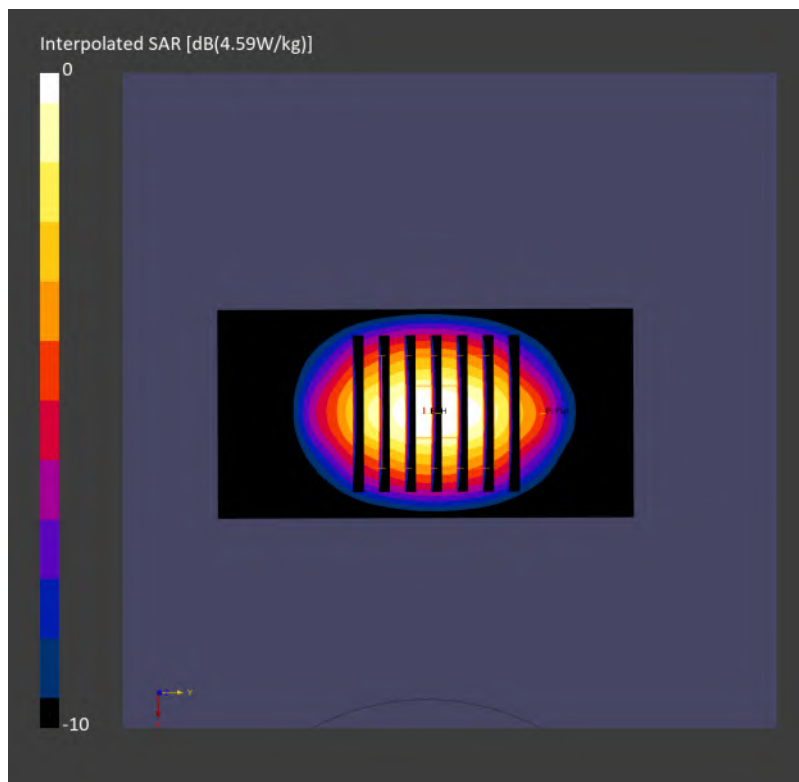

System Check_Head 2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.73$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.35, 7.83, 7.39); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.35 W/kg; SAR (10g) = 1.11 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.34 W/kg; SAR (8g) = 1.24 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

TSL Correction: Positive only

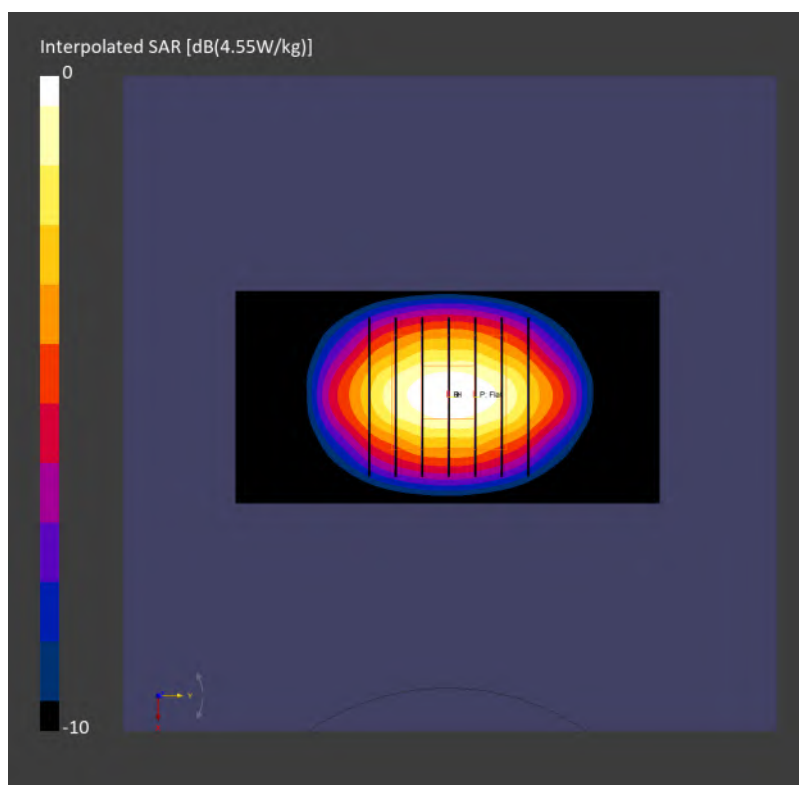

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.70$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.45 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.42 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

TSL Correction: Positive only

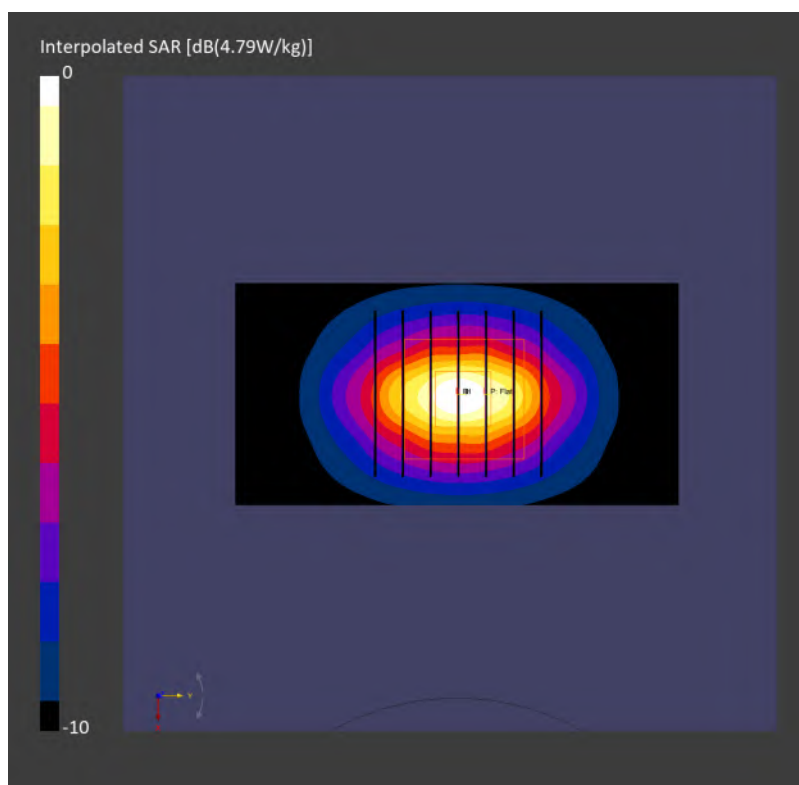

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.75$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.45 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.43 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.4 %

TSL Correction: Positive only

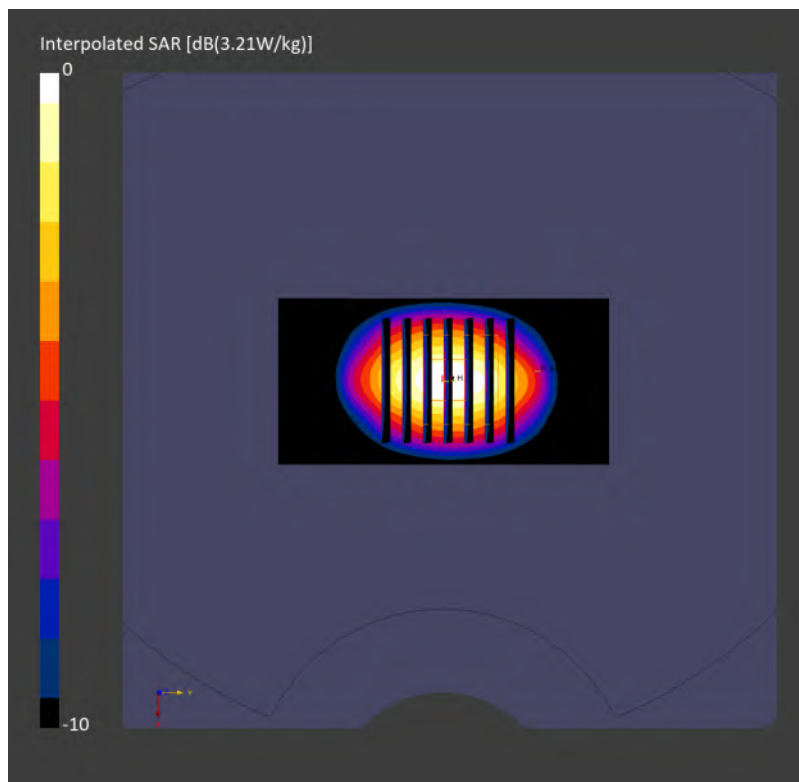

System Check_Head_2300MHz**DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.77$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.6, 7.06, 7.54); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.49 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

TSL Correction: Positive only

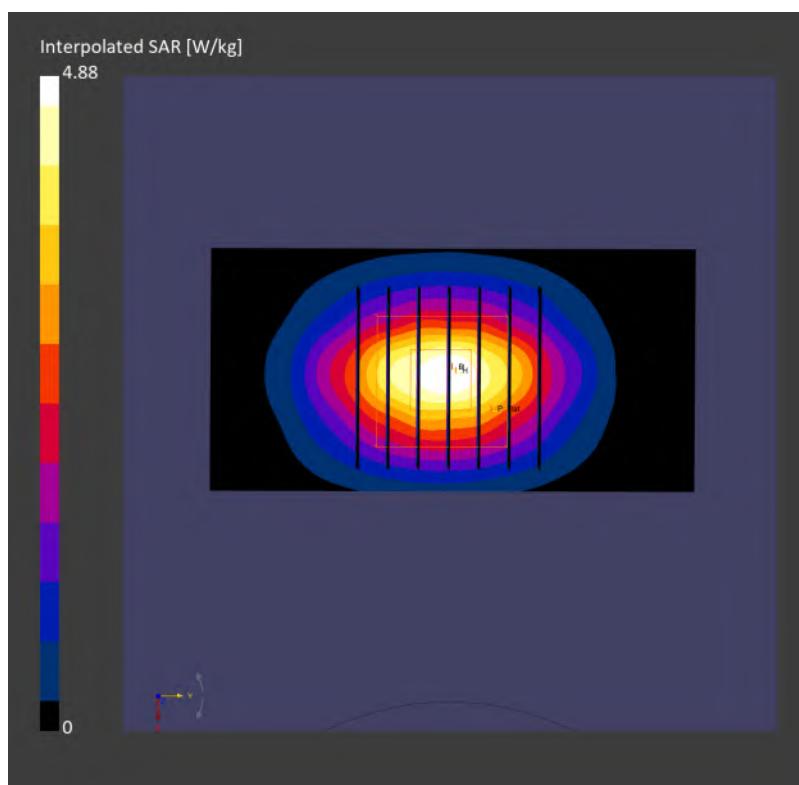

System Check_Head 2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260905 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.72$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.35, 7.83, 7.39); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.44 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

TSL Correction: Positive only

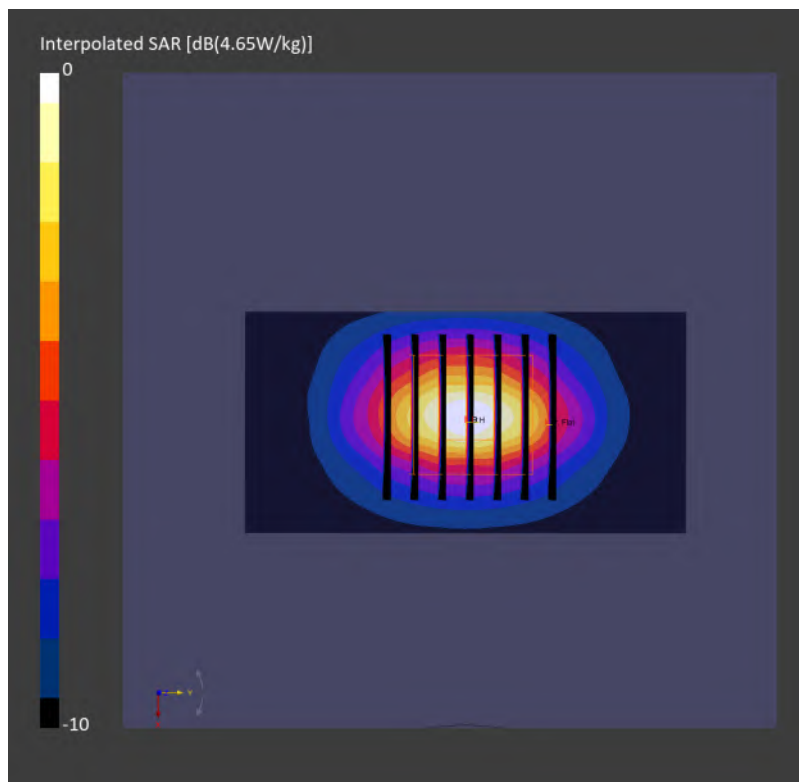

System Check_Head_2300MHz

DUT: D2300V2-1006

Communication System: UID 0, CW; Frequency: 2300 MHz

Medium: HSL_600~7200_260913 Medium parameters used: $f = 2300$ MHz; $\sigma = 1.742$ S/m; $\epsilon_r = 39.921$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.20, 7.66, 7.53) @ 2300 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (71x71x1): Interpolated grid: $dx=1.200$ mm, $dy=1.200$ mm

Maximum value of SAR (interpolated) = 21.4 W/kg

Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 116.8 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 25.7 W/kg

SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.29 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 51.9%

Maximum value of SAR (measured) = 21.5 W/kg

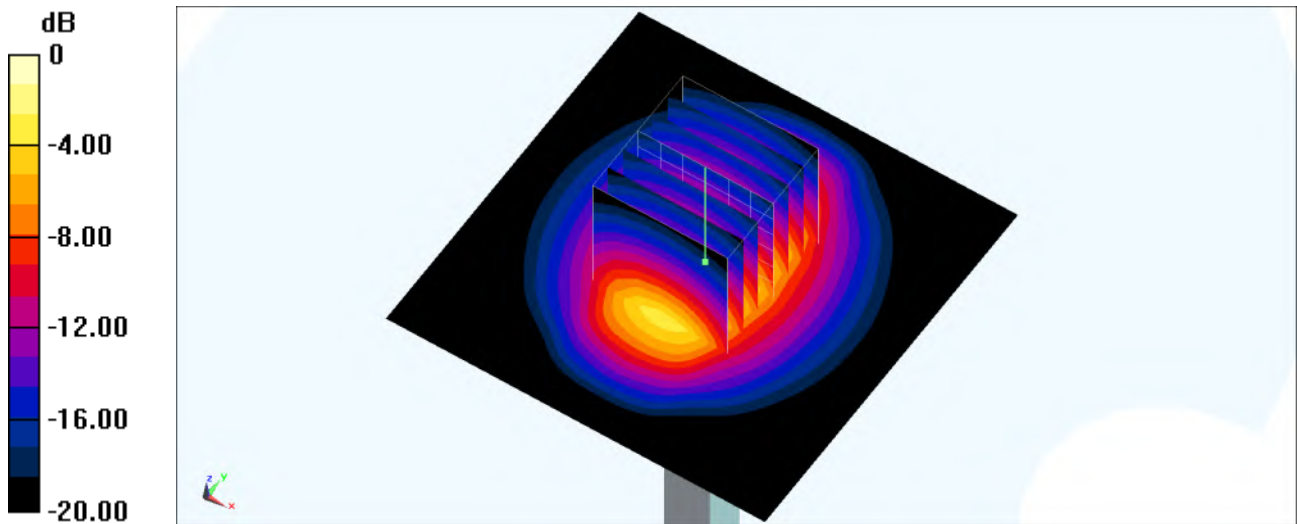

0 dB = 21.5 W/kg = 13.32 dBW/kg

System Check_Head 2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.08, 7.54, 7.12); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.08 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.07 dB

SAR (1g) = 2.44 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.1 %

TSL Correction: Positive only

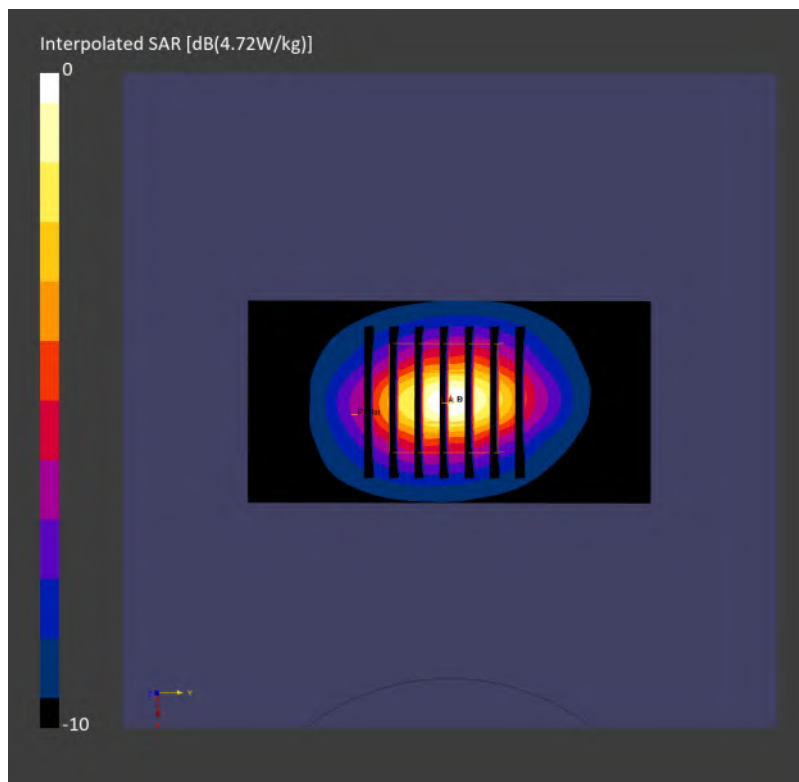

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.87$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.44, 6.91, 7.38); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.63 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.2 %

TSL Correction: Positive only

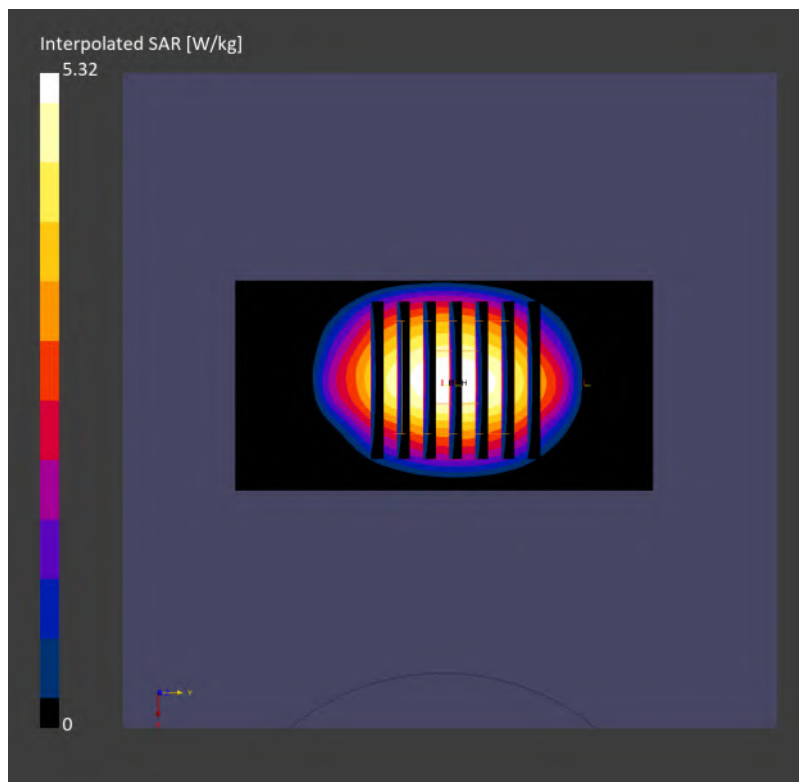

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.88$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.44, 6.91, 7.38); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.57 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.03 dB

SAR (1g) = 2.55 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.4 %

TSL Correction: Positive only

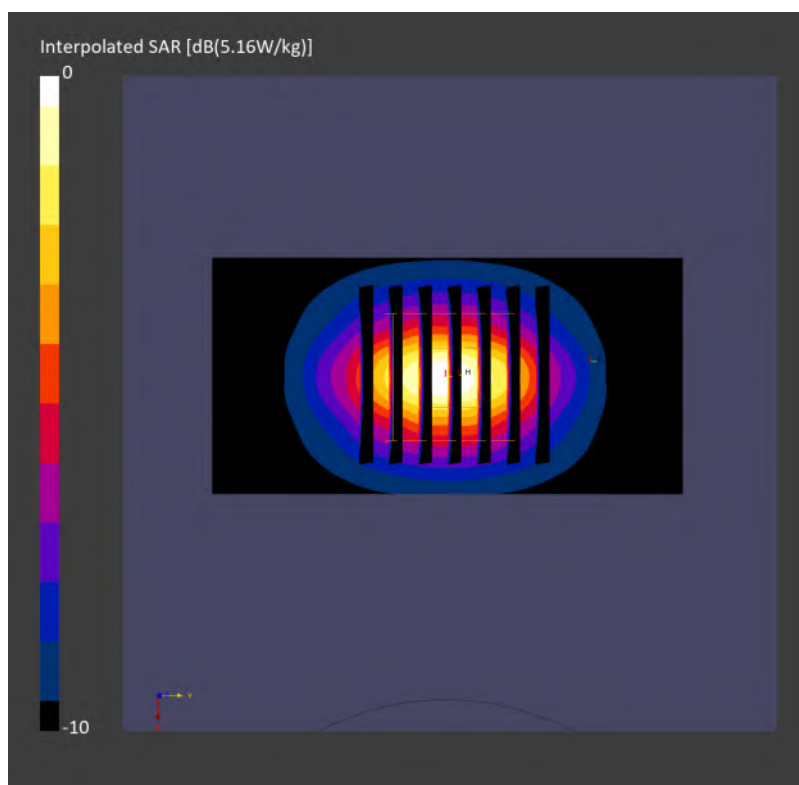

System Check_Head_2450MHz**DUT: D2450V2 - SN736**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260905 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.86$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.44, 6.91, 7.38); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.24 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.61 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.0 %

TSL Correction: Positive only

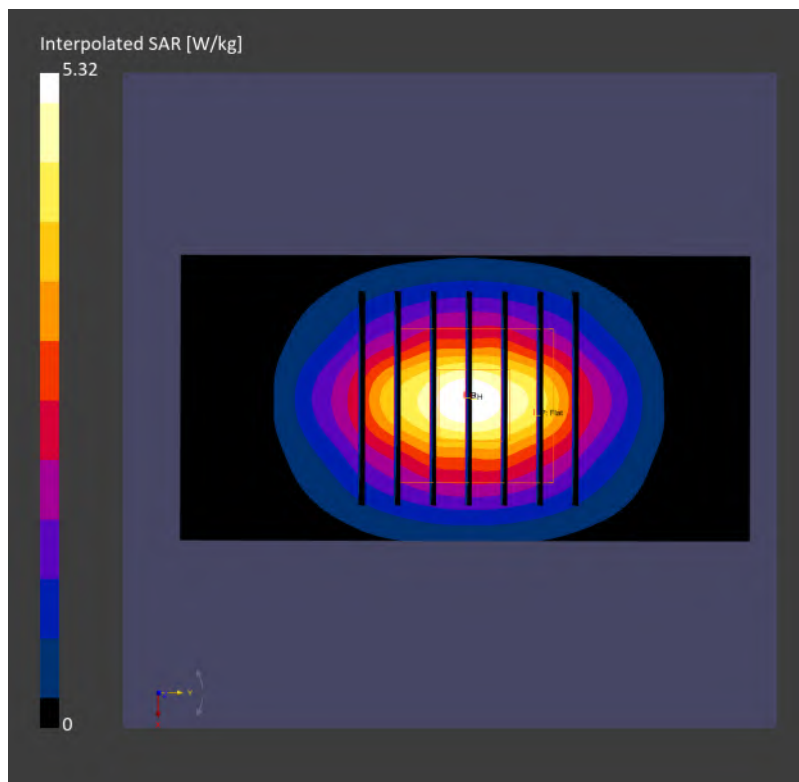

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260820 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.03$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.66 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

TSL Correction: Positive only

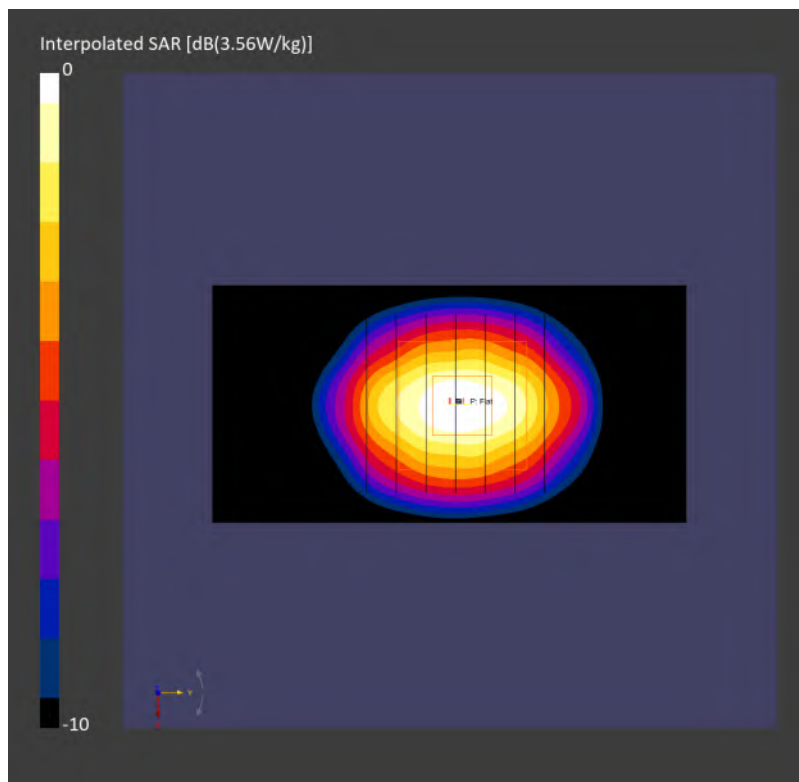

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260822 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.04, 7.16, 6.86); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.9 W/kg; SAR (10g) = 5.80 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 13.3 W/kg; SAR (8g) = 6.86 W/kg; SAR (10g) = 6.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 83.8 %

TSL Correction: Positive only

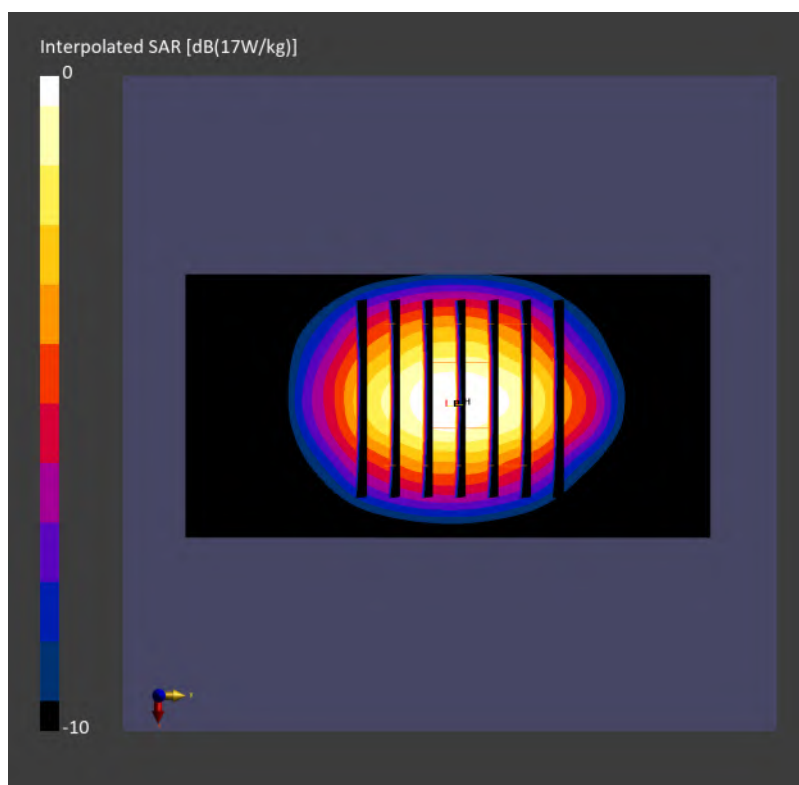

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600~7200_260823 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.961$ S/m; $\epsilon_r = 39.4$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 24.3 W/kg

Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 117.5 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 30.5 W/kg

SAR(1 g) = 14.7 W/kg; SAR(10 g) = 6.56 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8 mm

Ratio of SAR at M2 to SAR at M1 = 48.6%

Maximum value of SAR (measured) = 25.0 W/kg

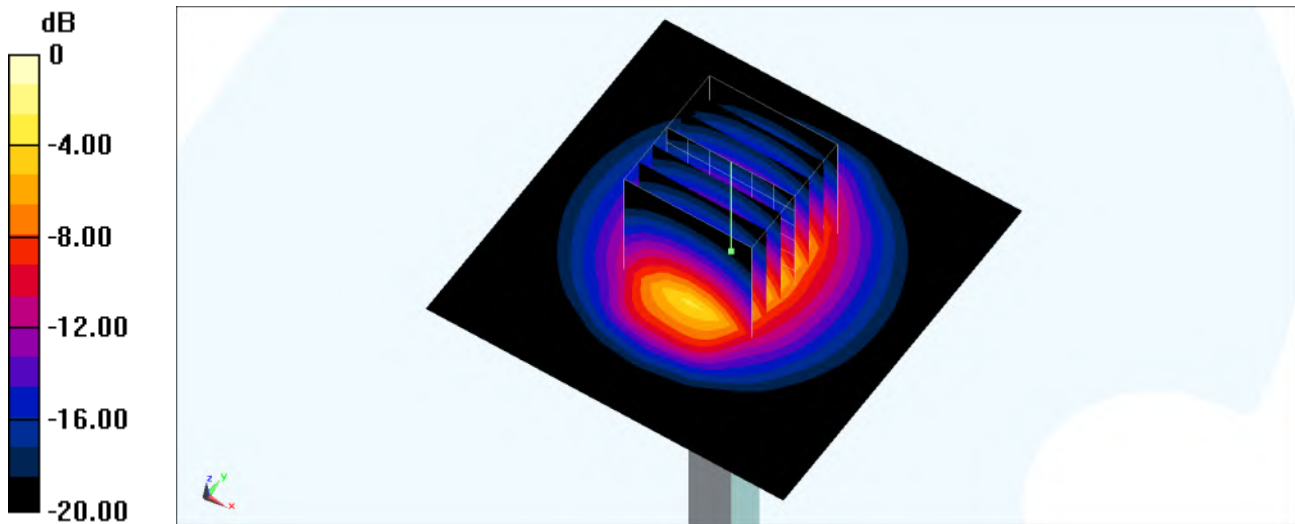

0 dB = 25.0 W/kg = 13.98 dBW/kg

System Check_Head 2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260823 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.15, 7.62, 7.2); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.88 W/kg; SAR (10g) = 1.25 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.92 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.8 %

TSL Correction: Positive only

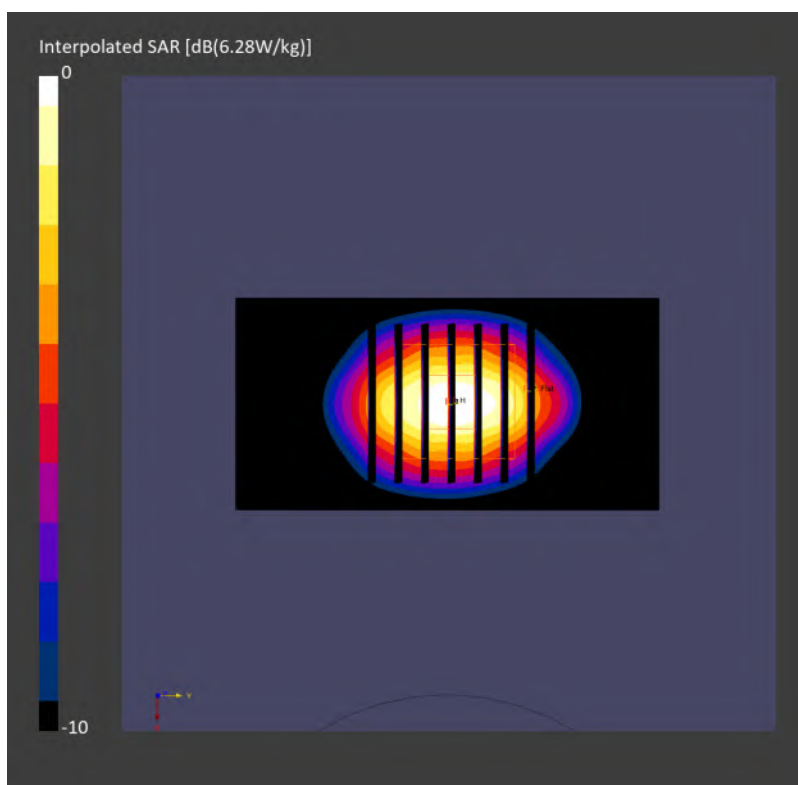

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.64 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.60 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.9 %

TSL Correction: Positive only

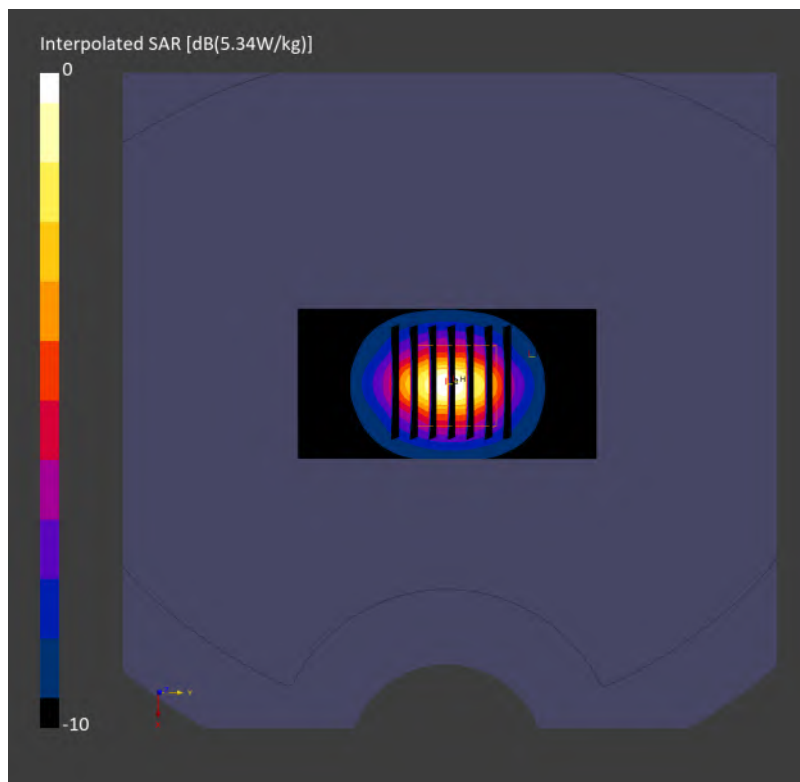

System Check_Head_2600MHz

DUT: D2600V2-1008

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.959$ S/m; $\epsilon_r = 39.387$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.75 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 52.10 V/m; Power Drift = -0.11 dB


Peak SAR (extrapolated) = 5.68 W/kg

SAR(1 g) = 2.86 W/kg; SAR(10 g) = 1.31 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 50.9%

Maximum value of SAR (measured) = 4.71 W/kg

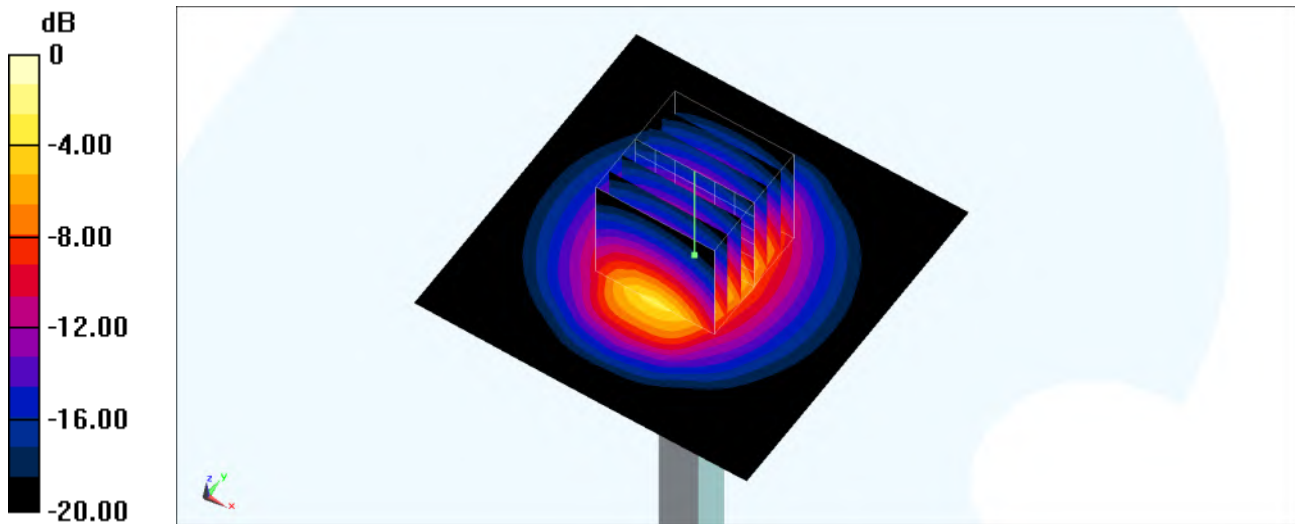

0 dB = 4.71 W/kg = 6.73 dBW/kg

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.959$ S/m; $\epsilon_r = 39.387$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.40 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.44 V/m; Power Drift = 0.10 dB


Peak SAR (extrapolated) = 5.45 W/kg

SAR(1 g) = 2.61 W/kg; SAR(10 g) = 1.16 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 48.1%

Maximum value of SAR (measured) = 4.43 W/kg

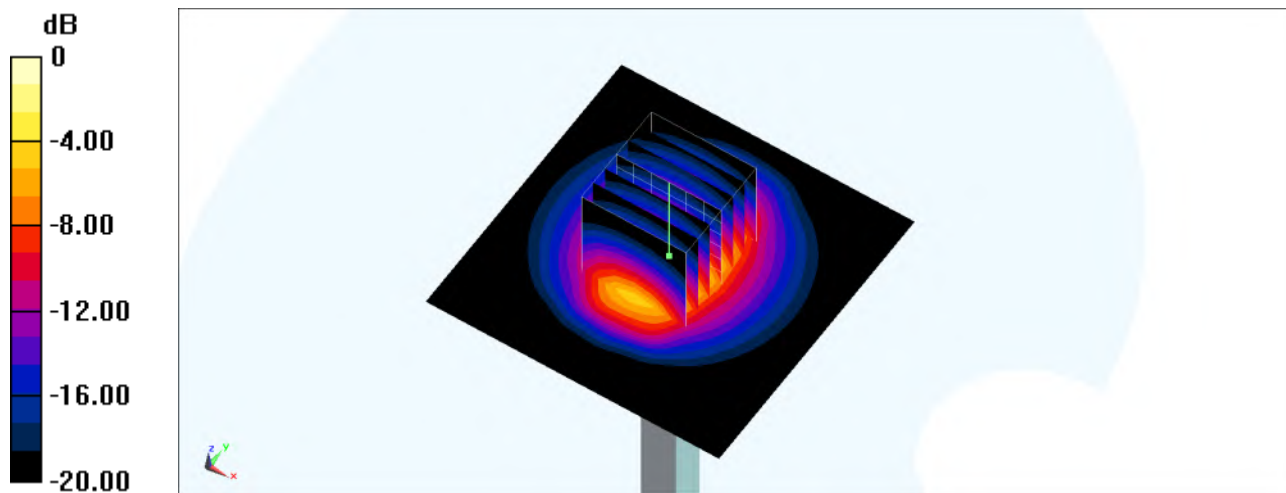

0 dB = 4.43 W/kg = 6.46 dBW/kg

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260826 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.957$ S/m; $\epsilon_r = 39.375$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.36 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.84 V/m; Power Drift = 0.04 dB


Peak SAR (extrapolated) = 5.49 W/kg

SAR(1 g) = 2.62 W/kg; SAR(10 g) = 1.16 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 47.9%

Maximum value of SAR (measured) = 4.45 W/kg

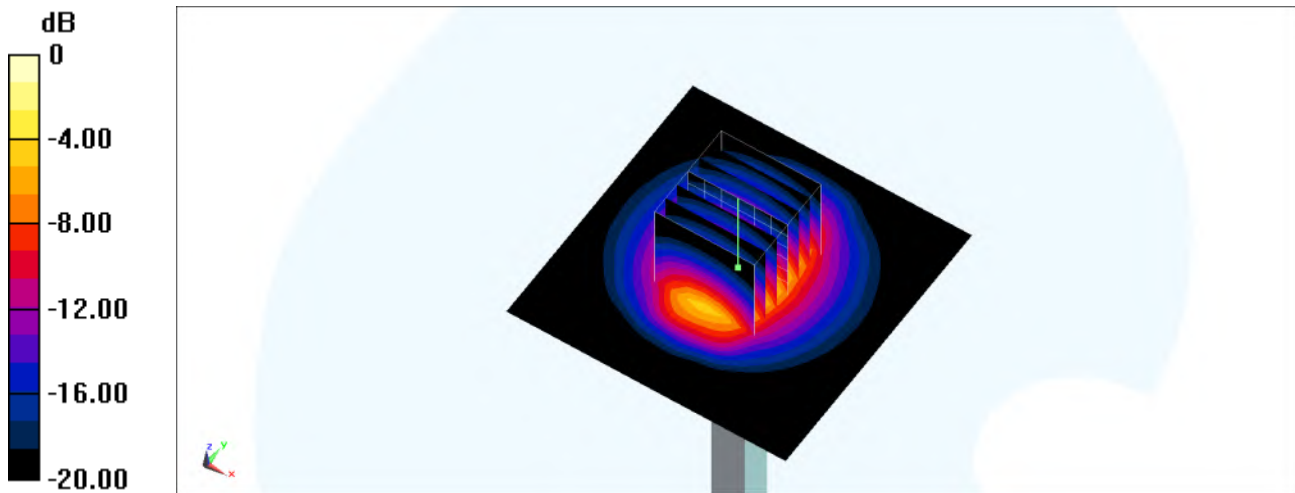

0 dB = 4.45 W/kg = 6.48 dBW/kg

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.913$ S/m; $\epsilon_r = 41.357$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.25 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.59 V/m; Power Drift = 0.08 dB


Peak SAR (extrapolated) = 5.38 W/kg

SAR(1 g) = 2.62 W/kg; SAR(10 g) = 1.15 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 47.7%

Maximum value of SAR (measured) = 4.39 W/kg

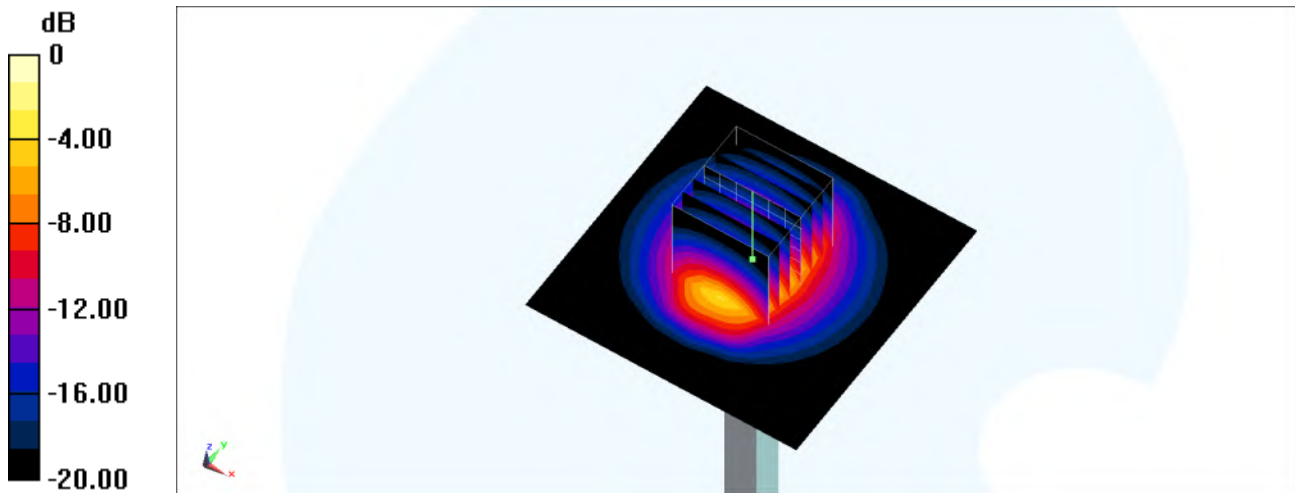

0 dB = 4.39 W/kg = 6.42 dBW/kg

System Check_Head 2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.15, 7.62, 7.2); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.54 W/kg; SAR (10g) = 1.13 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.54 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.2 %

TSL Correction: Positive only

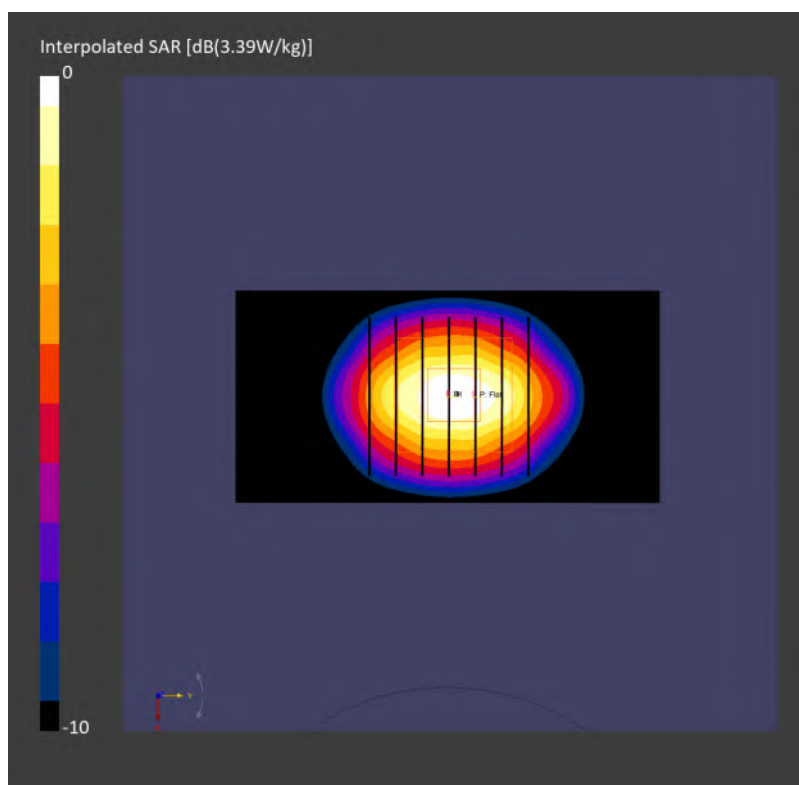

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.955$ S/m; $\epsilon_r = 39.362$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.36 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.74 V/m; Power Drift = 0.07 dB


Peak SAR (extrapolated) = 5.47 W/kg

SAR(1 g) = 2.61 W/kg; SAR(10 g) = 1.16 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 48%

Maximum value of SAR (measured) = 4.48 W/kg

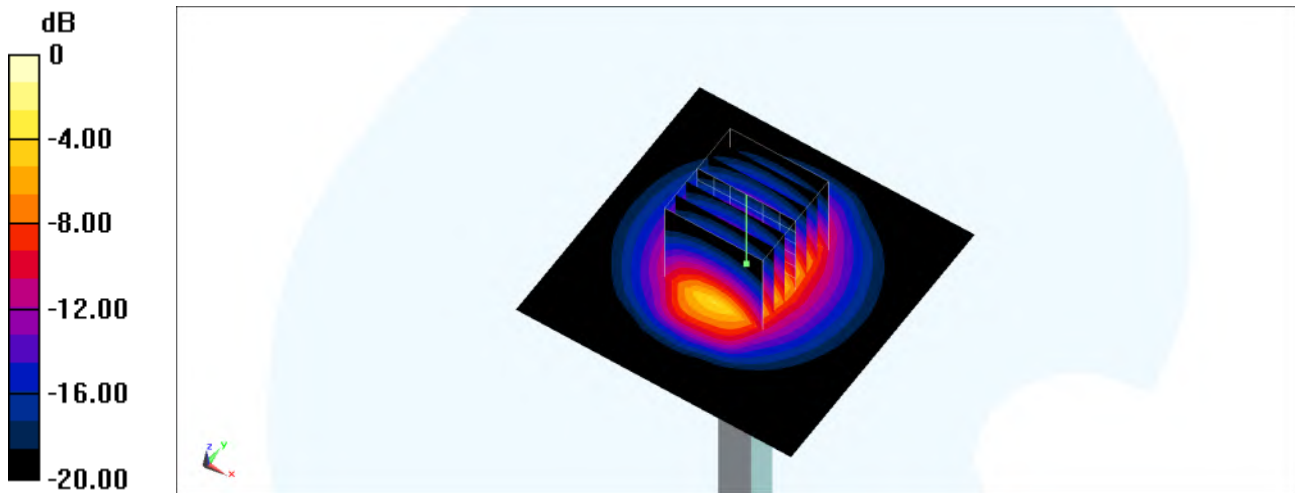

0 dB = 4.48 W/kg = 6.51 dBW/kg

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.954$ S/m; $\epsilon_r = 39.35$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: $dx=1.200$ mm, $dy=1.200$ mm

Maximum value of SAR (interpolated) = 4.36 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 49.73 V/m; Power Drift = 0.07 dB


Peak SAR (extrapolated) = 5.49 W/kg

SAR(1 g) = 2.62 W/kg; SAR(10 g) = 1.16 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 47.8%

Maximum value of SAR (measured) = 4.45 W/kg

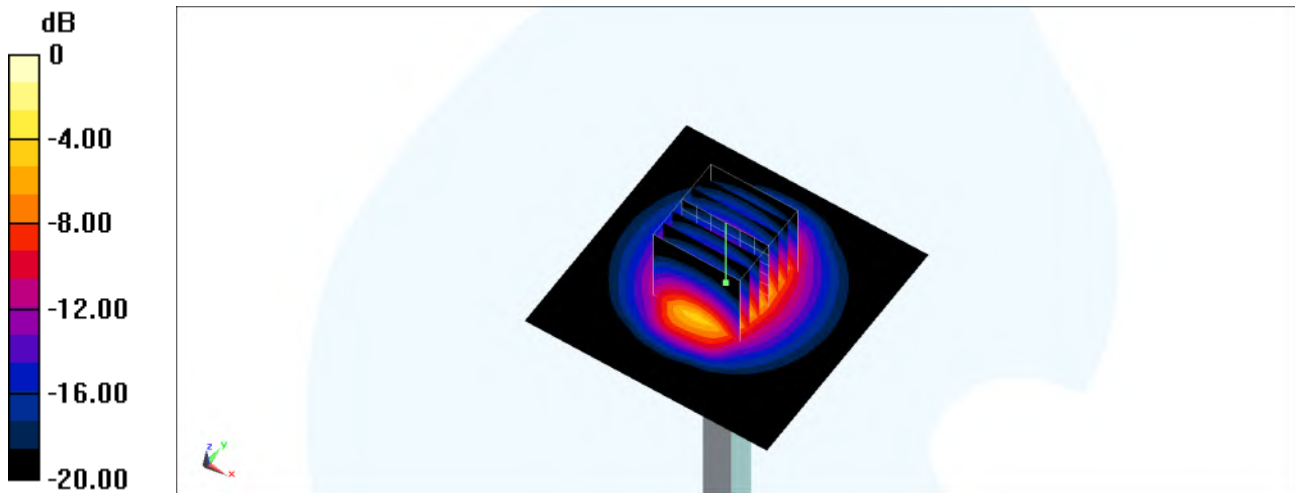

0 dB = 4.45 W/kg = 6.48 dBW/kg

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.63 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.59 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.5 %

TSL Correction: Positive only

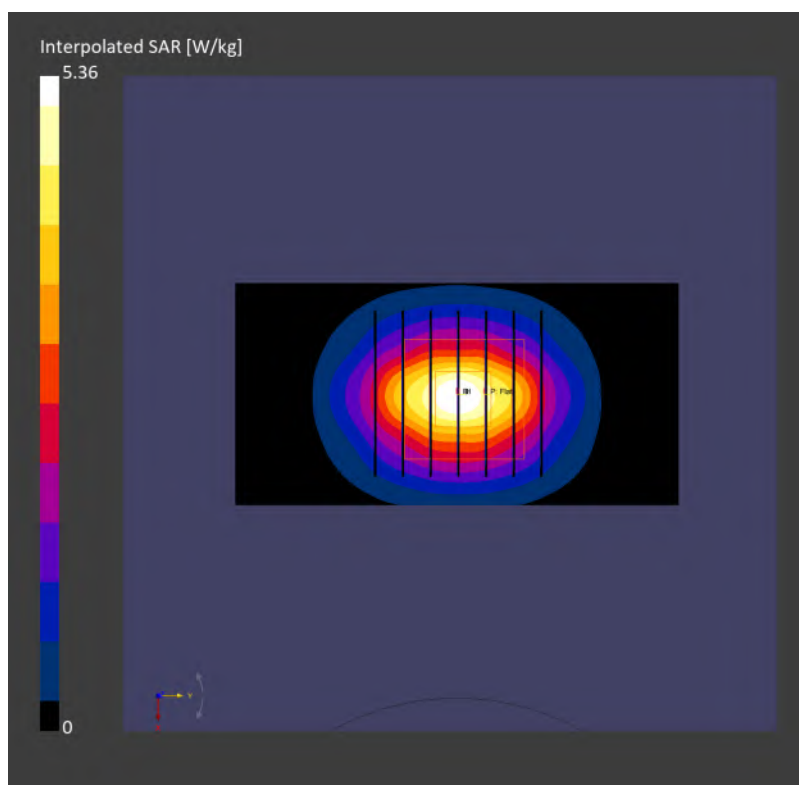

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.967$ S/m; $\epsilon_r = 38.92$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.41 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.74 V/m; Power Drift = 0.05 dB


Peak SAR (extrapolated) = 5.51 W/kg

SAR(1 g) = 2.62 W/kg; SAR(10 g) = 1.16 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 48%

Maximum value of SAR (measured) = 4.50 W/kg

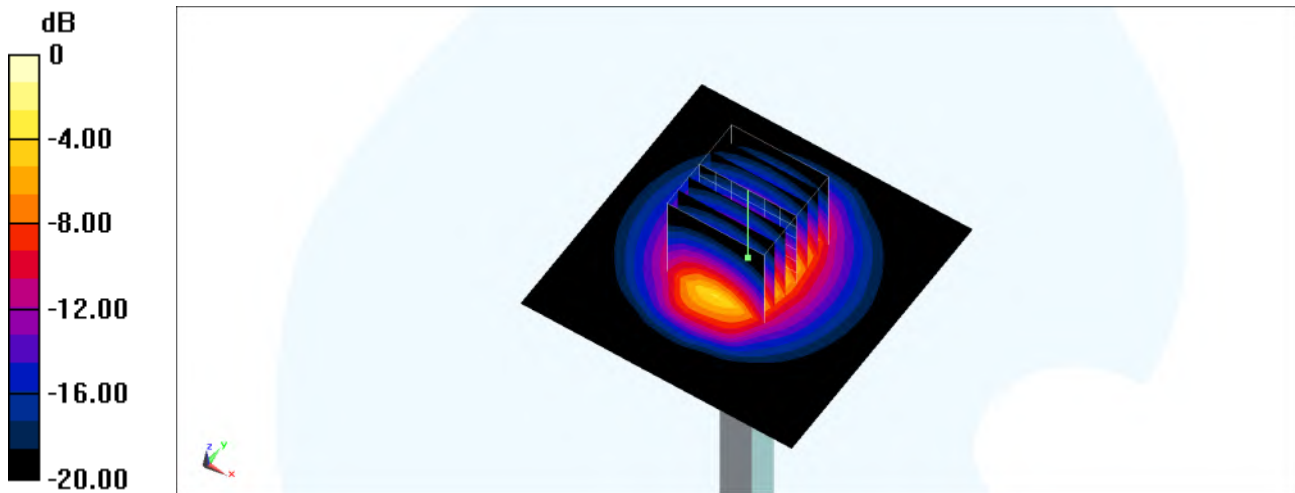

0 dB = 4.50 W/kg = 6.53 dBW/kg

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.65 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.6 %

TSL Correction: Positive only

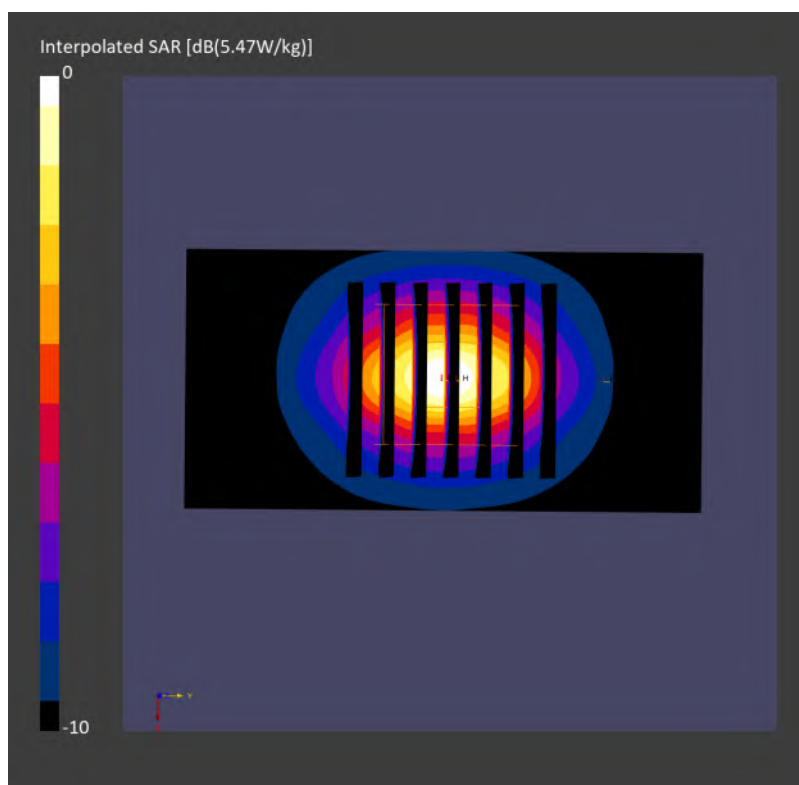

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.954$ S/m; $\epsilon_r = 38.97$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: $dx=1.200$ mm, $dy=1.200$ mm

Maximum value of SAR (interpolated) = 4.37 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 49.53 V/m; Power Drift = 0.08 dB


Peak SAR (extrapolated) = 5.42 W/kg

SAR(1 g) = 2.6 W/kg; SAR(10 g) = 1.15 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 48%

Maximum value of SAR (measured) = 4.43 W/kg

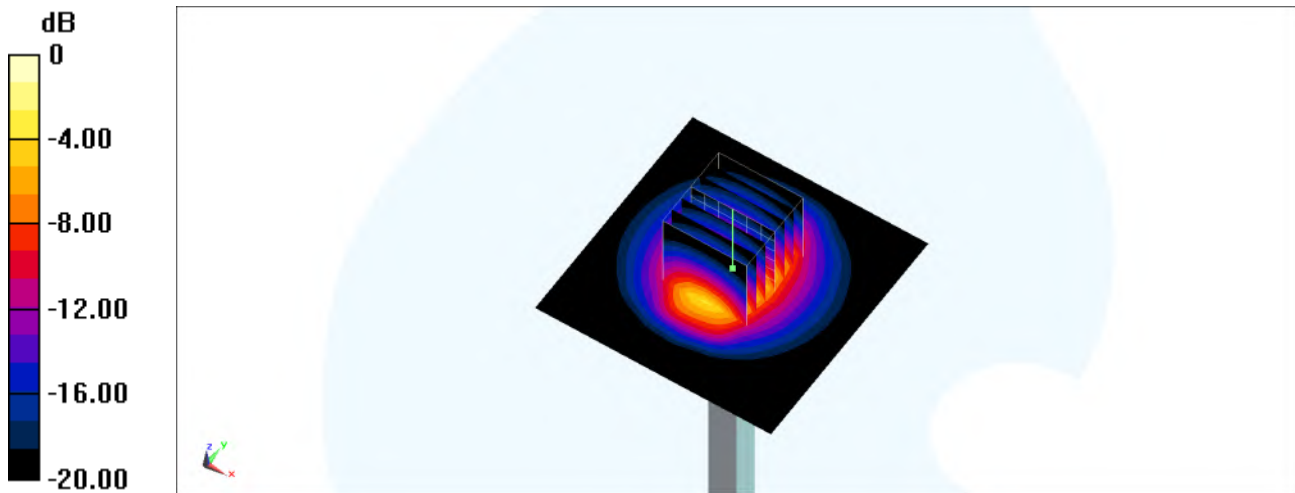

0 dB = 4.43 W/kg = 6.46 dBW/kg

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260901 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 38.94$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.36 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.50 V/m; Power Drift = 0.06 dB


Peak SAR (extrapolated) = 5.44 W/kg

SAR(1 g) = 2.6 W/kg; SAR(10 g) = 1.15 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 48%

Maximum value of SAR (measured) = 4.44 W/kg

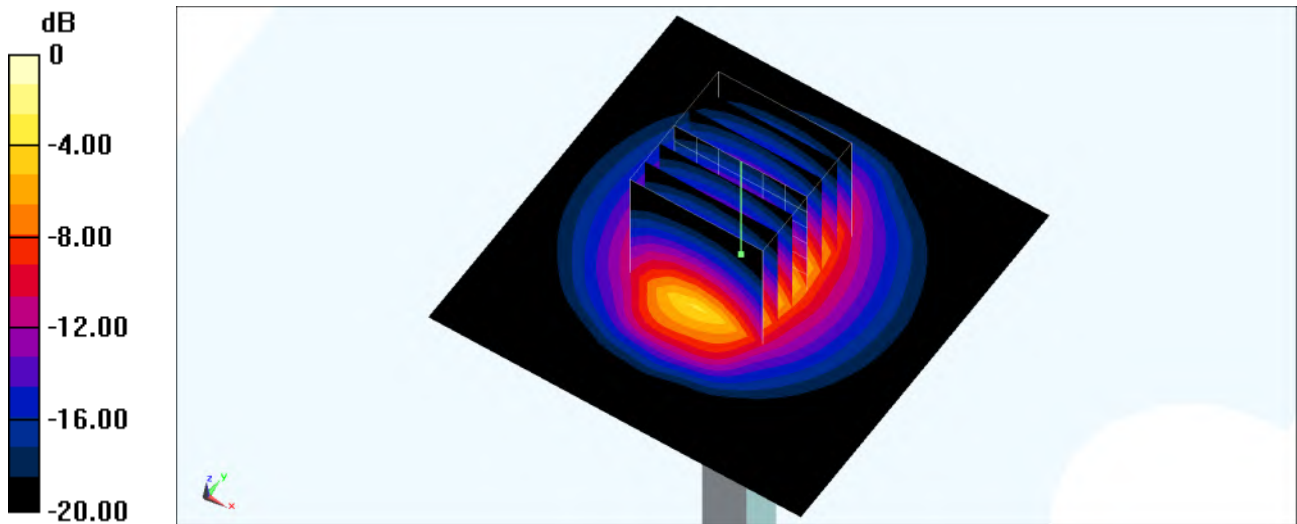

0 dB = 4.44 W/kg = 6.47 dBW/kg

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.951$ S/m; $\epsilon_r = 38.97$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.36 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.82 V/m; Power Drift = 0.06 dB


Peak SAR (extrapolated) = 5.45 W/kg

SAR(1 g) = 2.61 W/kg; SAR(10 g) = 1.15 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 48.2%

Maximum value of SAR (measured) = 4.40 W/kg

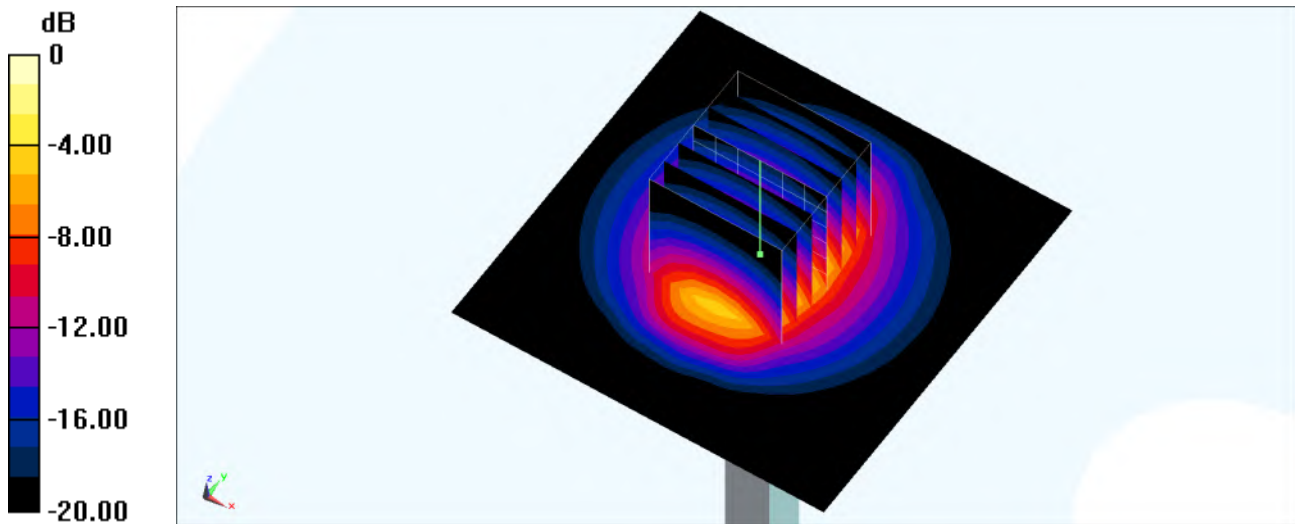

0 dB = 4.40 W/kg = 6.43 dBW/kg

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 38.89$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.36 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.81 V/m; Power Drift = 0.05 dB


Peak SAR (extrapolated) = 5.45 W/kg

SAR(1 g) = 2.6 W/kg; SAR(10 g) = 1.15 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.9 mm

Ratio of SAR at M2 to SAR at M1 = 48%

Maximum value of SAR (measured) = 4.45 W/kg

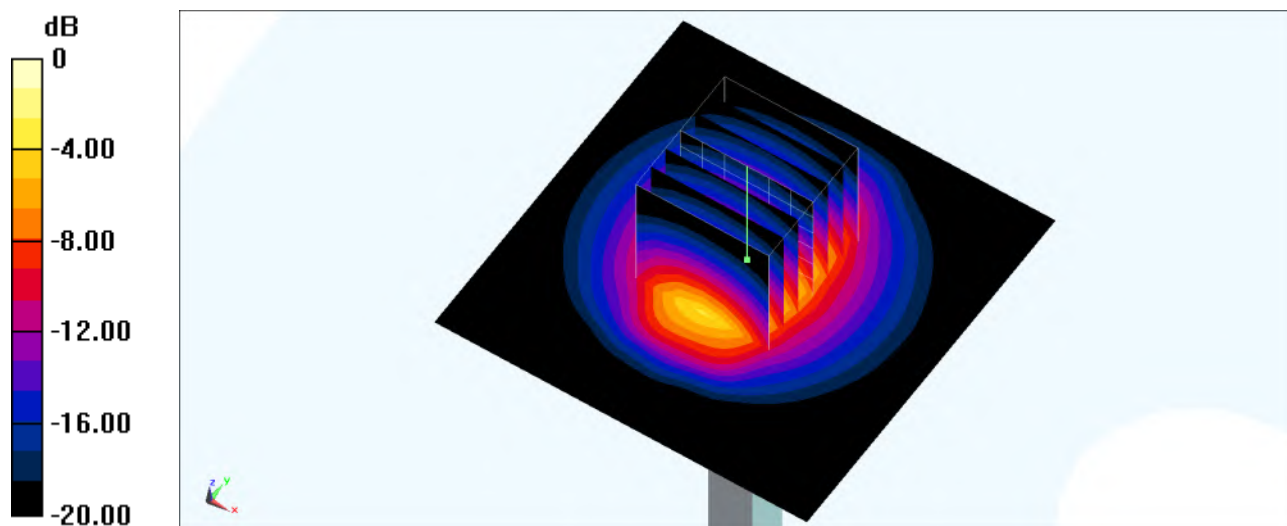

0 dB = 4.45 W/kg = 6.48 dBW/kg

System Check_Head_2600MHz

DUT: D2600V2-1078

Communication System: UID 0, CW ; Frequency: 2600 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 2600$ MHz; $\sigma = 1.911$ S/m; $\epsilon_r = 38.73$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7, 7.45, 7.32) @ 2600 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: $dx=1.200$ mm, $dy=1.200$ mm

Maximum value of SAR (interpolated) = 4.27 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 50.08 V/m; Power Drift = -0.10 dB


Peak SAR (extrapolated) = 5.35 W/kg

SAR(1 g) = 2.57 W/kg; SAR(10 g) = 1.13 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8.5 mm

Ratio of SAR at M2 to SAR at M1 = 48%

Maximum value of SAR (measured) = 4.32 W/kg

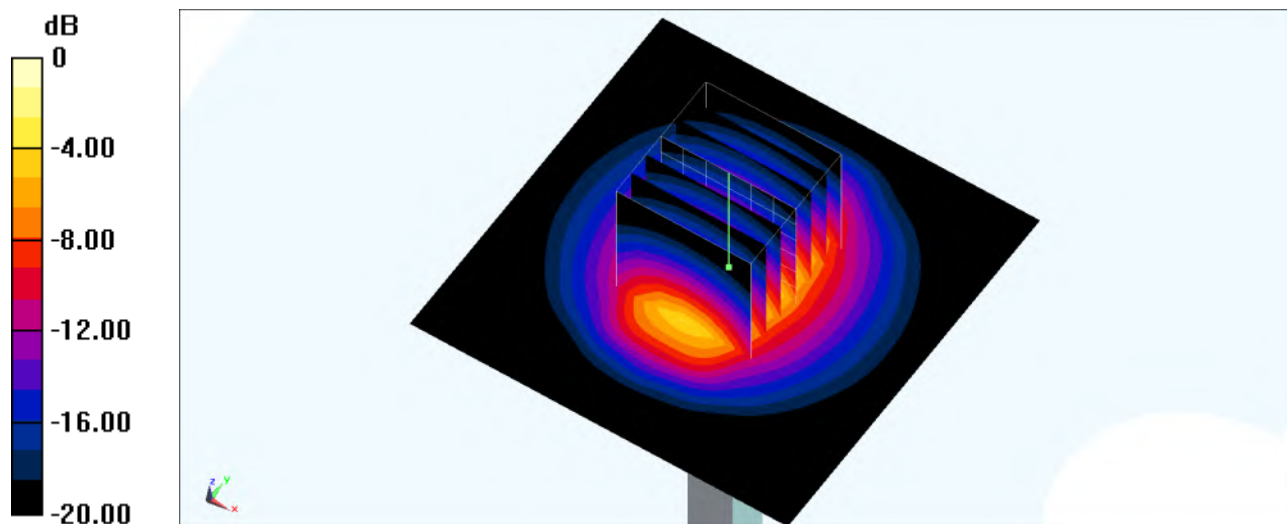

0 dB = 4.32 W/kg = 6.35 dBW/kg

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.72 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.67 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.5 %

TSL Correction: Positive only

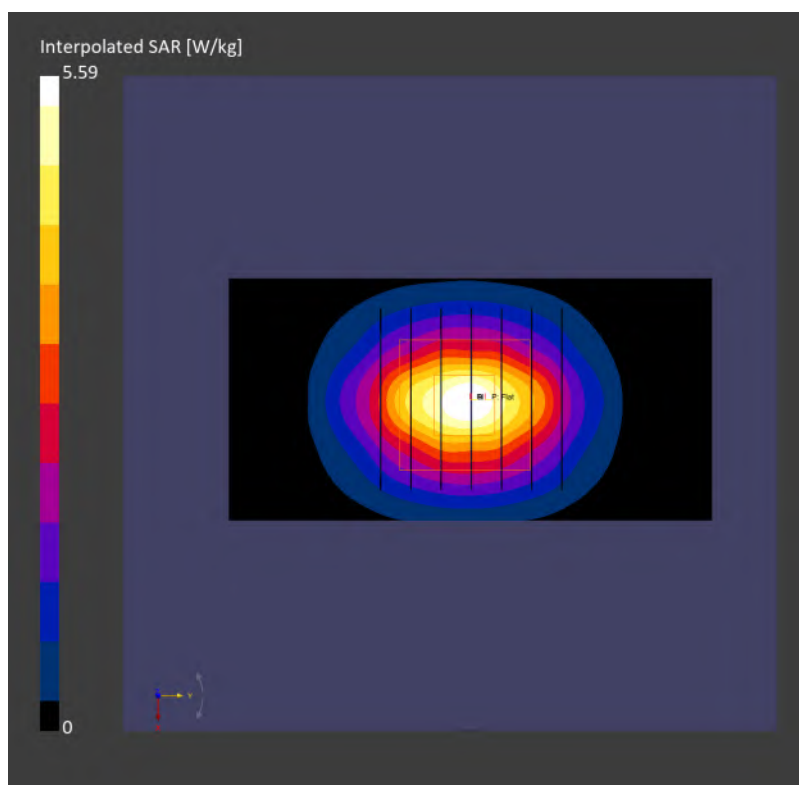

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260905 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.90$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(4.56, 4.48, 4.37); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.57 W/kg; SAR (10g) = 1.16 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.54 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 10.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.1 %

TSL Correction: Positive only

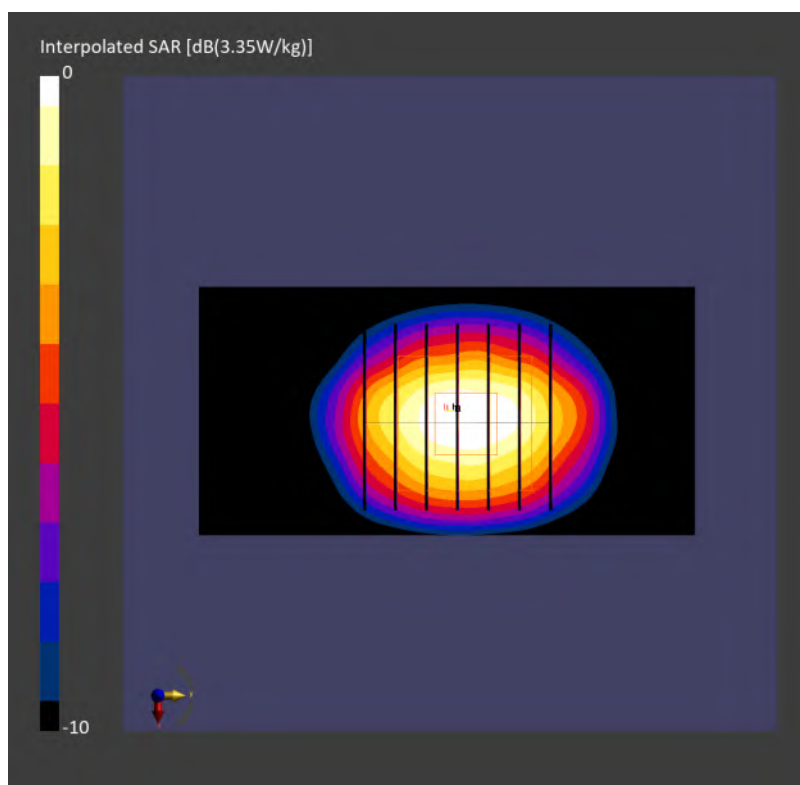

System Check_Head 2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260905 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.15, 7.62, 7.2); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.56 W/kg; SAR (10g) = 1.13 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.60 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.9 %

TSL Correction: Positive only

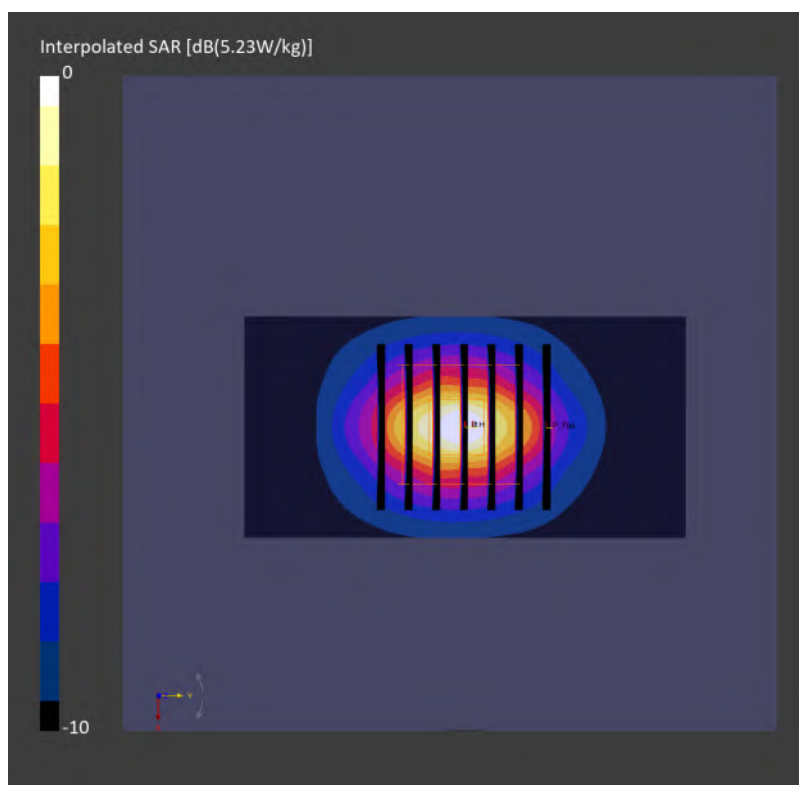

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(4.56, 4.48, 4.37); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.63 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 10.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.4 %

TSL Correction: Positive only

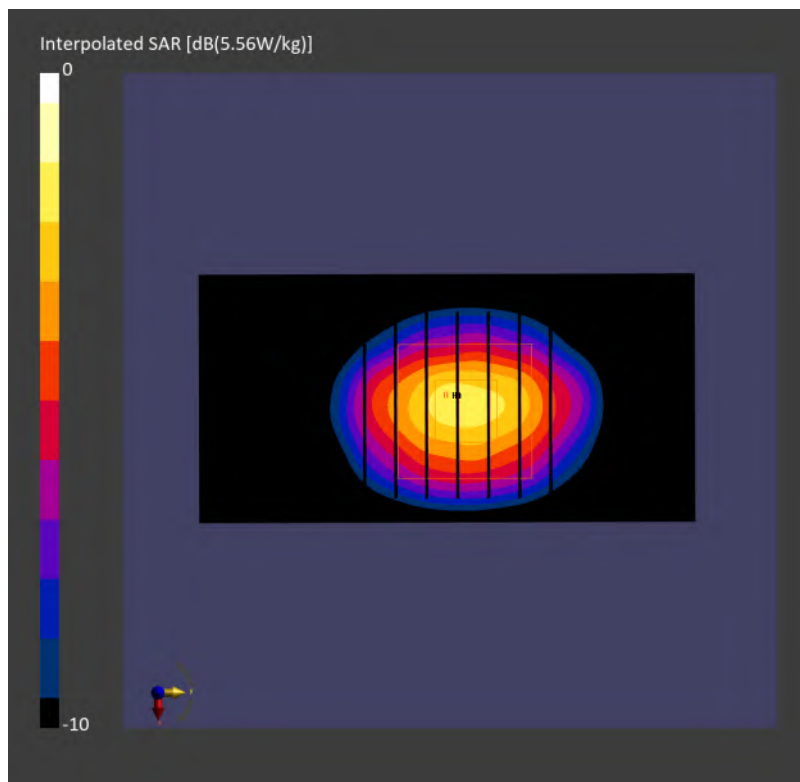

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260907 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: ES3DV3 - SN3115; ConvF(4.56, 4.48, 4.37); Calibrated: 2026-08-18
- Sensor-Surface: 3.0 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.64 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 10.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.2 %

TSL Correction: Positive only

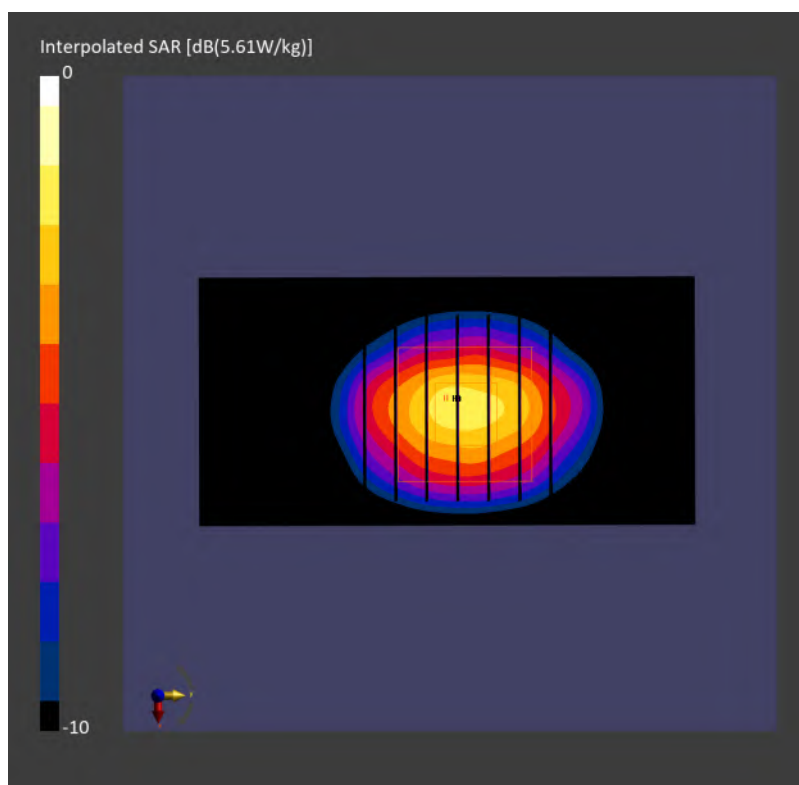

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260909 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.32, 6.8, 7.27); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.64 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.61 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.2 %

TSL Correction: Positive only

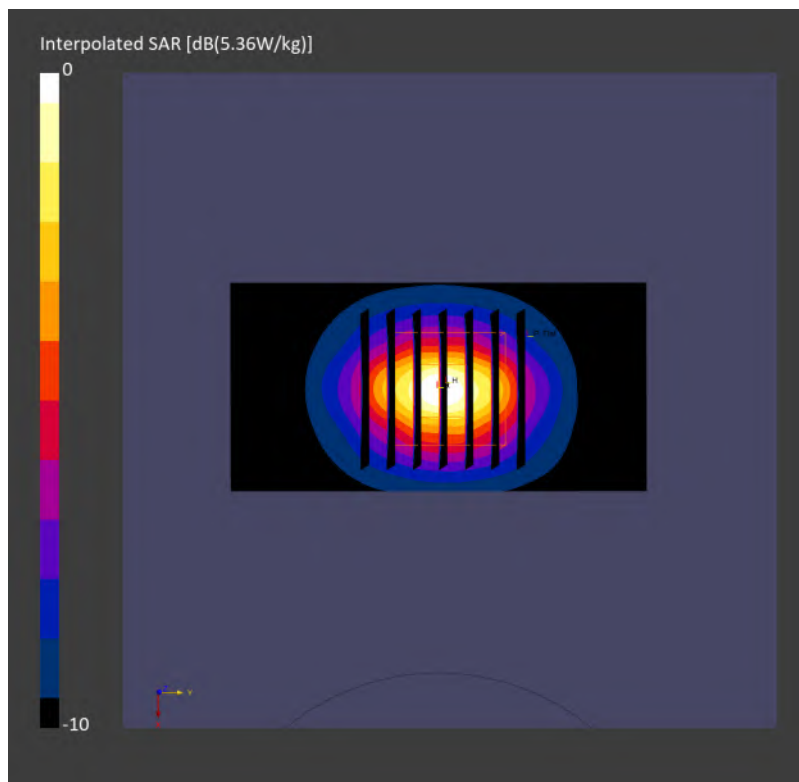

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260821 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.82$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.79, 6.3, 6.74); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 5.74 W/kg; SAR (10g) = 2.21 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 6.17 W/kg; SAR (8g) = 2.62 W/kg; SAR (10g) = 2.33 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

TSL Correction: Positive only

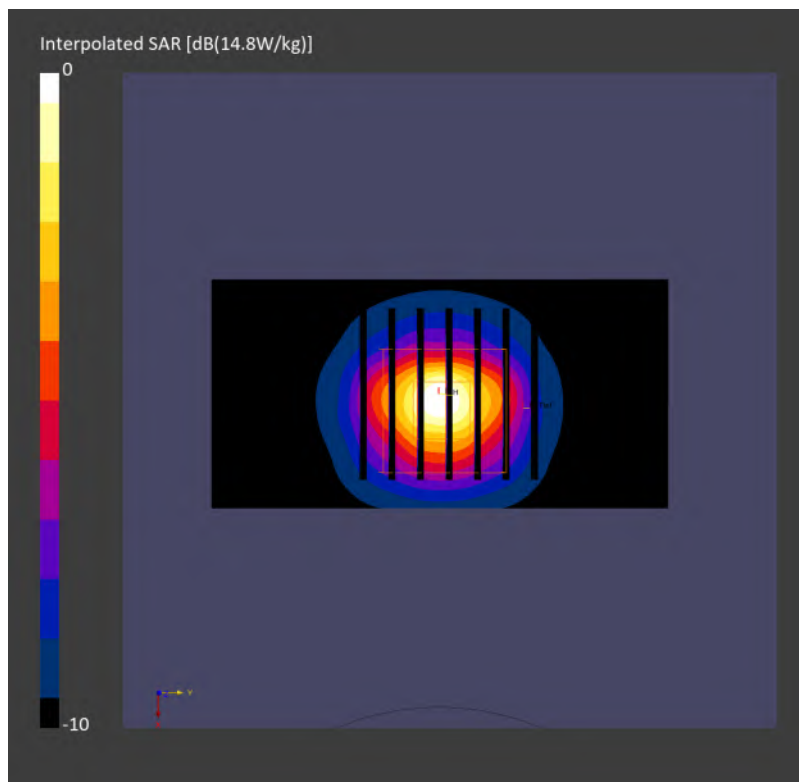

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260823 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.70$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(6.67, 6.78, 6.49); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.01 W/kg; SAR (10g) = 2.28 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 6.29 W/kg; SAR (8g) = 2.80 W/kg; SAR (10g) = 2.49 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.7 %

TSL Correction: Positive only

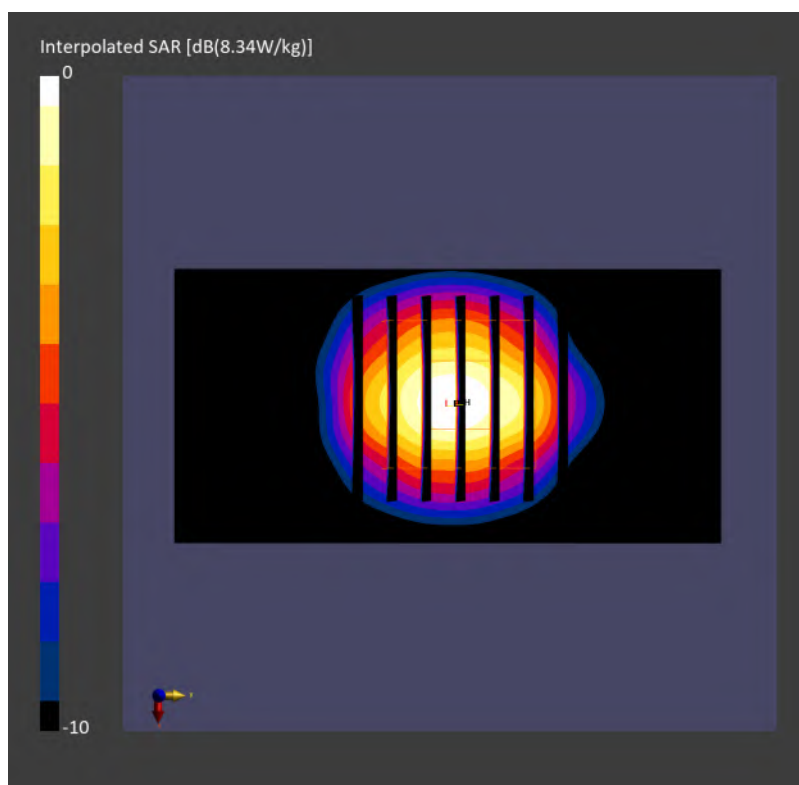

System Check_Head 3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.74$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.54, 6.97, 6.58); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.54 W/kg; SAR (10g) = 2.43 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 6.58 W/kg; SAR (8g) = 2.84 W/kg; SAR (10g) = 2.52 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 77.4 %

TSL Correction: Positive only

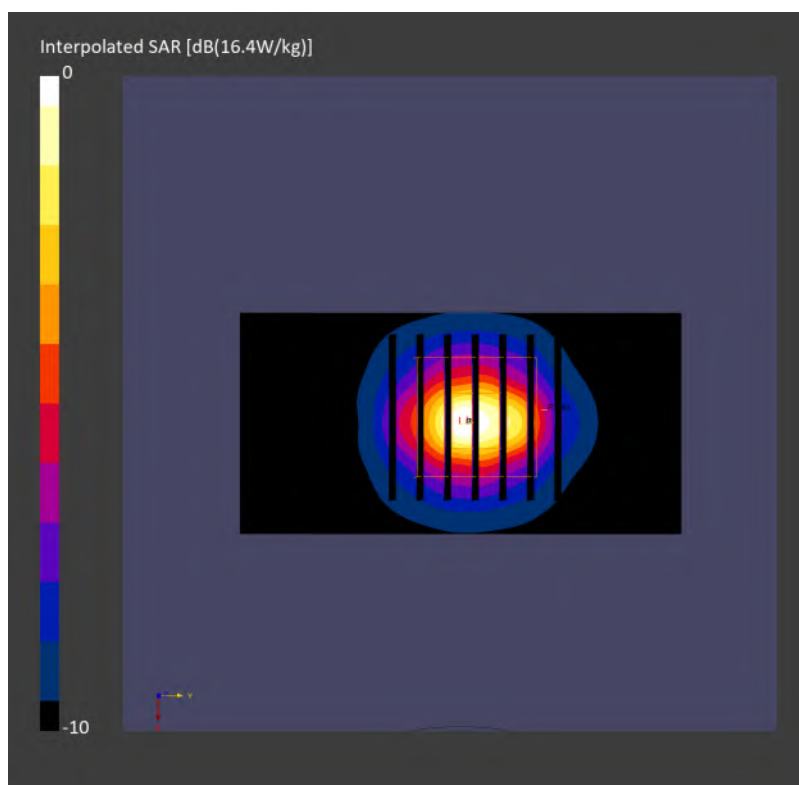

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.70$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.79, 6.3, 6.74); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.08 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.10 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

TSL Correction: Positive only

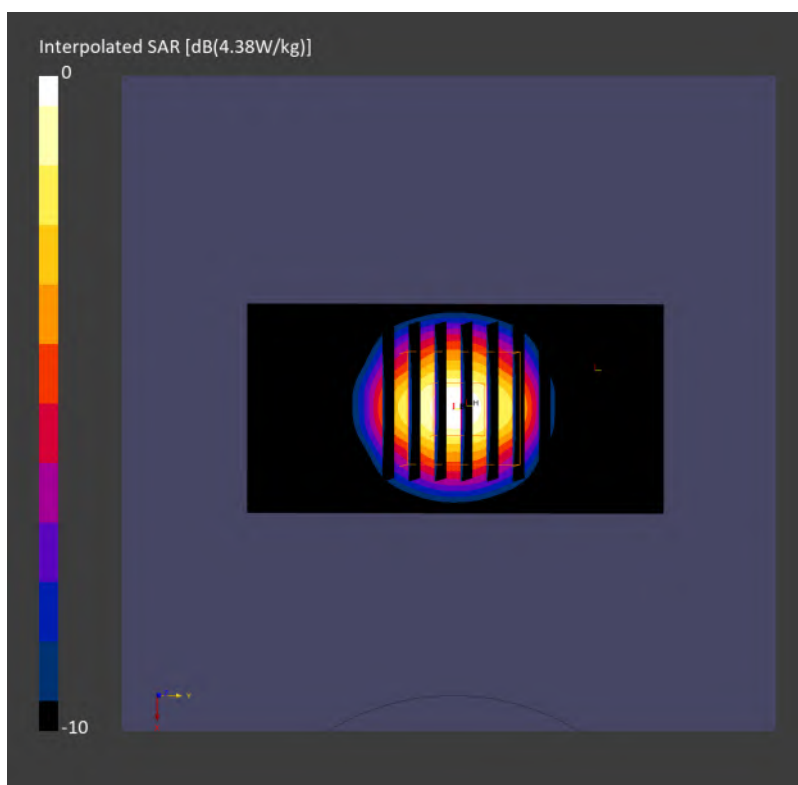

System Check_Head 3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.75$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.54, 6.97, 6.58); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.06 W/kg; SAR (10g) = 1.15 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.11 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.2 %

TSL Correction: Positive only

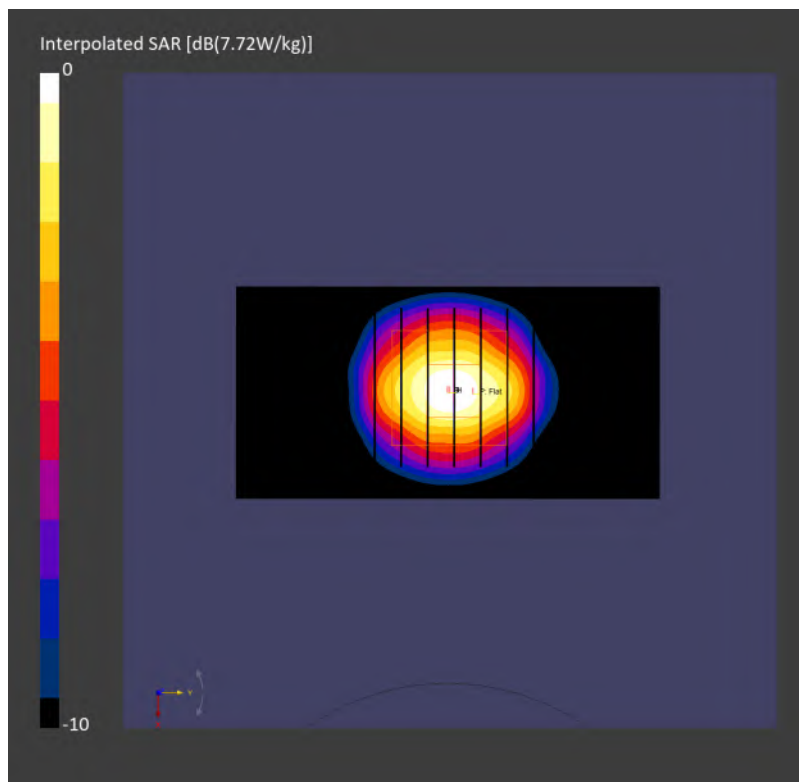

System Check_Head 3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.74$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.54, 6.97, 6.58); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.00 W/kg; SAR (10g) = 1.13 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.03 dB

SAR (1g) = 3.09 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.3 %

TSL Correction: Positive only

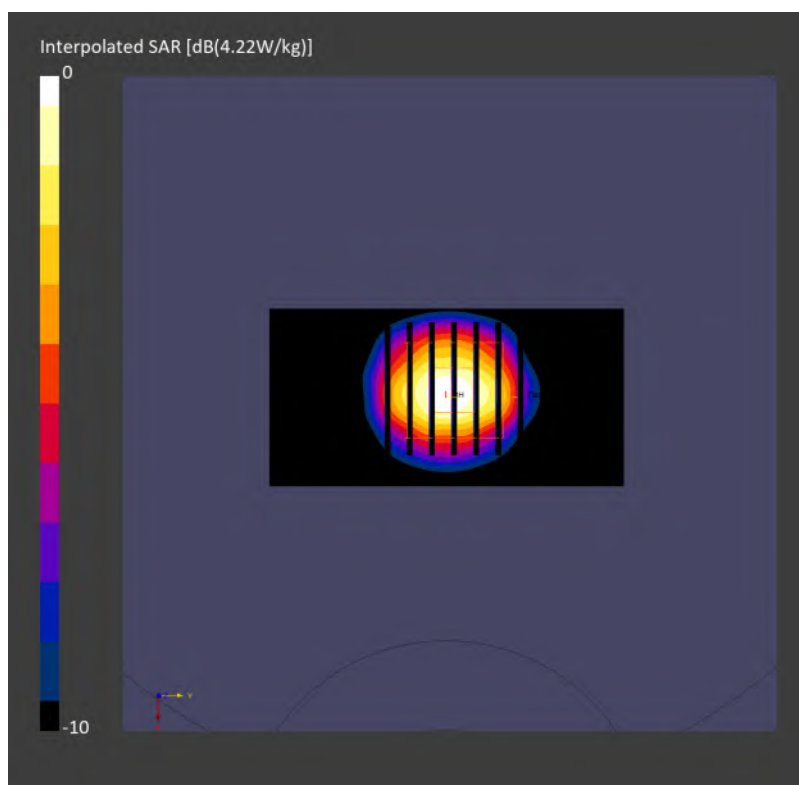

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.66$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.54, 6.97, 6.58); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.22 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

TSL Correction: Positive only

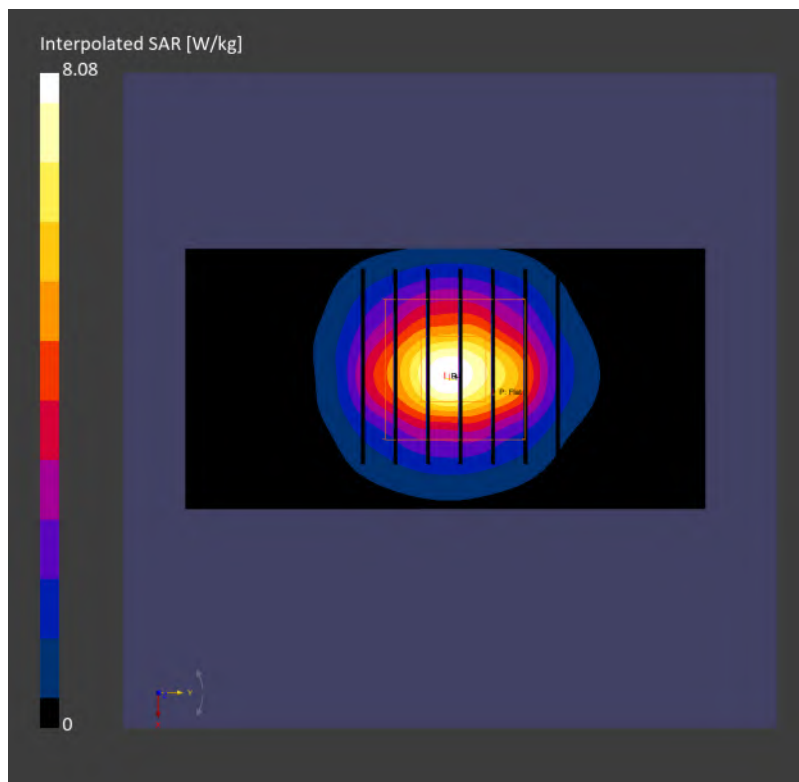

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.68$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.79, 6.3, 6.74); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.99 W/kg; SAR (10g) = 1.12 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 2.99 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.1 %

TSL Correction: Positive only

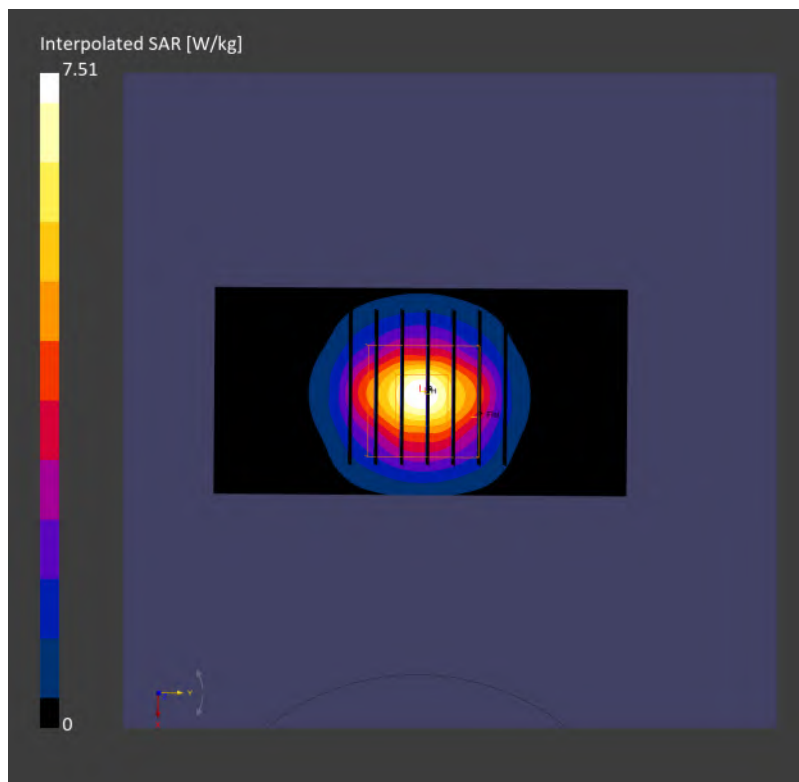

System Check_Head 3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.66$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.54, 6.97, 6.58); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.02 W/kg; SAR (10g) = 1.12 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

TSL Correction: Positive only

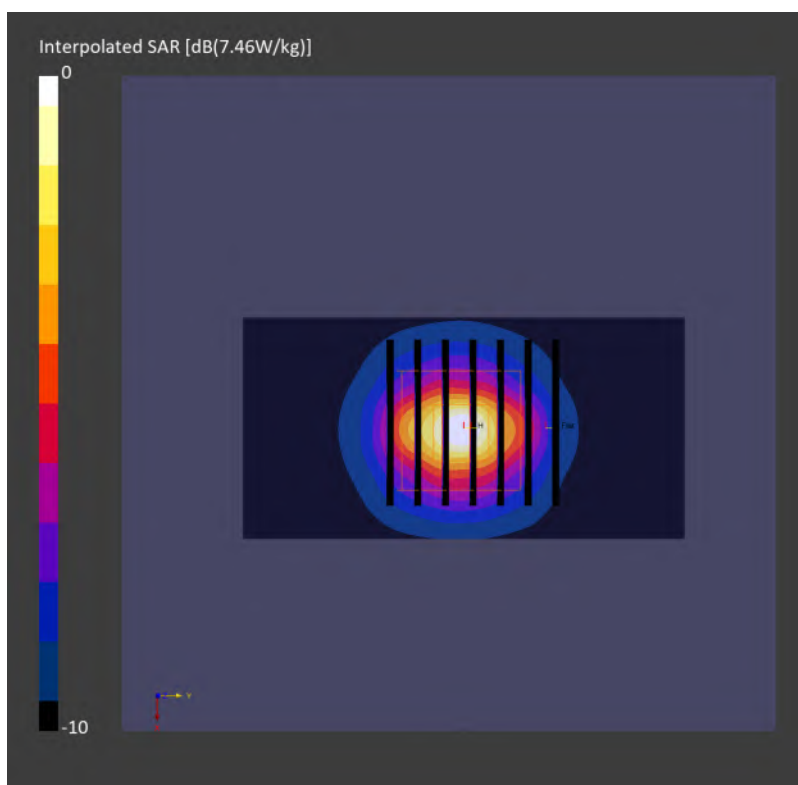

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260908 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.68$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.79, 6.3, 6.74); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 3.23 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.0 %

TSL Correction: Positive only

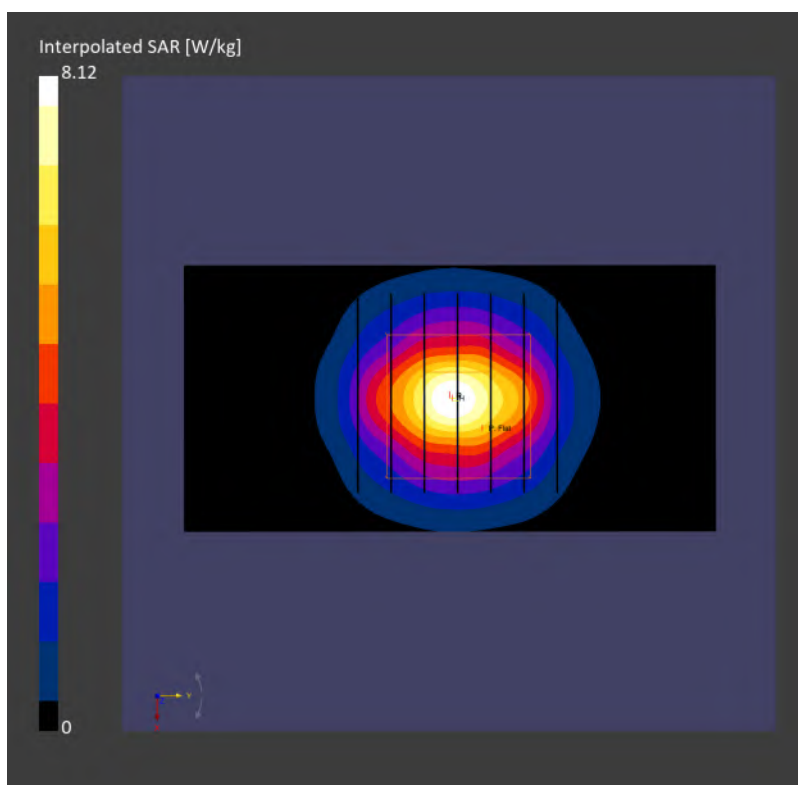

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260908 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.72$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.52, 6.94, 6.82); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.17 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

TSL Correction: Positive only

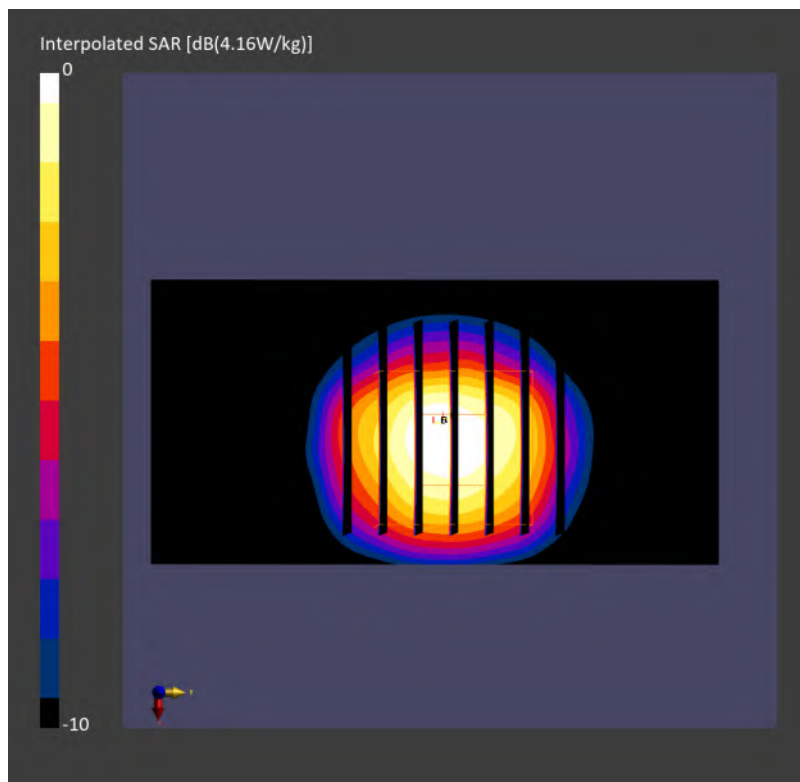

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260909 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.67$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.52, 6.94, 6.82); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.04 W/kg; SAR (10g) = 1.21 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.12 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

TSL Correction: Positive only

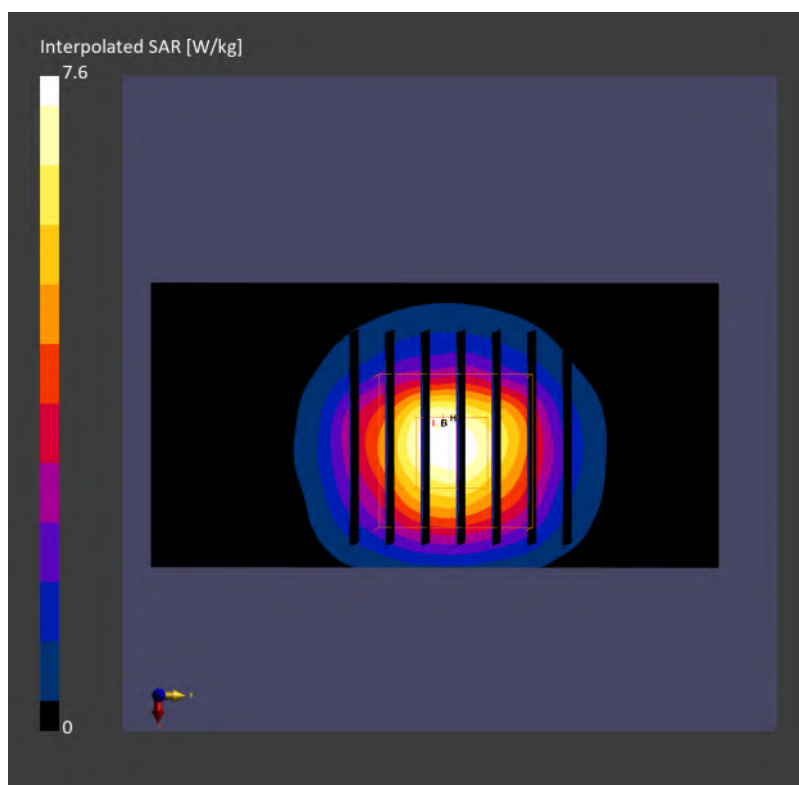

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260910 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.77$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.52, 6.94, 6.82); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.12 W/kg; SAR (10g) = 1.25 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.23 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.3 %

TSL Correction: Positive only

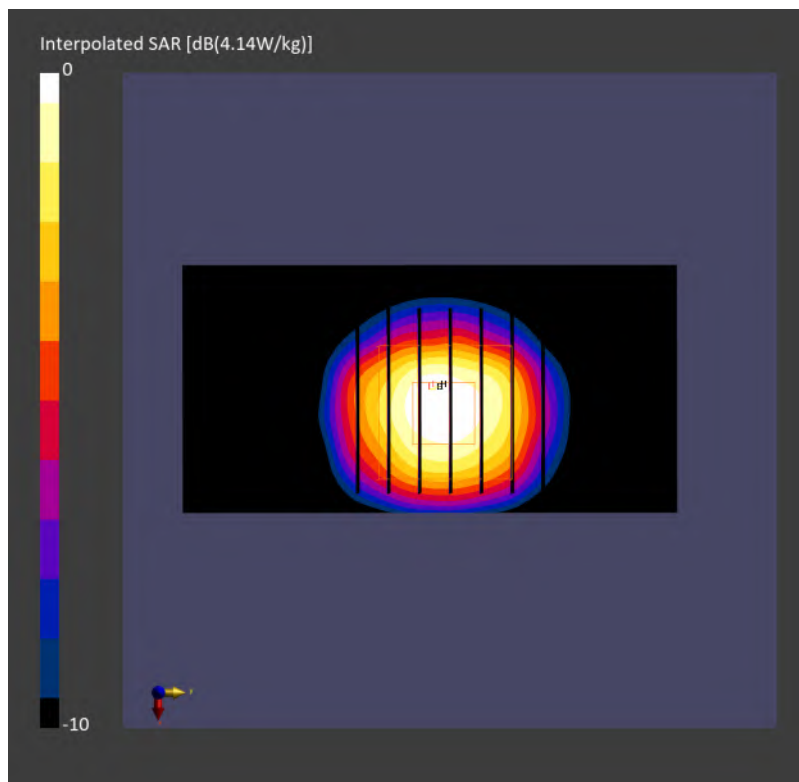

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260911 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.75$ S/m; $\epsilon_r = 36.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.52, 6.94, 6.82); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.09 W/kg; SAR (10g) = 1.23 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.18 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.2 %

TSL Correction: Positive only

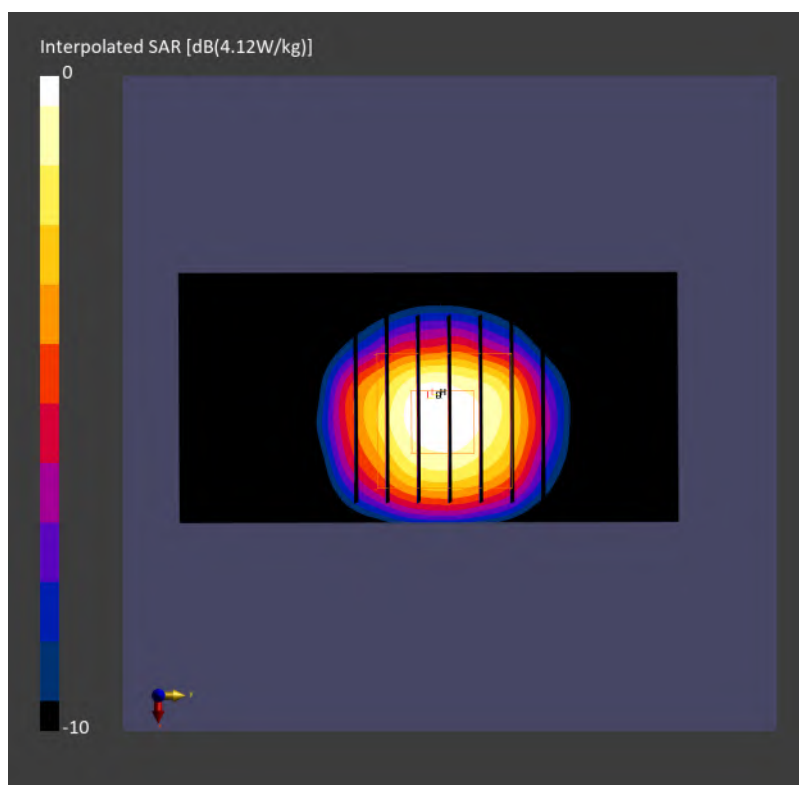

System Check_Head_3500MHz

DUT: D3500V2 - SN1014

Communication System: UID 0, CW; Frequency: 3500 MHz

Medium: HSL_600~7200_260917 Medium parameters used: $f = 3500$ MHz; $\sigma = 2.695$ S/m; $\epsilon_r = 36.736$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.52, 6.94, 6.82) @ 3500 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=100mW/Area Scan (61x61x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

Maximum value of SAR (interpolated) = 11.6 W/kg

Pin=100mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=1.4mm

Reference Value = 67.14 V/m; Power Drift = 0.13 dB


Peak SAR (extrapolated) = 15.4 W/kg

SAR(1 g) = 6.05 W/kg; SAR(10 g) = 2.27 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8 mm

Ratio of SAR at M2 to SAR at M1 = 75.9%

Maximum value of SAR (measured) = 11.6 W/kg

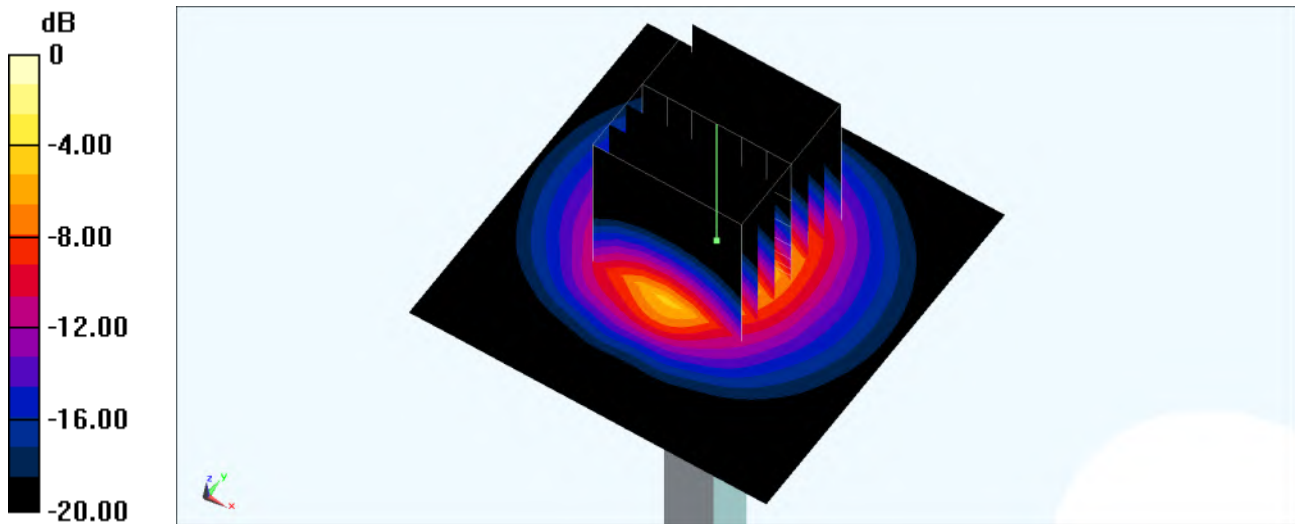

0 dB = 11.6 W/kg = 10.64 dBW/kg

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260821 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.98$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.74, 6.25, 6.69); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.04 W/kg; SAR (10g) = 2.19 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 6.64 W/kg; SAR (8g) = 2.72 W/kg; SAR (10g) = 2.42 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.4 %

TSL Correction: Positive only

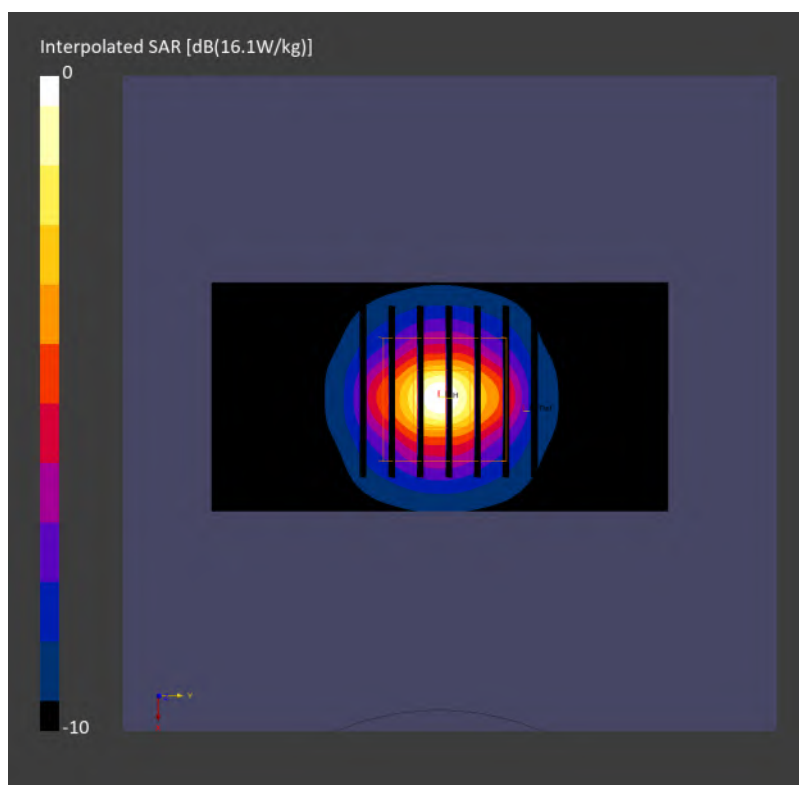

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260823 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.88$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(6.61, 6.72, 6.43); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.25 W/kg; SAR (10g) = 2.30 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.51 W/kg; SAR (8g) = 2.83 W/kg; SAR (10g) = 2.51 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 78.3 %

TSL Correction: Positive only

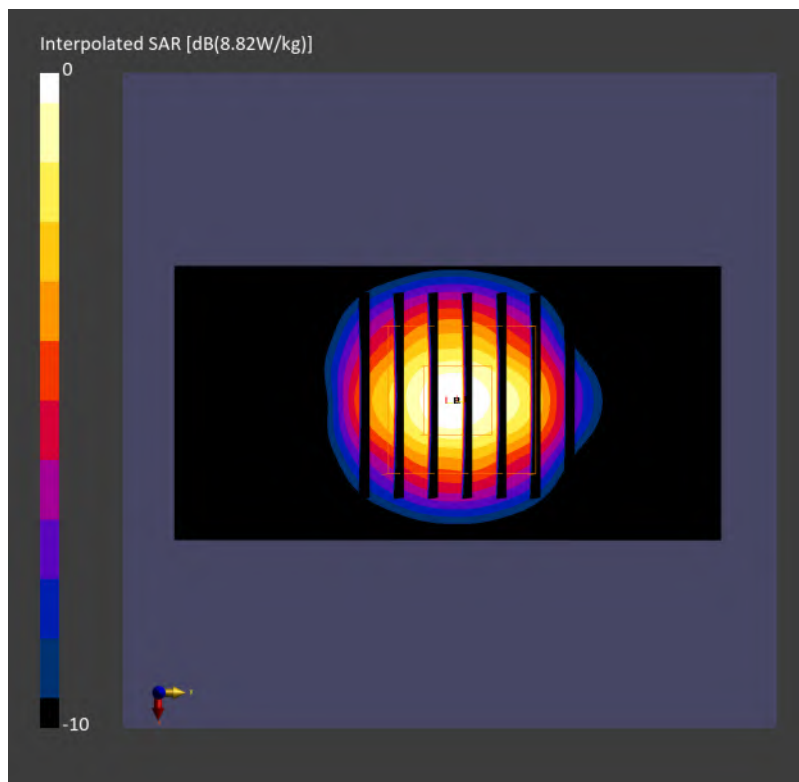

System Check_Head 3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.68, 7.12, 6.72); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.35 W/kg; SAR (10g) = 2.29 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 6.45 W/kg; SAR (8g) = 2.72 W/kg; SAR (10g) = 2.41 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

TSL Correction: Positive only

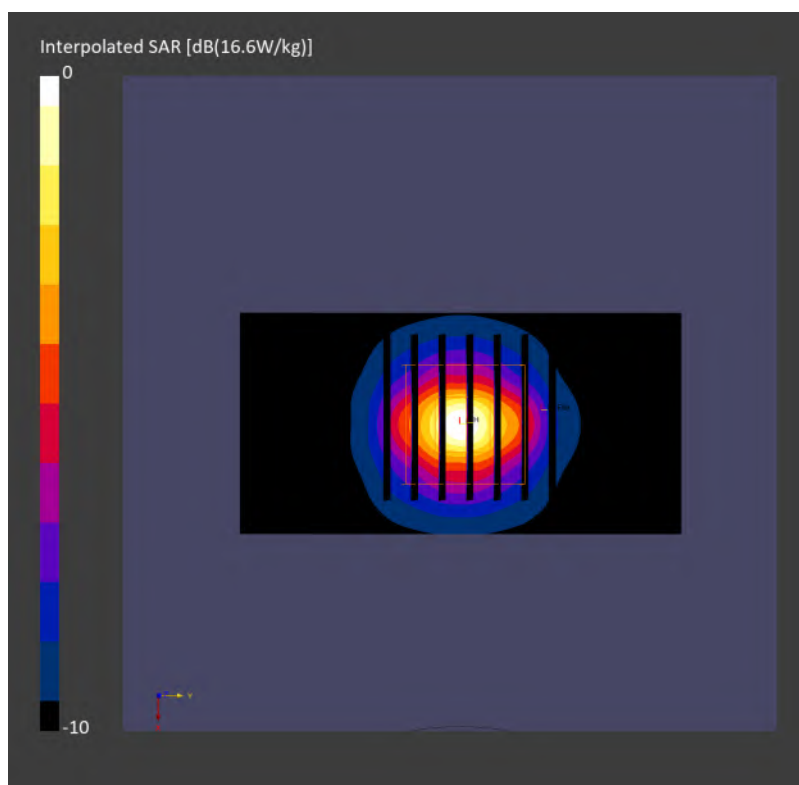

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.87$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.74, 6.25, 6.69); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.18 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.26 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.7 %

TSL Correction: Positive only

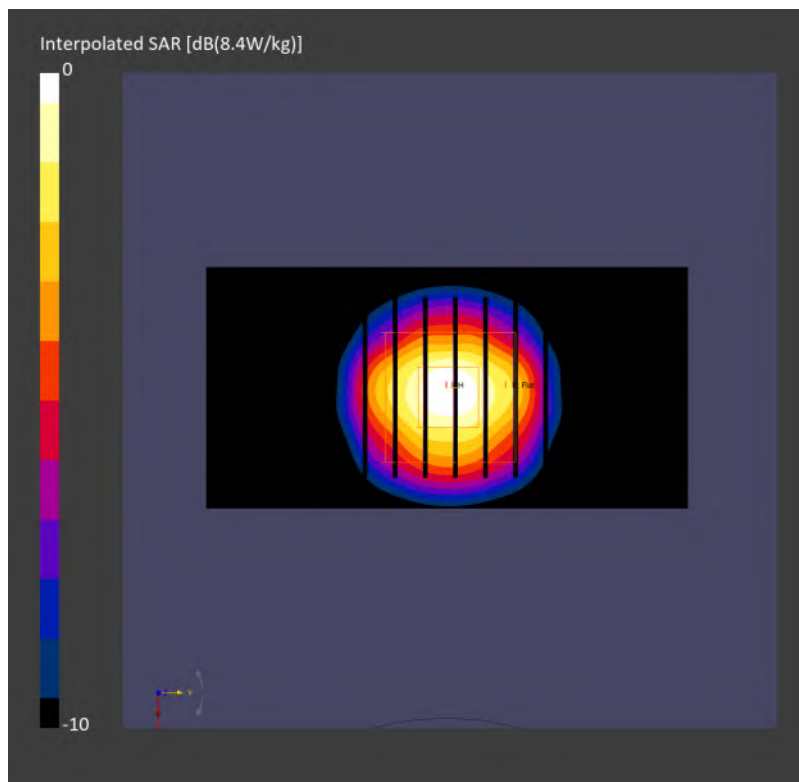

System Check_Head 3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.93$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.68, 7.12, 6.72); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.08 W/kg; SAR (10g) = 1.12 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.16 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

TSL Correction: Positive only

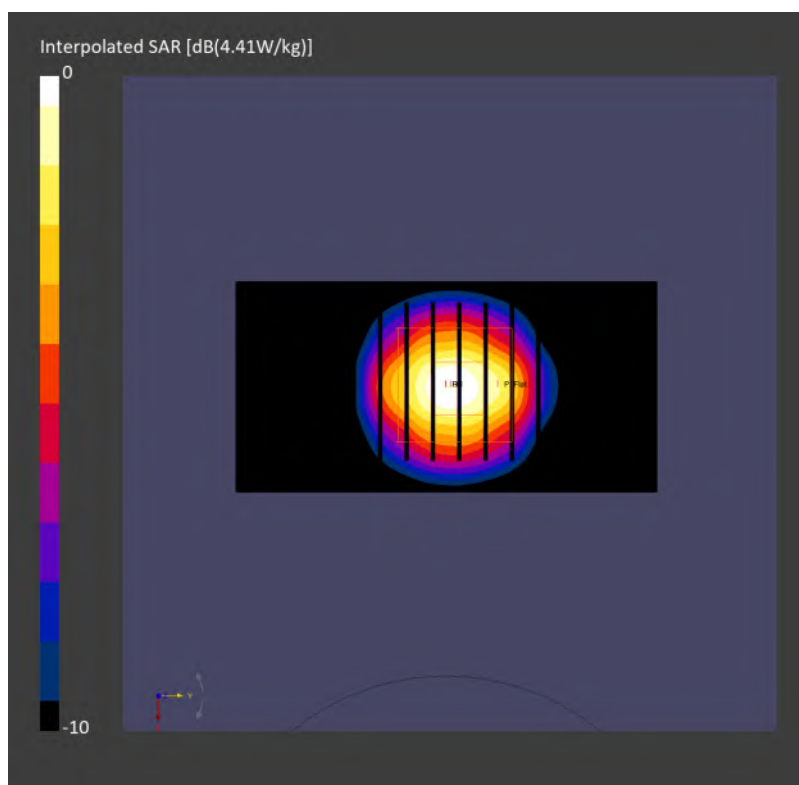

System Check_Head 3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.68, 7.12, 6.72); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.12 W/kg; SAR (10g) = 1.13 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.16 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.0 %

TSL Correction: Positive only

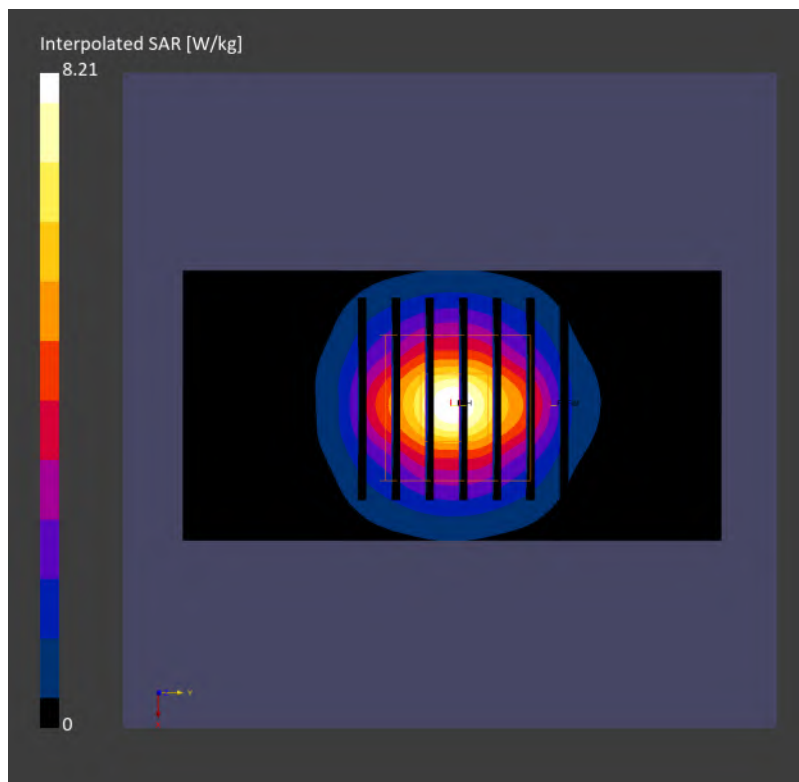

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.84$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.68, 7.12, 6.72); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.14 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

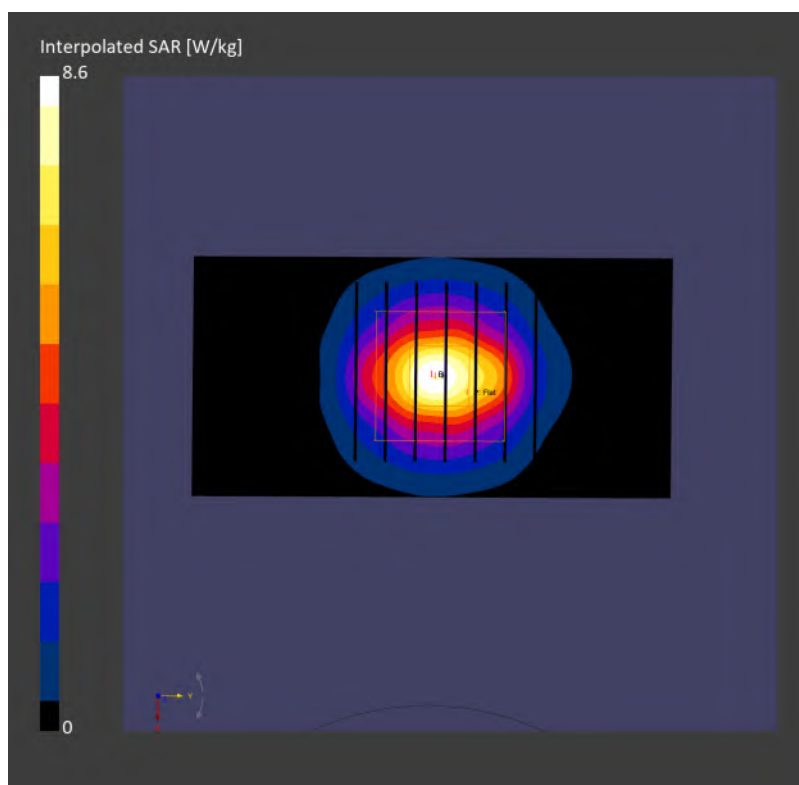

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.85$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.74, 6.25, 6.69); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.32 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

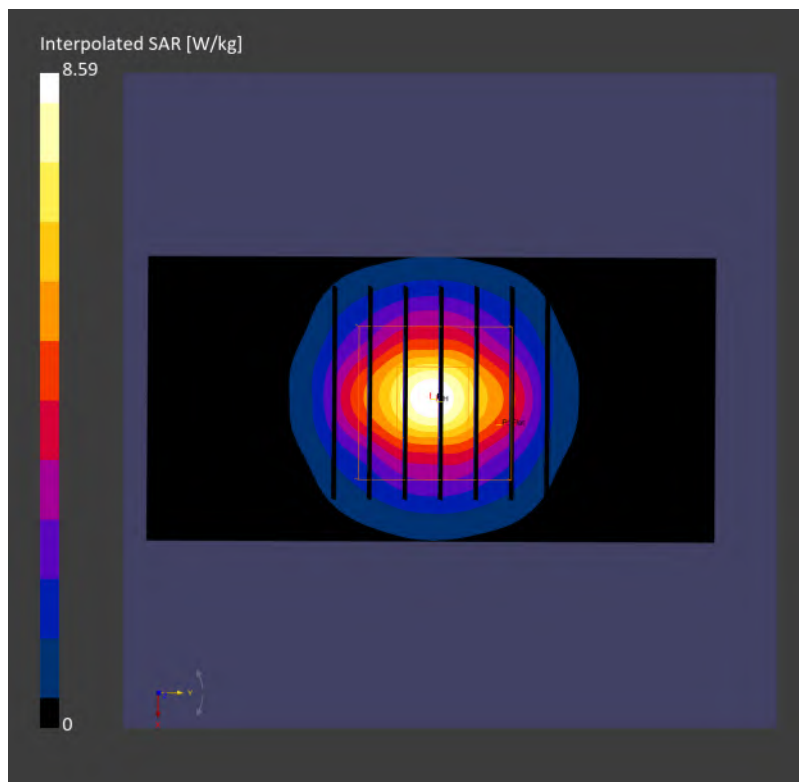

System Check_Head 3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.83$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.68, 7.12, 6.72); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.06 W/kg; SAR (10g) = 1.10 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.17 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

TSL Correction: Positive only

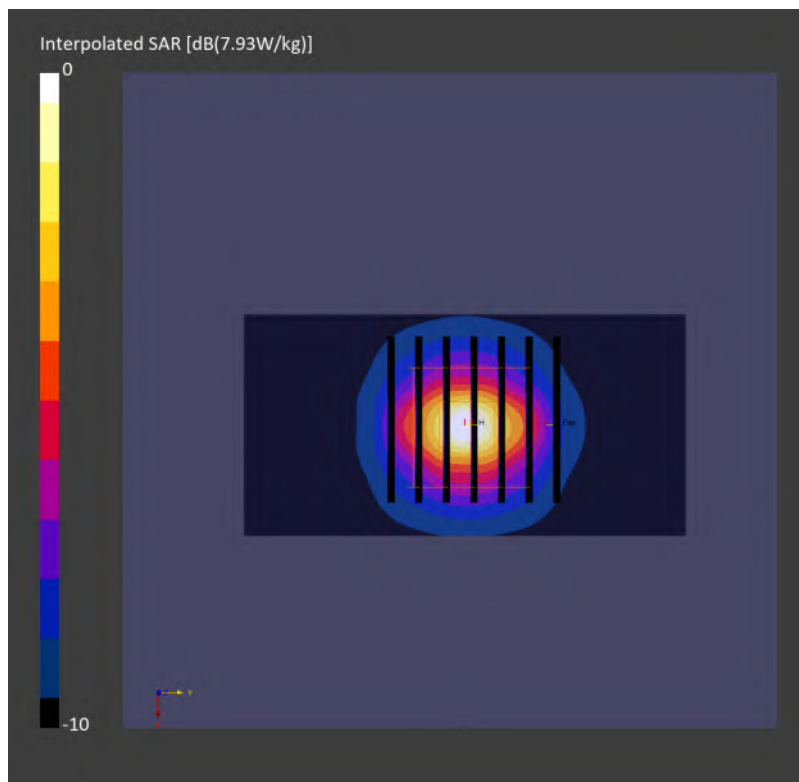

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260908 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.86$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.74, 6.25, 6.69); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.29 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.8 %

TSL Correction: Positive only

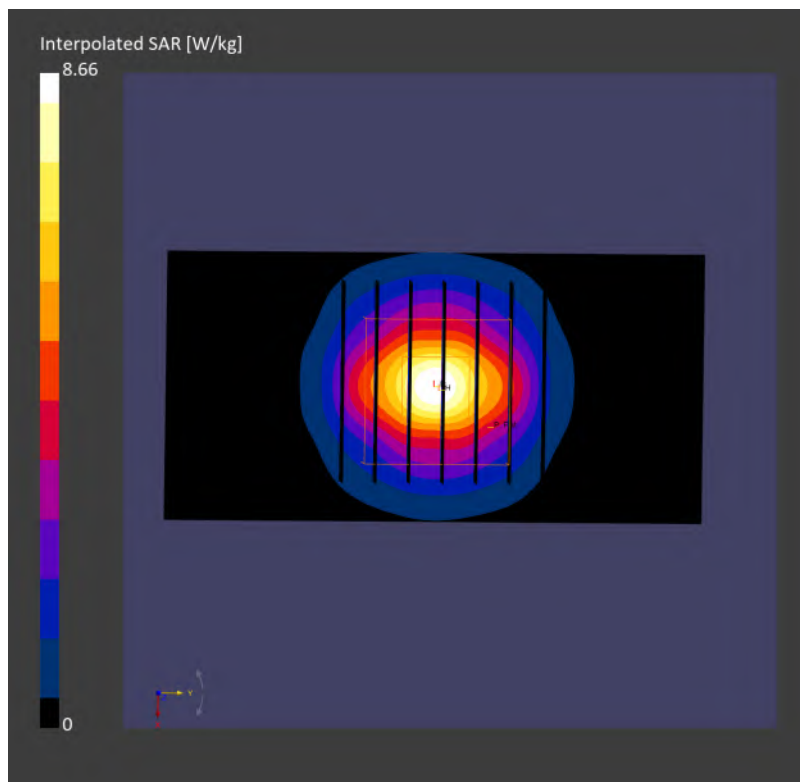

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260912 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.47, 6.89, 6.77); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.15 W/kg; SAR (10g) = 1.20 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.22 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

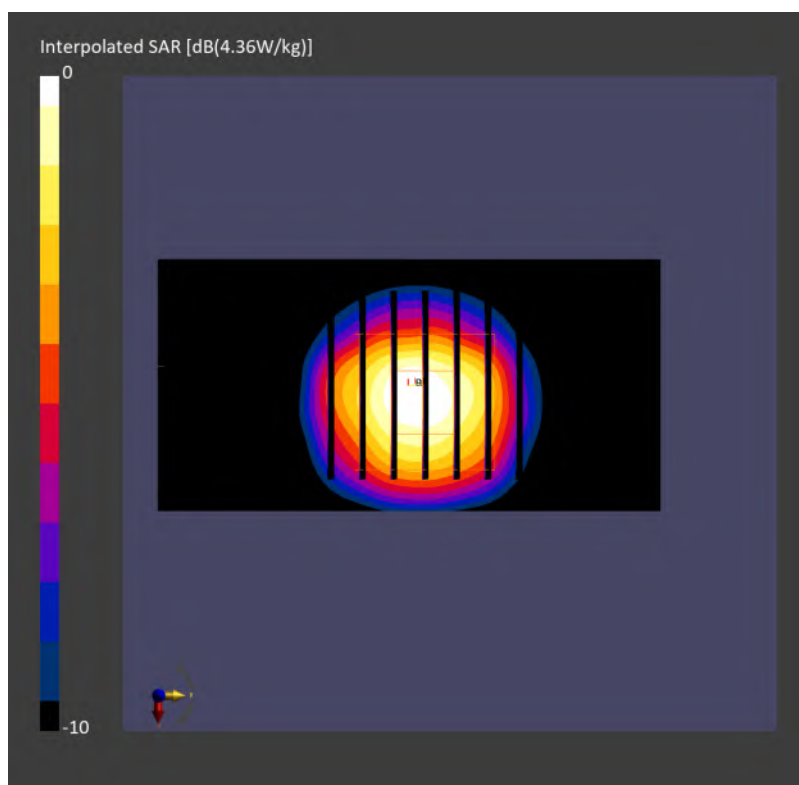

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260913 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.47, 6.89, 6.77); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.14 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.21 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

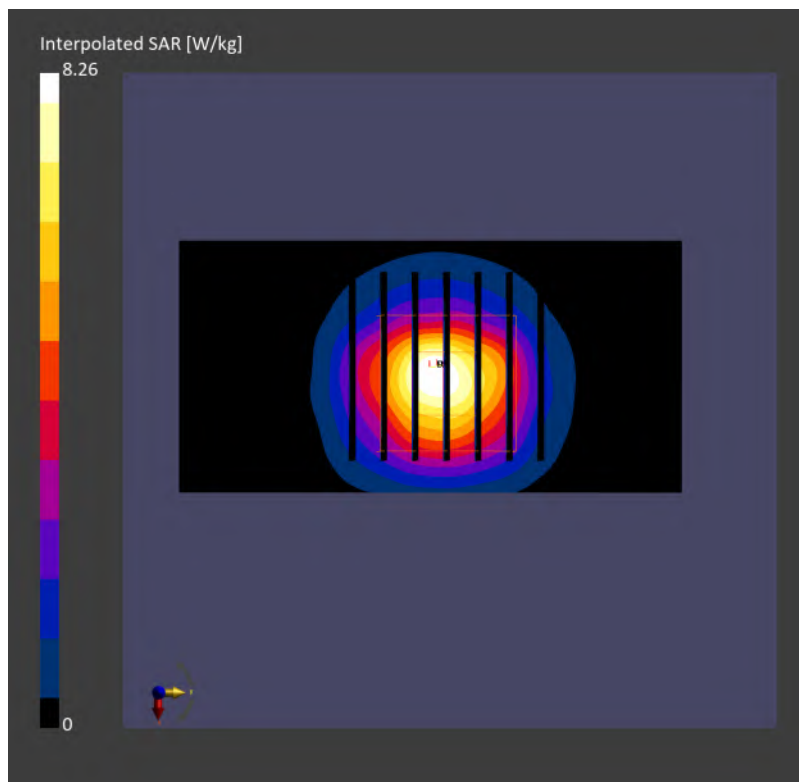

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260914 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.47, 6.89, 6.77); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 3.20 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

TSL Correction: Positive only

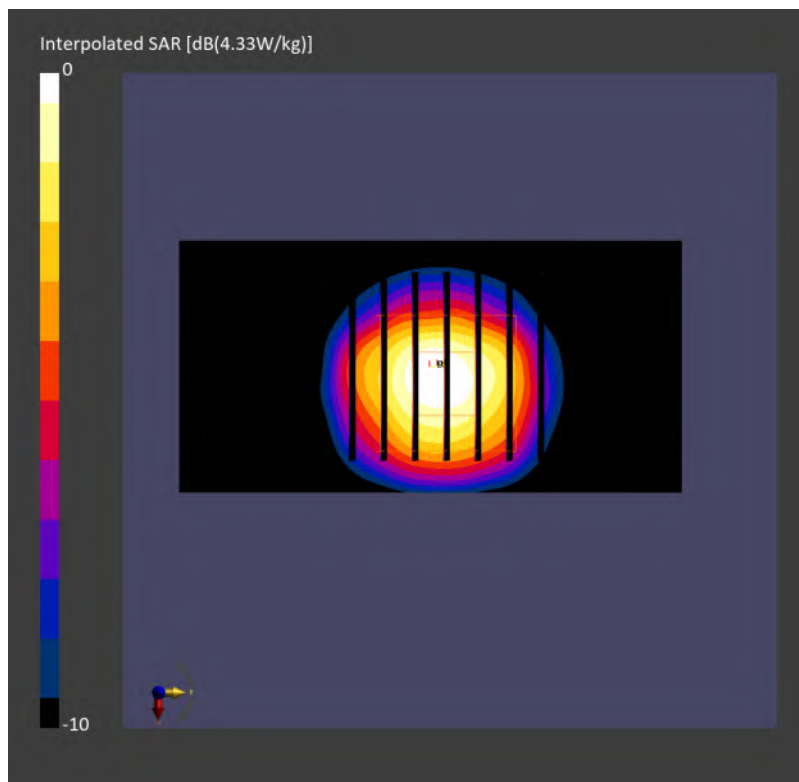

System Check_Head_3700MHz**DUT: D3700V2 - SN1022**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260915 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.47, 6.89, 6.77); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm) : Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.20 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.1 %

TSL Correction: Positive only

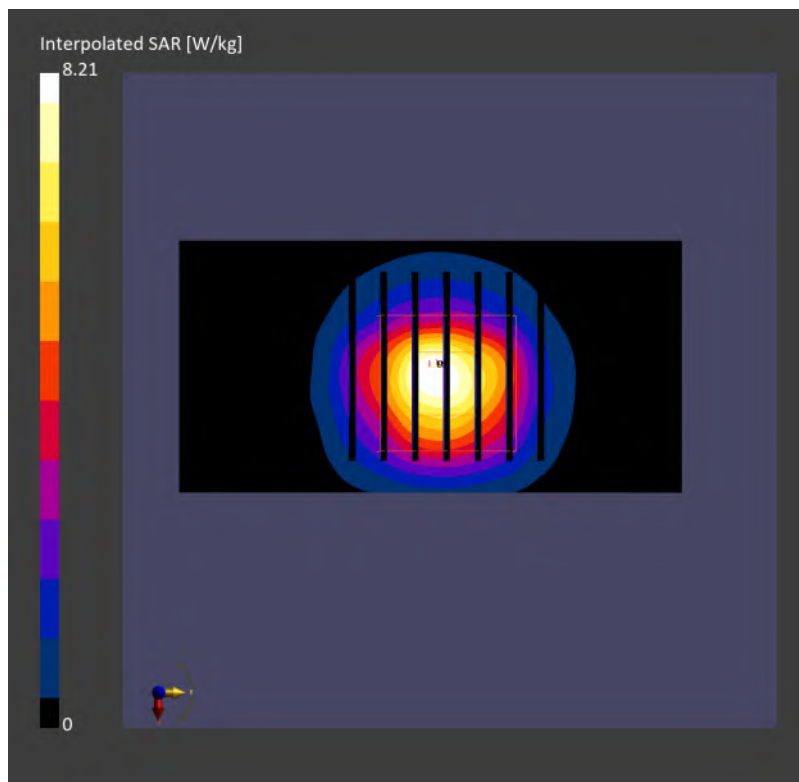

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: UID 0, CW; Frequency: 3700 MHz

Medium: HSL_600~7200_260916 Medium parameters used: $f = 3700$ MHz; $\sigma = 2.998$ S/m; $\epsilon_r = 37.518$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.47, 6.89, 6.77) @ 3700 MHz; Calibrated: 2026/8/14
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn699; Calibrated: 2026/2/13
- Phantom: SAM_Right; Type: SAM; Serial: 1303
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7501)

Pin=100mW/Area Scan (61x61x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

Maximum value of SAR (interpolated) = 13.5 W/kg

Pin=100mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=1.4mm

Reference Value = 70.37 V/m; Power Drift = 0.06 dB


Peak SAR (extrapolated) = 18.2 W/kg

SAR(1 g) = 6.83 W/kg; SAR(10 g) = 2.48 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 8 mm

Ratio of SAR at M2 to SAR at M1 = 75.2%

Maximum value of SAR (measured) = 13.6 W/kg

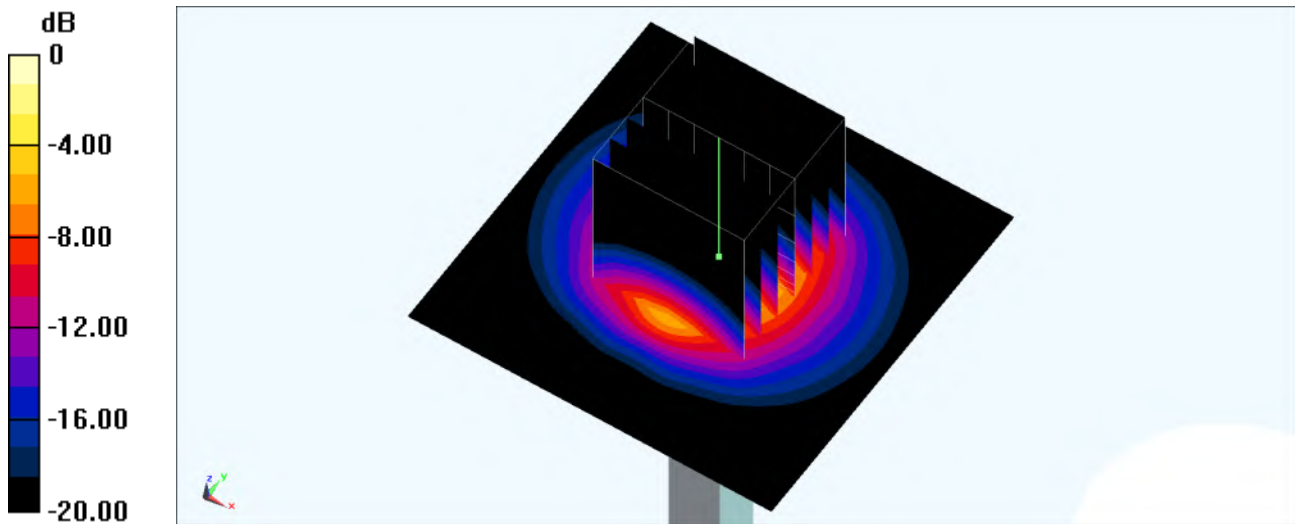

0 dB = 13.6 W/kg = 11.34 dBW/kg

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260821 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.17$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.66, 6.19, 6.62); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.50 W/kg; SAR (10g) = 2.27 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.57 W/kg; SAR (8g) = 2.64 W/kg; SAR (10g) = 2.32 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.2 %

TSL Correction: Positive only

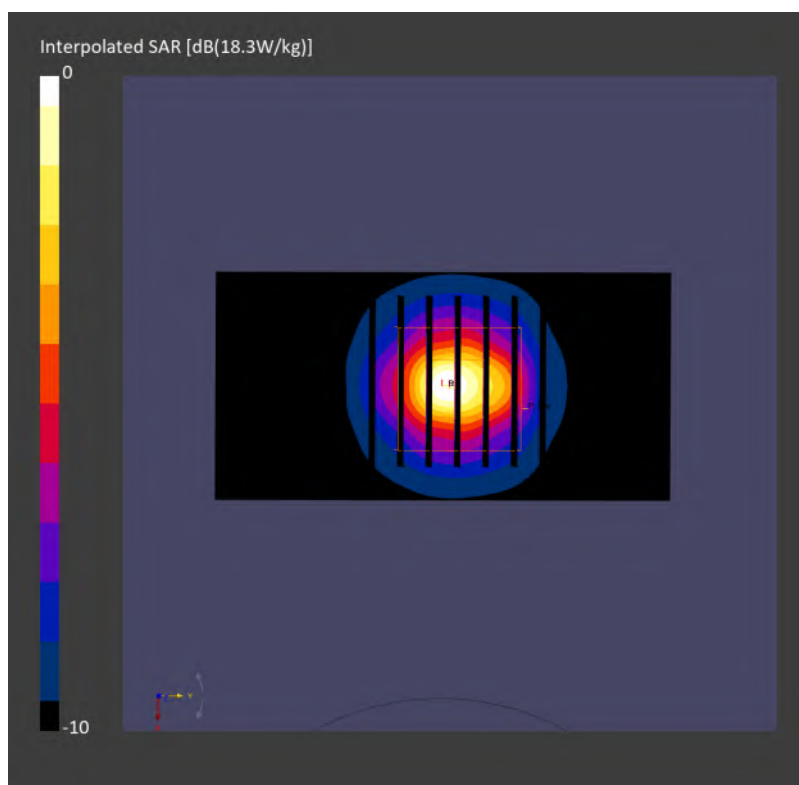

System Check_Head 3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.12$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.46, 6.89, 6.5); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.22 W/kg; SAR (10g) = 2.17 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.03 dB

SAR (1g) = 6.44 W/kg; SAR (8g) = 2.59 W/kg; SAR (10g) = 2.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.4 %

TSL Correction: Positive only

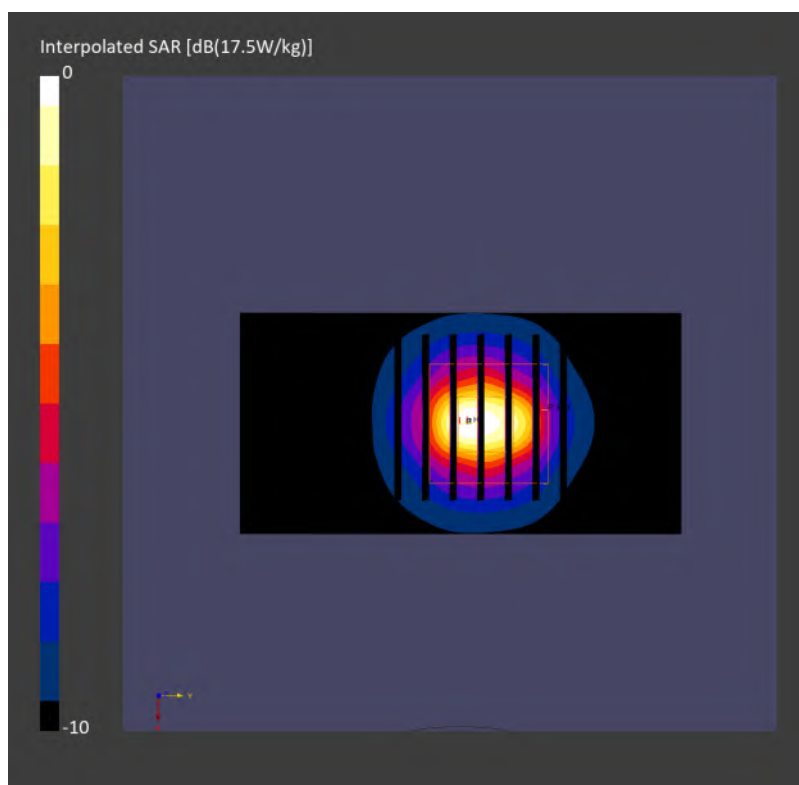

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.66, 6.19, 6.62); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.97 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 2.99 W/kg; SAR (8g) = 1.20 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.6 %

TSL Correction: Positive only

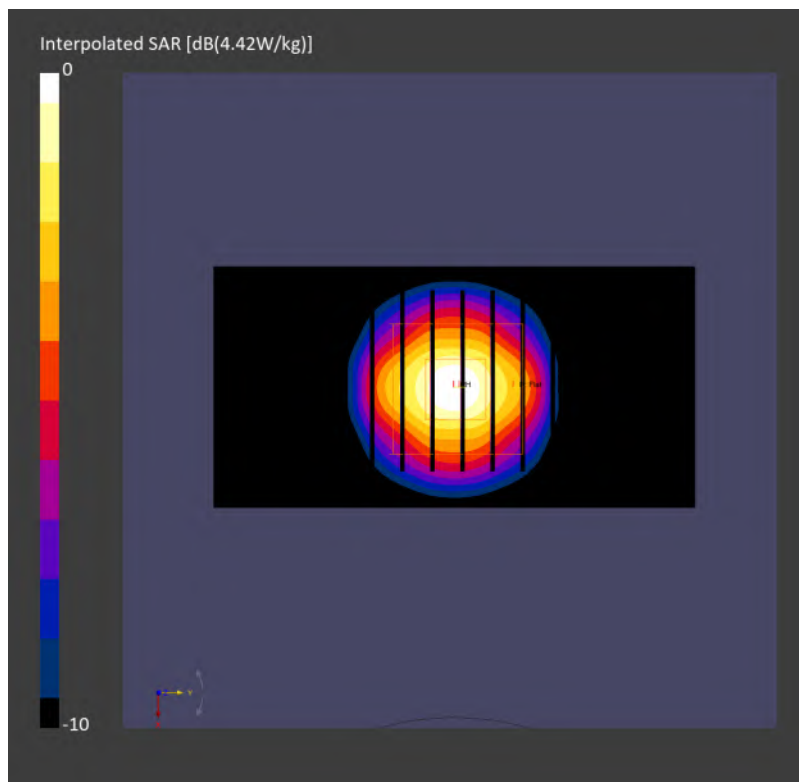

System Check_Head 3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.46, 6.89, 6.5); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.87 W/kg; SAR (10g) = 1.00 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.06 dB

SAR (1g) = 2.97 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

TSL Correction: Positive only

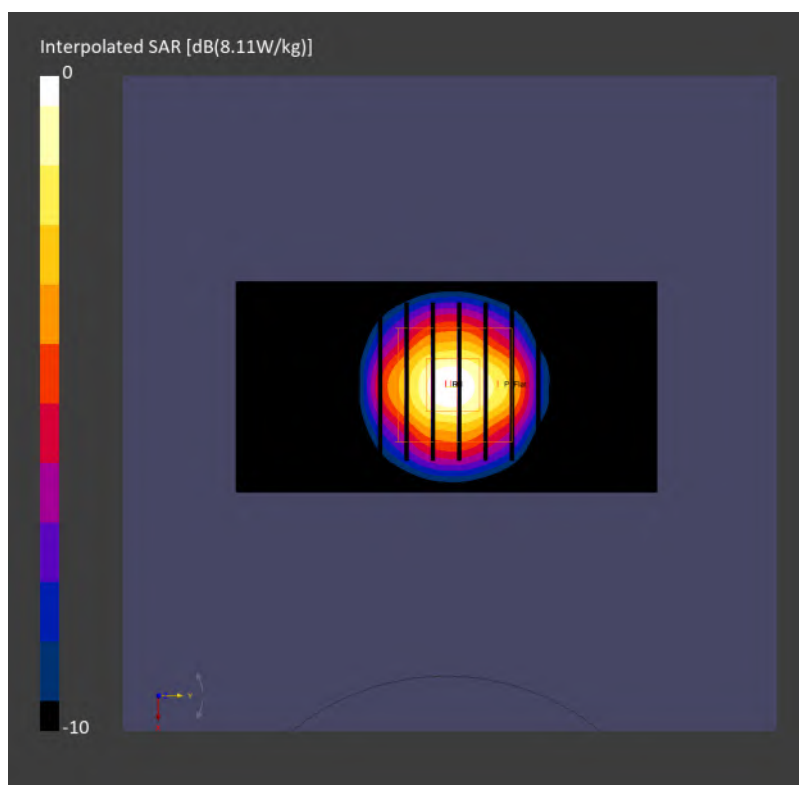

System Check_Head 3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.08$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.46, 6.89, 6.5); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.95 W/kg; SAR (10g) = 1.02 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 3.03 W/kg; SAR (8g) = 1.23 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.6 %

TSL Correction: Positive only

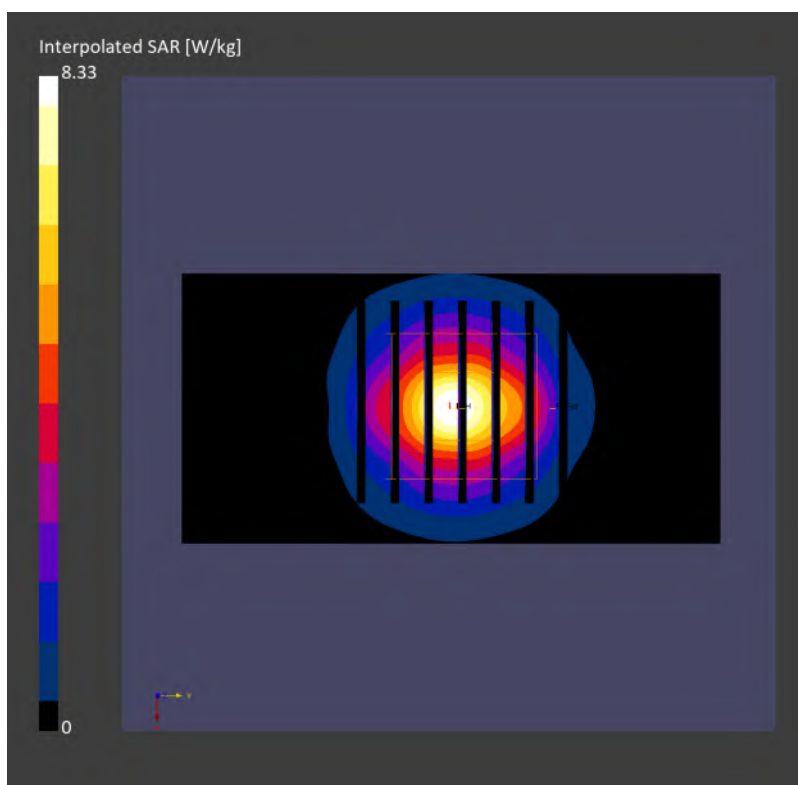

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.05$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.46, 6.89, 6.5); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.45 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.59 W/kg; SAR (8g) = 1.43 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.2 %

TSL Correction: Positive only

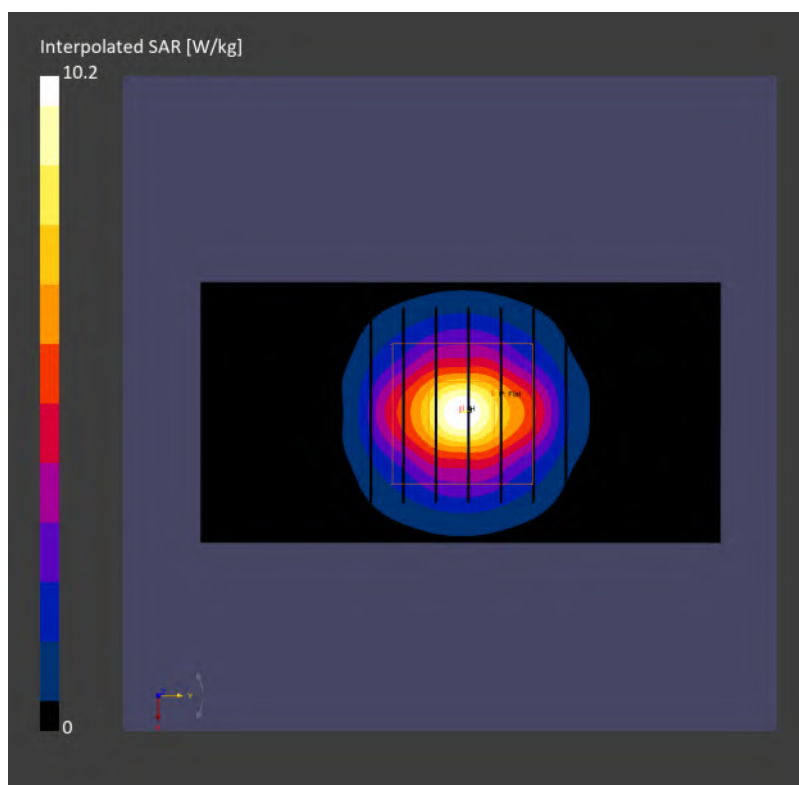

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.03$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.66, 6.19, 6.62); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.97 W/kg; SAR (10g) = 1.06 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 3.14 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.3 %

TSL Correction: Positive only

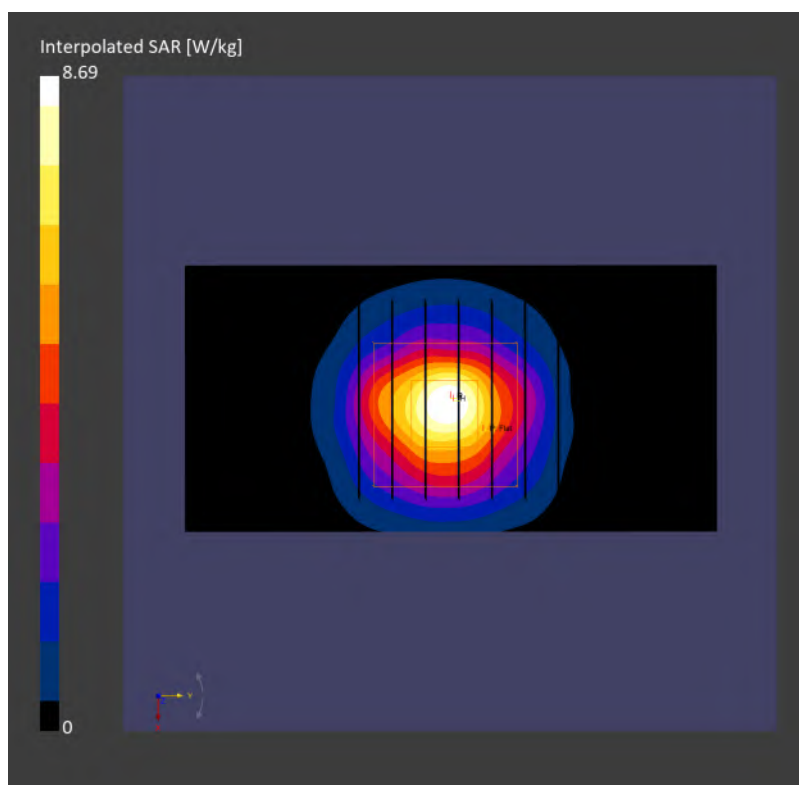

System Check_Head 3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.01$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.46, 6.89, 6.5); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.77 W/kg; SAR (10g) = 0.981 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 2.97 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 7.7 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

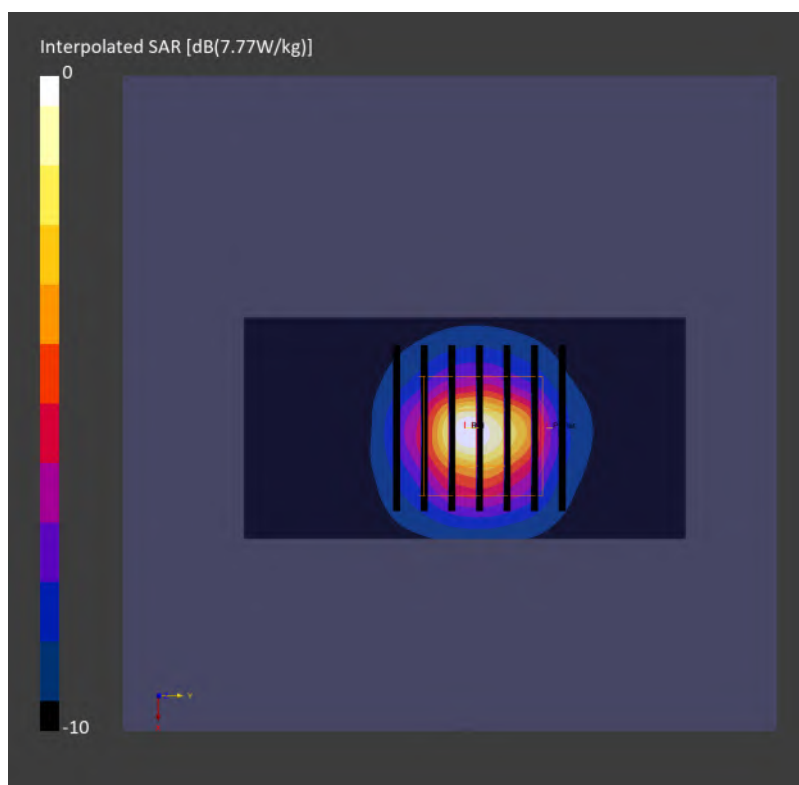

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260908 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.02$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(6.66, 6.19, 6.62); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.94 W/kg; SAR (10g) = 1.05 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 3.12 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.4 %

TSL Correction: Positive only

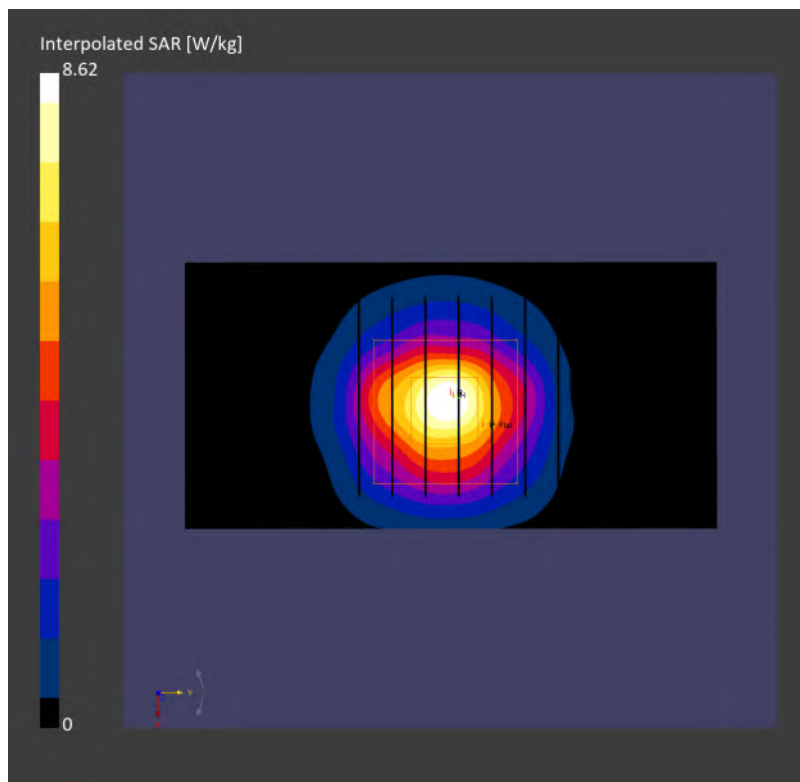

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.49$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.8, 5.38, 5.76); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.49 W/kg; SAR (10g) = 0.987 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.03 dB

SAR (1g) = 3.67 W/kg; SAR (8g) = 1.23 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.8 %

TSL Correction: Positive only

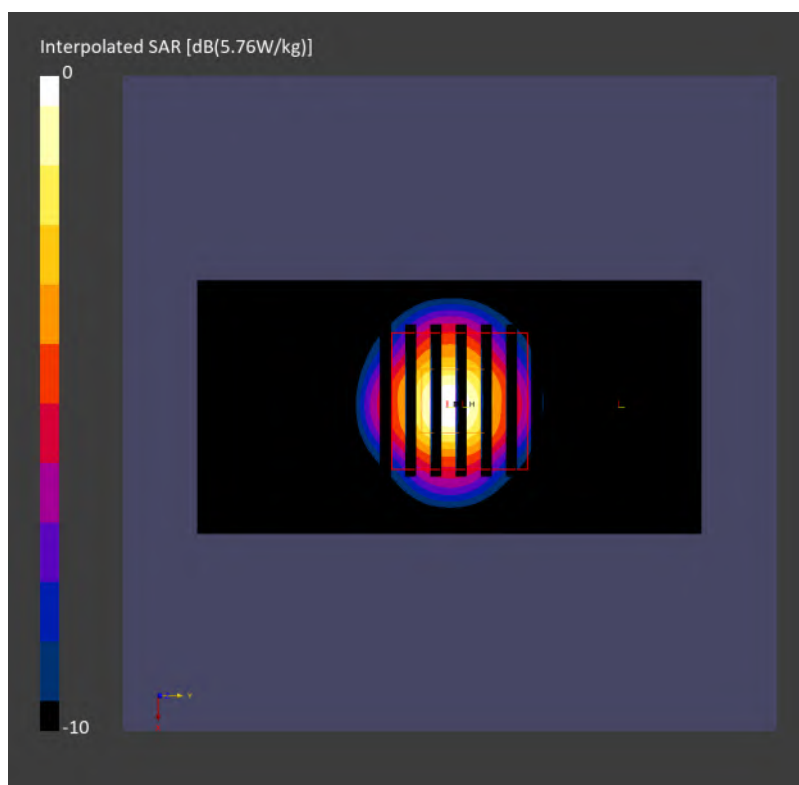

System Check_Head 5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.55$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(5.4, 5.76, 5.43); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.60 W/kg; SAR (10g) = 1.00 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.14 dB

SAR (1g) = 4.12 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 6.9 mm

Ratio of SAR at M2 to SAR at M1 = 65.7 %

TSL Correction: Positive only

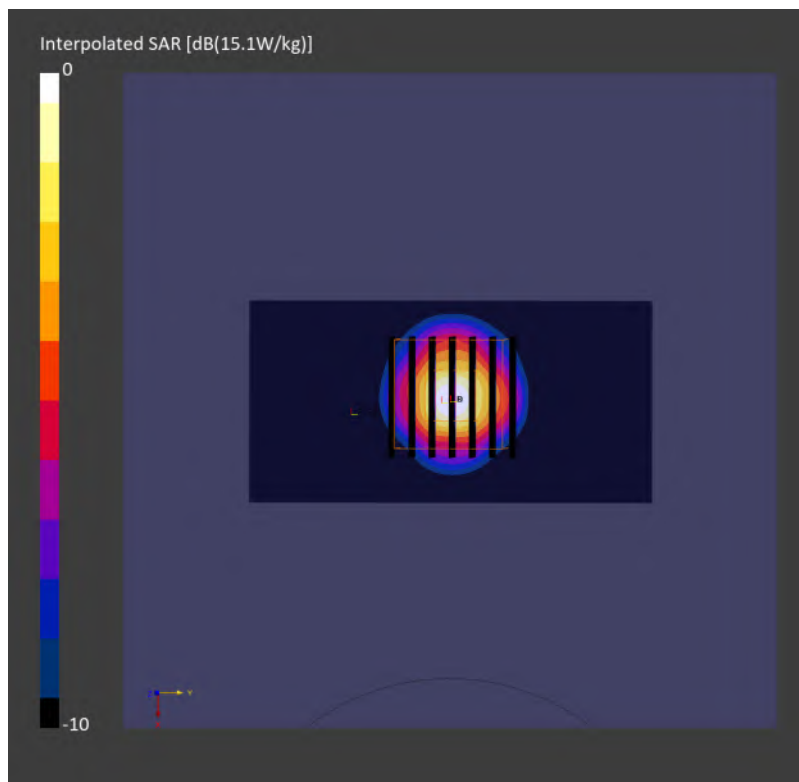

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.53$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.8, 5.38, 5.76); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 0.966 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 3.67 W/kg; SAR (8g) = 1.24 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.6 %

TSL Correction: Positive only

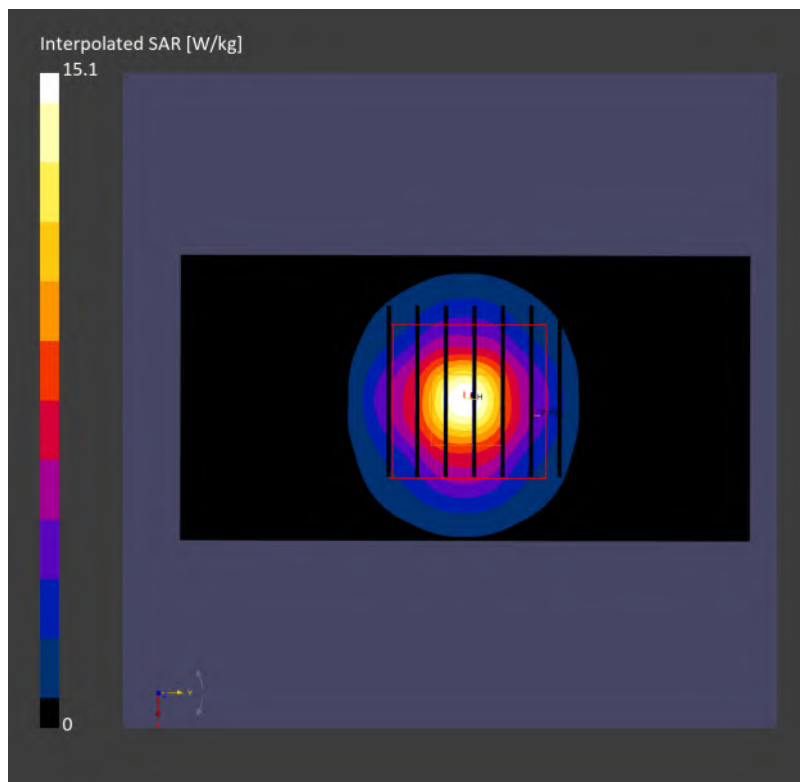

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.90$ S/m; $\epsilon_r = 36.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.38, 5.0, 5.35); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.58 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.04 dB

SAR (1g) = 3.84 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 59.8 %

TSL Correction: Positive only

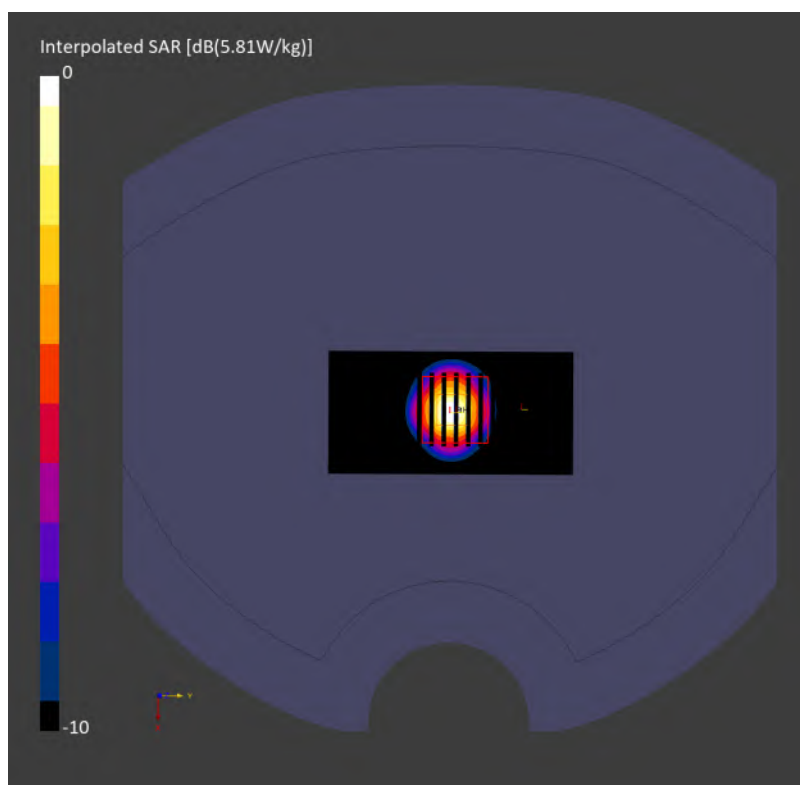

System Check_Head 5600MHz_260902**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.95$ S/m; $\epsilon_r = 34.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(4.92, 5.24, 4.95); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.94 W/kg; SAR (10g) = 1.09 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.12 dB

SAR (1g) = 4.57 W/kg; SAR (8g) = 1.54 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 6.9 mm

Ratio of SAR at M2 to SAR at M1 = 62.5 %

TSL Correction: Positive only

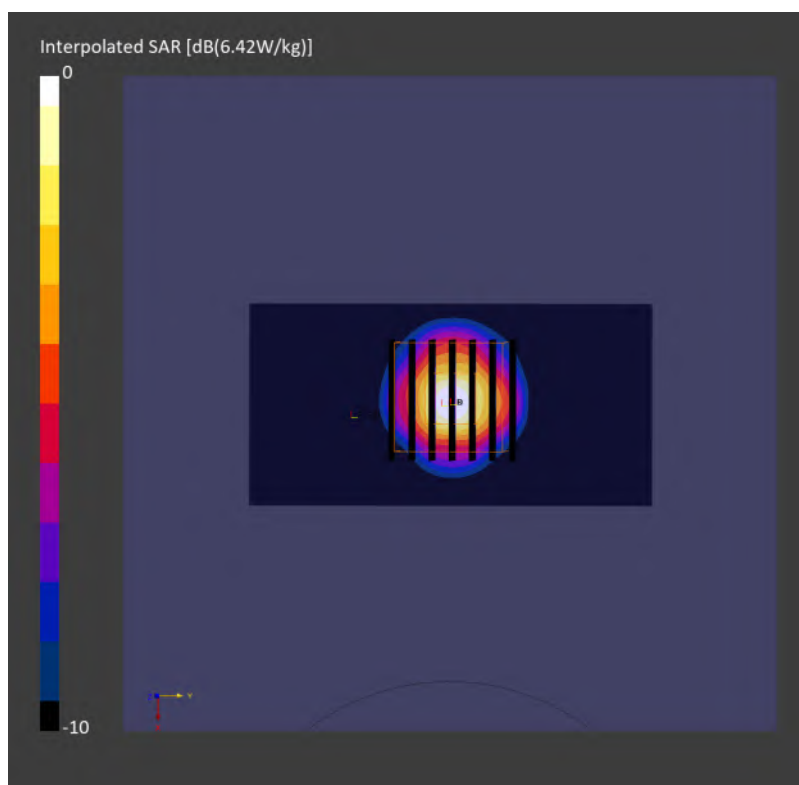

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.89$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.38, 5.0, 5.35); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.63 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.03 dB

SAR (1g) = 3.99 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 59.7 %

TSL Correction: Positive only

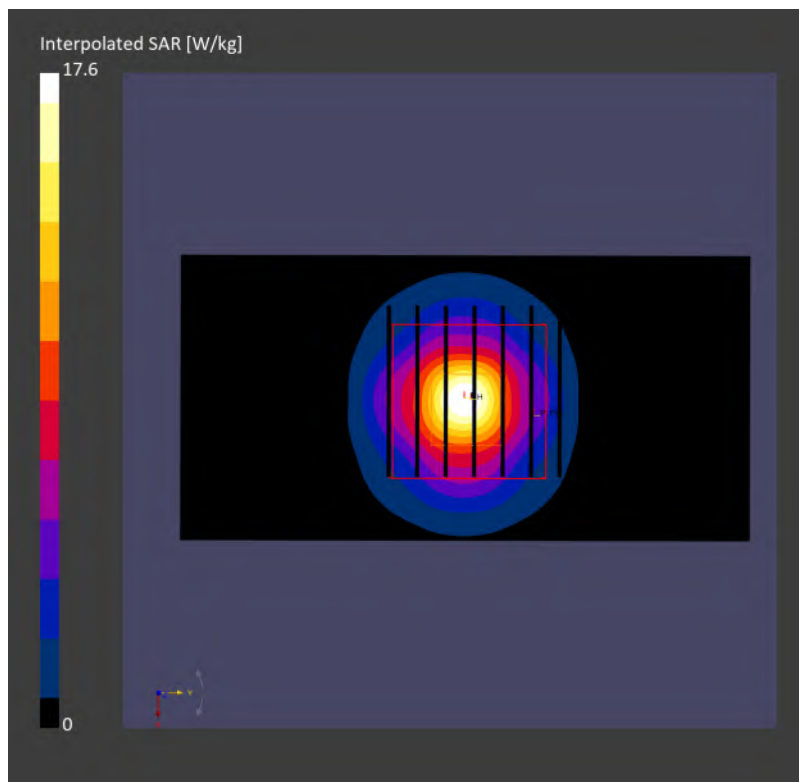

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.14$ S/m; $\epsilon_r = 36.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.23, 4.86, 5.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.48 W/kg; SAR (10g) = 0.977 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.03 dB

SAR (1g) = 3.74 W/kg; SAR (8g) = 1.24 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 57.9 %

TSL Correction: Positive only

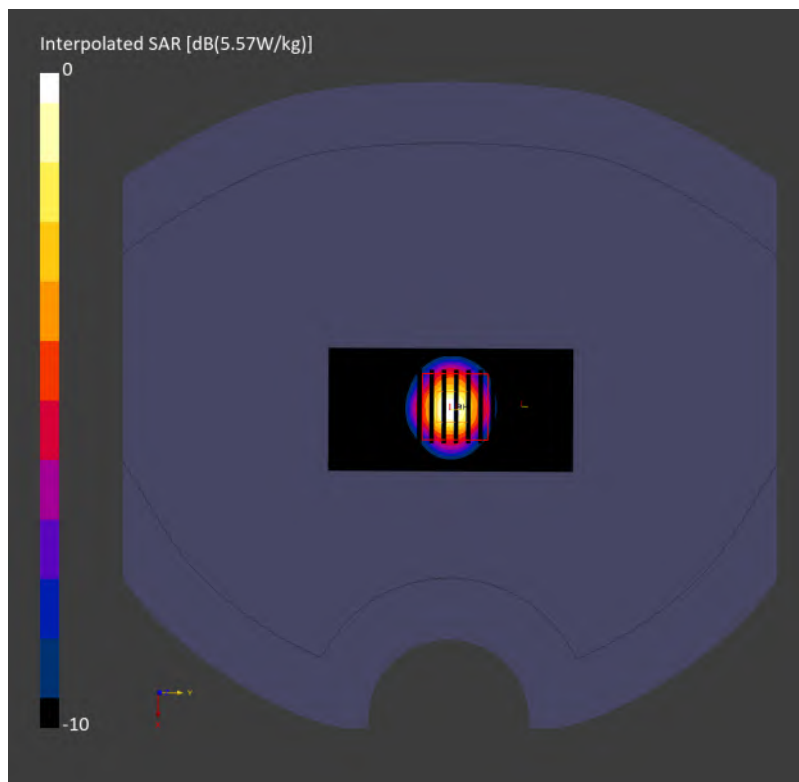

System Check_Head 5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.19$ S/m; $\epsilon_r = 34.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(4.86, 5.17, 4.88); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 0.918 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.05 dB

SAR (1g) = 3.86 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 60.4 %

TSL Correction: Positive only

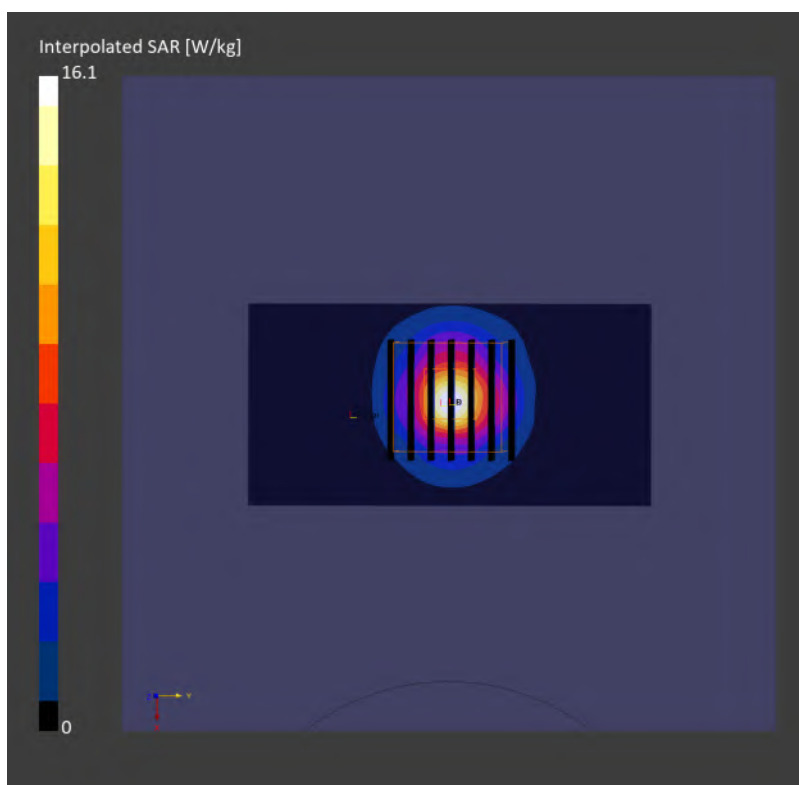

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.13$ S/m; $\epsilon_r = 34.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.23, 4.86, 5.19); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.91 W/kg; SAR (10g) = 1.07 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 4.41 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 57.8 %

TSL Correction: Positive only

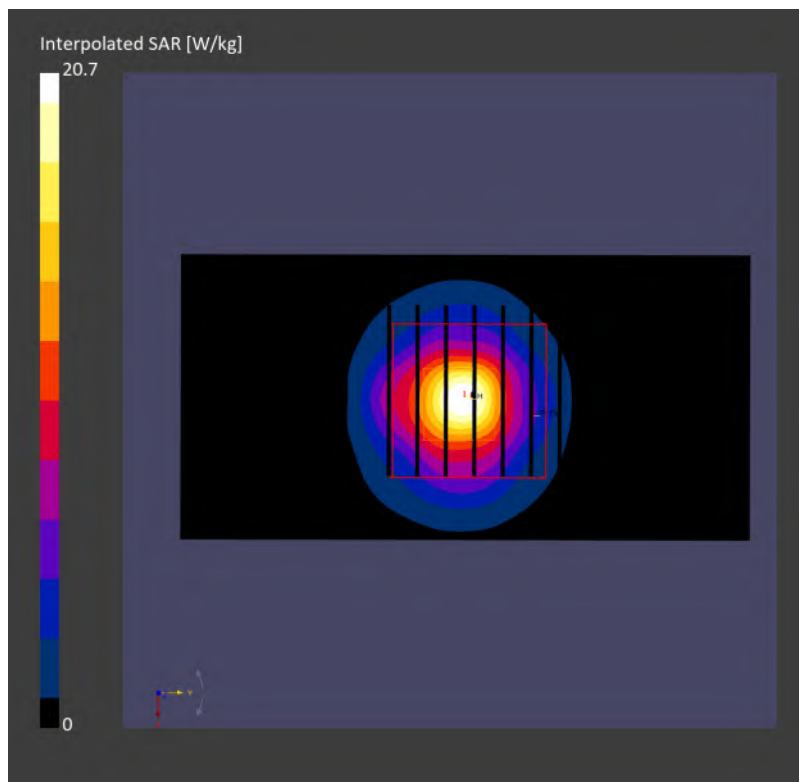

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1083**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_600-7200_260907 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 5.84$ S/m; $\epsilon_r = 33.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(5.49, 5.1, 5.45); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2025-12-03
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0-

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 28.4 W/kg; SAR (10g) = 5.34 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (23.8 mm x 23.8 mm x 22.9 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.09 dB


SAR (1g) = 30.5 W/kg; SAR (8g) = 6.83 W/kg; SAR (10g) = 5.64 W/kg

Smallest distance from peaks to all points 3 dB below = 4.8 mm

Ratio of SAR at M2 to SAR at M1 = 52.0 %

psAPD (1.0cm², sq) = 305 [W/m²]; psAPD (4.0cm², sq) = 137 [W/m²]

TSL Correction: Positive only

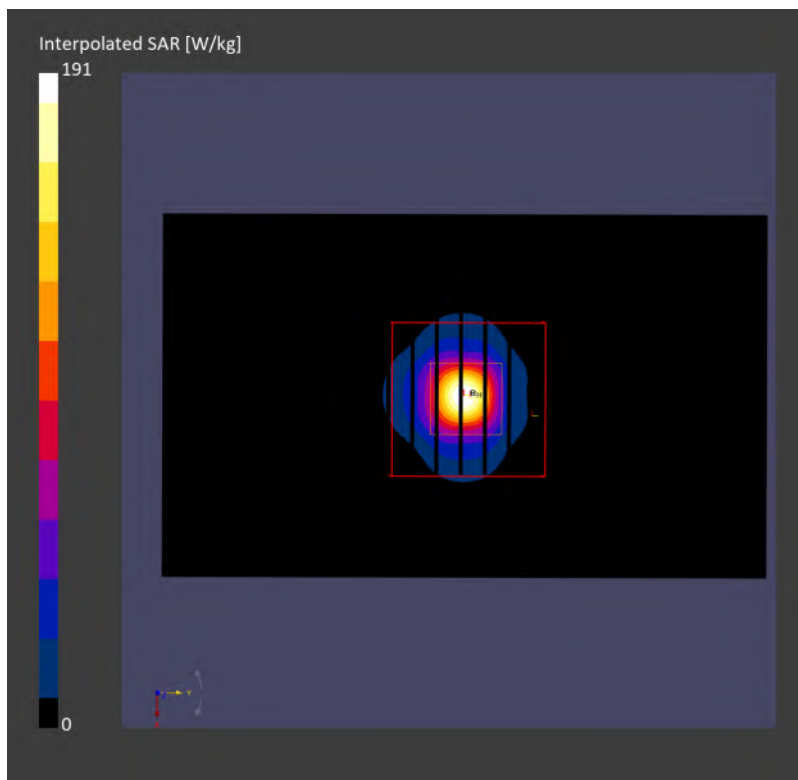

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1083**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_600-7200_260917 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 5.98$ S/m; $\epsilon_r = 34.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.51, 5.61, 5.37); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2025-11-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 23.5 W/kg; SAR (10g) = 4.83 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (23.8 mm x 23.8 mm x 22.9 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.00 dB


SAR (1g) = 27.8 W/kg; SAR (8g) = 6.31 W/kg; SAR (10g) = 5.20 W/kg

Smallest distance from peaks to all points 3 dB below = 4.2 mm

Ratio of SAR at M2 to SAR at M1 = 55.7 %

psAPD (1.0cm², sq) = 278 [W/m²]; psAPD (4.0cm², sq) = 126 [W/m²]

TSL Correction: Positive only

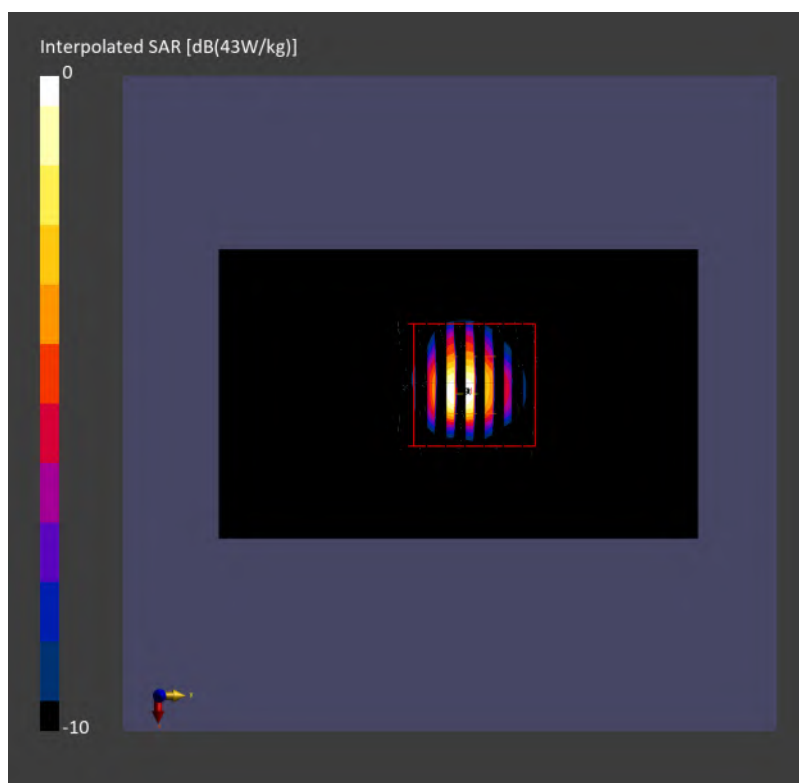

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_261008 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.07$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.46, 6.89, 6.5); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.03 W/kg; SAR (10g) = 2.11 W/kg;

TSL Correction: No correction

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.03 dB

SAR (1g) = 6.22 W/kg; SAR (8g) = 2.56 W/kg; SAR (10g) = 2.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: No correction

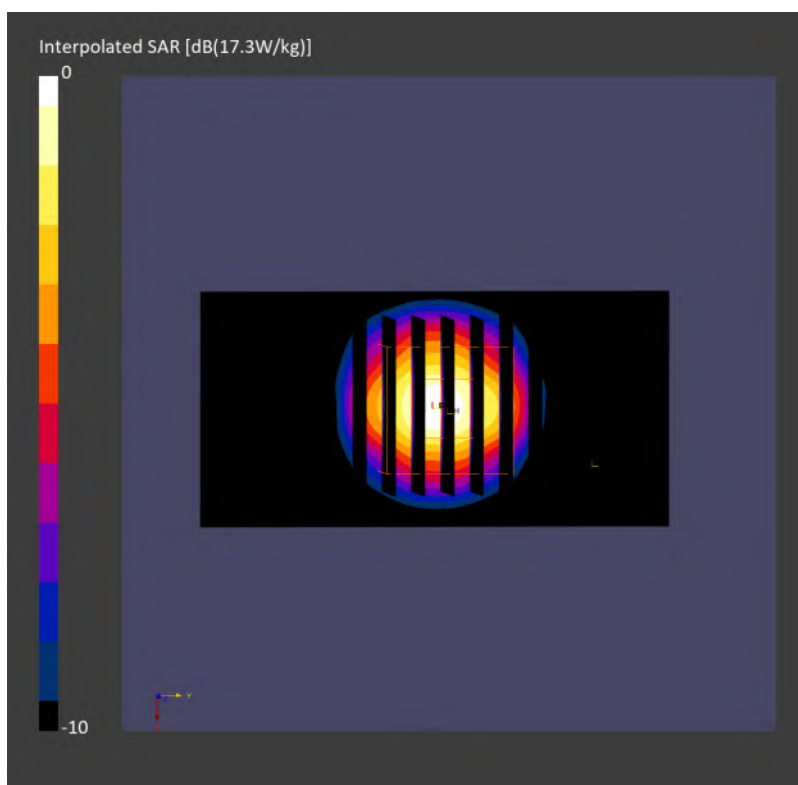

Measurement Report for Device
Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	Software Version	DUT Type
Device,	70.0 x 50.0 x 8.0	3.2.0.1840	5G Verification Source

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Frequency [MHz]	Conversion Factor
5G	FRONT, 10.00	10000.0	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave – 1044	Air –	EUmmWV4 – SN9461_F1–55GHz, 2025–10–15	DAE4 Sn1805, 2026–05–19

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120.0 x 120.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0

Measurement Results

Date	2026–09–07
Avg. Area [cm ²]	4.00
psPDn+ [W/m ²]	56.7
psPDtot+ [W/m ²]	56.9
H _{max} [A/m]	0.414
E _{max} [V/m]	155
max _(Stot) [W/m ²]	63.5
Power Drift [dB]	0.02
IPDn	99.3

