

System Check_Head_13MHz**DUT: CLA-13 - SN1022**

Communication System: CW; Frequency: 13.000 MHz

Medium: HSL_4-250_260906 Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.758$ S/m; $\epsilon_r = 55.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(14.15, 14.46, 14.12); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156_Gap_0414; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=30.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.511 W/kg; SAR (10g) = 0.413 W/kg;

TSL Correction: Positive only

Pin=30.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 0.491 W/kg; SAR (8g) = 0.321 W/kg; SAR (10g) = 0.308 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 75.7 %

TSL Correction: Positive only

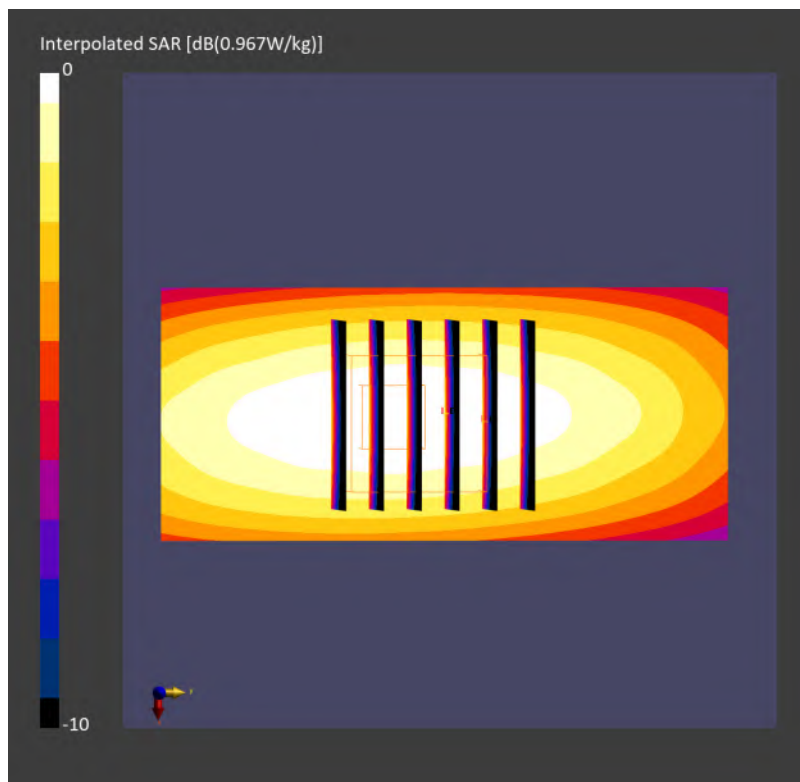

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.906$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.14 W/kg; SAR (10g) = 1.43 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.14 W/kg; SAR (8g) = 1.51 W/kg; SAR (10g) = 1.44 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

TSL Correction: Positive only

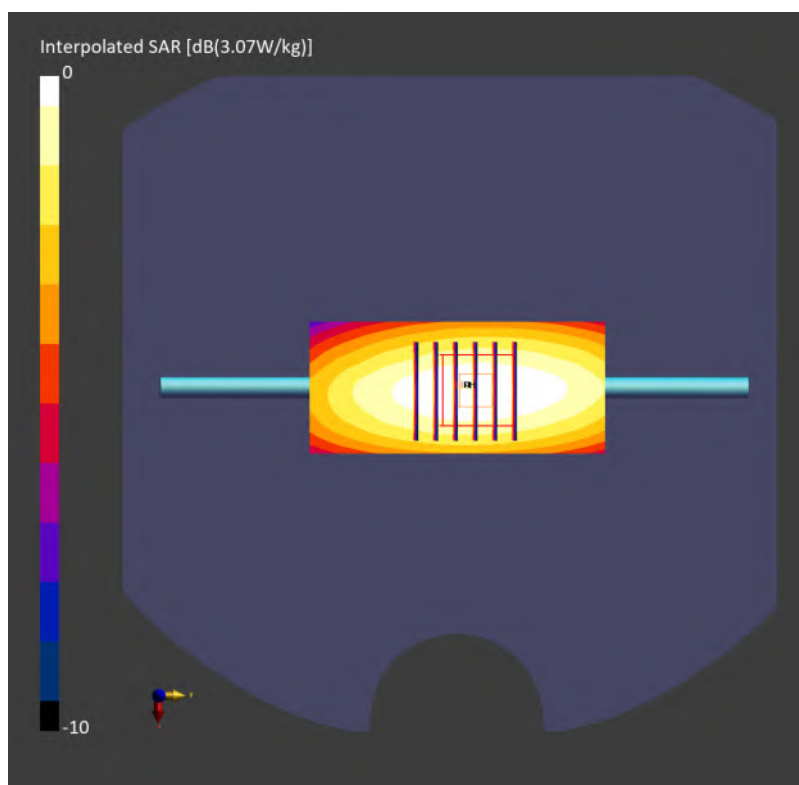

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.903$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.12 W/kg; SAR (10g) = 1.42 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.12 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.43 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

TSL Correction: Positive only

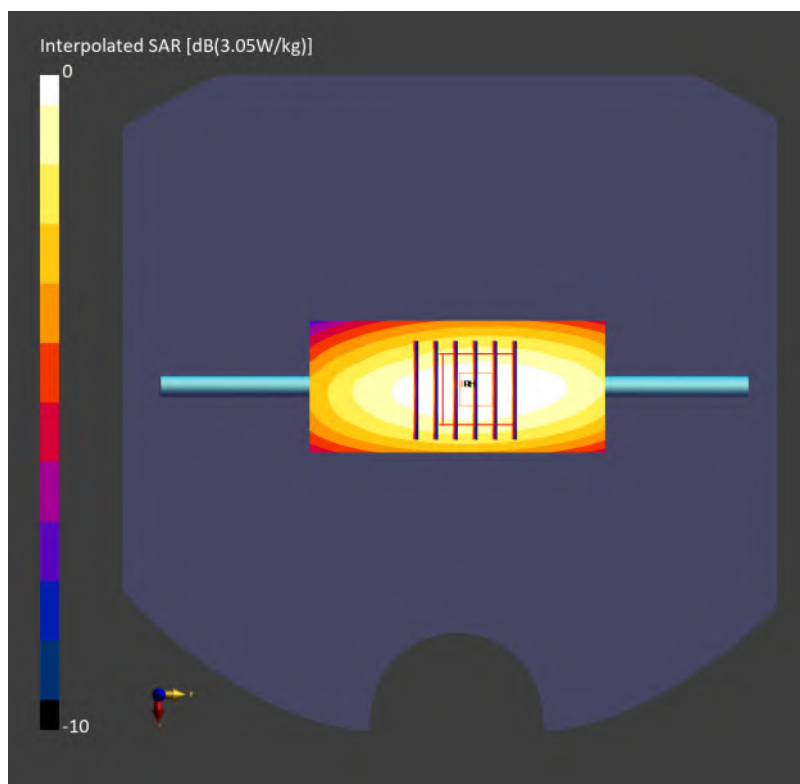

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.880$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.98, 9.68, 9.75); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.34 W/kg; SAR (10g) = 1.55 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.33 W/kg; SAR (8g) = 1.65 W/kg; SAR (10g) = 1.56 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 89.8 %

TSL Correction: Positive only

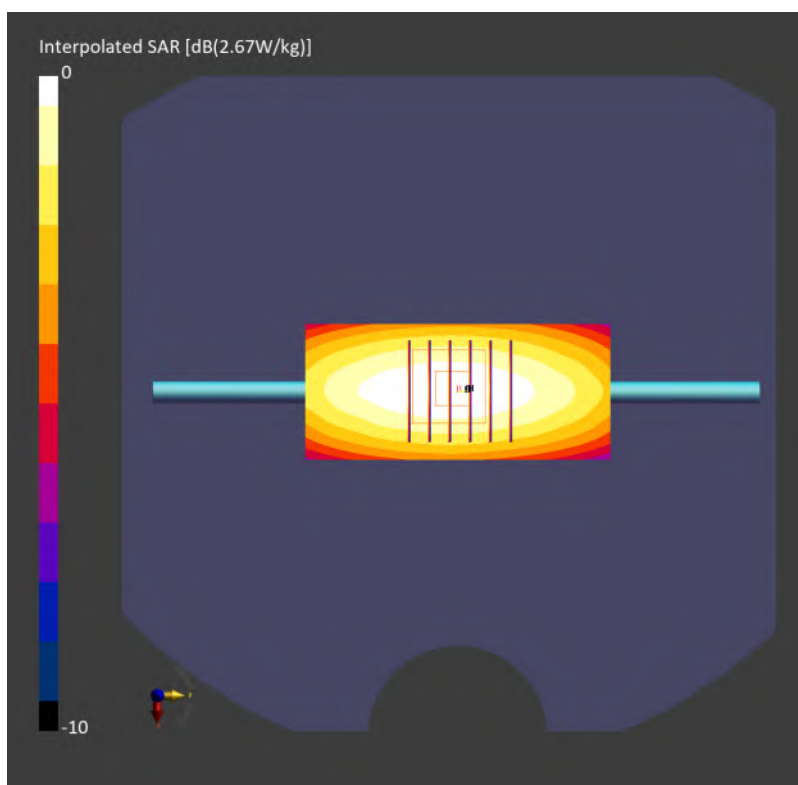

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.26 W/kg; SAR (10g) = 1.51 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 2.26 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.52 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

TSL Correction: Positive only

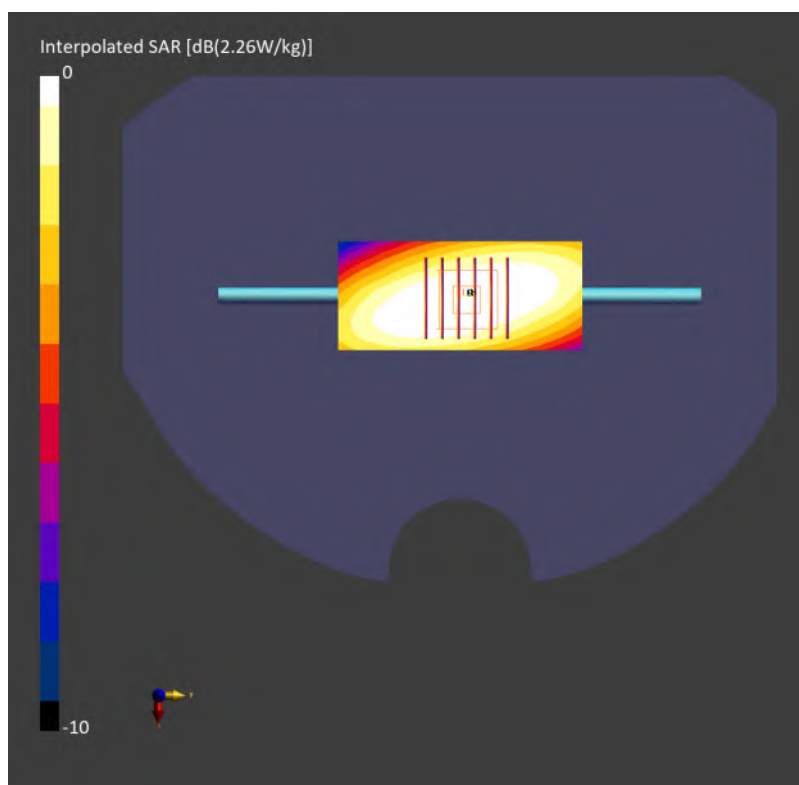

System Check_Head_750MHz**DUT: D750V3 - SN1117**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260901 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.887$ S/m; $\epsilon_r = 45.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.96, 8.94, 8.55); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.14 W/kg; SAR (10g) = 1.42 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.14 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.43 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 89.8 %

TSL Correction: Positive only

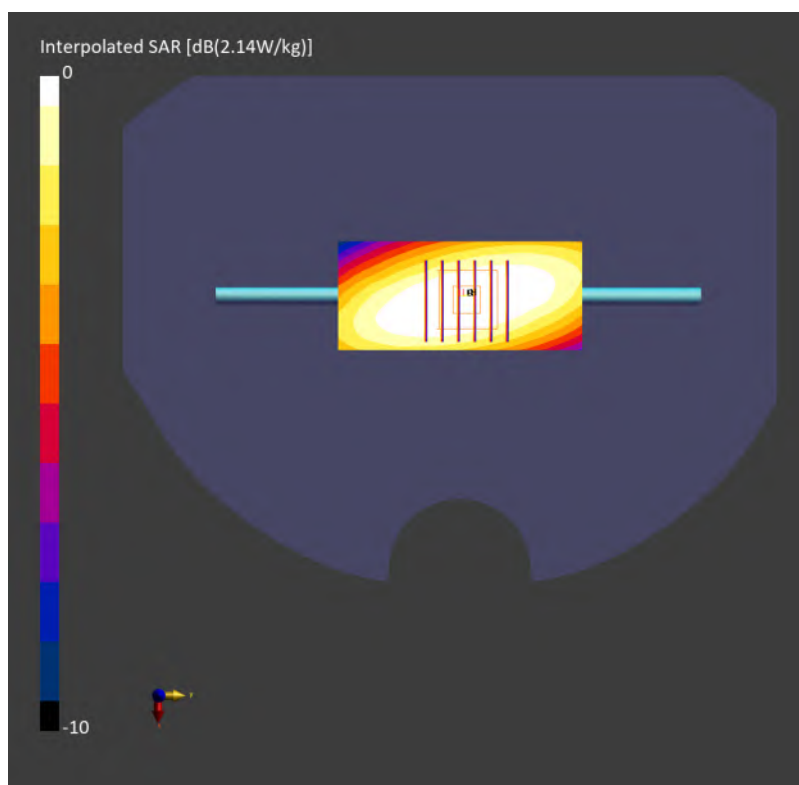

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260918 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.900$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.14, 9.72, 9.56); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.15 W/kg; SAR (10g) = 1.43 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.18 W/kg; SAR (8g) = 1.54 W/kg; SAR (10g) = 1.46 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 88.0 %

TSL Correction: Positive only

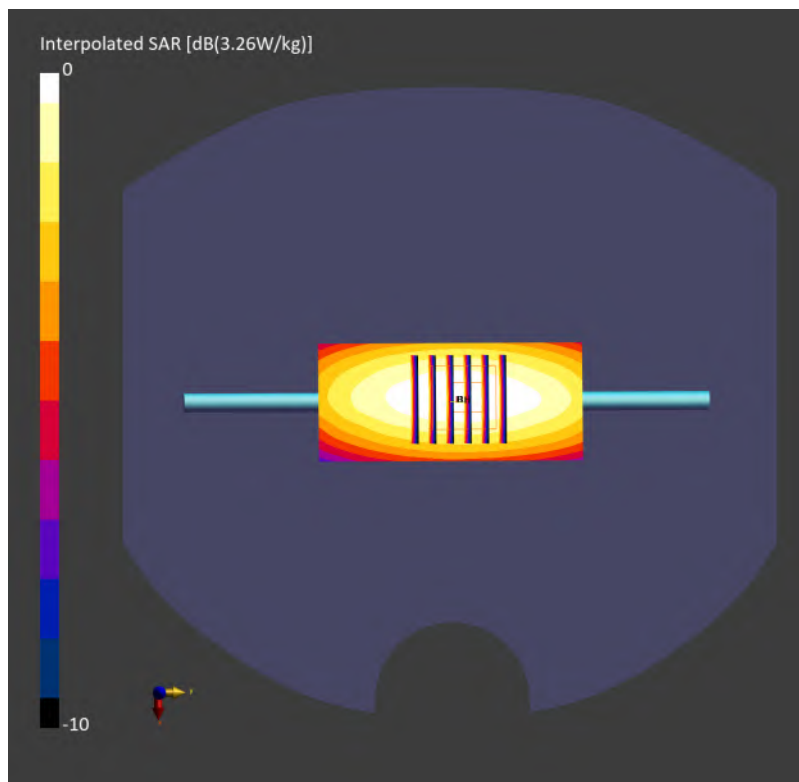

System Check_Head_750MHz**DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_600-7200_260919 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.884$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.14, 9.72, 9.56); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.13 W/kg; SAR (10g) = 1.42 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.17 W/kg; SAR (8g) = 1.53 W/kg; SAR (10g) = 1.45 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 88.1 %

TSL Correction: Positive only

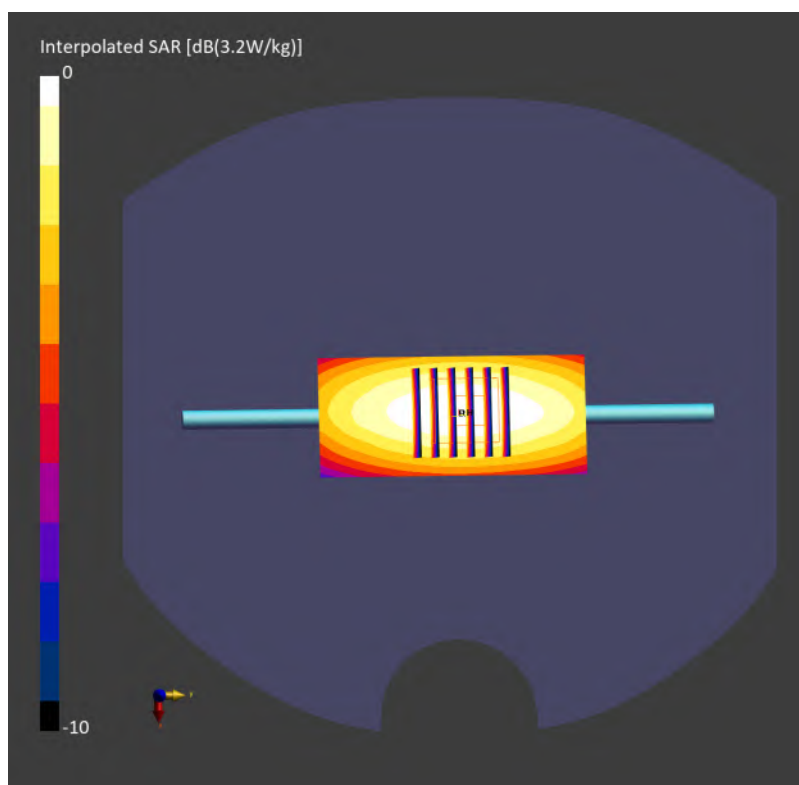

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260824 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.938$ S/m; $\epsilon_r = 42.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.63 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 2.47 W/kg; SAR (8g) = 1.73 W/kg; SAR (10g) = 1.64 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

TSL Correction: Positive only

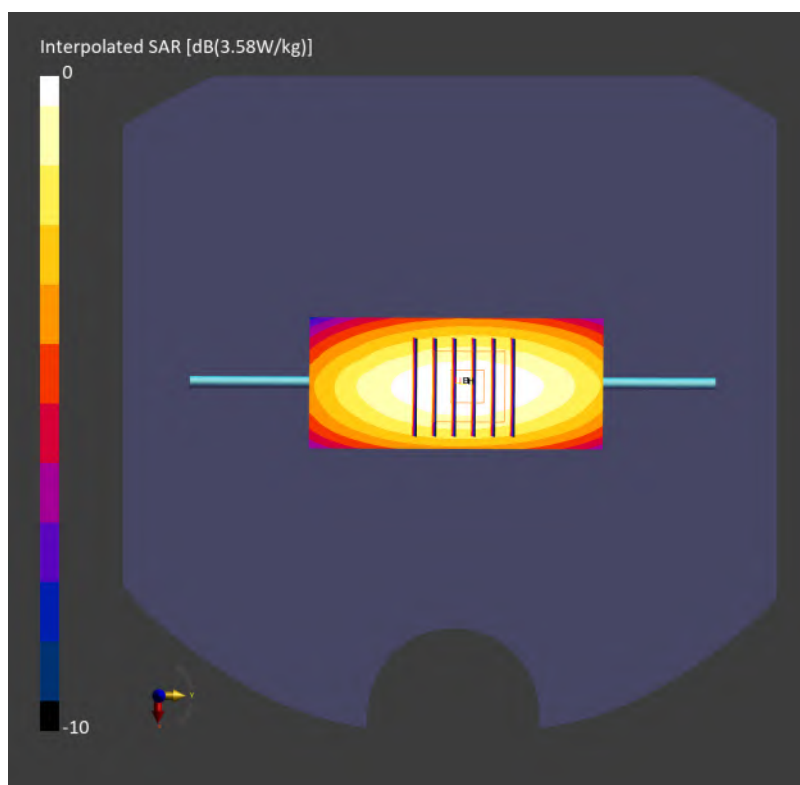

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260825 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.935$ S/m; $\epsilon_r = 42.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.62 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.47 W/kg; SAR (8g) = 1.73 W/kg; SAR (10g) = 1.64 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

TSL Correction: Positive only

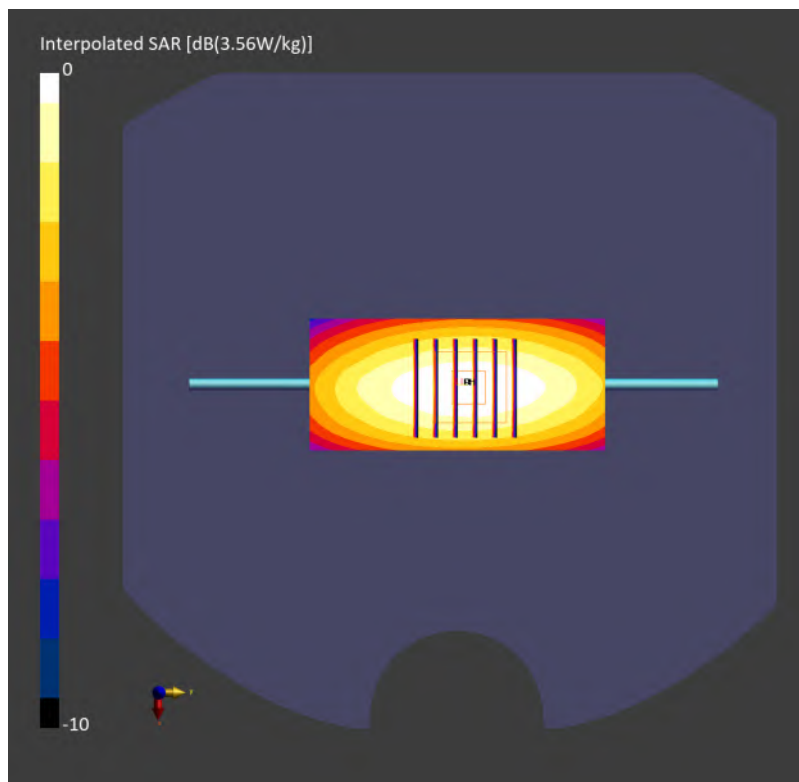

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.909$ S/m; $\epsilon_r = 42.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.97, 9.66, 9.74); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.65 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.77 W/kg; SAR (10g) = 1.68 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 89.7 %

TSL Correction: Positive only

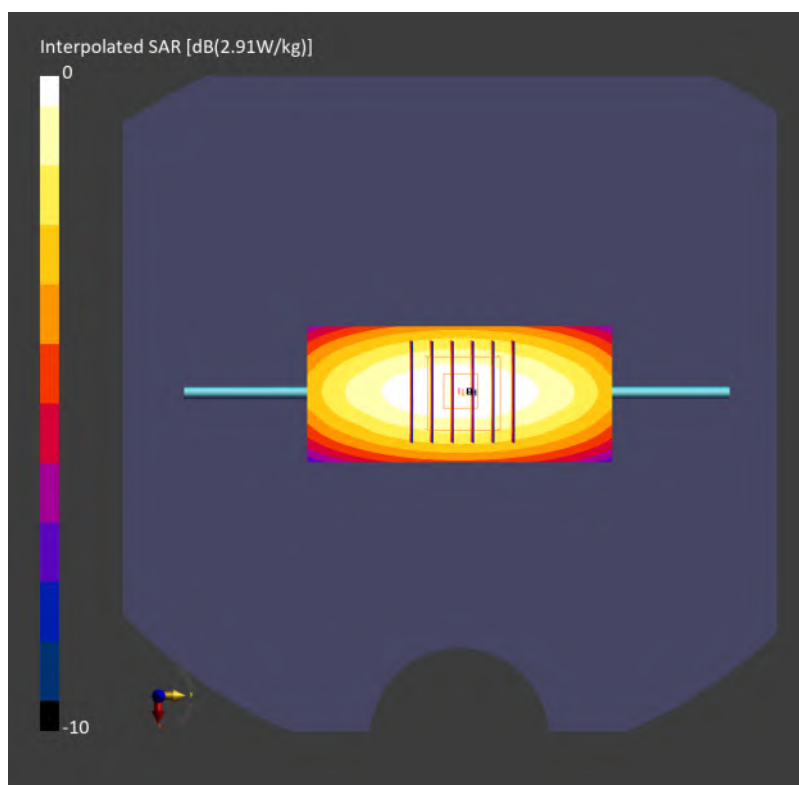

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.941$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.44 W/kg; SAR (10g) = 1.60 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.43 W/kg; SAR (8g) = 1.70 W/kg; SAR (10g) = 1.62 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

TSL Correction: Positive only

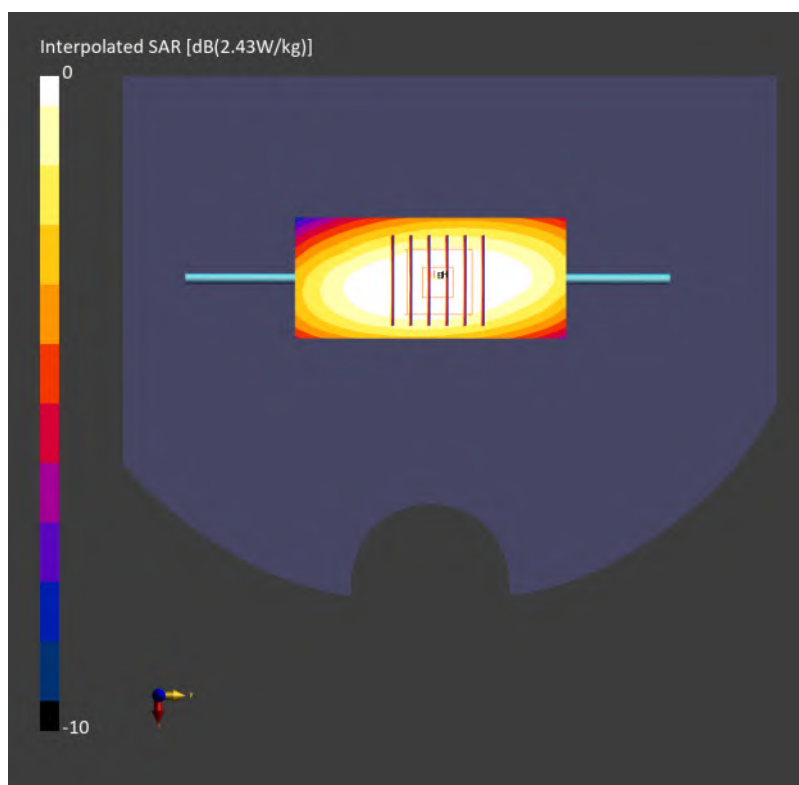

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260901 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.915$ S/m; $\epsilon_r = 44.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.40 W/kg; SAR (10g) = 1.57 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.67 W/kg; SAR (10g) = 1.59 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

TSL Correction: Positive only

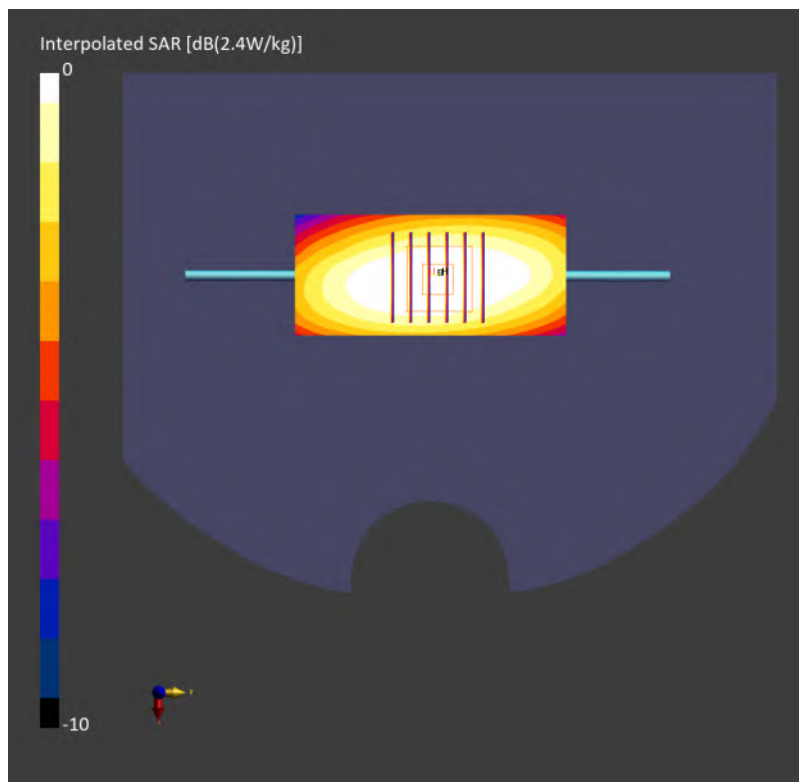

System Check_Head_835MHz**DUT: D835V2 - SN4d167**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_600-7200_260908 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.960$ S/m; $\epsilon_r = 43.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.81, 8.79, 8.4); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.51 W/kg; SAR (10g) = 1.66 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.50 W/kg; SAR (8g) = 1.75 W/kg; SAR (10g) = 1.66 W/kg

Smallest distance from peaks to all points 3 dB below = 16.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

TSL Correction: Positive only

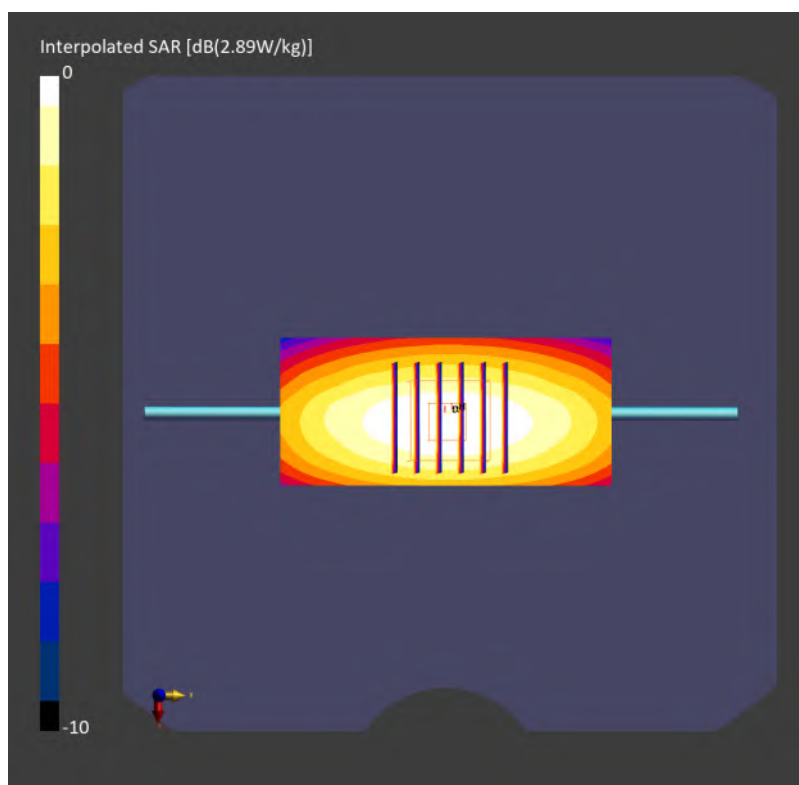

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260826 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.93 W/kg; SAR (10g) = 4.79 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 8.81 W/kg; SAR (8g) = 5.14 W/kg; SAR (10g) = 4.75 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

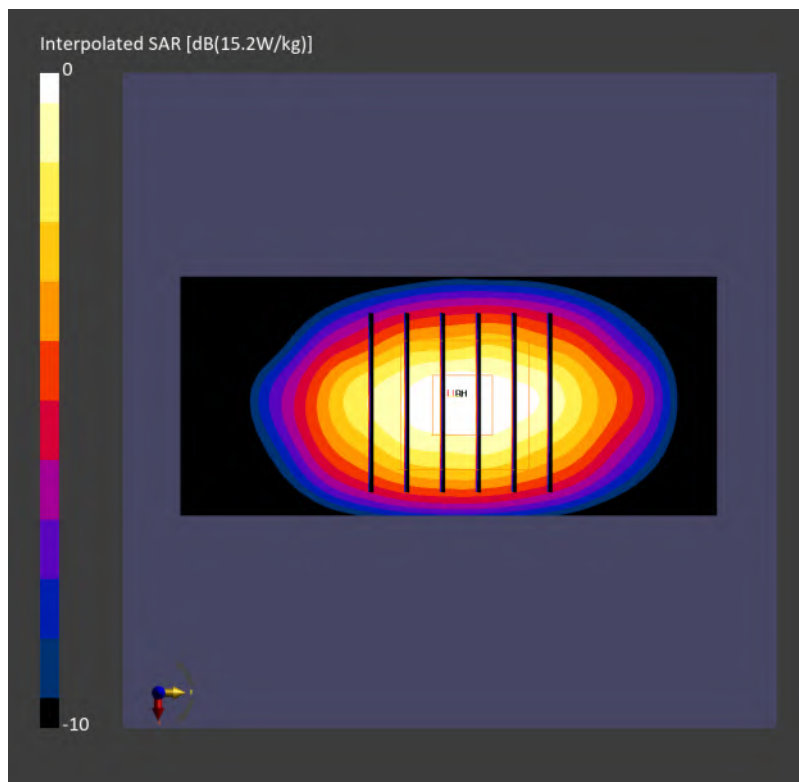

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 8.90 W/kg; SAR (10g) = 4.78 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 8.78 W/kg; SAR (8g) = 5.12 W/kg; SAR (10g) = 4.73 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

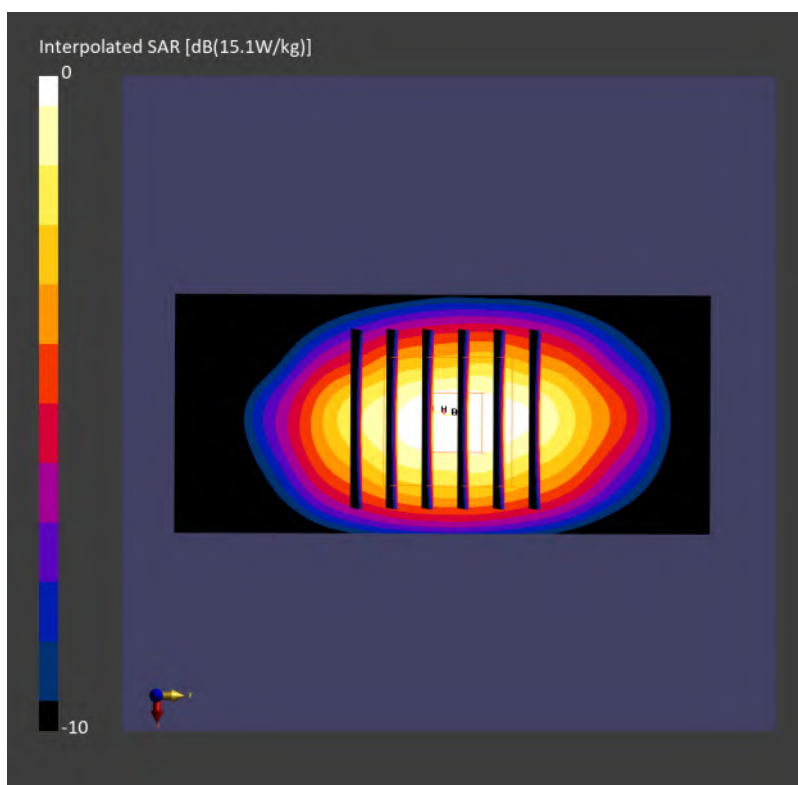

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.30$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.26, 8.0, 8.07); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.27 W/kg; SAR (10g) = 4.84 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 9.12 W/kg; SAR (8g) = 5.23 W/kg; SAR (10g) = 4.83 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

TSL Correction: Positive only

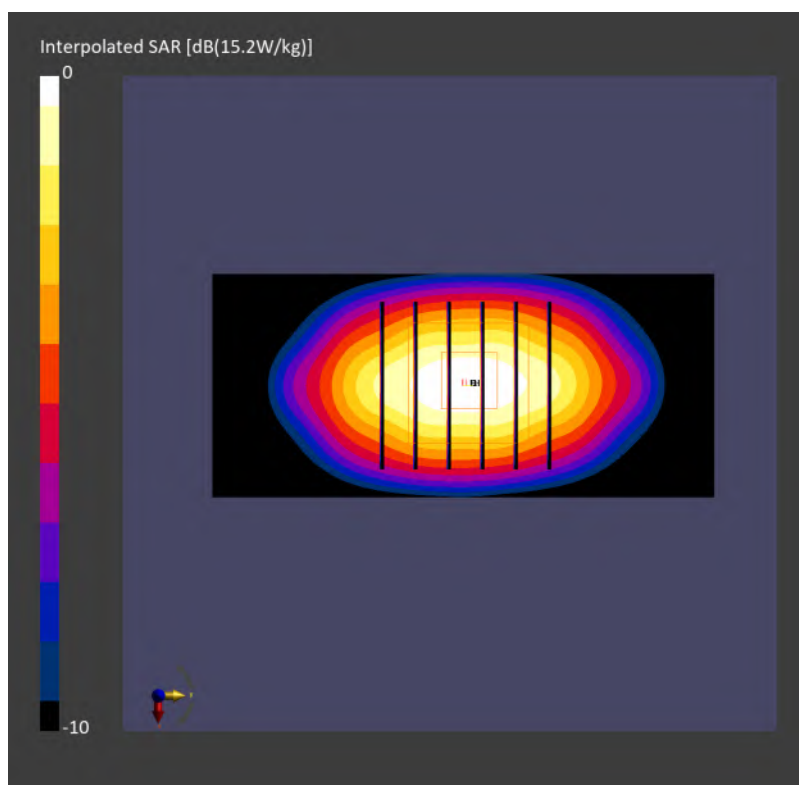

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(7.39, 7.38, 7.05); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.940 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 1.74 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.932 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 85.6 %

TSL Correction: Positive only

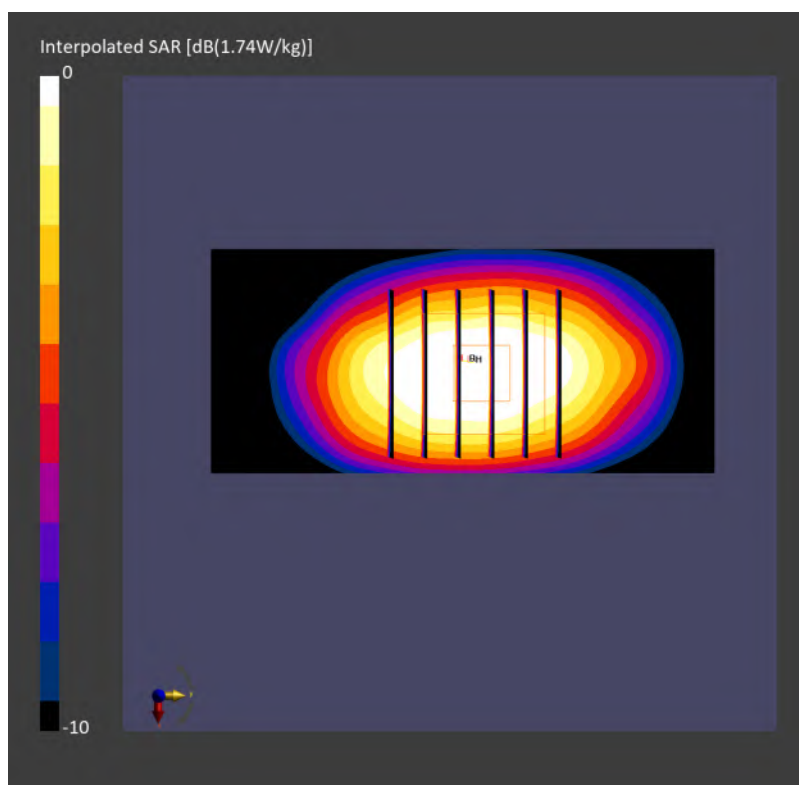

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260915 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.73, 8.22, 8.09); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.07 W/kg; SAR (10g) = 4.83 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 9.13 W/kg; SAR (8g) = 5.31 W/kg; SAR (10g) = 4.91 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.4 %

TSL Correction: Positive only

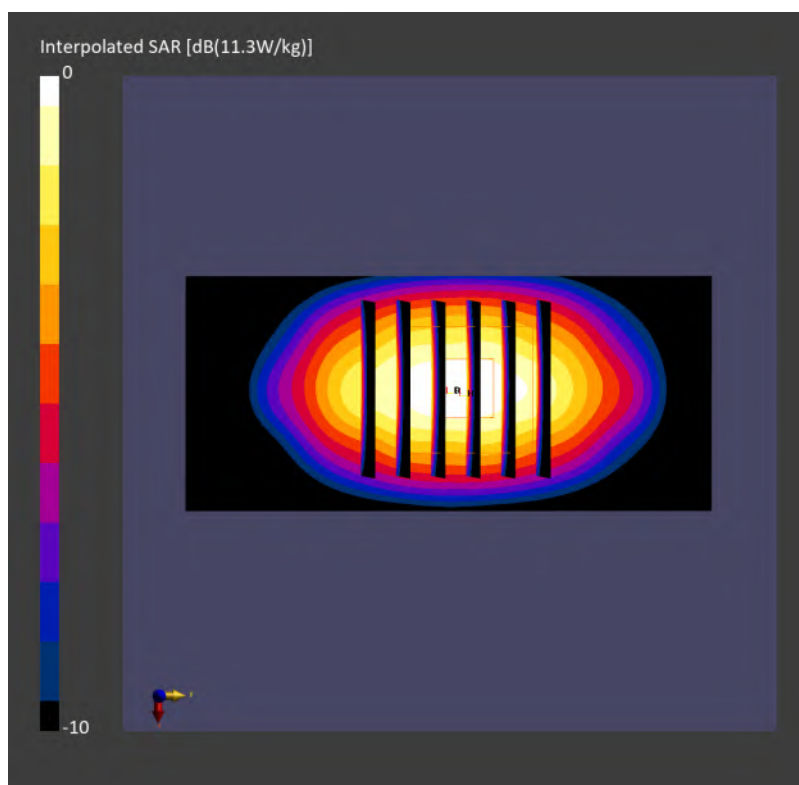

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260916 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.73, 8.22, 8.09); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.04 W/kg; SAR (10g) = 4.81 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.02 dB

SAR (1g) = 9.10 W/kg; SAR (8g) = 5.29 W/kg; SAR (10g) = 4.88 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

TSL Correction: Positive only

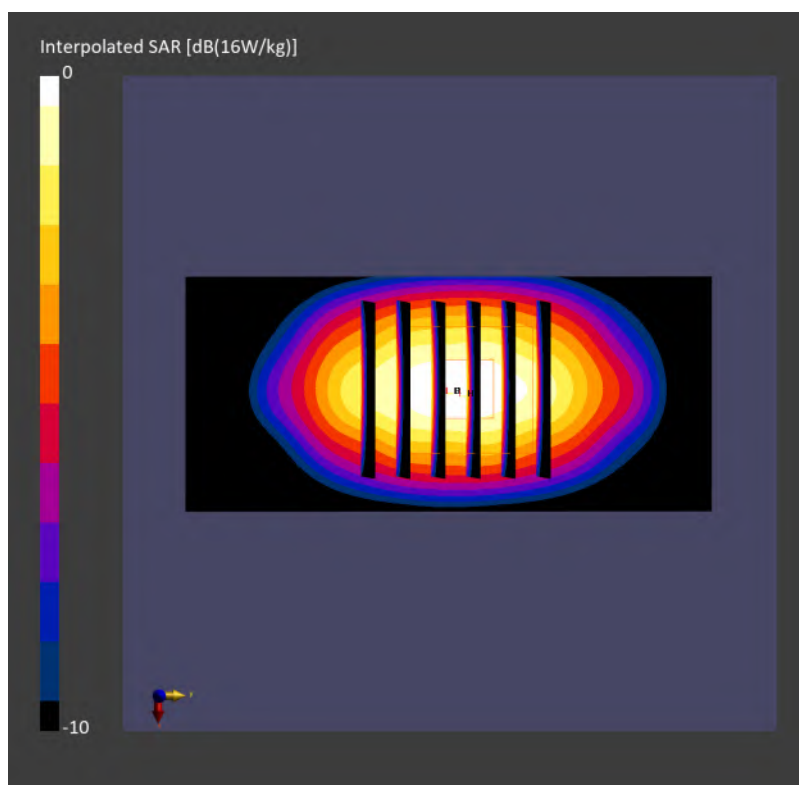

System Check_Head_1750MHz**DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_600-7200_260917 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.73, 8.22, 8.09); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.00 W/kg; SAR (10g) = 4.79 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 9.06 W/kg; SAR (8g) = 5.27 W/kg; SAR (10g) = 4.87 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

TSL Correction: Positive only

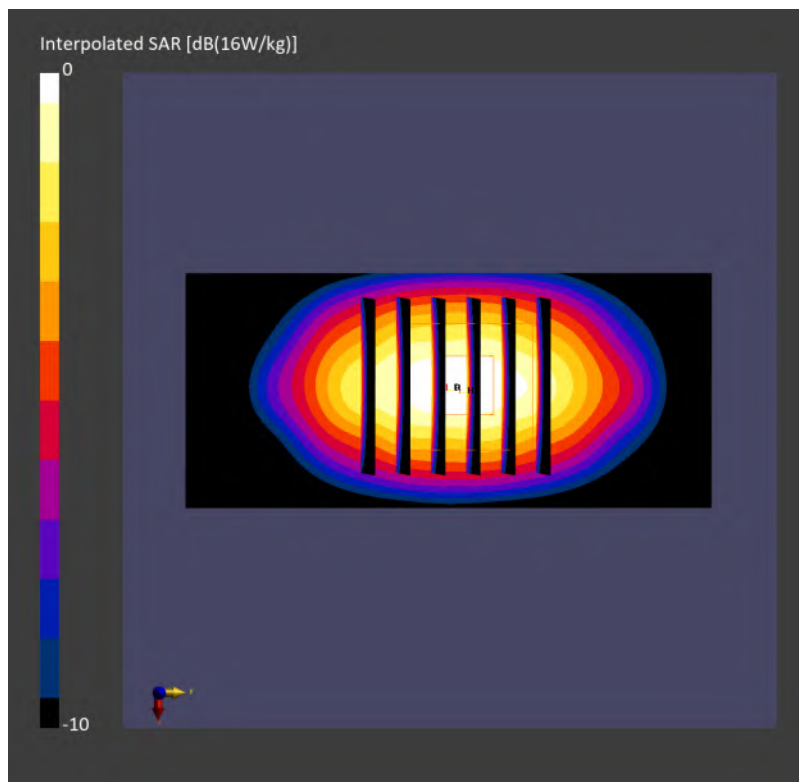

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260826 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.6 W/kg; SAR (10g) = 5.50 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 10.5 W/kg; SAR (8g) = 5.97 W/kg; SAR (10g) = 5.50 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

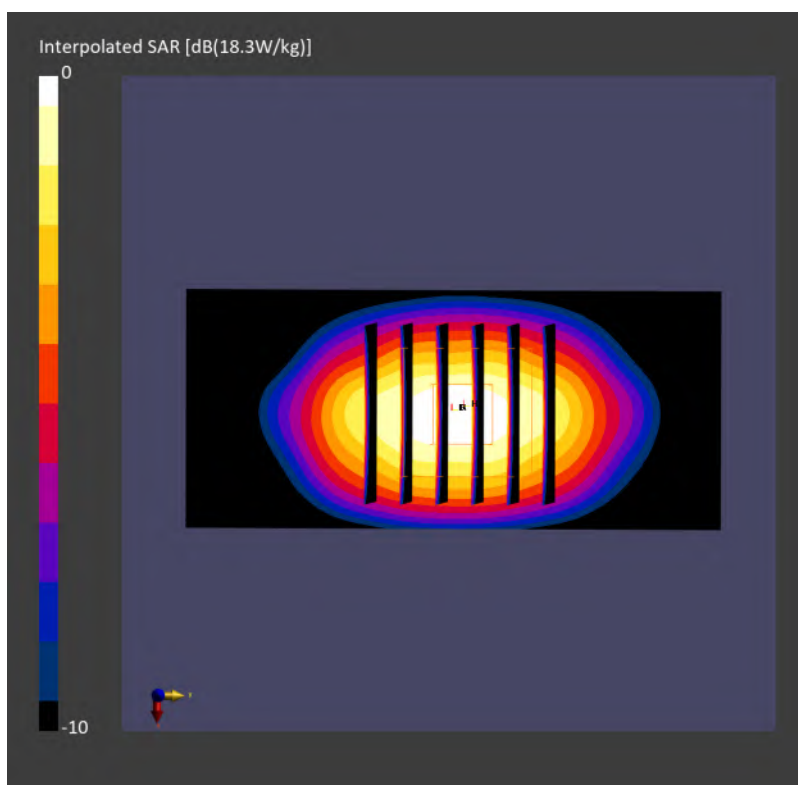

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260827 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.5 W/kg; SAR (10g) = 5.47 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 10.4 W/kg; SAR (8g) = 5.94 W/kg; SAR (10g) = 5.47 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.9 %

TSL Correction: Positive only

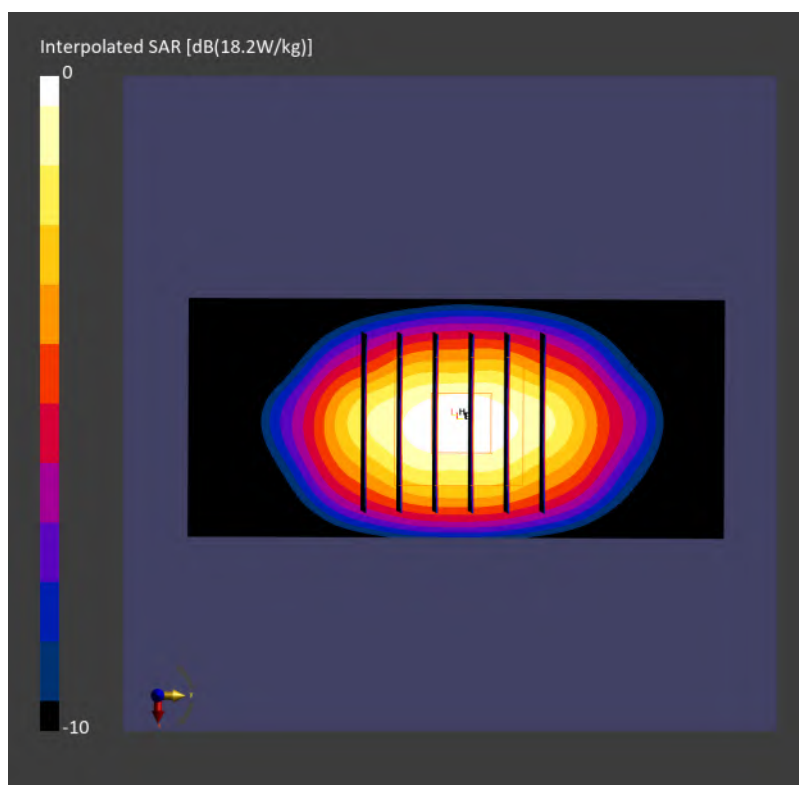

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.08, 7.83, 7.89); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.2 W/kg; SAR (10g) = 5.21 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 10.1 W/kg; SAR (8g) = 5.70 W/kg; SAR (10g) = 5.24 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 85.4 %

TSL Correction: Positive only

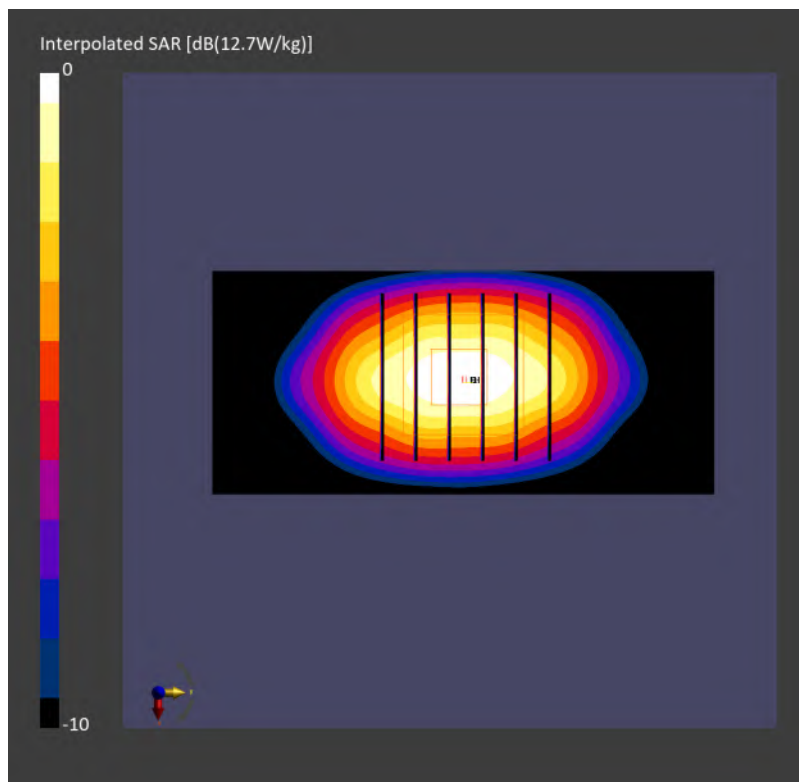

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.47$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.93, 6.92, 6.61); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.98 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 1.97 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.7 %

TSL Correction: Positive only

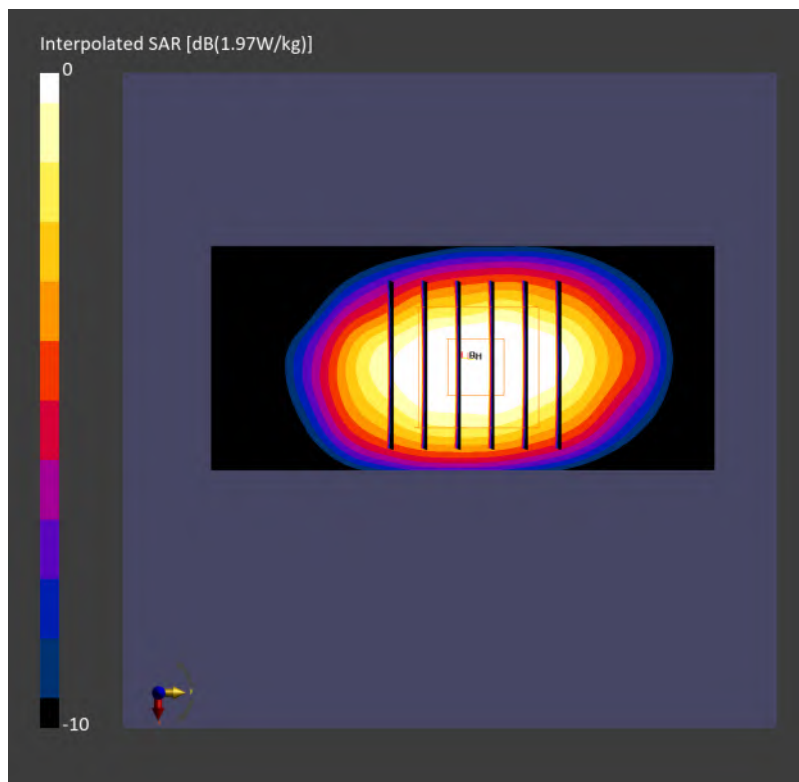

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260916 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.49, 7.97, 7.84); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.2 W/kg; SAR (10g) = 5.29 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 10.3 W/kg; SAR (8g) = 5.83 W/kg; SAR (10g) = 5.36 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

TSL Correction: Positive only

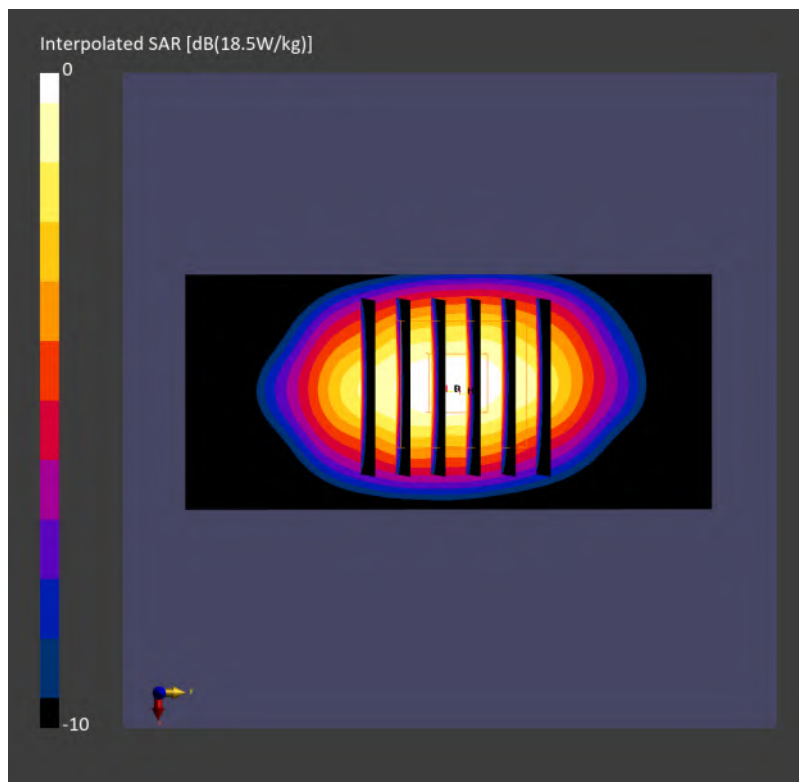

System Check_Head_1900MHz**DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_600-7200_260917 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.46$ S/m; $\epsilon_r = 40.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.49, 7.97, 7.84); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 10.3 W/kg; SAR (10g) = 5.32 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 10.3 W/kg; SAR (8g) = 5.86 W/kg; SAR (10g) = 5.39 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 85.2 %

TSL Correction: Positive only

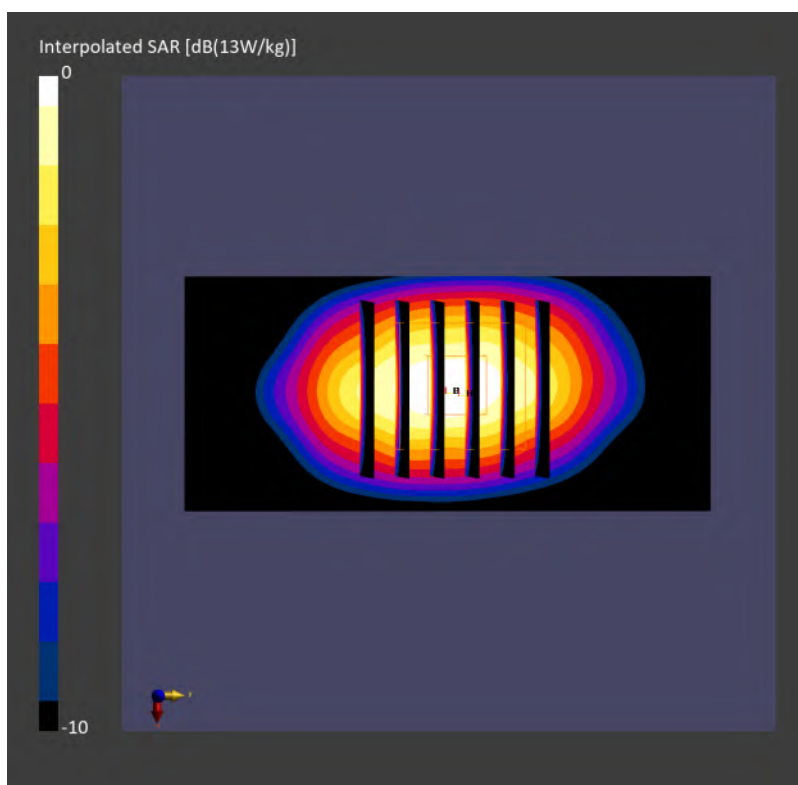

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.73$ S/m; $\epsilon_r = 41.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.72, 6.71, 6.41); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.30 W/kg; SAR (10g) = 1.11 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 2.29 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 9.3 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

TSL Correction: Positive only

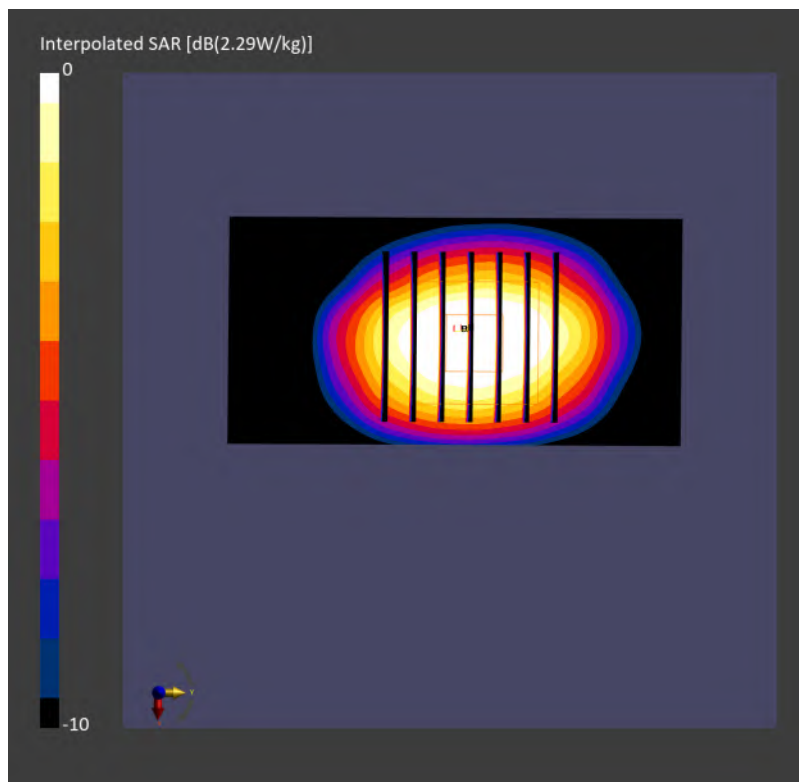

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.66$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.76, 7.52, 7.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.9 W/kg; SAR (10g) = 6.11 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.01 dB

SAR (1g) = 12.8 W/kg; SAR (8g) = 6.75 W/kg; SAR (10g) = 6.13 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

TSL Correction: Positive only

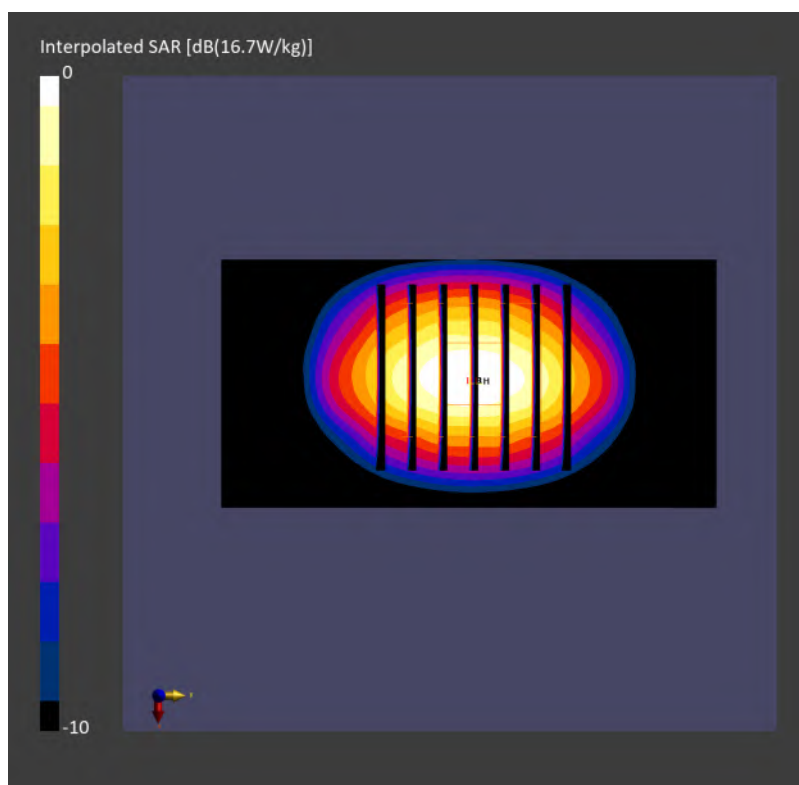

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 39.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.46, 7.23, 7.29); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.0 W/kg; SAR (10g) = 6.42 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 13.9 W/kg; SAR (8g) = 7.16 W/kg; SAR (10g) = 6.48 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

TSL Correction: Positive only

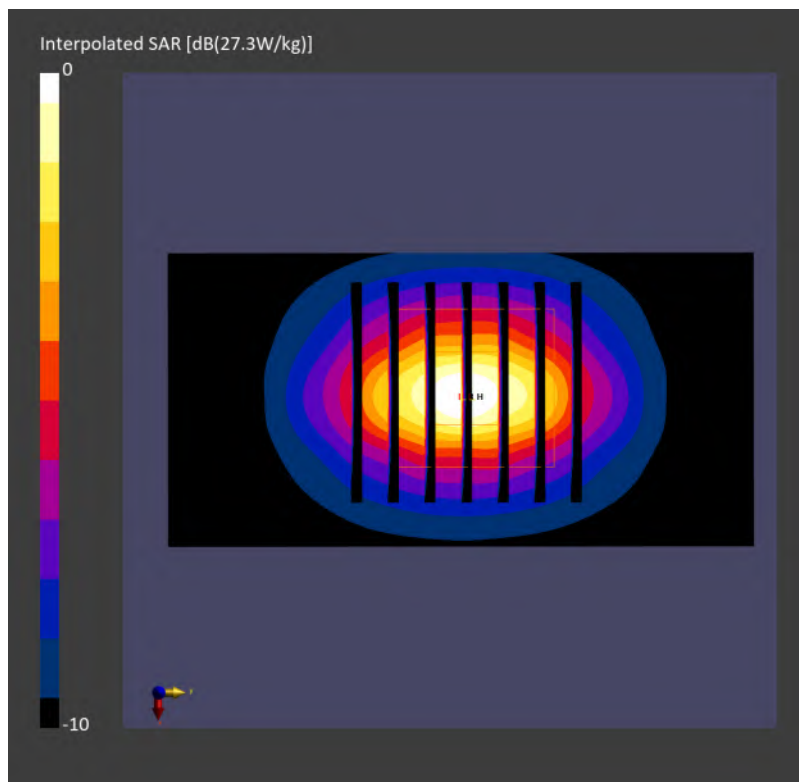

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.54, 6.53, 6.24); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.54 W/kg; SAR (10g) = 1.19 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.52 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

TSL Correction: Positive only

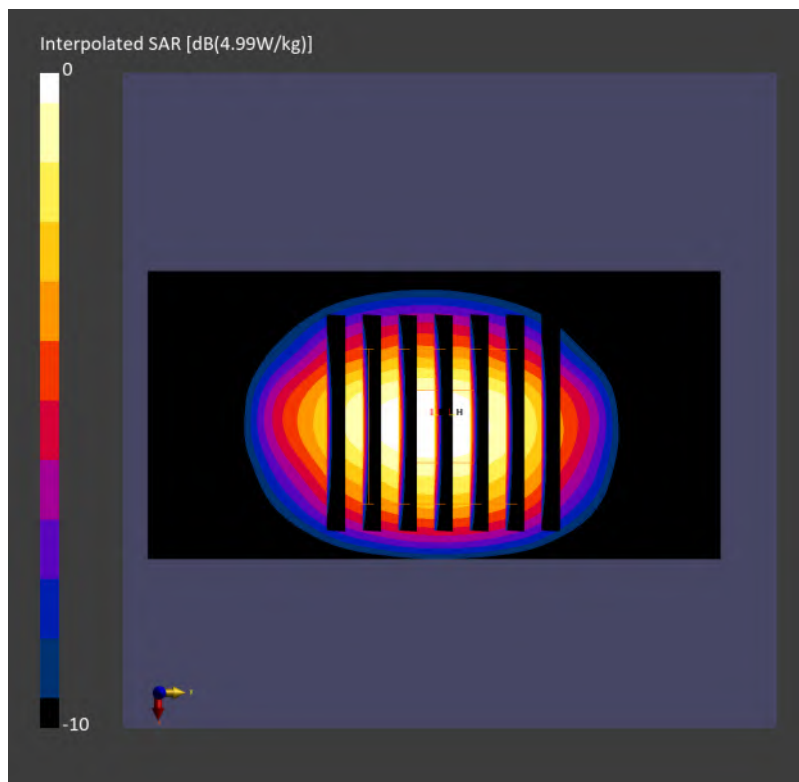

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.46, 7.23, 7.29); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.8 W/kg; SAR (10g) = 6.33 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 13.7 W/kg; SAR (8g) = 7.07 W/kg; SAR (10g) = 6.40 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.1 %

TSL Correction: Positive only

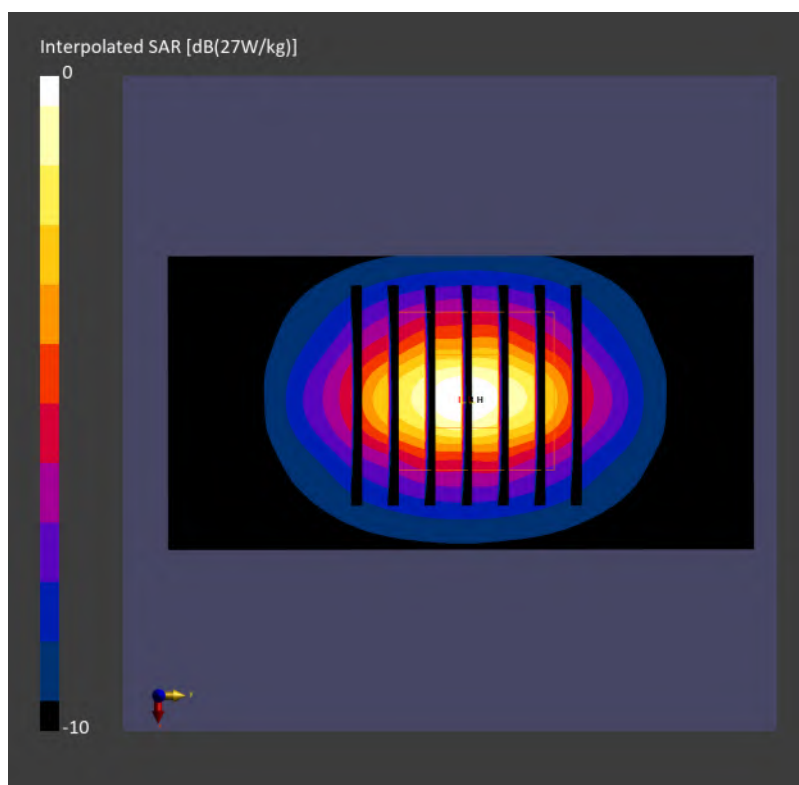

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260828 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.0 W/kg; SAR (10g) = 5.95 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 13.1 W/kg; SAR (8g) = 6.56 W/kg; SAR (10g) = 5.92 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

TSL Correction: Positive only

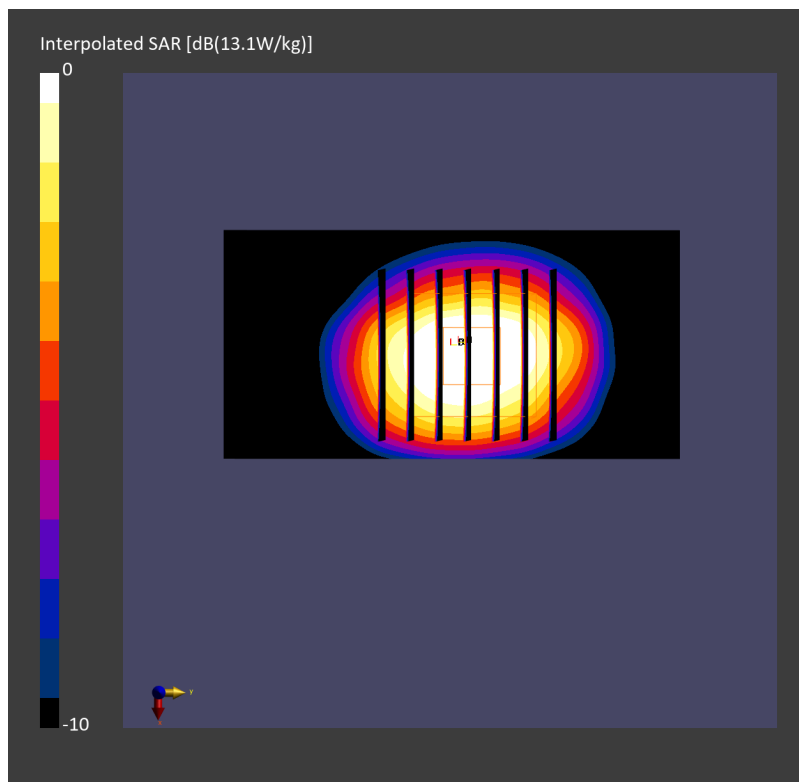

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260829 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.89$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.62, 7.39, 7.44); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.4 W/kg; SAR (10g) = 6.31 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 14.3 W/kg; SAR (8g) = 7.05 W/kg; SAR (10g) = 6.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 81.1 %

TSL Correction: Positive only

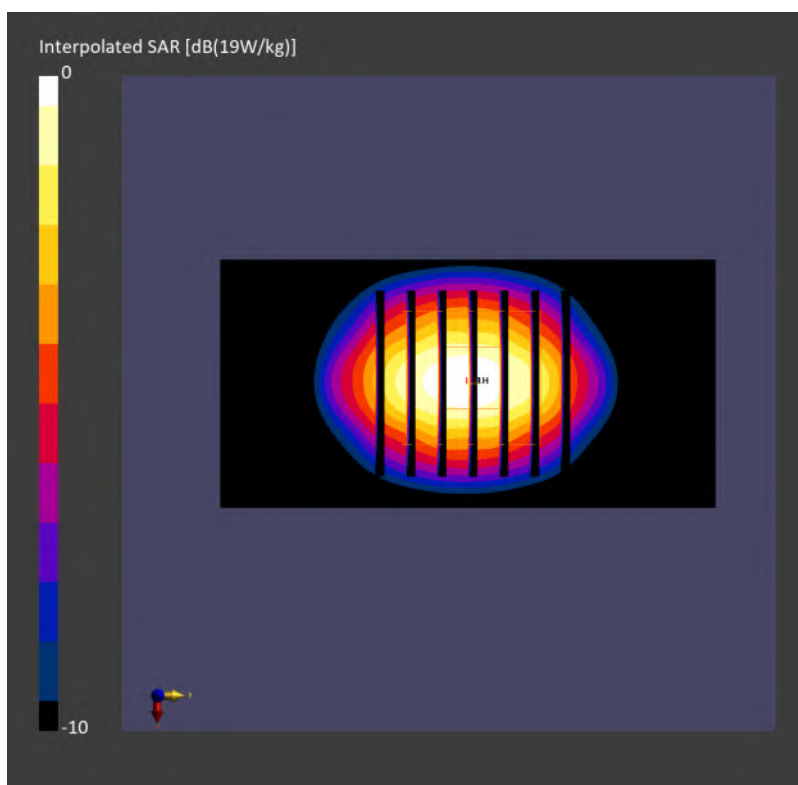

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 12.8 W/kg; SAR (10g) = 5.87 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 12.9 W/kg; SAR (8g) = 6.50 W/kg; SAR (10g) = 5.86 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.4 %

TSL Correction: Positive only

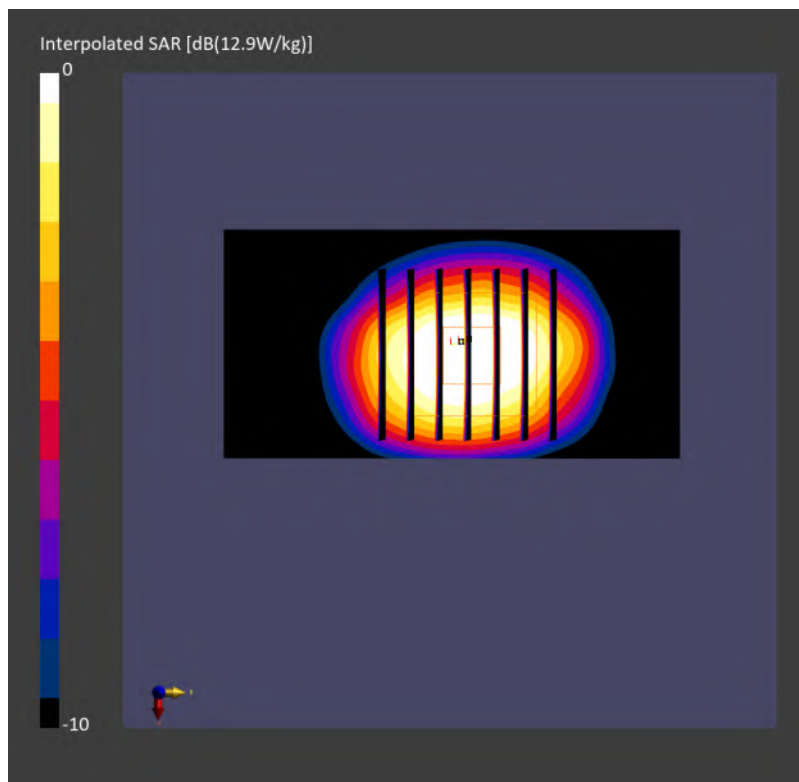

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260904 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.2 W/kg; SAR (10g) = 5.95 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 13.2 W/kg; SAR (8g) = 6.59 W/kg; SAR (10g) = 5.94 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

TSL Correction: Positive only

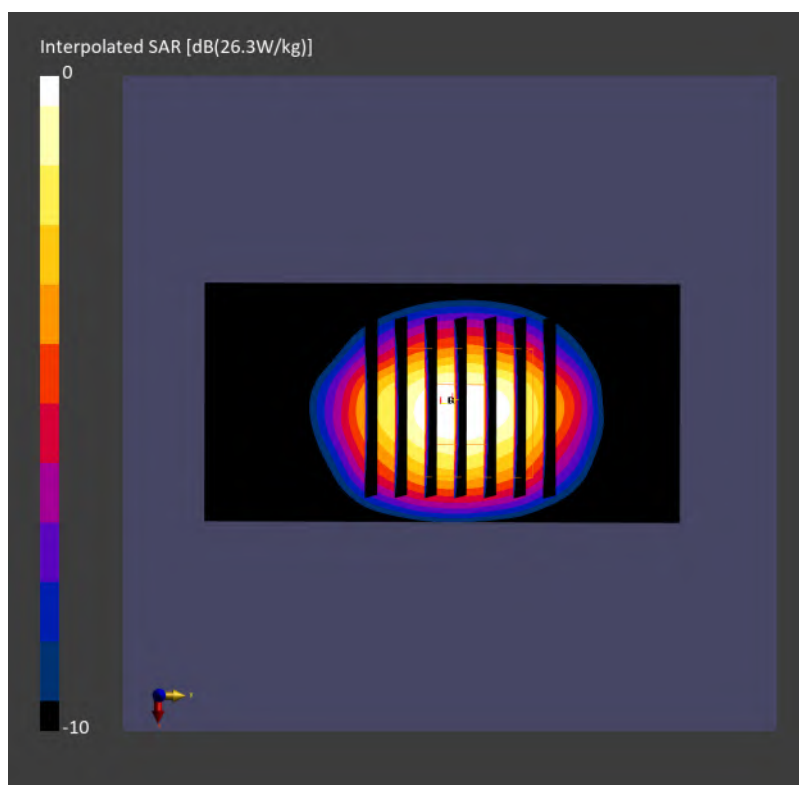

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260905 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.90$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(6.74, 6.73, 6.43); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.0 W/kg; SAR (10g) = 5.88 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 13.1 W/kg; SAR (8g) = 6.51 W/kg; SAR (10g) = 5.88 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

TSL Correction: Positive only

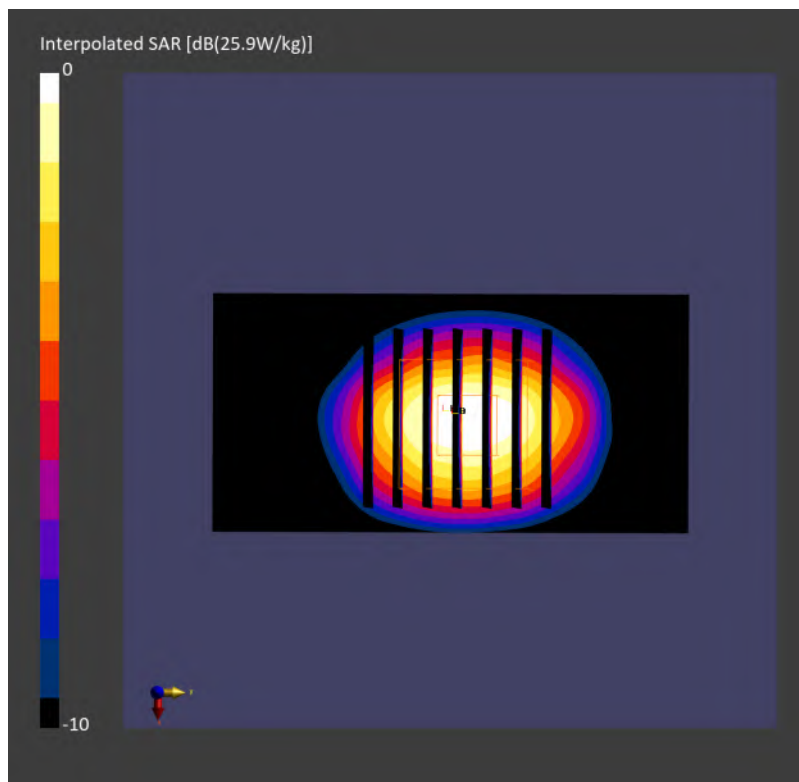

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260907 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.0, 7.45, 7.32); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.2 W/kg; SAR (10g) = 6.25 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 14.1 W/kg; SAR (8g) = 7.01 W/kg; SAR (10g) = 6.32 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

TSL Correction: Positive only

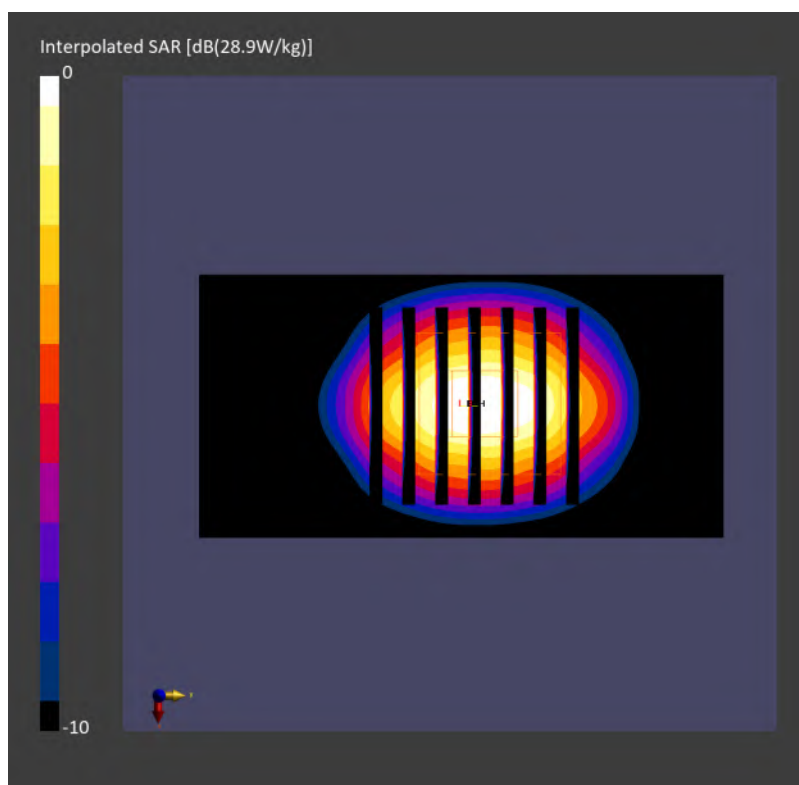

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260908 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.0, 7.45, 7.32); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.4 W/kg; SAR (10g) = 5.85 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 13.4 W/kg; SAR (8g) = 6.60 W/kg; SAR (10g) = 5.95 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

TSL Correction: Positive only

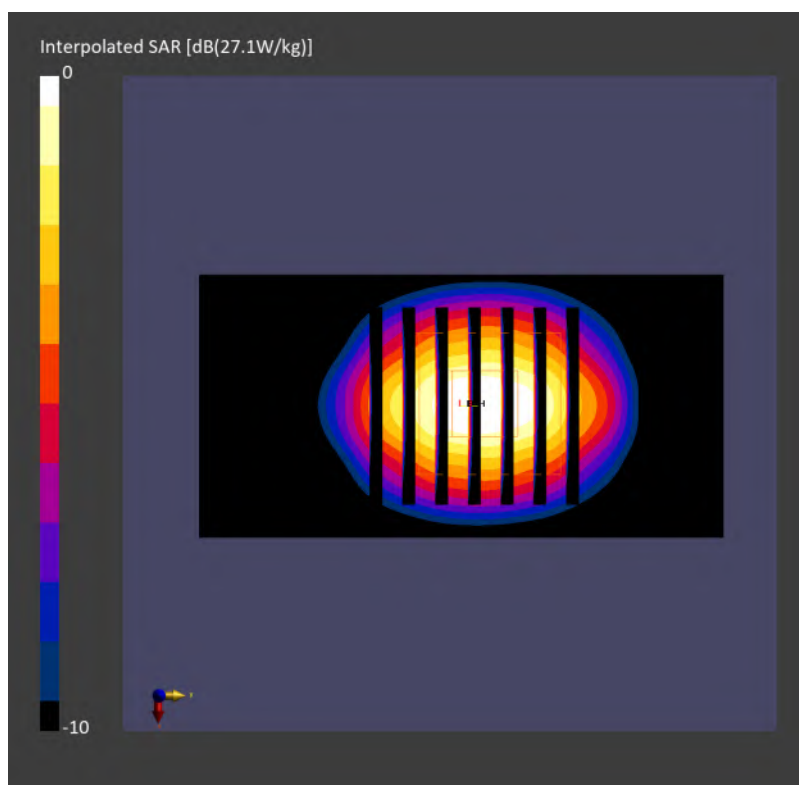

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260909 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.0, 7.45, 7.32); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.8 W/kg; SAR (10g) = 6.10 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.00 dB

SAR (1g) = 13.9 W/kg; SAR (8g) = 6.88 W/kg; SAR (10g) = 6.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

TSL Correction: Positive only

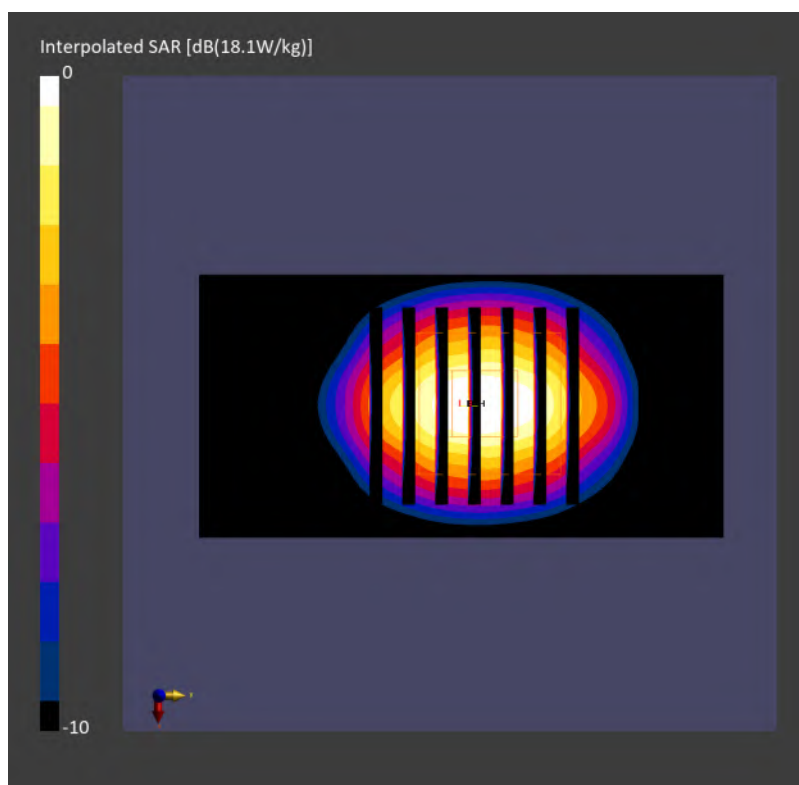

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260910 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.0, 7.45, 7.32); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.9 W/kg; SAR (10g) = 6.13 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 13.9 W/kg; SAR (8g) = 6.92 W/kg; SAR (10g) = 6.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 80.5 %

TSL Correction: Positive only

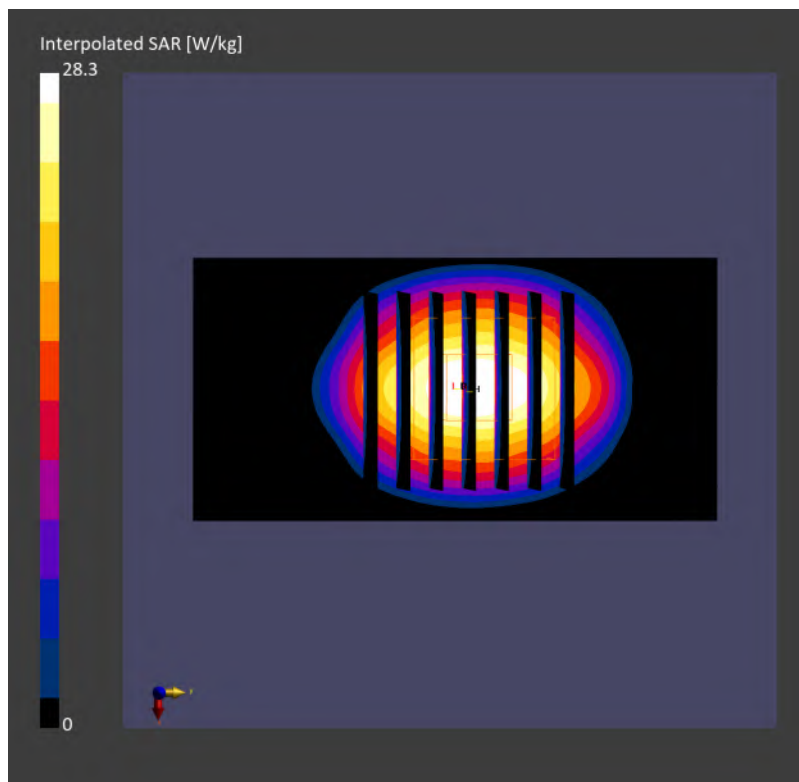

System Check_Head_2600MHz**DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_600-7200_260911 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.0, 7.45, 7.32); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.3 W/kg; SAR (10g) = 5.83 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.01 dB

SAR (1g) = 13.3 W/kg; SAR (8g) = 6.58 W/kg; SAR (10g) = 5.93 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

TSL Correction: Positive only

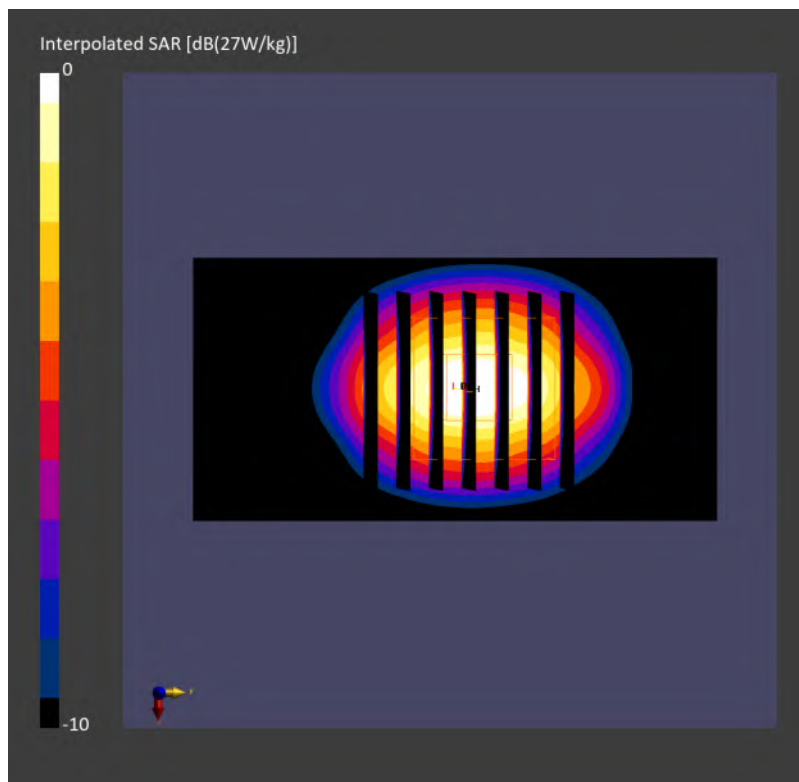

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.66$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.66 W/kg; SAR (10g) = 2.50 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.80 W/kg; SAR (8g) = 2.90 W/kg; SAR (10g) = 2.56 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.4 %

TSL Correction: Positive only

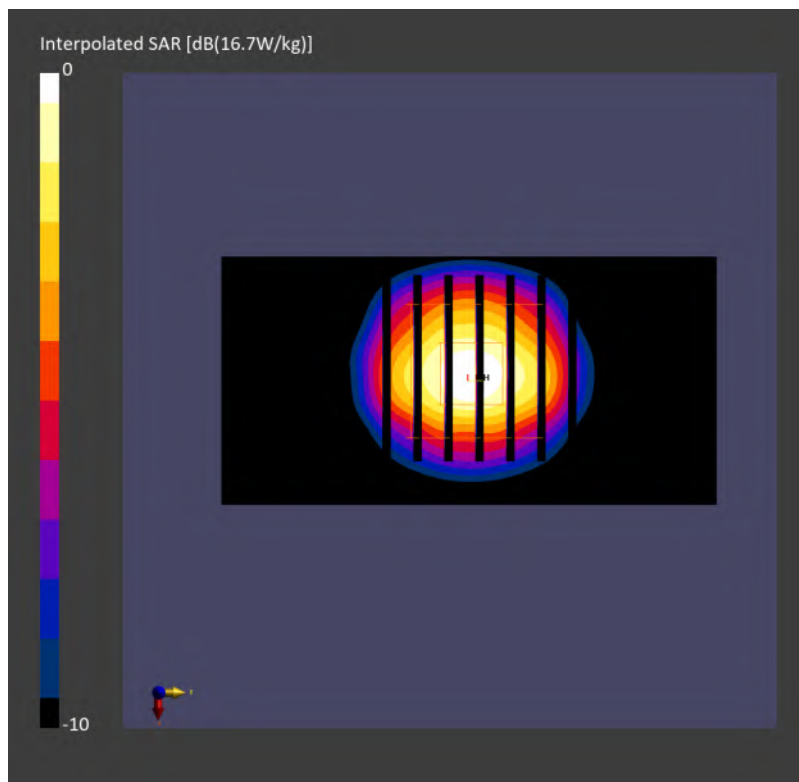

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.71$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.94, 5.93, 5.67); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.49 W/kg; SAR (10g) = 2.46 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.59 W/kg; SAR (8g) = 2.85 W/kg; SAR (10g) = 2.53 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.2 %

TSL Correction: Positive only

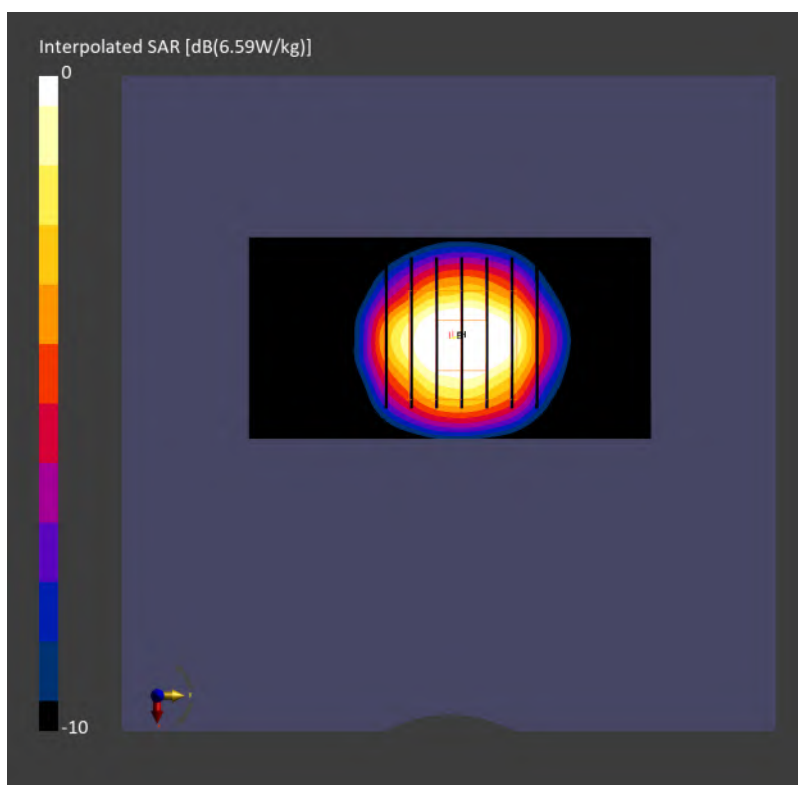

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.72$ S/m; $\epsilon_r = 39.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.94, 5.93, 5.67); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.55 W/kg; SAR (10g) = 2.48 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.66 W/kg; SAR (8g) = 2.88 W/kg; SAR (10g) = 2.55 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.3 %

TSL Correction: Positive only

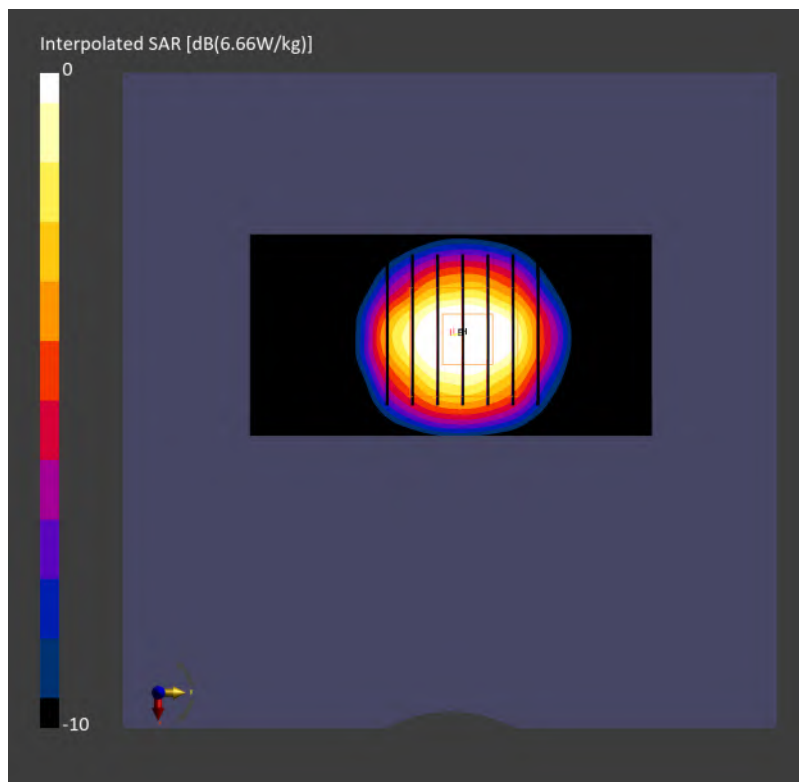

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.80$ S/m; $\epsilon_r = 40.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.73, 6.52, 6.57); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.97 W/kg; SAR (10g) = 2.64 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 7.12 W/kg; SAR (8g) = 3.05 W/kg; SAR (10g) = 2.70 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 76.4 %

TSL Correction: Positive only

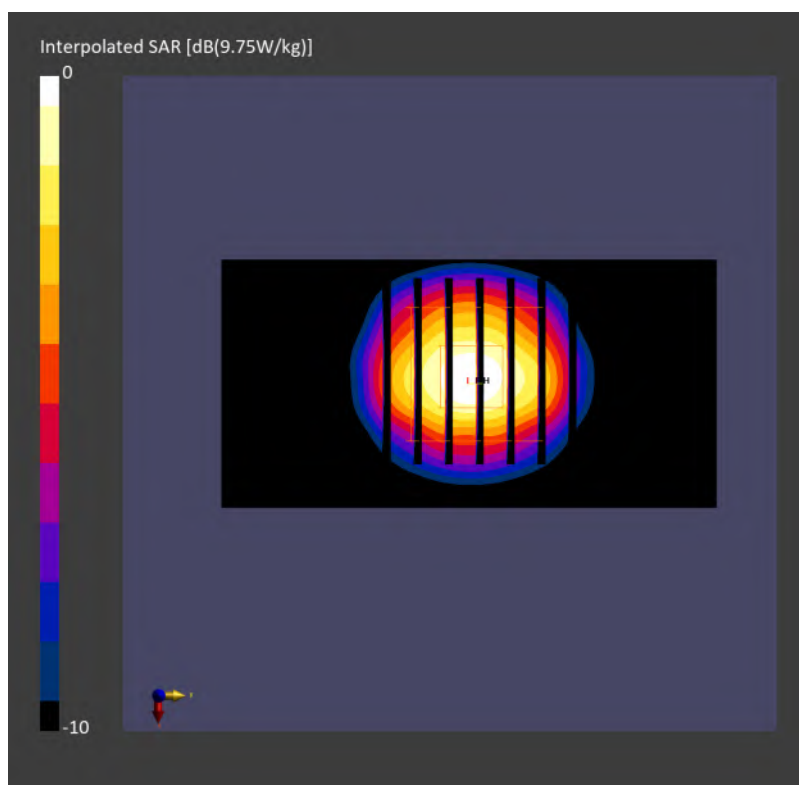

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.73$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.94, 5.93, 5.67); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.45 W/kg; SAR (10g) = 2.46 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.56 W/kg; SAR (8g) = 2.82 W/kg; SAR (10g) = 2.50 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

TSL Correction: Positive only

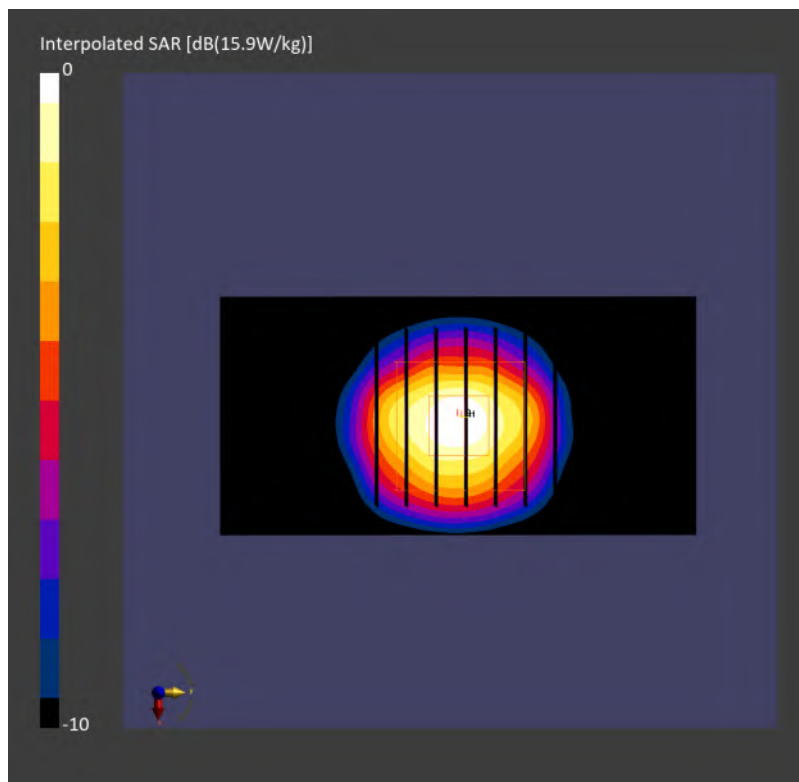

System Check_Head_3500MHz**DUT: D3500V2 - SN1014**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_600-7200_260907 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.74$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.94, 5.93, 5.67); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.47 W/kg; SAR (10g) = 2.47 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.59 W/kg; SAR (8g) = 2.84 W/kg; SAR (10g) = 2.51 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

TSL Correction: Positive only

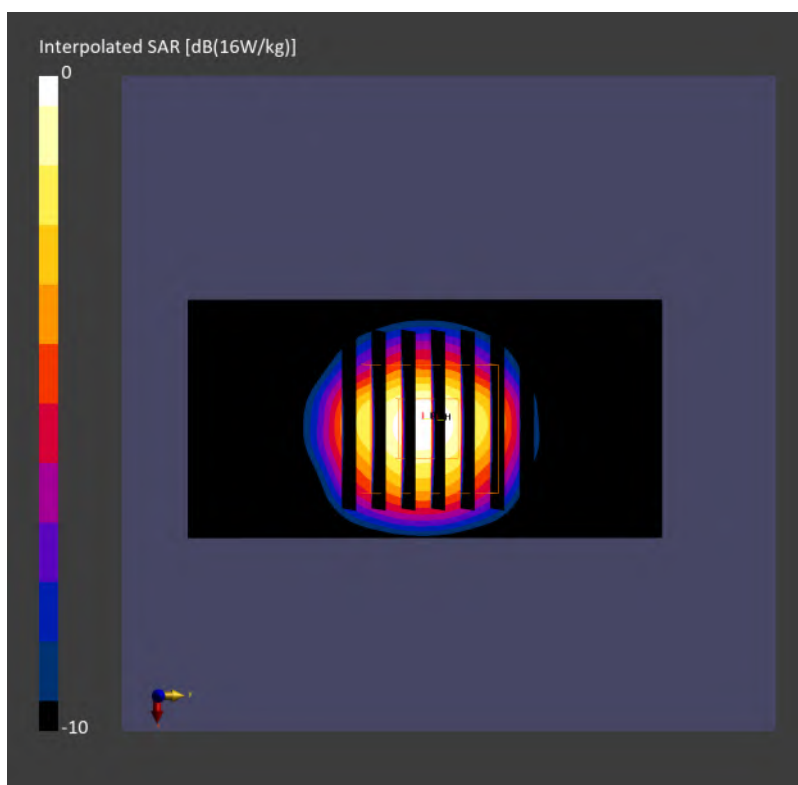

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.83$ S/m; $\epsilon_r = 38.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.71 W/kg; SAR (10g) = 2.42 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 6.86 W/kg; SAR (8g) = 2.83 W/kg; SAR (10g) = 2.49 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.2 %

TSL Correction: Positive only

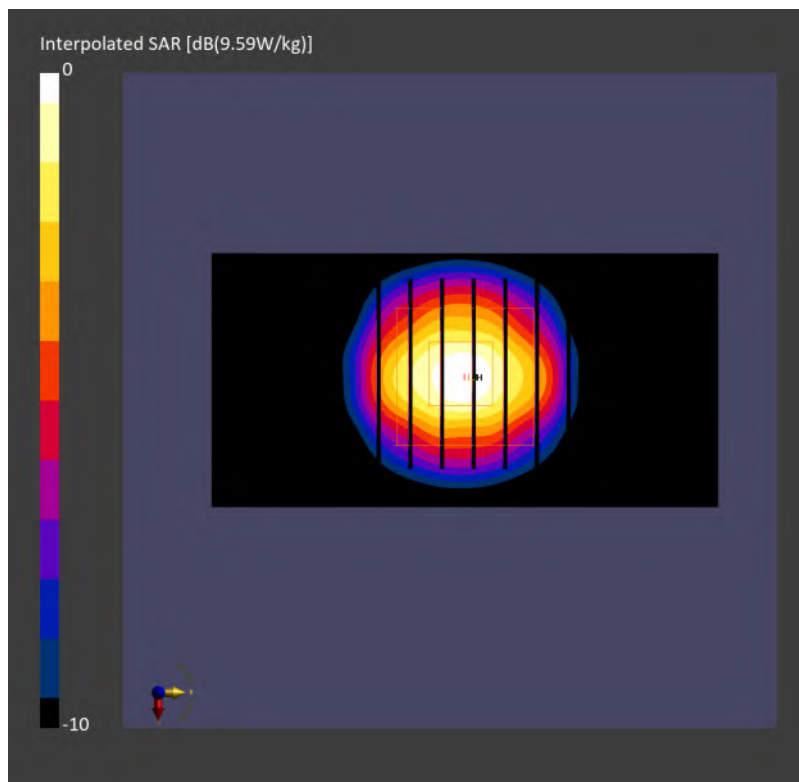

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.89$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.56 W/kg; SAR (10g) = 2.45 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.73 W/kg; SAR (8g) = 2.83 W/kg; SAR (10g) = 2.50 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.8 %

TSL Correction: Positive only

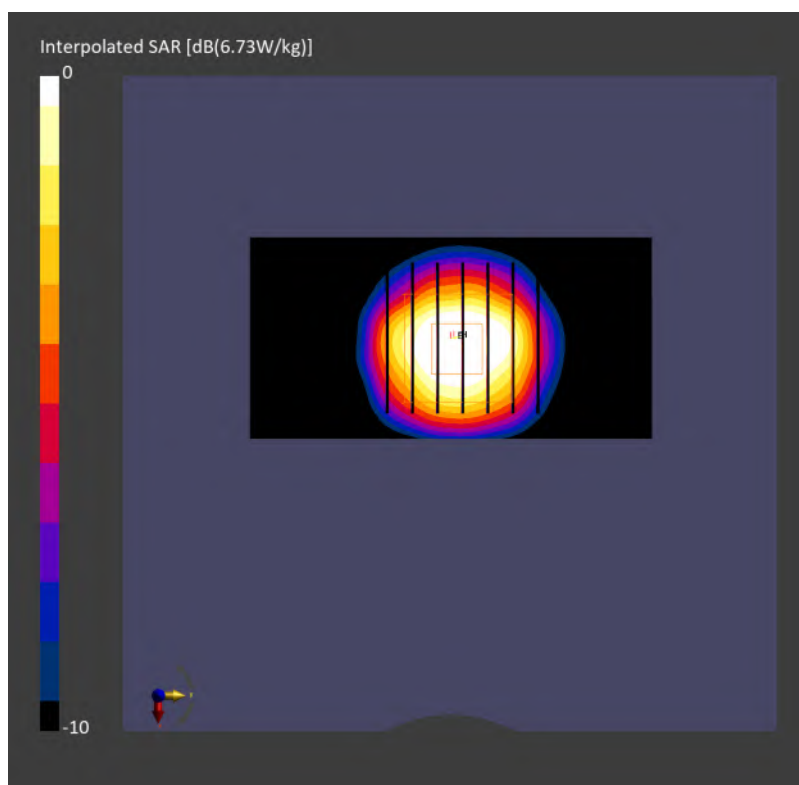

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.90$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.68 W/kg; SAR (10g) = 2.49 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.86 W/kg; SAR (8g) = 2.88 W/kg; SAR (10g) = 2.55 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.8 %

TSL Correction: Positive only

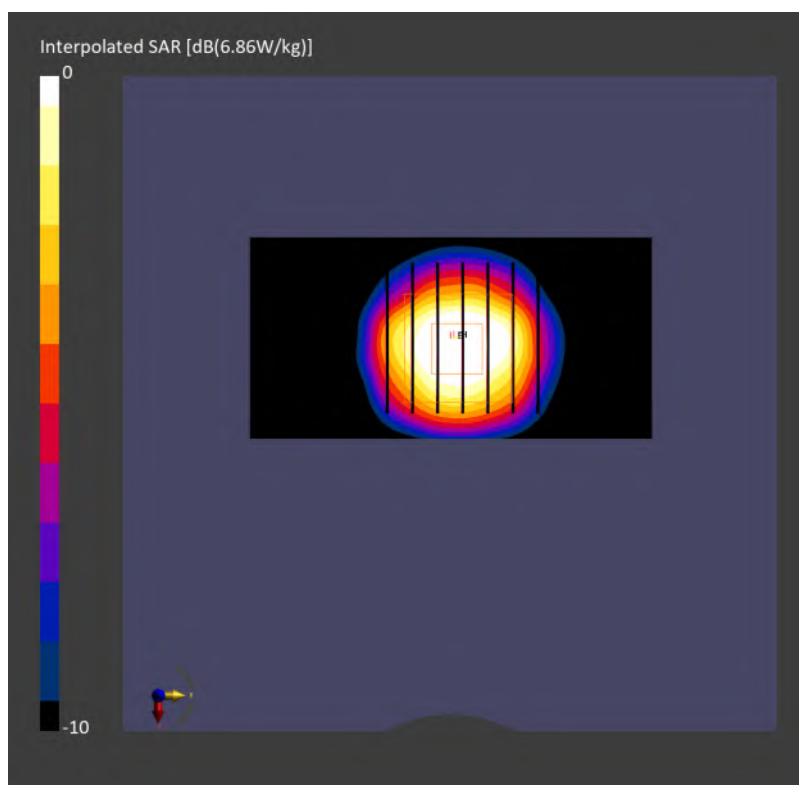

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.87, 6.66, 6.71); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.12 W/kg; SAR (10g) = 2.58 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 7.25 W/kg; SAR (8g) = 3.02 W/kg; SAR (10g) = 2.66 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

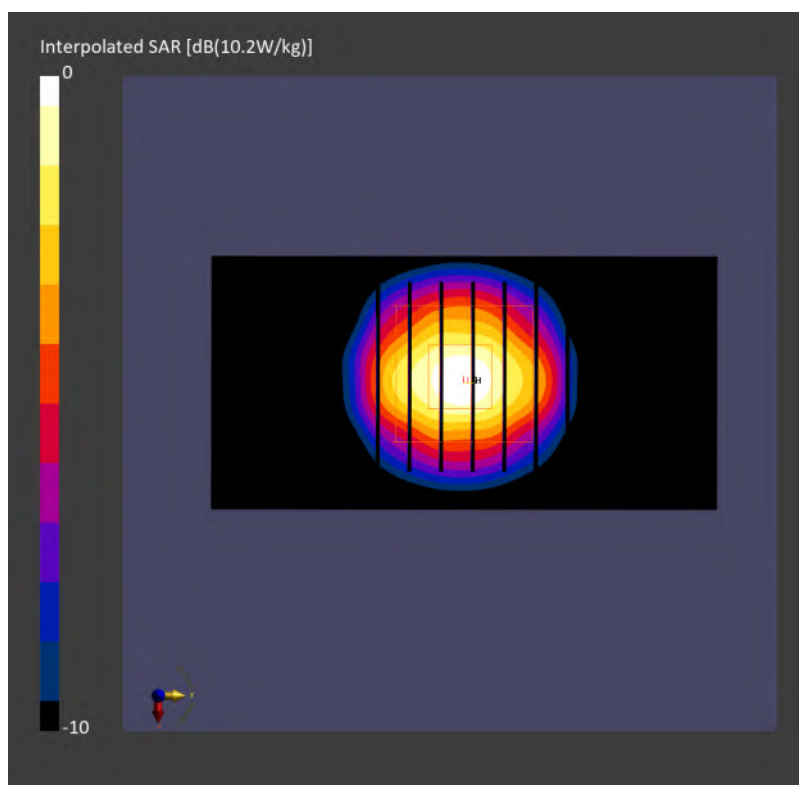

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.62 W/kg; SAR (10g) = 2.48 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.80 W/kg; SAR (8g) = 2.86 W/kg; SAR (10g) = 2.52 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

TSL Correction: Positive only

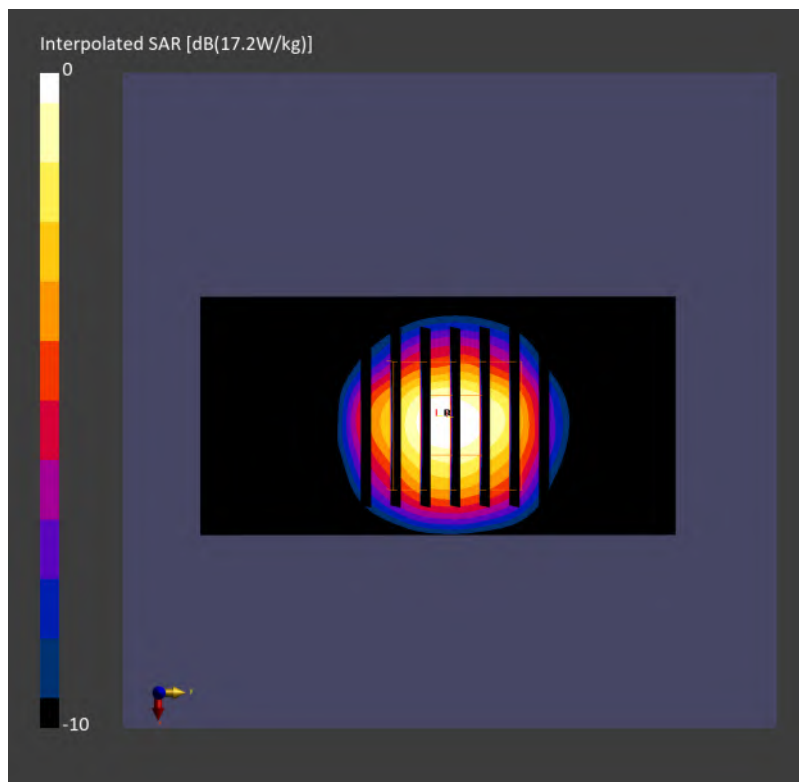

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260907 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.64 W/kg; SAR (10g) = 2.49 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.82 W/kg; SAR (8g) = 2.87 W/kg; SAR (10g) = 2.53 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.5 %

TSL Correction: Positive only

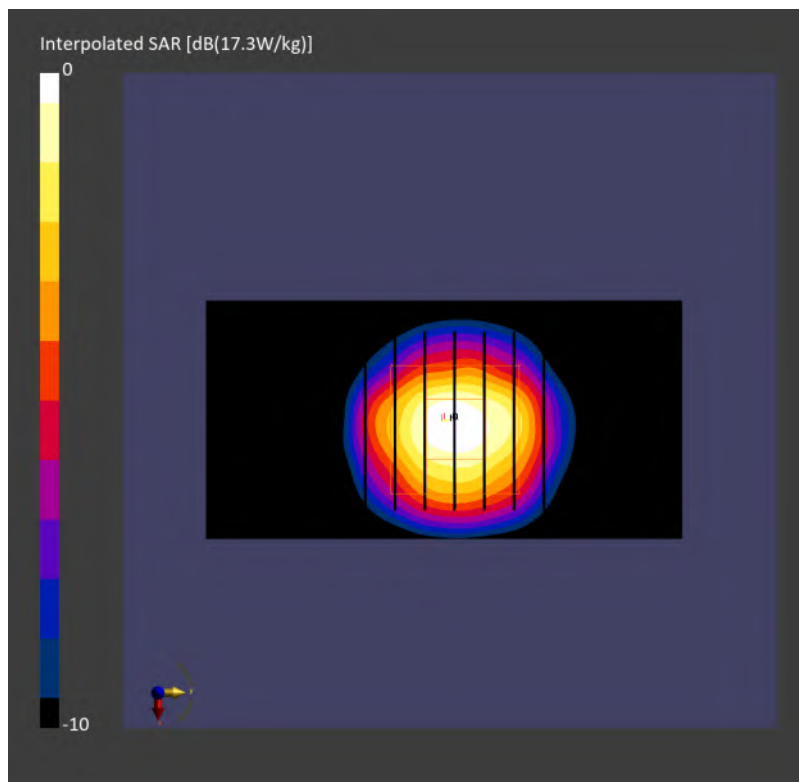

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260912 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.89$ S/m; $\epsilon_r = 38.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.47, 6.89, 6.77); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.54 W/kg; SAR (10g) = 2.36 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 6.65 W/kg; SAR (8g) = 2.76 W/kg; SAR (10g) = 2.44 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

TSL Correction: Positive only

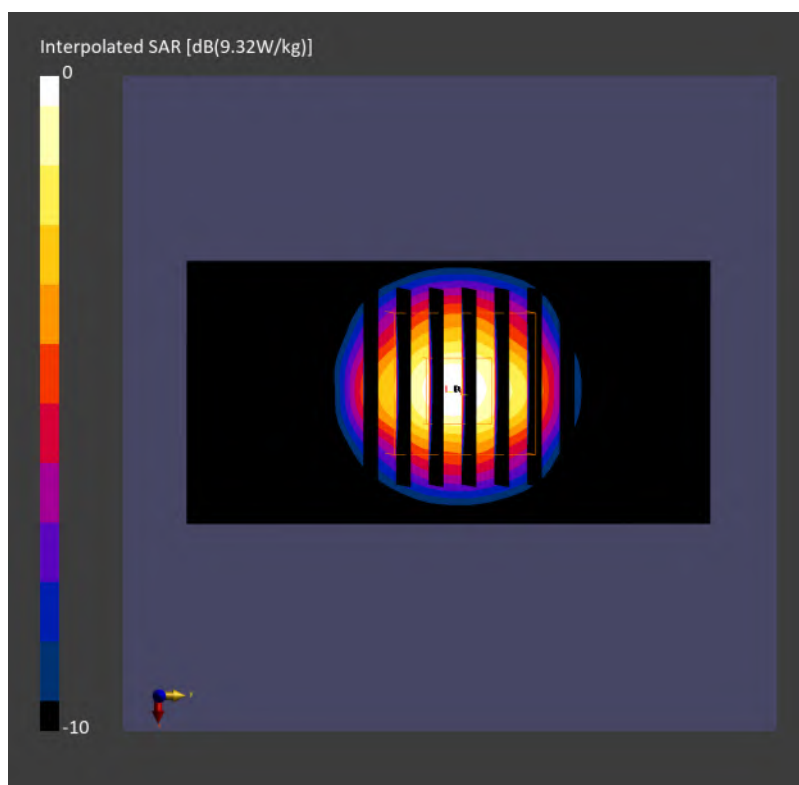

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260913 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.96$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.47, 6.89, 6.77); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.08 W/kg; SAR (10g) = 2.57 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 7.21 W/kg; SAR (8g) = 3.01 W/kg; SAR (10g) = 2.65 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.7 %

TSL Correction: Positive only

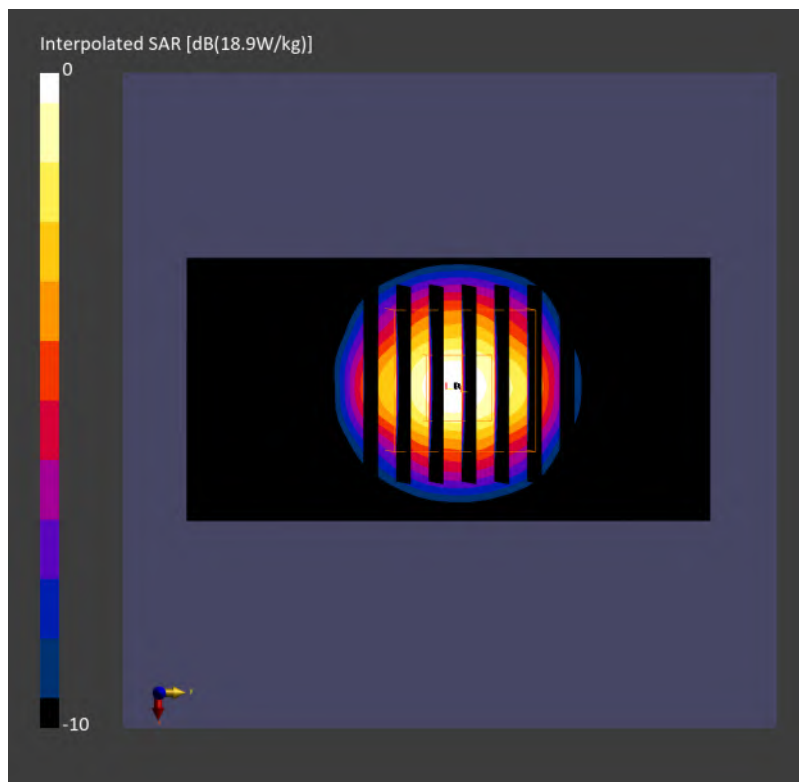

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_600-7200_260914 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 2.83$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.47, 6.89, 6.77); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.82 W/kg; SAR (10g) = 2.46 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 6.92 W/kg; SAR (8g) = 2.87 W/kg; SAR (10g) = 2.53 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.8 %

TSL Correction: Positive only

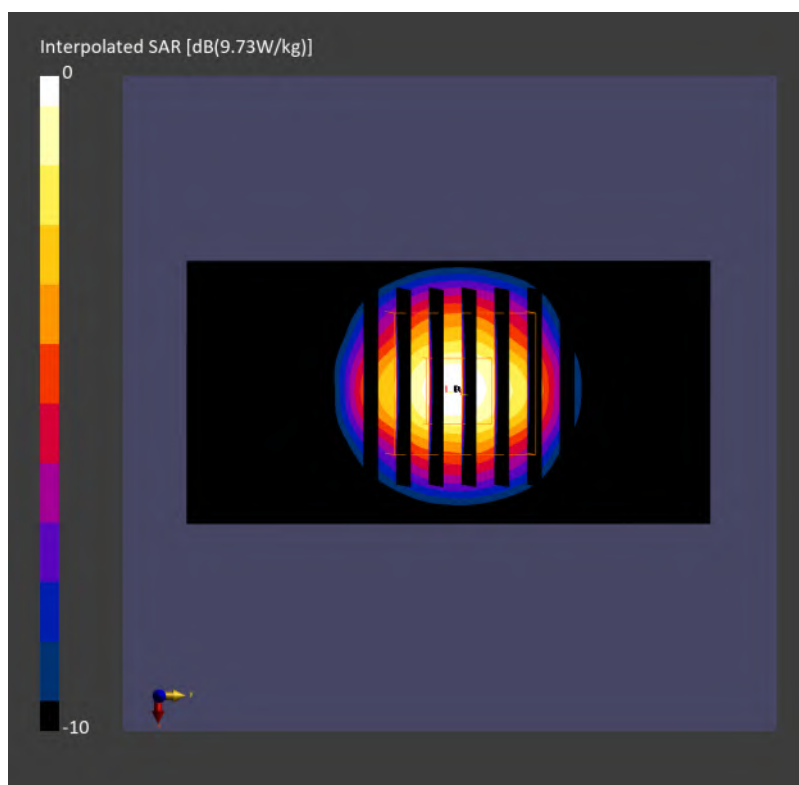

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260830 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.04$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.84 W/kg; SAR (10g) = 2.34 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 6.92 W/kg; SAR (8g) = 2.75 W/kg; SAR (10g) = 2.41 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.0 %

TSL Correction: Positive only

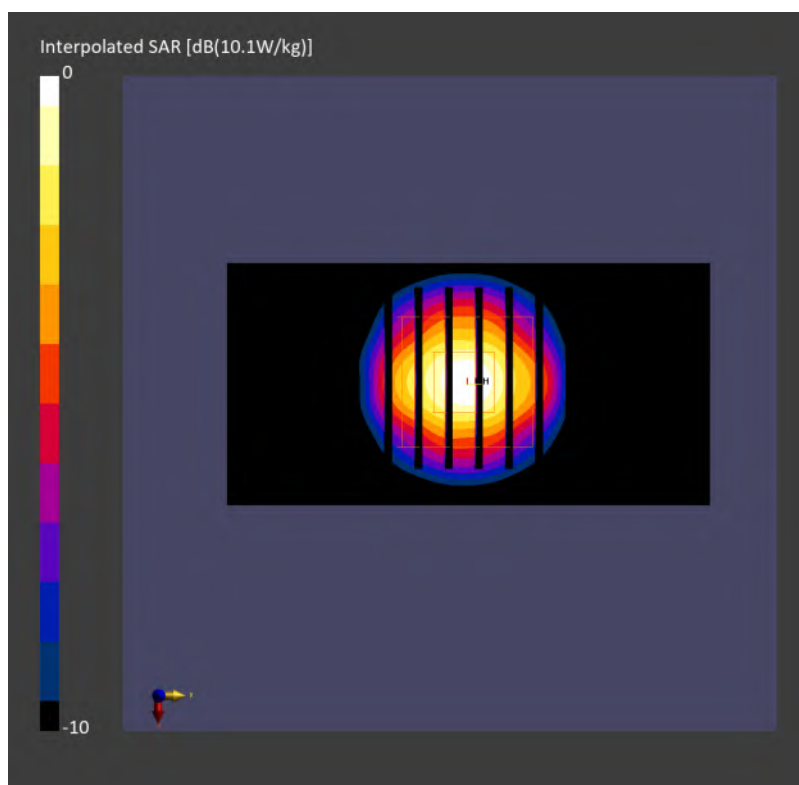

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260831 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 36.8$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.38 W/kg; SAR (10g) = 2.26 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 6.60 W/kg; SAR (8g) = 2.66 W/kg; SAR (10g) = 2.34 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

TSL Correction: Positive only

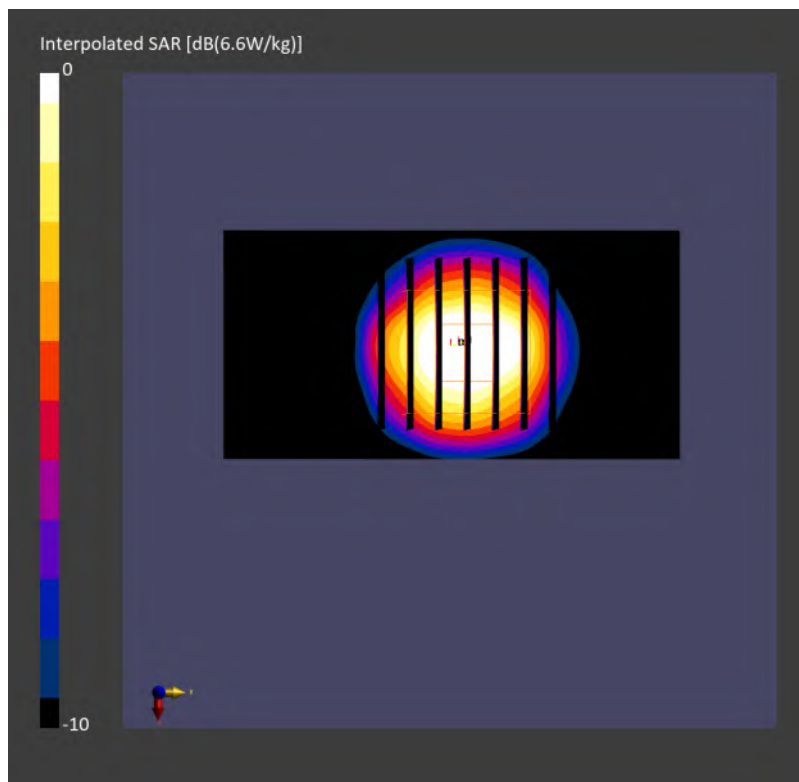

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.46 W/kg; SAR (10g) = 2.28 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.66 W/kg; SAR (8g) = 2.68 W/kg; SAR (10g) = 2.36 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.9 %

TSL Correction: Positive only

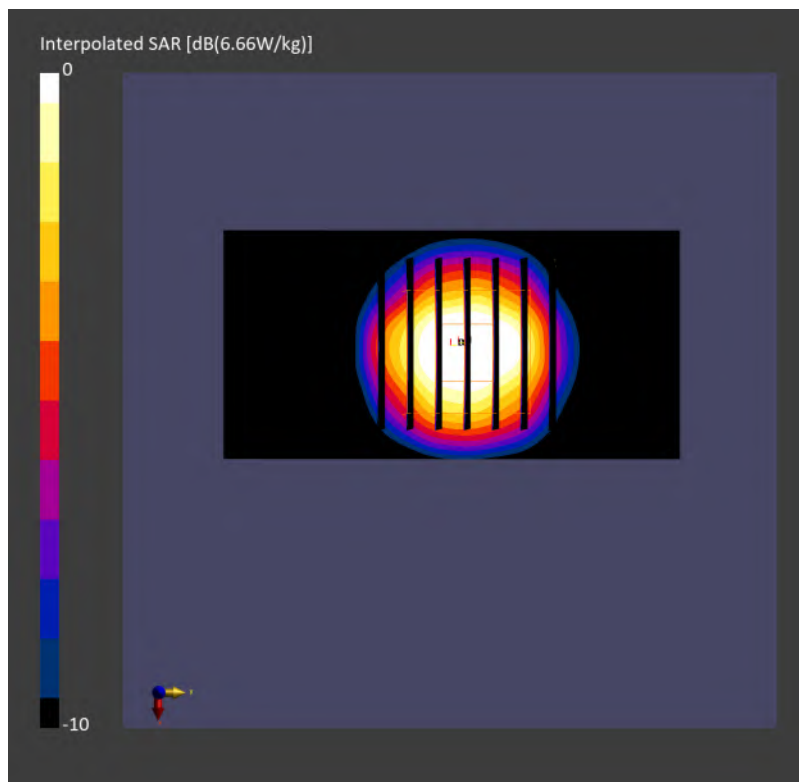

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260902 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(6.84, 6.63, 6.68); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.07 W/kg; SAR (10g) = 2.44 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 7.18 W/kg; SAR (8g) = 2.89 W/kg; SAR (10g) = 2.52 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.0 %

TSL Correction: Positive only

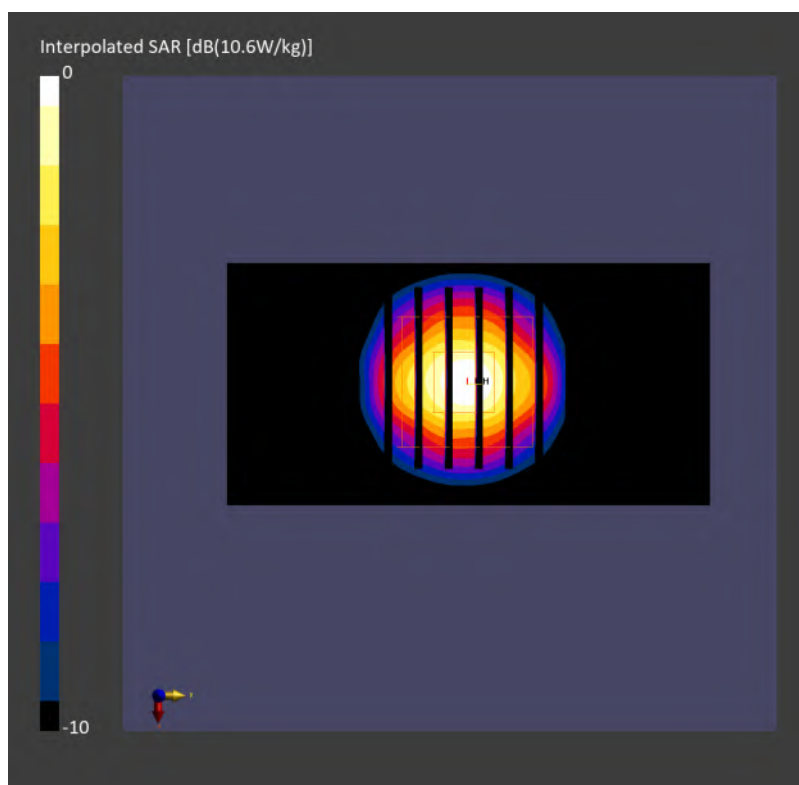

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260906 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.11$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.29 W/kg; SAR (10g) = 2.25 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 6.53 W/kg; SAR (8g) = 2.63 W/kg; SAR (10g) = 2.31 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

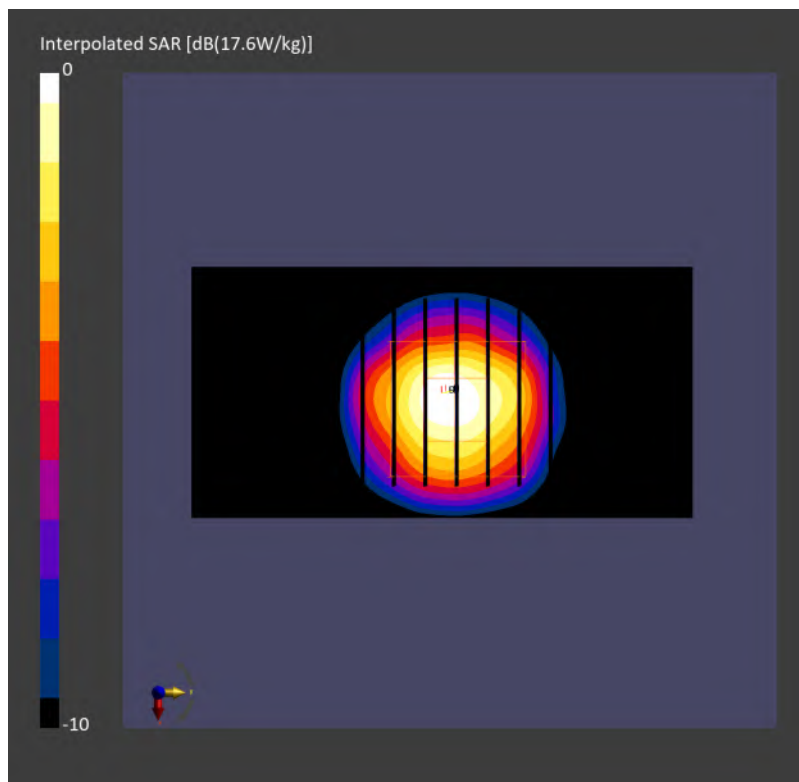

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260907 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.12$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(5.9, 5.89, 5.63); Calibrated: 2025-11-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2025-10-15
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.31 W/kg; SAR (10g) = 2.26 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.02 dB

SAR (1g) = 6.56 W/kg; SAR (8g) = 2.64 W/kg; SAR (10g) = 2.32 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

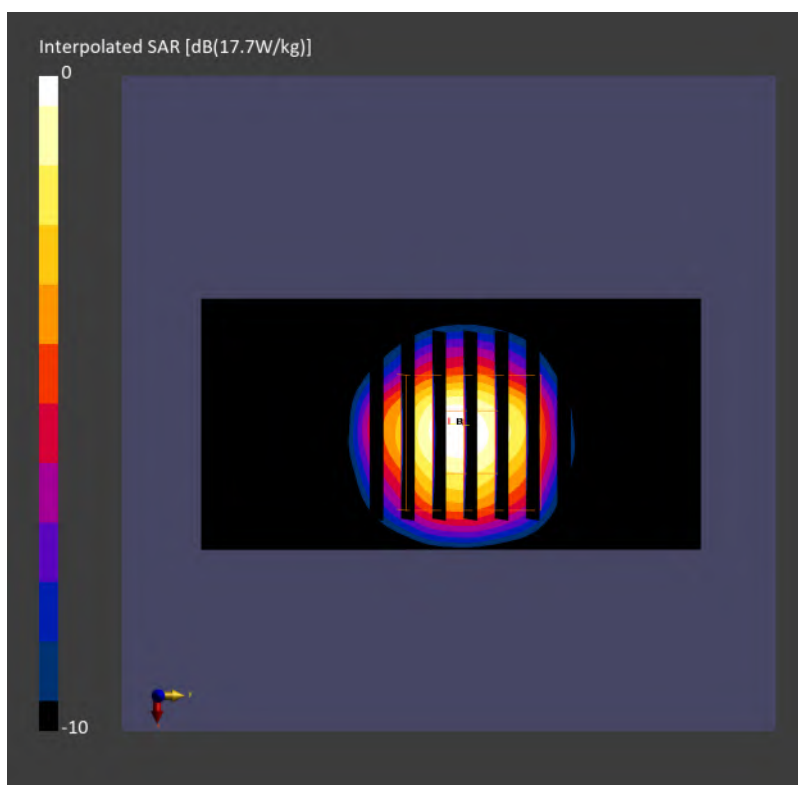

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260913 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.13$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.37, 6.77, 6.66); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.94 W/kg; SAR (10g) = 2.41 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 7.09 W/kg; SAR (8g) = 2.84 W/kg; SAR (10g) = 2.50 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.6 %

TSL Correction: Positive only

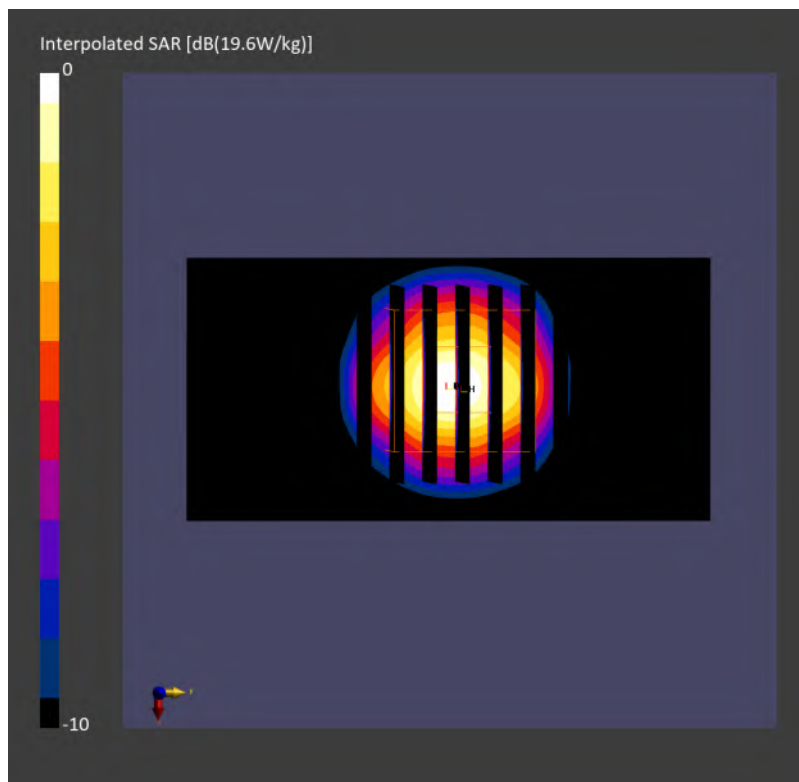

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_260914 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.02$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.37, 6.77, 6.66); Calibrated: 2026-08-14
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2025-10-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.72 W/kg; SAR (10g) = 2.32 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 6.86 W/kg; SAR (8g) = 2.74 W/kg; SAR (10g) = 2.40 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.5 %

TSL Correction: Positive only

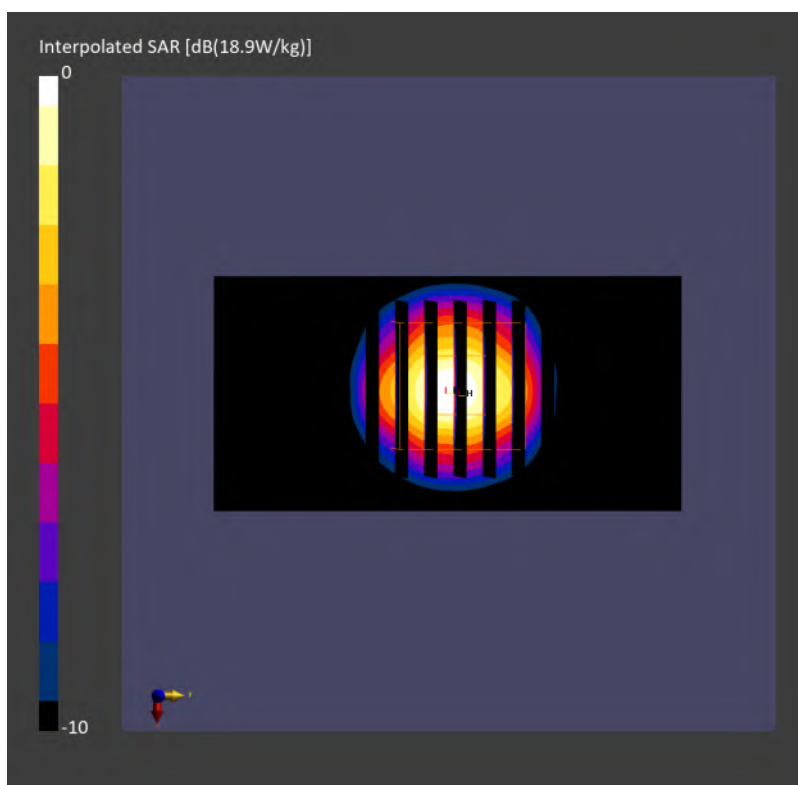

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.56$ S/m; $\epsilon_r = 34.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(5.66, 5.49, 5.53); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.35 W/kg; SAR (10g) = 2.06 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 7.89 W/kg; SAR (8g) = 2.63 W/kg; SAR (10g) = 2.26 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.5 %

TSL Correction: Positive only

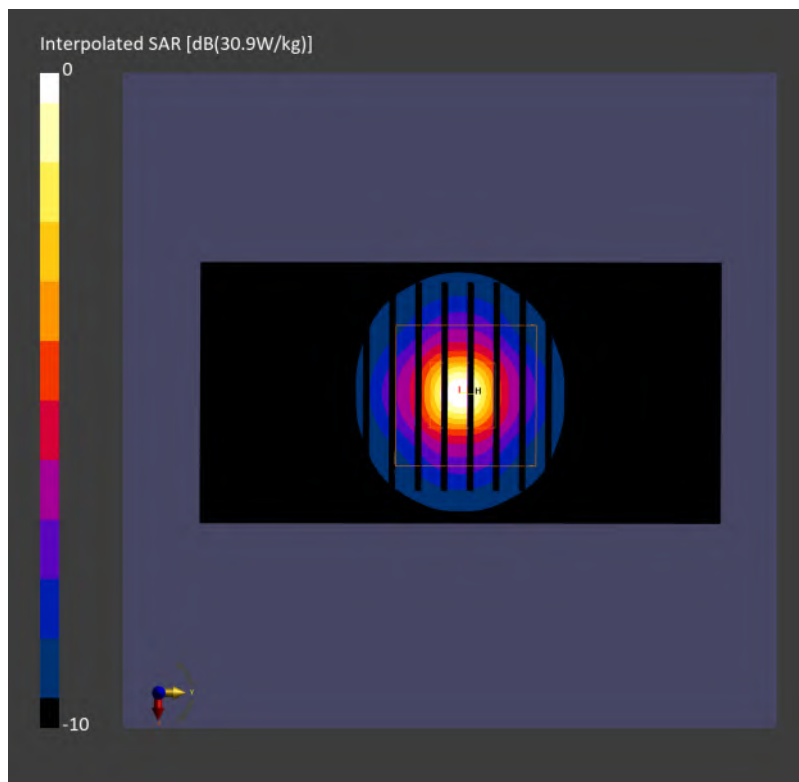

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260905 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.60$ S/m; $\epsilon_r = 36.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(5.66, 5.49, 5.53); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.57 W/kg; SAR (10g) = 2.13 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 8.12 W/kg; SAR (8g) = 2.71 W/kg; SAR (10g) = 2.33 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.5 %

TSL Correction: Positive only

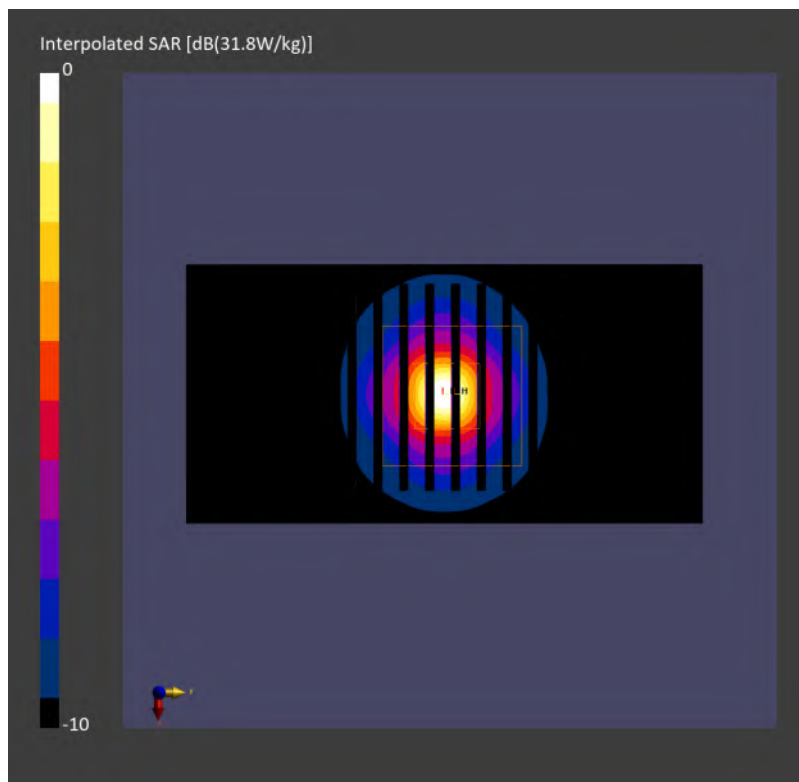

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.94$ S/m; $\epsilon_r = 34.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(5.27, 5.11, 5.15); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.95 W/kg; SAR (10g) = 2.20 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.00 dB

SAR (1g) = 8.60 W/kg; SAR (8g) = 2.83 W/kg; SAR (10g) = 2.44 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.5 %

TSL Correction: Positive only

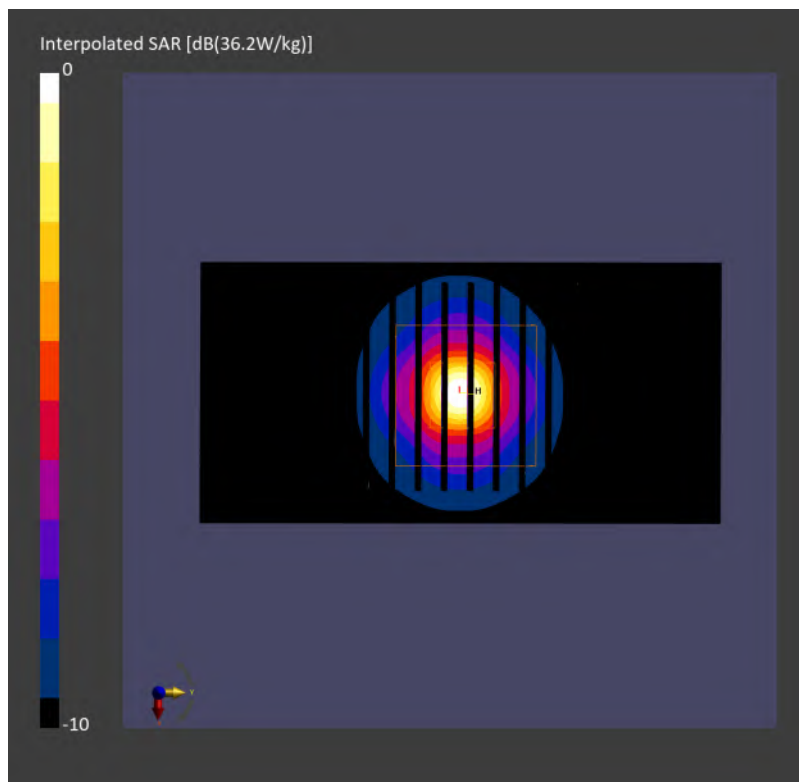

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260905 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.99$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(5.27, 5.11, 5.15); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 8.11 W/kg; SAR (10g) = 2.24 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 8.75 W/kg; SAR (8g) = 2.88 W/kg; SAR (10g) = 2.48 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.4 %

TSL Correction: Positive only

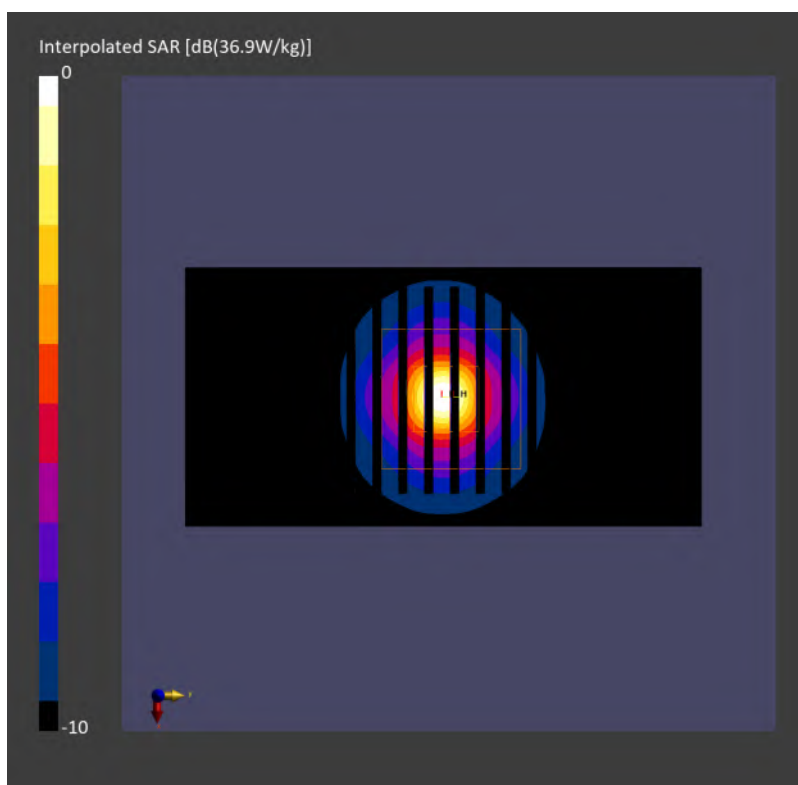

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260903 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.19$ S/m; $\epsilon_r = 33.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(5.21, 5.05, 5.09); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.56 W/kg; SAR (10g) = 2.09 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.01 dB

SAR (1g) = 8.22 W/kg; SAR (8g) = 2.70 W/kg; SAR (10g) = 2.33 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 59.5 %

TSL Correction: Positive only

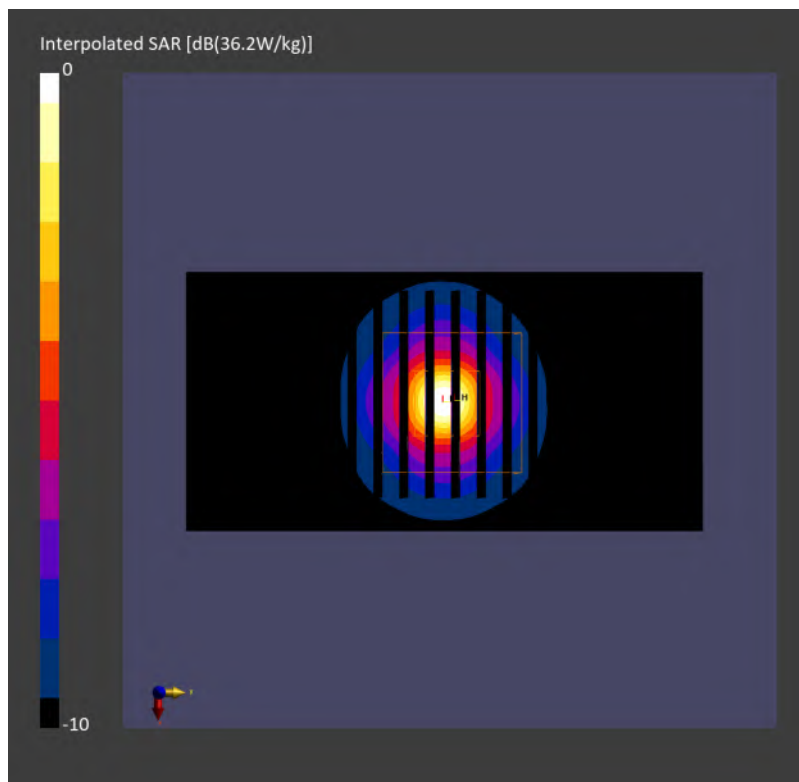

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260905 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.23$ S/m; $\epsilon_r = 35.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(5.21, 5.05, 5.09); Calibrated: 2026-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn661; Calibrated: 2026-05-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.67 W/kg; SAR (10g) = 2.12 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (32.0 mm x 32.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = 0.00 dB

SAR (1g) = 8.32 W/kg; SAR (8g) = 2.73 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 59.6 %

TSL Correction: Positive only

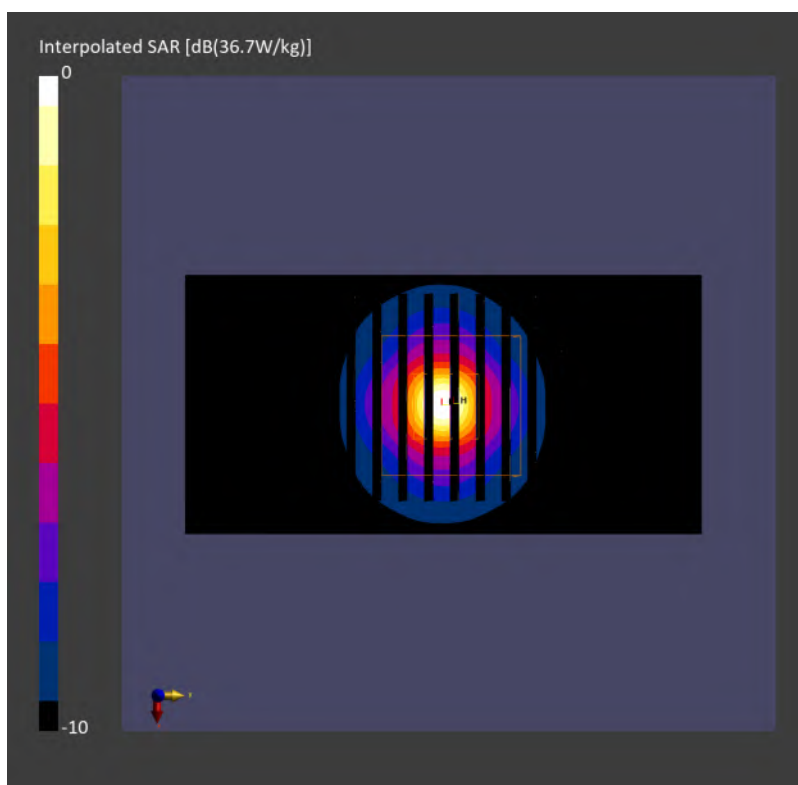

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260923 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.71$ S/m; $\epsilon_r = 38.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.28, 7.08, 7.07); Calibrated: 2026-03-17
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2026-05-19
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.53 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 2.55 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

TSL Correction: Positive only

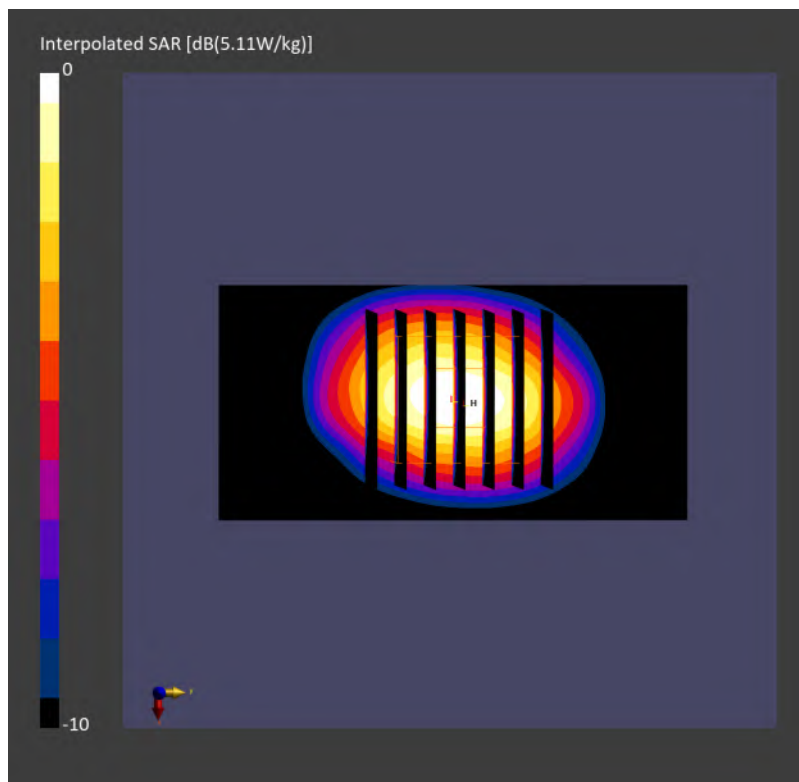

System Check_Head_3900MHz**DUT: D3900V2 - SN1092**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_600-7200_261008 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.07$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(6.46, 6.89, 6.5); Calibrated: 2026-01-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2026-02-13
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.03 W/kg; SAR (10g) = 2.11 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 29.1 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 6.22 W/kg; SAR (8g) = 2.56 W/kg; SAR (10g) = 2.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

TSL Correction: Positive only

