

# Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

## Calibration Certificate

### Dosimetric E-Field Probe

Type:

**ET3DV6**

Serial Number:

**1508**

Place of Calibration:

**Zurich**

Date of Calibration:

**October 25, 2001**

Calibration Interval:

**12 months**

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

*N. Edlószi-Neviana*

Approved by:

*Alain Käfer*

# Probe ET3DV6

## SN:1508

|               |                  |
|---------------|------------------|
| Manufactured: | October 24, 1999 |
| Remade:       | October 11, 2001 |
| Recalibrated: | October 25, 2001 |

Calibrated for System DASY3

**DASY3 - Parameters of Probe: ET3DV6 SN:1508**

## Sensitivity in Free Space

## Diode Compression

|       |                                                 |       |              |
|-------|-------------------------------------------------|-------|--------------|
| NormX | <b>1.62</b> $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP X | <b>97</b> mV |
| NormY | <b>1.51</b> $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP Y | <b>97</b> mV |
| NormZ | <b>1.49</b> $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP Z | <b>97</b> mV |

## Sensitivity in Tissue Simulating Liquid


|             |                               |                             |                                  |
|-------------|-------------------------------|-----------------------------|----------------------------------|
| <b>Head</b> | <b>450 MHz</b>                | $\epsilon_r = 40.4 \pm 5\%$ | $s = 0.87 \pm 5\% \text{ mho/m}$ |
| ConvF X     | <b>6.82</b> extrapolated      | Boundary effect:            |                                  |
| ConvF Y     | <b>6.82</b> extrapolated      | Alpha                       | <b>0.25</b>                      |
| ConvF Z     | <b>6.82</b> extrapolated      | Depth                       | <b>2.86</b>                      |
| <b>Head</b> | <b>900 MHz</b>                | $\epsilon_r = 41.5 \pm 5\%$ | $s = 0.97 \pm 5\% \text{ mho/m}$ |
| <b>Head</b> | <b>835 MHz</b>                | $\epsilon_r = 41.5 \pm 5\%$ | $s = 0.90 \pm 5\% \text{ mho/m}$ |
| ConvF X     | <b>6.35</b> $\pm 9.5\%$ (k=2) | Boundary effect:            |                                  |
| ConvF Y     | <b>6.35</b> $\pm 9.5\%$ (k=2) | Alpha                       | <b>0.35</b>                      |
| ConvF Z     | <b>6.35</b> $\pm 9.5\%$ (k=2) | Depth                       | <b>2.68</b>                      |
| <b>Head</b> | <b>1500 MHz</b>               | $\epsilon_r = 40.4 \pm 5\%$ | $s = 1.23 \pm 5\% \text{ mho/m}$ |
| ConvF X     | <b>5.72</b> interpolated      | Boundary effect:            |                                  |
| ConvF Y     | <b>5.72</b> interpolated      | Alpha                       | <b>0.47</b>                      |
| ConvF Z     | <b>5.72</b> interpolated      | Depth                       | <b>2.43</b>                      |
| <b>Head</b> | <b>1800 MHz</b>               | $\epsilon_r = 40.0 \pm 5\%$ | $s = 1.40 \pm 5\% \text{ mho/m}$ |
| <b>Head</b> | <b>1900 MHz</b>               | $\epsilon_r = 40.0 \pm 5\%$ | $s = 1.40 \pm 5\% \text{ mho/m}$ |
| ConvF X     | <b>5.41</b> $\pm 9.5\%$ (k=2) | Boundary effect:            |                                  |
| ConvF Y     | <b>5.41</b> $\pm 9.5\%$ (k=2) | Alpha                       | <b>0.53</b>                      |
| ConvF Z     | <b>5.41</b> $\pm 9.5\%$ (k=2) | Depth                       | <b>2.31</b>                      |

## Sensor Offset

|                            |                                 |    |
|----------------------------|---------------------------------|----|
| Probe Tip to Sensor Center | <b>2.7</b>                      | mm |
| Optical Surface Detection  | <b>1.4 <math>\pm</math> 0.2</b> | mm |


## Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

**f = 30 MHz, TEM cell if110**

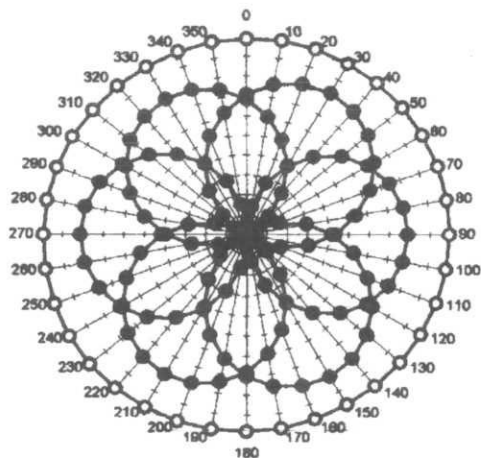


—●— X    - - - ● - - Y    ····· ● ····· Z    —○— Tot

**f = 100 MHz, TEM cell if110**

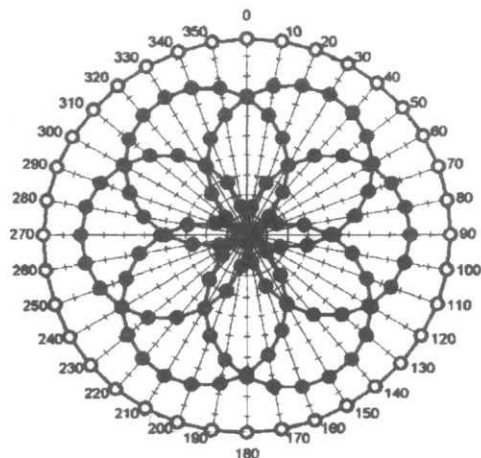


—●— X    - - - ● - - Y    ····· ● ····· Z    —○— Tot

**f = 300 MHz, TEM cell if110**

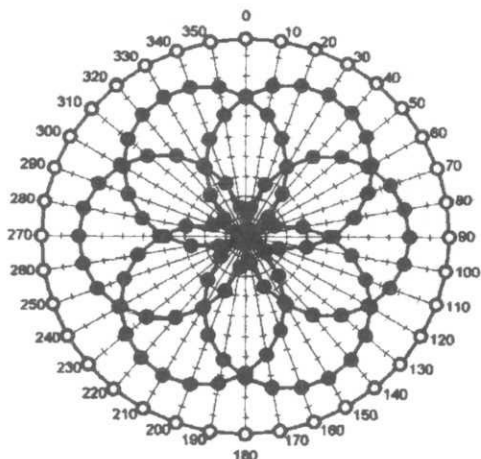


—●— X    - - - ● - - Y    ····· ● ····· Z    —○— Tot


**f = 900 MHz, TEM cell if110**

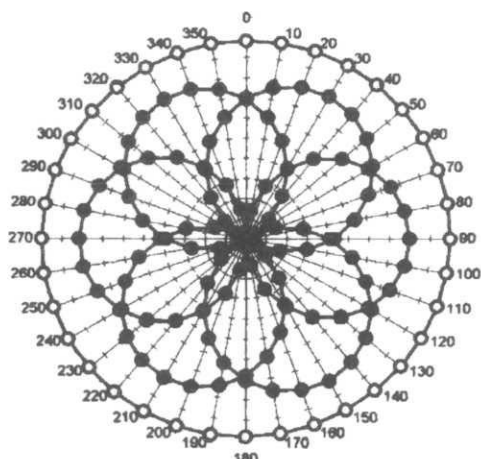

—●— X    - - - ● - - Y    ····· ● ····· Z    —○— Tot

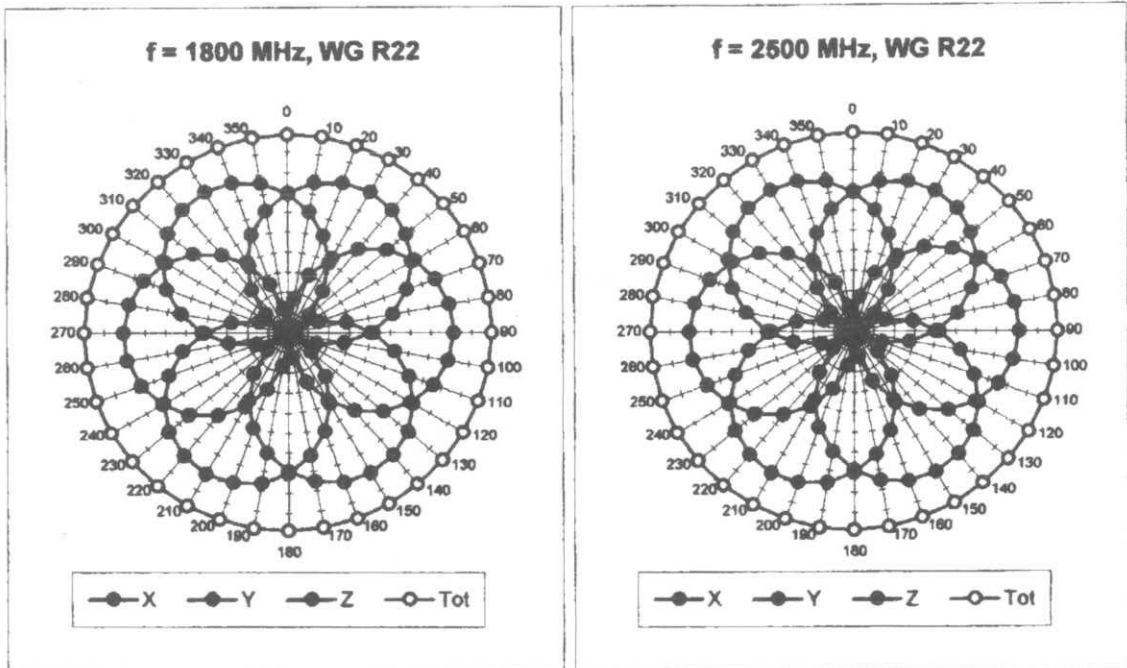


### Isotropy Error ( $\phi$ ), $\theta = 0^\circ$


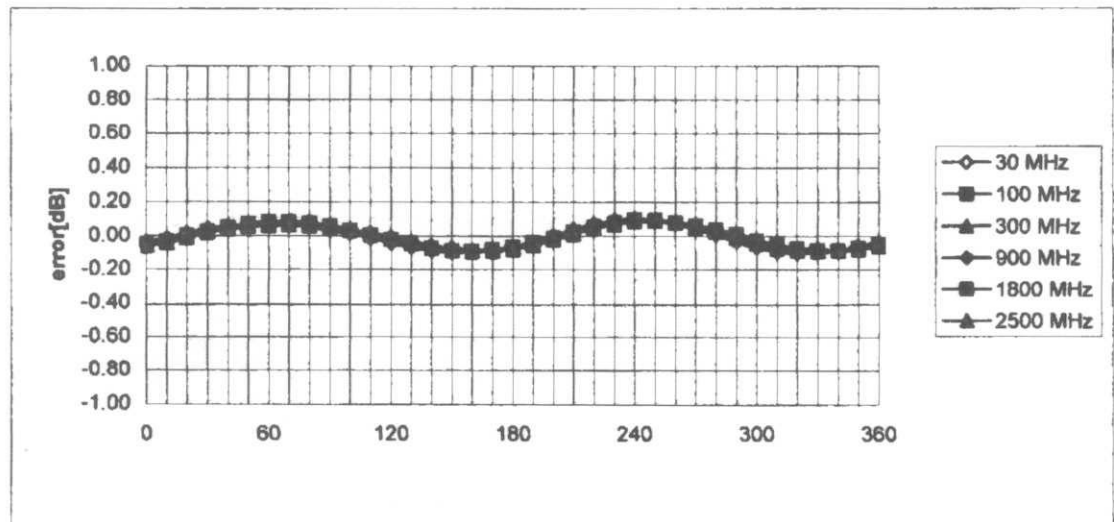


## Frequency Response of E-Field


( TEM-Cell:ifi110, Waveguide R22)

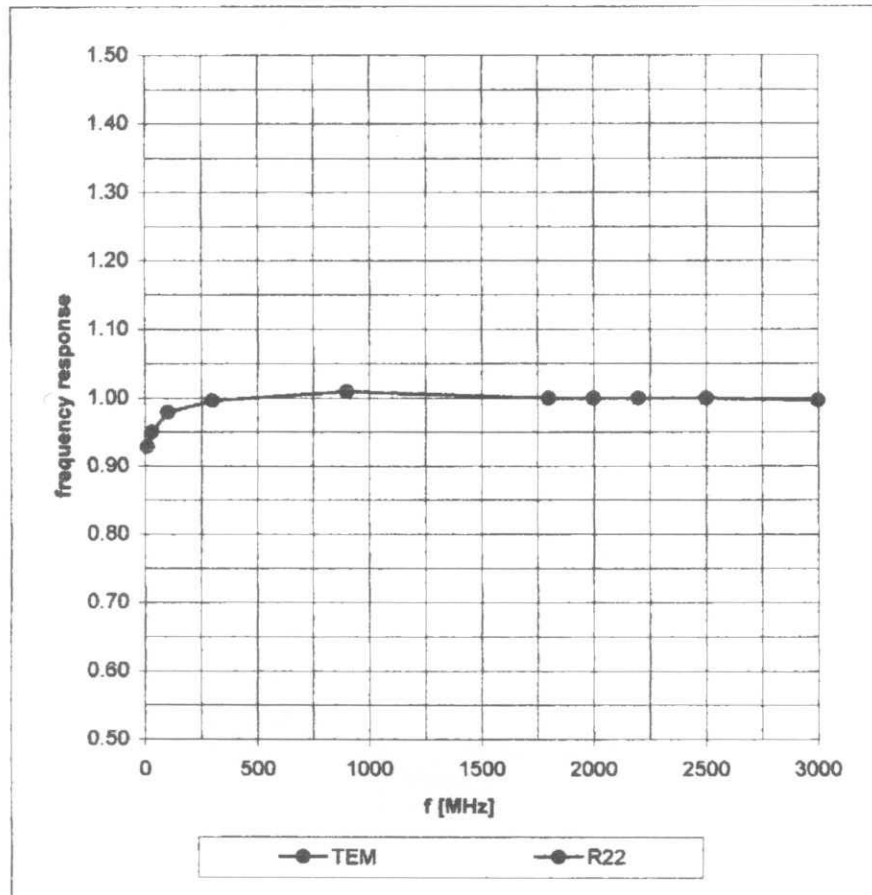

# Dynamic Range $f(\text{SAR}_{\text{brain}})$ ( Waveguide R22 )

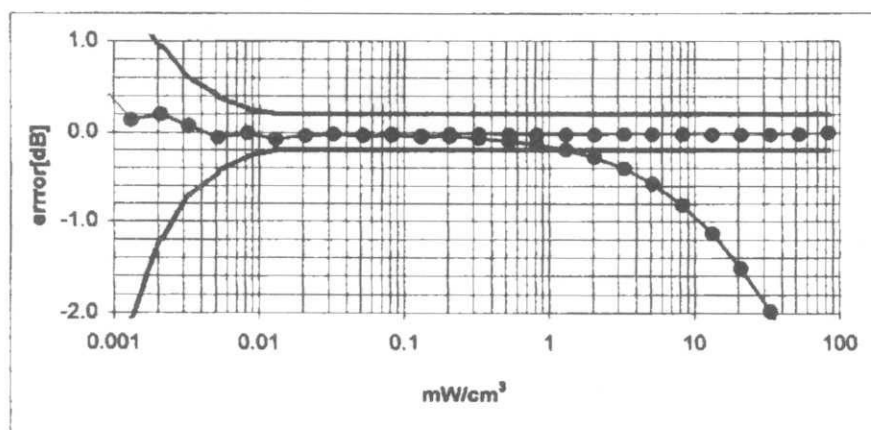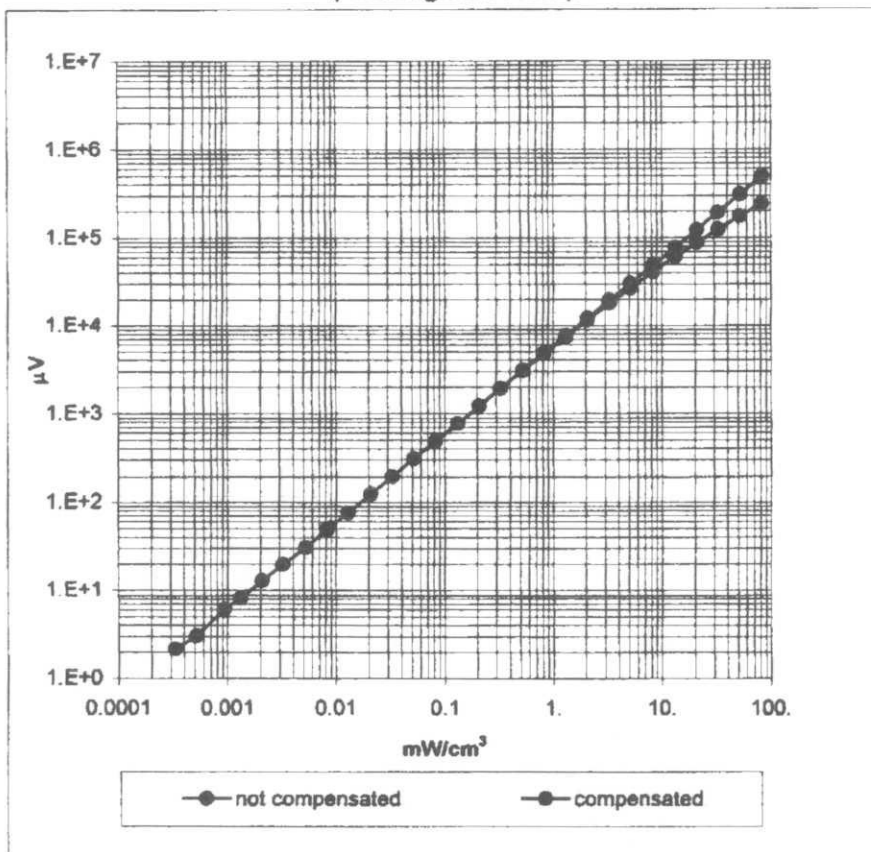

## Conversion Factor Assessment

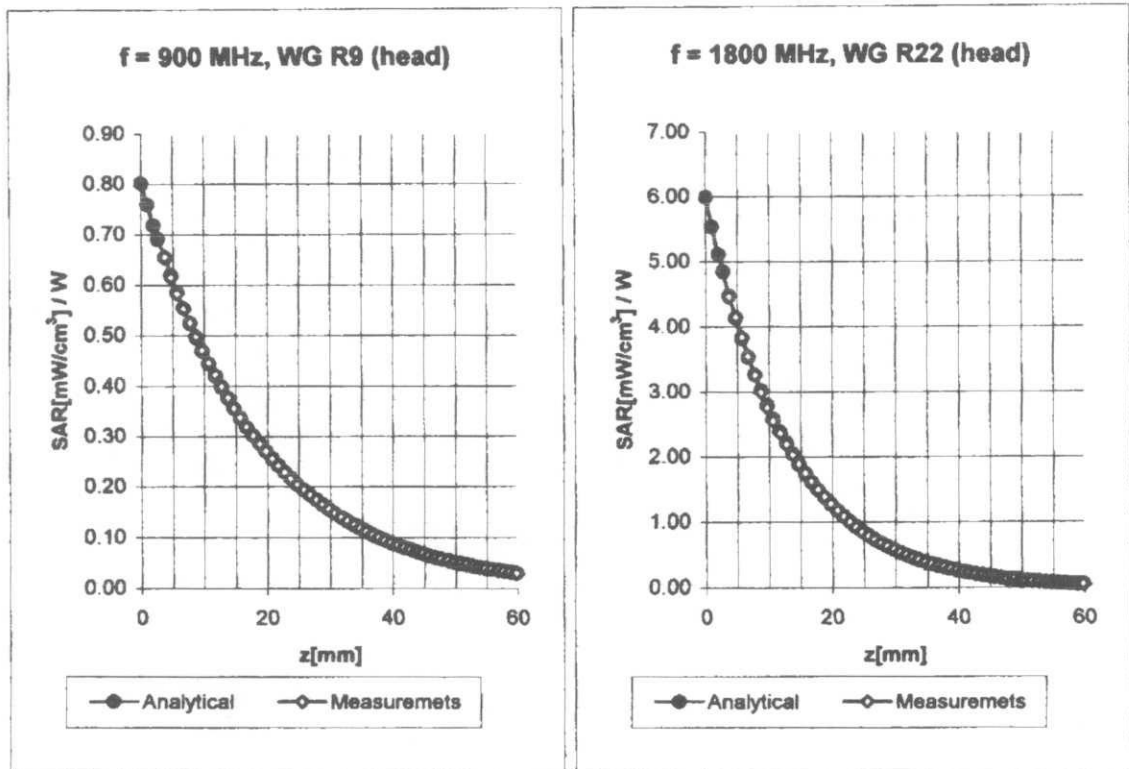

**Head**      **800 - 1000 MHz**

$\epsilon_r = 39.0 - 43.5$

$\sigma = 0.80 - 1.10 \text{ mho/m}$

ConvF X      **6.35**  $\pm 9.5\%$  (k=2)

Boundary effect:

ConvF Y      **6.35**  $\pm 9.5\%$  (k=2)

Alpha      **0.35**

ConvF Z      **6.35**  $\pm 9.5\%$  (k=2)

Depth      **2.68**

**Head**      **1700 - 1910 MHz**

$\epsilon_r = 39.5 - 41.0$

$\sigma = 1.20 - 1.55 \text{ mho/m}$

ConvF X      **5.41**  $\pm 9.5\%$  (k=2)

Boundary effect:

ConvF Y      **5.41**  $\pm 9.5\%$  (k=2)


Alpha      **0.53**

ConvF Z      **5.41**  $\pm 9.5\%$  (k=2)

Depth      **2.31**

## Deviation from Isotropy in HSL

Error ( $\theta, \phi$ ),  $f = 900$  MHz

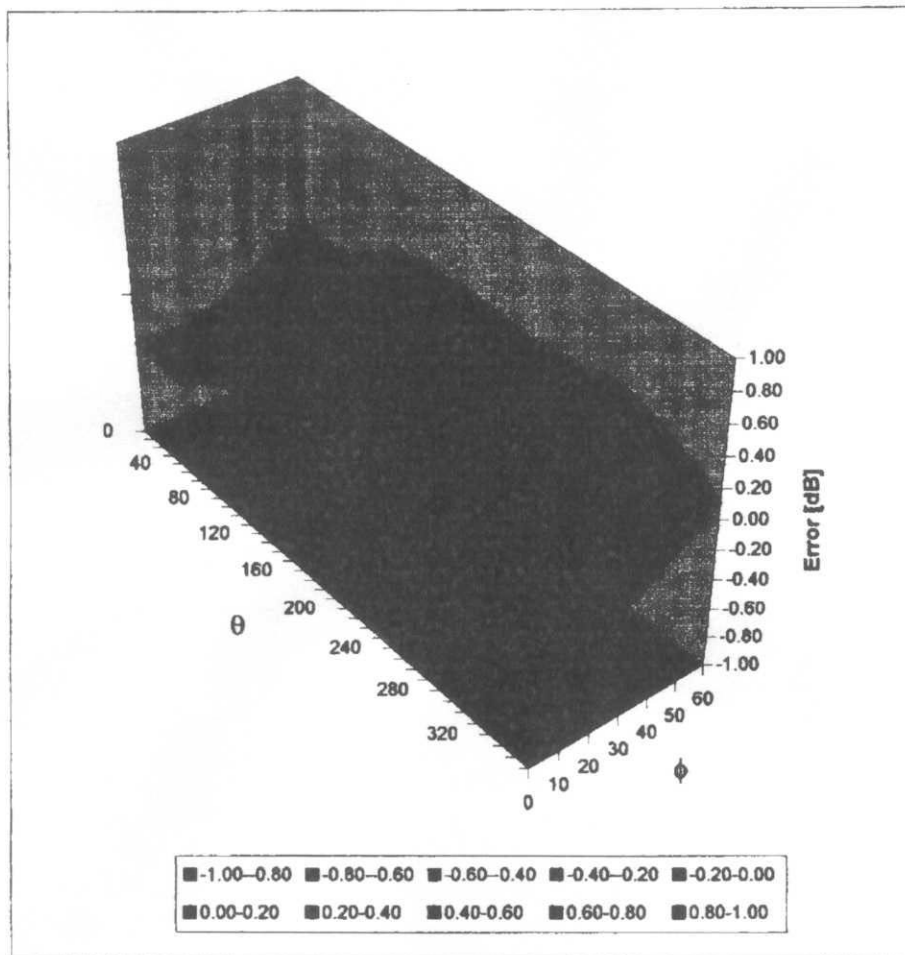

**Additional Conversion Factors**  
for Dosimetric E-Field Probe

Type:

**ET3DV6**

Serial Number:

**1508**

Place of Assessment:

**Zurich**

Date of Assessment:


**November 14, 2001**

Probe Calibration Date:

**October 25, 2001**

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



## Dosimetric E-Field Probe ET3DV6 SN:1508

Conversion factor ( $\pm$  standard deviation)

|          |       |               |                                                                       |
|----------|-------|---------------|-----------------------------------------------------------------------|
| 835 MHz  | ConvF | $6.5 \pm 8\%$ | $\epsilon_r = 41.5$<br>$\sigma = 0.90 \text{ mho/m}$<br>(head tissue) |
| 1950 MHz | ConvF | $5.1 \pm 8\%$ | $\epsilon_r = 40.0$<br>$\sigma = 1.40 \text{ mho/m}$<br>(head tissue) |
| 835 MHz  | ConvF | $6.2 \pm 8\%$ | $\epsilon_r = 55.2$<br>$\sigma = 0.97 \text{ mho/m}$<br>(body tissue) |
| 900 MHz  | ConvF | $6.1 \pm 8\%$ | $\epsilon_r = 55.0$<br>$\sigma = 1.05 \text{ mho/m}$<br>(body tissue) |
| 1800 MHz | ConvF | $5.0 \pm 8\%$ | $\epsilon_r = 53.3$<br>$\sigma = 1.52 \text{ mho/m}$<br>(body tissue) |
| 1950 MHz | ConvF | $4.7 \pm 8\%$ | $\epsilon_r = 53.3$<br>$\sigma = 1.52 \text{ mho/m}$<br>(body tissue) |