

**HAC\_E\_Dipole\_835****DUT: HAC-Dipole 835 MHz**

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: EF3DV3 - SN4047; ConvF(1, 1, 1) @ 835 MHz; Calibrated: 2020/1/24

- Sensor-Surface: (Fix Surface)

- Electronics: DAE4 Sn1311; Calibrated: 2019/8/27

- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;

- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7470)

**E Scan - measurement distance from the probe sensor center to CD835 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x361x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 141.7 V/m; Power Drift = -0.05 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 118.9 V/m

Average value of Total=(118+118.9) / 2 = 118.45 V/m

PMF scaled E-field



|                                      |                                      |                                      |
|--------------------------------------|--------------------------------------|--------------------------------------|
| Grid 1 <b>M4</b><br><b>117.7 V/m</b> | Grid 2 <b>M4</b><br><b>118.0 V/m</b> | Grid 3 <b>M4</b><br><b>112.0 V/m</b> |
| Grid 4 <b>M4</b><br><b>64.39 V/m</b> | Grid 5 <b>M4</b><br><b>64.56 V/m</b> | Grid 6 <b>M4</b><br><b>62.44 V/m</b> |
| Grid 7 <b>M4</b><br><b>117.6 V/m</b> | Grid 8 <b>M4</b><br><b>118.9 V/m</b> | Grid 9 <b>M4</b><br><b>114.8 V/m</b> |

**Cursor:**

Total = 118.9 V/m

E Category: M4

Location: 1, 73.5, 9.7 mm

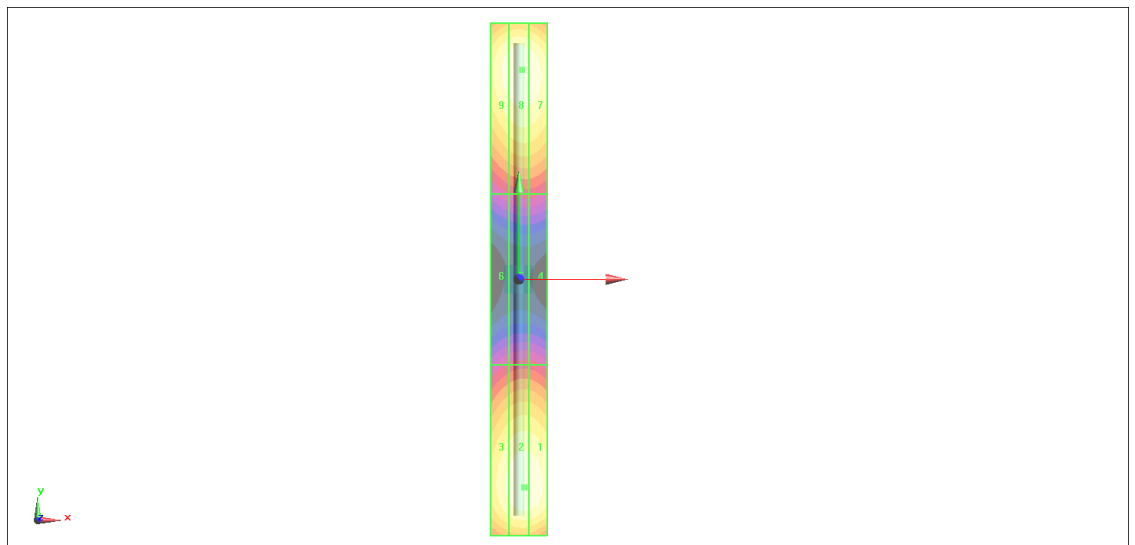

0 dB = 118.9 V/m = 41.51 dBV/m

**HAC\_E\_Dipole\_1880****DUT: HAC Dipole 1880 MHz**

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: EF3DV3 - SN4047; ConvF(1, 1, 1) @ 1880 MHz; Calibrated: 2020/1/24

- Sensor-Surface: (Fix Surface)

- Electronics: DAE4 Sn1311; Calibrated: 2019/8/27

- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;

- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7470)

**E Scan - measurement distance from the probe sensor center to CD1880 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x181x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 171.1 V/m; Power Drift = 0.02 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 91.88 V/m

Average value of Total=(90.88+91.88) / 2 = 91.38 V/m

PMF scaled E-field



|                                      |                                      |                                      |
|--------------------------------------|--------------------------------------|--------------------------------------|
| Grid 1 <b>M3</b><br><b>90.07 V/m</b> | Grid 2 <b>M3</b><br><b>90.88 V/m</b> | Grid 3 <b>M3</b><br><b>87.55 V/m</b> |
| Grid 4 <b>M3</b><br><b>64.88 V/m</b> | Grid 5 <b>M3</b><br><b>65.01 V/m</b> | Grid 6 <b>M3</b><br><b>63.86 V/m</b> |
| Grid 7 <b>M3</b><br><b>90.68 V/m</b> | Grid 8 <b>M3</b><br><b>91.88 V/m</b> | Grid 9 <b>M3</b><br><b>89.41 V/m</b> |

**Cursor:**

Total = 91.88 V/m

E Category: M3

Location: 0.5, 33.5, 9.7 mm

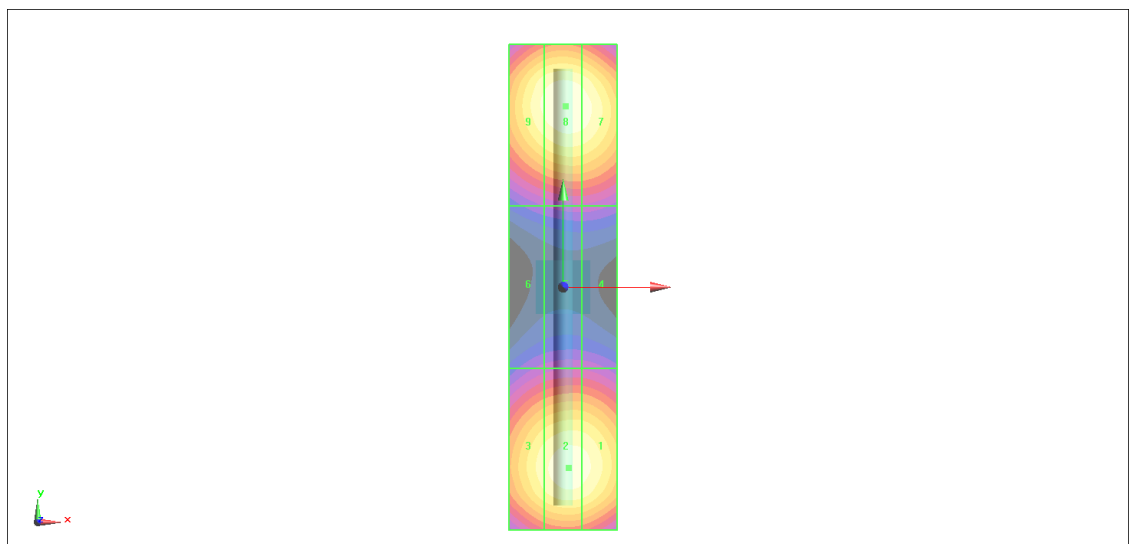

0 dB = 91.88 V/m = 39.26 dBV/m

**HAC\_E\_Dipole\_2450****DUT: HAC Dipole 2450 MHz**

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: EF3DV3 - SN4047; ConvF(1, 1, 1) @ 2450 MHz; Calibrated: 2020/1/24

- Sensor-Surface: (Fix Surface)

- Electronics: DAE4 Sn1311; Calibrated: 2019/8/27

- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;

- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.14 (7483)

**E Scan - measurement distance from the probe sensor center to CD2450 = 10mm & 15mm**  
**2/Hearing Aid Compatibility Test at 15mm distance (41x181x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 79.93 V/m; Power Drift = 0.01 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 85.43 V/m

Average value of Total=(84.63+85.43) / 2 = 85.03 V/m

PMF scaled E-field



|                                      |                                      |                                      |
|--------------------------------------|--------------------------------------|--------------------------------------|
| Grid 1 <b>M3</b><br><b>84.41 V/m</b> | Grid 2 <b>M3</b><br><b>84.63 V/m</b> | Grid 3 <b>M3</b><br><b>81.74 V/m</b> |
| Grid 4 <b>M3</b><br><b>75.51 V/m</b> | Grid 5 <b>M3</b><br><b>75.82 V/m</b> | Grid 6 <b>M3</b><br><b>73.75 V/m</b> |
| Grid 7 <b>M3</b><br><b>84.09 V/m</b> | Grid 8 <b>M3</b><br><b>85.43 V/m</b> | Grid 9 <b>M3</b><br><b>83.21 V/m</b> |

**Cursor:**

Total = 85.43 V/m

E Category: M3

Location: 0.5, 24.5, 9.7 mm

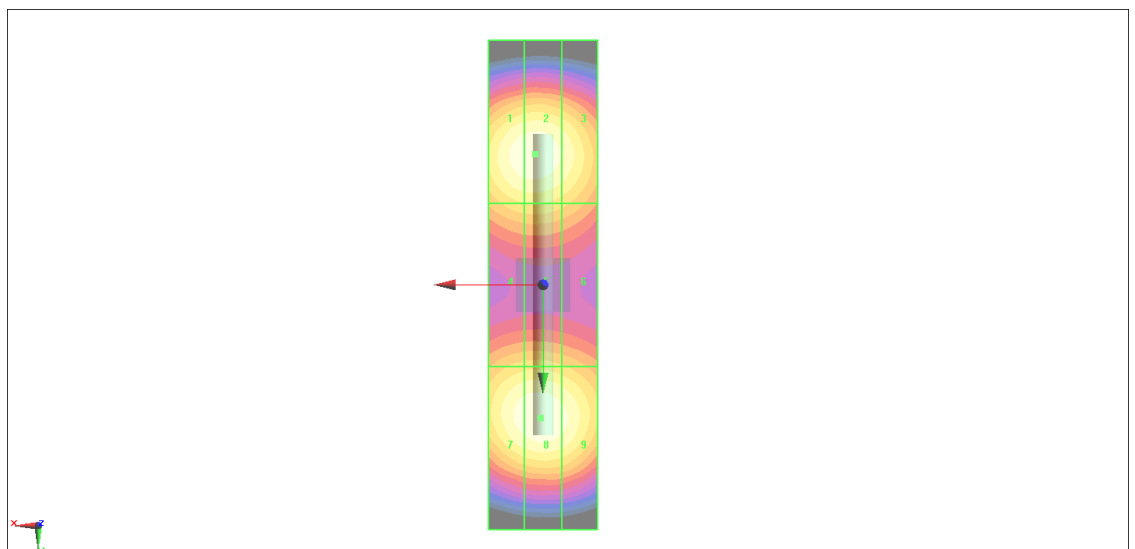

0 dB = 85.43 V/m = 38.63 dBV/m

**HAC\_E\_Dipole\_2600****DUT: HAC Dipole 2600 MHz**

Communication System: CW; Frequency: 2600 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: EF3DV3 - SN4047; ConvF(1, 1, 1) @ 2600 MHz; Calibrated: 2020/1/24

- Sensor-Surface: (Fix Surface)

- Electronics: DAE4 Sn1311; Calibrated: 2019/8/27

- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;

- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7470)

**E Scan - measurement distance from the probe sensor center to CD2600 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x181x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 69.62 V/m; Power Drift = 0.02 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 87.56 V/m

Average value of Total=(86.25+87.56) / 2 = 86.905 V/m

PMF scaled E-field



|                                      |                                      |                                      |
|--------------------------------------|--------------------------------------|--------------------------------------|
| Grid 1 <b>M3</b><br><b>85.51 V/m</b> | Grid 2 <b>M3</b><br><b>86.25 V/m</b> | Grid 3 <b>M3</b><br><b>83.59 V/m</b> |
| Grid 4 <b>M3</b><br><b>79.27 V/m</b> | Grid 5 <b>M3</b><br><b>79.79 V/m</b> | Grid 6 <b>M3</b><br><b>77.87 V/m</b> |
| Grid 7 <b>M3</b><br><b>86.44 V/m</b> | Grid 8 <b>M3</b><br><b>87.56 V/m</b> | Grid 9 <b>M3</b><br><b>85.02 V/m</b> |

**Cursor:**

Total = 87.56 V/m

E Category: M3

Location: 0.5, 23, 9.7 mm

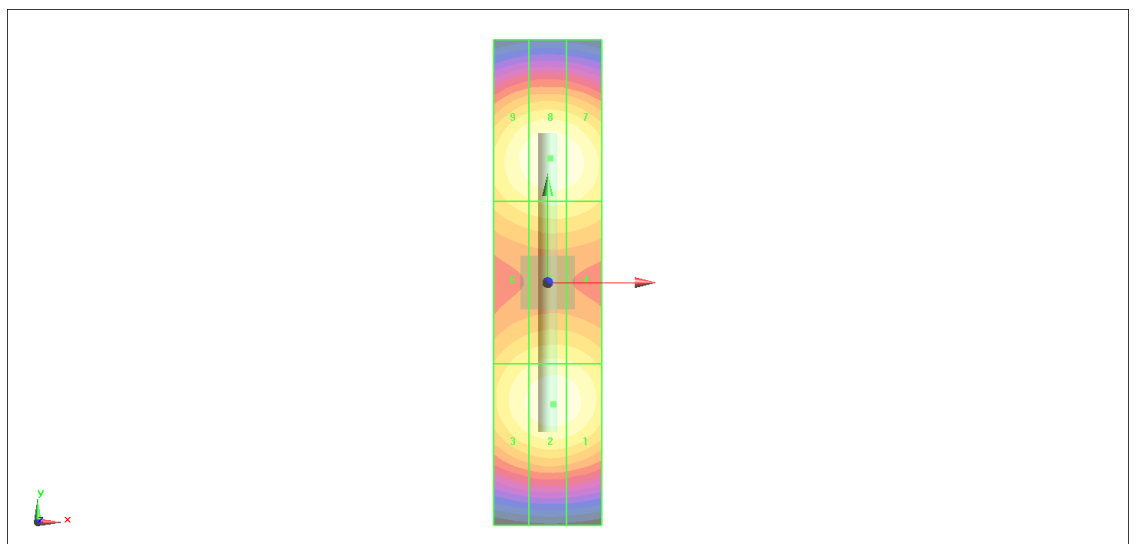

0 dB = 87.56 V/m = 38.85 dBV/m