



HAC Test Report IHDT6FF1

Date of test: 8/18/2005
Date of Report: 8/25/2005

Laboratory: Motorola Mobile Devices Business Product Safety & Compliance Laboratory
600 N. US Highway 45
Room: MW113
Libertyville, Illinois 60048

Test Responsible: Scott Kelley
Disability Access Manager

Statement of Compliance: Motorola declares under its sole responsibility that portable cellular telephone FCC ID IHDT6FF1 to which this declaration relates, complies with recommendations and guidelines FCC 47 CFR §20.19. The measurements were performed to ensure compliance to the ANSI PC63.19-2001 rd 3.6 standard. It also declares that the product was tested in accordance with the appropriate measurement standards, guidelines and recommended practices. Any deviations from these standards, guidelines and recommended practices are noted below:

(none)

Results Summary: **Max E Field emission = 38.15 dB V/m @ 1880 MHz**
Max H Field emission = -13.11 dB A/m @ 1850 MHz
M Category = M3



©Motorola, Inc. 2005

This test report shall not be reproduced except in full, without written approval of the laboratory.

The results and statements contained herein relate only to the items tested. The names of individuals involved may be mentioned only in connection with the statements or results from this report.

Motorola encourages all feedback, both positive and negative, on this test report.

Table of Contents

1. INTRODUCTION	3
2. DESCRIPTION OF THE DEVICE UNDER TEST.....	3
3. TEST EQUIPMENT USED.....	3
4. SYSTEM ACCURACY VERIFICATION.....	4
5. PROBE MODULATION FACTOR	5
6. TEST RESULTS.....	6
APPENDIX 1: HAC DISTRIBUTION PLOTS FOR SYSTEM ACCURACY VERIFICATION	8
APPENDIX 2: HAC DISTRIBUTION PLOTS FOR E-FIELD AND H-FIELD	9
APPENDIX 3: PROBE CALIBRATION CERTIFICATE	12
APPENDIX 4: MEASUREMENT UNCERTAINTY BUDGET.....	13
A4.1 Motorola Uncertainty Budget for RF HAC Testing.....	14
A4.2 Probe Rotation Contributions to Isotropy Error	14

1. Introduction

The Motorola Mobile Devices Business Product Safety Laboratory has performed Hearing Aid Compatibility (HAC) measurements for the portable cellular phone (FCC ID IHDT6FF1). The portable cellular phone was tested in accordance with ANSI PC63.19-2001 rd 3.6 standard. The test results presented herein clearly demonstrate compliance FCC 47 CFR § 20.19. This report demonstrates compliance for near field emissions only and not for the T-coil performance compliance.

2. Description of the Device Under Test

Table 1: Information for the Device Under Test

FCC ID Number	IHDT6FF1									
Serial number	TA19100942									
Mode(s) of Operation	GSM 900	GSM 1800	GSM 1900	GPRS 900	GPRS 1800	GPRS 1900	EDGE 900	EDGE 1800	EDGE 1900	BlueTooth
Modulation Mode(s)	GMSK	GMSK	GMSK	GMSK	GMSK	GMSK	8PSK	8PSK	8PSK	GMSK
Maximum Output Power Setting	33.00 dBm	30.00 dBm	30.00 dBm	33.00 dBm	30.00 dBm	30.00 dBm	28.00 dBm	26.00 dBm	26.00 dBm	0.00 - 4.00 dBm
Duty Cycle	1:8	1:8	1:8	2:8	2:8	2:8	2:8	2:8	2:8	1:1
Transmitting Frequency Rang(s)	880.2-914.8 MHz	1710.2-1784.8 MHz	1850.2-1909.8 MHz	880.2-914.8 MHz	1710.2-1784.8 MHz	1850.2-1909.8 MHz	880.2-914.8 MHz	1710.2-1784.8 MHz	1850.2-1909.8 MHz	2400 - 2483.5 MHz
Production Unit or Identical Prototype (47 CFR §2.908)	Identical Prototype									
Device Category	Portable									

3. Test Equipment Used

The Motorola Mobile Devices Business Product Safety & Compliance Laboratory utilizes a Dosimetric Assessment System (Dasy4™ v4.5) manufactured by Schmid & Partner Engineering AG (SPEAG™), of Zurich Switzerland. All the HAC measurements are taken within a shielded enclosure. The measurement uncertainty budget is given in Appendix 6. The list of calibrated equipment used for the measurements is shown below.

Table 2: Dosimetric System Equipment

Description	Serial Number	Cal Due Date
DAE3	SN378	7/8/2006
E-Field Probe ER3DV6R	SN2247	7/20/2006
H-Field Probe H3DV6	SN6074	7/8/2006
Planar Dipole 1880 MHz	P1880-003	

Table 3: Additional Test Equipment

Description	Serial Number	Cal Due Date
Signal Generator E4432B	GB38450359	2/22/2006
3db Attenuator	50579	12/27/2005
Power Supply 6632B	01N992	12/17/2005
Directional Coupler 778D	18610	03/24//2006
Power Meter E4416A	GB41293246	2/25/2006
Power Meter E4419B	GB39511086	03/22//2006
Power Sensor #1 – E9301A	US39211013	12/28/2005
Power Sensor #2 - E9323A	US40412053	2/18/2006

4. System Accuracy Verification

A system accuracy verification of the DASY4 v4.5 test system was performed using the measurement equipment listed in Section 3.1. The weekly system accuracy verification occurs in free space. Note that the 1cm probe to dipole separation is measured from the top edge of the dipole to the calibration reference point of the probe.

Measurements were performed to see if the measured E-field and H-field values were within +/- 25% from the Planar Dipole target values indicated in ANSI PC63.19-2001 RD 3.6. These tests were done at 835 MHz and/or 1880 MHz. These frequencies are within each operating band and are within 2MHz of the mid-band frequency of the test device. The obtained results from the system accuracy verification are displayed in the table below. The Field contour plots are included in Appendix 1.

Table 4: Dipole Measurement Summary

F (MHz)	Input Power (W)	Input Power (mW)	E-Field Results (V/m)	C63.19 Target (V/m)	% Deviation
1880	CW Measured, 8/15/2005	100	135.8	153.6	-11.6

F (MHz)	Input Power (W)	Input Power (mW)	H-Field Results (A/m)	C63.19 Target (A/m)	% Deviation
1880	CW Measured, 8/15/2005	100	0.405	0.4478	-9.6

5. Probe Modulation Factor

After every probe calibration, the modulated signal (CDMA, GSM, etc) and CW are performed at 835 MHz and 1880 MHz. The response of the probe system to a CW field at the frequency(s) of interest is compared to its response to a modulated signal with equal peak amplitude. Probe modulation factor (PMF) refers to the ratio of the CW signal measurement to the modulated signal measurement. For GSM, the PMF can be seen to be implemented in the DASY4 scans in Appendix 2 via the Crest Factor setting (Crest Factor = PMF^2). Due to limitations in the current DASY4 crest factor setting (setting can not be less than unity), for CDMA the PMF is applied later to the appropriate phone's measurements in Section 6.1 via the formula Peak Field = $20 * \log(Raw * PMF)$.

RF Field Probe Modulation Response was measured with the field probe and associated measurement equipment. The PMF was measured per ANSI PC63.19-2001 RD 3.6 using signal generator as follows:

1. Illuminate a dipole with a CW signal at the intended measurement frequency.
2. The probe was fixed at a set location relative to the dipole; located at the interpolated maximum of an area scan.
3. Record the reading of the probe measurement system of the CW signal.
4. Substitute a modulated signal of the same amplitude, using the same modulation as that used by the intended WD for the CW signal.
5. Record the reading of the probe measurement system of the modulated signal.
6. The ratio of the CW to modulated signal reading is the probe modulation factor.

Table 5: PMF Measurement Summary

f (MHz)	Protocol	Peak Power (mW)	E-Field Probe SN 2247		H-Field Probe SN 6074	
			E-Field (V/m)	E-Field Modulation Factor	H-Field (A/m)	H-Field Modulation Factor
1880	CW	100	145.7	3.05	0.4419	2.96
	GSM	100	47.7		0.1495	

6. Test Results

The phone was tested in all normal configurations for the ear use. When applicable, each configuration is tested with the antenna in its fully extended and fully retracted positions. These test configurations are tested at the high, middle and low frequency channels of each applicable operating mode; for example, GSM, CDMA, and TDMA.

The DASY4 v4.5 measurement system specified in section 3.1 was utilized within the intended operations as set by the SPEAG™ setup. The default settings for the grid spacing of the scan were set to 5mm as shown in the Field plots included in Appendix 2 and 3.

The 5cm x 5cm area measurement grid is centered on the acoustic output of the device. The WD reference plane is parallel to the device and contains the highest point on its contour in the area of the phone that normally rests against the user's ear. The device is positioned such that the WD reference plane is located 10mm from, and parallel to, the measurement plane. The measurement plane contains the nearest point on the probe element relative to the WD. The following figure shows the orientation of the measurement grid with respect to the device under test.



Figure 1: Orientation of Wireless Device and Measurement Plane

The E-Field and H-Field maximum values are shown in tables 6 and 7. Also shown are the measured conducted output powers, the measured drift, excluded area, and the measured field strength. PMF measurement is taken from Section 5. Per Section 5, for GSM phones the PMF can be seen to be implemented in the DASY4 scans in Appendix 2 via the Crest Factor setting (Crest Factor = PMF^2). Due to limitations in the current DASY4 crest factor setting (setting can not be less than unity), for CDMA phones the PMF is applied later to the appropriate phone's measurements in Section 6.1 via the formula Peak Field = $20 * \log(Raw * PMF)$. The worst-case test conditions are indicated with **bold numbers** in the following table and are detailed in Appendix 2: HAC distribution plots for E-Field and H-Field.

**Table 6: HAC E-Field measurement results for the portable cellular telephone
FCC ID IHDT6FF1 at highest possible output power.**

Frequency Band (MHz)	Antenna position	Channel Setting	Conducted Output Power (dBm)	Excluded Cells	Peak Field (V/m)	Peak Field converted to (dB V/m)	FCC Limit (dB V/m)	Rating
GSM 1900MHz	Fixed	512	30.04	3,6,9	80.2	38.08	38.5	M3
		661	30.02	3,6,9	80.8	38.15	38.5	M3
		810	30.02	3,6,9	63.6	36.07	38.5	M3

**Table 7: HAC H-Field measurement results for the portable cellular telephone
FCC ID IHDT6FF1 at highest possible output power**

Frequency Band (MHz)	Antenna position	Channel Setting	Conducted Output Power (dBm)	Excluded Cells	Peak Field (A/m)	Peak Field converted to (dB A/m)	FCC Limit (dB A/m)	Rating
GSM 1900MHz	Fixed	512	30.04	6,8,9	0.221	-13.11	-11.9	M3
		661	30.02	6,8,9	0.219	-13.19	-11.9	M3
		810	30.02	6,8,9	0.182	-14.80	-14.4	M4

Appendix 1

HAC distribution plots for the system accuracy verification

Test Laboratory: Motorola

E-Field; CW 1880 MHz; -11.6% GOOD

DUT: Planar Dipole 1880 MHz;

Procedure Notes: 1880 MHz HAC Validation / Dipole Sn# P1880-003; Input Power = 100mW;

Communication System: CW mode; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air; Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³


DASY4 Configuration:

- Probe: ER3DV6R - SN2247; ConvF(1, 1, 1); Calibrated: 7/20/2005
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn378; Calibrated: 7/8/2005
- Phantom: HAC Phantom, Rev.3 (4-Aug-05); Type: Free Space; Serial: n/a;
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 147

HAC Main Procedure/E-Field PLANAR: 1880 HAC Validation (41x181x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of E_tot (interpolated) = 135.8 V/m

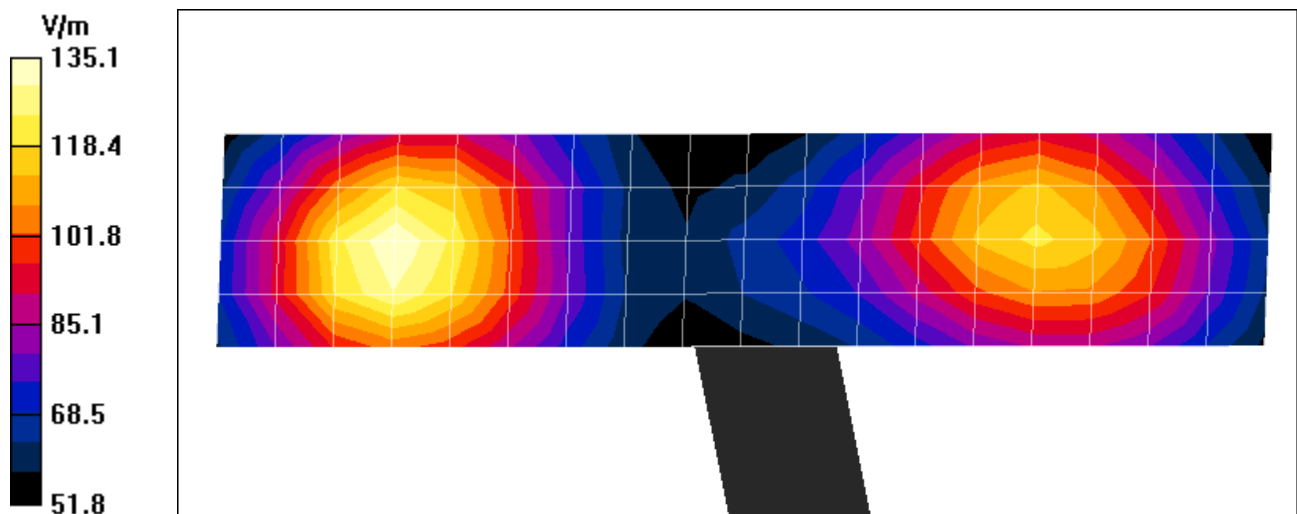

Test Laboratory: Motorola

H-Field; CW 1880 MHz; -9.6% GOOD

DUT: Planar Dipole 1880 MHz;

Procedure Notes: 1880 MHz HAC Validation / Dipole Sn# P1880-003; Input Power = 100 mW;

Communication System: CW mode; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air; Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³


DASY4 Configuration:

- Probe: H3DV6 - SN6074; ; Calibrated: 7/20/2005
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn378; Calibrated: 7/8/2005
- Phantom: HAC Phantom, Rev.3 (4-Aug-05); Type: Free Space; Serial: n/a;
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 147

HAC Main Procedure/H-Field PLANAR: 1880 HAC Validation (41x181x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of H_tot (interpolated) = 0.405 A/m

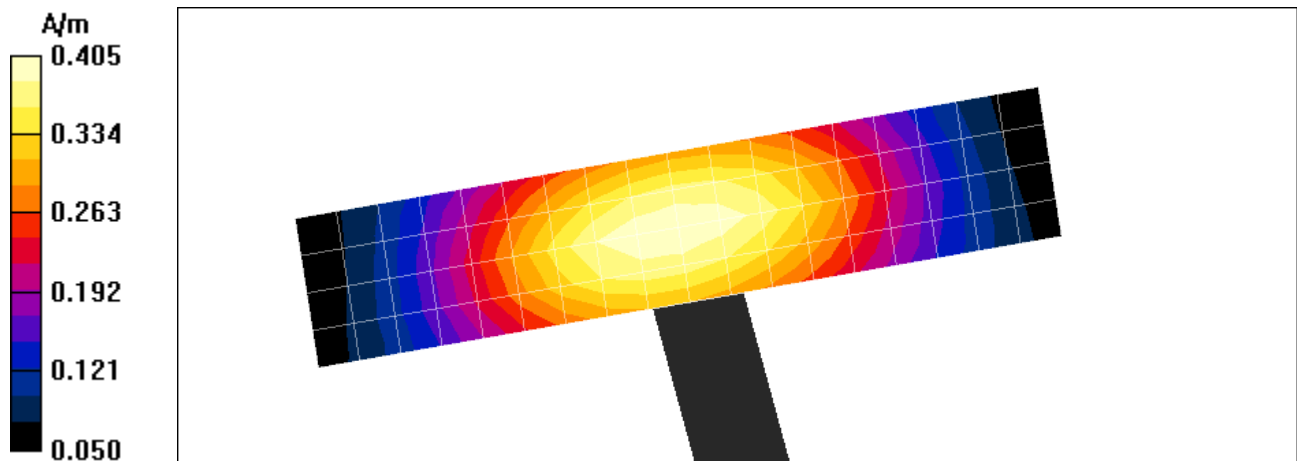

Appendix 2

HAC distribution plots for E-Field and H-Field

Date/Time: 8/18/2005 11:23:47 AM

Test Laboratory: Motorola**Serial: TA19100942**

Procedure Notes: Pwr Step: 00 (OTA) Antenna Position: INTERNAL Accessory Model #: N/A

Communication System: GSM 1900; Frequency: 1880 MHz;

Communication System Channel Number: 661; Duty Cycle: 1:9.33

Medium: Air; Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³

DASY4 Configuration:

- Probe: ER3DV6R - SN2247; ConvF(1, 1, 1); Calibrated: 7/20/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn378; Calibrated: 7/8/2005
- Phantom: HAC Phantom, Rev.3 (4-Aug-05); Type: Free Space; Serial: n/a;
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 147


Power Drift: 0.0745 dB

E in V/m (Time averaged)

Grid 1	Grid 2	Grid 3
23.6	26.5	24.7
Grid 4	Grid 5	Grid 6
22.0	25.5	25.6
Grid 7	Grid 8	Grid 9
20.2	20.2	28.3

E in V/m (Slot averaged)

Grid 1	Grid 2	Grid 3
72.2	80.8	75.5
Grid 4	Grid 5	Grid 6
67.3	77.9	78.1
Grid 7	Grid 8	Grid 9
61.7	61.8	86.3

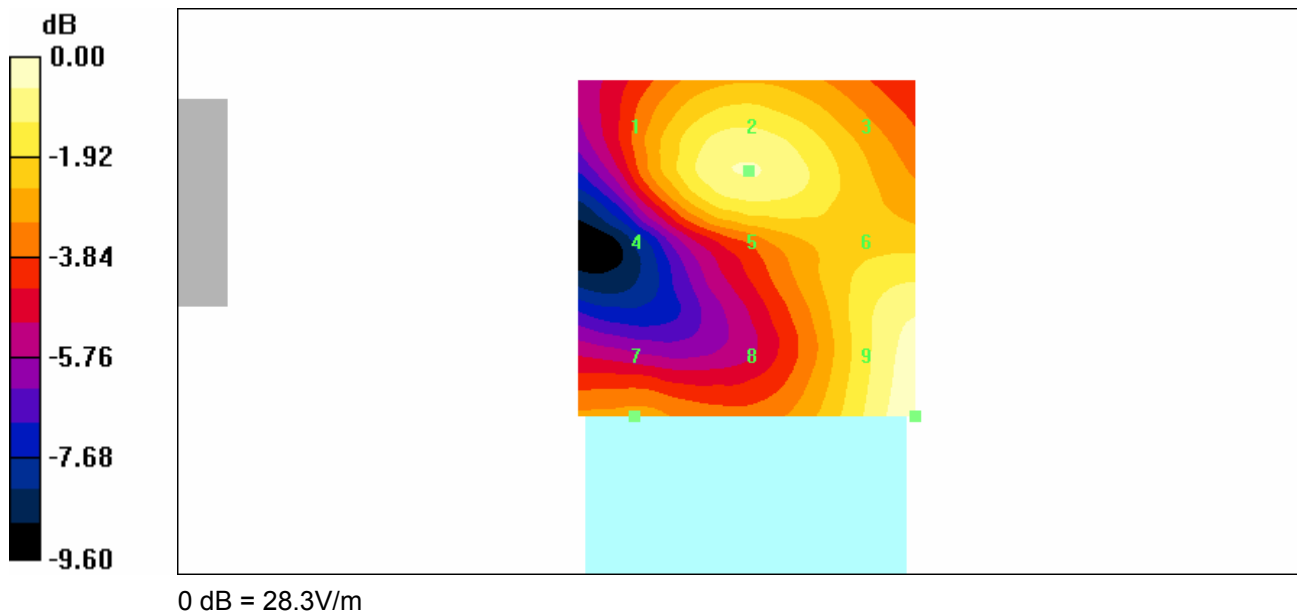

Date/Time: 8/18/2005 12:47:31 PM

Test Laboratory: Motorola

Serial: TA19100942

Procedure Notes: Pwr Step: 00 (OTA) Antenna Position: INTERNAL Accessory Model #: N/A;

Communication System: GSM 1900; Frequency: 1850.2 MHz;

Communication System Channel Number: 512; Duty Cycle: 1:8.74

Medium: Air; Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³

DASY4 Configuration:

- Probe: H3DV6 - SN6074; ; Calibrated: 7/20/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn378; Calibrated: 7/8/2005
- Phantom: HAC Phantom, Rev.3 (4-Aug-05); Type: Free Space; Serial: n/a;
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 147


Power Drift: -0.128 dB

H in A/m (Time averaged)

Grid 1 0.042	Grid 2 0.054	Grid 3 0.055
Grid 4 0.052	Grid 5 0.075	Grid 6 0.077
Grid 7 0.050	Grid 8 0.075	Grid 9 0.079

H in A/m (Slot averaged)

Grid 1 0.124	Grid 2 0.158	Grid 3 0.163
Grid 4 0.154	Grid 5 0.221	Grid 6 0.229
Grid 7 0.149	Grid 8 0.220	Grid 9 0.234

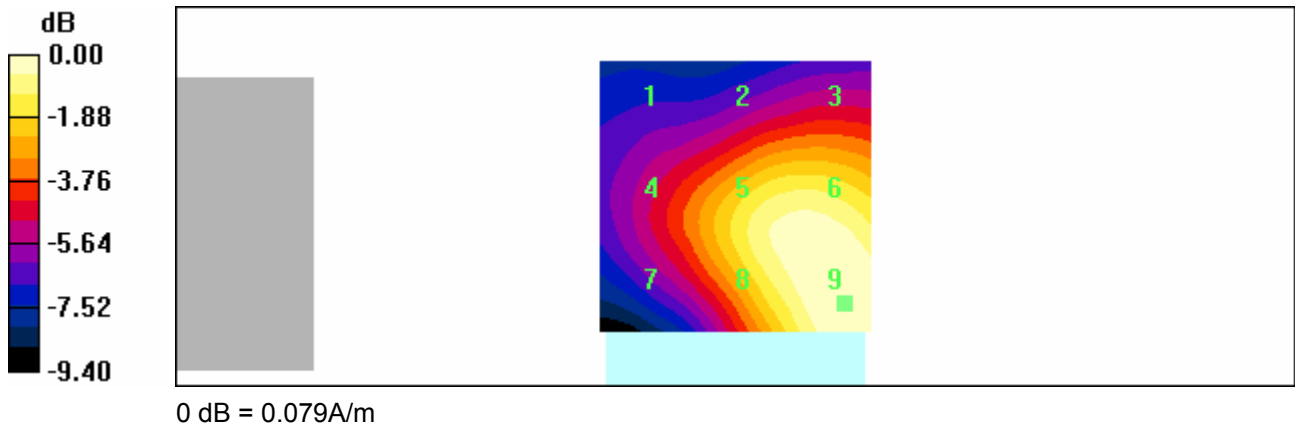

Appendix 3

Probe Calibration Certificate



Accredited by the Swiss Federal Office of Metrology and Accreditation
**The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 108**

Client **Motorola MDb**

Certificate No: **ER3-2247_Jul05**

CALIBRATION CERTIFICATE

Object **ER3DV6R - SN:2247**

Calibration procedure(s) **QA CAL-02.v4
Calibration procedure for E-field probes optimized for close near field
evaluations in air**

Calibration date: **July 20, 2005**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	3-May-05 (METAS, No. 251-00466)	May-06
Power sensor E4412A	MY41495277	3-May-05 (METAS, No. 251-00466)	May-06
Power sensor E4412A	MY41498087	3-May-05 (METAS, No. 251-00466)	May-06
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-05 (METAS, No. 251-00467)	May-06
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe ER3DV6	SN: 2328	6-Oct-04 (SPEAG, No. ER3-2328_Oct04)	Oct-05
DAE4	SN: 907	21-Jun-05 (SPEAG, No. DAE4-907_Jun05)	Jun-06

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov 05

Calibrated by: **Name** Nico Vetterli **Function** Laboratory Technician

Approved by: **Name** Katja Pokovic **Technical Manager**

Issued: July 20, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

NORM _{x,y,z}	sensitivity in free space
DCP	diode compression point
Polarization ϕ	ϕ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1309-1996, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", 1996.

Methods Applied and Interpretation of Parameters:

- *NORM_{x,y,z}*: Assessed for E-field polarization $\vartheta = 0$ for XY sensors and $\vartheta = 90$ for Z sensor ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide).
- *NORM(f)_{x,y,z}* = *NORM_{x,y,z}* * *frequency_response* (see Frequency Response Chart).
- *DCP_{x,y,z}*: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- *Spherical isotropy (3D deviation from isotropy)*: in a locally homogeneous field realized using an open waveguide setup.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the *NORM_x* (no uncertainty required).

Probe ER3DV6R

SN:2247

Manufactured:	February 1, 2000
Last calibrated:	March 6, 2000
Recalibrated:	July 20, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

DASY - Parameters of Probe: ER3DV6R SN:2247Sensitivity in Free Space [$\mu\text{V}/(\text{V}/\text{m})^2$]Diode Compression^ANormX **1.76 $\pm$ 10.1 % (k=2)**DCP X **97 mV**NormY **1.51 $\pm$ 10.1 % (k=2)**DCP Y **97 mV**NormZ **1.47 $\pm$ 10.1 % (k=2)**DCP Z **96 mV**

Frequency Correction

X **0.0**Y **0.0**Z **0.0**

Sensor Offset

(Probe Tip to Sensor Center)

X **2.5 mm**Y **2.5 mm**Z **2.5 mm**

Connector Angle


214 °

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.





^A numerical linearization parameter: uncertainty not required

Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide R22)

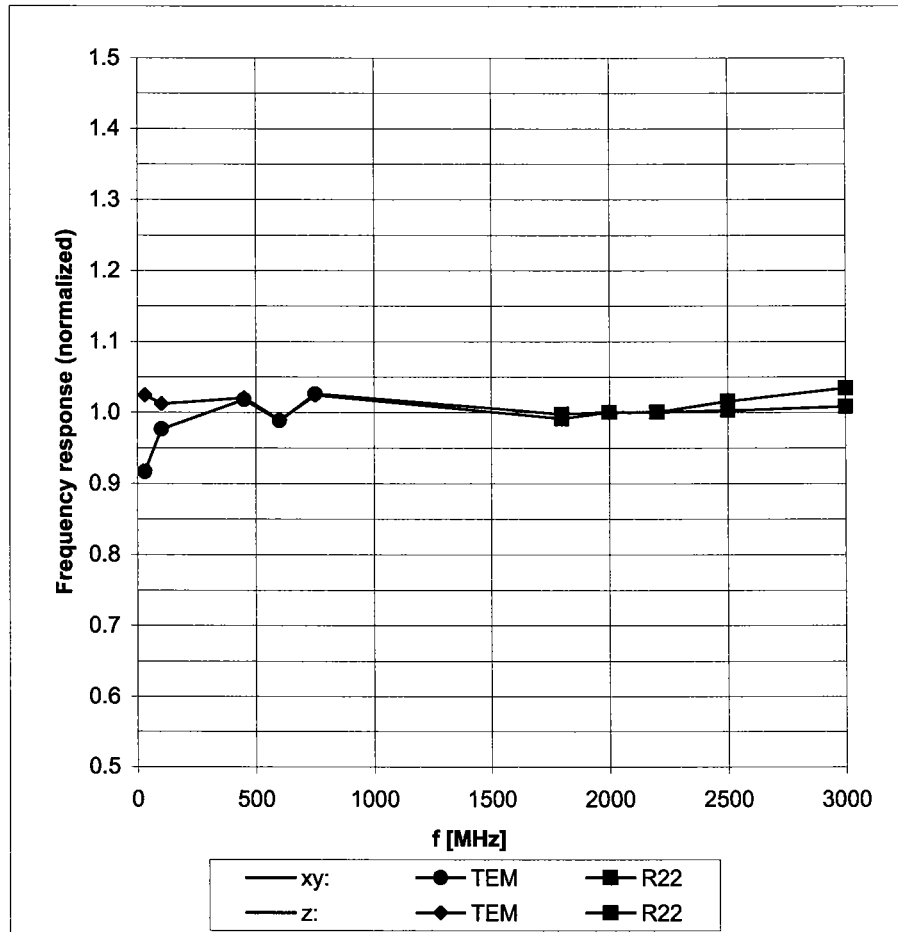

Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

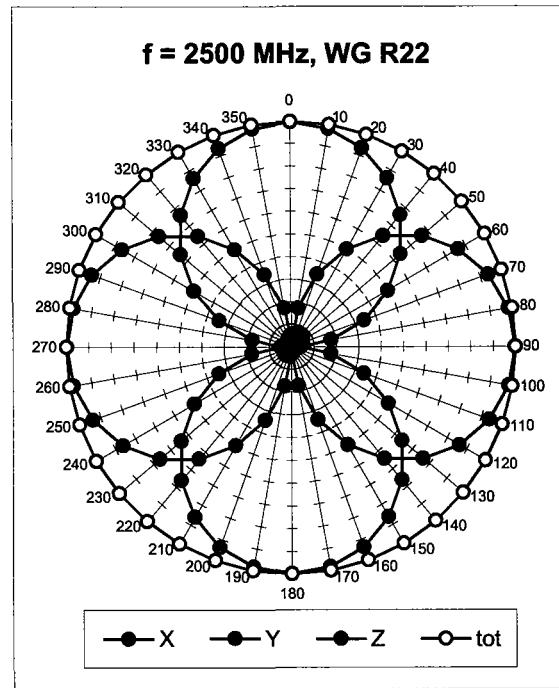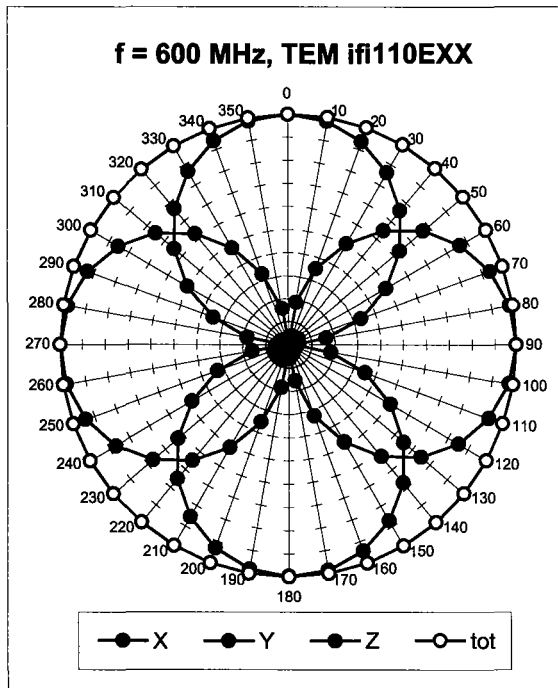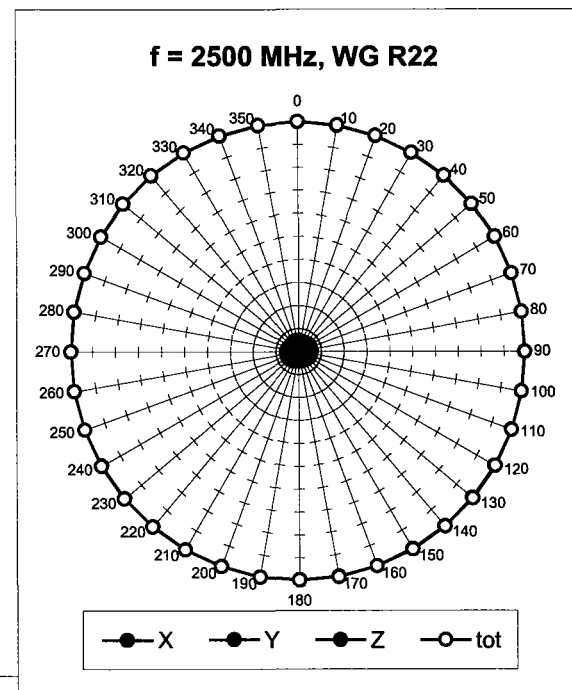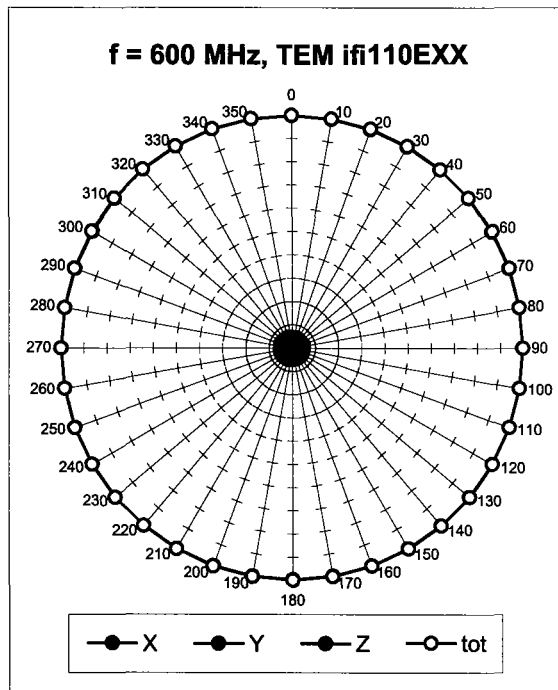
Receiving Pattern (ϕ), $\vartheta = 0^\circ$ Receiving Pattern (ϕ), $\vartheta = 90^\circ$ 

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

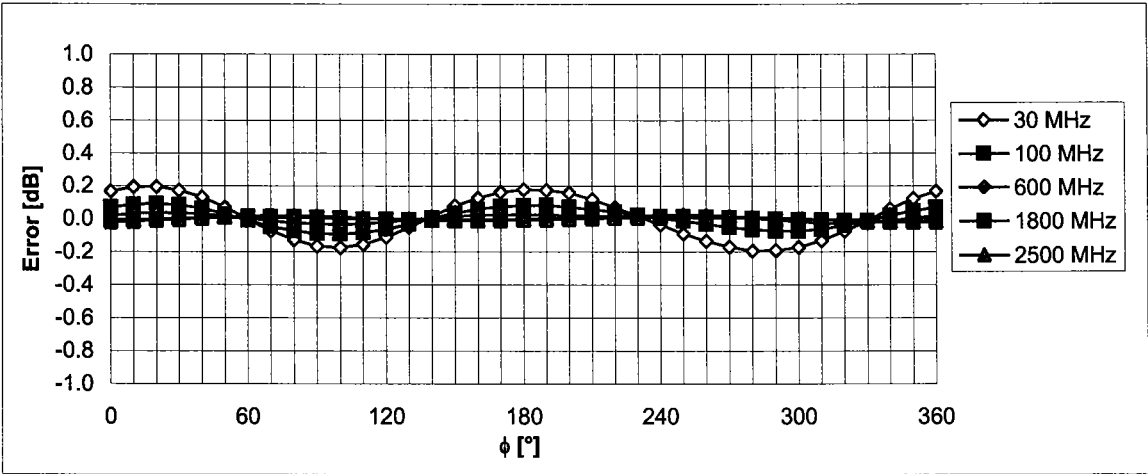

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)



Receiving Pattern (ϕ), $\vartheta = 90^\circ$

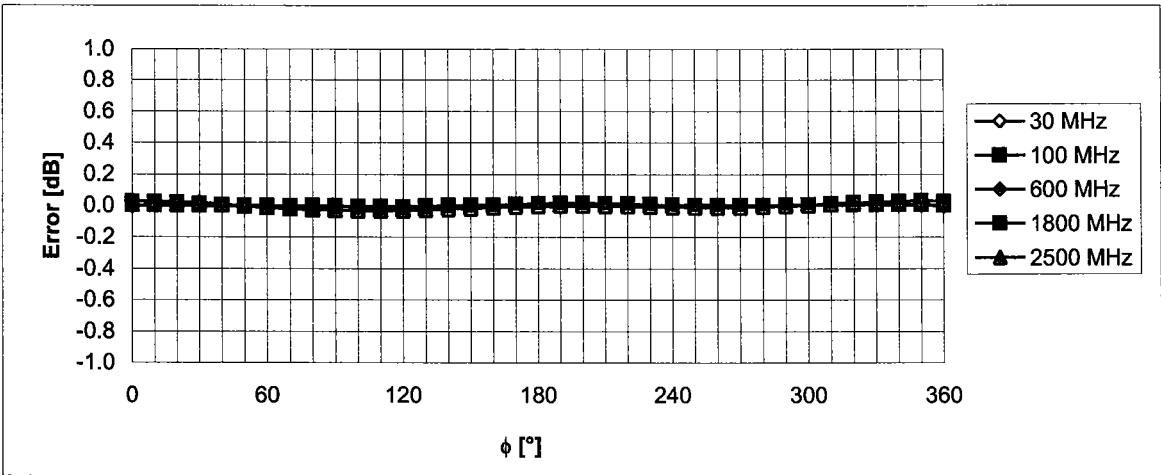

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

Dynamic Range f(E-field)

(Waveguide R22, $f = 1800$ MHz)

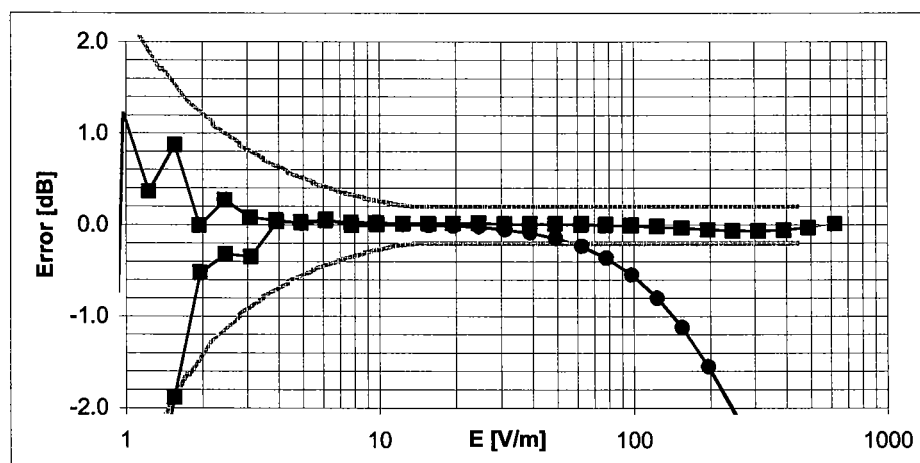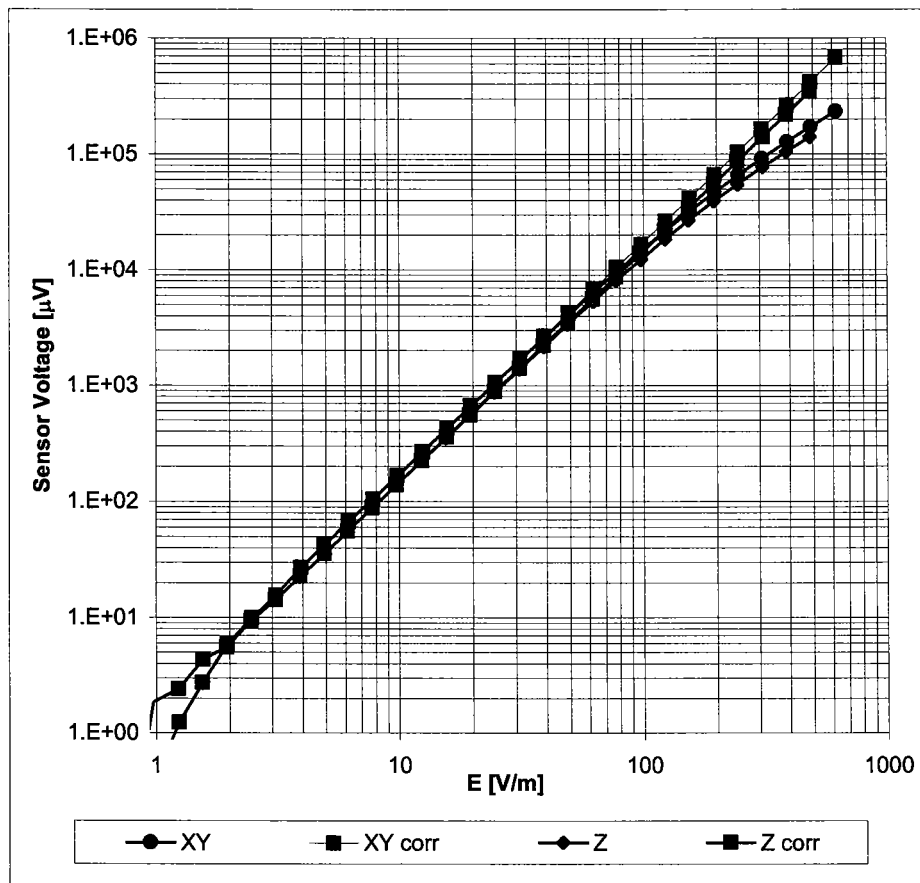

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)



Accredited by the Swiss Federal Office of Metrology and Accreditation
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Motorola MDB**

Certificate No: **H3-6074_Jul05**

CALIBRATION CERTIFICATE

Object **H3DV6 - SN:6074**

Calibration procedure(s) **QA CAL-03.v4**
Calibration procedure for H-field probes optimized for close near field evaluations in air

Calibration date: **July 20, 2005**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	3-May-05 (METAS, No. 251-00466)	May-06
Power sensor E4412A	MY41495277	3-May-05 (METAS, No. 251-00466)	May-06
Power sensor E4412A	MY41498087	3-May-05 (METAS, No. 251-00466)	May-06
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-05 (METAS, No. 251-00467)	May-06
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe H3DV6	SN: 6182	6-Oct-04 (SPEAG, No. H3-6182_Oct04)	Oct-05
DAE4	SN: 907	21-Jun-05 (SPEAG, No. DAE4-907_Jun05)	Jun-06

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov 05

Calibrated by: **Nico Vetterli** **Laboratory Technician**

Approved by: **Katja Pokovic** **Technical Manager**

Issued: July 20, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

NORM _{x,y,z}	sensitivity in free space
DCP	diode compression point
Polarization ϕ	ϕ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1309-1996, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", 1996.

Methods Applied and Interpretation of Parameters:

- X, Y, Z_{a0a1a2} : Assessed for E-field polarization $\vartheta = 90$ for XY sensors and $\vartheta = 0$ for Z sensor ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide).
- $X, Y, Z(f)_{a0a1a2} = X, Y, Z_{a0a1a2} \cdot \text{frequency_response}$ (see Frequency Response Chart).
- $DCP_{x,y,z}$: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- *Spherical isotropy (3D deviation from isotropy)*: in a locally homogeneous field realized using an open waveguide setup.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the X_{a0a1a2} (no uncertainty required).

Probe H3DV6

SN:6074

Manufactured:	October 2, 2000
Last calibrated:	September 18, 2003
Recalibrated:	July 20, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

DASY - Parameters of Probe: H3DV6 SN:6074Sensitivity in Free Space [A/m / $\sqrt{(\mu\text{V})}$]

	a0	a1	a2
X	2.732E-03	-1.128E-4	2.808E-5 $\pm$ 5.1 % (k=2)
Y	2.654E-03	-8.281E-5	-6.750E-5 $\pm$ 5.1 % (k=2)
Z	3.180E-03	-2.987E-4	-2.131E-5 $\pm$ 5.1 % (k=2)

Diode Compression¹

DCP X	86 mV
DCP Y	86 mV
DCP Z	86 mV

Sensor Offset (Probe Tip to Sensor Center)

X	3.0 mm
Y	3.0 mm
Z	3.0 mm


Connector Angle 190 °

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.





¹ numerical linearization parameter: uncertainty not required


Frequency Response of H-Field

(TEM-Cell:ifi110, Waveguide R22)

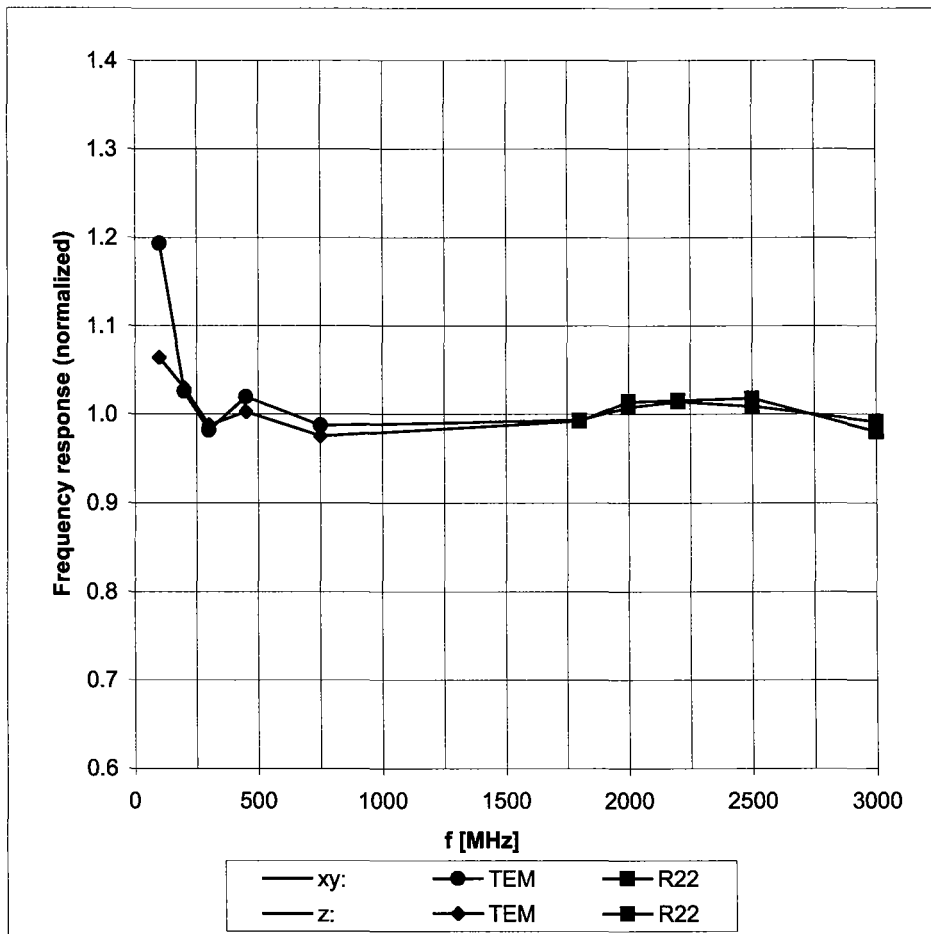


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

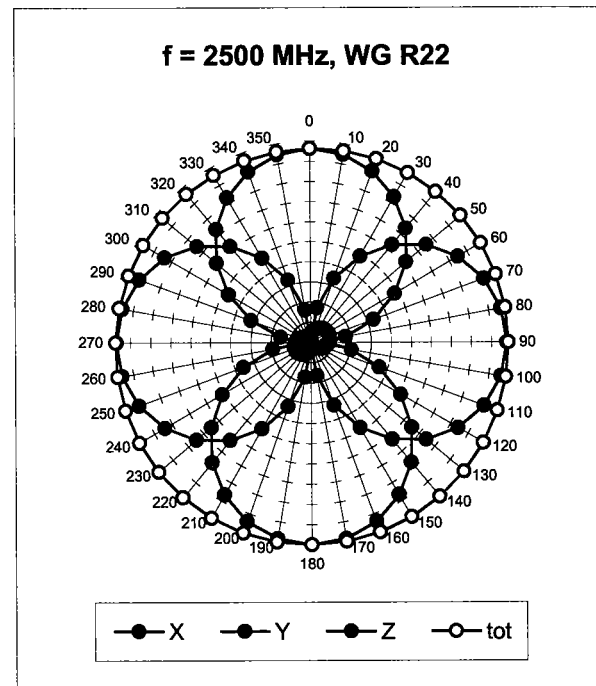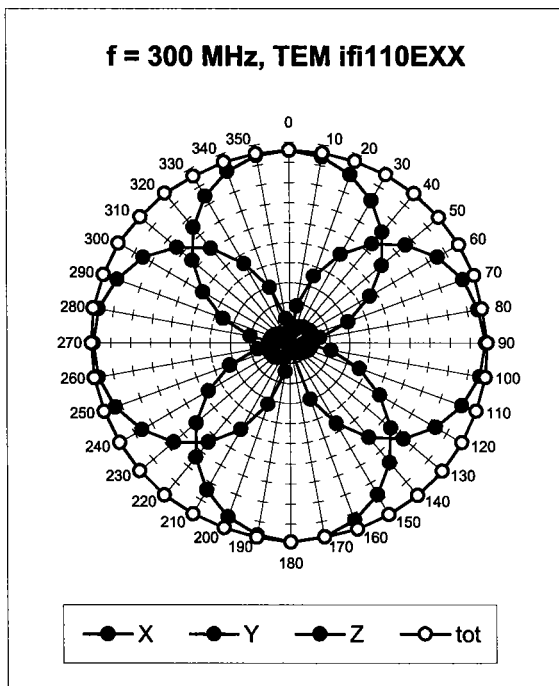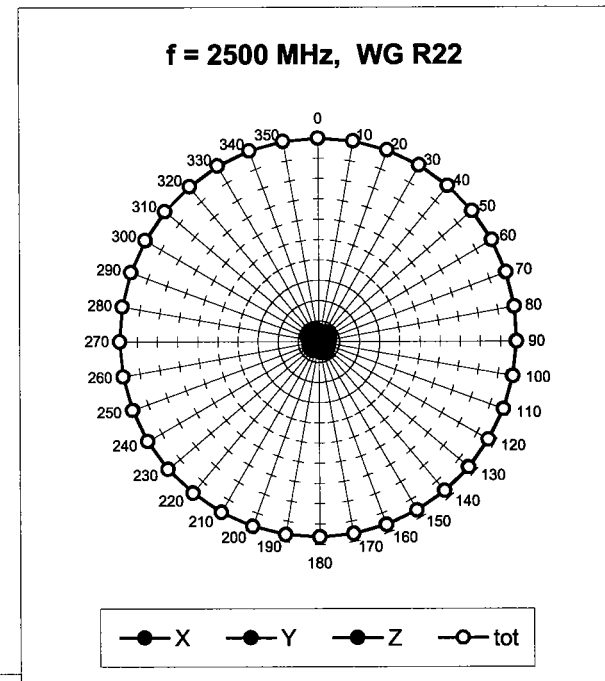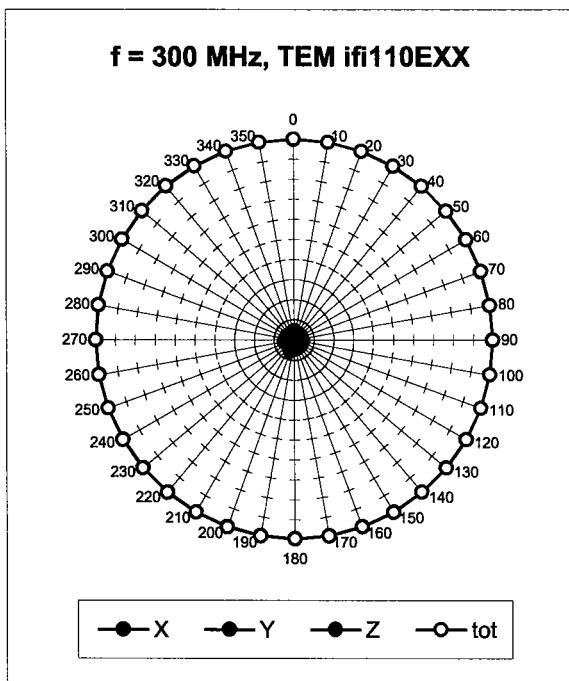Receiving Pattern (ϕ), $\vartheta = 90^\circ$ **Receiving Pattern (ϕ), $\vartheta = 0^\circ$** 

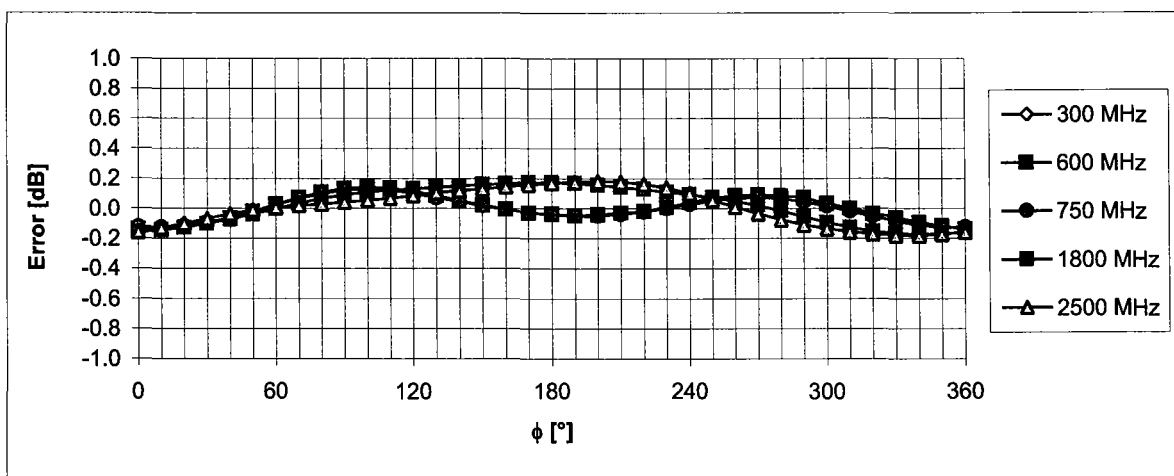Receiving Pattern (ϕ), $\vartheta = 90^\circ$ 



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

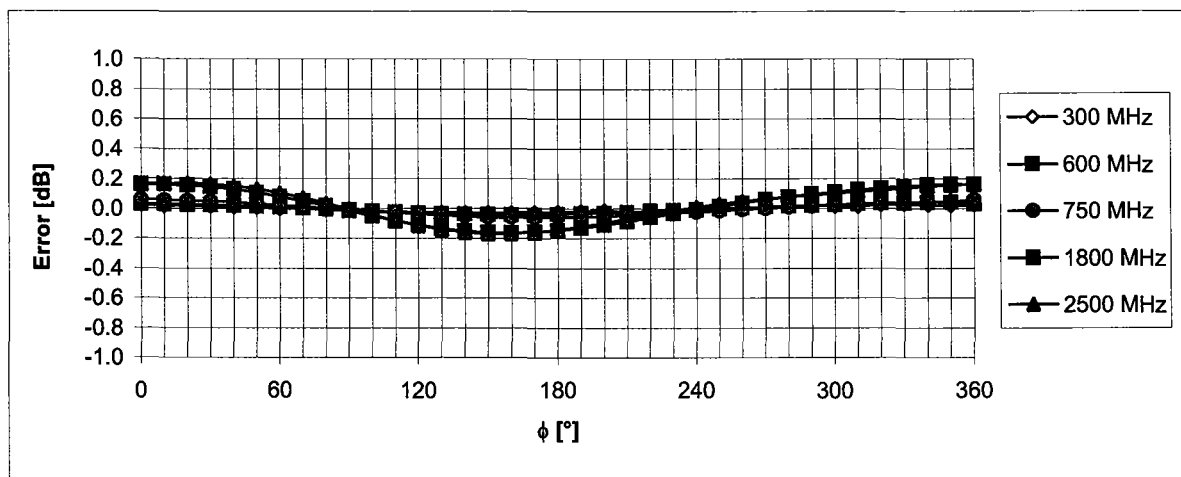Receiving Pattern (ϕ), $\vartheta = 0^\circ$ 

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

Dynamic Range f(H-field)

(Waveguide R22, $f = 1800$ MHz)

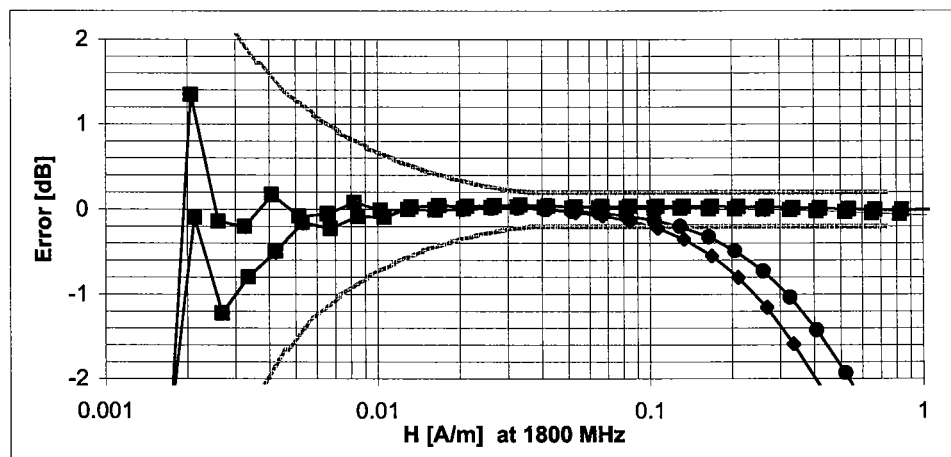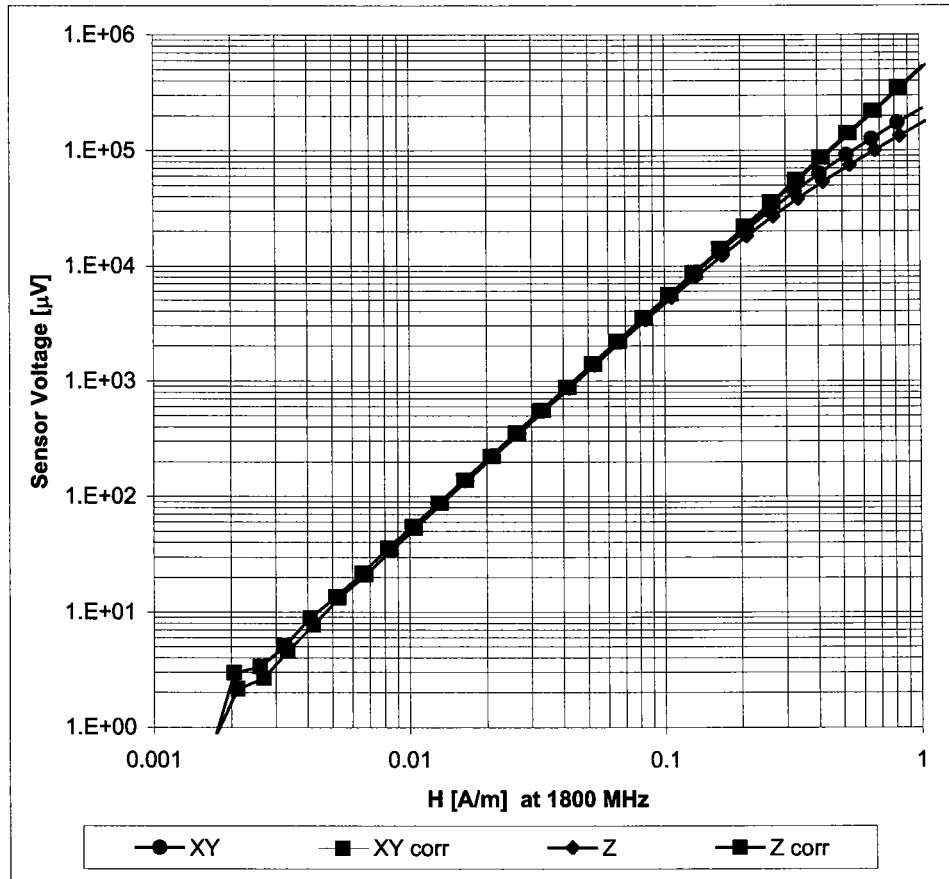

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Appendix 4

Measurement Uncertainty Budget

A4.1 Motorola Uncertainty Budget for RF HAC Testing

TABLE A4.1: Motorola Uncertainty Budget

UNCERTAINTY DESCRIPTION	Uncertainty Value (+/- %)	Prob. Dist.	Div.	(ci) E	(ci) H	Std. Unc. E	Std. Unc. H	Source
MEASUREMENT SYSTEM								
Probe Calibration	5.1%	N	1.0000	1	1	5.1%	5.1%	SPEAG HAC Extension Application Note (April 2005)
Axial Isotropy	7.8%	R	1.7321	1	0.786	4.5%	3.5%	Motorola Evaluation
Sensor Displacement	16.5%	R	1.7321	1	0.145	9.5%	1.4%	SPEAG HAC Extension Application Note (April 2005)
Boundary Effects	2.4%	R	1.7321	1	1	1.4%	1.4%	SPEAG HAC Extension Application Note (April 2005)
Linearity	4.7%	R	1.7321	1	1	2.7%	2.7%	SPEAG HAC Extension Application Note (April 2005)
Scaling to Peak Envelope Power	2.0%	R	1.7321	1	1	1.2%	1.2%	SPEAG HAC Extension Application Note (April 2005)
System Detection Limit	1.0%	R	1.7321	1	1	0.6%	0.6%	SPEAG HAC Extension Application Note (April 2005)
Readout Electronics	0.3%	N	1.0000	1	1	0.3%	0.3%	SPEAG HAC Extension Application Note (April 2005)
Response Time	0.8%	R	1.7321	1	1	0.5%	0.5%	SPEAG HAC Extension Application Note (April 2005)
Integration Time	2.6%	R	1.7321	1	1	1.5%	1.5%	SPEAG HAC Extension Application Note (April 2005)
RF Reflections	5.6%	R	1.7321	1	1	3.2%	3.2%	Motorola Evaluation
Probe Positioner	1.2%	R	1.7321	1	0.67	0.7%	0.5%	SPEAG HAC Extension Application Note (April 2005)
Probe Positioning	4.7%	R	1.7321	1	0.67	2.7%	1.8%	SPEAG HAC Extension Application Note (April 2005)
Extrap. & Interpolation	1.0%	R	1.7321	1	1	0.6%	0.6%	SPEAG HAC Extension Application Note (April 2005)
TEST SAMPLE RELATED								
Total Device Positioning	3.2%	R	1.7321	1	1.306	1.8%	2.4%	Motorola Evaluation
Device Holder & Phantom	2.4%	R	1.7321	1	1	1.4%	1.4%	SPEAG HAC Extension Application Note (April 2005)
Power Drift	5.0%	R	1.7321	1	1	2.9%	2.9%	SPEAG HAC Extension Application Note (April 2005)
PHANTOM AND SETUP RELATED								
Phantom Thickness	0.0%	R	1.7321	1	0.67	0.0%	0.0%	SPEAG HAC Extension Application Note (April 2005)
Combined Std.Uncertainty						13.5%	9.2%	
Expanded Std. Uncertainty on Power						27.0%	18.3%	

A4.2 Probe Rotation Contributions to Isotropy Error

Probe is rotated for maximum reading at the interpolated maximum location. Thirteen mobile devices were used to determine the probe isotropy uncertainty factors in section A4.1. Based on the resulting 82 E-Field probe rotations and 82 H-Field probe rotations, the upper 95% confidence interval value was calculated for each. These values represent a conservative assessment of the effect of the probe isotropy and have been appropriately included in the respective E- and H- uncertainty budgets.

TABLE A4.2: Probe Rotation Data Summary

	AVE	ST.DEV	Sample Size (n)	2 σ	(ci)	Standard Uncertainty
E-field	4.4%	1.7%	82	7.8%	1	4.5%
H-field	3.8%	1.2%	82	6.1%	0.786	3.5%

Isotropy error measurements were taken for 13 products across the respective frequency bands. The +2 σ values of all measurements was used as a worst case value for the uncertainty budget. Any significant differences between bands was also evaluated.