

Appendix C: System Check Plots

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
CLA-13 – SN1041	24.5	Flat	0	CW, 0	13.000	14.3, 16.56,15.27

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	22.8	23.4	16.4.0.5005	ELI V8.0 – 2216	Head Simulating Liquid	0.752	52.9	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 36.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.137	6.37
psSAR10g	0.084	0.69
Peak SAR (Extrapolated)	0.287	8.07
psAPD (4.0 cm², sq)	N/A	N/A

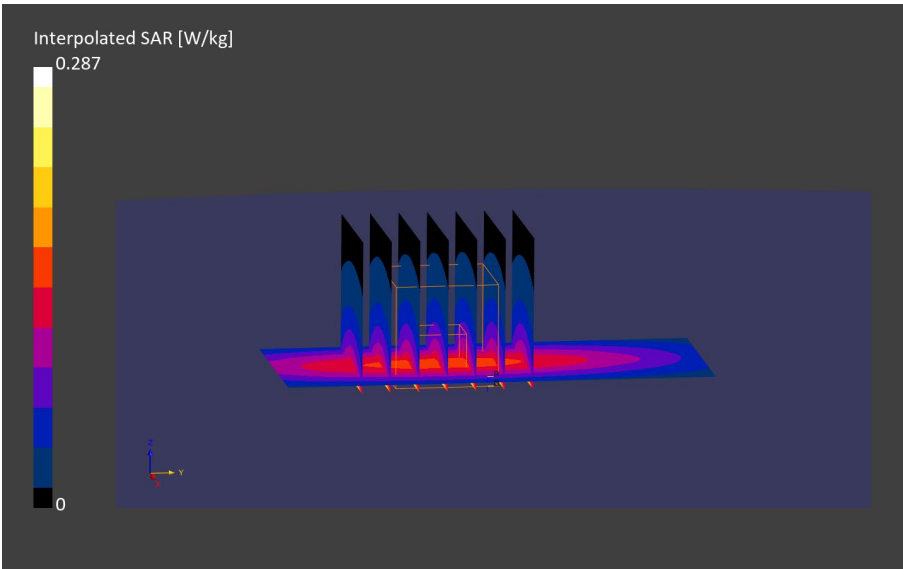

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.62, 9.46,9.15

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-24	20.6	20.3	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	0.836	43.4	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.403	-7.47
psSAR10g	0.267	-6.37
Peak SAR (Extrapolated)	0.562	-11
psAPD (4.0 cm², sq)	N/A	N/A

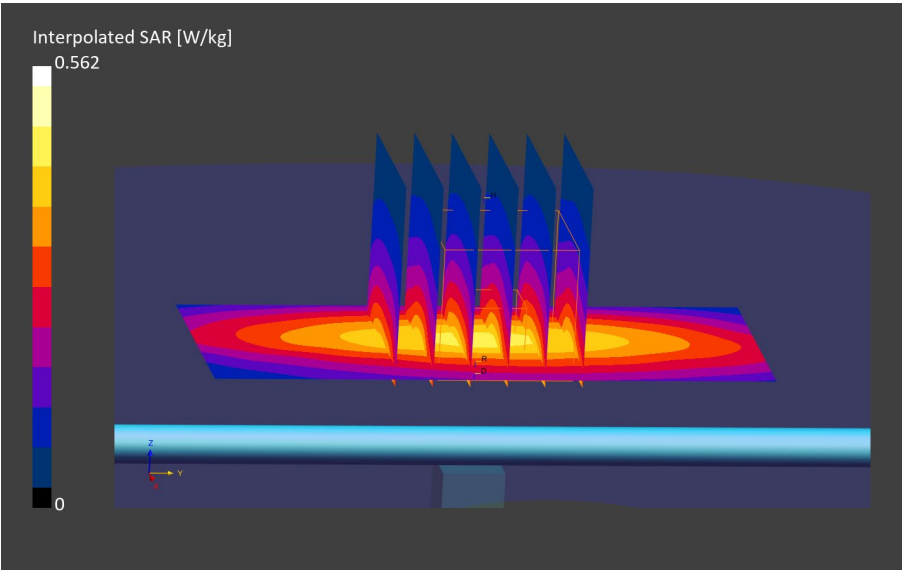

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1640V2 – SN356	17.0	Flat	10	CW, 0	1640.000	7.94, 7.8, 7.55

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-05	20.8	20.6	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.24	41.5	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.66	-3.15
psSAR10g	0.903	-3.13
Peak SAR (Extrapolated)	2.74	-9.49
psAPD (4.0 cm², sq)	N/A	N/A

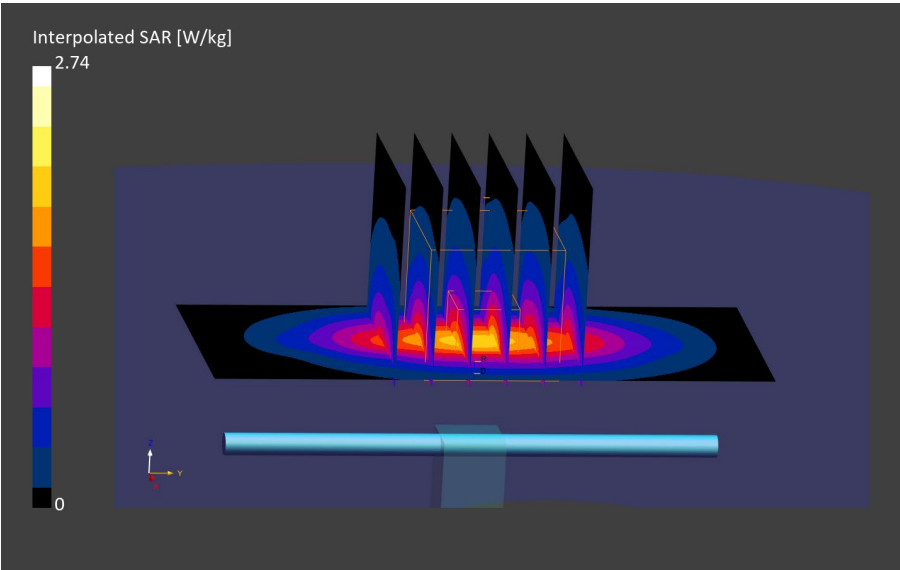

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.68, 7.4, 7.37

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	21.3	21.1	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.36	43.8	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.80	-1.6
psSAR10g	0.966	0.39
Peak SAR (Extrapolated)	3.06	-5.92
psAPD (4.0 cm², sq)	N/A	N/A

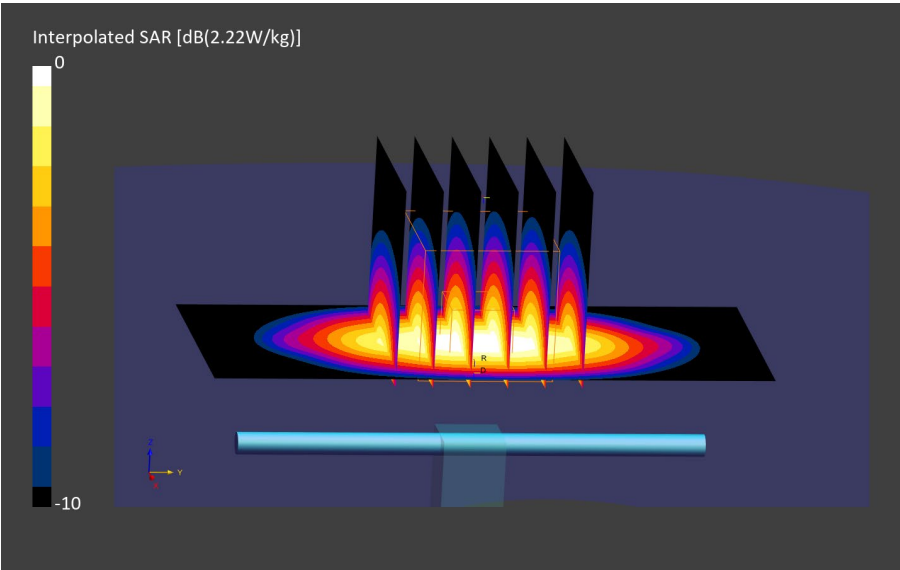

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.23, 6.96,6.94

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	21.3	21.1	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.45	43.5	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.02	1.27
psSAR10g	1.06	0.71
Peak SAR (Extrapolated)	3.58	-0.93
psAPD (4.0 cm², sq)	N/A	N/A

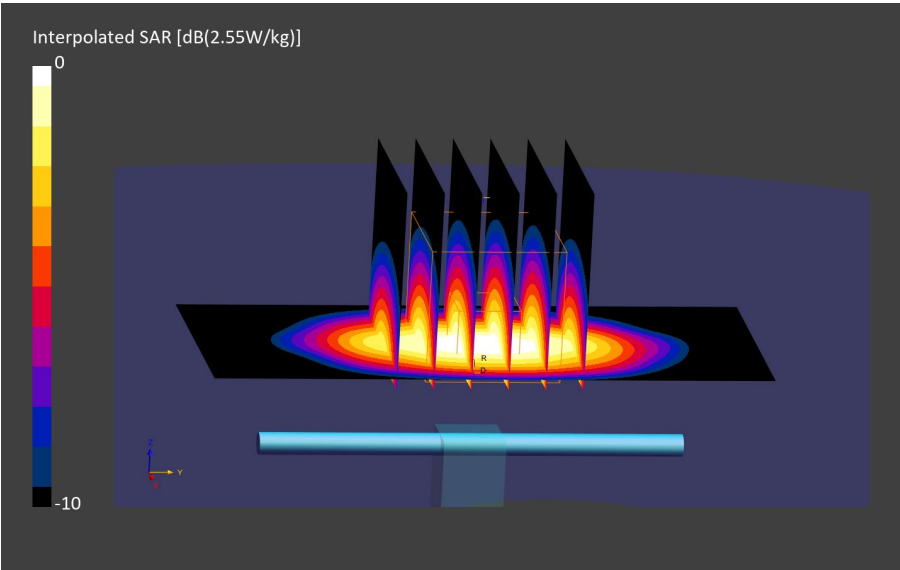

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.59, 7.46, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-05	20.8	20.6	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.40	41.1	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.90	-4.75
psSAR10g	1.00	-4.99
Peak SAR (Extrapolated)	3.28	-9.23
psAPD (4.0 cm², sq)	N/A	N/A

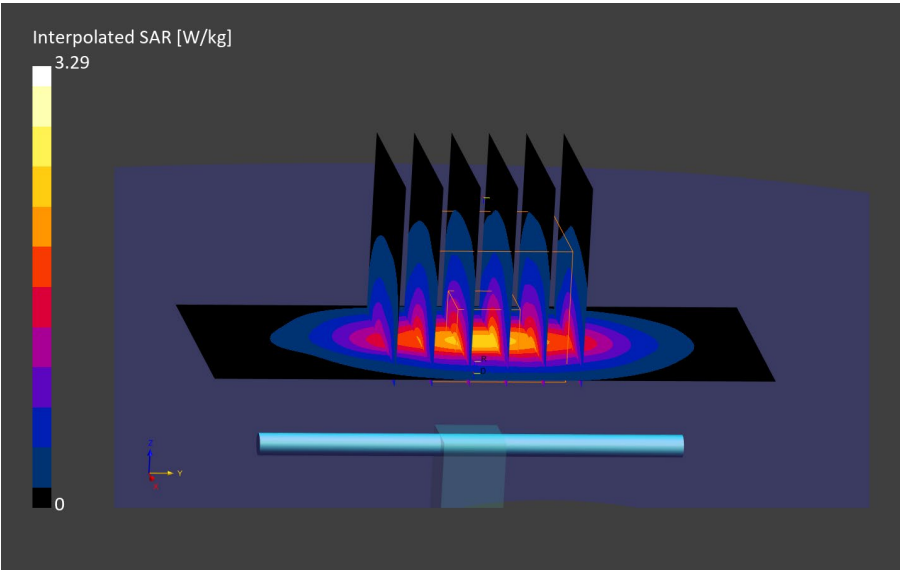

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.59, 7.46, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-22	22.3	21.6	18.0.0.7250	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.41	41.5	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.88	-5.75
psSAR10g	0.991	-5.84
Peak SAR (Extrapolated)	3.36	-7.02
psAPD (4.0 cm², sq)	N/A	N/A

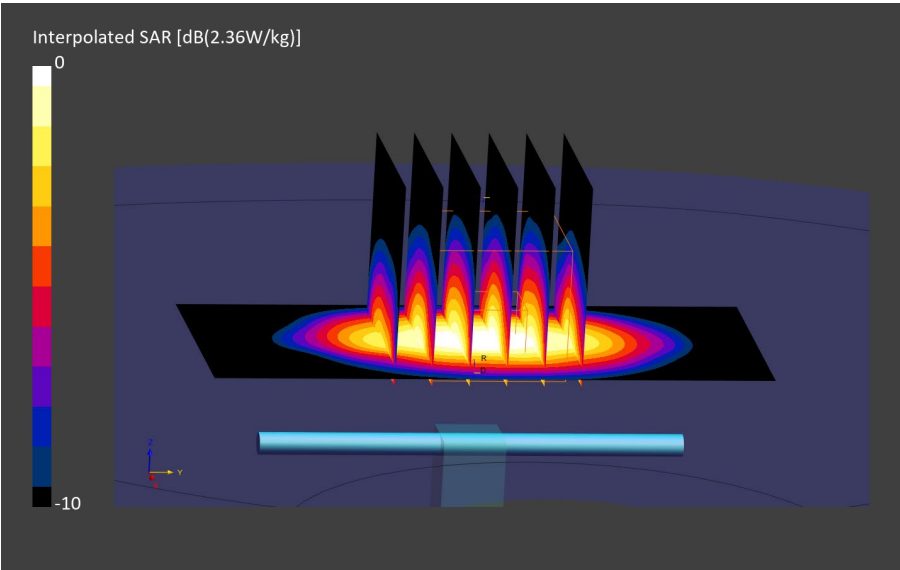

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2100V2 – SN1068	17.0	Flat	10	CW, 0	2100.000	7.46, 7.34, 7.1

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-05	20.8	20.6	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.53	40.8	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.04	-7.91
psSAR10g	1.04	-6.95
Peak SAR (Extrapolated)	3.78	-5.61
psAPD (4.0 cm², sq)	N/A	N/A

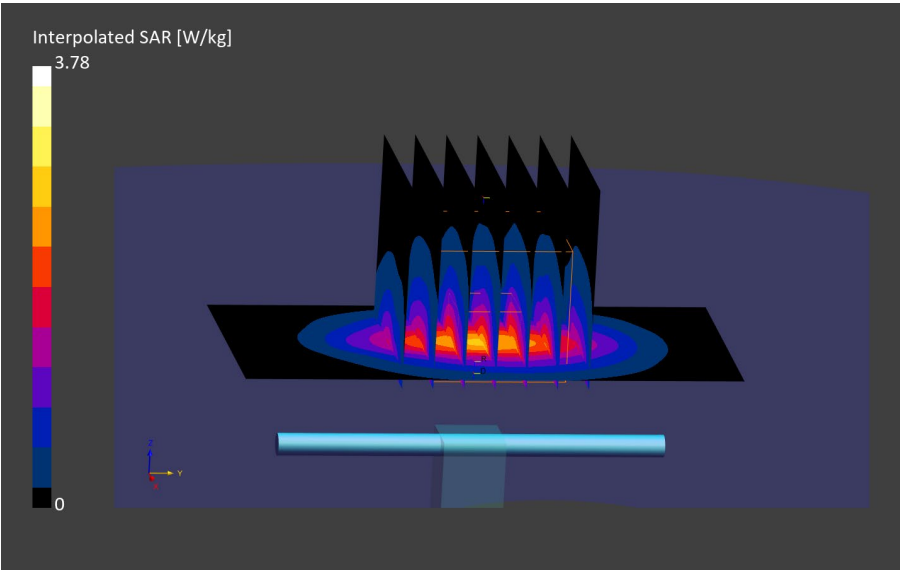

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	7.39, 7.44, 7.43

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-05-20	22.3	21.5	17.0.4.7034	Twin-SAM V8.0 – 2233	Head Simulating Liquid	1.86	42.2	EX3DV4 – SN7971, 2026-04-14	DAE4ip Sn1862, 2026-01-08

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.47	-2.6
psSAR10g	1.17	-1.5
Peak SAR (Extrapolated)	4.96	-5.02
psAPD (4.0 cm², sq)	N/A	N/A

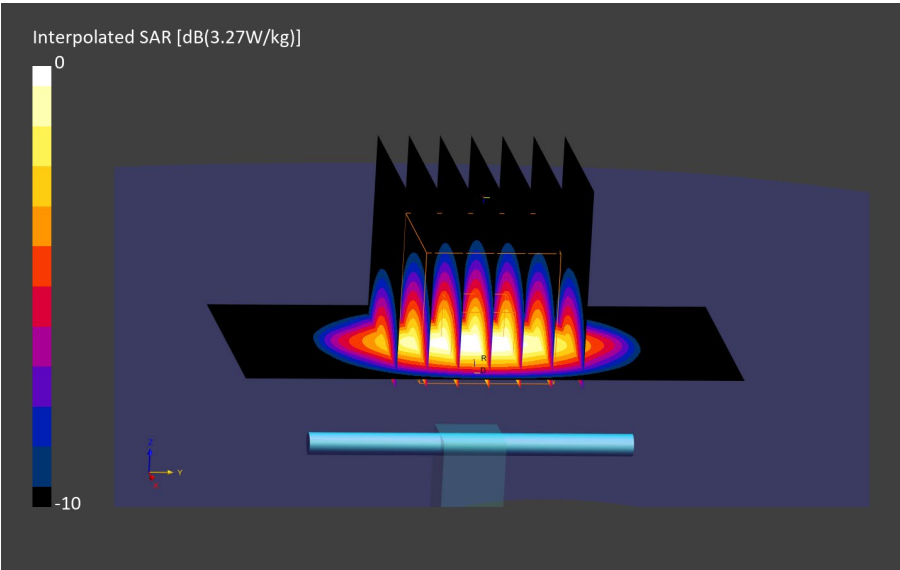

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.94, 6.68, 6.66

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-22	22.1	21.8	18.0.0.7250	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.84	41.7	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.49	-1.81
psSAR10g	1.18	-0.66
Peak SAR (Extrapolated)	4.96	-5.02
psAPD (4.0 cm², sq)	N/A	N/A

