

Appendix C: System Check Plots

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
CLA-13 – SN1041	24.5	Flat	0	CW, 0	13.000	14.3, 16.56,15.27

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-17	23.4	23.8	16.4.0.5005	ELI V8.0 – 2216	Head Simulating Liquid	0.765	51.5	EX3DV4 – SN7872, 2025-08-08	DAE4ip Sn1843, 2025-07-30

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.140	8.7
psSAR10g	0.085	1.89
Peak SAR (Extrapolated)	0.292	9.98
psAPD (4.0 cm², sq)	N/A	N/A

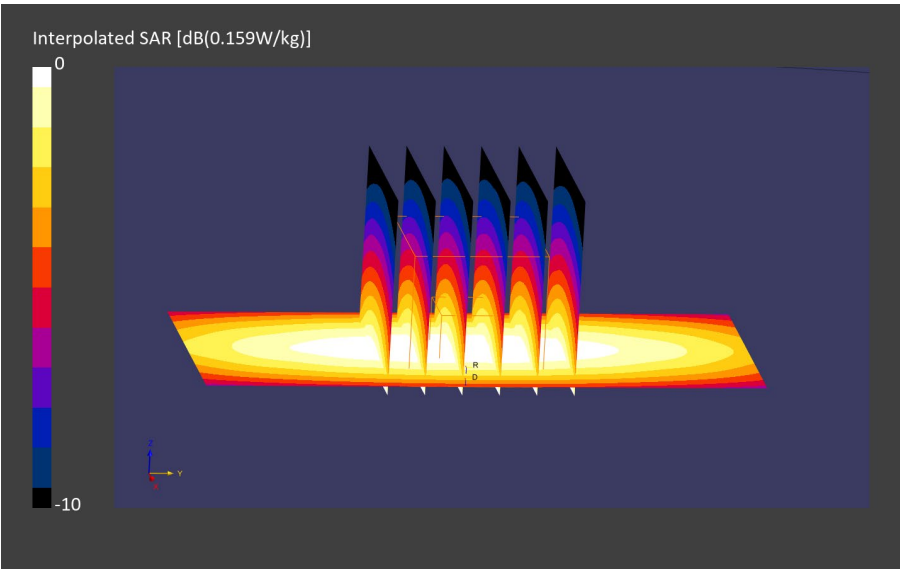

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D750V3 – SN1235	17.0	Flat	15	CW, 0	750.000	9.62, 9.46, 9.15

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-04-29	23.7	22.1	17.0.4.7034	Twin-SAM V8.0 – 2238	Head Simulating Liquid	0.891	41.7	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	0.408	-6.32
psSAR10g	0.273	-4.27
Peak SAR (Extrapolated)	0.601	-4.83
psAPD (4.0 cm², sq)	N/A	N/A

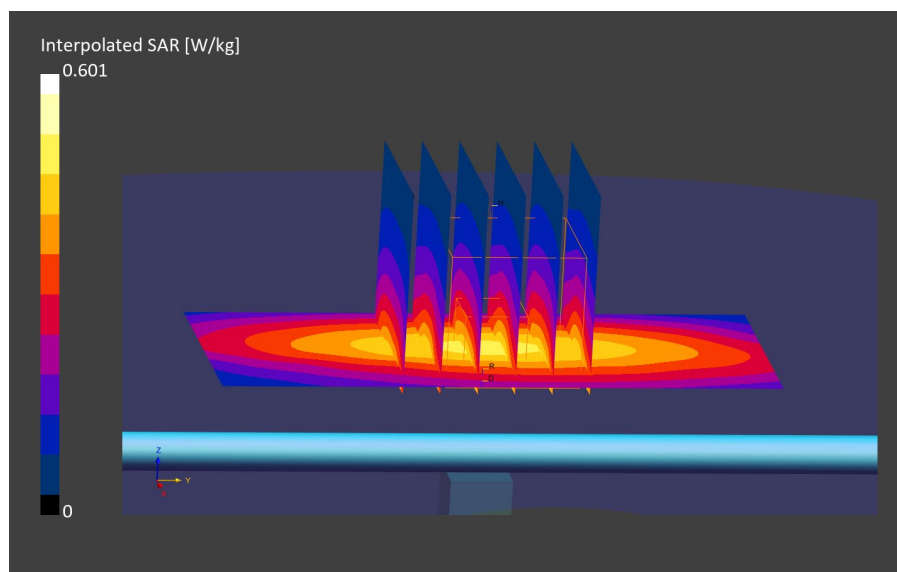

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1640V2 – SN356	17.0	Flat	10	CW, 0	1640.000	7.94, 7.8, 7.55

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-10	20.6	20.6	18.0.0.7250	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.26	41.1	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.62	-5.49
psSAR10g	0.889	-4.64
Peak SAR (Extrapolated)	2.71	-10.48
psAPD (4.0 cm², sq)	N/A	N/A

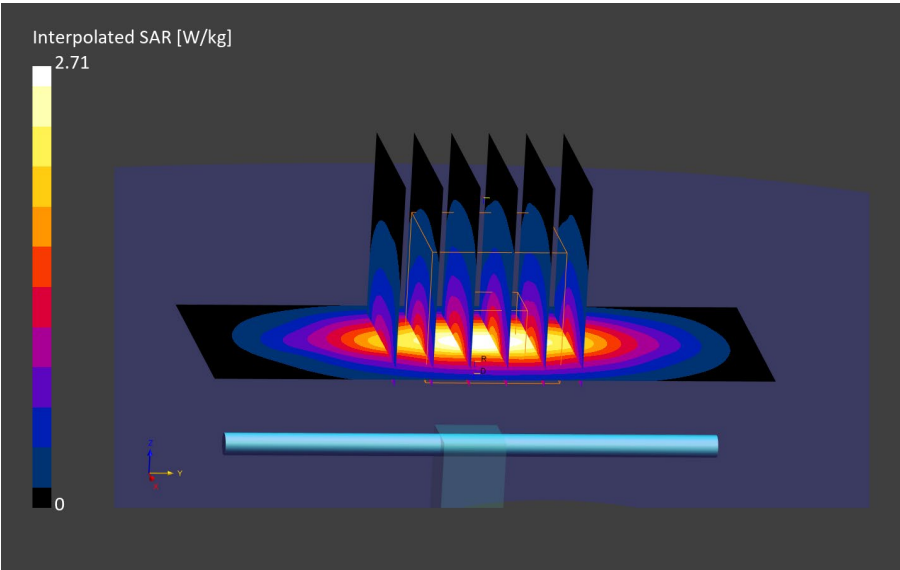

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1750V2 – SN1205	17.0	Flat	10	CW, 0	1750.000	7.68, 7.4, 7.37

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-04-29	23.5	23	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.34	41.2	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.78	-2.7
psSAR10g	0.950	-1.28
Peak SAR (Extrapolated)	3.23	-0.7
psAPD (4.0 cm², sq)	N/A	N/A

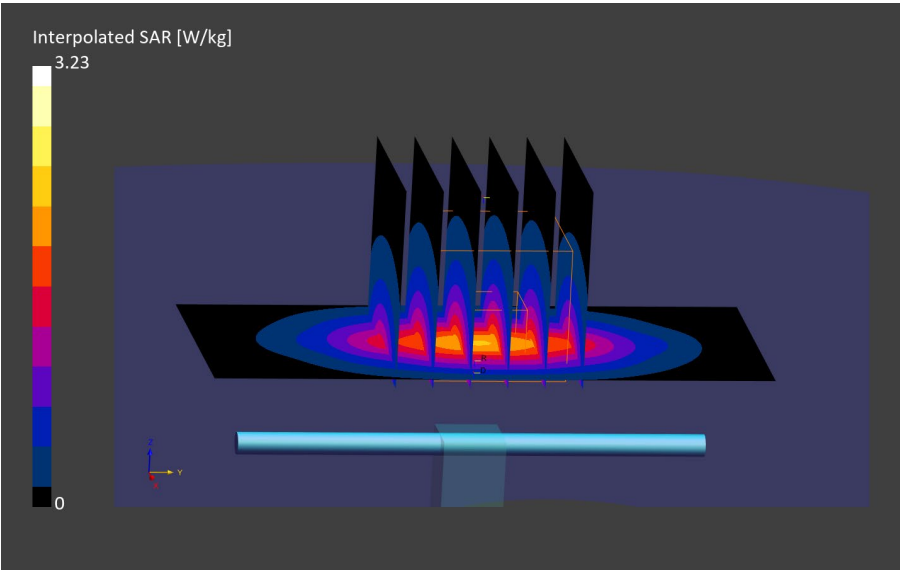

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.23, 6.96,6.94

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-04-29	23.5	23	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.43	41.0	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.05	2.77
psSAR10g	1.07	1.66
Peak SAR (Extrapolated)	3.80	5.16
psAPD (4.0 cm², sq)	N/A	N/A

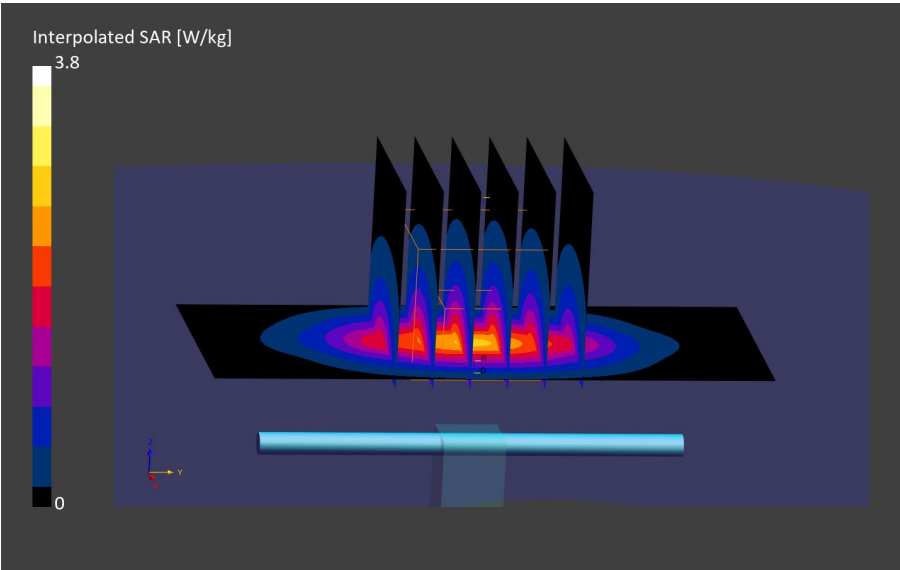

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D1900V2 – SN5d252	17.0	Flat	10	CW, 0	1900.000	7.59, 7.46, 7.22

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-27	22.7	22.3	18.0.0.7250	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.40	41.4	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	1.92	-3.75
psSAR10g	1.01	-4.04
Peak SAR (Extrapolated)	3.41	-5.63
psAPD (4.0 cm², sq)	N/A	N/A

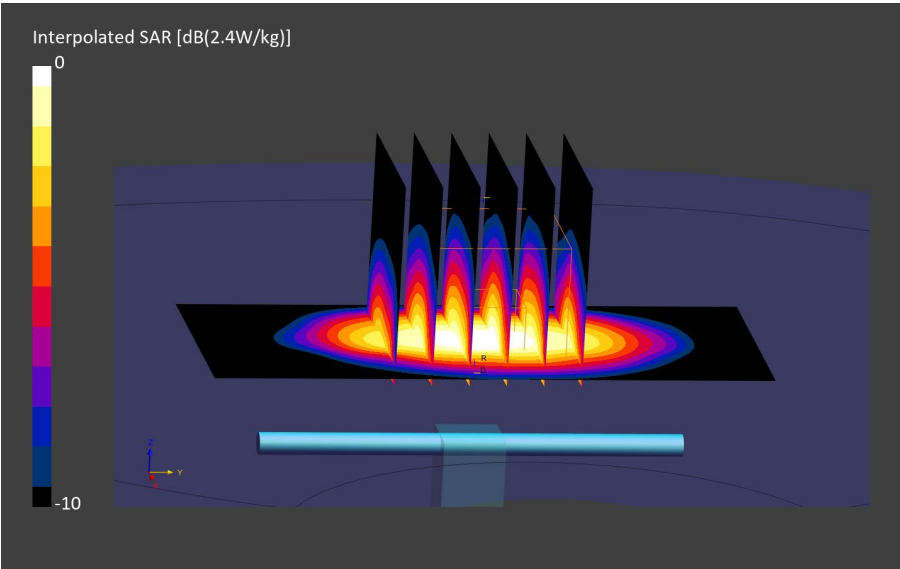

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2100V2 – SN1068	17.0	Flat	10	CW, 0	2100.000	7.46, 7.34, 7.1

Test Setup


Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-06-27	22.7	22.3	18.0.0.7250	Twin-SAM V8.0 – 2238	Head Simulating Liquid	1.52	41.1	EX3DV4 – SN7969, 2026-01-13	DAE4ip Sn1933, 2026-01-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.09	-5.65
psSAR10g	1.06	-5.16
Peak SAR (Extrapolated)	3.91	-2.36
psAPD (4.0 cm², sq)	N/A	N/A

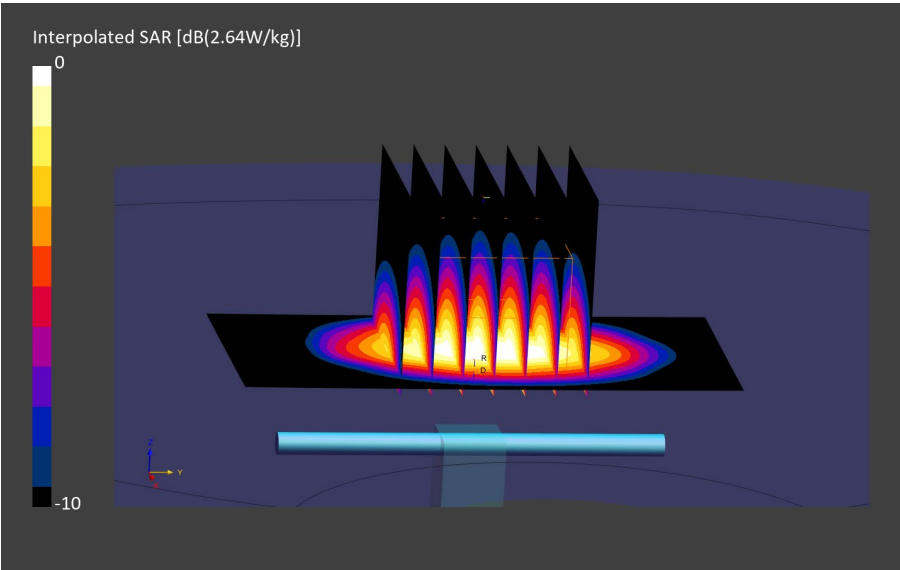

RF SAFETY LABORATORY

System Verification

Verification Conditions

Verification Source	Power [dBm]	Phantom Section	Test Distance [mm]	Signal, UID	Frequency [MHz]	ConvF (x, y, z)
D2450V2 – SN1112	17.0	Flat	10	CW, 0	2450.000	6.94, 6.68, 6.66

Test Setup

Test Date	Ambient Temp [°C]	TSL Temp [°C]	Measurement SW	Phantom	TSL Type	Cond. [S/m]	Perm.	Probe, Cal. Date	DAE, Cal. Date
2026-04-28	23	22.4	17.0.4.7034	Twin-SAM V8.0 – 2164	Head Simulating Liquid	1.82	40.6	EX3DV4 – SN7853, 2025-11-07	DAE4ip Sn1844, 2025-11-05

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 31.2
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Grading Ratio	N/A	1.5

Measurement Results

	SAR [W/kg] or APD [W/m²]	Deviation [%]
psSAR1g	2.50	-1.42
psSAR10g	1.17	-1.5
Peak SAR (Extrapolated)	5.03	-3.68
psAPD (4.0 cm², sq)	N/A	N/A

