

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 1(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

APPENDIX D: PROBE & DIPOLE CALIBRATION DATA

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 2(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client: **RTS (RIM Testing Services)**

Certificate No: **ES3-3225_Jan12**

CALIBRATION CERTIFICATE

Object: **ES3DV3 - SN:3225**

Calibration procedure(s): **QA CAL-01.v6, QA CAL-23.v4, QA CAL-25.v4
Calibration procedure for dosimetric E-field probes**

Calibration date: **January 11, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&PE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	5841290874	31-Mar-11 (No. 217-01372)	Apr-12
Power sensor E4412A	5N41408087	31-Mar-11 (No. 217-01372)	Apr-12
Reference 3 dB Attenuator	SN: 05084 (3x)	29-Mar-11 (No. 217-01368)	Apr-12
Reference 20 dB Attenuator	SN: 05086 (20x)	29-Mar-11 (No. 217-01367)	Apr-12
Reference 30 dB Attenuator	SN: 05129 (30x)	29-Mar-11 (No. 217-01370)	Apr-12
Reference Probe E530V2	SN: 3013	29-Dec-11 (No. E53-3013_Dec11)	Dec-12
CAL-4	SN: 604	3-May-11 (No. D464-604_May11)	May-12
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8640C	US3040201700	4-Aug-08 (in house check Apr-11)	In house check Apr-13
Network Analyser HP 8753B	US37360555	18-Oct-01 (in house check Oct-11)	In house check Oct-12

Calibrated by:	Name Jeloni Kasrell	Function Laboratory Technician	Signature 
Approved by:	Name Katja Pitschke	Function Technical Manager	Signature 

Issued: January 12, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 3(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
S Servizio svizzero di tarature
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 106**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConcF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization β	β rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\beta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}: Assessed for E-field polarization $\beta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E-field uncertainty inside TSL (see below ConcF).
- NORM_{eff}(_{x,y,z}) = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConcF.
- DCP_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A_{x,y,z}, B_{x,y,z}, C_{x,y,z}, VR_{x,y,z}: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConcF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f < 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConcF whereby the uncertainty corresponds to that given for ConcF. A frequency dependent ConcF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): In a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 4(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3 – SN:3225

January 11, 2012

Probe ES3DV3

SN:3225

Manufactured: September 1, 2009
Calibrated: January 11, 2012

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 5(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3– SN:3225

January 11, 2012

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3225

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/\sqrt{V/m})^2$ ^a	1.26	1.26	1.30	± 10.1 %
DCP $(mV)^2$	101.2	100.8	101.2	

Modulation Calibration Parameters

usb	Communication System Name	PAR		A dB	B dB	C dB	VR mV	Unc ^b (k=2)
10000	CW	0.00	X	0.00	0.00	1.00	103.9	±1.3 %
			Y	0.00	0.00	1.00	113.4	
			Z	0.00	0.00	1.00	110.4	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^a The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 8 and 9).

^b Numerical linearization parameter: uncertainty not required.

^c Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 6(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3– SN:3225

January 11, 2012

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3225

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ¹	Relative Permittivity ²	Conductivity (S/m) ²	CoefF X	CoefF Y	CoefF Z	Alpha	Depth (mm)	Unct. (k=2)
750	41.9	0.89	6.42	6.42	6.42	0.27	2.04	± 12.0 %
900	41.5	0.97	6.06	6.06	6.06	0.35	1.74	± 12.0 %
1810	40.0	1.40	5.23	5.23	5.23	0.73	1.21	± 12.0 %
1950	40.0	1.40	4.98	4.98	4.98	0.58	1.41	± 12.0 %
2450	39.2	1.80	4.50	4.50	4.50	0.79	1.26	± 12.0 %
2600	39.0	1.95	4.32	4.32	4.32	0.77	1.32	± 12.0 %

¹ Frequency validity of a 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the CoefF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

² At frequencies below 3 GHz, the validity of tissue parameters (ρ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ρ and σ) is restricted to ± 5%. The uncertainty is the RSS of the CoefF uncertainty for indicated target tissue parameters.

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 7(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3- SN:3225

January 11, 2012

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3225

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^a	Conductivity (S/m) ^a	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
750	55.5	0.96	6.27	6.27	6.27	0.36	1.74	± 12.0 %
900	55.0	1.05	6.07	6.07	6.07	0.29	2.02	± 12.0 %
1810	53.3	1.52	4.92	4.92	4.92	0.50	1.57	± 12.0 %
1950	53.3	1.52	4.87	4.87	4.87	0.50	1.49	± 12.0 %
2450	52.7	1.95	4.30	4.30	4.30	0.68	1.16	± 12.0 %
2600	52.5	2.16	4.12	4.12	4.12	0.80	0.99	± 12.0 %

^c Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the 'ConvF' uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


^a At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the 'ConvF' uncertainty for indicated target tissue parameters.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 8(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3043- SM-3225

January 11, 2012

Frequency Response of E-Field (TEM-Cell: R1110 EXX, Waveguide: R22)

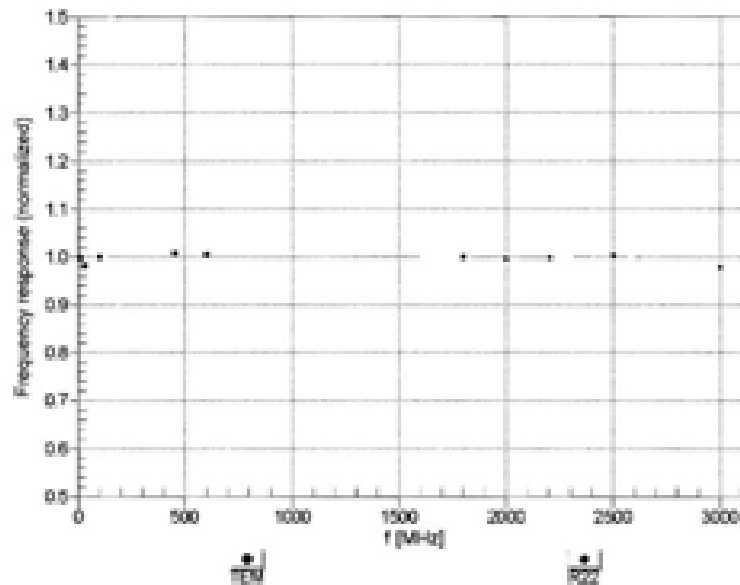
Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02



FCC ID:
L6ARFL110LW
L6ARFP120LW

IC
2503A-RFL110LW
2503A-RFP120LW

ES3073- 3M3225

January 11, 2012

Receiving Pattern (ϕ), $\theta = 0^\circ$

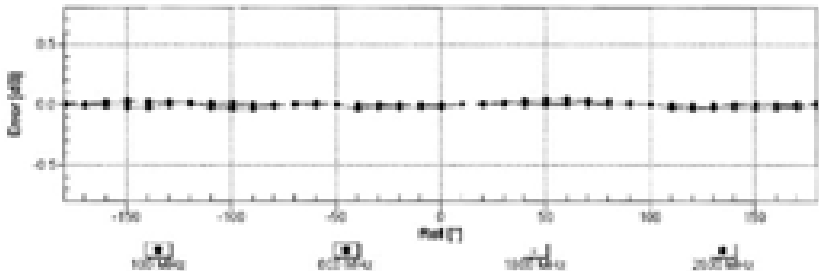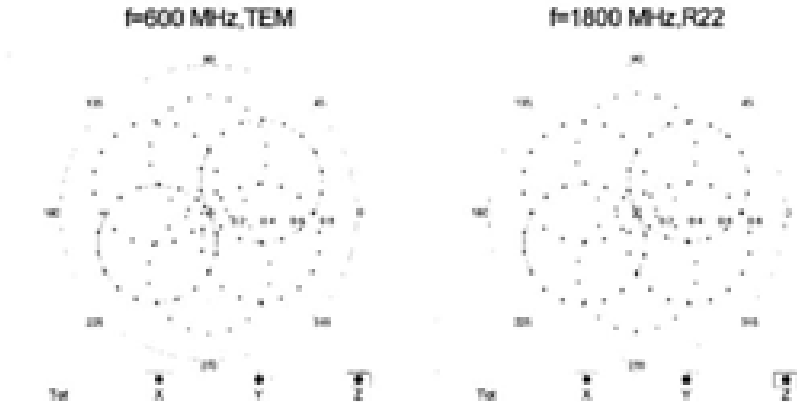

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02


FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

ES30V3- SN-3225

January 11, 2012

Dynamic Range f(SAR_{head})
(TEM cell , f = 900 MHz)

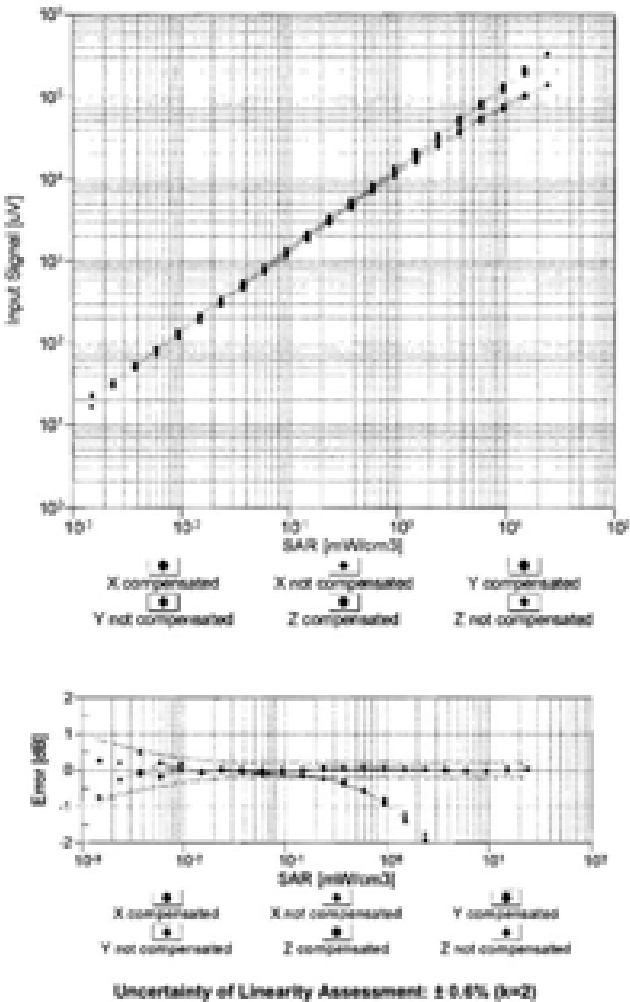

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02


FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

ES33DV3- SW3225


January 11, 2012

Conversion Factor Assessment

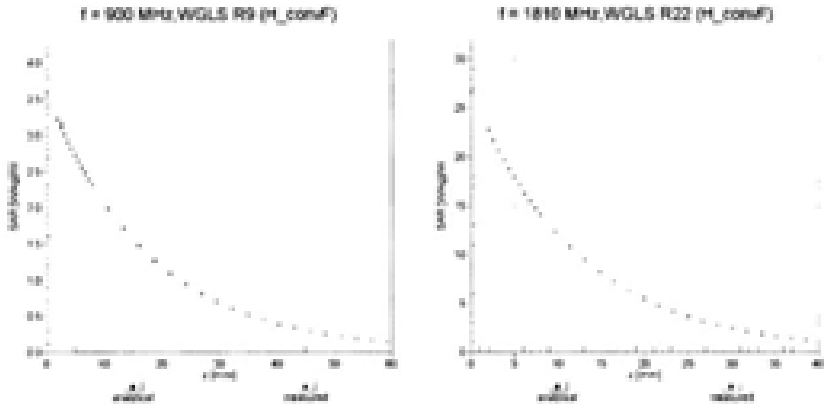

Deviation from Isotropy in Liquid

Error (a, b), f = 900 MHz

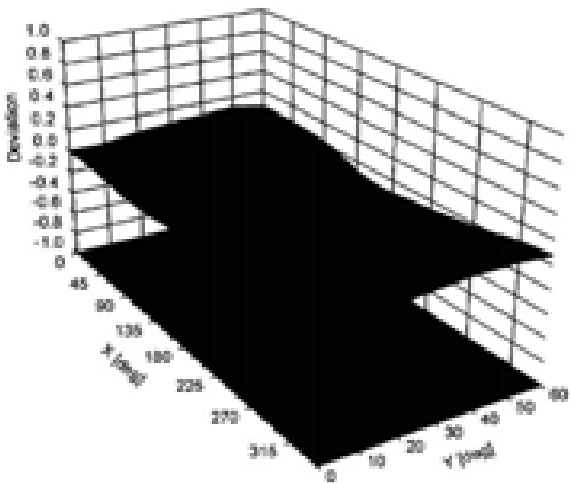

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 12(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3–SN:3225

January 11, 2012

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3225

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	332 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 13(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SIS 100**

Client **RTS (RIM Testing Services)**

Certificate No: **ES3-3225_Jan13**

CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3225**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-23.v4, QA CAL-25.v4**
Calibration procedure for dosimetric E-field probes

Calibration date: **January 10, 2013**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter F44196	0841760874	26-Mar-12 (No. 217-01008)	Apr-12
Power sensor E44134	8714149087	26-Mar-12 (No. 217-01008)	Apr-12
Reference 1-dB Attenuator	SN: 85054 (70)	27-Mar-12 (No. 217-01001)	Apr-12
Reference 20-dB Attenuator	SN: 80060 (206)	27-Mar-12 (No. 217-01009)	Apr-12
Reference 30-dB Attenuator	SN: 80129 (306)	27-Mar-12 (No. 217-01002)	Apr-12
Reference Probe E53DV2	SN: 3213	26-Dec-12 (No. 8325-3013_Dec12)	Dec-12
DAF4	SN: 660	20-Jun-12 (No. DAF4-660_Jun12)	Jun-12
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8448C	US0642UC1700	4-Aug-99 (in house check Apr-11)	In house check: Apr-12
Network Analyzer HP 8713B	US03730046	18-Oct-01 (in house check Oct-12)	In house check: Oct-12

	Name	Function	Signature
Calibrated by:	Jeton Kaspari	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
Issued: January 14, 2013 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 14(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
$NORM_{x,y,z}$	sensitivity in free space
ConvF	sensitivity in TSL / $NORM_{x,y,z}$
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORM_{x,y,z}$ are only intermediate values, i.e., the uncertainties of $NORM_{x,y,z}$ does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- $NORM(f)_{x,y,z} = NORM_{x,y,z} \cdot \text{frequency_response}$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP $_{x,y,z}$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- $A_{x,y,z}$, $B_{x,y,z}$, $C_{x,y,z}$, $D_{x,y,z}$, $VR_{x,y,z}$: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORM_{x,y,z} \cdot \text{ConvF}$ whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 15(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 16(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3 – SN:3225

January 10, 2013

Probe ES3DV3

SN:3225

Manufactured: September 1, 2009
Calibrated: January 10, 2013

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 17(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3- SN:3225

January 10, 2013

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3225

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc. (k=2)
Norm ($\mu V/V/m$) ¹	1.28	1.18	1.31	$\pm 10.1\%$
DCP (mV) ²	100.5	101.5	99.9	

Modulation Calibration Parameters

US	Communication System Name		A dB	B dB- $\sqrt{\mu V}$	C	D dB	VR mV	Unc. ³ (k=2)
0	CW	X	0.0	0.0	1.0	0.00	107.5	$\pm 2.7\%$
		Y	0.0	0.0	1.0		108.4	
		Z	0.0	0.0	1.0		105.9	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

¹ The uncertainties of NormX,Y,Z do not affect the E₁ field uncertainty inside T35, (see Pages 5 and 6).

² Numerical linearization parameter; uncertainty not required.

³ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 18(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 19(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3– SN:3225

January 18, 2013

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3225

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ¹	Relative Permittivity ²	Conductivity (S/m) ²	CorrF X	CorrF Y	CorrF Z	Alpha	Depth (mm)	Unc. (k=2)
750	41.9	0.89	6.56	6.56	6.56	0.42	1.54	± 12.0 %
900	41.5	0.97	6.19	6.19	6.19	0.43	1.52	± 12.0 %
1810	40.0	1.40	5.35	5.35	5.35	0.63	1.39	± 12.0 %
1950	40.0	1.40	5.09	5.09	5.09	0.60	1.23	± 12.0 %
2450	39.2	1.80	4.65	4.65	4.65	0.61	1.63	± 12.0 %
2600	39.0	1.96	4.43	4.43	4.43	0.60	1.32	± 12.0 %

¹ Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the CorrF² uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

² At frequencies below 3 GHz, the validity of tissue parameters (ρ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ρ and σ) is restricted to ± 5%. The uncertainty is the RSS of the CorrF² uncertainty for indicated target tissue parameters.

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 20(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3- SN:3225

January 10, 2013

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3225

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ¹	Relative Permittivity ²	Conductivity (S/m) ²	CorrF X	CorrF Y	CorrF Z	Alpha	Depth (mm)	Unc. (k=2)
750	55.5	0.96	6.27	6.27	6.27	0.48	1.51	± 12.0 %
900	55.0	1.05	6.12	6.12	6.12	0.73	1.25	± 12.0 %
1810	53.3	1.52	5.04	5.04	5.04	0.57	1.47	± 12.0 %
1850	53.3	1.52	4.94	4.94	4.94	0.58	1.50	± 12.0 %
2450	52.7	1.95	4.35	4.35	4.35	0.70	1.16	± 12.0 %
2600	52.5	2.16	4.11	4.11	4.11	0.67	0.99	± 12.0 %

¹ Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 25), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the CorrF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

² At frequencies below 3 GHz, the validity of tissue parameters (ρ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ρ and σ) is restricted to ± 5%. The uncertainty is the RSS of the CorrF uncertainty for indicated target tissue parameters.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 21(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW


	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 22(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES330v3- Rev 3/2010

January 10, 2013

Frequency Response of E-Field

(TEM-Cell: ifi110 EXX, Waveguide: R22)

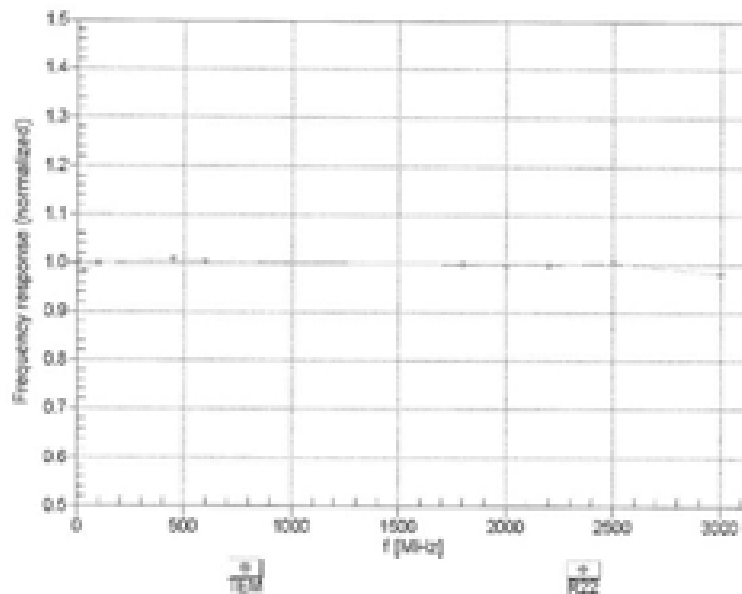

Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 23(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3-3225

January 10, 2013

Receiving Pattern (ϕ), $\theta = 0^\circ$

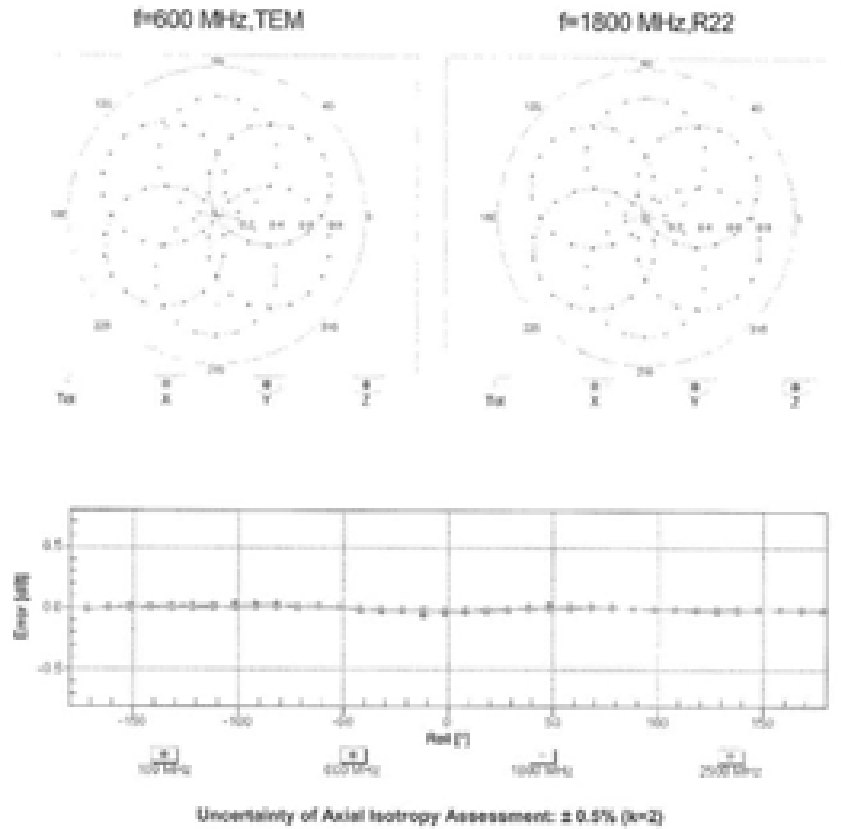

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 24(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02


FCC ID:
L6ARFL110LW
L6ARFP120LW

IC
2503A-RFL110LW
2503A-RFP120LW

ES3-3225

January 18, 2013

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f = 900 \text{ MHz}$)

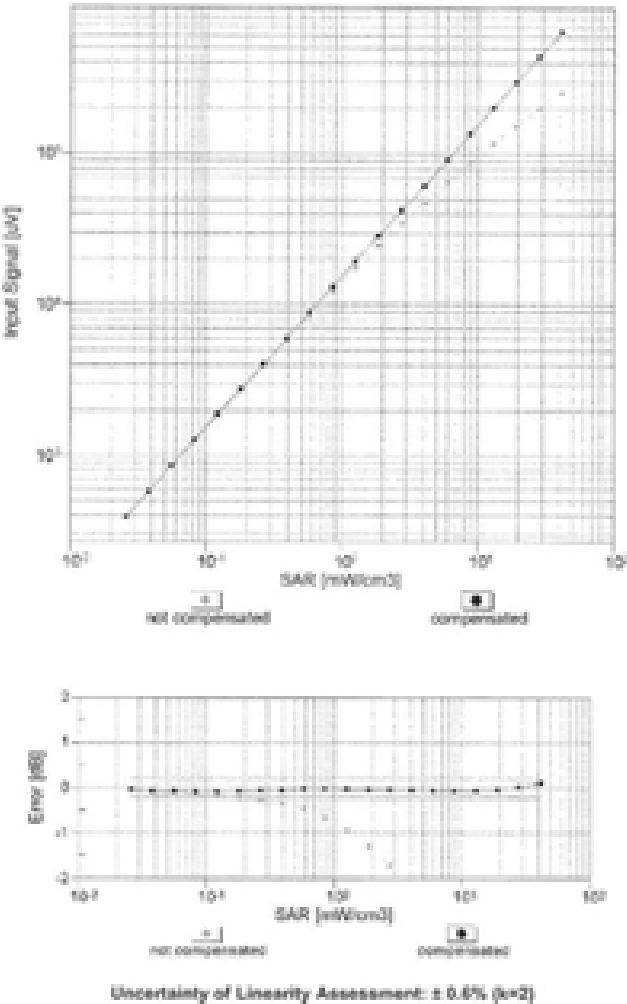

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02


FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**


ES33225-3M3225

January 10, 2013

Conversion Factor Assessment

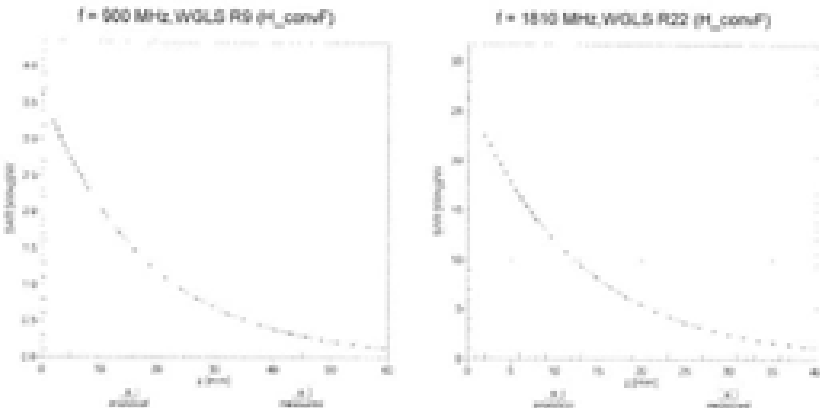

Deviation from Isotropy in Liquid Error (ϕ , θ), f = 900 MHz

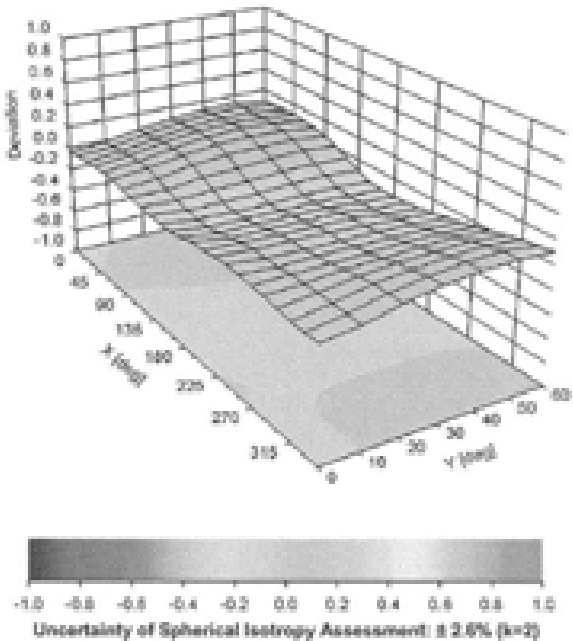

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 27(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 28(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ES3DV3- SN:3225

January 18, 2013

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3225

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	8.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 29(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Calibration Laboratory of
Schmid & Partner
Engineering AG
Engenhurststrasse 43, 8004 Zurich, Switzerland



§ Schweizerischer Kalibrierdienst
§ Service suisse d'étalonnage
§ Servizio svizzero di taratura
§ Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **EX3-3592_Nov12**

CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN 3592**

Calibration procedure(s): **QA CAL-01.v8, QA CAL-14.v3, QA CAL-23.v4, QA CAL-25.v4
Calibration procedure for dosimetric E-field probes**

Calibration date: **November 14, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 2)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	0841293874	29-Mar-12 (No. 217-01908)	Apr-13
Power sensor E4413A	MHR1698687	29-Mar-12 (No. 217-01908)	Apr-13
Reference 3 dB Attenuator	SN: 55054 (30)	27-Mar-12 (No. 217-01537)	Apr-13
Reference 20 dB Attenuator	SN: 55085 (20)	27-Mar-12 (No. 217-01529)	Apr-13
Reference 30 dB Attenuator	SN: 55129 (30)	27-Mar-12 (No. 217-01532)	Apr-13
Reference Probe E530V2	SN: 3043	29-Dec-11 (No. E53-3013, Dec11)	Dec-12
DA64	SN: 690	29-Jun-12 (No. DA64-690_Jun12)	Jun-13
Secondary Standards			
RF generator HP 8640C	US3642001700	4-Aug-09 (in house check Apr-11)	In house check: Apr-13
Network Analyzer HP 8753E	US37360585	18-Oct-01 (in house check Oct-02)	In house check: Oct-13

Calibrated by:	Name David Loubser	Function Laboratory Technician	Signature 
Approved by:	Name Katja Petrovic	Technical Manager	
Issued: November 14, 2012			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 30(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S
C
S
Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Service suisse di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
$NORM_{x,y,z}$	sensitivity in free space
$ConvF$	sensitivity in TSL / $NORM_{x,y,z}$
DCP	diode compression point
CF	crest factor (Vduty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization β	β rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\beta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$: Assessed for E-field polarization $\beta = 0$ ($f \leq 900$ MHz: TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORM_{x,y,z}$ are only intermediate values, i.e., the uncertainties of $NORM_{x,y,z}$ does not affect the E-field uncertainty inside TSL (see below $ConvF$).
- $NORM(f)_{x,y,z} = NORM_{x,y,z} \cdot \text{frequency_response}$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of $ConvF$.
- $DCP_{x,y,z}$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- $A_{x,y,z}$; $B_{x,y,z}$; $C_{x,y,z}$; $VR_{x,y,z}$: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- $ConvF$ and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORM_{x,y,z} \cdot ConvF$ whereby the uncertainty corresponds to that given for $ConvF$. A frequency dependent $ConvF$ is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 31(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 32(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

EX3DV4 - SN:3592

November 14, 2012

Probe EX3DV4

SN:3592

Manufactured: September 18, 2006
Calibrated: November 14, 2012

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 33(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

EX3DV4– SN:3592

November 14, 2012

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3592

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm. $(\mu V/(V/m)^2)^A$	0.49	0.47	0.41	$\pm 10.1\%$
DCP $(mV)^B$	95.2	96.1	100.6	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dB	C dB	VR mV	Unc ^C (k=2)
5	OW	0.00	X	0.0	0.0	1.0	101.4	$\pm 3.0\%$
			Y	0.0	0.0	1.0	104.3	
			Z	0.0	0.0	1.0	109.2	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm.X,Y,Z do not affect the E₁ field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter; uncertainty not required.

^C Uncertainty is determined using the rms. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 34(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 35(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

EX3DV4 - SN:3592

November 14, 2012

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3592

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ¹	Relative Permittivity ²	Conductivity (S/m) ²	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unc. (k=2)
2600	39.0	1.96	6.45	6.45	6.45	0.53	0.79	± 12.0 %
5200	36.0	4.66	4.73	4.73	4.73	0.40	1.80	± 13.1 %
5500	35.6	4.96	4.28	4.28	4.28	0.44	1.80	± 13.1 %
5800	35.3	5.27	4.12	4.12	4.12	0.48	1.80	± 13.1 %

¹ Frequency validity of ± 100 kHz only applies for DASY v4.4 and higher (see Page 23), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

² At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 36(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 37(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

EX3DV4--SN:3592

November 14, 2012

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3592

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^a	Relative Permittivity ^b	Conductivity (S/m) ^c	CorrF X	CorrF Y	CorrF Z	Alpha	Depth (mm)	Unc. (k=2)
2600	52.5	2.16	6.59	6.59	6.59	0.60	0.50	± 12.0 %
5200	49.0	5.30	4.02	4.02	4.02	0.48	1.00	± 13.1 %
5500	48.6	5.65	3.66	3.66	3.66	0.56	1.00	± 13.1 %
5800	48.2	6.00	3.57	3.57	3.57	0.57	1.00	± 13.1 %

^a Frequency validity of ± 100 MHz only applies for DASY v6.4 and higher (see Page 2); else it is restricted to ± 50 MHz. The uncertainty is the RSS of the CorrF^b uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


^b At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formulae is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the CorrF^c uncertainty for indicated target tissue parameters.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 38(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

EQSDM--SN 3592

November 14, 2012

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

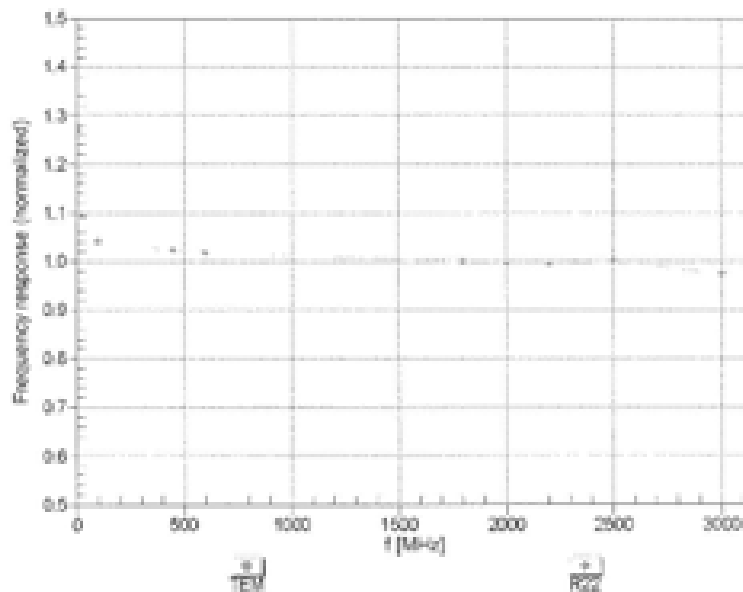


Uncertainty of Frequency Response of E-Field: $\pm 6.3\%$ ($k=2$)

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 39(134)	
Author Data Andrew Becker		Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

EX00V4-SN3092

November 14, 2012

Receiving Pattern (ϕ), $\theta = 0^\circ$

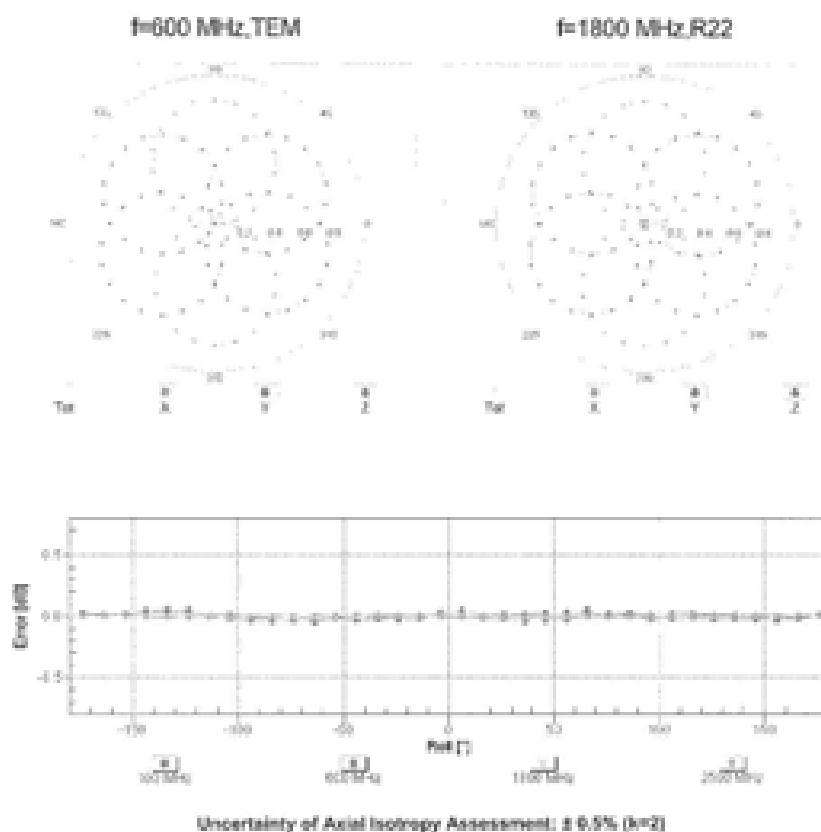

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 40(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02



FCC ID:
L6ARFL110LW
L6ARFP120LW

IC
2503A-RFL110LW
2503A-RFP120LW

E00044-EN-3592

November 14, 2012

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f = 900 \text{ MHz}$)

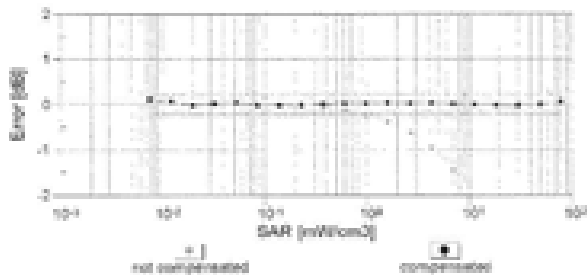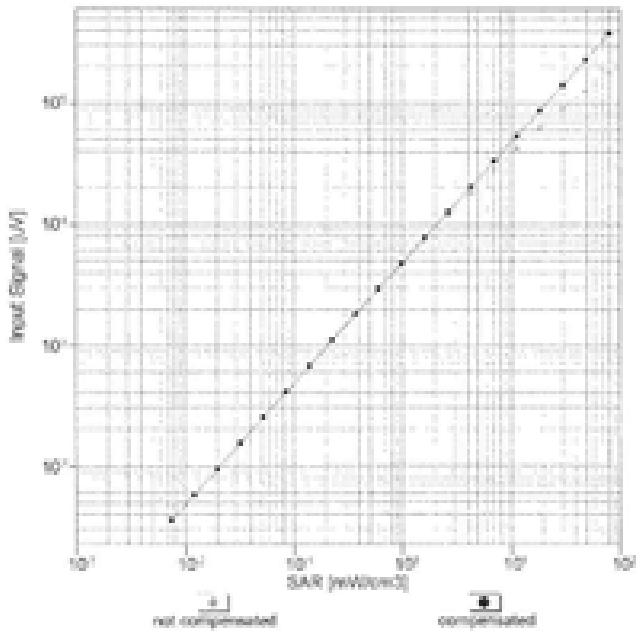

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02


FCC ID:
L6ARFL110LW
L6ARFP120LW

IC
2503A-RFL110LW
2503A-RFP120LW


EX03D44- 0M-3592

November 14, 2012

Conversion Factor Assessment

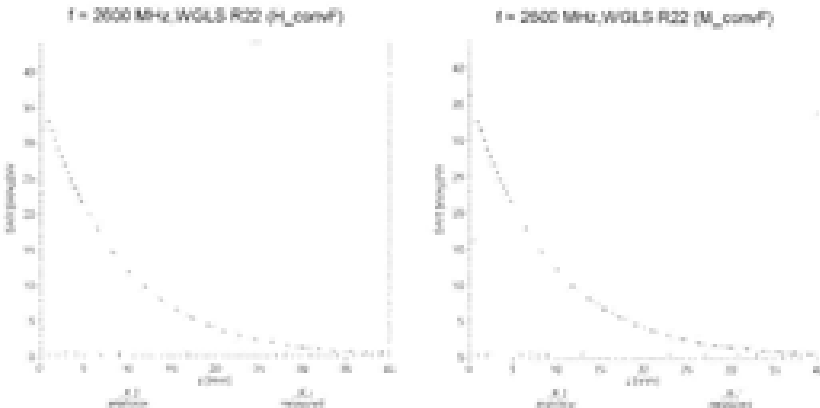

Deviation from Isotropy in Liquid Error (φ, θ), f = 900 MHz

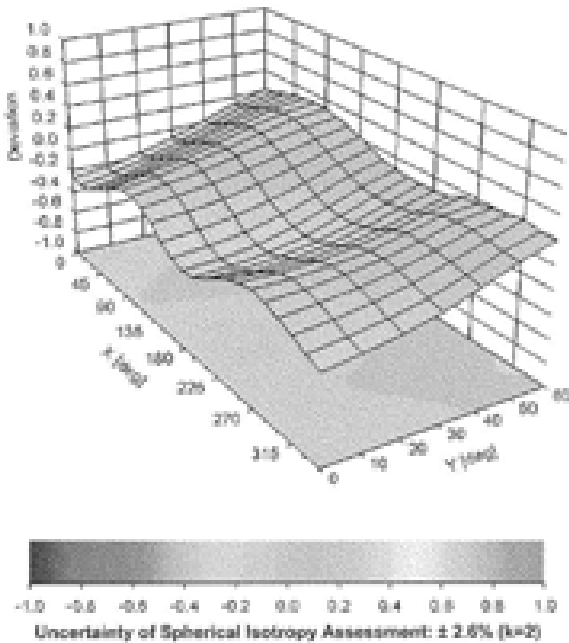

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 43(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 44(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

EX3DV4 – SN:3592

November 14, 2012

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3592

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-13.6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 45(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAC)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates.

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **ET3-1644_Nov12**

CALIBRATION CERTIFICATE

Object **ET3DV8 - SN:1644**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-23.v4, QA CAL-25.v4
Calibration procedure for dosimetric E-field probes**

Calibration date: **November 13, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity = 70%.

Calibration Equipment used (M&PE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E44199	GB4128074	29-Mar-12 (No. 217-01508)	Apr-13
Power sensor E4413A	MF41498087	29-Mar-12 (No. 217-01508)	Apr-13
Reference 3 dB Attenuator	SN: 55054 (30)	27-Mar-12 (No. 217-01520)	Apr-13
Reference 20 dB Attenuator	SN: 55086 (20)	27-Mar-12 (No. 217-01528)	Apr-13
Reference 30 dB Attenuator	SN: 55179 (30)	27-Mar-12 (No. 217-01532)	Apr-13
Reference Probe ES30V2	SN: 3013	29-Dec-11 (No. 853-3013, Dec-11)	Dec-12
DAE4	SN: 686	20-Jun-12 (No. 0A14460 Jun-12)	Jun-13
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	U52643U1700	4-Aug-09 (in house check Apr-10)	In-house check Apr-13
Network Analyser HP 8733C	U527360595	18-Oct-01 (in house check Oct-12)	In-house check Oct-13

Calibrated by:	Name Jeton Kastner	Function Laboratory Technician	Signature 
Approved by:	Name Katja Peters	Technical Manager	

Issued: November 13, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 46(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zughausstrasse 41, 8584 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
$NORM_{x,y,z}$	sensitivity in free space
$ConvF$	sensitivity in TSL / $NORM_{x,y,z}$
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2006

Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). $NORM_{x,y,z}$ are only intermediate values, i.e., the uncertainties of $NORM_{x,y,z}$ does not affect the E-field uncertainty inside TSL (see below $ConvF$).
- $NORM(f)_{x,y,z} = NORM_{x,y,z} \cdot \text{frequency_response}$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of $ConvF$.
- $DCP_{x,y,z}$: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- $A_{x,y,z}$; $B_{x,y,z}$; $C_{x,y,z}$; $VR_{x,y,z}$: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- $ConvF$ and Boundary Effect Parameters: Assessed in fat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to $NORM_{x,y,z} \cdot ConvF$ whereby the uncertainty corresponds to that given for $ConvF$. A frequency dependent $ConvF$ is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a fat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 47(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ET3DV6 - SN:1644

November 13, 2012

Probe ET3DV6

SN:1644

Manufactured: November 7, 2001
Calibrated: November 13, 2012

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 48(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ET3DV6- SN:1644

November 13, 2012

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1644

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu W/V/m)^2$ ²	1.71	1.97	1.98	$\pm 10.1\%$
DCP $(mV)^2$	99.5	98.7	97.5	

Modulation Calibration Parameters

URD	Communication System Name	FAR		A dB	B dB	C dB	VR mV	Unc ³ (k=2)
0	Cel	0.00	X	0.0	0.0	1.0	193.5	$\pm 3.5\%$
			Y	0.0	0.0	1.0	212.0	
			Z	0.0	0.0	1.0	201.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

² The uncertainties of NormX,Y,Z do not affect the E² field uncertainty inside T3a (see Pages 5 and 6).

³ Numerical linearization parameter; uncertainty not required.

⁴ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 49(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ET3DV6 - SN:1644

November 13, 2012

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1644

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^a	Relative Permittivity ^b	Conductivity (S/m) ^c	CorrF X	CorrF Y	CorrF Z	Alpha	Depth (mm)	Uncl. (k=2)
750	41.9	0.89	6.57	6.57	6.57	0.44	2.25	± 12.0 %
900	41.5	0.97	6.24	6.24	6.24	0.38	2.52	± 12.0 %
1810	40.0	1.40	5.21	5.21	5.21	0.60	2.19	± 12.0 %
1950	40.0	1.40	5.16	5.16	5.16	0.60	2.09	± 12.0 %
3450	39.2	1.60	4.60	4.60	4.60	0.65	2.00	± 12.0 %

^a Frequency validity of a 100 MHz only applies for DASY v4.4 and higher (see Page 2), also it is restricted to ± 50 MHz. The uncertainty is the RSS of the CorrF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^b At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be related to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the CorrF uncertainty for indicated target tissue parameters.

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 50(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ET3DV6- SN:1644

November 13, 2012

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1644

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^d	Conductivity (S/m) ^e	Coeff X	Coeff Y	Coeff Z	Alpha	Depth (mm)	Unc. (k=2)
750	55.5	0.86	6.30	6.30	6.30	0.33	2.61	± 12.0 %
900	55.0	1.05	6.06	6.06	6.06	0.31	2.99	± 12.0 %
1810	53.3	1.52	4.75	4.75	4.75	0.80	2.40	± 12.0 %
1950	53.3	1.52	4.75	4.75	4.75	0.80	2.28	± 12.0 %
2450	52.7	1.95	4.11	4.11	4.11	0.50	2.15	± 12.0 %

^c Frequency validity of ± 150 MHz only applies for EASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the Coeff uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


^d At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the Coeff uncertainty for indicated target tissue parameters.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 51(134)
	Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02 FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ET30V6- SR-1644

November 13, 2012

Frequency Response of E-Field (TEM-Cell: R1110 E3X, Waveguide: R22)

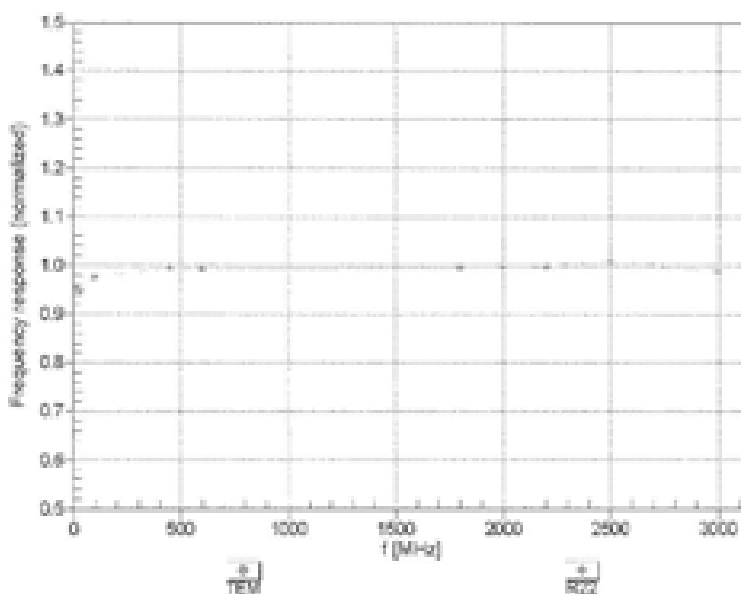

Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02


FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

ET307V6- SN:1944

November 13, 2012

Receiving Pattern (ϕ), $\theta = 0^\circ$

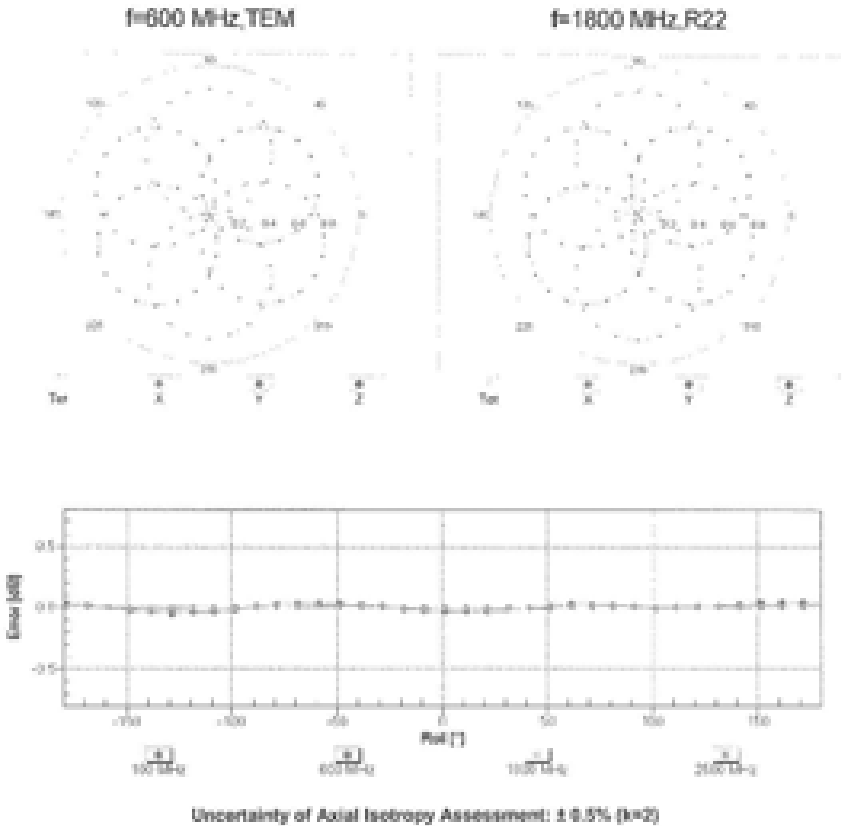

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02



FCC ID:
L6ARFL110LW
L6ARFP120LW

IC
2503A-RFL110LW
2503A-RFP120LW

ET30146- 3N1044

November 13, 2012

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f = 900 \text{ MHz}$)

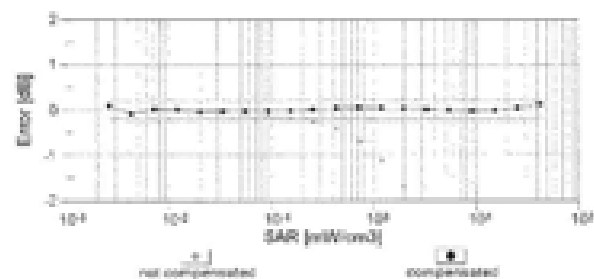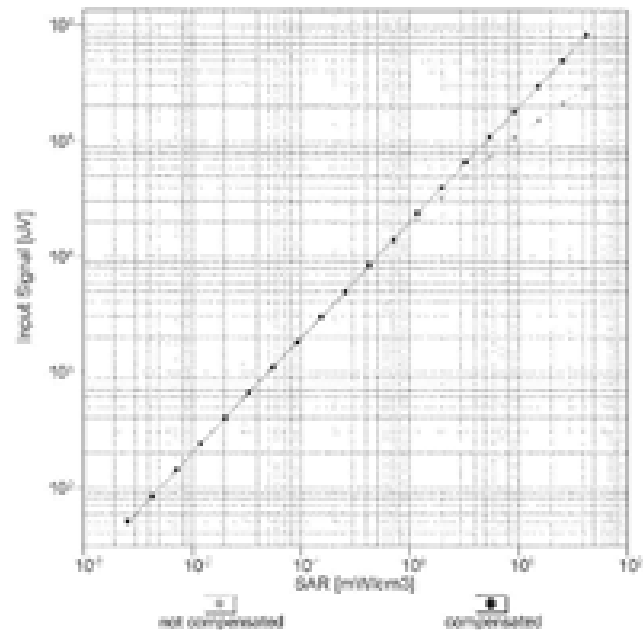

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02


FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**


ET30V6-SR1644

November 13, 2012

Conversion Factor Assessment

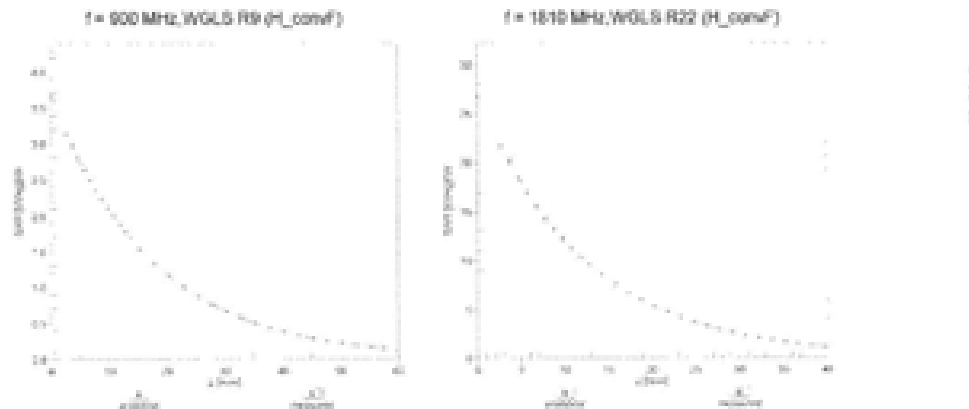

Deviation from Isotropy in Liquid Error (ϕ , θ), f = 900 MHz

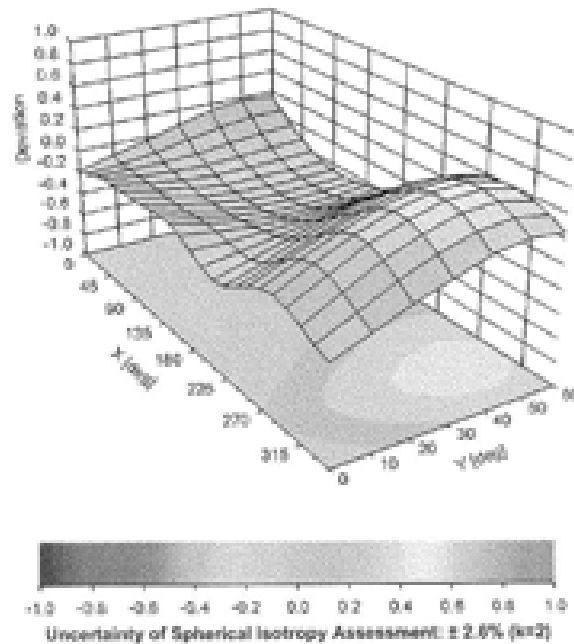

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 55(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

ET3DV6 - SN:1644

November 13, 2012

DASY/EASY - Parameters of Probe: ET3DV6 - SN:1644

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	41.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	enabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	6.8 mm
Probe Tip to Sensor X Calibration Point	2.7 mm
Probe Tip to Sensor Y Calibration Point	2.7 mm
Probe Tip to Sensor Z Calibration Point	2.7 mm
Recommended Measurement Distance from Surface	4 mm

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 56(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 57(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RIM**

Certificate No: **D750V3-1021_Jan11**

CALIBRATION CERTIFICATE

Object **D750V3 - SN: 1021**

Calibration procedure(s) **QA CAL-05.v8**
Calibration procedure for dipole validation kits

Calibration date: **January 05, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23 ± 3)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	G857480704	06-Oct-10 (No. 217-01288)	Oct-11
Power sensor HP 8481A	US37282783	06-Oct-10 (No. 217-01288)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES30V3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in-house)	Scheduled Check
Power sensor HP 8481A	MY41062317	18-Oct-02 (in house check Oct-08)	In-house check: Oct-11
RF generator RLS SMT-06	100005	4-Aug-09 (in house check Oct-09)	In-house check: Oct-11
Network Analyzer HP 8733E	US37390585 54205	18-Oct-01 (in house check Oct-10)	In-house check: Oct-11

Calibrated by: **Name: Jason Kalliyel**
Jason Kalliyel

Function: **Laboratory Technician**
Laboratory Technician

Signature

Approved by: **Katja Pokorski**

Technical Manager

Issued: January 6, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D750V3-1021_Jan11**

Page 1 of 6

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 58(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 59(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 8.

DASY Version	DASY5	V52.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	$dx, dy, dz = 5 \text{ mm}$	
Frequency	$750 \text{ MHz} \pm 1 \text{ MHz}$	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	$(22.0 \pm 0.2) \text{ °C}$	$42.3 \pm 6 \%$	$0.91 \text{ mho/m} \pm 6 \%$
Head TSL temperature during test	$(22.0 \pm 0.2) \text{ °C}$	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.12 mW / g
SAR normalized	normalized to 1W	8.48 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	$8.38 \text{ mW / g} \pm 17.0 \%$ (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.38 mW / g
SAR normalized	normalized to 1W	5.52 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	$5.45 \text{ mW / g} \pm 16.5 \%$ (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 60(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.1 Ω - 1.7 jΩ
Return Loss	- 29.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.033 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 04, 2010

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 61(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date/Time: 05.01.2011 15:51:17

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1021

Communication System: CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: HSL750

Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.91 \text{ mho/m}$; $\epsilon_r = 42.3$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.37, 6.37, 6.37); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 4.5L; Type: QD000P49AA; Serial: 1001
- Measurement SW: DASY52, V52.6 Build (401)
- Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)

P_{in}=250mW; dip=15mm; dist=3.0mm/Zoom Scan (7x7x7)/Cube 0; Measurement grid:


$dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 53.5 V/m; Power Drift = -0.00432 dB

Peak SAR (extrapolated) = 3.24 W/kg

SAR(1 g) = 2.12 mW/g; SAR(10 g) = 1.38 mW/g

Maximum value of SAR (measured) = 2.48 mW/g

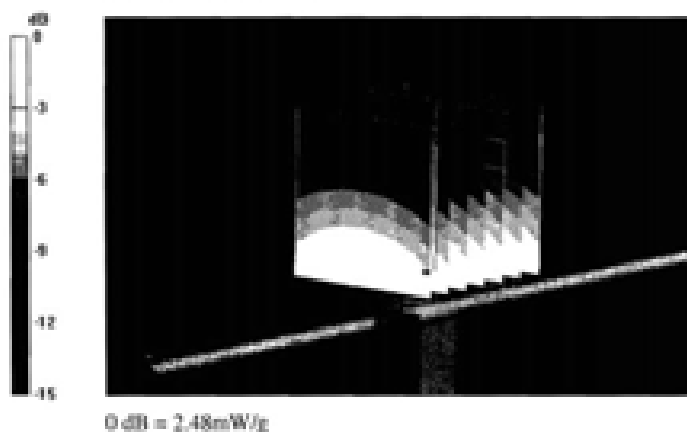



Author Data
Andrew Becker


Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02

FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

Impedance Measurement Plot for Head TSL

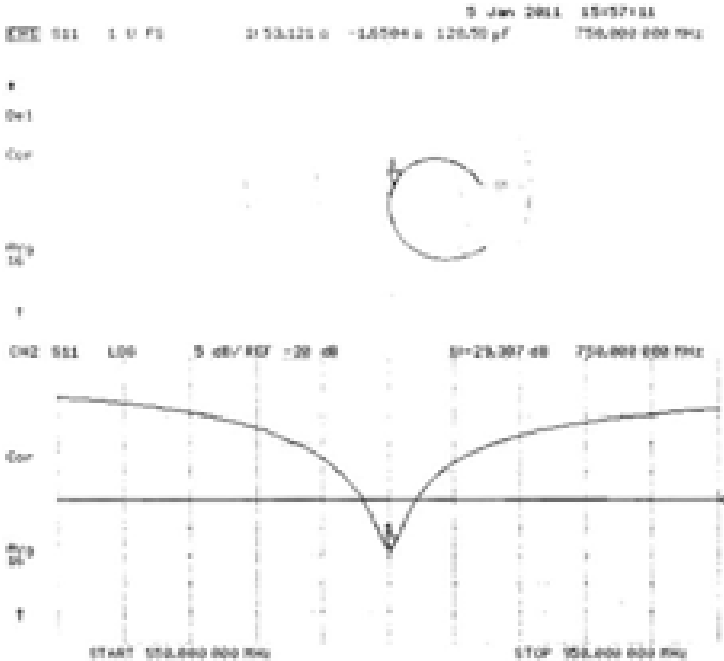

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 63(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D750V3-1021_Jan13**

CALIBRATION CERTIFICATE

Object **D750V3 - SN: 1021**

Calibration procedure(s) **QA CAL-05.v9
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **January 07, 2013**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MPE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter CPM-400A	04501460704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8441A	US37292783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20-dB Attenuator	SN: 1058 (20x)	27-Mar-12 (No. 217-01630)	Apr-13
Type-N mismatch combination	SN: 1047.3 / 06327	27-Mar-12 (No. 217-01630)	Apr-13
Reference Probe E530V3	SN: 3205	28-Dec-12 (No. E53-3205_Dec12)	Dec-13
DA614	SN: 601	27-Jun-12 (No. DA614-601_Jun12)	Jun-13

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8441A	MP11092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SM1-05	100005	04-Aug-09 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8713E	US37300585 34206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13

	Name	Function	Signature
Calibrated by:	Lail Klyener	Laboratory Technician	
Approved by:	Katja Polowik	Technical Manager	

Issued: January 8, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D750V3-1021_Jan13

Page 1 of 6

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 64(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 45, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields: Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 65(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52-6.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	8.46 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.58 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.31 W/kg ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 66(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.7 Ω - 0.2 j Ω
Return Loss	> 25.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.000 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 01, 2010

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 67(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date: 07.01.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1021

Communication System: CW; Frequency: 750 MHz

Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.89 \text{ S/m}$; $\epsilon_r = 41.4$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN:205; Core:R(6.28, 6.28, 6.28); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sa601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.4(1052); SEMCAD X 14.6.8(7028)

Dipole Calibration for Head Tissue/ $P_{in}=250 \text{ mW}$, $d=15\text{mm}$ /Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $d_x=5\text{mm}$, $d_y=5\text{mm}$, $d_z=5\text{mm}$

Reference Value = 54.107 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.23 W/kg

SAR(1 g) = 2.12 W/kg; SAR(10 g) = 1.38 W/kg

Maximum value of SAR (measured) = 2.47 W/kg

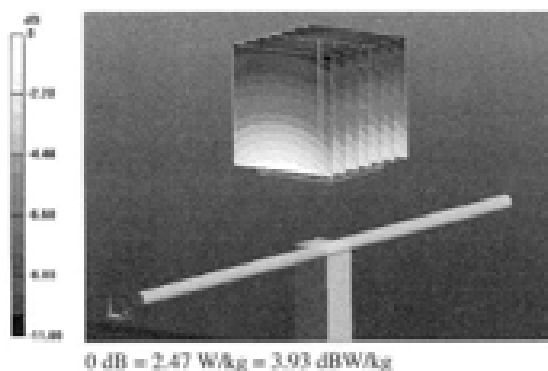

Author Data
Andrew Becker


Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02

FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

Impedance Measurement Plot for Head TSL

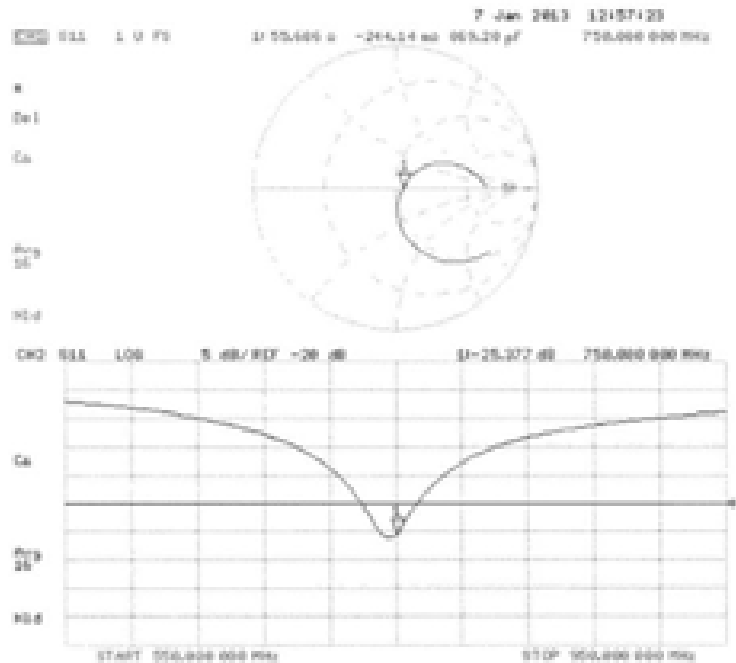

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 69(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 70(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D835V2-446_Jan11**

CALIBRATION CERTIFICATE

Object **D835V2 - SN: 446**

Calibration procedure(s) **QA CAL-05.v8**
Calibration procedure for dipole validation kits

Calibration date: **January 21, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	G837480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37282763	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES30V3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MPE1062317	18-Oct-02 (in house check Oct-08)	In house check: Oct-11
RF generator R&S SM1-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyser HP 8713E	US37380585 (S4206)	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by:	Oliver Hey	Function Laboratory Technician	Signature 
Approved by:	Katja Pokorski	Technical Manager	

Issued: January 21, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D835V2-446_Jan11**

Page 1 of 6

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 71(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields: Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 72(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom 1/4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	805 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.3 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature during test	(21.8 ± 0.2) °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.39 mW / g
SAR normalized	normalized to 1W	9.56 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	9.63 mW / g ± 17.9 % (n=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.56 mW / g
SAR normalized	normalized to 1W	6.24 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	6.37 mW / g ± 16.5 % (n=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 73(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.8 Ω ± 7.7 jΩ
Return Loss	~ 22.2 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.360 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 24, 2001

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 74(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date/Time: 21.01.2011 10:18:05

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:446

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL900

Medium parameters used: $f = 835$ MHz; $\sigma = 0.89$ mho/m; $\epsilon_r = 41.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3206; ConvF(6.03, 6.03, 6.03); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAB4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- Measurement SW: DASY52, V52.6.1 Build (408)
- Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)


Pin=250 mW /d=15mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.426 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 3.600 W/kg

SAR(1 g) = 2.39 mW/g; SAR(10 g) = 1.56 mW/g

Maximum value of SAR (measured) = 2.790 mW/g

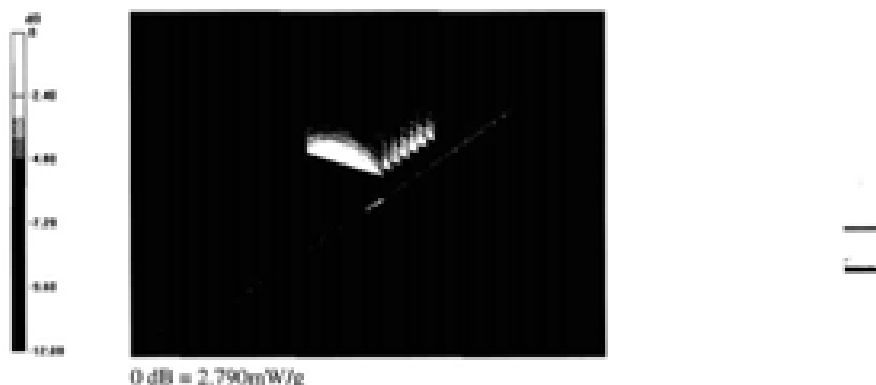

Author Data
Andrew Becker


Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02

FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

Impedance Measurement Plot for Head TSL

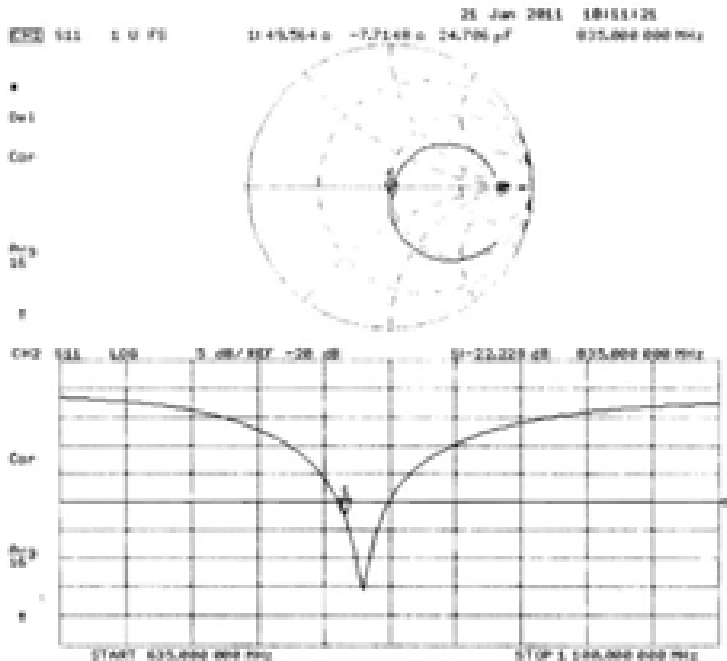

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 76(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 45, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client: **RTS (RIM Testing Services)**

Certificate No: **D835V2-446_Jan13**

CALIBRATION CERTIFICATE

Object: **D835V2 - SN: 446**

Calibration procedure(s): **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **January 07, 2013**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 3°C and humidity < 70%.

Calibration Equipment used (MTE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-642A	0820460704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37262783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5056 (304)	27-Mar-12 (No. 217-01530)	Apr-13
Type-N mismatch combination	SN: 5047.3 / 06327	27-Mar-12 (No. 217-01530)	Apr-13
Reference Probe ESGDV3	SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
DAE4	SN: 601	27-Jun-12 (No. DAE4-601_Jun12)	Jun-13

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41062017	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
HP generator N65 SAIT-05	100005	04-Aug-09 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8713B	US37390585 54206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13

	Name	Function	Signature
Calibrated by:	Leif Rysner	Laboratory Technician	
Approved by:	Katja Polowik	Technical Manager	

Issued: January 8, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D835V2-446_Jan13**

Page 1 of 6

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 77(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 78(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V92.6.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.0 ± 6 %	0.92 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.39 W/kg ± 17.6 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.55 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.13 W/kg ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 79(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.1 Ω - 6.5 j Ω
Return Loss	- 23.7 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.385 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 24, 2001

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 80(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date: 07.01.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: DR35V2; Serial: DR35V2 - SN: 446

Communication System: CW; Frequency: 835 MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.92 \text{ S/m}$; $\epsilon_r = 42$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.05, 6.05, 6.05); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.4(1052); SEMCAD X 14.6.8(7028)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0;


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 56.650 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.61 W/kg

SAR(1 g) = 2.38 W/kg; SAR(10 g) = 1.55 W/kg

Maximum value of SAR (measured) = 2.79 W/kg

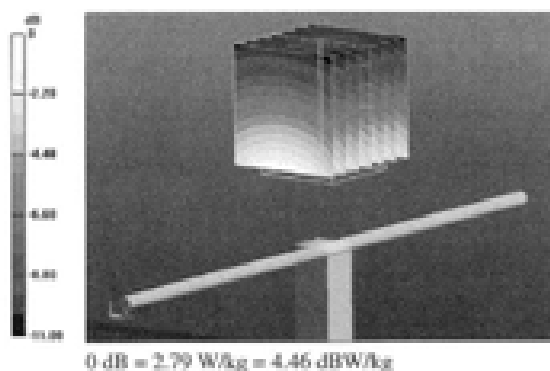

Author Data
Andrew Becker


Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02

FCC ID:
L6ARFL110LW
L6ARFP120LW

IC
2503A-RFL110LW
2503A-RFP120LW

Impedance Measurement Plot for Head TSL

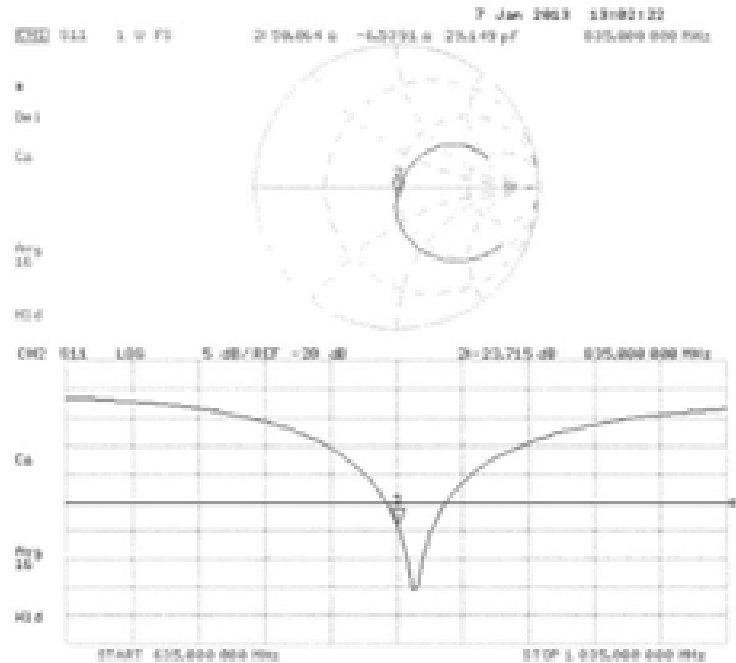

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 82(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 83(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zugstrasse 40, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D835V2-4d043_Apr11**

CALIBRATION CERTIFICATE

Object **D835V2 - SN: 4d043**

Calibration procedure(s) **QA CAL-05.v8**
Calibration procedure for dipole validation kits

Calibration date: **April 07, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (23 ± 3)°C and humidity < 70%.

Calibration Equipment used (NISTE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-402A	0807480704	06-Oct-10 (No. 217-01060)	Oct-11
Power sensor HP 8481A	US07290780	06-Oct-10 (No. 217-01060)	Oct-11
Reference 30 dB Attenuator	SN: 3086 (10g)	29-Mar-11 (No. 217-01060)	Apr-12
Type-N mismatch combination	SN: 5047 2 / 06007	29-Mar-11 (No. 217-01071)	Apr-12
Reference Probe ES20V3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	18-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MTH 1062117	18-Oct-02 (in house check Oct-09)	In house check Oct-11
HP generator P&S SMT-06	100805	4-Aug-09 (in house check Oct-09)	In house check Oct-11
Network Analyzer HP 8752B	US07390585 54056	18-Oct-04 (in house check Oct-10)	In house check Oct-11

Calibrated by: **Jelena Kasirali** Function: **Laboratory Technician**

Approved by: **Katja Polenko** Technical Manager

Signature



Issued April 7, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D835V2-4d043_Apr11**

Page 1 of 6

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 84(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zughausstrasse 41, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 85(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Specor
Zoom Scan Resolution	$dx, dy, dz = 5 \text{ mm}$	
Frequency	$935 \text{ MHz} \pm 1 \text{ MHz}$	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	$(22.0 \pm 0.2) \text{ °C}$	$40.6 \pm 6 \%$	$0.98 \text{ mho/m} \pm 6 \%$
Head TSL temperature during test	$(22.0 \pm 0.2) \text{ °C}$	---	---

SAR result with Head TSL

SAR averaged over 1 cm ² (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.33 mW / g
SAR normalized	normalized to 1W	9.32 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	9.43 mW / g $\pm 17.6 \%$ (k=2)

SAR averaged over 10 cm ² (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.52 mW / g
SAR normalized	normalized to 1W	6.08 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	6.14 mW / g $\pm 16.5 \%$ (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 86(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.8 Ω - 3.4 j Ω
Return Loss	-27.2 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.291 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Design Modification by End User

The dipole has been modified with Teflon Rings (TR) placed within identified markings close to the end of each dipole arm. Calibration has been performed with TR attached to the dipole.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	April 07, 2006

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 87(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date/Time: 07.04.2011 09:28:21

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d043

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL900

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.88 \text{ mho/m}$; $\epsilon_r = 40.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; Cores F(6.03, 6.03, 6.03); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Set601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)

P_{in}=250 mW /d=15mm/Cube 0;


Measurement grid: d_x=5mm, d_y=5mm, d_z=5mm

Reference Value = 57.201 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 3.504 W/kg

SAR(1 g) = 2.33 mW/g; SAR(10 g) = 1.52 mW/g

Maximum value of SAR (measured) = 2.730 mW/g

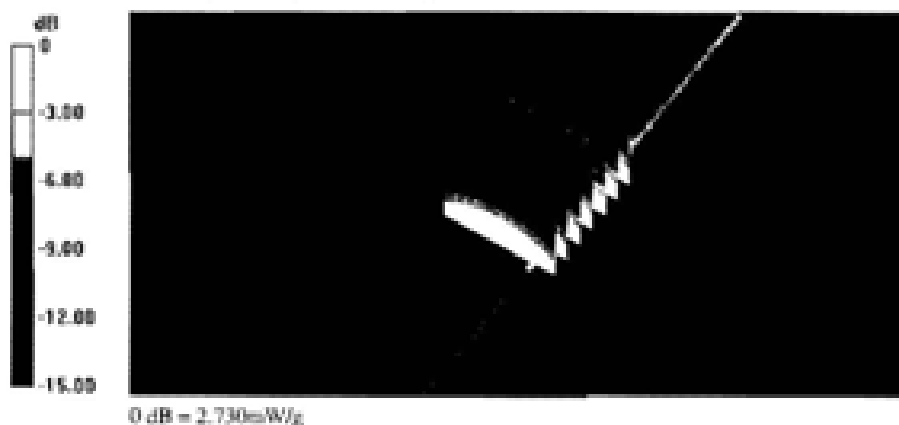

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 89(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service


Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D1800V2-2d020_Jan11**

CALIBRATION CERTIFICATE

Object	D1800V2 - SN: 2d020		
Calibration procedure(s)	QA CAL-05.v8 Calibration procedure for dipole validation kits		
Calibration date:	January 13, 2011		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (MATE critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	0803480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37392763	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20-dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047 2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe E530V3	SN: 3205	30-Apr-10 (No. E53-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MPH1000317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SM7-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8713C	US37390585 54206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11
Calibrated by:	Name Dimos Iliev	Function Laboratory Technician	Signature 
Approved by:	Name Katja Pokorski	Technical Manager	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: January 13, 2011			

Certificate No: **D1800V2-2d020_Jan11**

Page 1 of 6

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 90(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 91(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.6 ± 6 %	1.38 mho/m ± 6 %
Head TSL temperature during test	(21.3 ± 0.2) °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.78 mW / g
SAR normalized	normalized to 1W	39.1 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	39.3 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.13 mW / g
SAR normalized	normalized to 1W	20.5 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.5 mW / g ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 92(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$46.5 \Omega - 7.3 j\Omega$
Return Loss	-21.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.216 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 07, 2001

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 93(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date/Time: 13.01.2011 12:34:12

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN:2d020

Communication System: CW; Frequency: 1800 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: $f = 1800 \text{ MHz}$; $\sigma = 1.38 \text{ mho/m}$; $\epsilon_r = 38.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.05, 5.05, 5.05); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.6.1 Build (408)
- Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.654 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 17.902 W/kg

SAR(1 g) = 9.78 mW/g; SAR(10 g) = 5.13 mW/g

Maximum value of SAR (measured) = 12.051 mW/g

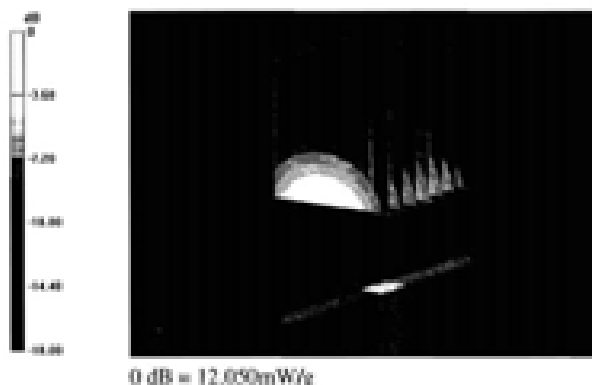

Author Data
Andrew Becker


Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02

FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

Impedance Measurement Plot for Head TSL

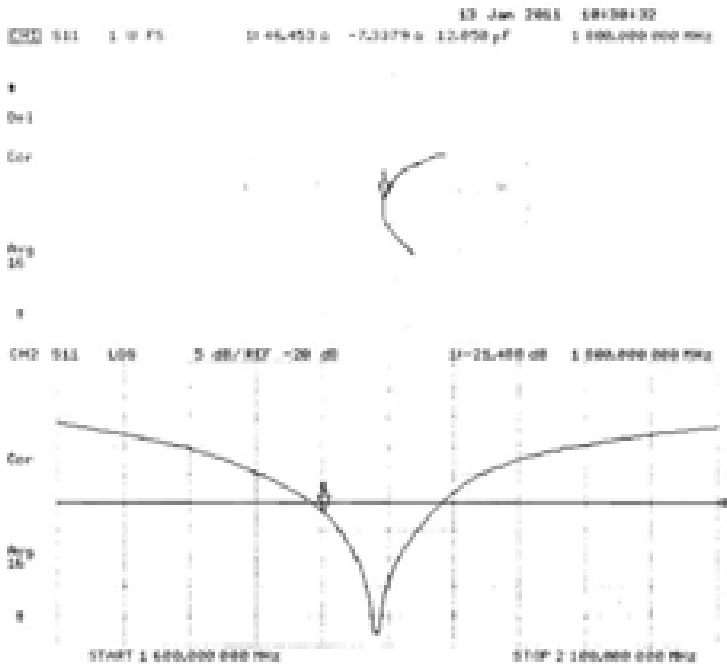

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 95(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D1800V2-2d020_Jan13**

CALIBRATION CERTIFICATE			
Object	D1800V2 - SN: 2d020		
Calibration procedure(s)	QA GAL-05.v9 Calibration procedure for dipole validation kits above 700 MHz		
Calibration date:	January 09, 2013		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (Si). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (MATE critical for calibration):			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	0807460704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	U507292780	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5058 (204)	27-Mar-12 (No. 217-01630)	Apr-13
Type-N mismatch combination	SN: 5047.3 / 06097	27-Mar-12 (No. 217-01630)	Apr-13
Reference Probe E530V3	SN: 3005	26-Dec-12 (No. E53-3005_Dec12)	Dec-13
DAE4	SN: 601	27-Jan-12 (No. 04E14-601_Jan12)	Jan-13
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MFV11002017	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator PLS SMT-06	100005	04-Aug-09 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8713C	U507290585 54706	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
Calibrated by:	Name Istvan El-Nasouj	Function Laboratory Technician	Signature 
Approved by:	Name Kajsa Polovic	Technical Manager	
Issued: January 8, 2013			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: D1800V2-2d020_Jan13

Page 1 of 6

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 96(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 97(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1:

DASY Version	DASY5	V52.8.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.9 ± 6 %	1.38 mho/m ± 6 %
Head TSL temperature change during test	± 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.61 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	38.5 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.06 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	20.3 W/kg ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 98(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	40.2 Ω - 8.3 jΩ
Return Loss	-20.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.216 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end-caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 07, 2001

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 99(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date: 09/01/2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 24020

Communication System: CW; Frequency: 1800 MHz

Medium parameters used: $f = 1800$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 38.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; CorrF(5.04, 5.04, 5.04); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.4(1052); SEMCAD X 14.6.8(7028)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.870 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 17.5 W/kg

SAR(1 g) = 9.61 W/kg; SAR(10 g) = 5.06 W/kg

Maximum value of SAR (measured) = 11.8 W/kg

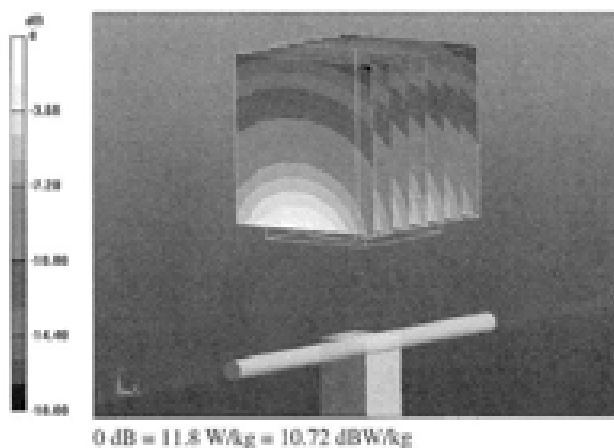

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 101(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 102(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zughausstrasse 43, 8034 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D1900V2-545_Jan11**

CALIBRATION CERTIFICATE

Object	D1900V2 - SN: 545		
Calibration procedure(s)	QA-CAL-05.v8 Calibration procedure for dipole validation kits		
Calibration date:	January 13, 2011		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (MATE critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	0807480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37262763	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5085 (20g)	30-Mar-10 (No. 217-01156)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe E530V3	SN: 3205	30-Apr-10 (No. E53-3205_Apr10)	Apr-11
DAE4	SN: 605	10-Jun-10 (No. 04E4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MFV41052317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SM1-06	100005	4-Aug-09 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37260565 54206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11
Calibrated by:	Name Dirk Baur	Function Laboratory Technician	Signature 
Approved by:	Name Ralph Finkbein	Technical Manager	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: January 14, 2011			

Certificate No: D1900V2-545_Jan11

Page 1 of 5

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 103(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields: Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 104(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.43 mho/m ± 6 %
Head TSL temperature during test	(21.2 ± 0.2) °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.2 mW / g
SAR normalized	normalized to 1W	40.8 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	40.8 mW / g ± 17.6 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.26 mW / g
SAR normalized	normalized to 1W	21.0 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.8 mW / g ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 105(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.8 Ω + 1.8 $j\Omega$
Return Loss	-34.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.189 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	November 15, 2001

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 106(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date/Time: 13.01.2011 14:52:49

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:545

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.43$ mho/m; $\epsilon_r = 38.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvR(5.09, 5.09, 5.09); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAB4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.6.1 Build (408)
- Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)


Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.053 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 18.648 W/kg

SAR(1 g) = 10.2 mW/g; SAR(10 g) = 5.26 mW/g

Maximum value of SAR (measured) = 12.743 mW/g

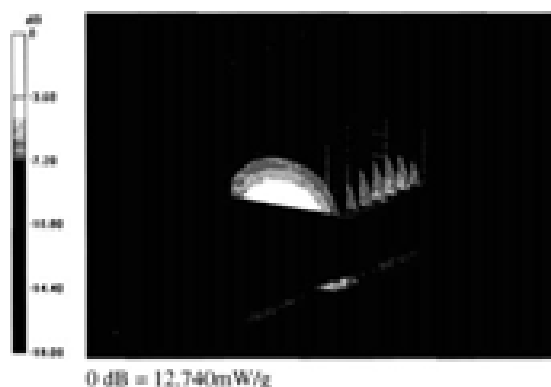

Author Data
Andrew Becker


Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02

FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

Impedance Measurement Plot for Head TSL

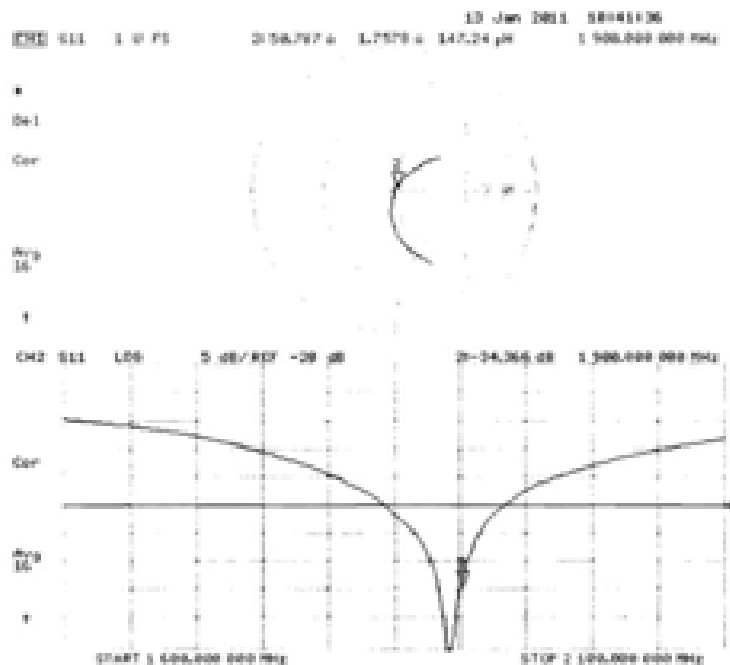

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 108(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No.: **D1900V2-545_Jan13**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 545**

Calibration procedure(s) **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **January 09, 2013**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature $22 \pm 3^\circ\text{C}$ and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-400A	0807180704	01-Nov-12 (No. 217-01040)	Oct-13
Power sensor HP 8481A	US37292763	01-Nov-12 (No. 217-01040)	Oct-13
Reference 20 dB Attenuator	SN: 5056 (204)	27-Mar-12 (No. 217-01520)	Apr-13
Type-N mismatch combination	SN: 5247.3 / 98327	27-Mar-12 (No. 217-01520)	Apr-13
Reference Probe E530V3	SN: 3005	26-Dec-12 (No. E53-3005_Dec12)	Dec-13
DAE4	SN: 601	27-Jun-12 (No. DAE4-001_Jun12)	Jun-13

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator RMS SM7 06	100005	04-Aug-09 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37290585 54206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13

Calibrated by:	Name Toris El-Nedouy	Function Laboratory Technician	Signature 
Approved by:	Katja Pokorski	Technical Manager	

Issued: January 9, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No.: **D1900V2-545_Jan13**

Page 1 of 6

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 109(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 110(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.60 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.4 ± 6 %	1.38 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm ² (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.0 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ² (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.26 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.1 W/kg ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 111(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$51.0 \Omega + 1.7 j\Omega$
Return Loss	-34.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.198 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	November 15, 2001

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 112(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date: 09/01/2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 545

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 39.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; CoreF(4.98, 4.98, 4.98); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sa601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.4(1052); SEMCAD X 14.6.8(7028)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.493 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 10 W/kg; SAR(10 g) = 5.26 W/kg

Maximum value of SAR (measured) = 12.2 W/kg

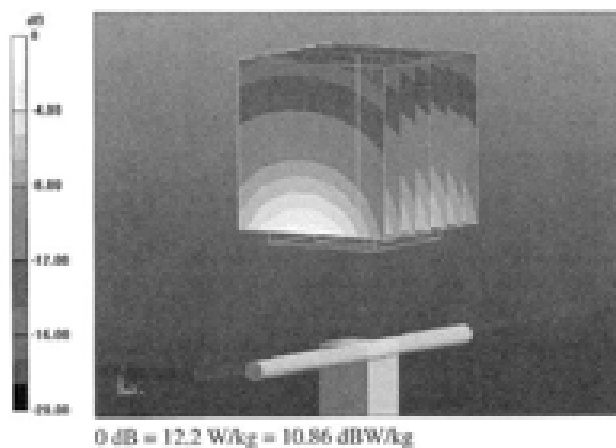

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 114(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 115(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
 Augthausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D1900V2-5d075_Apr11**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d075**
 Calibration procedure(s) **QA CAL-05.v8
Calibration procedure for dipole validation kits**
 Calibration date **April 5, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 3)°C and humidity < 70%.

Calibration Equipment used (MPE/E critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM 440x	45537460704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8441A	15327260783	06-Oct-10 (No. 217-01266)	Oct-11
Polyspace 20 dB Attenuator	SN: 1086 (J02)	29-Mar-11 (No. 217-01368)	Apr-12
Type-N mismatch combination	SN: 2047.2 / 06027	29-Mar-11 (No. 217-01371)	Apr-12
Reference Probe ES30V3	SN: 3205	30-Apr-10 (No. E53-3205_Apr10)	Apr-11
DA84	SN: 601	10-Jun-10 (No. DA84-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8441A	M141002517	18-Oct-07 (in house check Oct-08)	In house check Oct-11
RF generator R&S SM7-50	106055	4-Aug-06 (in house check Oct-06)	In house check Oct-11
Network Analyzer HP 8713C	15327260785 54206	18-Oct-01 (in house check Oct-10)	In house check Oct-11

Calibrated by: **Name: Jelle Moll** Function: **Laboratory Technician**
 Approved by: **Katja Polzella** Technical Manager

Signature



Issued: April 6, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D1900V2-5d075_Apr11**

Page 1 of 5

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 116(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zugwegstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 117(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V50.0.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.41 mho/m ± 6 %
Head TSL temperature during test	(21.3 ± 0.2) °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.2 mW / g
SAR normalized	normalized to 1W	40.8 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	40.4 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.29 mW / g
SAR normalized	normalized to 1W	21.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	21.0 mW / g ± 16.5 % (k=2)

		Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report		Page 118(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$53.5 \Omega + 6.1 j\Omega$
Return Loss	-23.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.197 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the loading line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	January 24, 2008

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 119(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date/Time: 05.04.2011 12:41:39

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:54075

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.41$ mho/m; $\epsilon_r = 39$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES01W3 - SNT006; Cal: H15.09, 5.09, 5.09; Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detectors)
- Electronic: DASA Sat00; Calibrated: 10.06.2010
- Phantom: Flat Phantom SAR (Front); Type: QD000P35AA; Serial: 1000
- Measurement SW: DASY52, V32.6.2 Build (424)
- Postprocessing SW: SIMCAD-X, V14.4.6 Build (2029)

Head / d=10mm, Pin=250 mW / Cube 0:


Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 97.376 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 18.796 W/kg


SAR(1 g) = 10.2 mW/g; SAR(10 g) = 5.29 mW/g

Maximum value of SAR (measured) = 12.476 mW/g

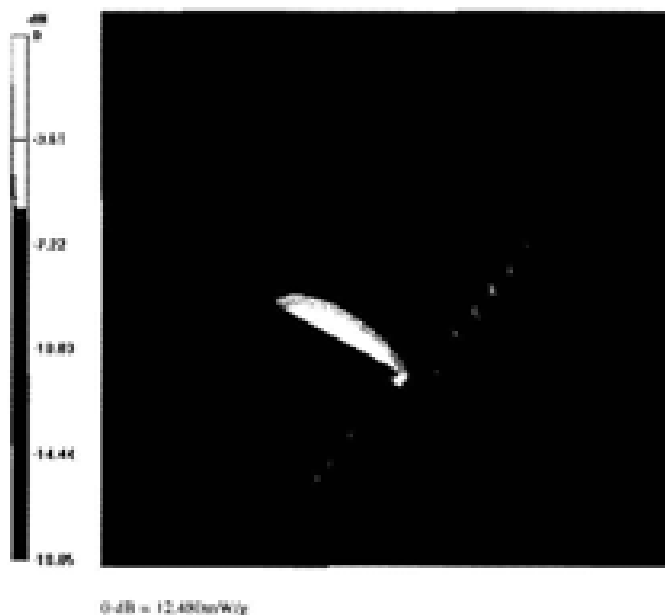

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 120(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Impedance Measurement Plot for Head TSL

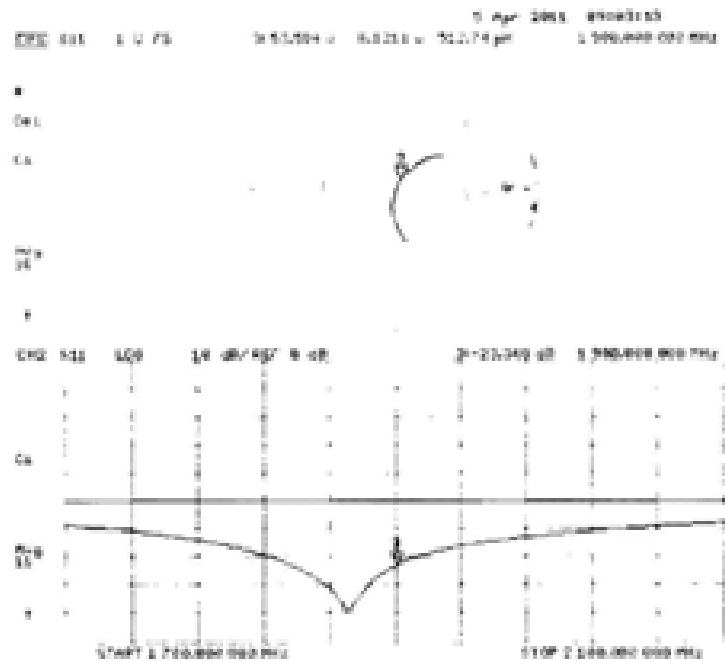

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 121(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client: **RTS (RIM Testing Services)**

Certificate No.: **D2450V2-747_Nov11**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN: 747**

Calibration procedure(s): **QA CAL-05.v6**
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **November 09, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 75%.

Calibration Equipment used (MELTE, official for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	08027482704	05-Oct-11 (No. 217-0145/1)	Oct-12
Power sensor HP 8481A	US37292785	05-Oct-11 (No. 217-0145/1)	Oct-12
Reference 20-dB Attenuator	SN: 5086 (20g)	29-Mar-11 (No. 217-01368)	Apr-12
Type-N mismatch combination	SN: 5047.2 / 06327	29-Mar-11 (No. 217-01371)	Apr-12
Reference Probe ES30V3	SN: 3205	29-Apr-11 (No. ES3-3205_Apr11)	Apr-12
DA44	SN: 601	04-Jul-11 (No. DA44-601_Jul11)	Jul-12
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41062017	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-09 (in house check Oct-11)	In house check: Oct-13
Network Analyser HP 8753E	US37390585 54206	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

Calibrated by: **Jeton Kasiner** (Name) **Laboratory Technician** (Function)  (Signature)
Approved by: **Katja Pokorski** (Name) **Technical Manager** (Function)  (Signature)

Issued: November 9, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **D2450V2-747_Nov11**

Page 1 of 5

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 122(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zughauserstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 123(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.7 ± 6 %	1.84 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.8 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	54.1 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.39 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	25.5 mW / g ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 124(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$52.5 \Omega + 1.3 j\Omega$
Return Loss	-31.2 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.581 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 01, 2003

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 125(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date: 09.11.2011

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 747

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.84$ mho/m; $\epsilon_r = 37.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 29.04.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Head Tissue/ $P_{in}=250$ mW, $d=10$ mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 102.1 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 28.853 W/kg

SAR(1 g) = 13.8 mW/g; SAR(10 g) = 6.39 mW/g


Maximum value of SAR (measured) = 17.782 mW/g

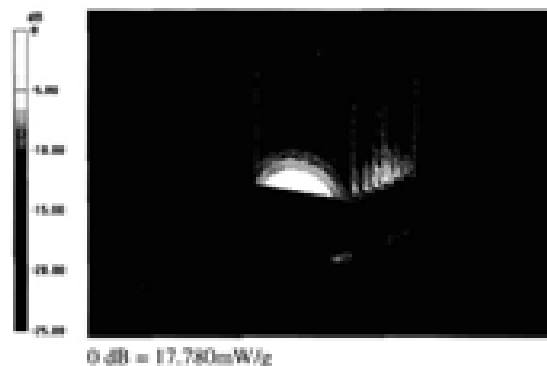



Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW
-------------------------------------	---	---	---	--

Impedance Measurement Plot for Head TSL

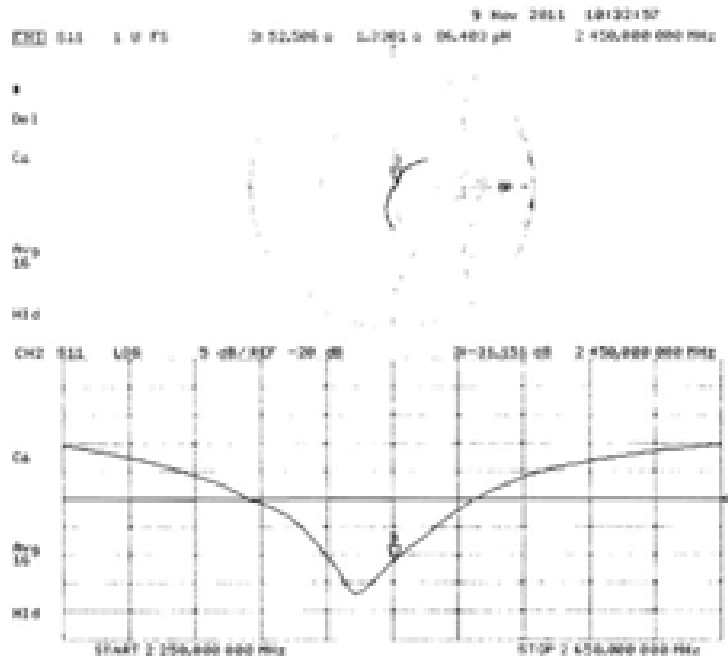

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 127(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zughausstrasse 49, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SGS 108**

Client **RTS (RIM Testing Services)**

Certificate No: **D5GHzV2-1033_Nov11**

CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN: 1033**

Calibration procedure(s) **QA CAL-22.v1**
Calibration procedure for dipole validation kits between 3-8 GHz

Calibration date: **November 15, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 2)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	0607480704	05-Oct-11 (No. 217-01401)	Oct-12
Power sensor HP 8481A	U537292783	05-Oct-11 (No. 217-01401)	Oct-12
Reference 20 dB Attenuator	SN: 5086 (20g)	29-Mar-11 (No. 217-01368)	Apr-12
Type-N mismatch combination	SN: 5047.2 / 06327	29-Mar-11 (No. 217-01371)	Apr-12
Reference Probe EX3DV4	SN: 3603	04-Mar-11 (No. EX3-3603_Mar11)	Mar-12
DAB4	SN: 601	04-Jul-11 (No. DAB4-601_Jul11)	Jul-12

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator RMS SMT-06	100005	04-Aug-09 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8713B	U537300585-54206	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

Calibrated by:	Name Dirce Bay	Function Laboratory Technician	Signature 
Approved by:	Name Rafal Polonski	Technical Manager	

Issued: November 15, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 128(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zugstrasse 43, 8054 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 129(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.6 ± 6 %	4.46 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.16 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	80.8 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.33 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	23.0 mW / g ± 16.5 % (k=2)

Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.2 ± 6 %	4.75 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.82 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	87.3 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.50 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.7 mW / g ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 130(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	33.7 ± 6 %	5.03 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.03 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	79.4 mW / g ± 17.6 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.28 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	22.5 mW / g ± 16.5 % (k=2)

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 131(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

Appendix

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	51.1 Ω - 8.7 $\mu\Omega$
Return Loss	- 21.2 dB

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	52.3 Ω - 2.7 $\mu\Omega$
Return Loss	- 29.2 dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	56.7 Ω - 4.3 $\mu\Omega$
Return Loss	- 22.6 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.202 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 09, 2004

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 132(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

DASY5 Validation Report for Head TSL

Date: 15.11.2011

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1033

Communication System: CW; Frequency: 5200 MHz; Frequency: 5500 MHz; Frequency: 5800 MHz
Medium parameters used: $f = 5200 \text{ MHz}$; $\sigma = 4.46 \text{ mho/m}$; $\epsilon_r = 34.6$; $\rho = 1000 \text{ kg/m}^3$, Medium parameters used: $f = 5500 \text{ MHz}$; $\sigma = 4.75 \text{ mho/m}$; $\epsilon_r = 34.2$; $\rho = 1000 \text{ kg/m}^3$, Medium parameters used: $f = 5800 \text{ MHz}$; $\sigma = 5.03 \text{ mho/m}$; $\epsilon_r = 33.7$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:


- Probe: EX3DV4 - SN3503; ConvF(5.41, 5.41, 5.41), ConvF(4.91, 4.91, 4.91), ConvF(4.81, 4.81, 4.81); Calibrated: 04.03.2011
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: $dx=4\text{mm}$, $dy=4\text{mm}$, $dz=1.4\text{mm}$
Reference Value = 65.595 V/m; Power Drift = 0.07 dB
Peak SAR (extrapolated) = 30.134 W/kg
SAR(1 g) = 8.16 mW/g; SAR(10 g) = 2.33 mW/g
Maximum value of SAR (measured) = 18.725 mW/g

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: $dx=4\text{mm}$, $dy=4\text{mm}$, $dz=1.4\text{mm}$
Reference Value = 66.819 V/m; Power Drift = 0.03 dB
Peak SAR (extrapolated) = 35.056 W/kg
SAR(1 g) = 8.82 mW/g; SAR(10 g) = 2.5 mW/g
Maximum value of SAR (measured) = 21.019 mW/g

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: $dx=4\text{mm}$, $dy=4\text{mm}$, $dz=1.4\text{mm}$
Reference Value = 62.220 V/m; Power Drift = 0.04 dB
Peak SAR (extrapolated) = 33.743 W/kg
SAR(1 g) = 8.03 mW/g; SAR(10 g) = 2.28 mW/g
Maximum value of SAR (measured) = 19.463 mW/g

	Document Appendix D for the BlackBerry® Smartphone Model RFP121LW SAR Report			Page 133(134)
Author Data Andrew Becker	Dates of Test Nov 22, 2012 – Feb 28, 2013	Test Report No RTS-6026-1303-02	FCC ID: L6ARFL110LW L6ARFP120LW	IC 2503A-RFL110LW 2503A-RFP120LW

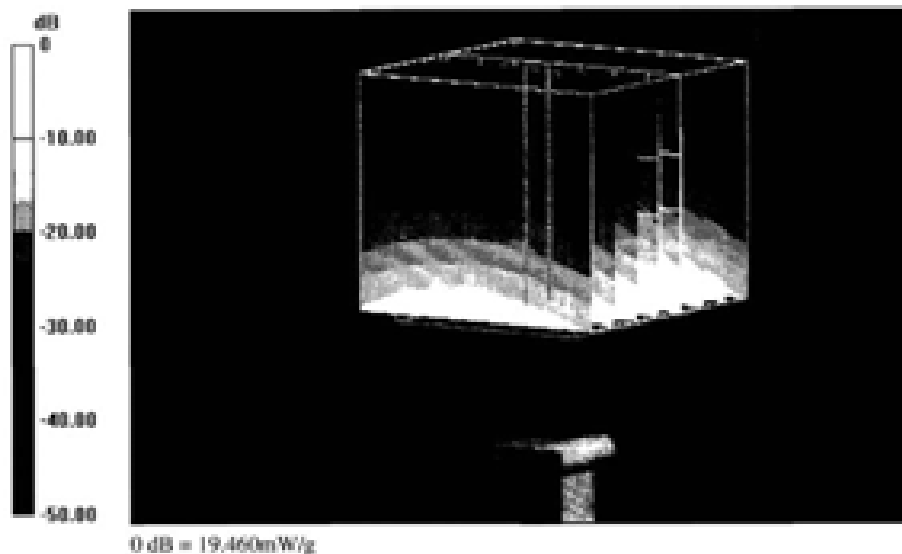

Author Data
Andrew Becker

Dates of Test
Nov 22, 2012 – Feb 28, 2013

Test Report No
RTS-6026-1303-02

FCC ID:
**L6ARFL110LW
L6ARFP120LW**

IC
**2503A-RFL110LW
2503A-RFP120LW**

Impedance Measurement Plot for Head TSL

