

APPENDIX

11. Photographs of Test Setup

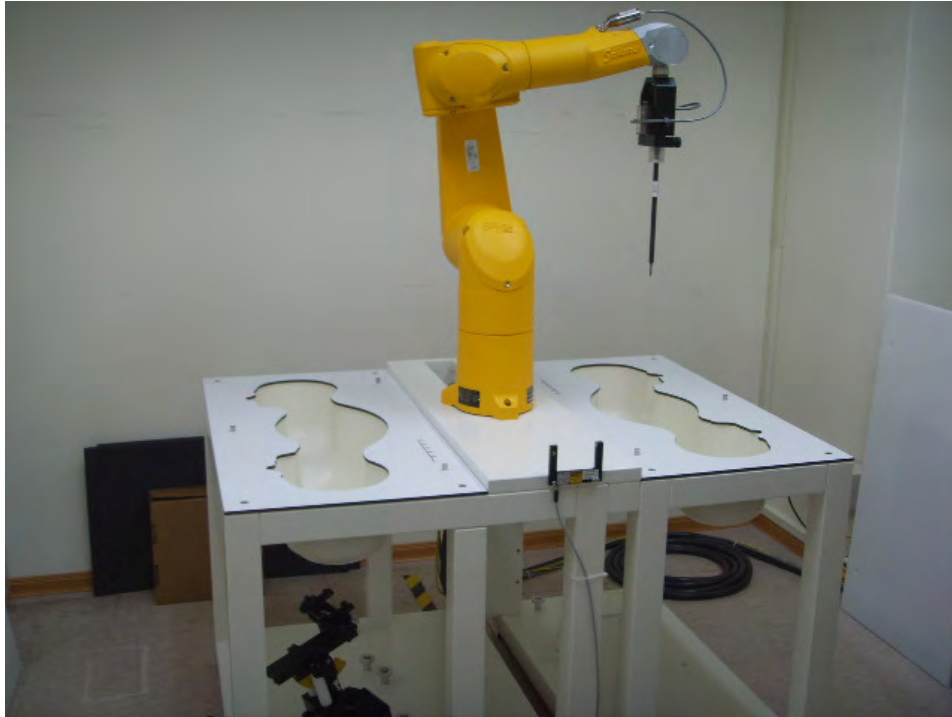


Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

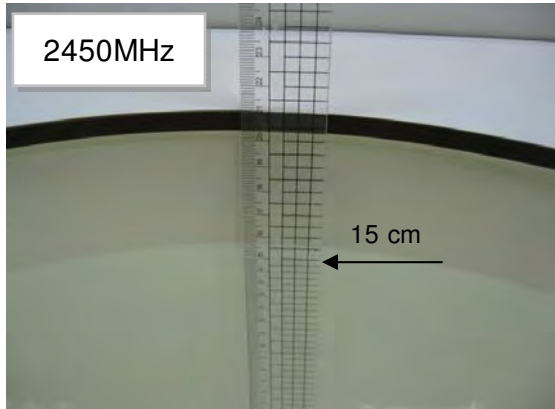


Fig.2.1

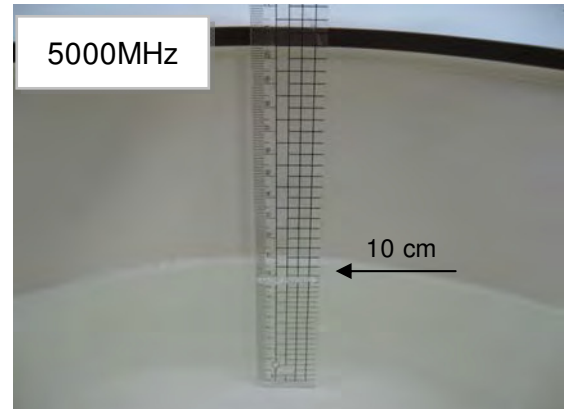


Fig.2.2

Body - distance between flat phantom and EUT is 0 mm



Fig.3 EUT Lap-held mode to flat phantom



Fig.4 EUT Top side to flat phantom



Fig.5 EUT Right side to flat phantom

12. Photographs of the EUT



Fig.6 Front view of EUT



Fig.7 Back view of EUT

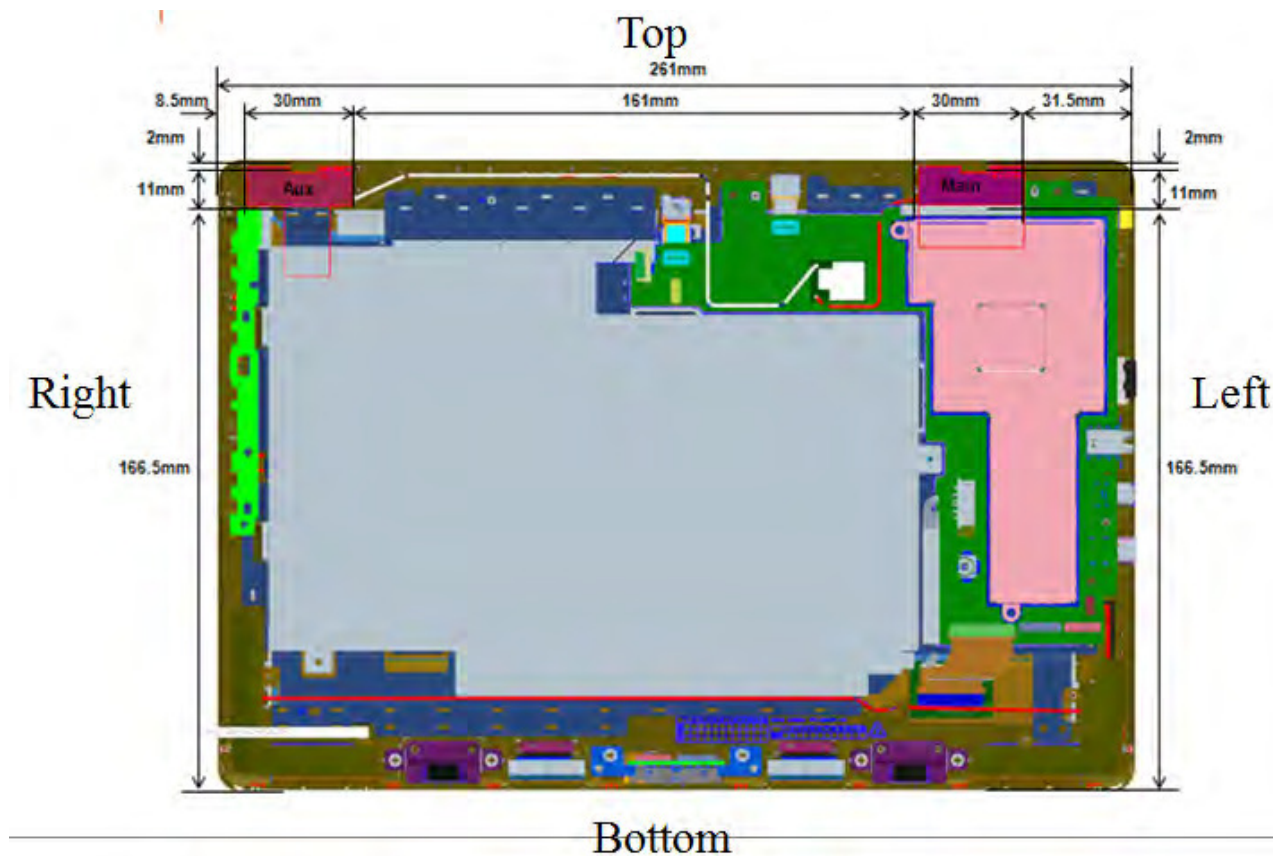


Fig.8 Antenna position of EUT (Back view)

- End of Report -