


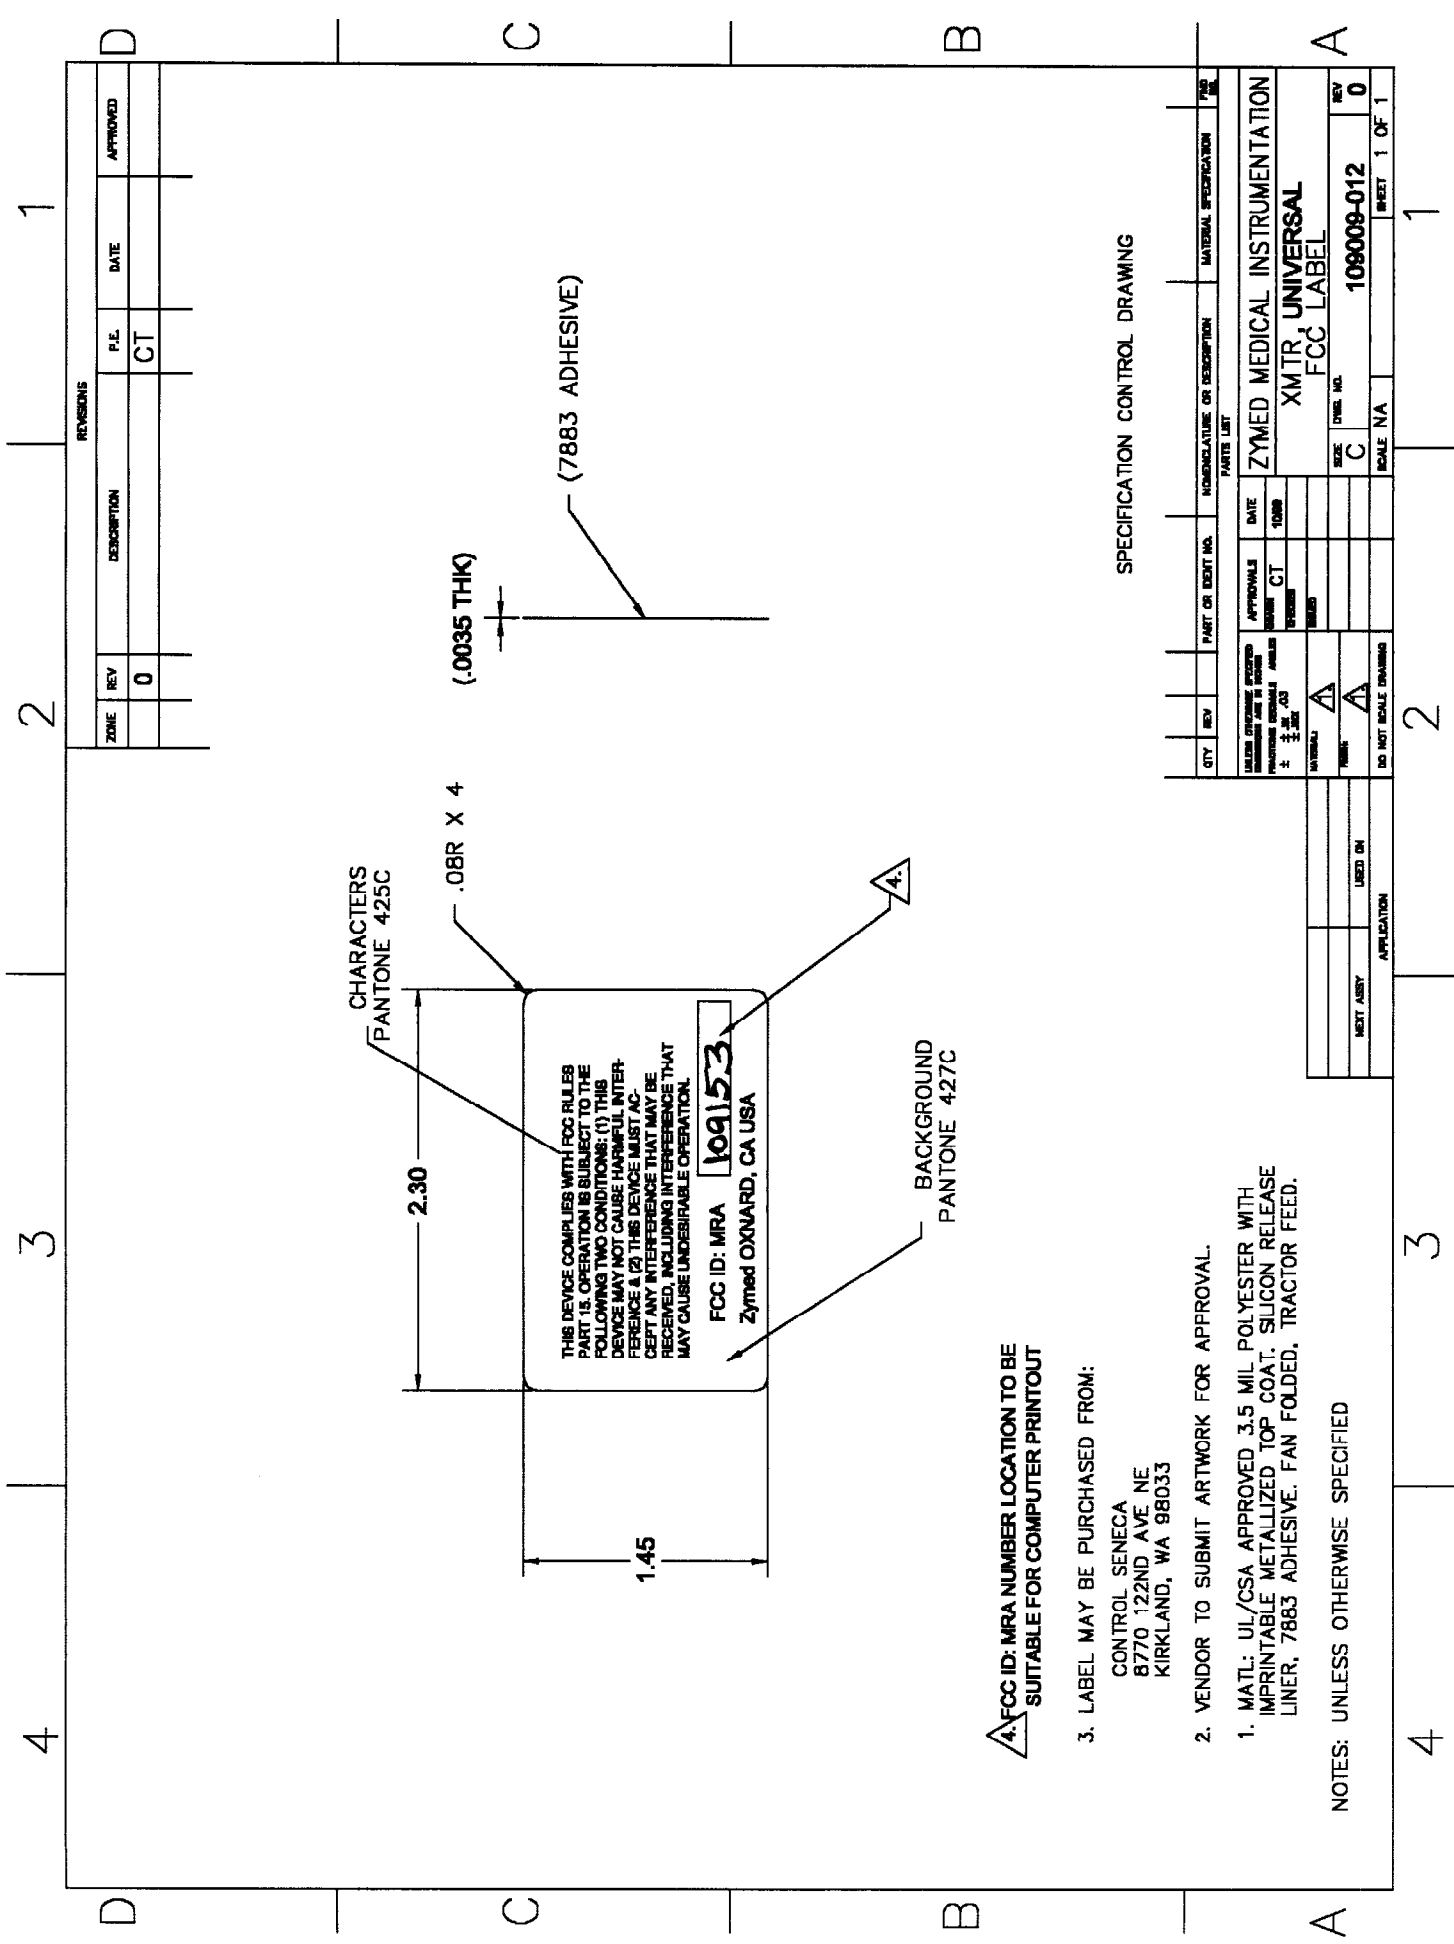

REVISIONS			
ZONE	REV	DESCRIPTION	DATE
	0	CT	

SPECIFICATION CONTROL DRAWING

QTY	REV	PART OR DETAIL NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	FIG NO
PARTS LIST					
APPROVALS		DATE	ZYMED MEDICAL INSTRUMENTATION		
DESIGNED BY		10/88	XMTR, UNIVERSAL		
CHECKED BY			FCC LABEL		
MATERIALS			SIZE	QTY	REV
FINISH			C	109009-012	0
DO NOT SCALE DRAWING			SCALE	NA	SHEET 1 OF 1

4. FCC ID: MRA NUMBER LOCATION TO BE SUITABLE FOR COMPUTER PRINTOUT

- 3. LABEL MAY BE PURCHASED FROM:
CONTROL SENECA
8770 122ND AVE NE
KIRKLAND, WA 98033
- 2. VENDOR TO SUBMIT ARTWORK FOR APPROVAL.
- 1. MATL: UL/CSA APPROVED 3.5 MIL POLYESTER WITH IMPRINTABLE METALLIZED TOP COAT. SILICON RELEASE LINER, 7883 ADHESIVE. FAN FOLDED, TRACTOR FEED.

NOTES: UNLESS OTHERWISE SPECIFIED

4 3 2 1




ASSEMBLY PROCEDURES (CONTINUED)



INSTALL SWITCH CAP FN 25 USING LOCTITE
242 FN 53.



INSTALL LABEL, ELECTROLEAD PLACEMENT
FN 32. INSTALL LABEL, FCC FN 33. INSTALL
INSTALL LABEL, MODEL NO./ SERIAL NO. FN 34.

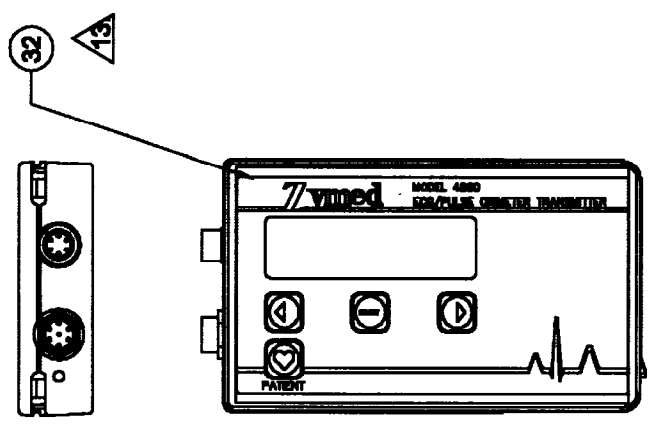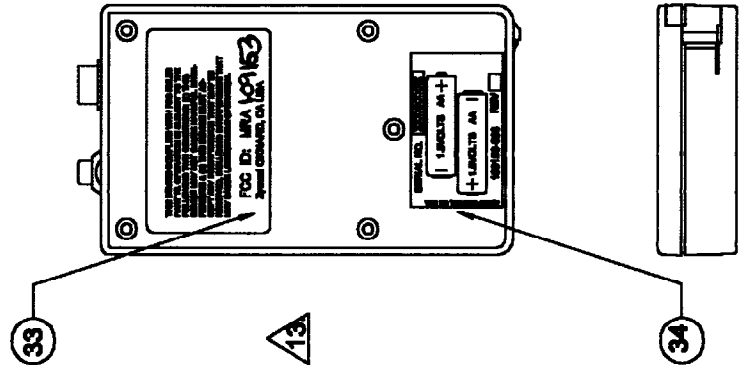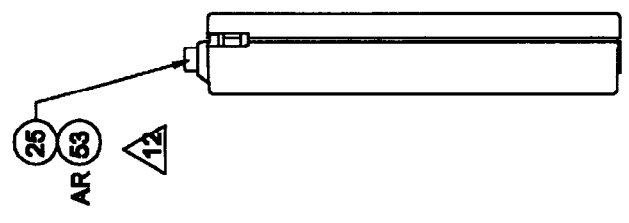

SIZE	FORM NO.	REV
C	109150-003	0
SCALE	NA	SHEET 5 OF 5

4 3 2 1