




WARNING: Improper routing of leads may result in a choking hazard



WARNING: Do NOT use in conjunction with a DEFIBRILLATOR

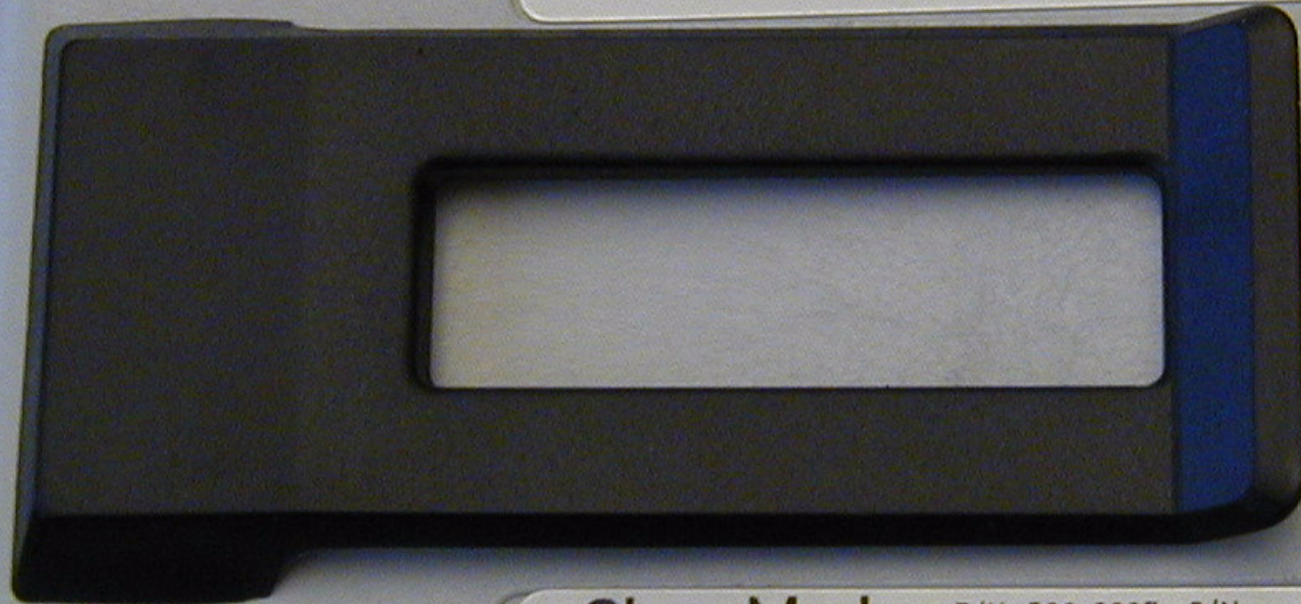

CleveMed

© • • • Cleveland Medical Devices Inc.

4415 Euclid Ave.
Cleveland, OH 44103

Freq: 905 - 928 MHz
FCC ID: N9Y0087

P/N: 502-0087 S/N: _____



RF CHANNEL: _____
US Patents 5,755,230,
6,167,258, 6,172,579B1
and other foreign patents
pending.