

NOTES:


1. ALL RESISTORS +/- 5% 200PPM EXCEPT AS NOTED
2. ALL CAPACITORS > 100pF X7R +/- 10% OR BETTER
3. ALL ELECTROLYTICS +/- 20% OR BETTER
4. ALL CAPACITORS < 10 pF NPO +/- 5%
5. ALL INDUCTORS +/- 10% Q>33 Rmax = < 2 OHMS

ALARM MODE 1 = FAST MOTION CAUSES ALARM
ALARM MODE 0 = NO MOTION CAUSES ALARM

ALARM RATES:

- 0 0 5SEC 60BPM
- 0 1 20SEC 75BPM
- 1 0 40SEC 100BPM
- 1 1 60SEC 150BPM

6. R23 INSTALLED WHEN NO ON/OFF SWITCH IS USED
7. R25 IS NOT PLACED, USED TO ENTER CALIBRATION MODE.
8. ONLY ONE OF U10 OR U11 IS INSTALLED, NOT BOTH.

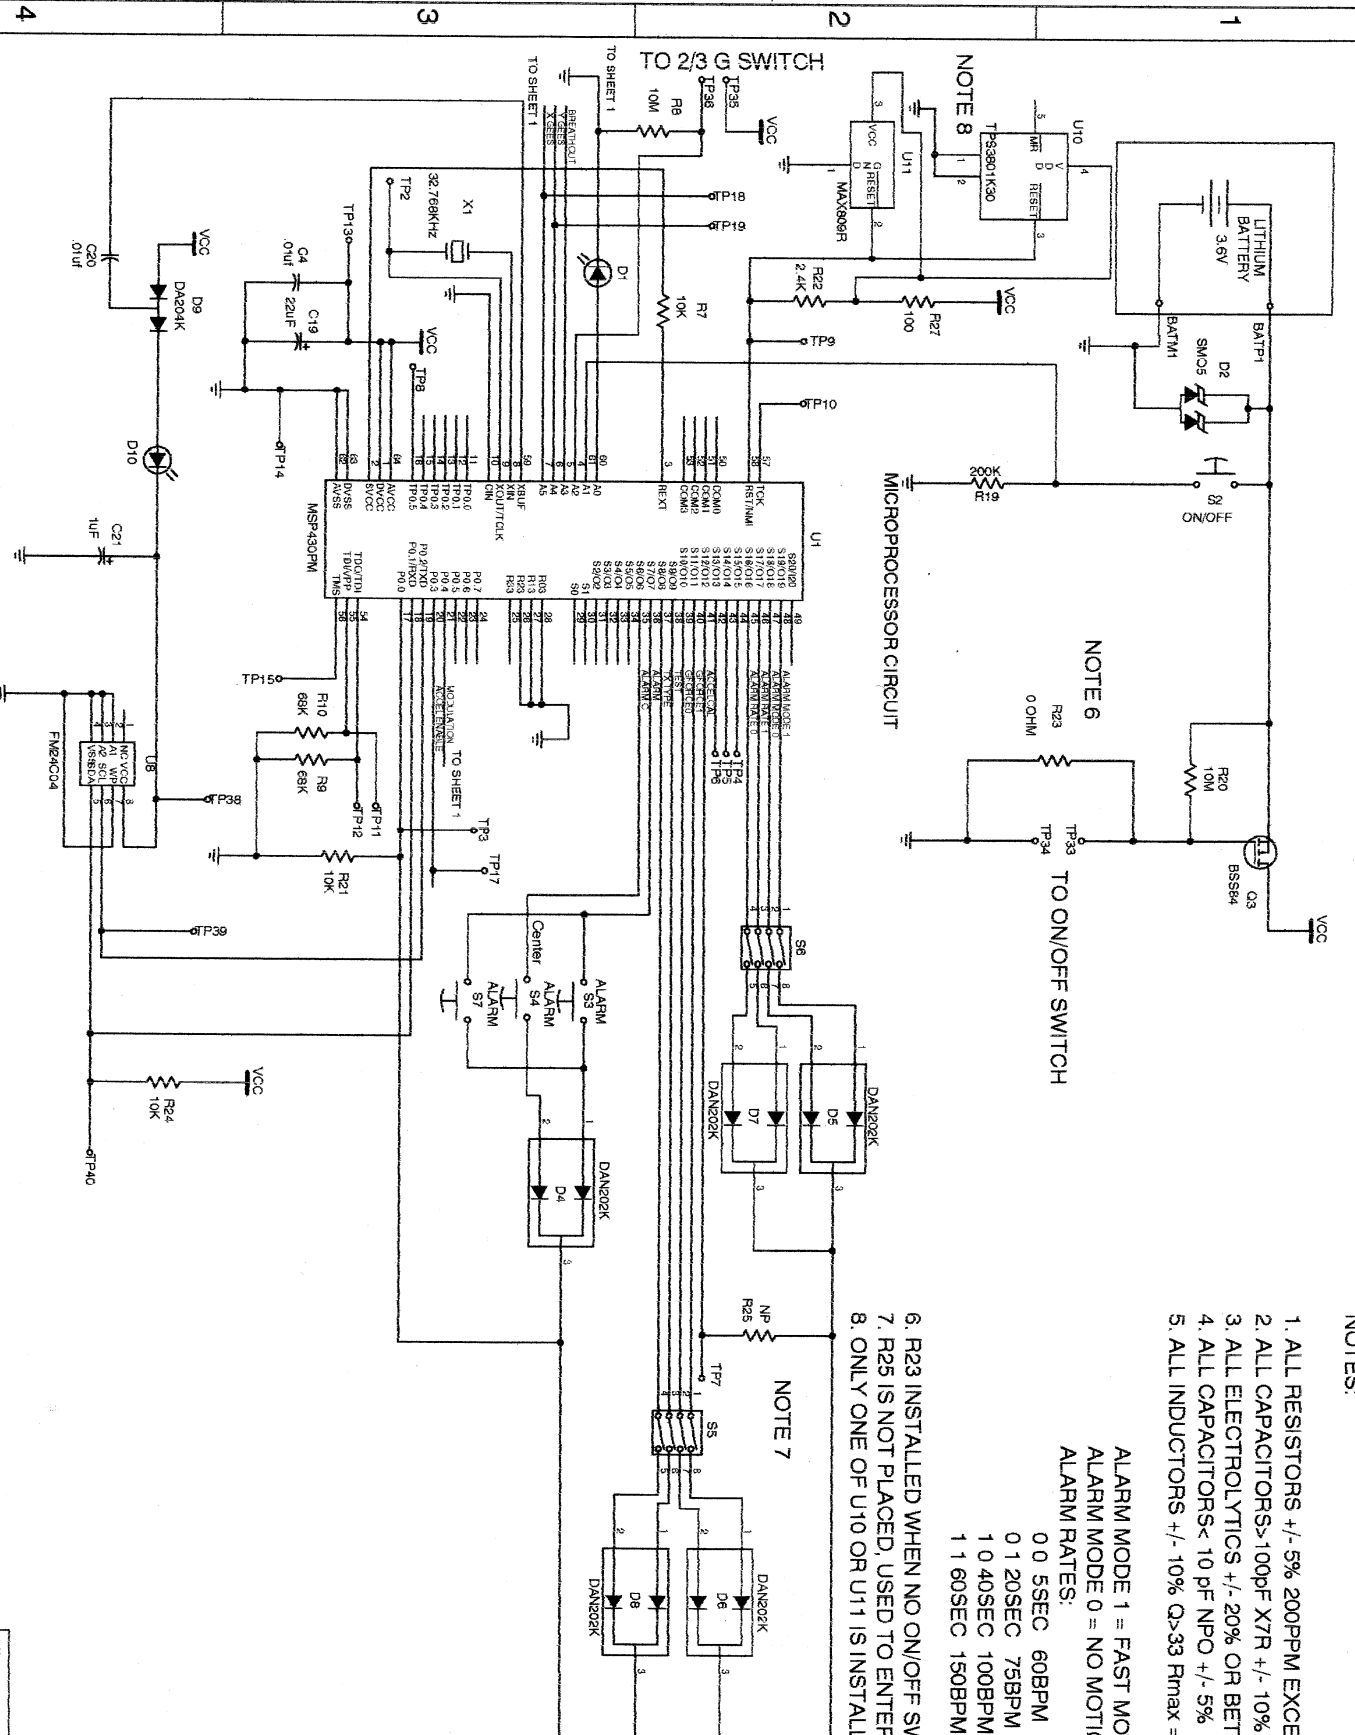

ECO#IAF104 11/13/99

Title
PERS FALL ALERT USER MODULE

1-PCB-0015

Size	Number	IAF0711
C		
Date	11/16/99	Drawn by gav
Filename	IAF711RB.S02	Sheet 2 of