

Appendix 2 Photodocumentation

Description: Test setup for measurements below
30 MHz

Medizintechnik/Nach-
richtentechnik/EMV

Department: FG

Test report reference:
M/FG-03/102

Page: 1 of 4

Date: 23. 1. 2003

checked by: *MA*



Appendix 2 Photodocumentation

Description: Test setup for measurements
between 30 MHz and 3 GHz

Medizintechnik/Nach-
richtentechnik/EMV


Department: FG

Test report reference:
M/FG-03/102

Page: 2 of 4

Date: 23. 1. 2003

checked by: *M*

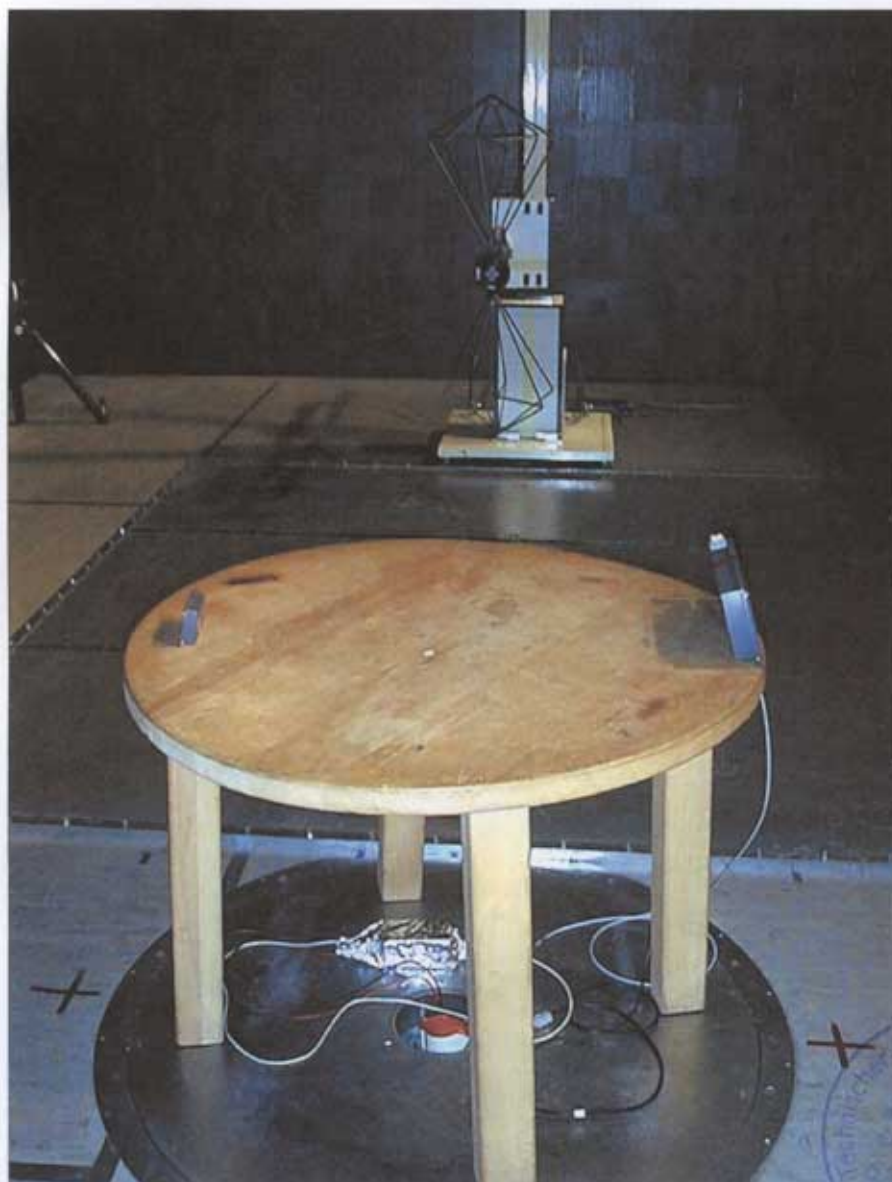

Appendix 2 Photodocumentation

Description: Test setup for measurements above
18 GHz

Medizintechnik/Nach-
richtentechnik/EMV


Department: FG

Test report reference:
M/FG-03/102

Page: 3 of 4

Date: 23. 1. 2003

checked by: *AM*

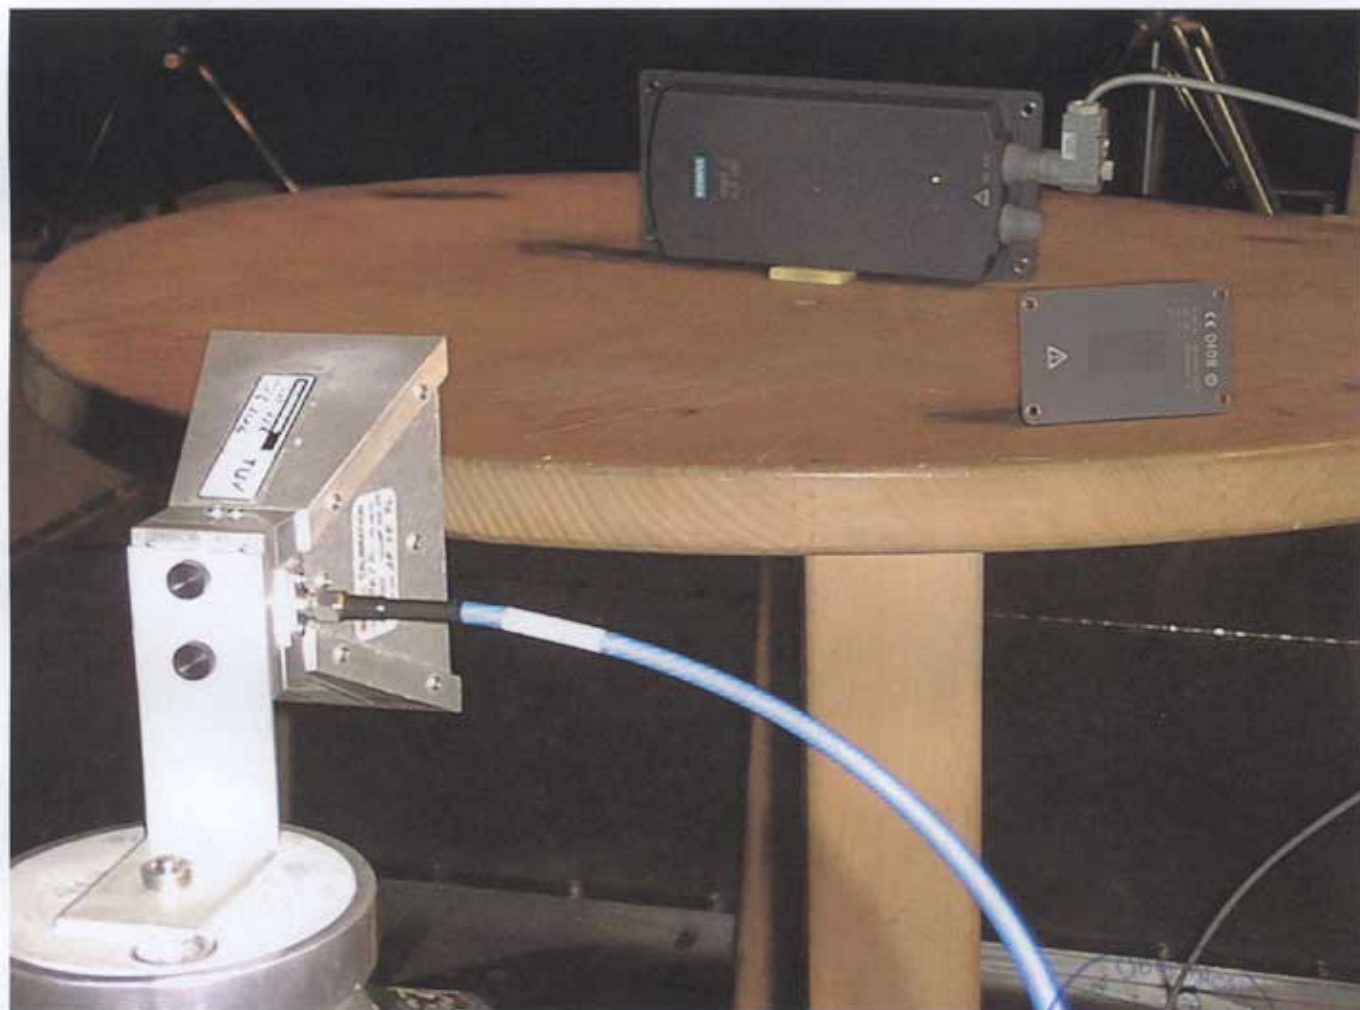

Appendix 2
Photodocumentation

Description: Detail view of test setup

Medizintechnik/Nachrichtentechnik/EMV

Department: FG

Test report reference:
M/FG-03/102

Page: 4 of 4

Date: 23. 1. 2003

checked by: 

