

Appendix 2  
Photodocumentation

**Description:** Test setup

Medizintechnik/Nach-  
richtentechnik/EMV

Department: FG

Test report reference:  
M/FG-03/130

Page: 13 of 16

Date: 4. 12. 2003

checked by: 



## Appendix 2 Photodocumentation

**Description:** Test setup in the frequency range  
30MHz - 1 GHz

Medizintechnik/Nach-  
richtentechnik/EMV


Department: FG

Test report reference:  
M/FG-03/130

Page: 14 of 16

Date: 4. 12. 2003

checked by:   *N*  

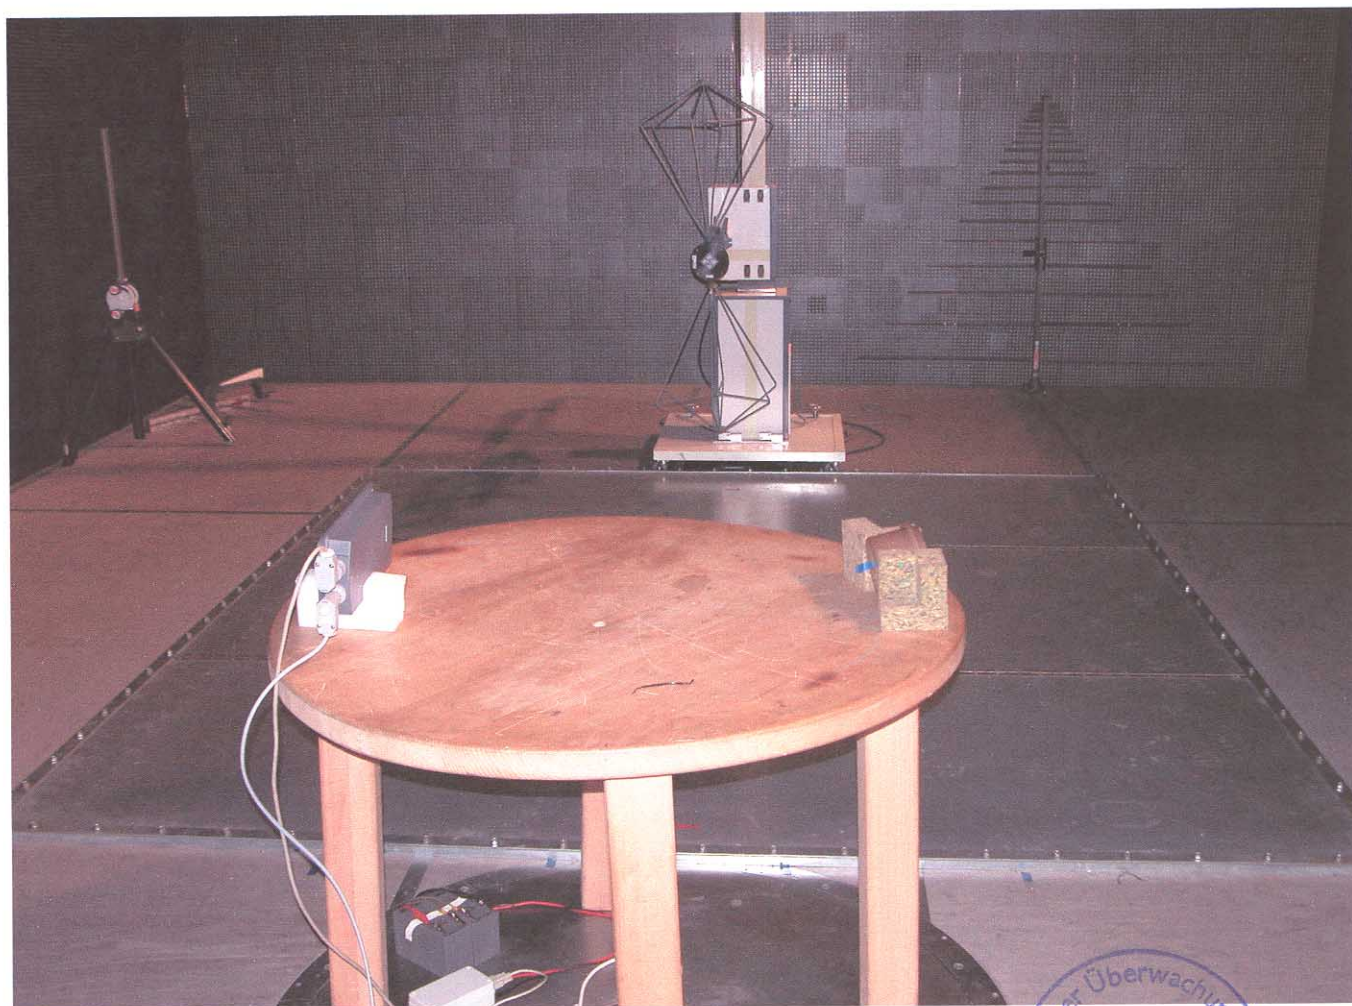

## Appendix 2 Photodocumentation

**Description:** Test setup in the frequency range 1 - 18 GHz

Medizintechnik/Nachrichtentechnik/EMV


Department: FG

Test report reference:  
M/FG-03/130

Page: 15 of 16

Date: 4. 12. 2003

checked by: 

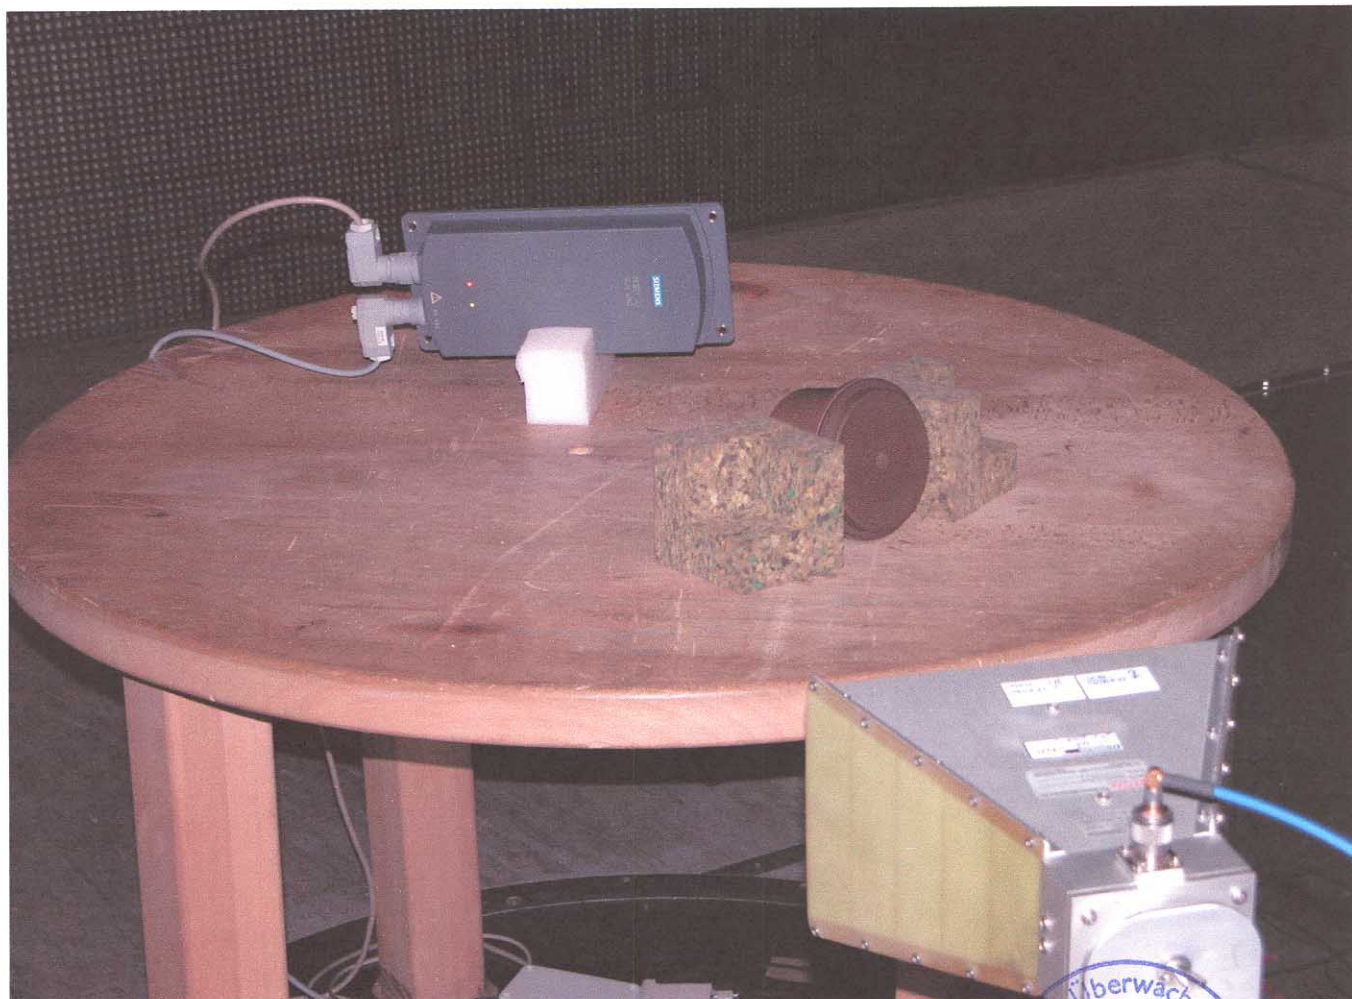

## Appendix 2 Photodocumentation

**Description:** Test setup in the frequency range  
above 18 GHz

Medizintechnik/Nach-  
richtentechnik/EMV

Department: FG

Test report reference:  
M/FG-03/130

Page: 16 of 16

Date: 4. 12. 2003

checked by: 

