

Appendix 2 Photodocumentation

Description: Test setup

Medizintechnik/Nach-
richtentechnik/EMV

Department: FG

Test report reference:
M/FG-03/131

Page: 13 of 16

Date: 4. 12. 2003

checked by: M



Appendix 2 Photodocumentation

Description: Test setup in the frequency range
30MHz - 1 GHz

Medizintechnik/Nach-
richtentechnik/EMV


Department: FG

Test report reference:
M/FG-03/131

Page: 14 of 16

Date: 4. 12. 2003

checked by: MA

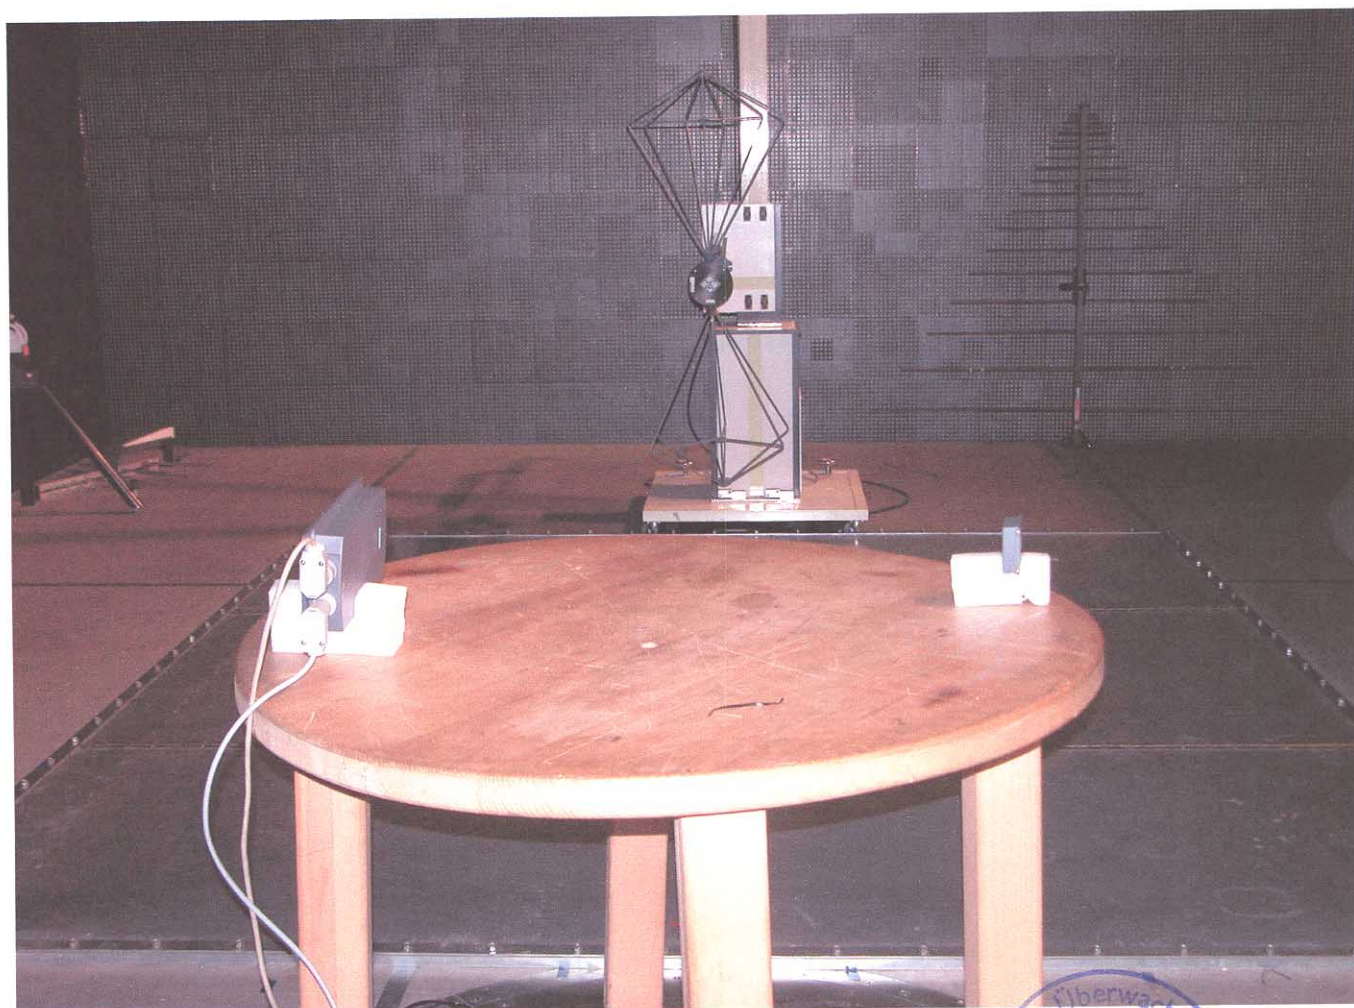

Appendix 2 Photodocumentation

Description: Test setup in the frequency range
1 - 18 GHz

Medizintechnik/Nach-
richtentechnik/EMV


Department: FG

Test report reference:
M/FG-03/131

Page: 15 of 16

Date: 4. 12. 2003

checked by: 

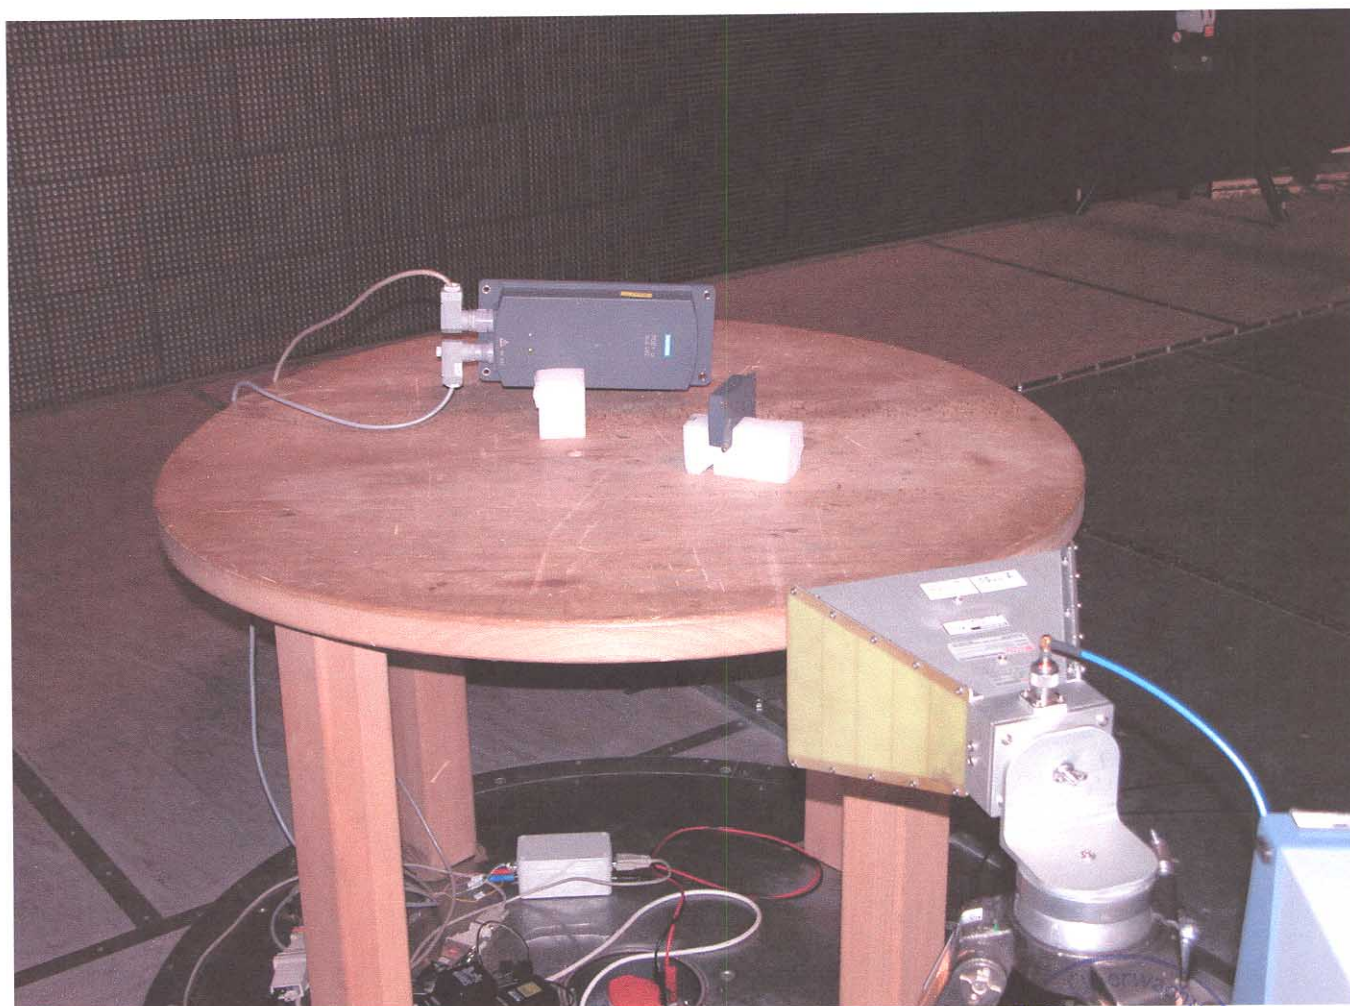

Appendix 2 Photodocumentation

Description: Test setup in the frequency range
above 18 GHz

Medizintechnik/Nach-
richtentechnik/EMV

Department: FG

Test report reference:
M/FG-03/131

Page: 16 of 16

Date: 4. 12. 2003

checked by: *M*

